



US0D1027596S

(12)

United States Design Patent

Borchert

(10)

Patent No.:

US D1,027,596 S

(45)

Date of Patent:

** May 21, 2024

(54) PINCH CLAMP

(71) Applicant: MASTERFLEX, LLC, Radnor, PA (US)

(72) Inventor: Sean Michael Borchert, Crystal Lake, IL (US)

(73) Assignee: MASTERFLEX, LLC, Radnor, PA (US)

(**) Term: 15 Years

(21) Appl. No.: 29/827,780

(22) Filed: Feb. 22, 2022

Related U.S. Application Data

(63) Continuation of application No. 17/670,996, filed on Feb. 14, 2022, now Pat. No. 11,692,633.

(51) LOC (14) Cl. 08-05

(52) U.S. Cl. USPC D8/72

(58) Field of Classification Search USPC D8/71-74, 323-329, 354-358, D8/360-360.1, 363-366, 373; D24/143 CPC A61B 2017/2808; A61B 17/1227; A61B 17/2833; A61B 17/1327 See application file for complete search history.

(56) References Cited

U.S. PATENT DOCUMENTS

5,320,389	A	6/1994	Dupont
5,474,268	A	12/1995	Yu
6,234,448	B1	5/2001	Porat
6,435,568	B1	8/2002	Fukano et al.
6,708,377	B2	3/2004	Maunder
6,796,586	B2	9/2004	Werth
7,066,441	B2	6/2006	Warburton
7,137,611	B2	11/2006	Aulicino
7,384,078	B2	6/2008	Cobb et al.
7,559,525	B2	7/2009	Grimes

D619,711	S *	7/2010	Lombardo	D8/395
8,028,378	B2	10/2011	Shor et al.	
8,177,187	B2	5/2012	Feast	
8,256,802	B2	9/2012	Werth	
(Continued)				

FOREIGN PATENT DOCUMENTS

EP 0762034 A1 3/1997

OTHER PUBLICATIONS

Bio-Ease-Sanitary-Clamp, TBL Plastics, Jan. 25, 2017, <https://tblplastics.com/wp-content/uploads/2017/01/Bio-Ease-Sanitary-Clamp-HD-Rev.-Jan-25-2017.pdf> (Year: 2017).* (Continued)

Primary Examiner — Karen S Acker
Assistant Examiner — Elizabeth S Ko
(74) Attorney, Agent, or Firm — Faegre Drinker Biddle & Reath LLP


(57) CLAIM

The ornamental design for a pinch clamp, as shown and described.

DESCRIPTION

FIG. 1 is a front right perspective view of a pinch clamp showing the new design;
FIG. 2 is a front view of the design shown in FIG. 1;
FIG. 3 is a rear view of the design shown in FIG. 1;
FIG. 4 is a left side view of the design shown in FIG. 1;
FIG. 5 is a right side view of the design shown in FIG. 1;
FIG. 6 is a top view of the design shown in FIG. 1; and,
FIG. 7 is a bottom view of the design shown in FIG. 1.
The broken lines shown in the figures are included for the purpose of illustrating environmental portions of the pinch clamp and form no part of the claimed design.
The dot-dash lines depict the boundaries of the claim and form no part thereof.

1 Claim, 7 Drawing Sheets

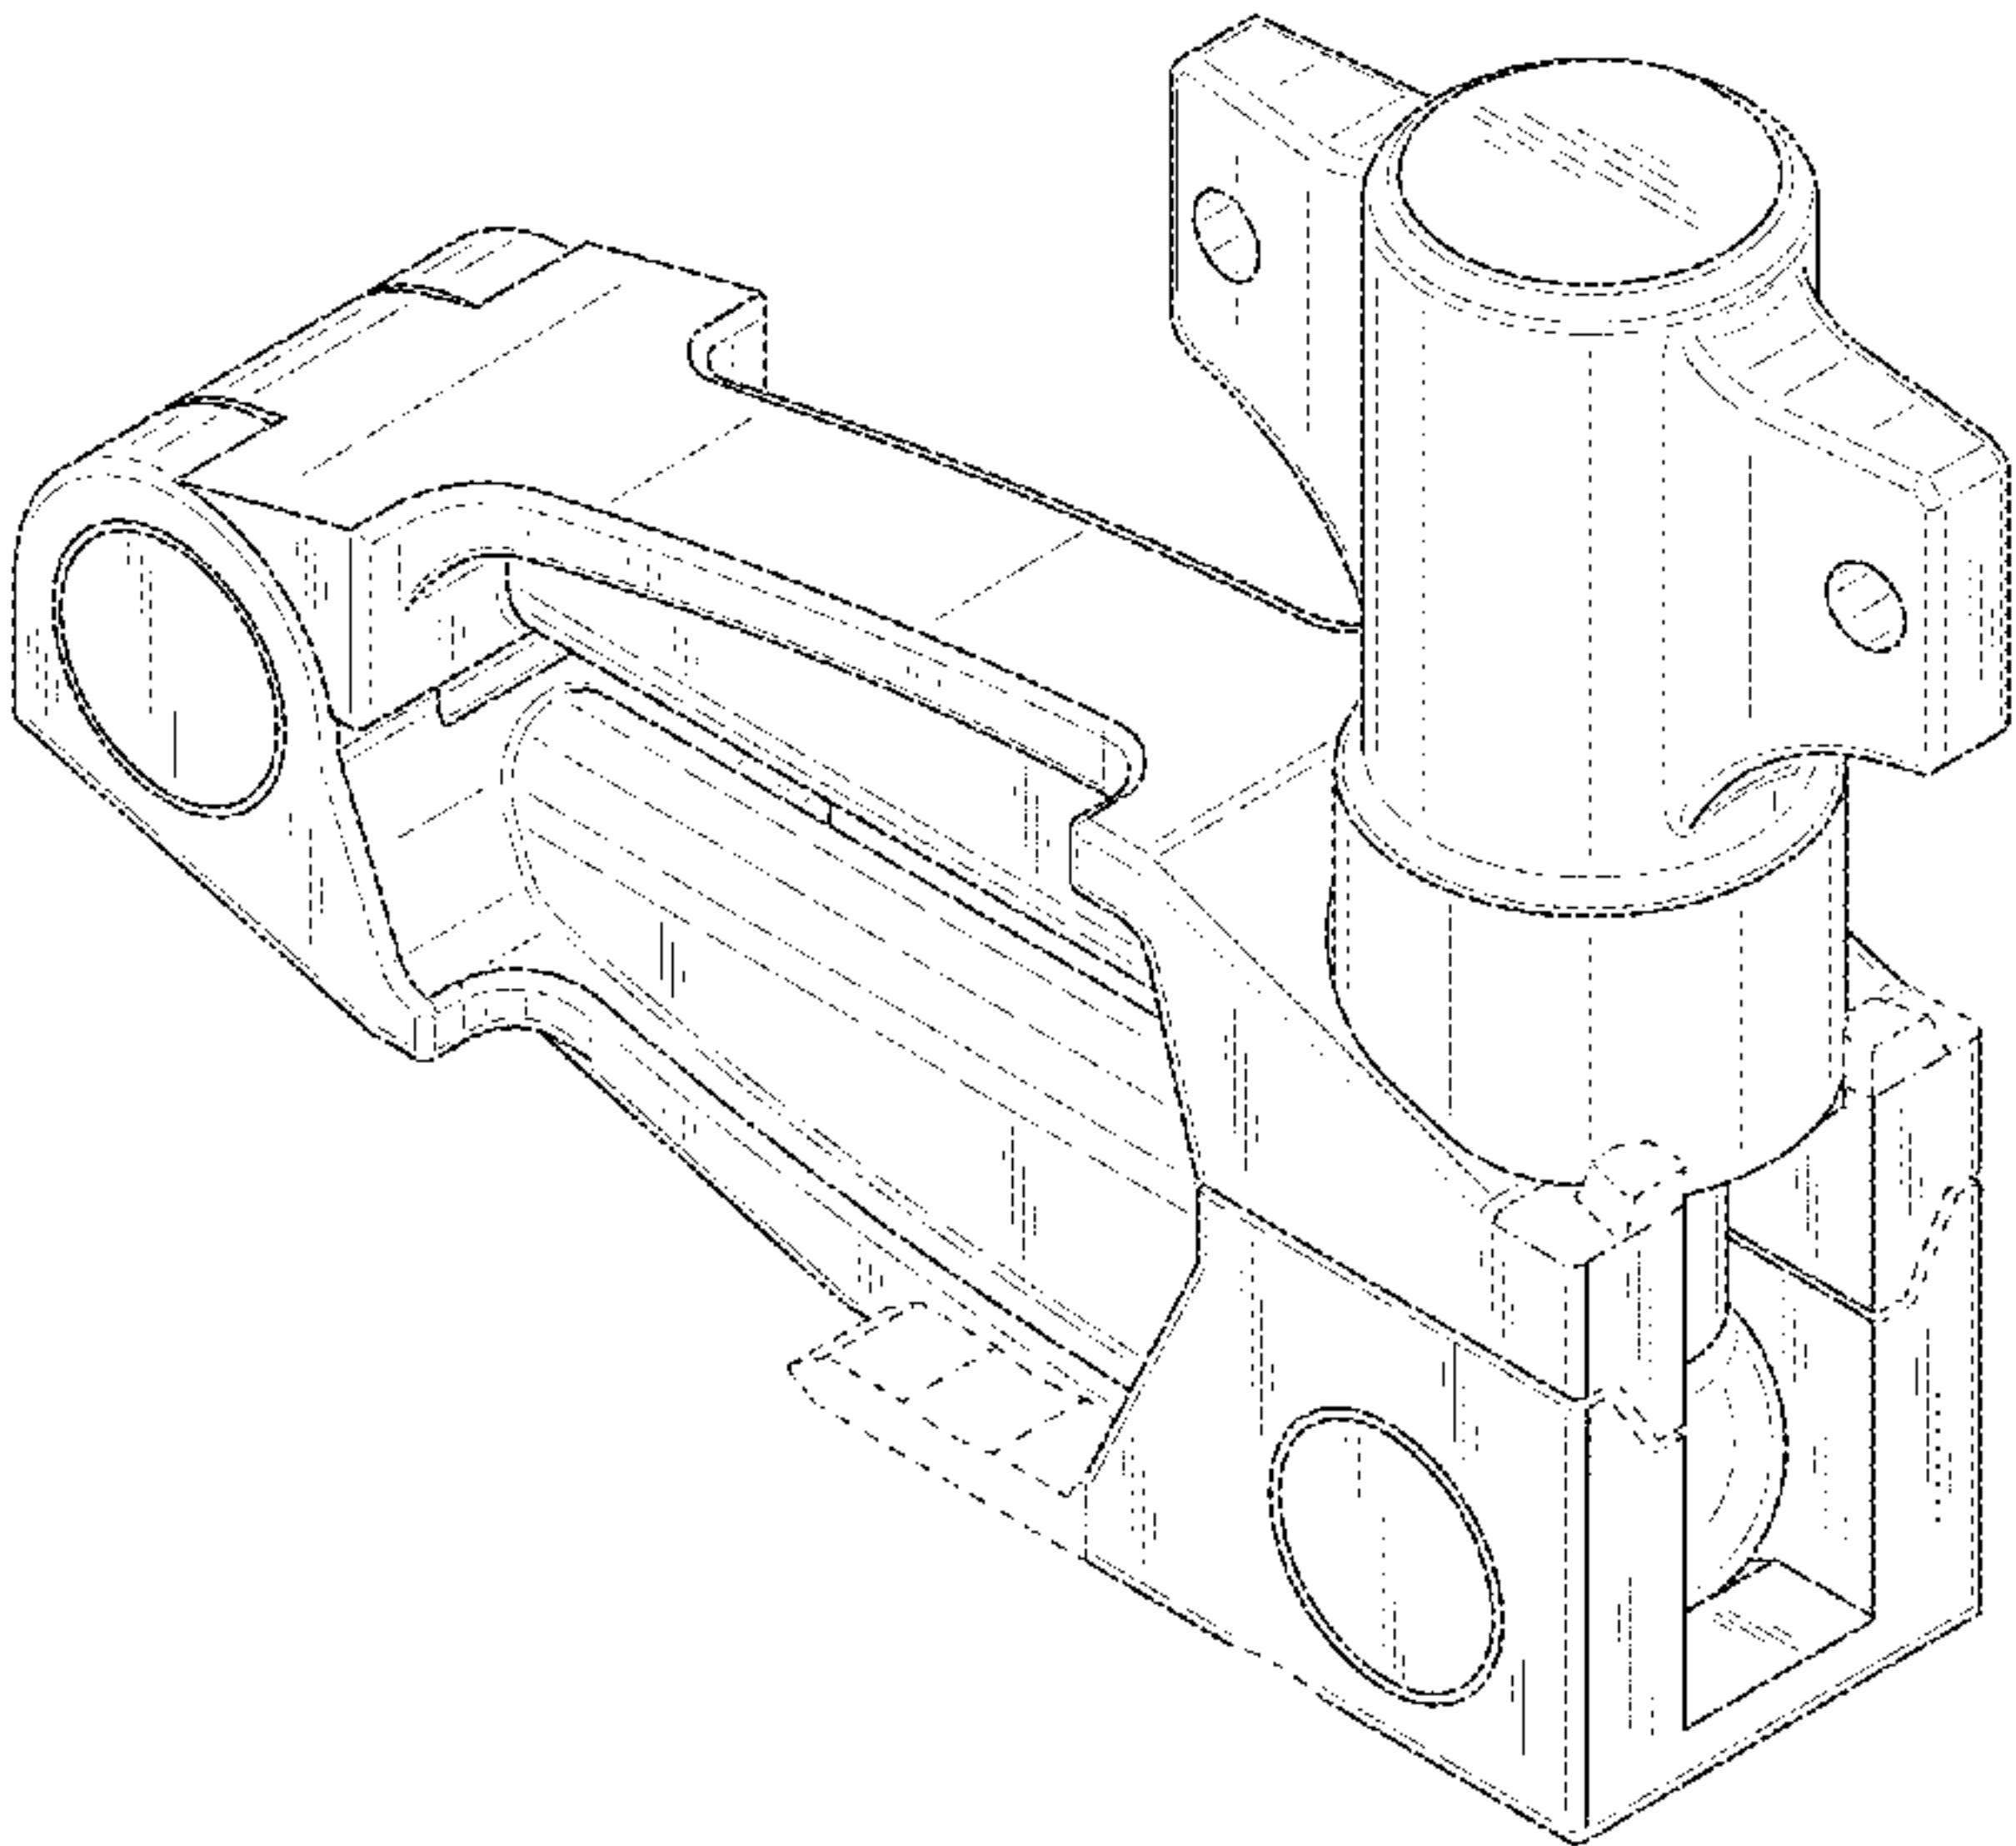

(56)

References Cited

U.S. PATENT DOCUMENTS

8,262,639	B2	9/2012	Mathias et al.	
8,328,457	B2	12/2012	Werth	
8,662,542	B2	3/2014	Werth	
8,888,398	B2	11/2014	Werth	
9,151,420	B2	10/2015	Mckiernan	
9,605,782	B2	3/2017	Werth	
9,677,674	B2	6/2017	Spink et al.	
9,879,813	B2	1/2018	Meola et al.	
D833,265	S	11/2018	Meola et al.	
D846,739	S *	4/2019	Baumer	D24/143
10,384,049	B2	8/2019	Stanton et al.	
10,556,301	B2	2/2020	Baker et al.	
D975,277	S *	1/2023	Miles	D24/143
2002/0169423	A1	11/2002	Zoltan et al.	
2006/0071187	A1 *	4/2006	Aulicino	A61M 39/284 251/4
2011/0163533	A1	7/2011	Snyder et al.	
2022/0128157	A1 *	4/2022	Nisler	F16K 7/061
2022/0390023	A1 *	12/2022	Borchert	A61M 39/283

OTHER PUBLICATIONS

Hose Pinch Clamp for Single Use, TBL Plastics, Nov. 14, 2023, <https://tblplastics.com/fittings/tubing-hose-clamp-bio-ease-hd/> (Year: 2023).*

Avantor Masterflex, Fisher Scientific, Nov. 14, 2023, <https://www.fishersci.com/shop/products/heavy-duty-tub-hose-closure-ea/NC0364471> (Year: 2023).*

* cited by examiner

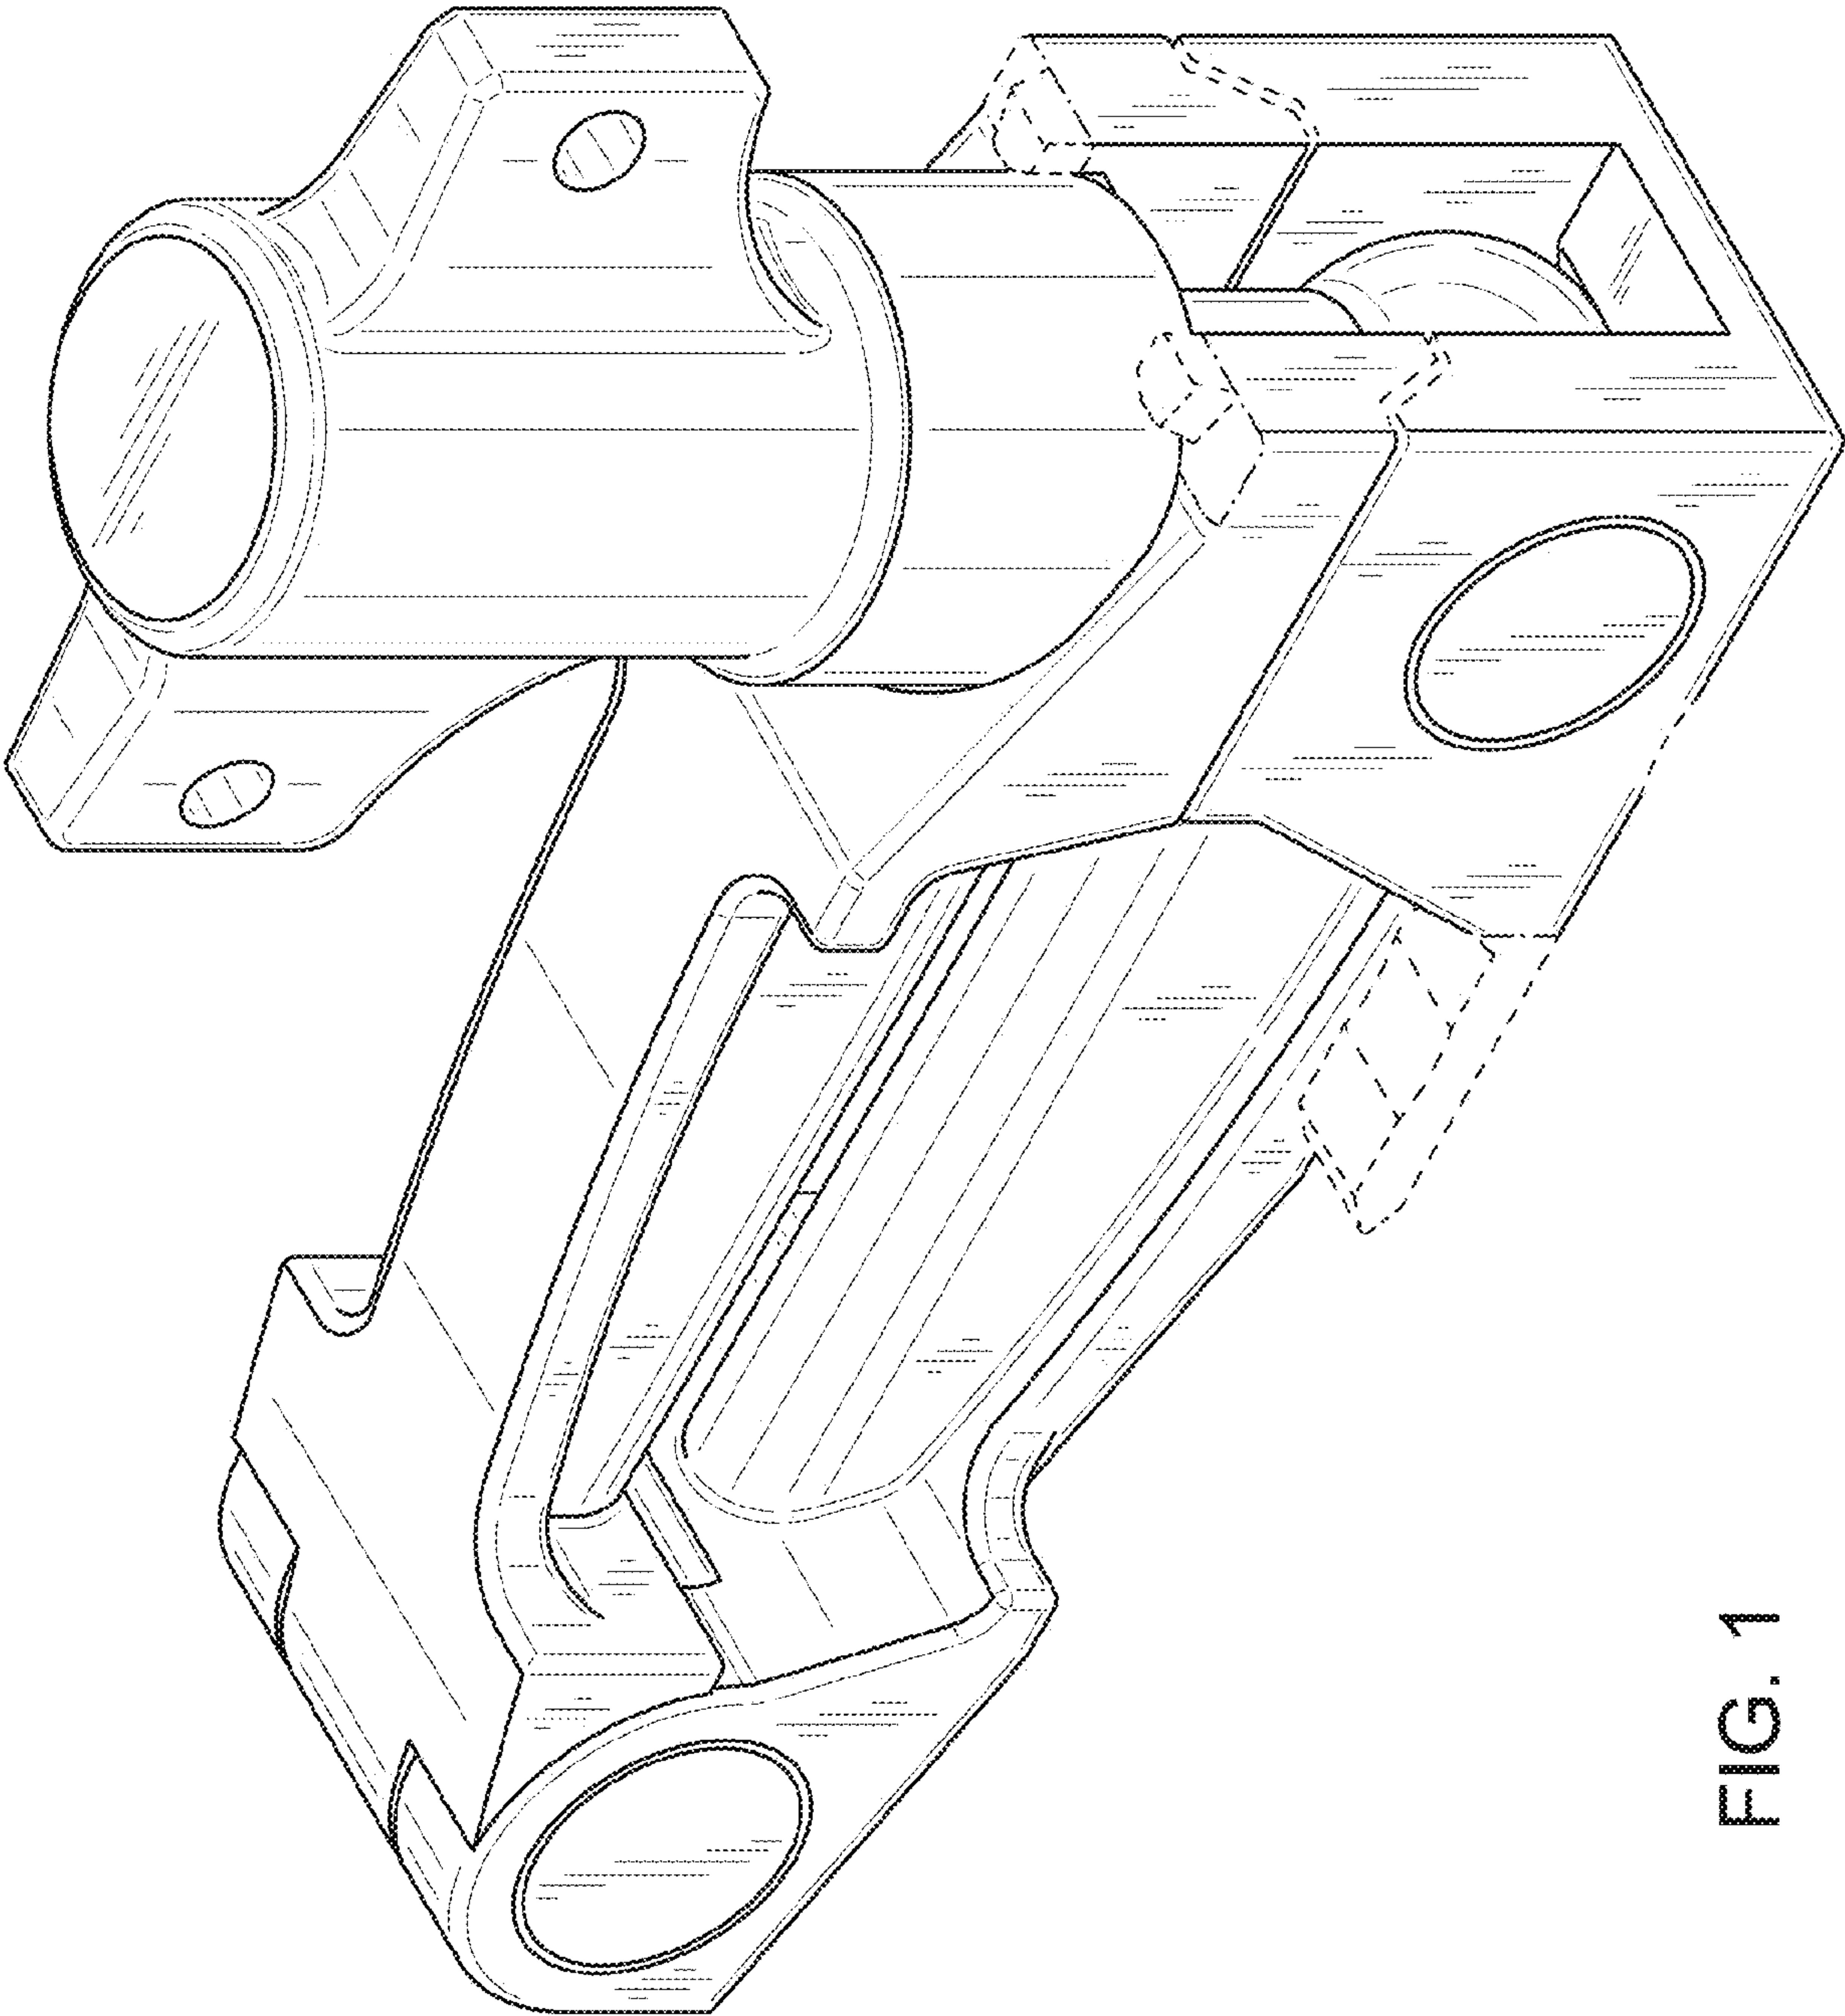


FIG. 1

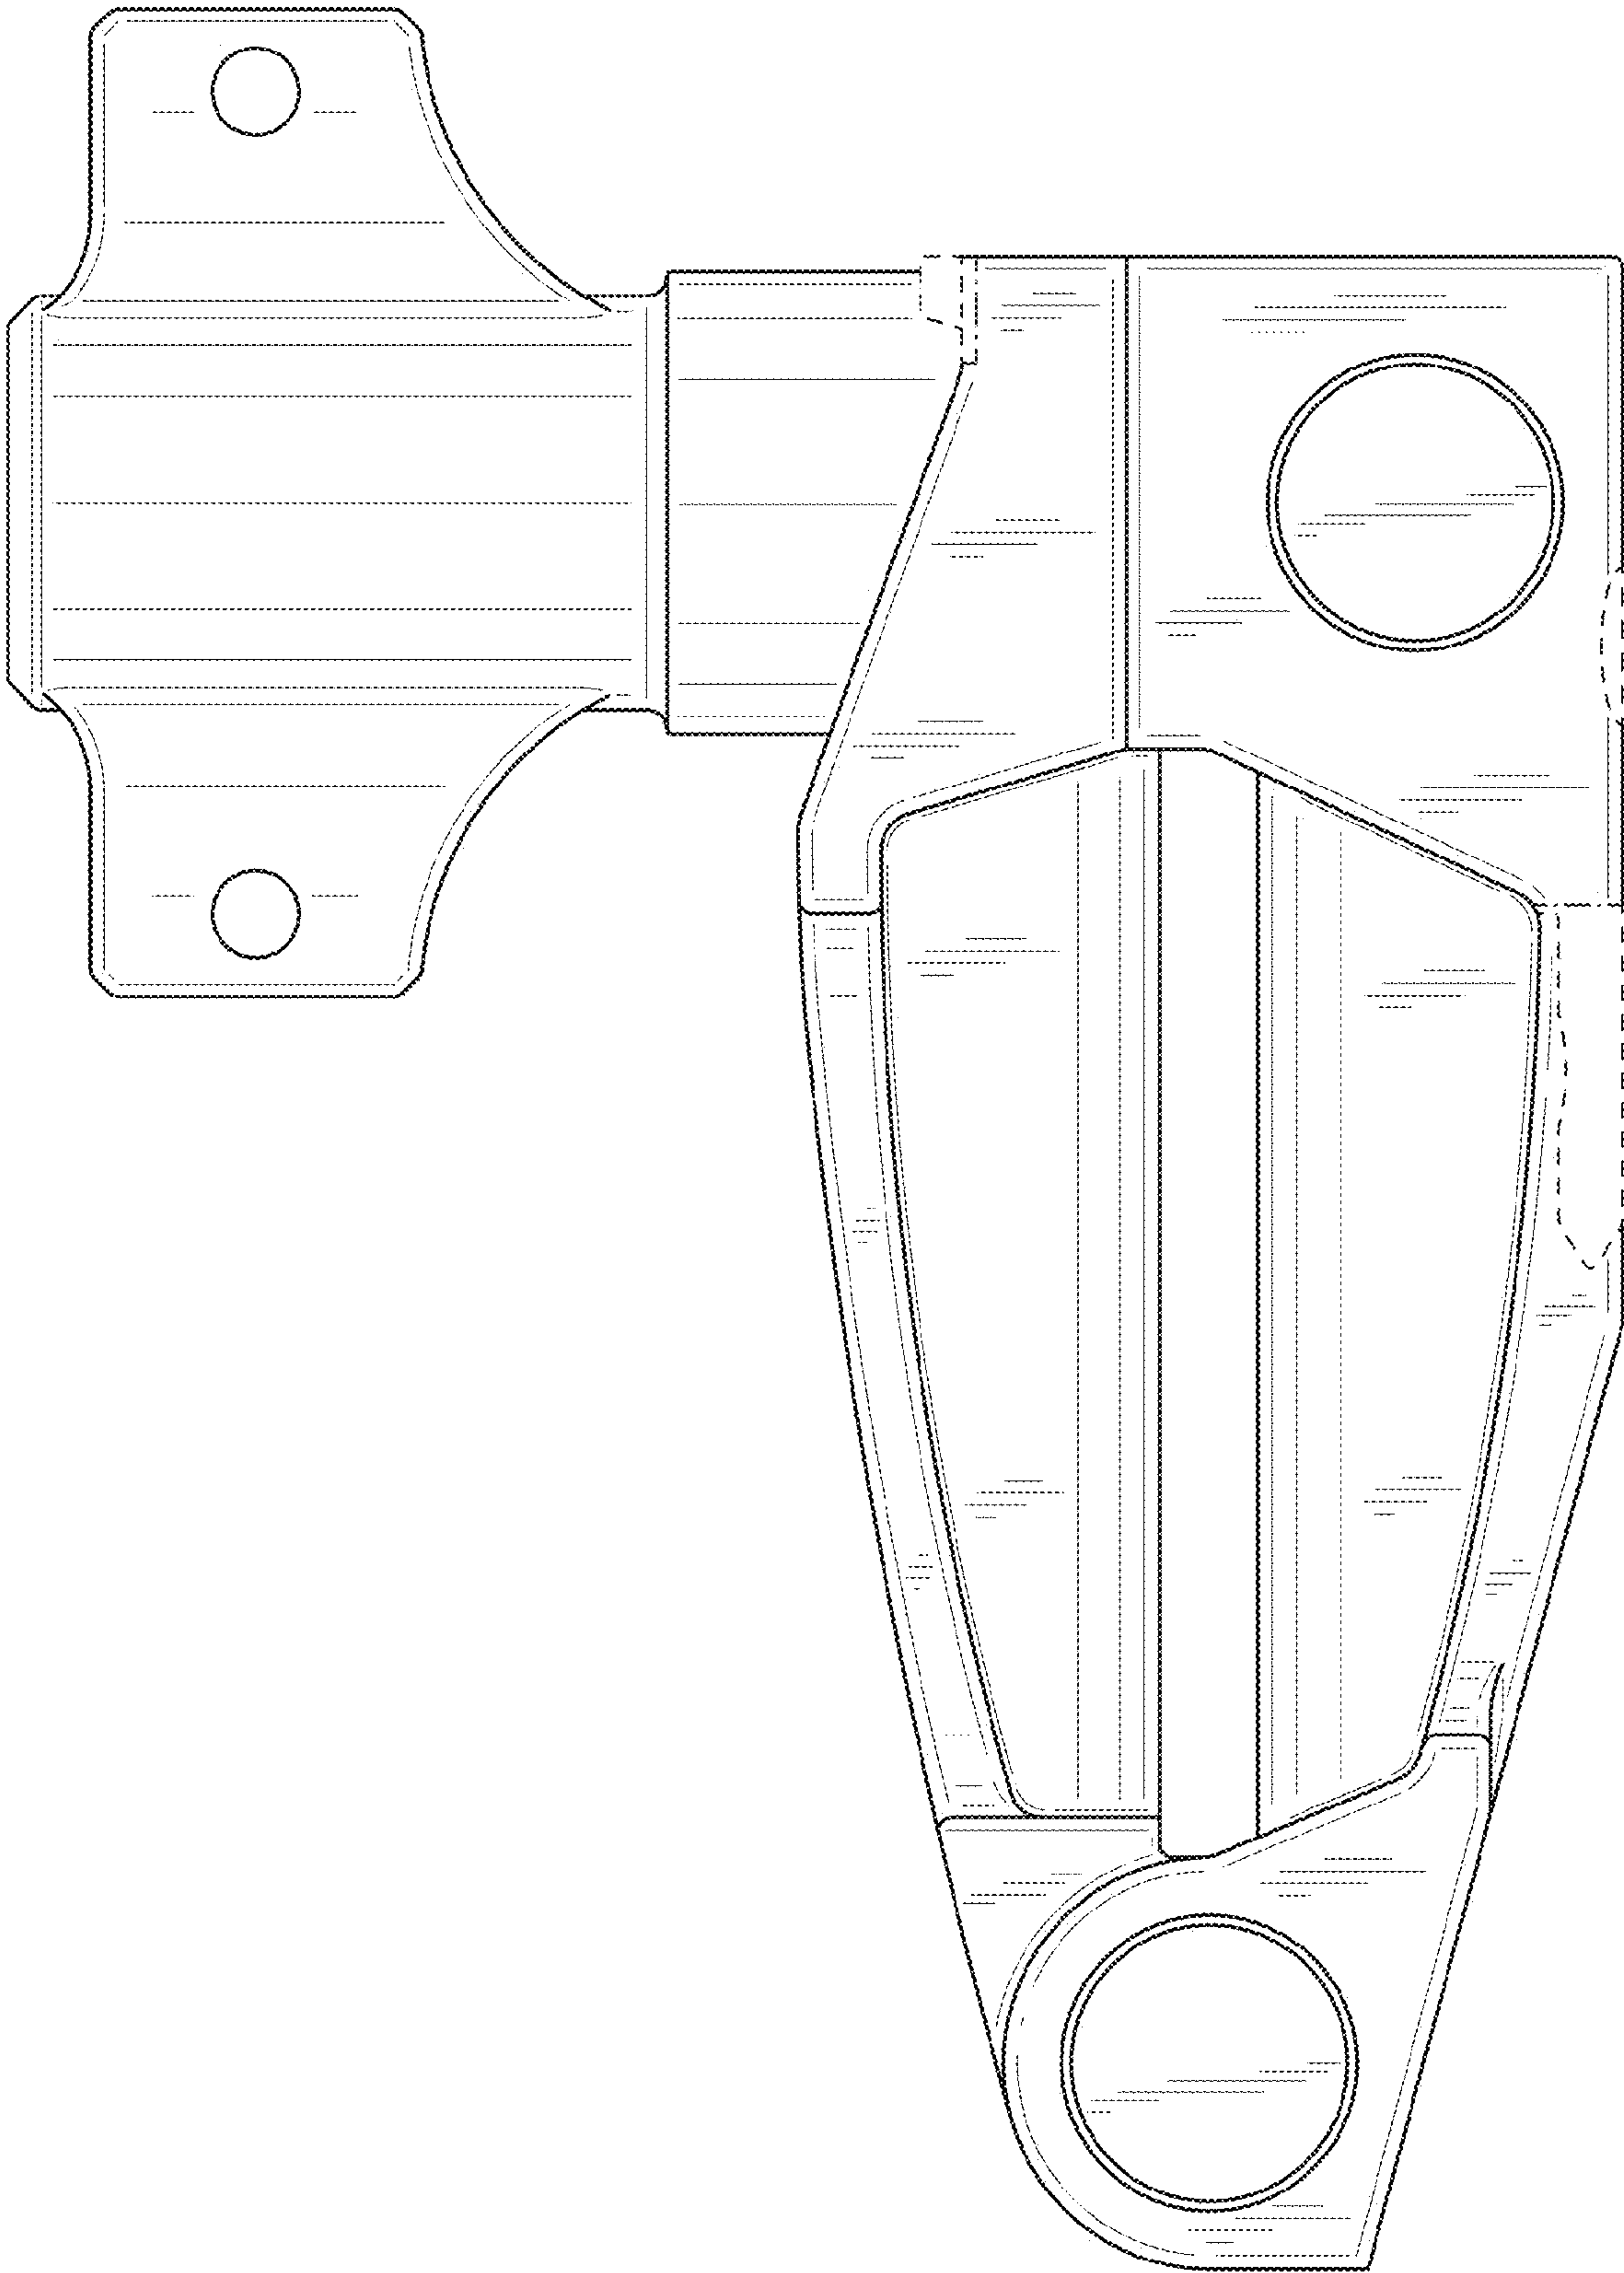


FIG. 2

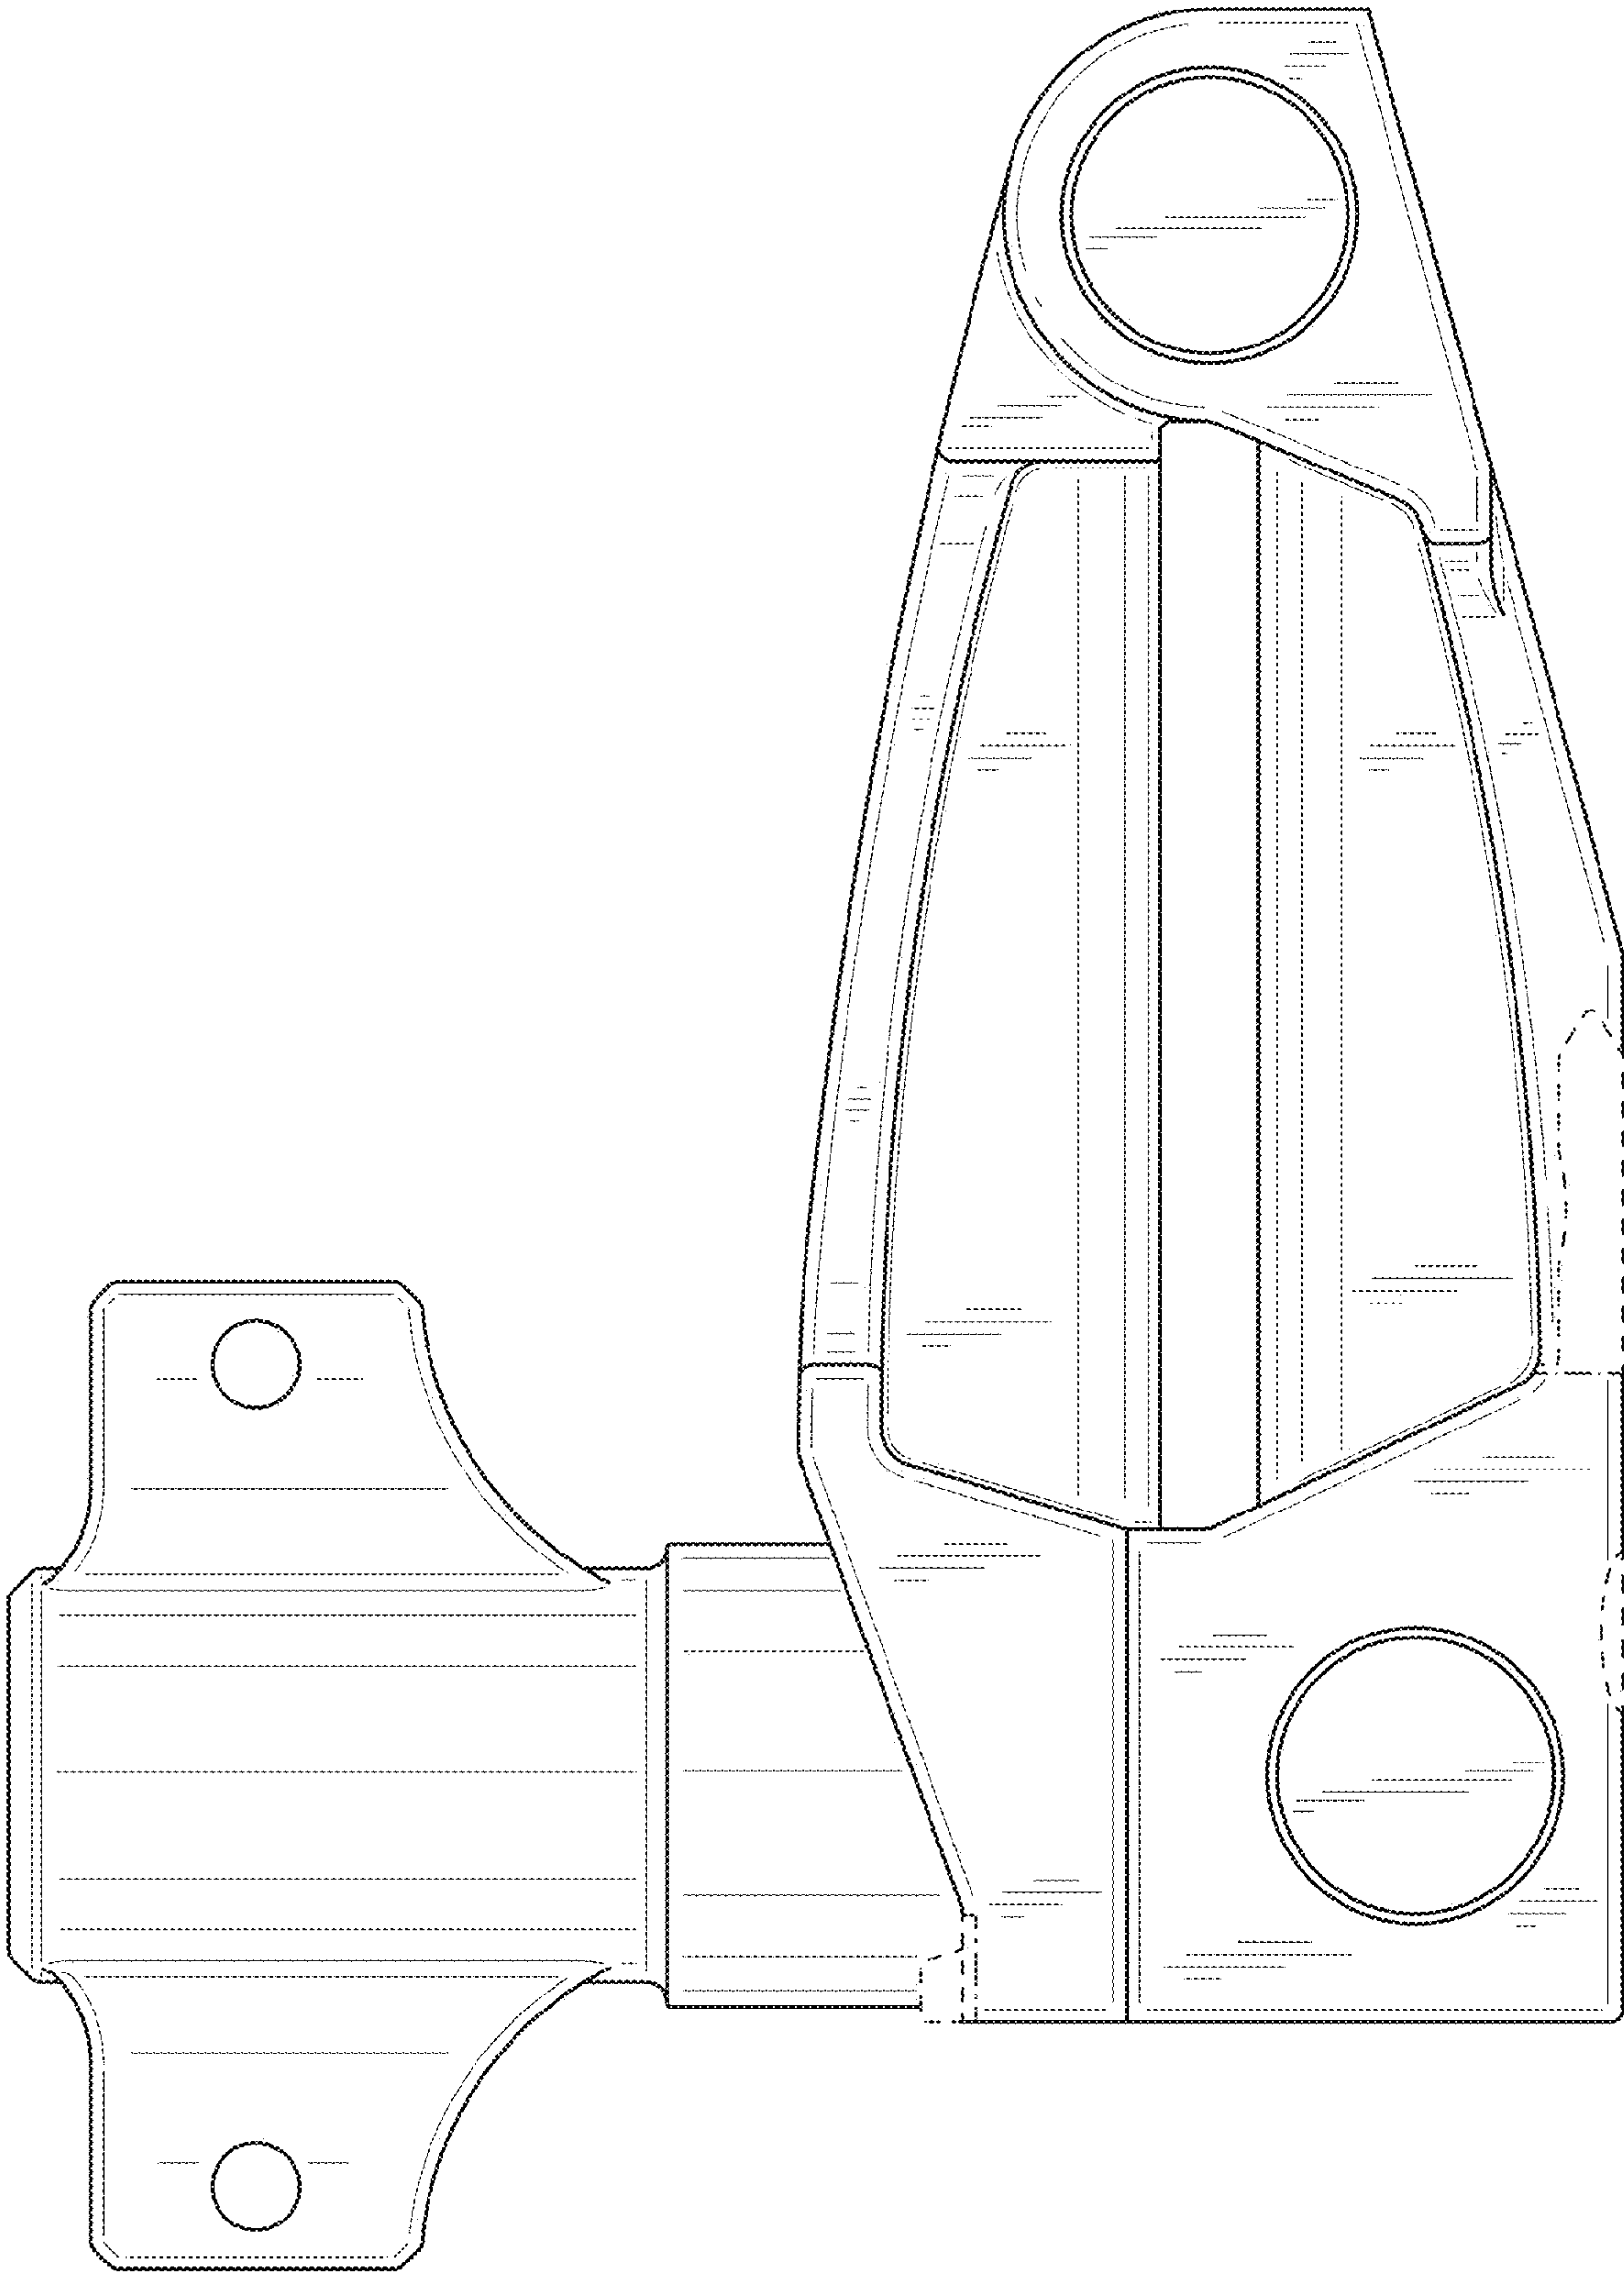


FIG. 3

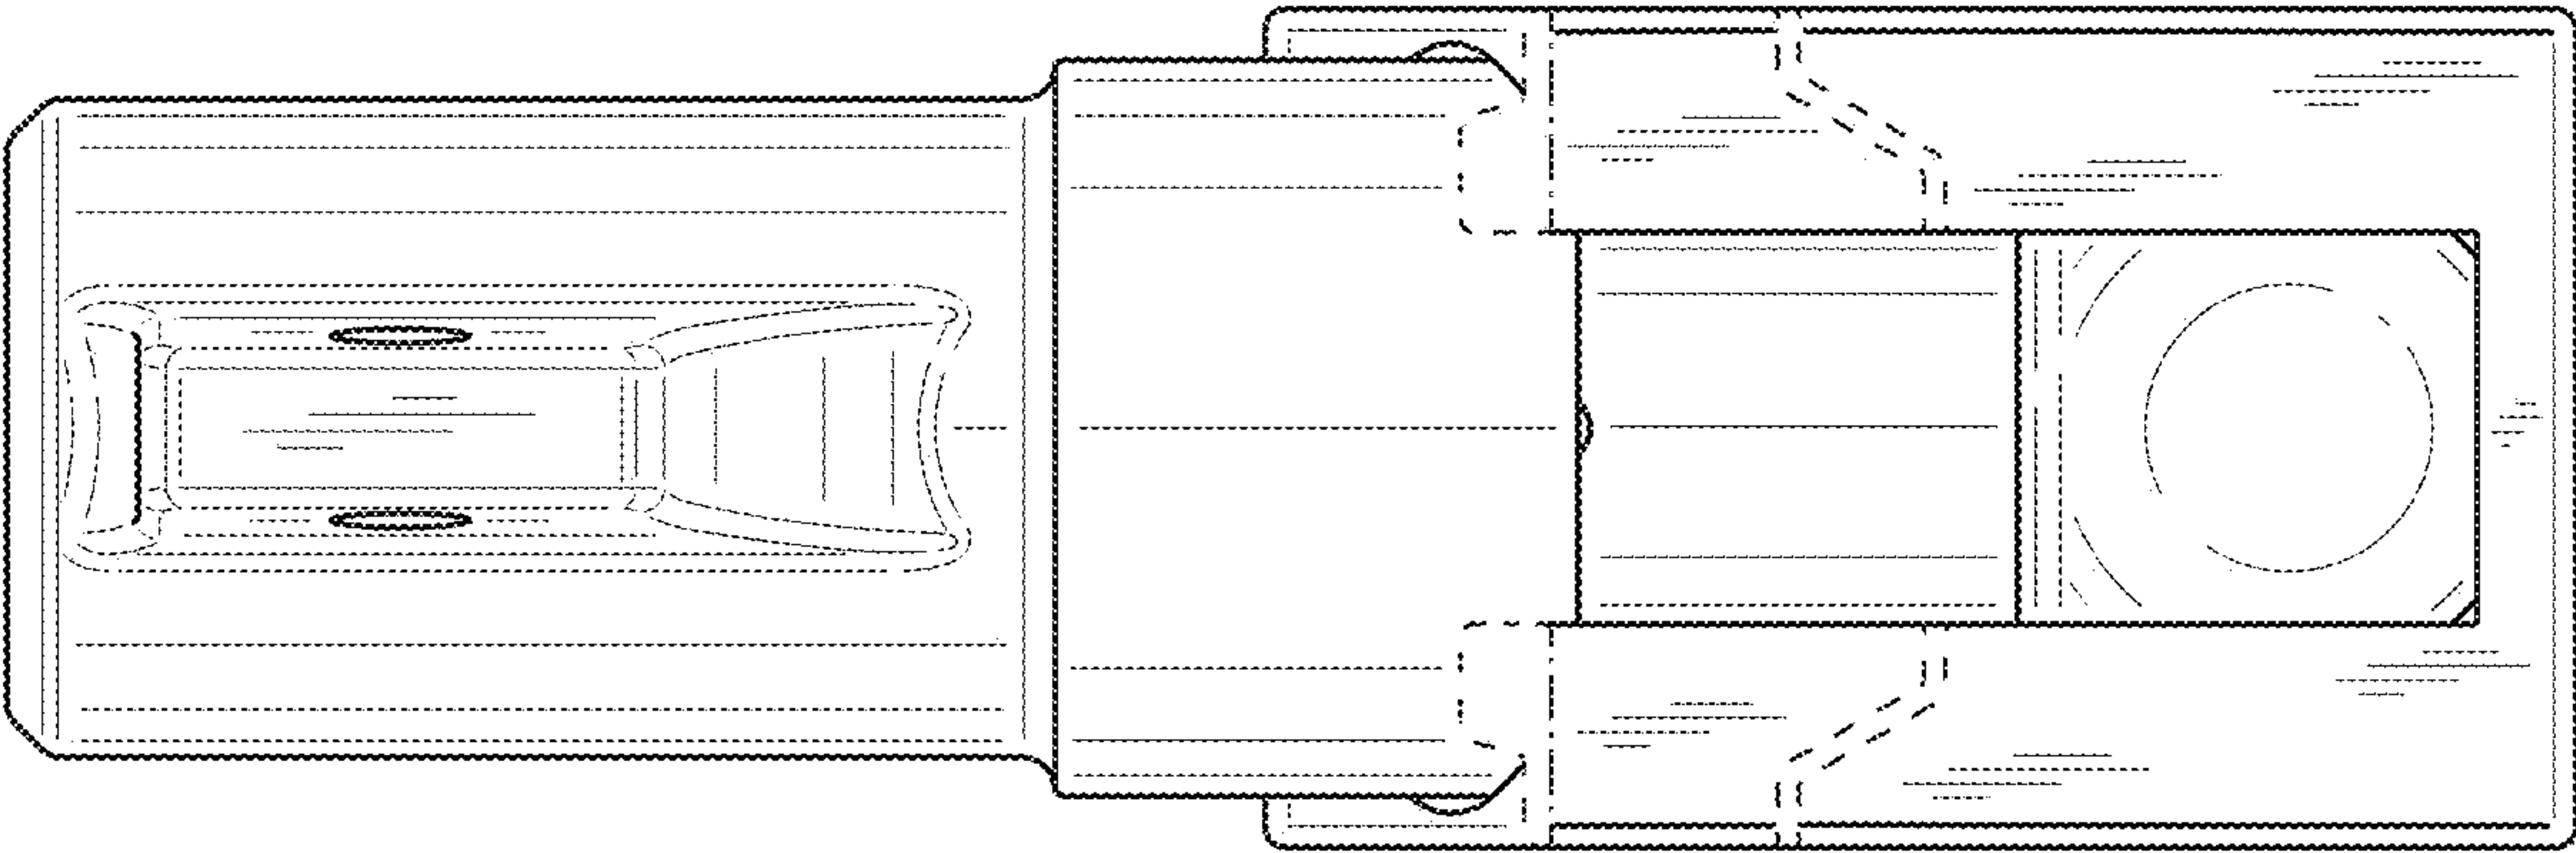


FIG. 4

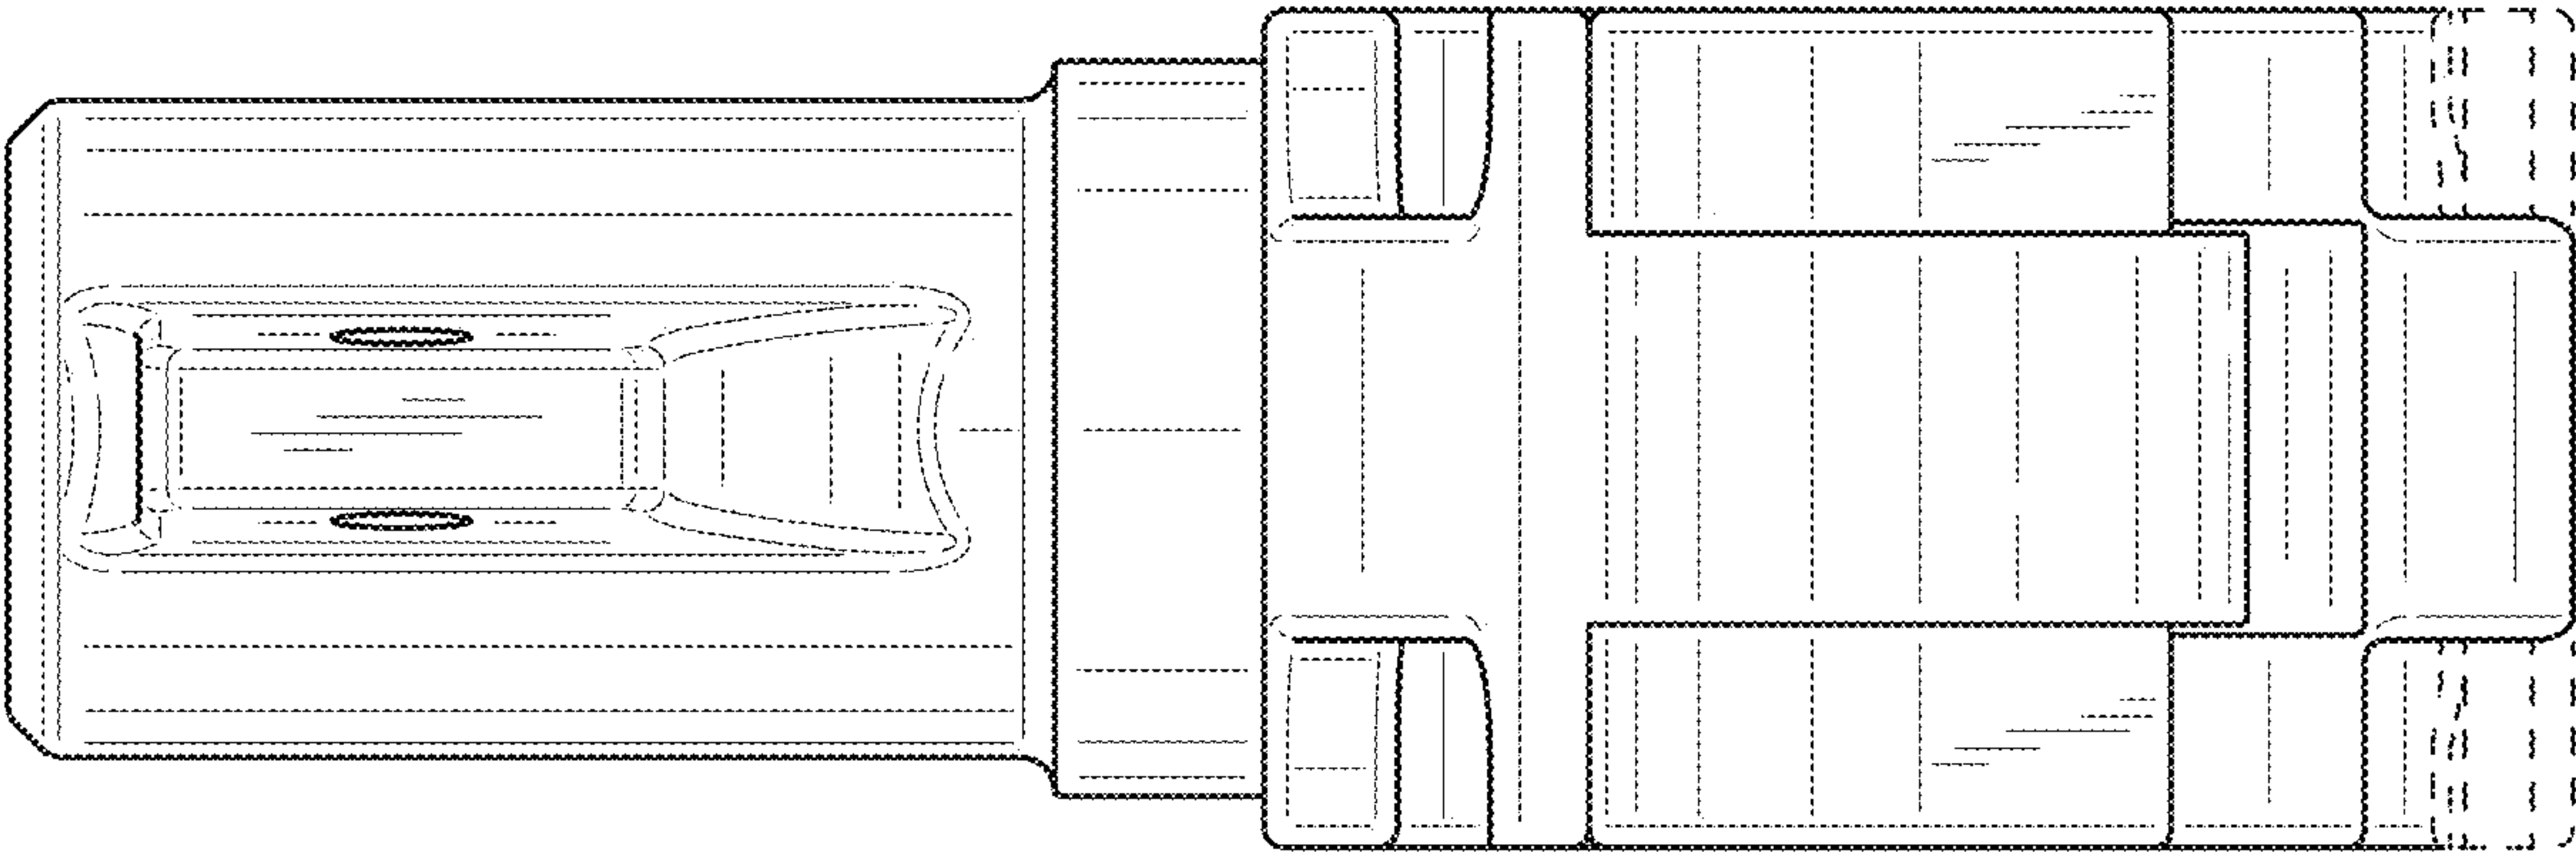


FIG. 5

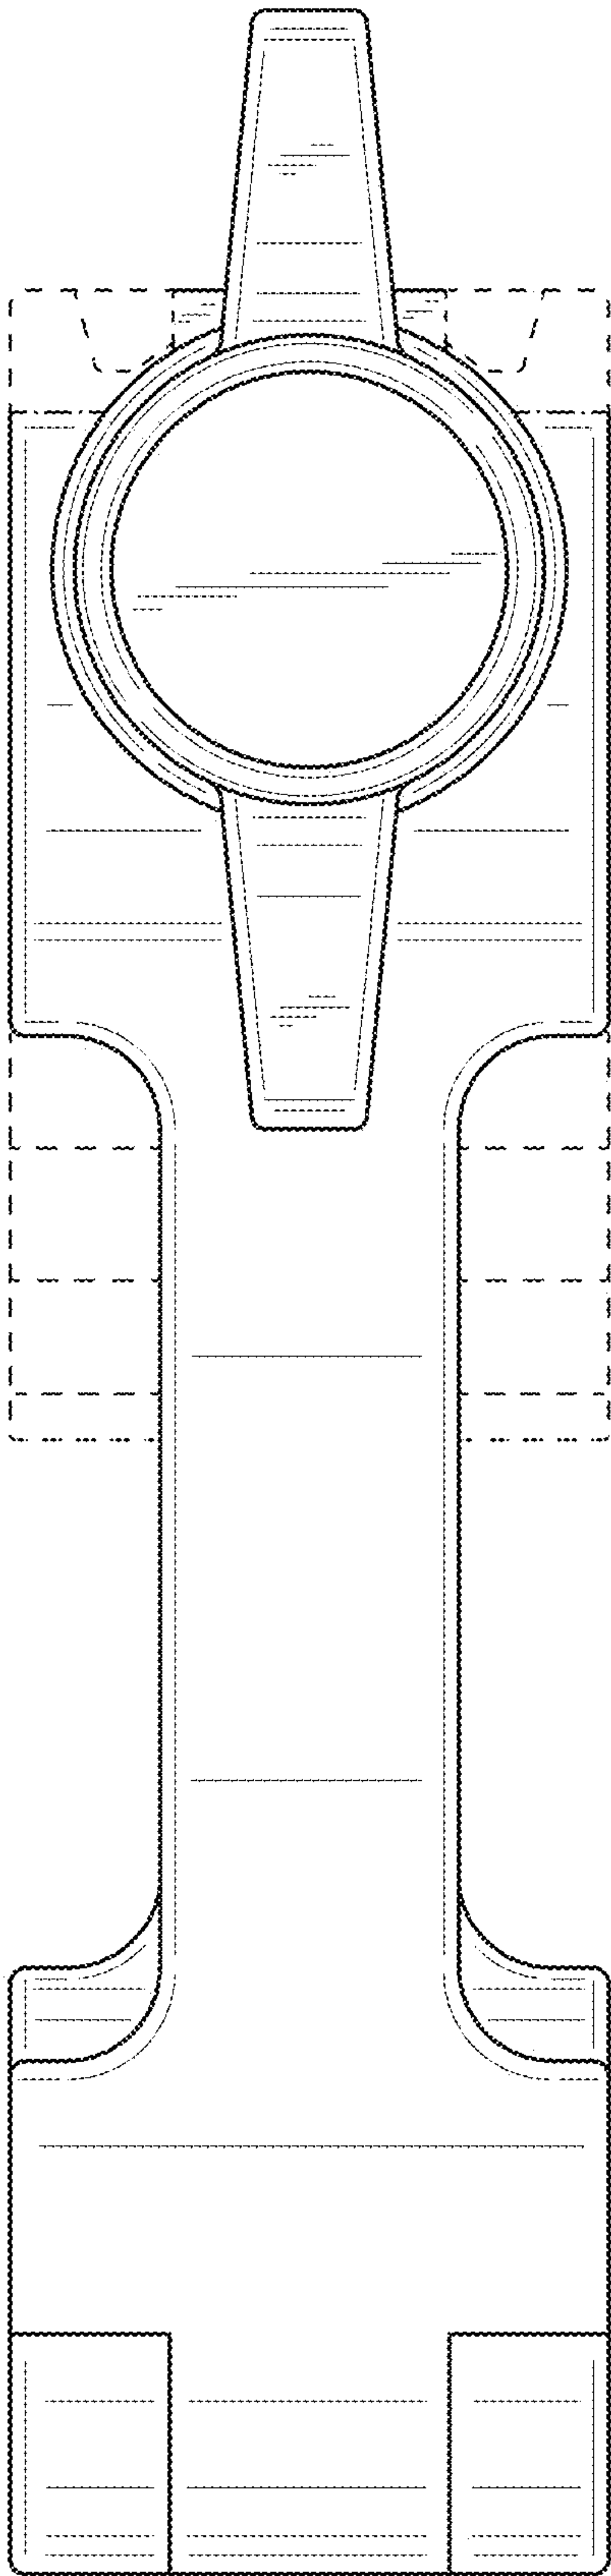


FIG. 6

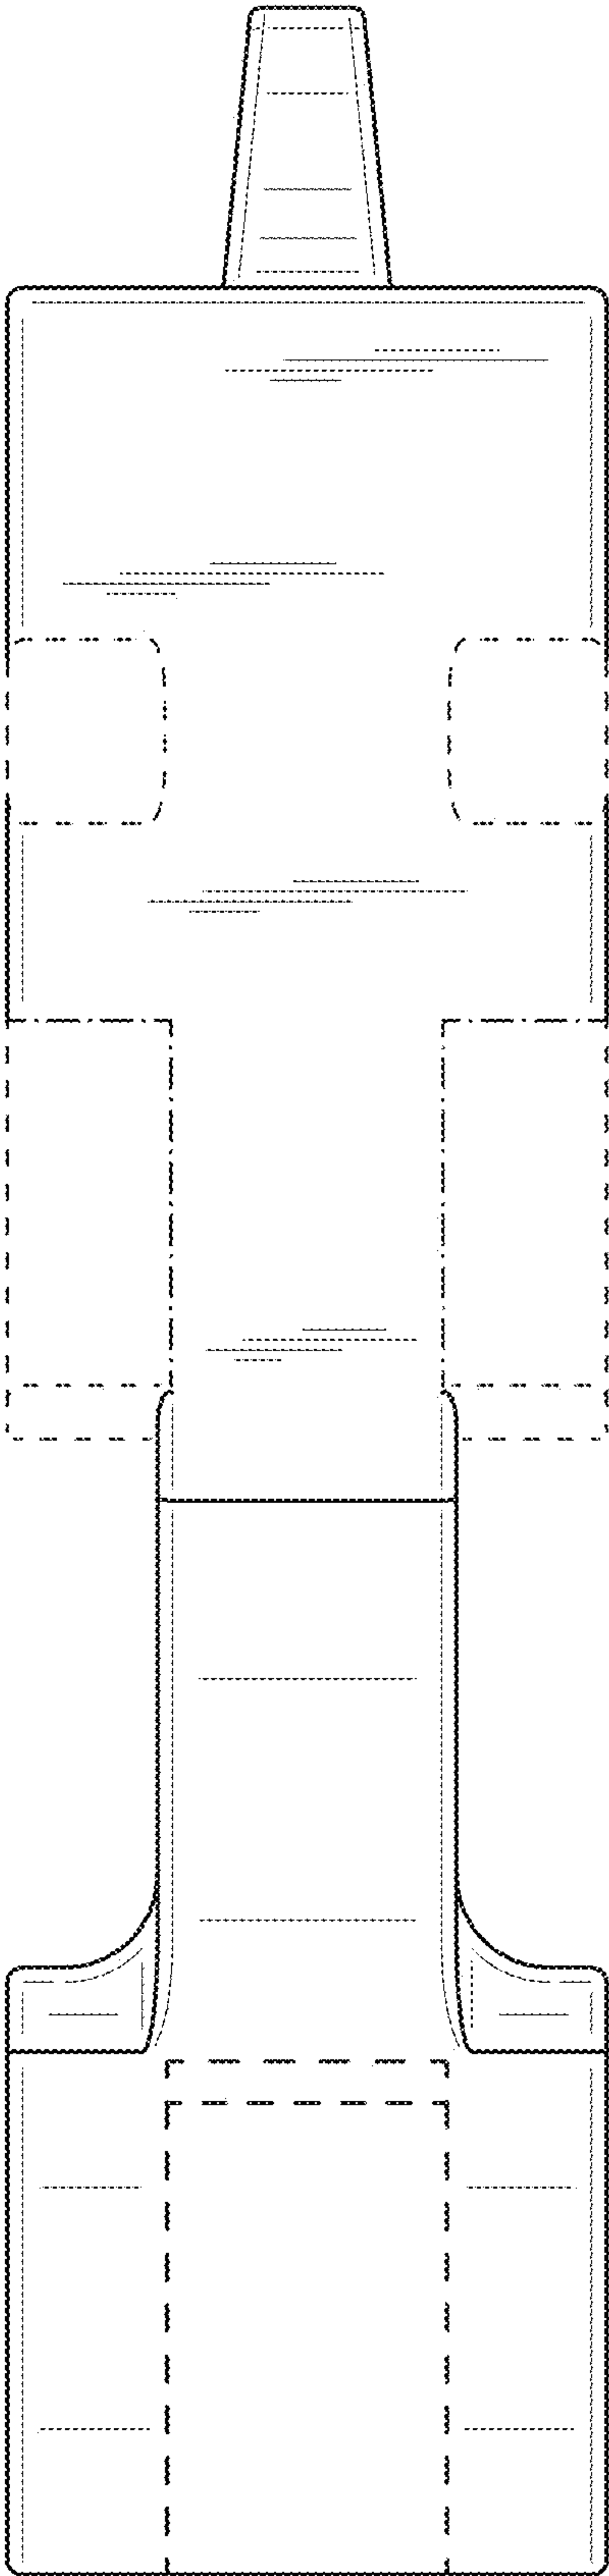


FIG. 7