

(12)

United States Design Patent

DeLorenzo et al.

(10)

Patent No.:

US D1,028,246 S

(45)

Date of Patent:

** May 21, 2024

(54)

HUB FOR A MEDICAL DEVICE

D837,368 S * 1/2019 Burkholz A61M 25/0097 D24/129

(71)

Applicant: ABIOMED, Inc., Danvers, MA (US)

D845,843 S 4/2019 Inoue et al.
D846,225 S 4/2019 Johanning et al.

(72)

Inventors: Charles DeLorenzo, Danvers, MA (US); Christopher Nason Korkuch, Beverly, MA (US); Glen R. Fantuzzi, Danvers, MA (US); Brian Chouinard, Danvers, MA (US)

(Continued)

FOREIGN PATENT DOCUMENTS

CA 207620 * 2/2022
CN 304033462 2/2017
(Continued)

(73) Assignee: Abiomed, Inc., Danvers, MA (US)

(**) Term: 15 Years

(21) Appl. No.: 29/813,975

(22) Filed: Nov. 2, 2021

(51) LOC (14) Cl. 24-02

(52) U.S. Cl.
USPC D24/129; D24/167

(58) Field of Classification Search
USPC D24/112, 127–129, 164, 166, 167, 169, D24/170, 184, 186, 216, 231
CPC A61M 25/0043; A61M 25/009; A61M 25/06; A61M 2025/0681; A61M 39/0693; A61M 2039/1033; A61M 2039/1066; A61M 39/10; A61M 39/12
See application file for complete search history.

(56) References Cited

U.S. PATENT DOCUMENTS

D345,419 S 3/1994 Horrigan et al.
D456,513 S * 4/2002 Crawford D24/169
D490,894 S 6/2004 Bogazzi
D490,896 S 6/2004 Bogazzi
D625,409 S * 10/2010 Chesnin D24/129
D634,156 S 3/2011 Fuller et al.
D634,424 S 3/2011 Morejon
D663,030 S 7/2012 Muerner et al.
D713,522 S * 9/2014 Woehr D24/112
D715,126 S 10/2014 Kim et al.
D715,955 S 10/2014 Hsu

OTHER PUBLICATIONS

Cook Medical G46168, posted date unavailable [retrieved online Dec. 4, 2023]. Retrieved from internet, <https://www.ciamedical.com/cook-medical-g46168-each-sheath-flexor-ureteral-access-12f-45cm> (Year: 2023).*

(Continued)

Primary Examiner — Lilyana Bekic
Assistant Examiner — Samantha K Pollack
(74) Attorney, Agent, or Firm — Botos Churchill IP Law LLP


(57) CLAIM

The ornamental design for a hub for a medical device, as shown and described.

DESCRIPTION

FIG. 1 is a top, front, right side perspective view of a hub for a medical device according to our new design;
FIG. 2 is a front elevation view thereof;
FIG. 3 is a rear elevation view thereof;
FIG. 4 is a left side elevation view thereof;
FIG. 5 is a right side elevation view thereof;
FIG. 6 is a top plan view thereof; and,
FIG. 7 is a bottom plan view thereof.
The broken lines illustrate portions of the hub for a medical device that form no part of the claimed design.

1 Claim, 7 Drawing Sheets

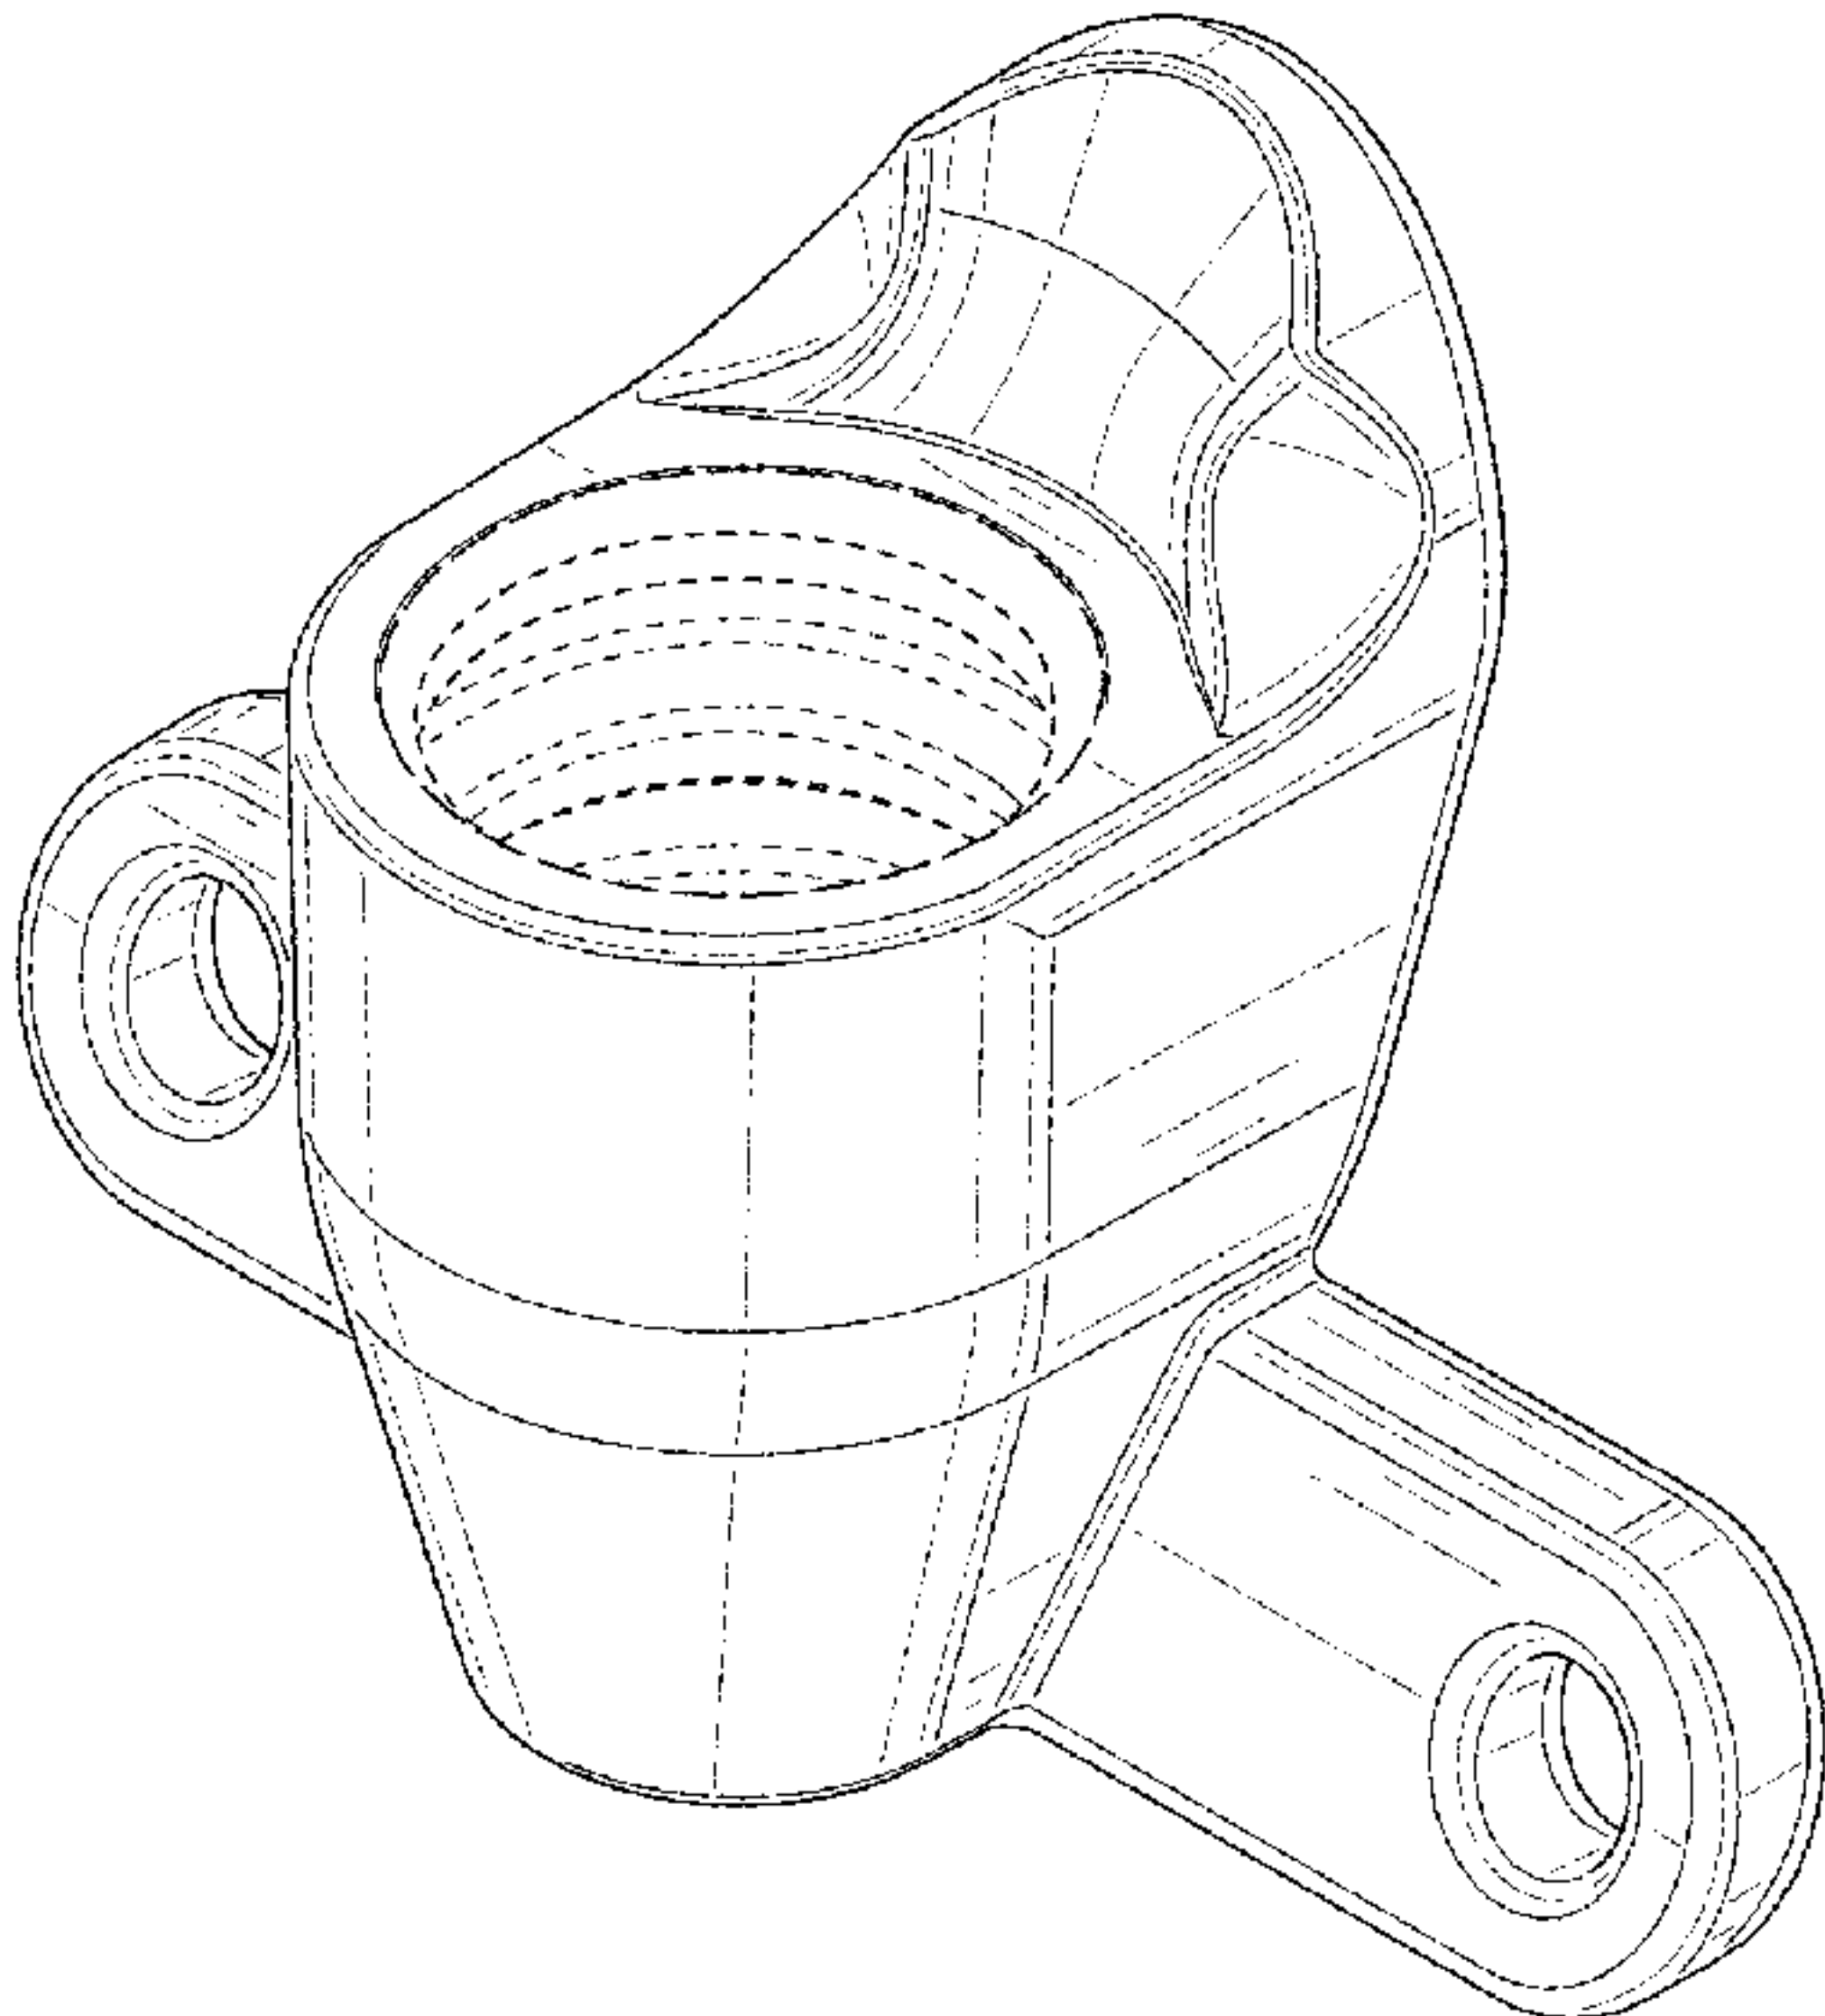

(56)

References Cited

U.S. PATENT DOCUMENTS

10,441,771 B2 * 10/2019 Bickhart A61M 39/0606
D870,883 S * 12/2019 Harding D24/130
D879,290 S 3/2020 Harman et al.
D887,993 S 6/2020 Decastro et al.
10,709,875 B2 7/2020 O’Carrol et al.
D900,308 S * 10/2020 Burkholz D24/129
D914,477 S 3/2021 Watson
D922,562 S 6/2021 Hulford et al.
D931,456 S 9/2021 Schumaier et al.
D940,889 S 1/2022 Hocking
D949,417 S 4/2022 Khubani et al.
D949,418 S 4/2022 Khubani et al.
D956,966 S * 7/2022 Suarez del Real Pena . D24/129
D975,866 S 1/2023 Marton et al.
2016/0220795 A1 * 8/2016 Korkuch A61M 25/008
2020/0016392 A1 * 1/2020 Kim B25B 27/14
2021/0220633 A1 * 7/2021 Feith A61M 39/14
2023/0134876 A1 * 5/2023 DeLorenzo A61M 25/0043
604/93.01
2023/0310827 A1 * 10/2023 Dong A61M 39/10
285/399
2023/0364393 A1 * 11/2023 Rajaram A61M 25/0023

FOREIGN PATENT DOCUMENTS

CN 306163859 11/2020
CN 307363432 * 5/2022
GB 6205119 * 4/2022

JP D13176290 12/2007
JP 1633708 S 6/2019
JP 1659556 S 5/2020
JP D1664821 * 7/2020
JP 1671048 S 10/2020
NZ 430704-0001 * 7/2023
TW D192842 9/2018
TW D199557 9/2019

OTHER PUBLICATIONS

Single-Access Technique for Impella-Assisted High-Risk PCI, posted Mar. 2020, [retrieved online Dec. 4, 2023]. Retrieved from internet, <https://citoday.com/articles/2020-mar-apr/single-access-technique-for-impella-assisted-high-risk-pci> (Year: 2020).*

Intensive Care Unit | LA | Teleflex, posted date unavailable. [retrieved online Dec. 4, 2023]. Retrieved from internet, <https://www.teleflex.com/la/en/product-areas/cardiac-care/intensive-care-unit/index.html> (Year: 2023).*

Abiomed’s Impella Low Profile Sheath Granted FDA Clearance, posted Oct. 17, 2022, [retrieved online Dec. 4, 2023], Retrieved from internet, <https://citoday.com/news/abiomed-impella-low-profile-sheath-granted-fda-clearance> (Year: 2022).*

U.S. FDA Grants 501(k) Clearance for Impella Low Profile Sheath, posted Oct. 17, 2022 [retrieved online Dec. 4, 2023]. Retrieved from internet, <https://www.businesswire.com/news/home/20221017005313/en/U.S.-FDA-Grants-510-k-Clearance-for-Impella-Low-Profile-Sheath> (Year: 2022).*

* cited by examiner

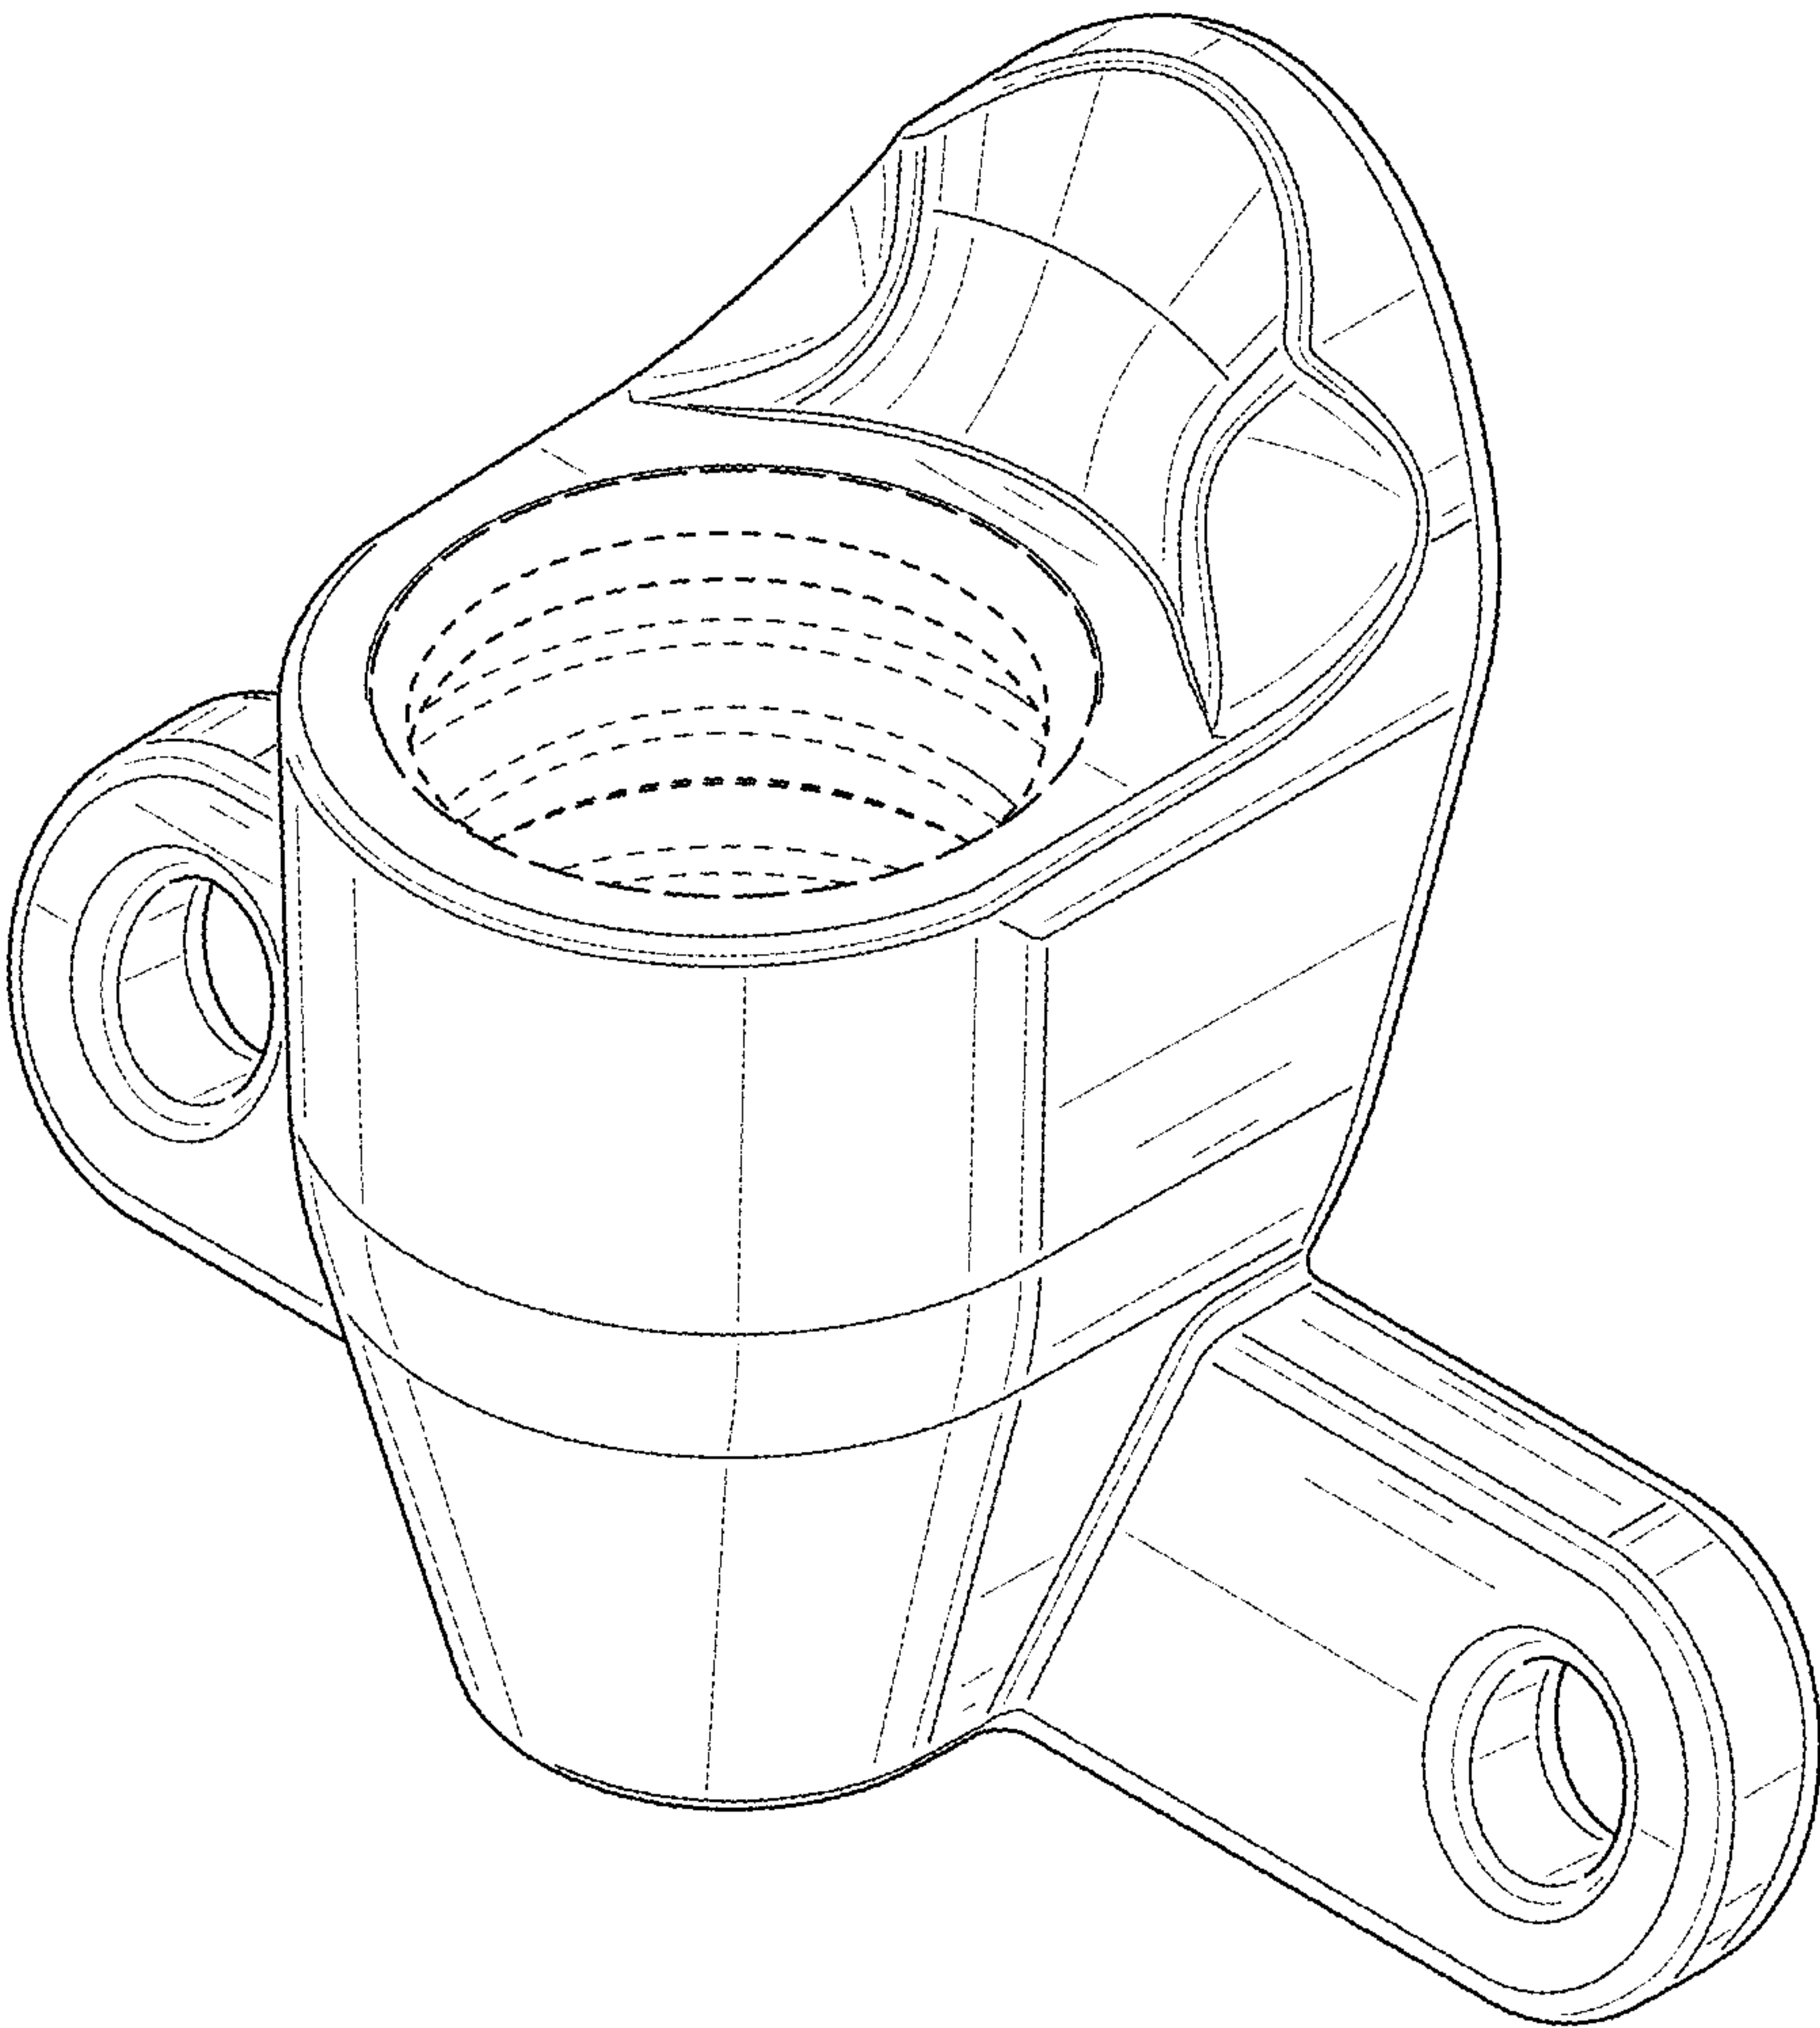


FIG. 1

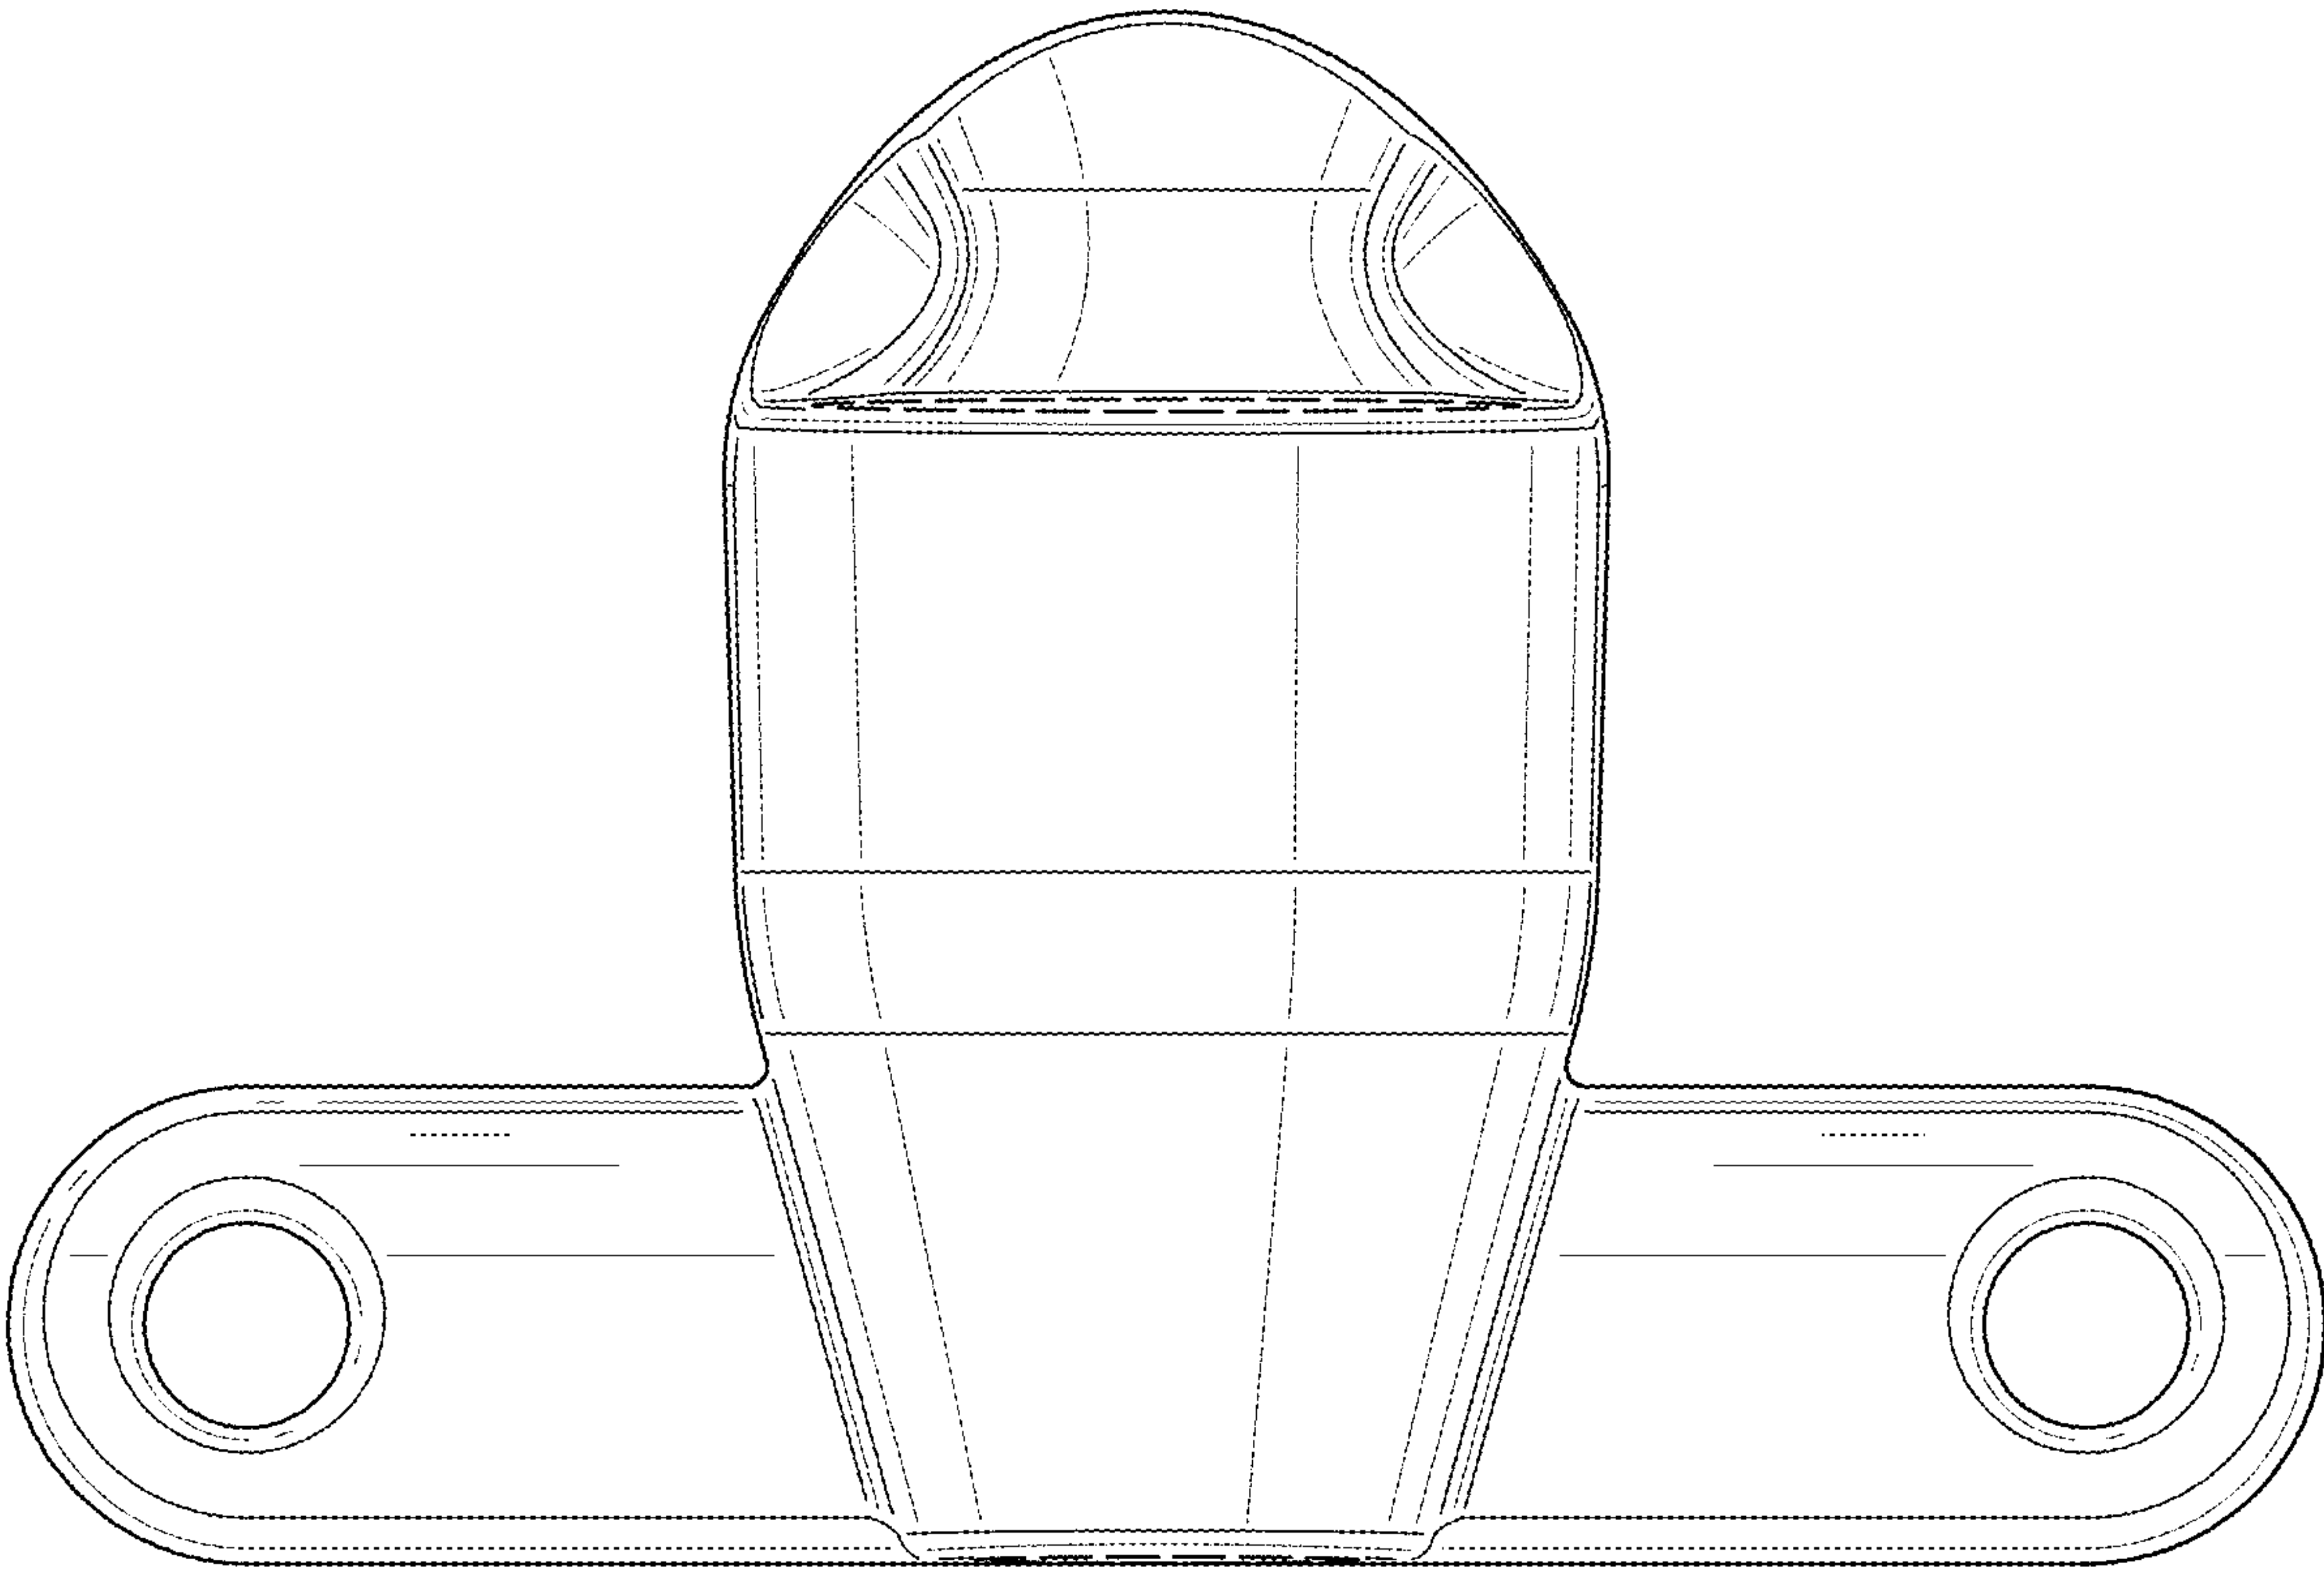


FIG. 2

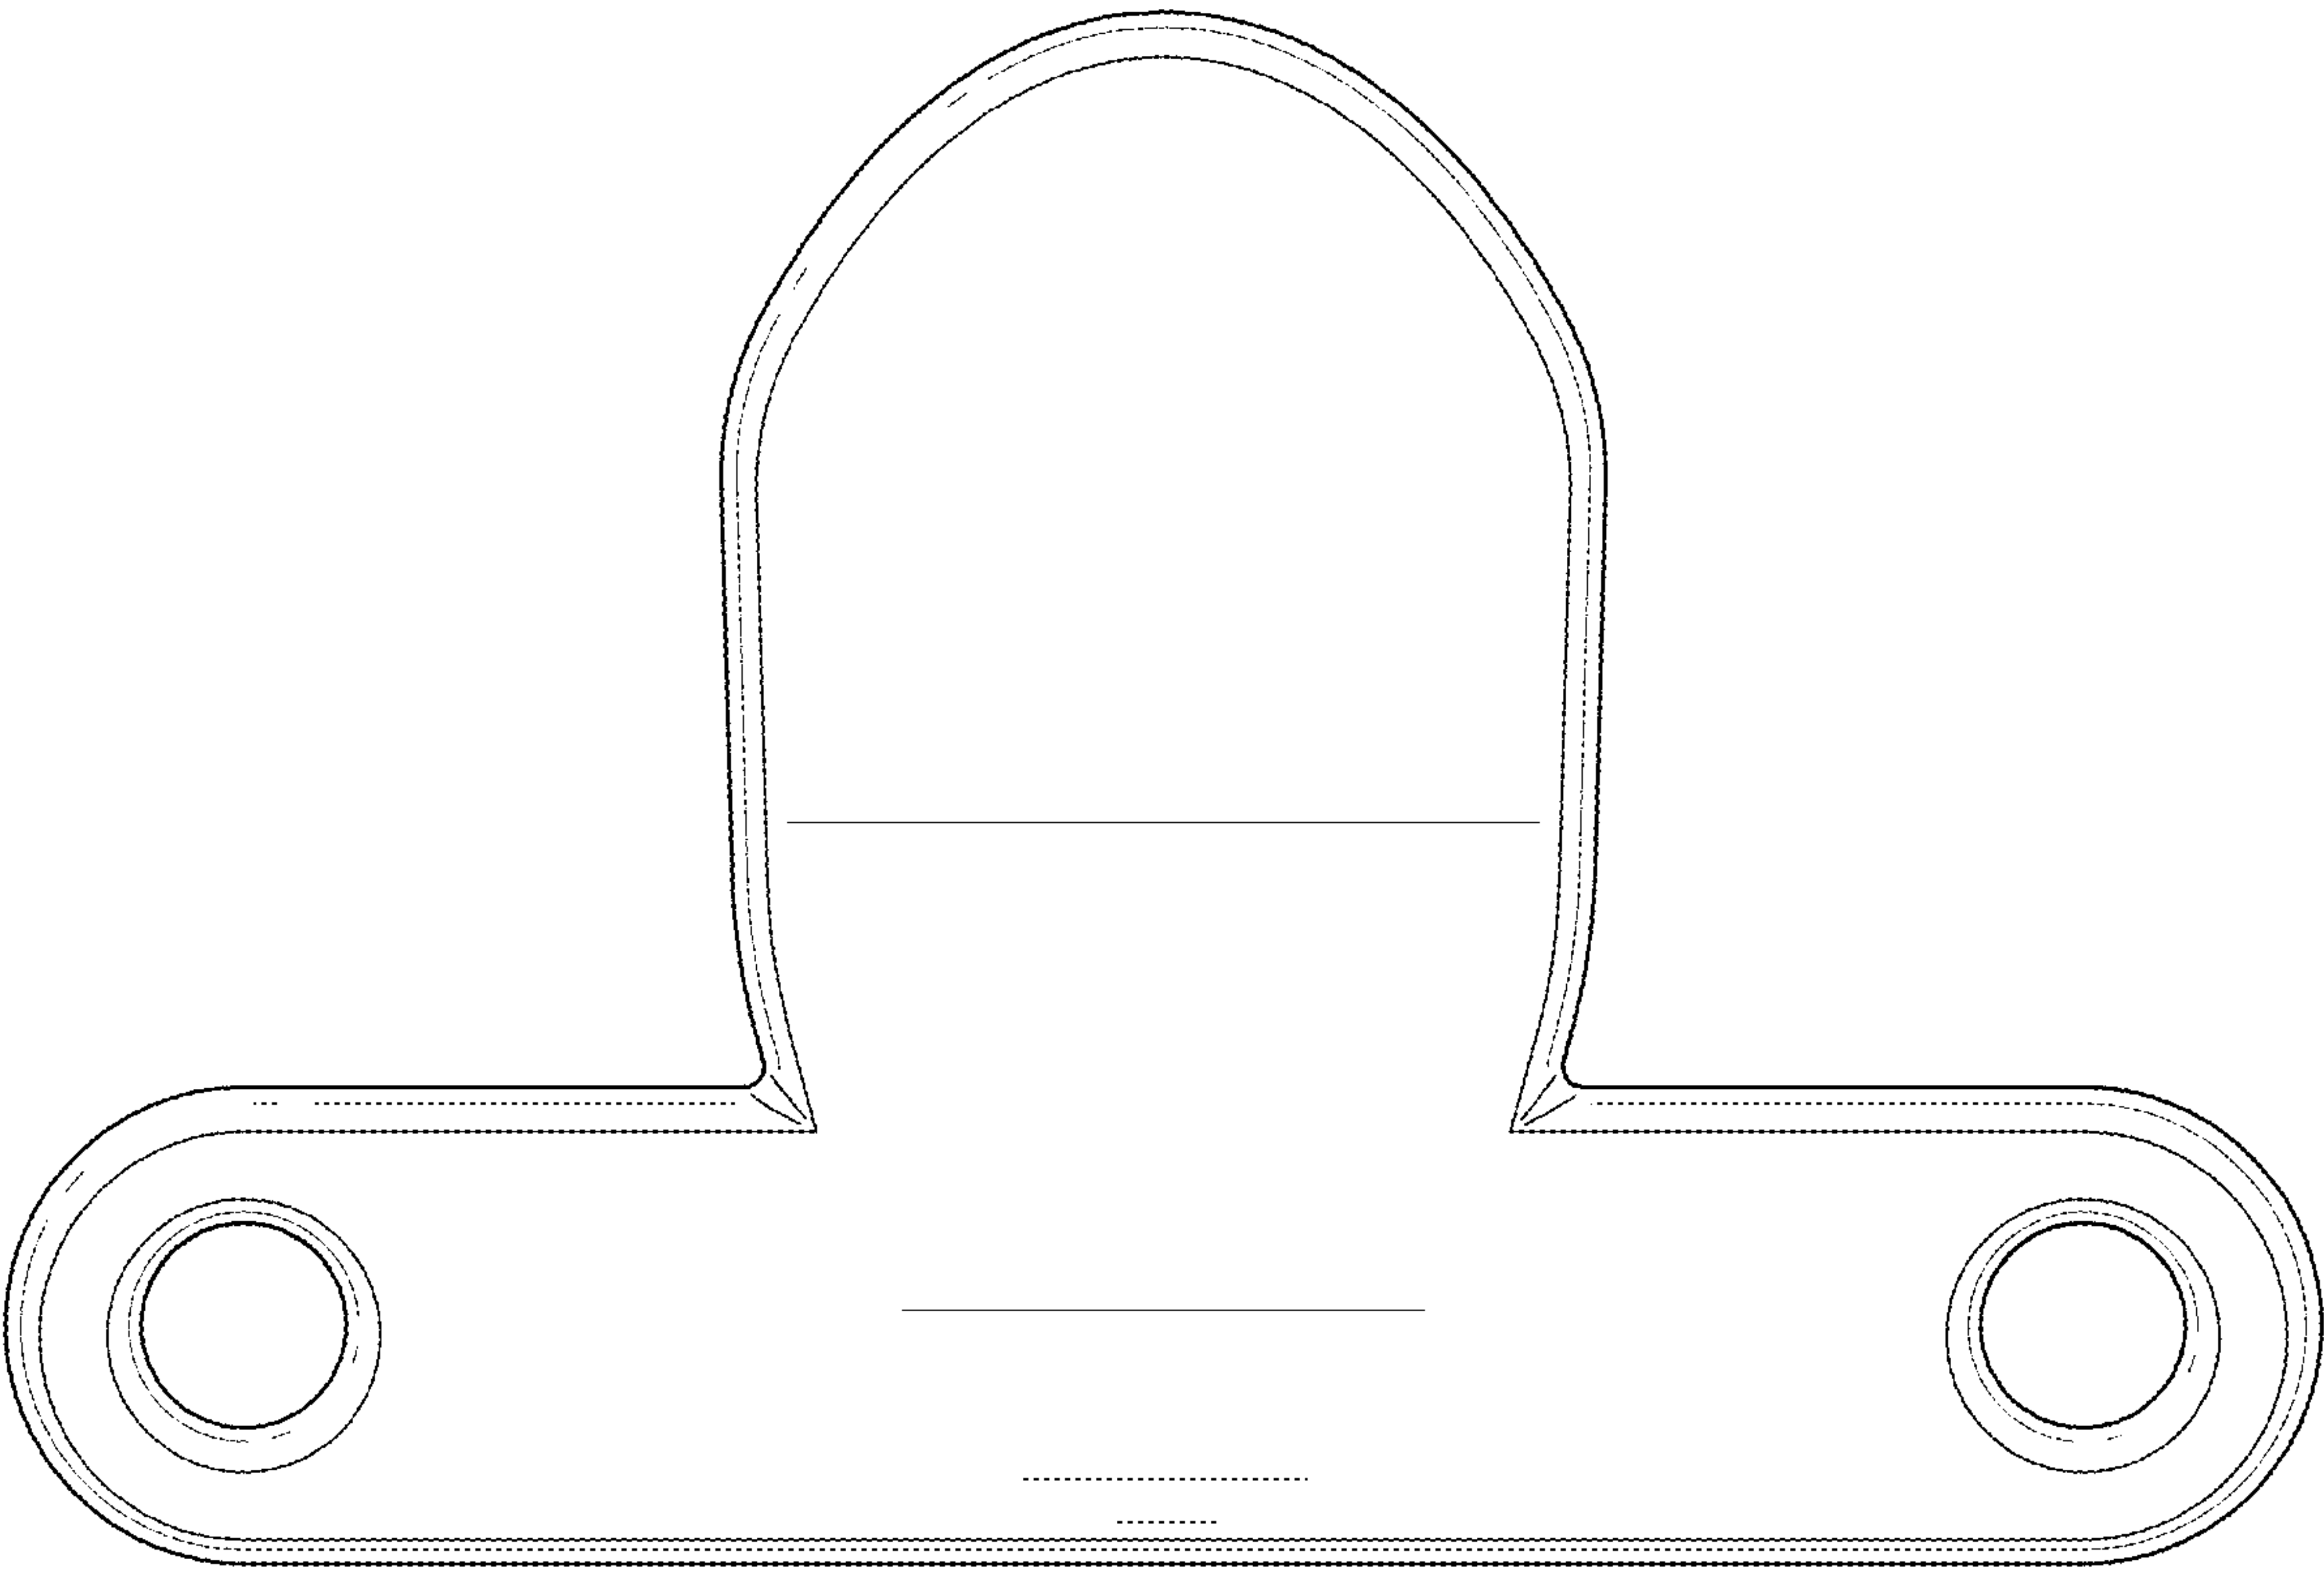


FIG. 3

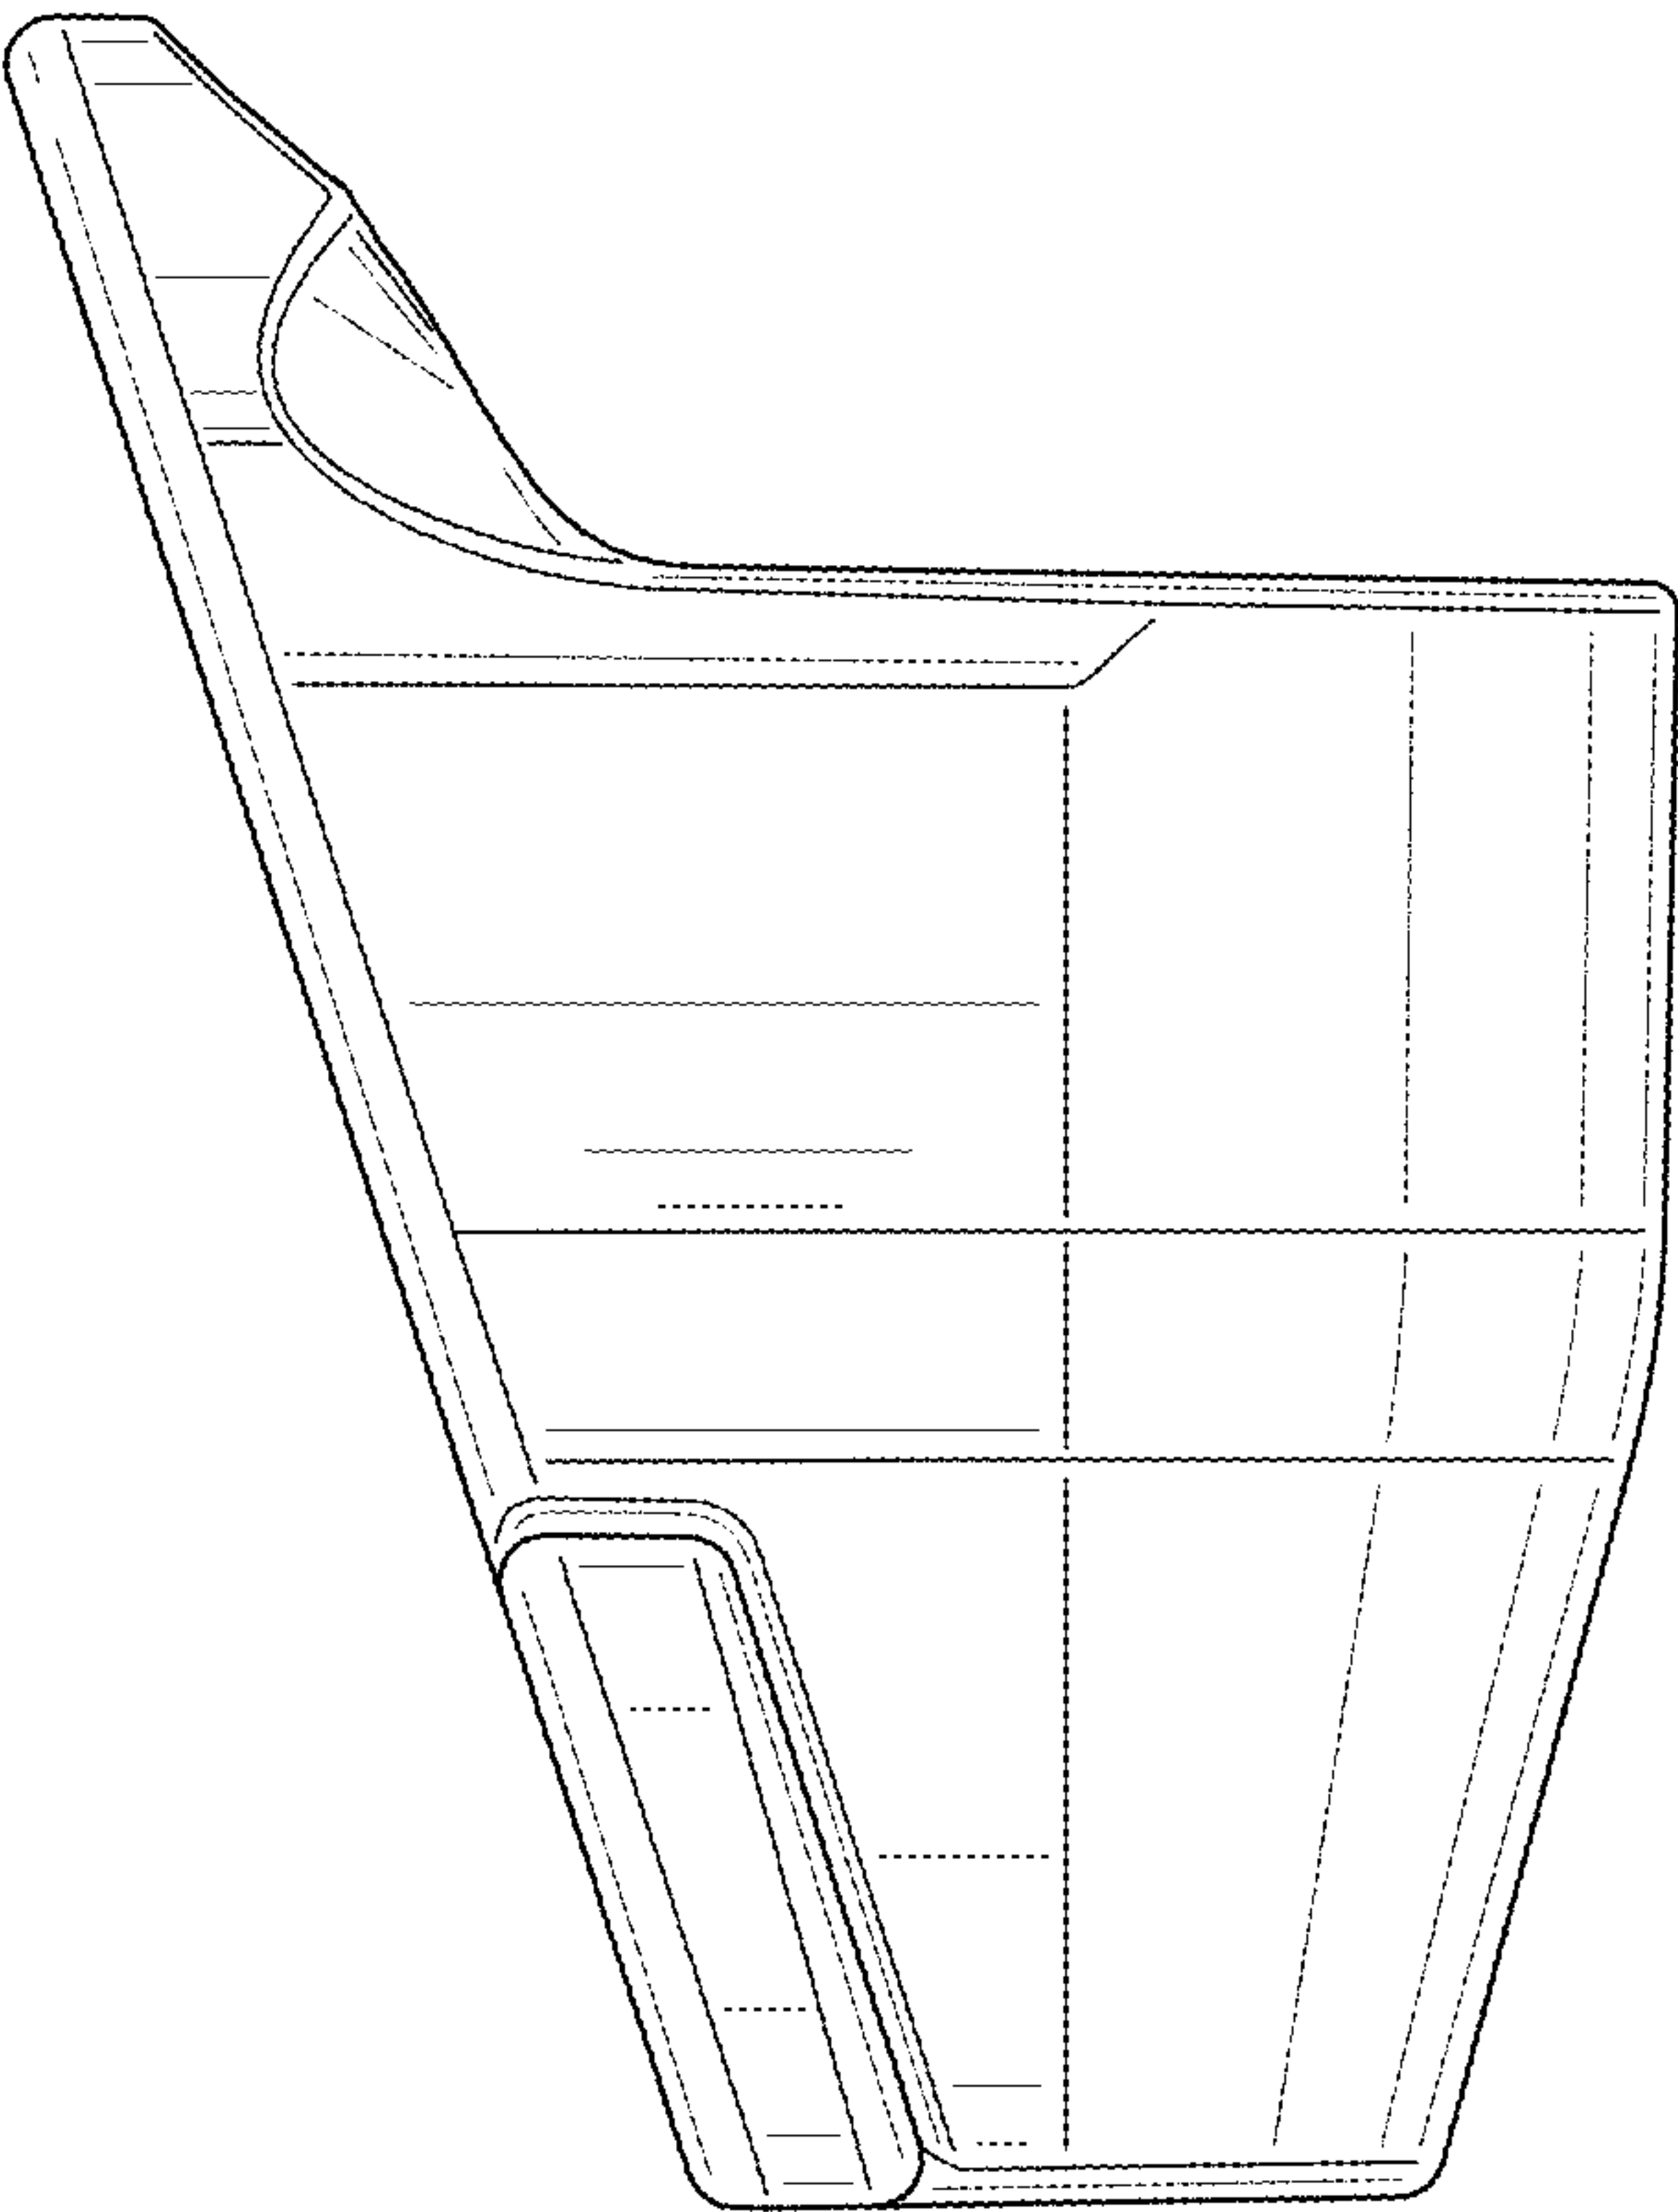


FIG. 4

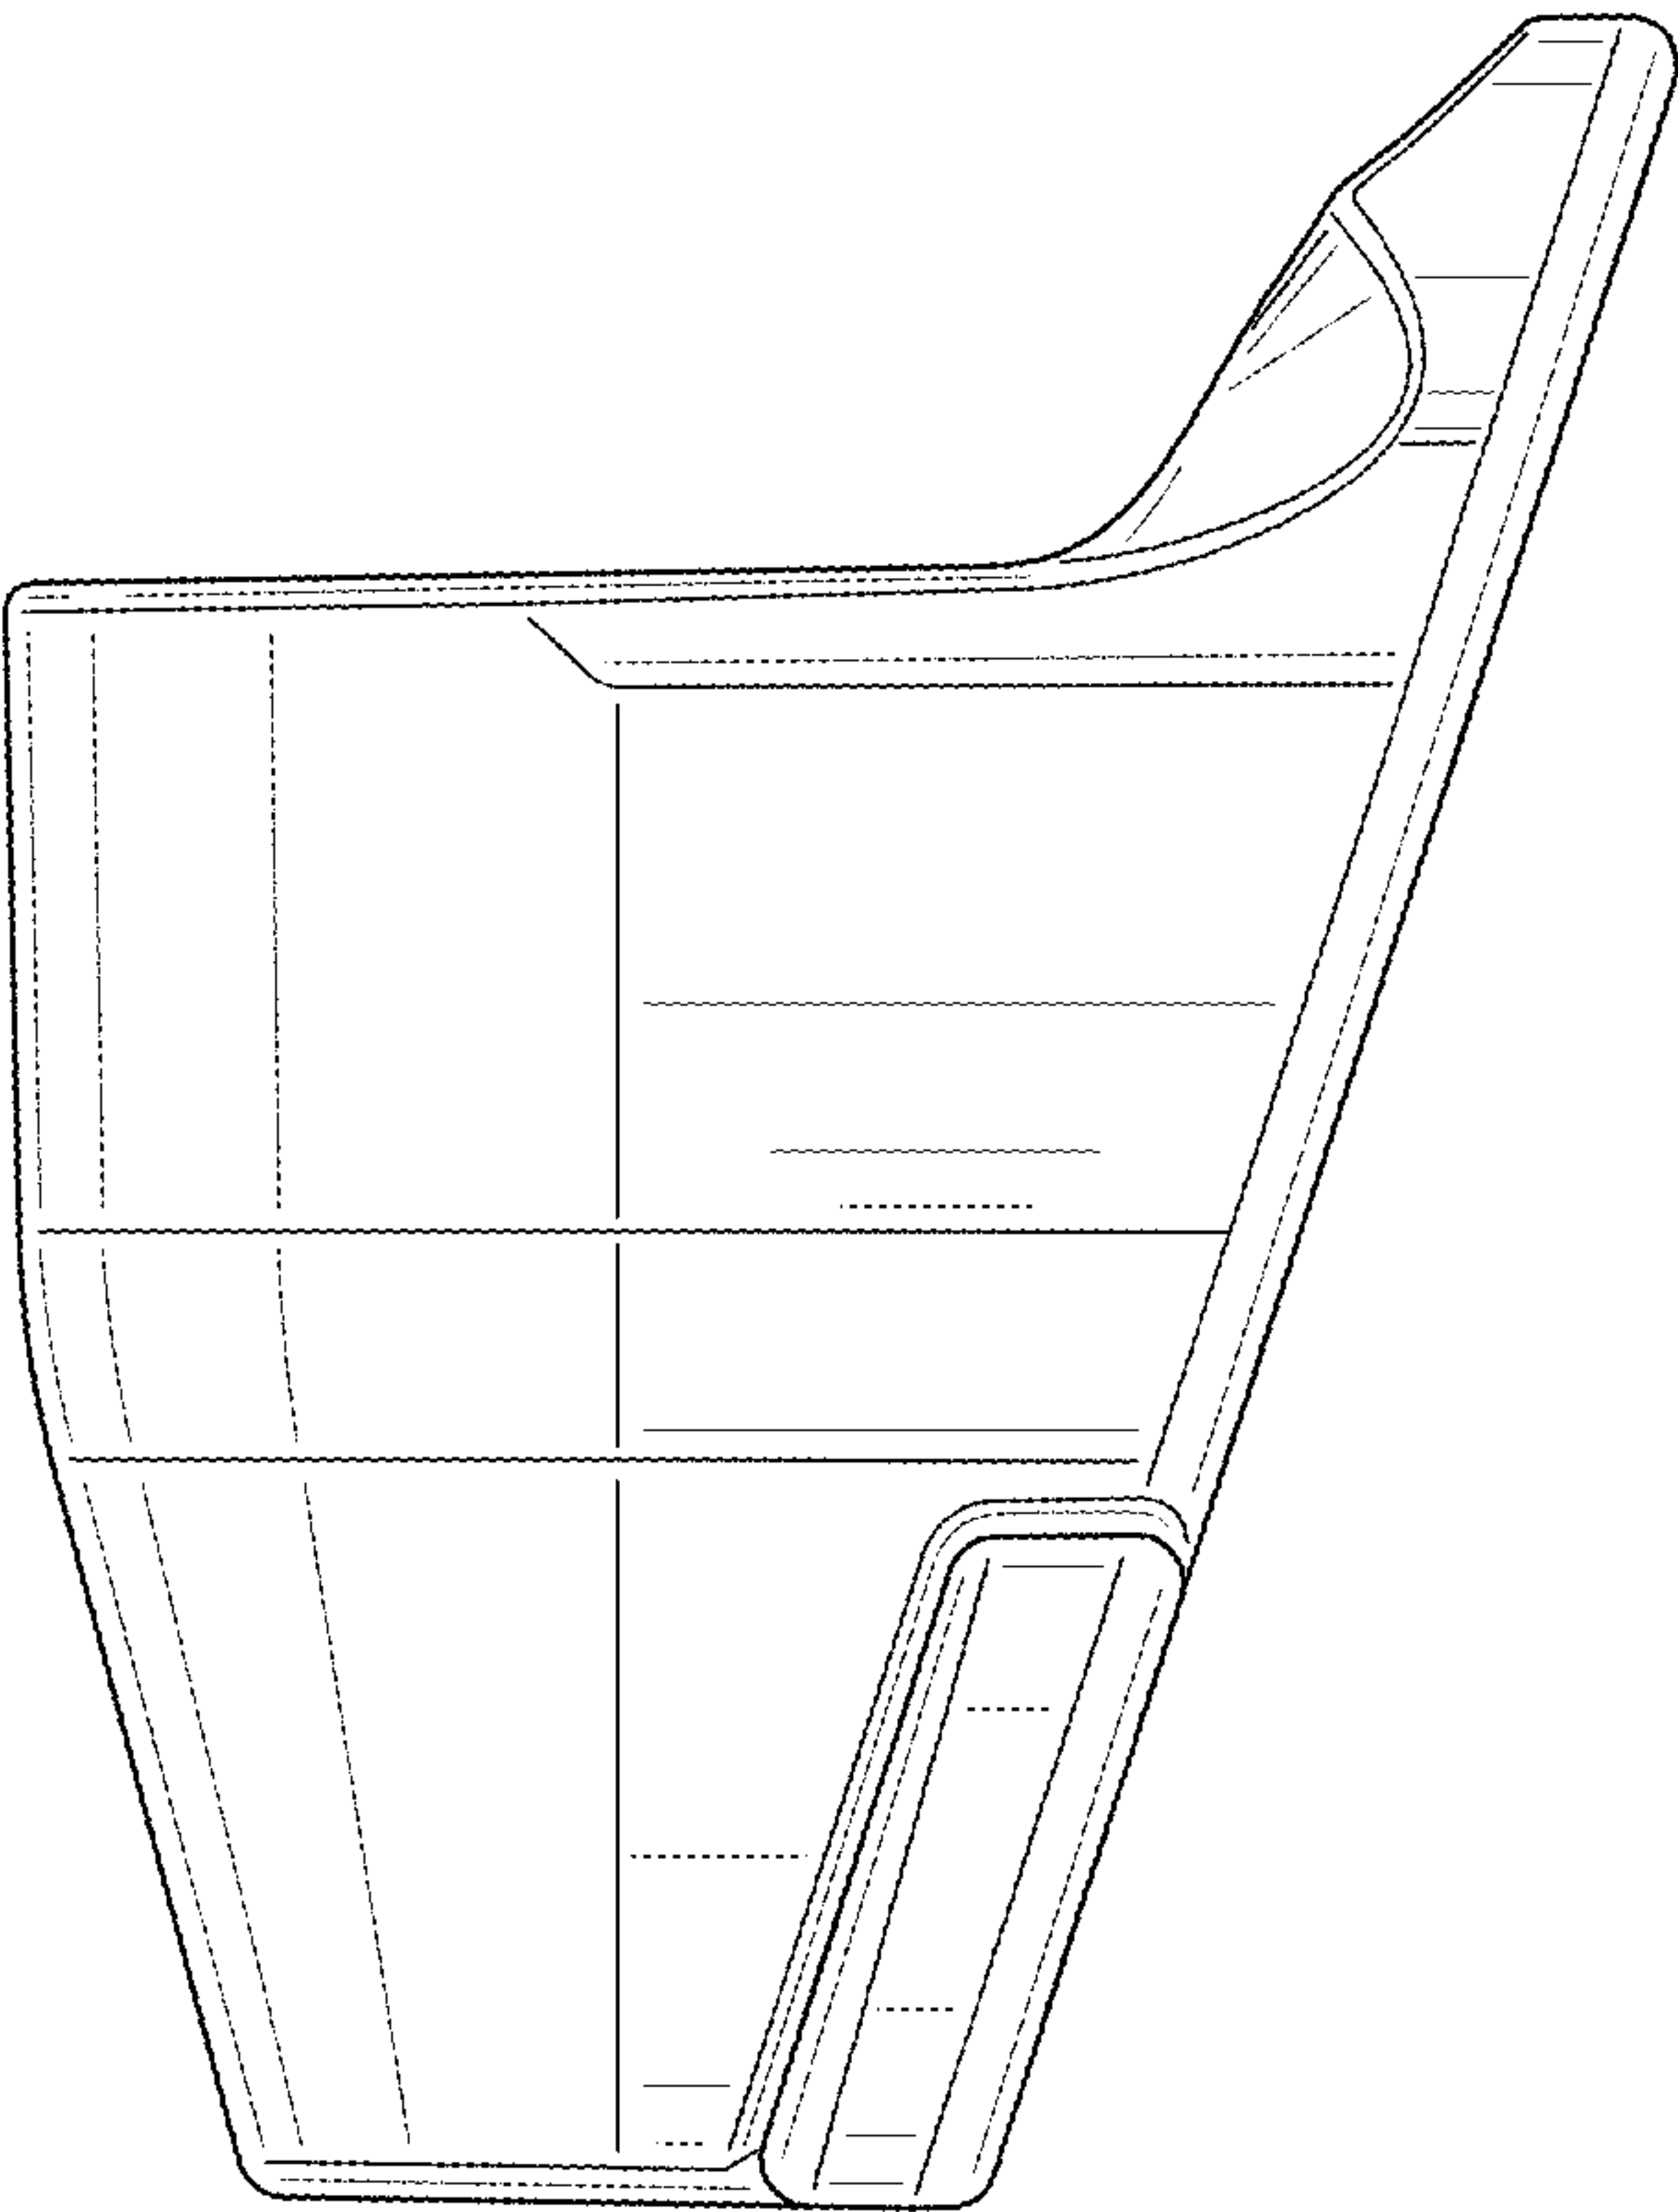


FIG. 5

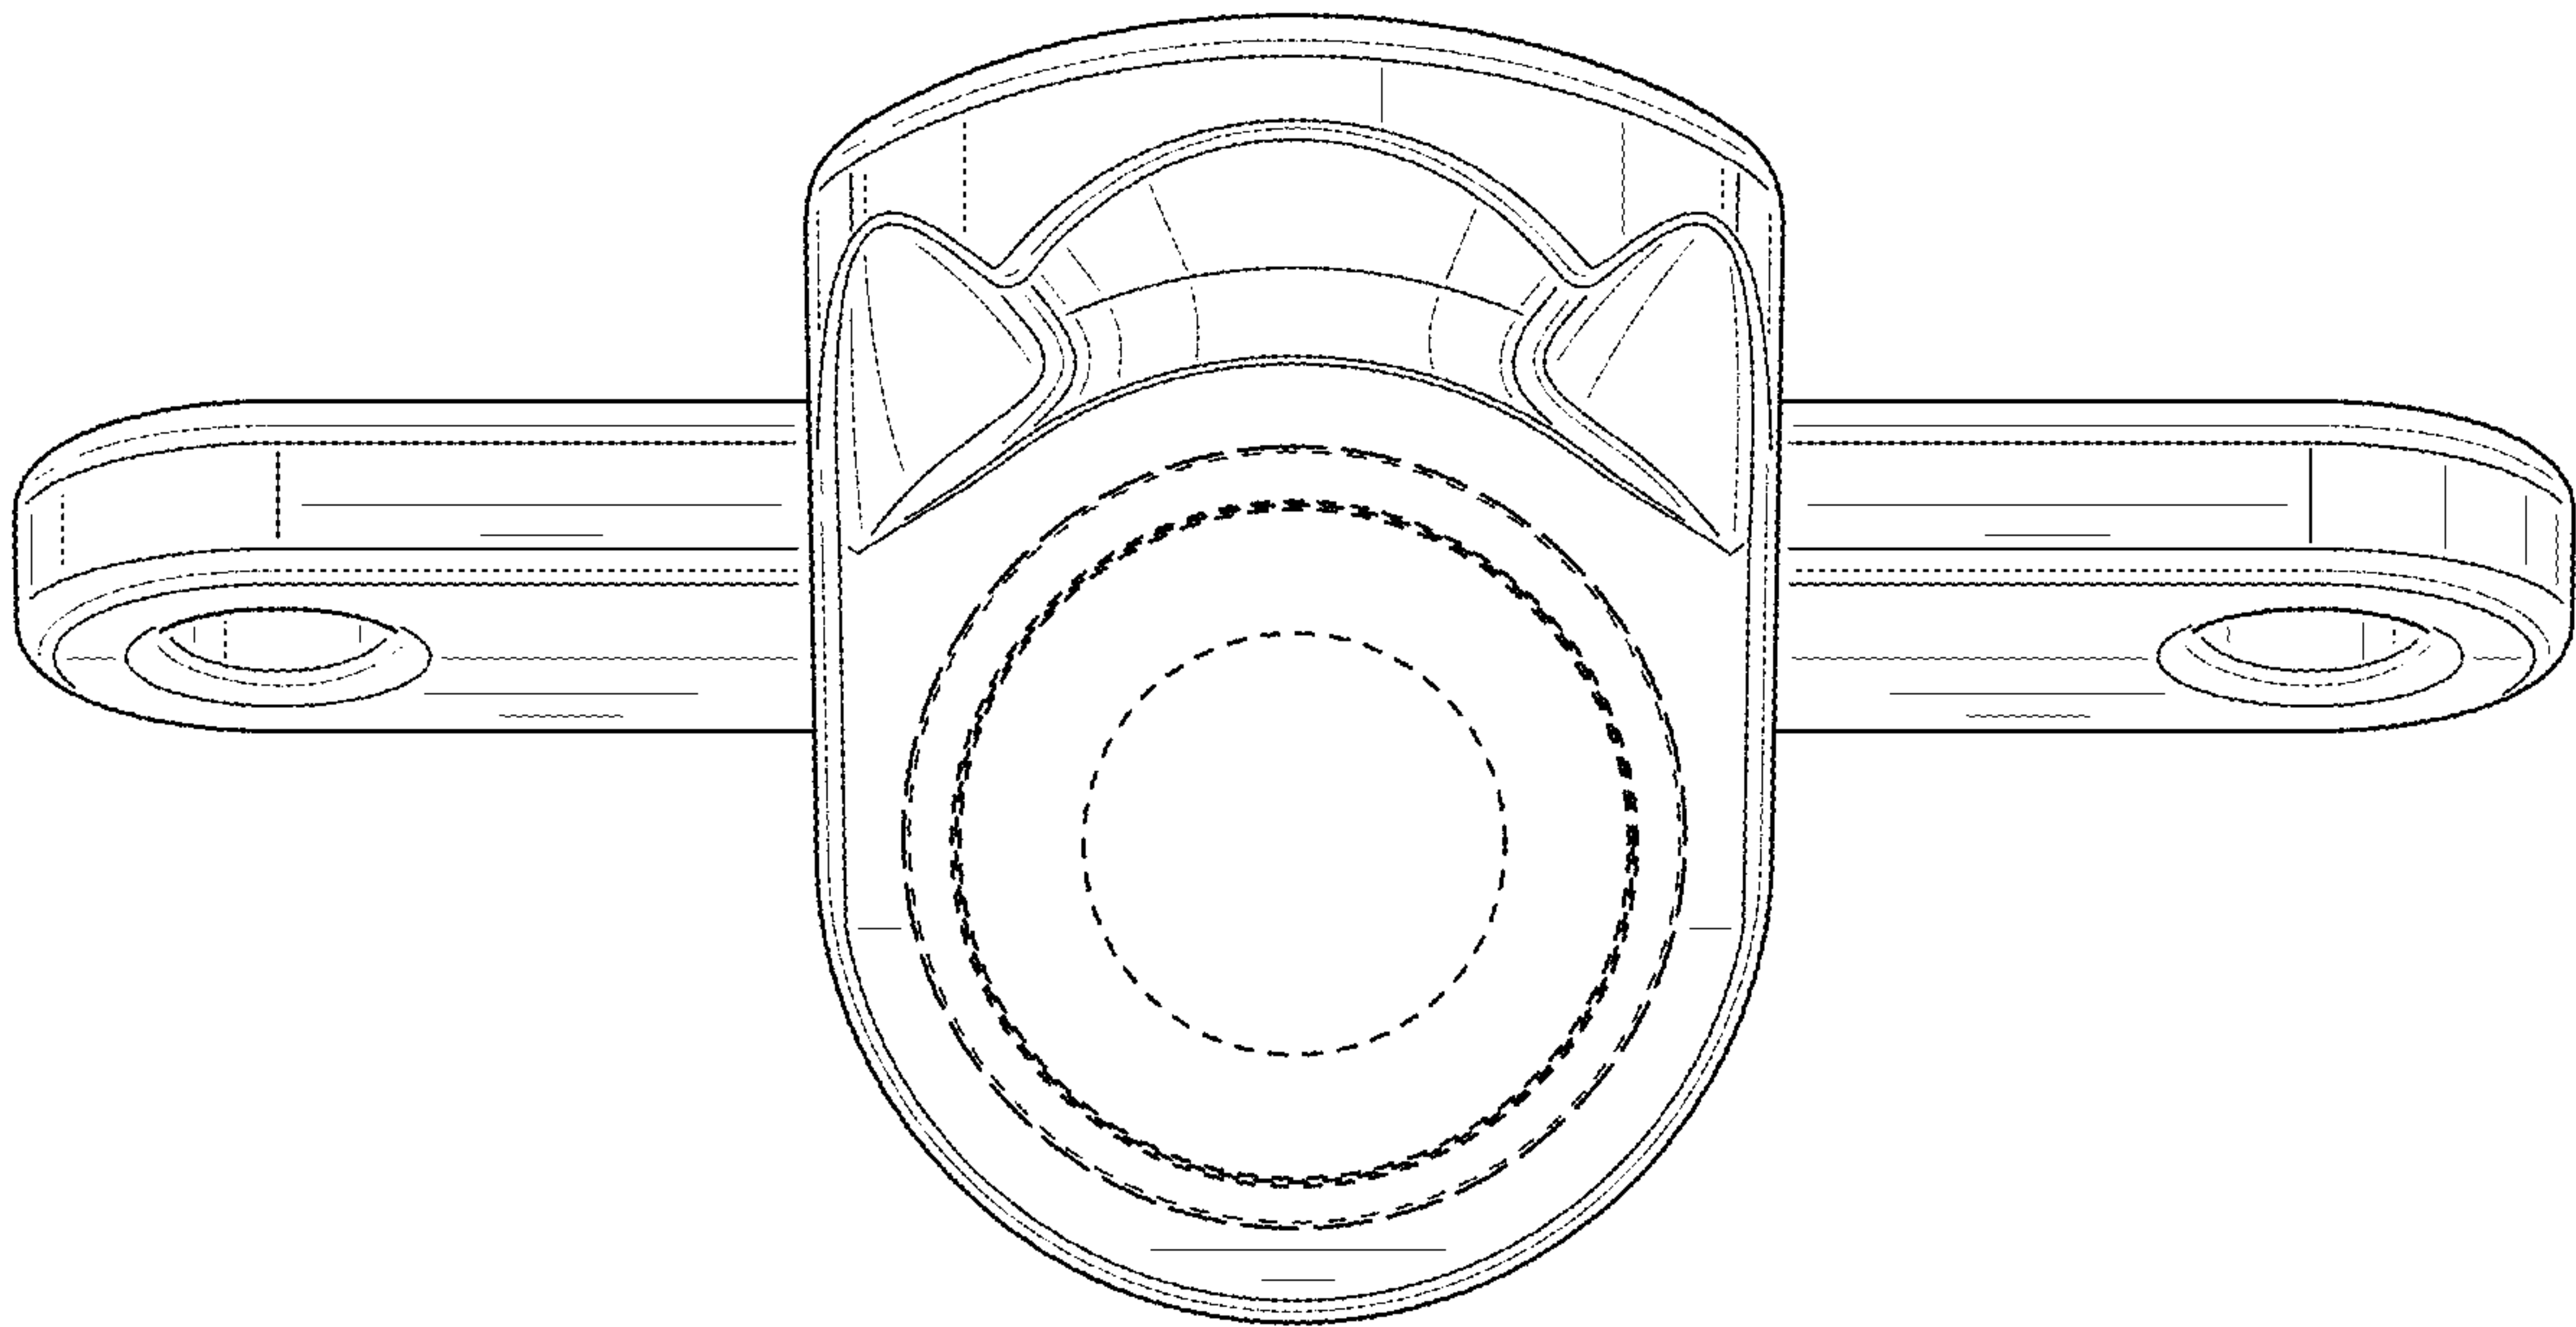


FIG. 6

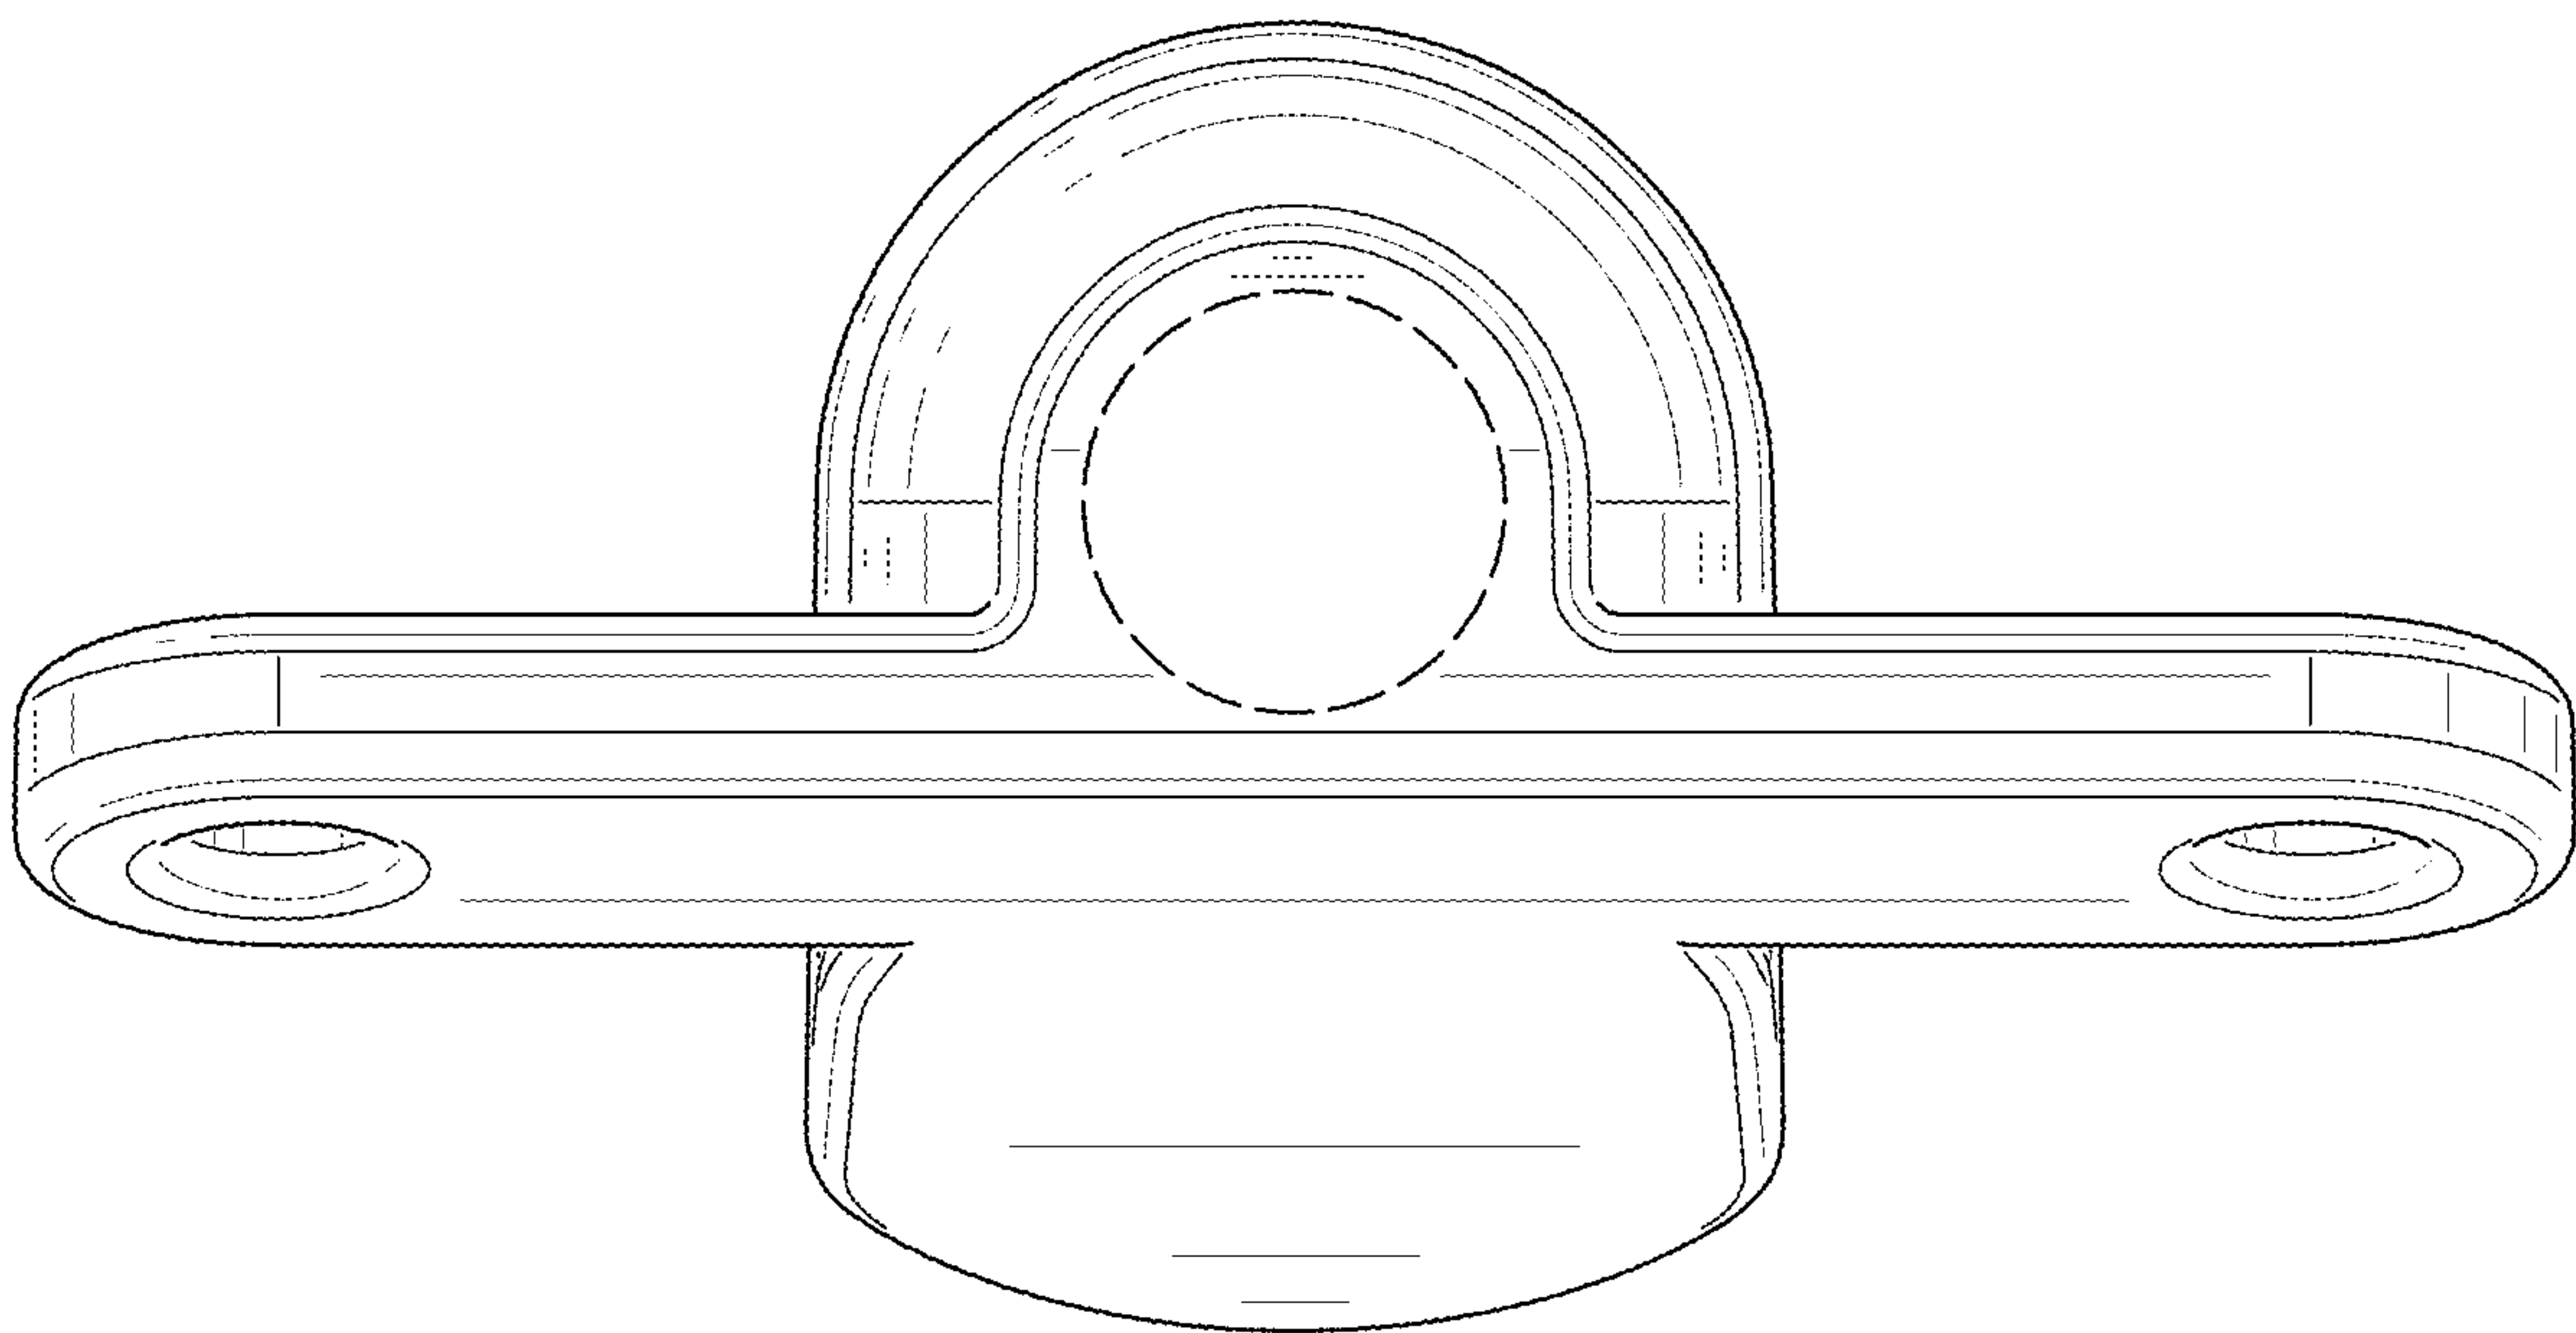


FIG. 7