



US0D1030070S

(12)

United States Design Patent

Tsai et al.

(10)

Patent No.:

US D1,030,070 S

(45)

Date of Patent:

** Jun. 4, 2024

(54) ULTRASOUND PROBE

(71) Applicants:**I-Hsuan Tsai**, Taipei (TW); **Tzu-Chien Lai**, Taipei (TW); **Chien Chiu**, Taipei (TW)

(72) Inventors: **I-Hsuan Tsai**, Taipei (TW); **Tzu-Chien Lai**, Taipei (TW); **Chien Chiu**, Taipei (TW)

(73) Assignee: **COMPAL ELECTRONICS, INC.**, Taipei (TW)

(**) Term: **15 Years**

(21) Appl. No.: **29/858,458**

(22) Filed: **Nov. 1, 2022**

(30) Foreign Application Priority Data

May 31, 2022 (TW) 111302609

(51) LOC (14) Cl. **24-02**

(52) U.S. Cl. **D24/187**

(58) Field of Classification Search

USPC D24/133, 137, 138, 141, 158, 160, 164, D24/165, 167, 170, 186, 187, 200; D10/57, 60, 78, 80

CPC G01N 29/265; A61B 8/4455; A61B 8/445; A61B 5/0095; A61B 8/4444; G01S 7/5208

See application file for complete search history.

(56) References Cited

U.S. PATENT DOCUMENTS

D27,065 S * 5/1897 Scheinkman D24/133

D667,115 S * 9/2012 Caballero D24/141

D672,508 S * 12/2012 Szymanski D24/146

D695,400 S * 12/2013 Sadot D28/7

D861,884 S * 10/2019 Moon D24/187

D862,710 S * 10/2019 Moon D24/187

D870,295 S * 12/2019 de Jonge D24/187

D875,259 S * 2/2020 Moon D24/187

D892,324 S * 8/2020 Yi D24/141

D961,106 S * 8/2022 He D24/215

D990,683 S * 6/2023 Yavuz D24/164

D1,004,784 S * 11/2023 Zhang D24/187

OTHER PUBLICATIONS

Vscan Air™ CL for MSK ultrasound. Online, published date unknown. Retrieved on Jan. 3, 2024 from URL: https://handheldultrasound.gehealthcare.com/msk-ultrasound/?utm_medium=cpc&utm_source=google&utm_campaign=USC-ULT-PCA-AlwaysOn-COV-SC&utm_term=ge%20msk%20ultrasound&utm_content=13910969716&npclid=EAIaIQobChMI2qGEqYL.*

* cited by examiner

Primary Examiner — Omeed Agilee
(74) Attorney, Agent, or Firm — JCIPRNET

(57) CLAIM

The ornamental design for an ultrasound probe, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of an ultrasound probe showing our new design;

FIG. 2 is another perspective view thereof;

FIG. 3 is a front view thereof;

FIG. 4 is a rear view thereof;

FIG. 5 is a left side view thereof;


FIG. 6 is a right side view thereof;

FIG. 7 is a top view thereof; and,

FIG. 8 is a bottom view thereof.

The broken lines illustrate portions of the ultrasound probe that form no part of the claimed design.

1 Claim, 8 Drawing Sheets

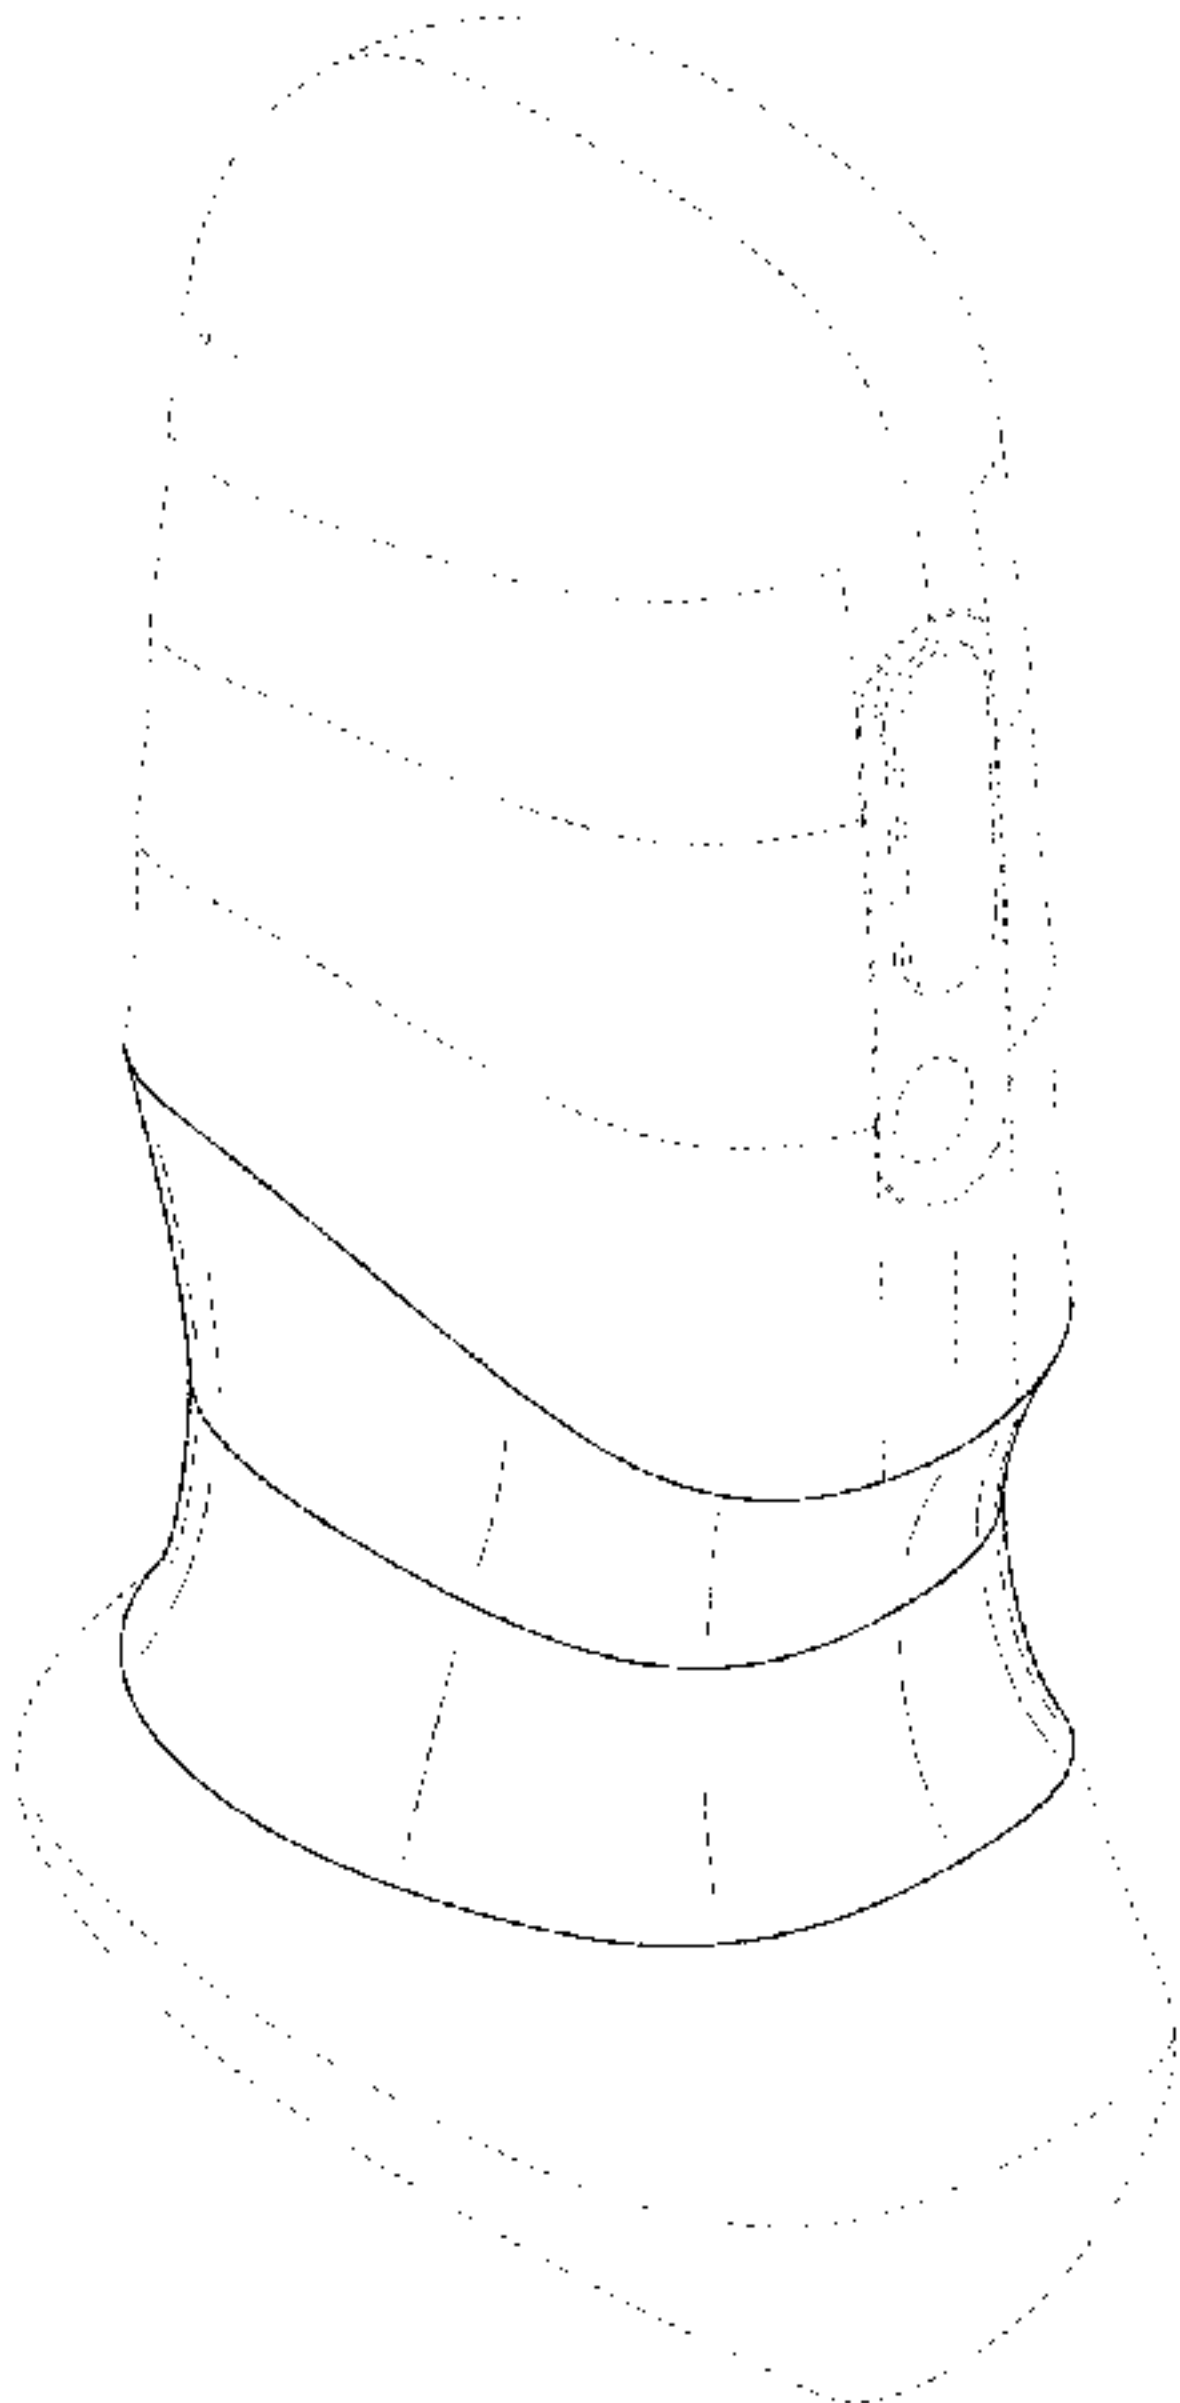

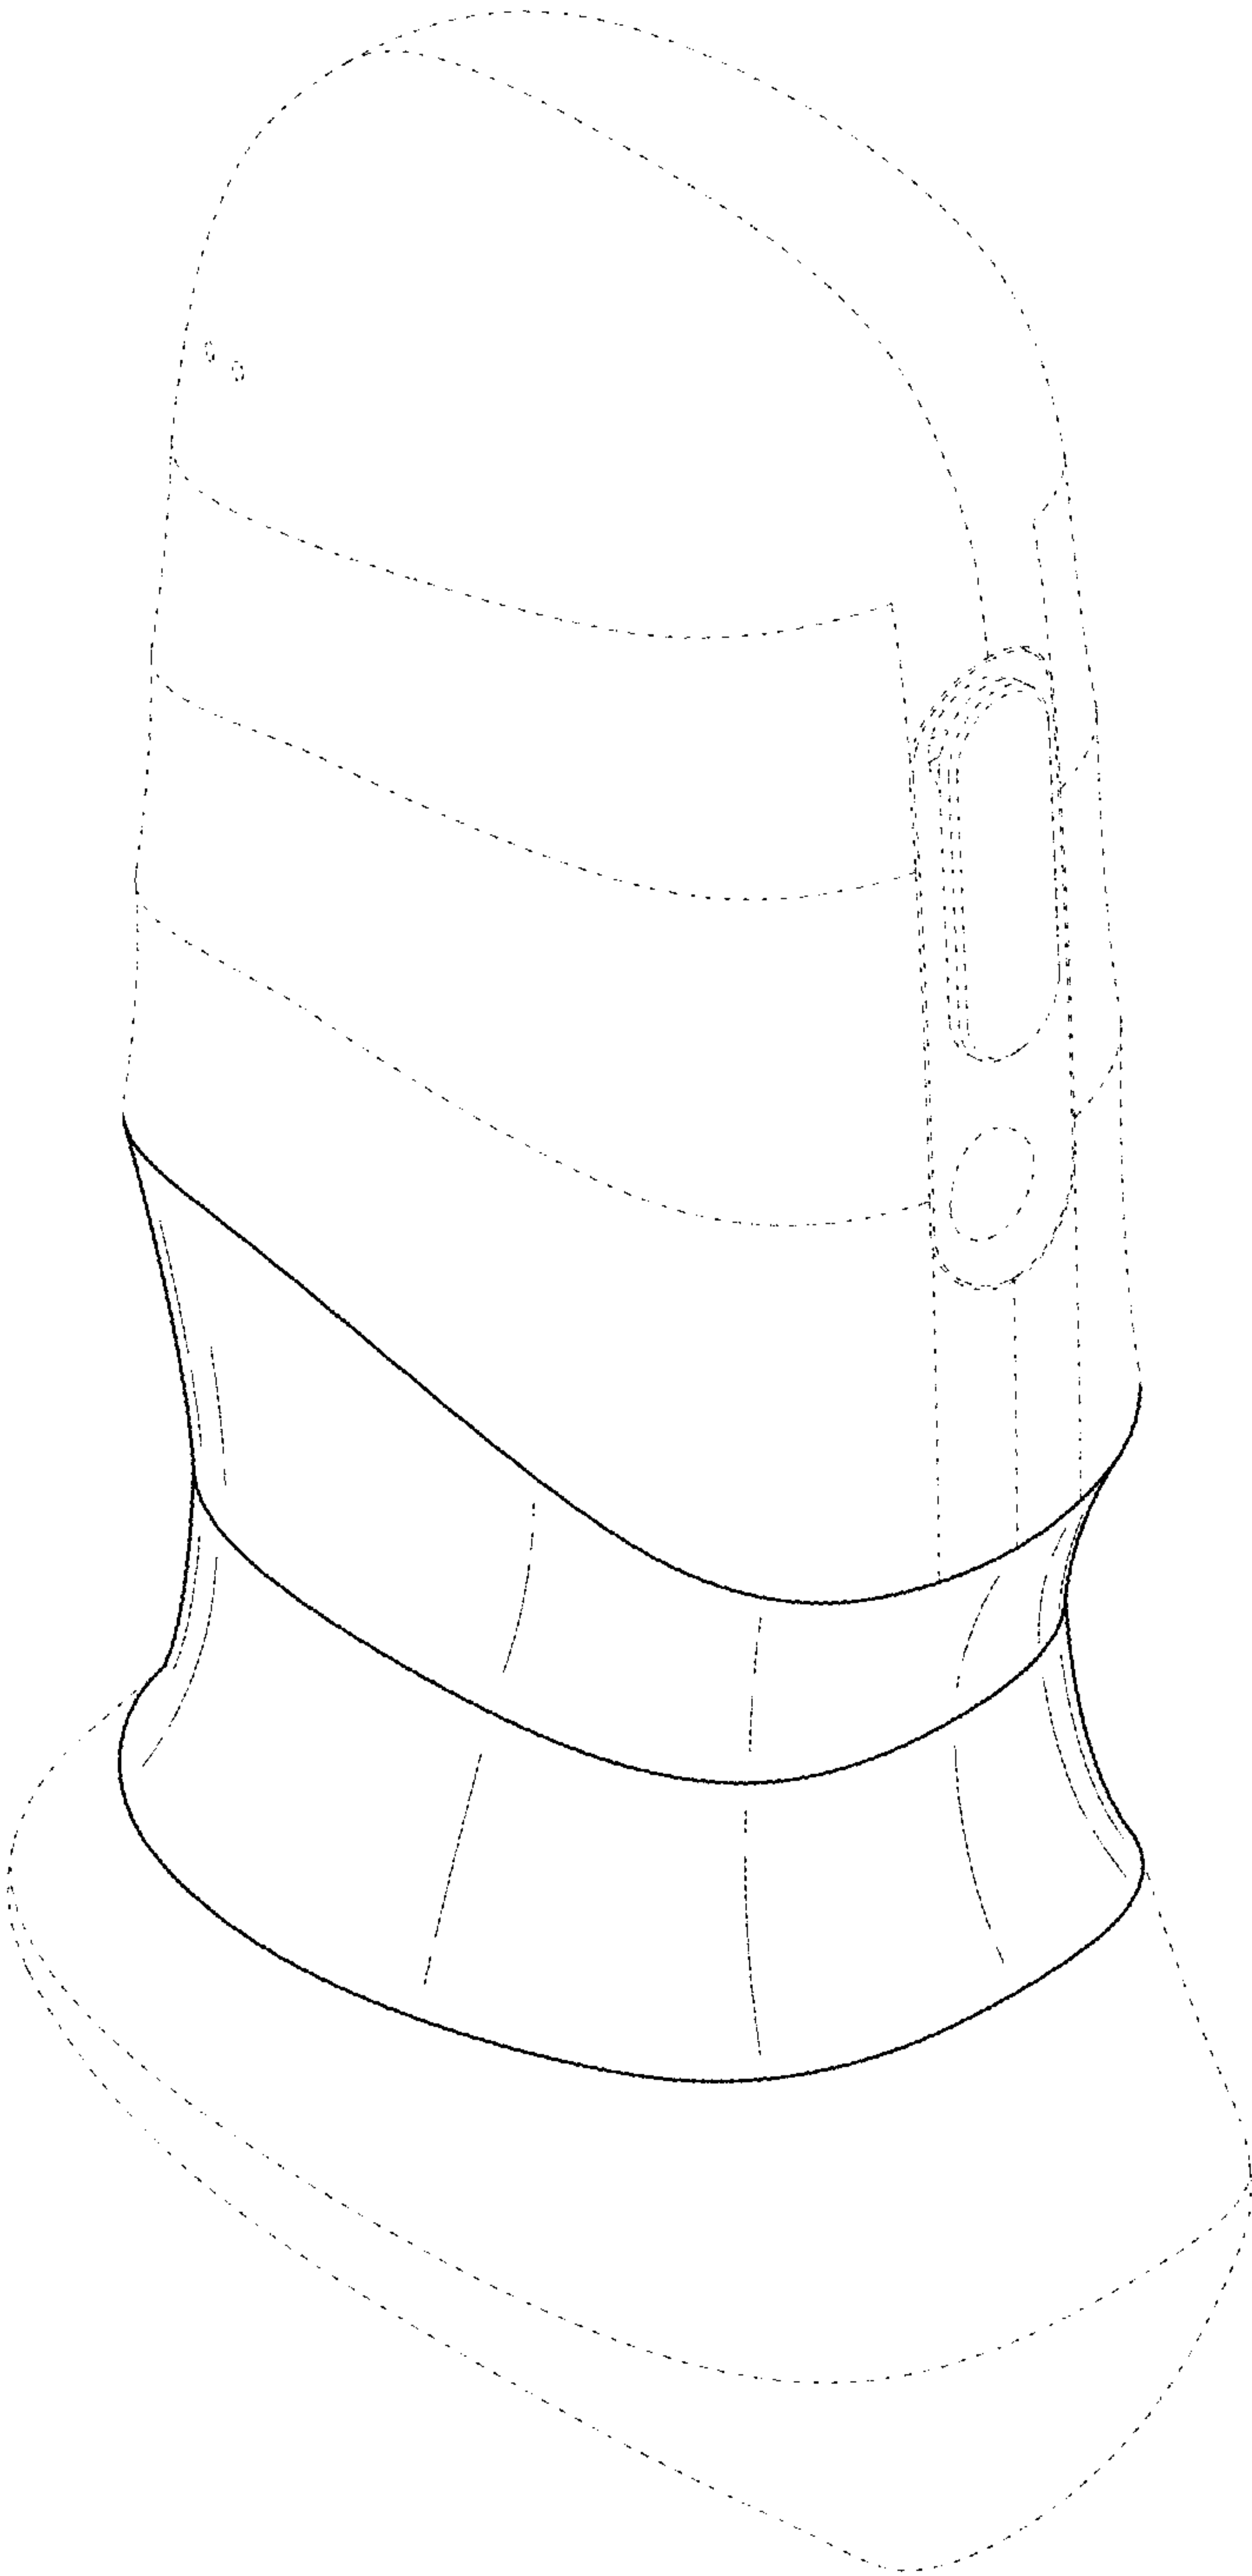


FIG. 1

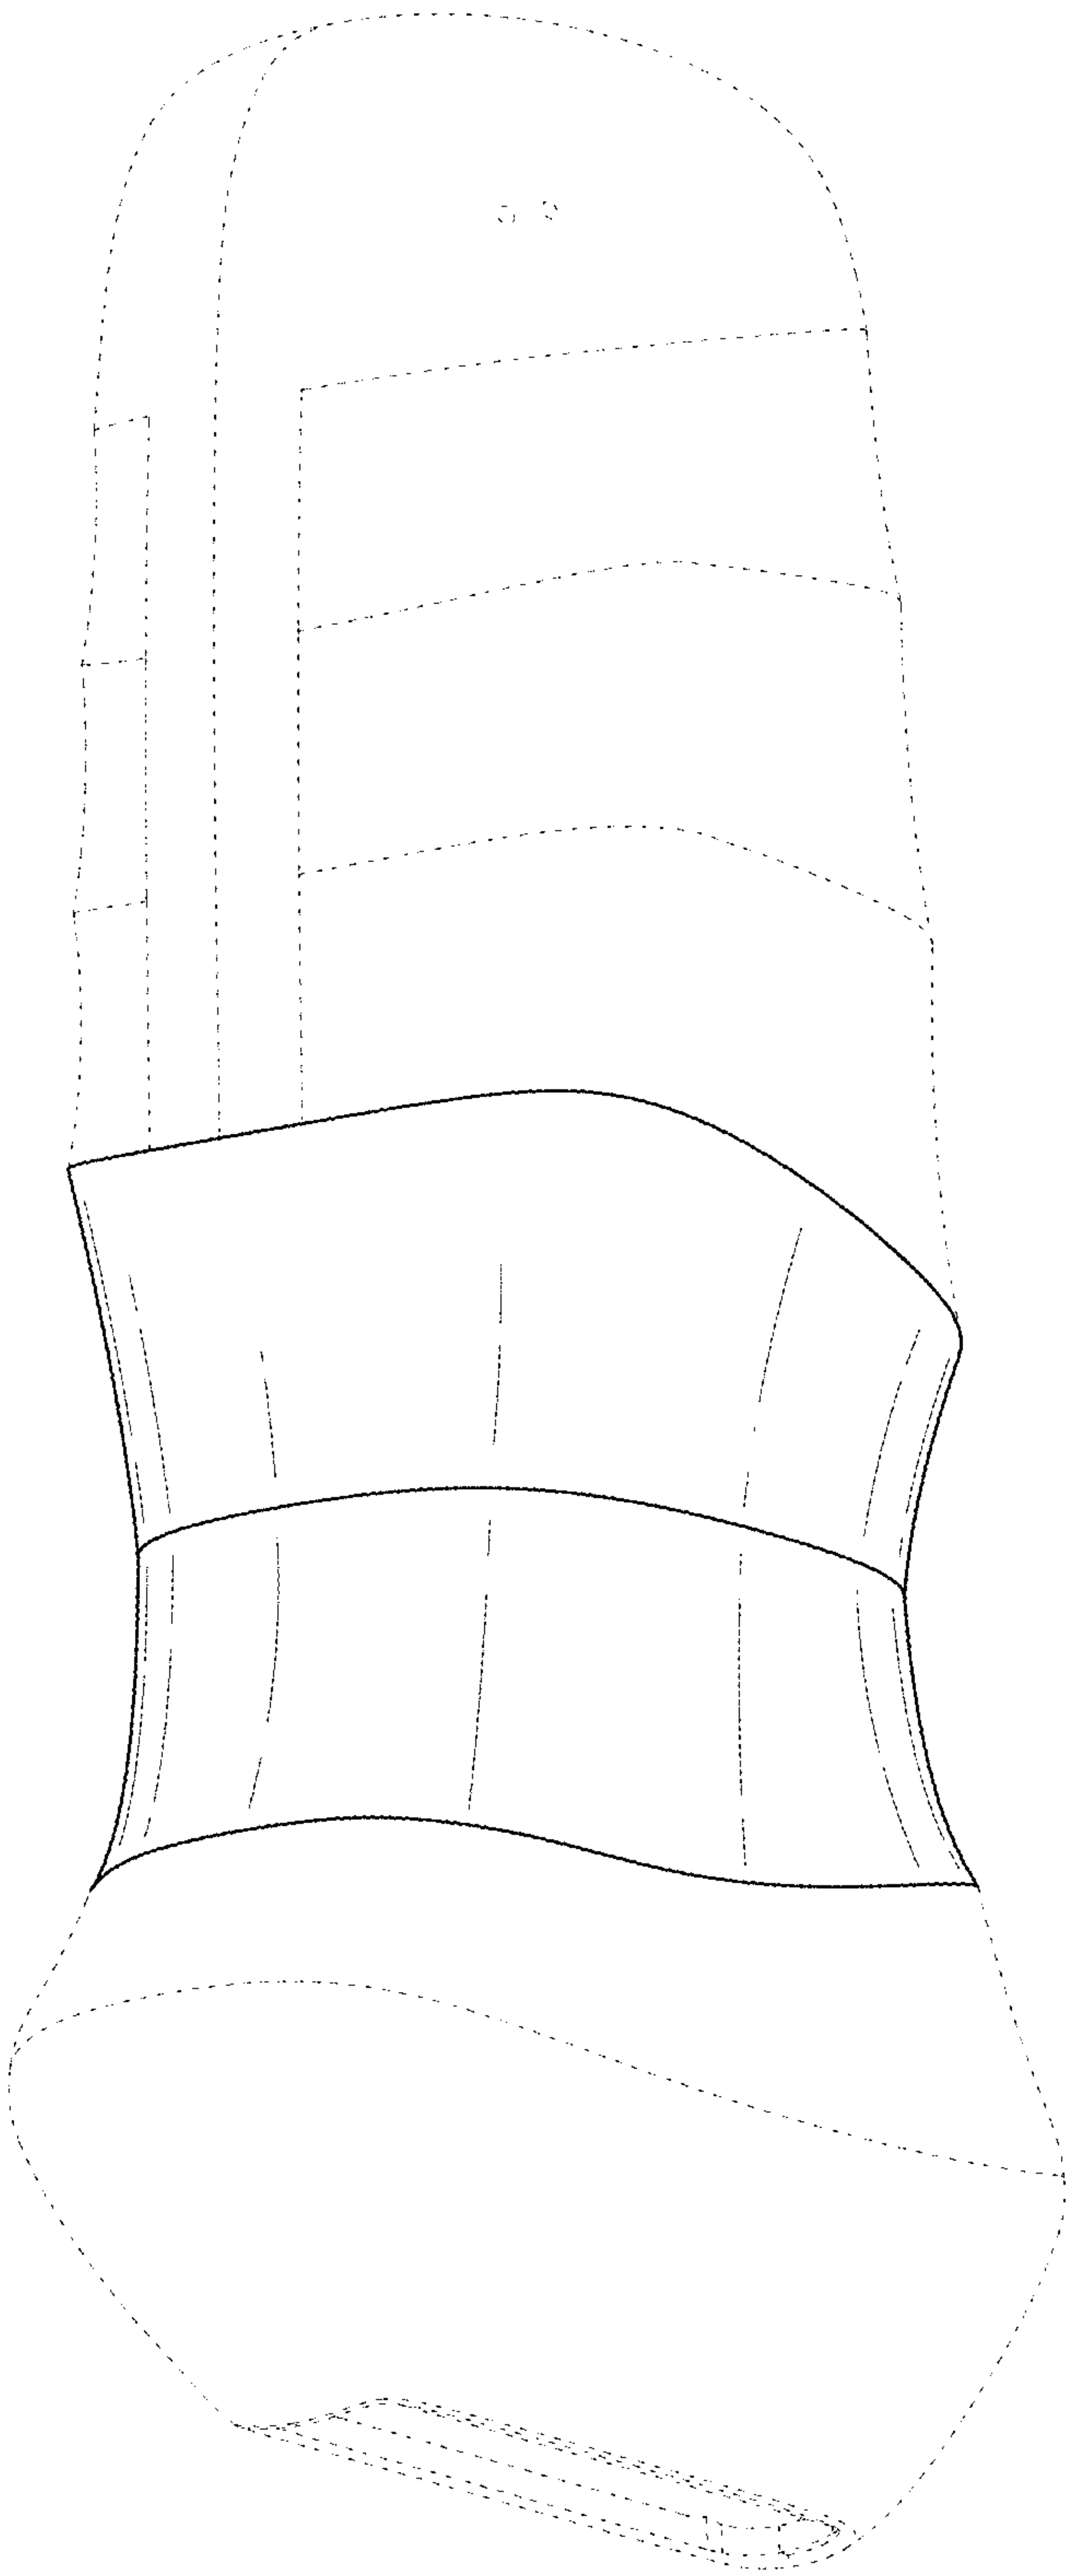


FIG. 2

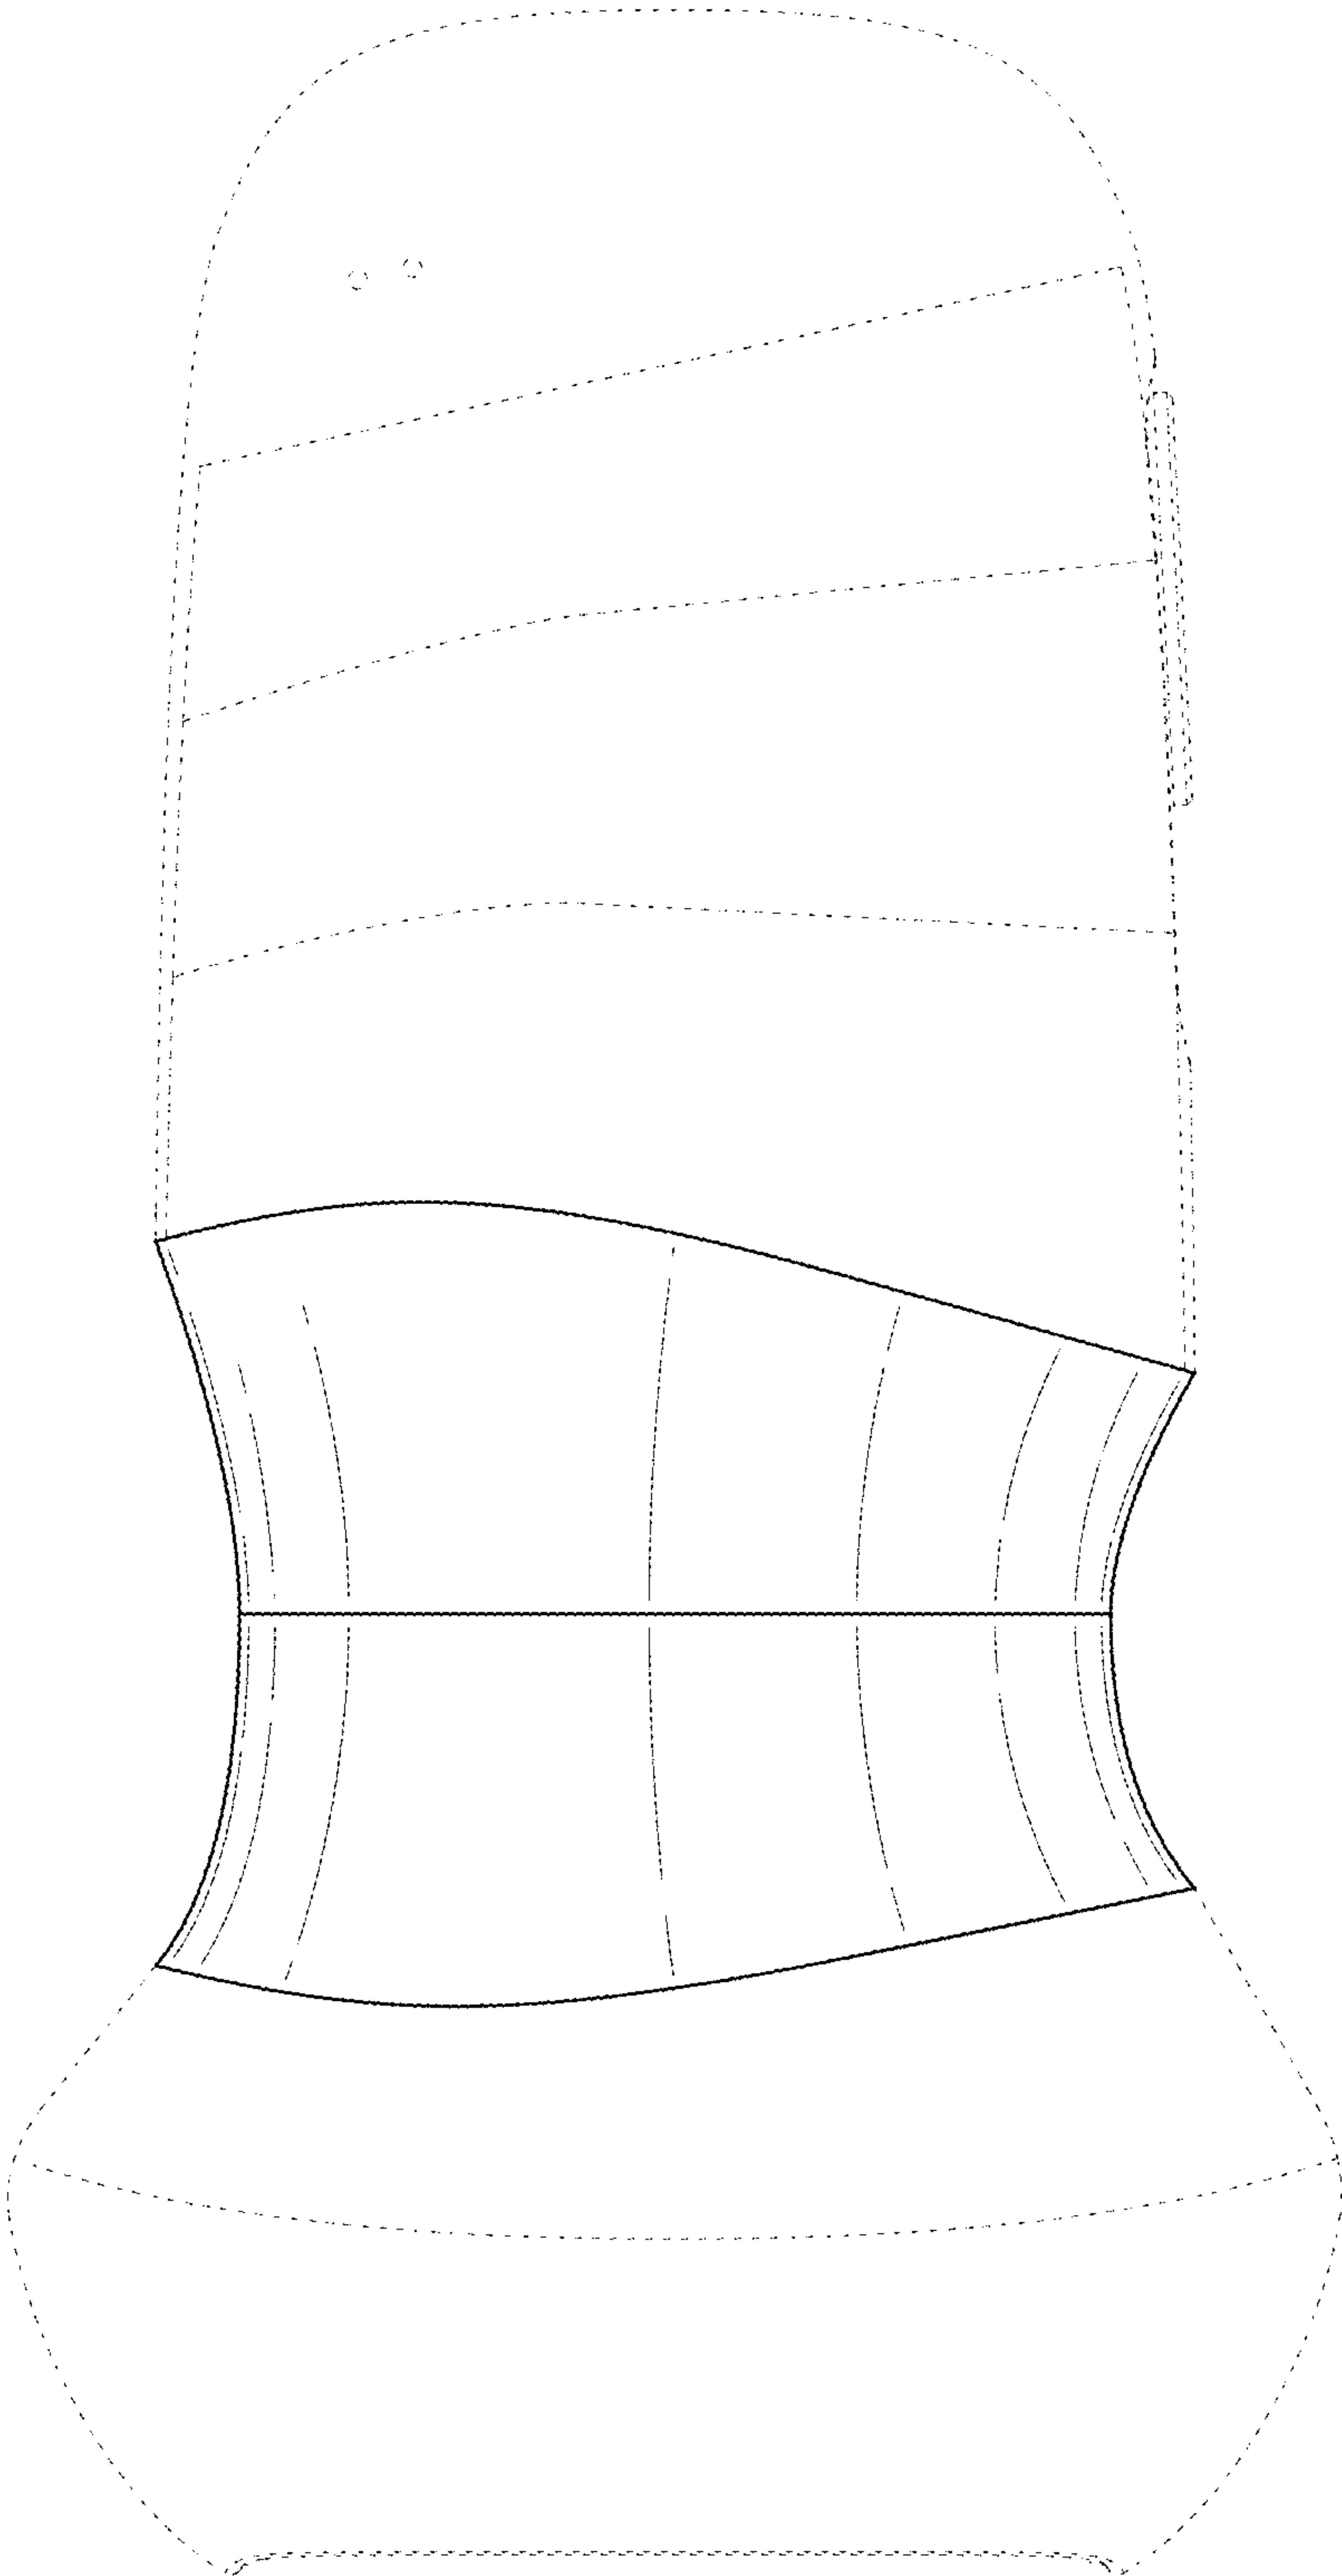


FIG. 3

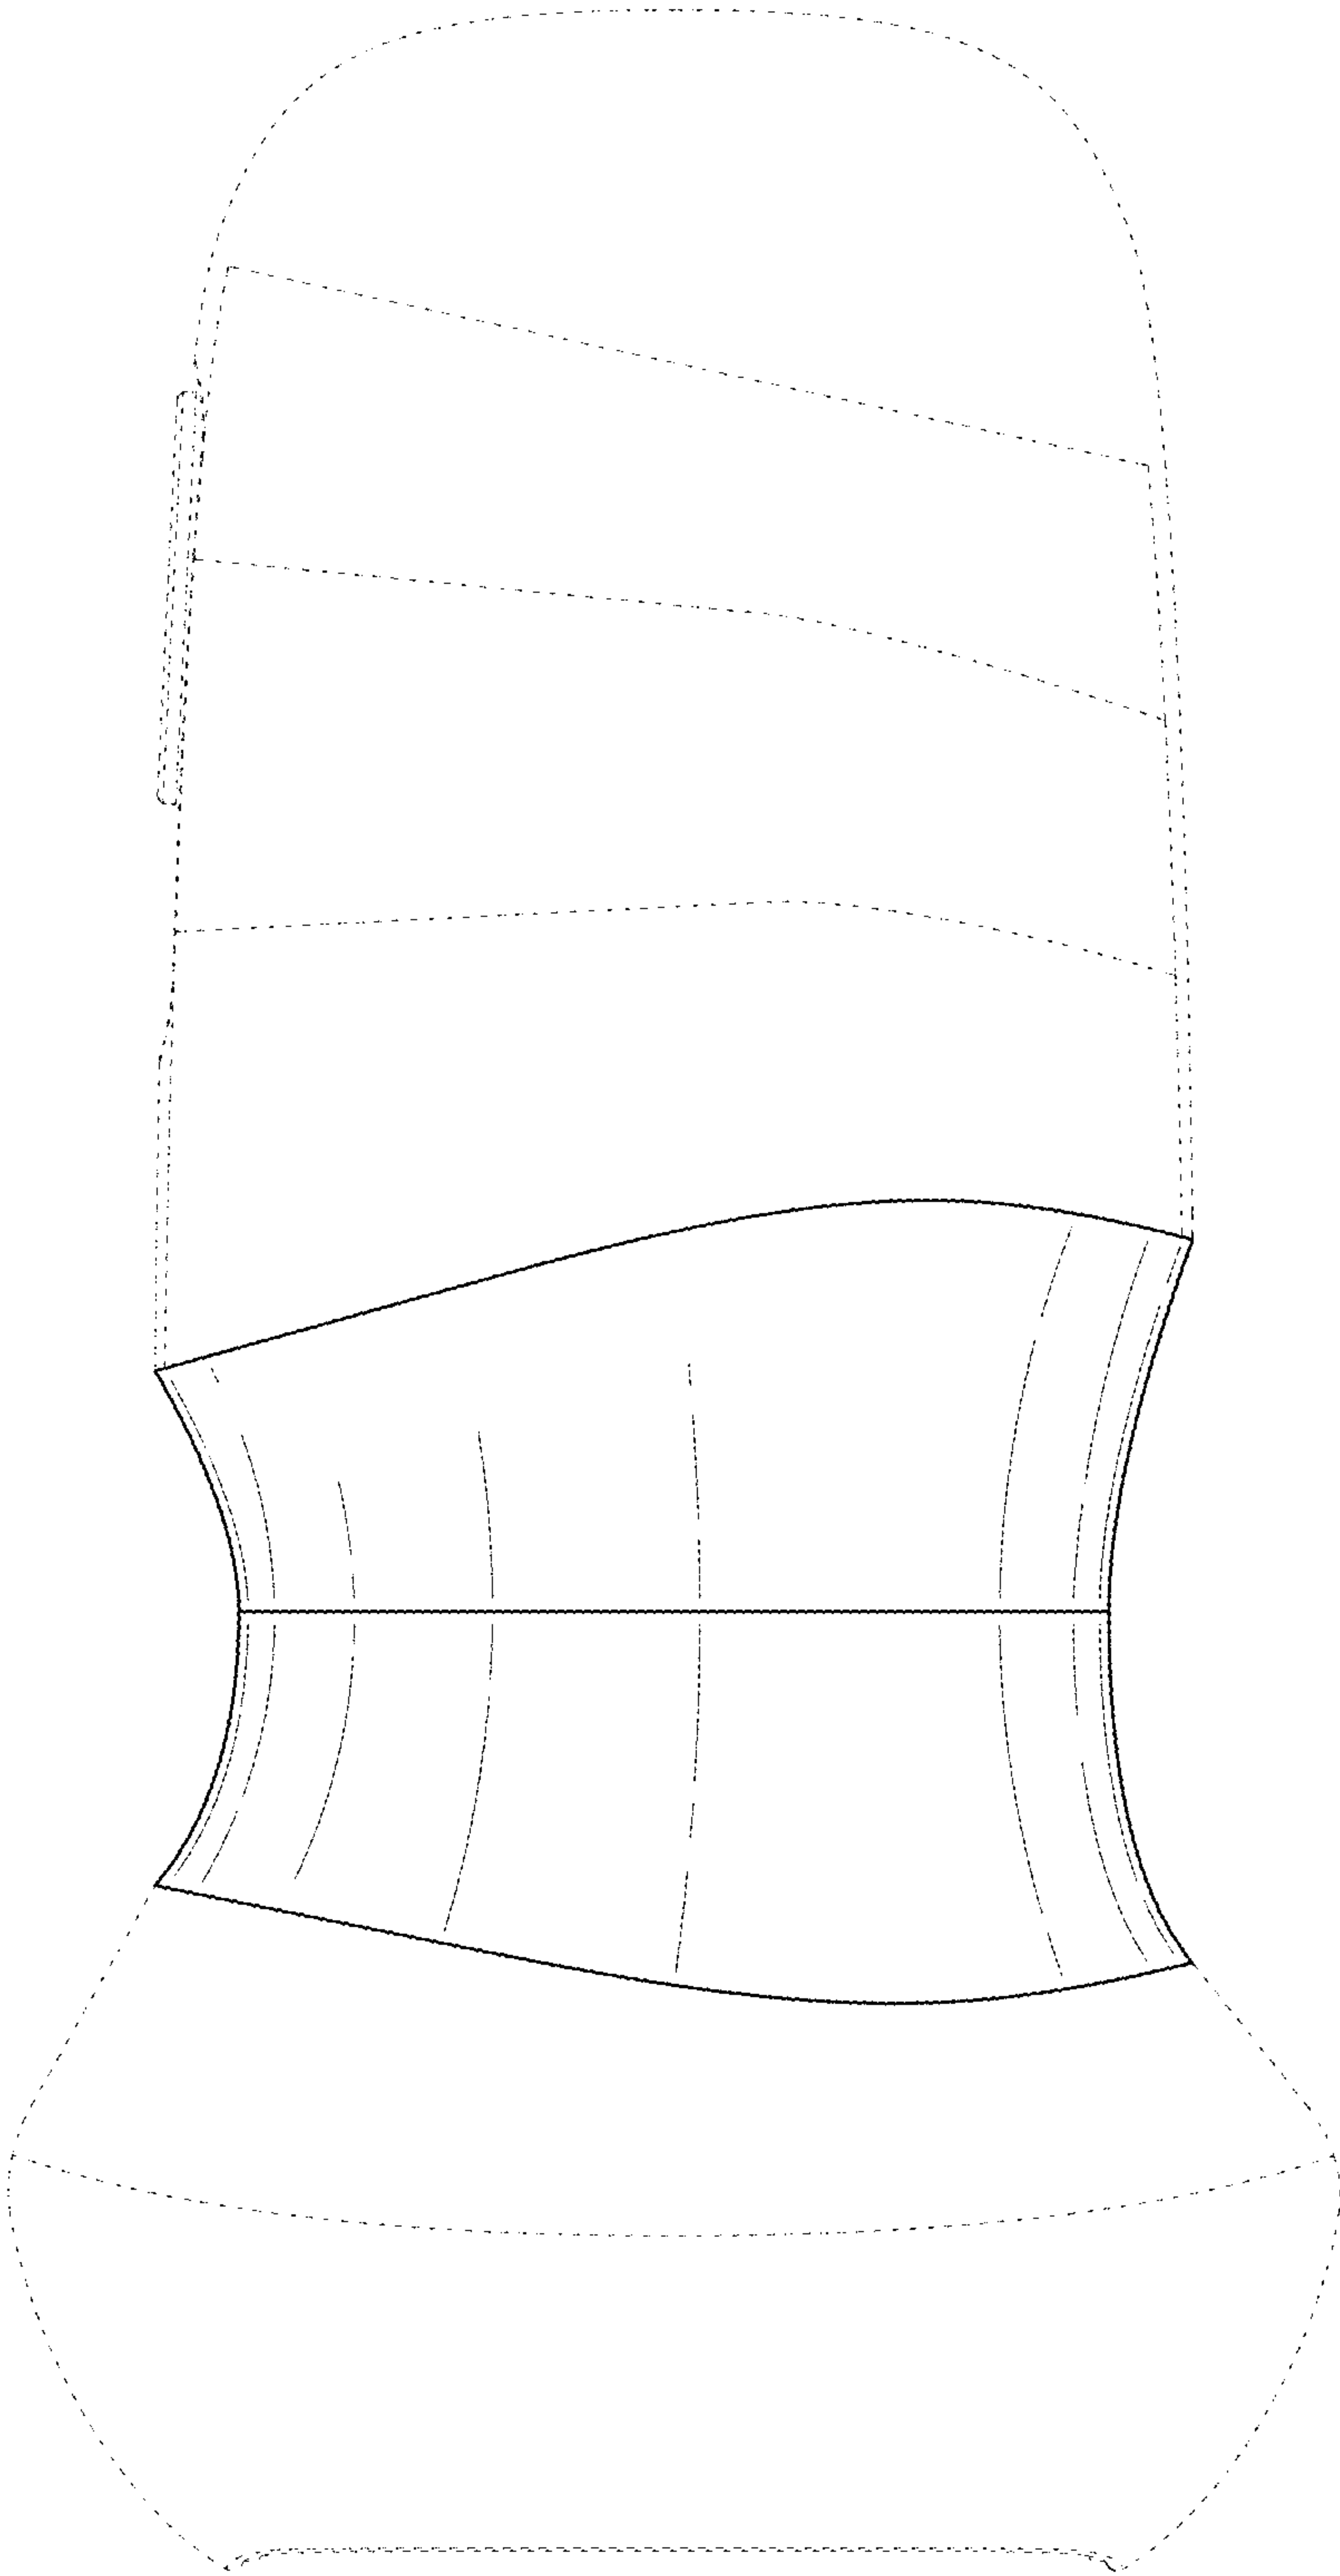


FIG. 4

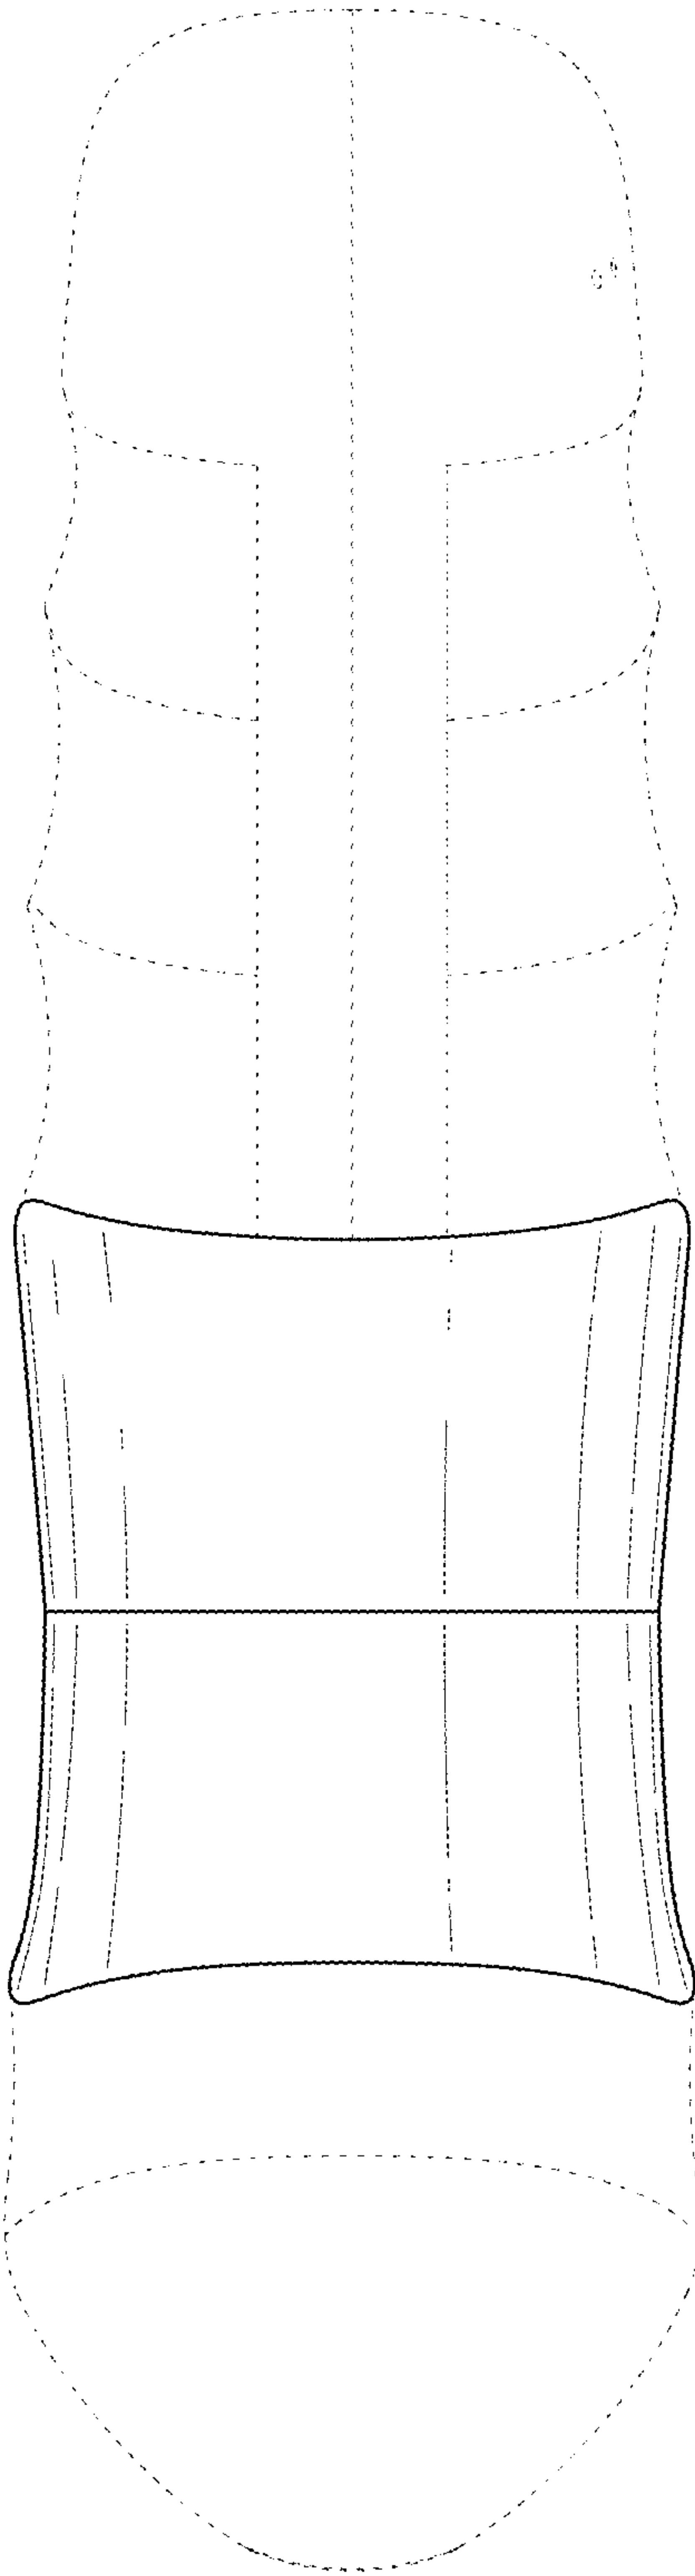


FIG. 5

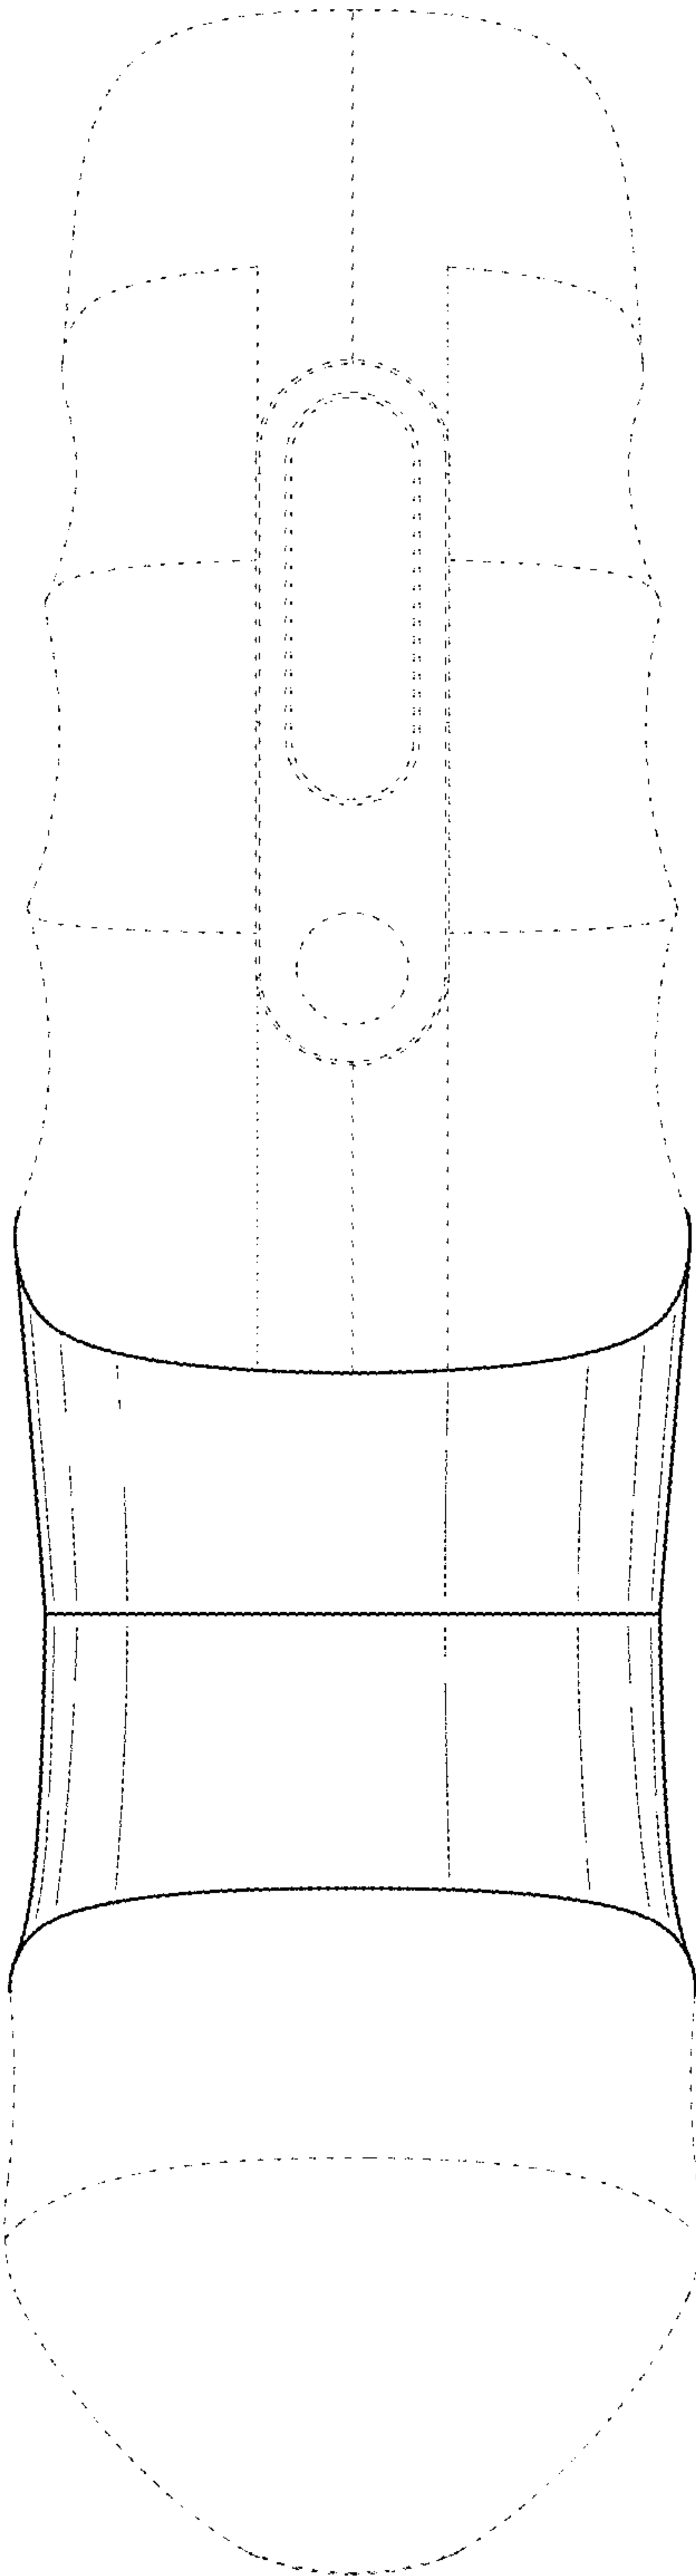


FIG. 6

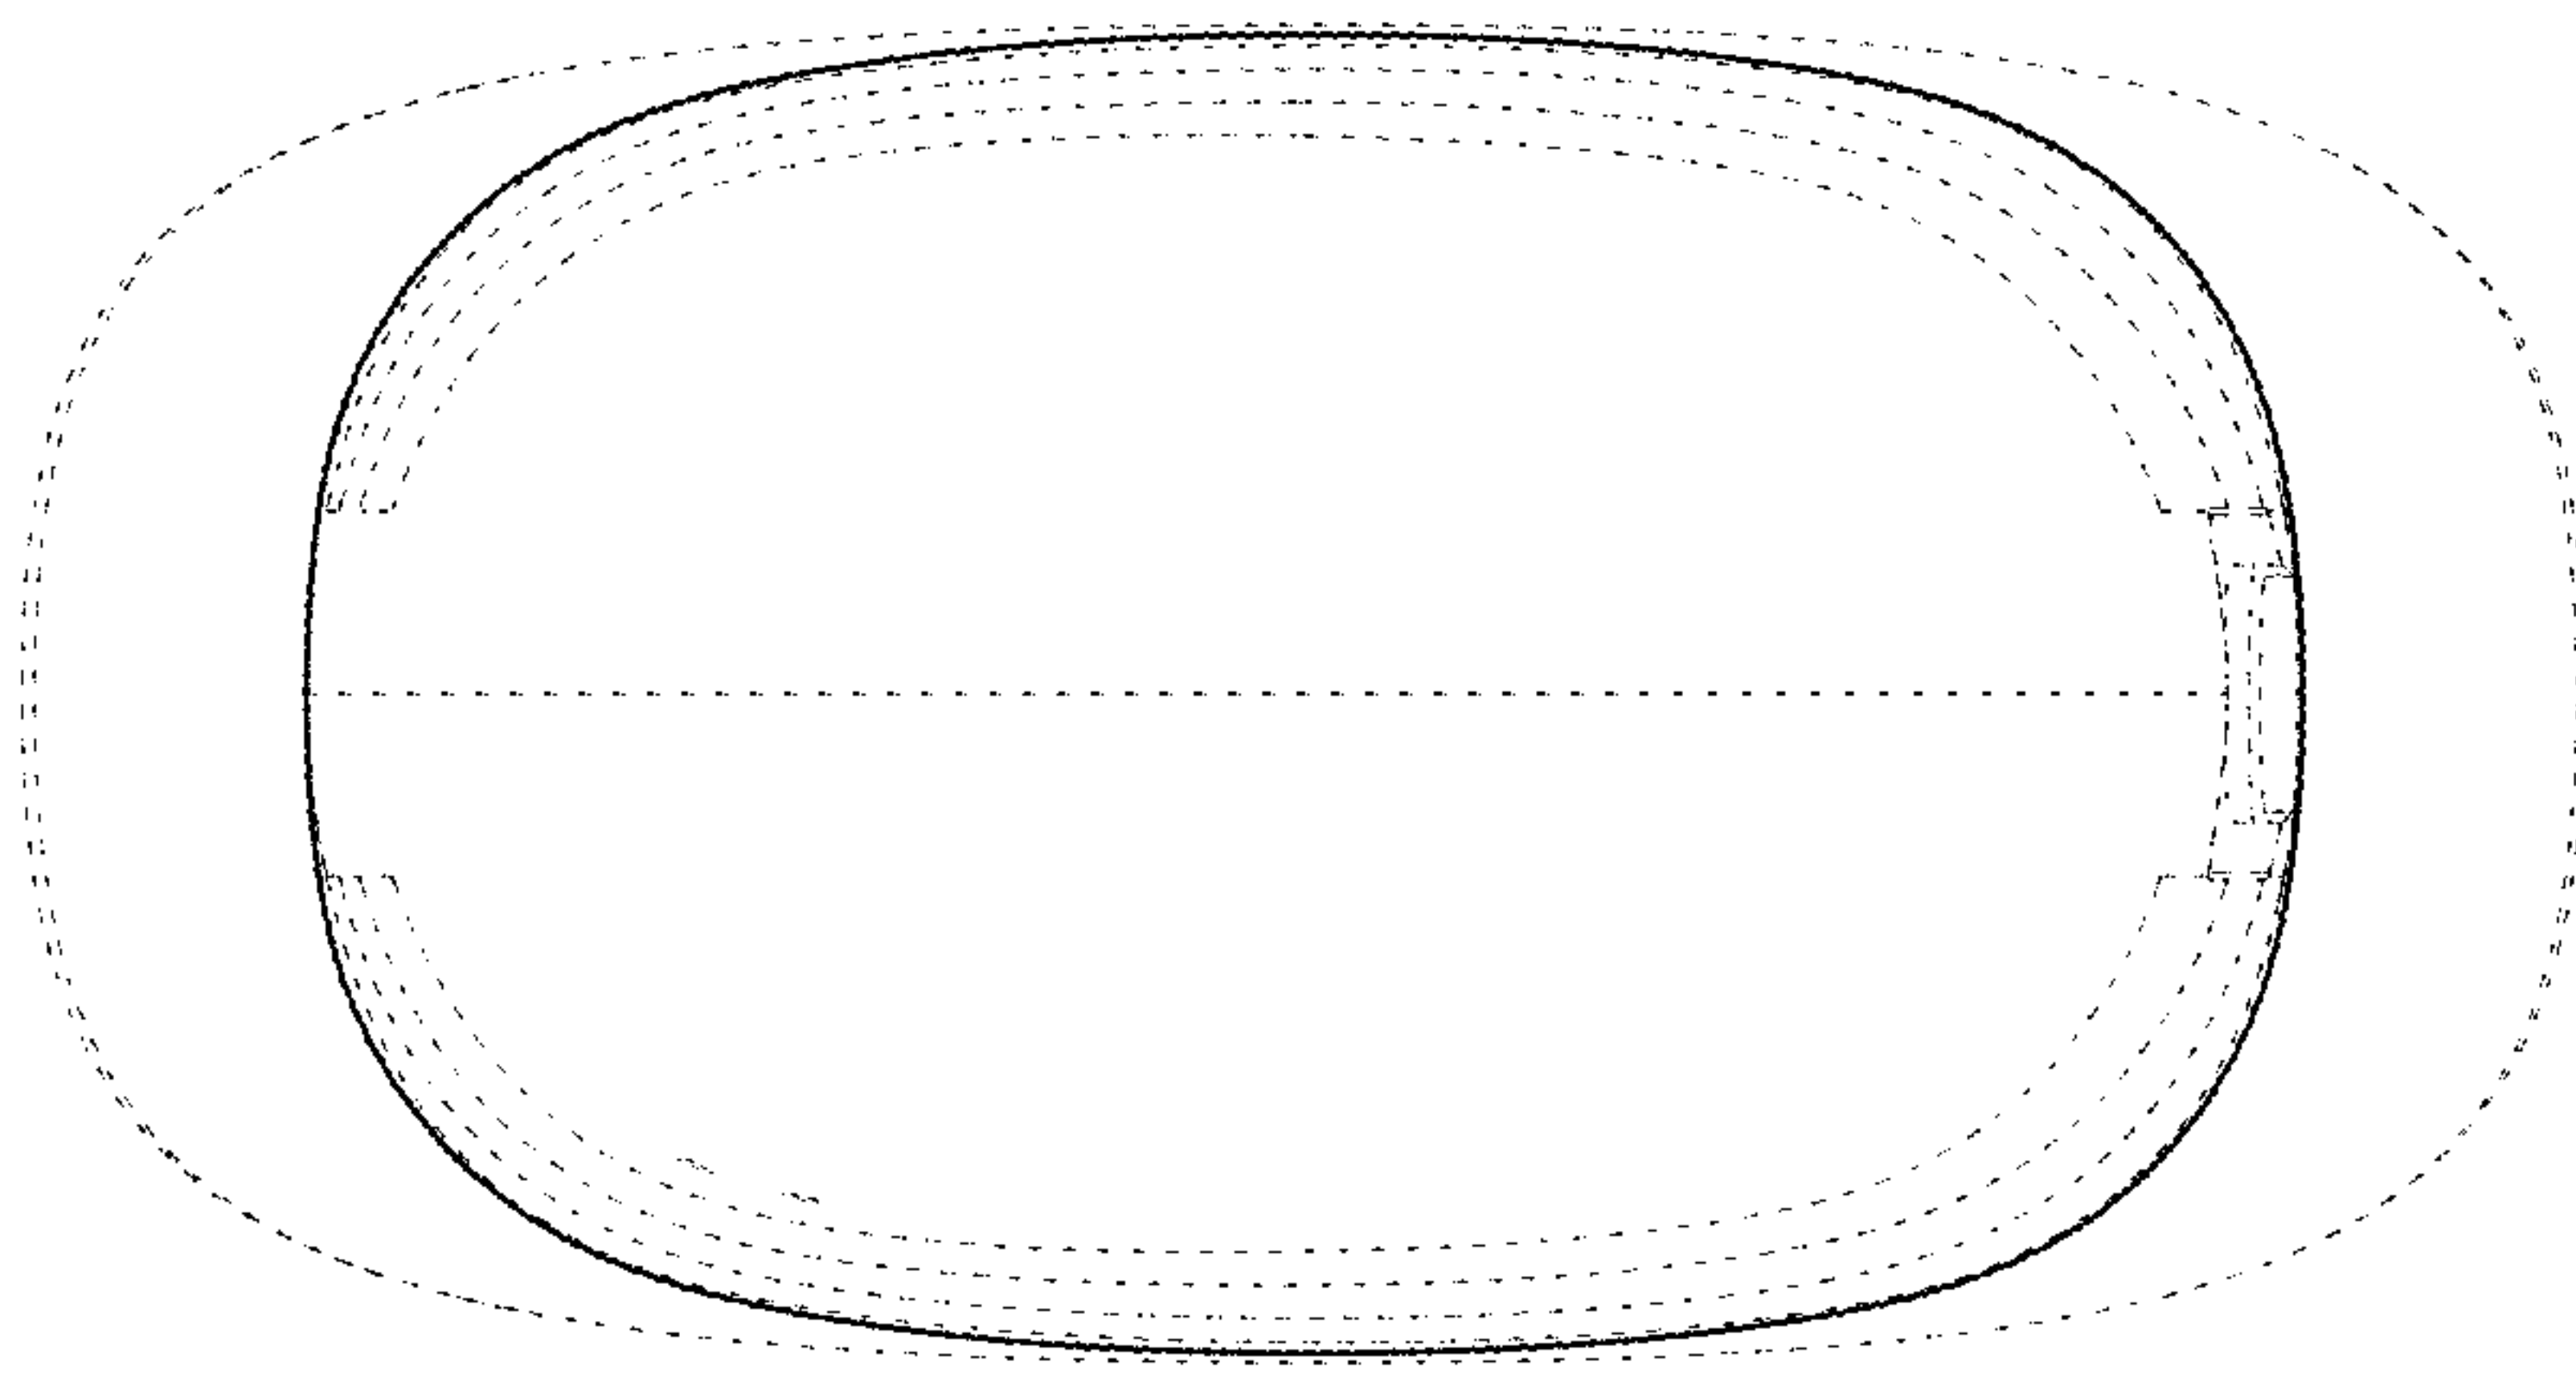


FIG. 7

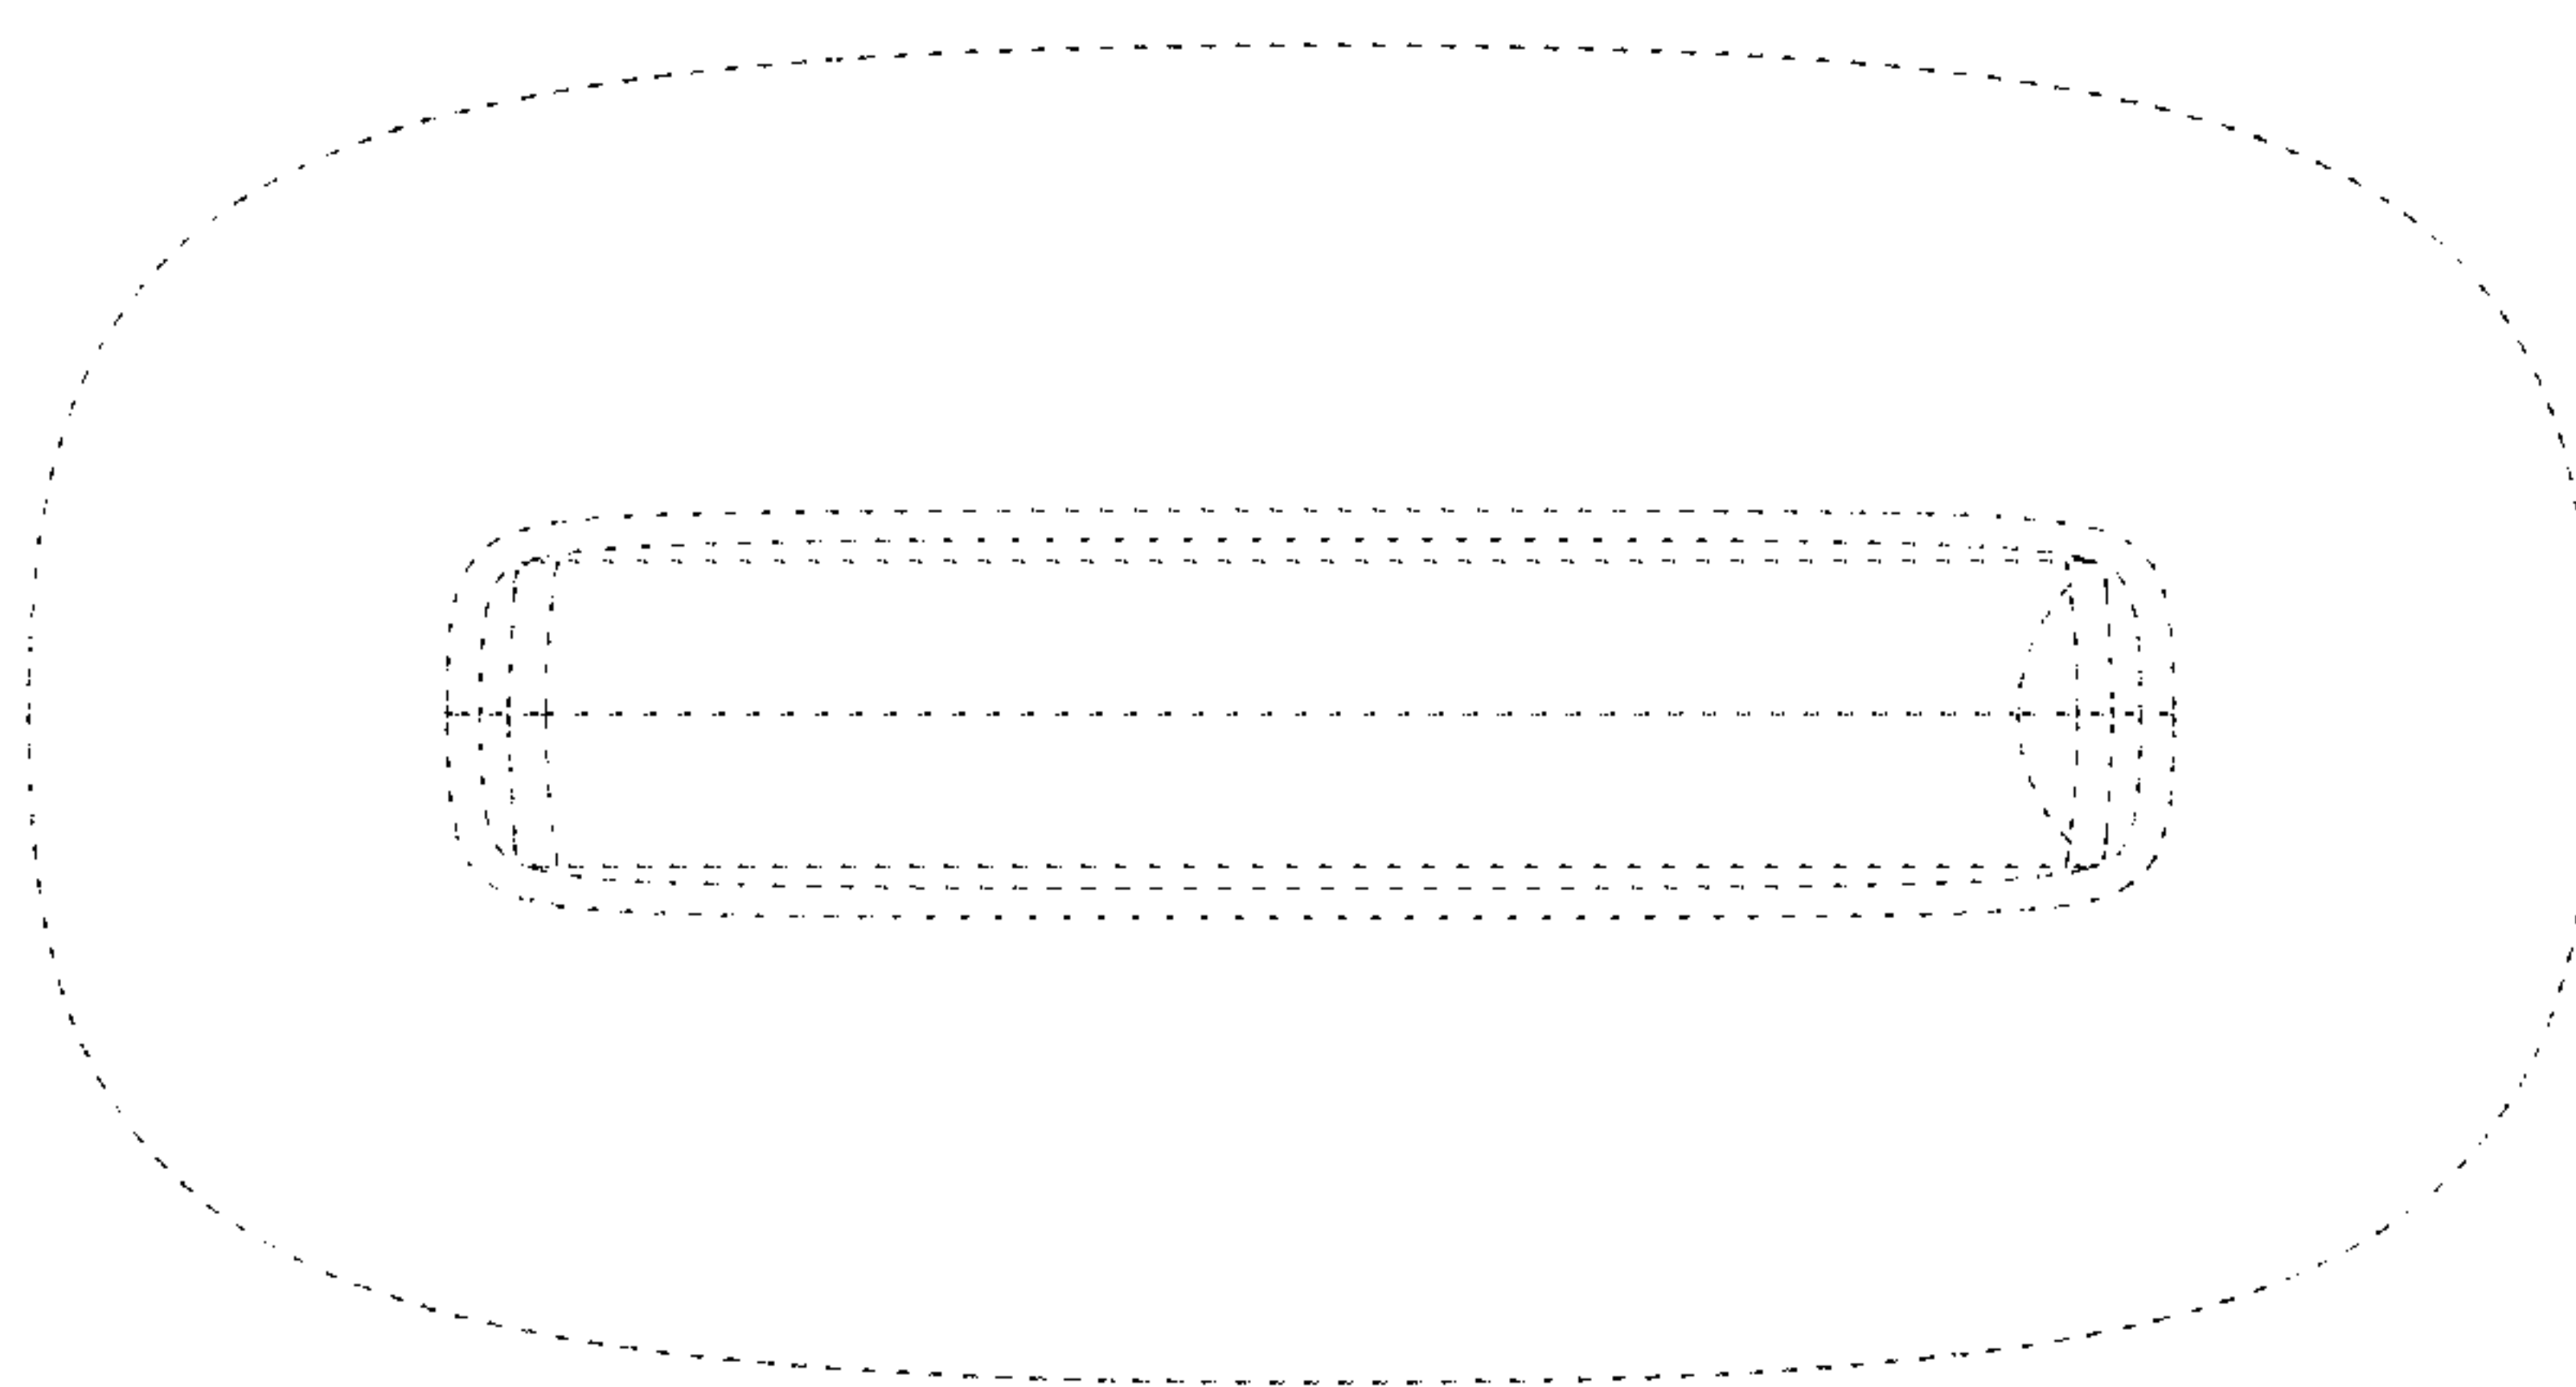


FIG. 8