



US0D1031021S

(12)

United States Design Patent

Choo et al.

(10)

Patent No.:

US D1,031,021 S

(45)

Date of Patent:

** Jun. 11, 2024

(54) CUSHION FRAME FOR RESPIRATORY MASK

(71) Applicant: ResMed Asia Pte. Ltd., Singapore (SG)

(72) Inventors: Kok Boon Choo, Singapore (SG); Han Cheng Lin, Singapore (SG); Jing Chen, Singapore (SG)

(73) Assignee: ResMed Asia Pte. Ltd., Singapore (SG)

(**) Term: 15 Years

(21) Appl. No.: 29/894,432

(22) Filed: Jun. 9, 2023

Related U.S. Application Data

(62) Division of application No. 29/733,384, filed on May 1, 2020, now Pat. No. Des. 1,003,428.

(51) LOC (14) Cl. 29-02

(52) U.S. Cl. USPC D24/110.4

(58) Field of Classification Search USPC D24/110, 110.1–110.6, 127 CPC A61M 16/06; A61M 16/0616; A61M 16/0622; A61M 16/0666; A61M 16/0672; A61M 16/0683 See application file for complete search history.

(56) References Cited

U.S. PATENT DOCUMENTS

D586,907 S	2/2009	Judson
D586,909 S	2/2009	Selvarajan
D597,199 S	7/2009	Smart
D623,288 S	9/2010	Lubke
D656,231 S	3/2012	Henry
D659,237 S	5/2012	Lubke
D664,250 S	7/2012	Scheiner

(Continued)

FOREIGN PATENT DOCUMENTS

CN	306935547	11/2021
CN	307174592	3/2022
KR	300930941.0000	11/2017

OTHER PUBLICATIONS

Dantanarayana et al., U.S. Appl. No. 29/666,398, filed Oct. 12, 2018 for “Respiratory Mask With Heat and Moisture Exchanger Unit”.

(Continued)

Primary Examiner — Daniel J Domino

Assistant Examiner — Lee D. Starr

(74) Attorney, Agent, or Firm — Nixon & Vanderhye P.C.


(57) CLAIM

The ornamental design for a cushion frame for respiratory mask, as shown and described.

DESCRIPTION

FIG. 1 is a front perspective view of a cushion frame for respiratory mask showing an embodiment of our new design; FIG. 2 is an enlarged front perspective view thereof in isolation; FIG. 3 is a front view thereof; FIG. 4 is a rear view thereof; FIG. 5 is a top view thereof; FIG. 6 is a bottom view thereof; FIG. 7 is a left side view thereof; FIG. 8 is a right side view thereof; and, FIG. 9 is a rear perspective view thereof. The broken lines in the FIGS. 2, 3, and 7-9 depict portions of the cushion frame for respiratory mask and form no part of the claimed design. All other broken lines depict environmental structure and form no part of the claimed design.

1 Claim, 6 Drawing Sheets

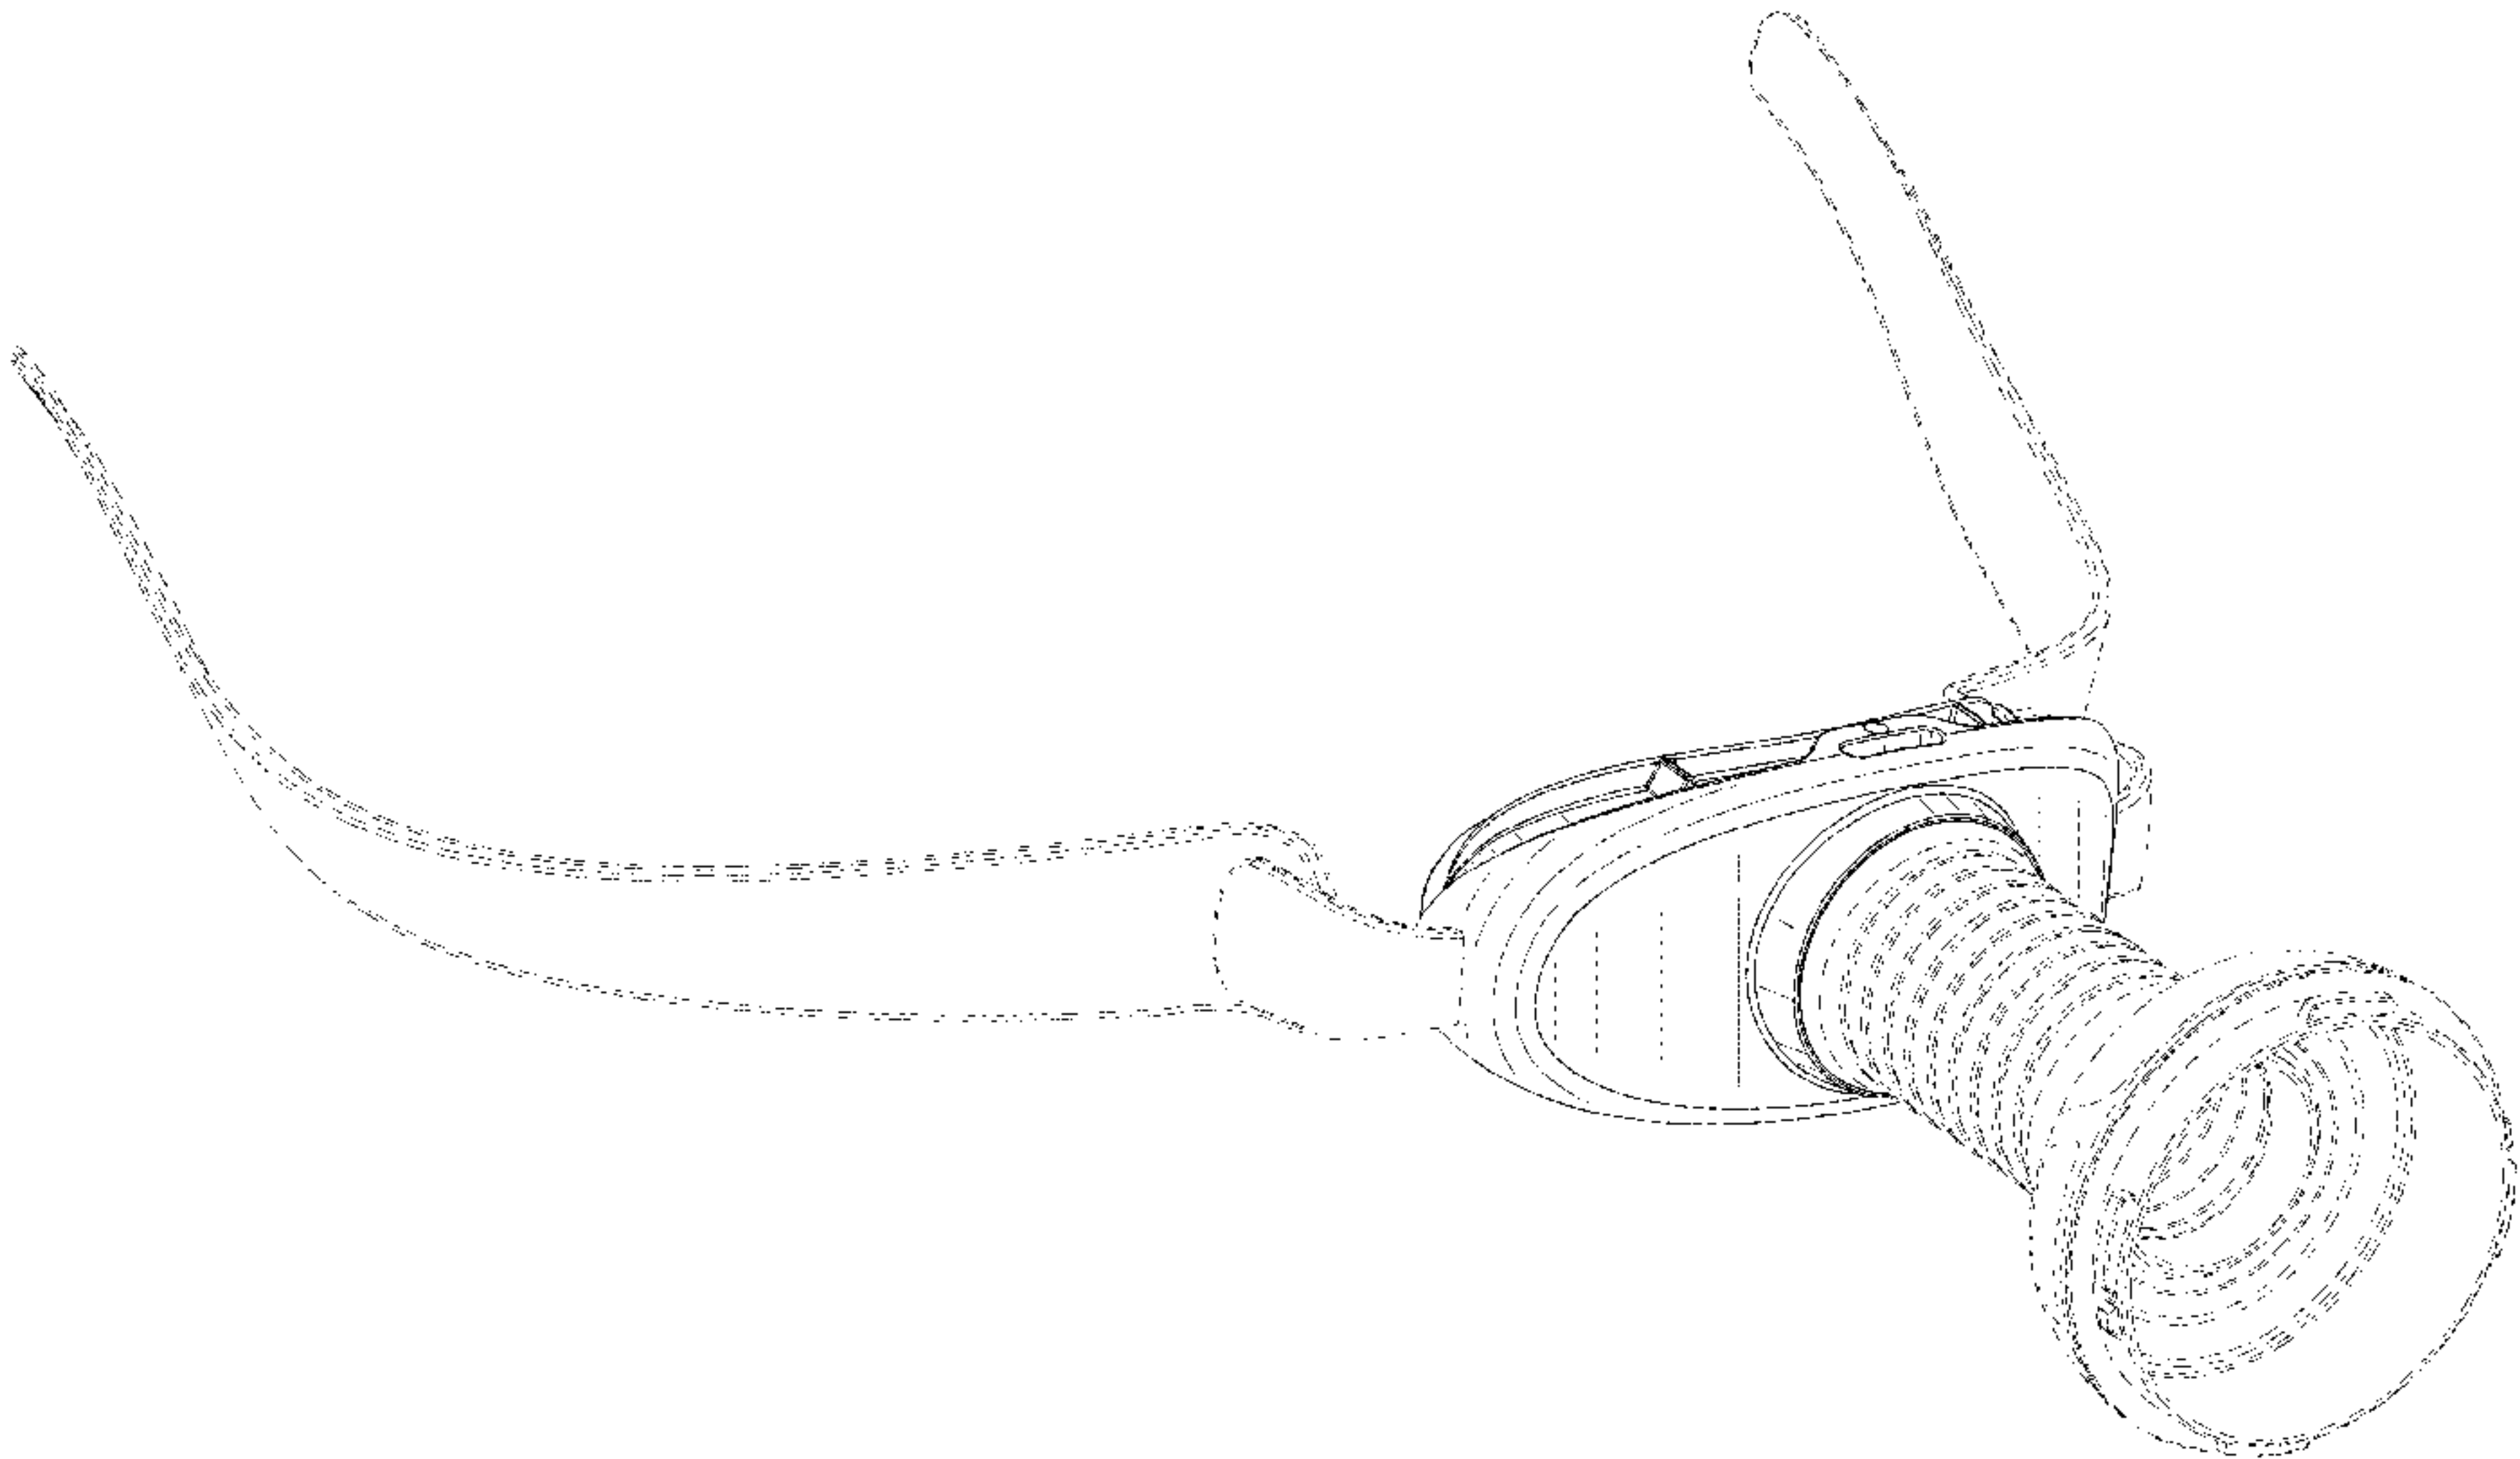

(56)

References Cited

U.S. PATENT DOCUMENTS

D669,576 S

10/2012

Smart

8,402,971 B2

3/2013

Scheiner

D691,712 S

10/2013

Judson

D692,554 S

10/2013

Siew

D704,329 S

5/2014

Collazo

D708,736 S

7/2014

Judson

D737,953 S

9/2015

Wells

D740,935 S

10/2015

Cullen

D743,535 S

11/2015

Wells

9,211,388 B2

12/2015

Swift

D751,687 S

3/2016

Daly

D757,252 S

5/2016

Von Moger

D757,927 S

5/2016

Lubke

D764,049 S

8/2016

Cullen

D770,036 S

10/2016

Walls

D771,238 S

11/2016

Scheiner

D787,661 S

5/2017

Edwards

D787,662 S

5/2017

Guney

D794,772 S

8/2017

Cullen

D805,630 S

12/2017

Formica

D808,516 S

1/2018

Edwards

D820,432 S

6/2018

Scheiner

D851,749 S

6/2019

Siew

D858,746 S

9/2019

Lee

D865,158 S

10/2019

Khera

10,543,332 B2

1/2020

Scheiner

D882,757 S

4/2020

Dantanarayana et al.

D895,103 S

9/2020

Dantanarayana

D927,682 S

8/2021

Khera

D930,148 S

9/2021

Dantanarayana

D938,576 S

12/2021

Khera

D950,708 S

5/2022

Dantanarayana

D958,970 S

7/2022

Eves

11,554,236 B2

1/2023

Haibach

11,583,651 B2 *

2/2023

Wells

A61M 16/06

11,612,711 B2 *

3/2023

Scheiner

A61M 16/06

128/206.21

D1,003,428 S *

10/2023

Choo

D24/110.4

2005/0155604 A1

7/2005

Ging

2006/0174887 A1

8/2006

Chandran

2012/0090622 A1

4/2012

Chang

2014/0000614 A1

1/2014

Chang

2016/0051784 A1

2/2016

Eury

2016/0082214 A1

3/2016

Barlow

2017/0000964 A1

1/2017

Shafer

2017/0368285 A1

12/2017

Wood

2018/0001044 A1

1/2018

Stephens

2018/0326173 A1

11/2018

Ewers

2020/0197649 A1

6/2020

Haibach

2022/0023572 A1

1/2022

Henry

2023/0057539 A1 *

2/2023

Chien

A61M 16/0816

OTHER PUBLICATIONS

Choo et al., U.S. Appl. No. 29/733,384, filed May 1, 2020, for “Respiratory Mask With Air Delivery Adapter,” (parent application).

ResMed AirFit N30 Nasal CPAP Mask with Headgear. Oldest review date: Feb. 29, 2020. Retrieval date: Dec. 8, 2022; retrieved from internet: <https://www.directhomemedical.com/airfit-n30-nasal-cpap-mask-resmedhtml> (Year: 2020).

ResMed AirMini Connector for AirFit P10 Series Nasal Pillow CPAP Masks. Oldest review date: Mar. 14, 2020. Retrieval date: Dec. 8, 2022, retrieved from internet: <https://www.directhomemedical.com/airmini-airfit-p10-nasal-pillow-mask-connector.html>, (Year: 2020).

ResMed AirFit N30: How to fit your slip-on nasal CPAP mask posted by ResMed. Youtube. Posting date: Oct. 21, 2019. Retrieval date: Dec. 8, 2022. Retrieved from internet: https://www.youtube.com/watch?v=_wqBYmYXWZ4 (Year: 2019).

ResMed Airfit N30 posted by Medgadget. Youtube. Posting date: Oct. 21, 2019. Retrieval date: Dec. 8, 2022. Retrieved from internet: https://www.youtube.com/watch?v=21_UXLmwZU4 (Year: 2019).

* cited by examiner

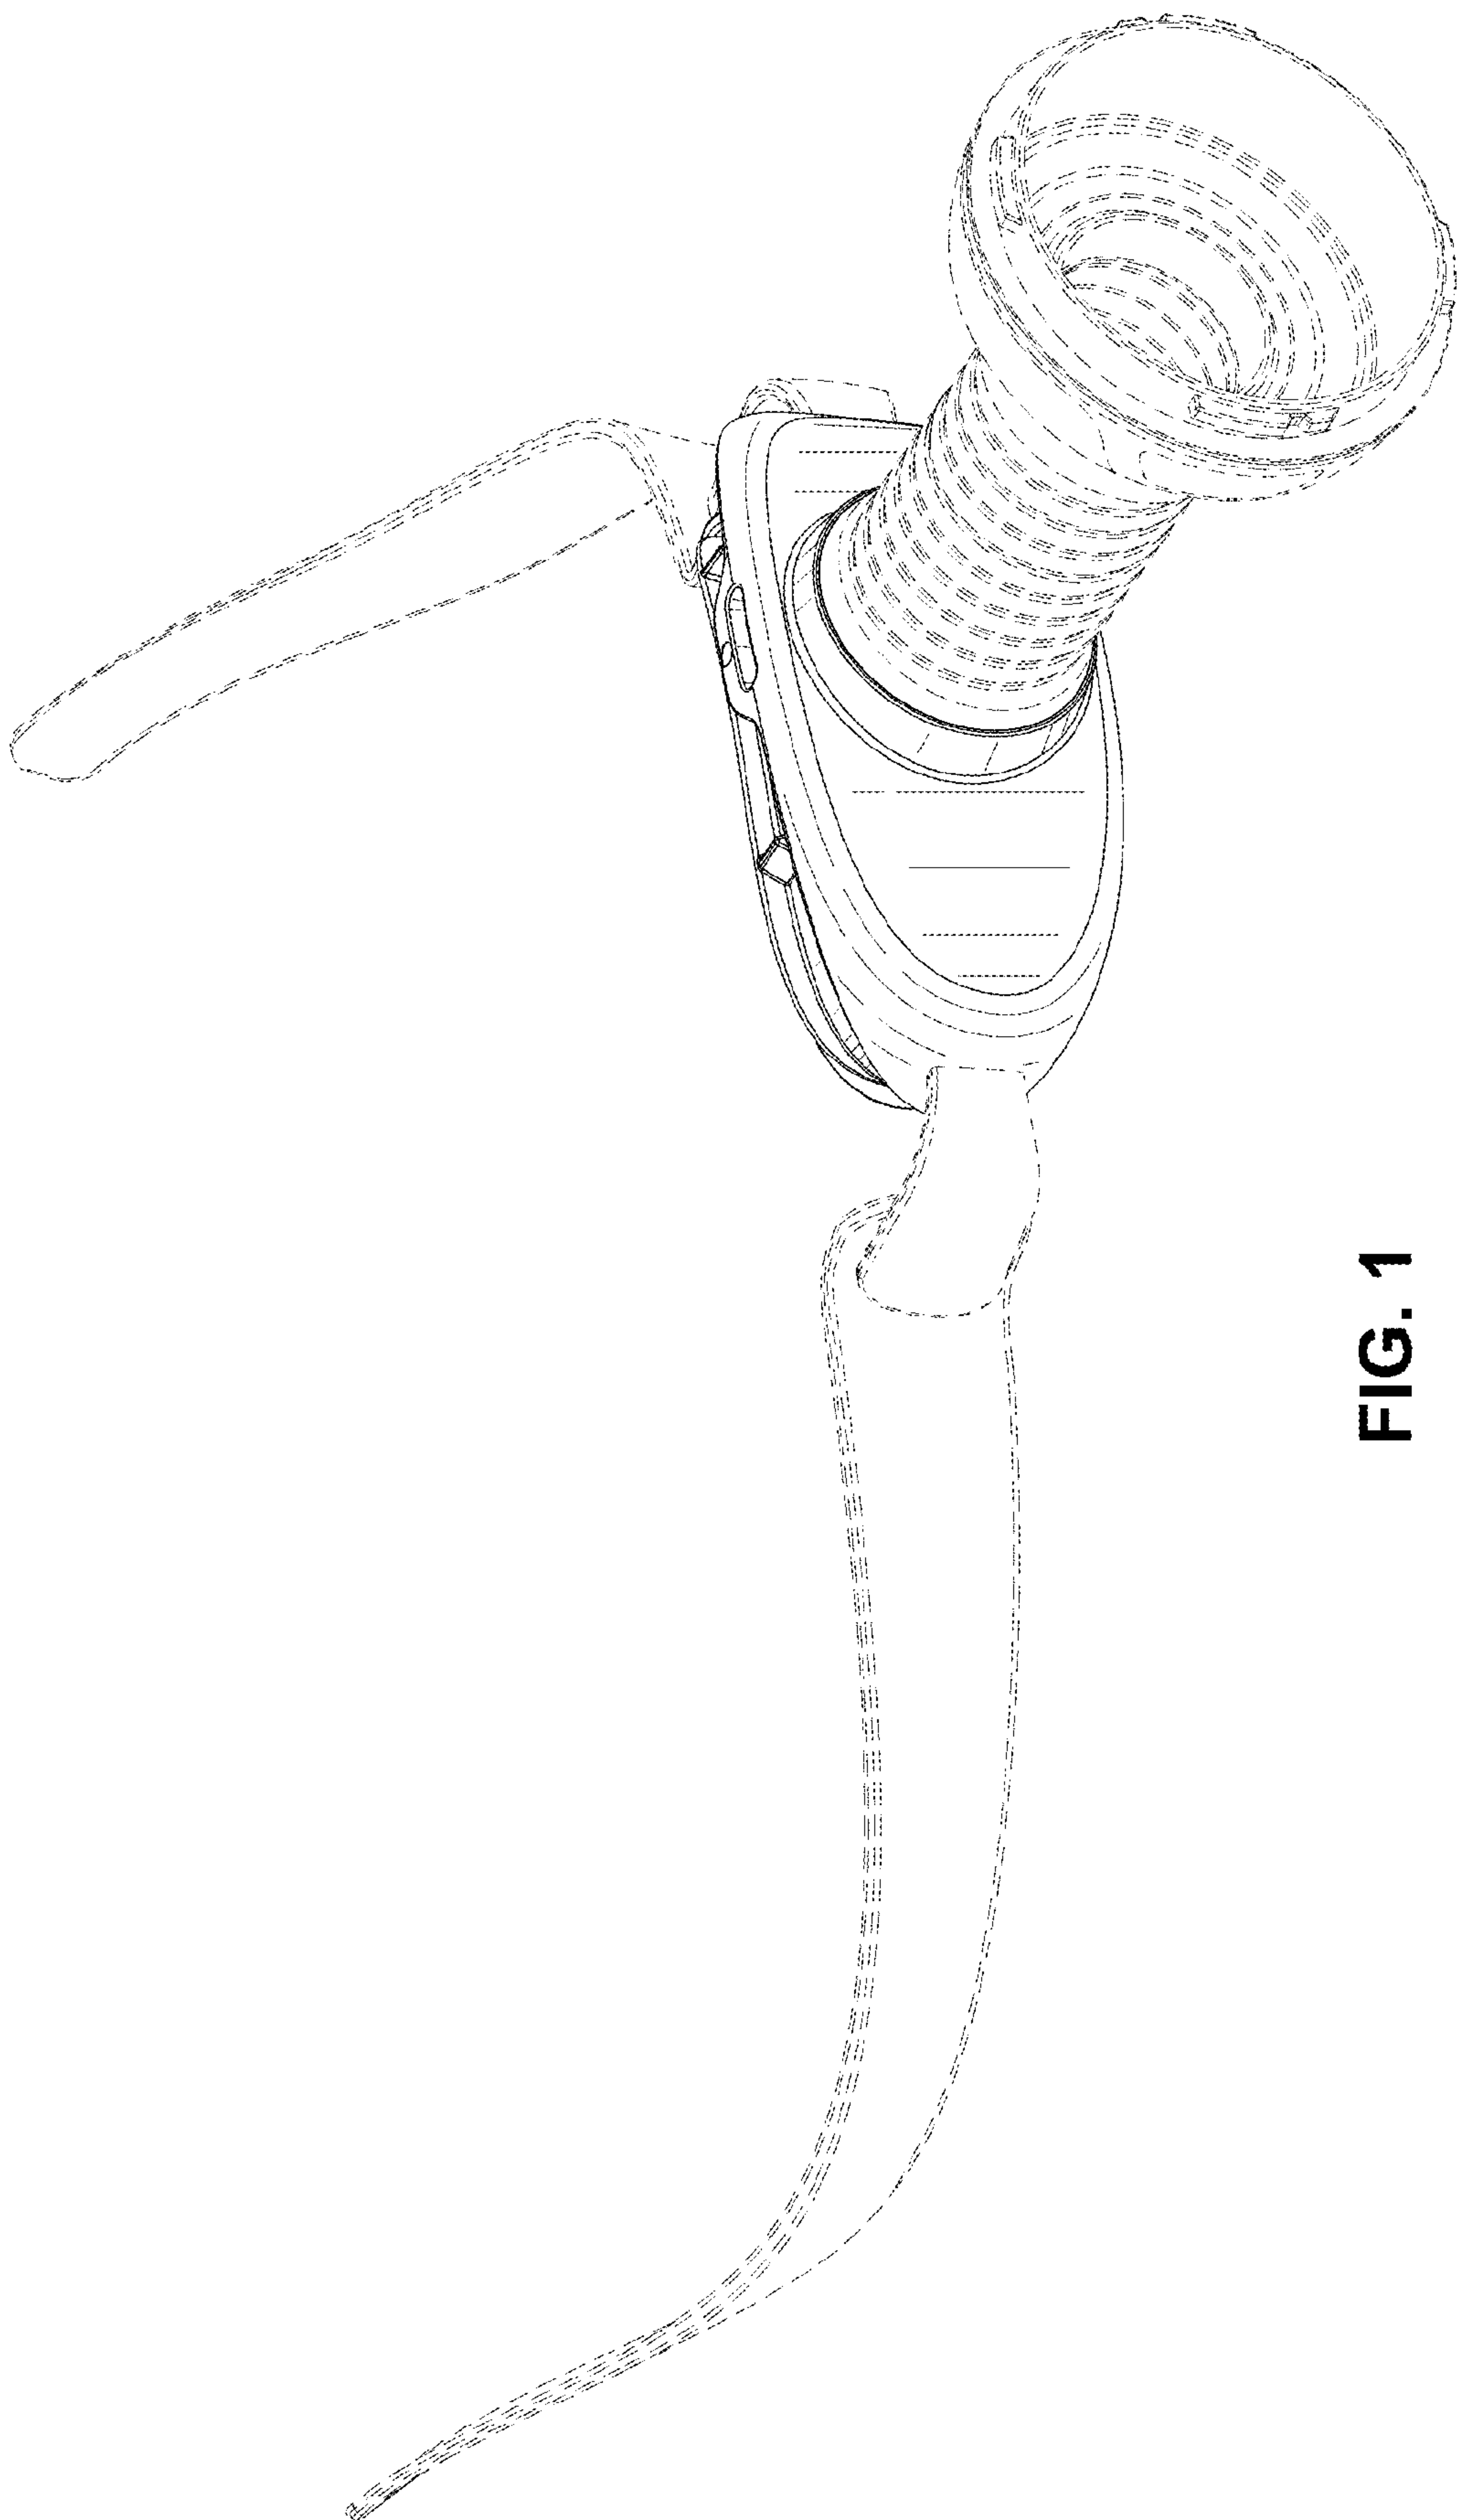


FIG. 1

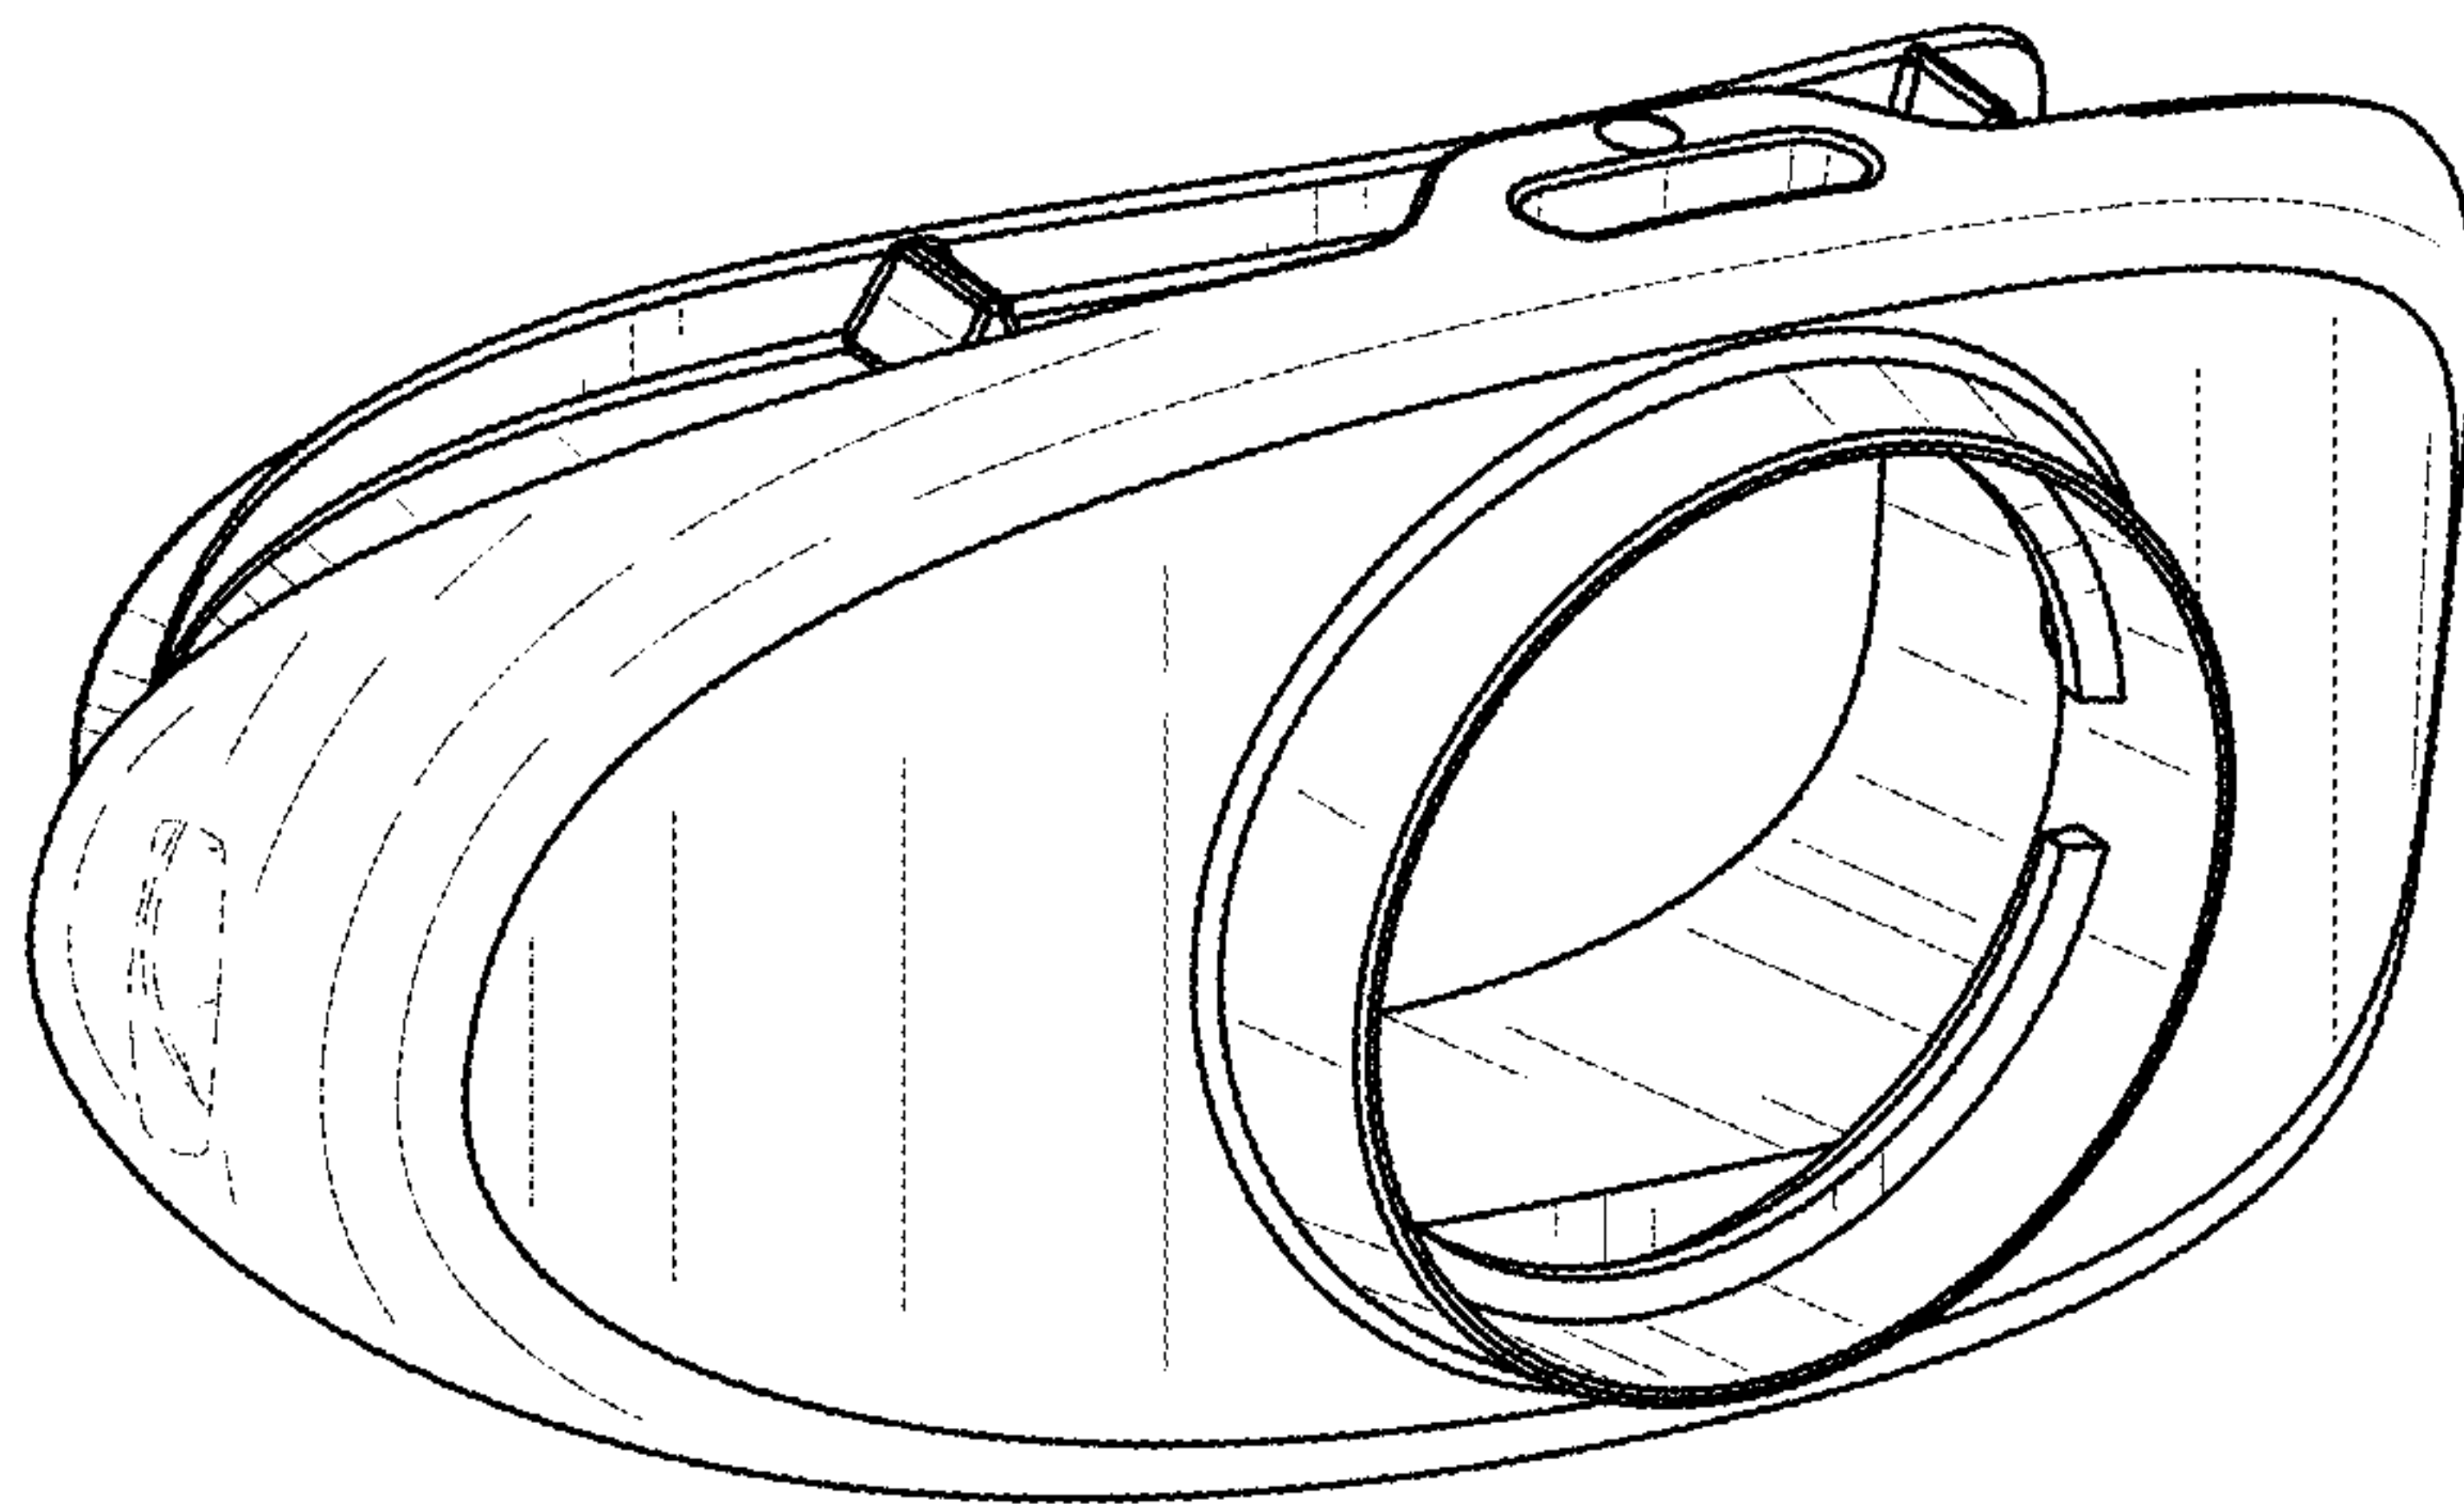


FIG. 2

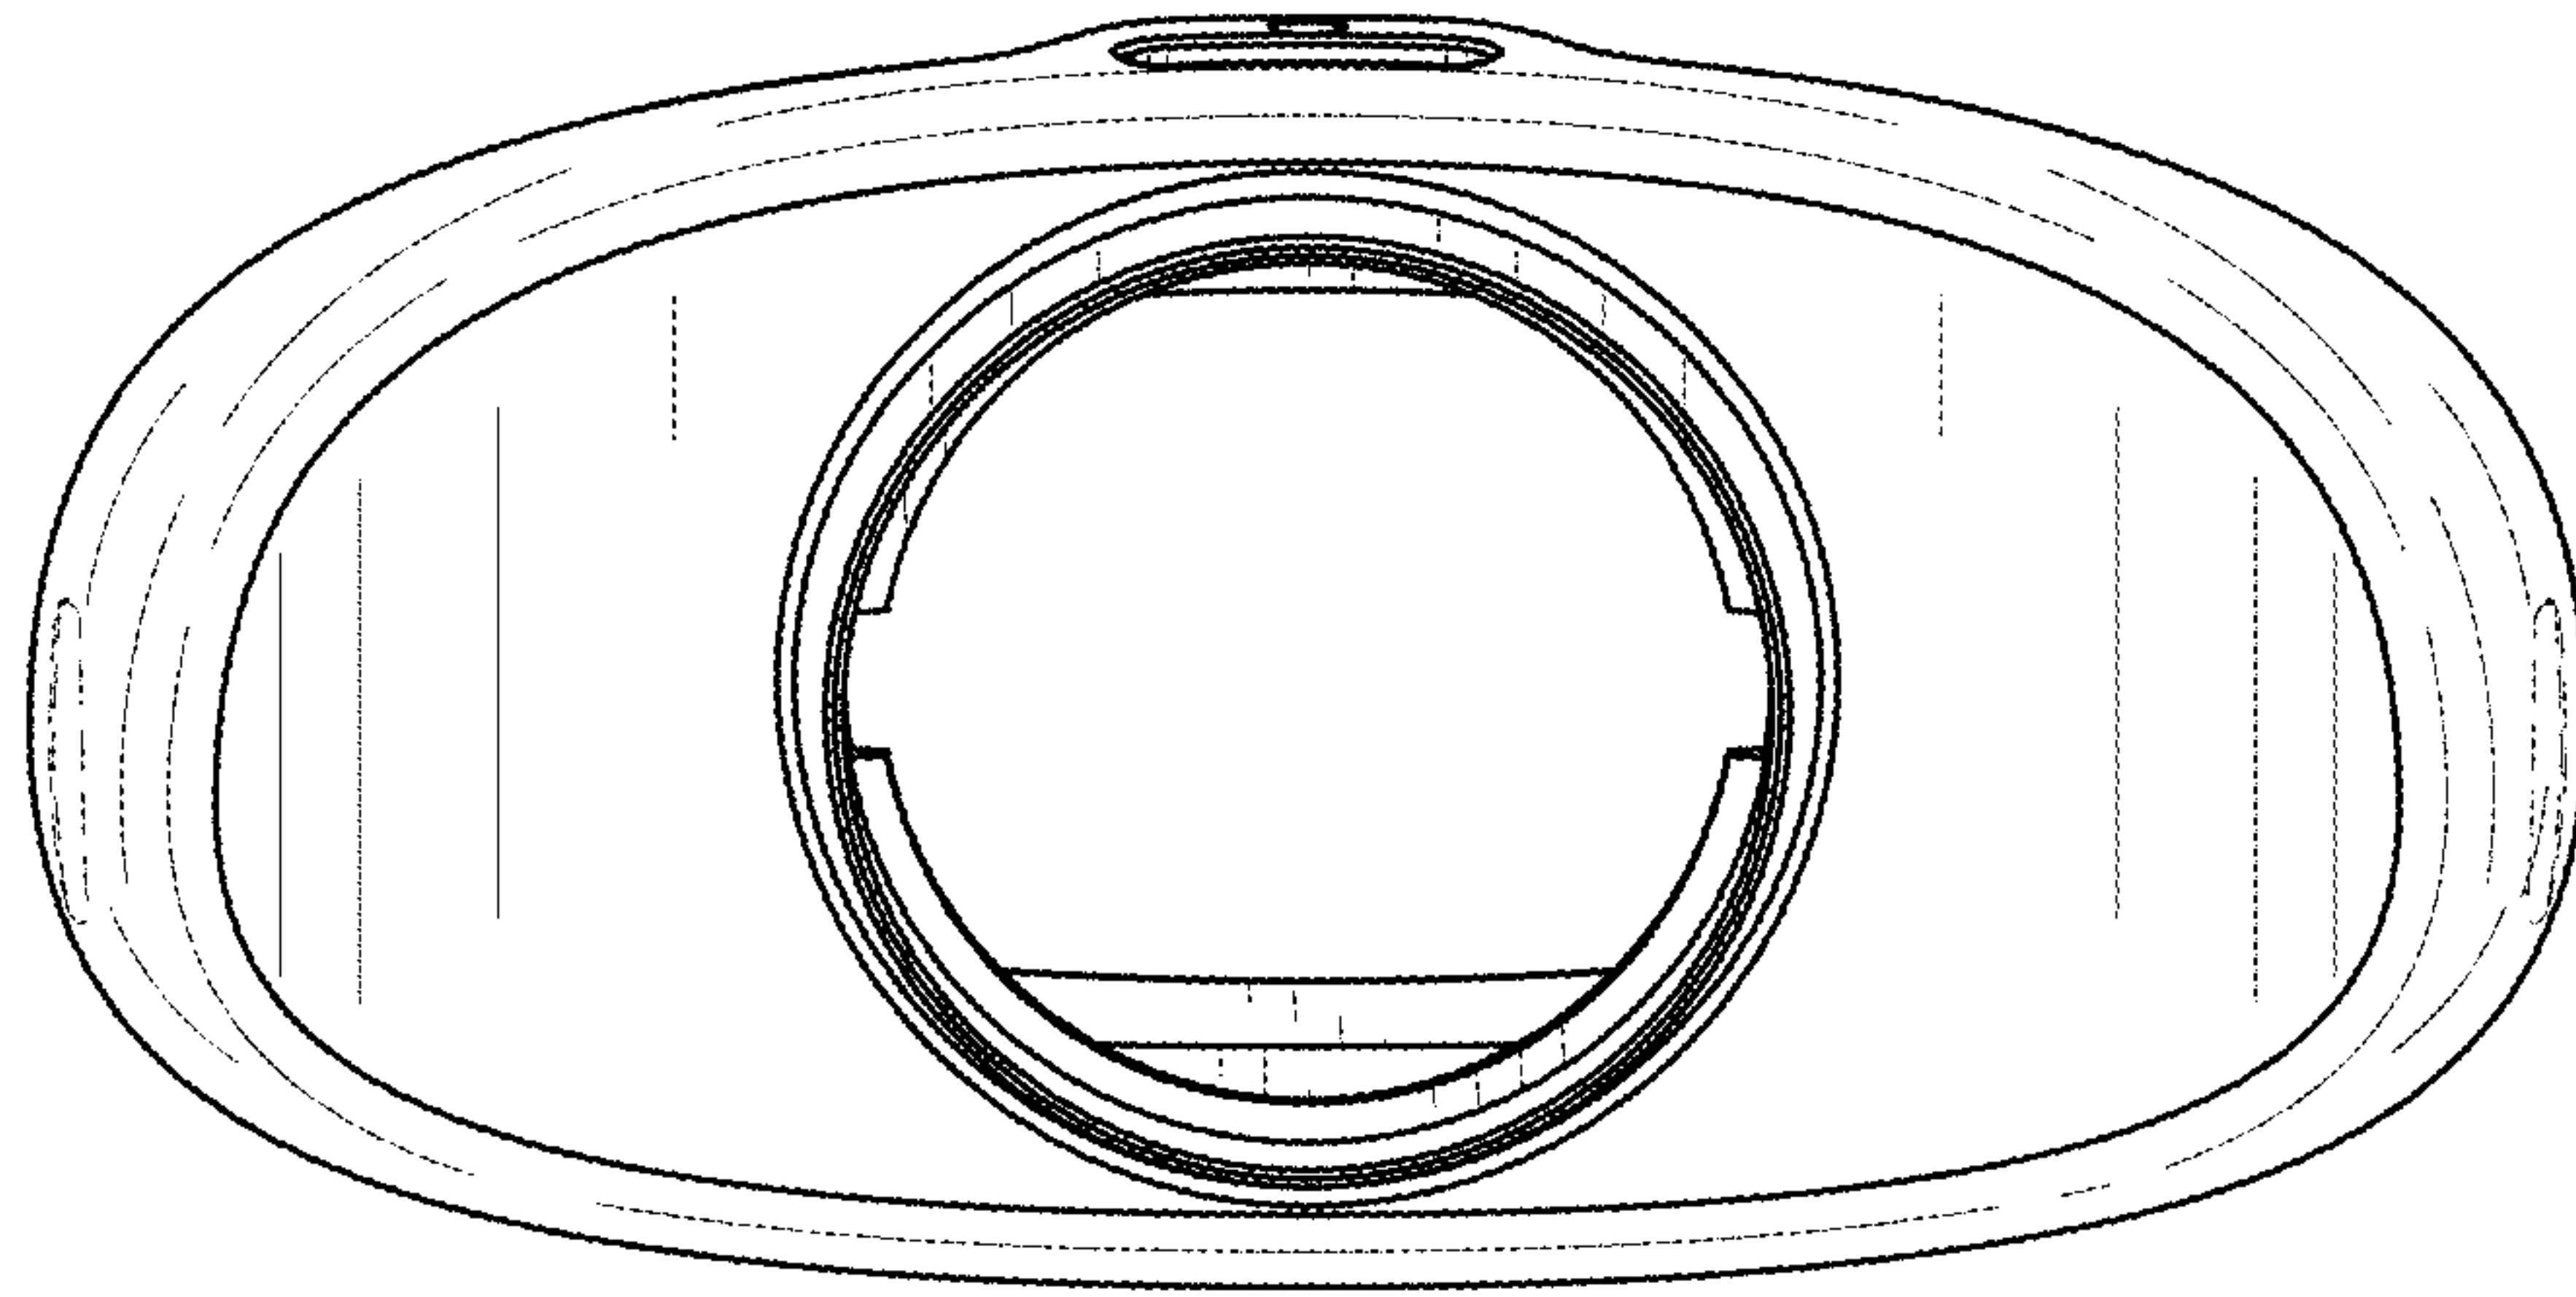


FIG. 3

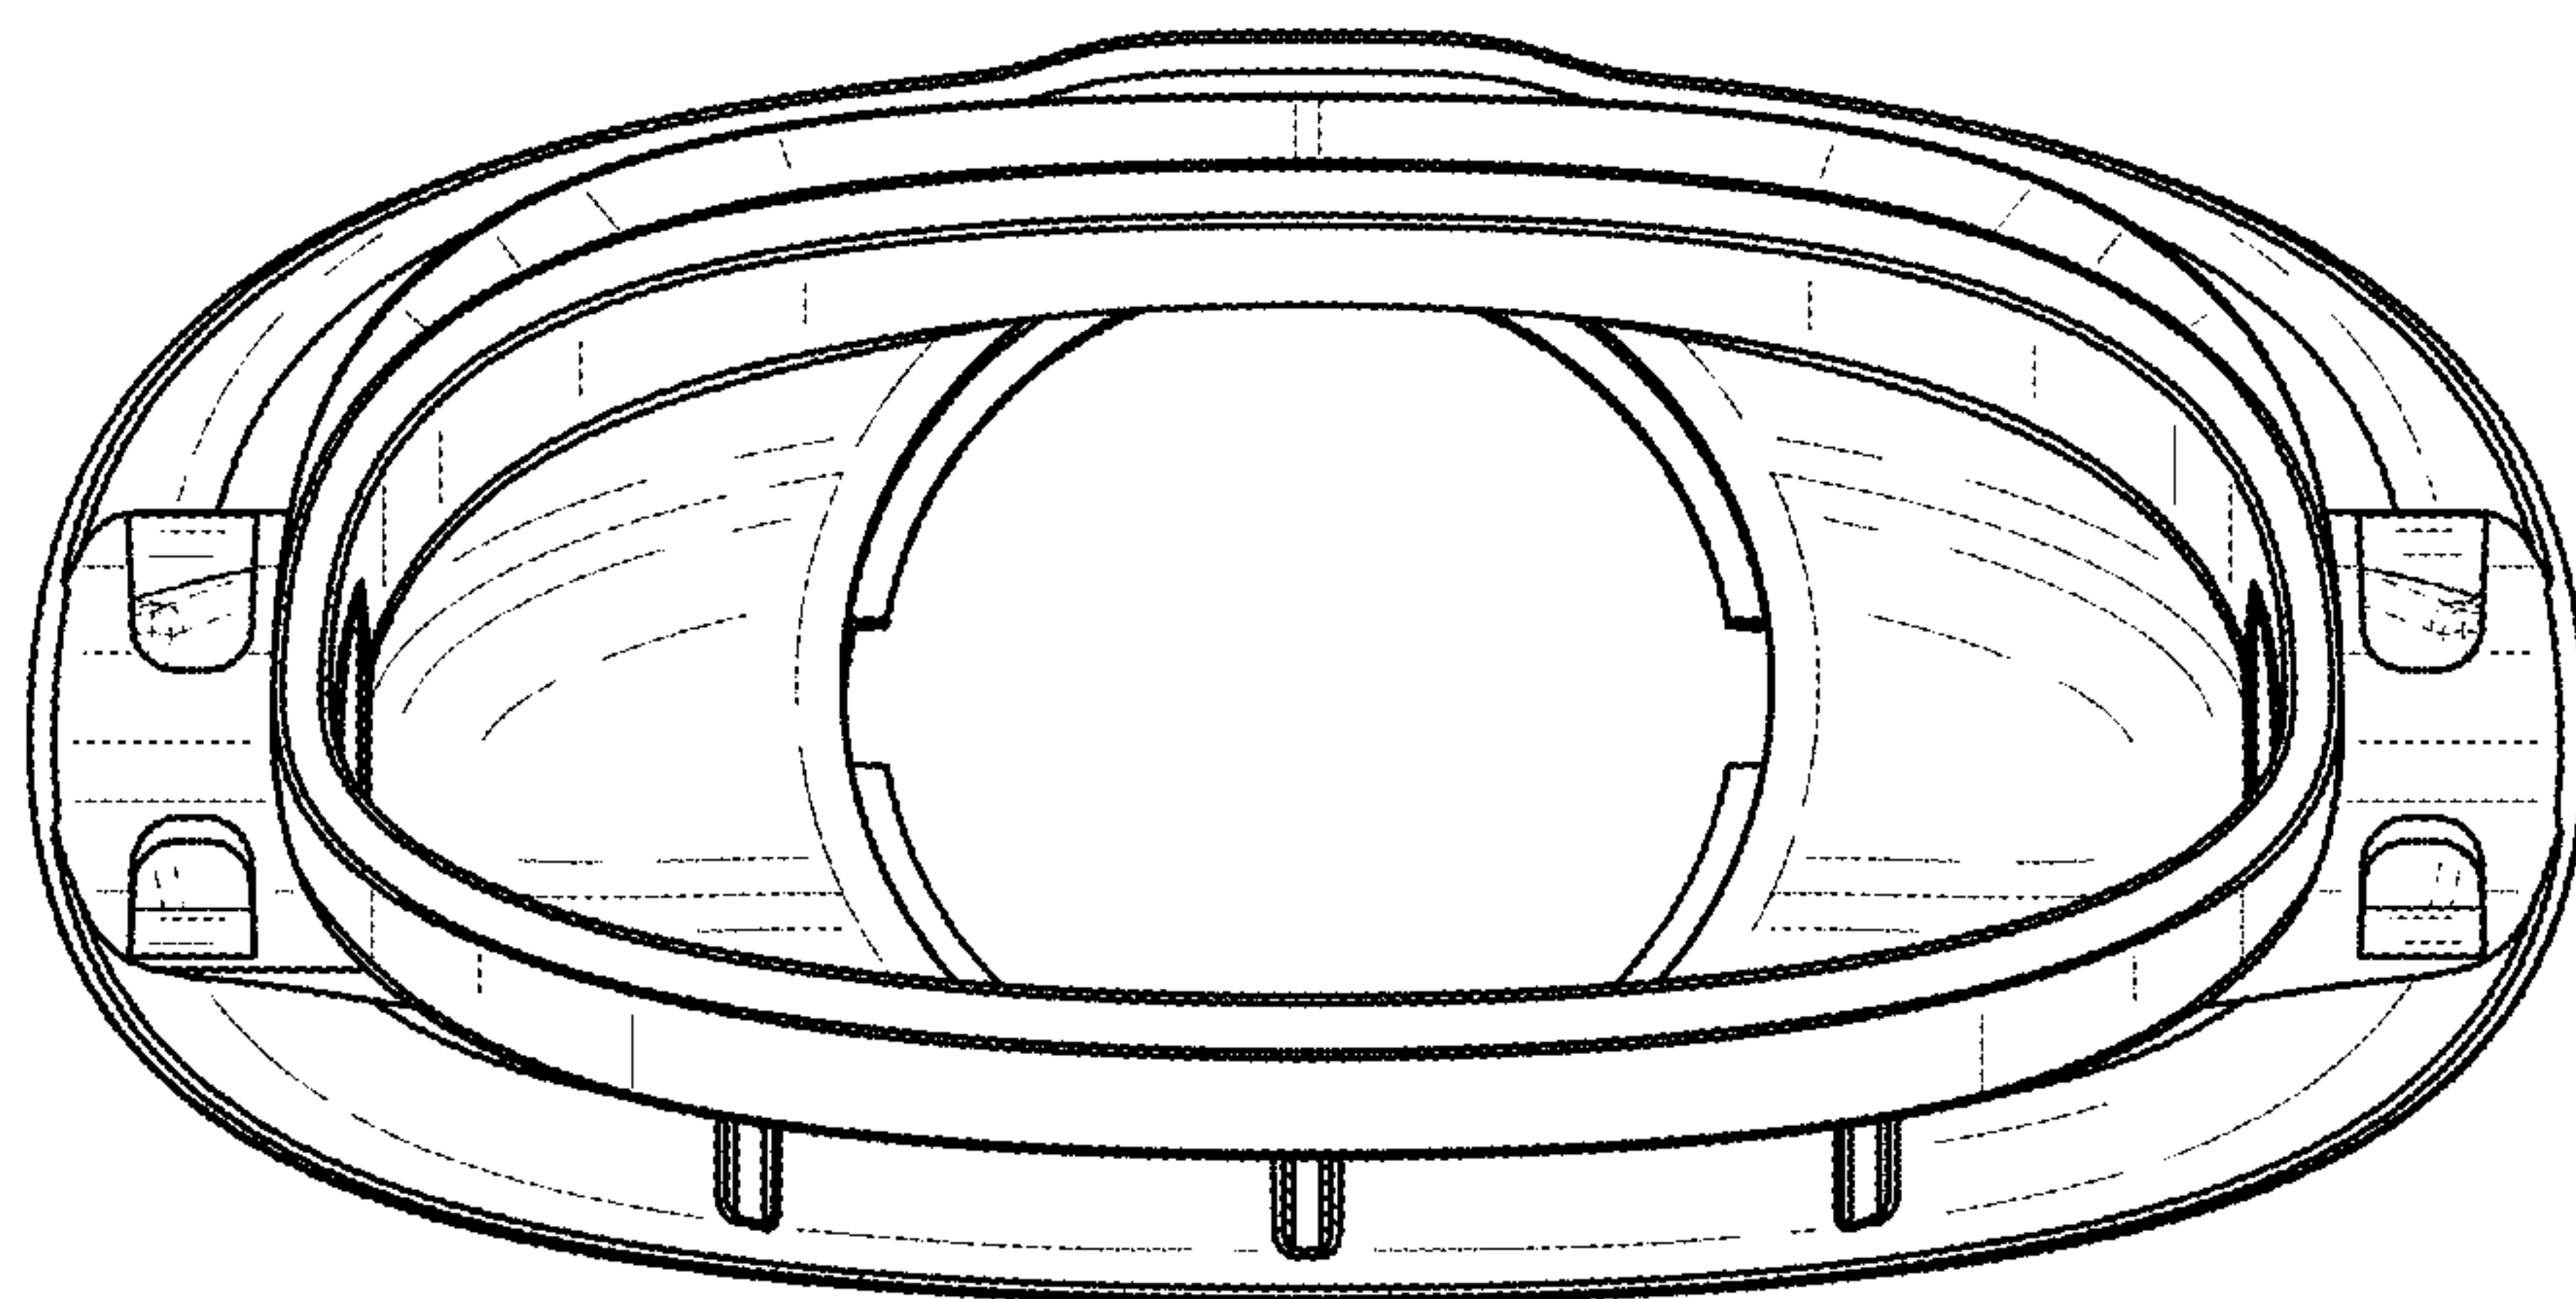


FIG. 4

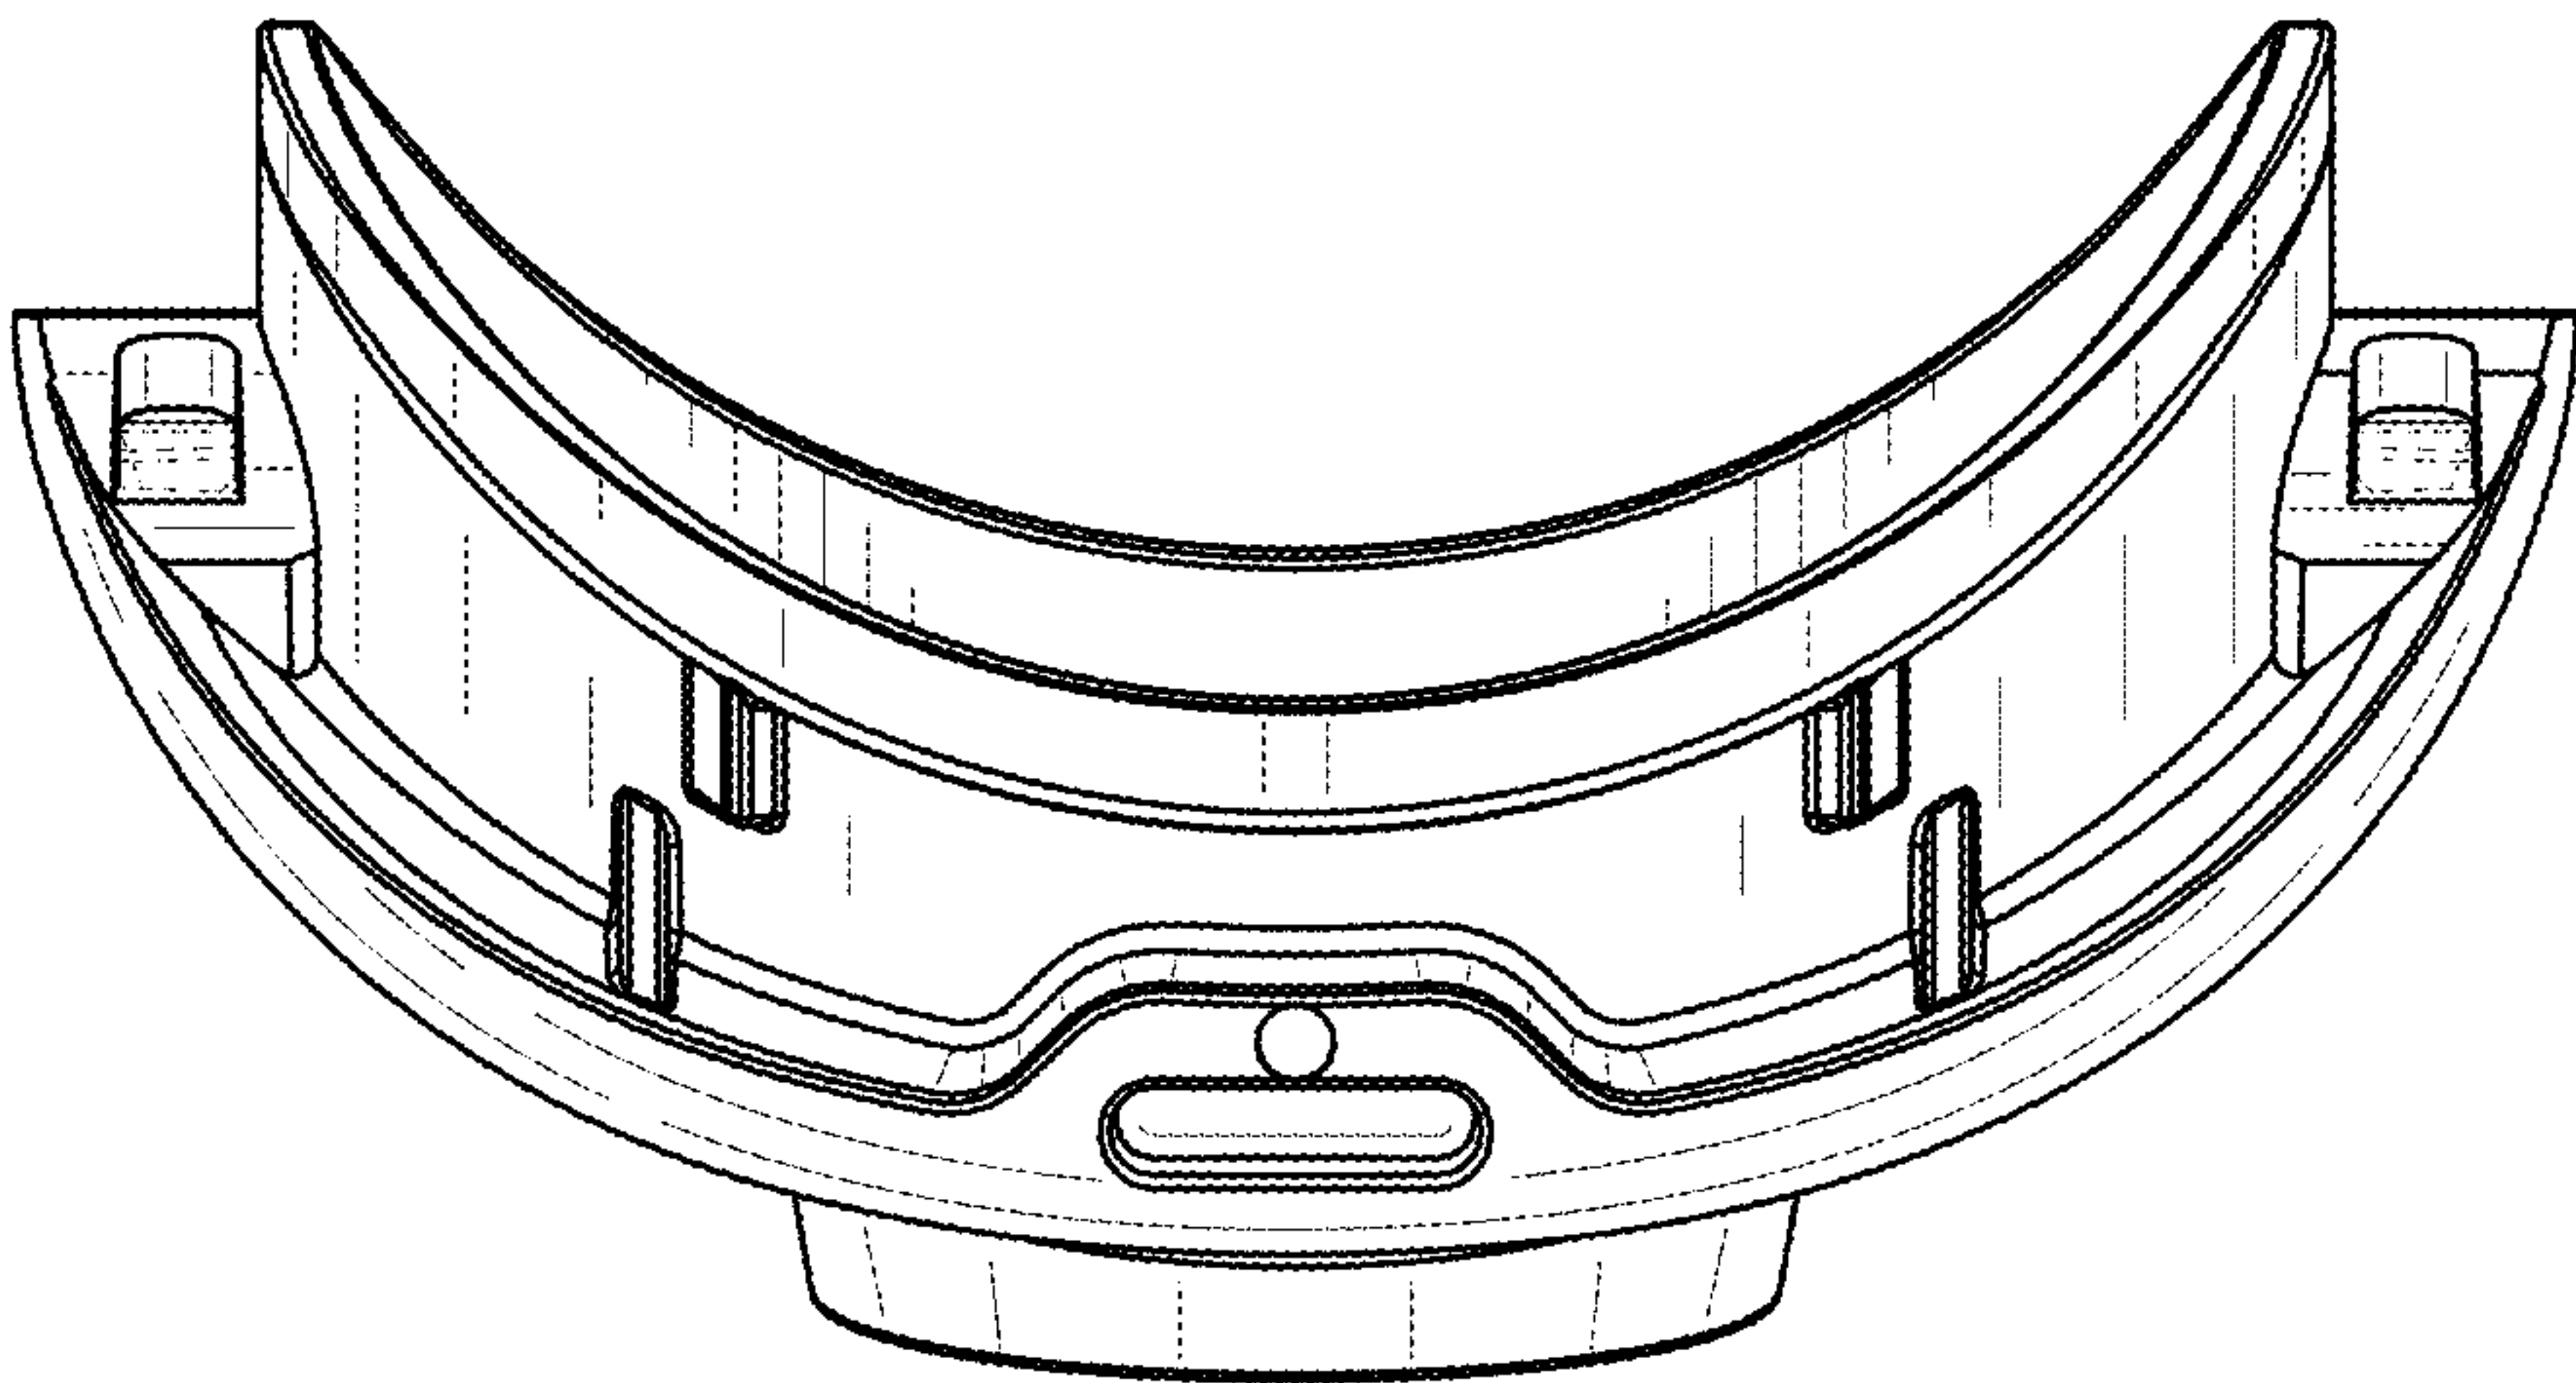


FIG. 5

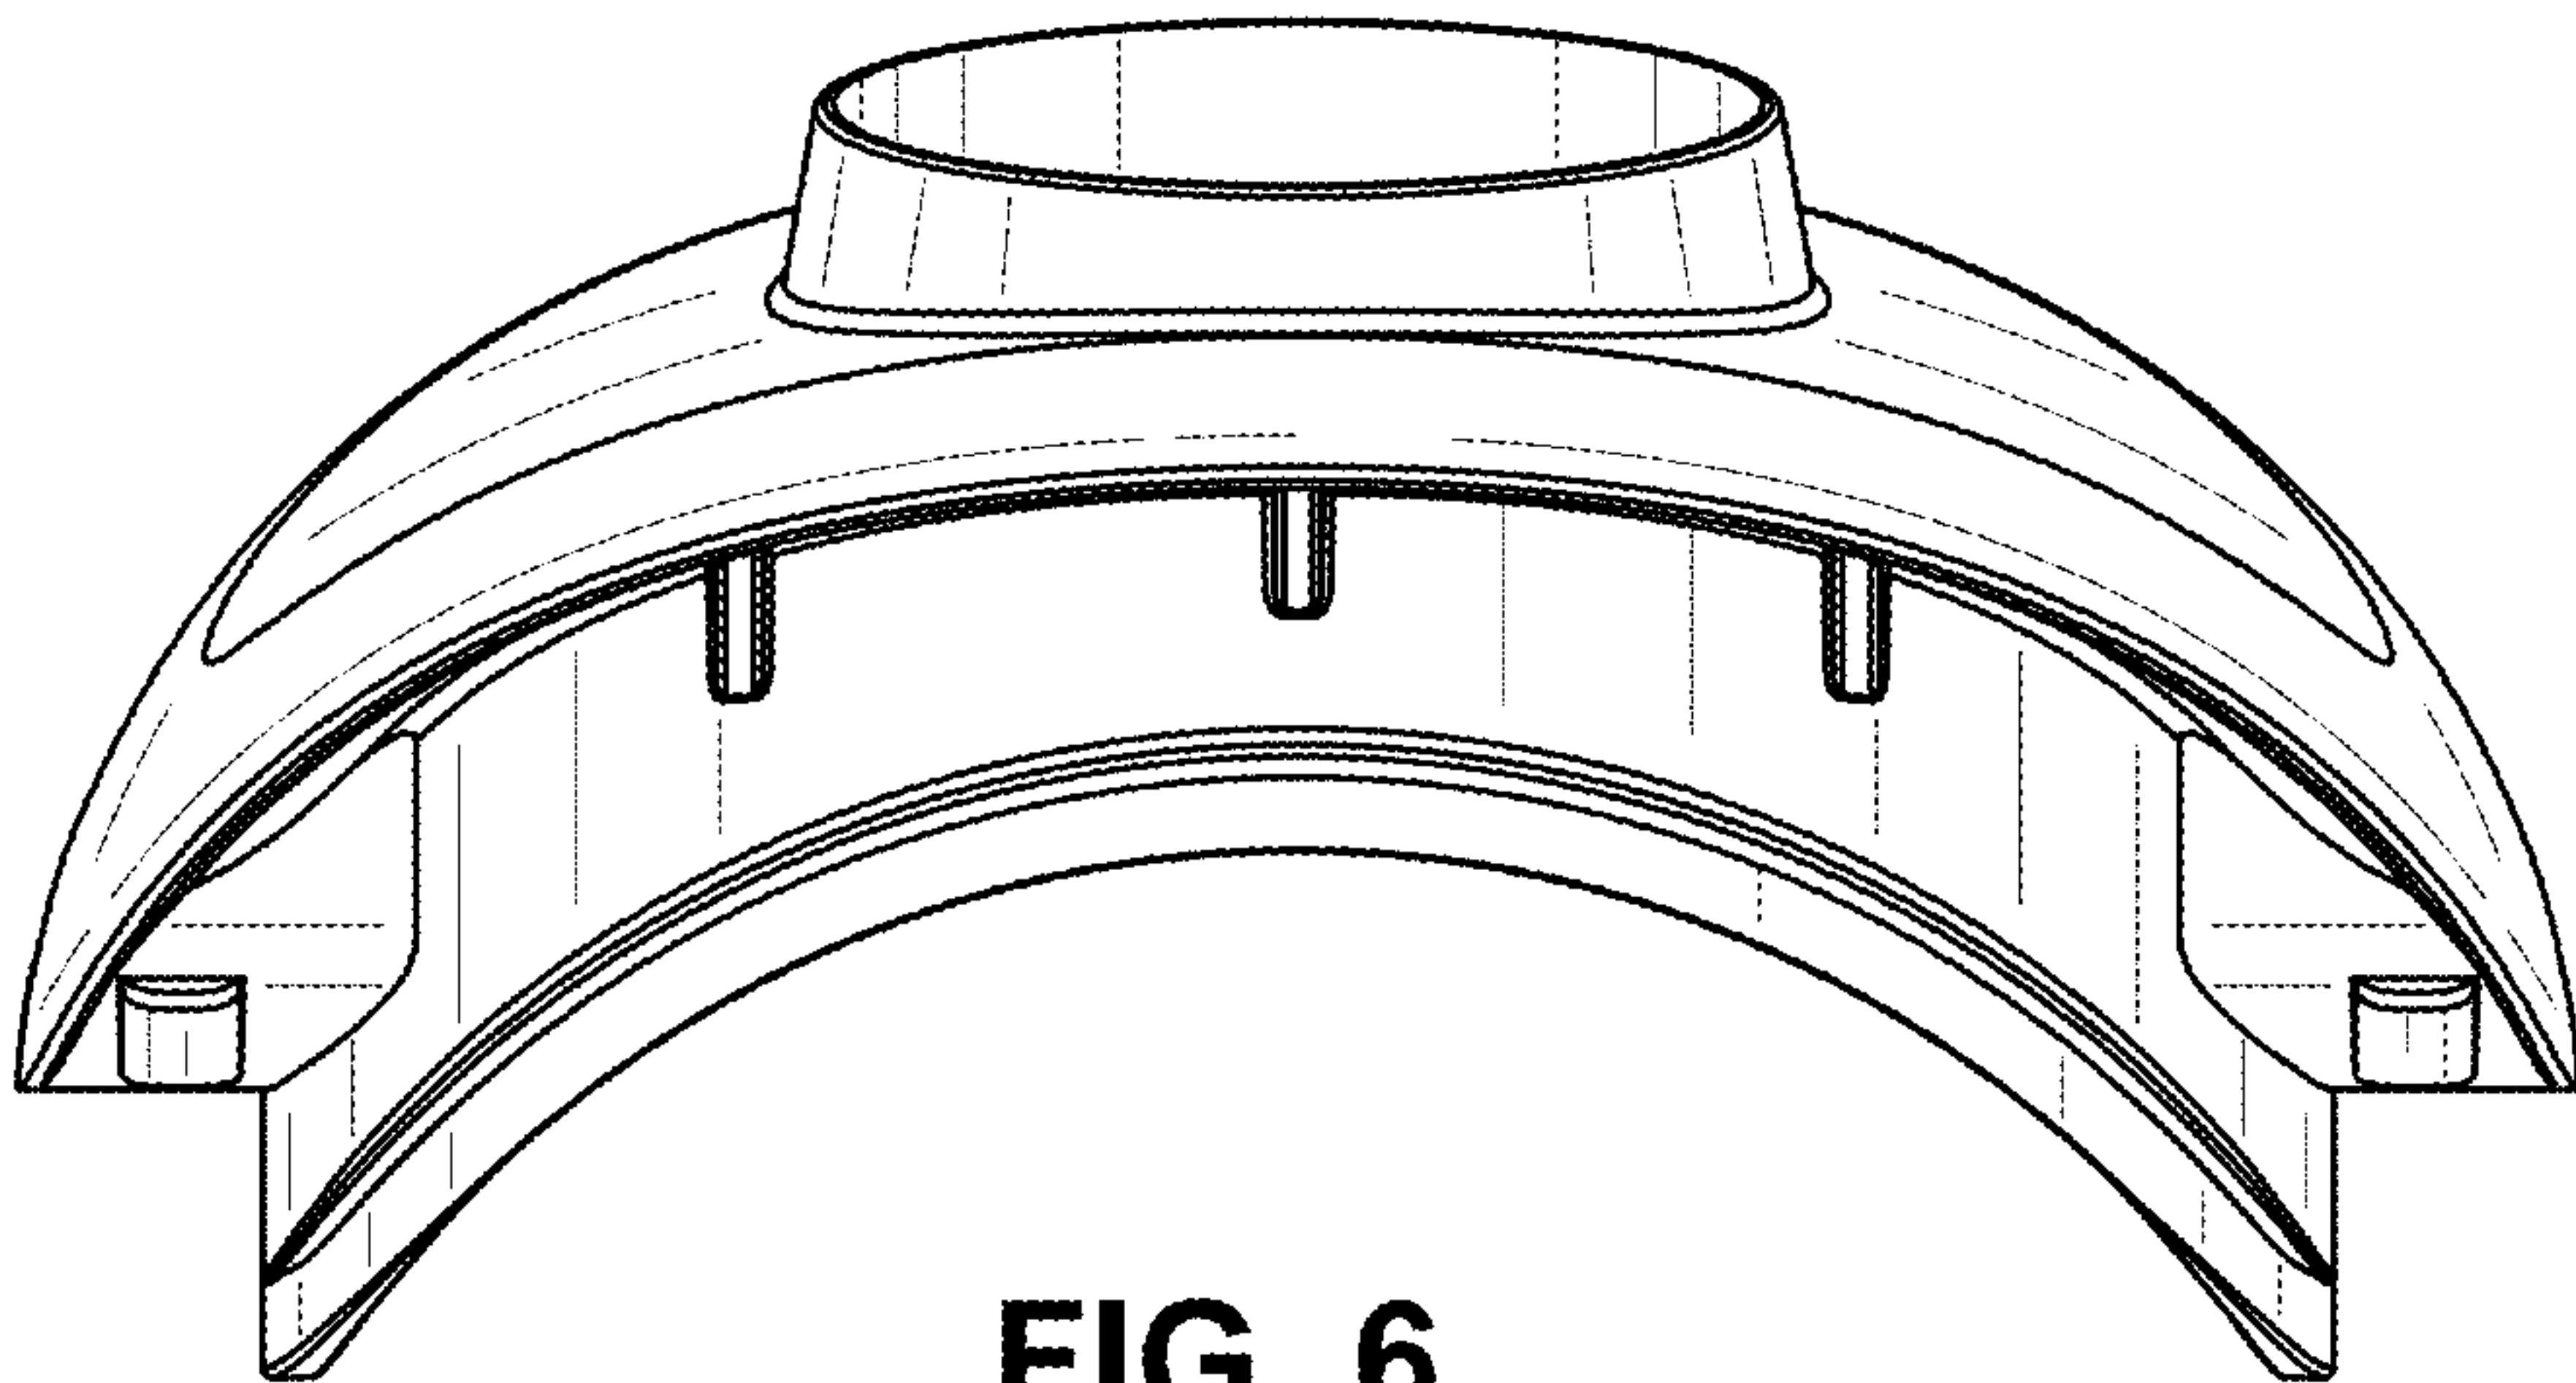


FIG. 6

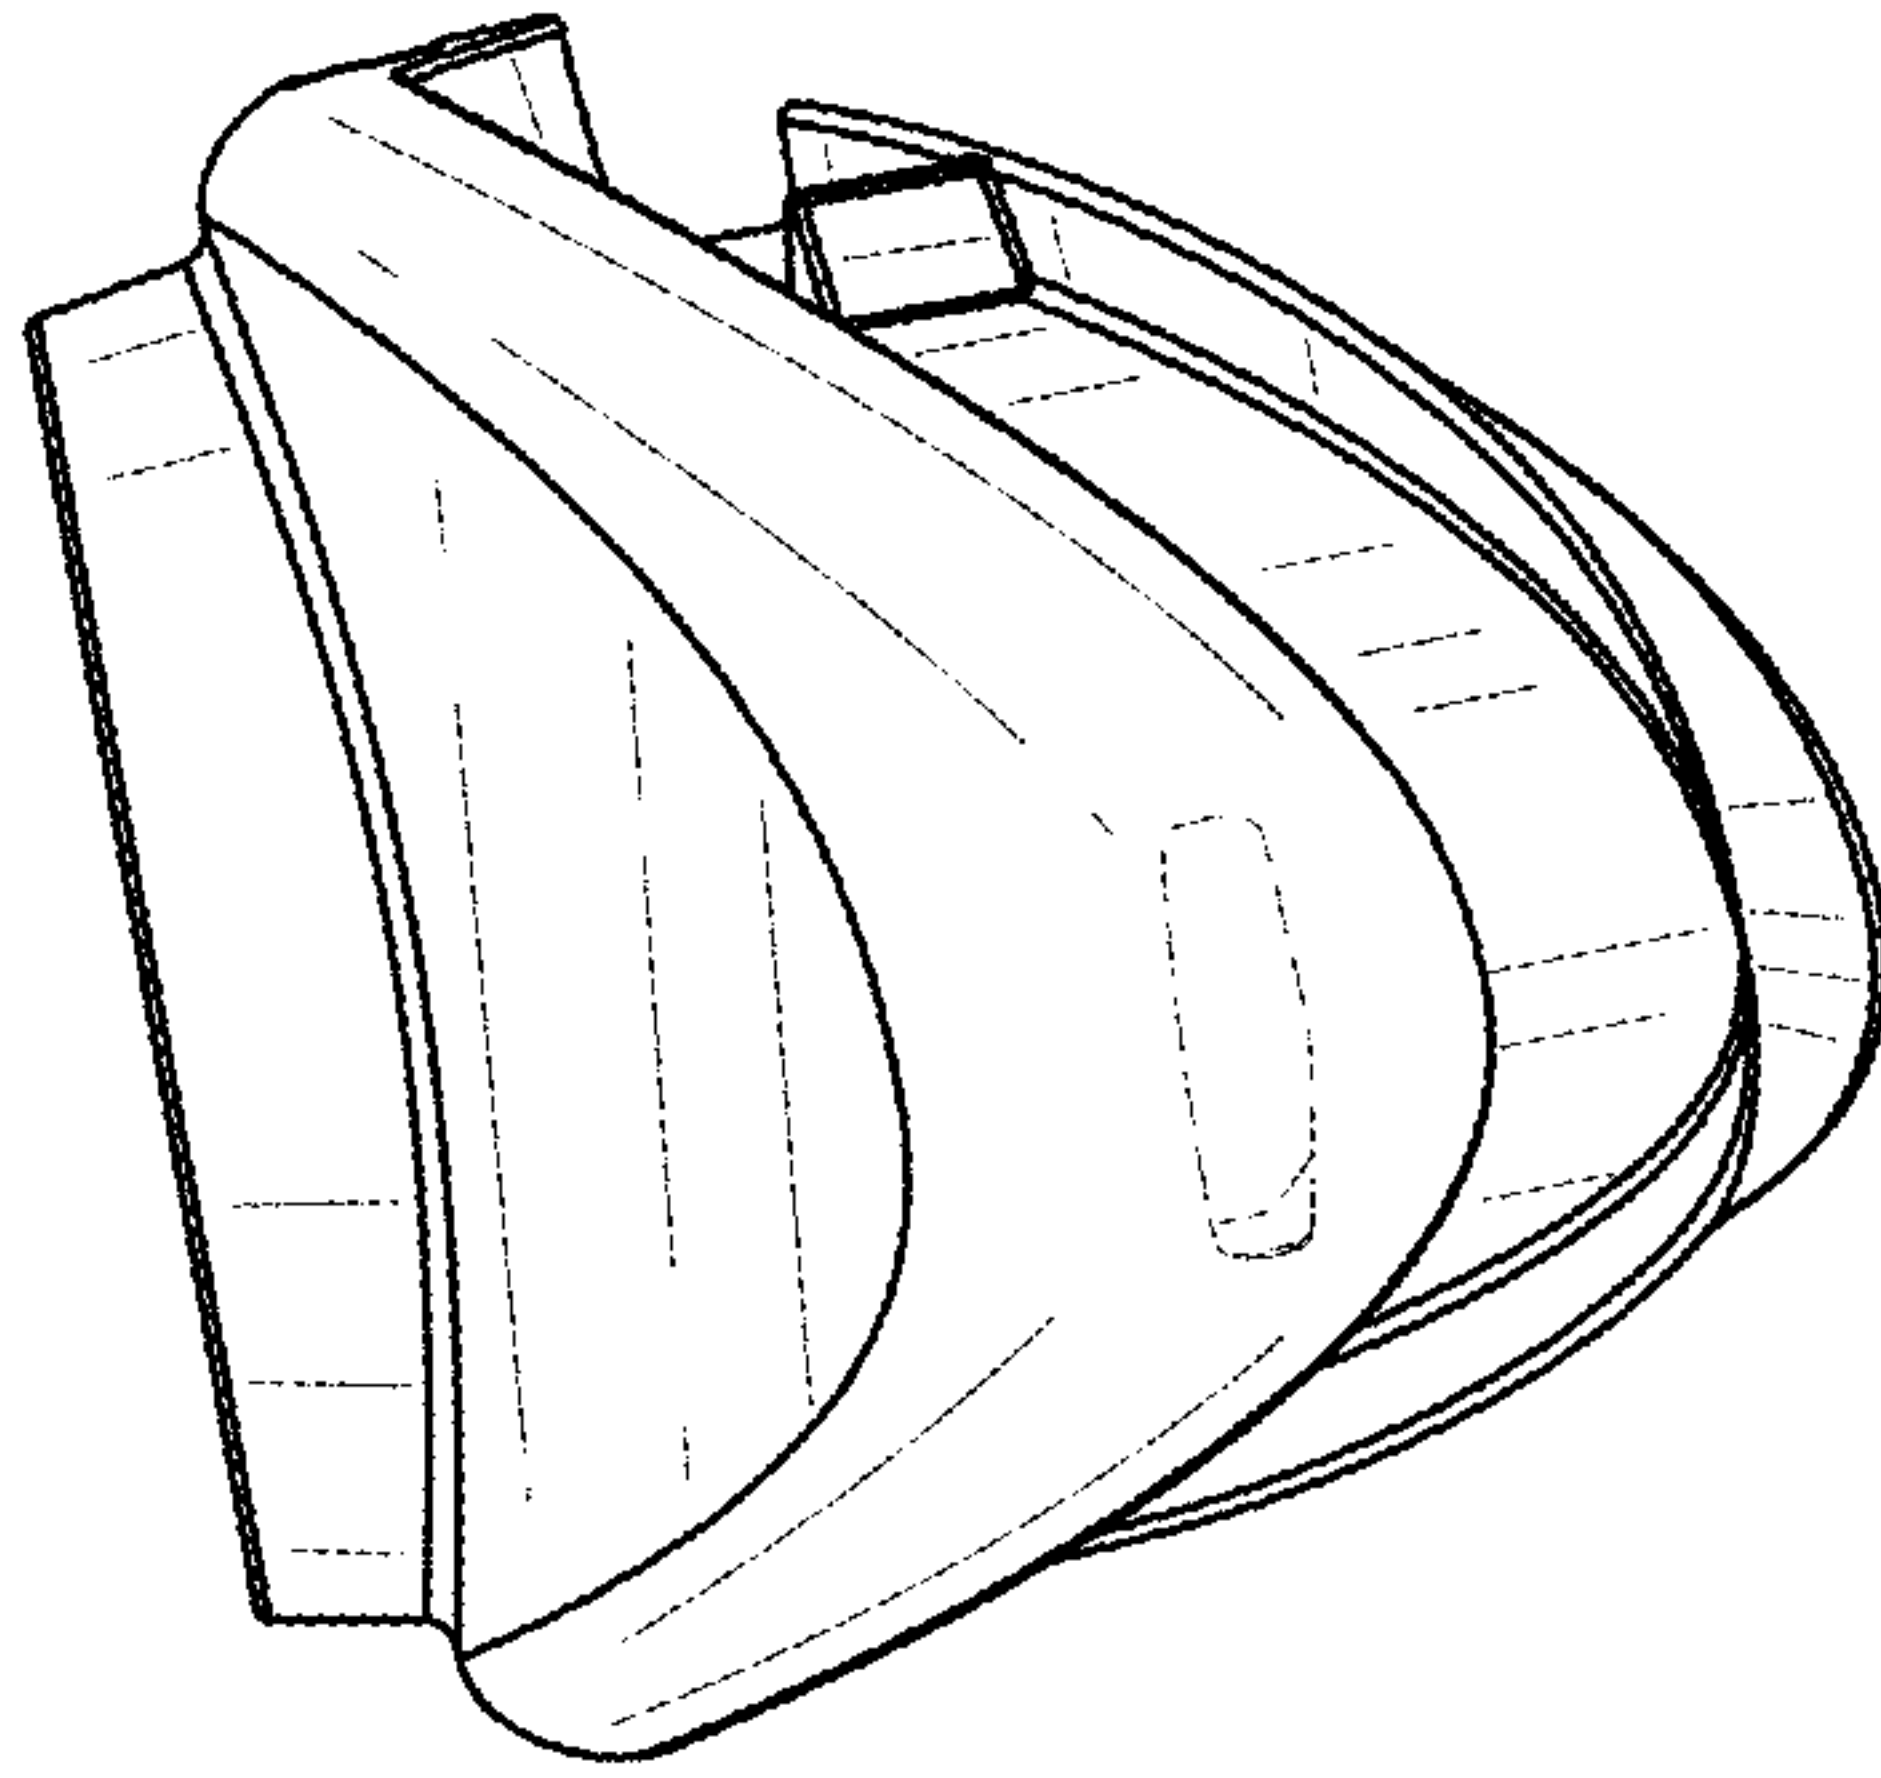


FIG. 7

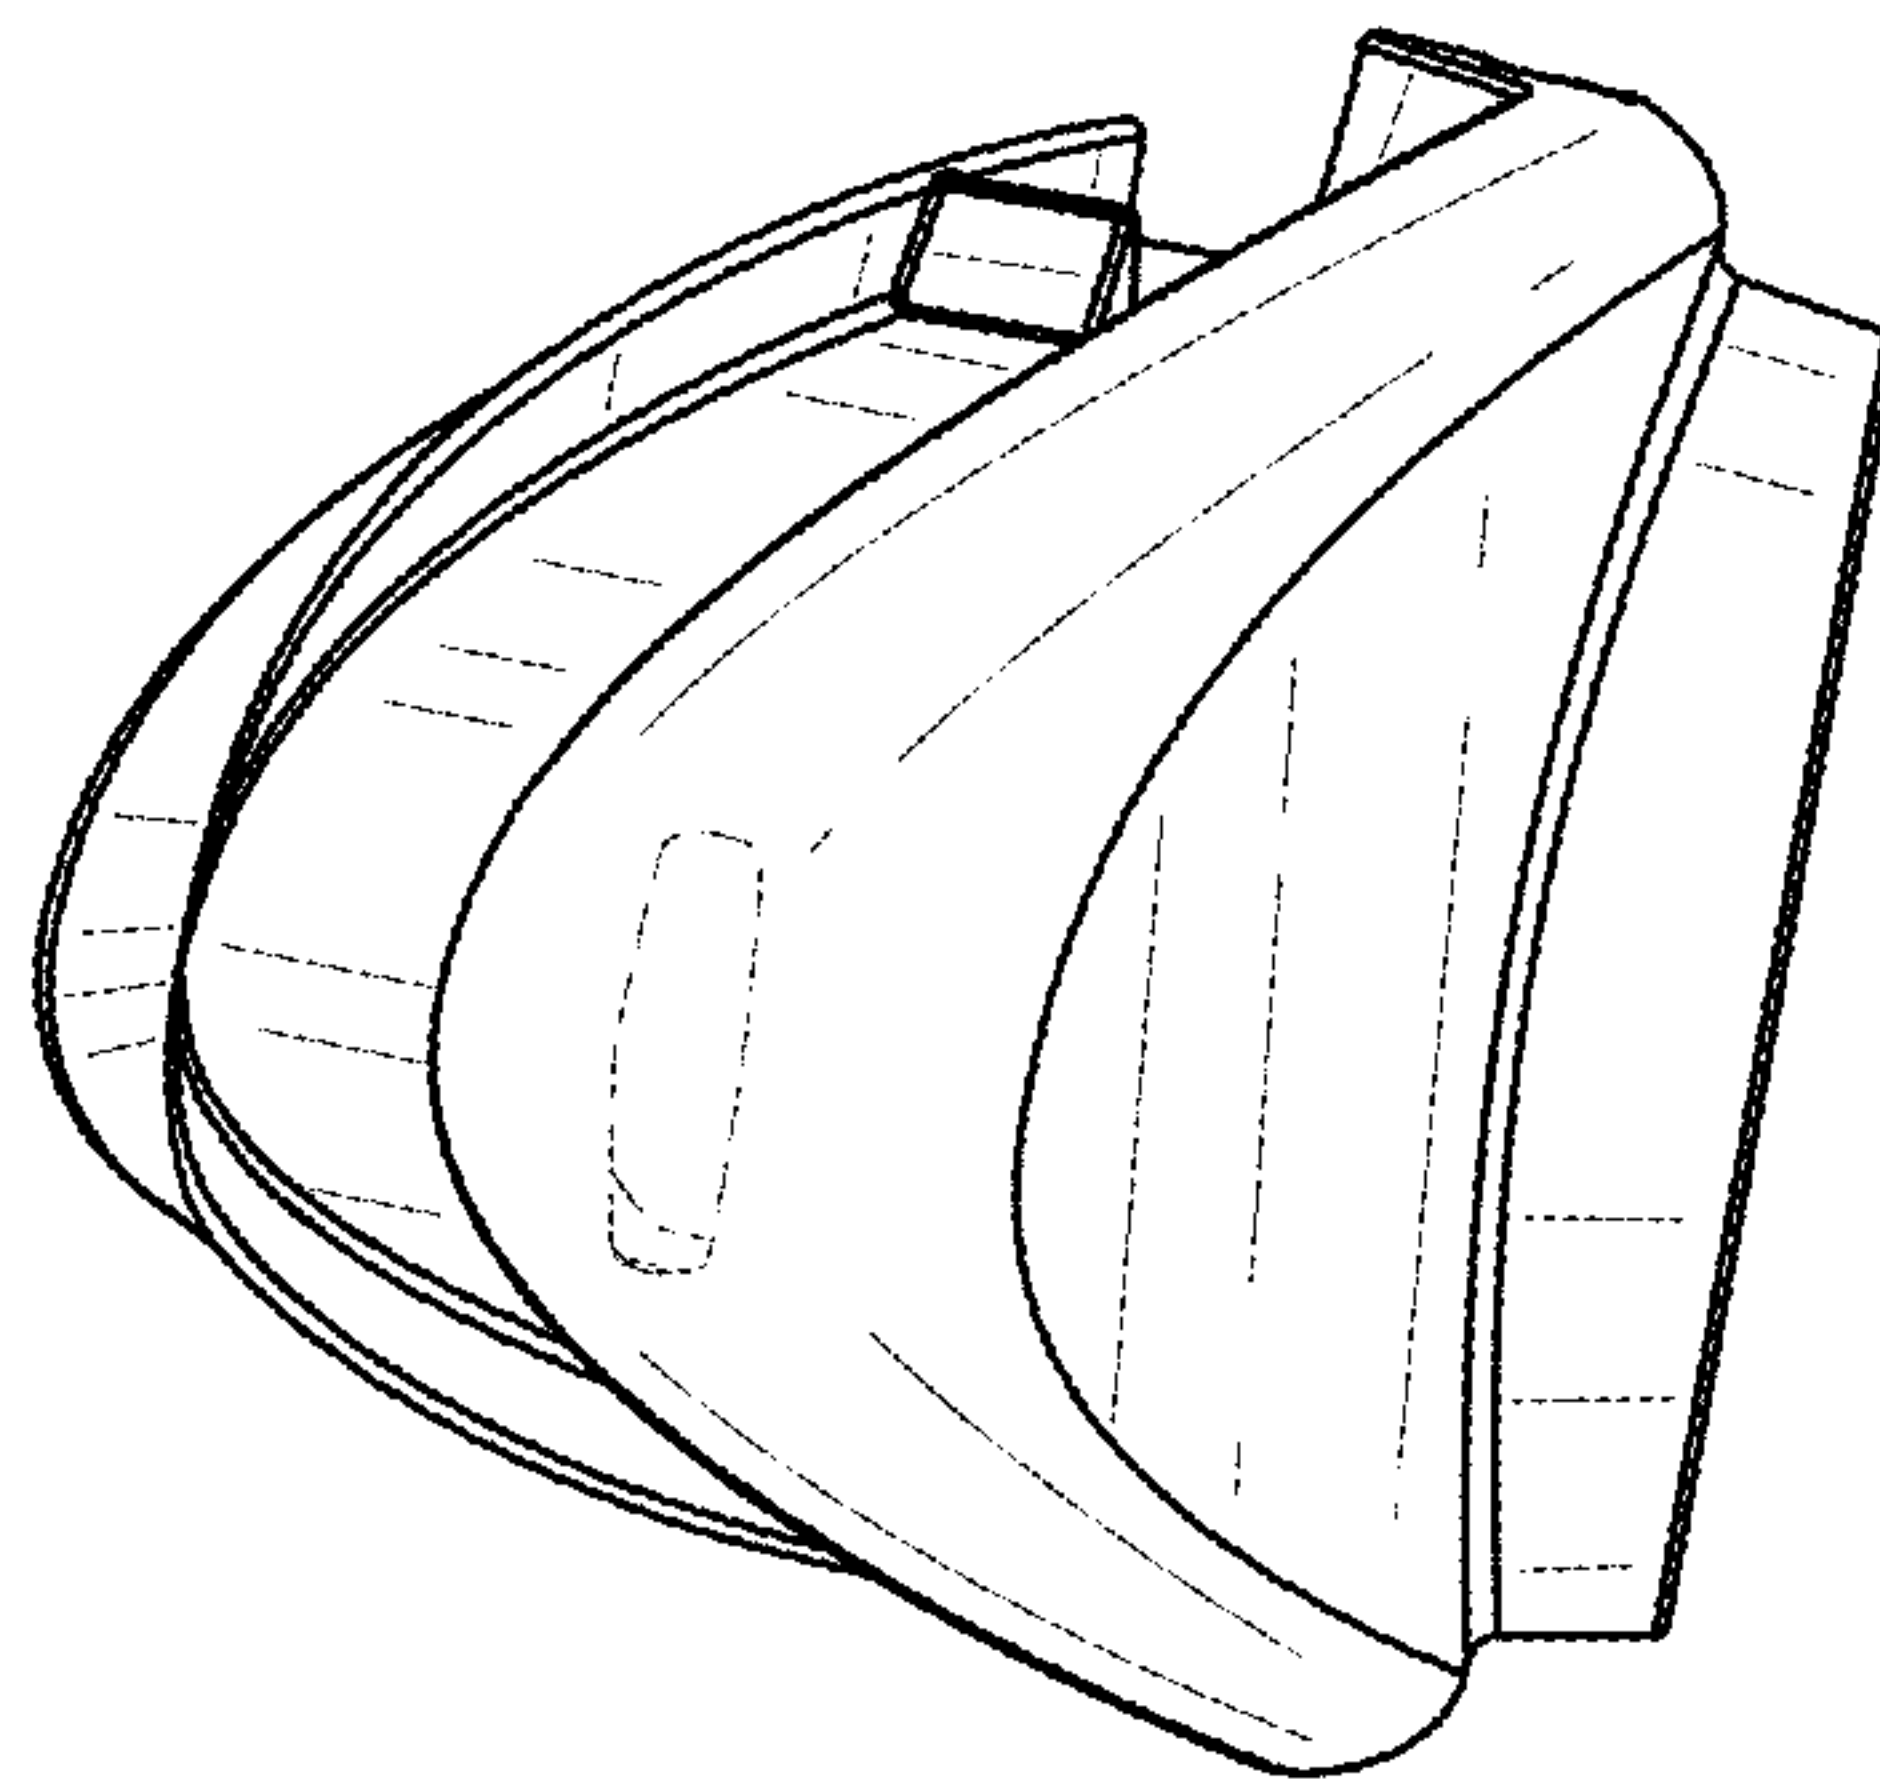


FIG. 8

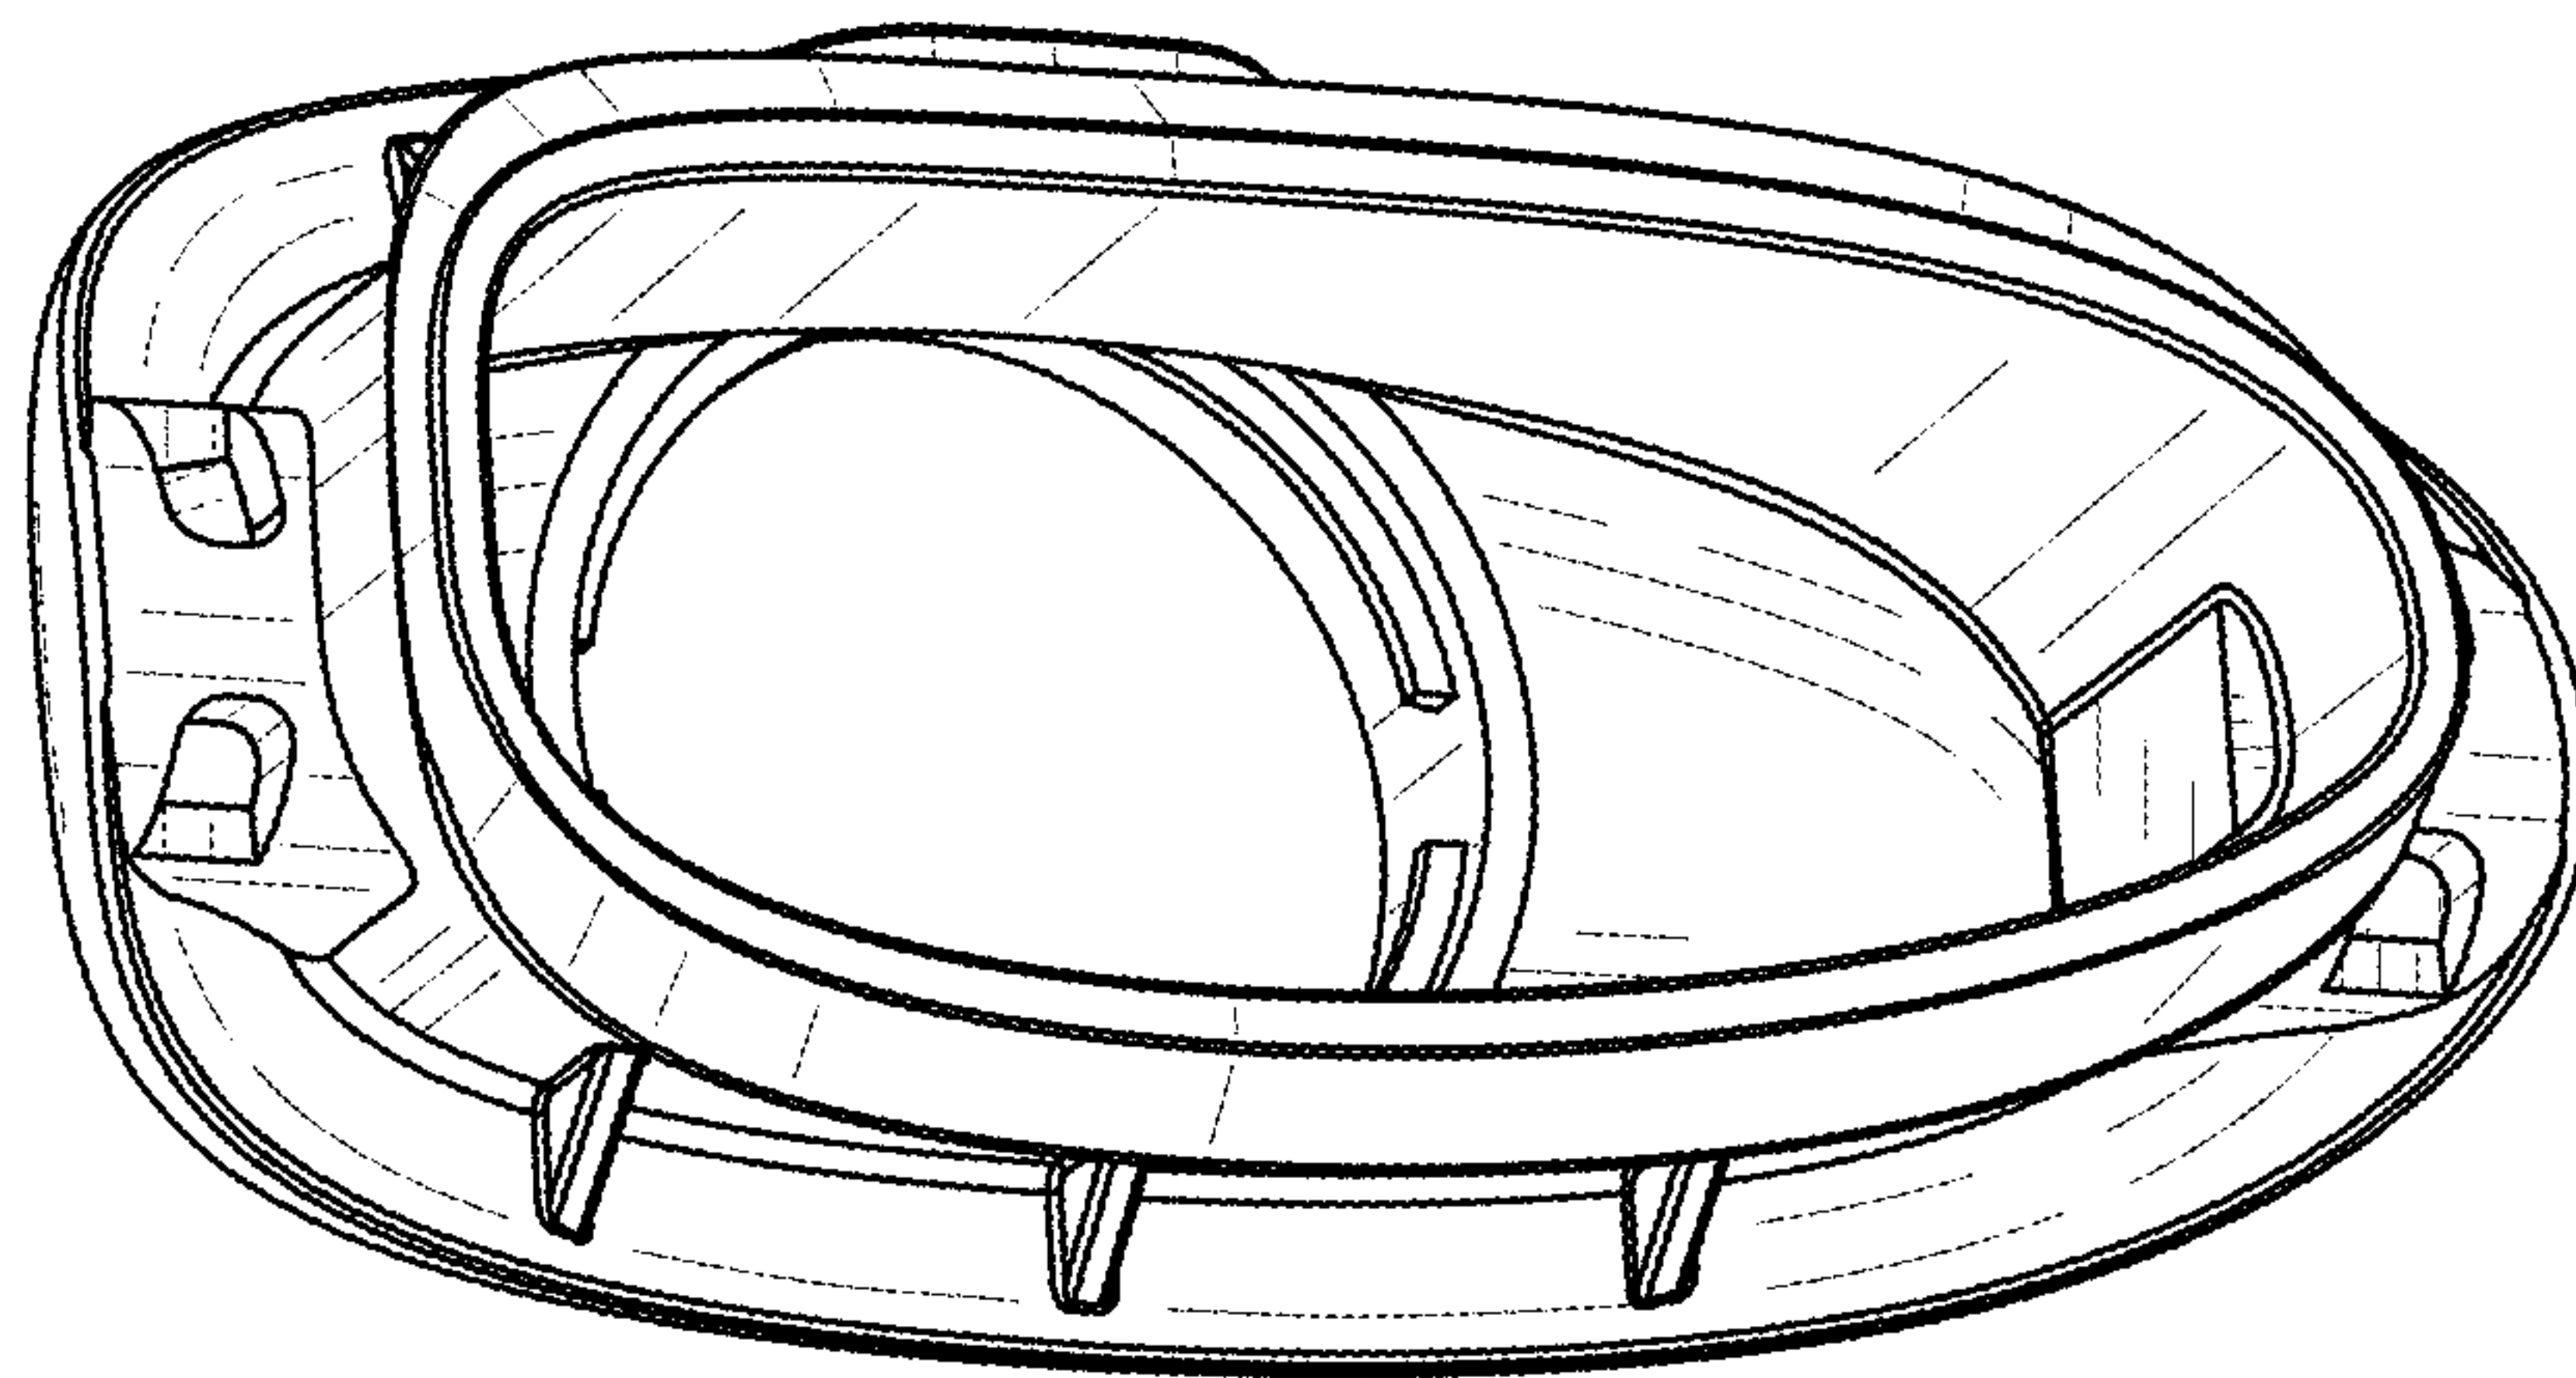


FIG. 9