

US0D1031031S

(12)

United States Design Patent

Payne et al.

(10)

Patent No.:

US D1,031,031 S

(45)

Date of Patent:

** Jun. 11, 2024

(54) SURGICAL HANDPIECE

(71) Applicant: Stryker Corporation, Kalamazoo, MI (US)

(72) Inventors: Dustin James Payne, Kalamazoo, MI (US); Daniel Reichert, Climax, MI (US); Craig E. Volstromer, Marshall, MI (US)

(73) Assignee: Stryker Corporation, Kalamazoo, MI (US)

(**) Term: 15 Years

(21) Appl. No.: 29/791,518

(22) Filed: Jan. 14, 2022

(51) LOC (14) Cl. 24-02

(52) U.S. Cl. USPC D24/133

(58) Field of Classification Search
USPC D24/127, 130, 133, 146, 147, 200, 214; D8/14, 14.1, 29.1, 29.2, 30, 61, 68, 93, D8/97, 300, 310, 311, 313, 2; D19/110, D19/115; D7/649; D23/223, 226, 229
CPC B26B 3/00; B26B 1/10; A61B 17/1617; A61B 17/3417; A61B 17/1624; A61B 17/162; A61B 17/1622; A61B 2017/00424; A61B 5/1411; B05C 17/103; B05C 17/116; B05C 17/01; B25D 2222/54
See application file for complete search history.

(56) References Cited

U.S. PATENT DOCUMENTS

D329,092 S	9/1992	Carusillo et al.	
D364,463 S	11/1995	Pitzen et al.	
5,993,454 A *	11/1999	Longo	B23Q 5/048 606/85
D420,879 S	2/2000	Watson et al.	
6,123,235 A	9/2000	Hsu	

D456,678 S	5/2002	Karten et al.	
D463,237 S	9/2002	Sims et al.	
D499,624 S *	12/2004	Concari	D8/68
D515,378 S *	2/2006	Wu	D8/68
D516,883 S	3/2006	Popov et al.	
(Continued)			

FOREIGN PATENT DOCUMENTS

EM 009086663-0001 * 7/2022

OTHER PUBLICATIONS

Zaguar Battery-powered surgical handpiece, imedicom.co.kr, [online], [site visited May 13, 2023], Available from internet, URL: https://imedicom.co.kr/portfolio/oscillating-saw-handpiece/?lang=en (Year: 2023).*

(Continued)

Primary Examiner — Samantha Q Lawrence
Assistant Examiner — Thanh Luu Wong
(74) Attorney, Agent, or Firm — Howard & Howard Attorneys PLLC


(57) CLAIM

The ornamental design for a surgical handpiece, as shown and described.

DESCRIPTION

FIG. 1 is a front, top, right-side perspective view of a surgical handpiece;
FIG. 2 is a rear, bottom, left-side perspective view thereof;
FIG. 3 is a right-side view thereof;
FIG. 4 is a left-side view thereof;
FIG. 5 is a front view thereof;
FIG. 6 is a rear view thereof;
FIG. 7 is a top view thereof; and,
FIG. 8 is a bottom view thereof.
The broken lines in the drawings depict portions of the surgical handpiece that form no part of the claimed design.

1 Claim, 6 Drawing Sheets

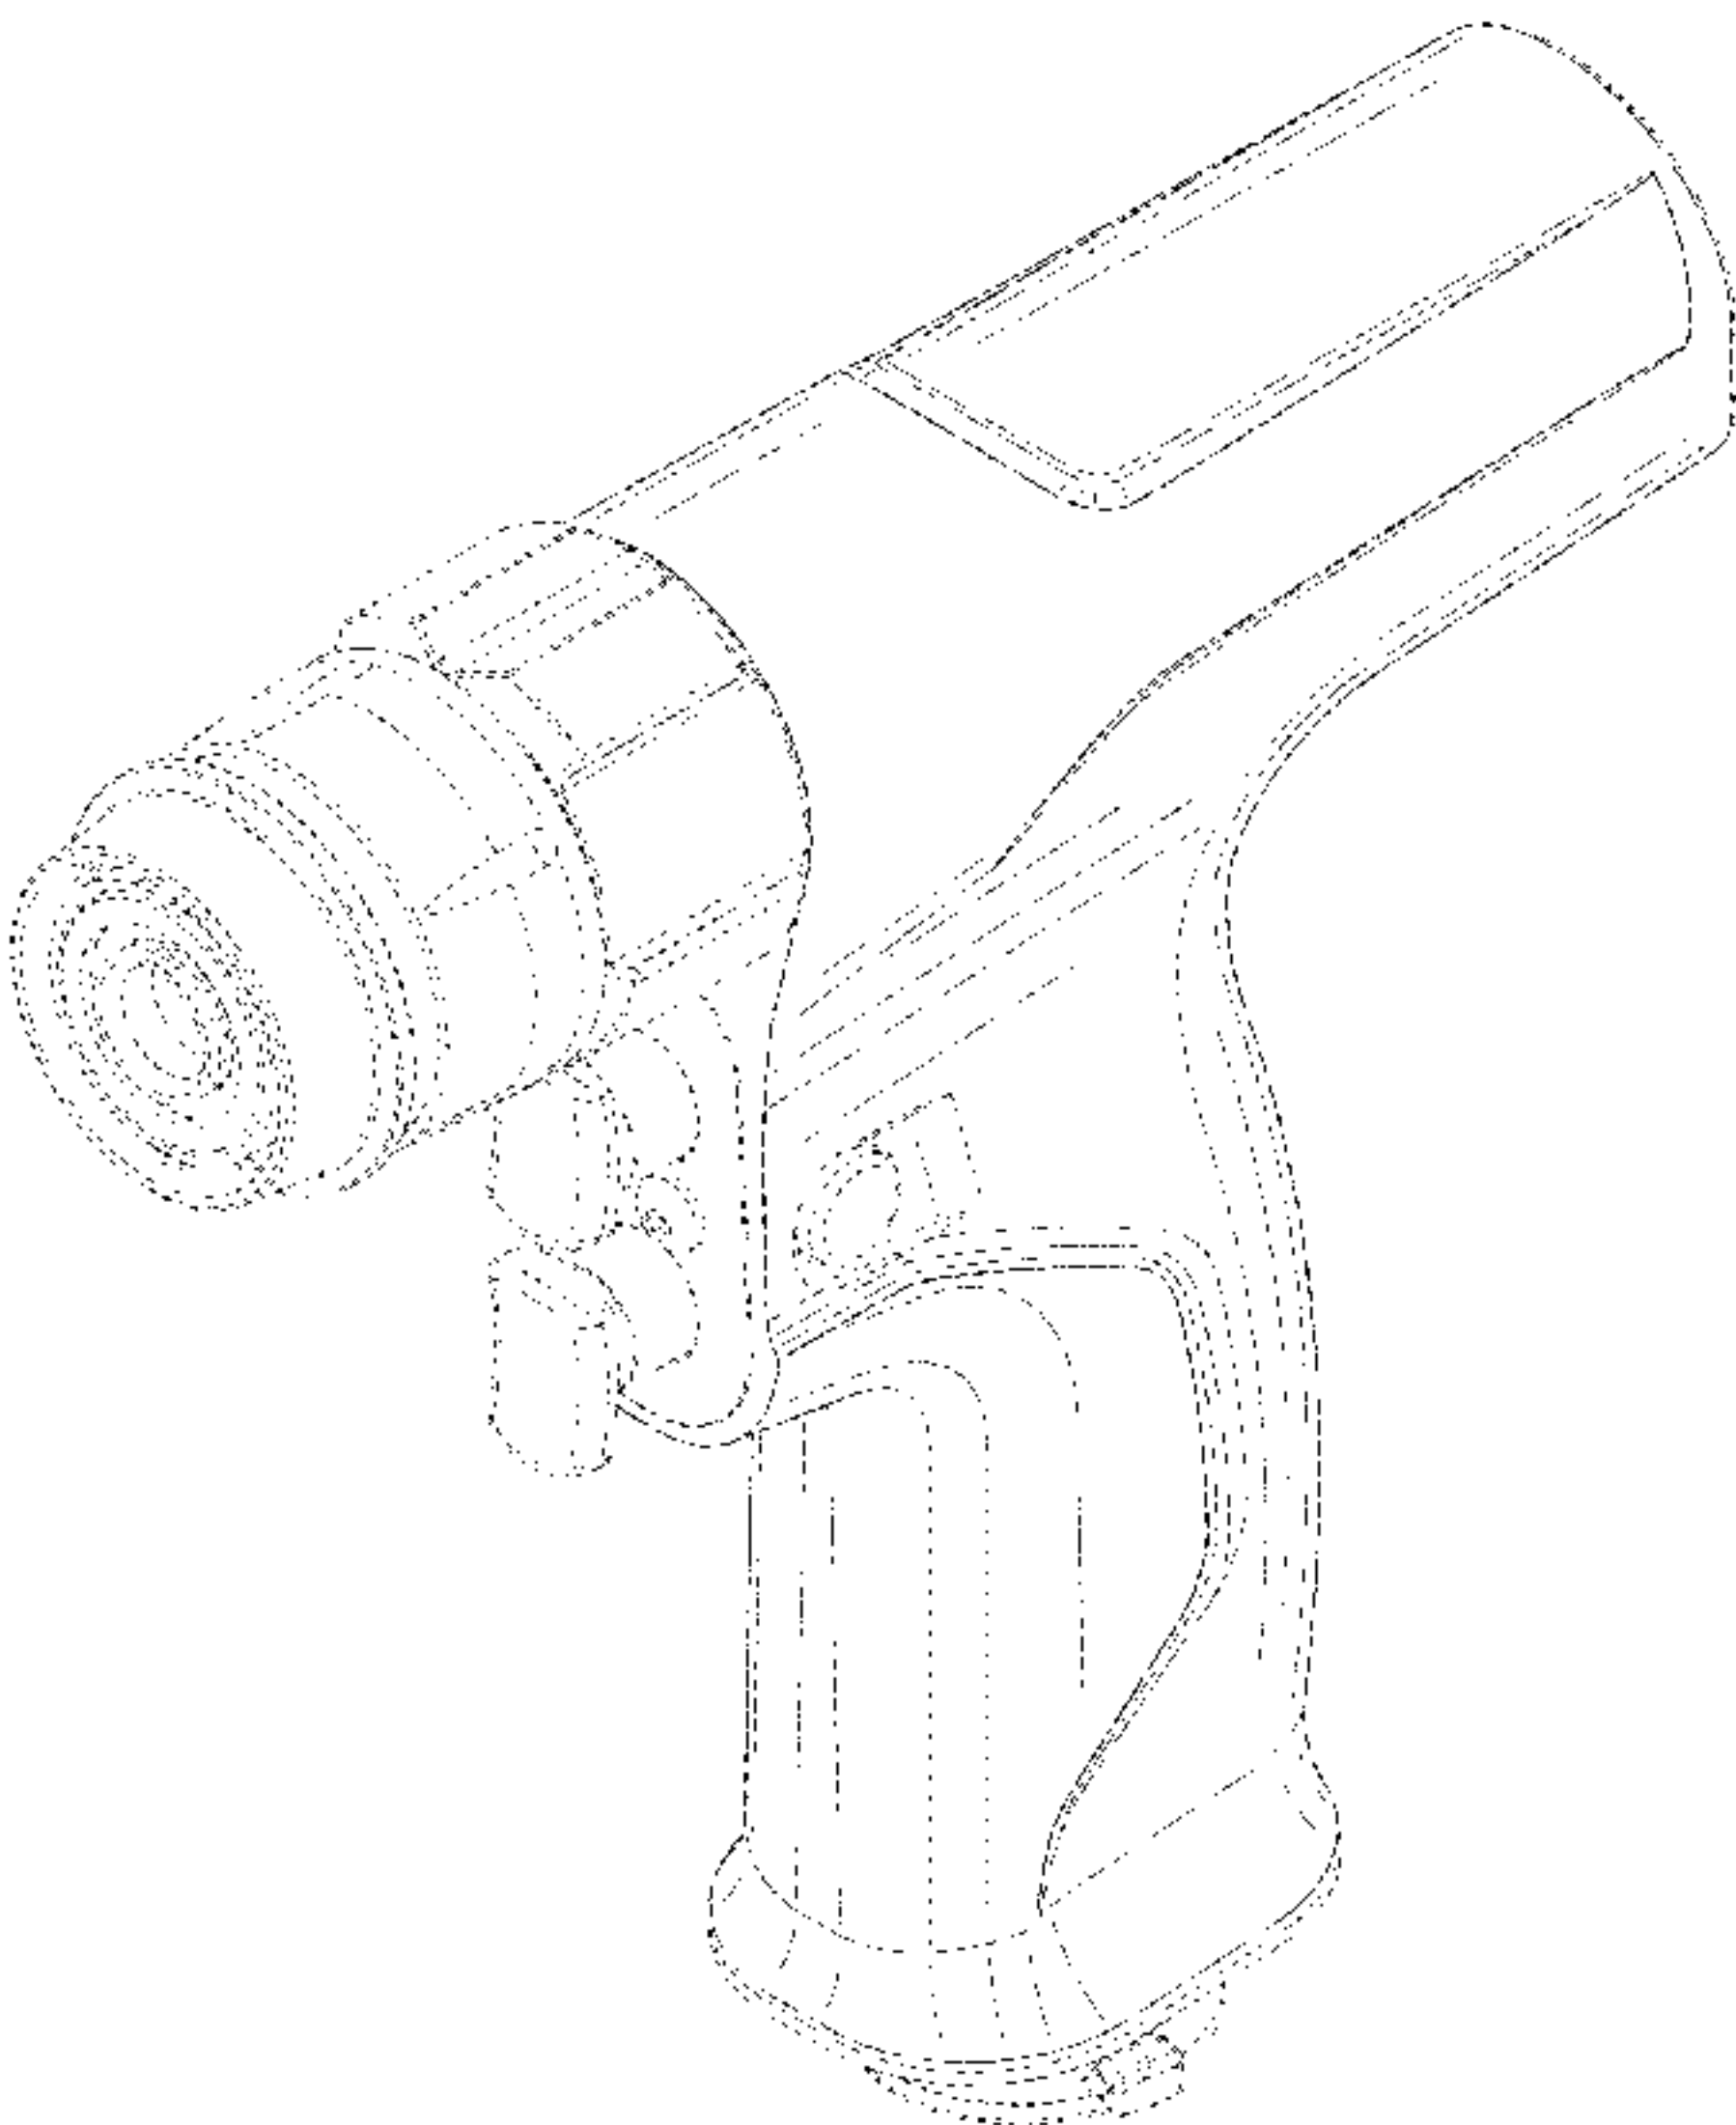

(56)

References Cited

U.S. PATENT DOCUMENTS

D531,874 S * 11/2006 Wu D8/68
7,195,230 B2 3/2007 Fast-Karberg et al.
D545,152 S * 6/2007 Lopano D8/14.1
D545,427 S * 6/2007 Gibson D24/113
D572,097 S * 7/2008 Yung-Kuan D28/13
D573,425 S 7/2008 Post et al.
D583,639 S * 12/2008 Axinte D8/30
D594,983 S 6/2009 Price et al.
7,637,392 B2 * 12/2009 Hsu B05C 17/0103
222/137

D620,593 S 7/2010 Tran et al.
D635,835 S 4/2011 Post
D660,663 S 5/2012 Brummitt
D673,020 S * 12/2012 Brummitt D8/14.1
D687,273 S 8/2013 Breitenmoser et al.
D687,549 S 8/2013 Johnson et al.
D700,966 S 3/2014 O'Leary et al.
D709,194 S 7/2014 Miller et al.
D713,933 S * 9/2014 Mammen D23/226
8,870,093 B2 * 10/2014 Brummitt B05B 7/0475
222/105

D725,978 S 4/2015 Uematsu et al.
D736,887 S * 8/2015 Schwarz D23/223
D743,547 S 11/2015 Chang et al.
D746,653 S * 1/2016 Furling D8/29.1
D759,237 S 6/2016 Heath et al.
D759,244 S * 6/2016 Leugers D24/146
D760,570 S * 7/2016 Zwicker D8/68
D778,439 S * 2/2017 Håkansson D8/60
D790,940 S * 7/2017 Dill D8/68
D794,196 S * 8/2017 Russell D24/146
D809,884 S * 2/2018 Huang D8/30
D817,136 S 5/2018 Becket
D817,137 S 5/2018 Becket
D824,489 S * 7/2018 Montoya D23/223
D824,490 S * 7/2018 Montoya D23/223

D831,212 S * 10/2018 Clifford D24/146
10,159,495 B1 12/2018 Lambert
D840,032 S * 2/2019 Clifford D24/146
D919,392 S * 5/2021 Moeller D8/29.1
D919,753 S * 5/2021 Chen D23/226
D921,840 S * 6/2021 Chen D23/226
D969,317 S * 11/2022 Sun D24/133
D979,015 S * 2/2023 Chen D23/226
2012/0043102 A1 2/2012 Okuda
2013/0022939 A1 * 1/2013 Golden A61C 3/14
433/215
2018/0078246 A1 * 3/2018 Chon A61B 17/1622
2021/0186524 A1 6/2021 Carusillo et al.

OTHER PUBLICATIONS

Medinaut Max Handpiece, imedicom.co.kr, [online], [site visited May 13, 2023], Available from internet, URL: <https://imedicom.co.kr/medinaut-max-handpiece/?lang=en> (Year: 2023).
NM-300 Mini Multifunctional Drill Saw System, orthopedicdrills.com, customer review oldest date Mar. 20, 2019 [online], [site visited May 13, 2023], Available from internet, URL: <https://www.orthopedicdrills.com/product/nm-300-mini-multifunctional-drill-saw-system> (Year: 2019).
Stryker Corporation, "Cordless Driver 3 / CD4 Proficiency Assessment," 2015, 4 pages.
Stryker Corporation, "Stryker Cordless Driver 3", 2017, 1 page.
Stryker Corporation, "Stryker Cordless Driver III", 2017, 1 page.
Stryker Instruments, "System 7 Recon Power Tools", 2013, 4 pages.
Stryker, "System 8 Power Tools Brochure", 2017, 5, pages.
Youtube, "Stryker Complete Cordless Driver 3 System with Biosteon ACL Kit", Jan. 18, 2016, 3 pages.
PR News Wire, "Depuy Synthes Launches the UNIUM System as a Next Generation Power Tools System for Trauma and Small Bone Procedures", <https://tinyurl.com/ydpky37y>, Nov. 22, 2021, 2 pages.

* cited by examiner

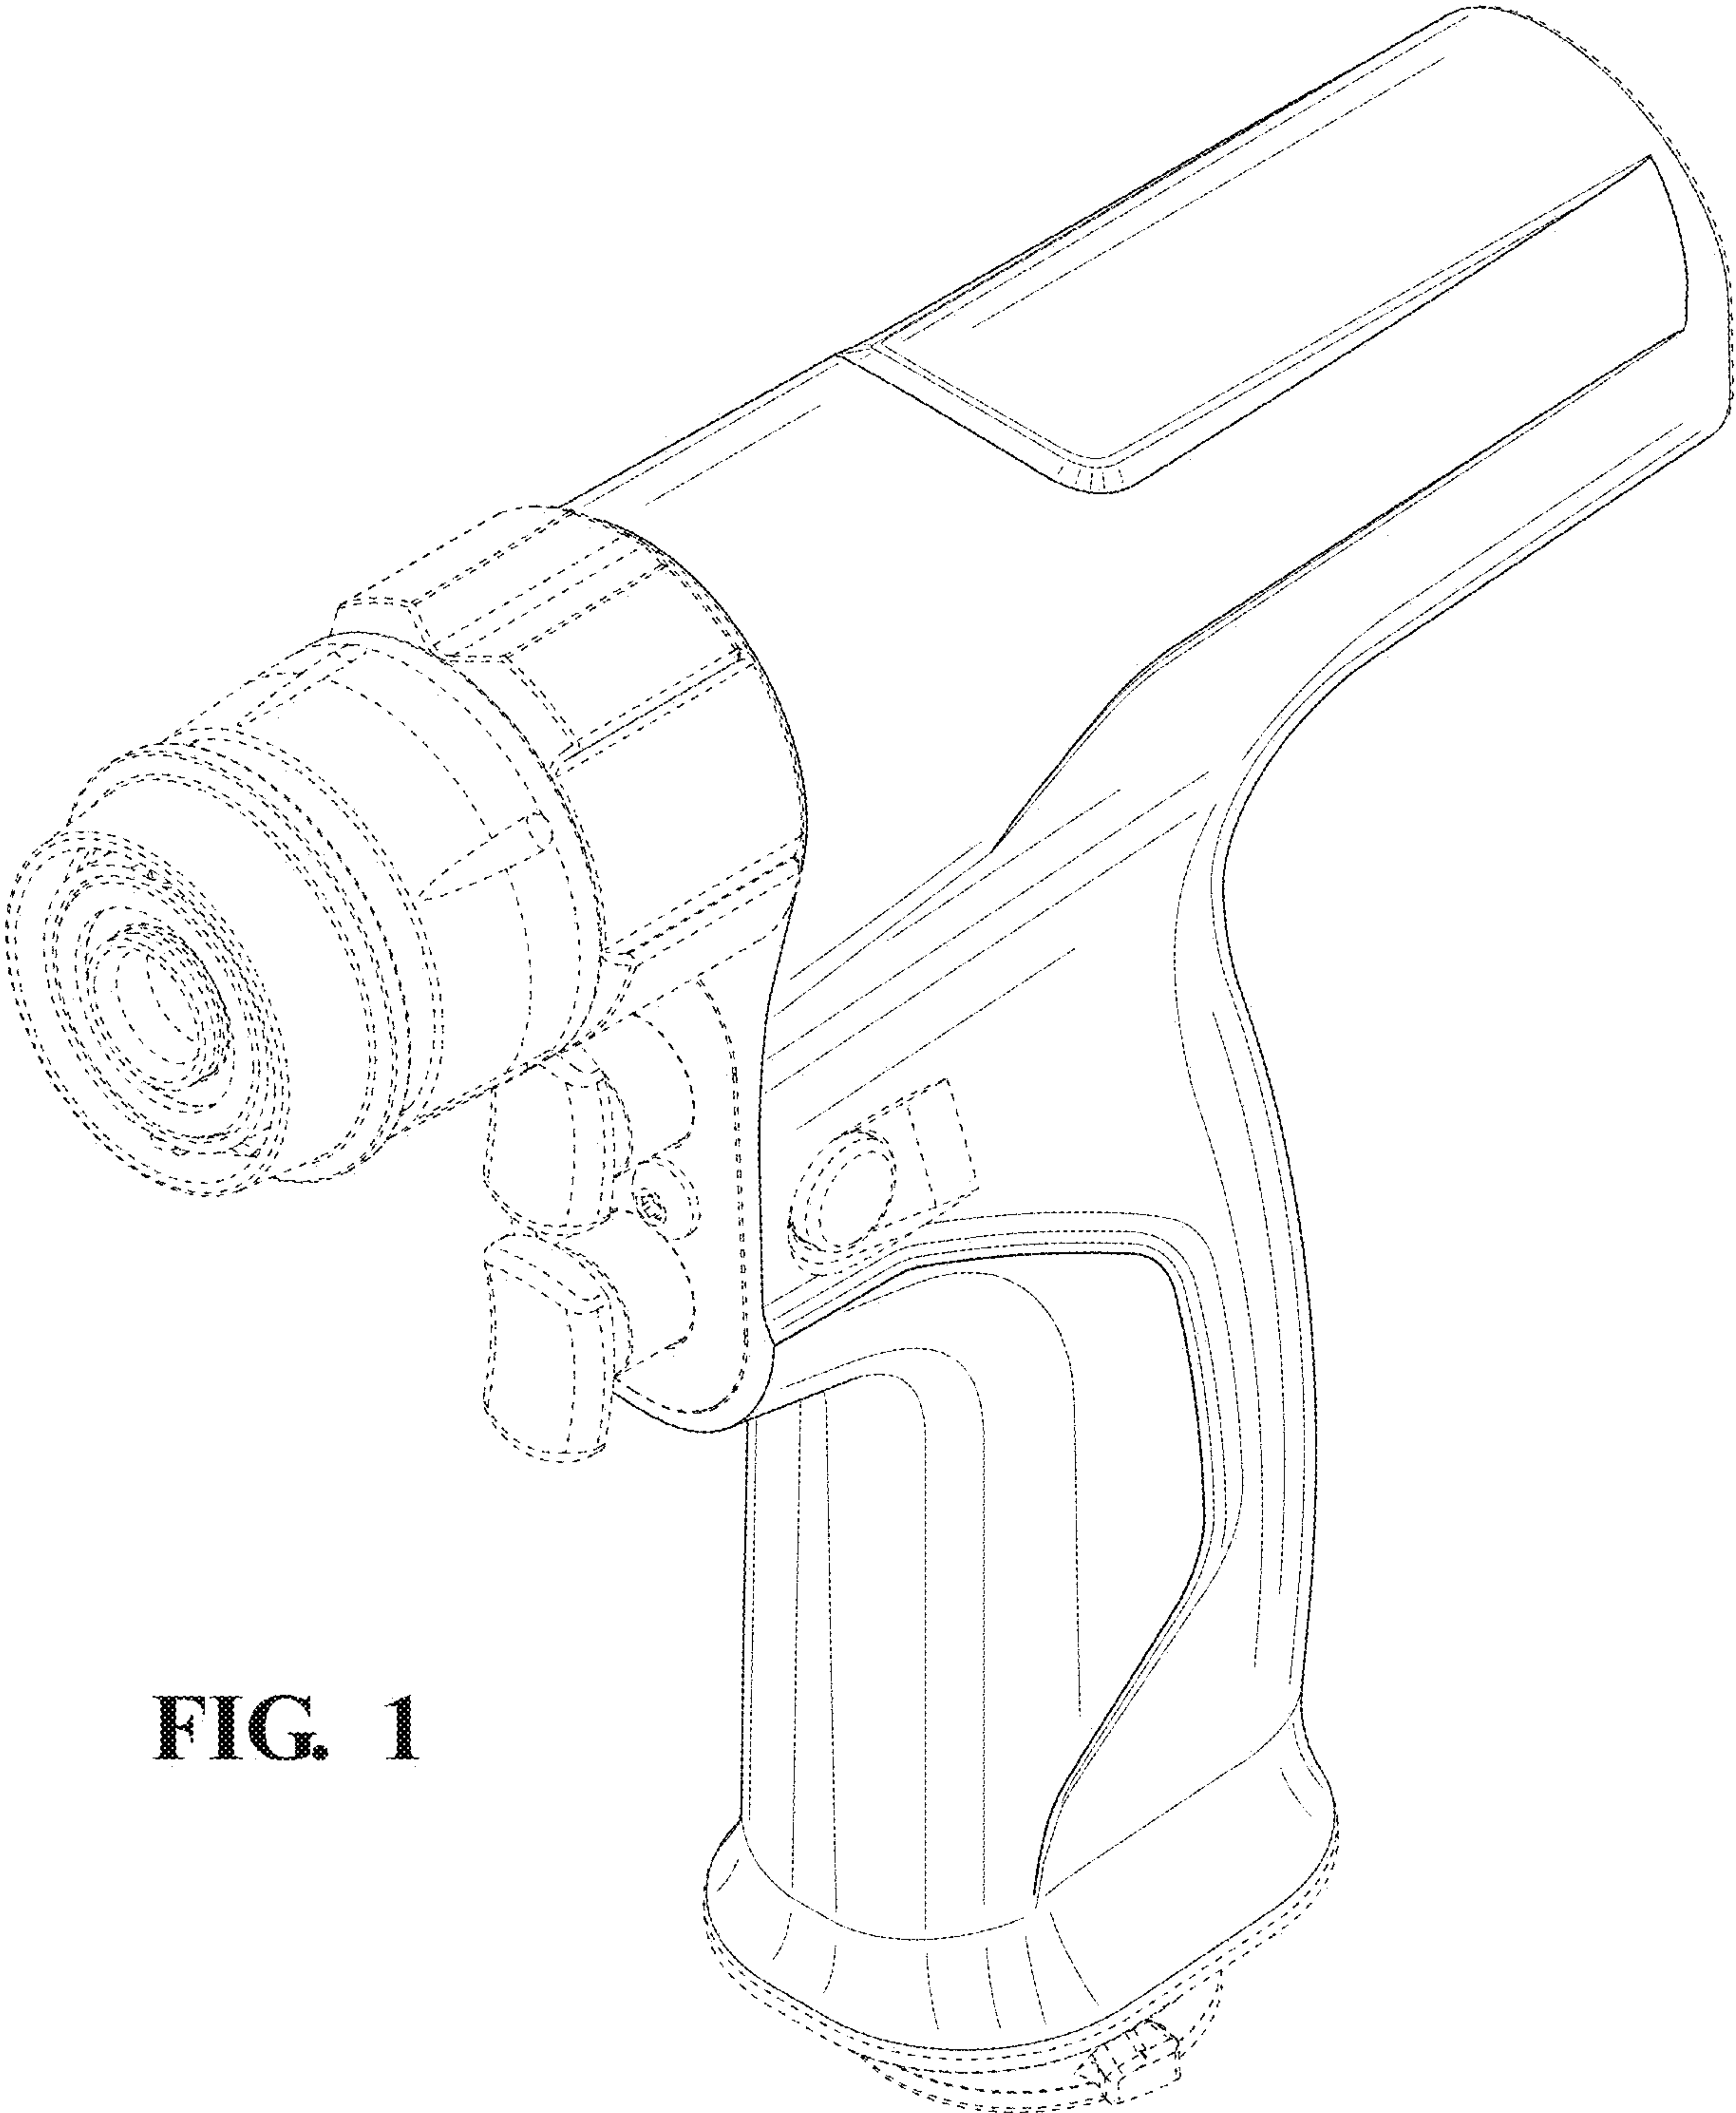


FIG. 1

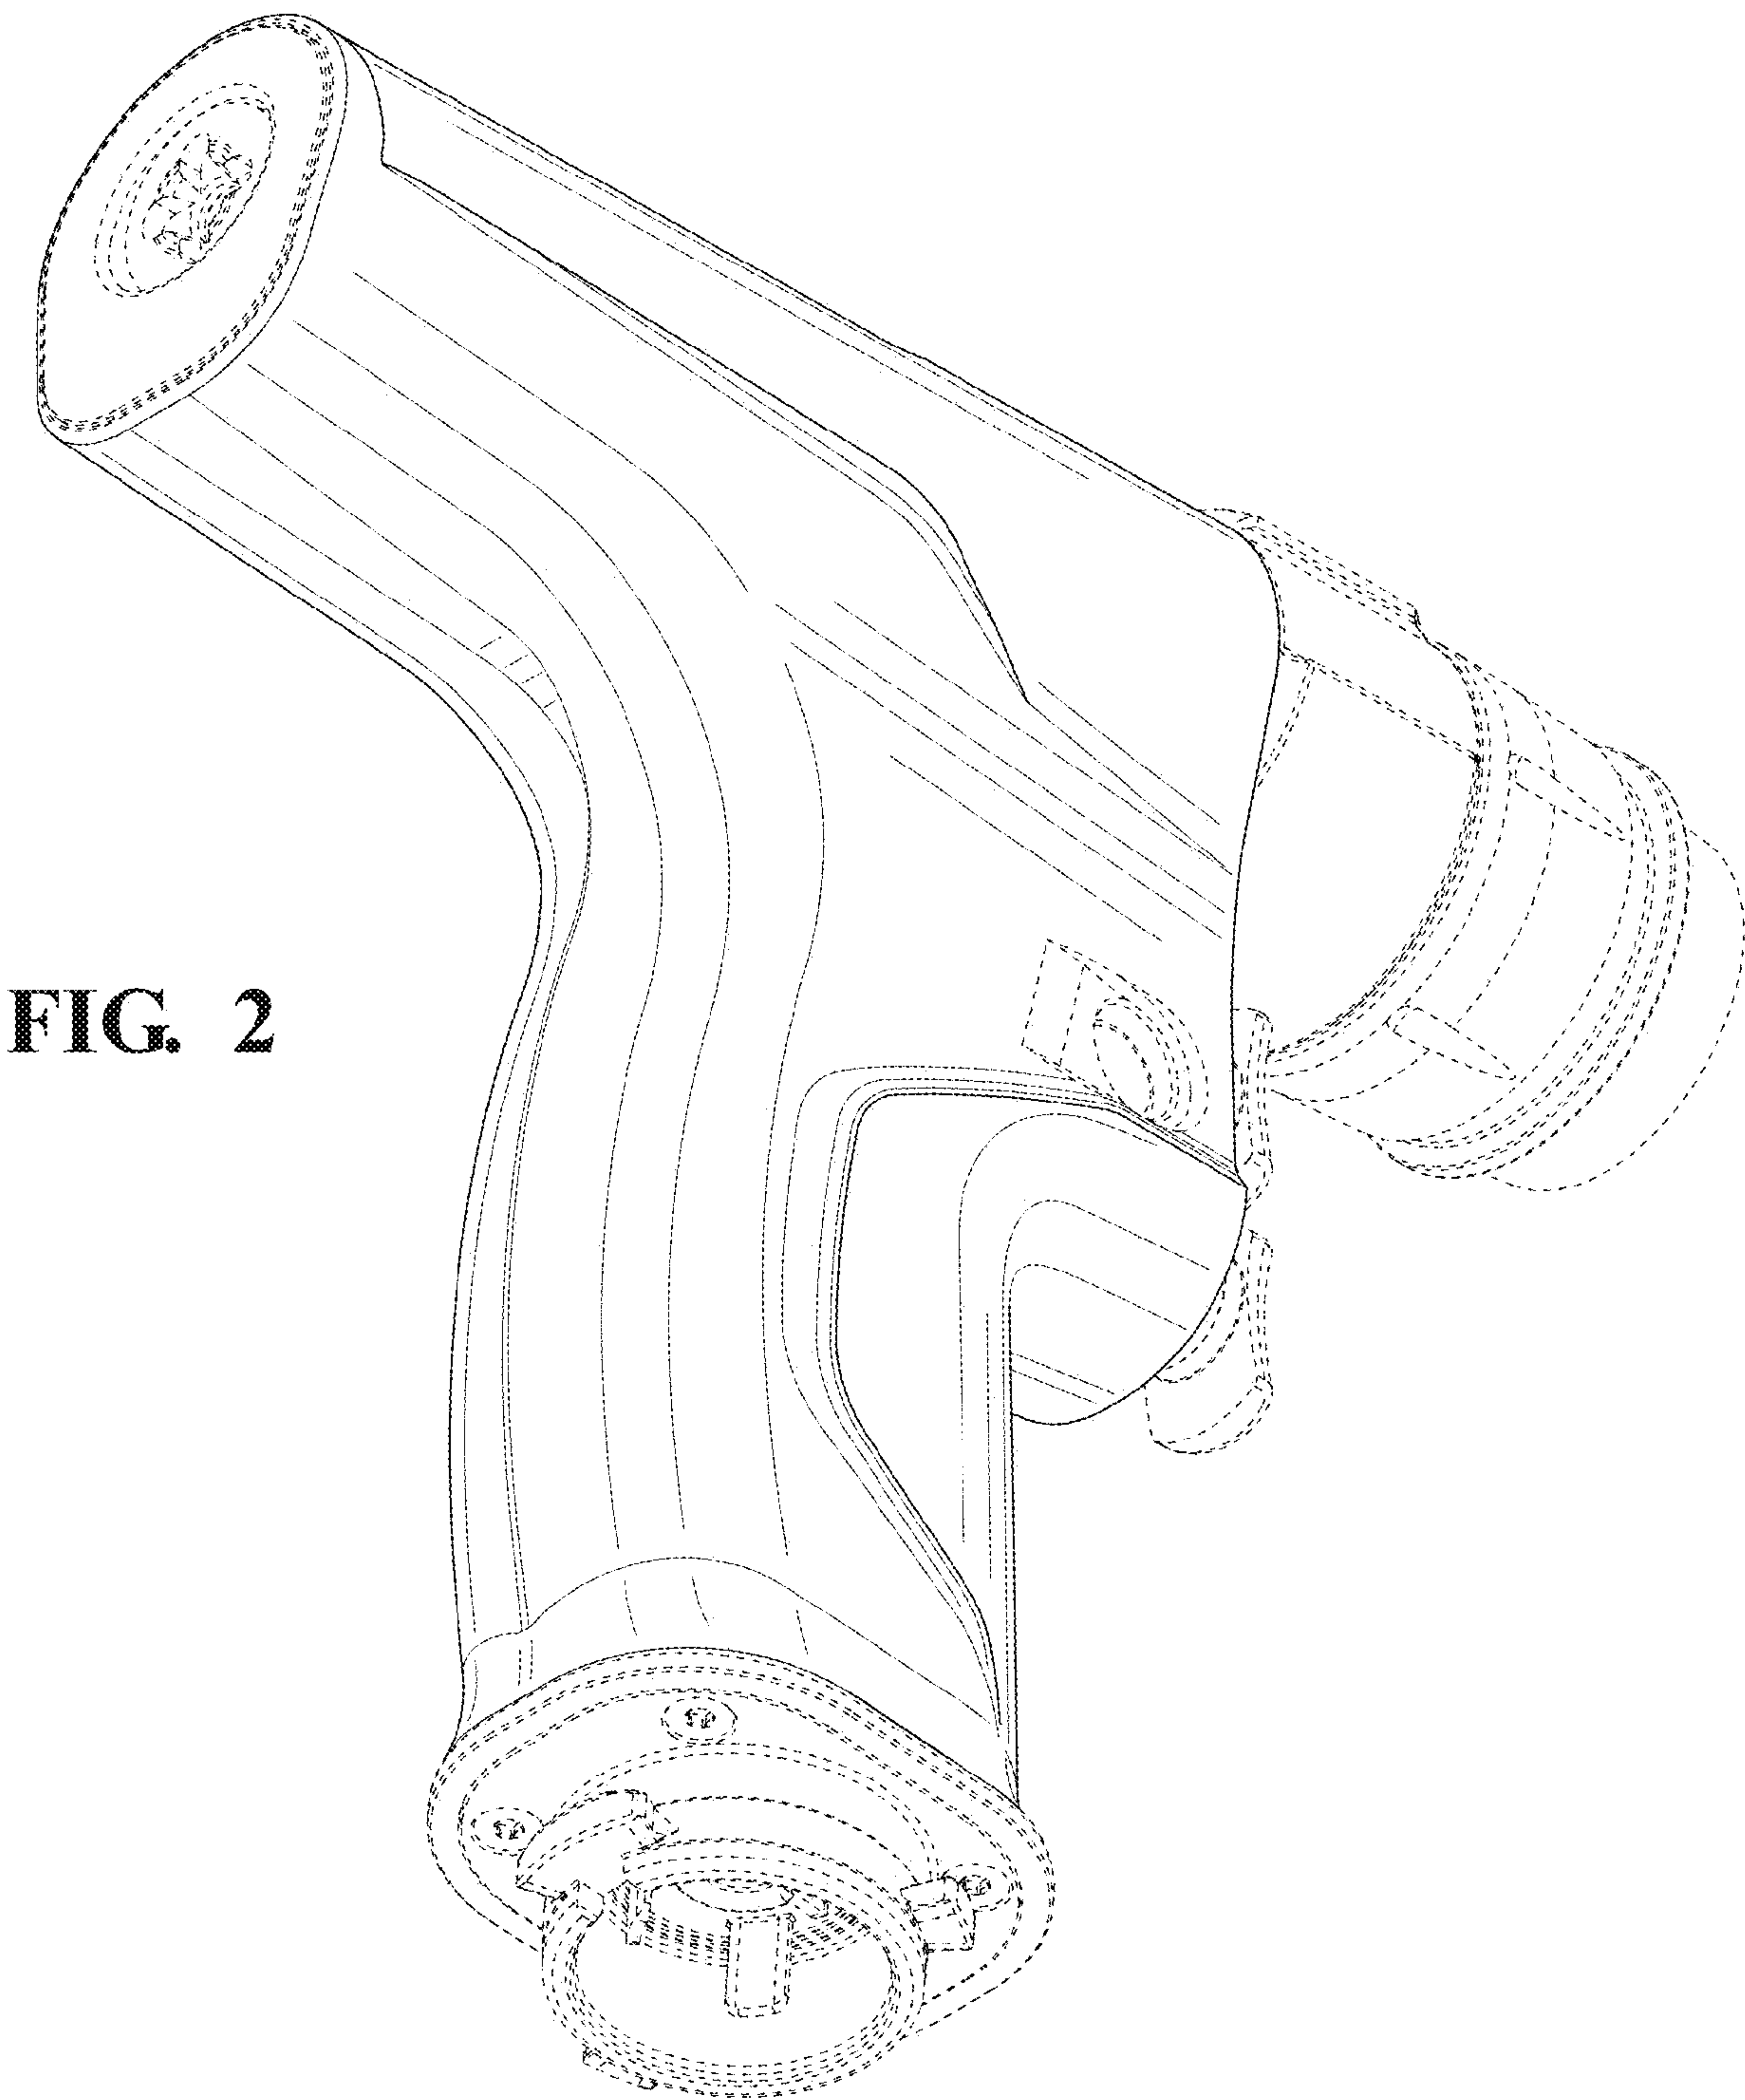
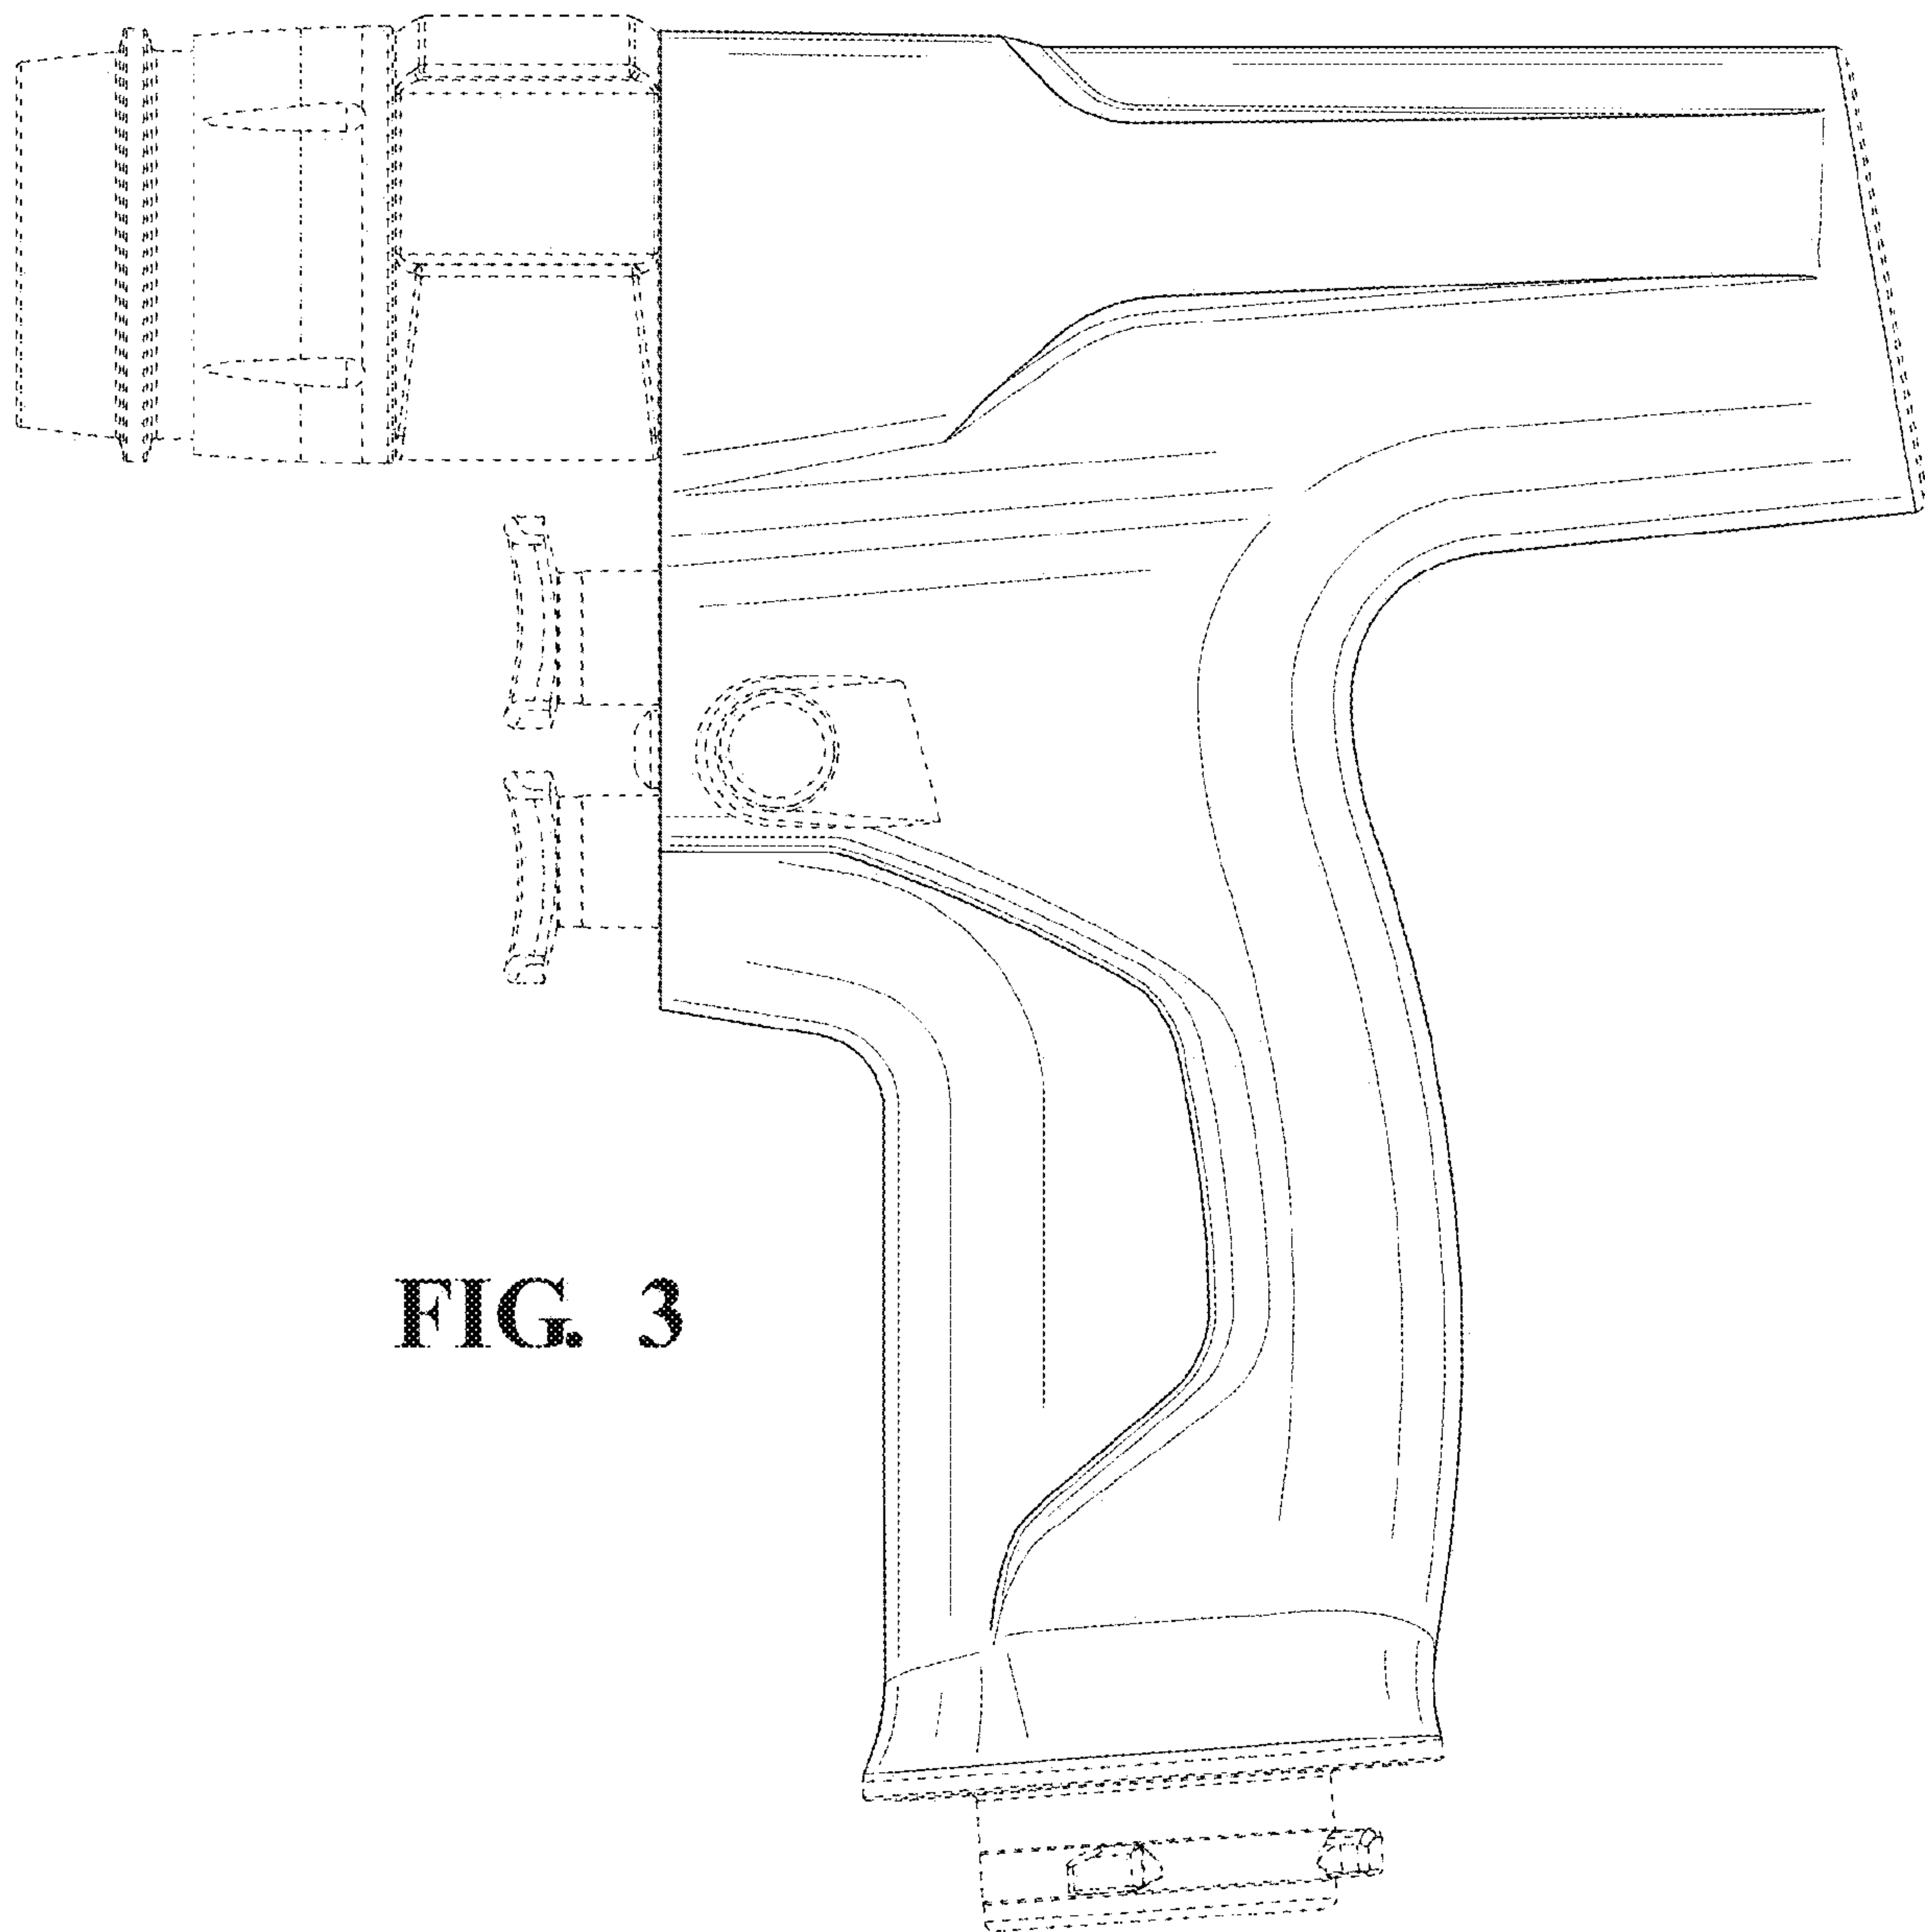


FIG. 2



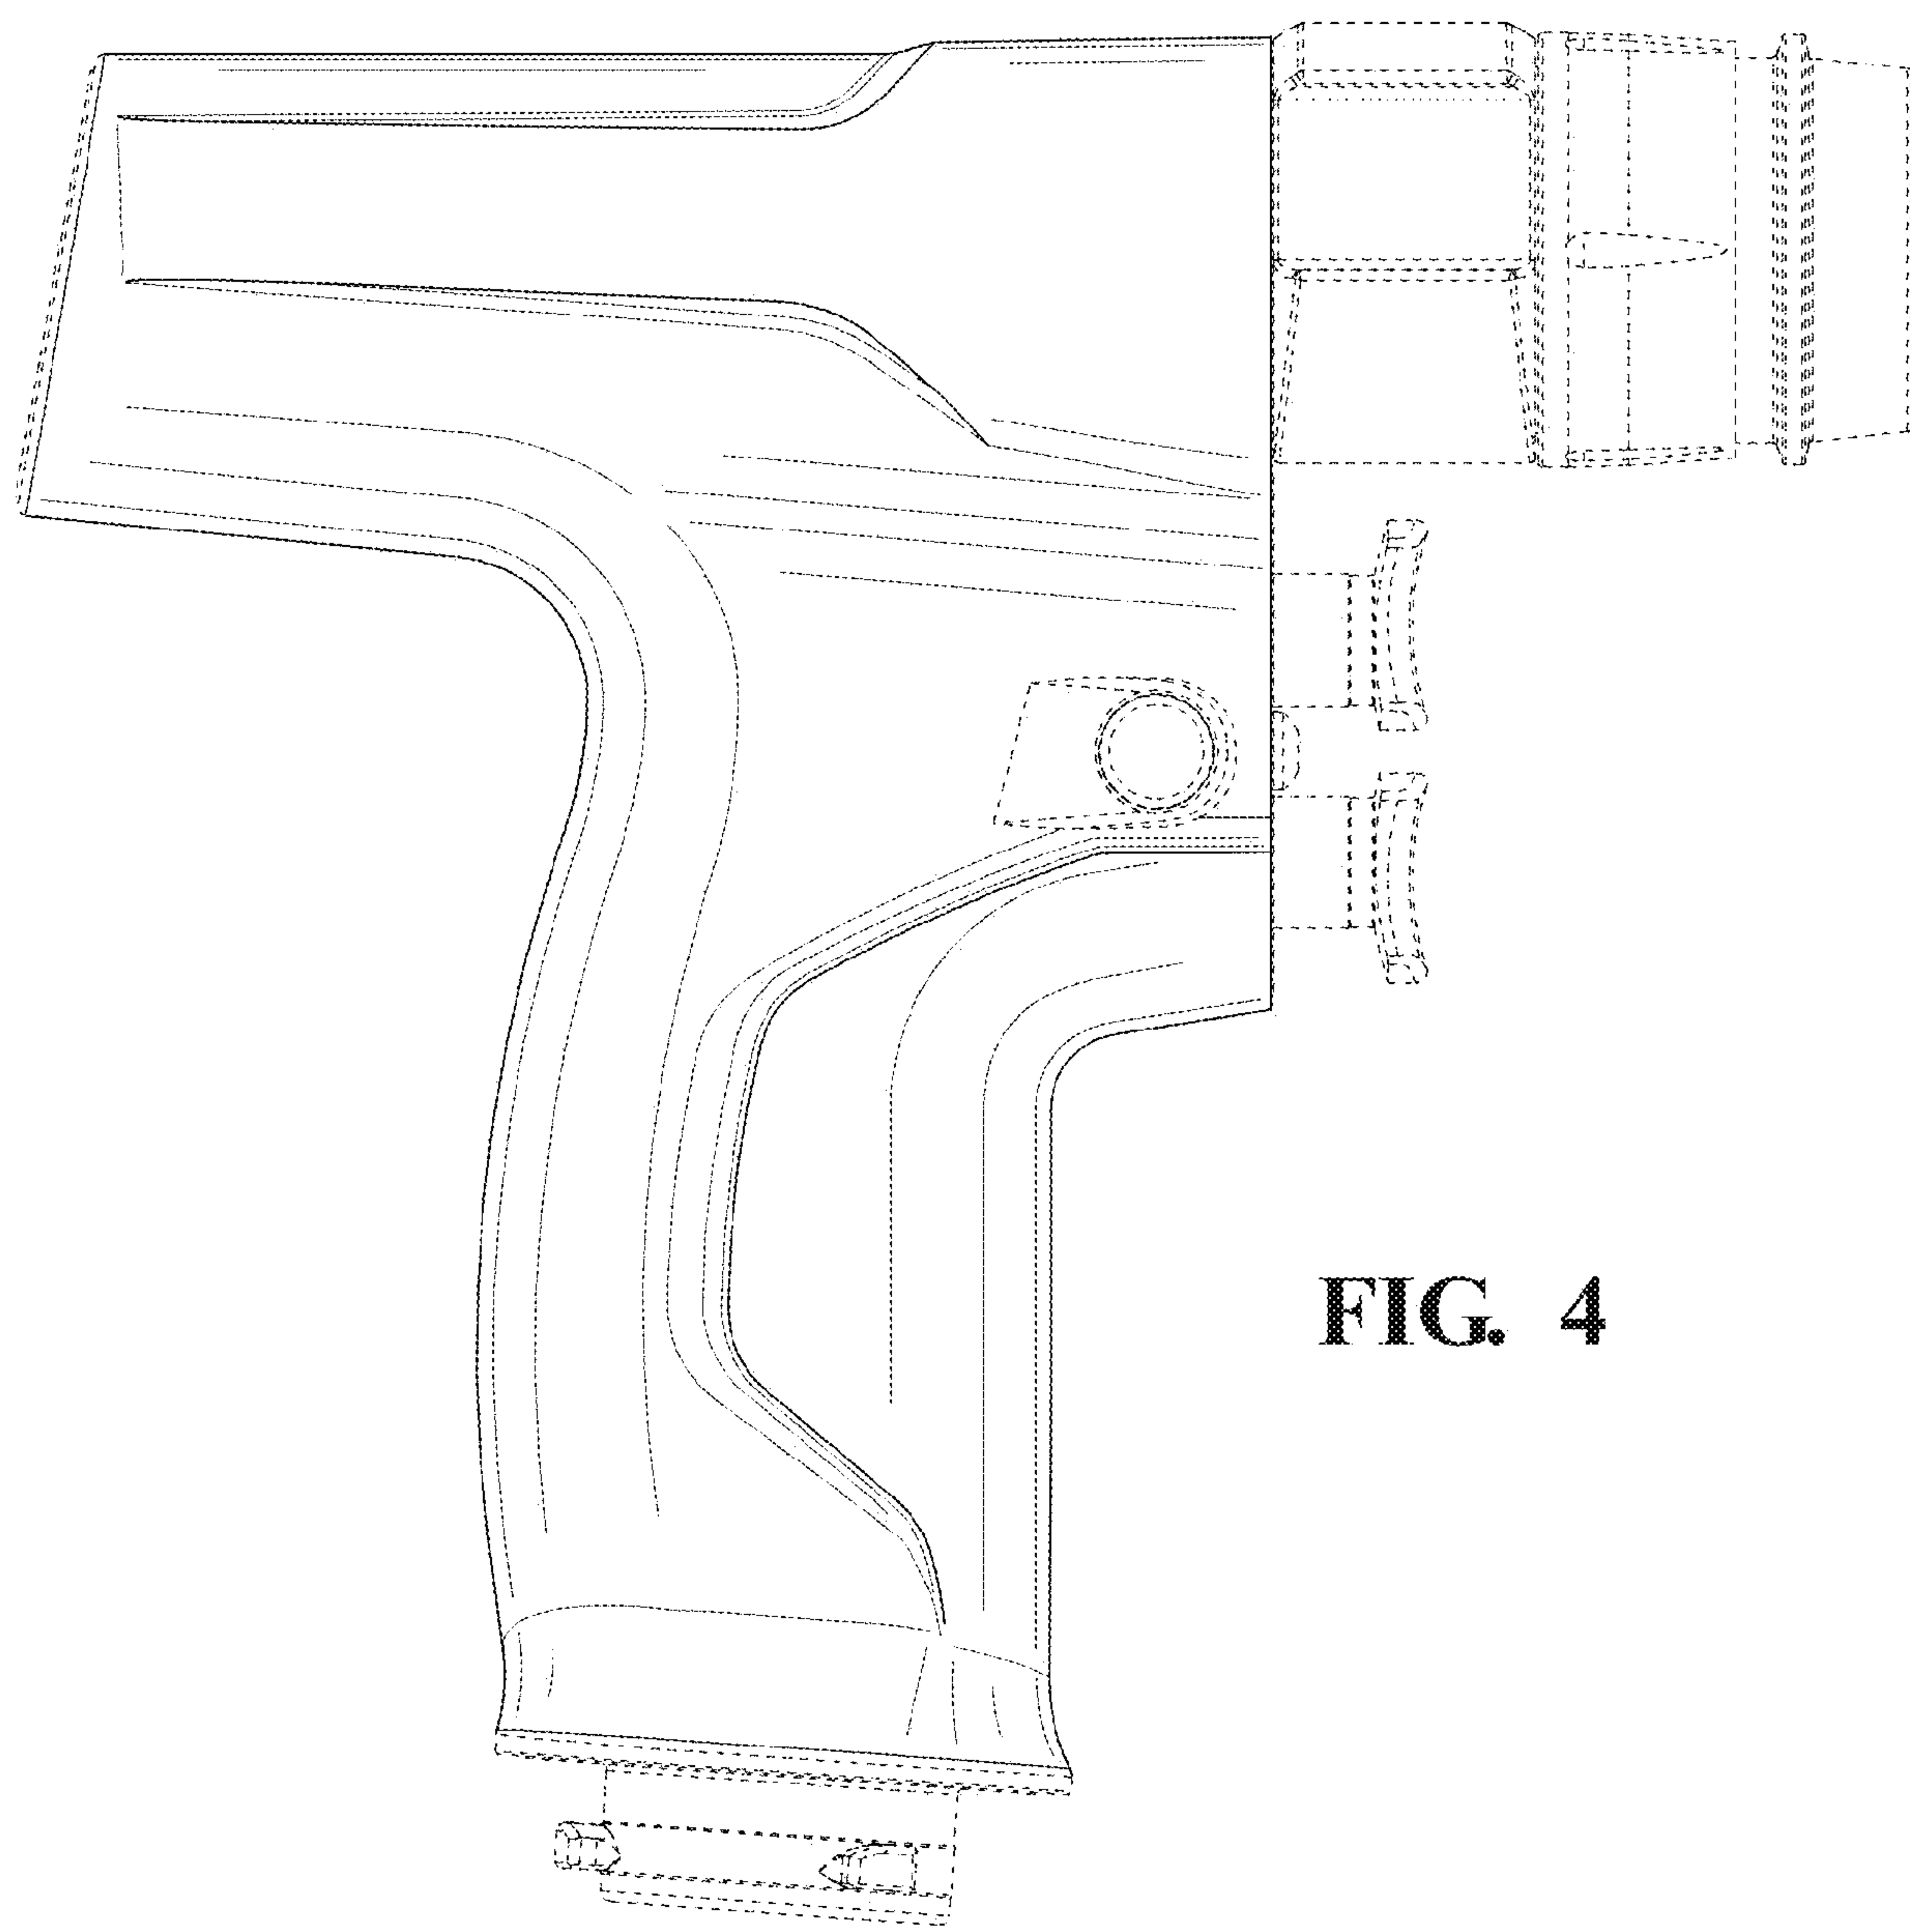


FIG. 4

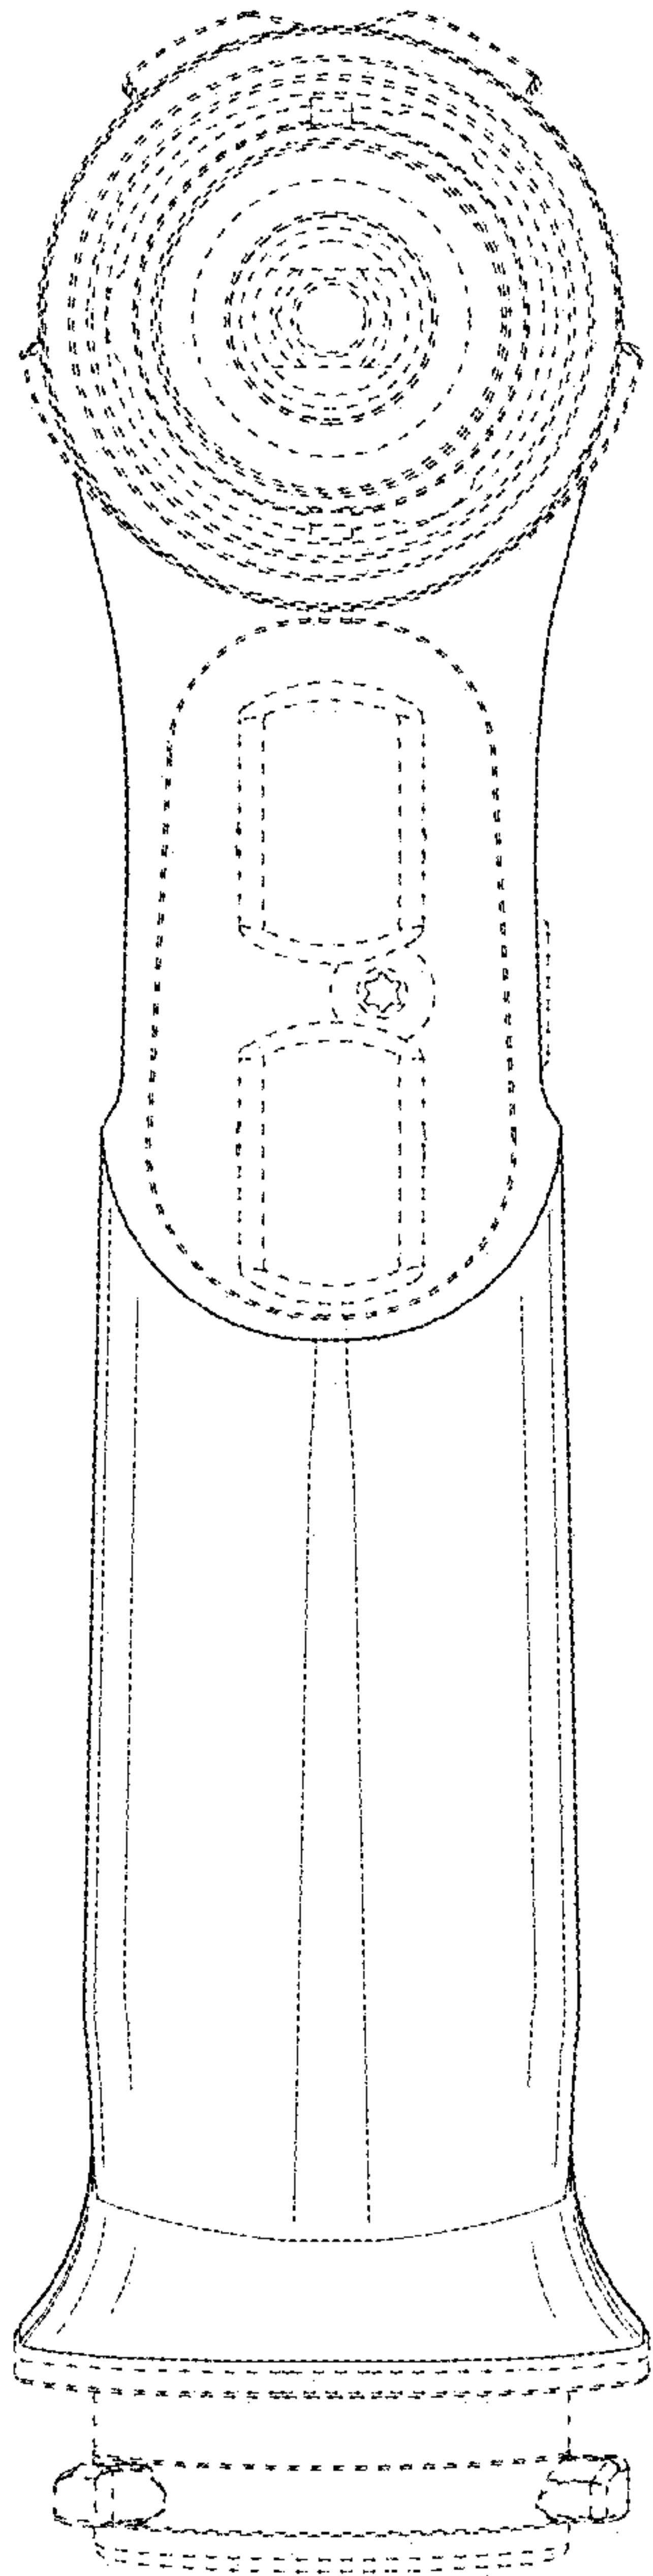


FIG. 5

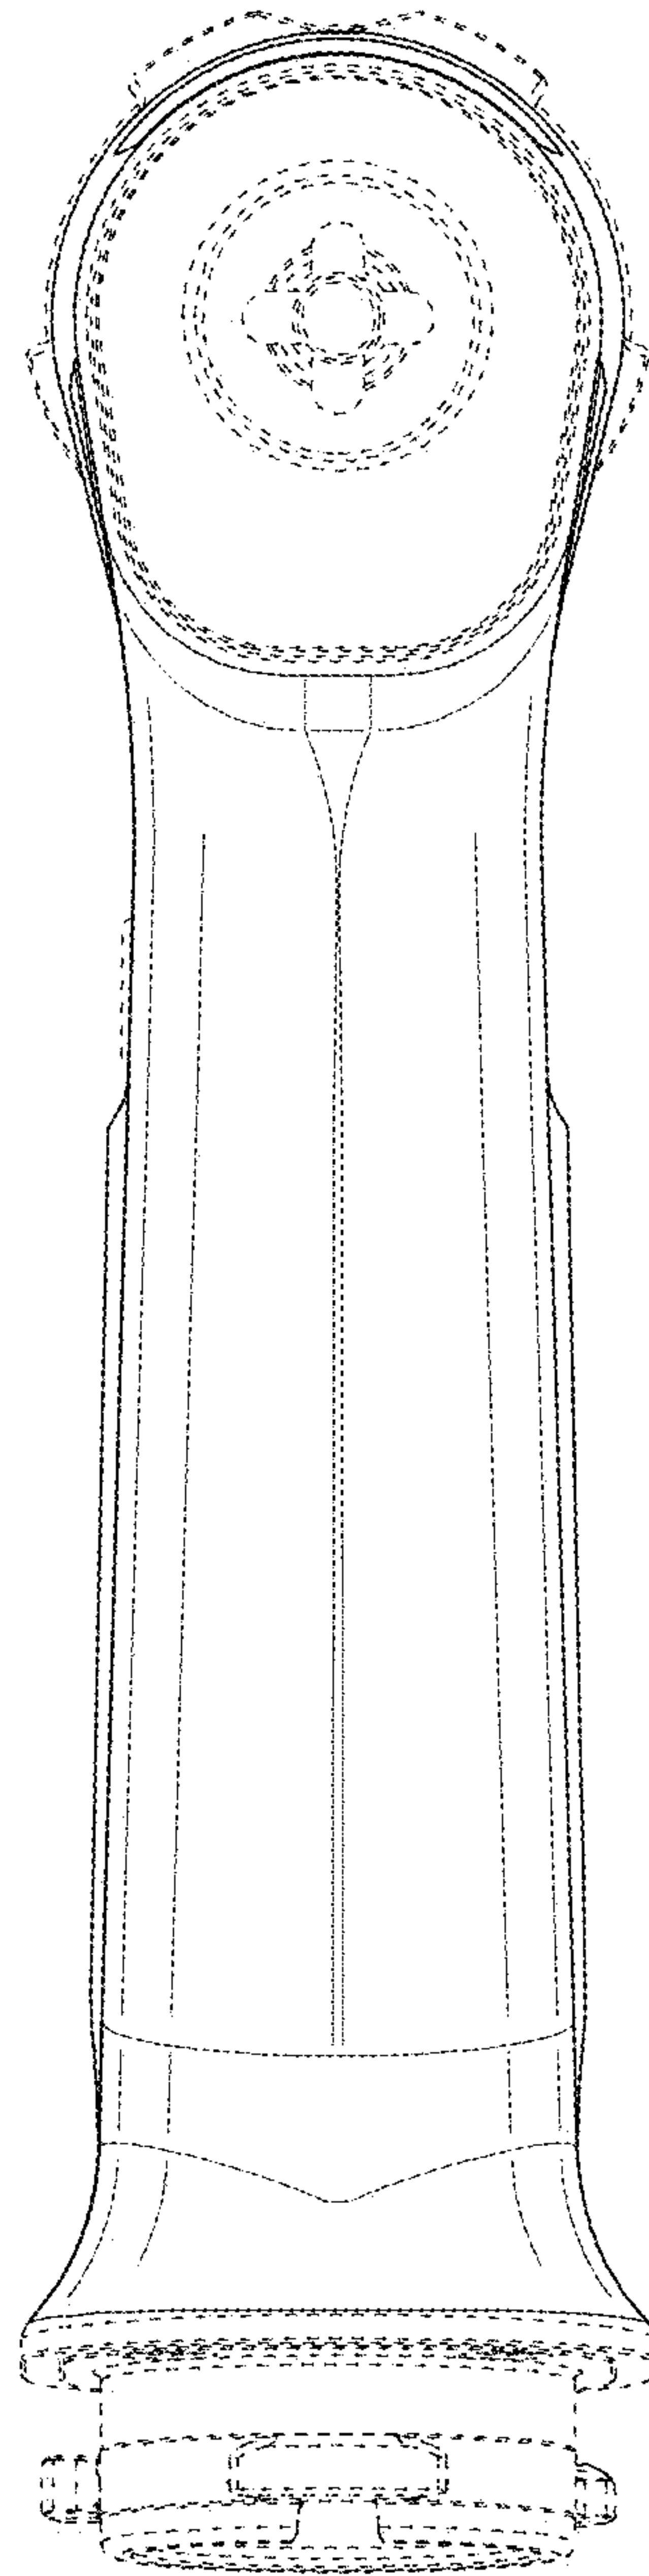


FIG. 6

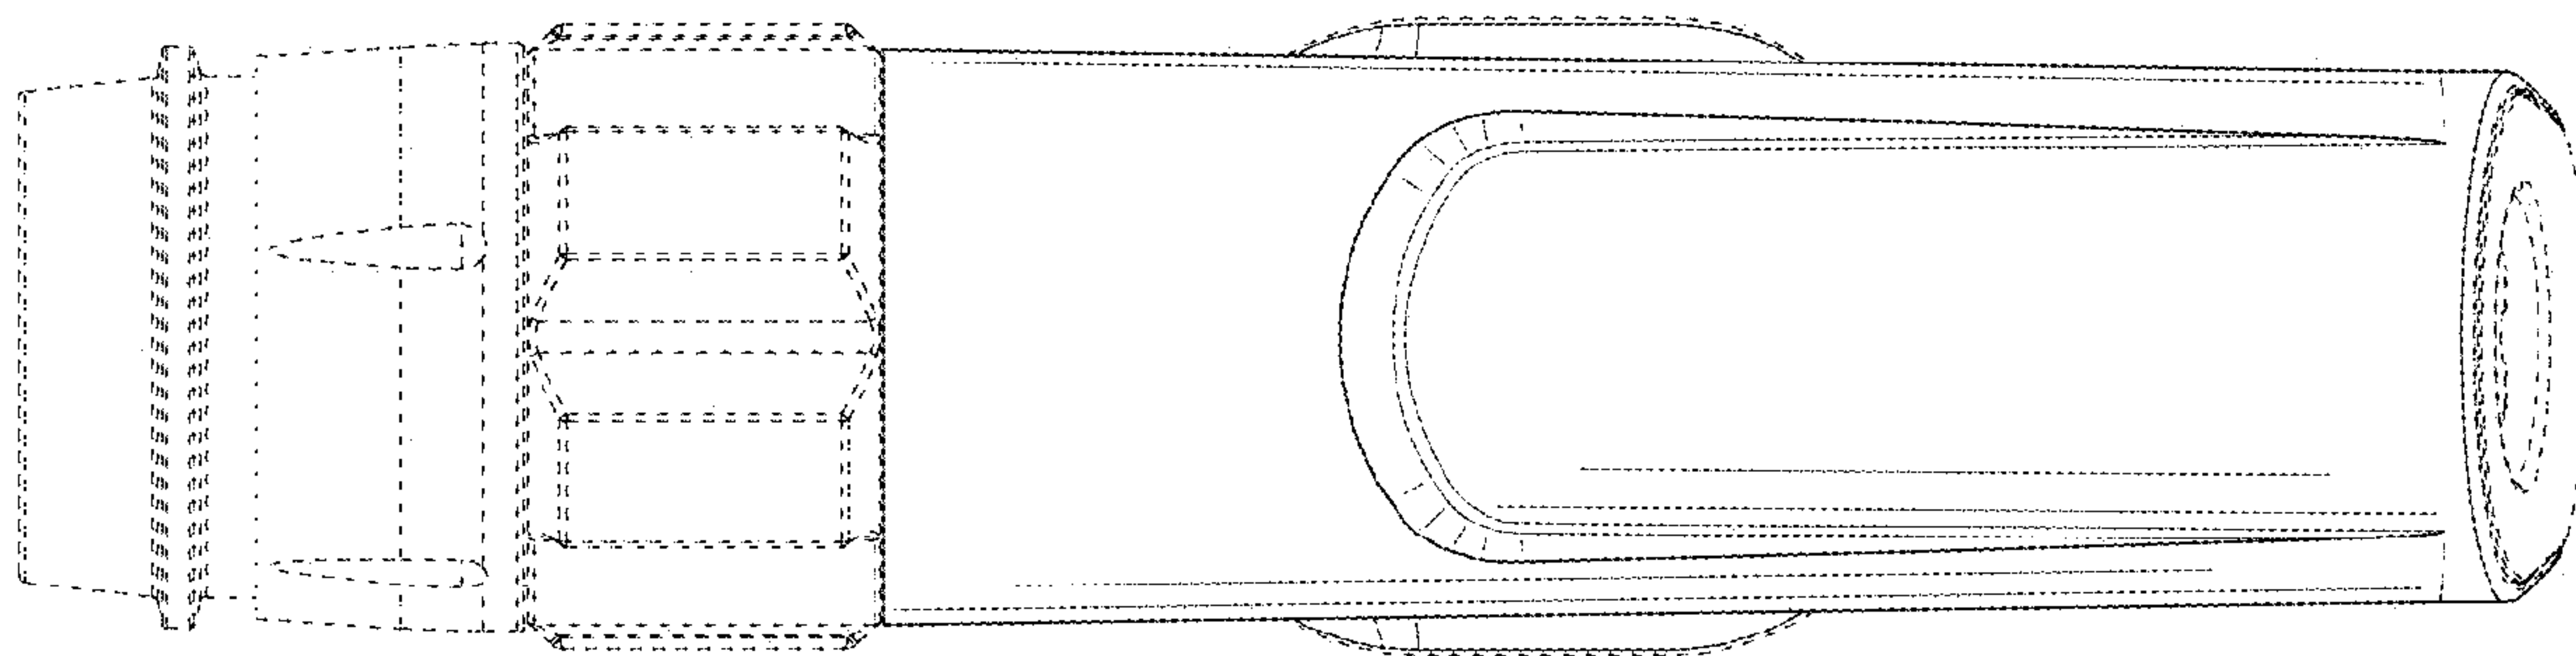


FIG. 7

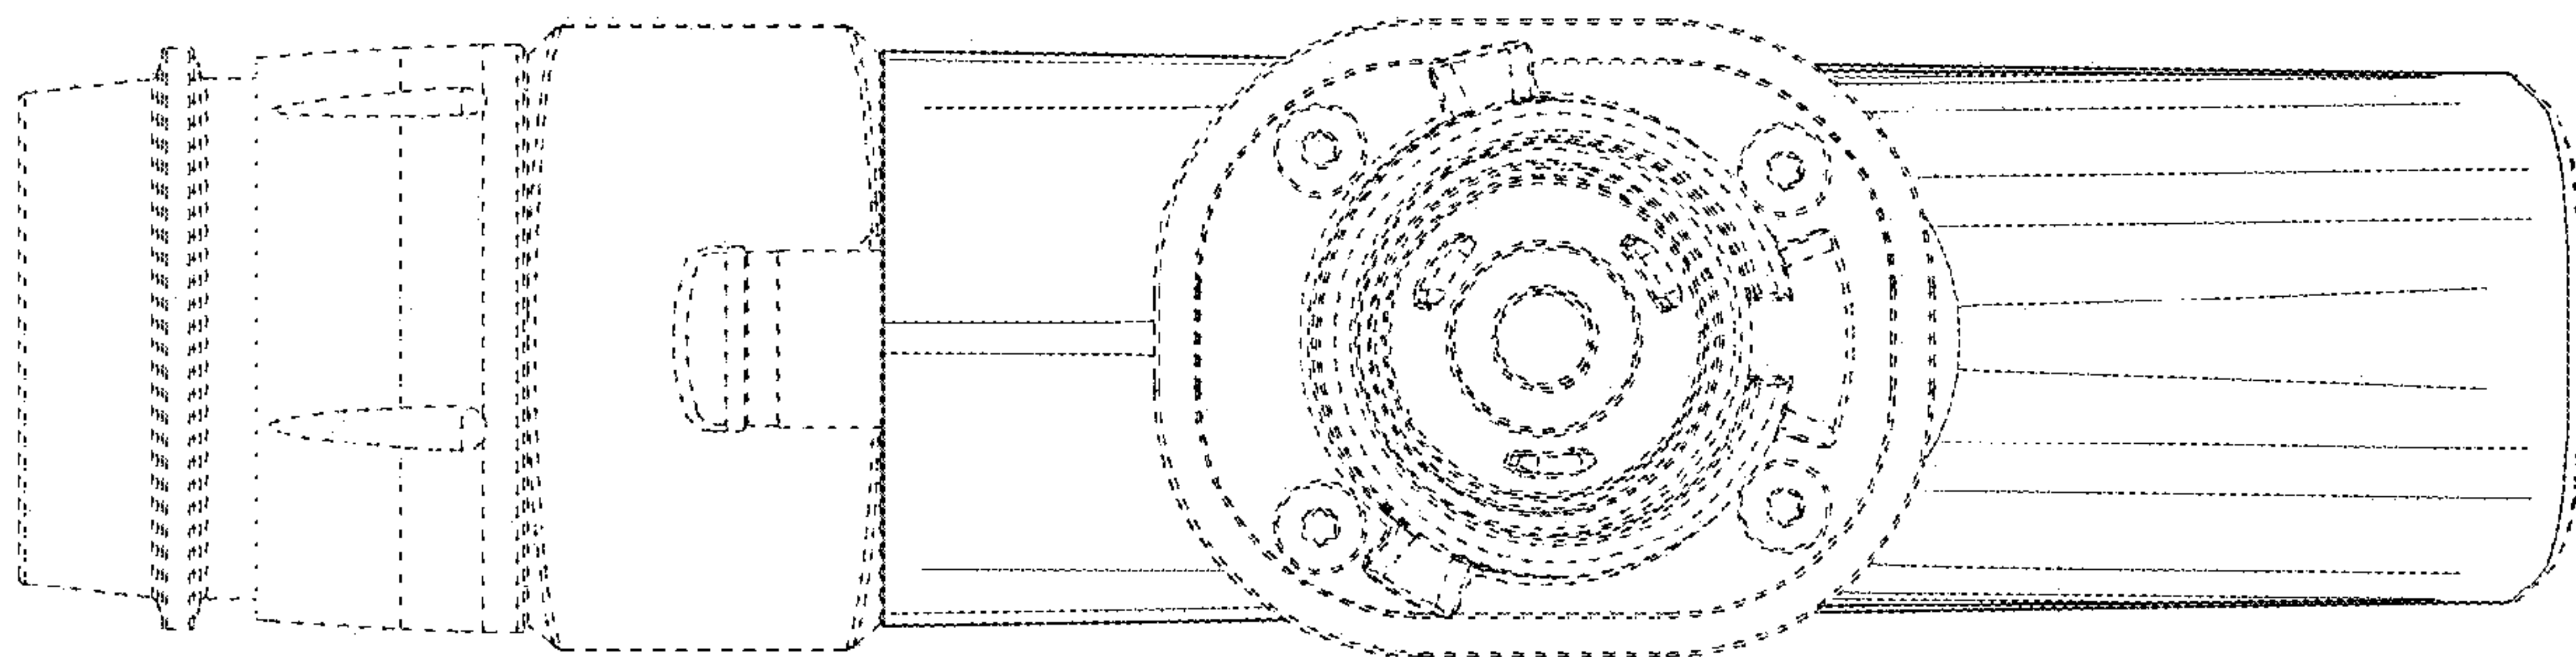


FIG. 8