

(12) **United States Design Patent**
Sedic

(10) **Patent No.: US D1,031,062 S**
(45) **Date of Patent: ** *Jun. 11, 2024**

(54) **STIMULATION DEVICE**

(71) Applicant: **FOREO Inc.**, Las Vegas, NV (US)

(72) Inventor: **Filip Sedic**, Stockholm (SE)

(73) Assignee: **FOREO Inc.**, Las Vegas, NV (US)

(*) Notice: This patent is subject to a terminal disclaimer.

(**) Term: **15 Years**

(21) Appl. No.: **29/846,569**

(22) Filed: **Jul. 18, 2022**

Related U.S. Application Data

(63) Continuation of application No. 29/805,327, filed on Aug. 26, 2021, now Pat. No. Des. 961,109, which is a continuation of application No. 29/705,116, filed on Sep. 10, 2019, now Pat. No. Des. 932,040.

(51) **LOC (14) Cl.** **24-01**

(52) **U.S. Cl.**
USPC **D24/215**

(58) **Field of Classification Search**
USPC D24/200, 211, 212, 213, 214, 215;
D28/7, 78; D10/1
CPC ... A61H 2015/0042; A61H 7/007; A61H 9/00
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D581,543	S	*	11/2008	Ferber		D24/215
D665,915	S	*	8/2012	Ma		D24/215
D737,990	S	*	9/2015	Lee		D24/215
D845,631	S	*	4/2019	Sedic		D4/100
D850,111	S	*	6/2019	Sedic		D4/100
D870,909	S	*	12/2019	Sedic		D24/215
D872,939	S	*	1/2020	Tammabattula		D28/63

D872,940	S	*	1/2020	Tammabattula		D28/63
D882,268	S	*	4/2020	Sedic		D4/100
D882,807	S	*	4/2020	Xiong		D24/214
D885,063	S	*	5/2020	Xiong		D4/116
D886,642	S	*	6/2020	Zhou		D10/22
D893,199	S	*	8/2020	Sedic		D4/137
D895,821	S	*	9/2020	Lin		D24/200
D932,040	S	*	9/2021	Sedic		D24/215
D932,041	S	*	9/2021	Sedic		D24/215
D932,043	S	*	9/2021	Sedic		D24/215

(Continued)

OTHER PUBLICATIONS

Foreo, “Bear”, Access Date: Feb. 28, 2024. <https://www.foreo.com/bear-collection?v=1625&p=125&s=1> (Year: 2024).*

(Continued)

Primary Examiner — Michael A Maharajh
(74) *Attorney, Agent, or Firm* — Evan Feldstein


(57) **CLAIM**

I claim the ornamental design for a stimulation device, as shown and described.

DESCRIPTION

FIG. 1 is a front view of a stimulation device.
FIG. 2 is a right side view of the stimulation device.
FIG. 3 is a left side view of the stimulation device.
FIG. 4 is a rear view of the stimulation device.
FIG. 5 is a bottom view of the stimulation device.
FIG. 6 is a top view of the stimulation device; and,
FIG. 7 is a perspective view of the stimulation device.
The broken lines shown in the drawings are for the purpose of illustrating portions of the stimulation device, which form no part of the claimed design. The letters FOREO and indicia shown in broken lines are for the purpose of illustrating environmental structure, which form no part of the claimed design.

1 Claim, 7 Drawing Sheets

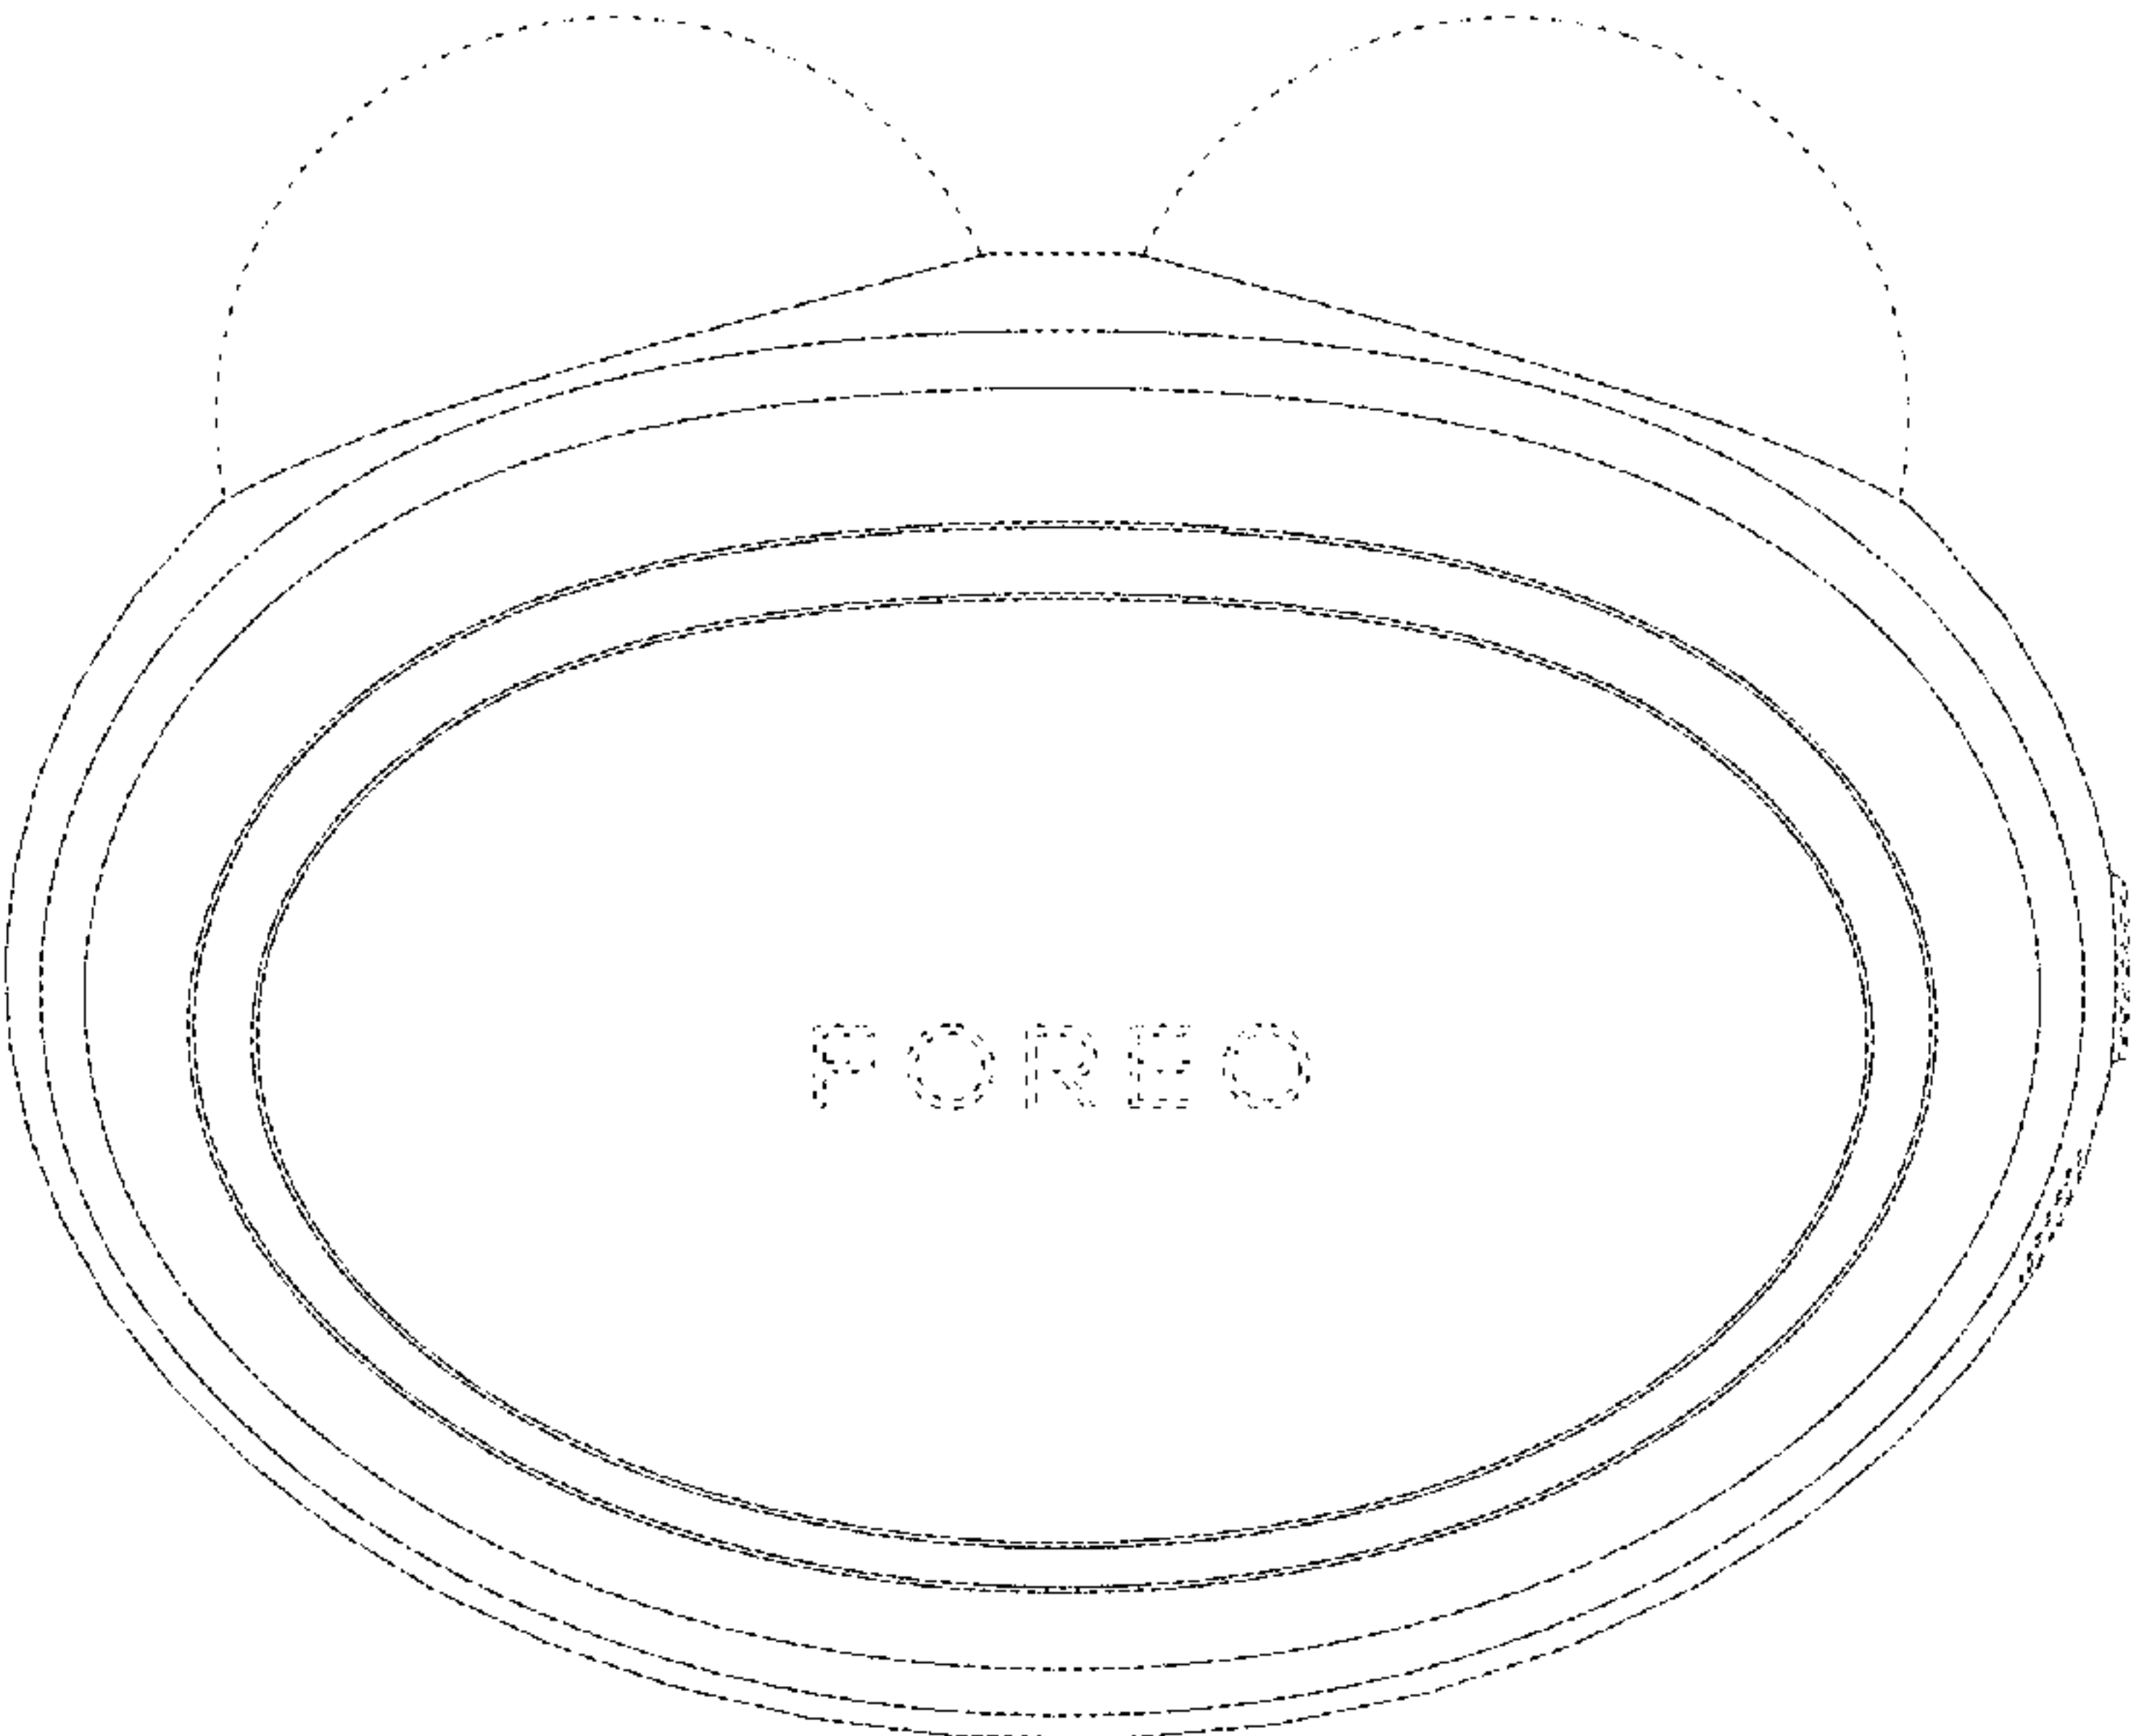

(56) **References Cited**

U.S. PATENT DOCUMENTS

D951,470	S	*	5/2022	Wersland		A61H 23/006
						D24/215
D953,553	S	*	5/2022	Peterson		D24/214
D961,800	S	*	8/2022	Sedic		D24/215
D1,015,555	S	*	2/2024	Lee		D24/214

OTHER PUBLICATIONS

Youtube, “Sculpting face with Foreo Bear”, Published Date: Jun. 25, 2020. <https://www.youtube.com/watch?v=0lku4TXK7IY> (Year: 2020).*

* cited by examiner

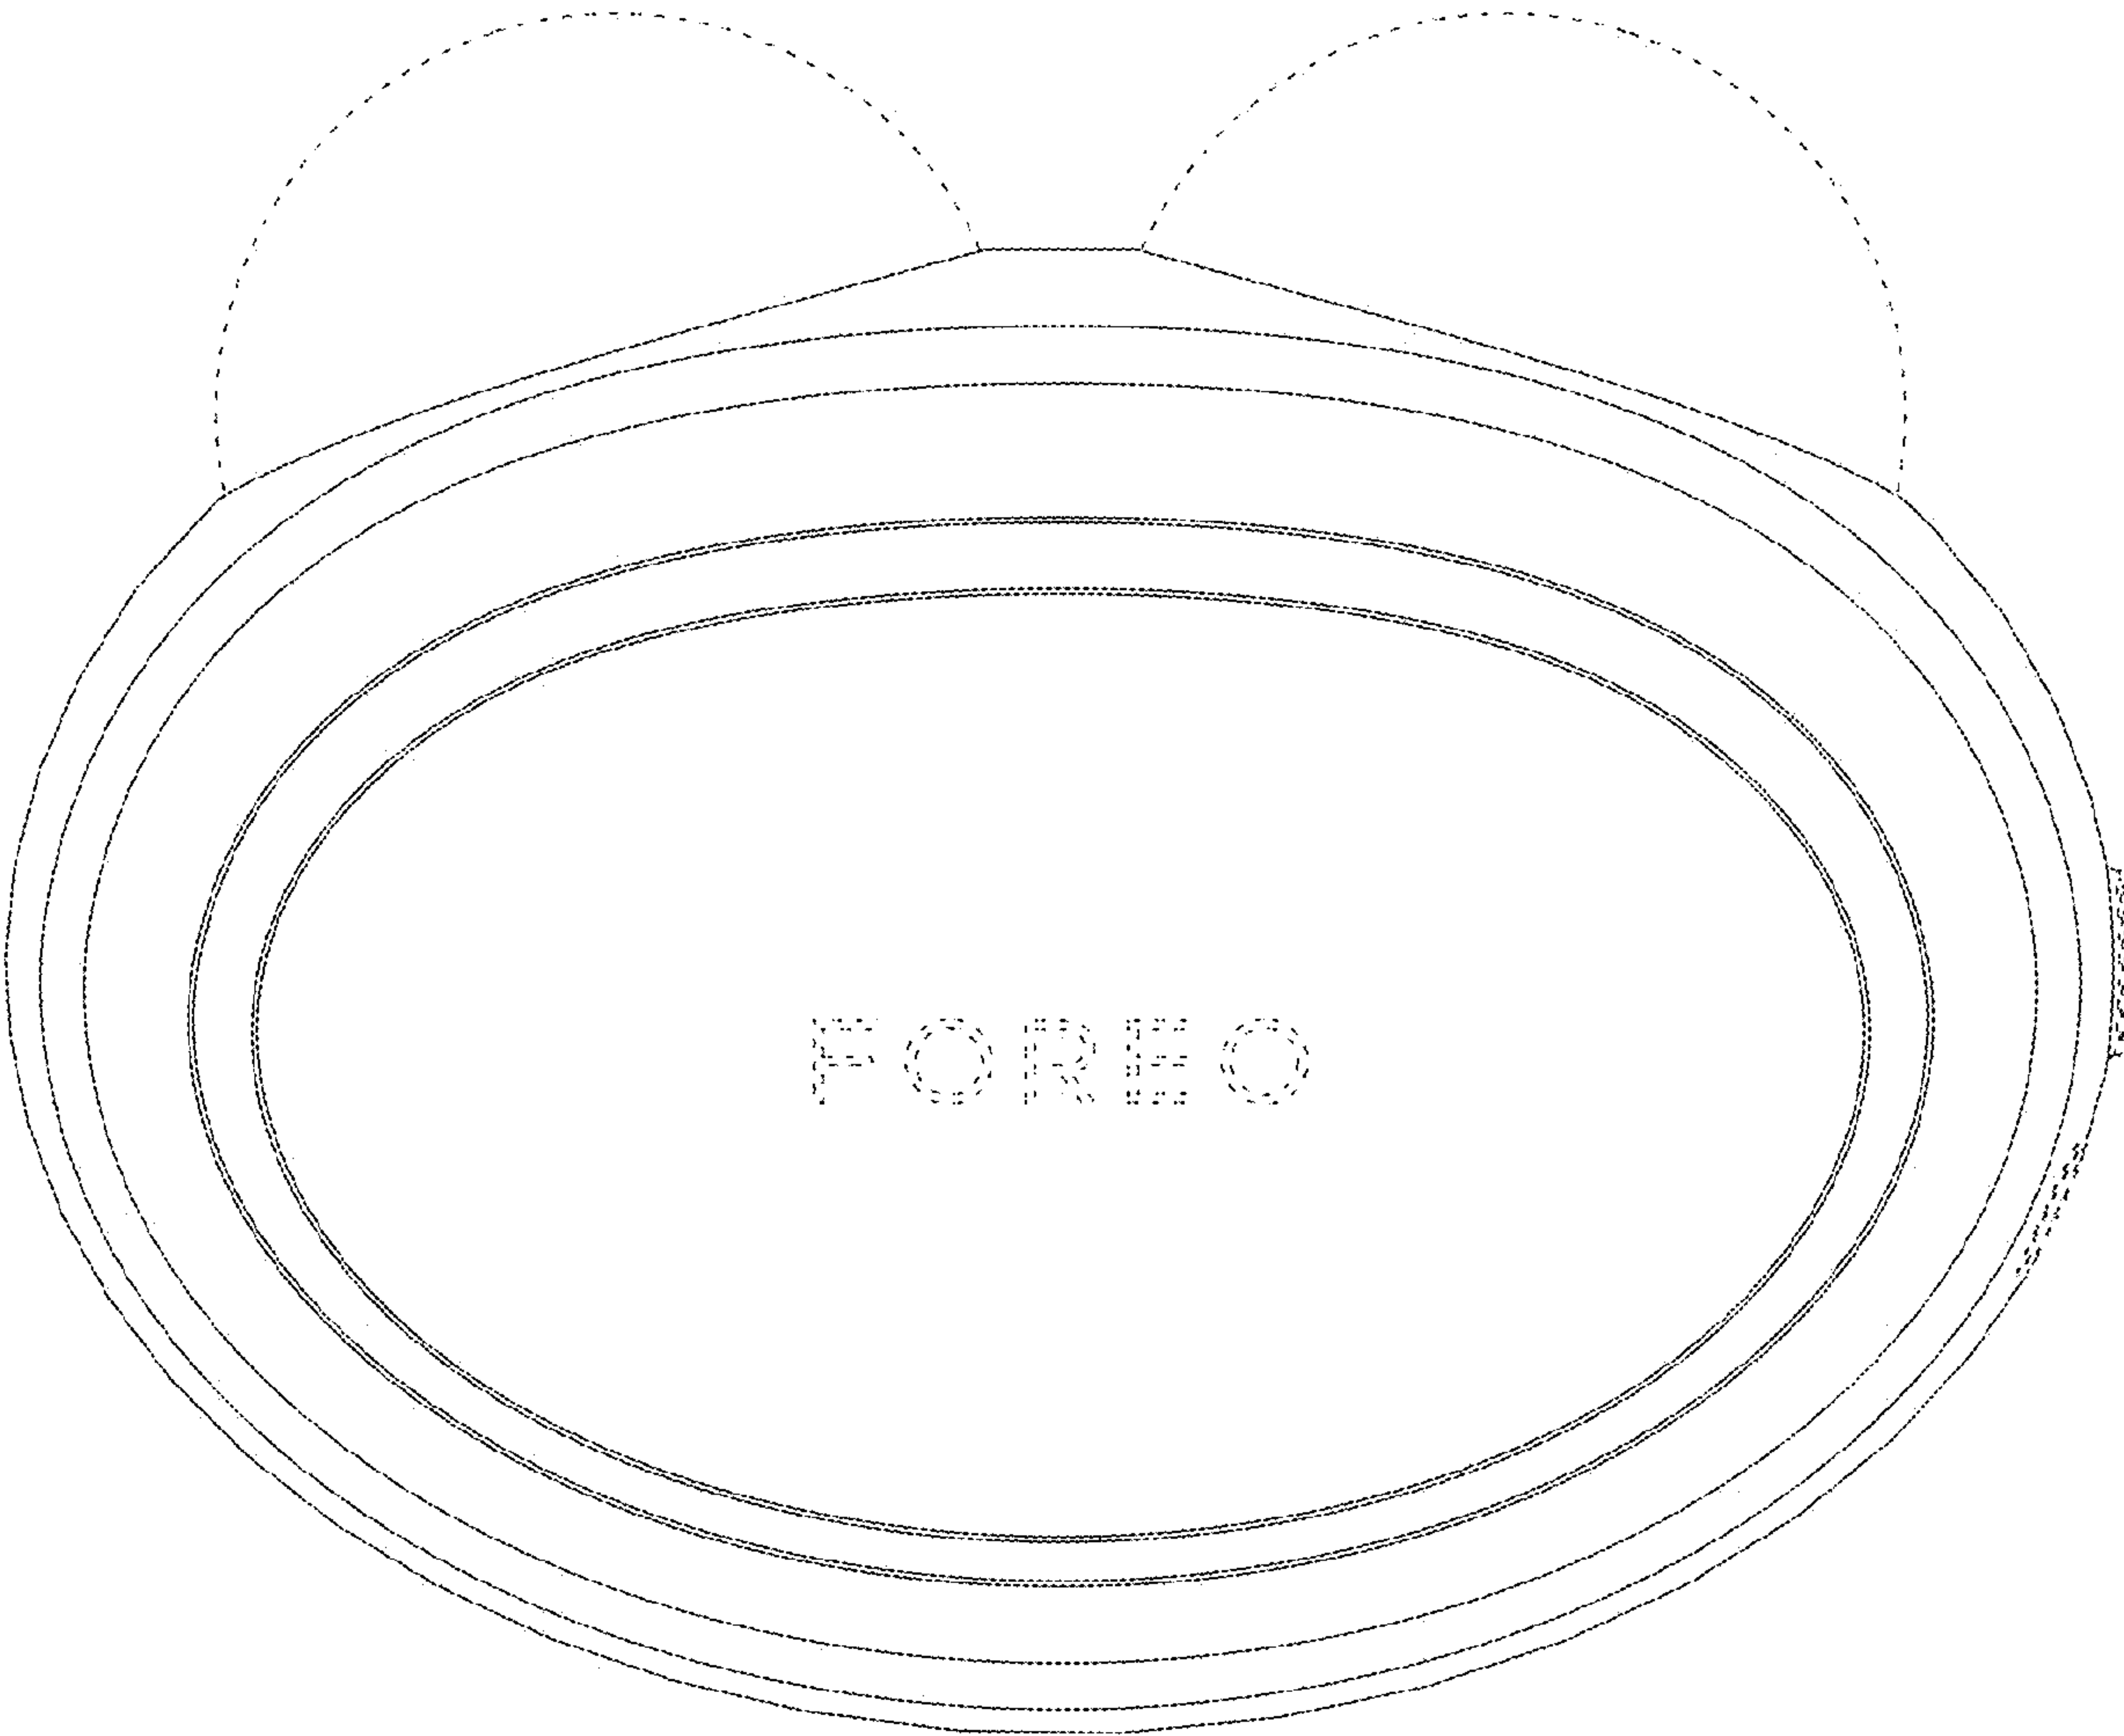


FIG. 1

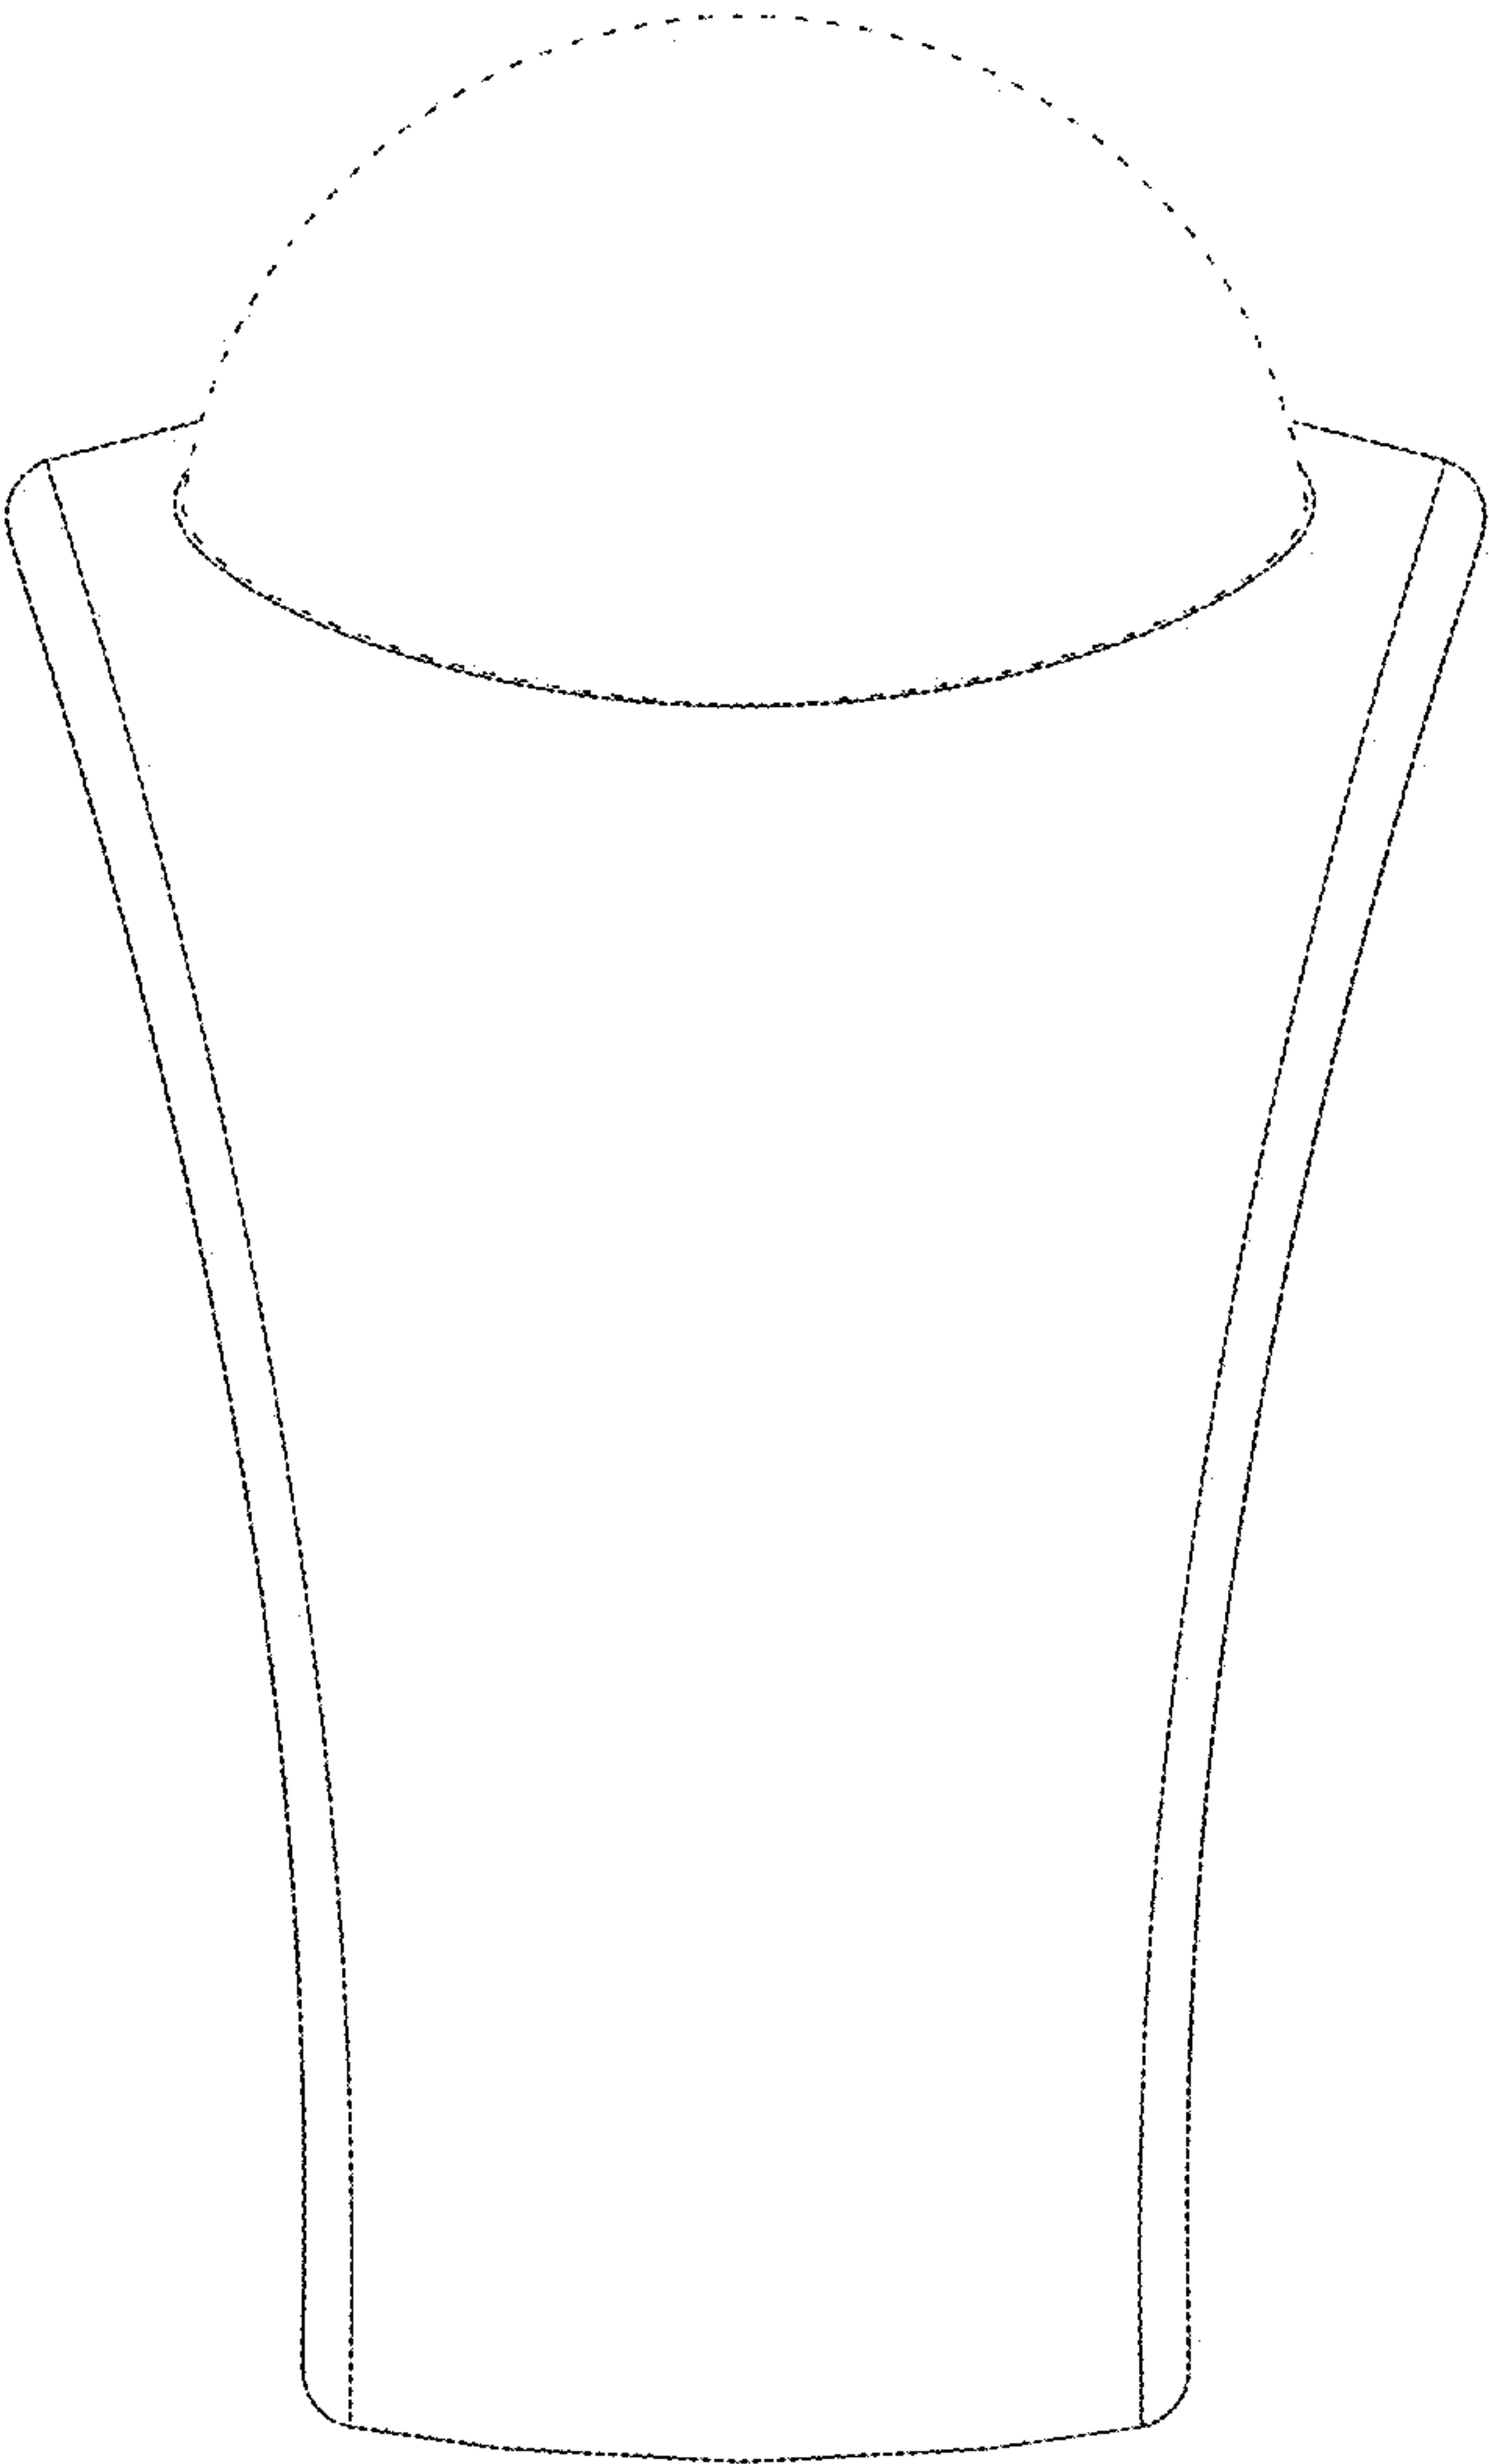


FIG. 2

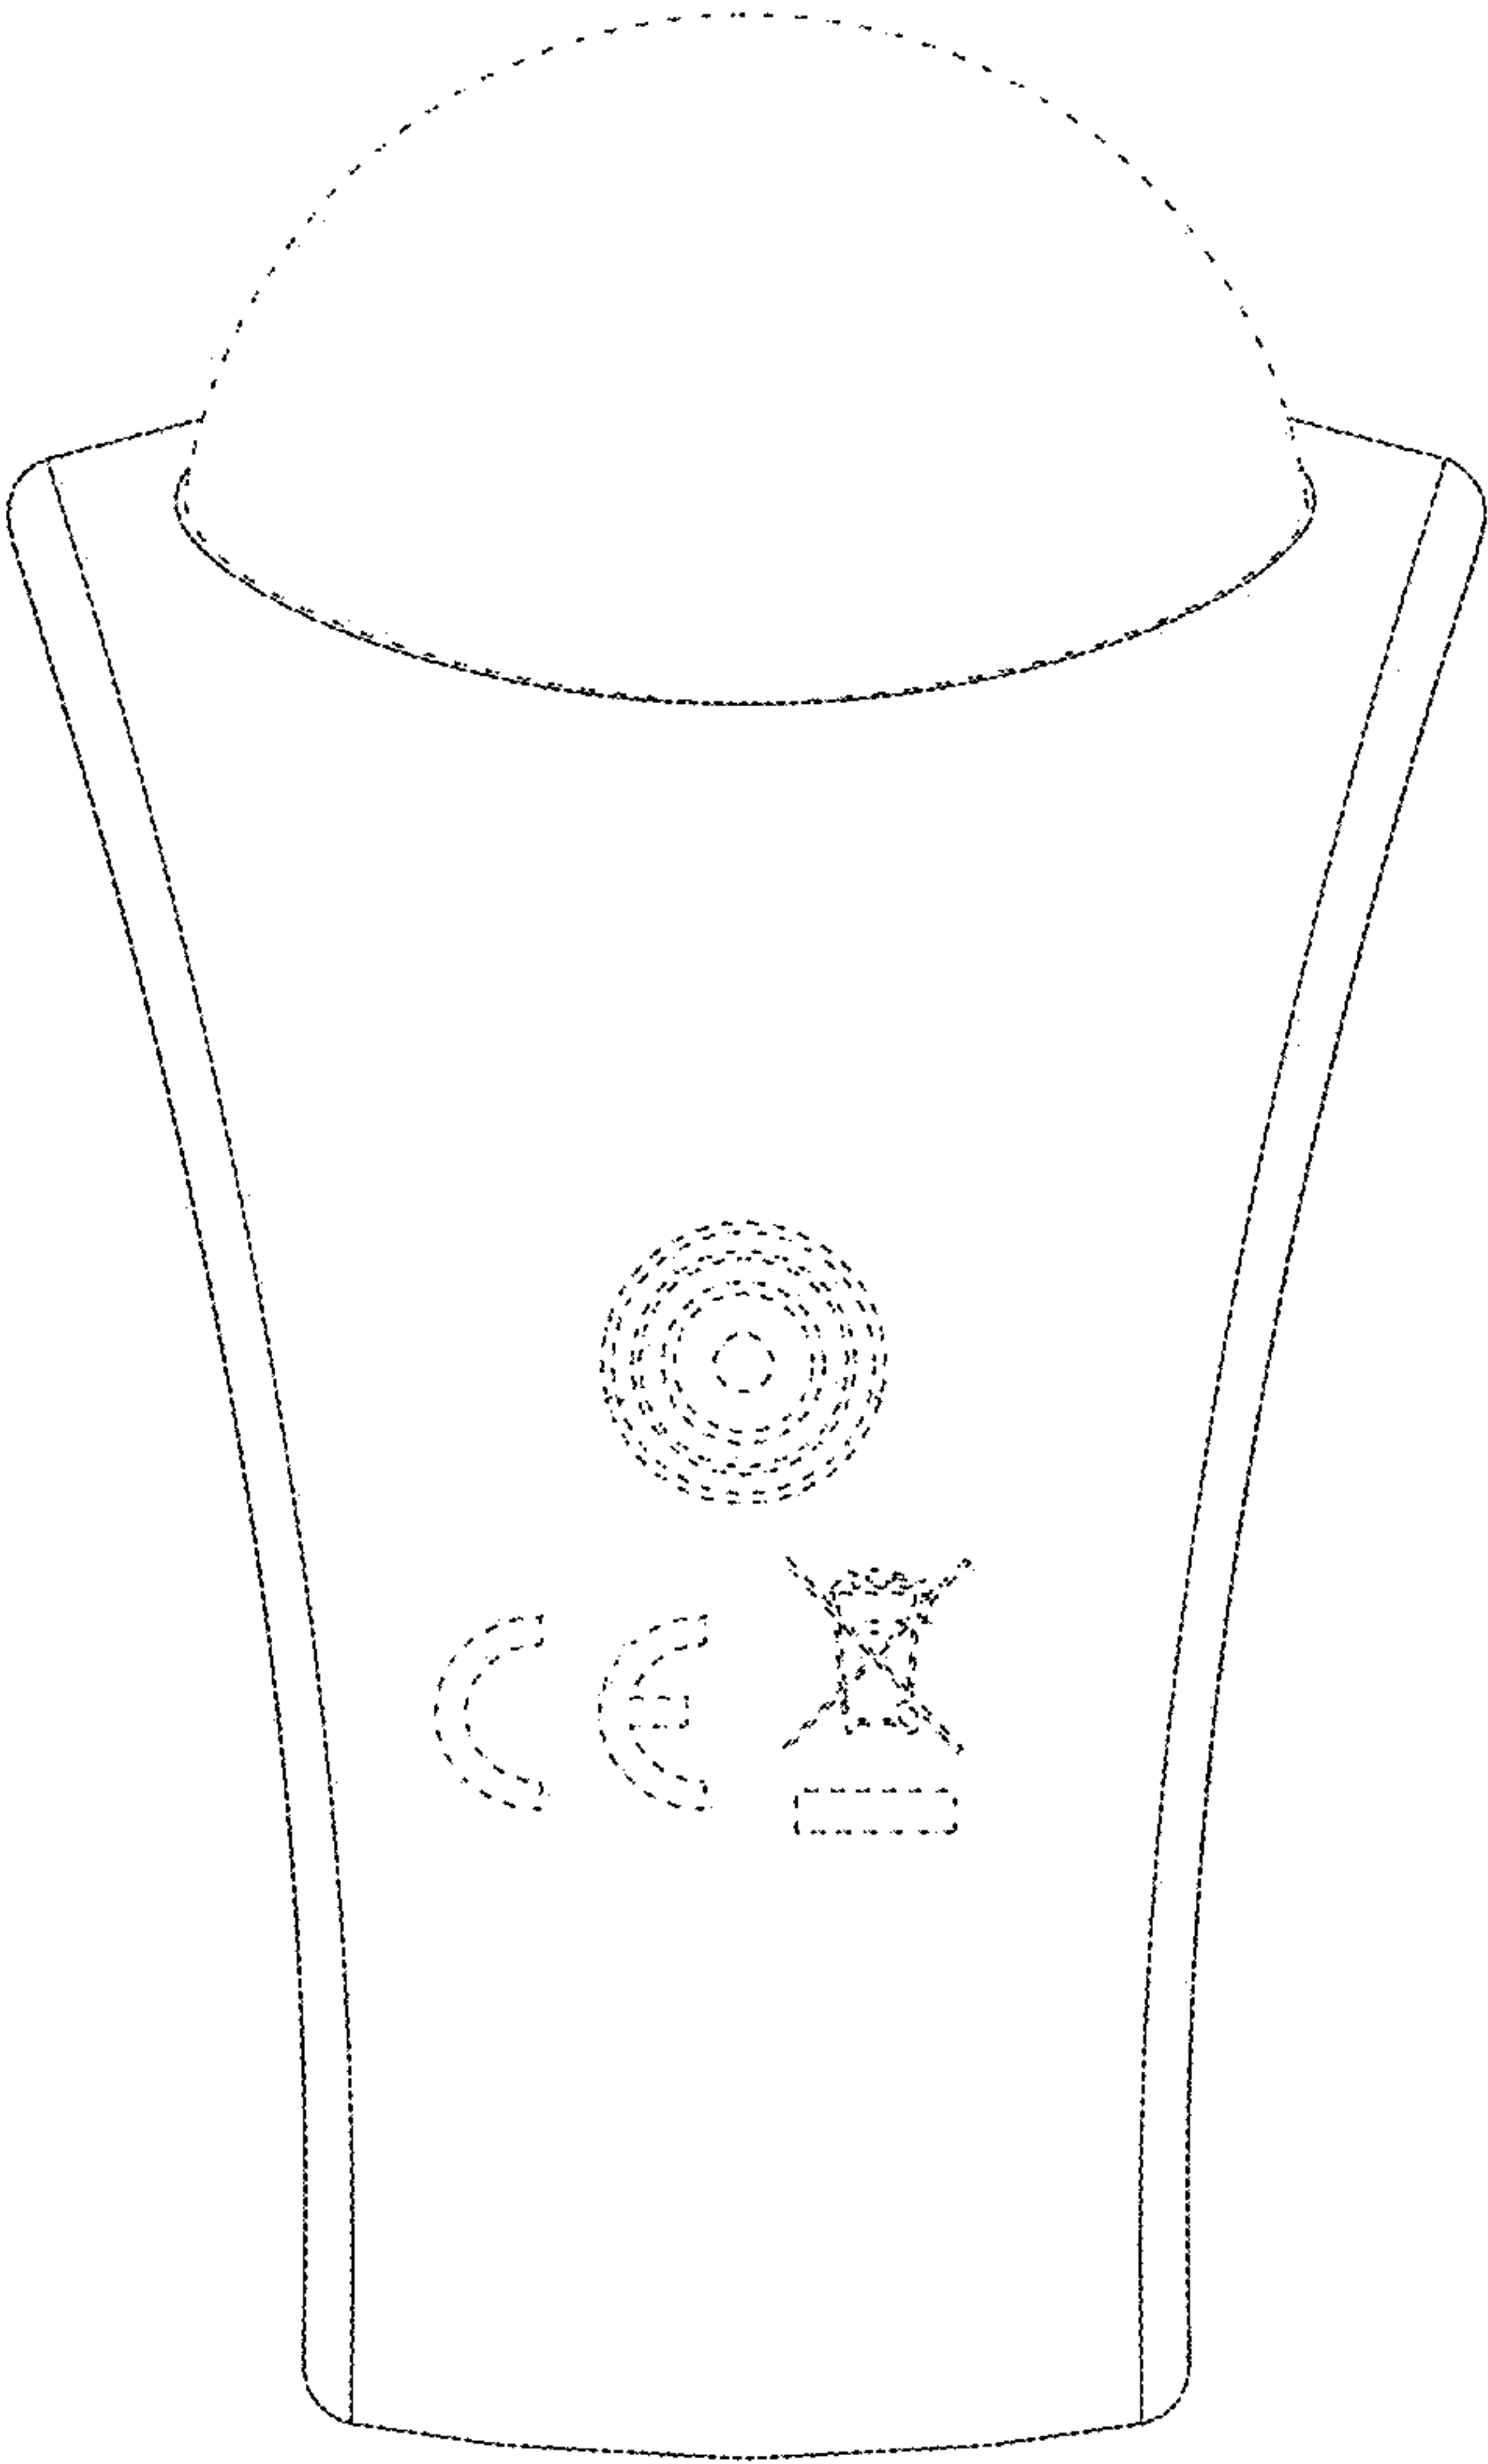


FIG. 3

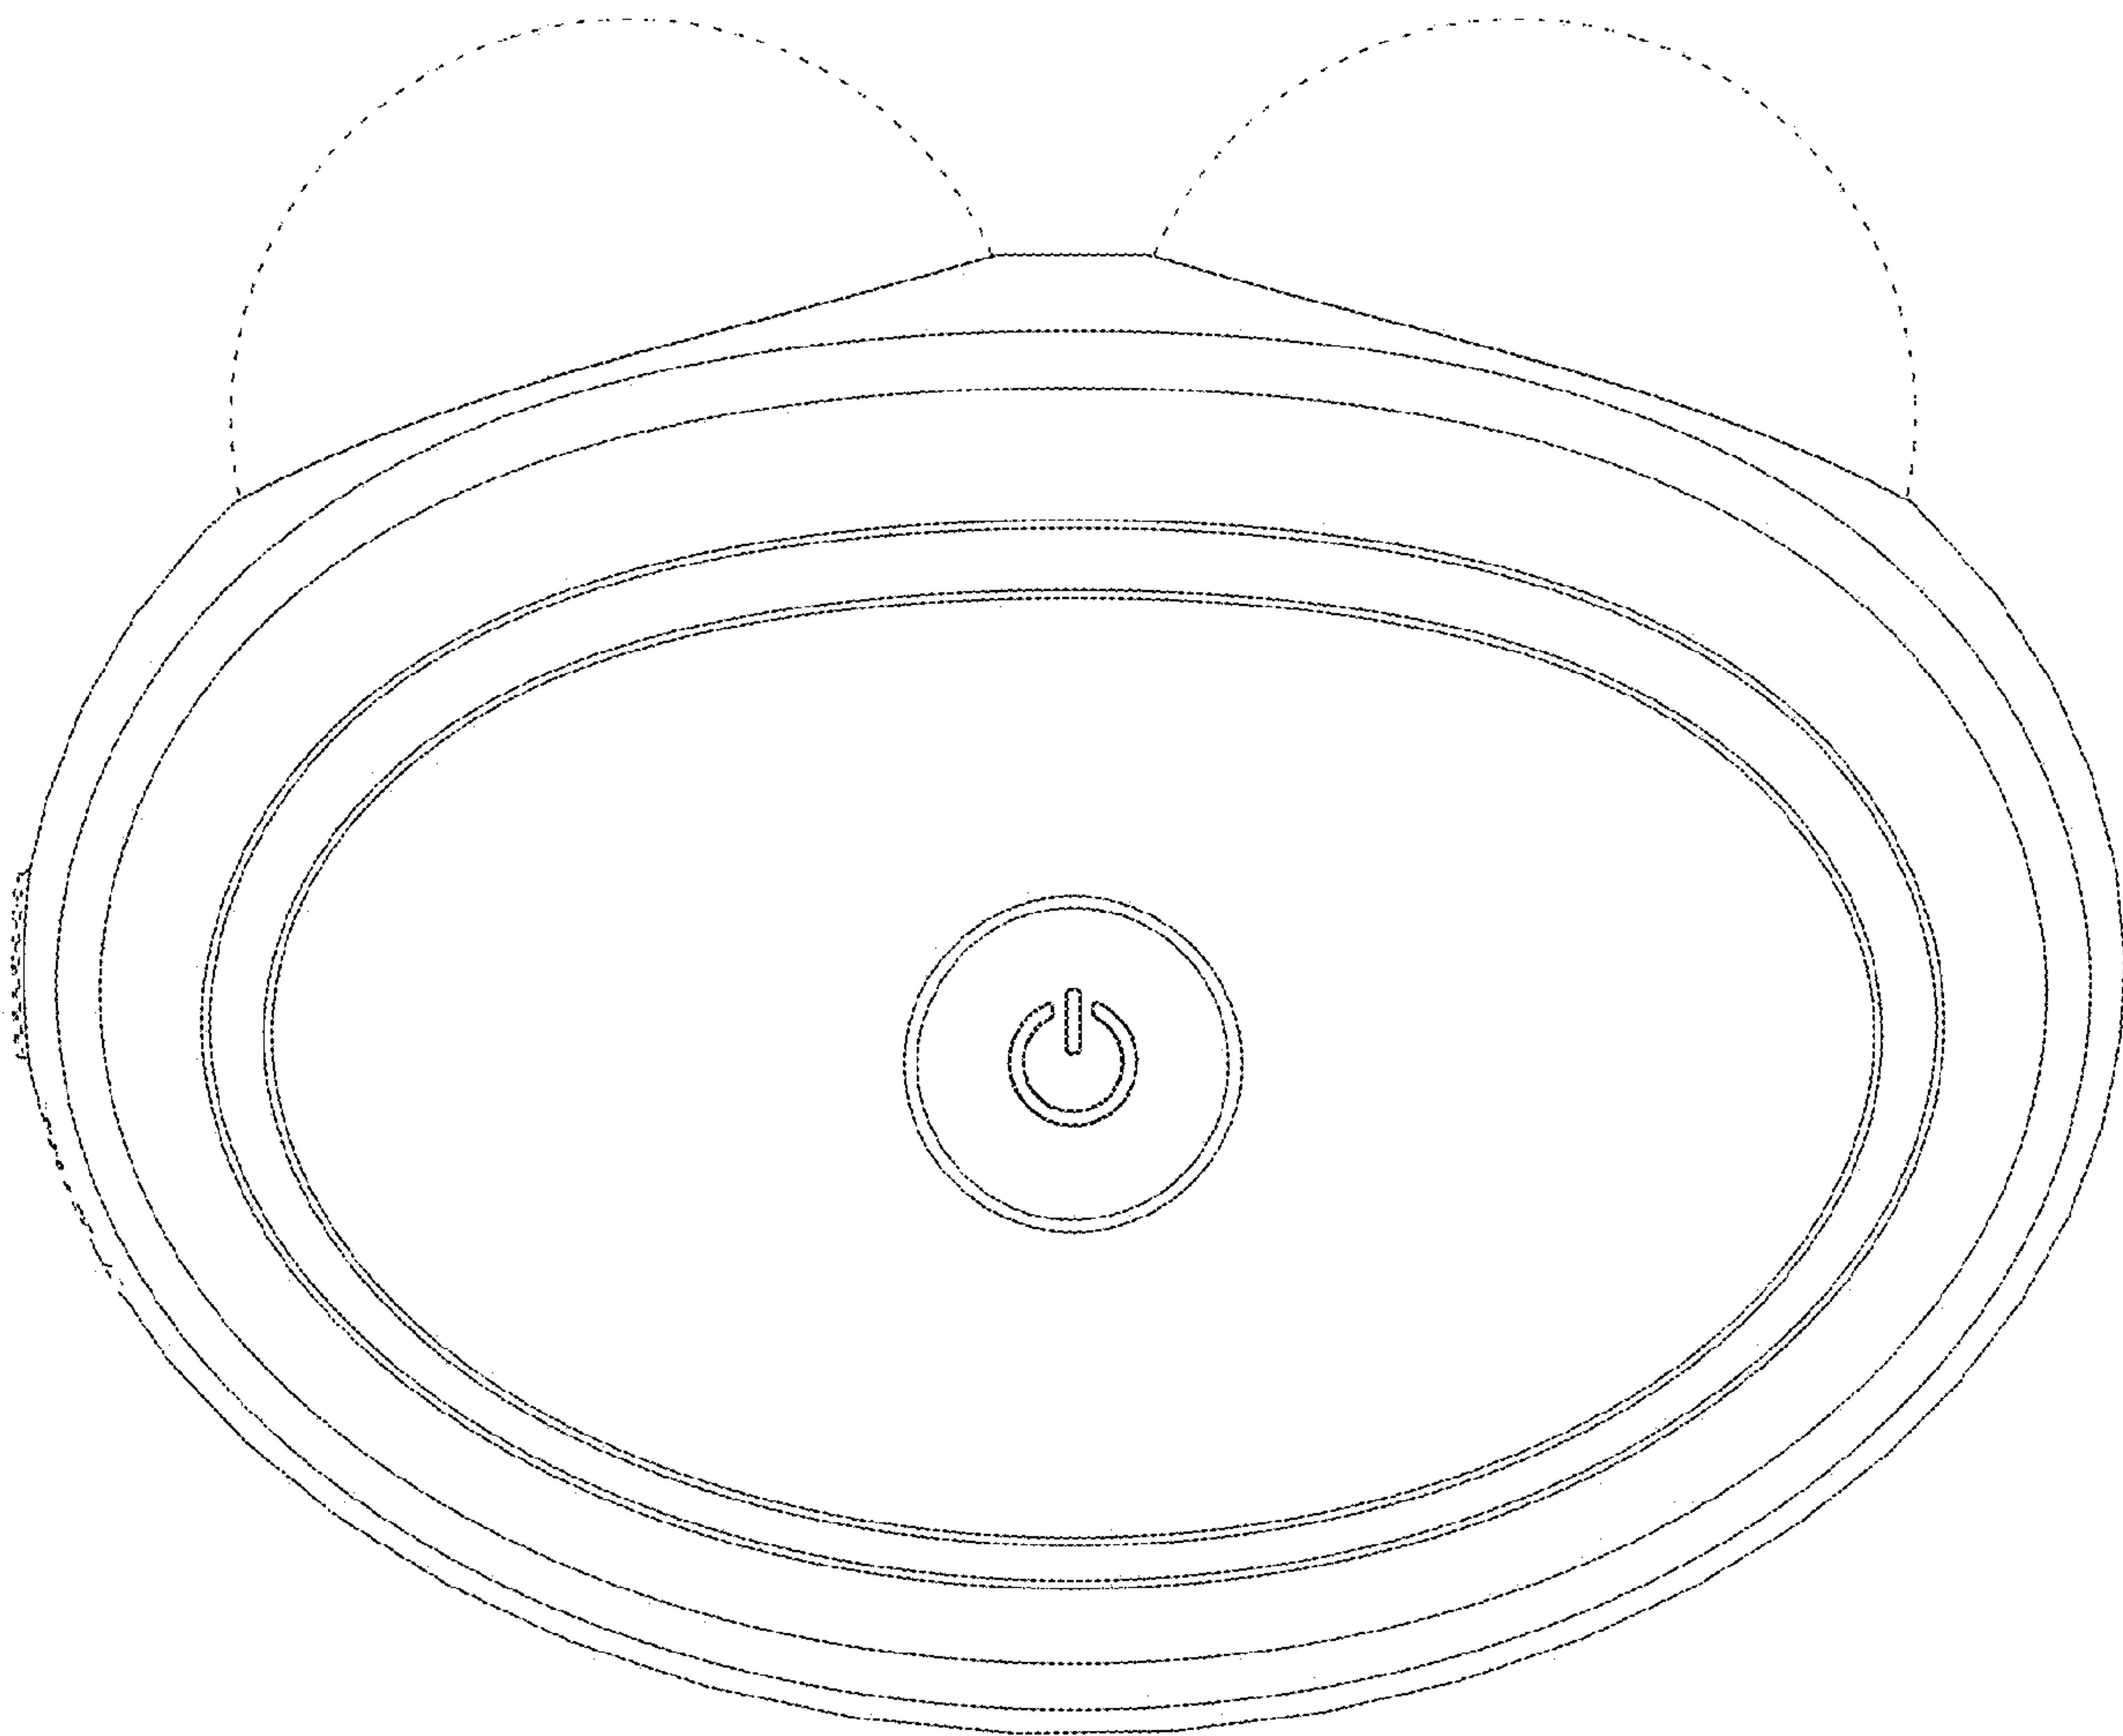


FIG. 4

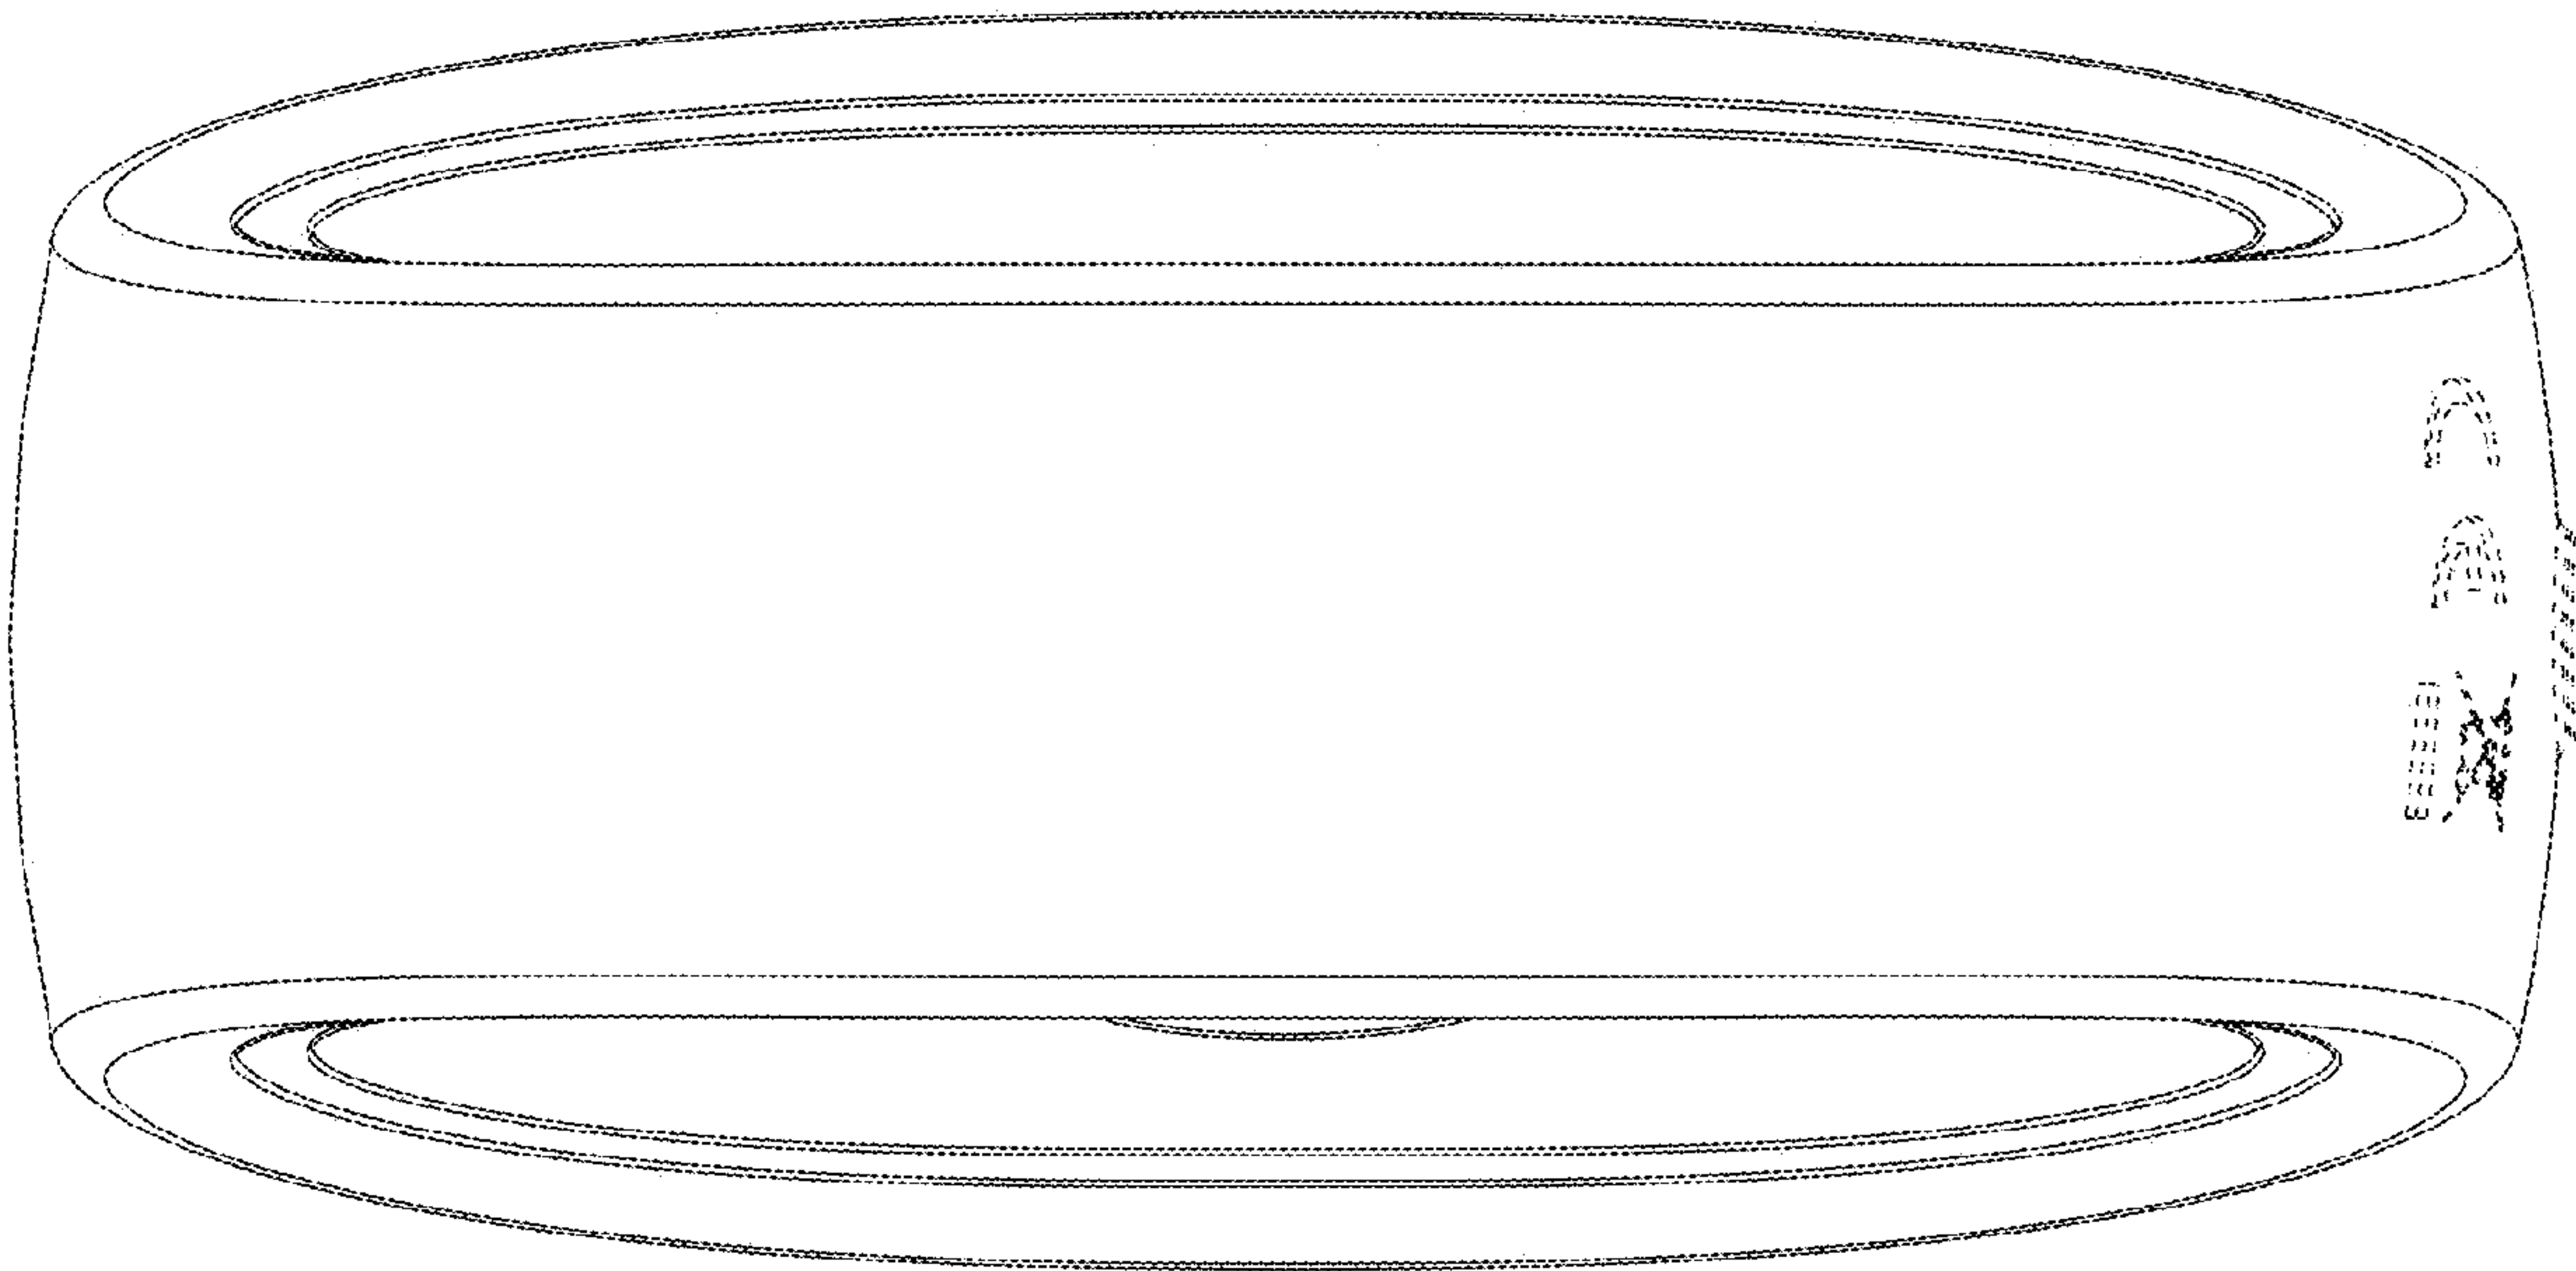


FIG. 5

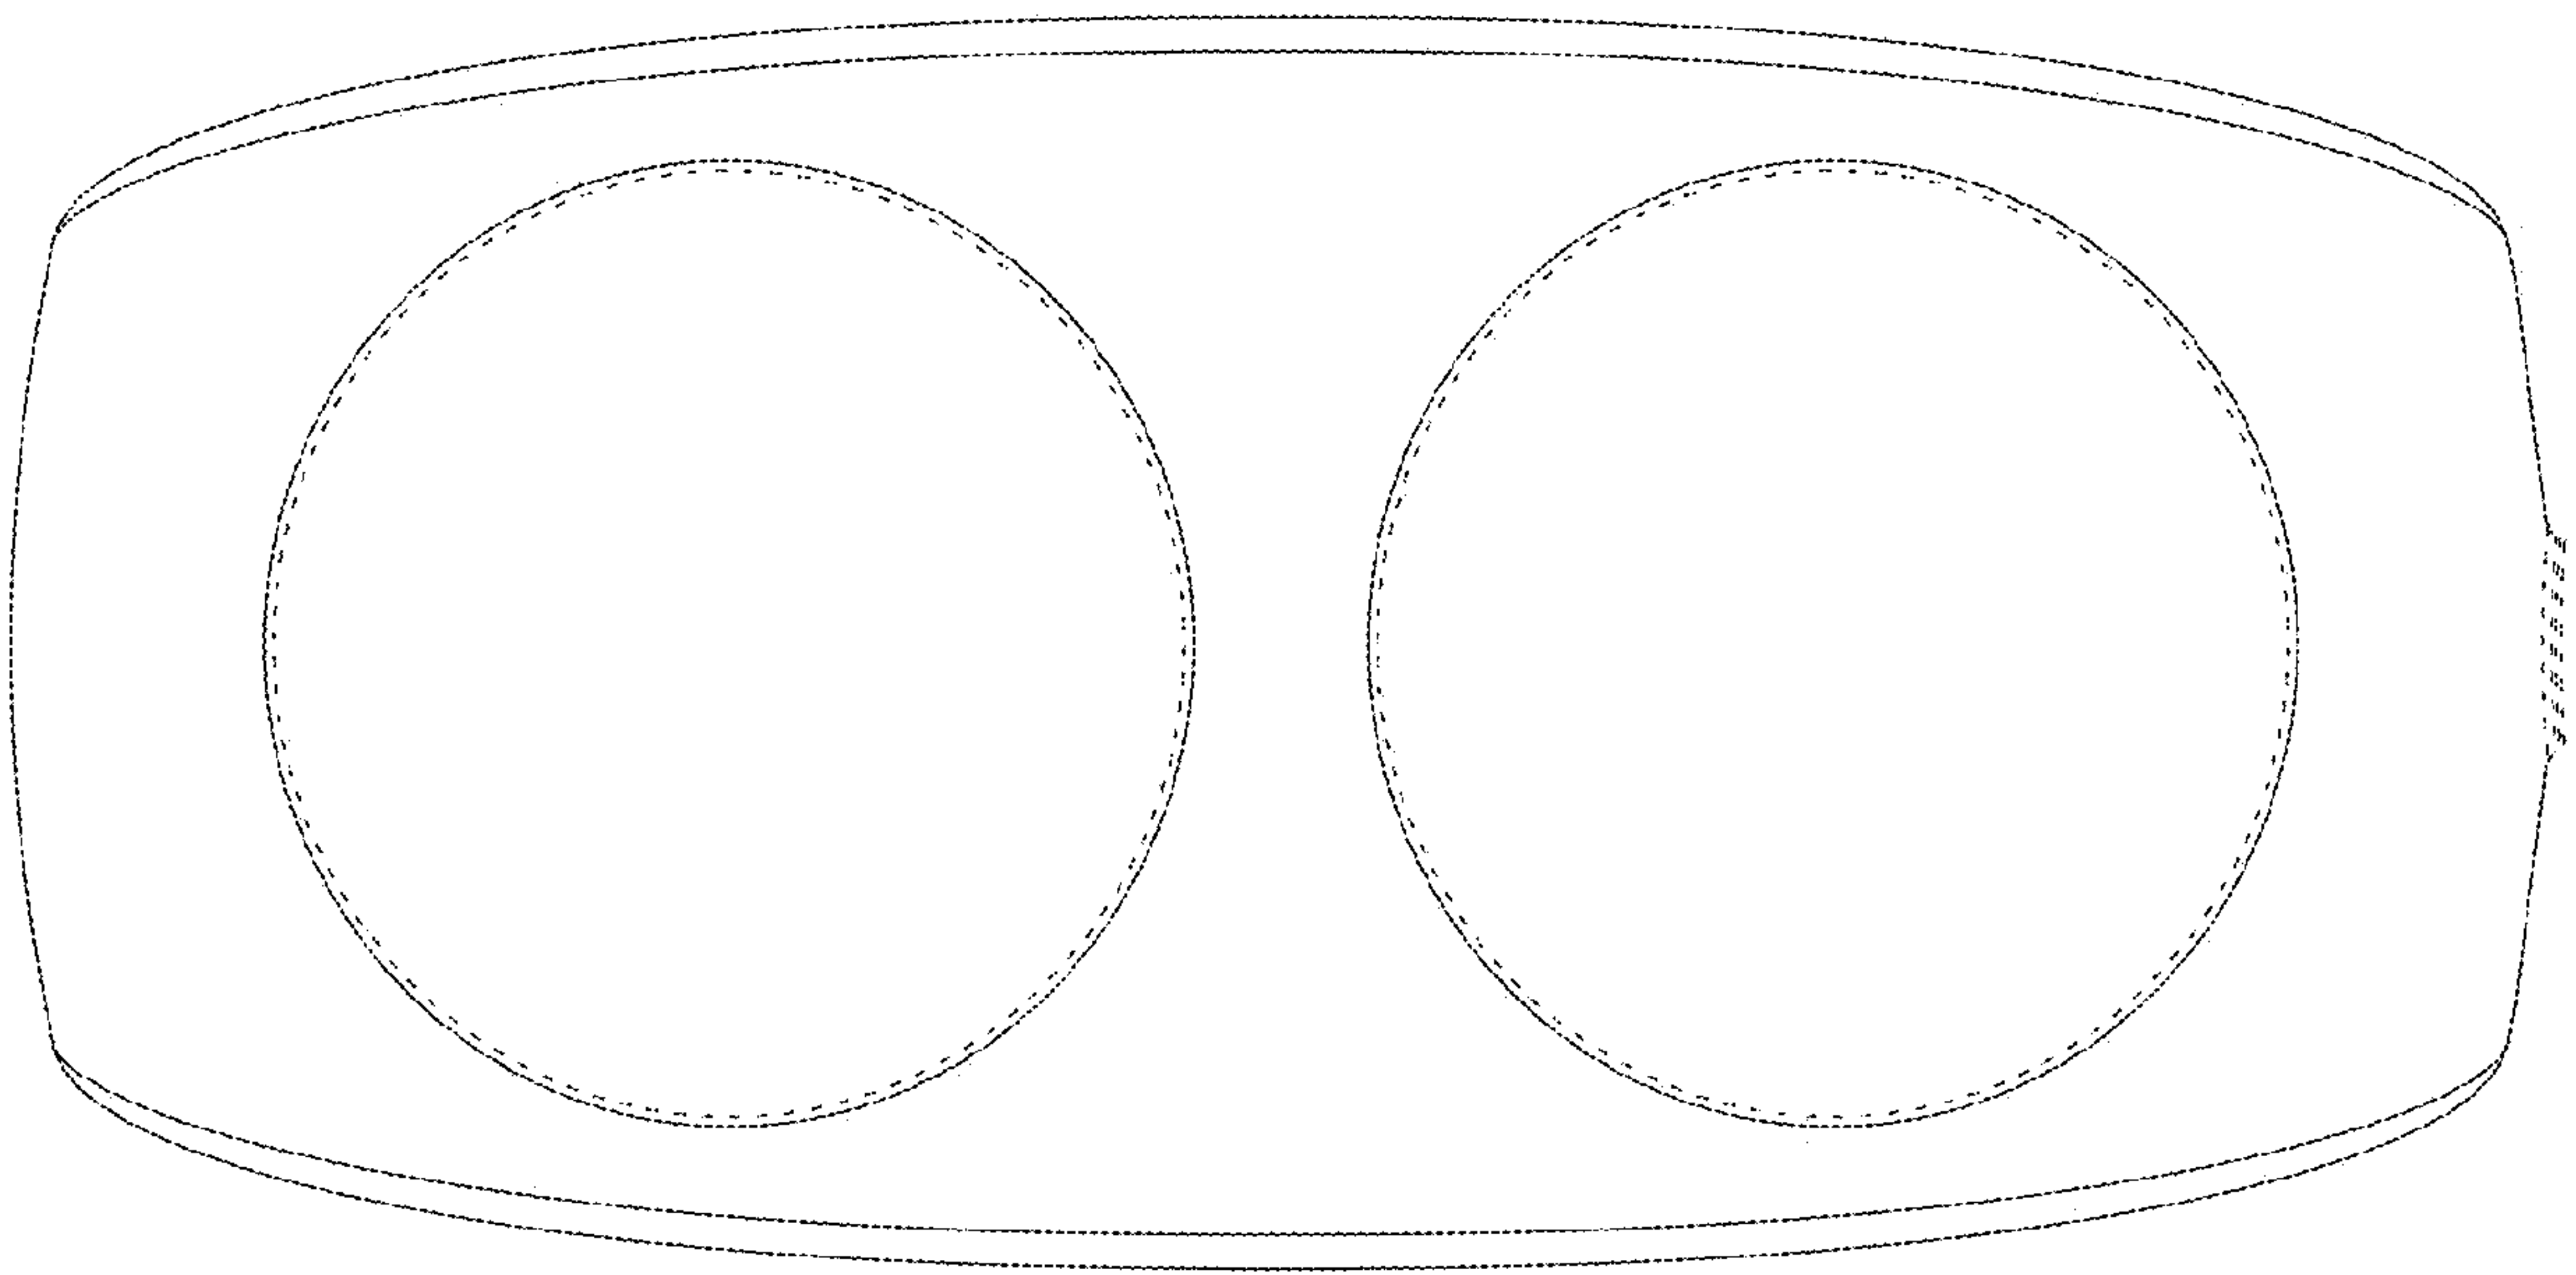


FIG. 6

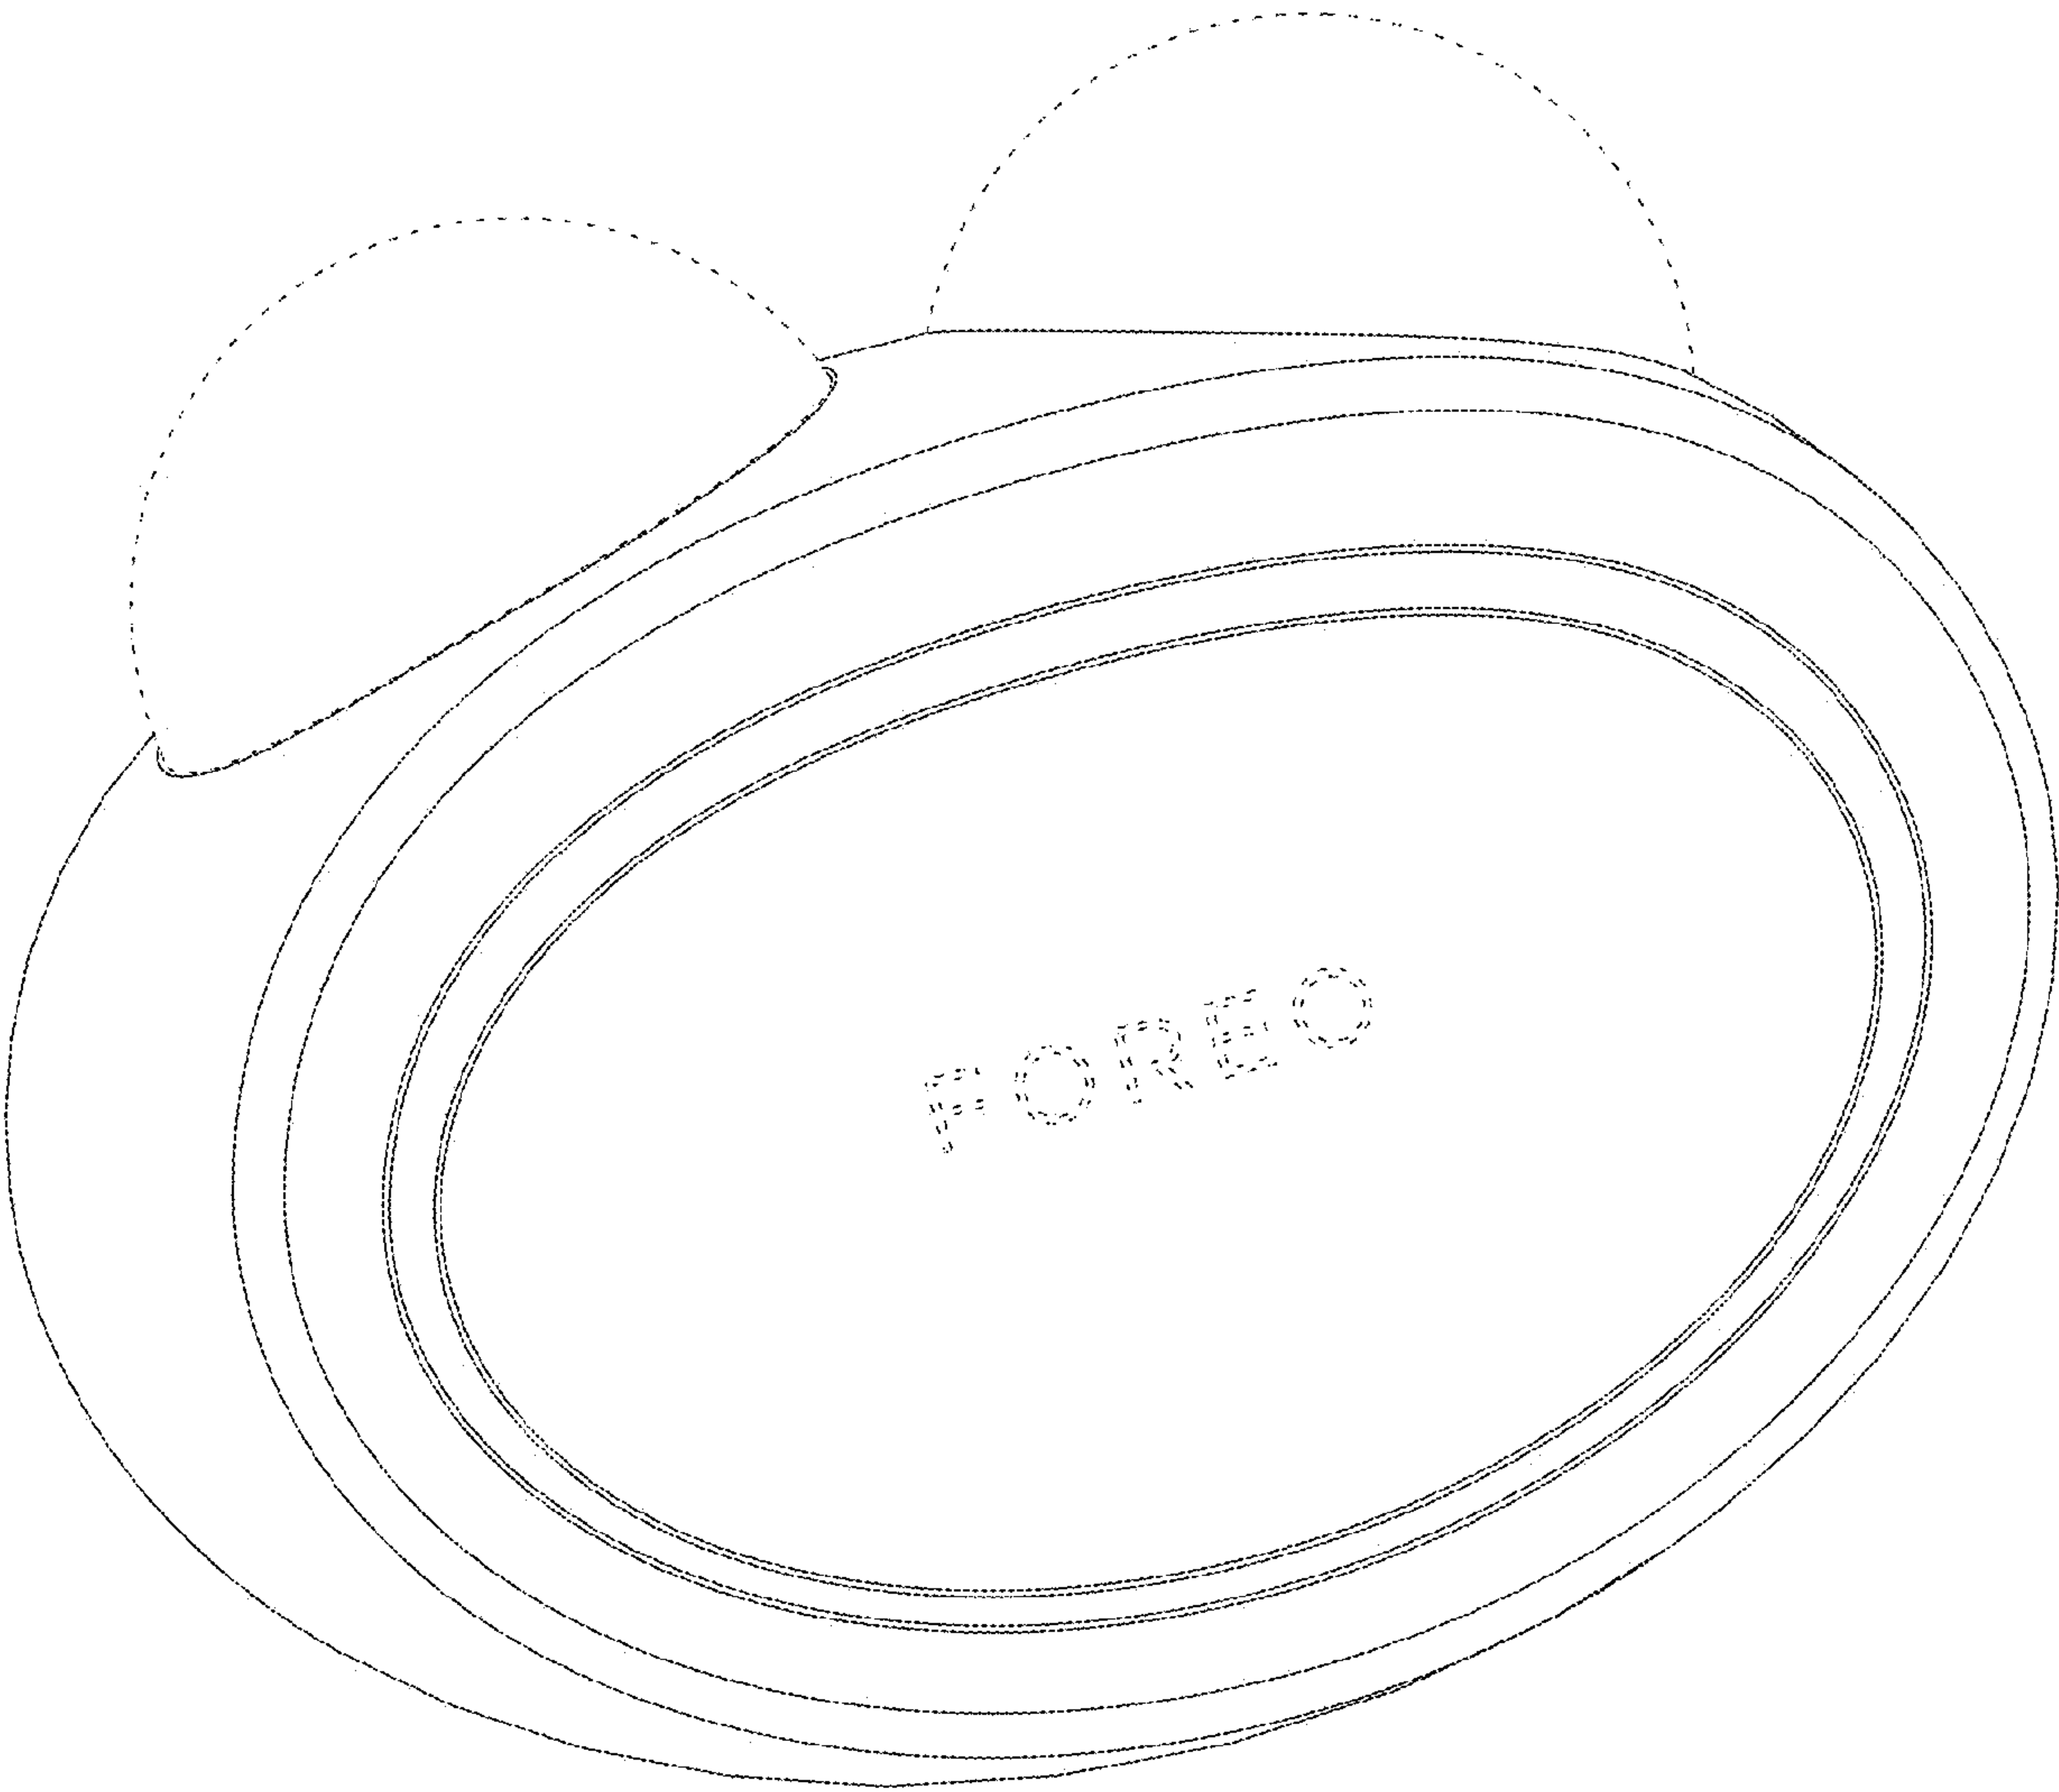


FIG. 7