



US0D1031971S

(12)

United States Design Patent

Babbage et al.

(10)

Patent No.:

US D1,031,971 S

(45)

Date of Patent:

** Jun. 18, 2024

(54) PATIENT INTERFACE CONNECTOR

(71) Applicant: Fisher & Paykel Healthcare Limited,
Auckland (NZ)

(72) Inventors: Sean Joel Babbage, Auckland (NZ);
Peter Geoffrey Hawkins, Auckland
(NZ); Kevin Peter O'Donnell,
Auckland (NZ); Jason Allan Klenner,
Auckland (NZ); Mark Thomas
O'Connor, Auckland (NZ); Milanjot
Singh Assi, Auckland (NZ)

(73) Assignee: FISHER & PAYKEL HEALTHCARE
LIMITED, Auckland (NZ)

(**) Term: 15 Years

(21) Appl. No.: 29/752,662

(22) Filed: Sep. 28, 2020

Related U.S. Application Data

(60) Division of application No. 29/666,359, filed on Oct.
11, 2018, now Pat. No. Des. 897,523, which is a
continuation of application No. 29/614,636, filed on
Aug. 21, 2017, now Pat. No. Des. 834,703, which is
a division of application No. 29/551,896, filed on Jan.
18, 2016, now Pat. No. Des. 796,027, which is a
division of application No. 29/470,958, filed on Oct.
25, 2013, now Pat. No. Des. 747,792.

(51) LOC (14) Cl. 29-02

(52) U.S. Cl.
USPC D24/110; D24/129

(58) Field of Classification Search
USPC D24/110, 110.4, 112, 128, 129

CPC A61B 34/20; A61B 2017/00477; A61M
39/10; A61M 39/1011

See application file for complete search history.

References Cited

U.S. PATENT DOCUMENTS

4,454,880	A	6/1984	Muto et al.	
D275,316	S *	8/1984	Hayes	D23/262
D319,310	S *	8/1991	Schneider	D24/129
5,335,656	A	8/1994	Nowe et al.	

(Continued)

FOREIGN PATENT DOCUMENTS

AU	2014/263285	C1	5/2014
AU	2019/202375	A2	4/2019

(Continued)

OTHER PUBLICATIONS

Japanese Patent Office, Notice of Reasons of Refusal, Application
No. JP 2019-06562, dated Jan. 18, 2021, in 4 pages.

(Continued)

Primary Examiner — Jennifer L Watkins
(74) Attorney, Agent, or Firm — Knobbe Martens Olson
& Bear LLP


CLAIM

The ornamental design for the patient interface connector, as
shown and described.

DESCRIPTION

FIG. 1 is a perspective view showing a patient interface
connector that embodies the design.
FIG. 2 is a front view thereof.
FIG. 3 is a rear view thereof.
FIG. 4 is a left side view thereof.
FIG. 5 is a right side view thereof.
FIG. 6 is a top view thereof; and,
FIG. 7 is bottom view thereof.

(Continued)

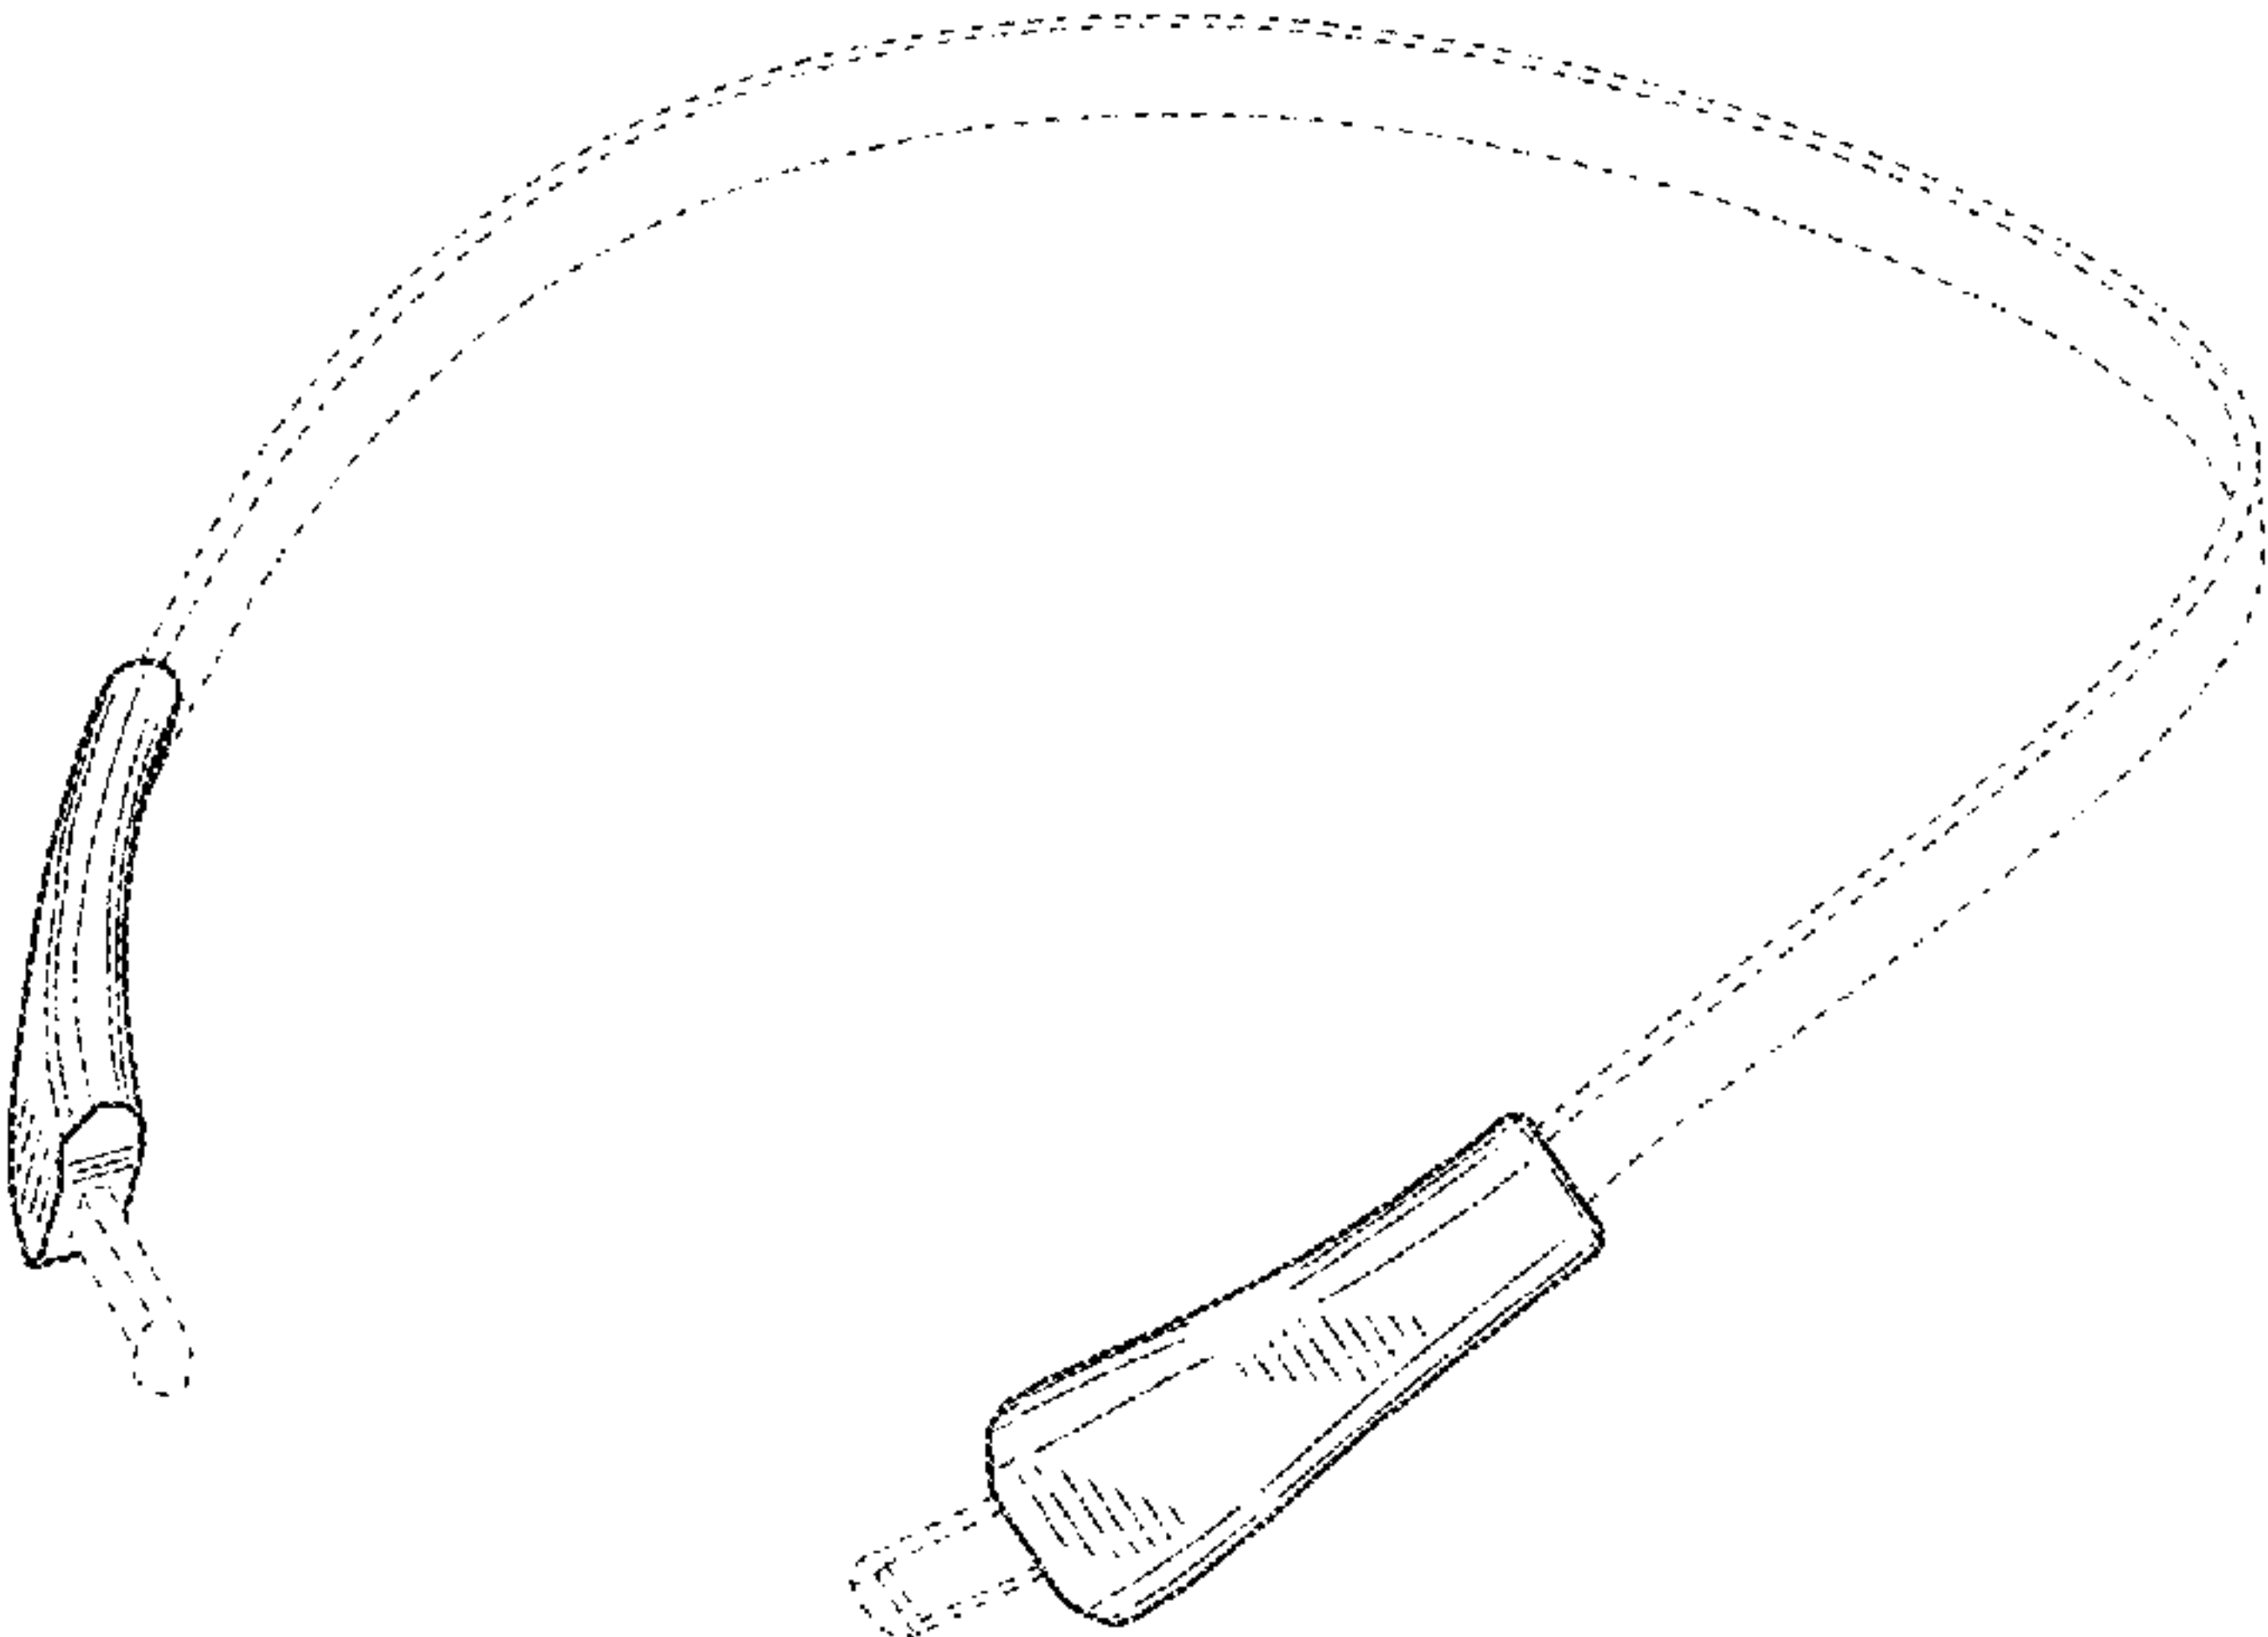

Where utilized, the broken lines show portions of the patient interface connector that form no part of the claimed design.

1 Claim, 7 Drawing Sheets

(56)

References Cited

U.S. PATENT DOCUMENTS

6,119,694 A 9/2000 Correa et al.
6,560,830 B1 * 5/2003 Chi A44B 11/266
24/642
D498,844 S * 11/2004 Diamond D24/130
D533,269 S 12/2006 McAuley et al.
7,178,525 B2 2/2007 Matula et al.
7,231,921 B2 6/2007 Palmer
D551,340 S 9/2007 Wood et al.
D556,900 S 12/2007 Guney et al.
D559,383 S 1/2008 Nalagatla et al.
D566,835 S 4/2008 Andrews et al.
D586,258 S 2/2009 Guney et al.
D586,911 S 2/2009 McAuley et al.
7,493,902 B2 2/2009 White et al.
7,559,327 B2 7/2009 Hernandez
D614,290 S 4/2010 Judson et al.
D627,059 S 11/2010 Wood et al.
D637,285 S 5/2011 Bradley et al.
7,987,850 B2 8/2011 Zollinger et al.
D650,741 S 12/2011 Sun et al.
8,177,770 B2 * 5/2012 Rasmussen A61M 39/10
604/523
D664,496 S 7/2012 Cohen
D665,496 S 8/2012 Lee
D692,554 S 10/2013 Slew et al.
D703,464 S 4/2014 Koch
D724,720 S 3/2015 O'Connor et al.
D745,141 S 12/2015 Hung
D747,792 S 1/2016 Babbage et al.
D766,711 S 9/2016 Babbage
D796,027 S * 8/2017 Babbage D24/110
D797,921 S 9/2017 Huang et al.
9,907,925 B2 3/2018 McAuley et al.
D815,735 S * 4/2018 Aliberti D8/396
D820,436 S * 6/2018 Kheradpir D24/112
D825,053 S 8/2018 Ronayne et al.
D849,243 S 5/2019 Wilson et al.
D859,646 S 9/2019 Scampoli et al.
10,406,311 B2 9/2019 O'Donnell et al.
D870,878 S * 12/2019 Wilson D24/110.4
D881,382 S 4/2020 Chang
D898,898 S * 10/2020 Walls D24/110.4
D912,243 S * 3/2021 Stengele D24/112
D977,087 S * 1/2023 Siew D24/110.4
2004/0244804 A1 12/2004 Olsen et al.
2004/0261797 A1 12/2004 White et al.
2005/0002882 A1 2/2005 Amari et al.

2005/0028822 A1 2/2005 Sleeper et al.
2006/0231103 A1 10/2006 Matula et al.
2007/0186931 A1 8/2007 Zollinger et al.
2008/0099024 A1 5/2008 Gunaratnam et al.
2009/0004808 A1 1/2009 Lee et al.
2009/0044808 A1 2/2009 Guney et al.
2010/0108073 A1 5/2010 Zollinger et al.
2010/0192957 A1 8/2010 Hobson et al.
2010/0258136 A1 10/2010 Doherty et al.
2011/0067704 A1 3/2011 Kooij et al.
2011/0271962 A1 11/2011 White et al.
2012/0204870 A1 8/2012 McAuley et al.
2012/0304999 A1 12/2012 Swift et al.
2013/0008447 A1 1/2013 Gunaratnam et al.
2013/0008449 A1 1/2013 Busch et al.
2016/0015296 A1 1/2016 Garaycochea
2019/0262574 A1 8/2019 Sweeney et al.
2019/0298961 A1 10/2019 Hsiung et al.
2019/0344036 A1 11/2019 O'Donnell et al.

FOREIGN PATENT DOCUMENTS

EP 2994181 B1 4/2019
EP 3626294 4/2020
GB 2465689 6/2010
JP 2009/039528 2/2009
NZ 724289 2/2019
WO WO 2007/114492 A1 10/2007
WO WO 2009/099995 8/2009
WO WO 2011/062510 11/2010
WO WO 2012/053910 4/2012
WO WO 2012/077036 6/2012
WO WO 2012/085755 6/2012
WO WO 2013/022356 A1 2/2013
WO WO 2014/015382 1/2014
WO WO 2014/142681 9/2014
WO WO 2014/182179 11/2014

OTHER PUBLICATIONS

Canadian Patent Office, Examination Report, Application No. 2,911,413, dated Dec. 24, 2020, in 6 pages.
Indian Patent Office, Examination Report, Application No. 3987/KOLNP/2015, dated Nov. 3, 2020, in 9 pages.
Examination Report; Application No. GB2004846.8; dated Jun. 12, 2020; 2 Pages.
Examination Report; Canadian Patent Application No. 2,911,413; dated May 28, 2020; 4 Pages.
Examination Report; Japanese Application No. 2019-065642; dated Apr. 6, 2020; 3 Pages total including office action summary.
Examination Report under Section 18(3), Application No. GB1519979. 7, dated Jun. 21, 2019, in 6 pages.
Extended European Search Report; Application No. 19205706.5-1122, dated Feb. 11, 2020, in 17 pages.
Taiwan Examination Report; Application No. 107134131, dated Aug. 2, 2019, 3 pages.

* cited by examiner

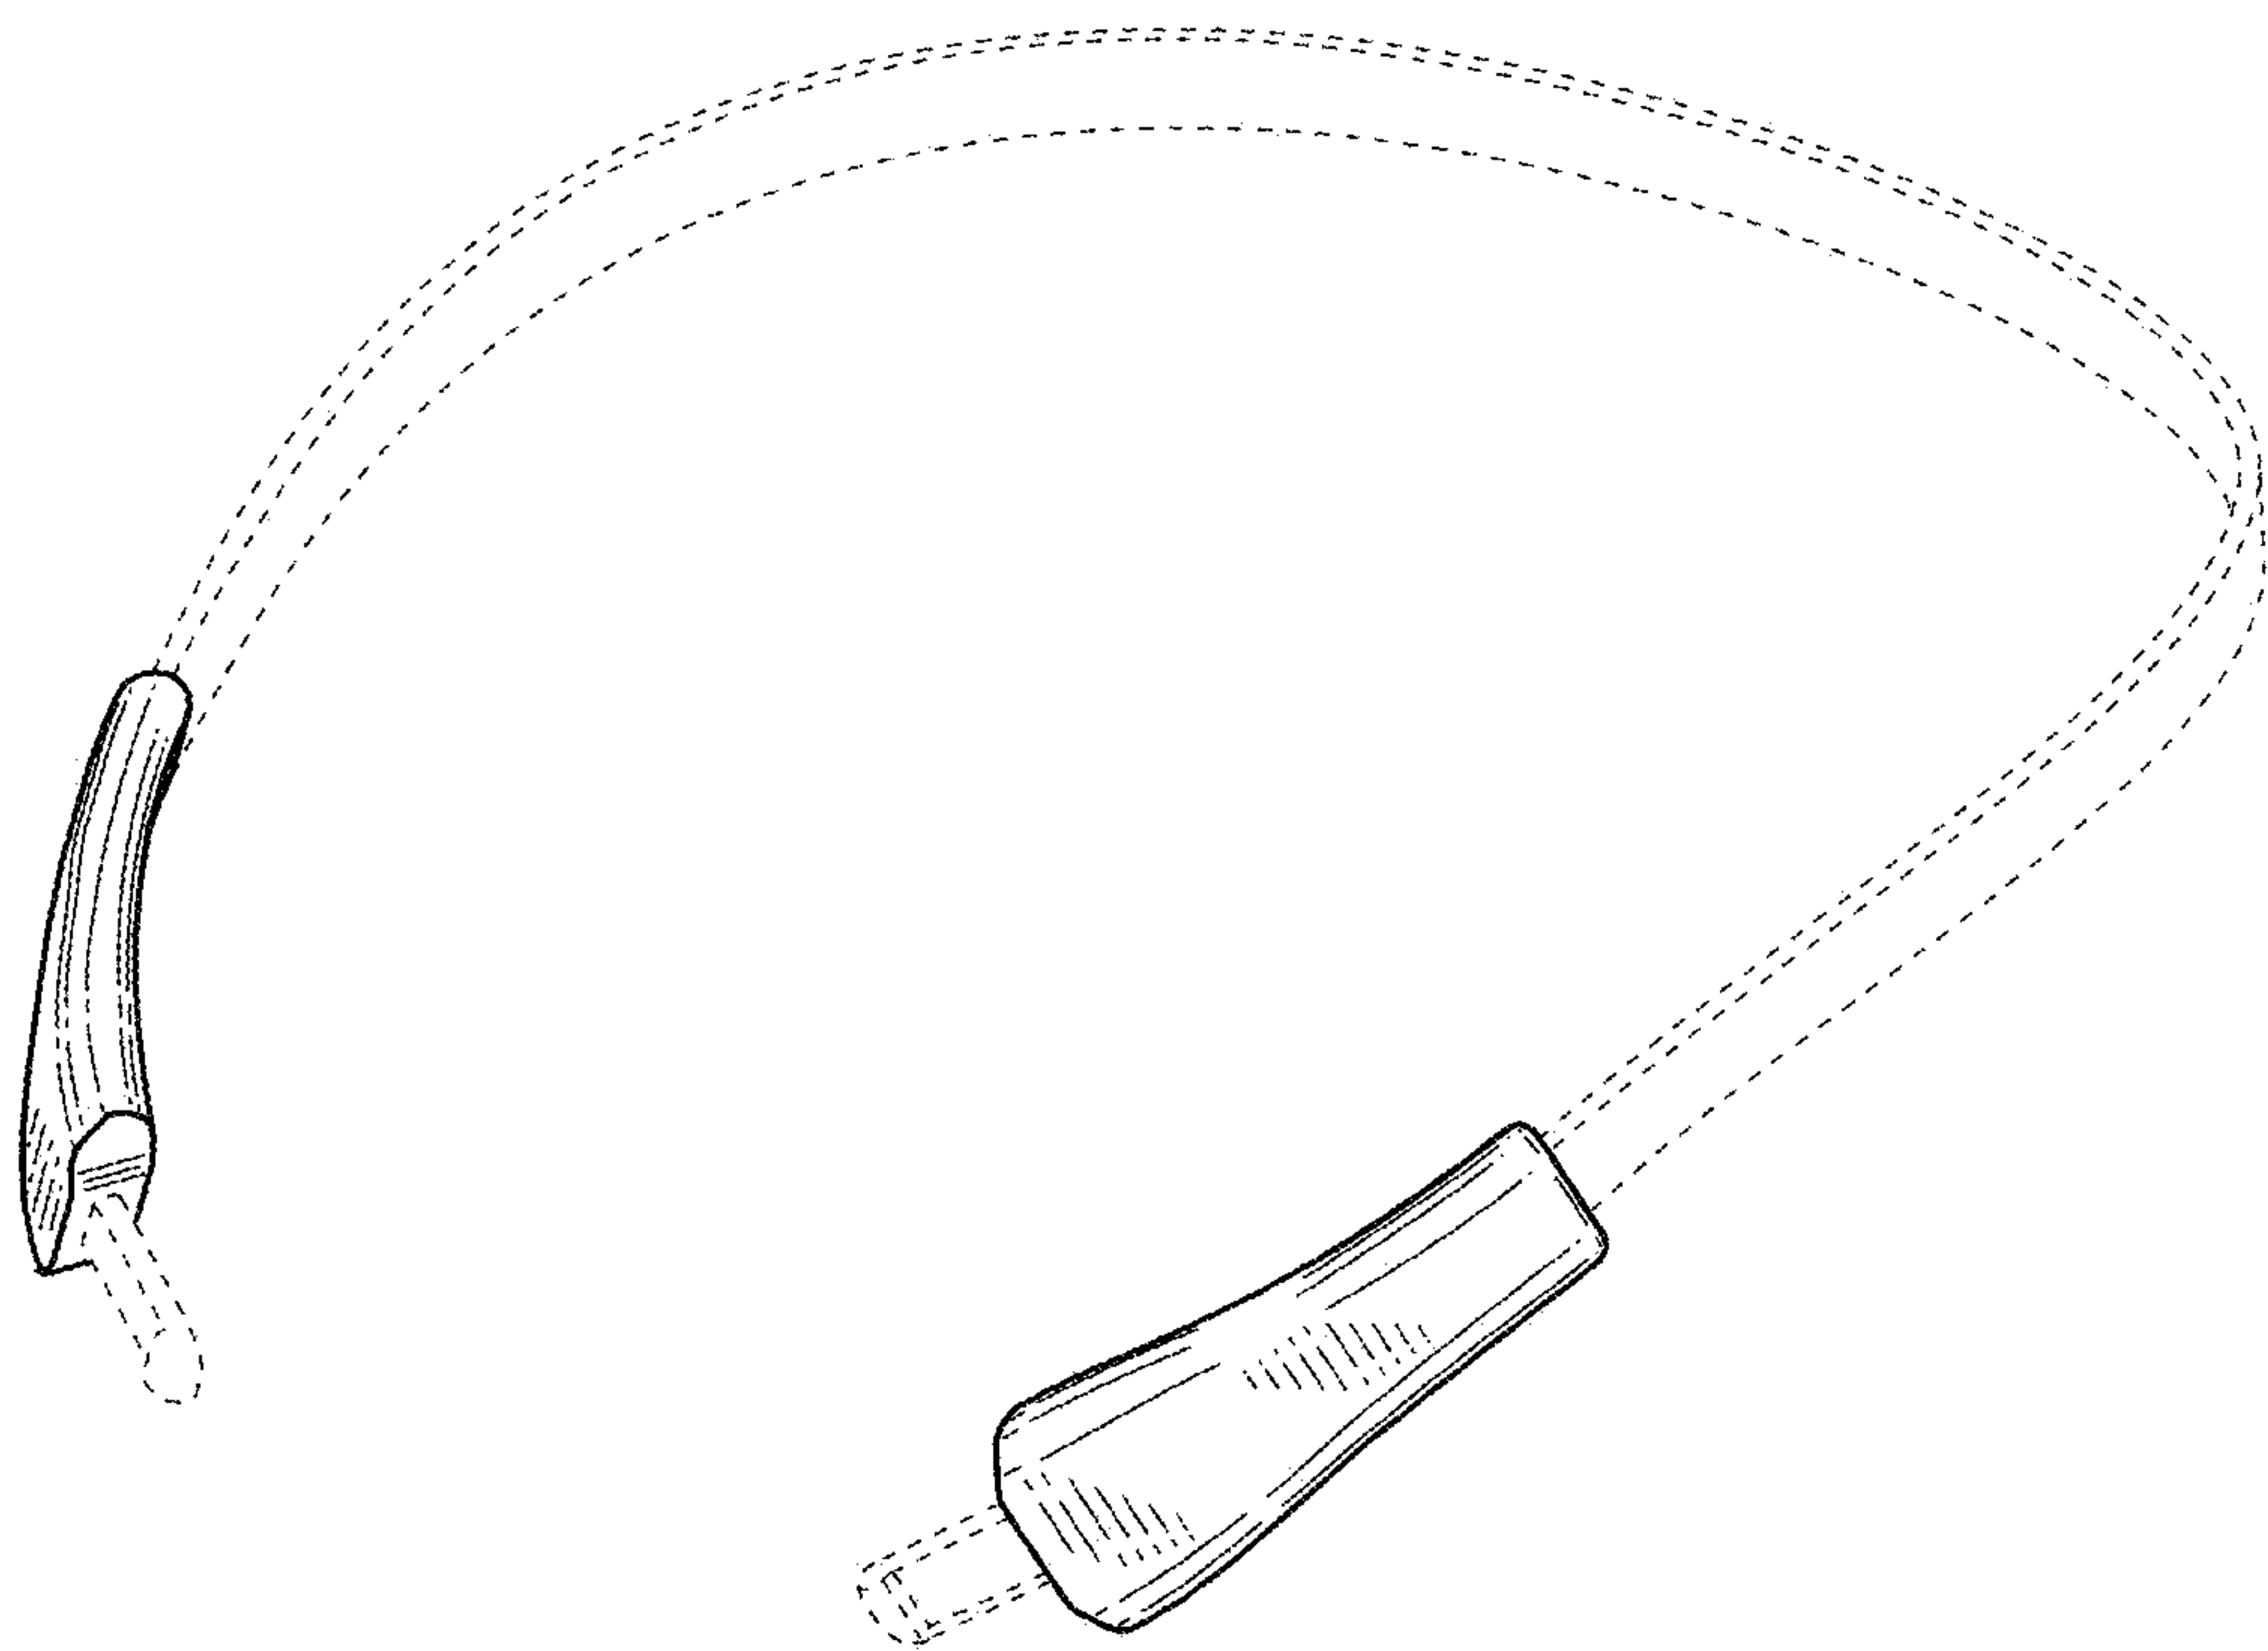


FIG. 1

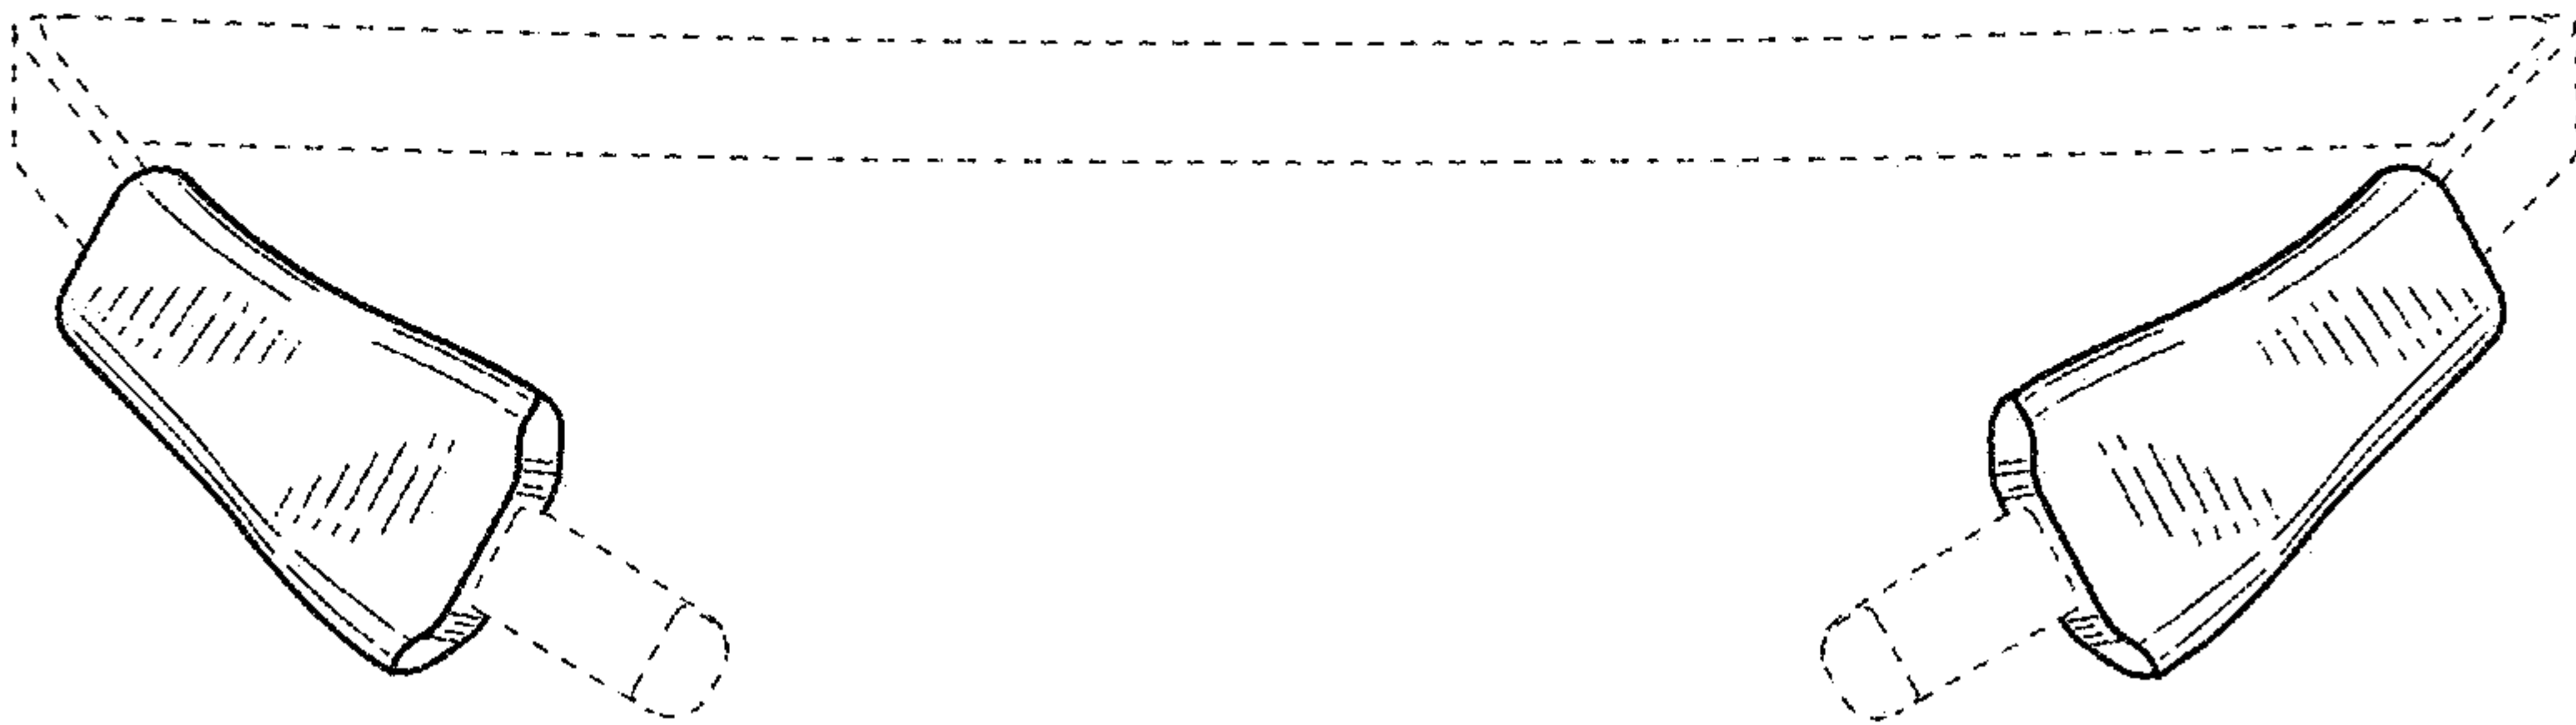


FIG. 2

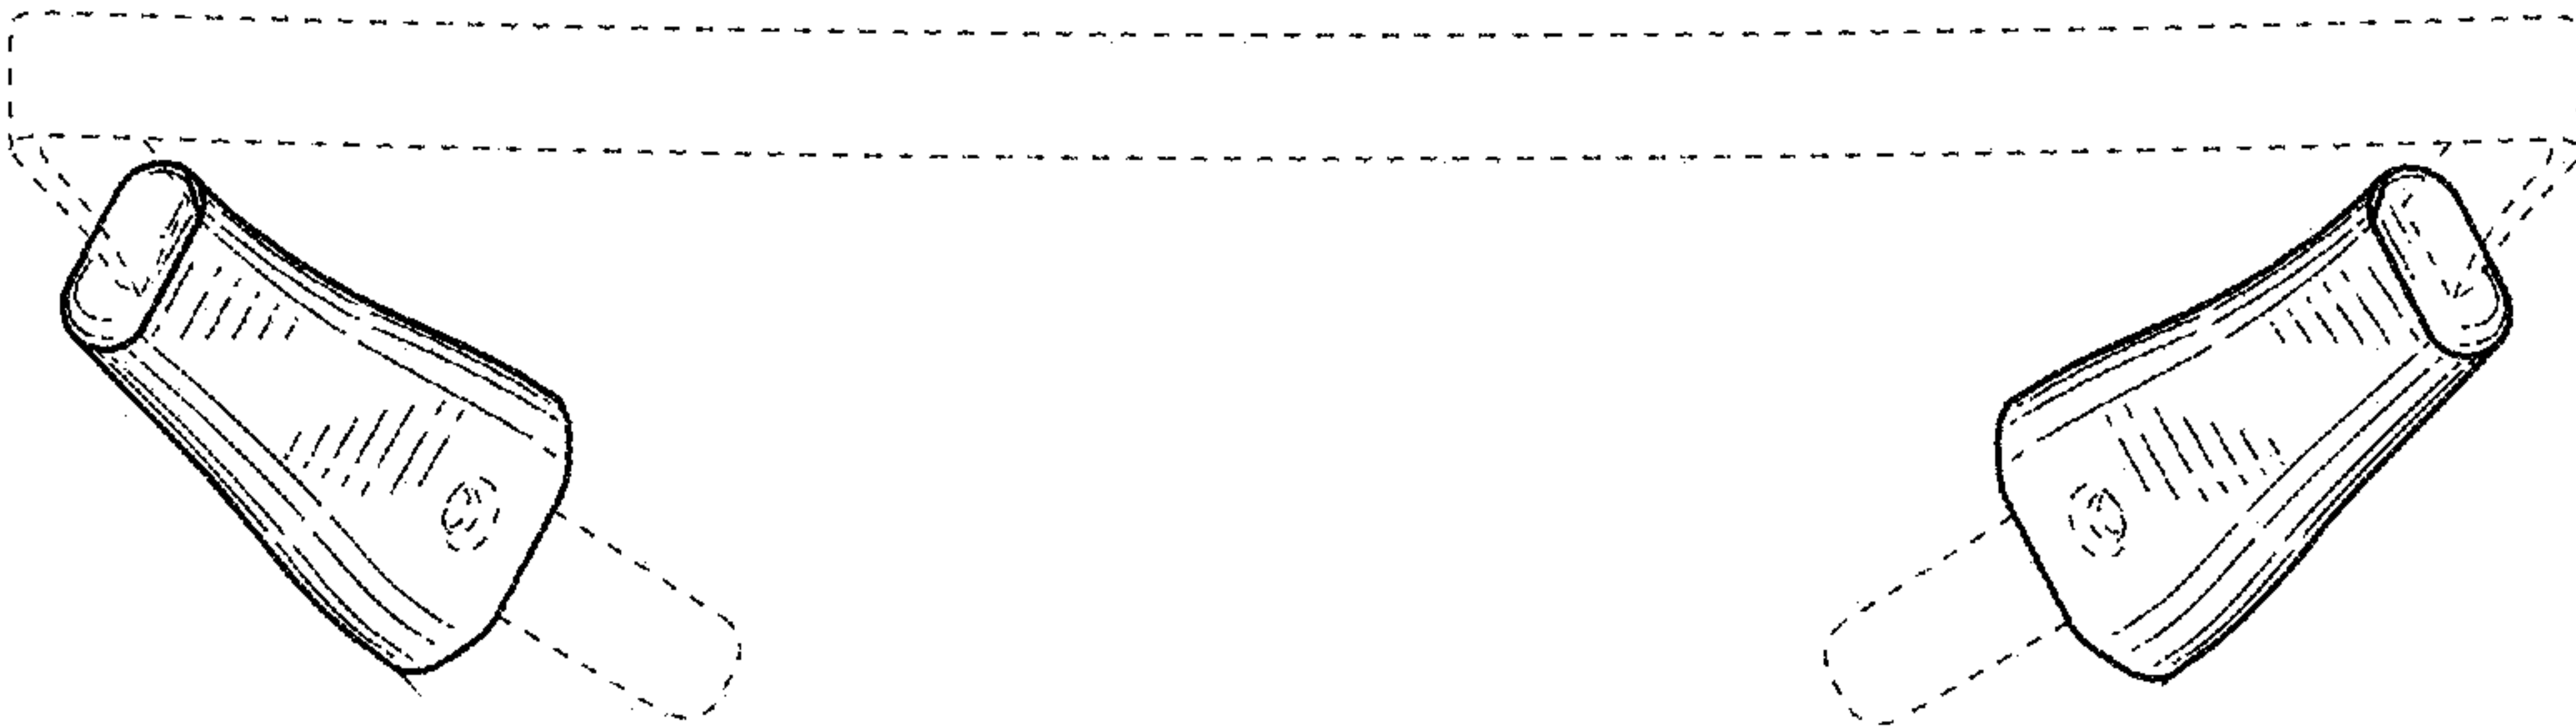


FIG. 3

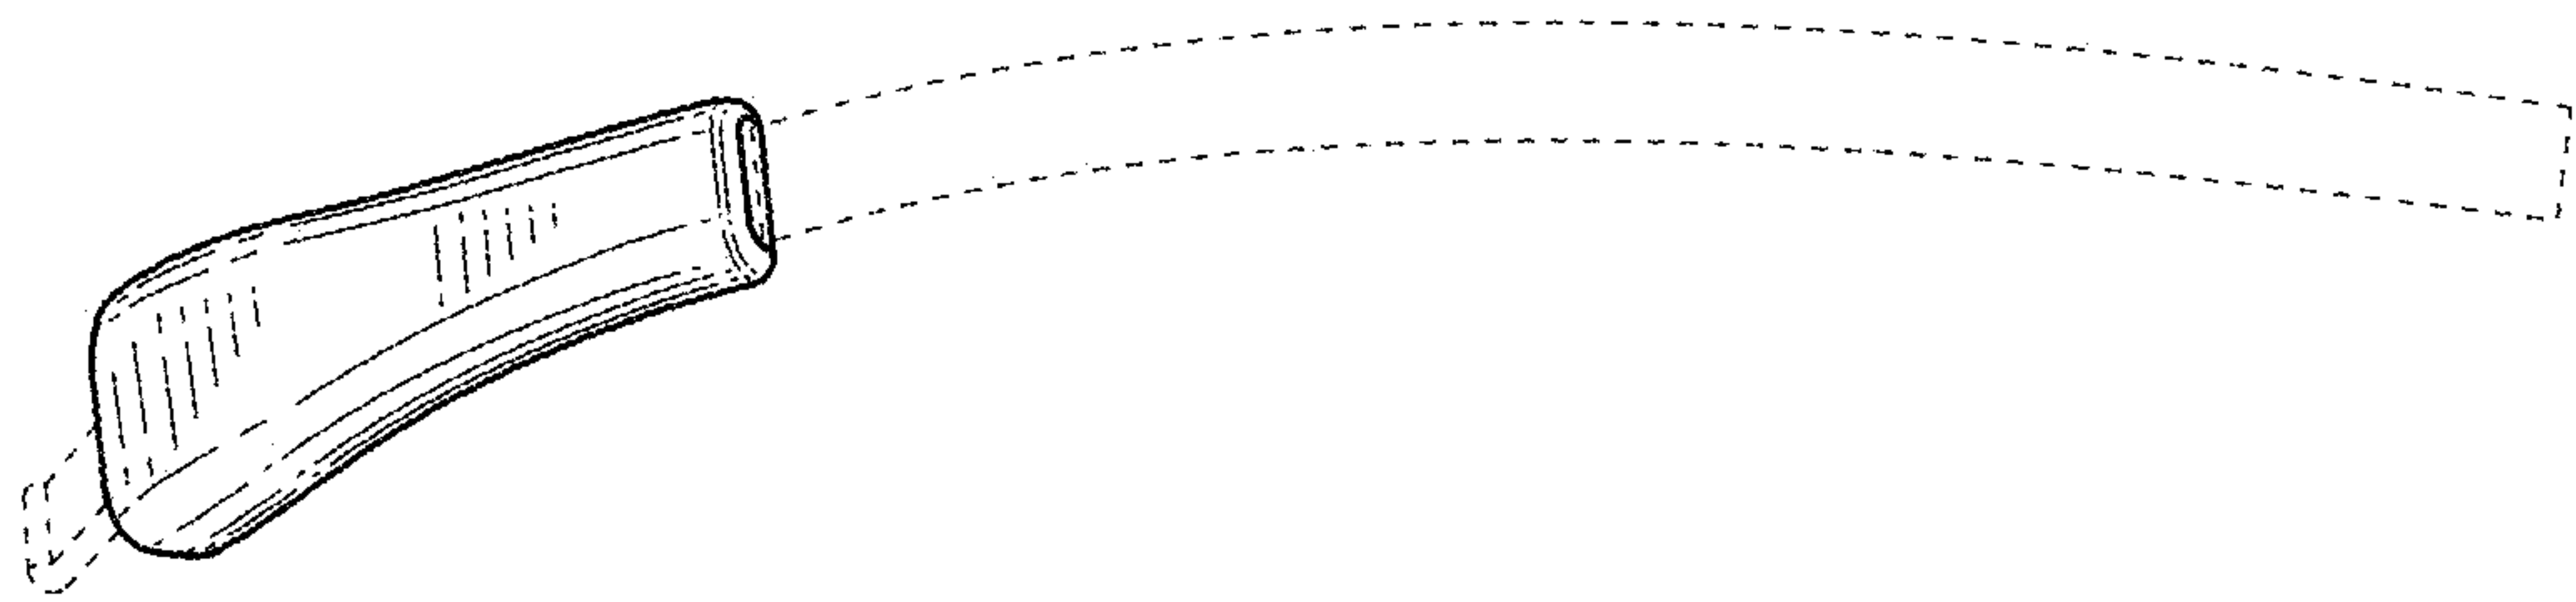


FIG. 4

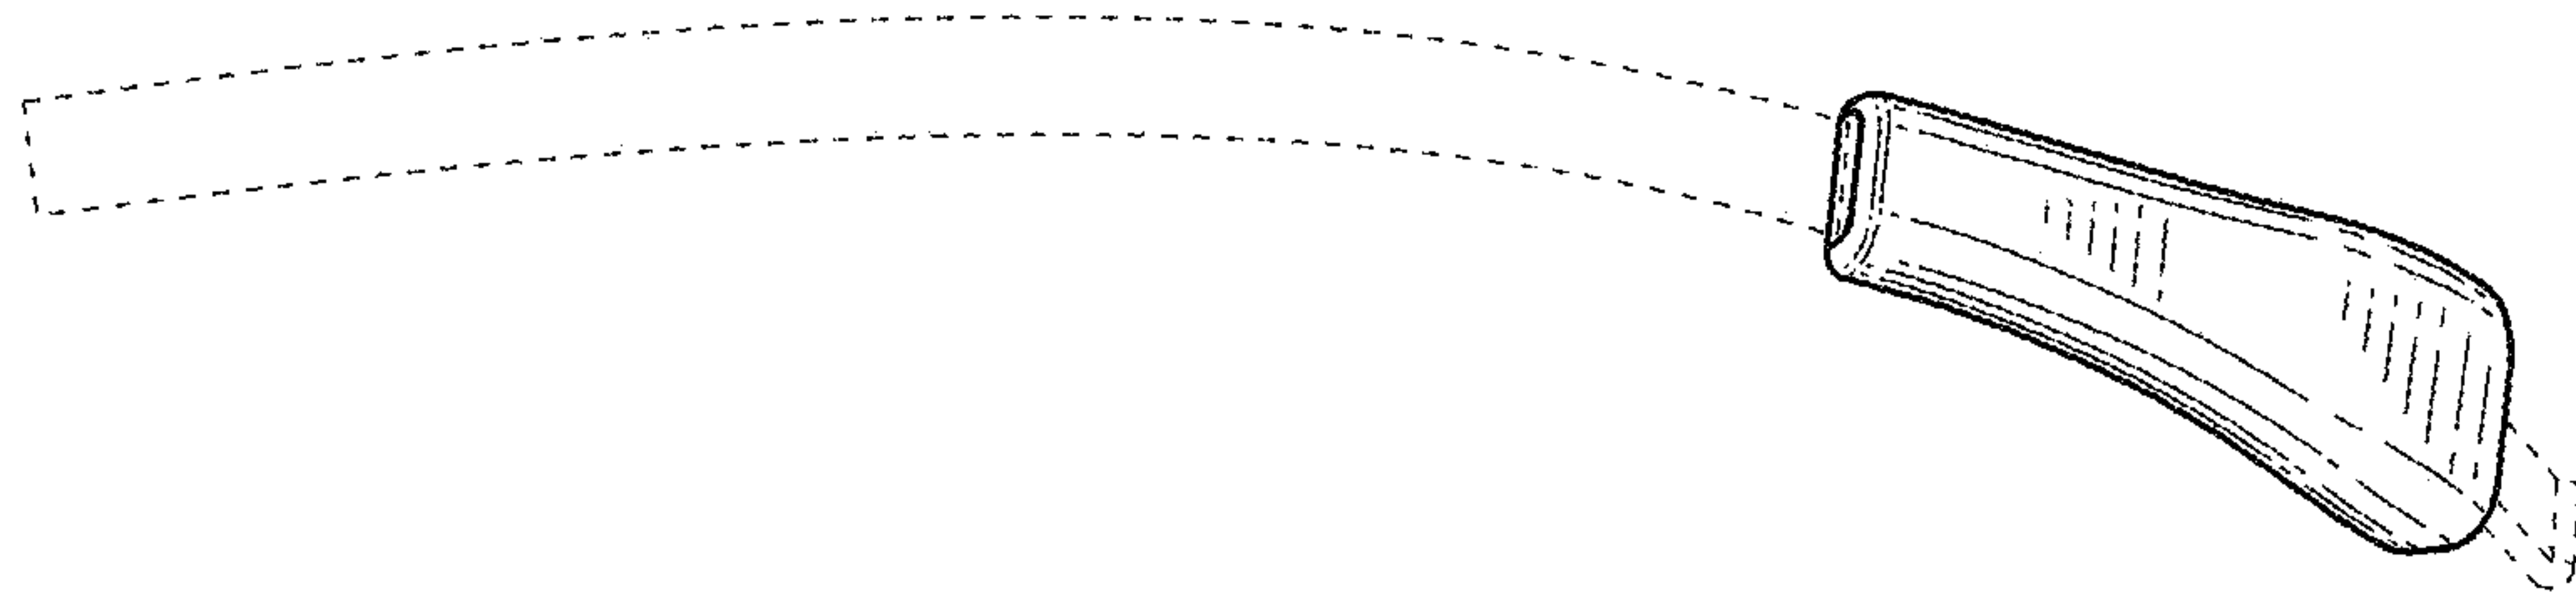


FIG. 5



FIG. 6

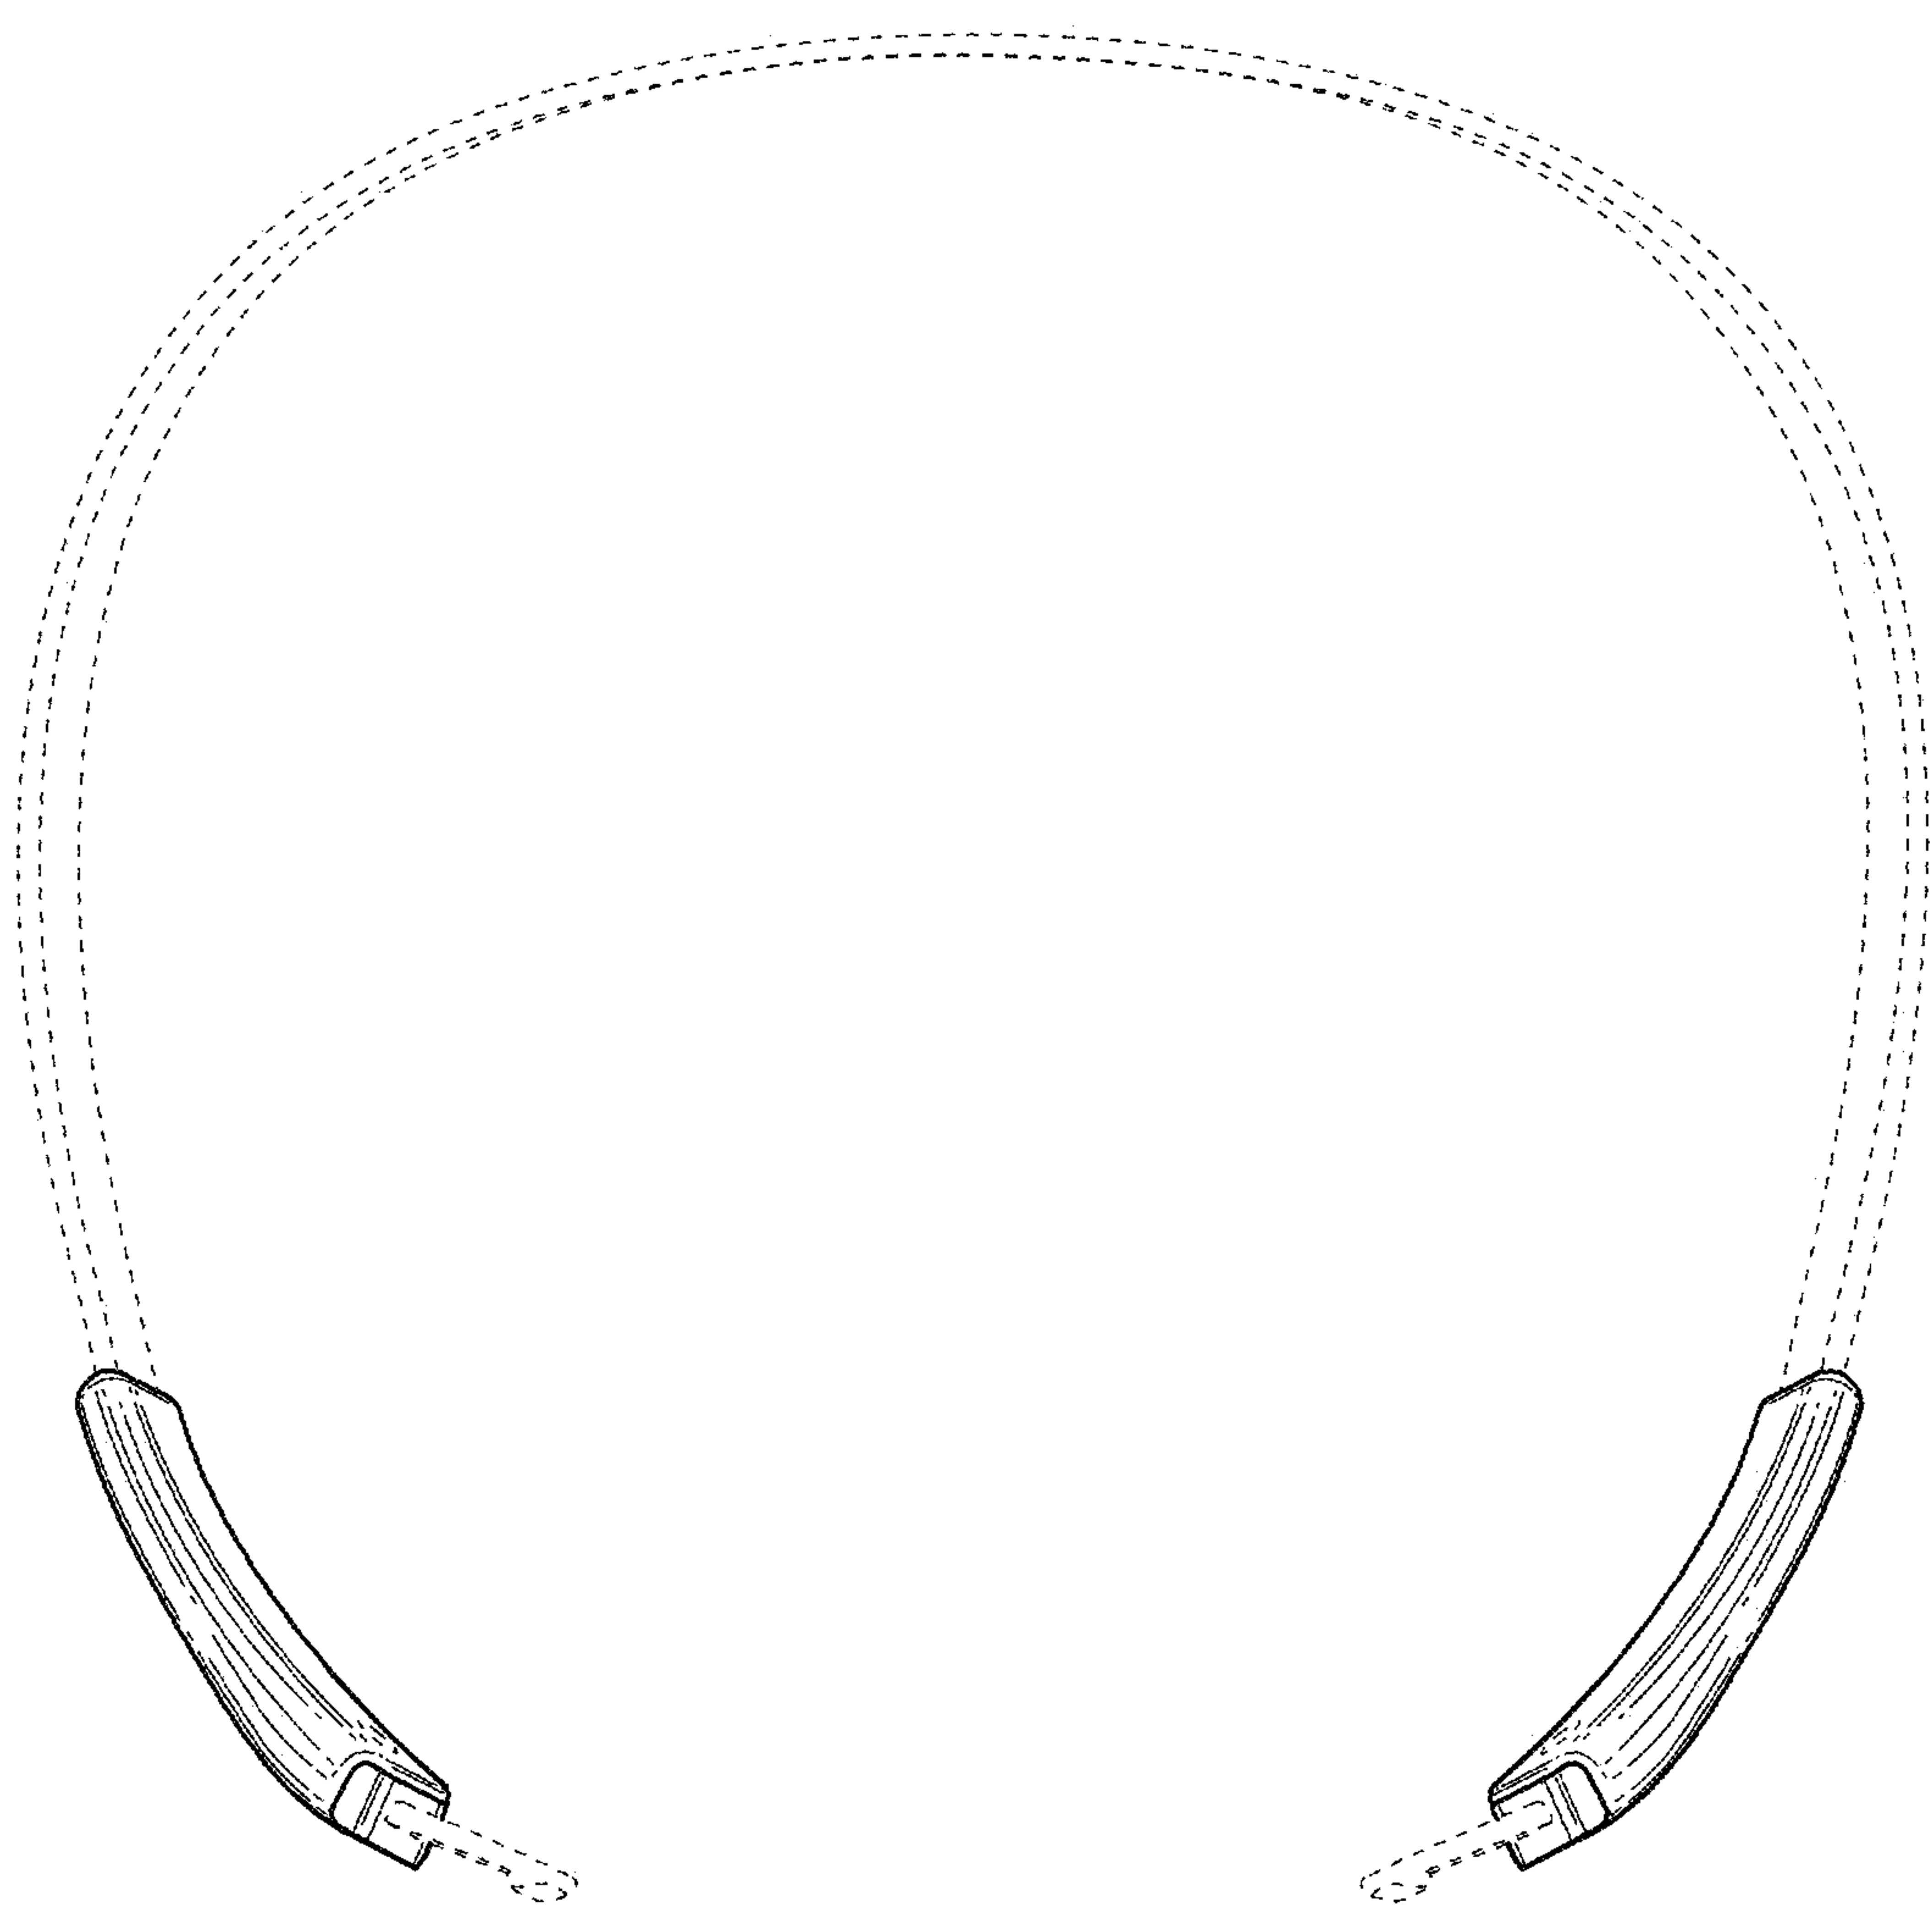


FIG. 7