



US0D1032837S

(12)

United States Design Patent

Stroh

(10)

Patent No.:

US D1,032,837 S

(45)

Date of Patent:

** Jun. 25, 2024

(54) SURGICAL CEMENT TAPPING TOOL

(71) Applicant: Shukla Medical, St. Petersburg, FL (US)

(72) Inventor: Austin Ryan Stroh, Lutz, FL (US)

(73) Assignee: Shukla Medical, St. Petersburg, FL (US)

(**) Term: 15 Years

(21) Appl. No.: 29/790,624

(22) Filed: Dec. 6, 2021

(51) LOC (14) Cl. 24-02

(52) U.S. Cl. USPC D24/146

(58) Field of Classification Search USPC D24/133, 146, 147, 155, 171, 200, 211, D24/215, 188; D8/82, 86, 89, 90; D7/649; D28/7 CPC A61B 17/16; A61B 17/1604; A61B 17/1615; A61B 17/1655; A61B 17/8802; A61B 17/152 See application file for complete search history.

(56) References Cited

U.S. PATENT DOCUMENTS

D216,286 S	*	12/1969	Valeska	D24/170
D255,048 S	*	5/1980	Miller	D24/147
D393,715 S	*	4/1998	Strickland	D24/133
D397,437 S	*	8/1998	Hlavicka	D24/146
D565,181 S	*	3/2008	Anitua Aldecoa	D24/156
D588,699 S	*	3/2009	Aldecoa	D24/156
D603,514 S	*	11/2009	Emanuelli	D24/156
D623,294 S	*	9/2010	Rhoades	D24/146
D629,519 S	*	12/2010	Horton	D24/155
D725,269 S	*	3/2015	Chung	D24/155
D794,188 S	*	8/2017	Naglapura	D8/86
D842,475 S	*	3/2019	Ben Shabat	D24/155
D857,897 S	*	8/2019	Loftus	D24/155
D872,264 S	*	1/2020	Thomé	D24/155

D952,855 S * 5/2022 Robbins A61B 17/7055 D24/155

D1,009,258 S * 12/2023 Leibowitz D24/133

D1,009,259 S * 12/2023 Leibowitz D24/133

(Continued)

OTHER PUBLICATIONS

Shukla Nail (S9NAIL), shuklamedical.com, revised Jul. 10, 2020, [online], [site visited Oct. 30, 2023], Available from internet, URL: https://www.shuklamedical.com/images/Product_Guides/070120/L3-NAIL-PG-070120.pdf (Year: 2020).*

Primary Examiner — Samantha Q Lawrence

Assistant Examiner — Thanh Luu Wong

(74) Attorney, Agent, or Firm — Kim IP Law Group LLC


(57) CLAIM

The ornamental design for a surgical cement tapping tool, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of a surgical cement tapping tool in accordance with the new design;
FIG. 2 is an enlarged partial right side view of the surgical cement tapping tool of FIG. 1;
FIG. 3 is an enlarged partial left side view of the surgical cement tapping tool of FIG. 1;
FIG. 4 is an enlarged partial top view of the surgical cement tapping tool of FIG. 1;
FIG. 5 is an enlarged partial bottom view of the surgical cement tapping tool of FIG. 1;
FIG. 6 is a front view of the surgical cement tapping tool of FIG. 1; and,
FIG. 7 is a rear view of the surgical cement tapping tool of FIG. 1.
In the drawings, the broken lines shown in FIGS. 1, 6 and 7 illustrate portions of the surgical cement tapping tool that form no part of the claimed design.

1 Claim, 6 Drawing Sheets

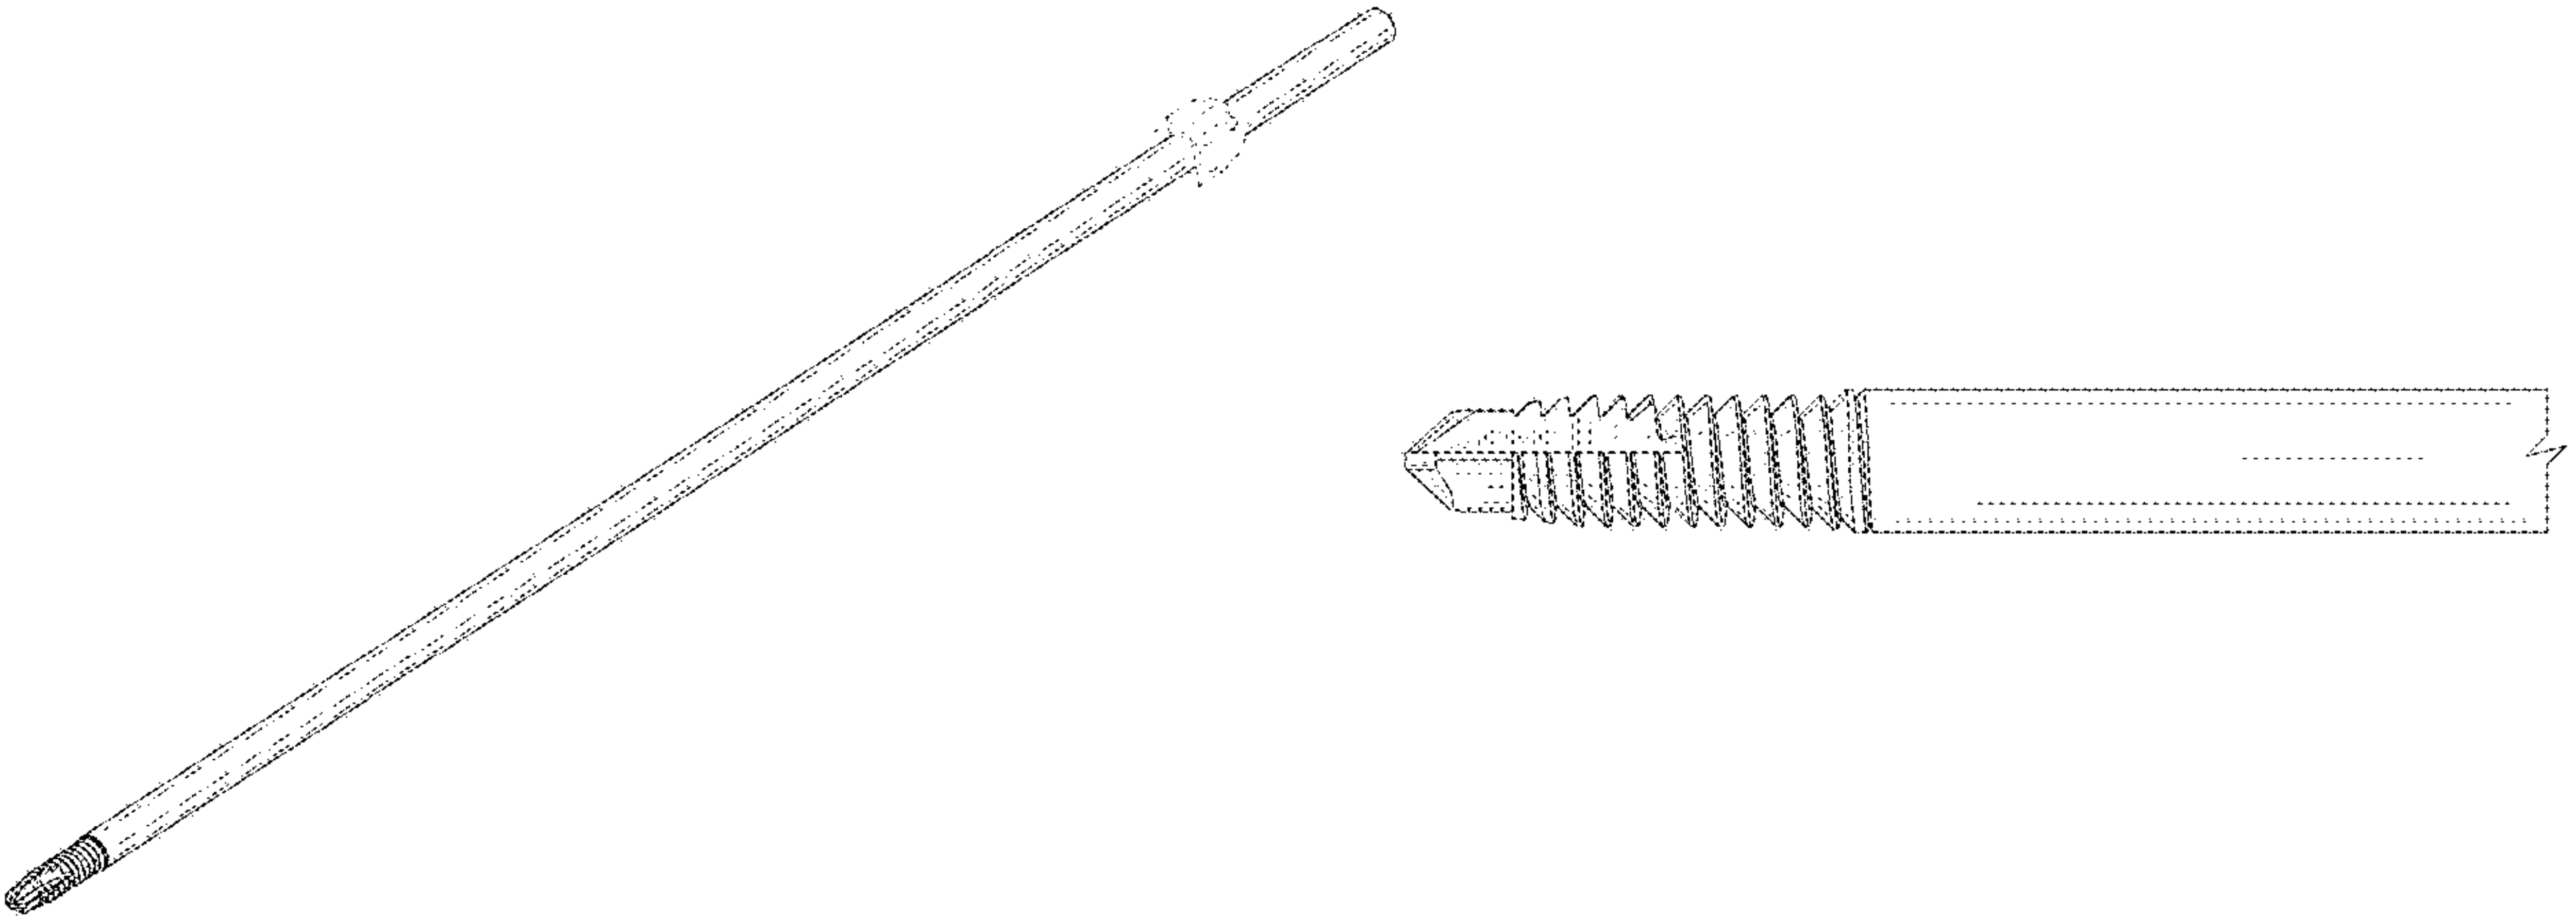

References Cited

D1,009,260	S	*	12/2023	Leibowitz	D24/133
D1,009,266	S	*	12/2023	Maruo	A61B 17/162
					D24/147
2007/0293867	A1	*	12/2007	Anitua	A61C 8/0089
					606/80
2008/0051793	A1	*	2/2008	Erickson	A61B 17/1671
					606/279
2013/0253521	A1	*	9/2013	Ellis	A61B 17/1655
					606/80

* cited by examiner

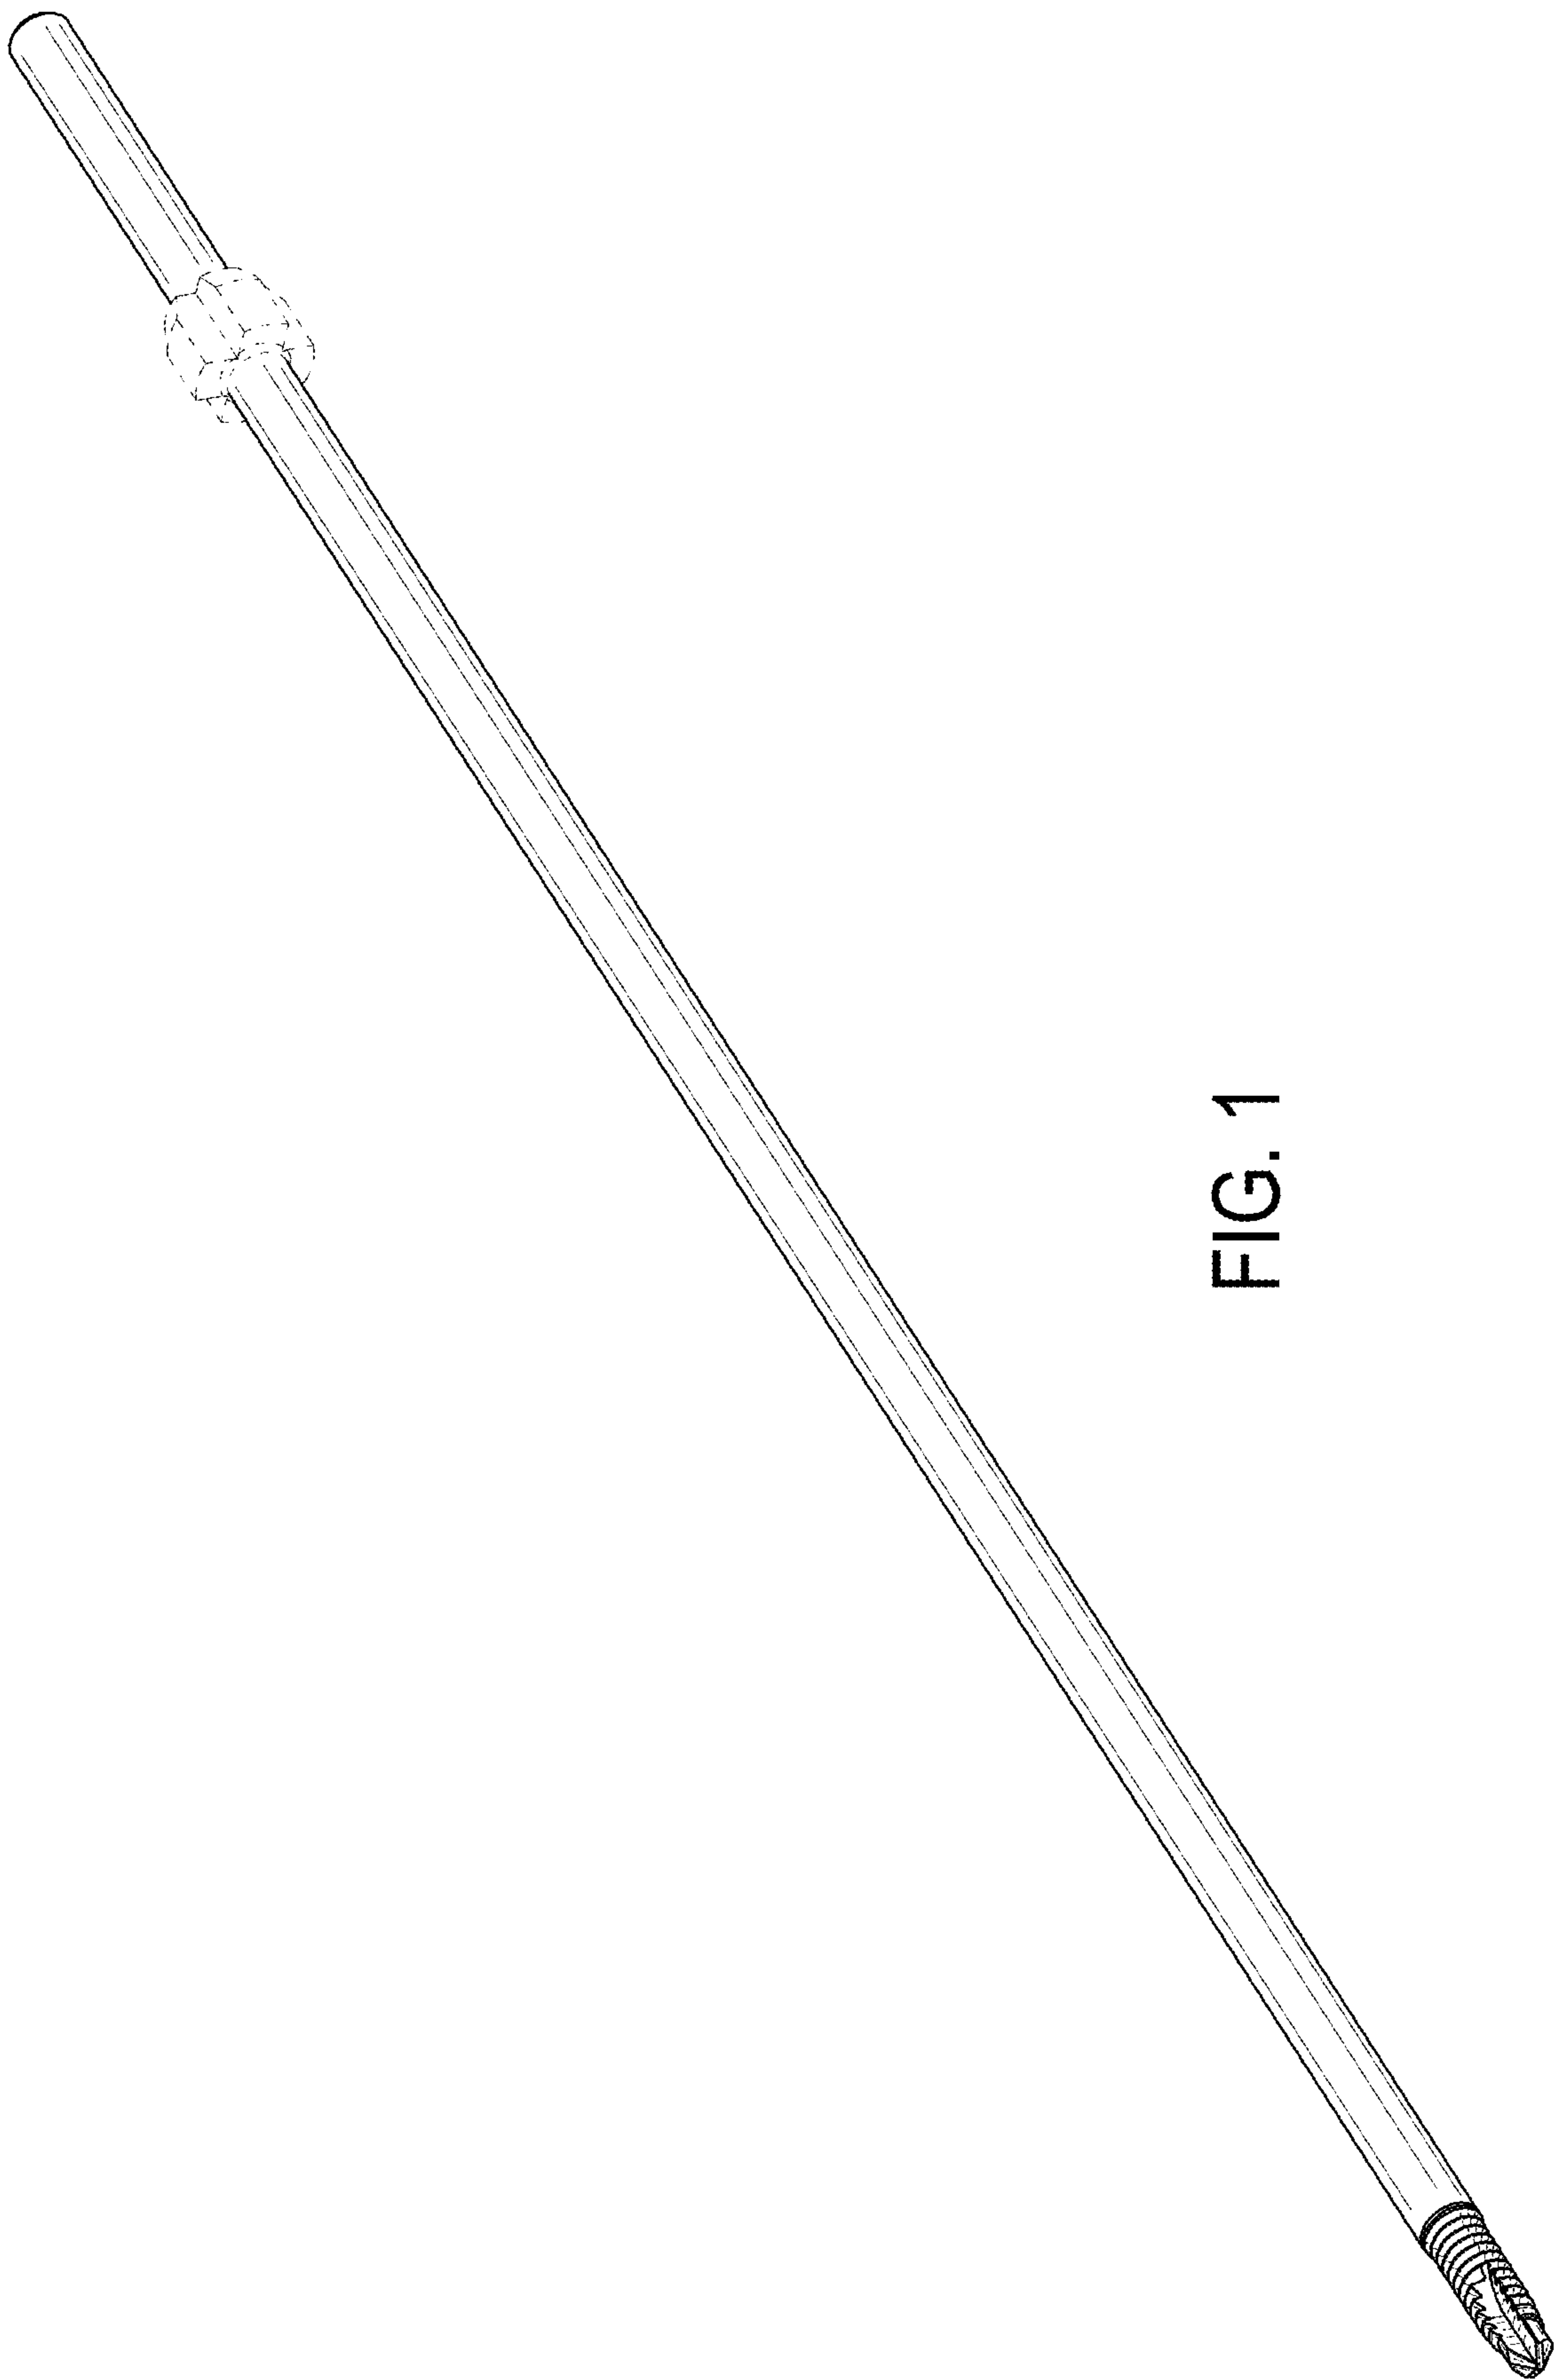


FIG. 1

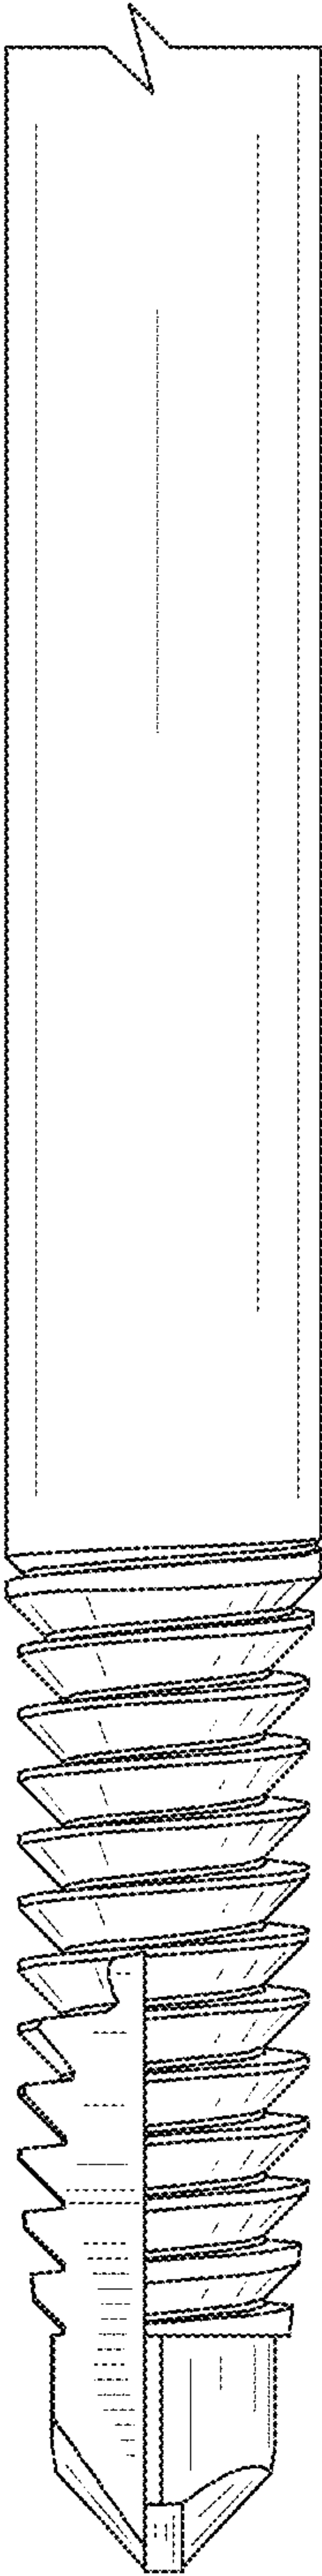


FIG. 2

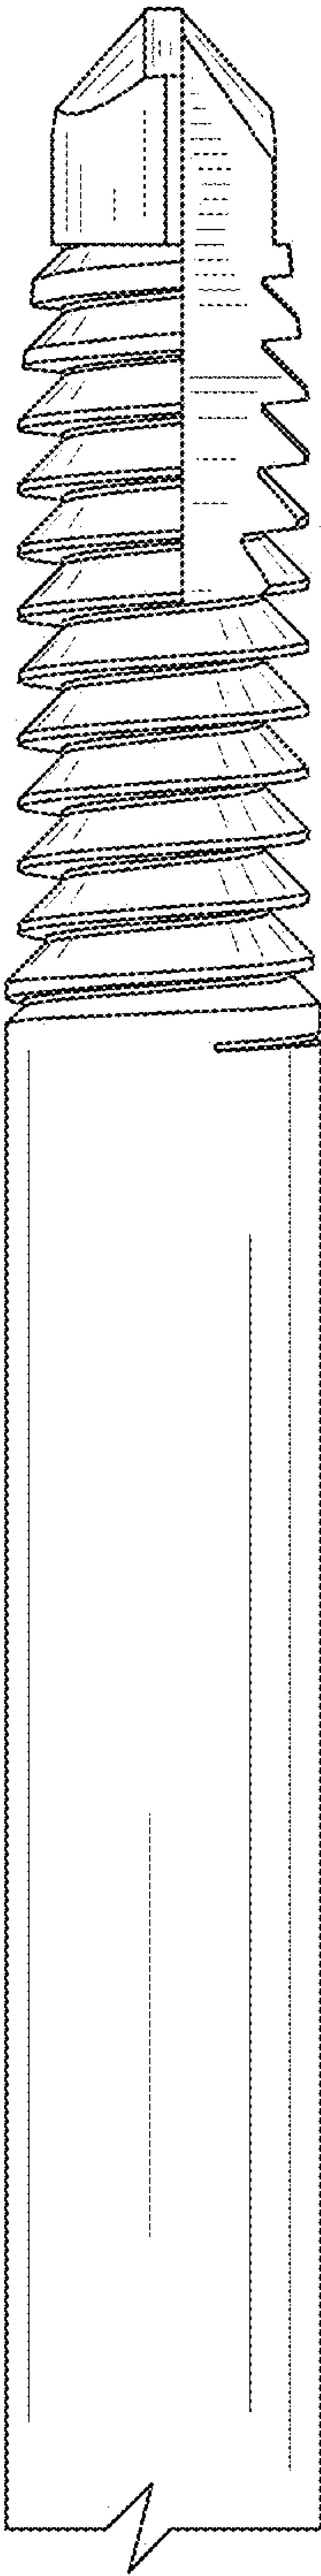


FIG. 3

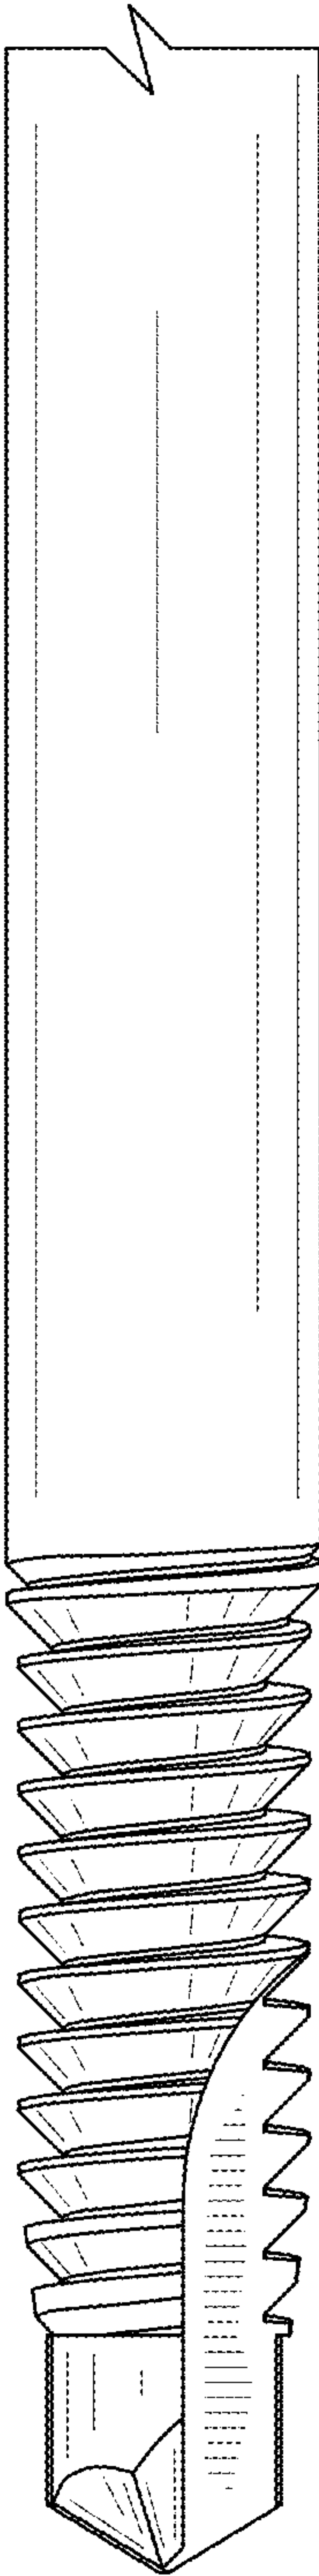


FIG. 4

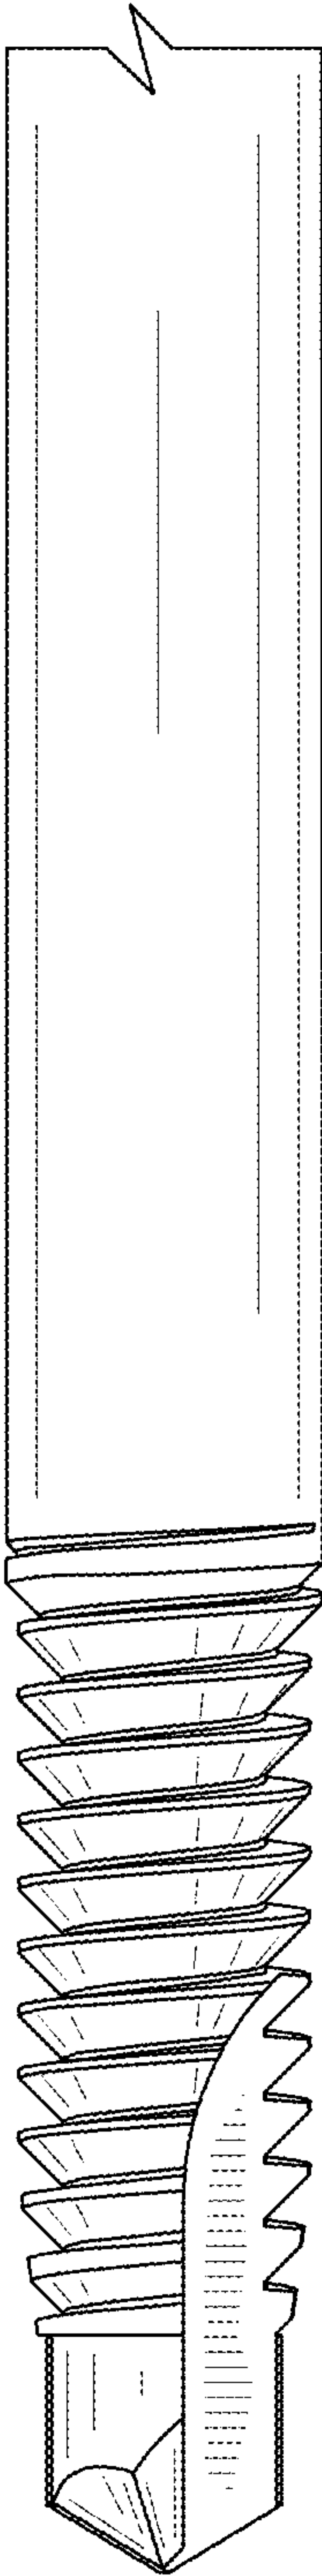


FIG. 5

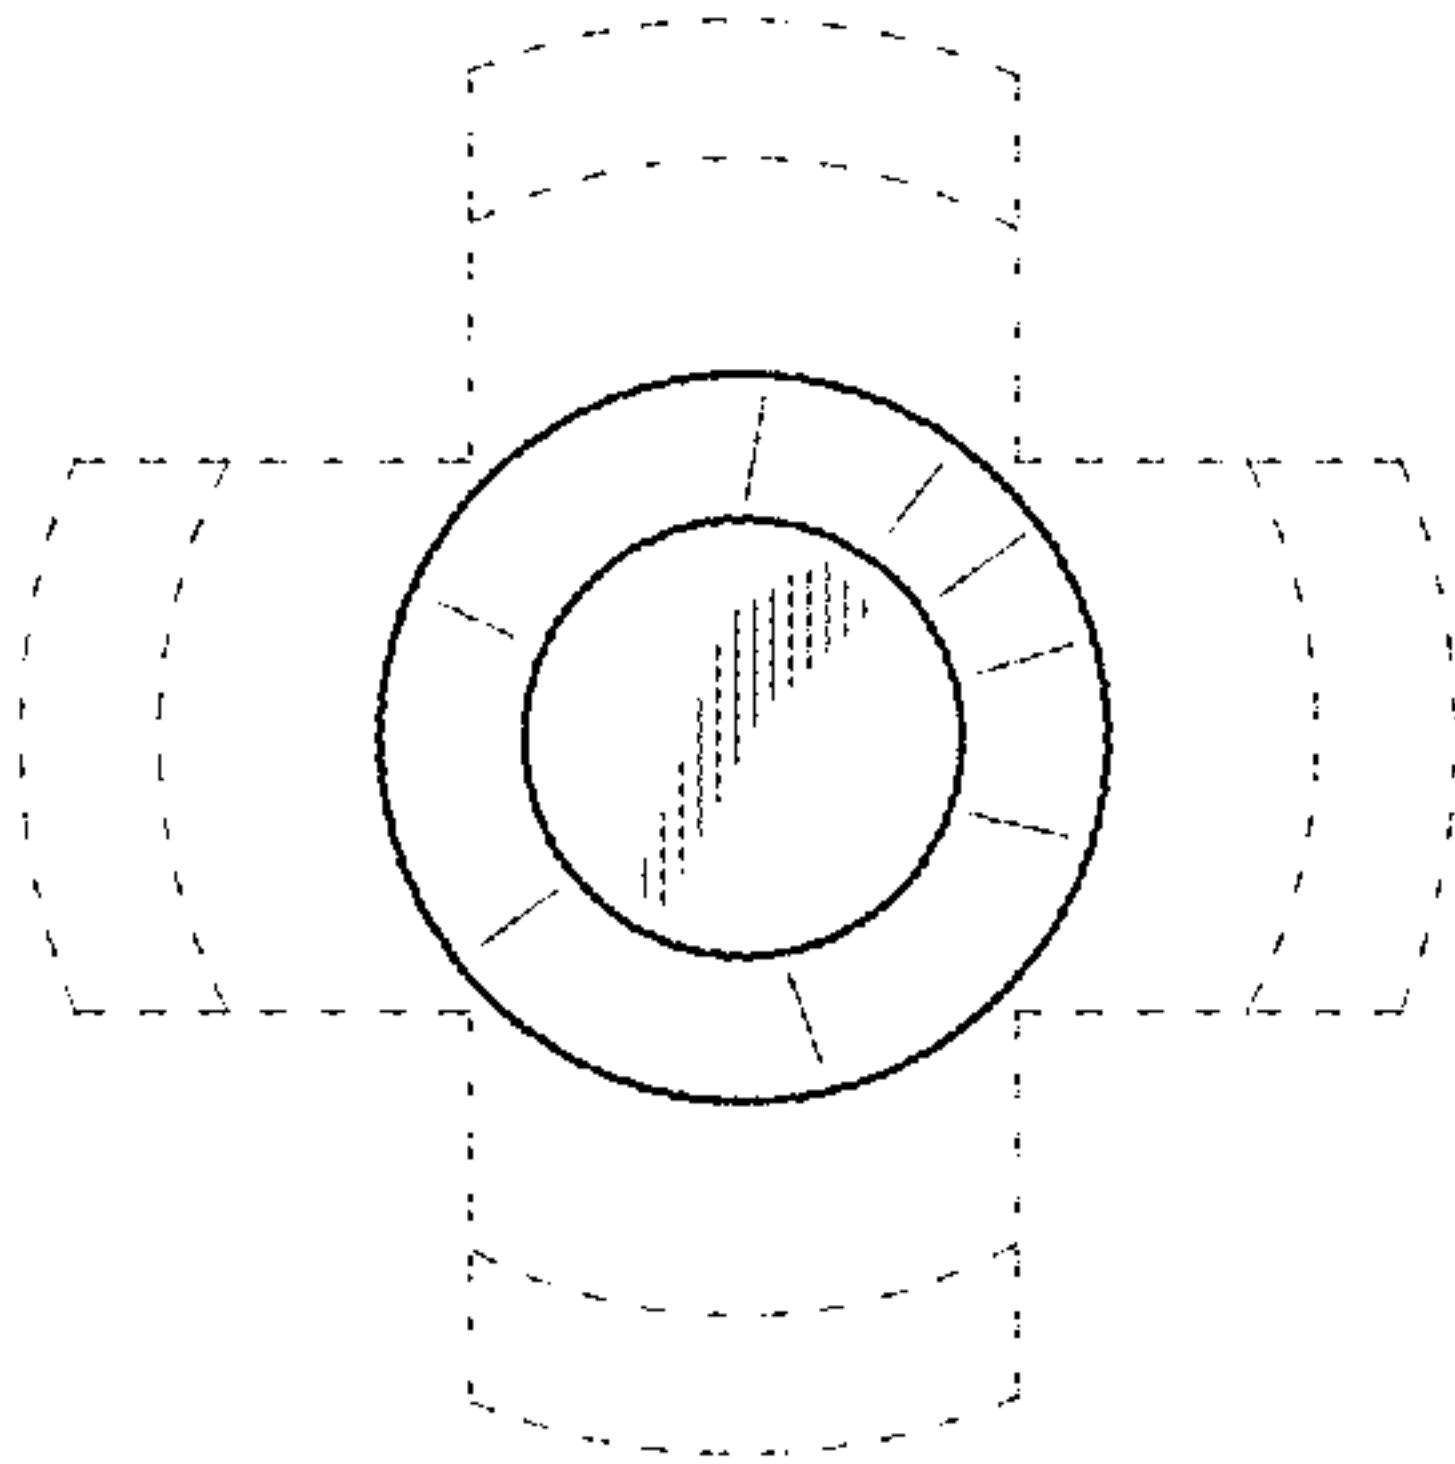


FIG. 6

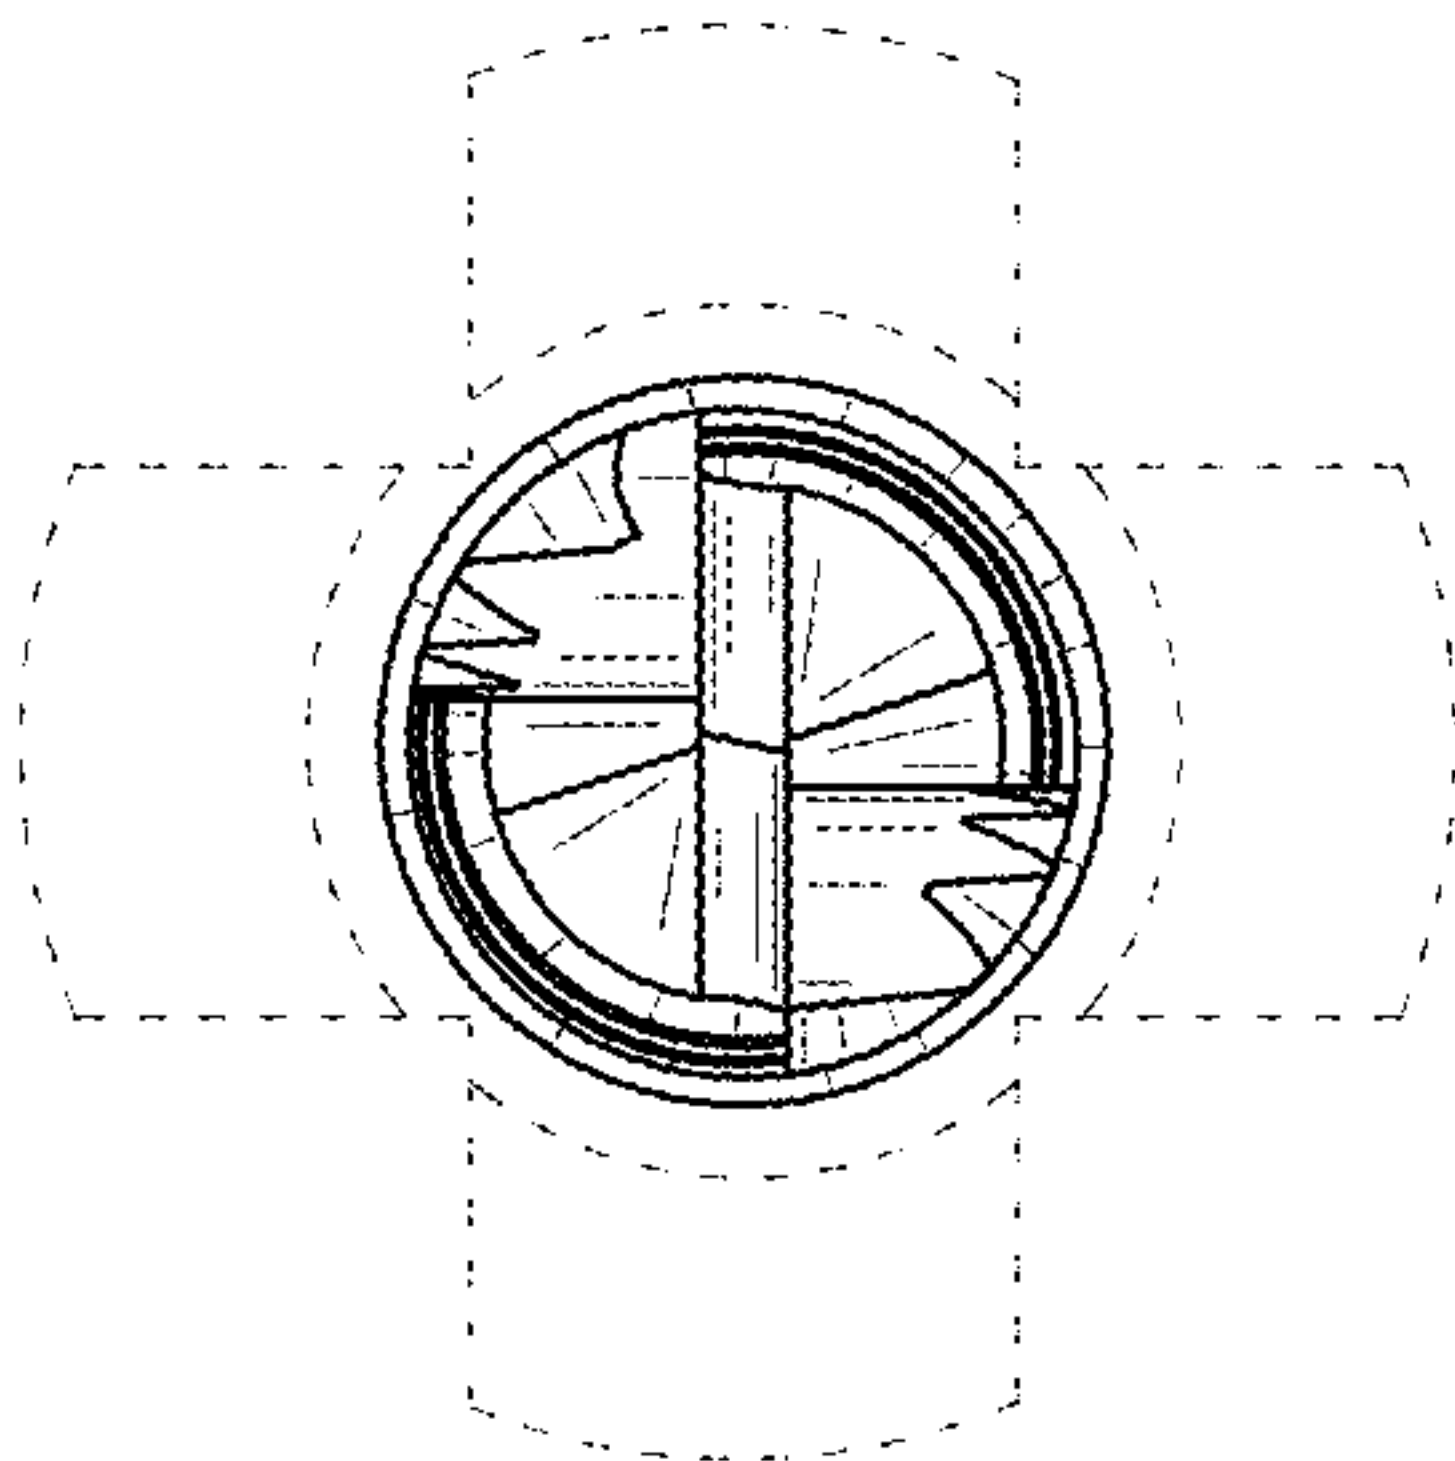


FIG. 7