



US0D1035003S

(12)

United States Design Patent

Peiris et al.

(10)

Patent No.:

US D1,035,003 S

(45)

Date of Patent:

** Jul. 9, 2024

(54) CONTAINER OF A FLUID TRAP FOR A RESPIRATORY DEVICE

(71) Applicant: Fisher & Paykel Healthcare Limited, Auckland (NZ)

(72) Inventors: Telge Nishan Chaturanga Peiris, Auckland (NZ); Paul Joseph Moody, Auckland (NZ); Nathan Lee Gray, Auckland (NZ)

(73) Assignee: Fisher & Paykel Healthcare Limited, Auckland (NZ)

D300,272 S 3/1989 Rudolph et al.

5,060,655 A 10/1991 Rudolph

D329,495 S 9/1992 Kotake

5,222,488 A * 6/1993 Forsgren B01D 46/521 55/DIG. 35

5,765,550 A 6/1998 Psaros et al.

5,947,954 A * 9/1999 Bonaldo A61M 39/26 604/905

6,244,311 B1 * 6/2001 Hand A61M 1/63 141/366

D449,106 S 10/2001 Madsen et al.

D472,636 S 4/2003 Haynes

D597,656 S * 8/2009 Bird D24/110

D605,282 S * 12/2009 Nichetti D24/108

(Continued)

(**) Term: 15 Years

Primary Examiner — Nathan M Johnston

(74) Attorney, Agent, or Firm — Knobbe, Martens, Olson and Bear, LLP

(21) Appl. No.: 29/878,843

(22) Filed: Jun. 28, 2023

Related U.S. Application Data

(62) Division of application No. 29/751,564, filed on Sep. 22, 2020, now Pat. No. Des. 995,783, which is a division of application No. 29/660,536, filed on Aug. 21, 2018, now Pat. No. Des. 900,319.

(51) LOC (14) Cl. 23-04

(52) U.S. Cl. D24/162; D24/110

(58) Field of Classification Search

USPC D24/110, 162, 164, 129, 165; 600/530, 600/533, 540, 538, 539; 128/200.24, 128/200.23, 201.28, 863, 205.23, 205.25, 128/204.25

CPC A61M 16/0808; A61M 16/206; A61M 16/0816; A61M 16/08; A61M 16/20

See application file for complete search history.

(56) References Cited

U.S. PATENT DOCUMENTS

D282,283 S 1/1986 Weigl et al.

D300,271 S 3/1989 Rudolph et al.

(57) CLAIM

The ornamental design for a container of a fluid trap for a respiratory device, as shown and described.

DESCRIPTION

FIG. 1 is a front, top, and side perspective view of a container of a fluid trap for a respiratory device embodying our new design;

FIG. 2 is a rear, bottom, and left side perspective view thereof;

FIG. 3 is a top view thereof;

FIG. 4 is a bottom view thereof;

FIG. 5 is a front view thereof;


FIG. 6 is a first side view thereof;

FIG. 7 is a second side view thereof; and,

FIG. 8 is a rear view of thereof.

Broken lines are used to illustrate portions of the container of a fluid trap for a respiratory device that form no part of the claimed design.

1 Claim, 7 Drawing Sheets

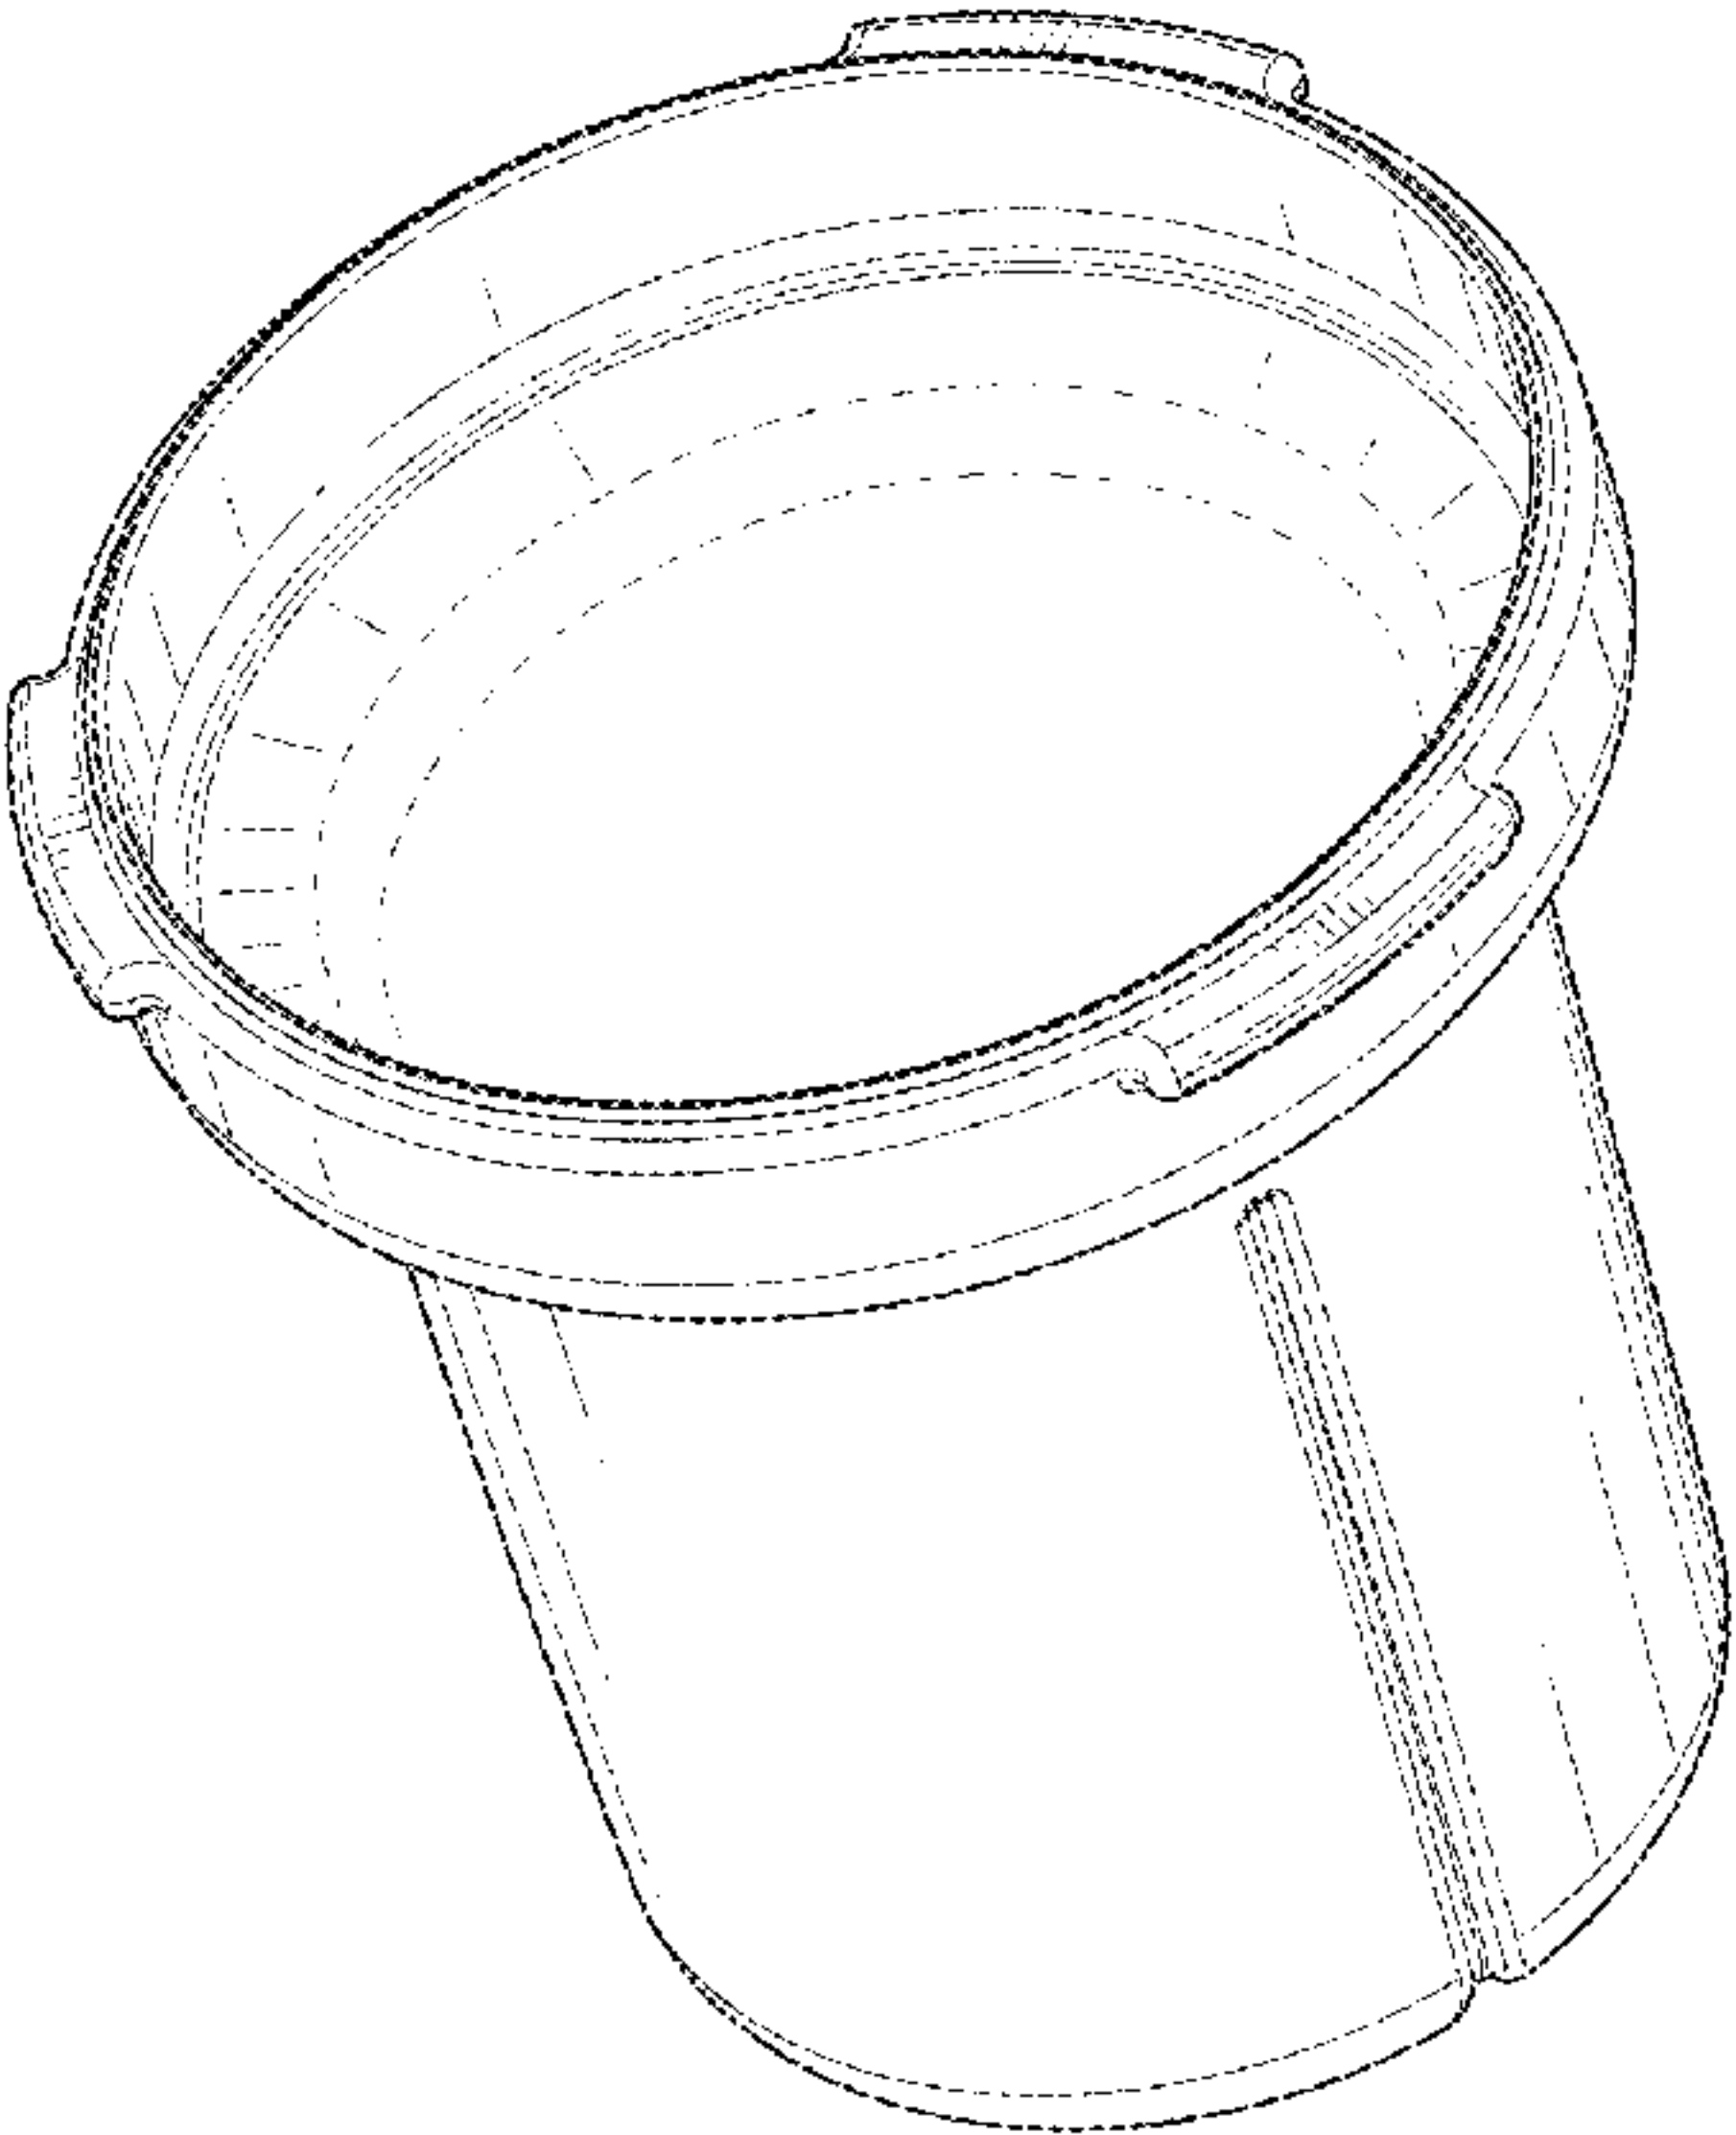

(56) **References Cited**

U.S. PATENT DOCUMENTS

D659,254	S	5/2012	Miyashita et al.	
D671,654	S	11/2012	Akamatsu et al.	
8,322,334	B2	12/2012	Lee et al.	
D679,026	S *	3/2013	Akamatsu	D24/232
8,408,209	B2	4/2013	Matsubara et al.	
D689,187	S	9/2013	Kruger	
D690,813	S	10/2013	Bizell et al.	
D691,717	S	10/2013	McLean et al.	
D693,001	S	11/2013	Wintter	
9,089,801	B1 *	7/2015	Gavlak	A61M 1/79
D818,580	S	5/2018	Khabiri et al.	
D828,550	S *	9/2018	Falleboe	D24/129
D831,202	S	10/2018	Ratner	
D833,599	S	11/2018	Nilsson et al.	
D834,712	S	11/2018	Gulliver et al.	
D851,240	S	6/2019	Baid	
D852,355	S	6/2019	Fiorenza	
D861,856	S	10/2019	Lin et al.	
D900,319	S	10/2020	Peiris et al.	
10,857,317	B2	12/2020	Costella et al.	
D919,799	S	5/2021	Zollinger	
D940,308	S	1/2022	Leibitzki et al.	
D959,657	S	8/2022	Legeais et al.	
2011/0106029	A1 *	5/2011	Garren	A61B 10/0045 604/319
2011/0114090	A1	5/2011	Piper	
2011/0201958	A1	8/2011	Lazar et al.	
2011/0232636	A1	9/2011	Von Hollen et al.	
2012/0227735	A1	9/2012	Abate et al.	
2013/0144248	A1 *	6/2013	Putter	A61M 5/165 604/405
2014/0081167	A1	3/2014	Lomask et al.	
2015/0265185	A1	9/2015	Brugnoli	
2017/0103634	A1	4/2017	Velez	
2020/0023154	A1	1/2020	Gray et al.	

* cited by examiner

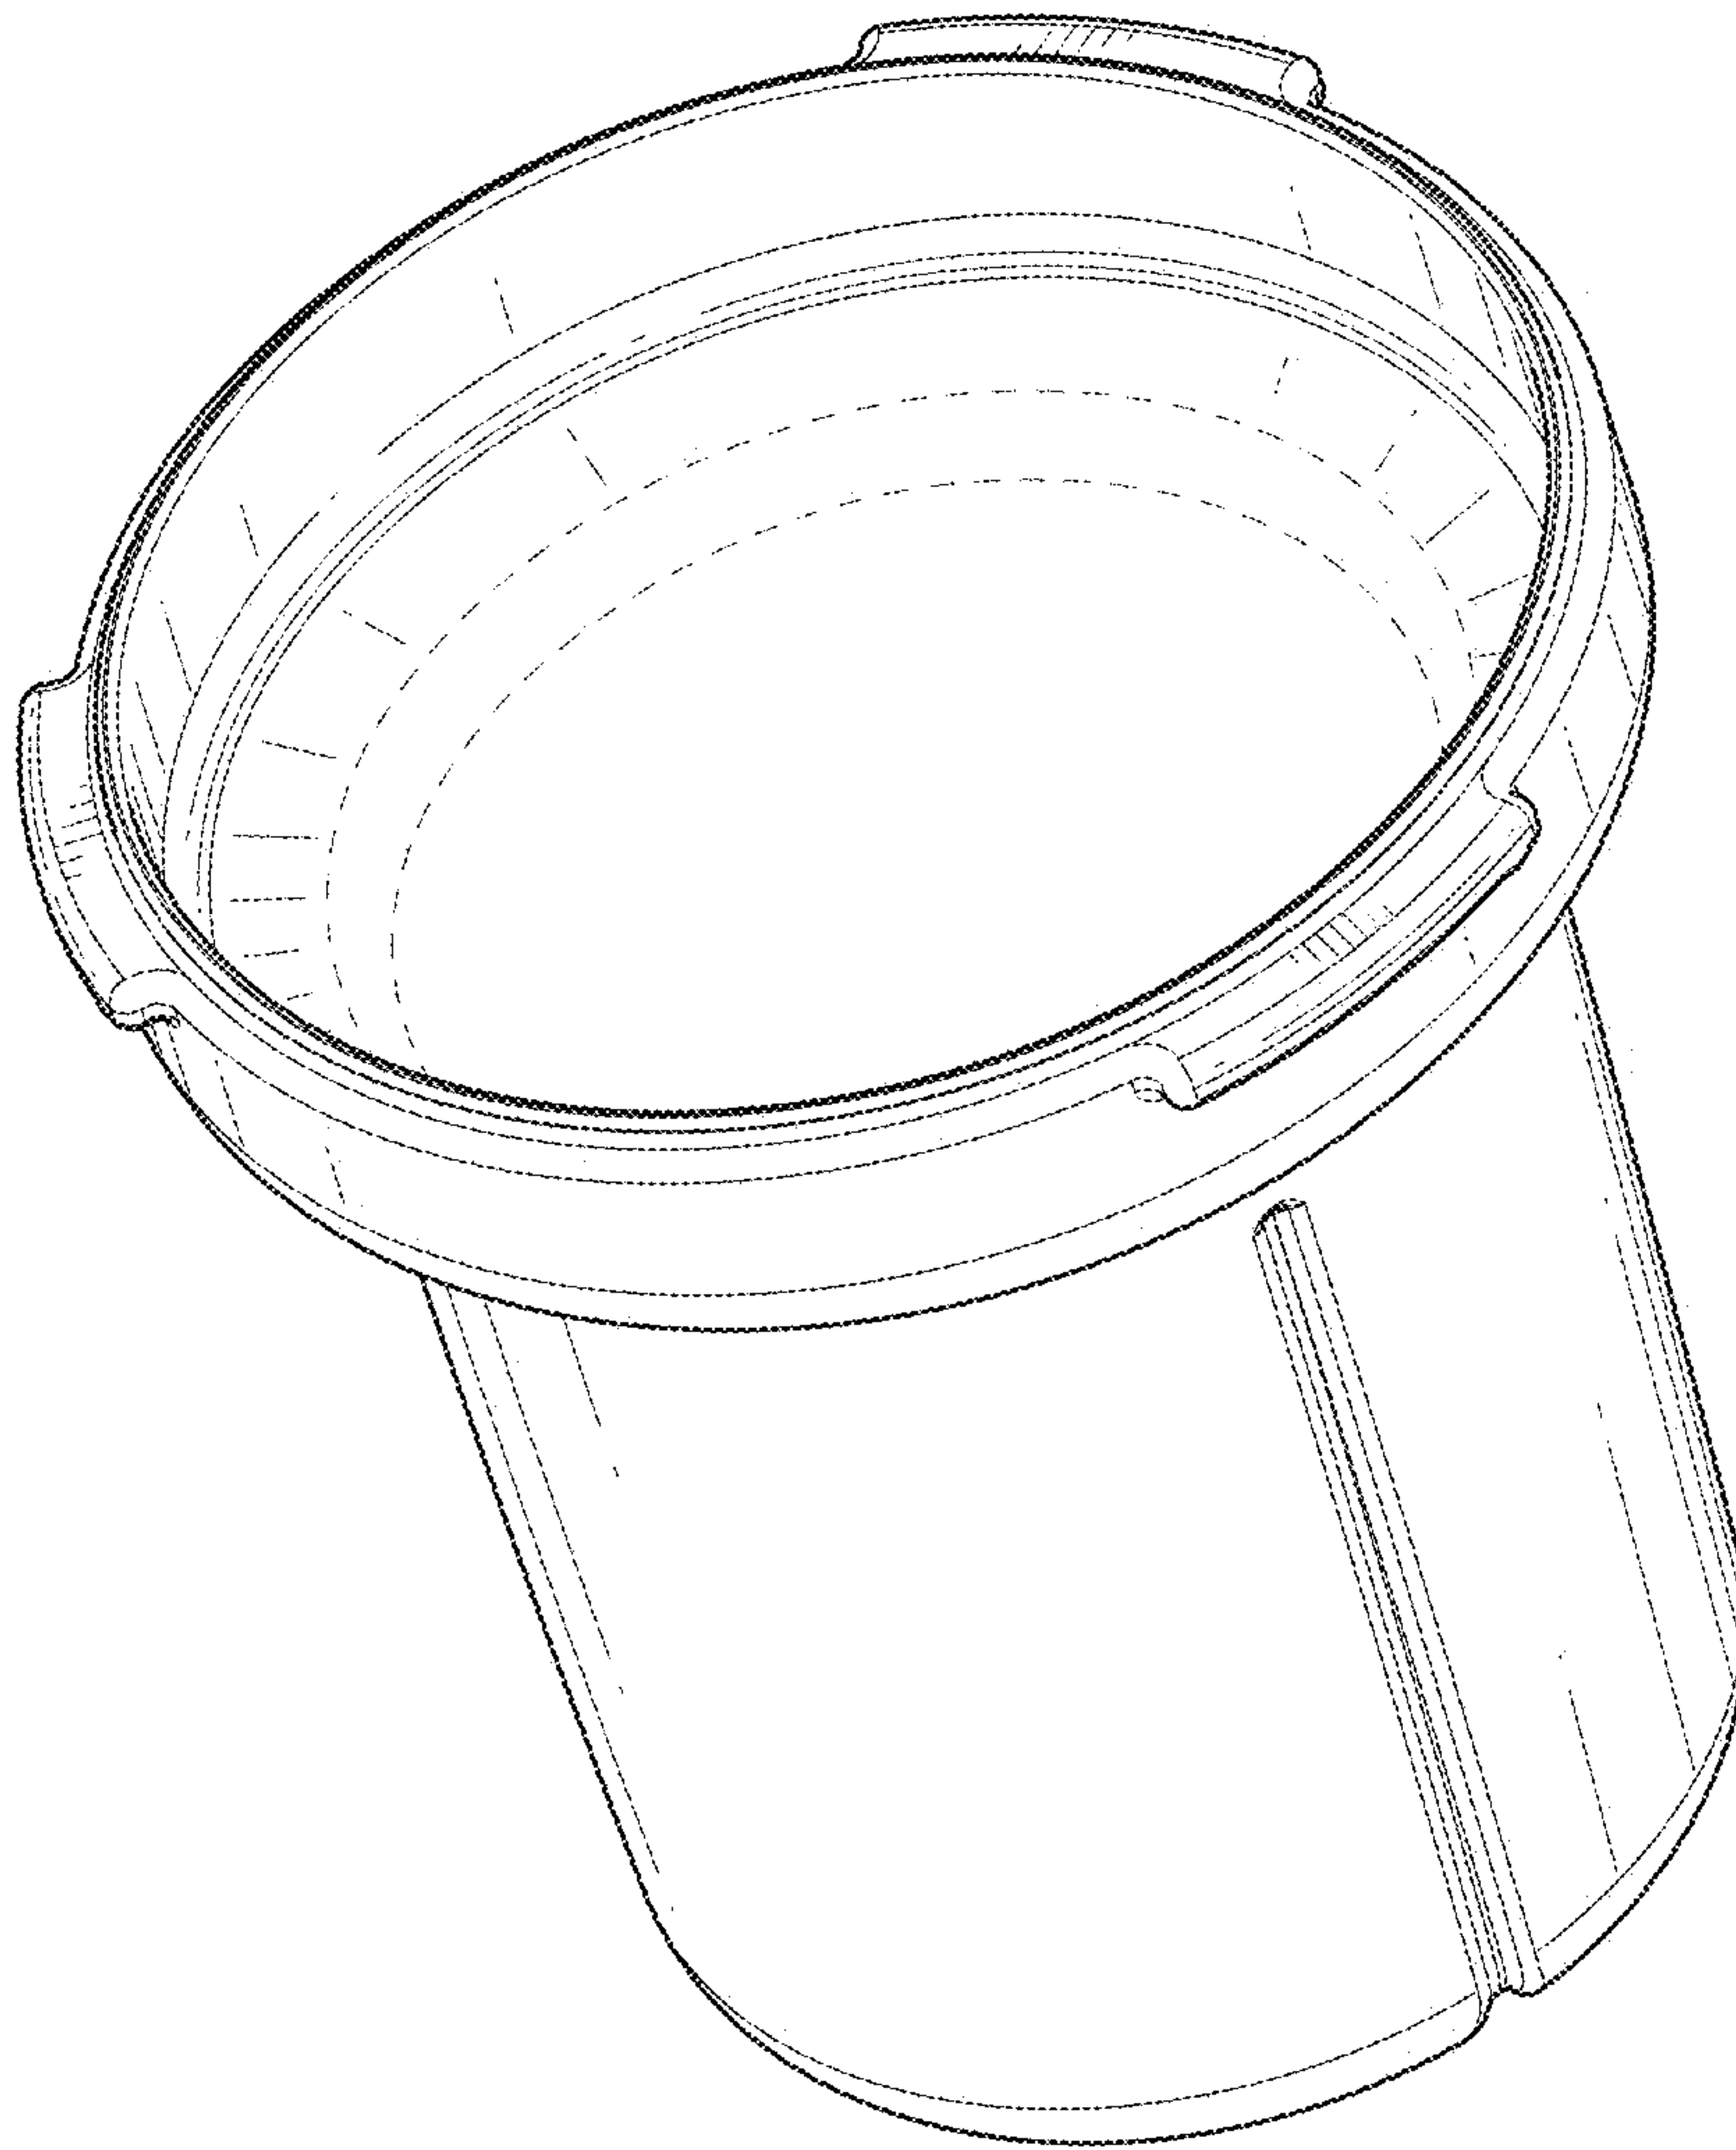


FIG. 1

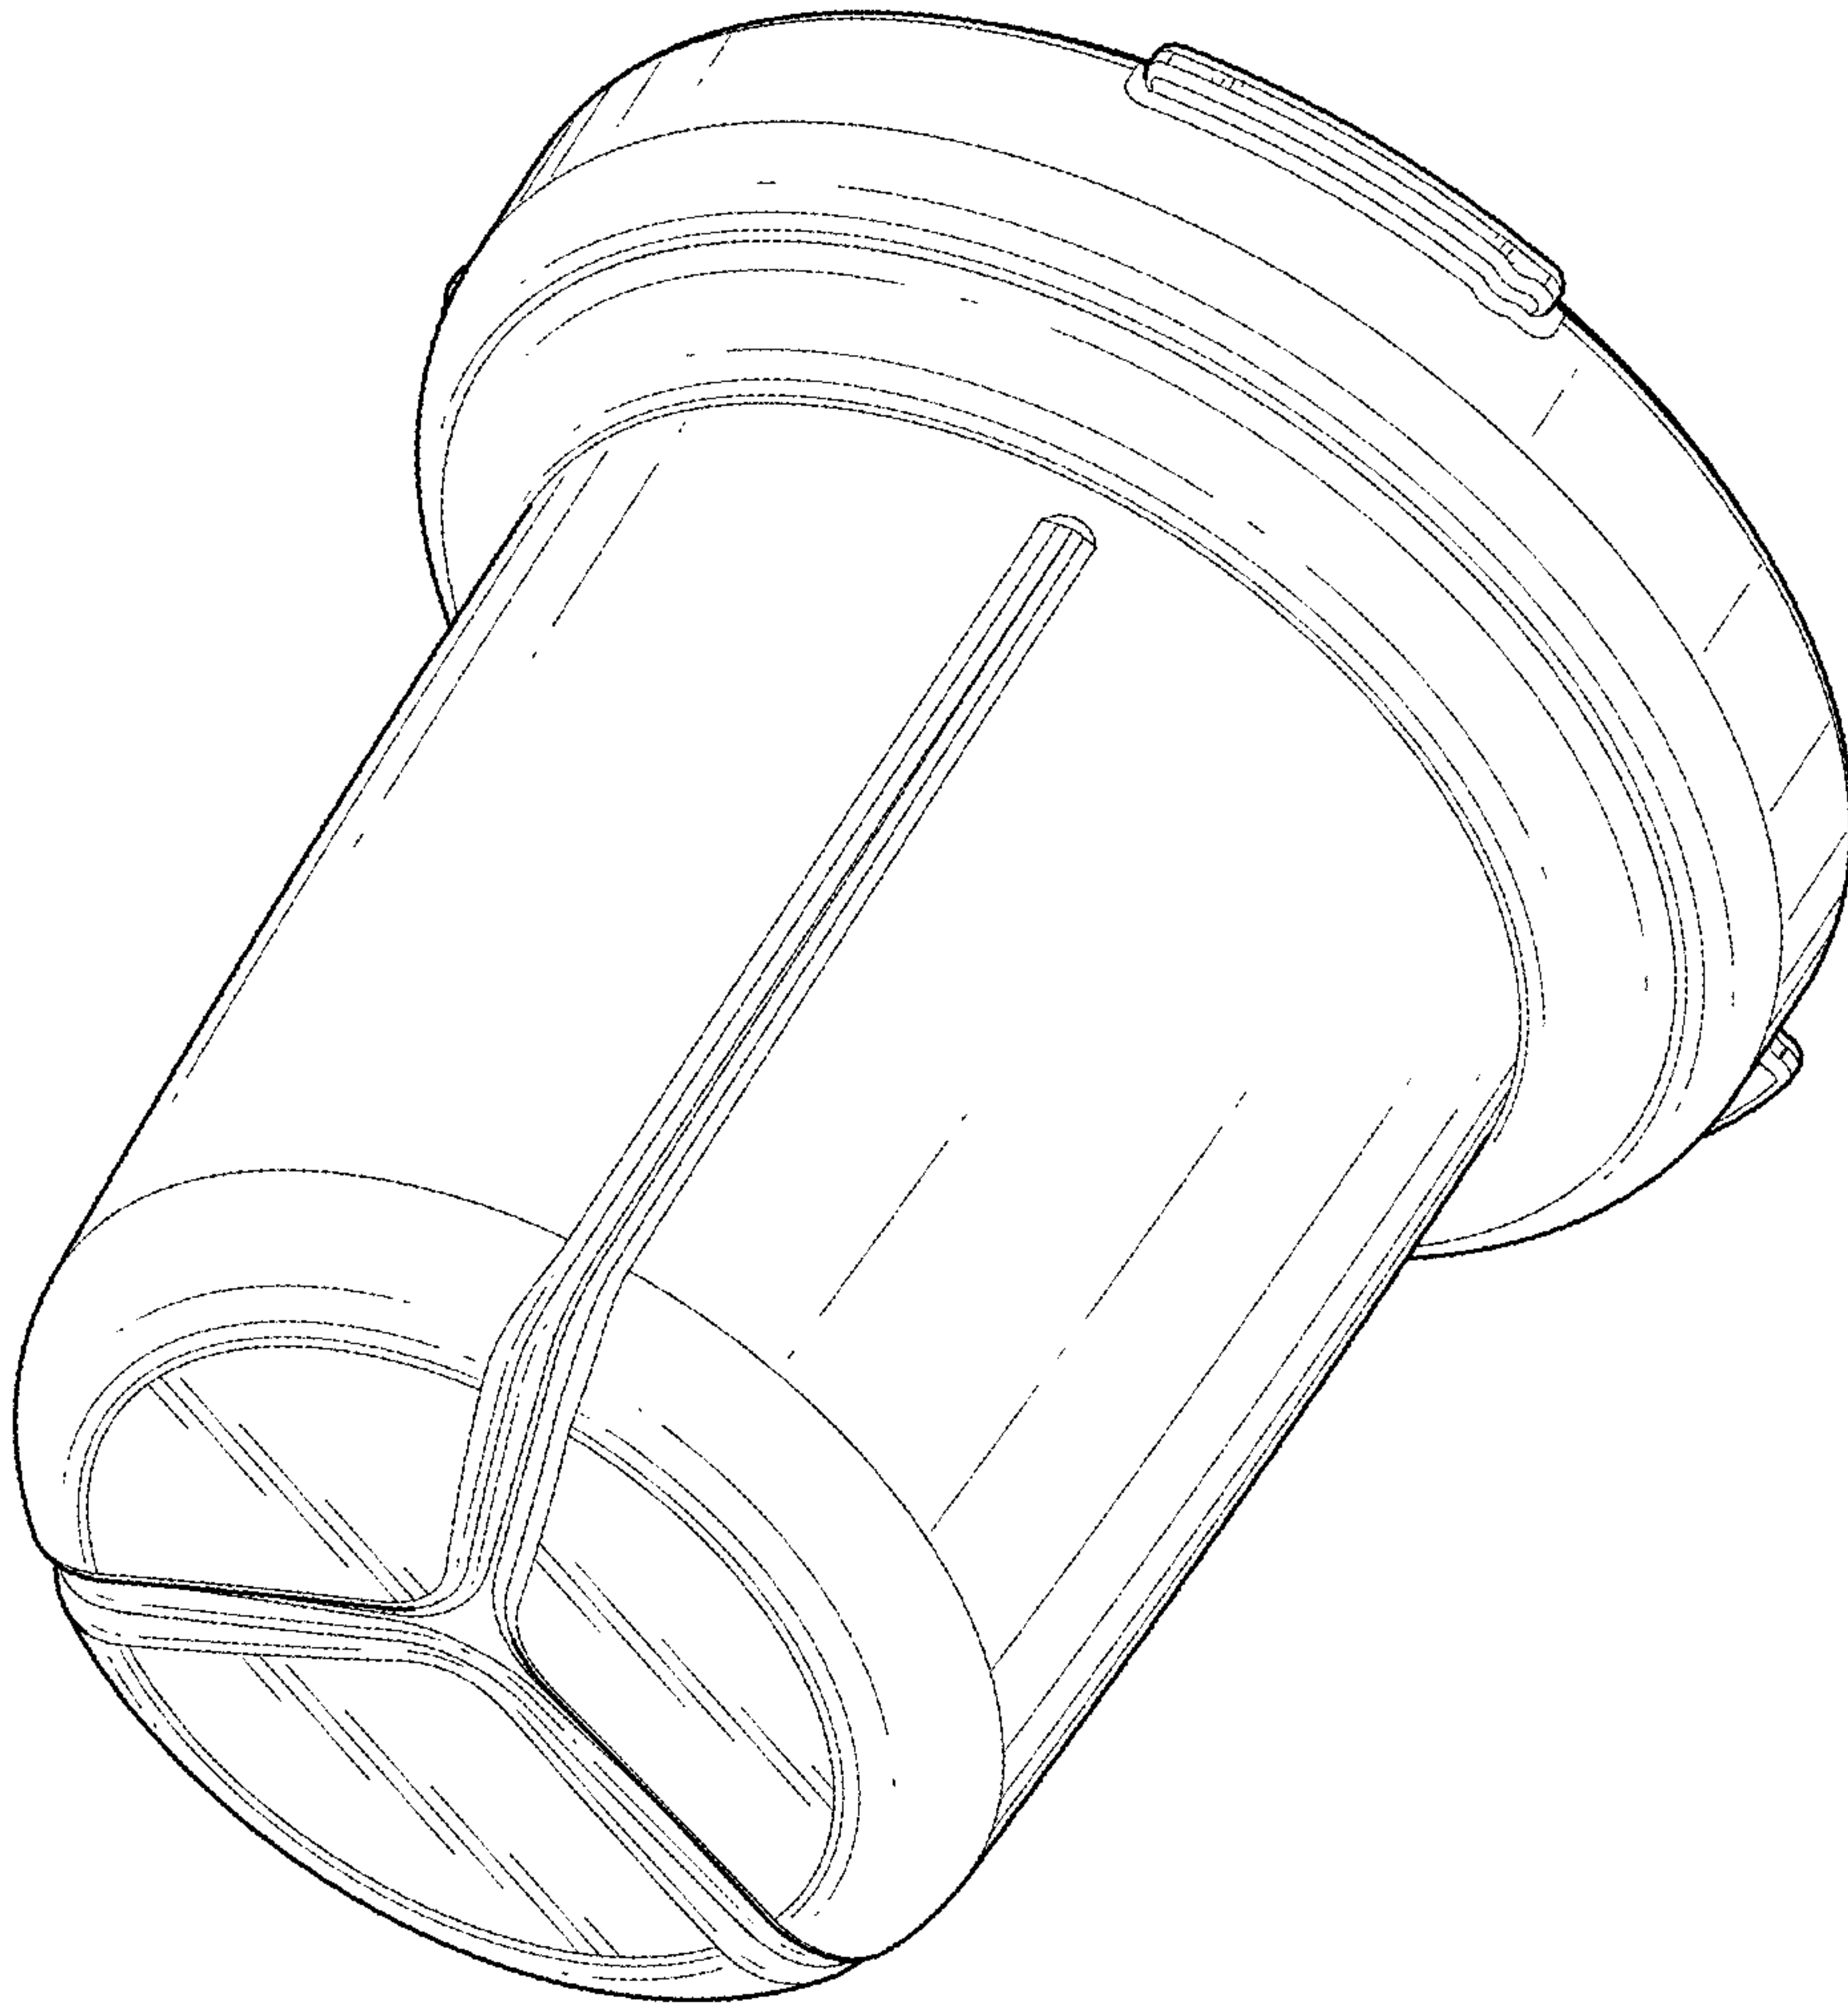


FIG. 2

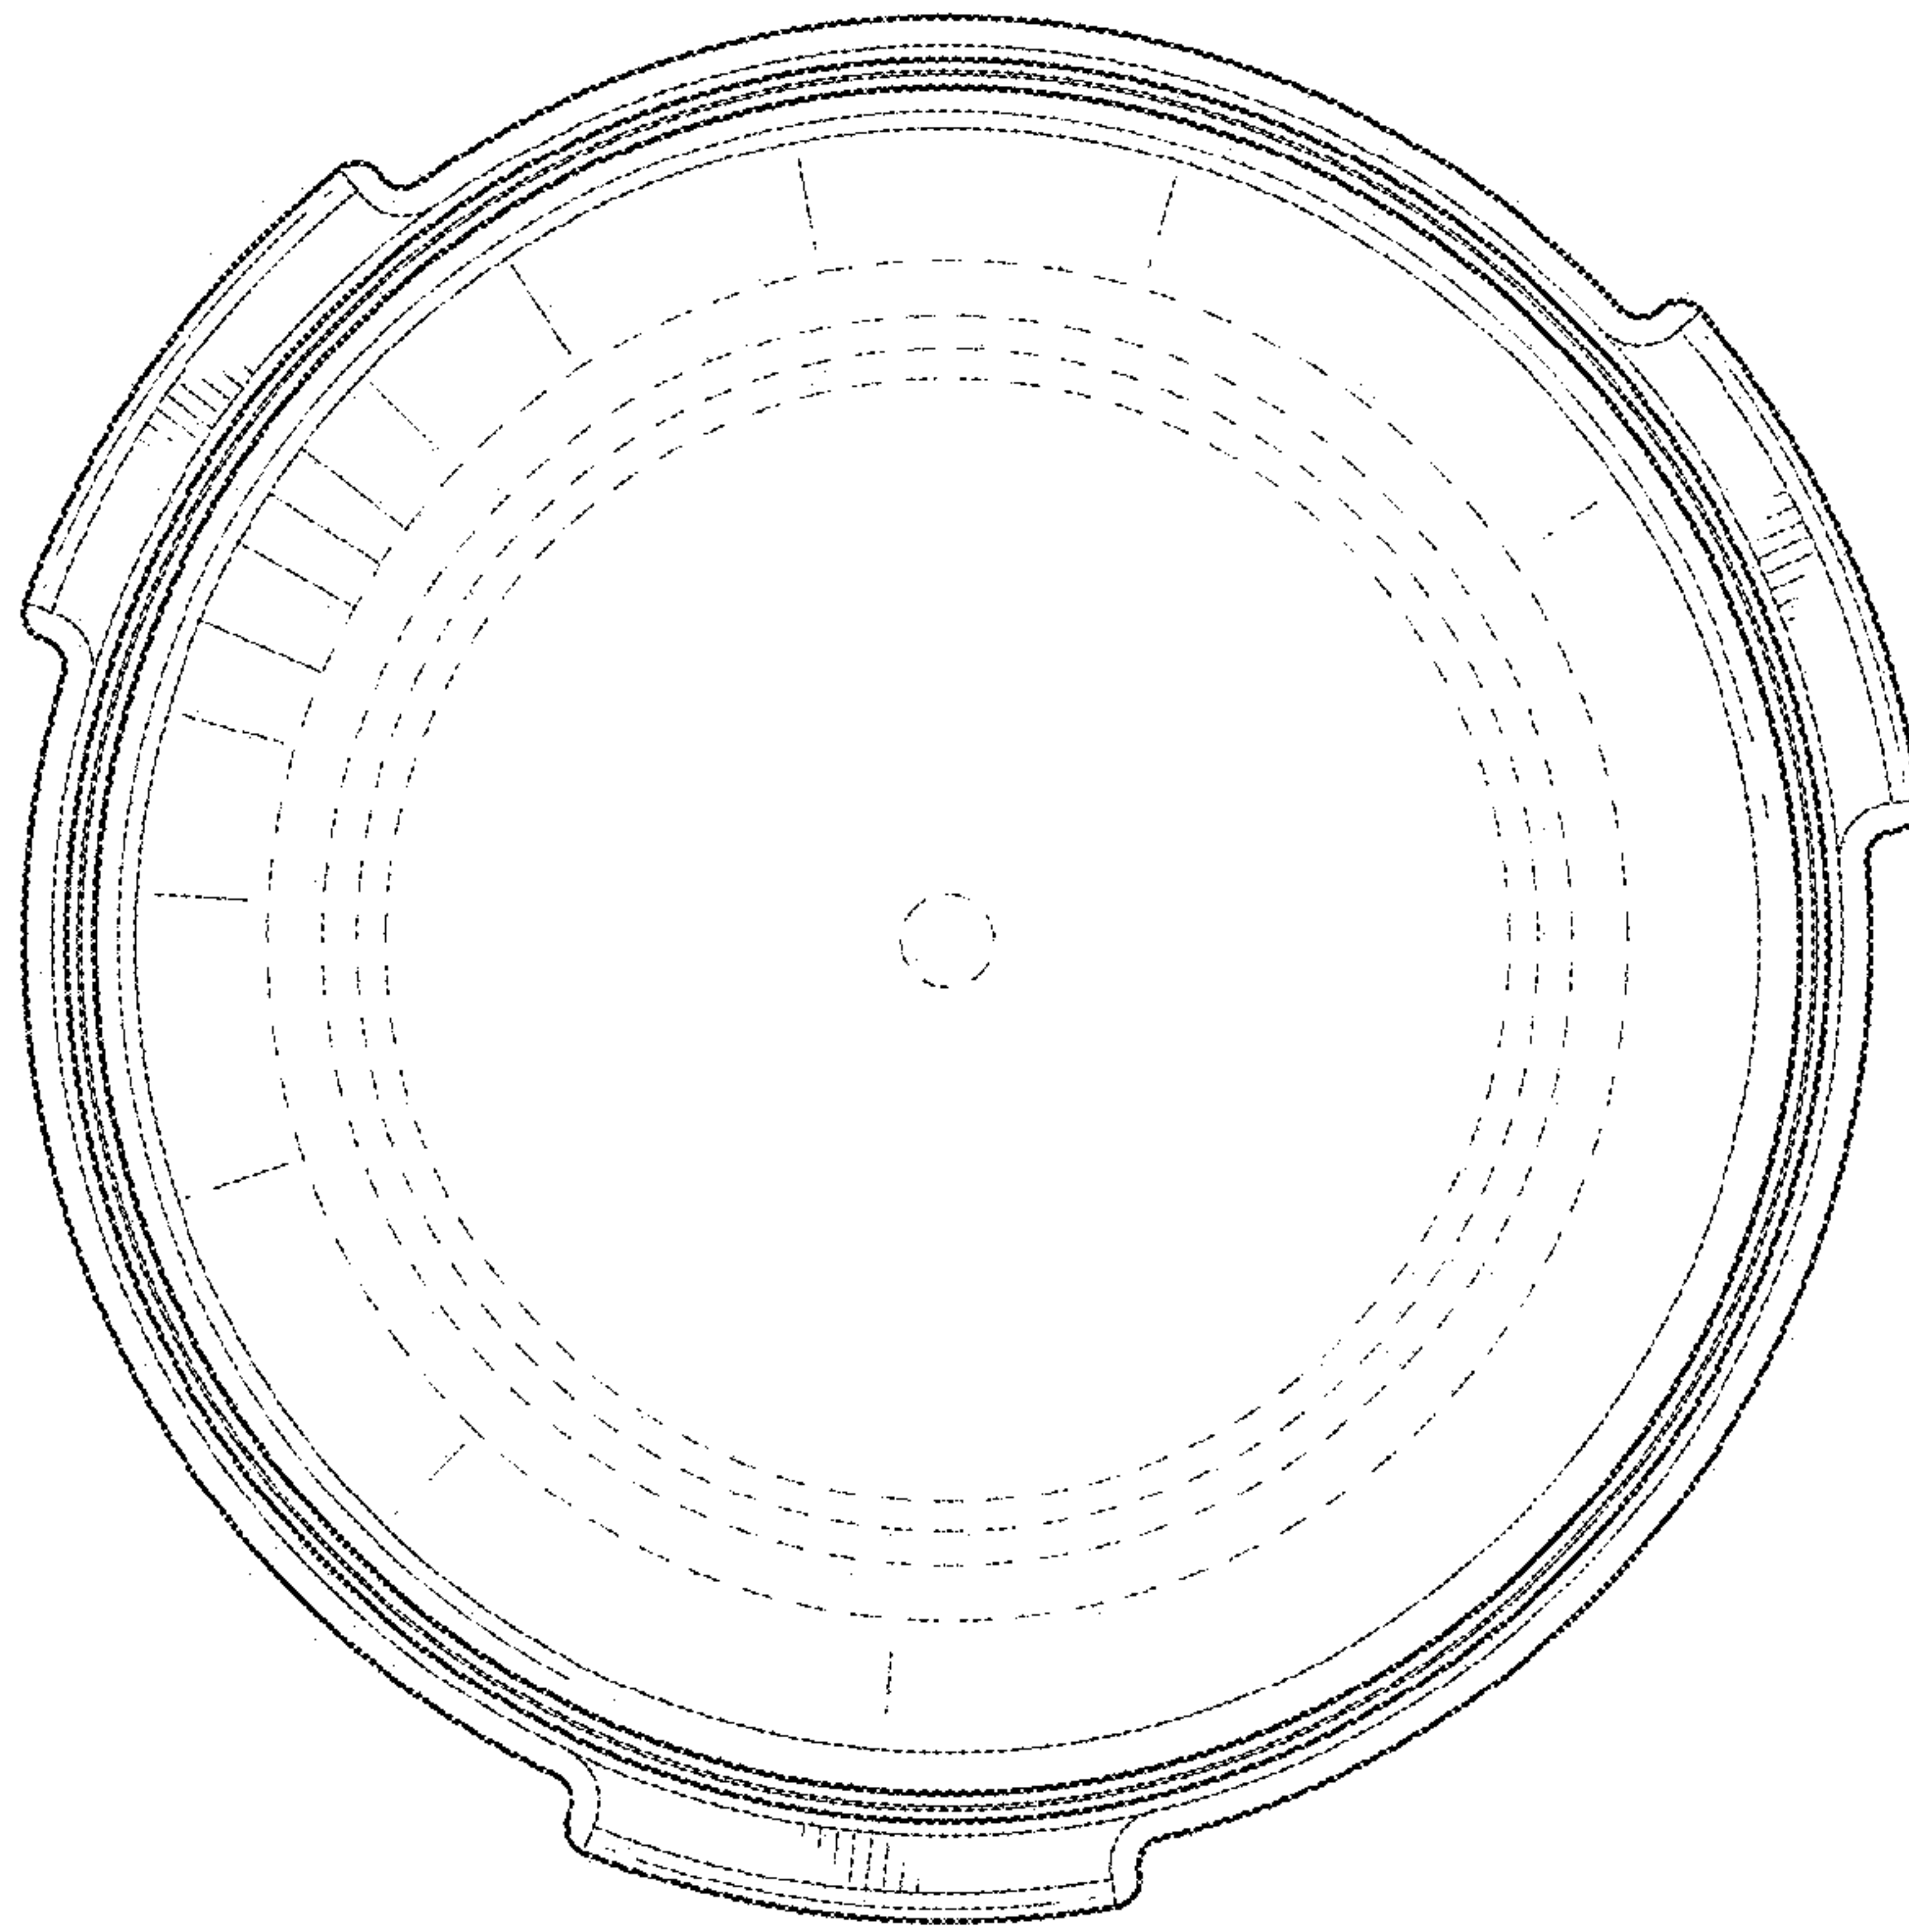


FIG. 3

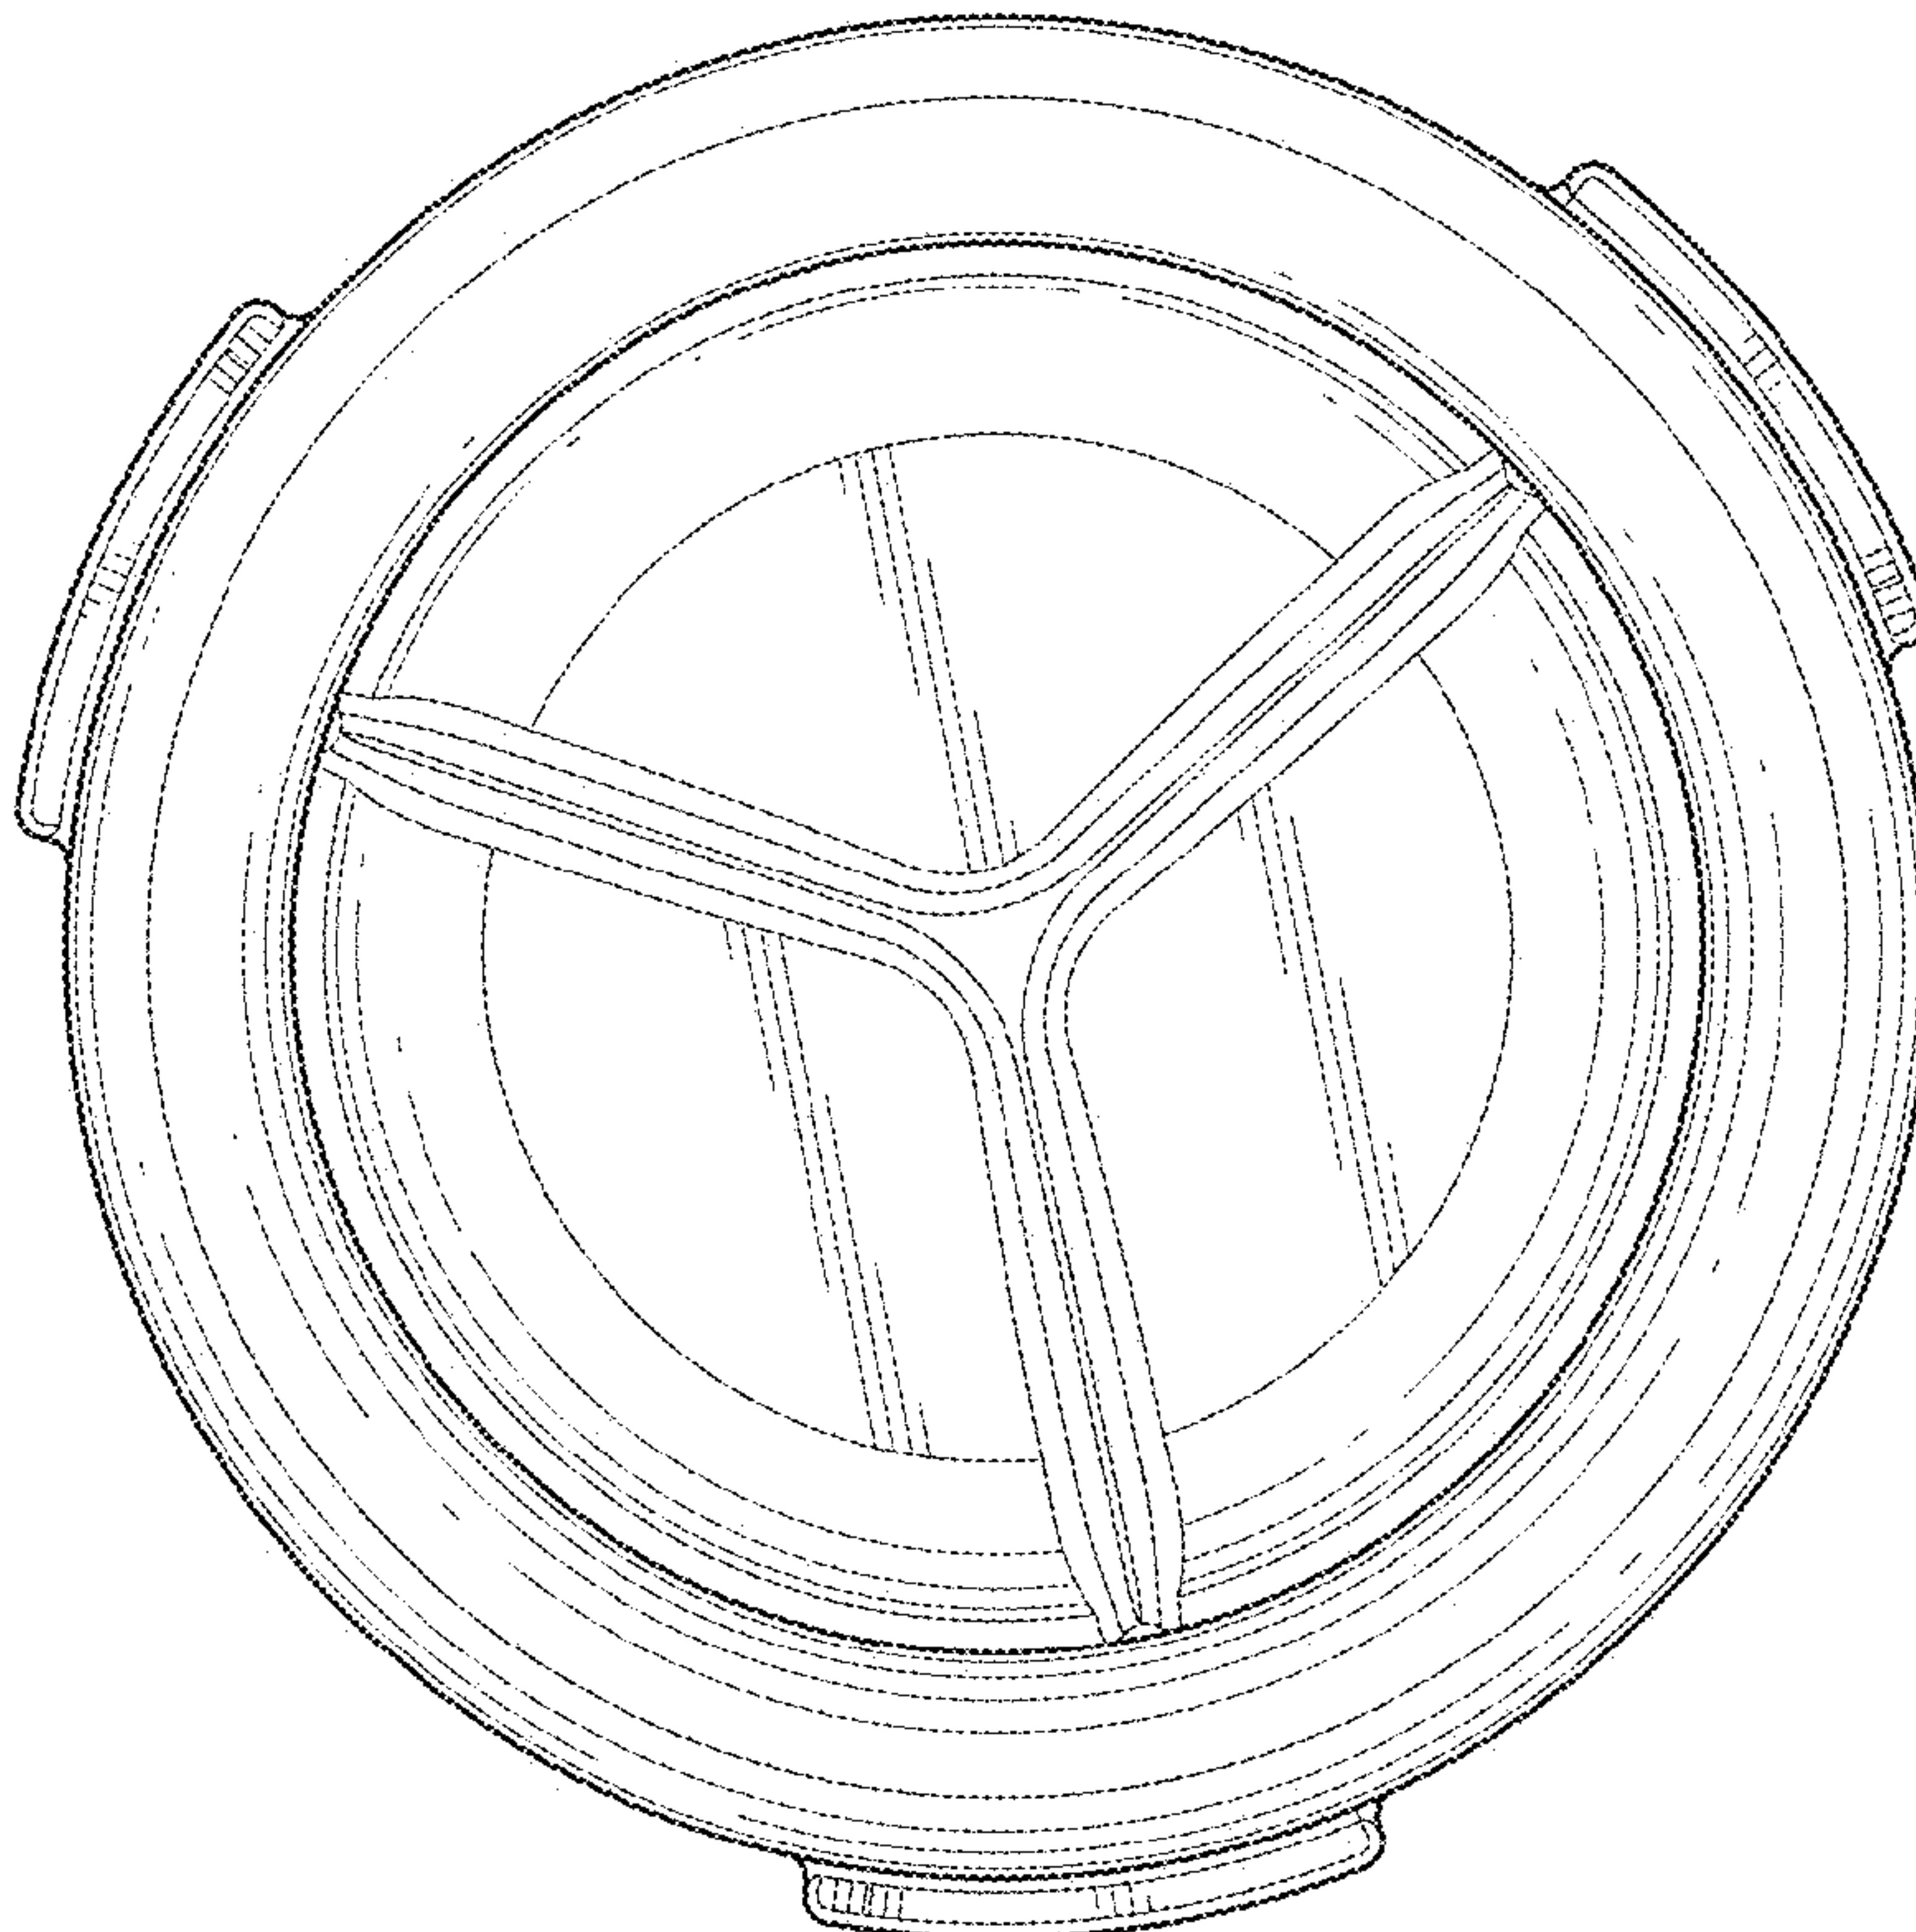


FIG. 4

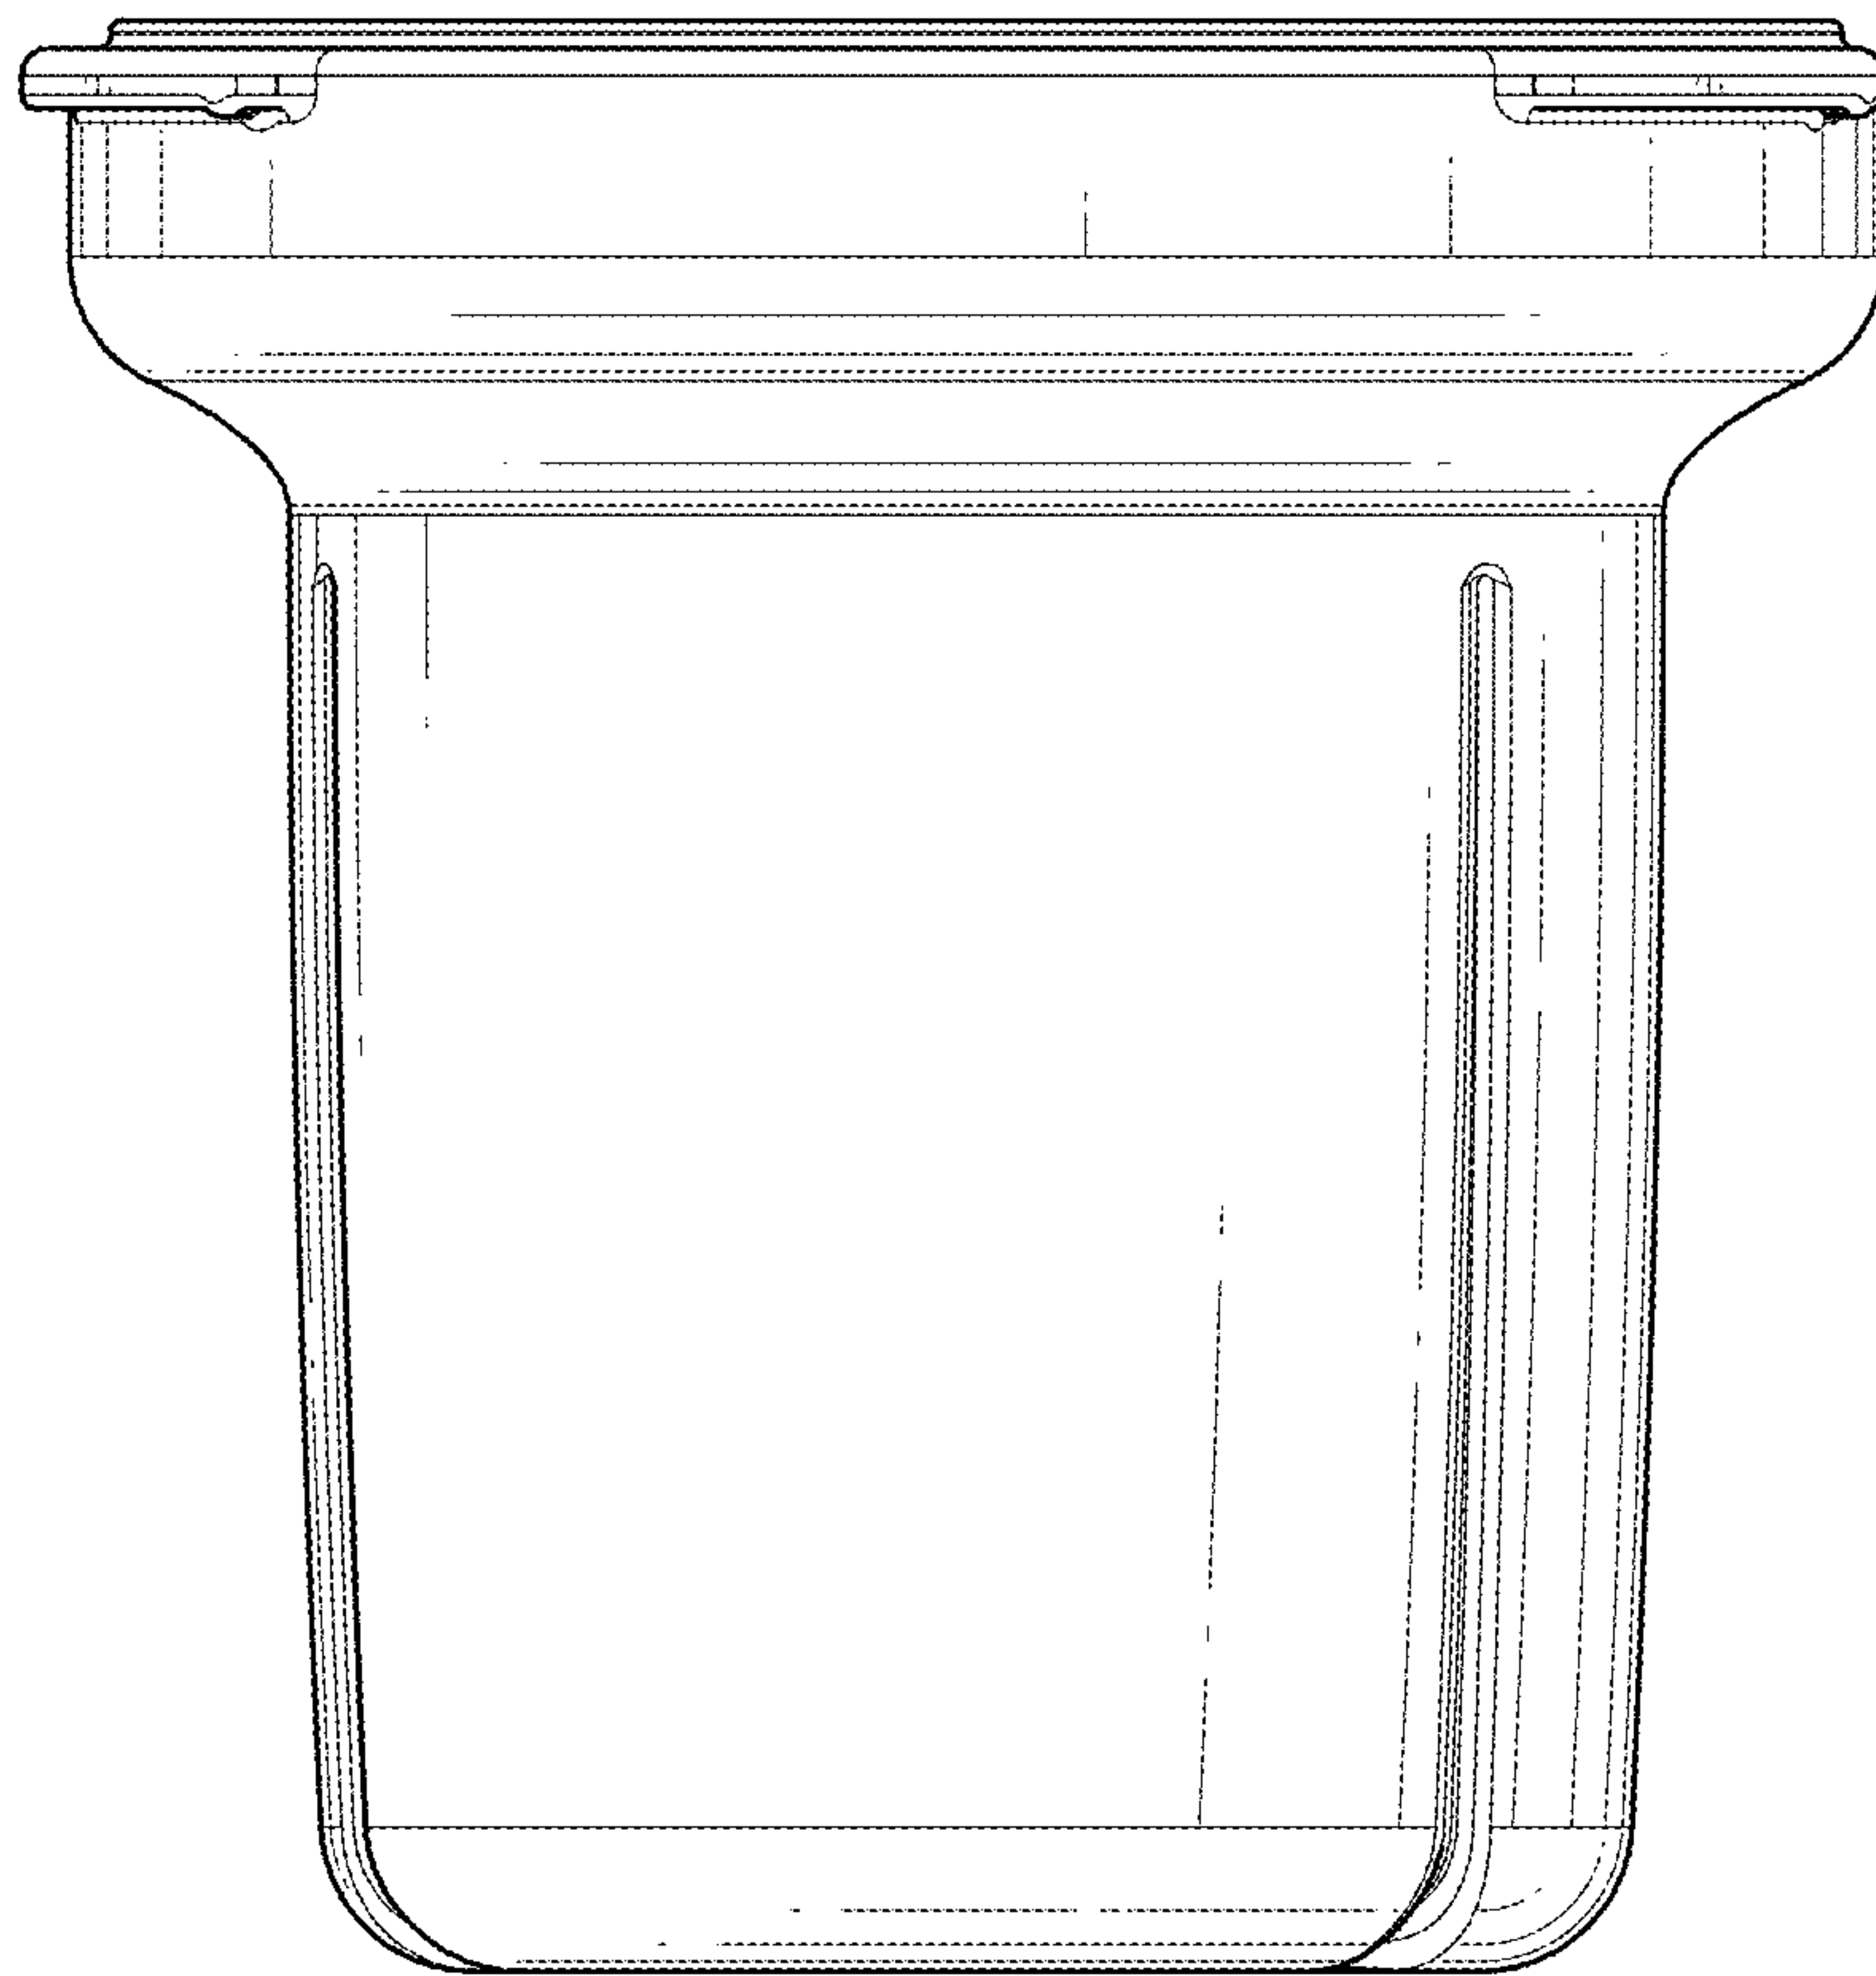


FIG. 5

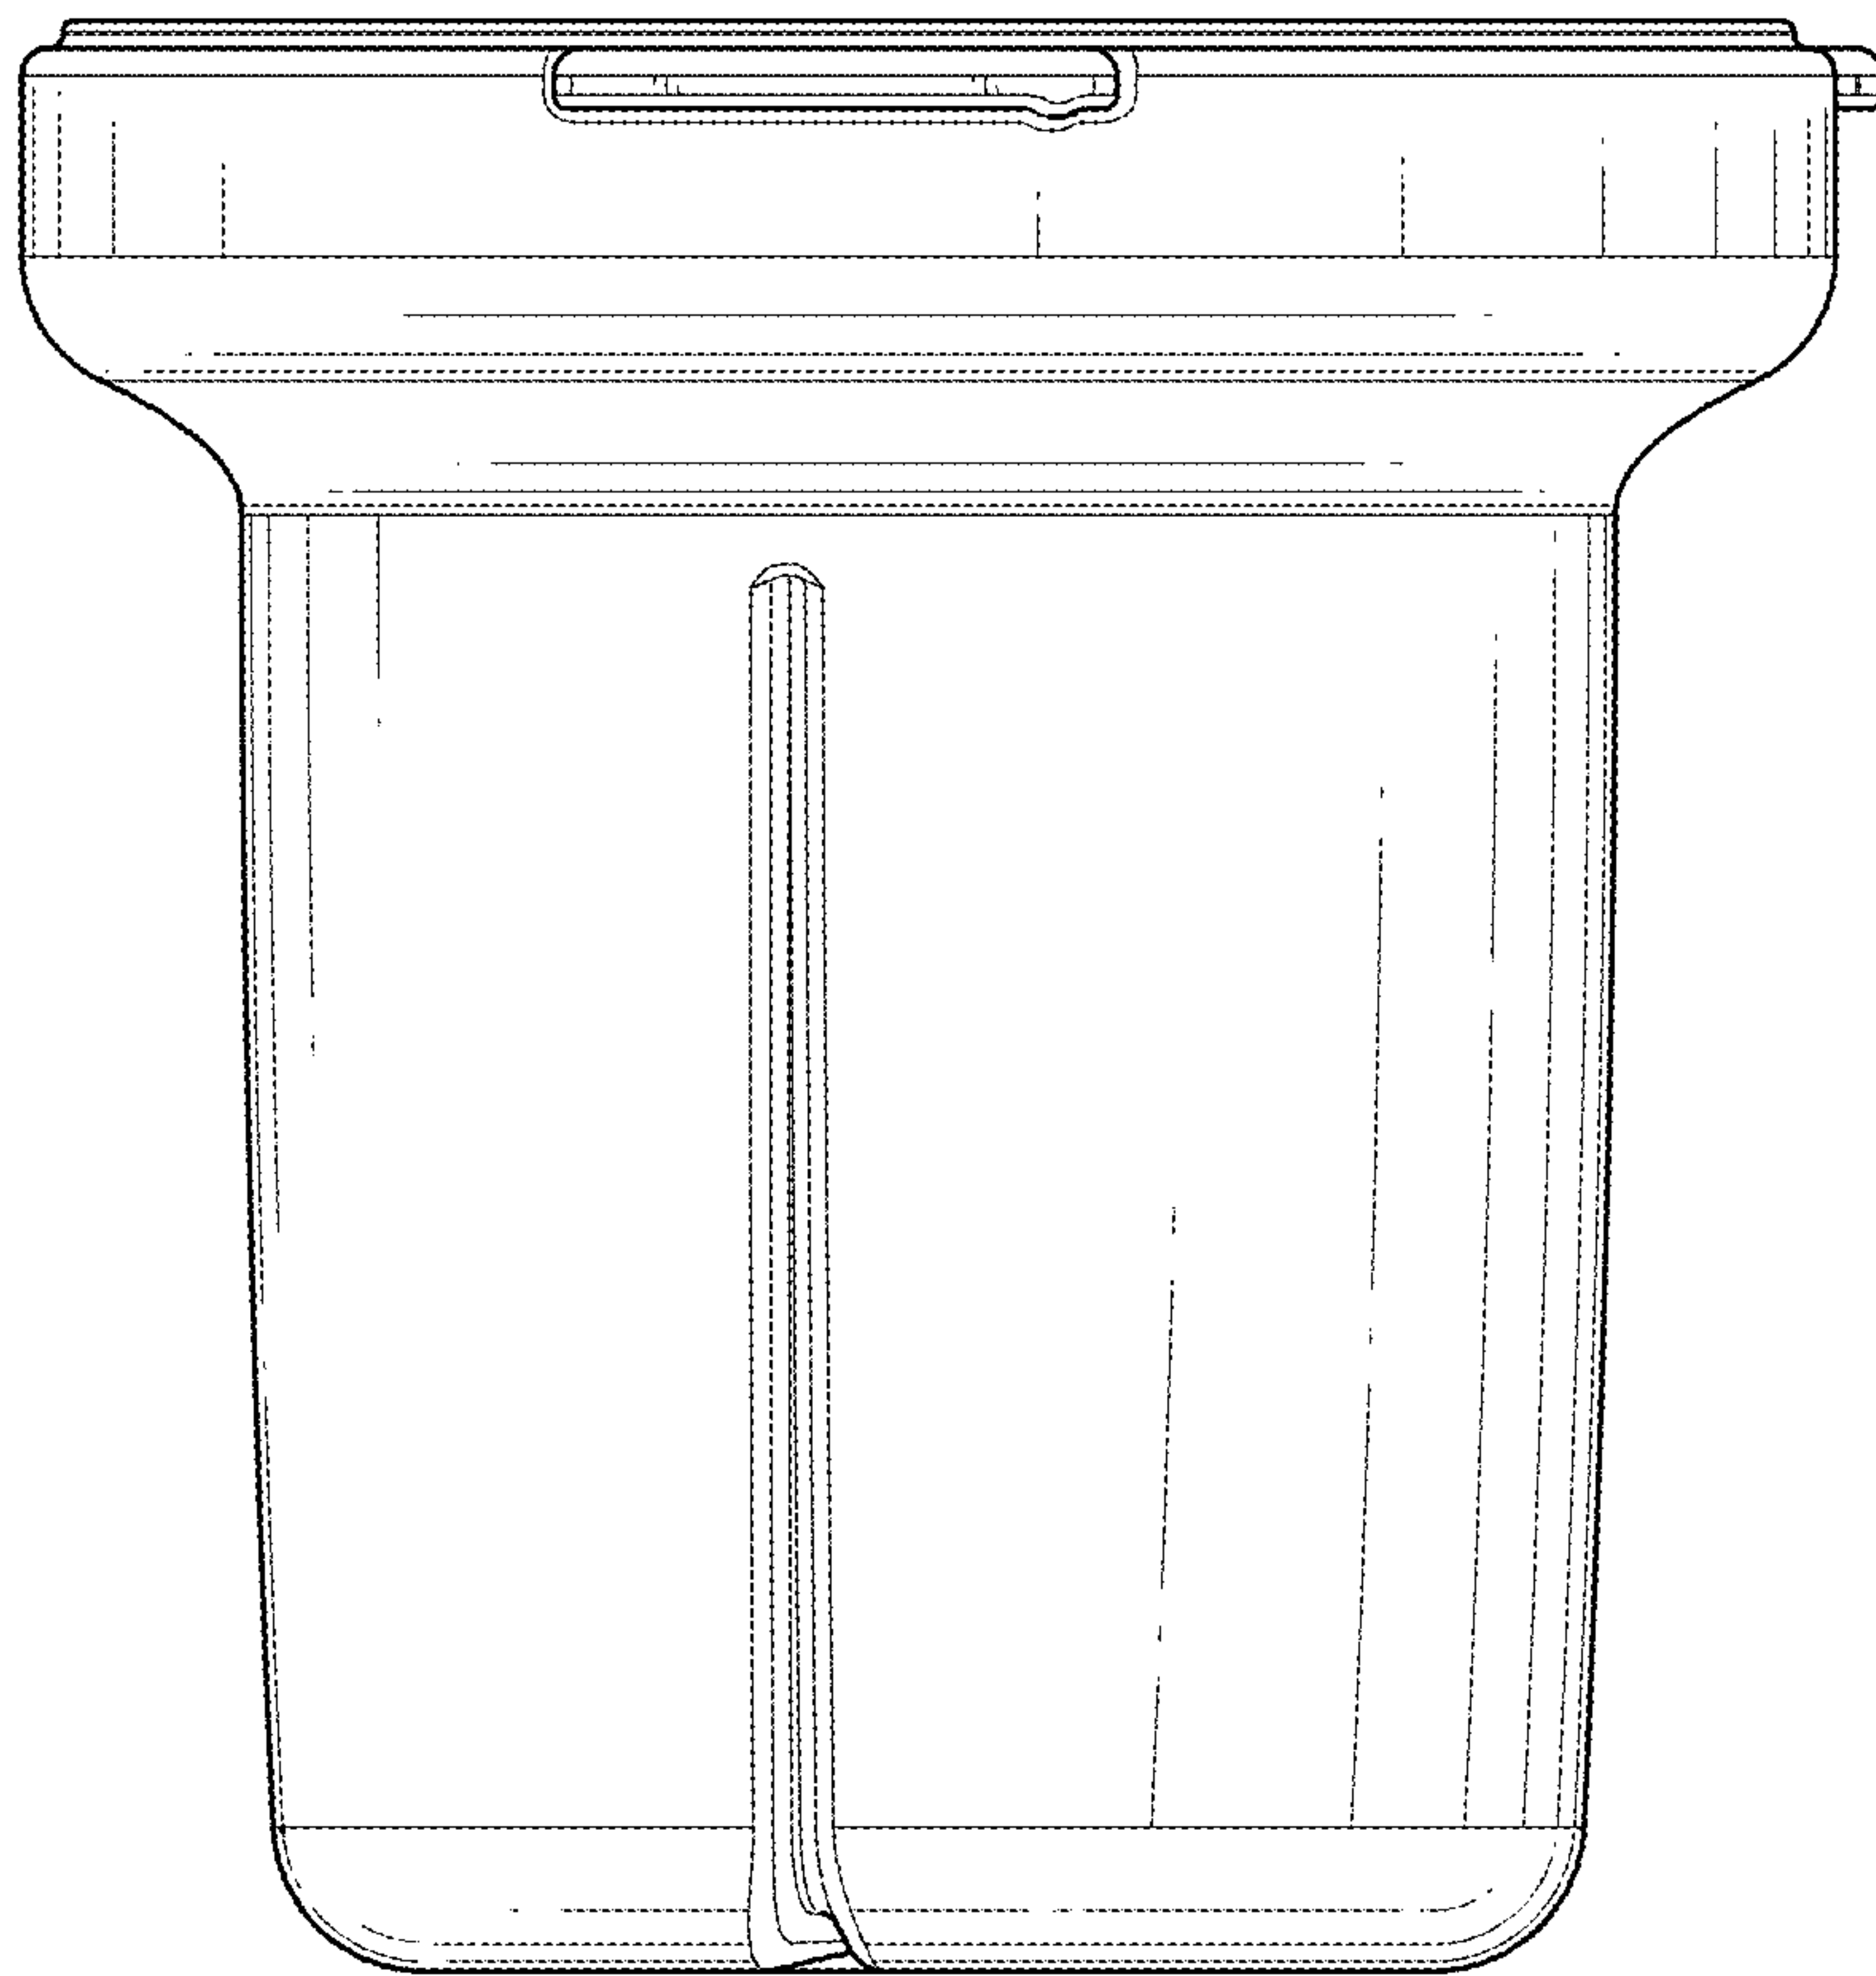


FIG. 6

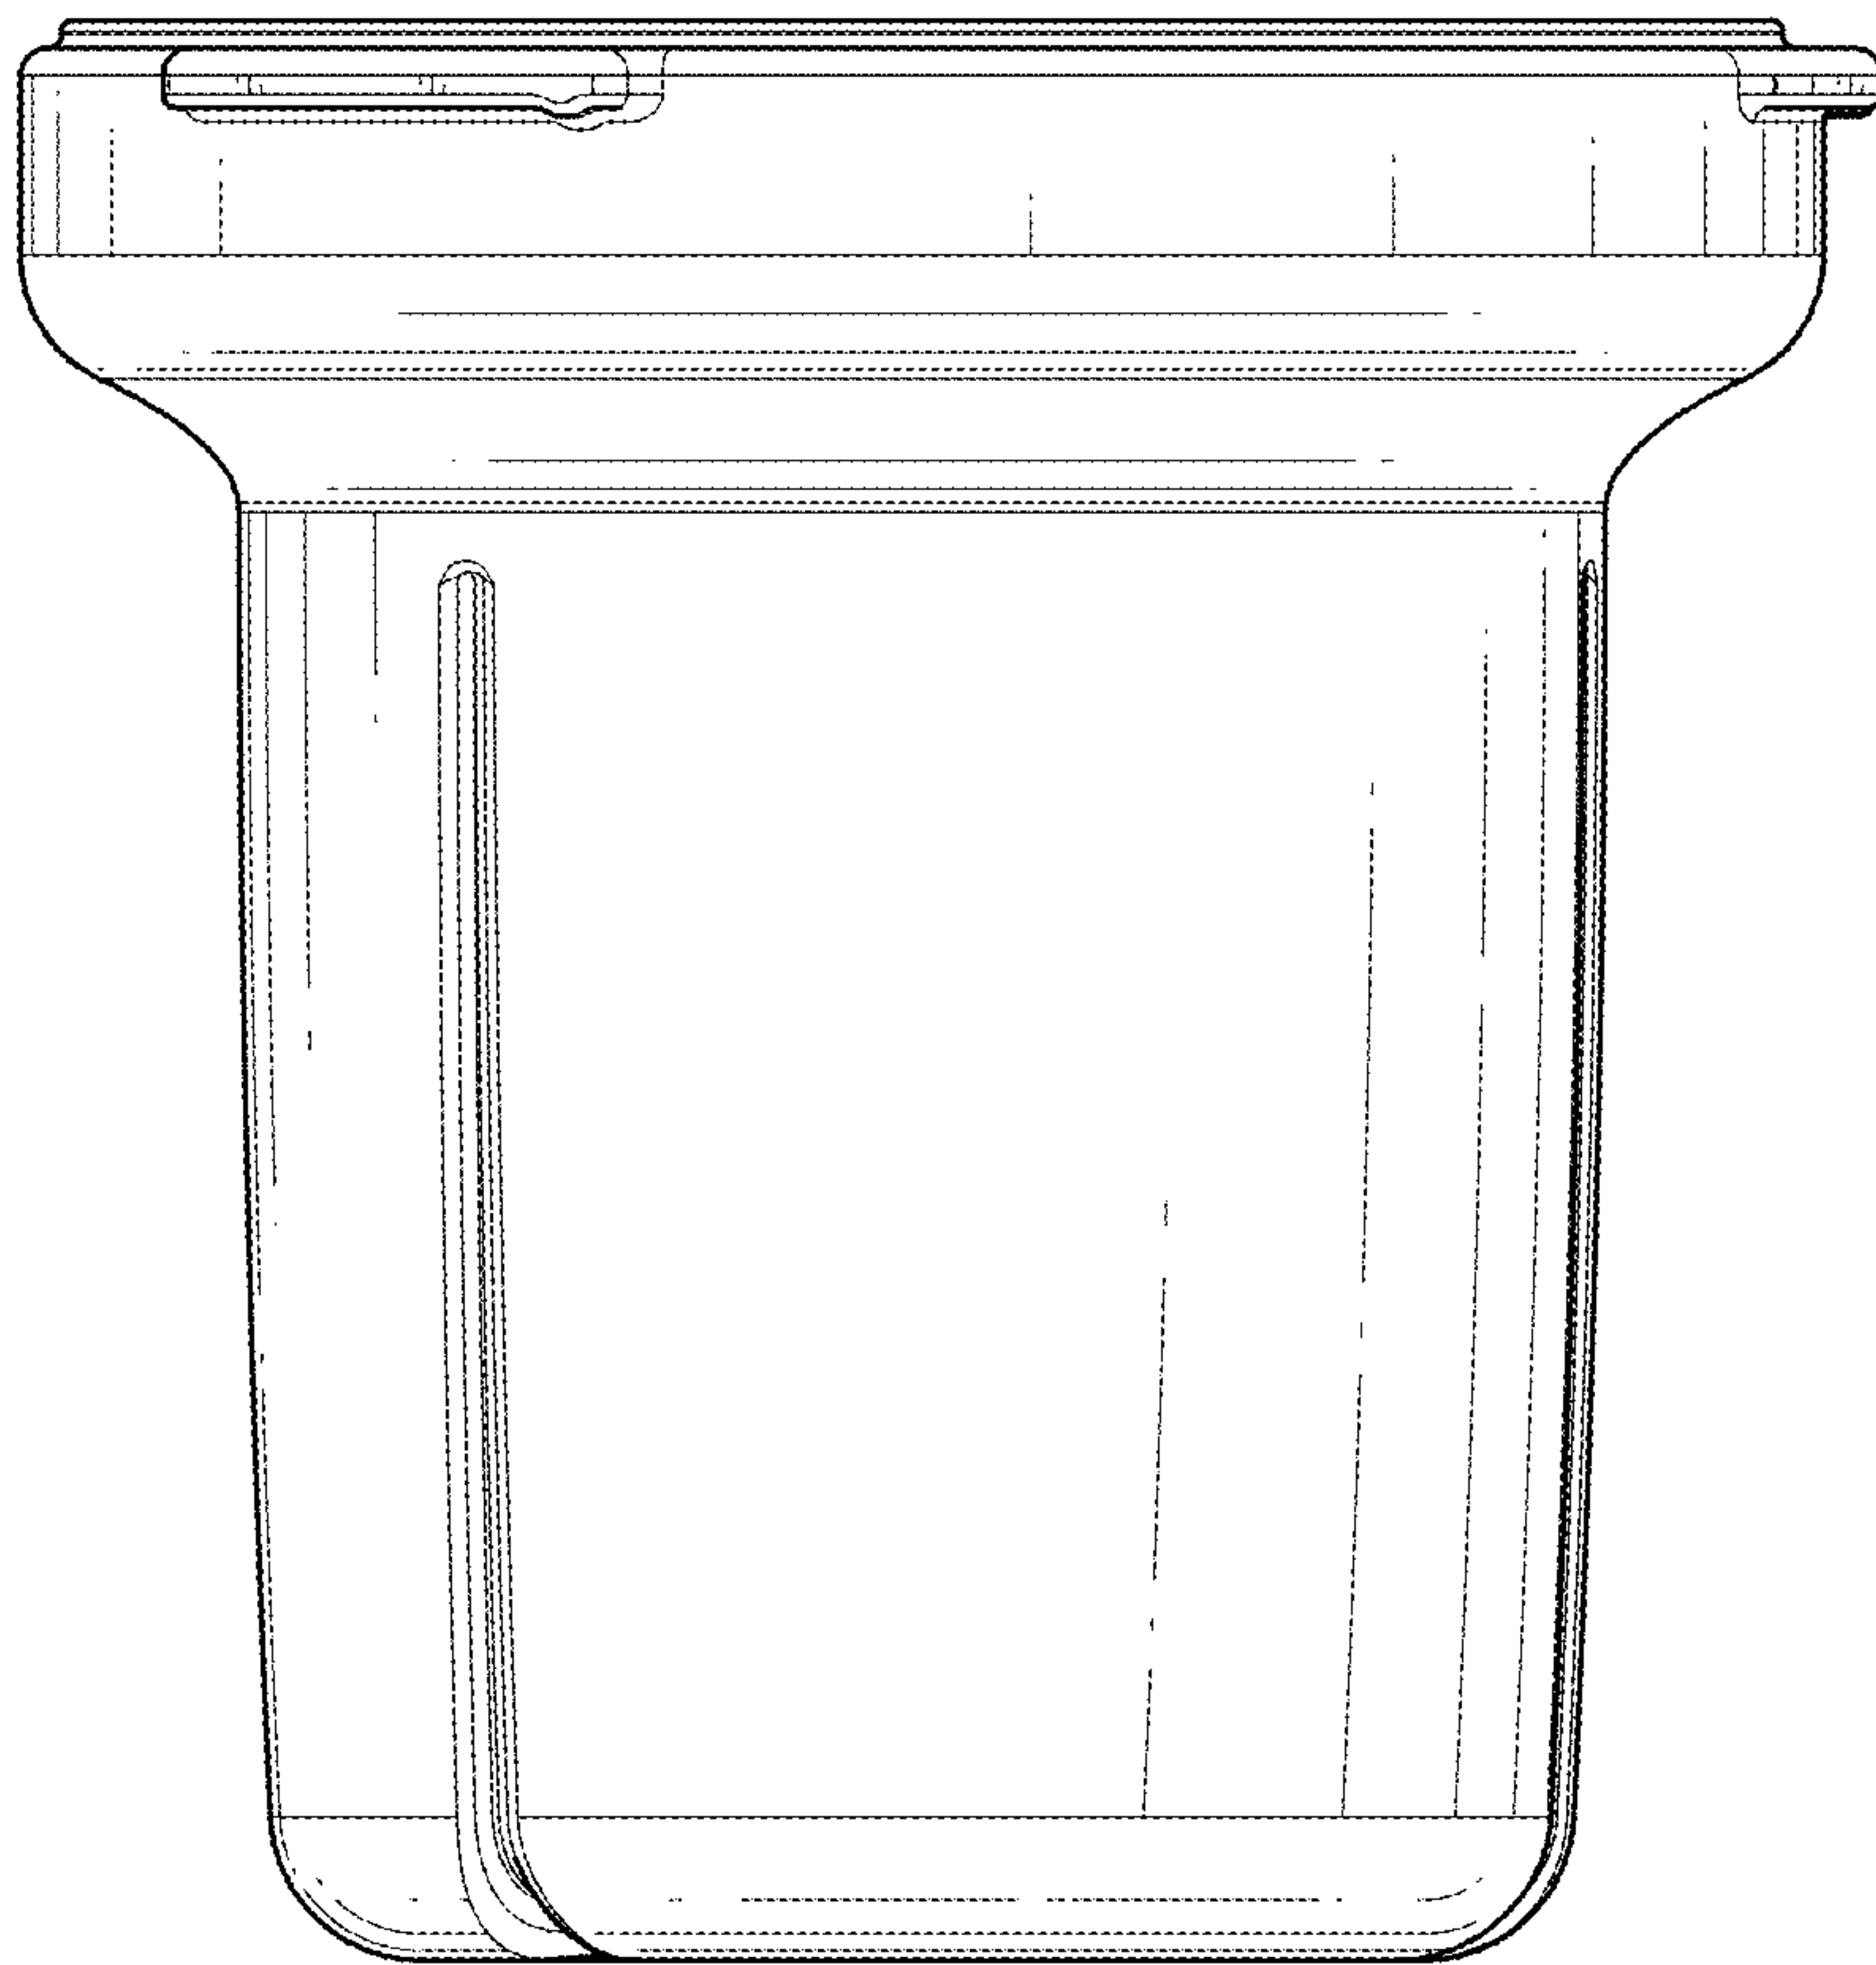


FIG. 7

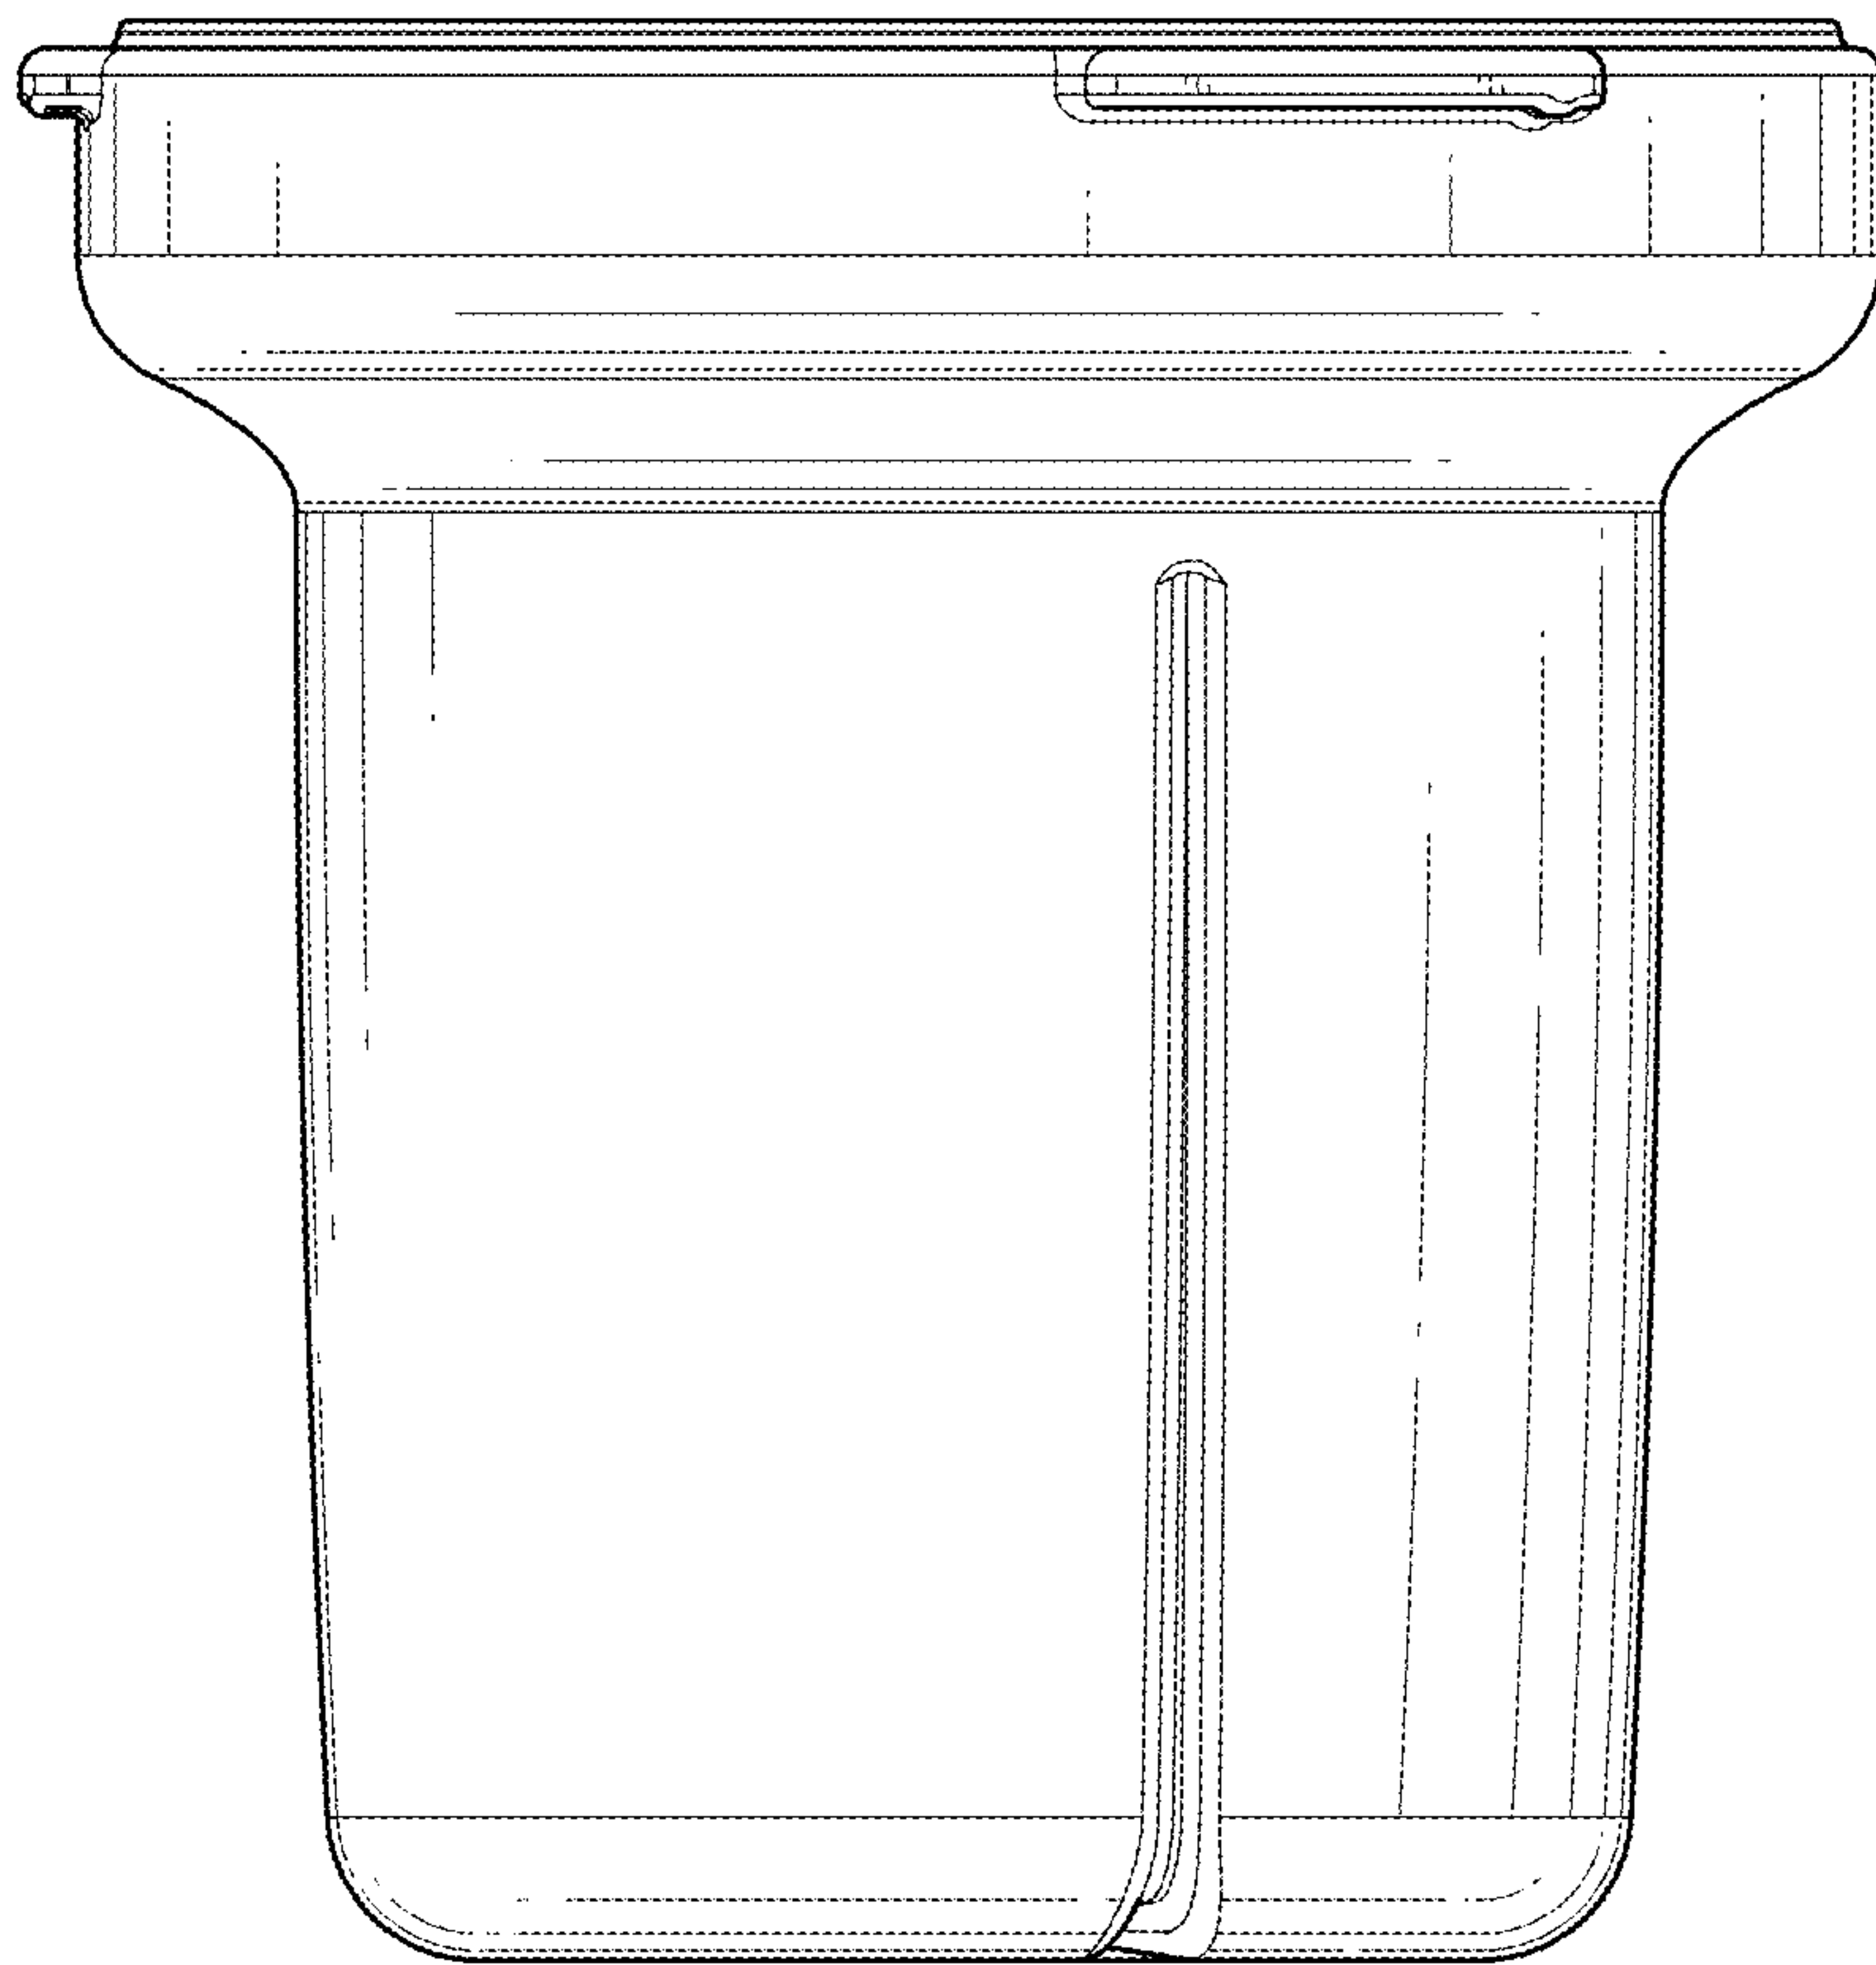


FIG. 8