



US0D1039687S

(12)

United States Design Patent

Nelsen et al.

(10) Patent No.: US D1,039,687 S

(45) Date of Patent: \*\* Aug. 20, 2024

(54) OCULAR IMPLANT DELIVERY DEVICE

(71) Applicant: Iantrek, Inc., Harrison, NY (US)

(72) Inventors: Daniel Nelsen, Central Falls, RI (US);  
Jonathan O’Keefe, Harrison, NY (US)

(73) Assignee: Iantrek, Inc., Harrison, NY (US)

(\*\*) Term: 15 Years

(21) Appl. No.: 29/816,809

(22) Filed: Nov. 24, 2021

(51) LOC (14) Cl. 24-02

(52) U.S. Cl.  
USPC D24/133

(58) Field of Classification Search  
USPC D24/127, 130, 133, 146, 147, 200, 214,  
D24/157, 144, 150; D8/2, 14, 14.1, 29.1,  
D8/29.2, 30, 61, 68, 93, 97, 300, 310,  
D8/311, 313; D19/110, 115; D7/649;  
D23/223, 226, 229  
CPC B26B 3/00; B26B 1/10; A61B 17/1617;  
A61B 17/3417; A61B 17/1624; A61B  
17/162; A61B 17/1622; A61B  
2017/00424; A61B 5/1411; A61B  
2090/062; A61B 17/3468; A61B  
2090/034; B05C 17/103; B05C 17/116;  
B05C 17/01; A61L 27/3645; A61L  
2430/16; A61F 9/00781  
See application file for complete search history.

(56) References Cited

U.S. PATENT DOCUMENTS

D289,198 S 4/1987 Karten  
5,484,434 A \* 1/1996 Cartmell A61B 18/1402  
606/45  
D378,939 S \* 4/1997 Smith D24/112  
D402,029 S 12/1998 Shinabarger

D493,530 S \* 7/2004 Reschke D24/144  
D592,746 S \* 5/2009 Highley D24/133  
D634,843 S \* 3/2011 Kim D24/140  
(Continued)

FOREIGN PATENT DOCUMENTS

GB 6219963 7/2022  
JP D1739057 3/2023

OTHER PUBLICATIONS

Microinvasive Glaucoma Surgery with the OMNI Surgical System,  
[online]. eyewire.news, Nov. 17, 2021 [retrieved on May 30, 2023].  
Retrieved from the Internet: <URL: https://eyewire.news/news/  
microinvasive-glaucoma-surgery-with-the-omni-surgical-system-is-  
associated-with-diminished-diurnal-iop-fluctuations> (Year: 2021).\*  
(Continued)

Primary Examiner — Samantha Q Lawrence  
Assistant Examiner — Thanh Luu Wong  
(74) Attorney, Agent, or Firm — Mintz Levin Cohn Ferris  
Glovsky and Popeo, P.C.


(57) CLAIM

The ornamental design for an ocular implant delivery device, as shown and described.

DESCRIPTION

FIG. 1 is a top, front, and right side perspective view of an ocular implant delivery device showing our design; FIG. 2 is a top, rear, and left side perspective view thereof; FIG. 3 is a front view thereof; FIG. 4 is a rear view thereof; FIG. 5 is a left side view thereof; FIG. 6 is a right side view thereof; FIG. 7 is a top view thereof; FIG. 8 is a bottom view thereof; and, FIG. 9 is an enlarged view of segment 9 shown in FIG. 1. The broken line areas illustrate portions of the ocular implant delivery device that form no part of the claimed design.

1 Claim, 8 Drawing Sheets

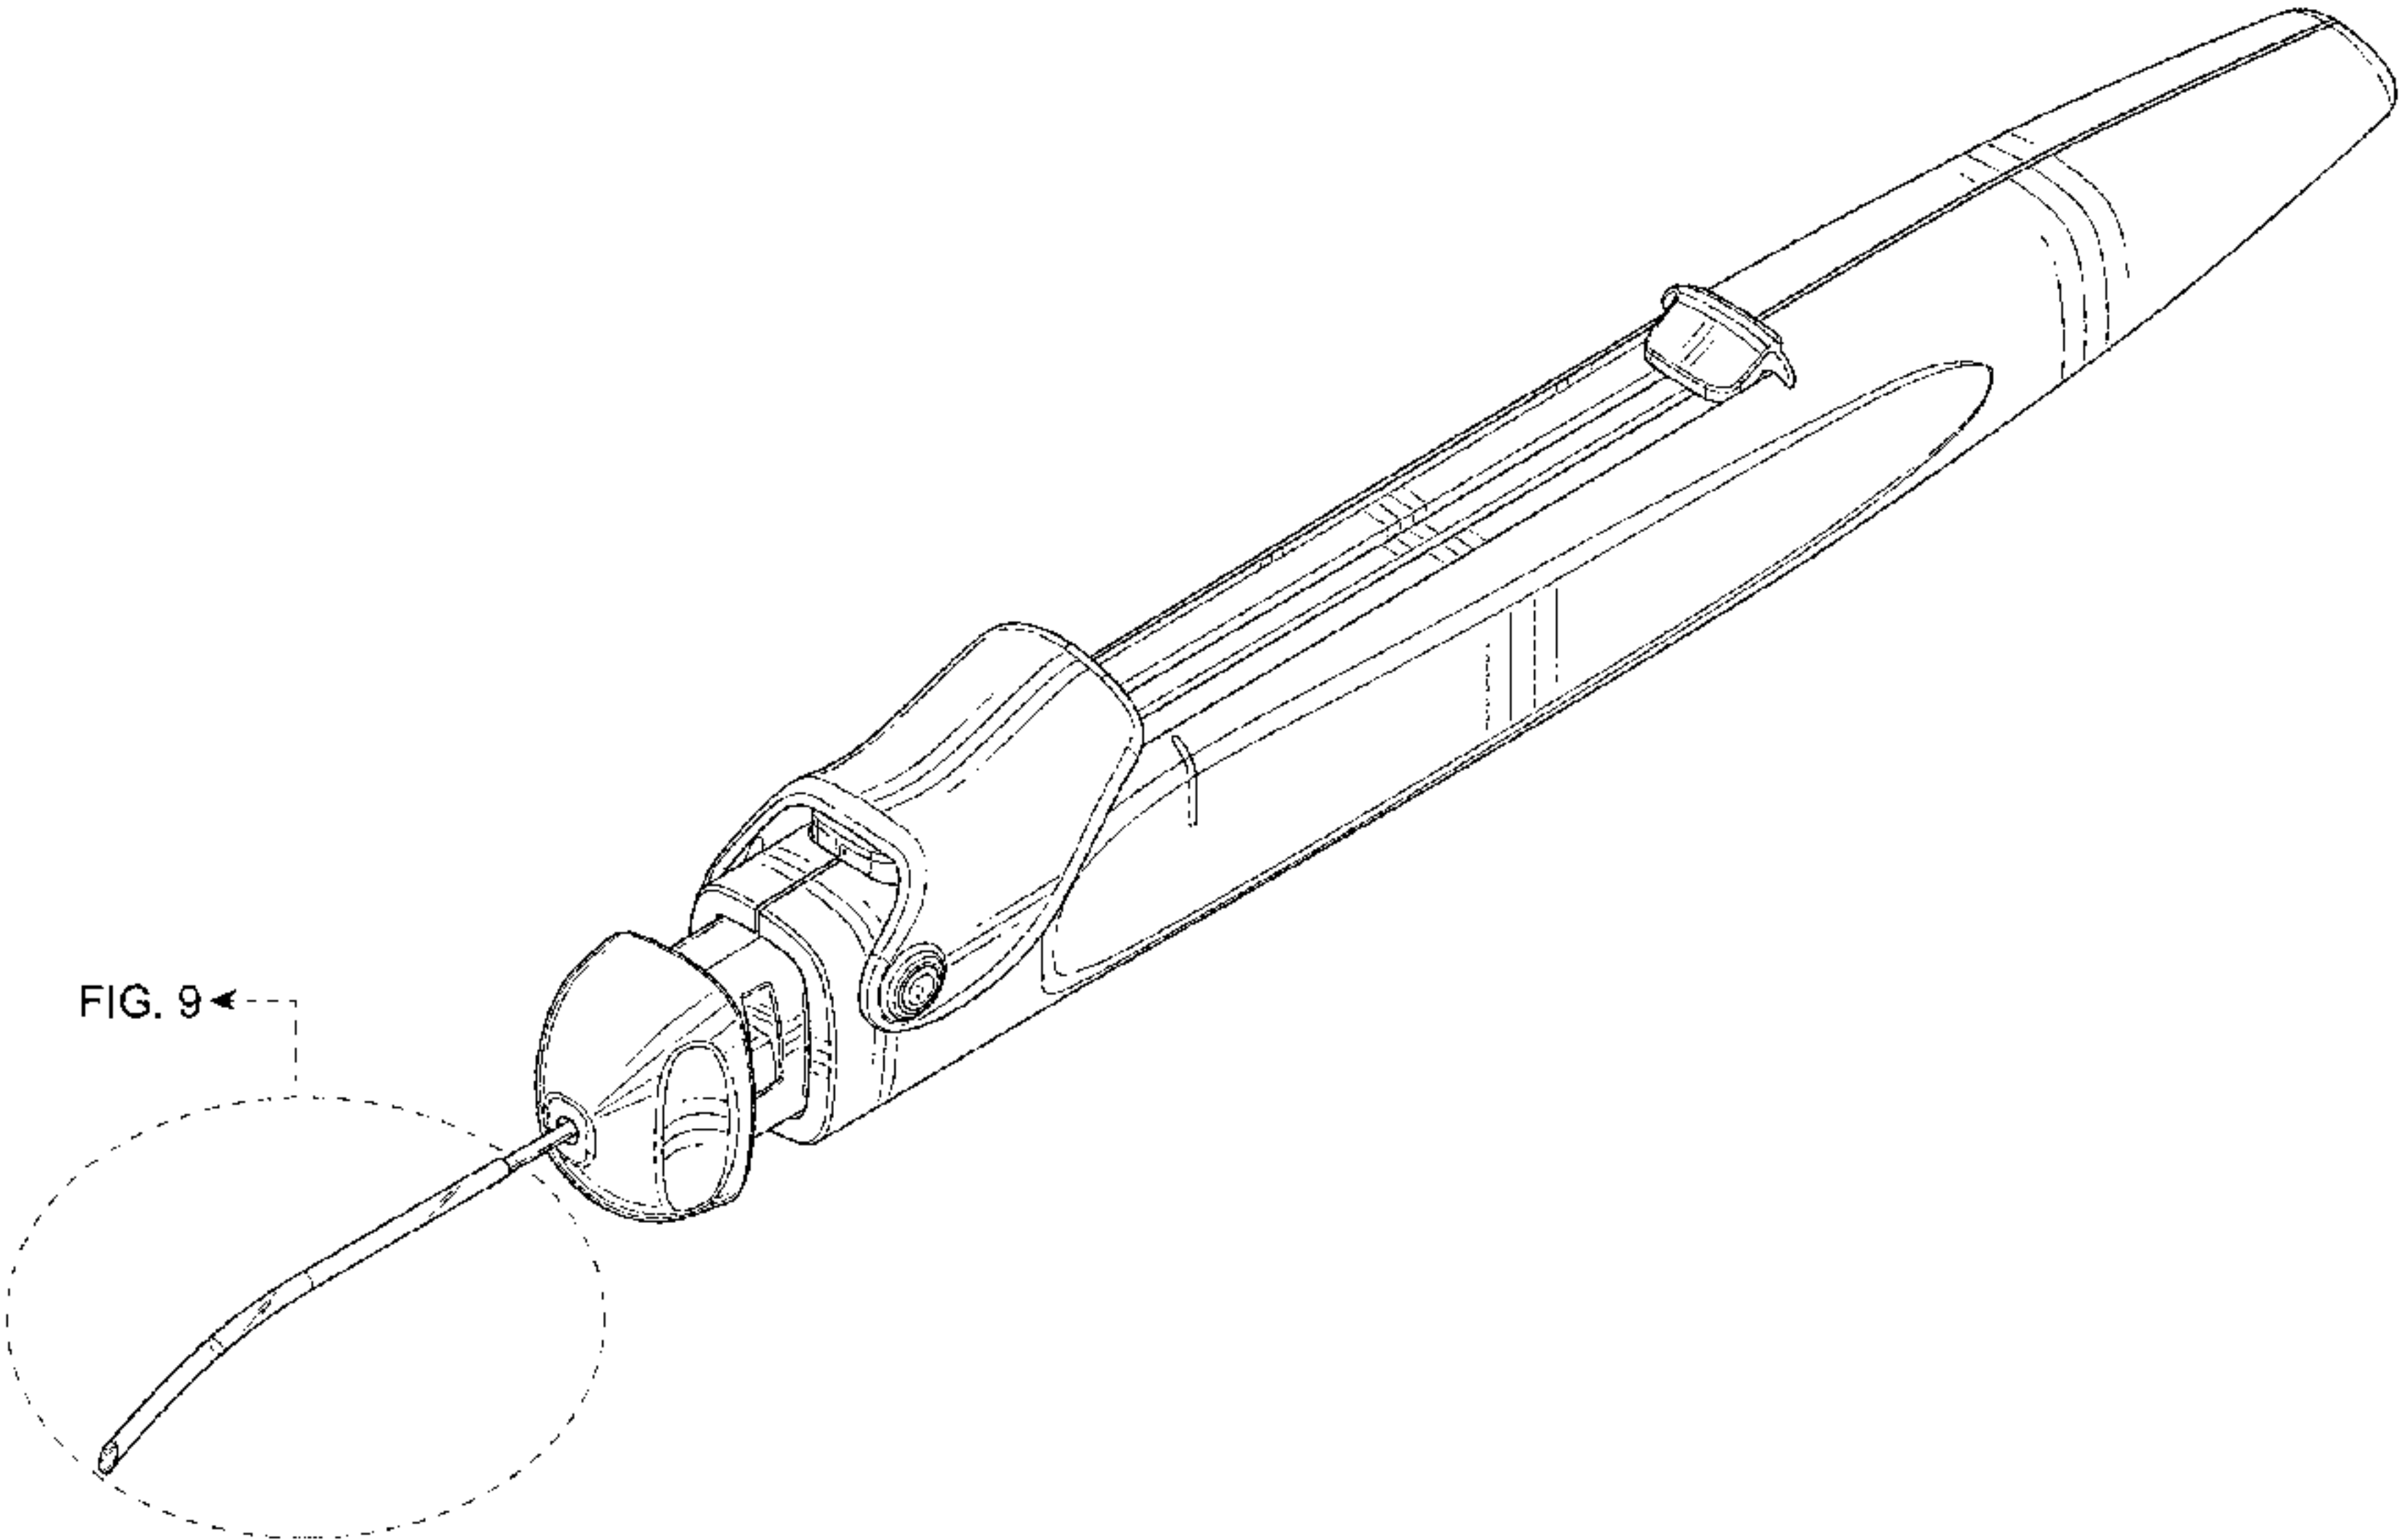

(56)

References Cited

U.S. PATENT DOCUMENTS

D654,586 S 2/2012 Hogerwerf et al.  
D672,040 S 12/2012 Delahoussaye et al.  
D708,327 S 7/2014 Wang et al.  
D708,737 S 7/2014 Sherman et al.  
8,790,293 B2 7/2014 Nazzaro et al.  
D710,495 S 8/2014 Wu et al.  
8,968,236 B2 3/2015 Jennings et al.  
9,155,656 B2 \* 10/2015 Schaller ..... A61F 9/00781  
9,173,775 B2 \* 11/2015 Haffner ..... A61F 9/0017  
D765,841 S \* 9/2016 Schuerg ..... D24/144  
D806,230 S \* 12/2017 Johnson ..... D24/112  
D851,755 S 6/2019 Nazzaro et al.  
D858,751 S 9/2019 Fischman  
10,543,122 B2 \* 1/2020 Kahook ..... A61F 9/0017  
10,780,218 B2 \* 9/2020 Novakovic ..... A61F 9/0017  
10,932,951 B2 \* 3/2021 Schaller ..... A61F 9/013  
D917,048 S 4/2021 Moroney et al.  
10,987,247 B2 \* 4/2021 Moreno ..... A61B 3/0008  
11,116,949 B2 \* 9/2021 Lee ..... A61M 25/0102  
D949,342 S 4/2022 Tran et al.  
11,344,712 B2 \* 5/2022 Painchaud ..... A61F 2/0095  
D954,954 S 6/2022 Rynerson  
11,376,040 B2 \* 7/2022 Kalina, Jr. .... A61F 9/007  
11,426,572 B2 \* 8/2022 Painchaud ..... A61M 37/0069  
11,464,542 B2 \* 10/2022 Rosenthal ..... A61B 17/24  
11,504,169 B2 \* 11/2022 Hoos ..... A61B 17/58  
11,504,270 B1 \* 11/2022 Badawi ..... A61M 5/3286  
11,612,729 B2 \* 3/2023 Painchaud ..... A61M 5/322  
604/60  
D988,509 S 6/2023 Ko  
2004/0215126 A1 10/2004 Ahmed  
2008/0221510 A1 \* 9/2008 Van Der Graaf . A61M 37/0069  
604/60  
2011/0009874 A1 \* 1/2011 Wardle ..... A61F 9/0017  
606/108  
2011/0060242 A1 \* 3/2011 Hausman ..... A61B 17/8875  
600/554  
2015/0360019 A1 \* 12/2015 Clancy ..... A61M 37/0069  
600/432  
2019/0358846 A1 \* 11/2019 Tsai ..... B26F 3/08

2020/0390601 A1 12/2020 Ianchulev  
2021/0361484 A1 11/2021 Ianchulev  
2023/0000680 A1 \* 1/2023 Ianchulev ..... A61L 27/3645  
2023/0021859 A1 1/2023 Chapuis

OTHER PUBLICATIONS

New Approaches in Supraciliary Micro-Invasive Glaucoma Surgery, [online]. healthcare.utah.edu, Nov. 12, 2022 [retrieved on May 30, 2023]. Retrieved from the Internet: <URL: https://healthcare.utah.edu/moran/news/2022/11/new-approaches-supraciliary-micro-invasive-glaucoma-surgery-migs> (Year: 2022).\*

First-in-human data for next-generation biostent and new suprachoroidal MIGS, [online]. eyeworld.org, Mar. 2023 [retrieved on May 30, 2023]. Retrieved from the Internet: <URL: https://www.eyeworld.org/2023/first-in-human-data-for-biostent-migs-device/> (Year: 023).\*

ISent Inject for Glaucoma, asiapacificyecentre.com.sg, [online], [site visited May 30, 2023], Available from internet, URL: https://www.asiapacificyecentre.com.sg/istent-inject-for-glaucoma/ (Year: 2023).\*


Spinlock XTX Clutches, amazon.com, first available date Jan. 3, 2020 [online], [site visited May 30, 2023], Available from internet, URL: https://www.amazon.com/Spinlock-XTX-Clutches-Various-Colors/dp/B083G9HKK1 (Year: 2020).\*

Fiab Disposable Electrocautery Pens, lifelinemedical.net, [online], [site visited May 30, 2023], Available from internet, URL: https://www.lifelinemedical.net/product/electrocautery-disposable-cauterization-pens/ (Year: 2023).\*

Fraiser Kansteiner, Roche recalls new eye therapy Susvimo on leakage fears, aims for market return within a year or so-, [Post date: Oct. 18, 2022], [Site seen Jun. 28, 2023], URL:https://www.fiercepharma.com/manufacturing/ roche-recalls-susvimo-implant-lucentis-leakage-fears-return-market-expected-within (Year: 2022). 2 pages.

Okeke, C. (2016, online). “Shifting Gears in Glaucoma with Suprachoroidal Shunts,”. millenniaeye.com, Sep. 2016, [retrieved on Aug. 16, 2023]. Retrieved from the Internet: URL: https://millenniaeye.com/articles/2016-sept-oct/shifting-gears-in-glaucoma-with-suprachoroidal-shunts (Year: 2016). 3 pages.

\* cited by examiner

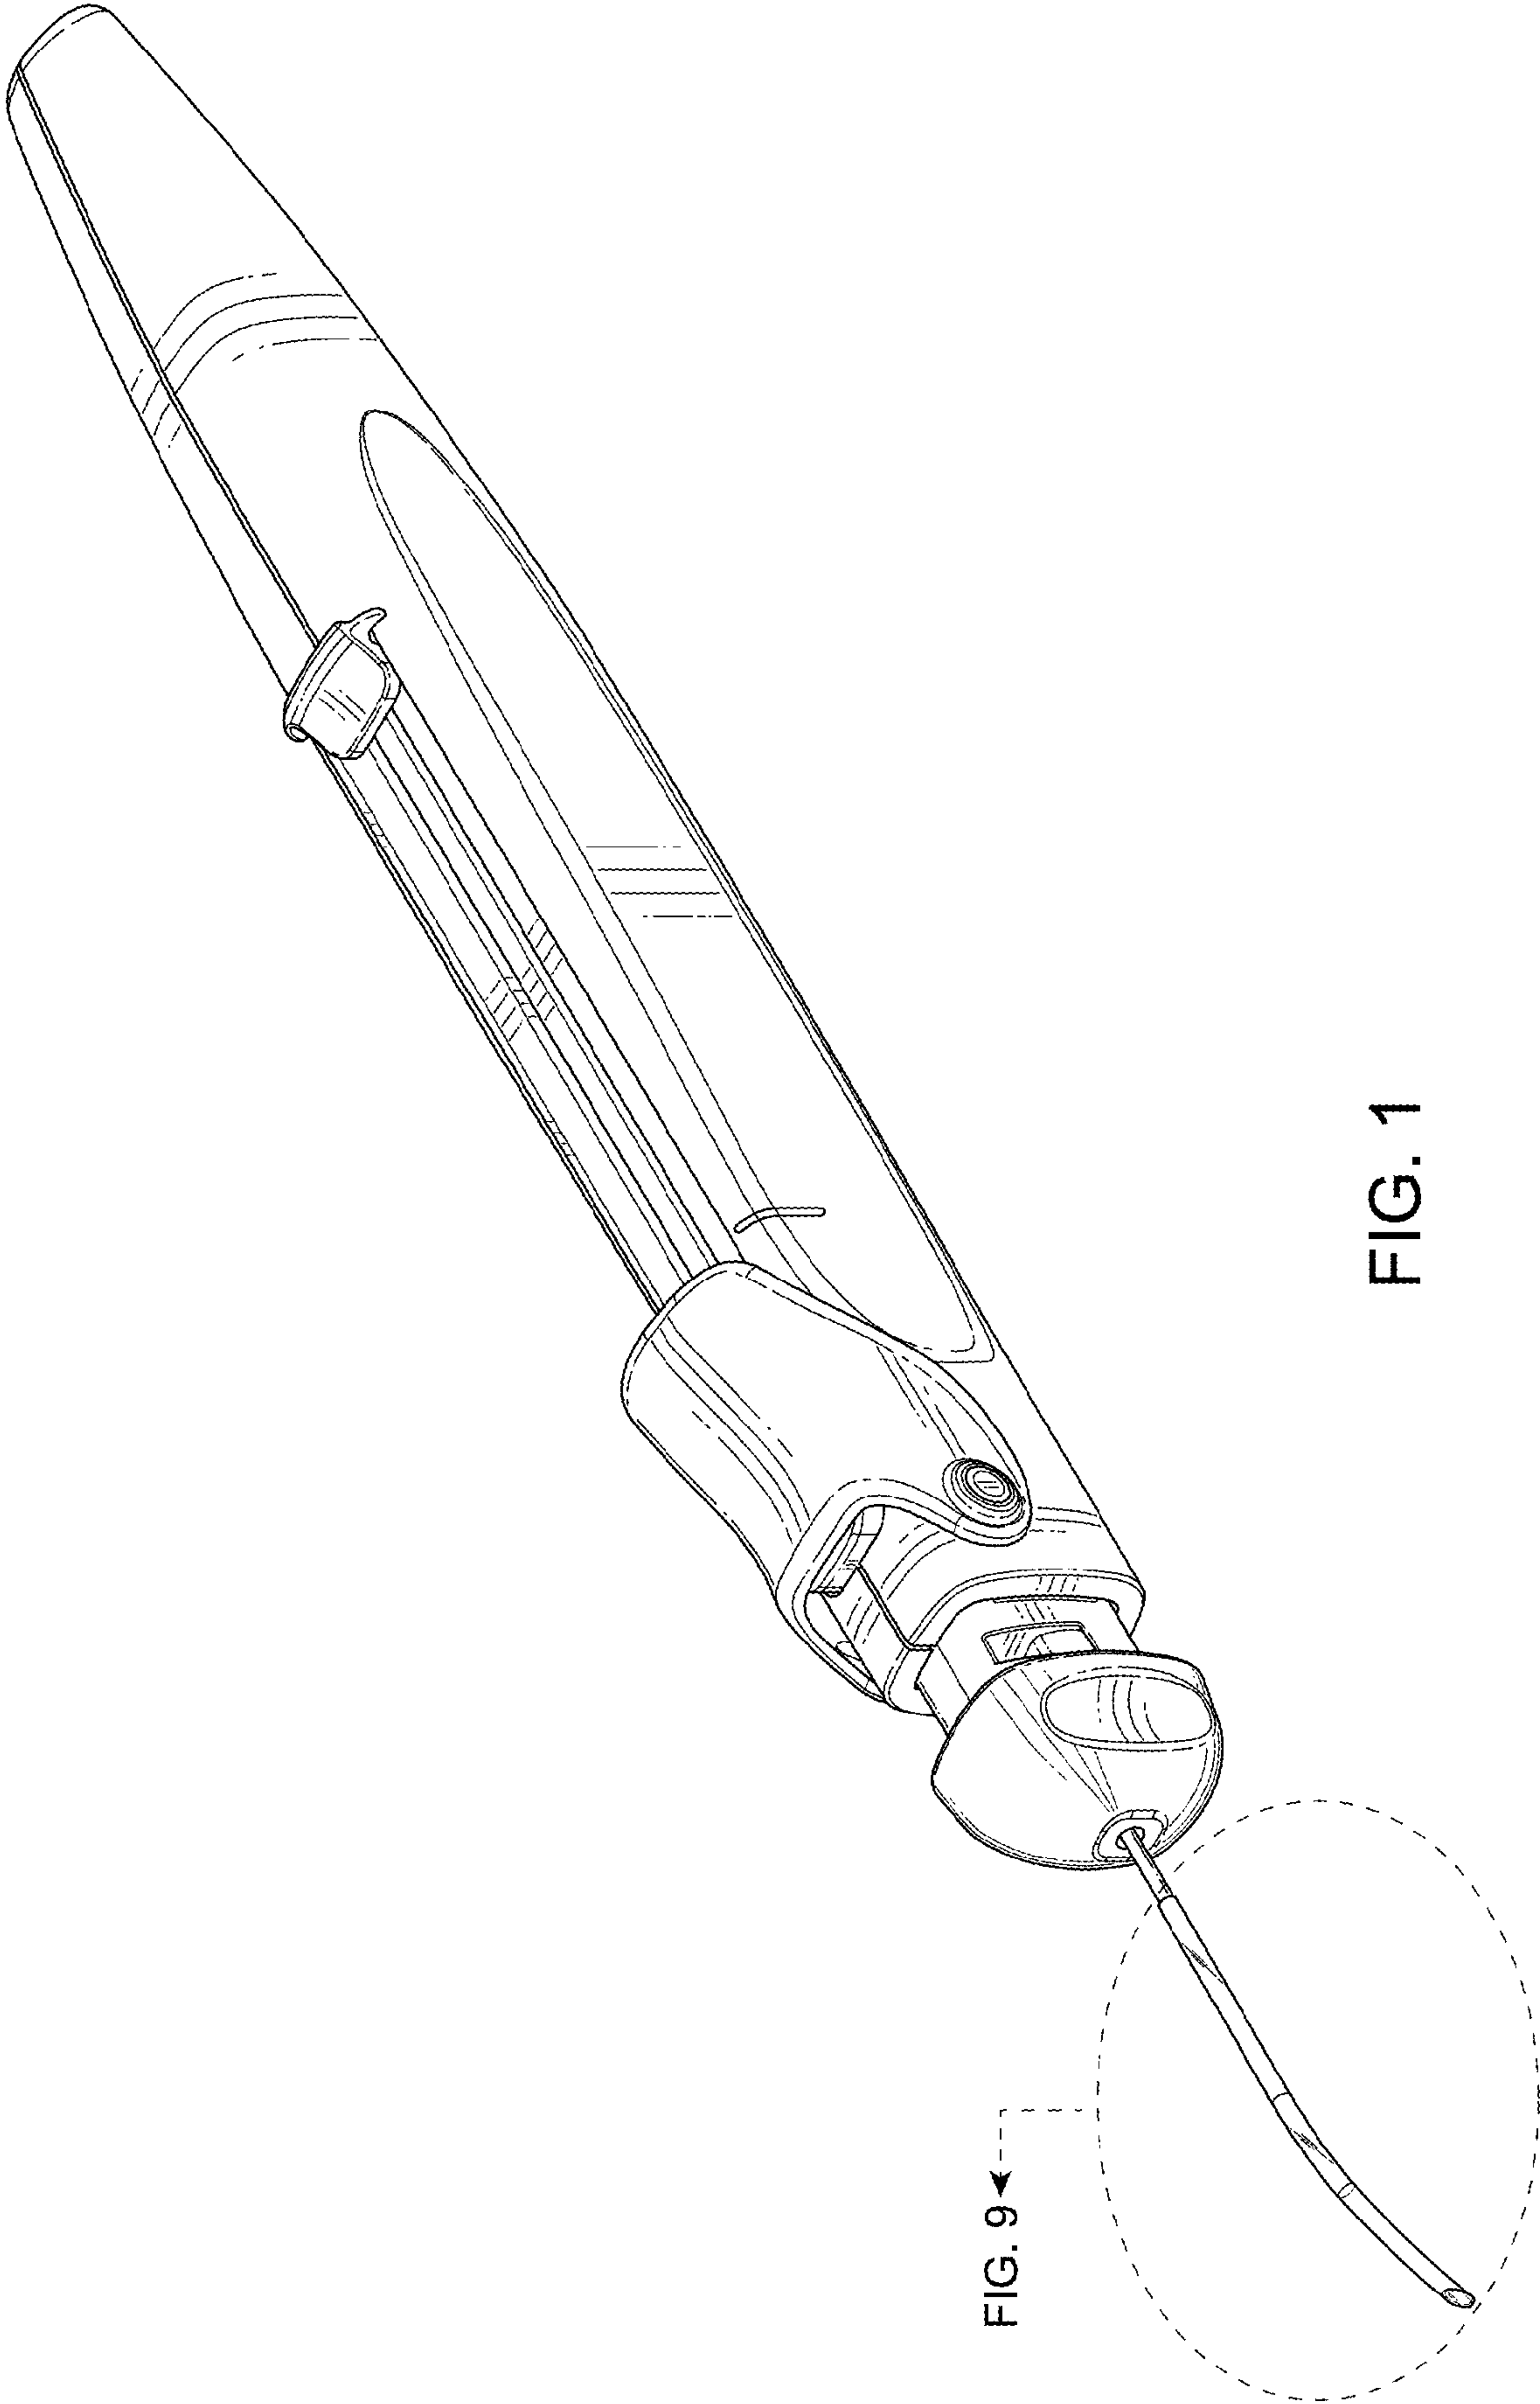

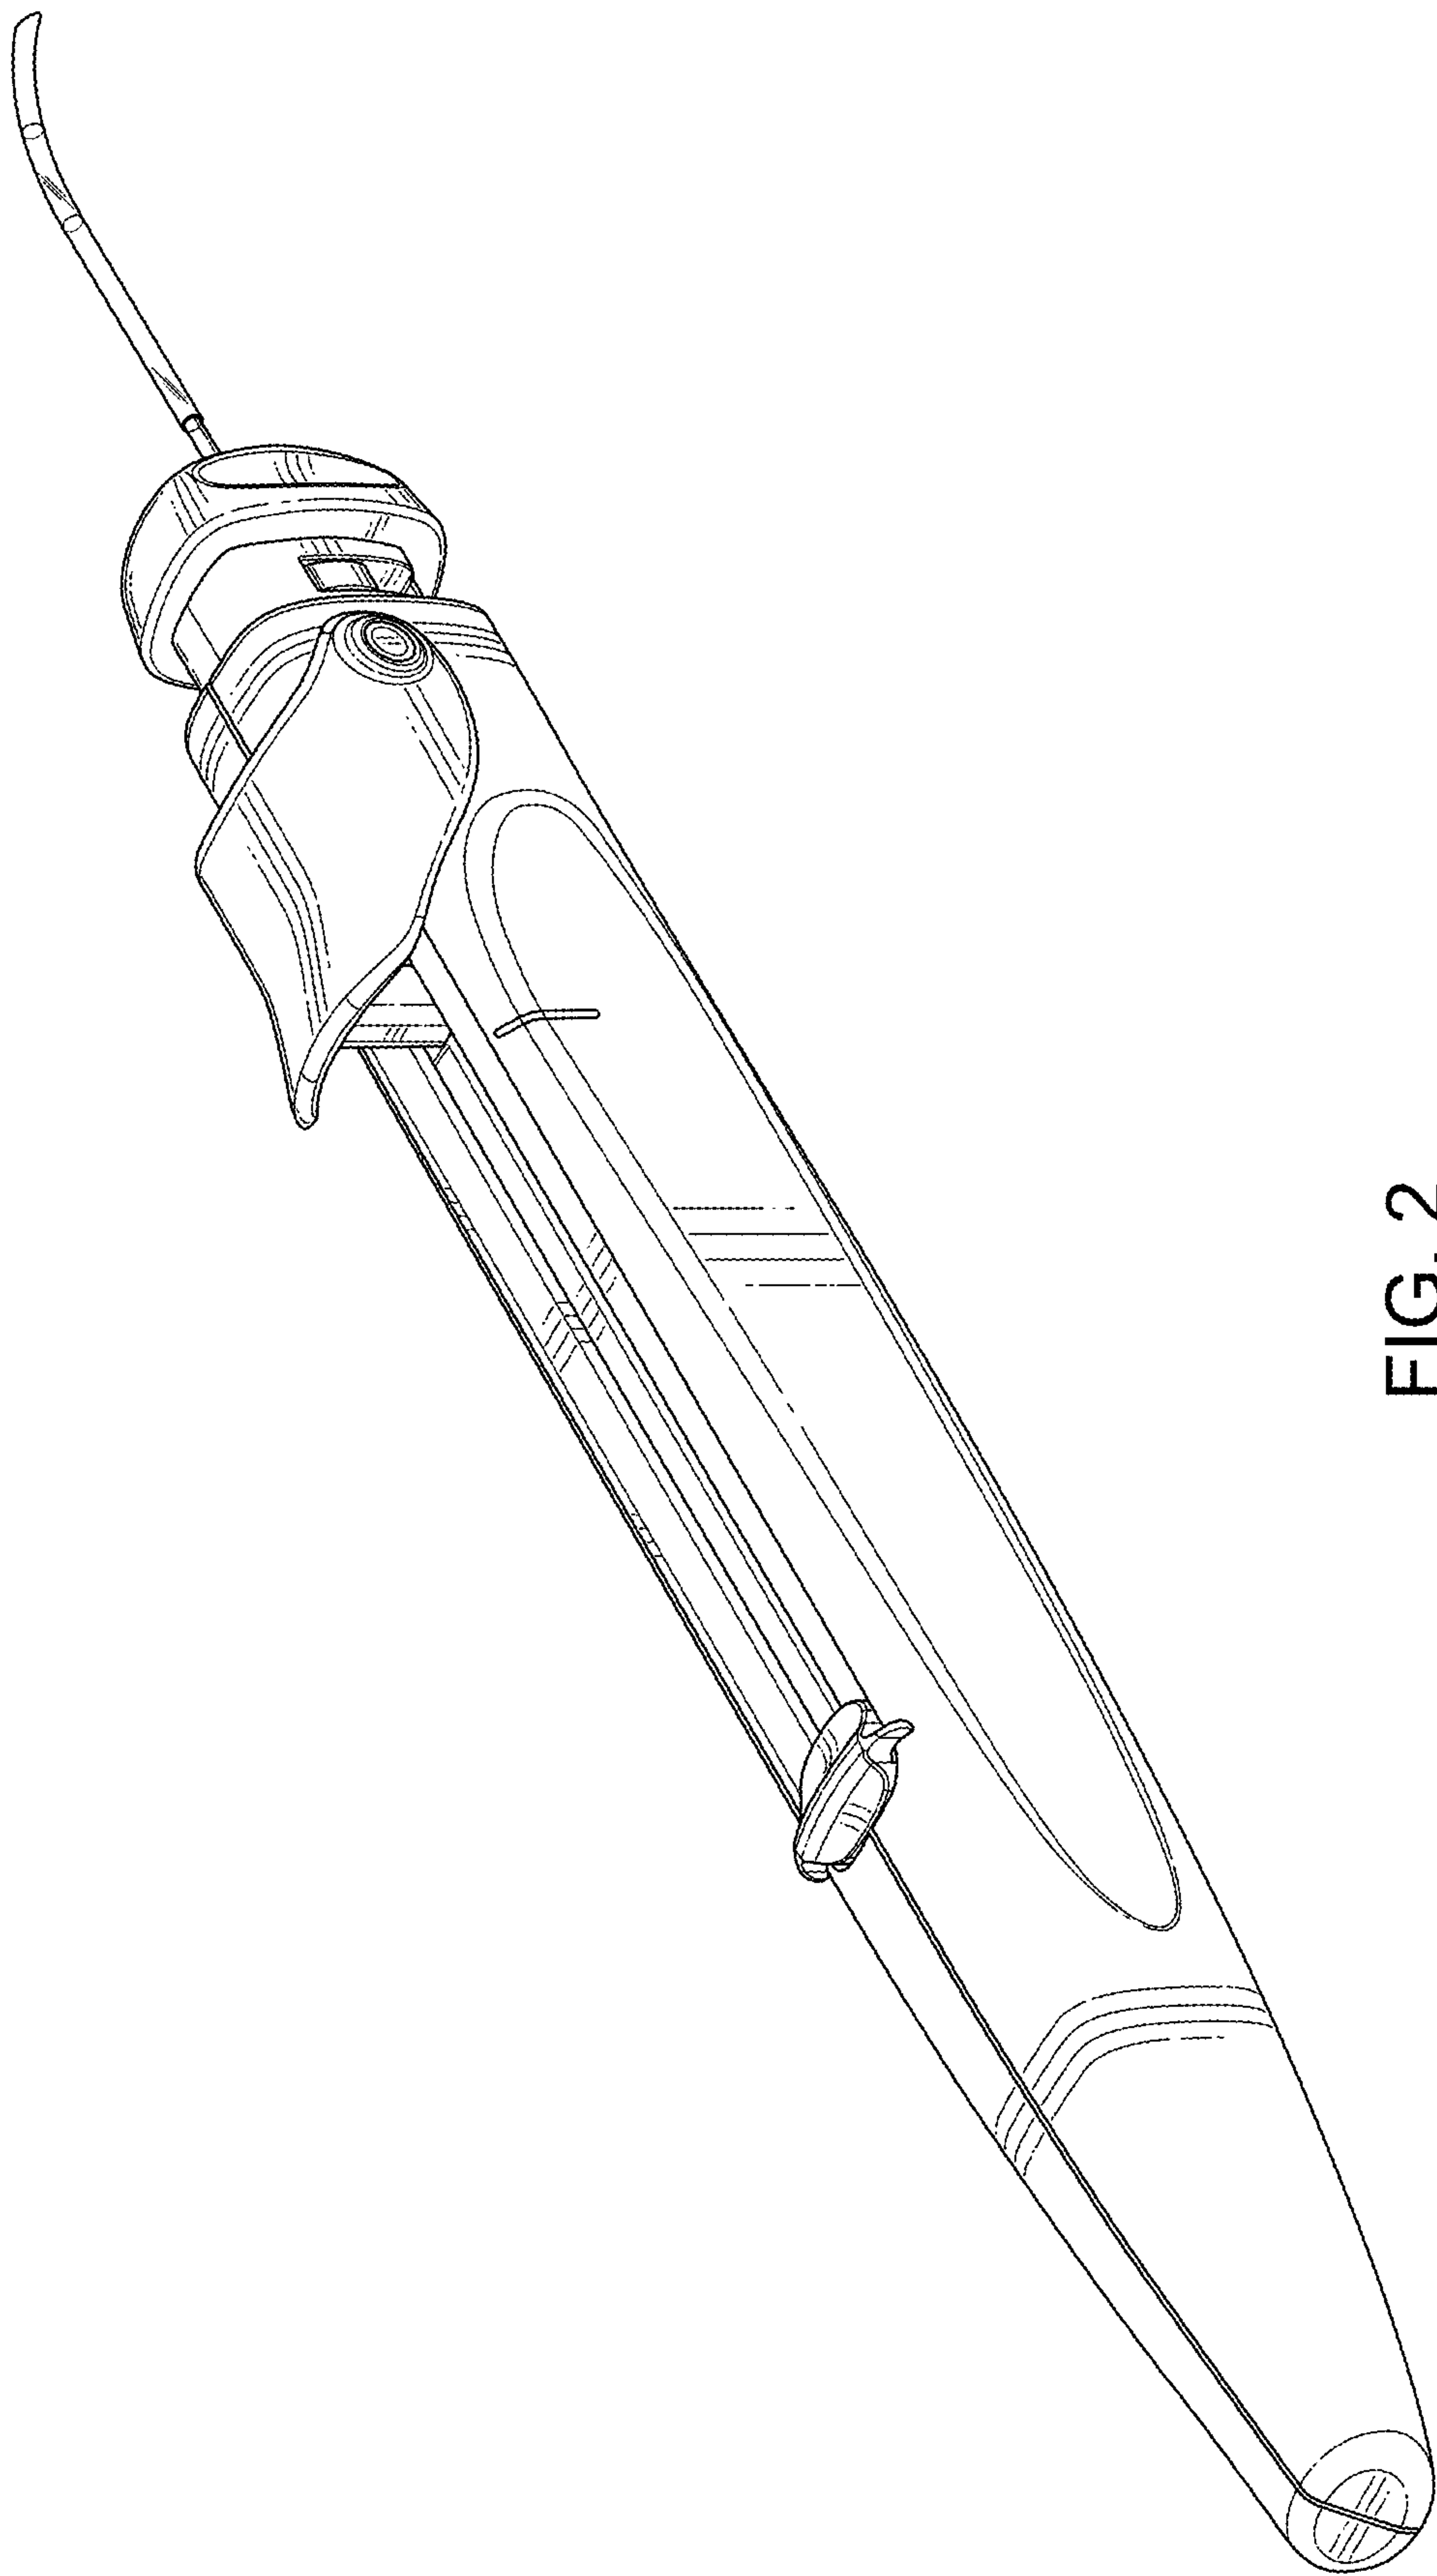


FIG. 2

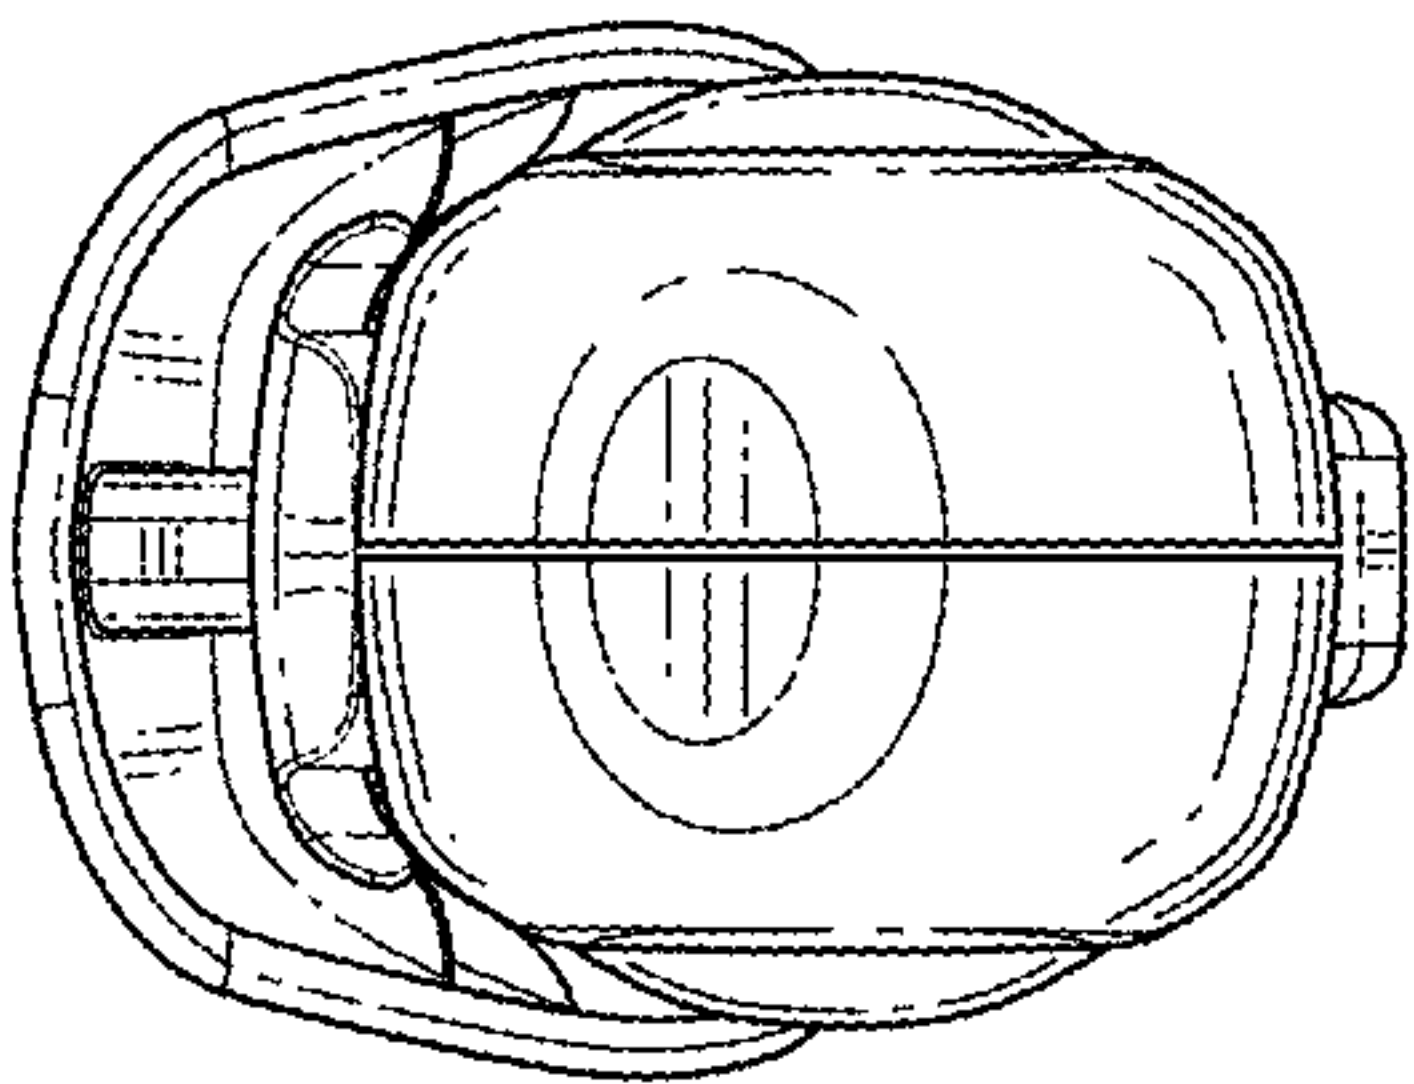


FIG. 4

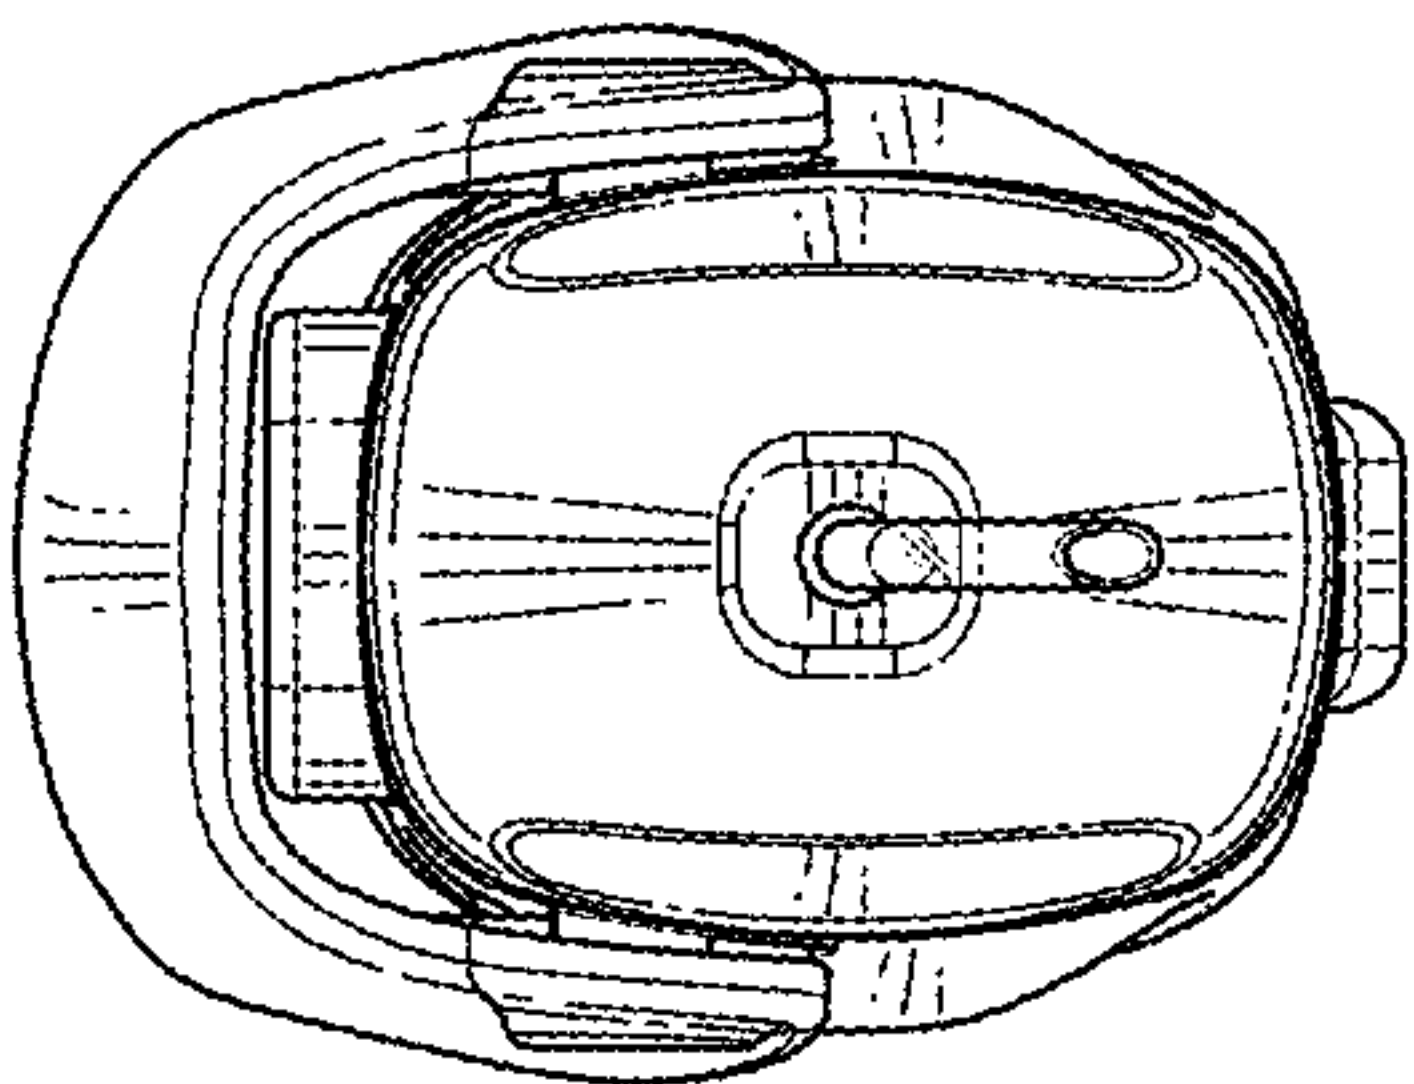


FIG. 3

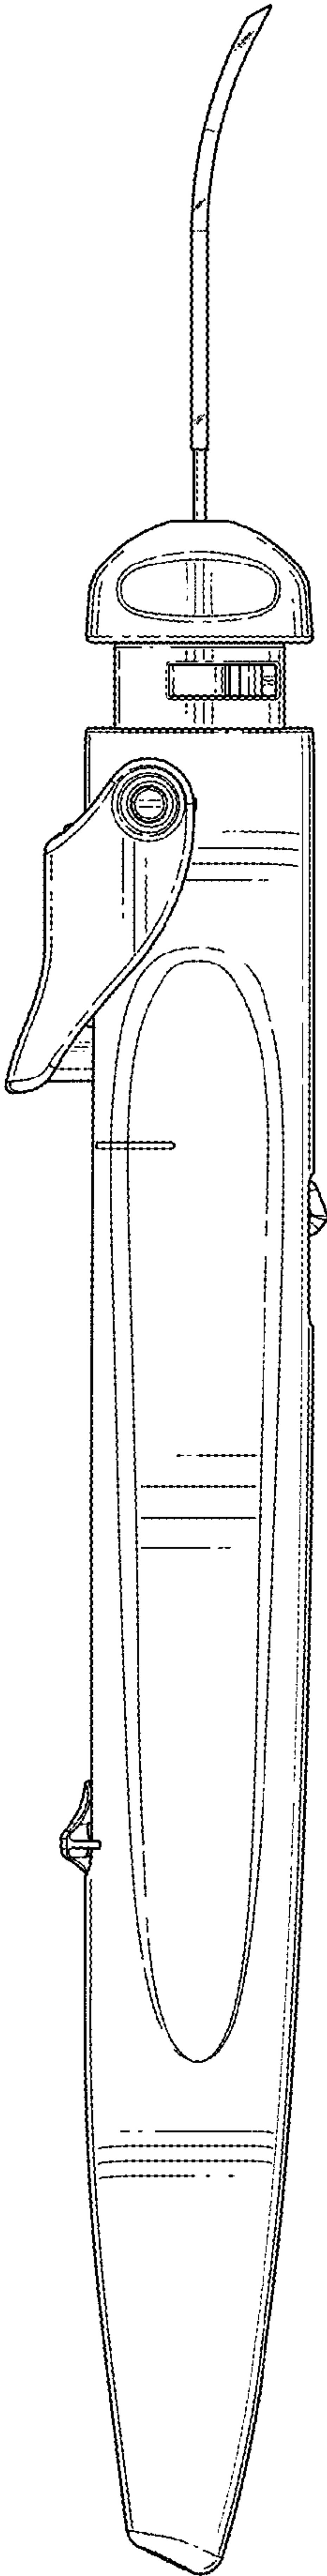


FIG. 5

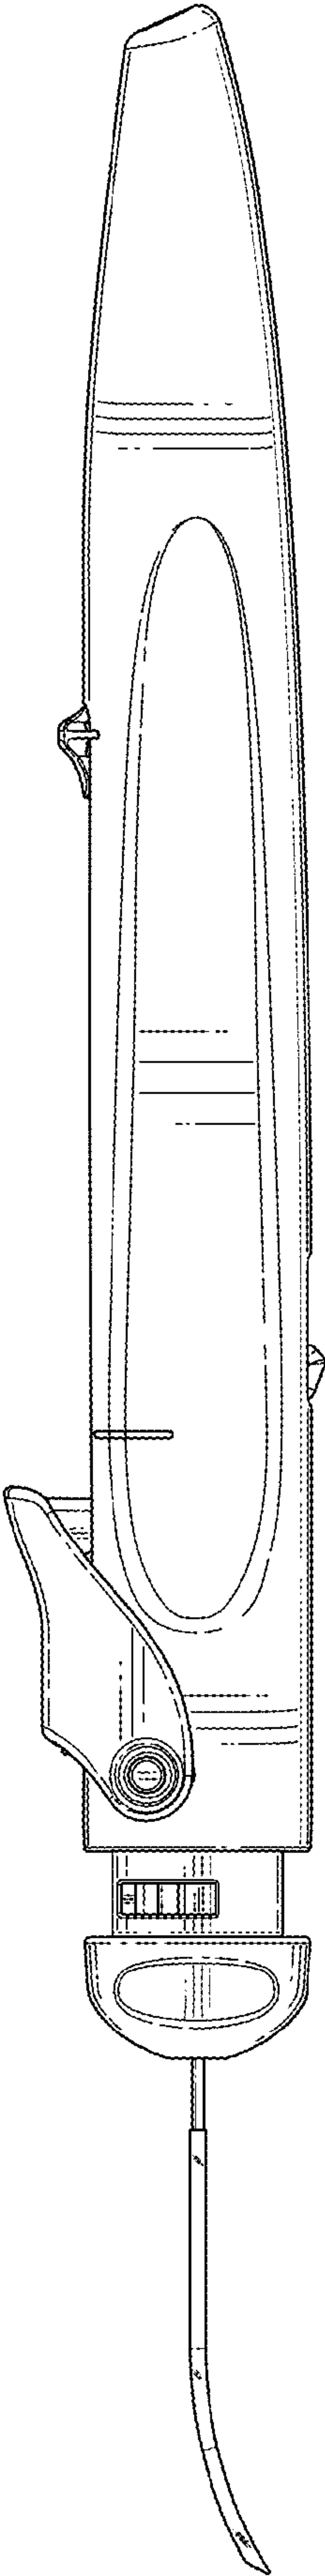


FIG. 6

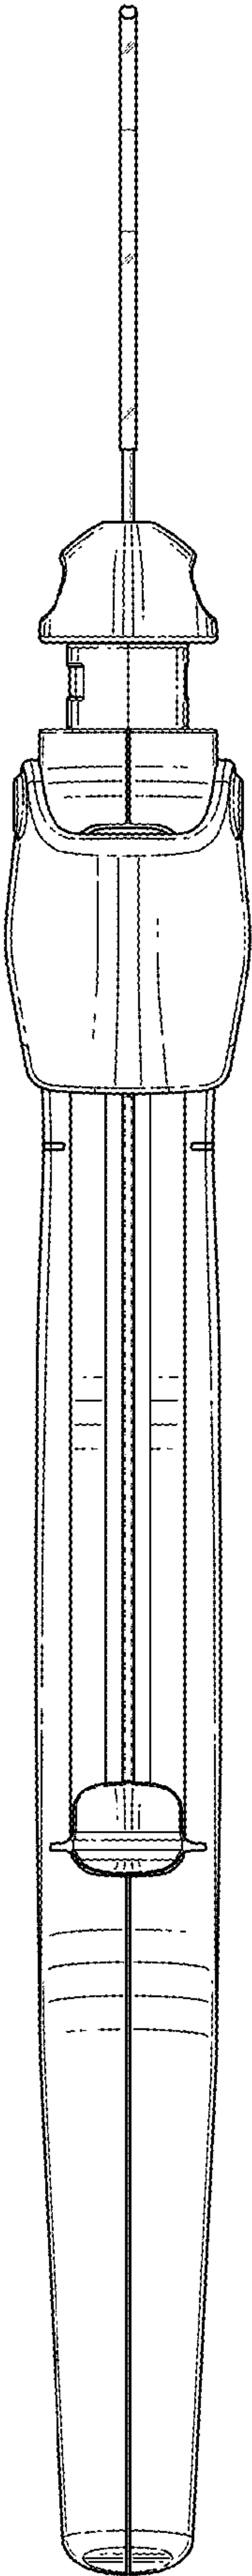


FIG. 7

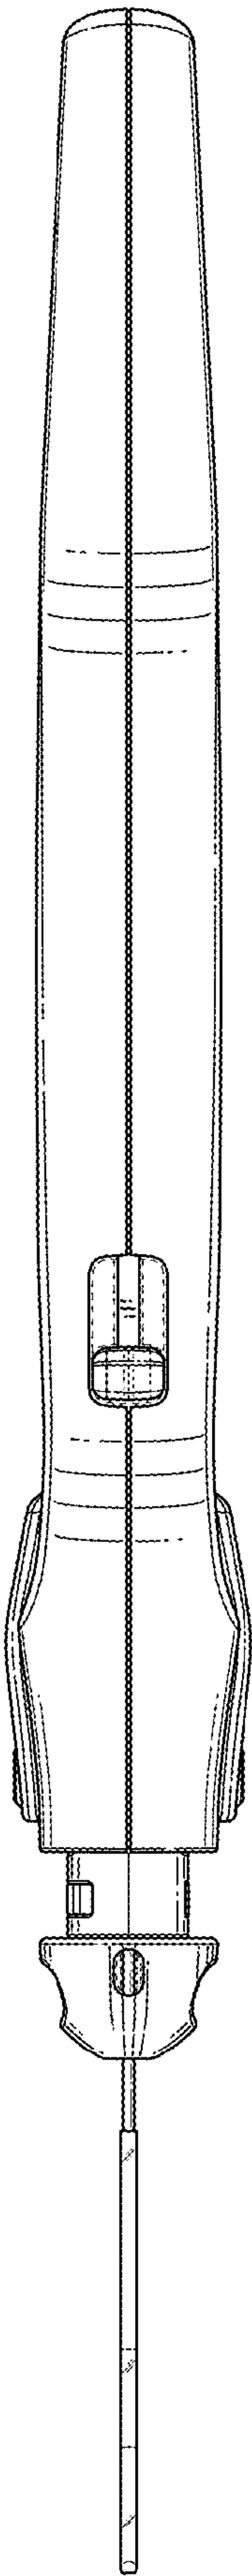


FIG. 8

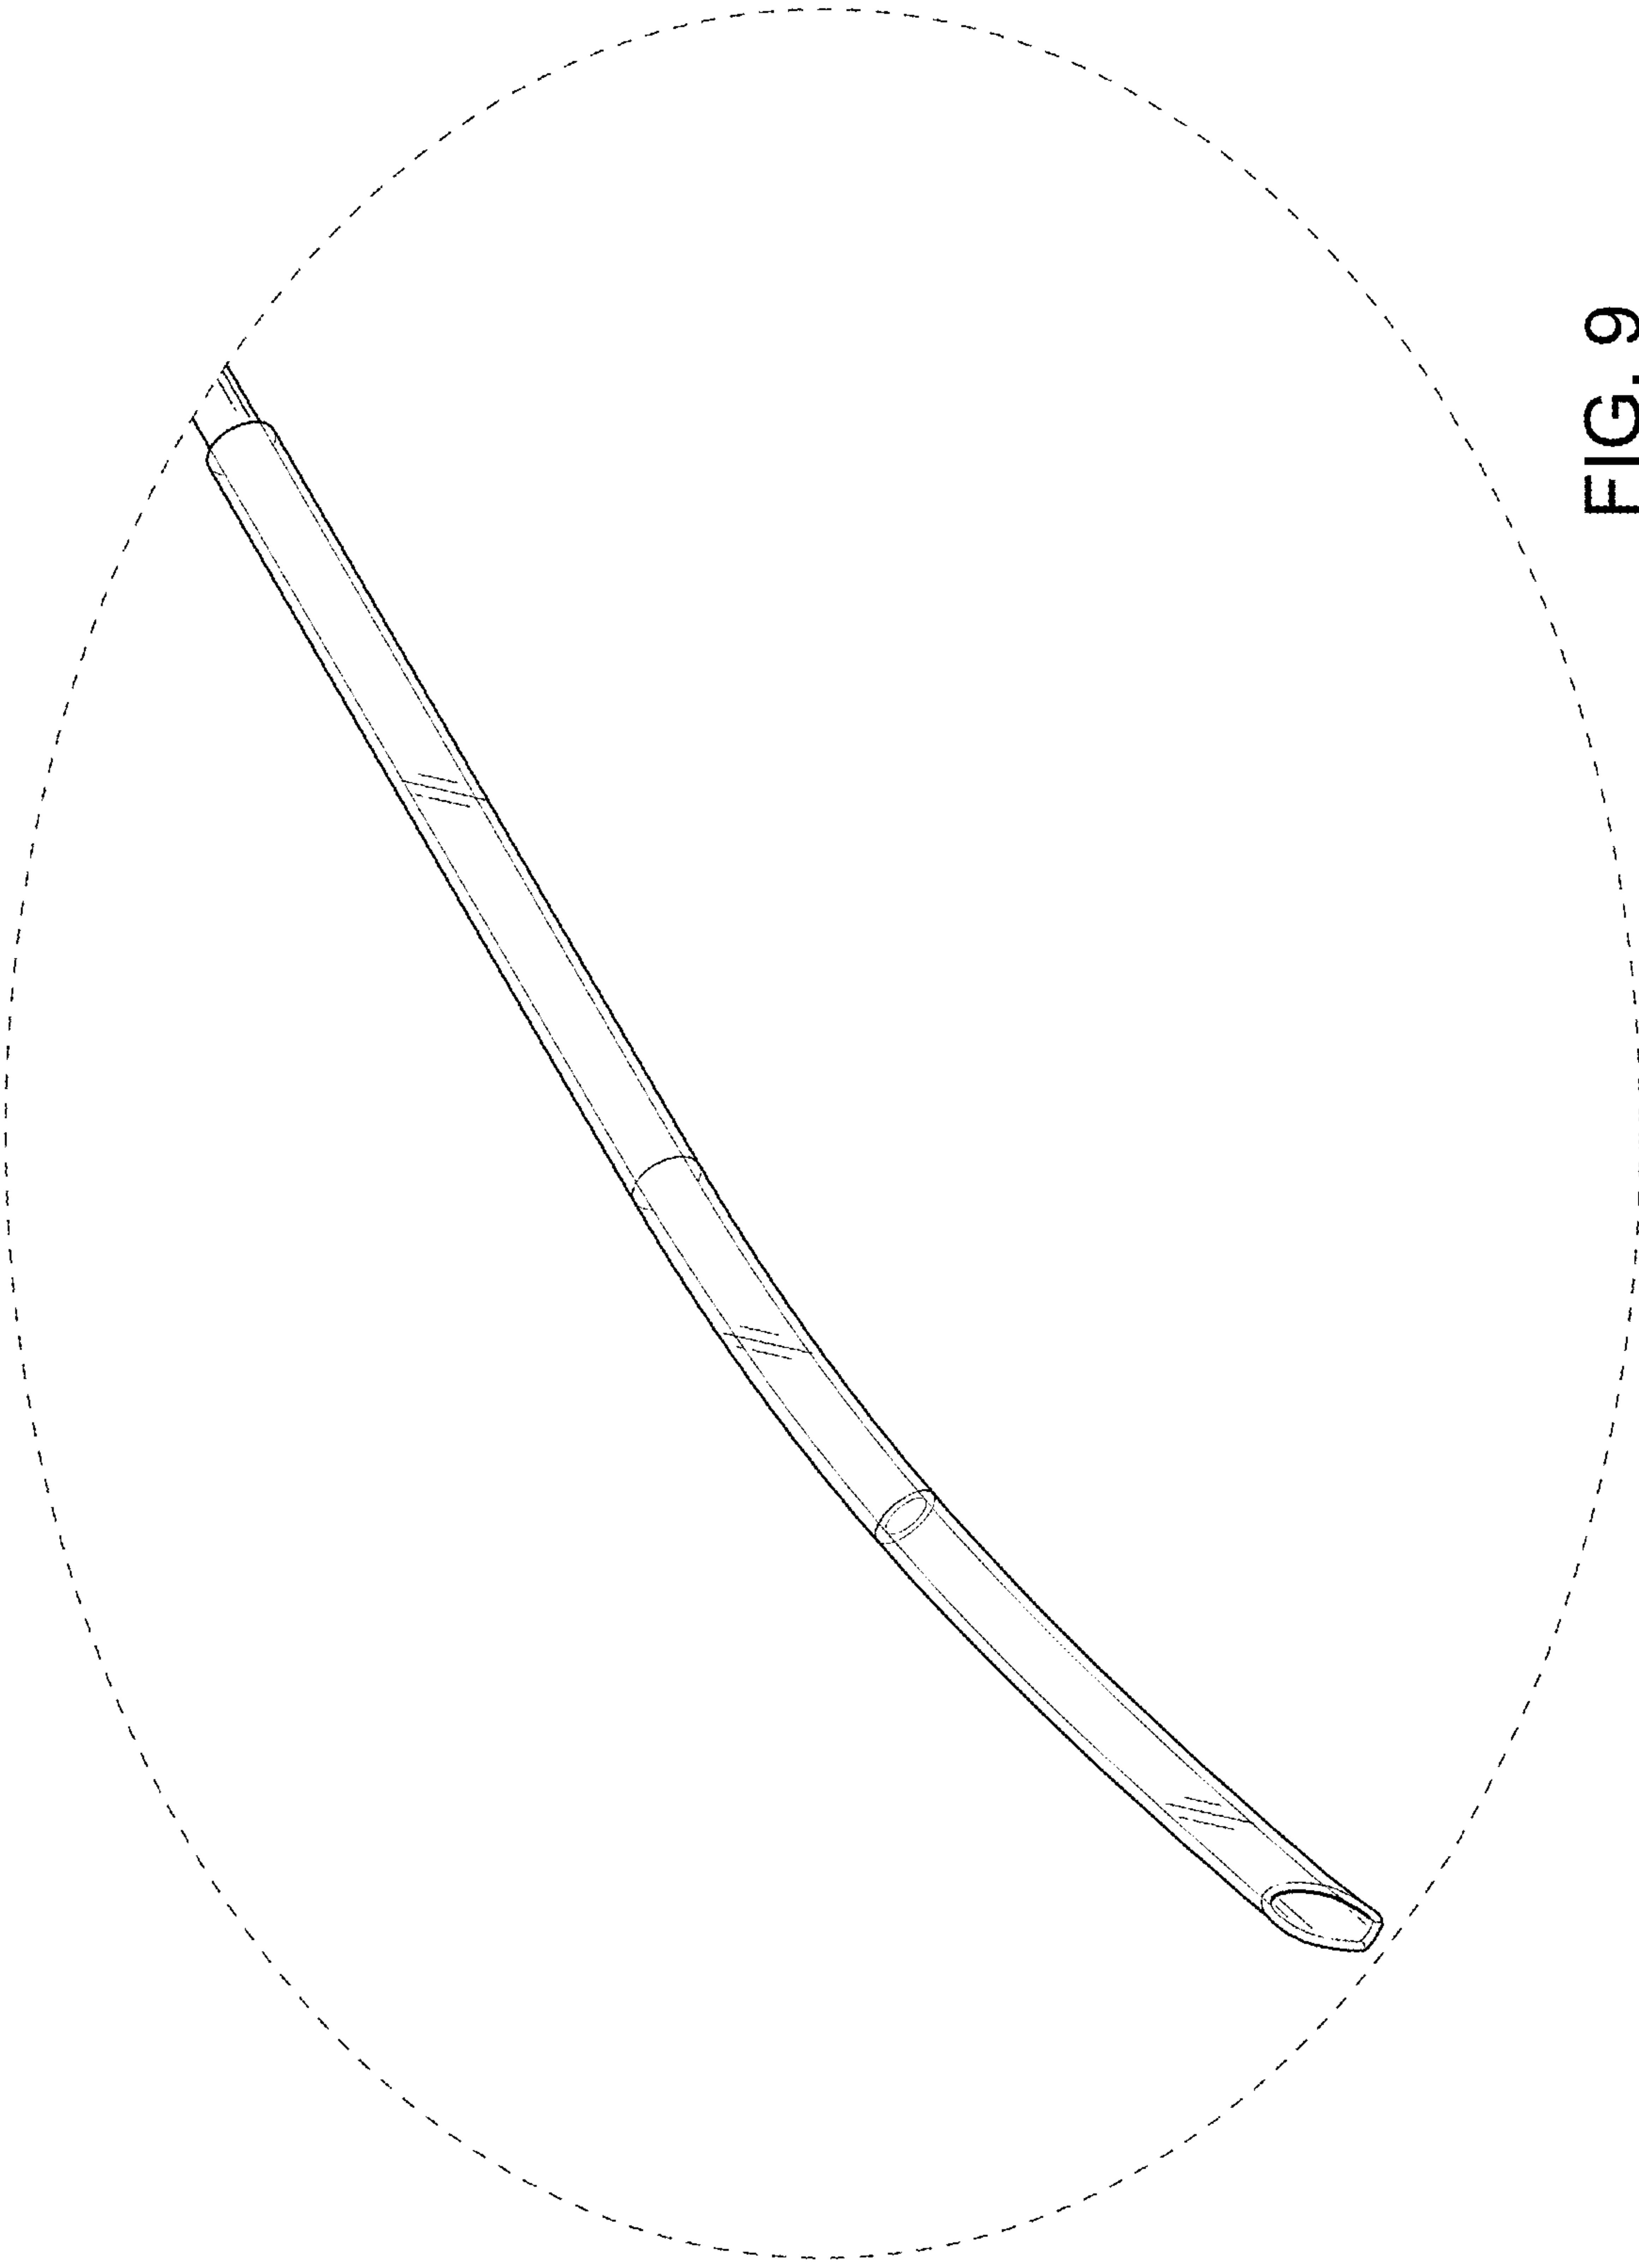


FIG. 9