



US0D1042825S

(12)

United States Design Patent

DeLorenzo et al.

(10)

Patent No.:

US D1,042,825 S

(45)

Date of Patent:

** Sep. 17, 2024

(54) HANDLE FOR A MEDICAL DEVICE

FOREIGN PATENT DOCUMENTS

(71) Applicant: ABIOMED, Inc., Danvers, MA (US)

CN 304033462 2/2017
CN 306163859 11/2020

(72) Inventors: Charles DeLorenzo, Danvers, MA (US); Christopher Nason Korkuch, Beverly, MA (US); Glen R. Fantuzzi, Danvers, MA (US); Brian Chouinard, Danvers, MA (US)

(Continued)

(73) Assignee: Abiomed, Inc., Danvers, MA (US)

(**) Term: 15 Years

(21) Appl. No.: 29/813,965

(22) Filed: Nov. 2, 2021

(51) LOC (14) Cl. 24-02

(52) U.S. Cl. USPC D24/133

(58) Field of Classification Search

USPC D24/127, 130, 133, 146, 147, 200, 214, D24/144, 108, 112, 113, 115, 207, 222, D24/224, 165; D19/110, 115; D23/223, D23/226, 229; D8/2, 82, 83, 84, 85, 86, D8/87, 80; D7/393, 396, 414
CPC B26B 3/00; B26B 1/10; A61B 17/1617; A61B 17/3417; A61B 17/1624; A61B 17/162; A61B 17/1622; A61B 5/1411; A61B 2017/00424; A61B 17/865; A61B 17/8875; A61B 2018/00589; A61B 2017/00464; B05C 17/103; B05C 17/116; B05C 17/01; B25B 23/04; B25B 23/06
See application file for complete search history.

(56) References Cited

U.S. PATENT DOCUMENTS

D345,419 S * 3/1994 Horrigan D24/130
D430,290 S * 8/2000 Cindrich D24/112
D490,894 S * 6/2004 Bogazzi D24/146
D490,896 S * 6/2004 Bogazzi D24/146
6,796,991 B2 * 9/2004 Nardeo A61M 25/0668 606/191
D589,143 S * 3/2009 Mauch D24/130

(Continued)

OTHER PUBLICATIONS

U.S. FDA Grants 510(k) Clearance for Impella Low Profile Sheath [online]. Businesswire.com, Oct. 17, 2022 [retrieved on Oct. 5, 2023]. Retrieved from the Internet: <https://www.businesswire.com/news/home/20221017005313/en/U.S.-FDA-Grants-510-k-Clearance-for-Impella-Low-Profile-Sheath> (Year: 2022).*

Primary Examiner — Samantha Q Lawrence

Assistant Examiner — Thanh Luu Wong

(74) Attorney, Agent, or Firm — Botos Churchill IP Law LLP


(57) CLAIM

The ornamental design for a handle for a medical device, as shown and described.

DESCRIPTION

FIG. 1 is a top, front, right side perspective view of a handle for a medical device showing our new design; FIG. 2 is a top, rear, right side perspective view thereof; FIG. 3 is a front elevation view thereof; FIG. 4 is a rear elevation view thereof; FIG. 5 is a left side elevation view thereof; FIG. 6 is a right side elevation view thereof; FIG. 7 is a top plan view thereof; and, FIG. 8 is a bottom plan view thereof. The dot-dash broken lines represent boundaries of the claimed design and form no part thereof. All other broken lines illustrate portions of the handle for a medical device that form no part of the claimed design.

1 Claim, 8 Drawing Sheets

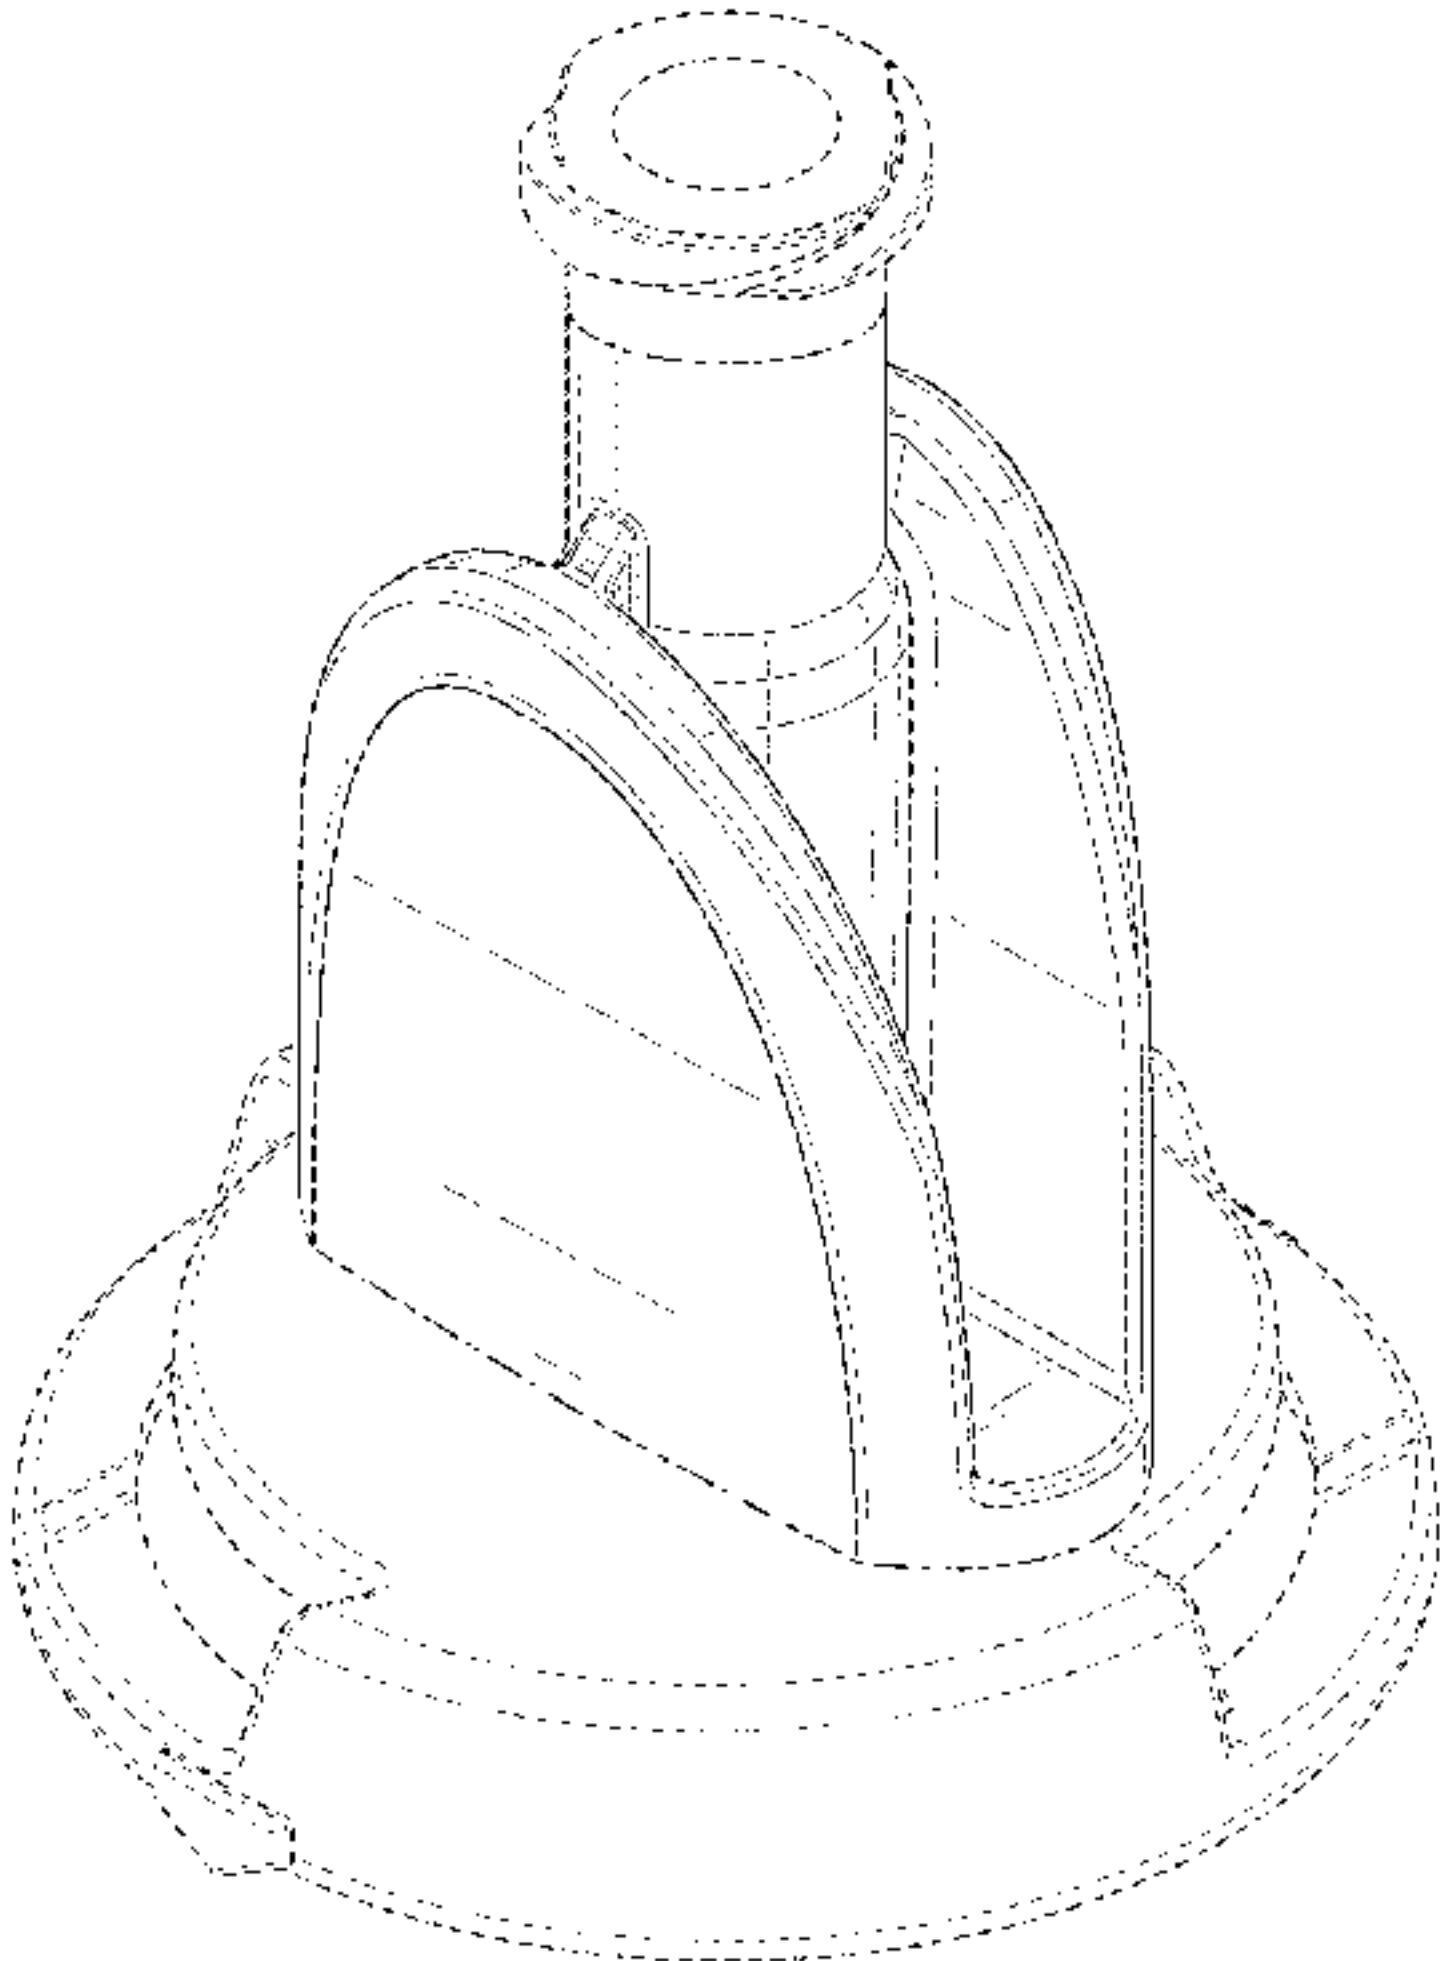

(56) **References Cited**

U.S. PATENT DOCUMENTS

D634,156 S	*	3/2011	Fuller	D7/393
D634,424 S	*	3/2011	Morejon	D24/146
D663,030 S	*	7/2012	Murner	D24/143
D715,126 S	*	10/2014	Kim	D7/393
D715,955 S	*	10/2014	Hsu	A61H 19/00 D24/215
D845,843 S		4/2019	Inoue et al.	
D846,225 S		4/2019	Johanning et al.	
D879,290 S		3/2020	Harman et al.	
D887,993 S		6/2020	Decastro et al.	
10,709,875 B2		7/2020	O’Carrol et al.	
D914,477 S	*	3/2021	Watson	D8/310
D922,562 S		6/2021	Hulford et al.	
D931,456 S	*	9/2021	Schumaier	D24/147
D940,889 S		1/2022	Hocking	
D949,417 S	*	4/2022	Khubani	D24/215
D949,418 S	*	4/2022	Khubani	D24/215
D975,866 S	*	1/2023	Marton	D24/215

FOREIGN PATENT DOCUMENTS

JP	D13176290	12/2007
JP	1633708 S	6/2019
JP	1659556 S	5/2020
JP	1671048 S	10/2020
TW	D192842	9/2018
TW	D199557	9/2019

* cited by examiner

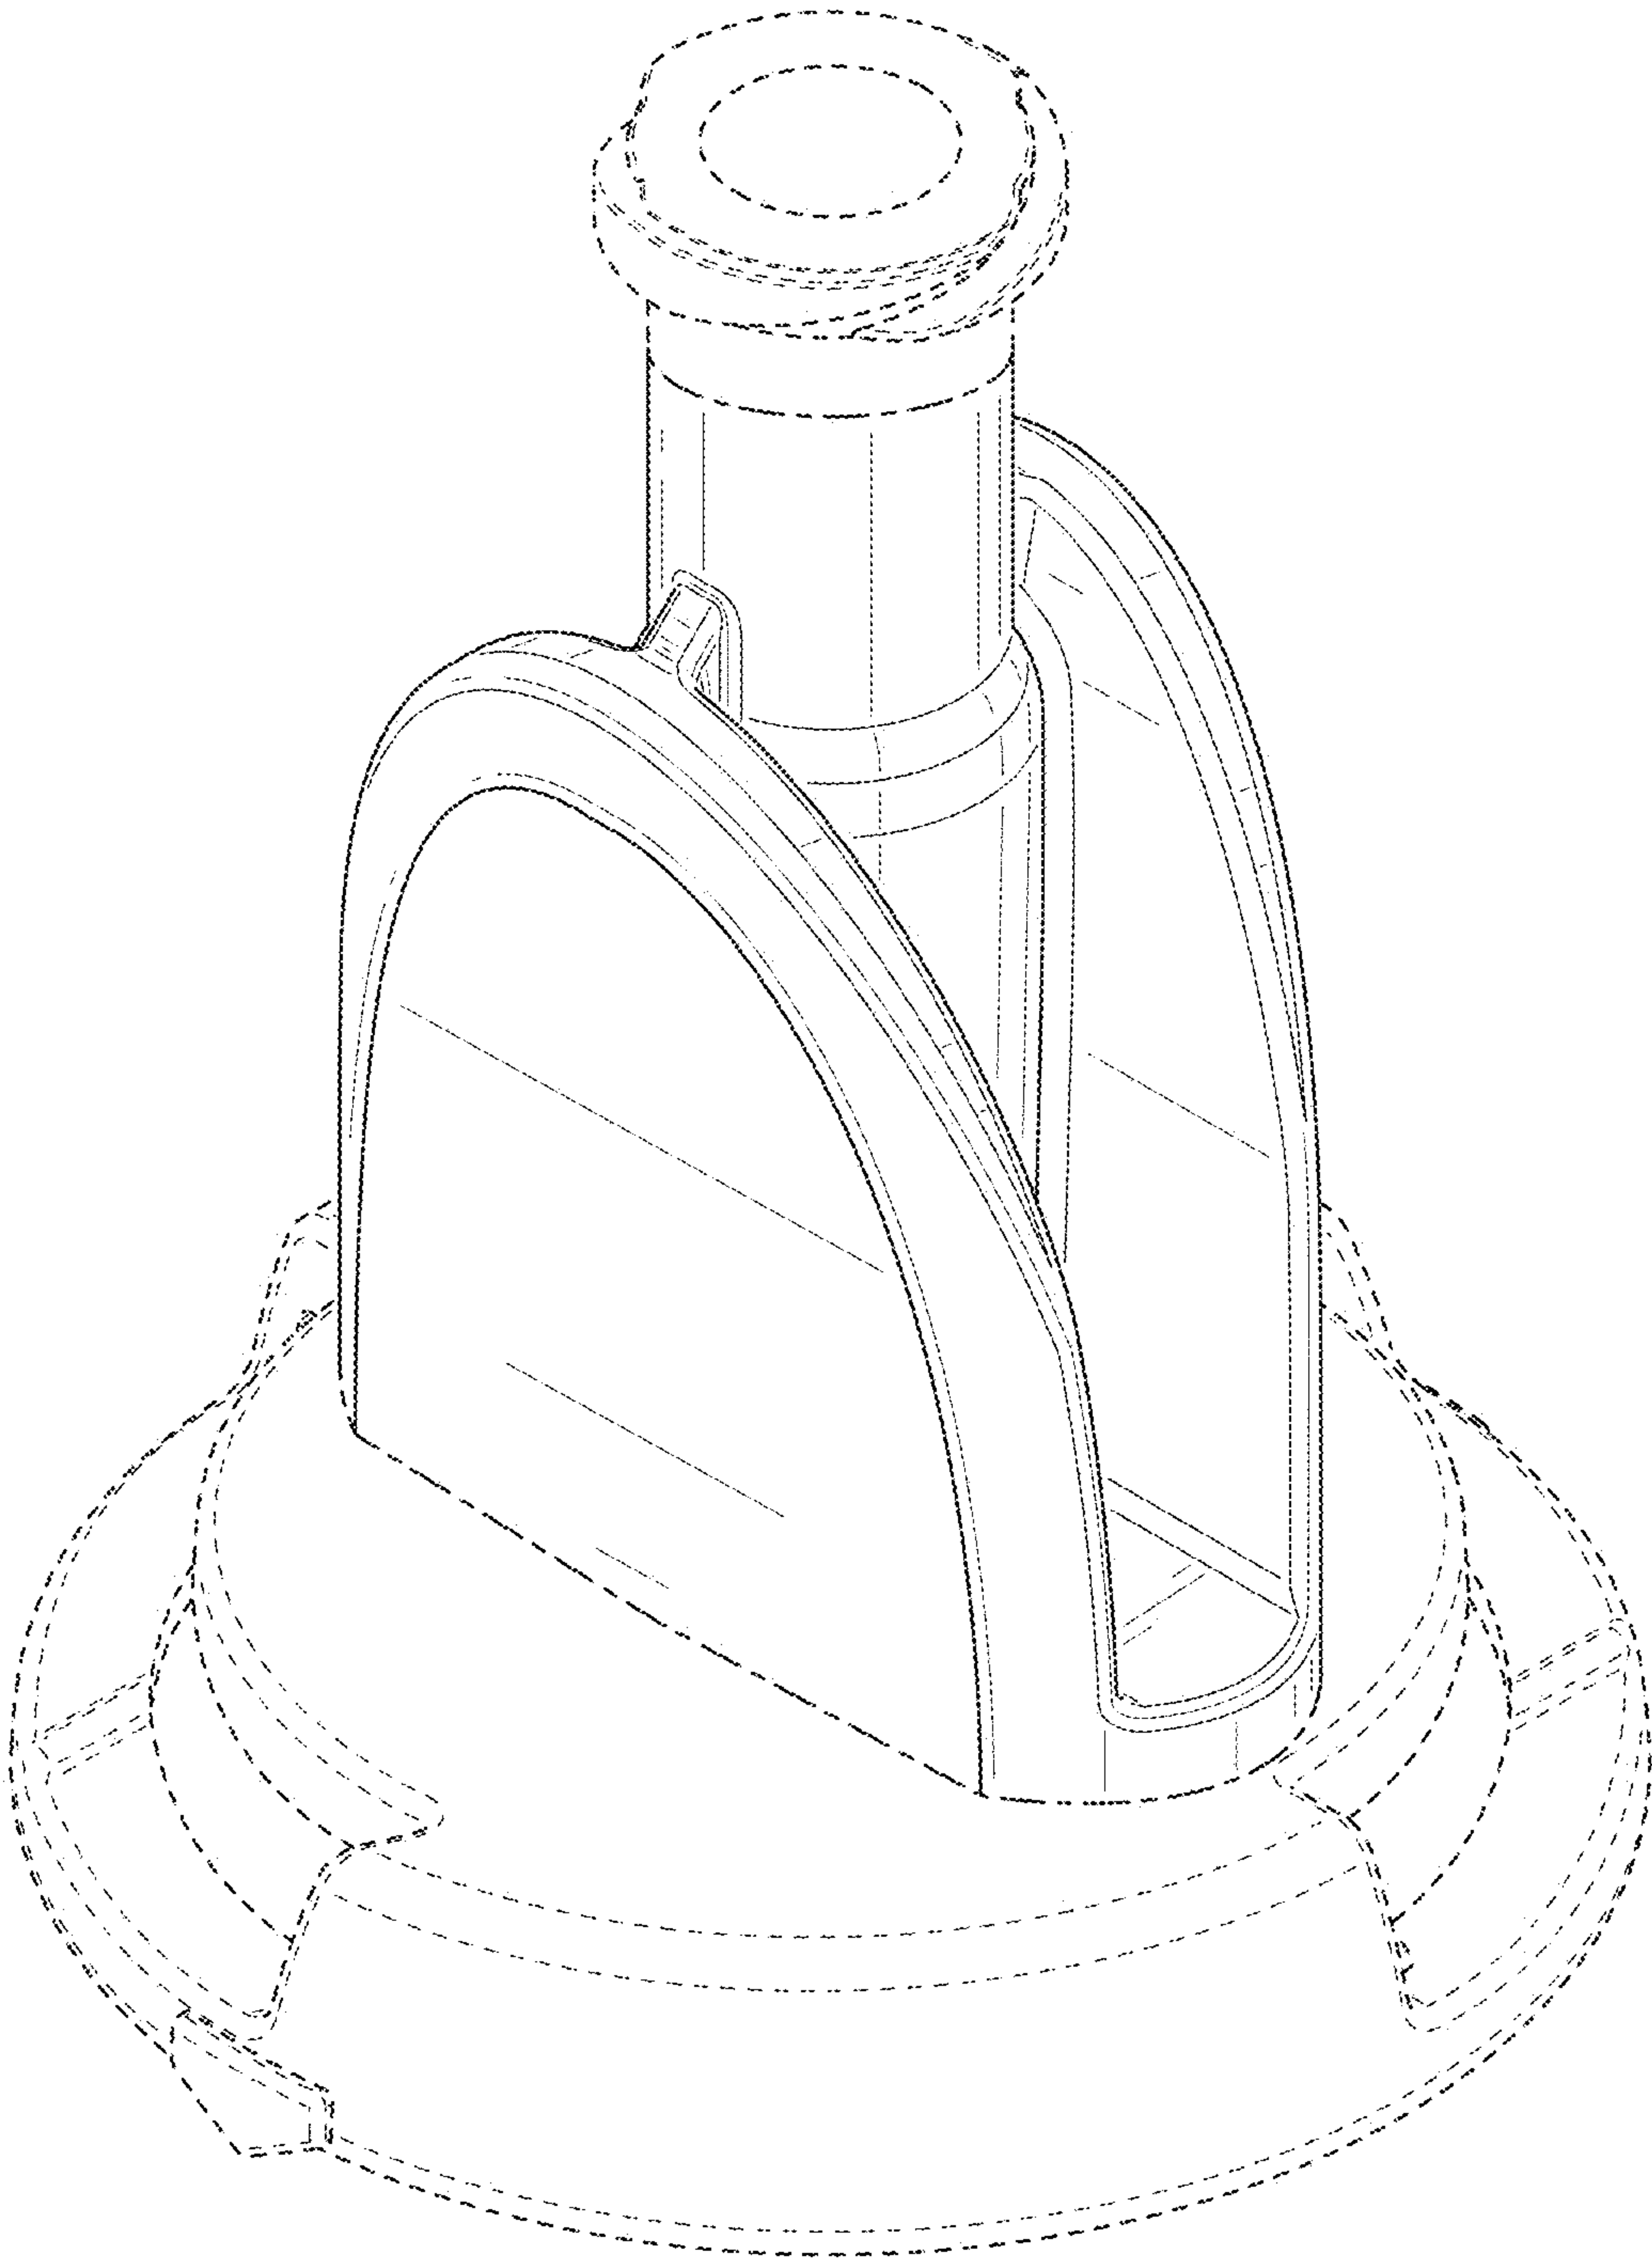


FIG. 1

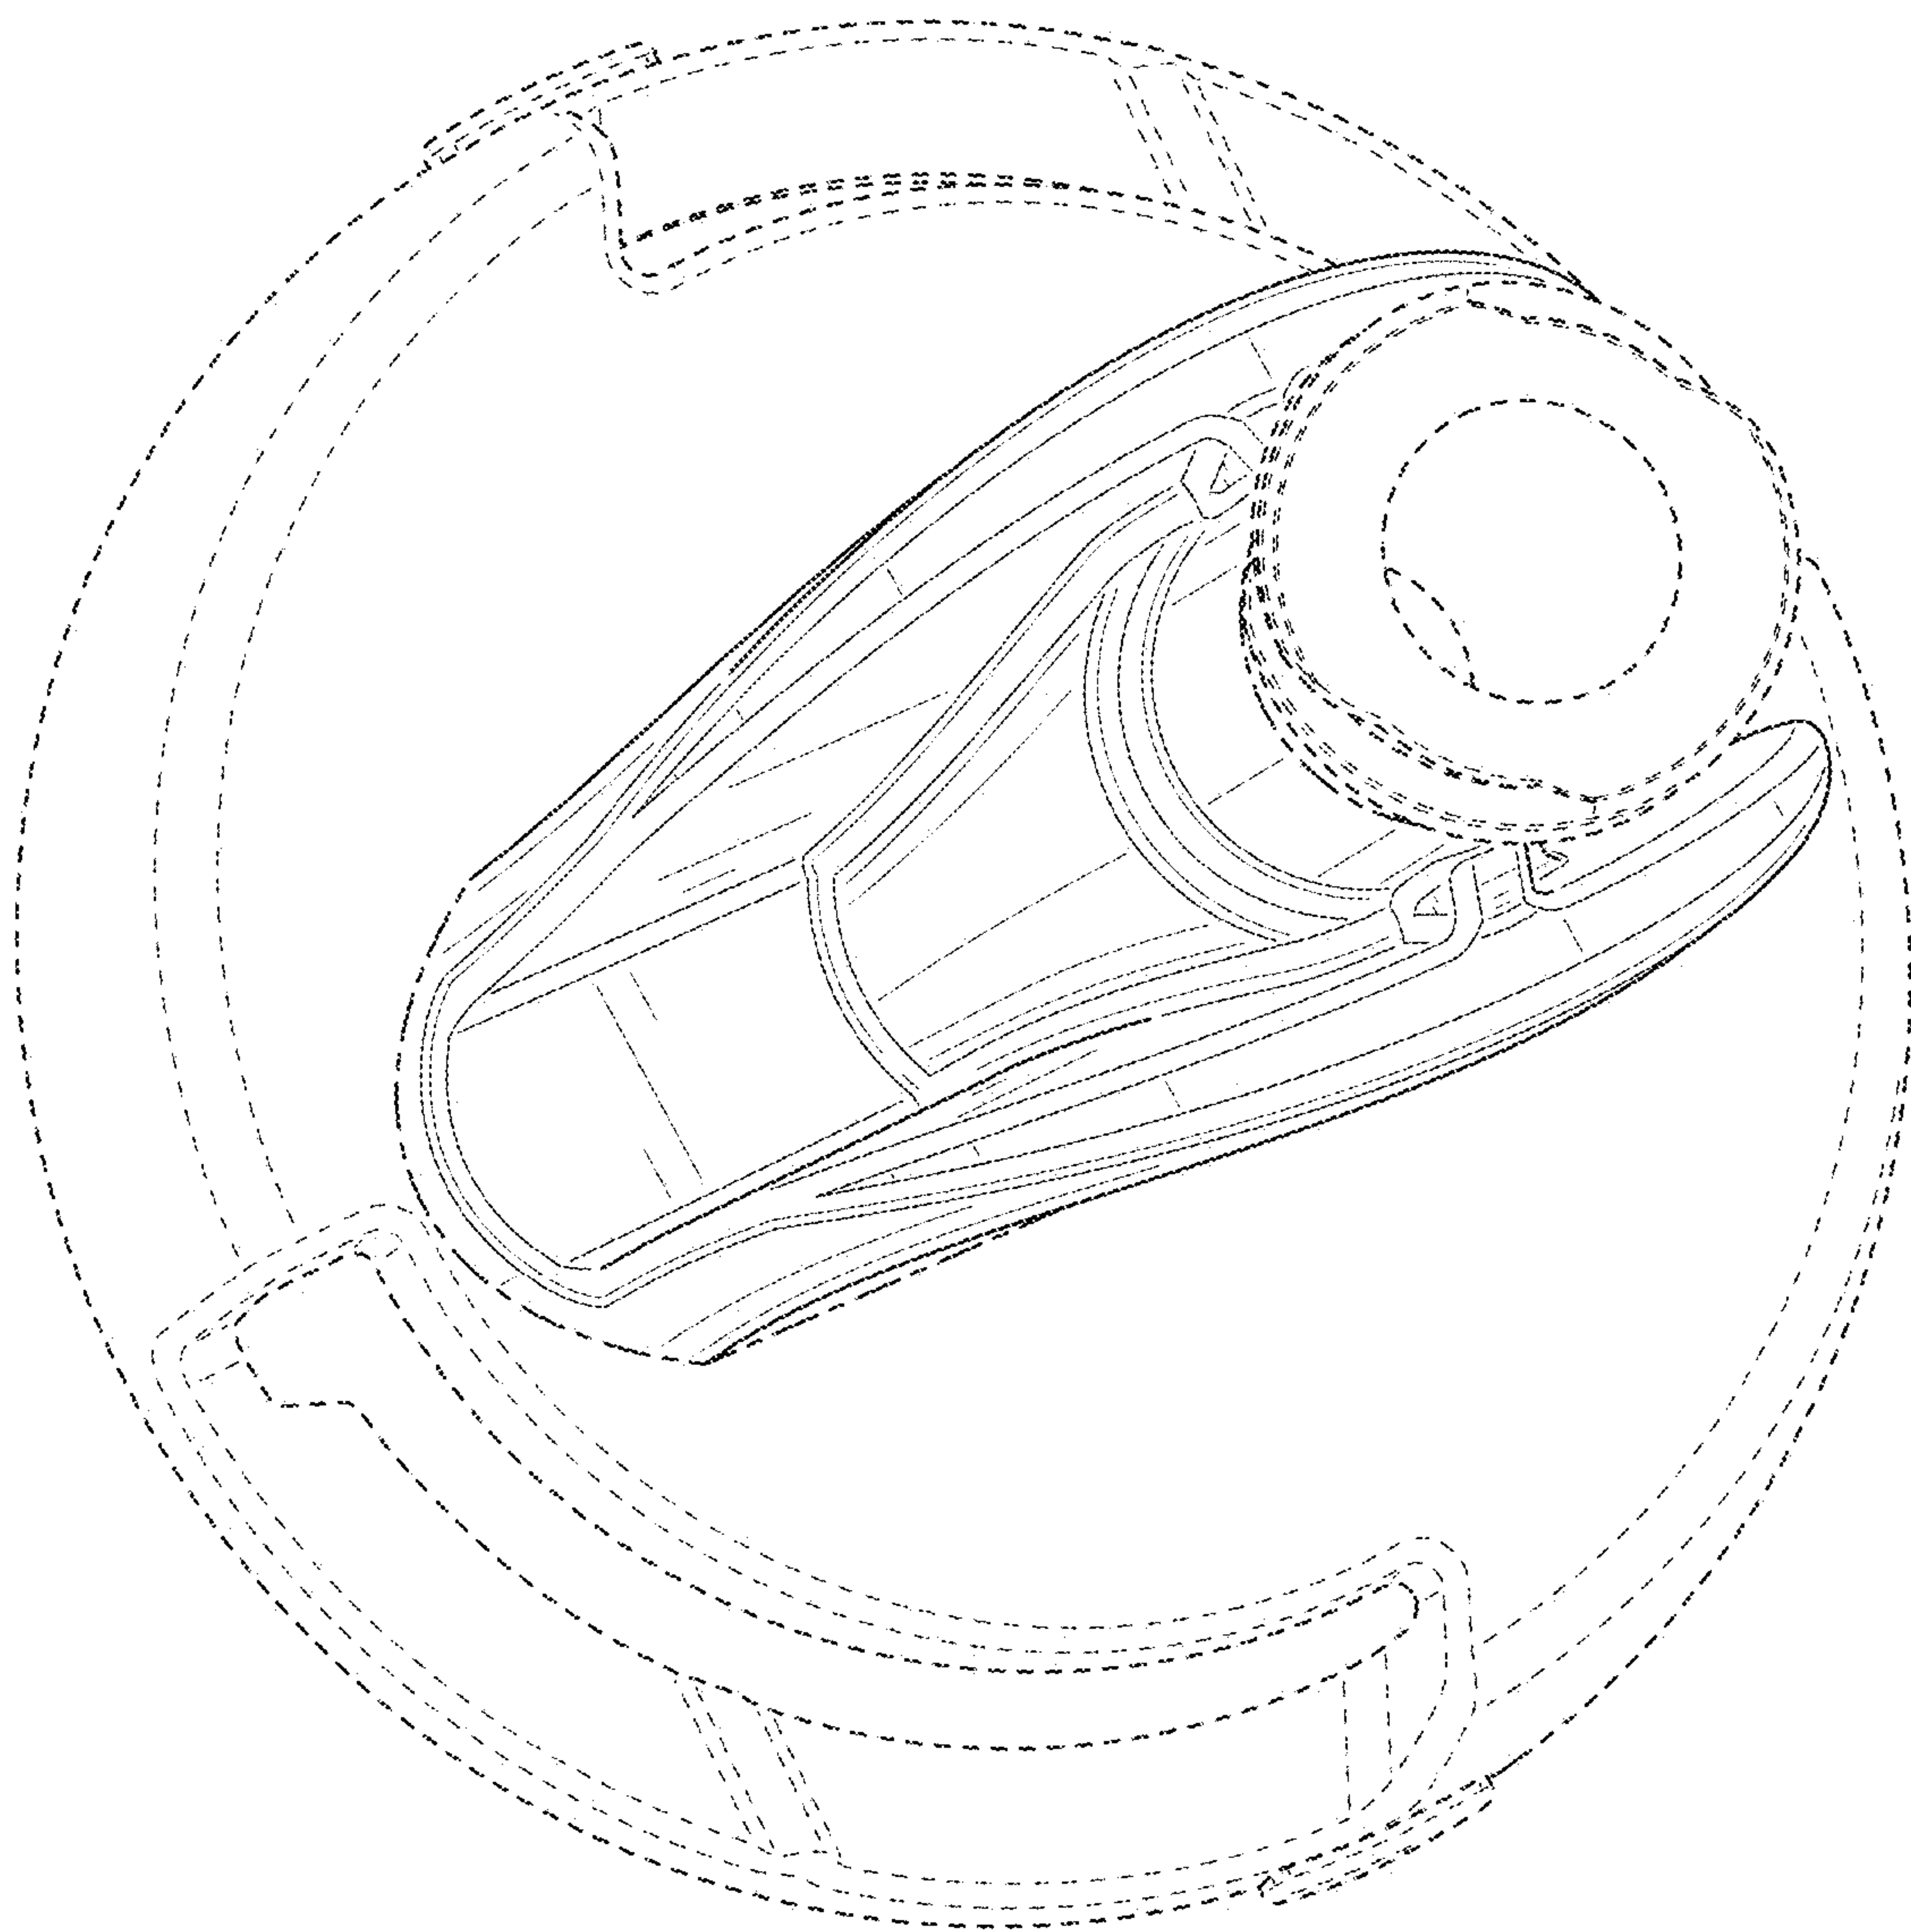


FIG. 2

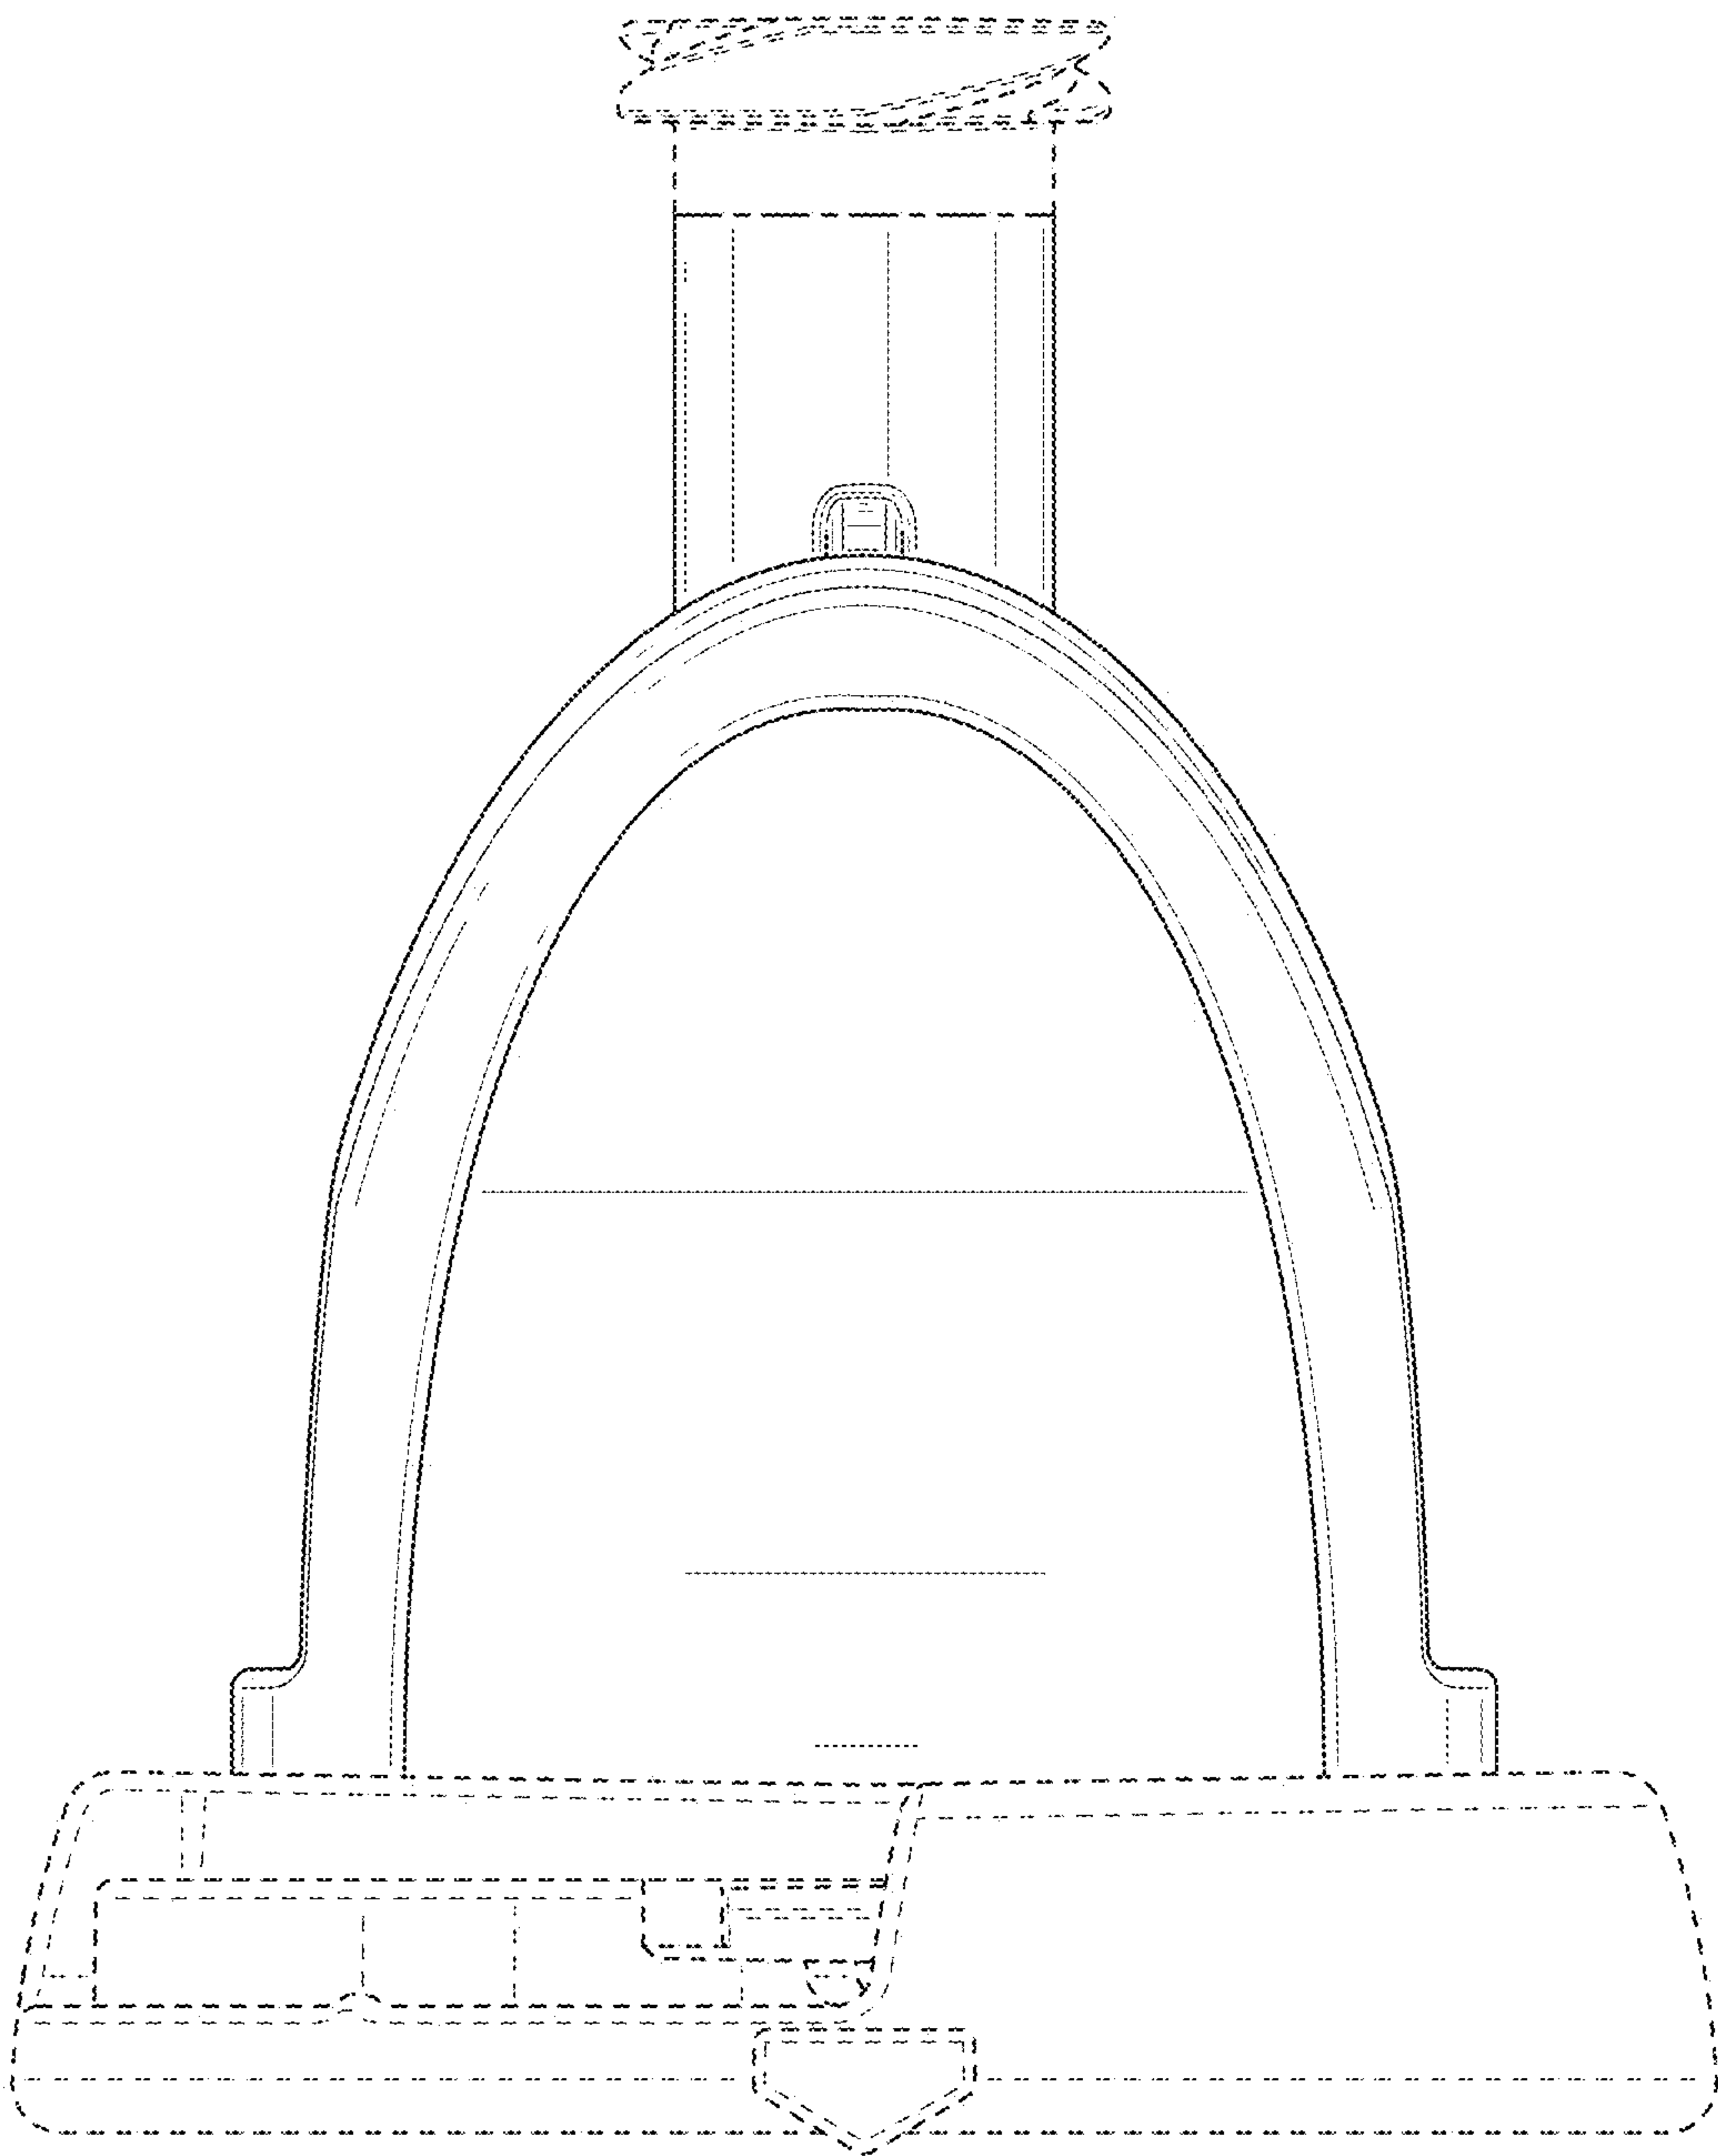


FIG. 3

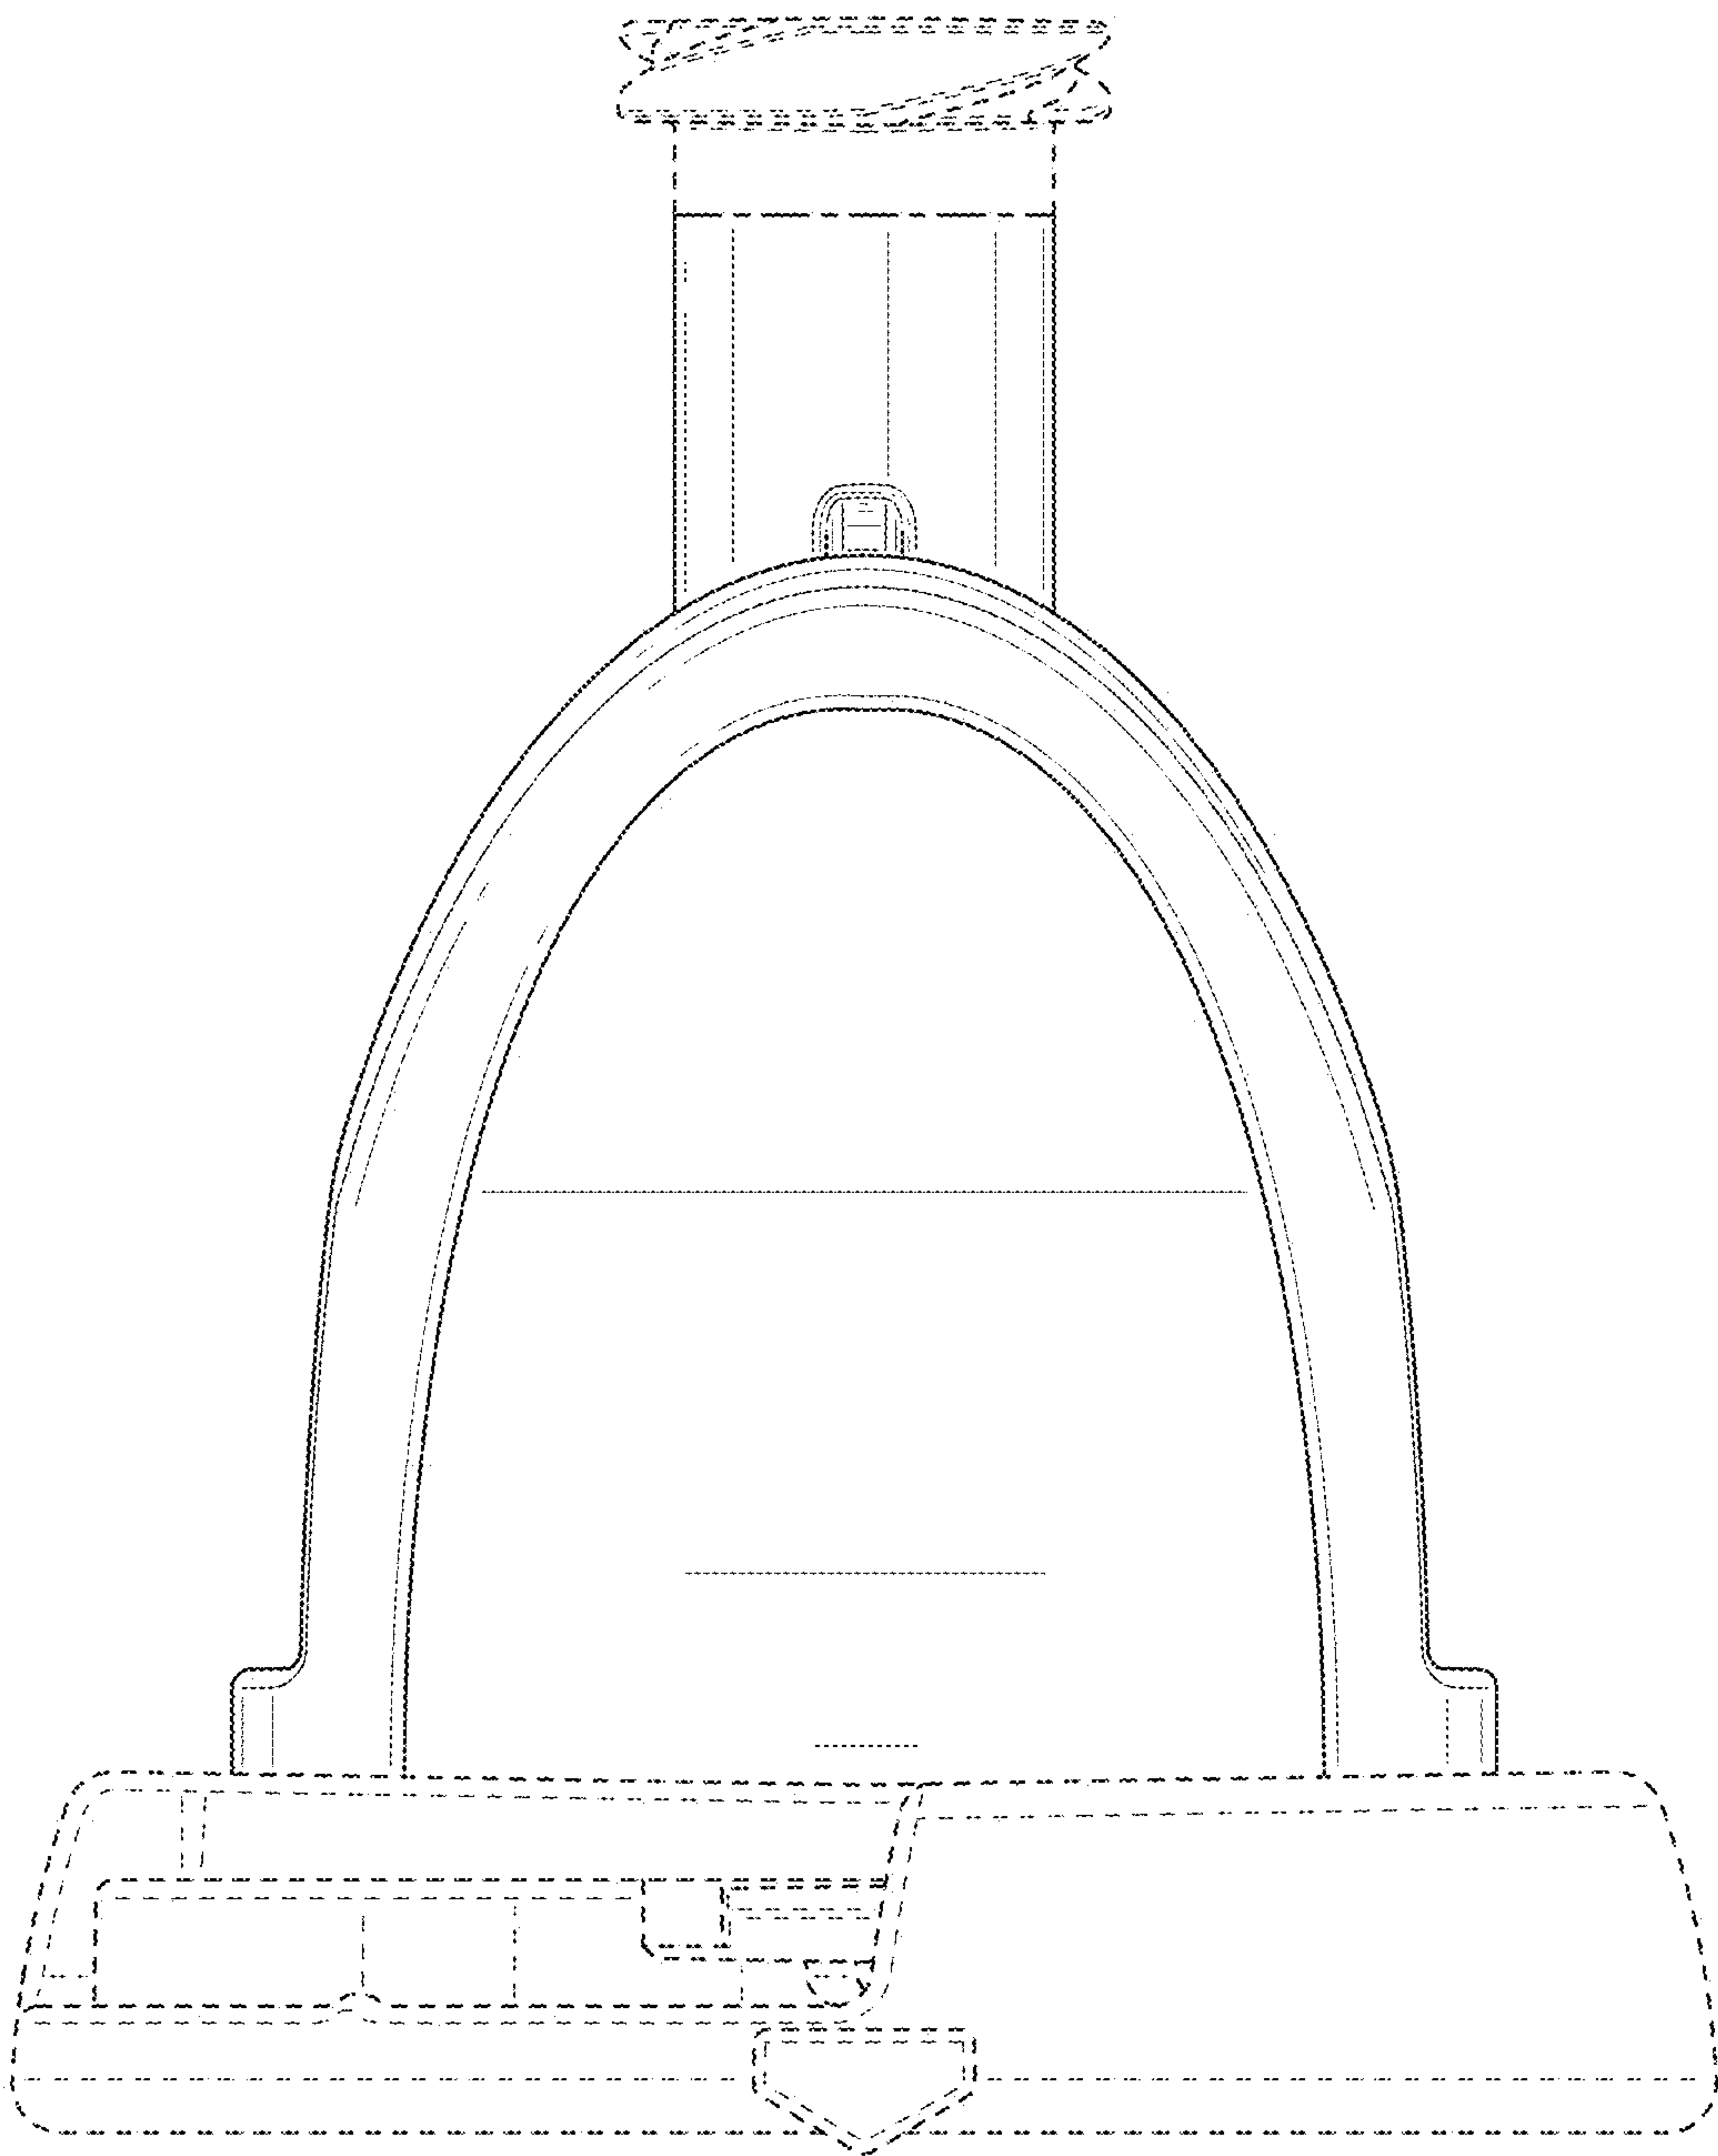


FIG. 4

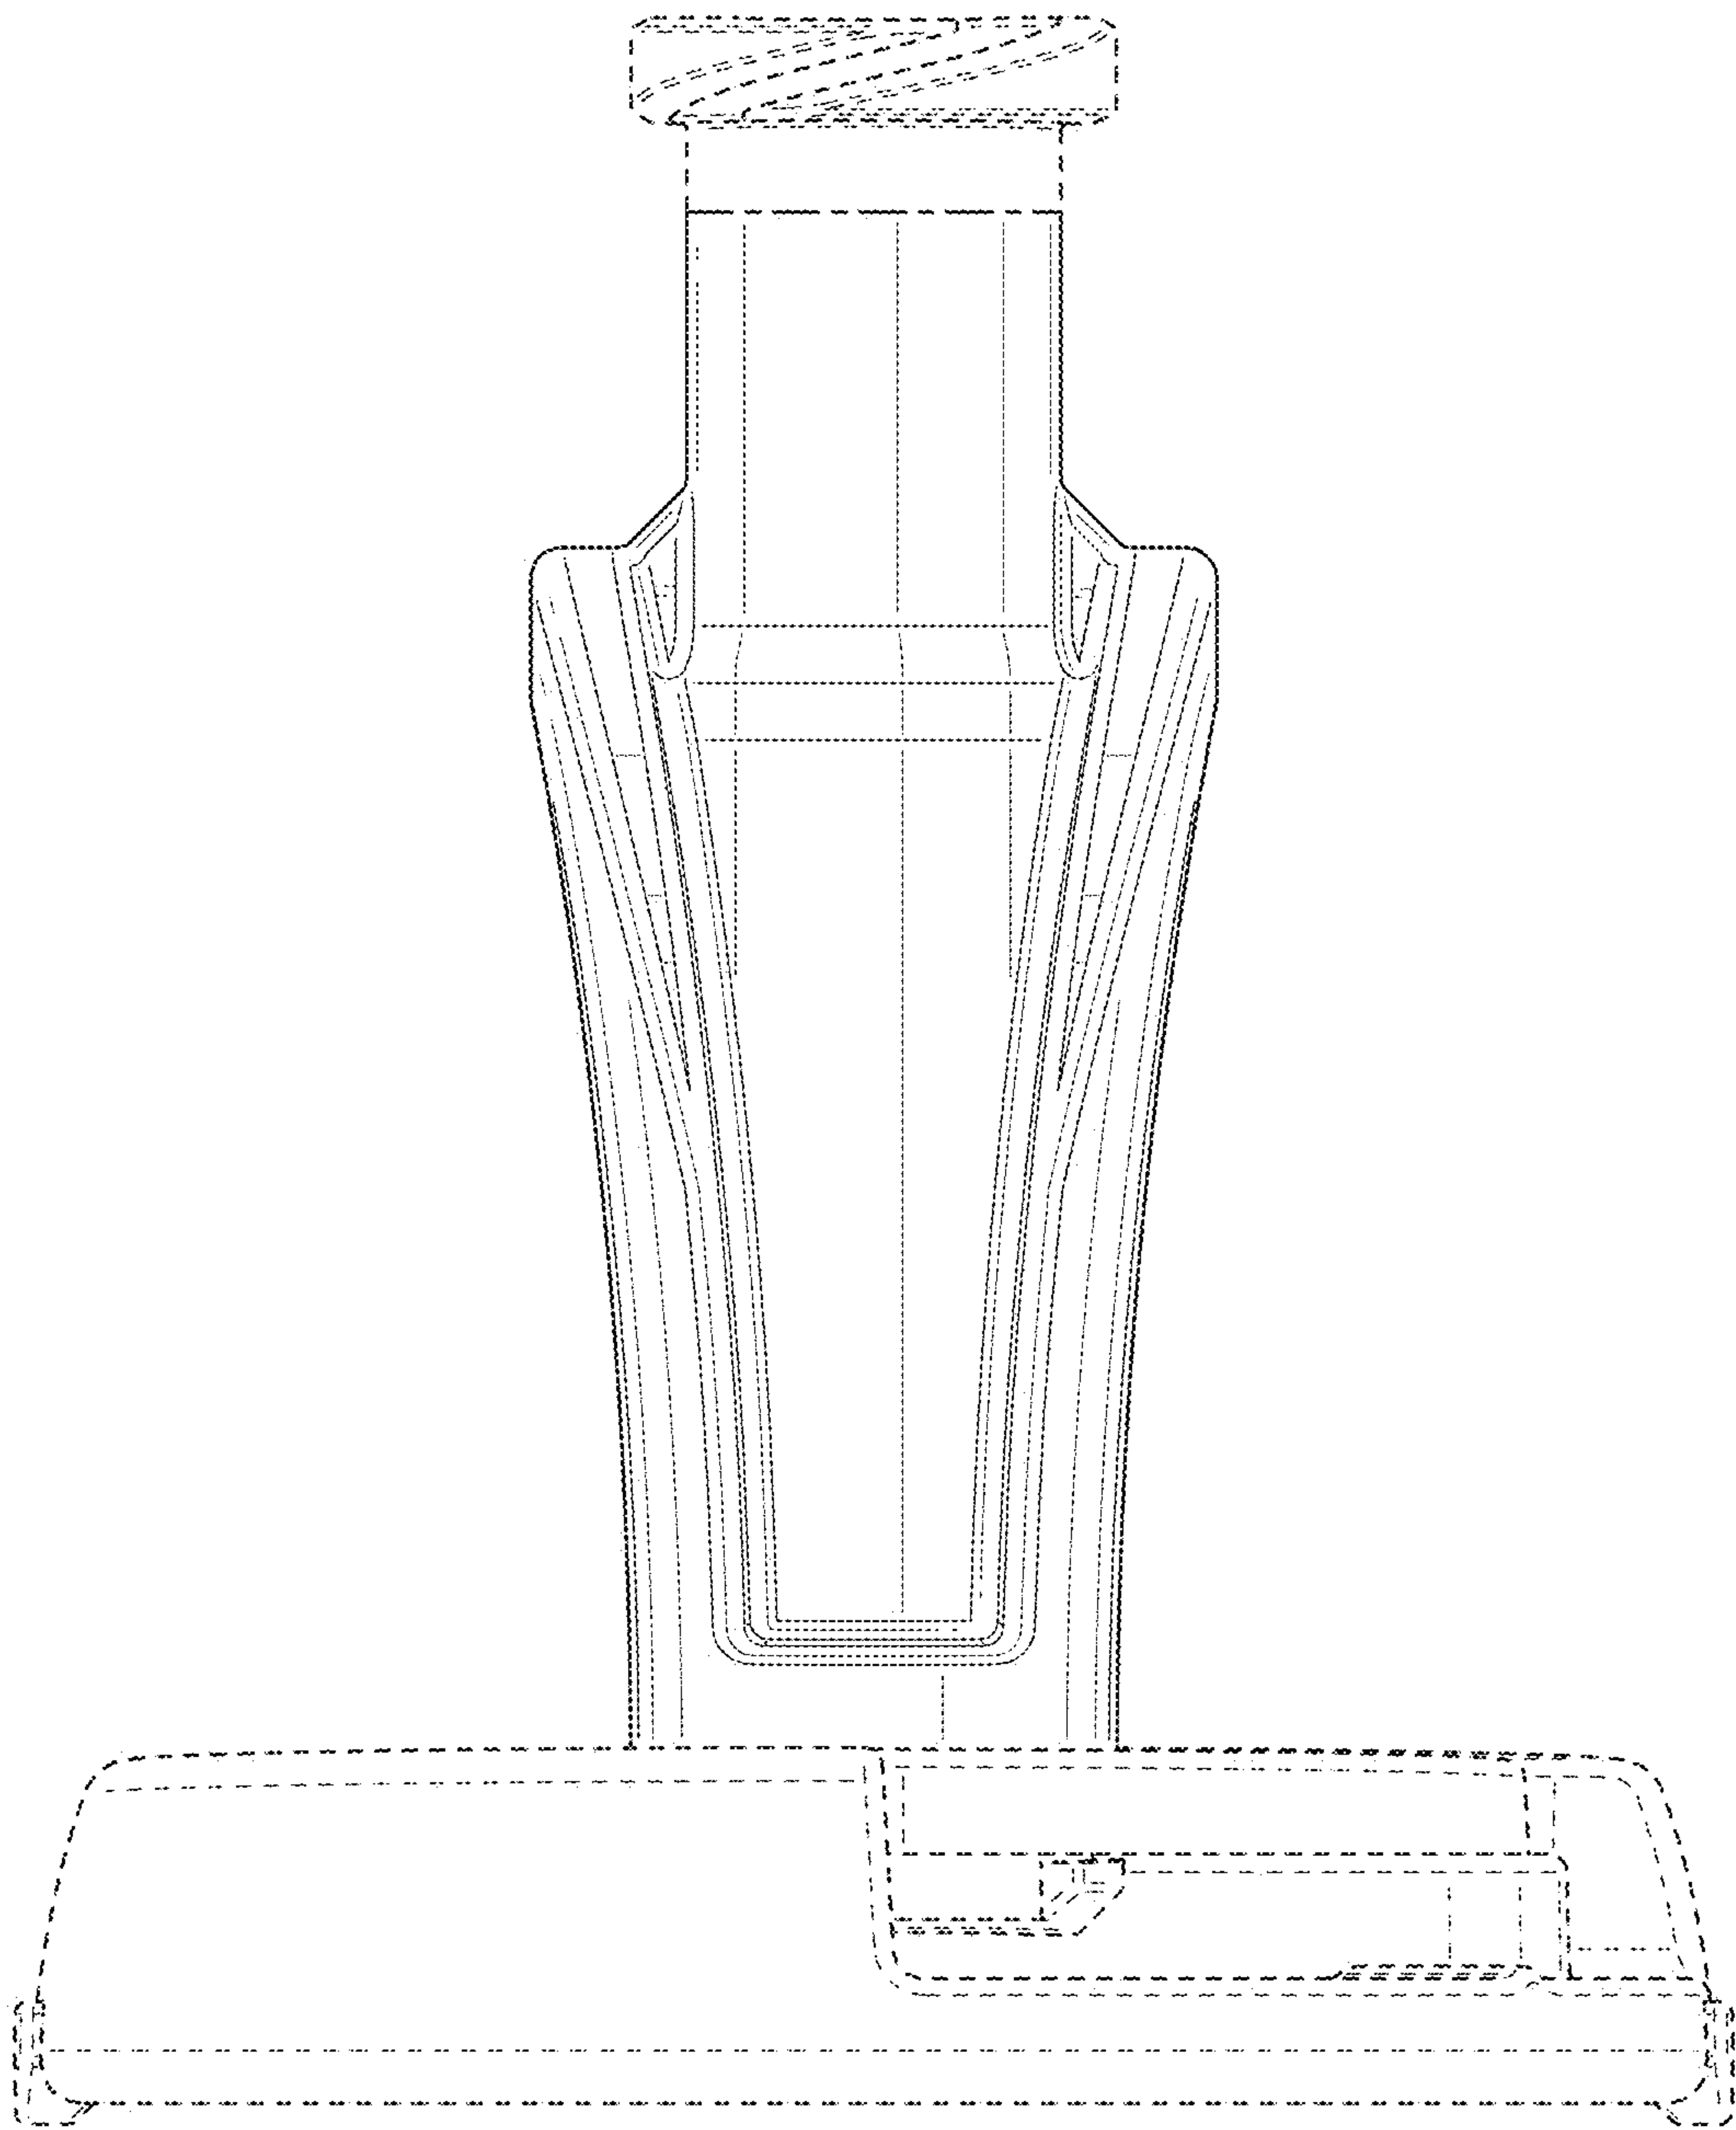


FIG. 5

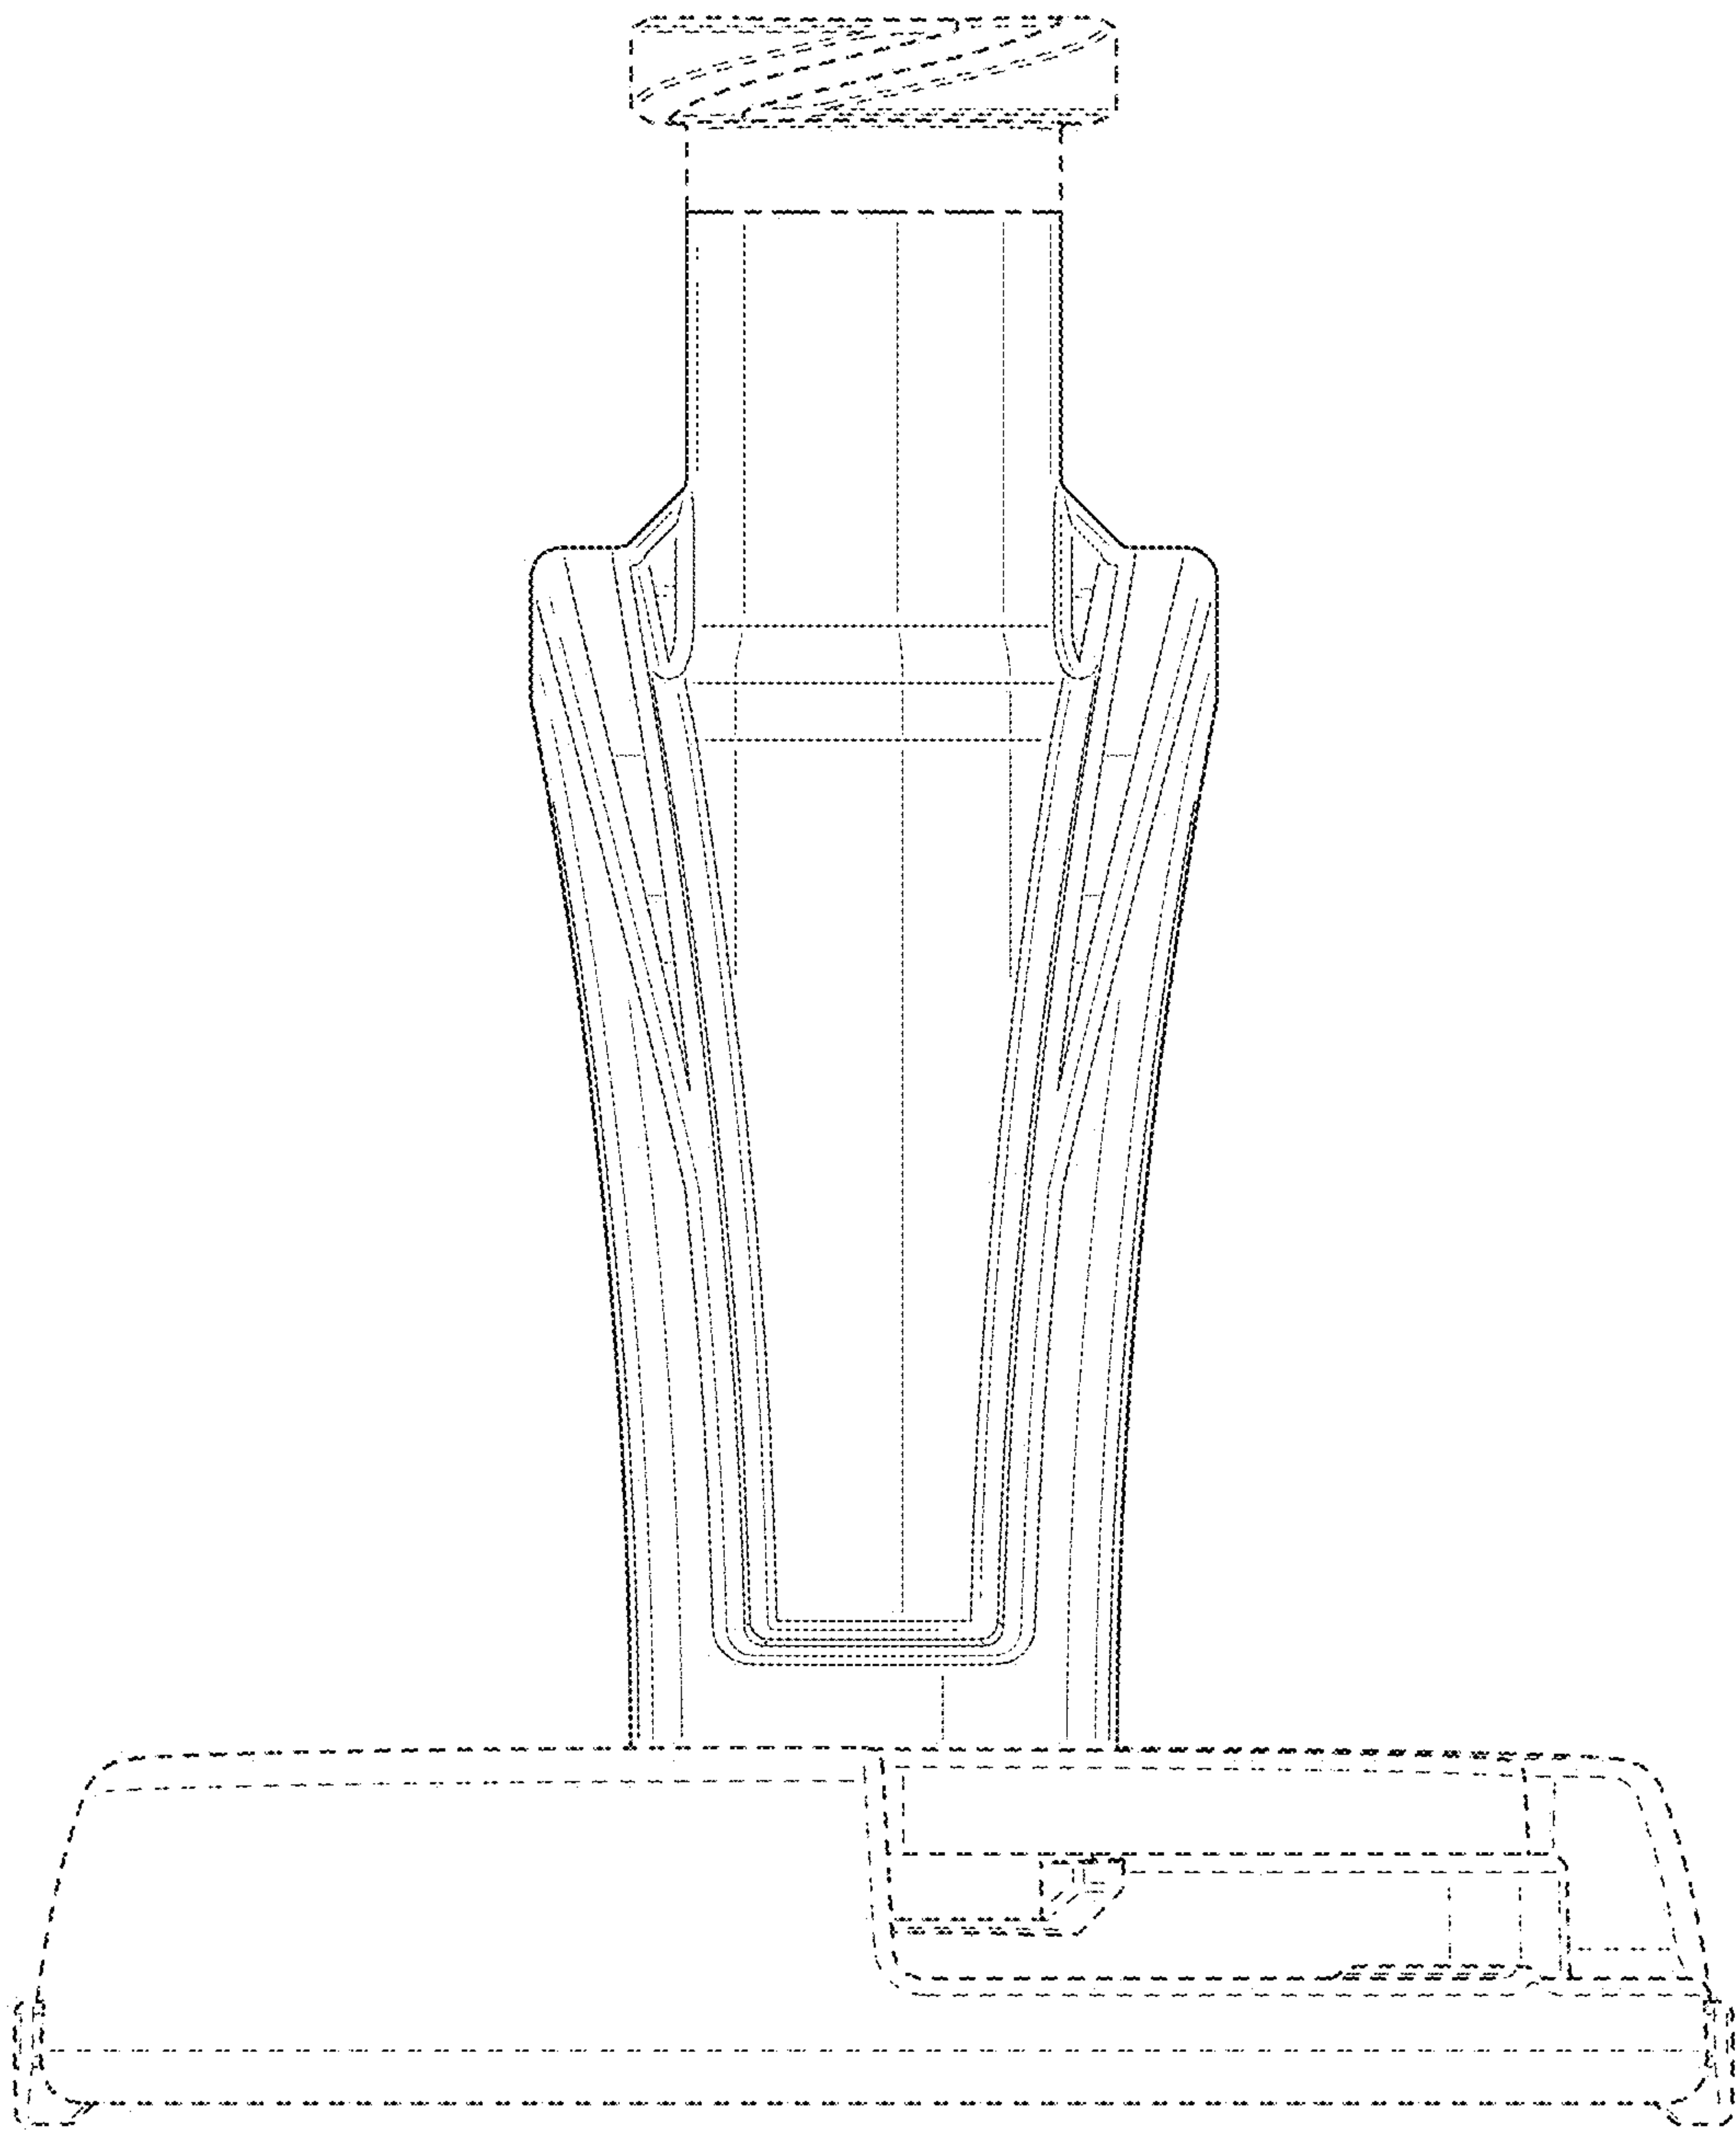


FIG. 6

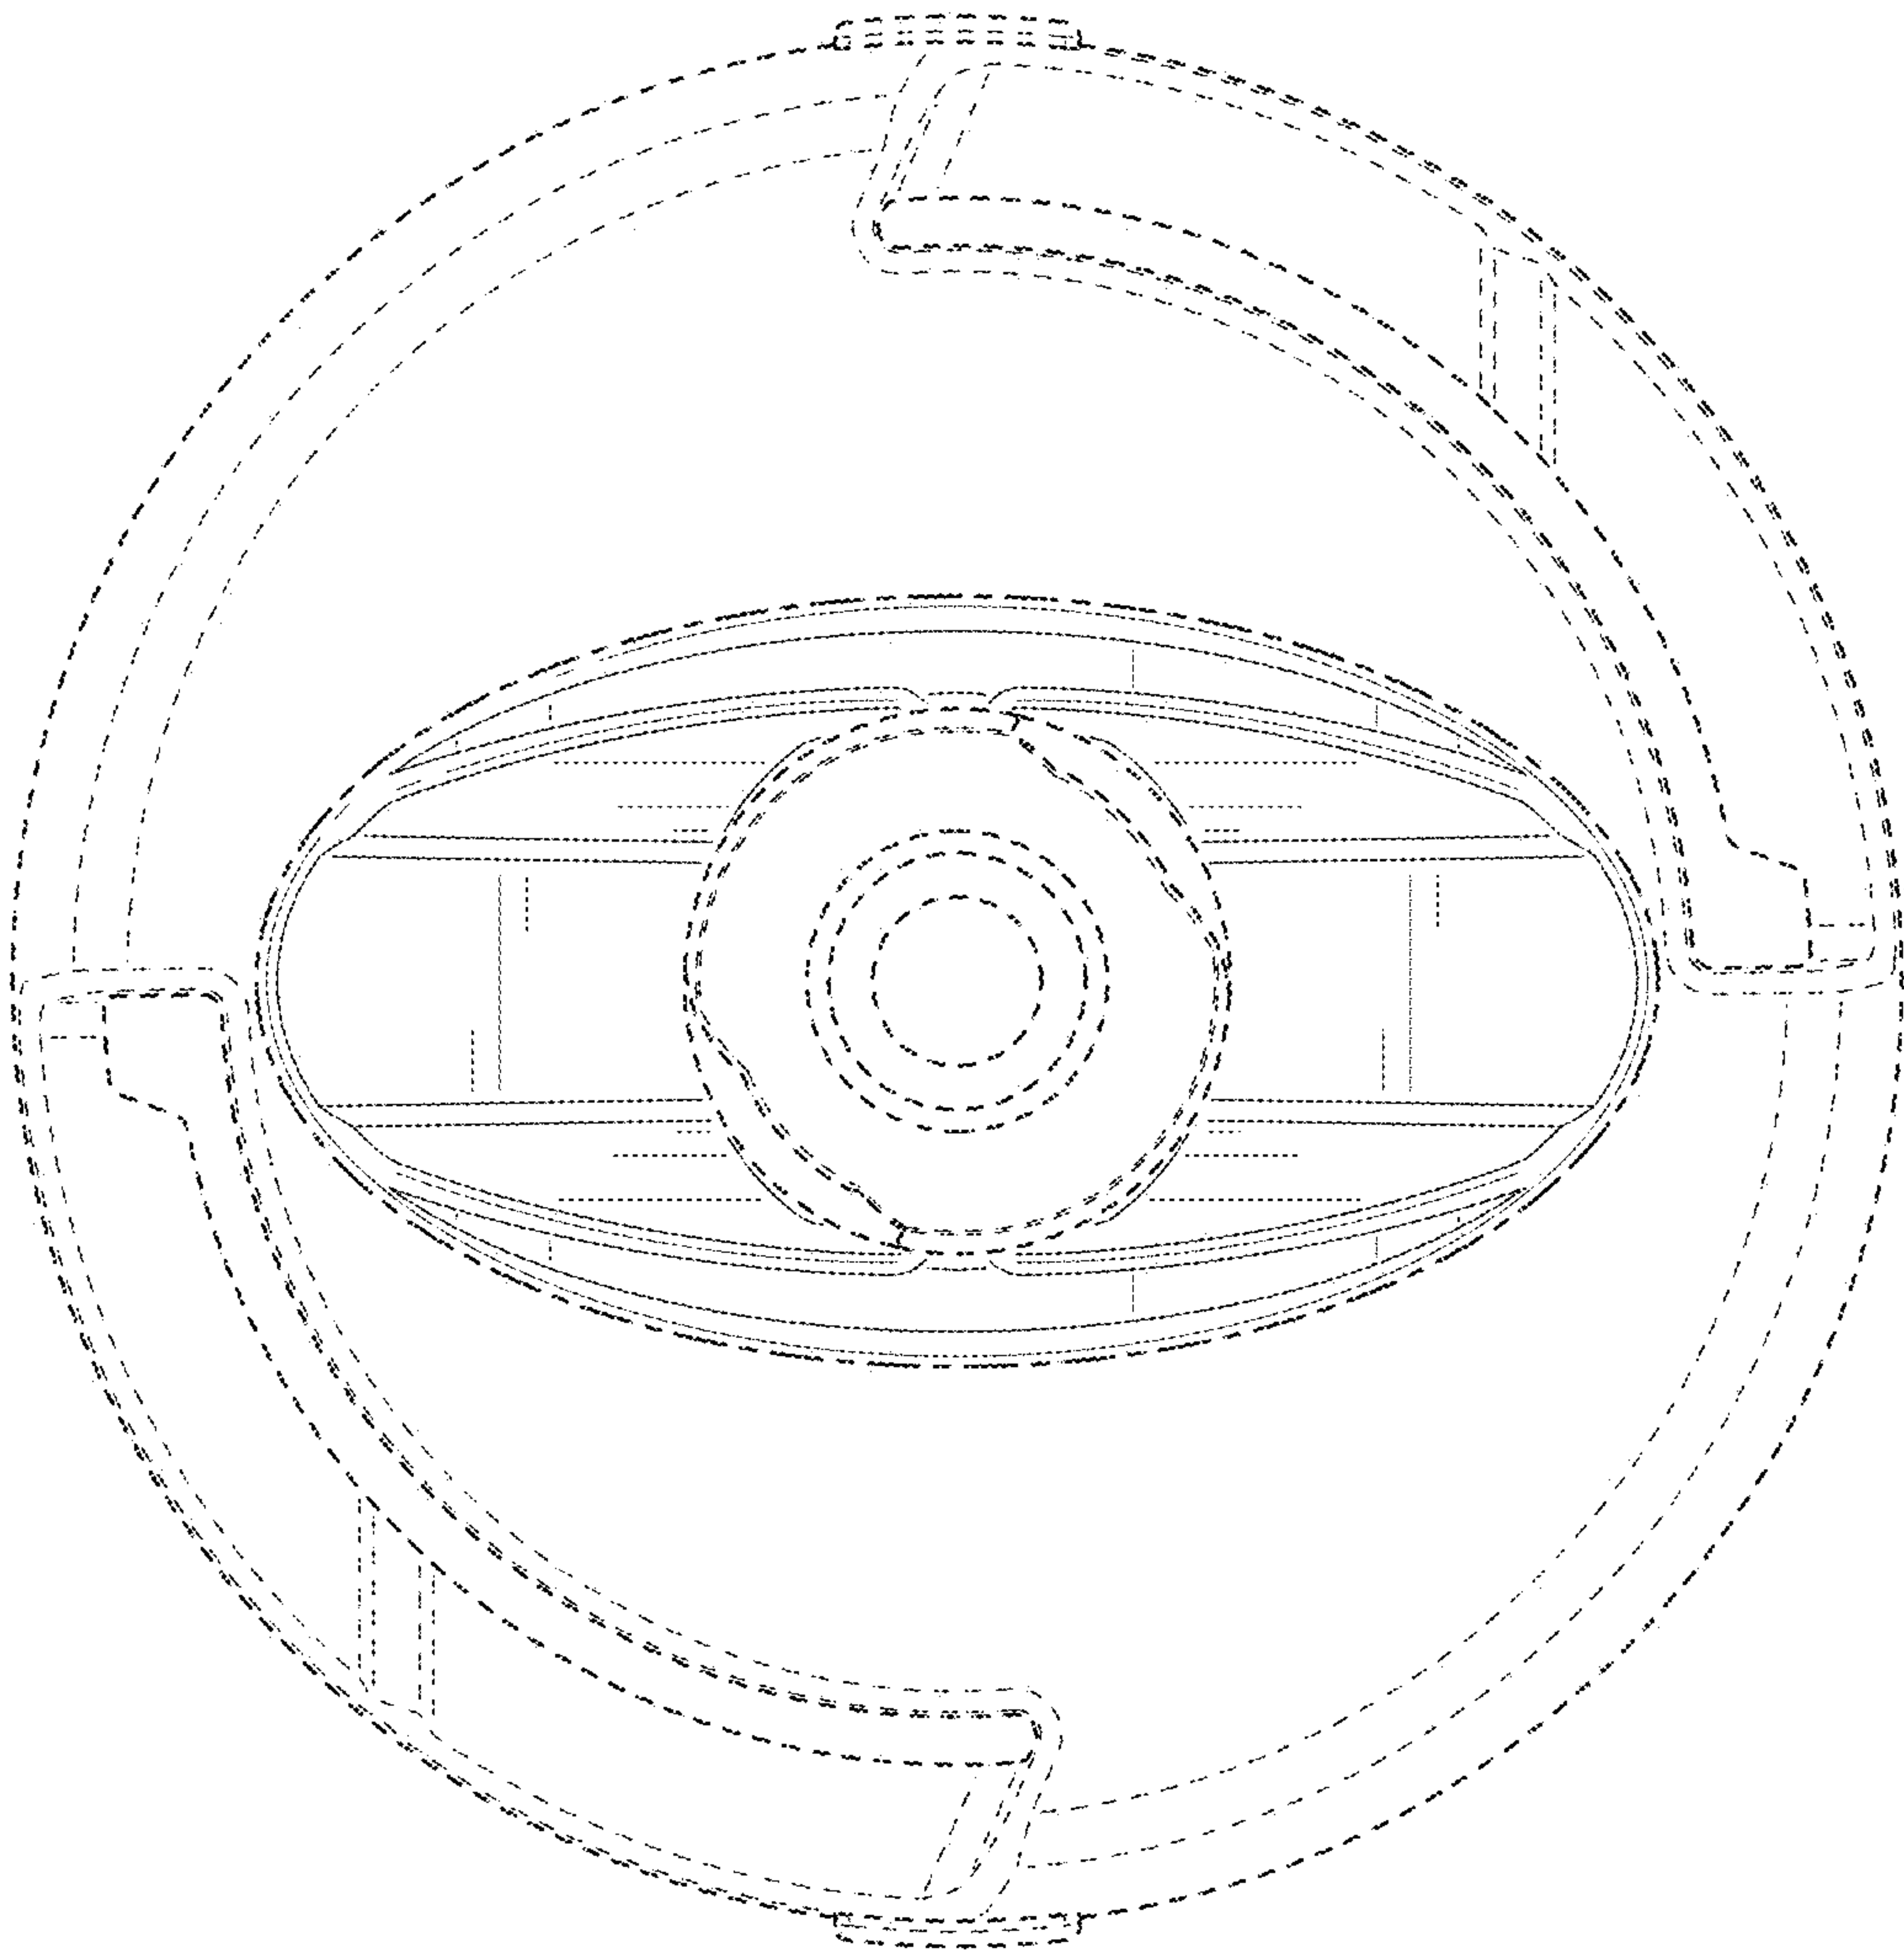


FIG. 7

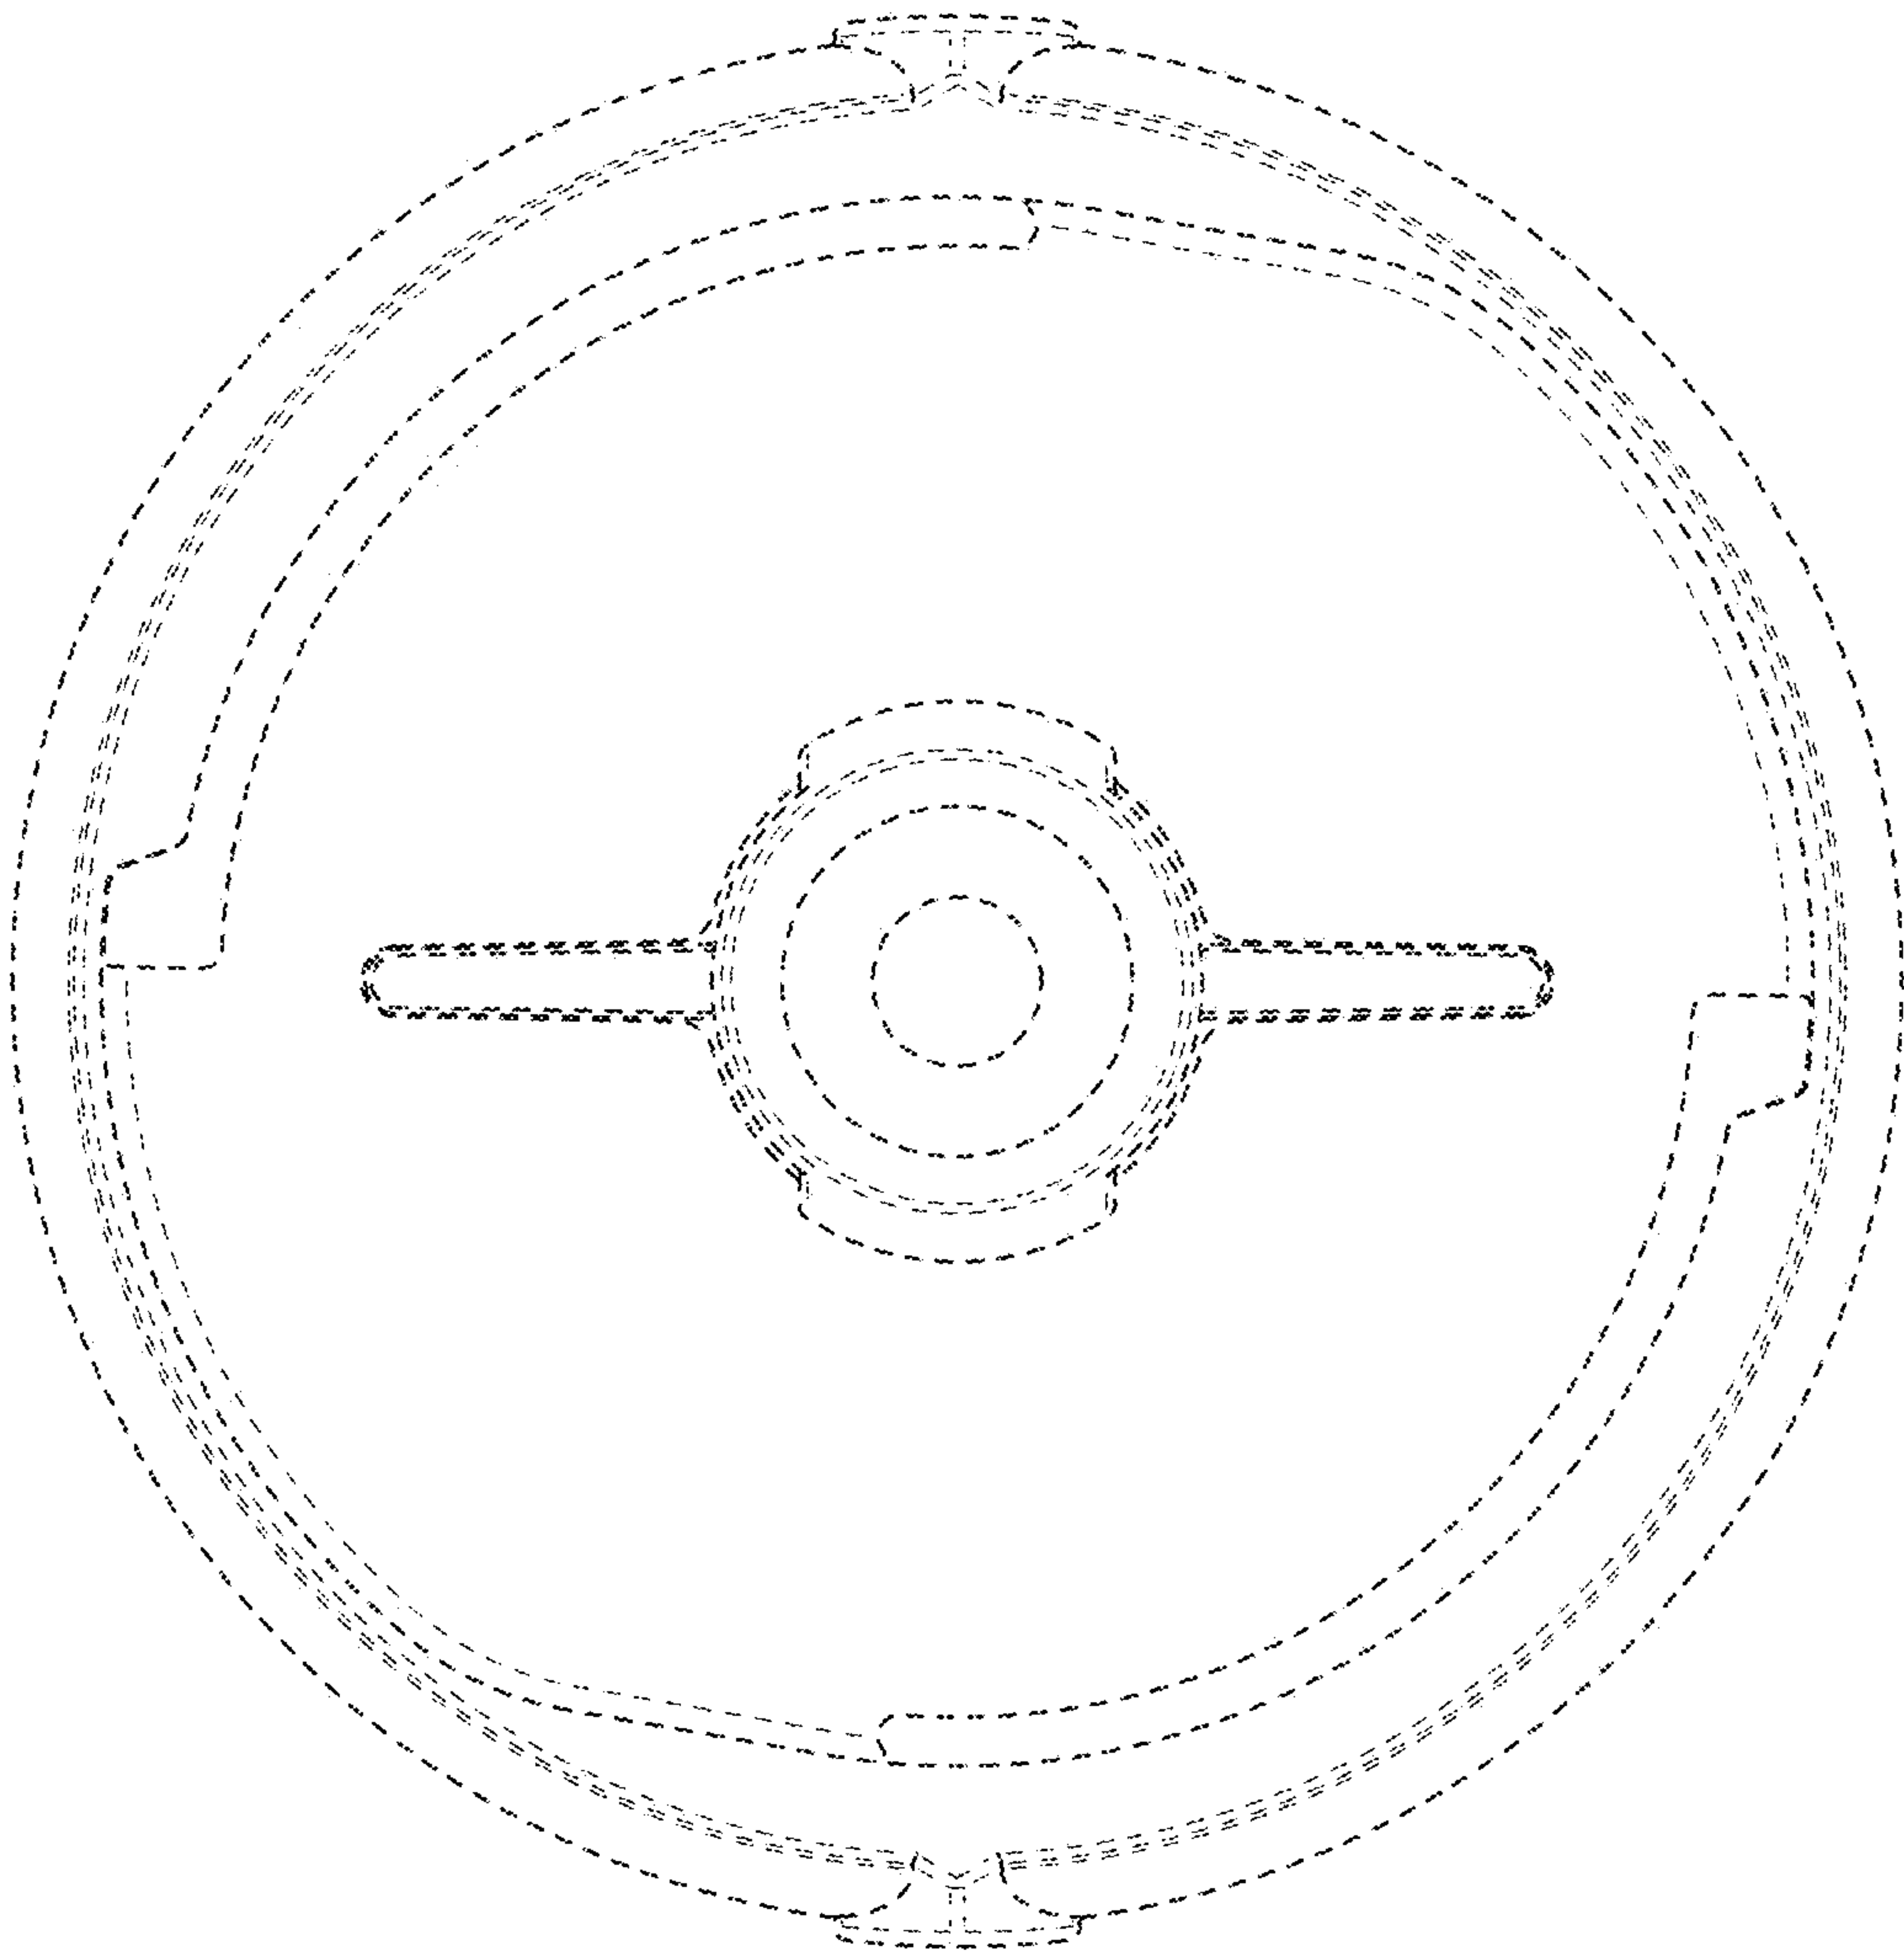


FIG. 8