



US0D1044227S

(12)

United States Design Patent

Zhang et al.

(10)

Patent No.:

US D1,044,227 S

(45)

Date of Patent:

** Oct. 1, 2024

(54) THERAPY SHOE

(71) Applicant: Kinreen Technology (Shenzhen) Co., Ltd., Shenzhen (CN)

(72) Inventors: Qiang Zhang, Shenzhen (CN); Bin Yi, Shenzhen (CN); Bing Hao, Shenzhen (CN); Meihua Gong, Shenzhen (CN); Fubao Cheng, Shenzhen (CN)

(73) Assignee: KINREEN TECHNOLOGY (SHENZHEN) CO., LTD., Shenzhen (CN)

(**) Term: 15 Years

(21) Appl. No.: 29/831,959

(22) Filed: Mar. 24, 2022

(51) LOC (14) Cl. 02-04

(52) U.S. Cl.

USPC D2/923; D24/209; D24/213

(58) Field of Classification Search

USPC D2/896–900, 909–911, 916–947, 951, D2/953, 954, 956, 968–979; D24/192, D24/212, 213, 209

CPC A43B 1/00; A43B 1/02; A43B 1/04; A43B 3/00; A43B 3/02; A43B 3/06; A43B 3/10; A43B 3/12; A43B 3/14; A43B 5/00; A43B 5/001; A43B 5/002; A43B 5/008; A43B 5/06; A43B 5/10; A43B 5/12; A43B 23/00; A43B 23/02; A43B 23/04

See application file for complete search history.

(56) References Cited

U.S. PATENT DOCUMENTS

D244,406	S	*	5/1977	Schonbrun	D2/919
D437,474	S	*	2/2001	Agnew	D2/907
D439,729	S	*	4/2001	Mastroianni	D2/907
D485,664	S	*	1/2004	Bray, Jr.	D2/951
D587,882	S	*	3/2009	Wolf	D2/909
D595,039	S	*	6/2009	Matis	D2/924

D609,886	S	*	2/2010	Murray	D2/923
7,814,680	B2	*	10/2010	Adami	A43B 3/16
					36/45
D639,537	S	*	6/2011	Countee	D2/976
D648,513	S	*	11/2011	McVicker	D2/923

(Continued)

FOREIGN PATENT DOCUMENTS

CN	307270452	*	4/2022
CN	307772473	*	1/2023

OTHER PUBLICATIONS

Neria Med Therapy Device Slipper, NeriaMed.com, [online], [site visited Mar. 5, 2024]. <URL: <https://www.neriamed.com/product-page/therapy-device-slipper>> (Year: 2023).*

(Continued)

Primary Examiner — Jonathan J Han

Assistant Examiner — Molly K. Orzechowski

(57)

CLAIM


The ornamental design for a therapy shoe, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of a therapy shoe showing our new design;
FIG. 2 is a second perspective view thereof;
FIG. 3 is a third perspective view thereof;
FIG. 4 is a right side elevational view thereof;
FIG. 5 is a left side elevational view thereof;
FIG. 6 is a front elevational view thereof;
FIG. 7 is a rear elevational view thereof;
FIG. 8 is a top plan view thereof; and,
FIG. 9 is a bottom plan view thereof.

The broken lines in the drawings are for the purpose of illustrating portions of the therapy shoe that form no part of the claimed design.

1 Claim, 9 Drawing Sheets

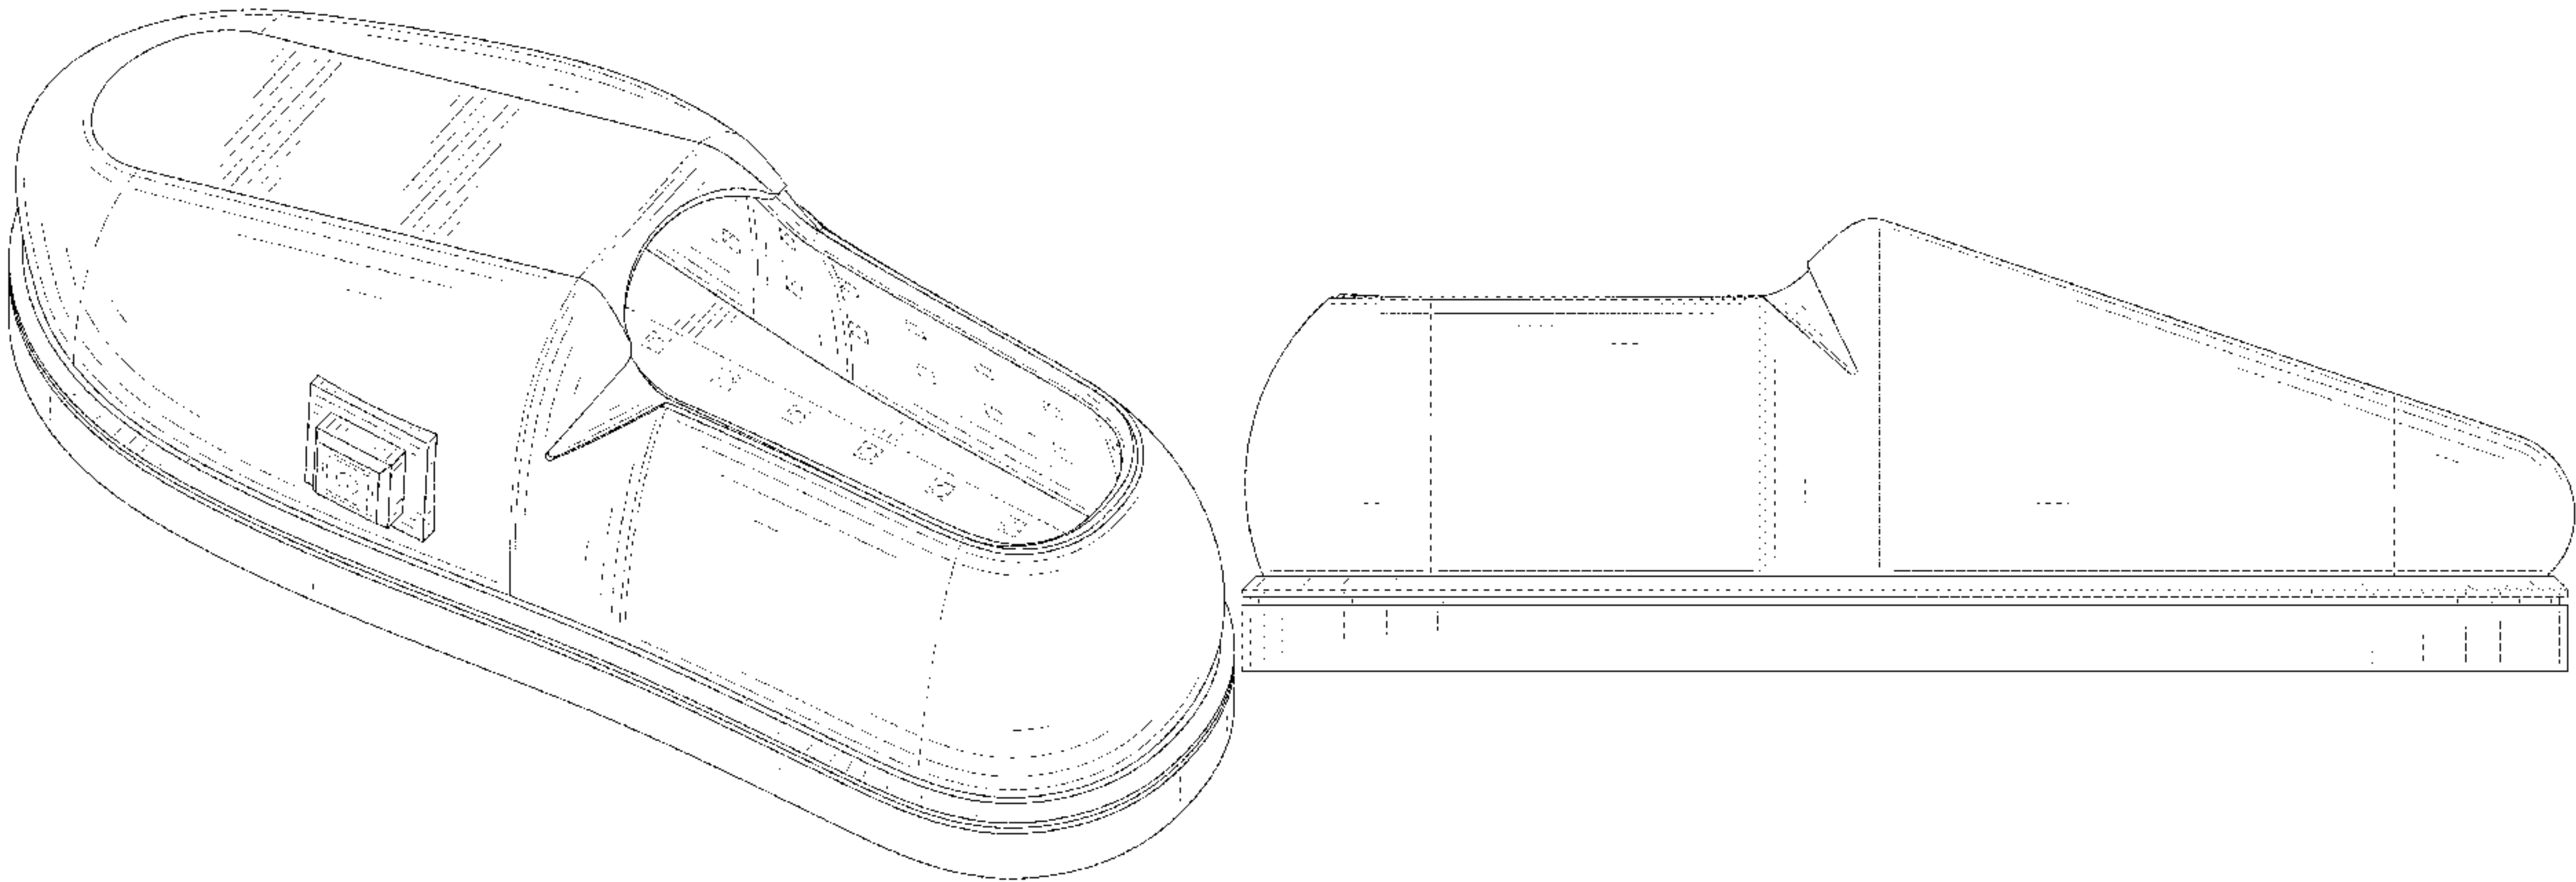

(56)

References Cited

U.S. PATENT DOCUMENTS

D661,884 S * 6/2012 Raysse D2/969
D685,170 S * 7/2013 Raysse D2/969
D688,446 S * 8/2013 Raysse D2/969
D690,488 S * 10/2013 Reed D2/942
D707,426 S * 6/2014 Lu D2/909
D720,920 S * 1/2015 Santos D2/923
D723,252 S * 3/2015 VanHorn D2/923
D723,788 S * 3/2015 Raysse D2/971
D787,165 S * 5/2017 Sassi D2/896
D793,679 S * 8/2017 Maier D2/969
D799,175 S * 10/2017 Leva D2/923
D801,012 S * 10/2017 Negra D2/923
D809,754 S * 2/2018 Kim D2/923
D813,505 S * 3/2018 Brown D2/896
D822,972 S * 7/2018 Lam D2/969
D825,900 S * 8/2018 Maier D2/969
D841,947 S * 3/2019 Grinstead D2/919
D858,047 S * 9/2019 Tæstensen D2/923
D869,828 S * 12/2019 El Rufaie D2/923
D876,785 S * 3/2020 Brown D2/969
D877,464 S * 3/2020 Phillips D2/900

D884,317 S * 5/2020 Hawthornthwaite D2/923
D891,046 S * 7/2020 Jenkins D2/939
D942,130 S * 2/2022 Teoh D2/919
D948,180 S * 4/2022 Lai D2/944
D960,534 S * 8/2022 Dunham D2/900
D960,540 S * 8/2022 Storch D2/923
D984,103 S * 4/2023 Zhang D2/957
D989,453 S * 6/2023 Lee D2/923
D995,999 S * 8/2023 Ding D2/896
D997,523 S * 9/2023 Yung D2/969
D1,000,764 S * 10/2023 Huang D2/924
D1,003,575 S * 11/2023 Mayhew D2/903
D1,011,705 S * 1/2024 Zhang D2/903
D1,013,336 S * 2/2024 García Pérez D2/923
D1,027,192 S * 5/2024 Liu D24/192

OTHER PUBLICATIONS

Talsafe 660nm LED Red Light and 880nm Near Infrared Light Therapy Devices Slippers, Amazon.com, [online], [site visited Mar. 5, 2024]. <URL: <https://www.amazon.com/TUOB-Infrared-Slippers-Physical-Administer/dp/B08GPMFD8S?th=1>> (Year: 2020).*

* cited by examiner

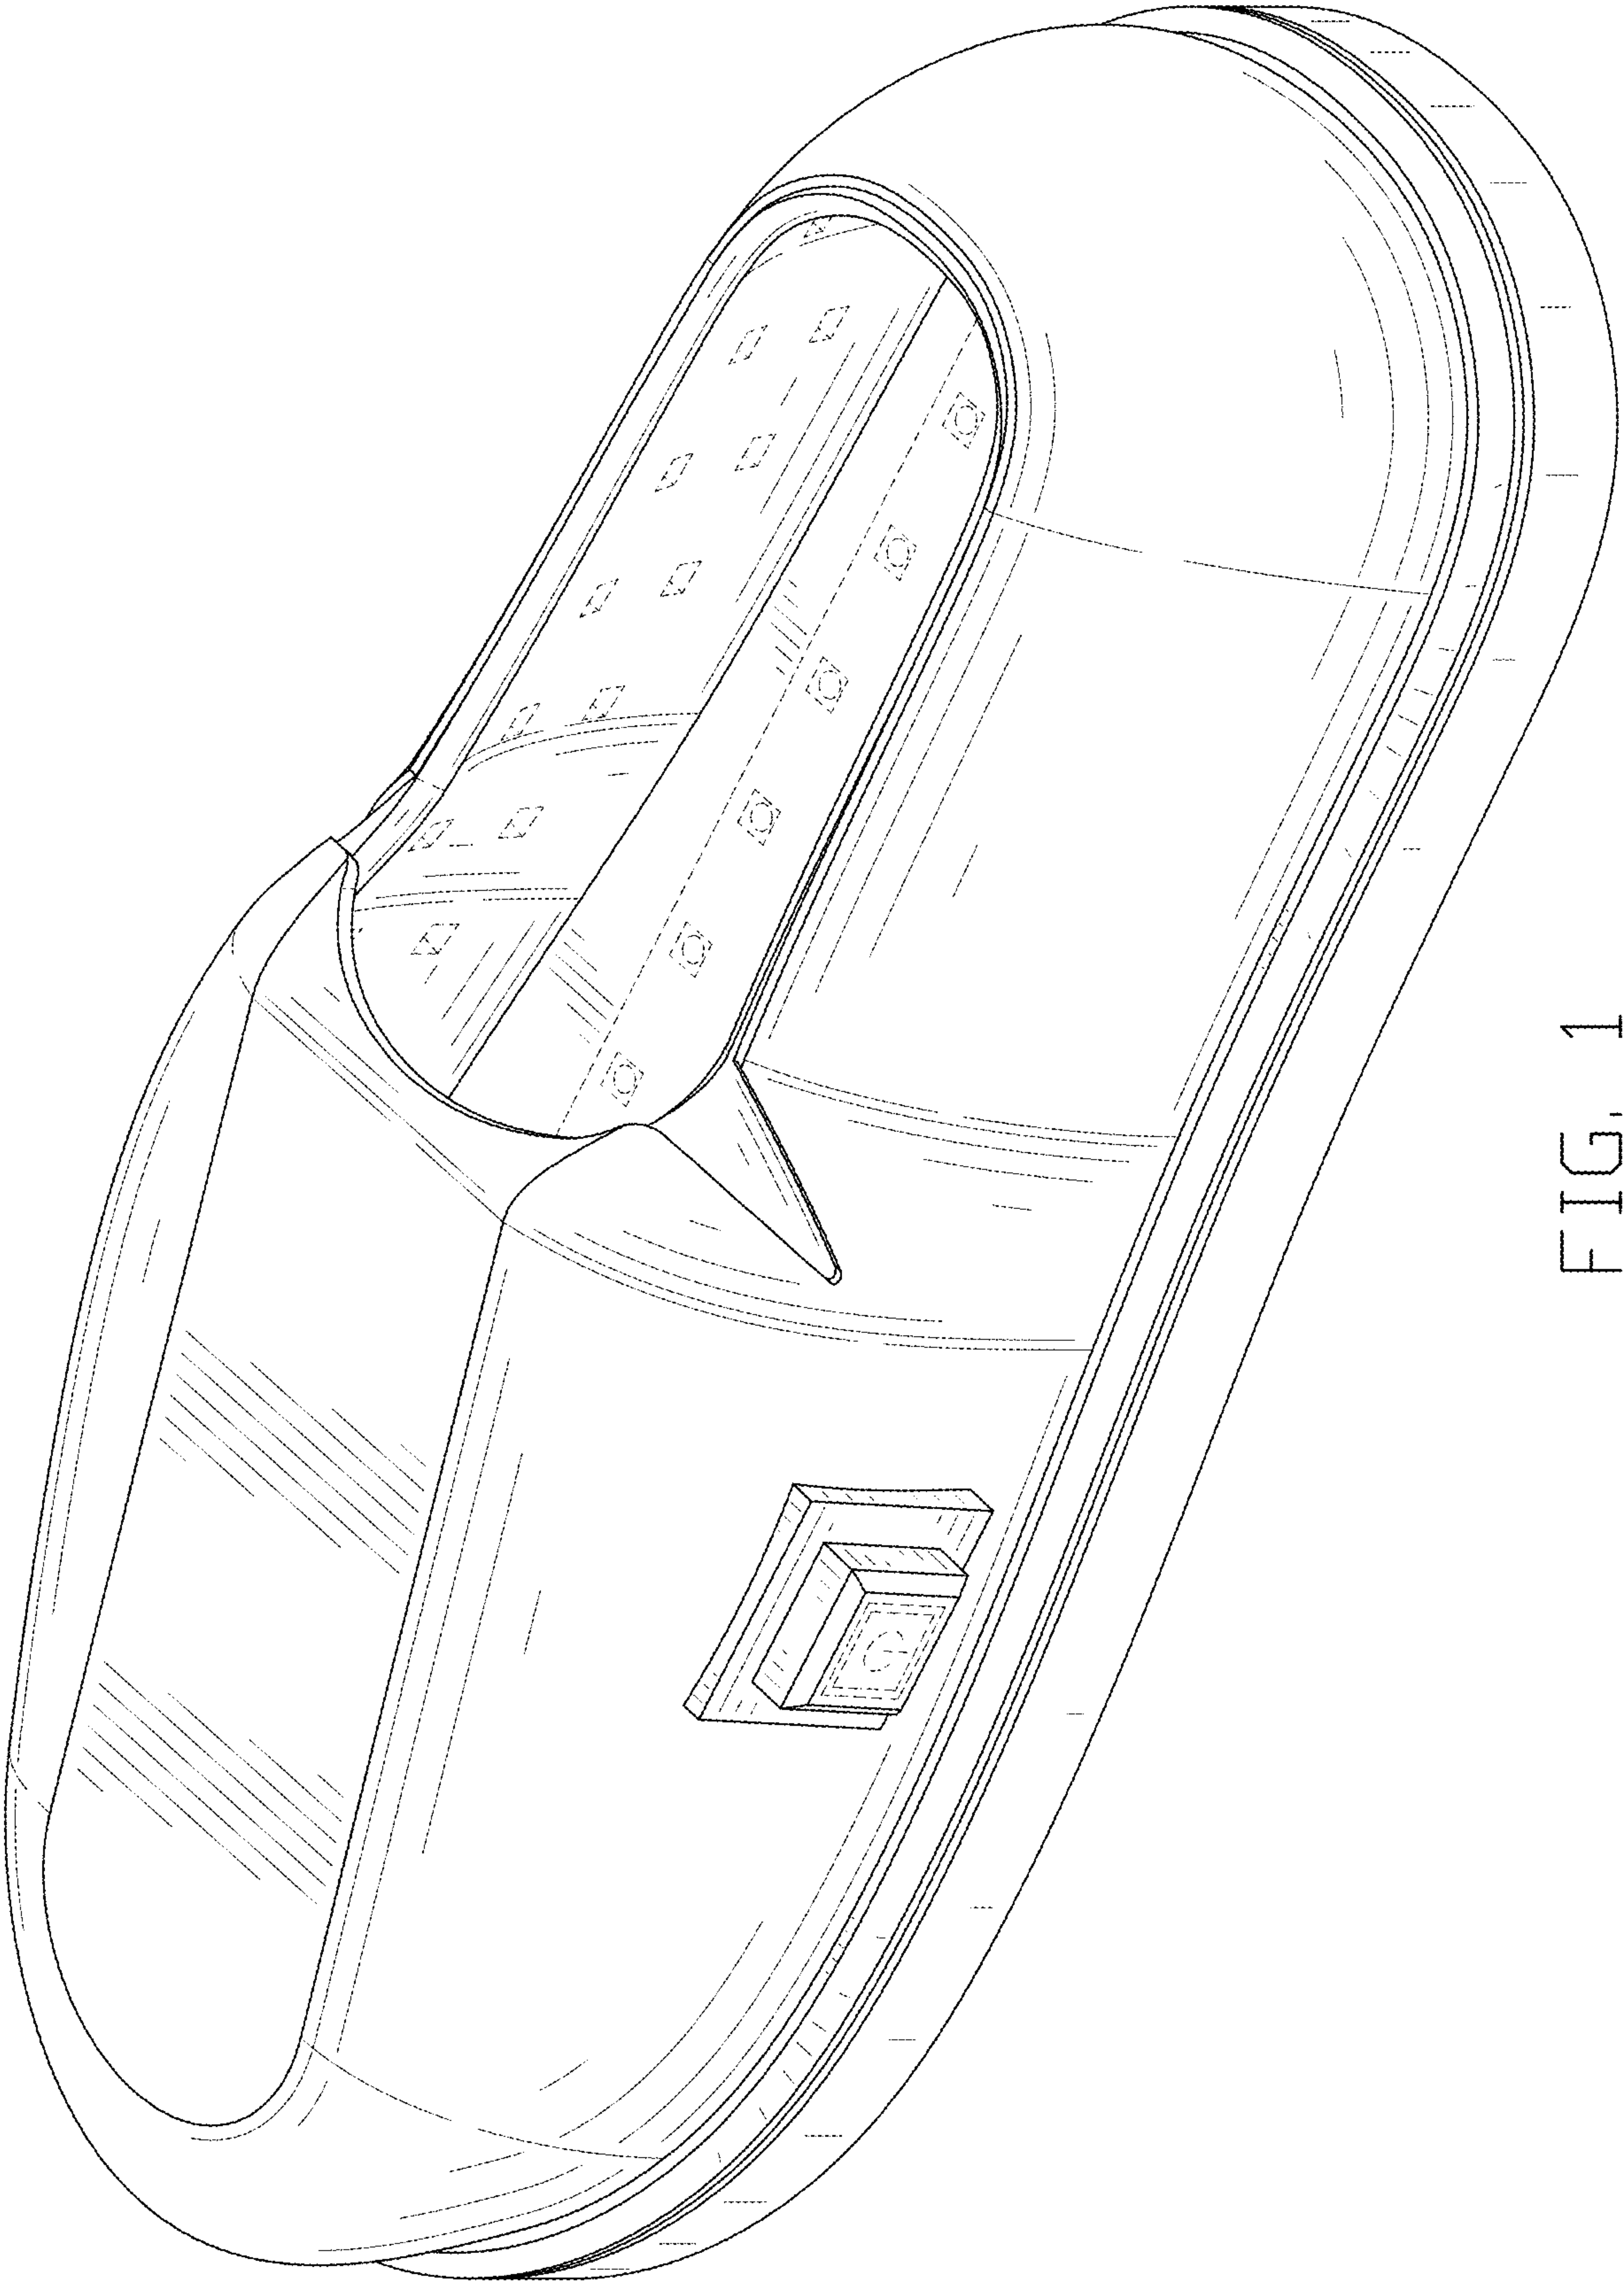


FIG. 1

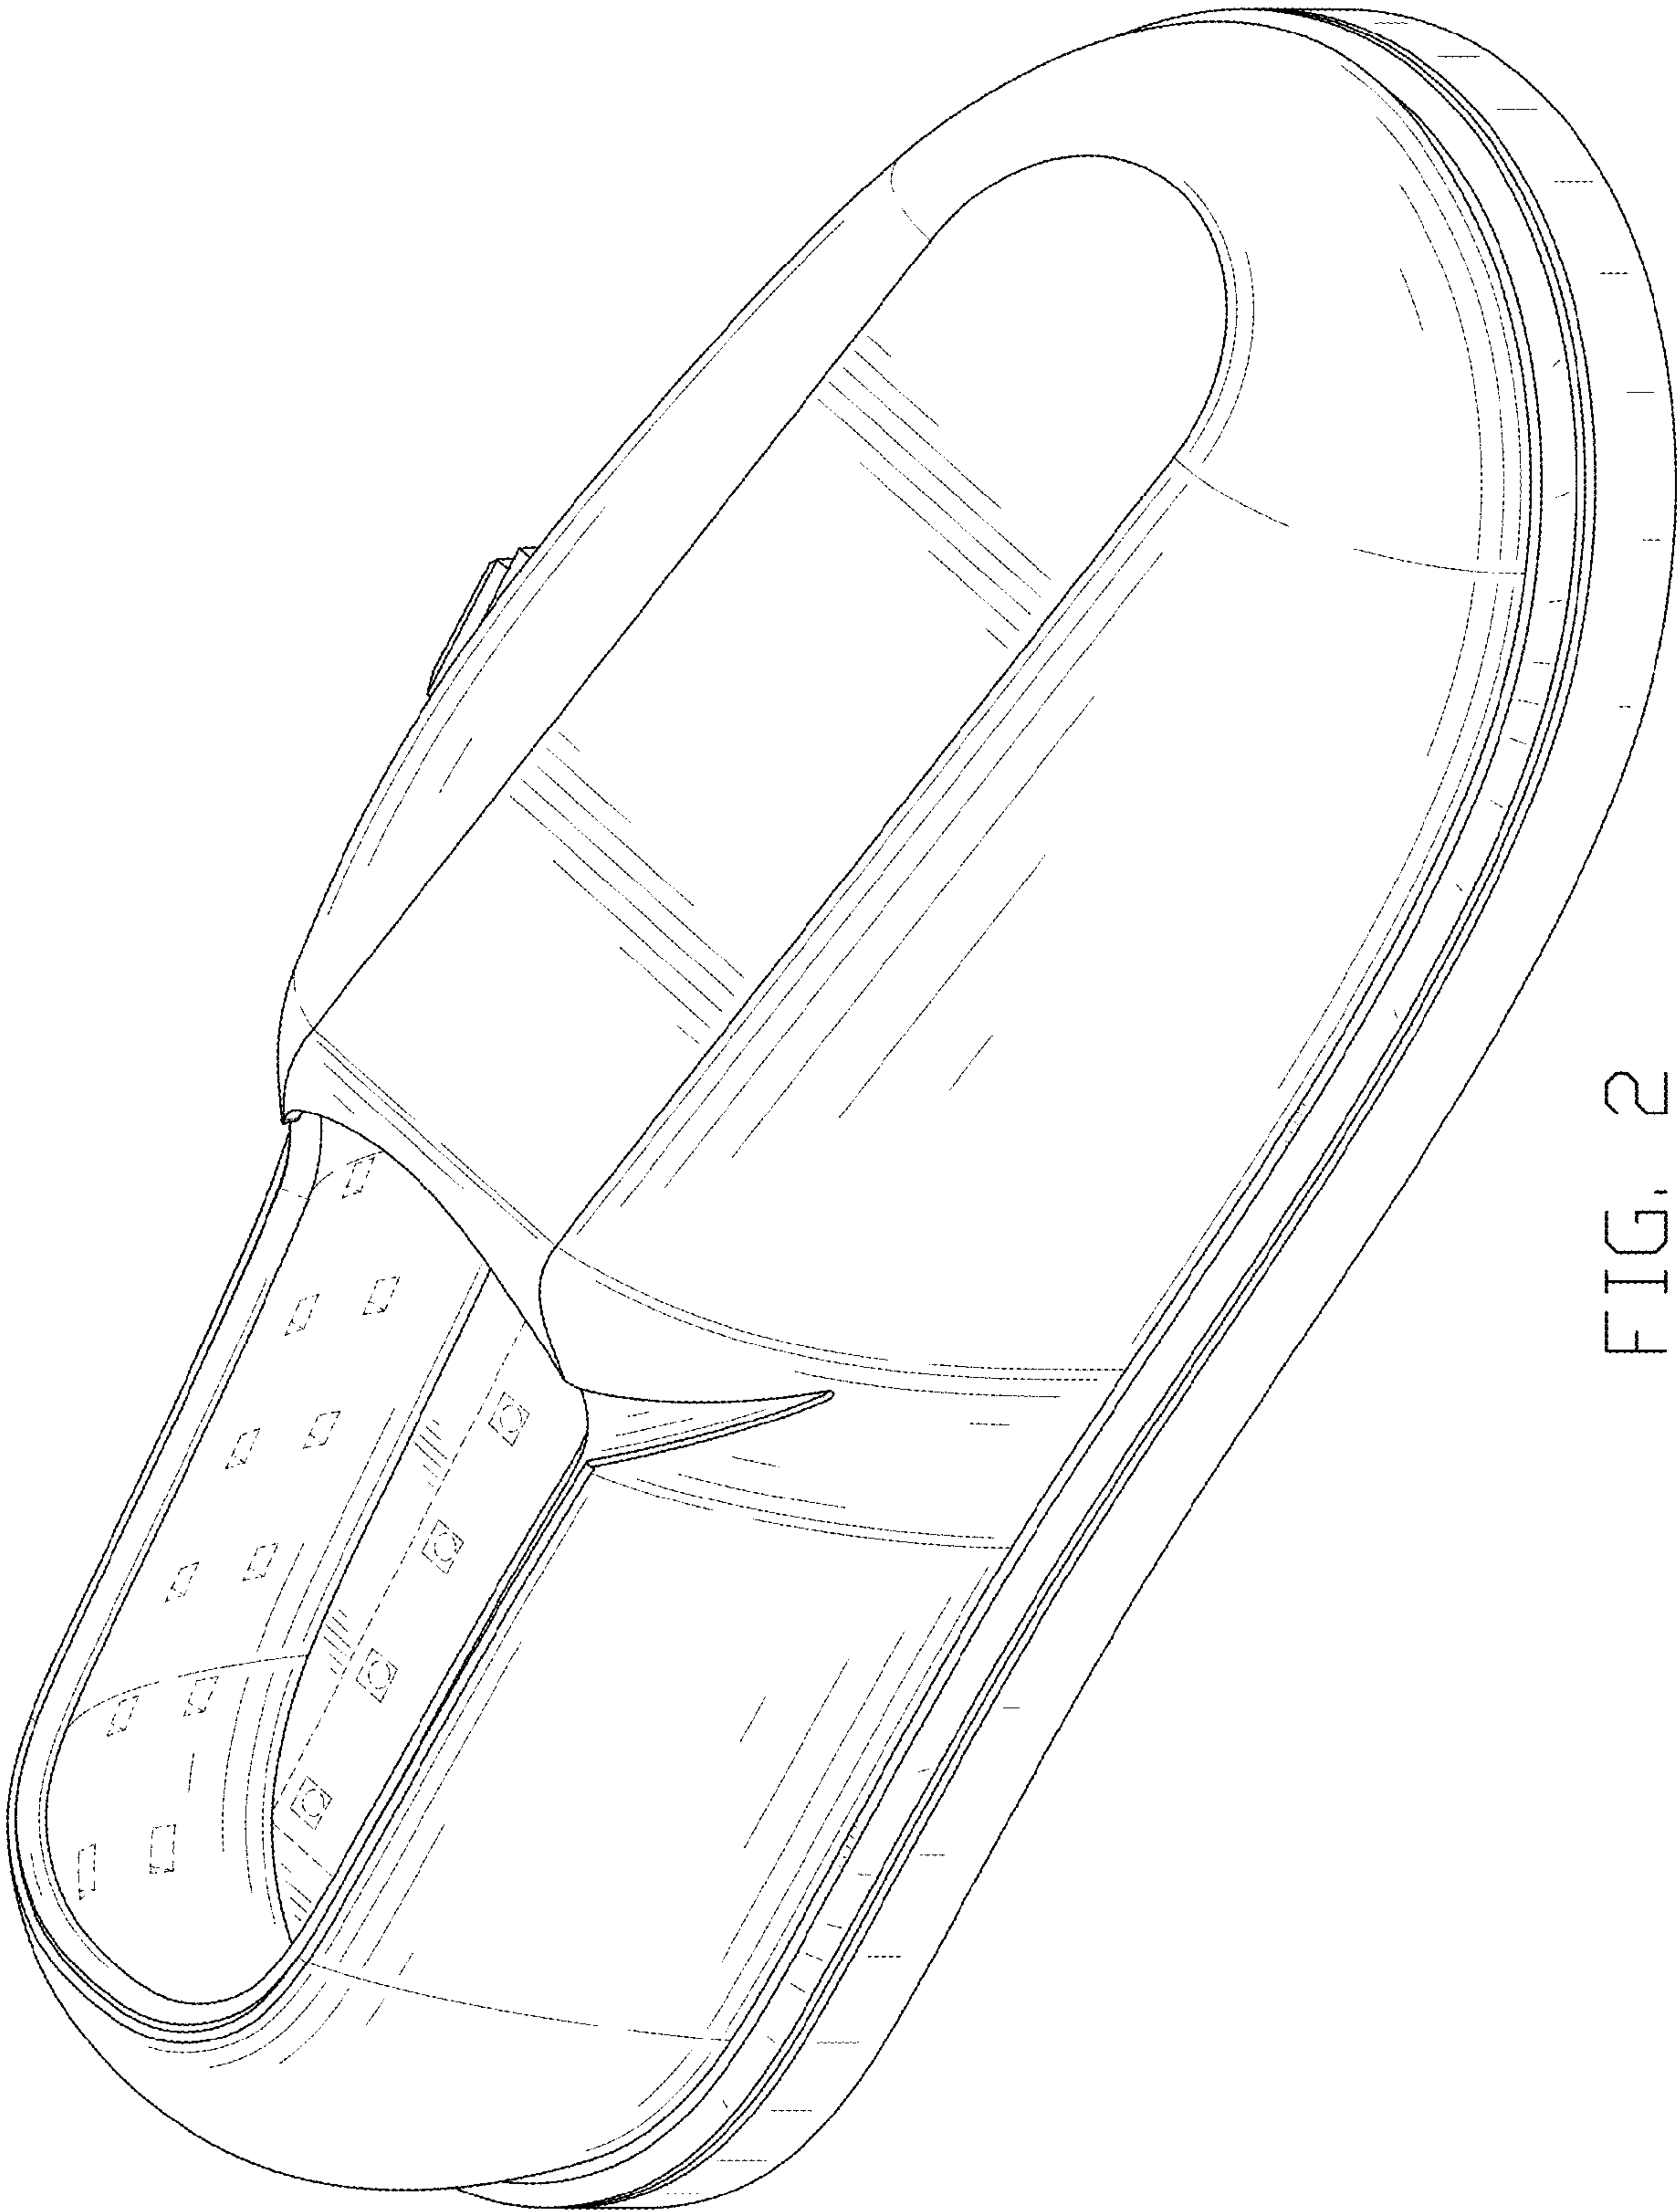


FIG. 2



FIG. 3

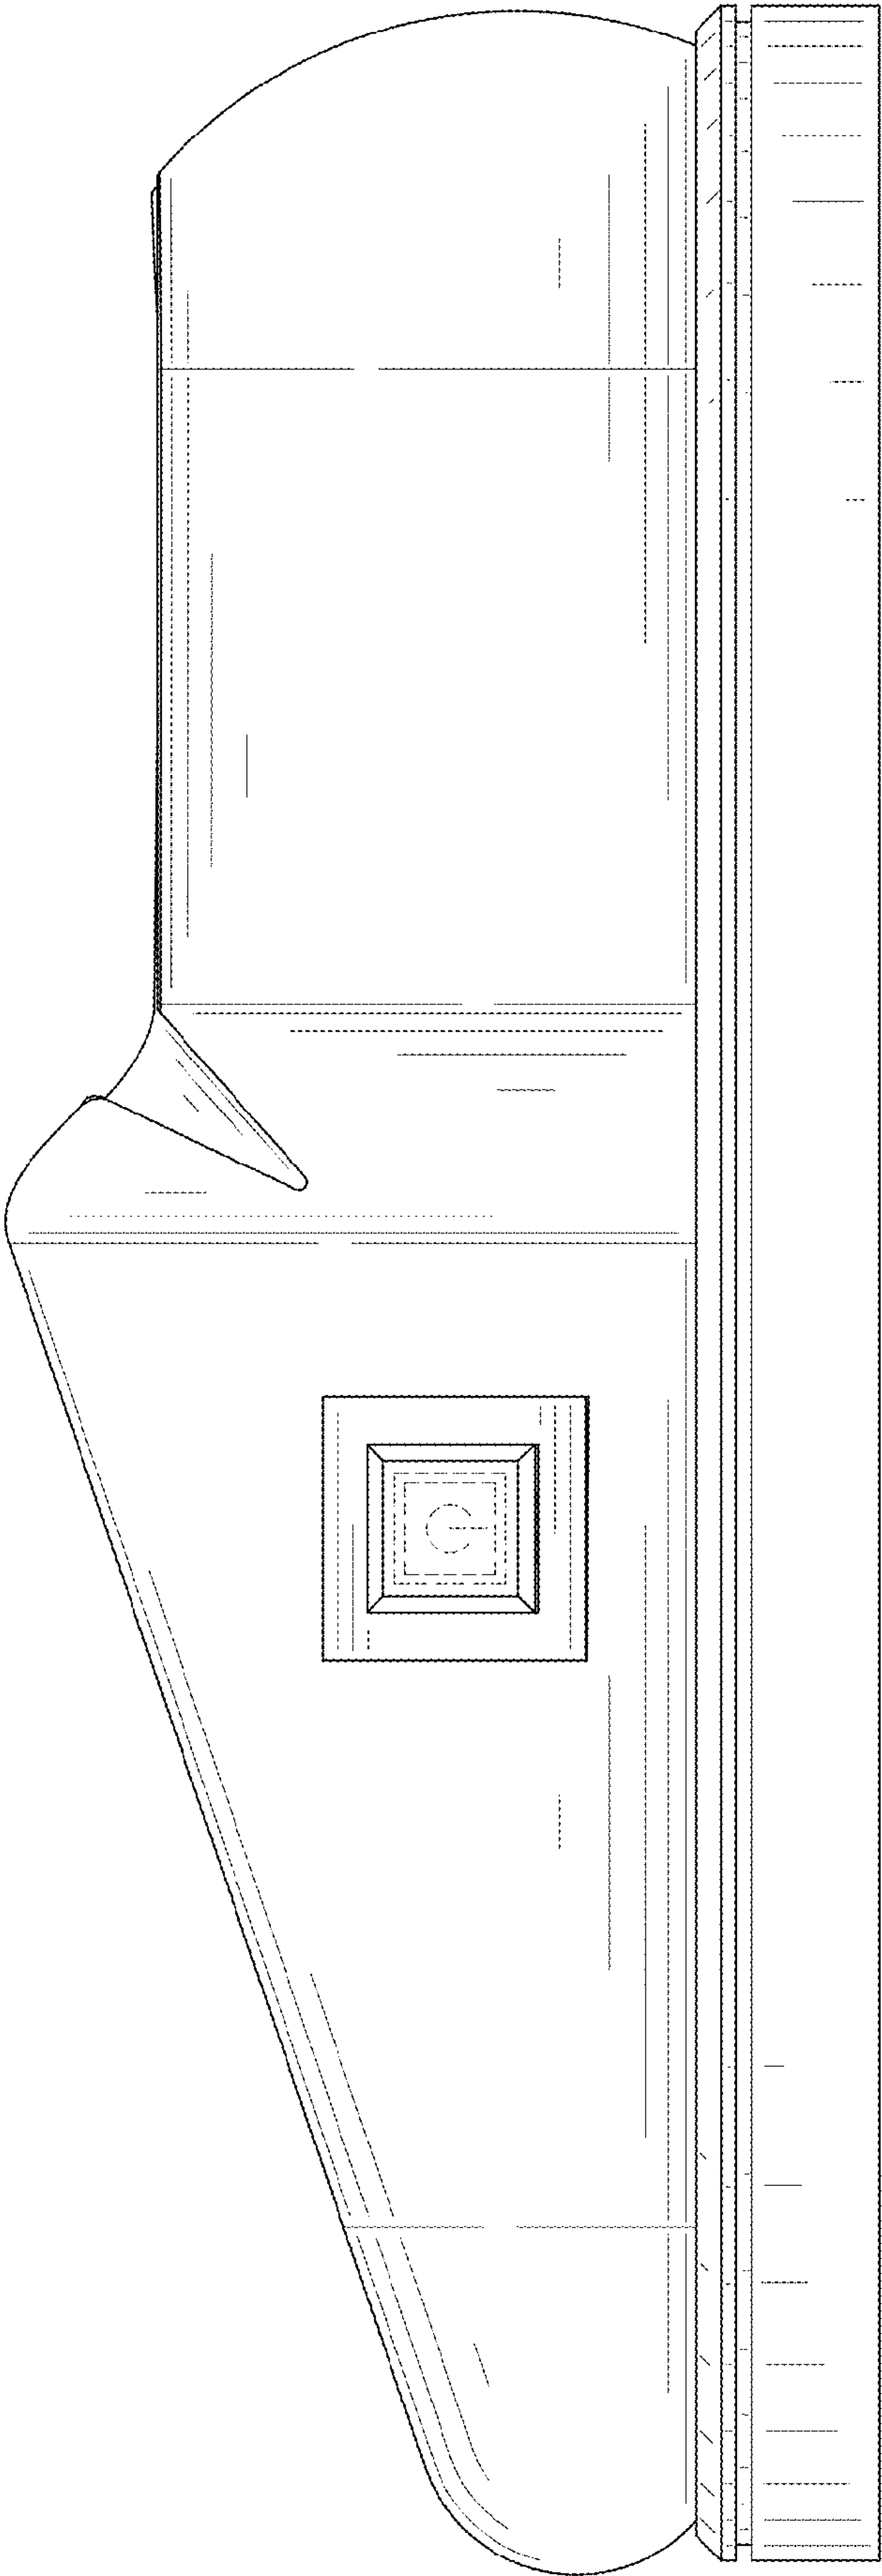


FIG. 4

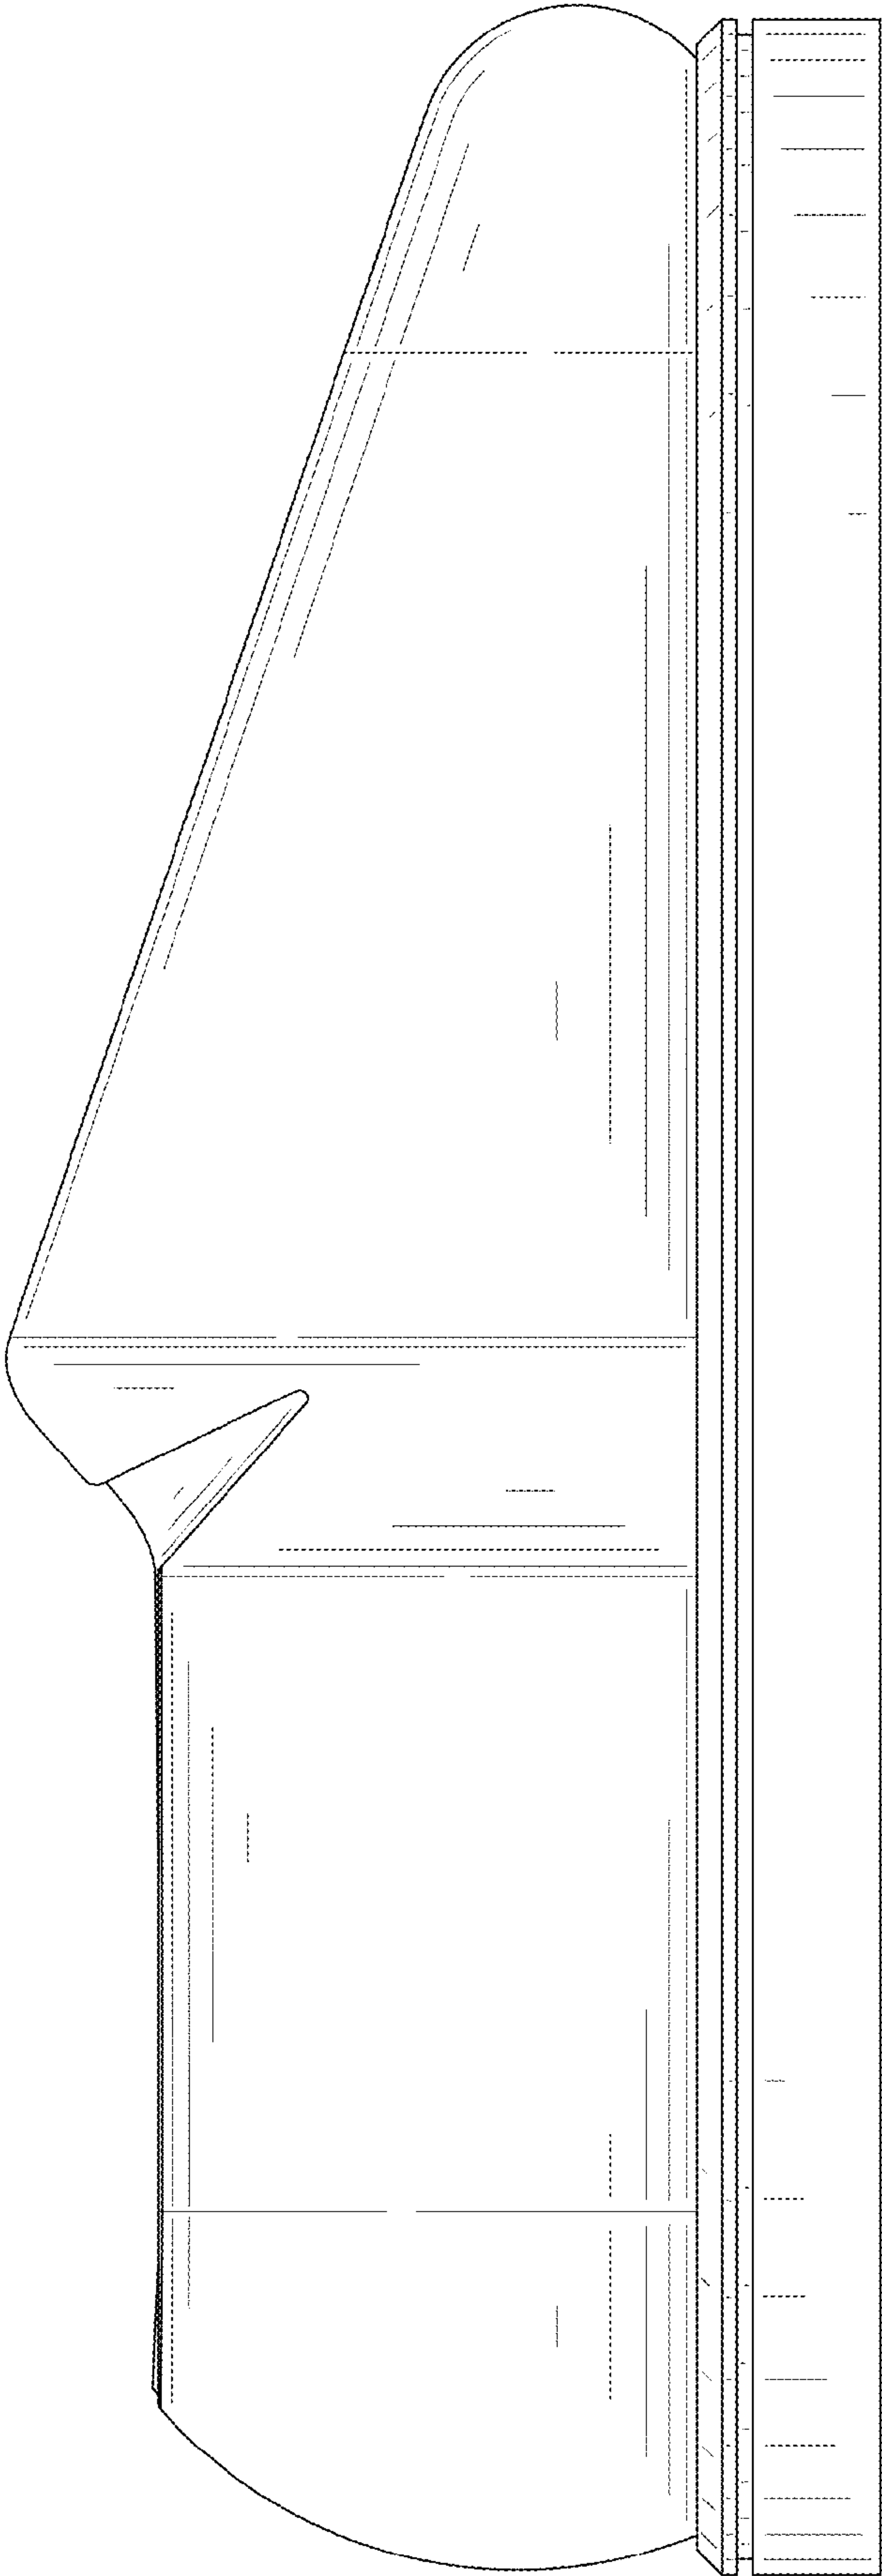


FIG. 5

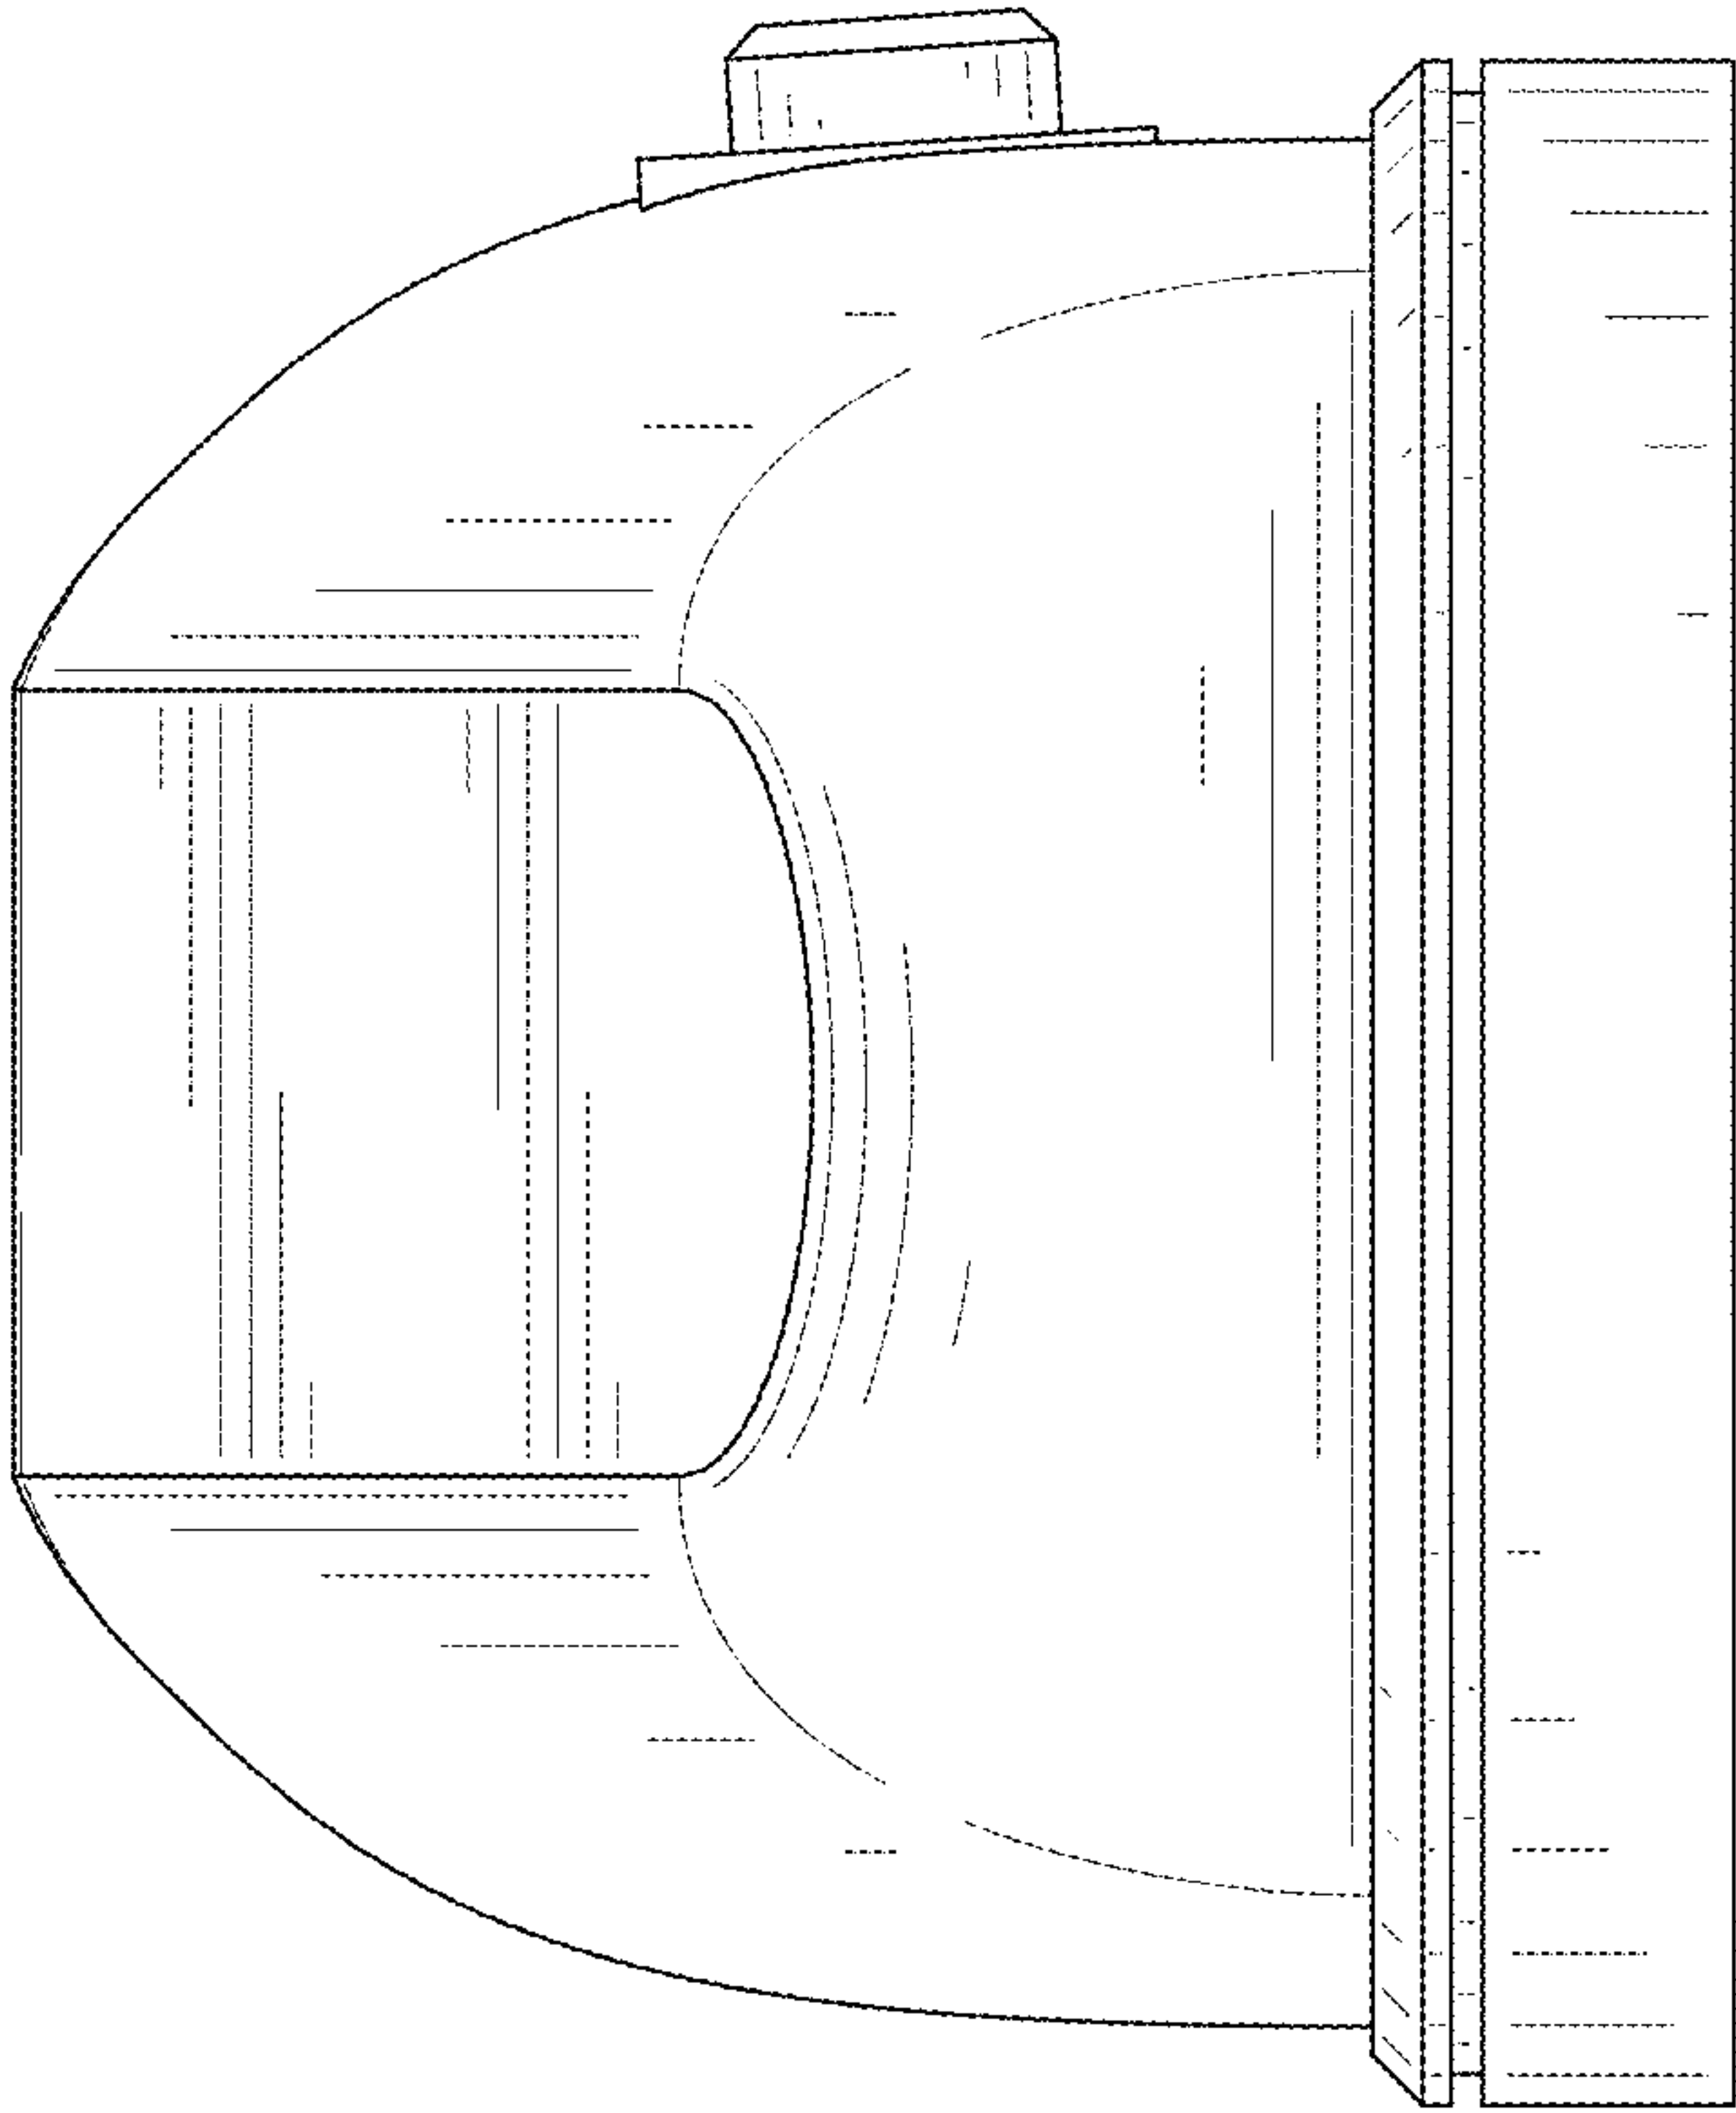


FIG. 6

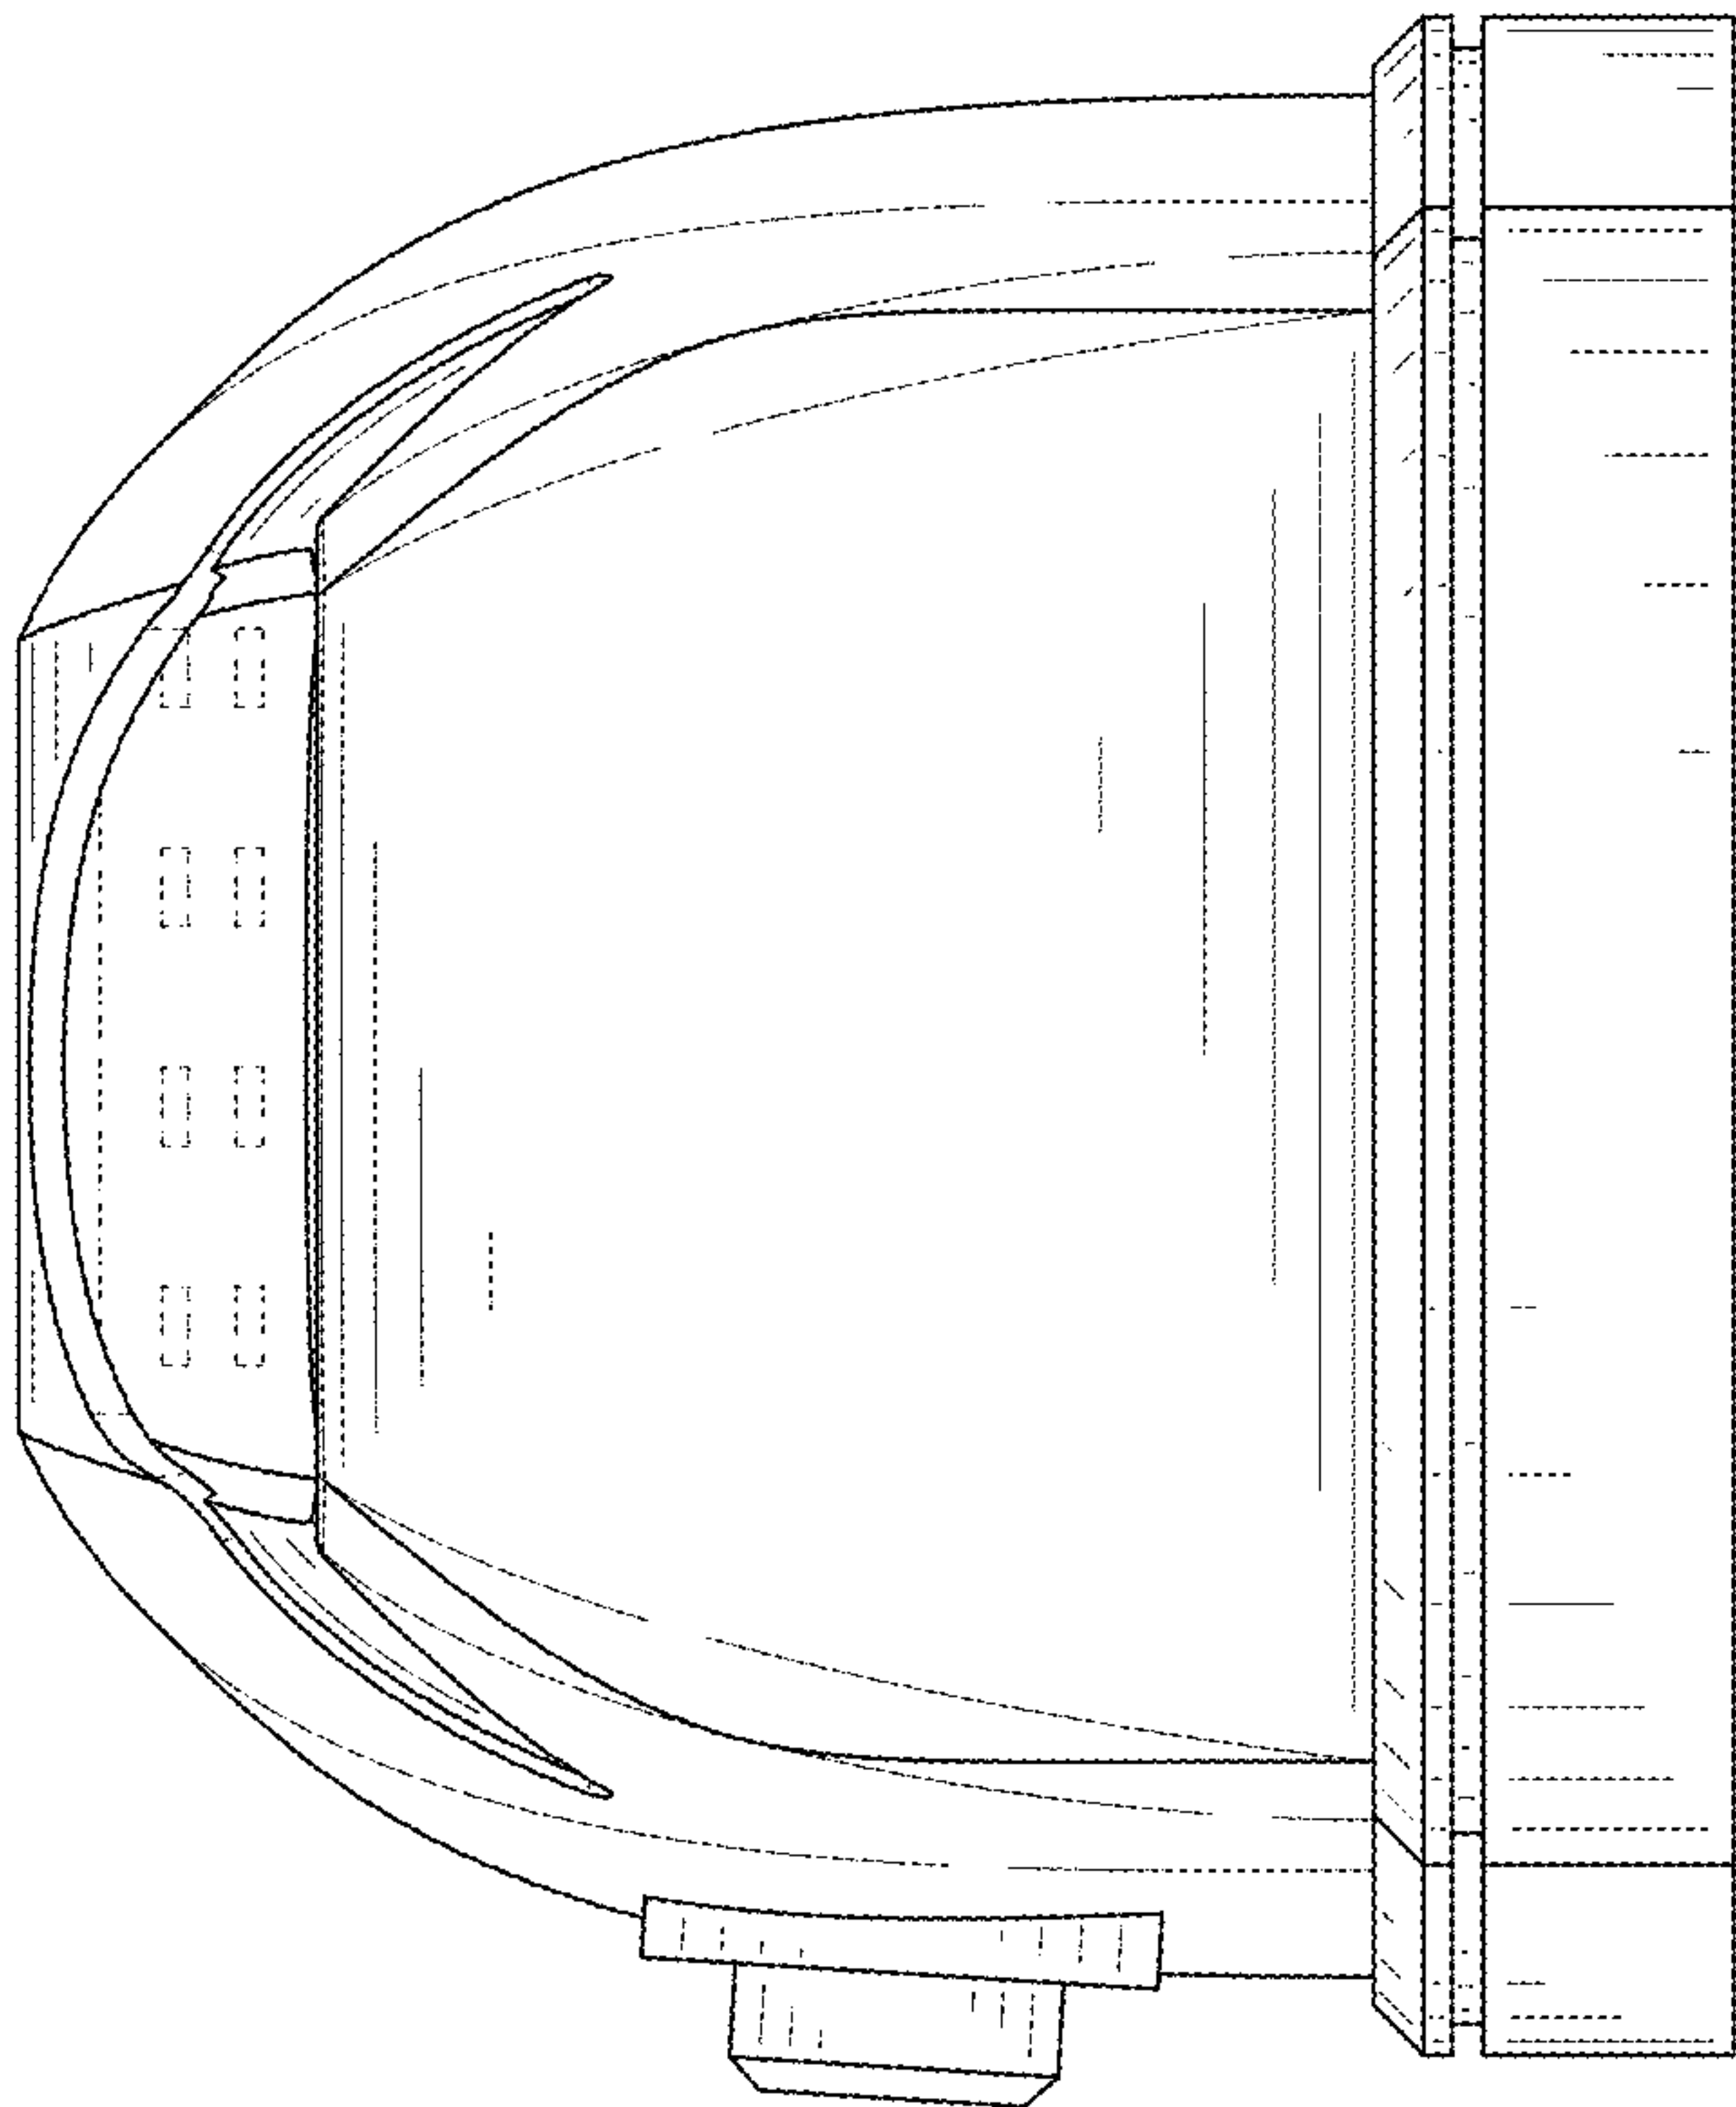


FIG. 7

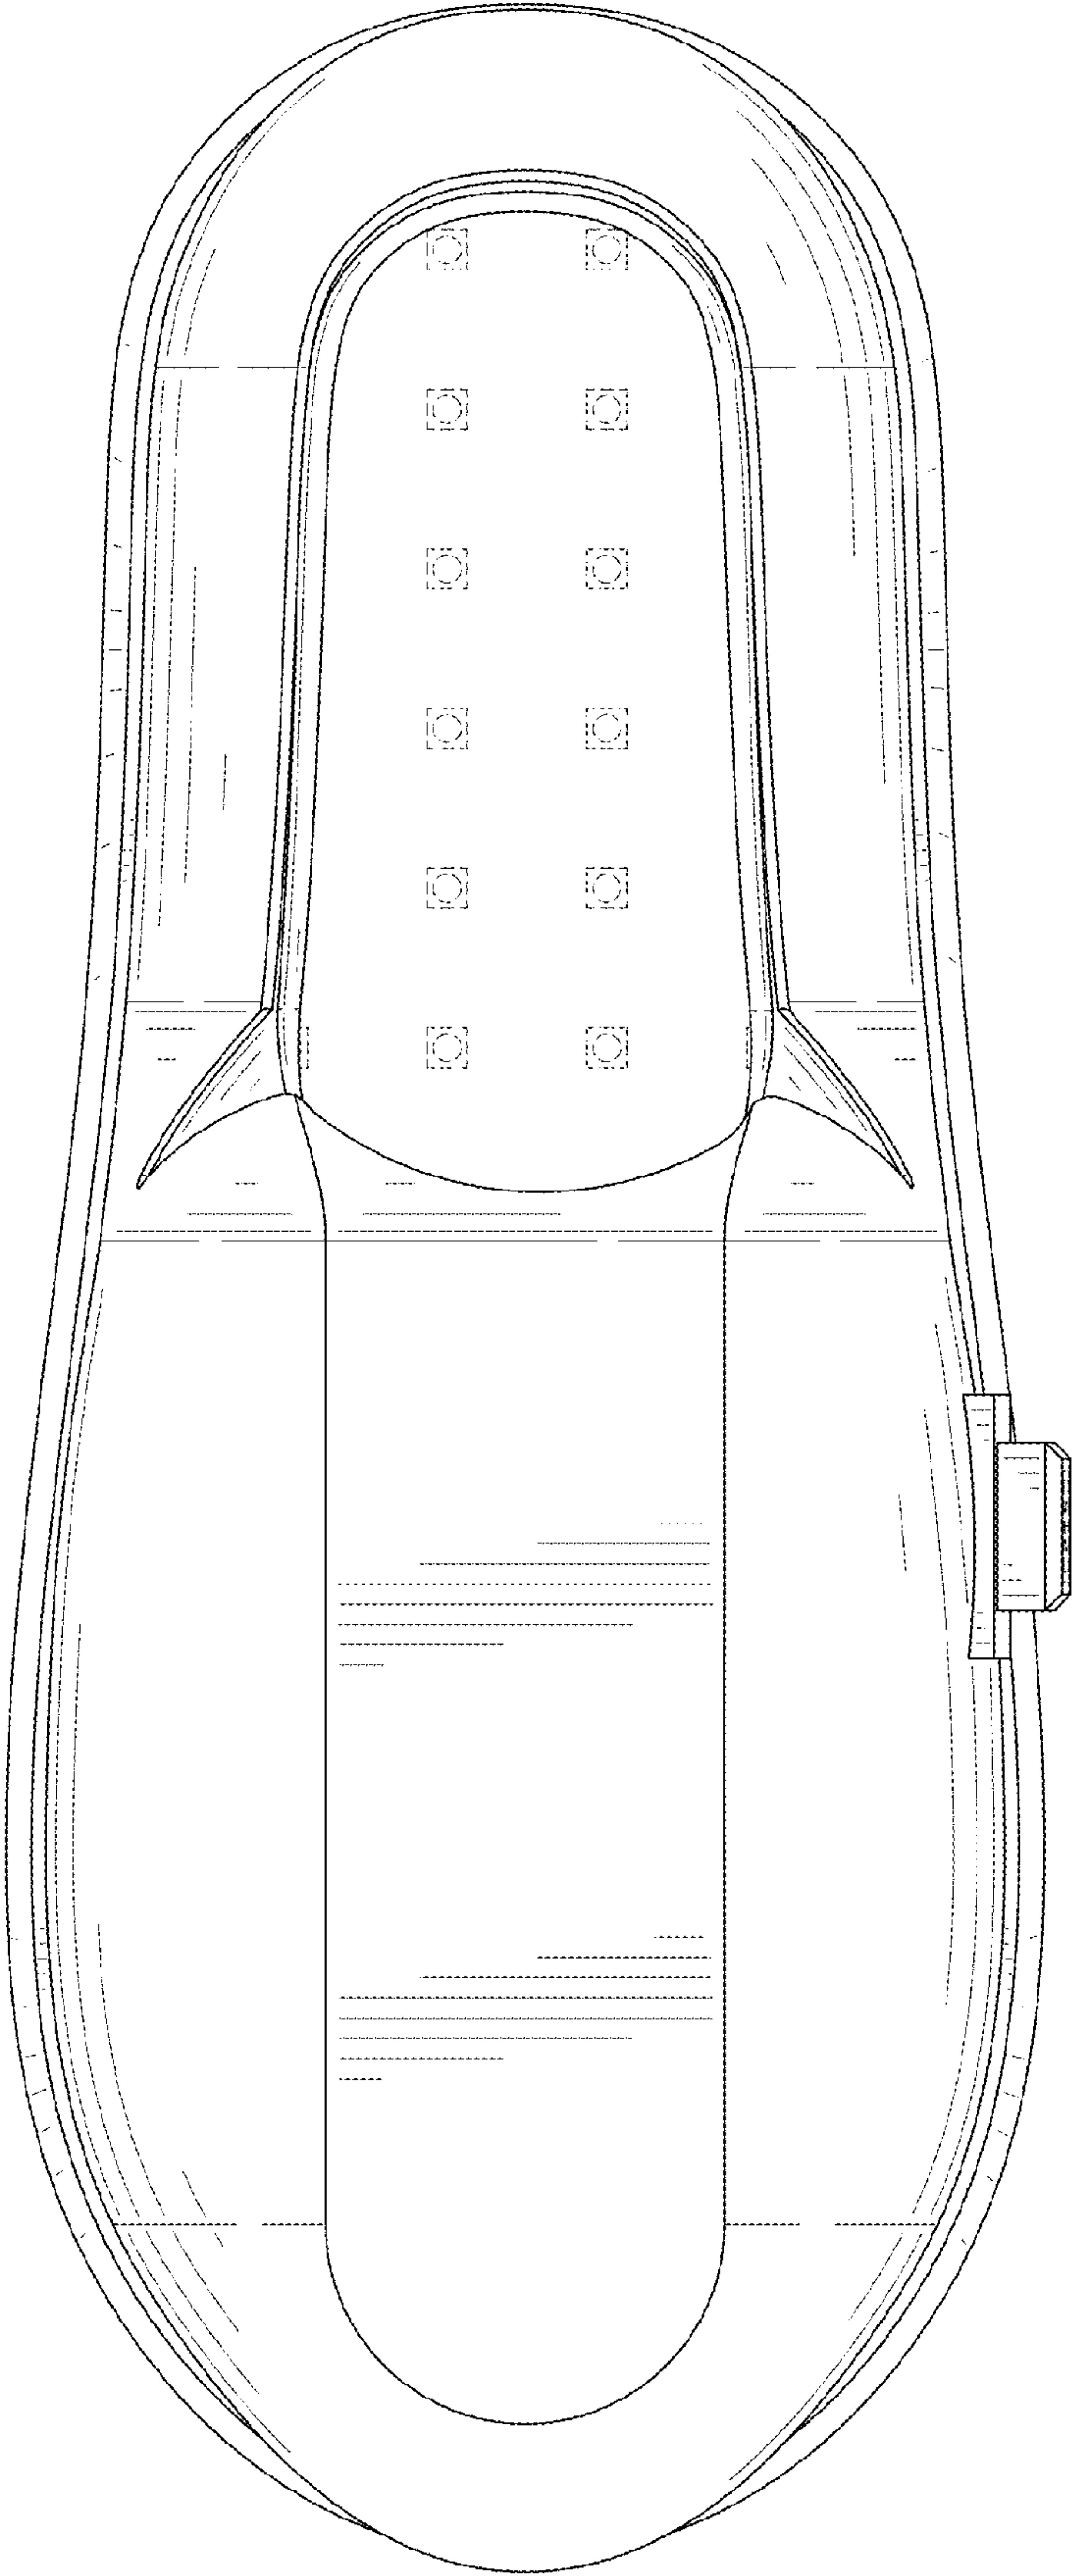


FIG. 8

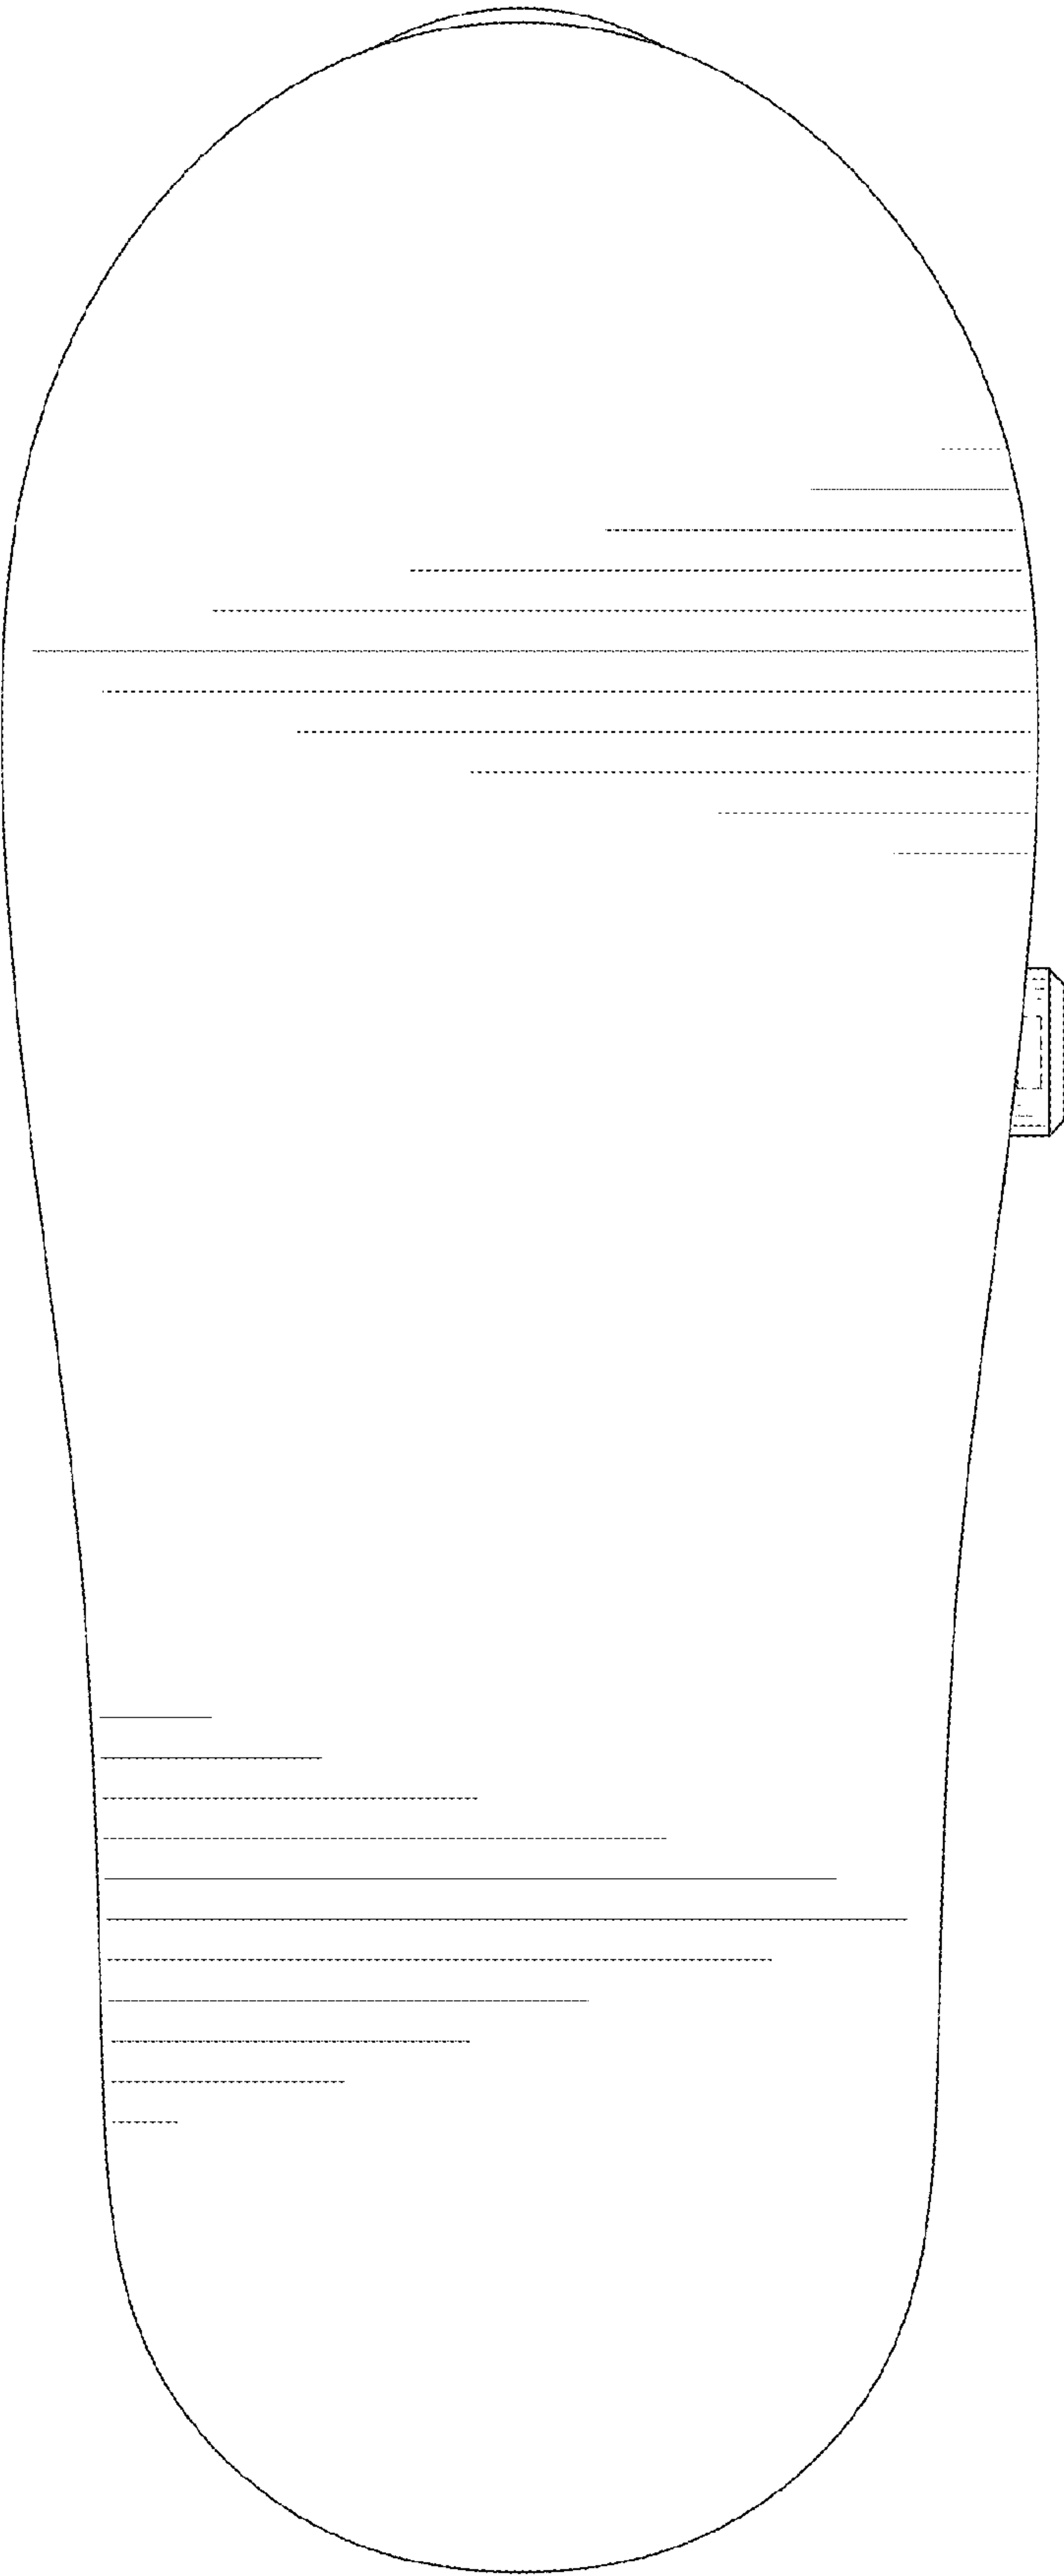


FIG. 9