

(12)

United States Design Patent

Held et al.

(10)

Patent No.:

US D1,046,130 S

(45)

Date of Patent:

** Oct. 8, 2024

(54) ENDOSCOPE HANDLE

(71) Applicant: OLYMPUS Winter & Ibe GmbH,
Hamburg (DE)

(72) Inventors: Fred Held, Hamburg (DE); Thomas
Maerzke, Hamburg (DE); Alrun
Thuemen, Hamburg (DE)

(73) Assignee: OLYMPUS WINTER & IBE GMBH,
Hamburg (DE)

(**) Term: 15 Years

(21) Appl. No.: 29/856,115

(22) Filed: Oct. 11, 2022

(51) LOC (14) Cl. 24-02

(52) U.S. Cl. D24/138

(58) Field of Classification Search

USPC D24/108, 111, 112, 118, 117, 127, 130,
D24/133, 135, 137, 138, 141, 143, 144,
D24/148, 152, 153, 154, 170, 176, 179,
D24/216, 222; D16/130, 132, 136, 200,
D16/202–206, 208, 218, 219

CPC A61B 1/00172; A61B 1/00009; A61B
1/00042; A61B 1/00043; A61B 1/00057;
A61B 1/00066; A61B 1/00105; A61B
1/00117; A61B 1/00128; A61B 1/00165;
A61B 1/00181; A61B 1/00183; A61B
1/0052

See application file for complete search history.

(56) References Cited

U.S. PATENT DOCUMENTS

D745,670 S	*	12/2015	Czupalla	D24/138
D779,053 S	*	2/2017	Kobida	D24/108
D795,424 S	*	8/2017	Sloss	D24/138
D798,445 S	*	9/2017	Heni	D24/133

D818,122 S	*	5/2018	Oberkircher	D24/144
D835,170 S	*	12/2018	Pilz	D16/130
D841,160 S	*	2/2019	Cranfield	D24/138
D844,137 S	*	3/2019	Sun	D24/138
D852,358 S	*	6/2019	Matuschek	D24/138
D864,388 S	*	10/2019	Barber	D24/133
D874,647 S	*	2/2020	Cranfield	D24/138
D919,804 S	*	5/2021	Cole	D24/133
D956,969 S	*	7/2022	Bast	D24/133
2015/0343121 A1	*	12/2015	Kobida	A61M 1/7411 604/187

OTHER PUBLICATIONS

Endoeye 3D Medical device, posted at ifdesign.com, posting date Dec. 30, 2018, retrieved Oct. 28, 2023, online, URL:https:// ifdesign.com/en/winner-ranking/project/endoeye-3d/235134 (Year: 2018).*

(Continued)

Primary Examiner — Jennifer L Rempfer
Assistant Examiner — Michelle Marquart Christeon
(74) Attorney, Agent, or Firm — Scully, Scott, Murphy & Presser, P.C.


(57) CLAIM

The ornamental design for an endoscope handle, as shown and described.

DESCRIPTION

FIG. 1 is an enlarged front view of an endoscope handle showing our new design;
FIG. 2 is a left-side view thereof, the right-side view being a mirror image thereof;
FIG. 3 is a top view thereof;
FIG. 4 is a top perspective view thereof; and
FIG. 5 is a bottom view thereof; and,
FIG. 6 is a left perspective view thereof.
The broken lines shown in the Drawings illustrate portions of the endoscope handle that form no part of the claimed design.

1 Claim, 6 Drawing Sheets

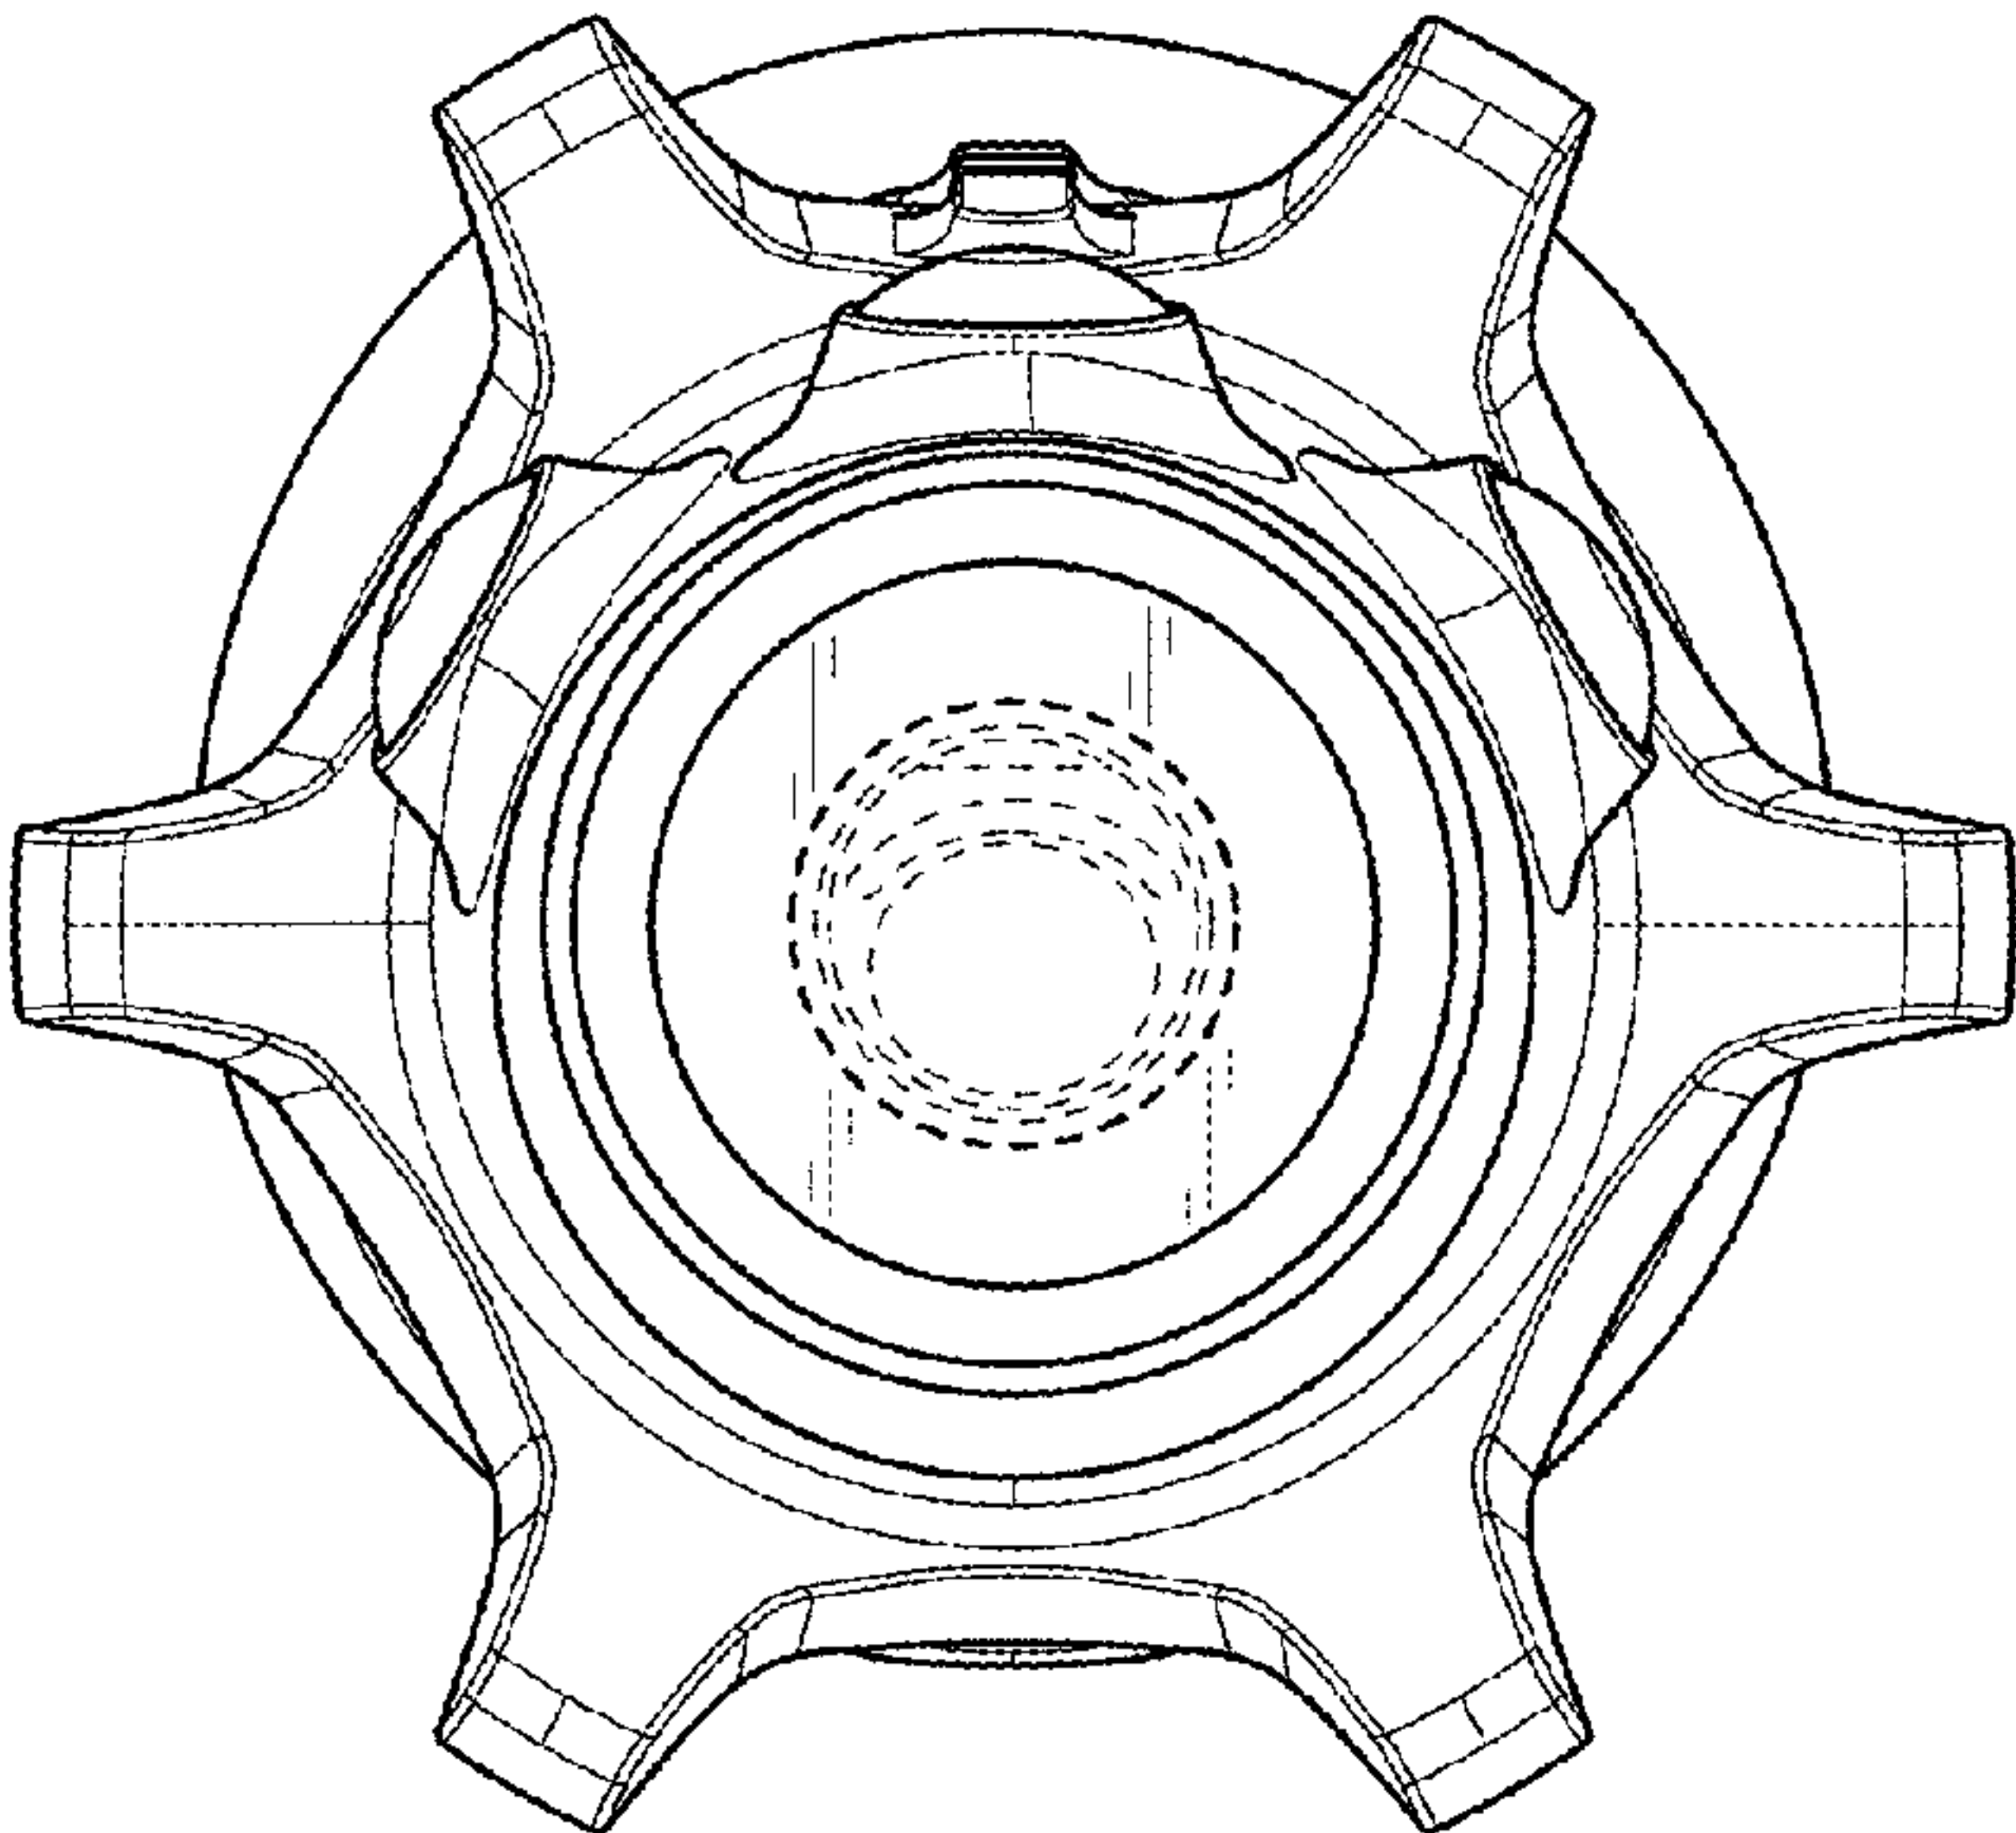

(56) **References Cited**

OTHER PUBLICATIONS

Olympus Visera Elite Ii 3D, posted at ifdesign.com, posting date Jun. 30, 2021, retrieved Oct. 28, 2023, online, URL:[https:// www.youtube.com/watch?v=IskCd6dfZvA&t=65s](https://www.youtube.com/watch?v=IskCd6dfZvA&t=65s) (Year: 2021).*

Endoeye Hdii catalog, posted at medfau.com, posting date unavailable, retrieved Oct. 28, 2023, online, URL:<chrome-extension://efaidnbmnnnibpcajpcgclefindmkaj/https://medfau.com/wp-content/uploads/2021/05/endoeye-hd-5mm.pdf>(Year: 2023 (Year: 2023)).*

Red Dot Group, “Red Dot Design Award Endoeye” published 2014; Olympus Winter & Ibe GmbH.

HD Endoeye High definition digital videolaparoscope—resolutionary imaging, Endoeye, Olympus Europa Holding GMBH, 2013.

Video Telescope, Endoeye HD II, Olympus, Copyright 2020 Olympus Winter & Ibe GmbH.

* cited by examiner

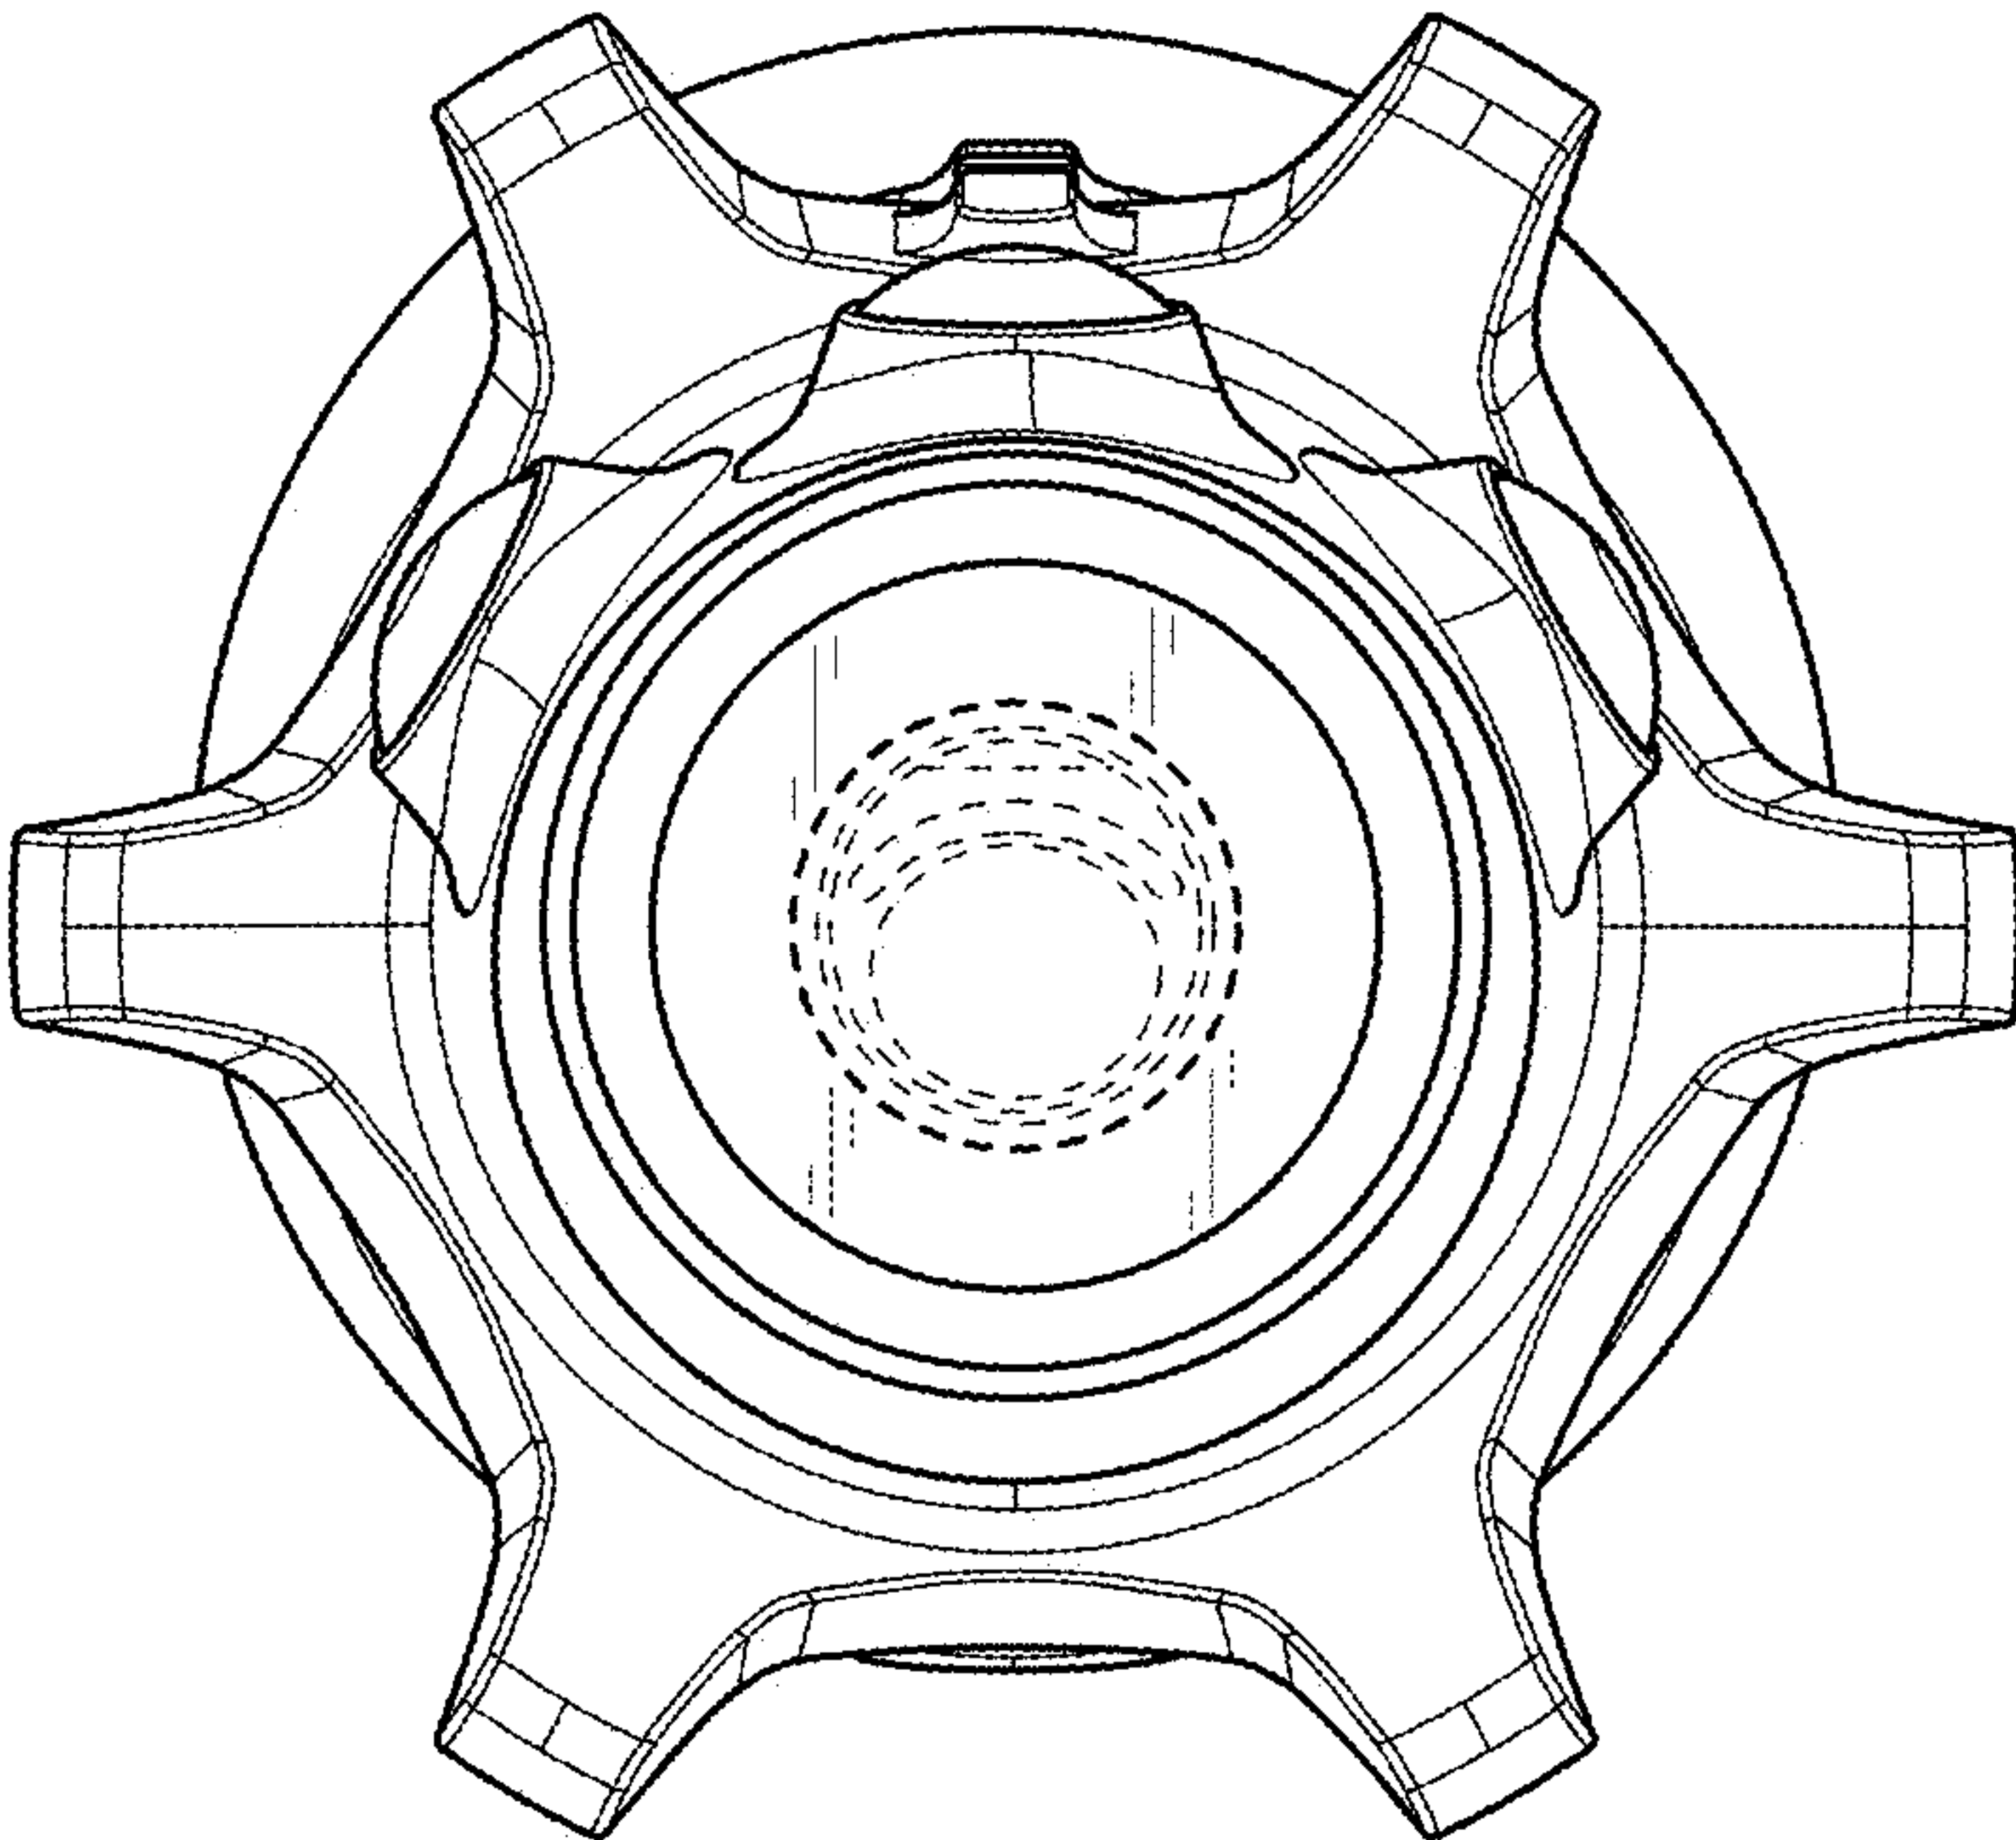


FIG. 1

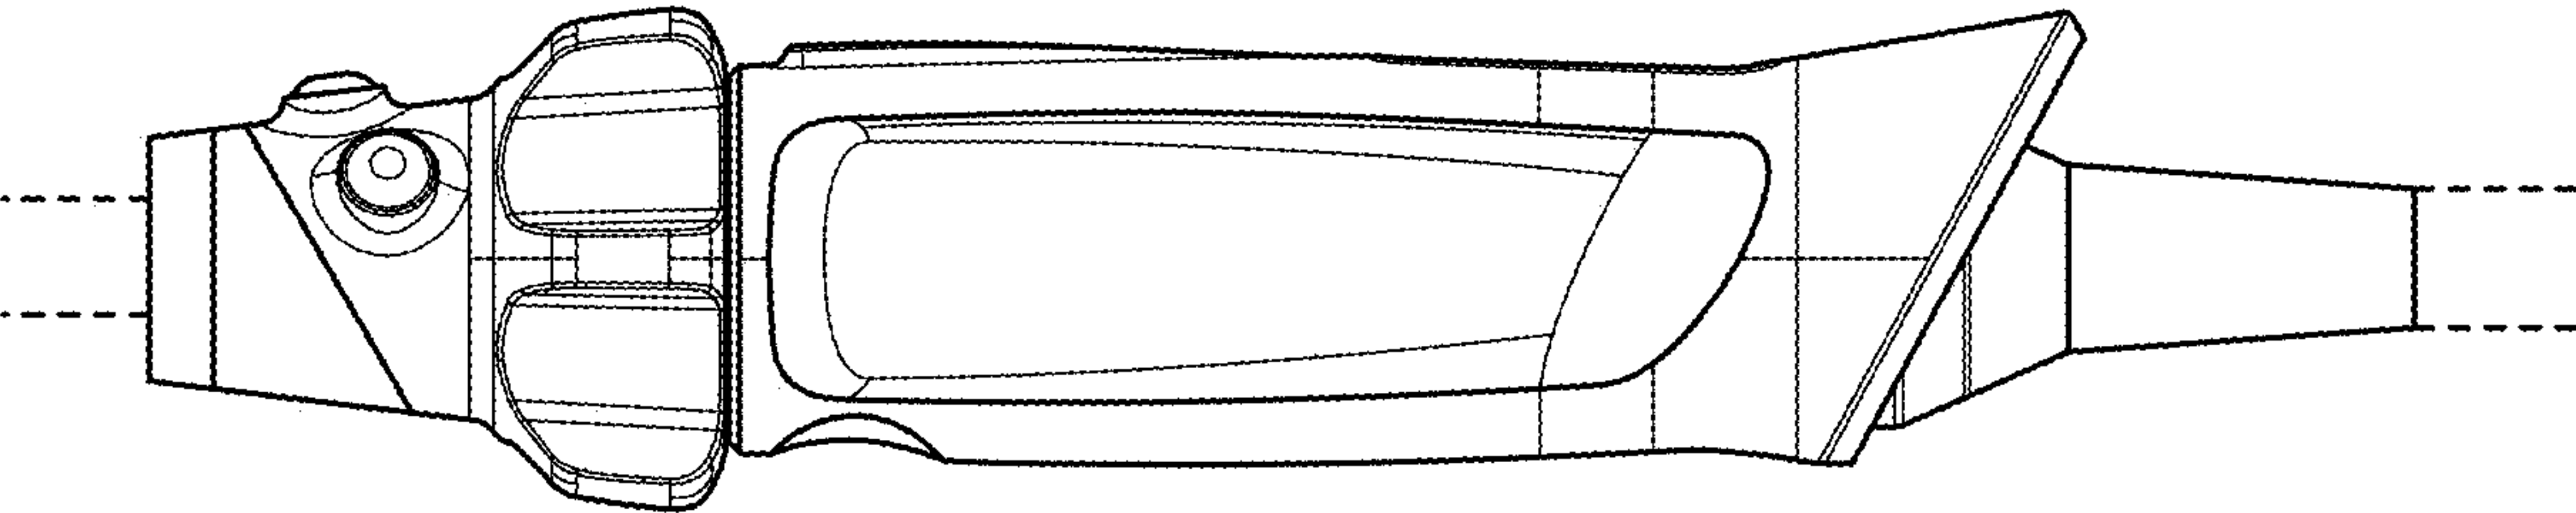


FIG. 2

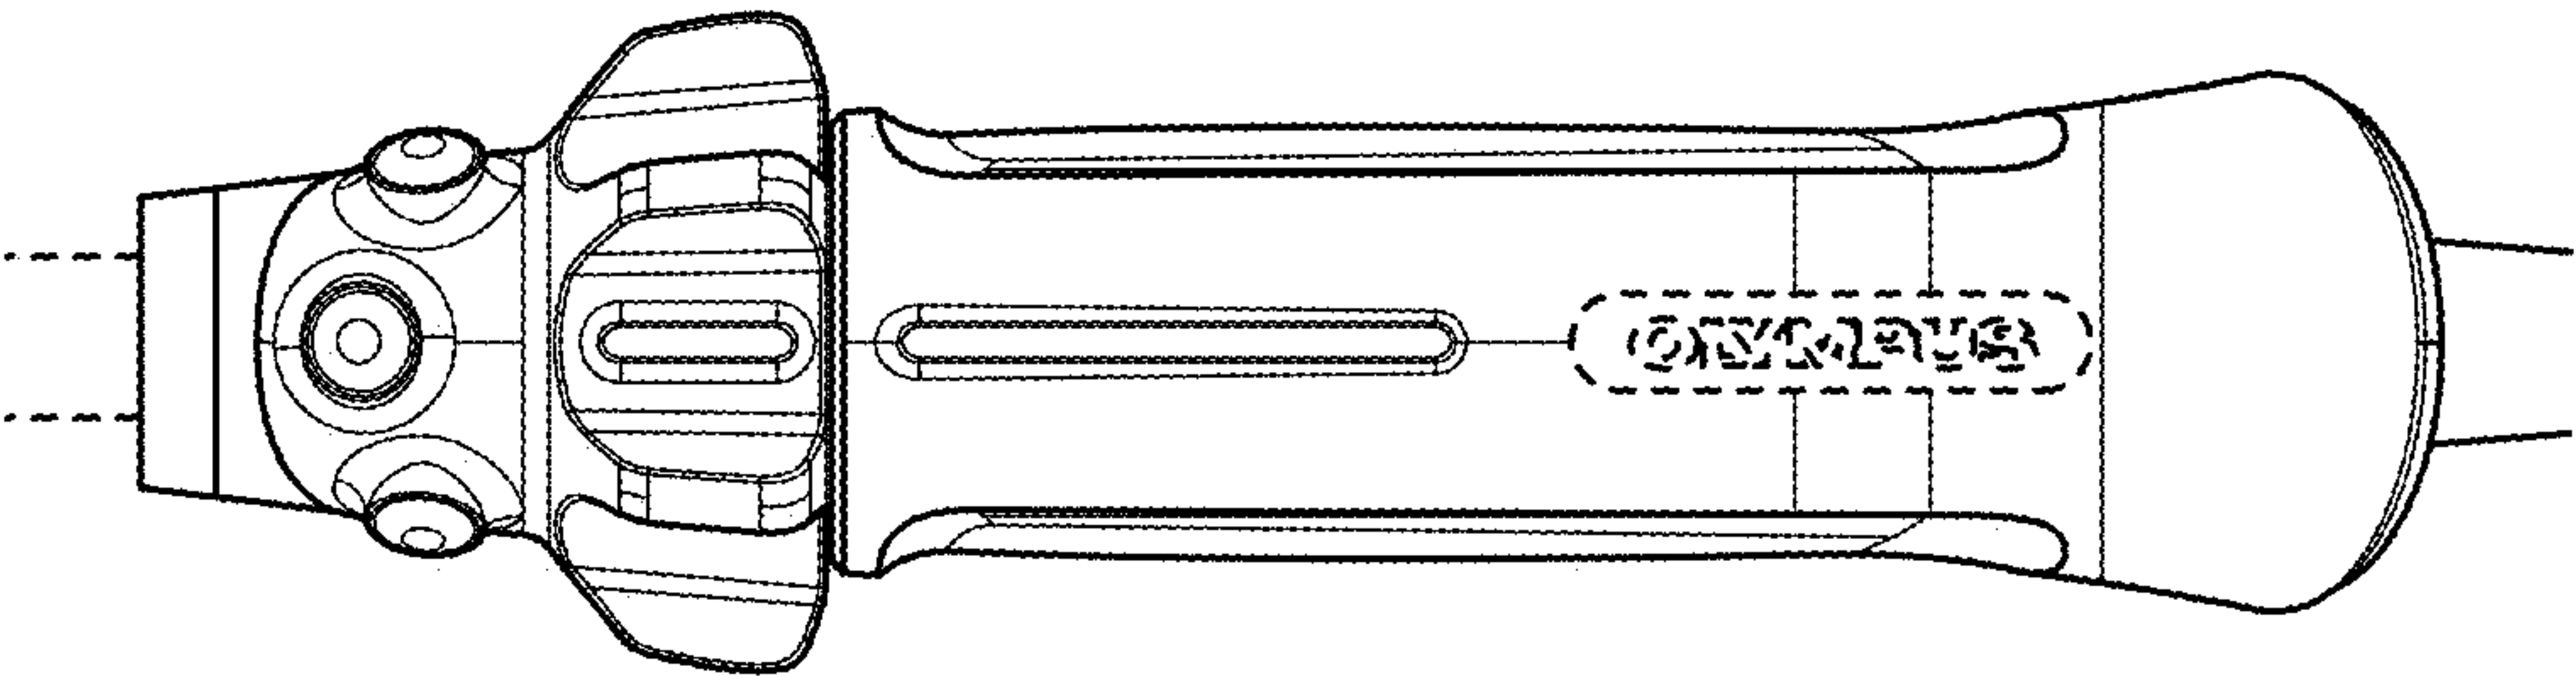


FIG. 3

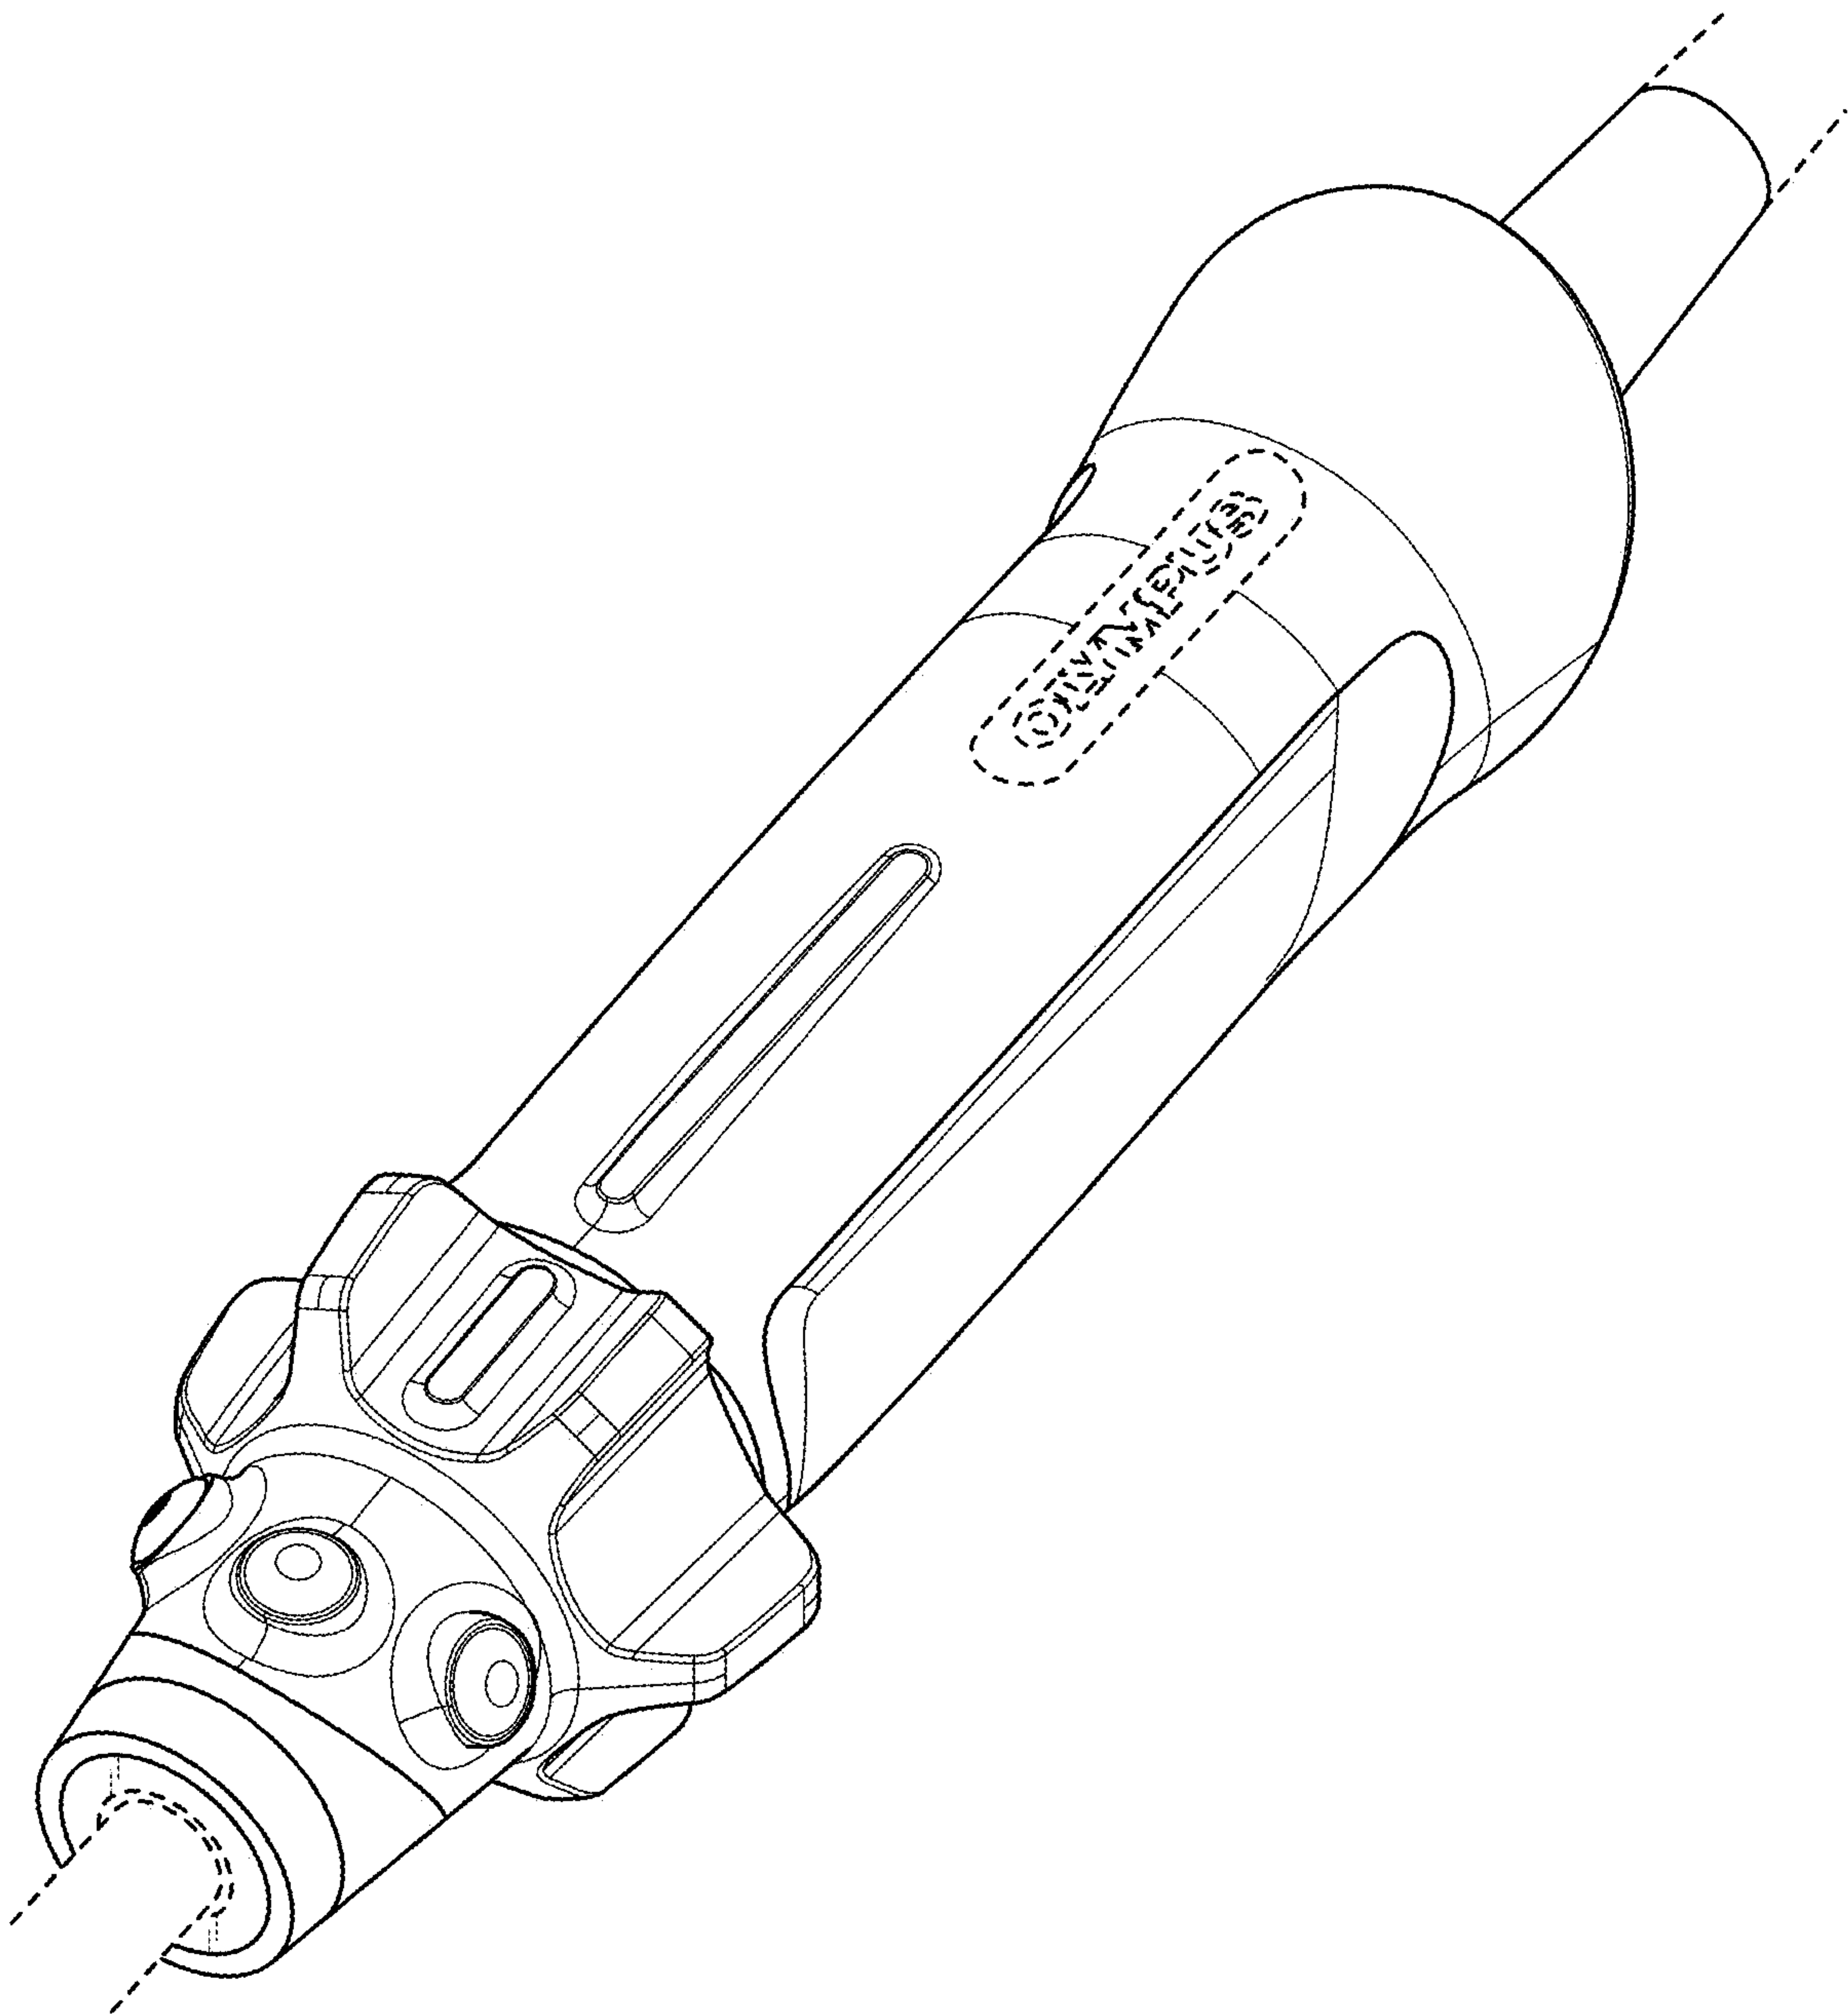


FIG. 4

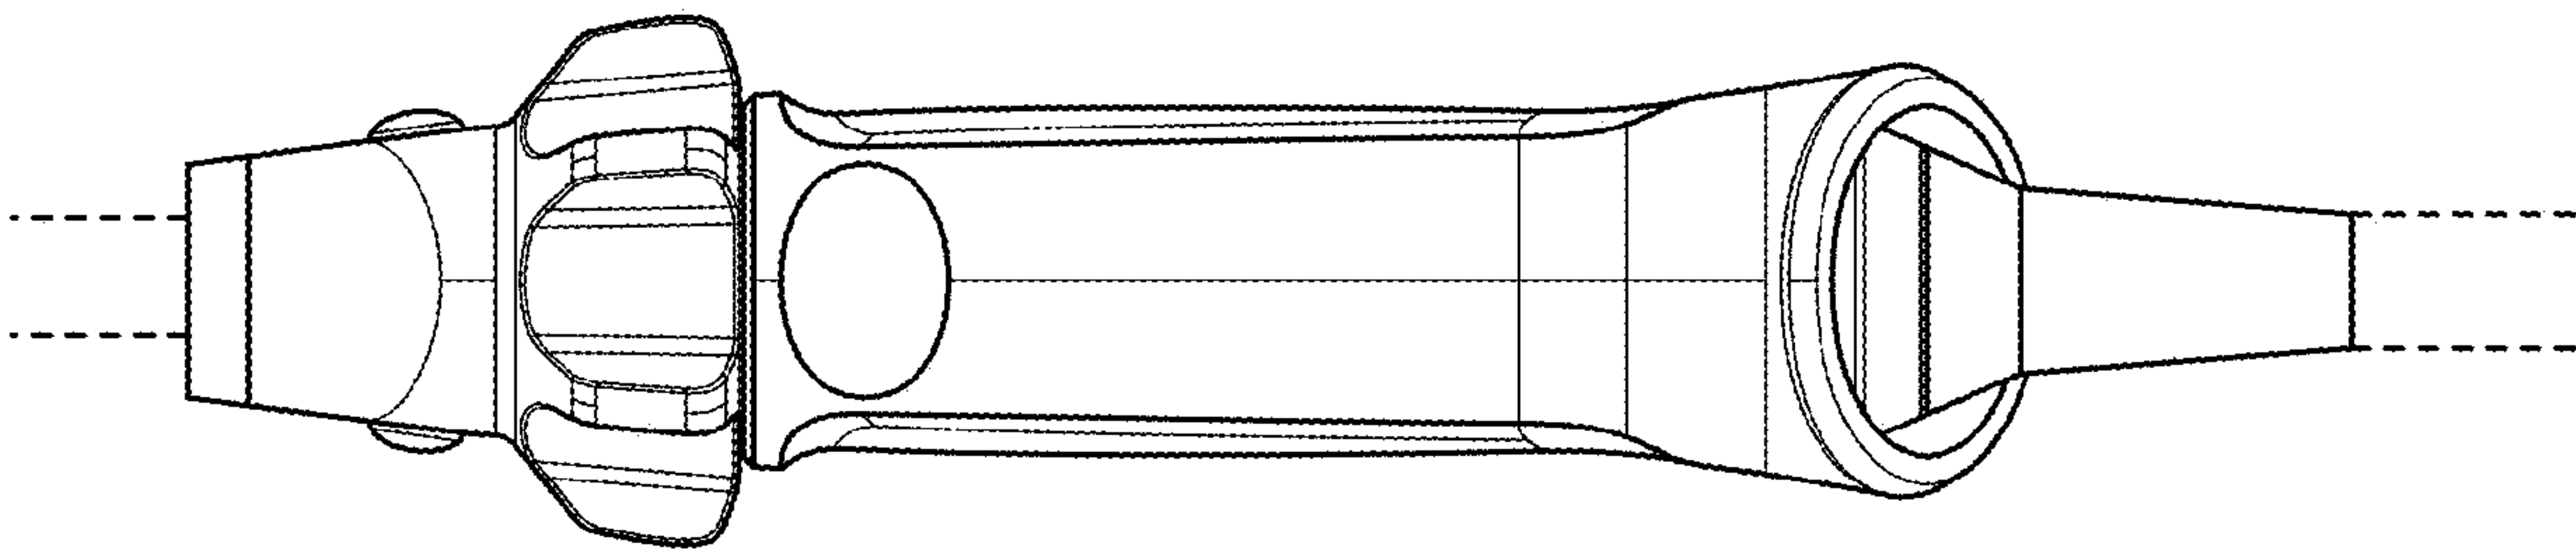


FIG. 5

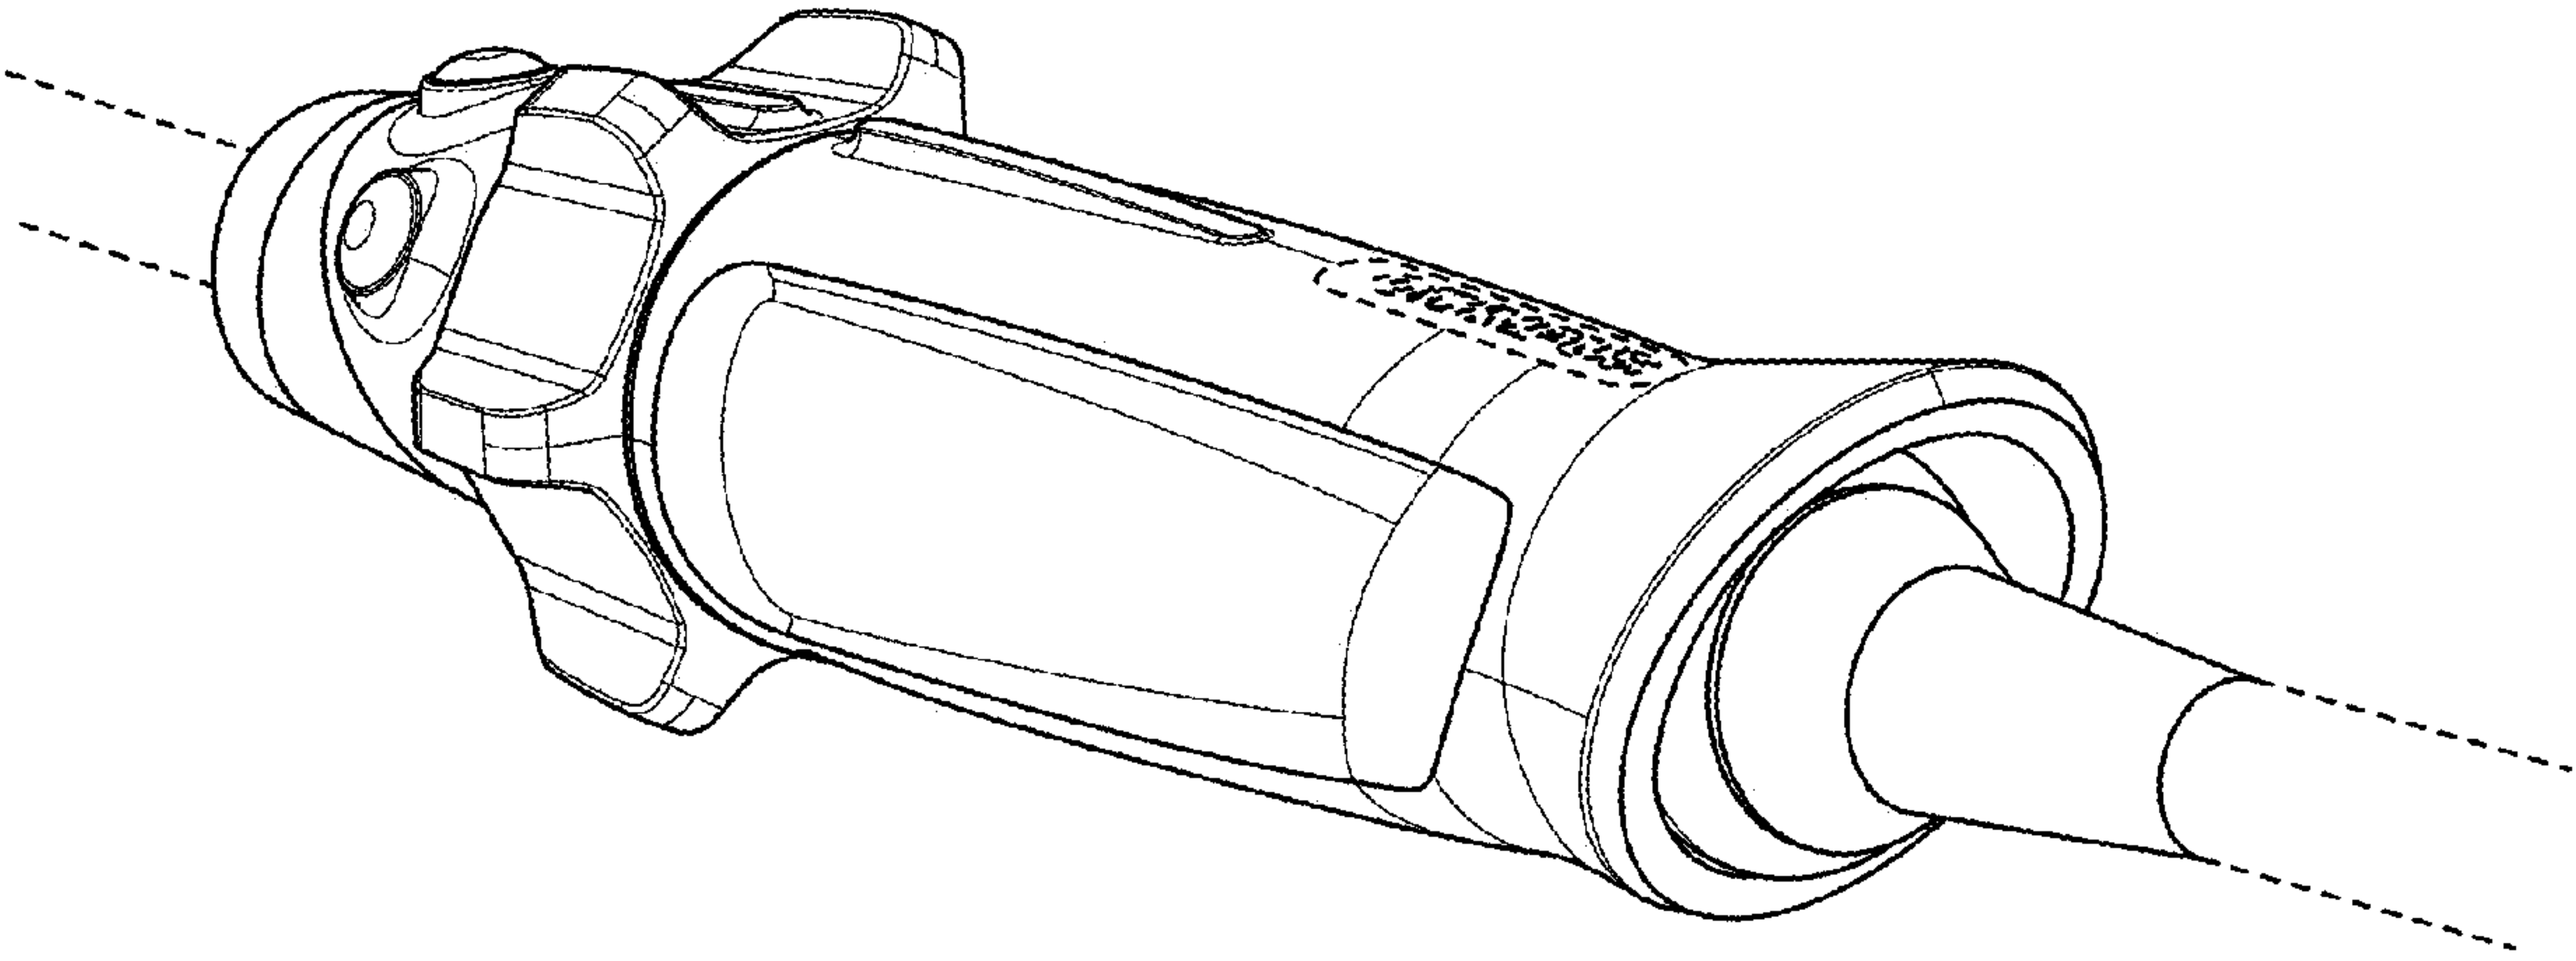


FIG. 6