



US0D1047137S

(12)

United States Design Patent

Young et al.

(10)

Patent No.:

US D1,047,137 S

(45)

Date of Patent:

** Oct. 15, 2024

(54) INJECTOR

(71) Applicant: **Oval Medical Technologies Limited**,
Cambridge (GB)

(72) Inventors: **Matthew Young**, Cambridge (GB);
Jose Alberto De Los Rios, Cambridge
(GB); **Marcus Agunloye**, Cambridge
(GB)

(73) Assignee: **OVAL MEDICAL TECHNOLOGIES
LIMITED**, Cambridge (GB)

(**) Term: **15 Years**

(21) Appl. No.: **29/873,918**

(22) Filed: **Apr. 11, 2023**

(30) Foreign Application Priority Data

Oct. 12, 2022 (EM) 009203813-0001
Oct. 12, 2022 (EM) 009203813-0002

(51) **LOC (14) Cl.** **24-02**
(52) **U.S. Cl.**
USPC **D24/113**

(58) **Field of Classification Search**
USPC D24/112–114, 133, 186, 127–131, 231,
D24/108
CPC A61M 5/3156; A61M 5/31591; A61M
5/3155; A61M 5/3157; A61M 5/31501
See application file for complete search history.

(56) References Cited

U.S. PATENT DOCUMENTS

D428,650 S * 7/2000 Bellhouse D24/114
D710,992 S * 8/2014 Dubuc D24/113
D824,023 S * 7/2018 Grimoldby D24/113
D897,185 S * 9/2020 Perkins, Jr. D8/303
D956,969 S * 7/2022 Bast D24/133

D982,744 S * 4/2023 Ryan D24/114
D990,666 S * 6/2023 Young D24/113
D990,667 S * 6/2023 Young D24/113
D996,606 S * 8/2023 Cowe D24/113
D1,022,197 S * 4/2024 Bajana Merizalde D24/138

FOREIGN PATENT DOCUMENTS

CN 306895636 * 10/2021
GB 6237875 * 11/2022
KR 301229617.0000 * 8/2023

OTHER PUBLICATIONS

Flexi-Q mMU Auto-Injector for Pre-Filled Syringes and Vials, Dali
Medical Devices, [Post date unknown], [Site seen: May 13, 2024],
Seen at URL: <https://www.dalimed.com/flexi-q-mmui/> (Year: 2024).*

(Continued)

Primary Examiner — Natasha Vujcic
Assistant Examiner — Gilbert B Ford
(74) Attorney, Agent, or Firm — HSML P.C.


(57) CLAIM

The ornamental design for an injector as shown and
described.

DESCRIPTION

FIG. 1 is a perspective view of an injector showing our new
design.
FIG. 2 is another perspective view of the injector with the
cap thereof removed.
FIG. 3 is a front view thereof.
FIG. 4 is a rear view thereof.
FIG. 5 is a left side view thereof.
FIG. 6 is a right side view thereof.
FIG. 7 is a top view thereof; and,
FIG. 8 is a bottom view thereof.
The dashed broken lines in the drawings show portions of
the injector that form no part of the claimed design.

1 Claim, 5 Drawing Sheets

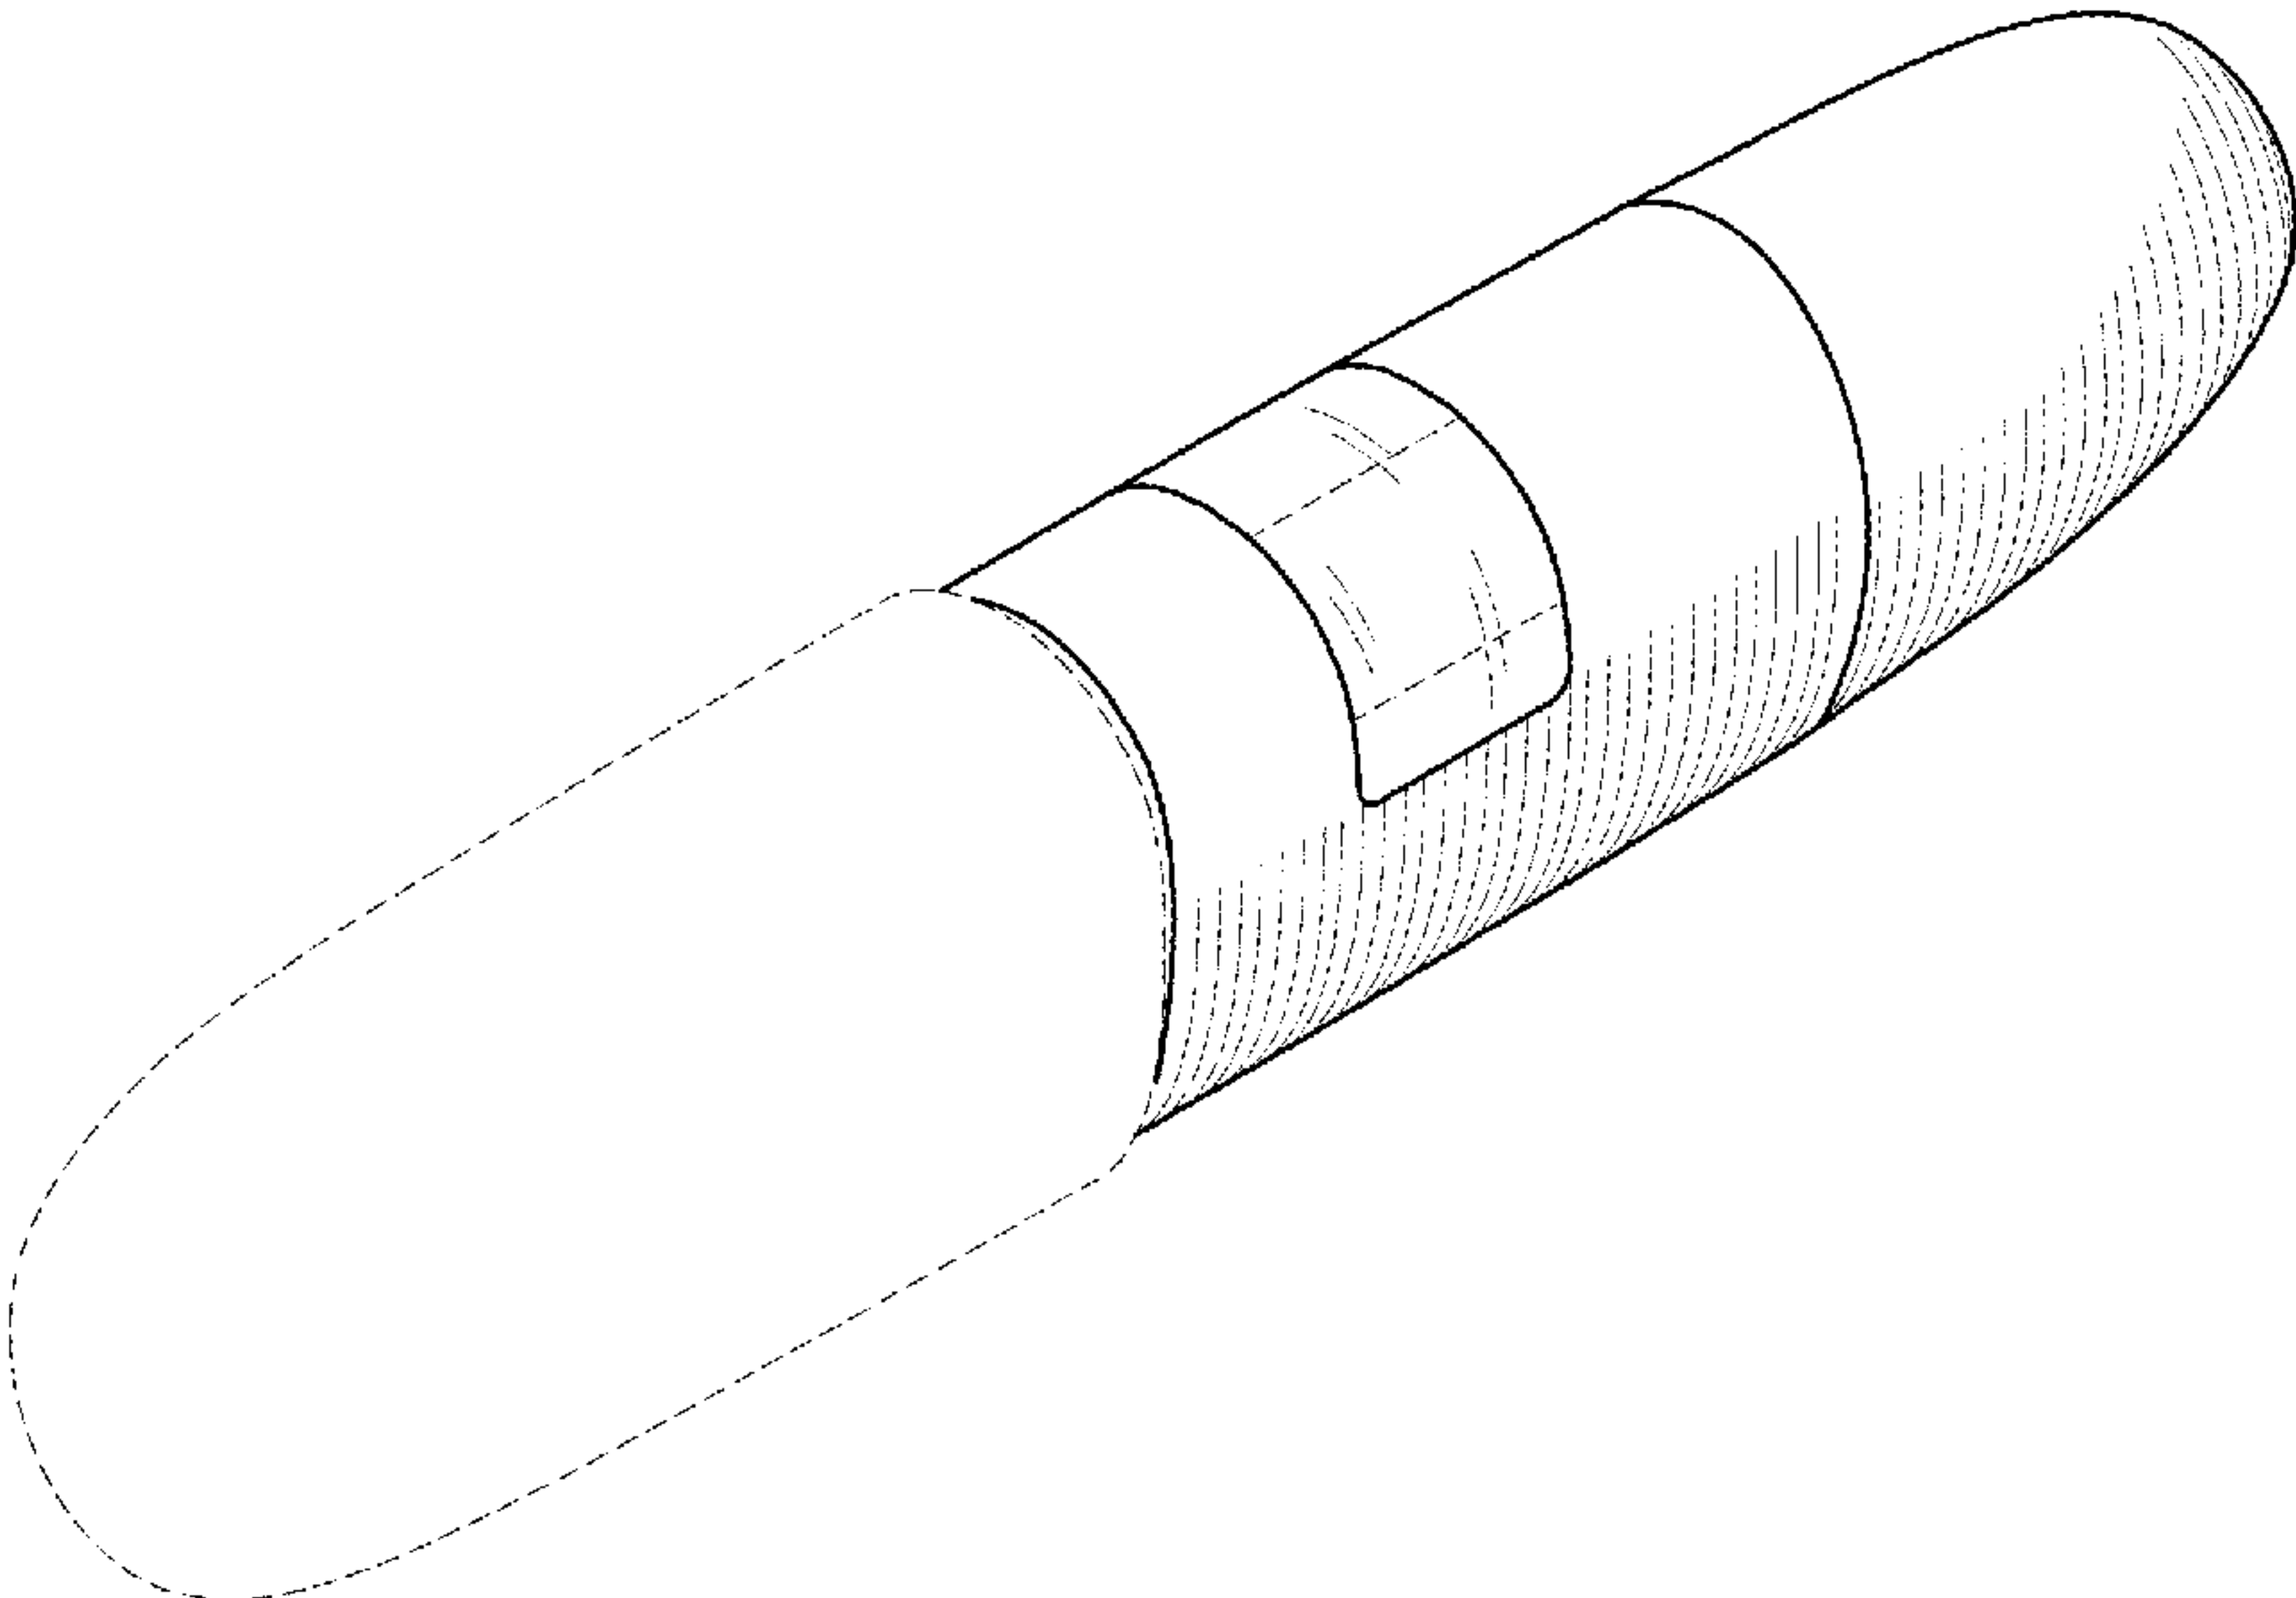

(56)

References Cited

OTHER PUBLICATIONS

Prefilled Primary Drug Container, Oval Medical, Pharmaceutical Online, [Post date: Sep. 24, 2020], [Site seen: May 13, 2024], URL:<https://www.pharmaceuticalonline.com/doc/improved-autoinjector-design-demonstrating-highly-consistent-performance-achieved-through-the-integration-of-a-cyclic-olefin-syringe-0001> (Year: 2020).*

“Special Feature—Injection Devices” Drug Device.com, [Post date: Sep. 1, 2023], [Site seen: May 13, 2024], Seen at URL: <https://drug-dev.com/special-feature-injection-devices-designing-in-sustainability-usability-digitization-for-patient-compliance/> (Year: 2023).*

* cited by examiner

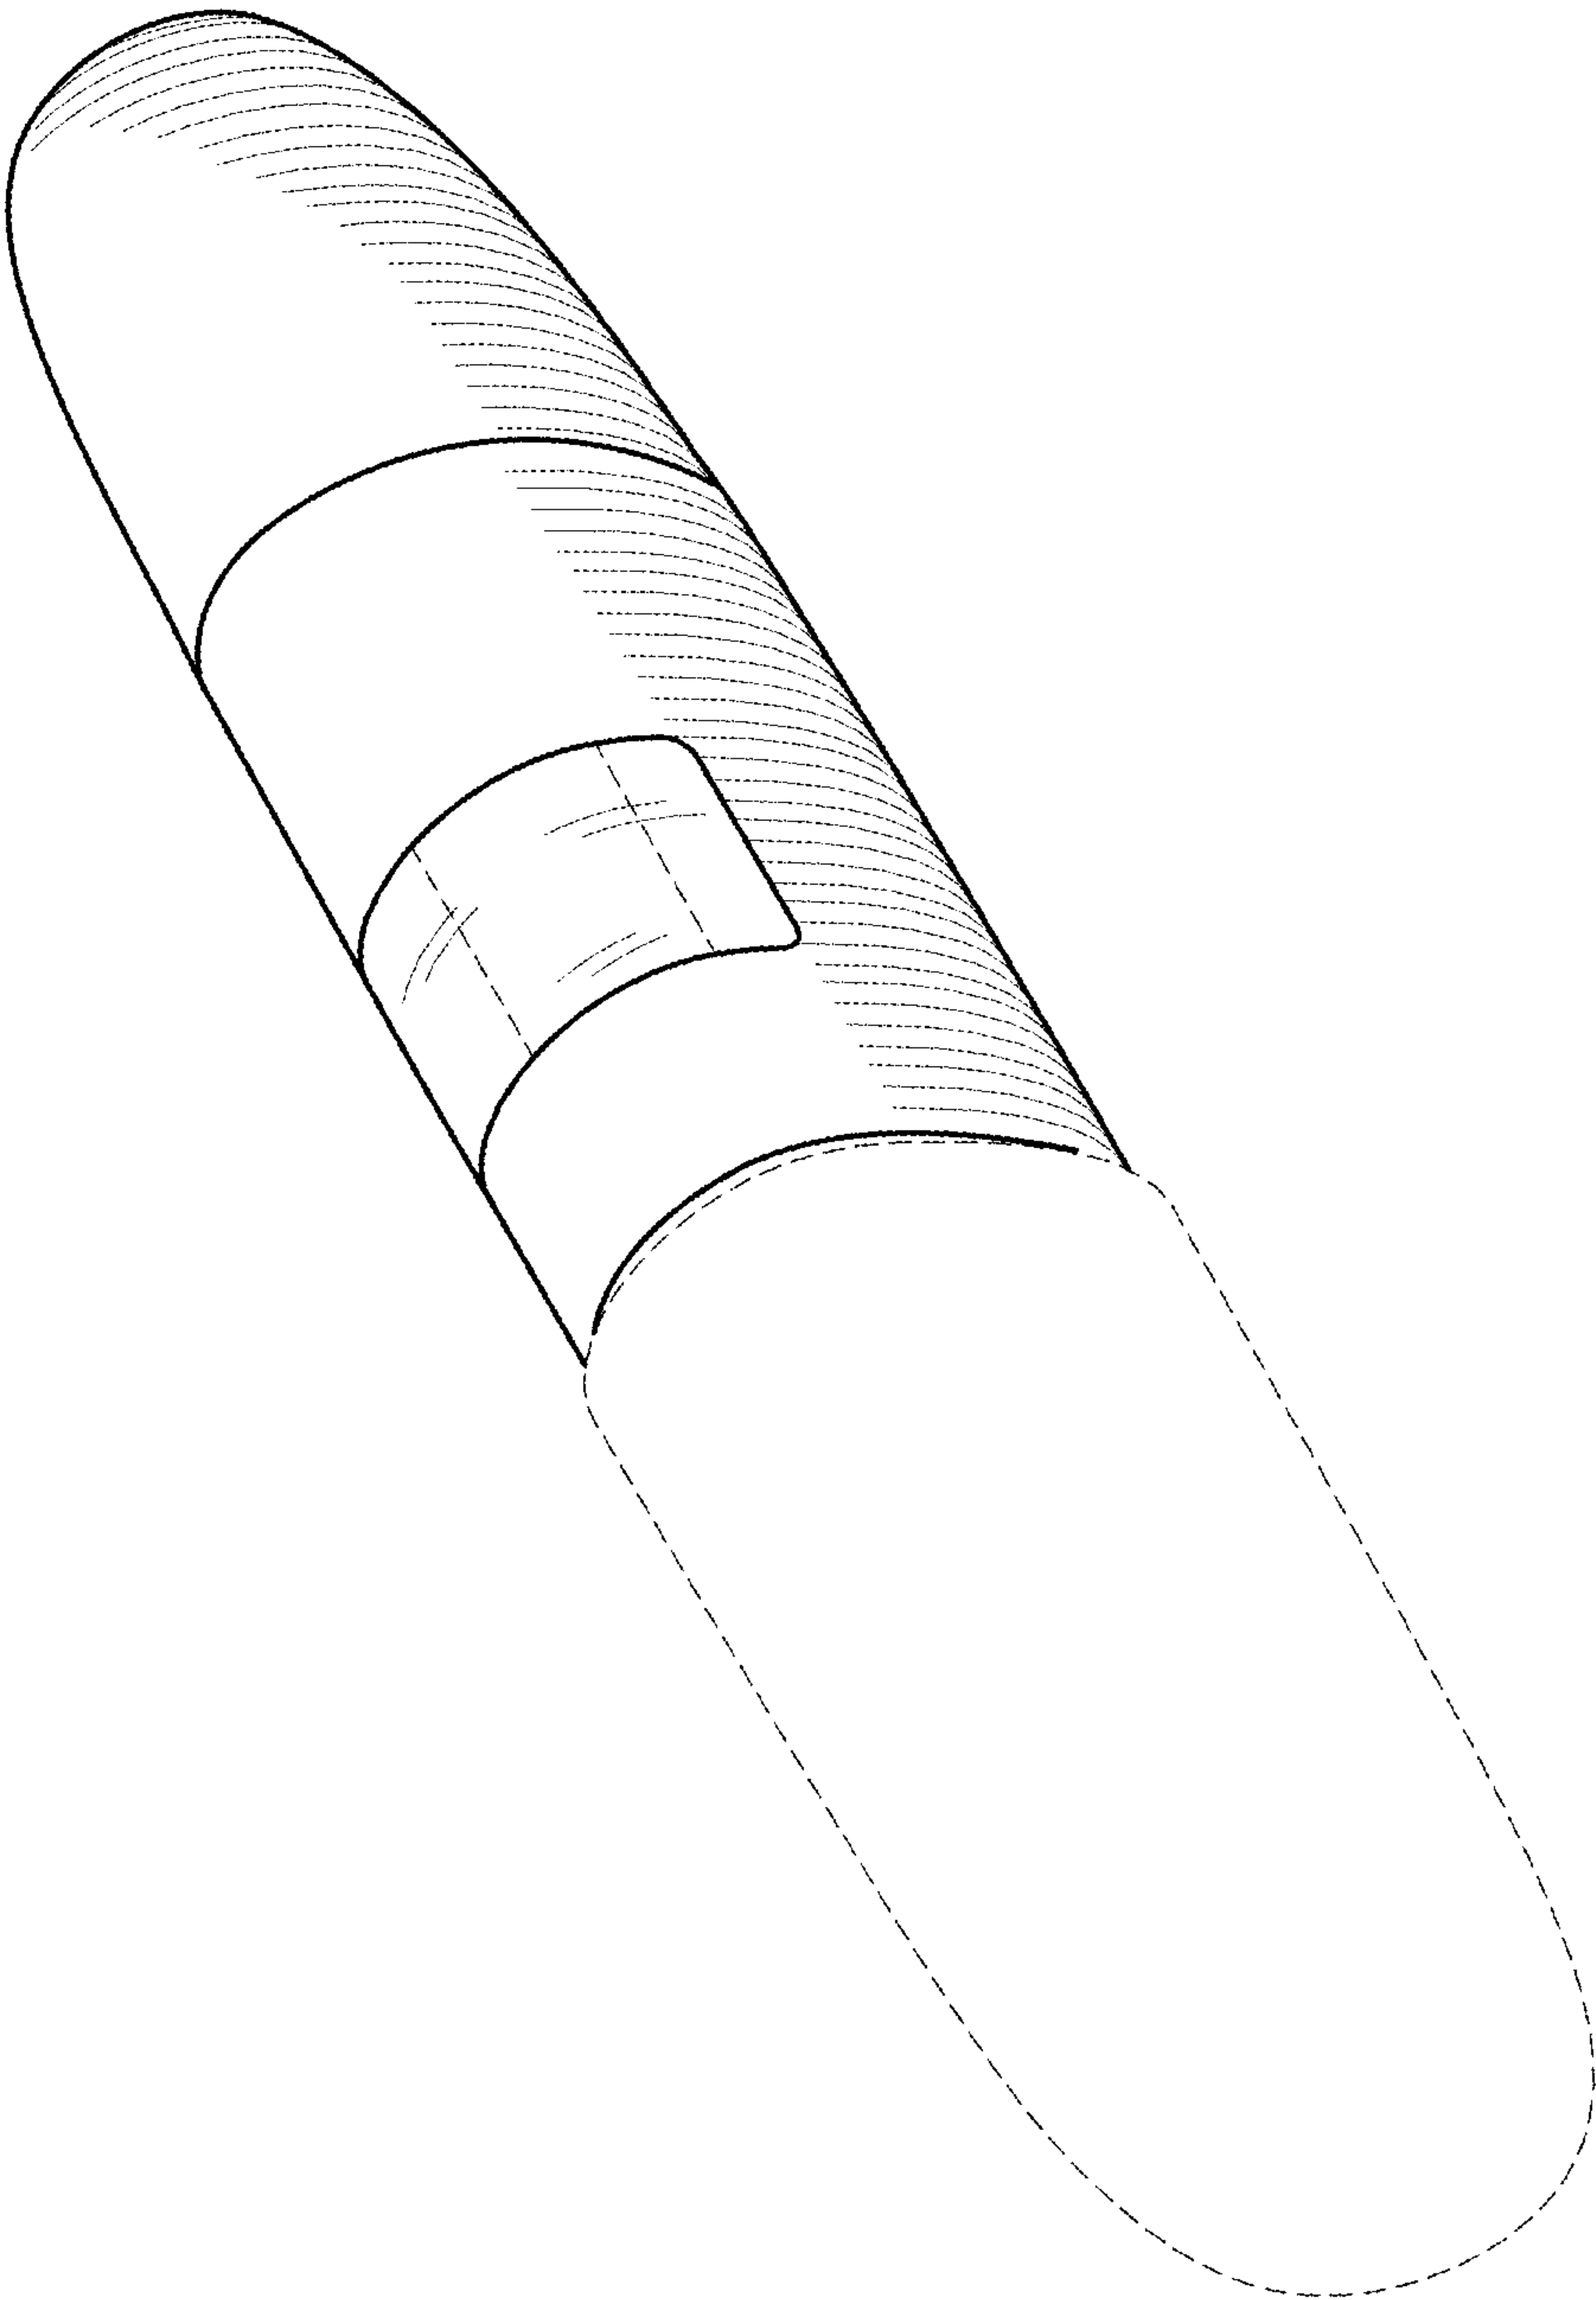


Fig. 1

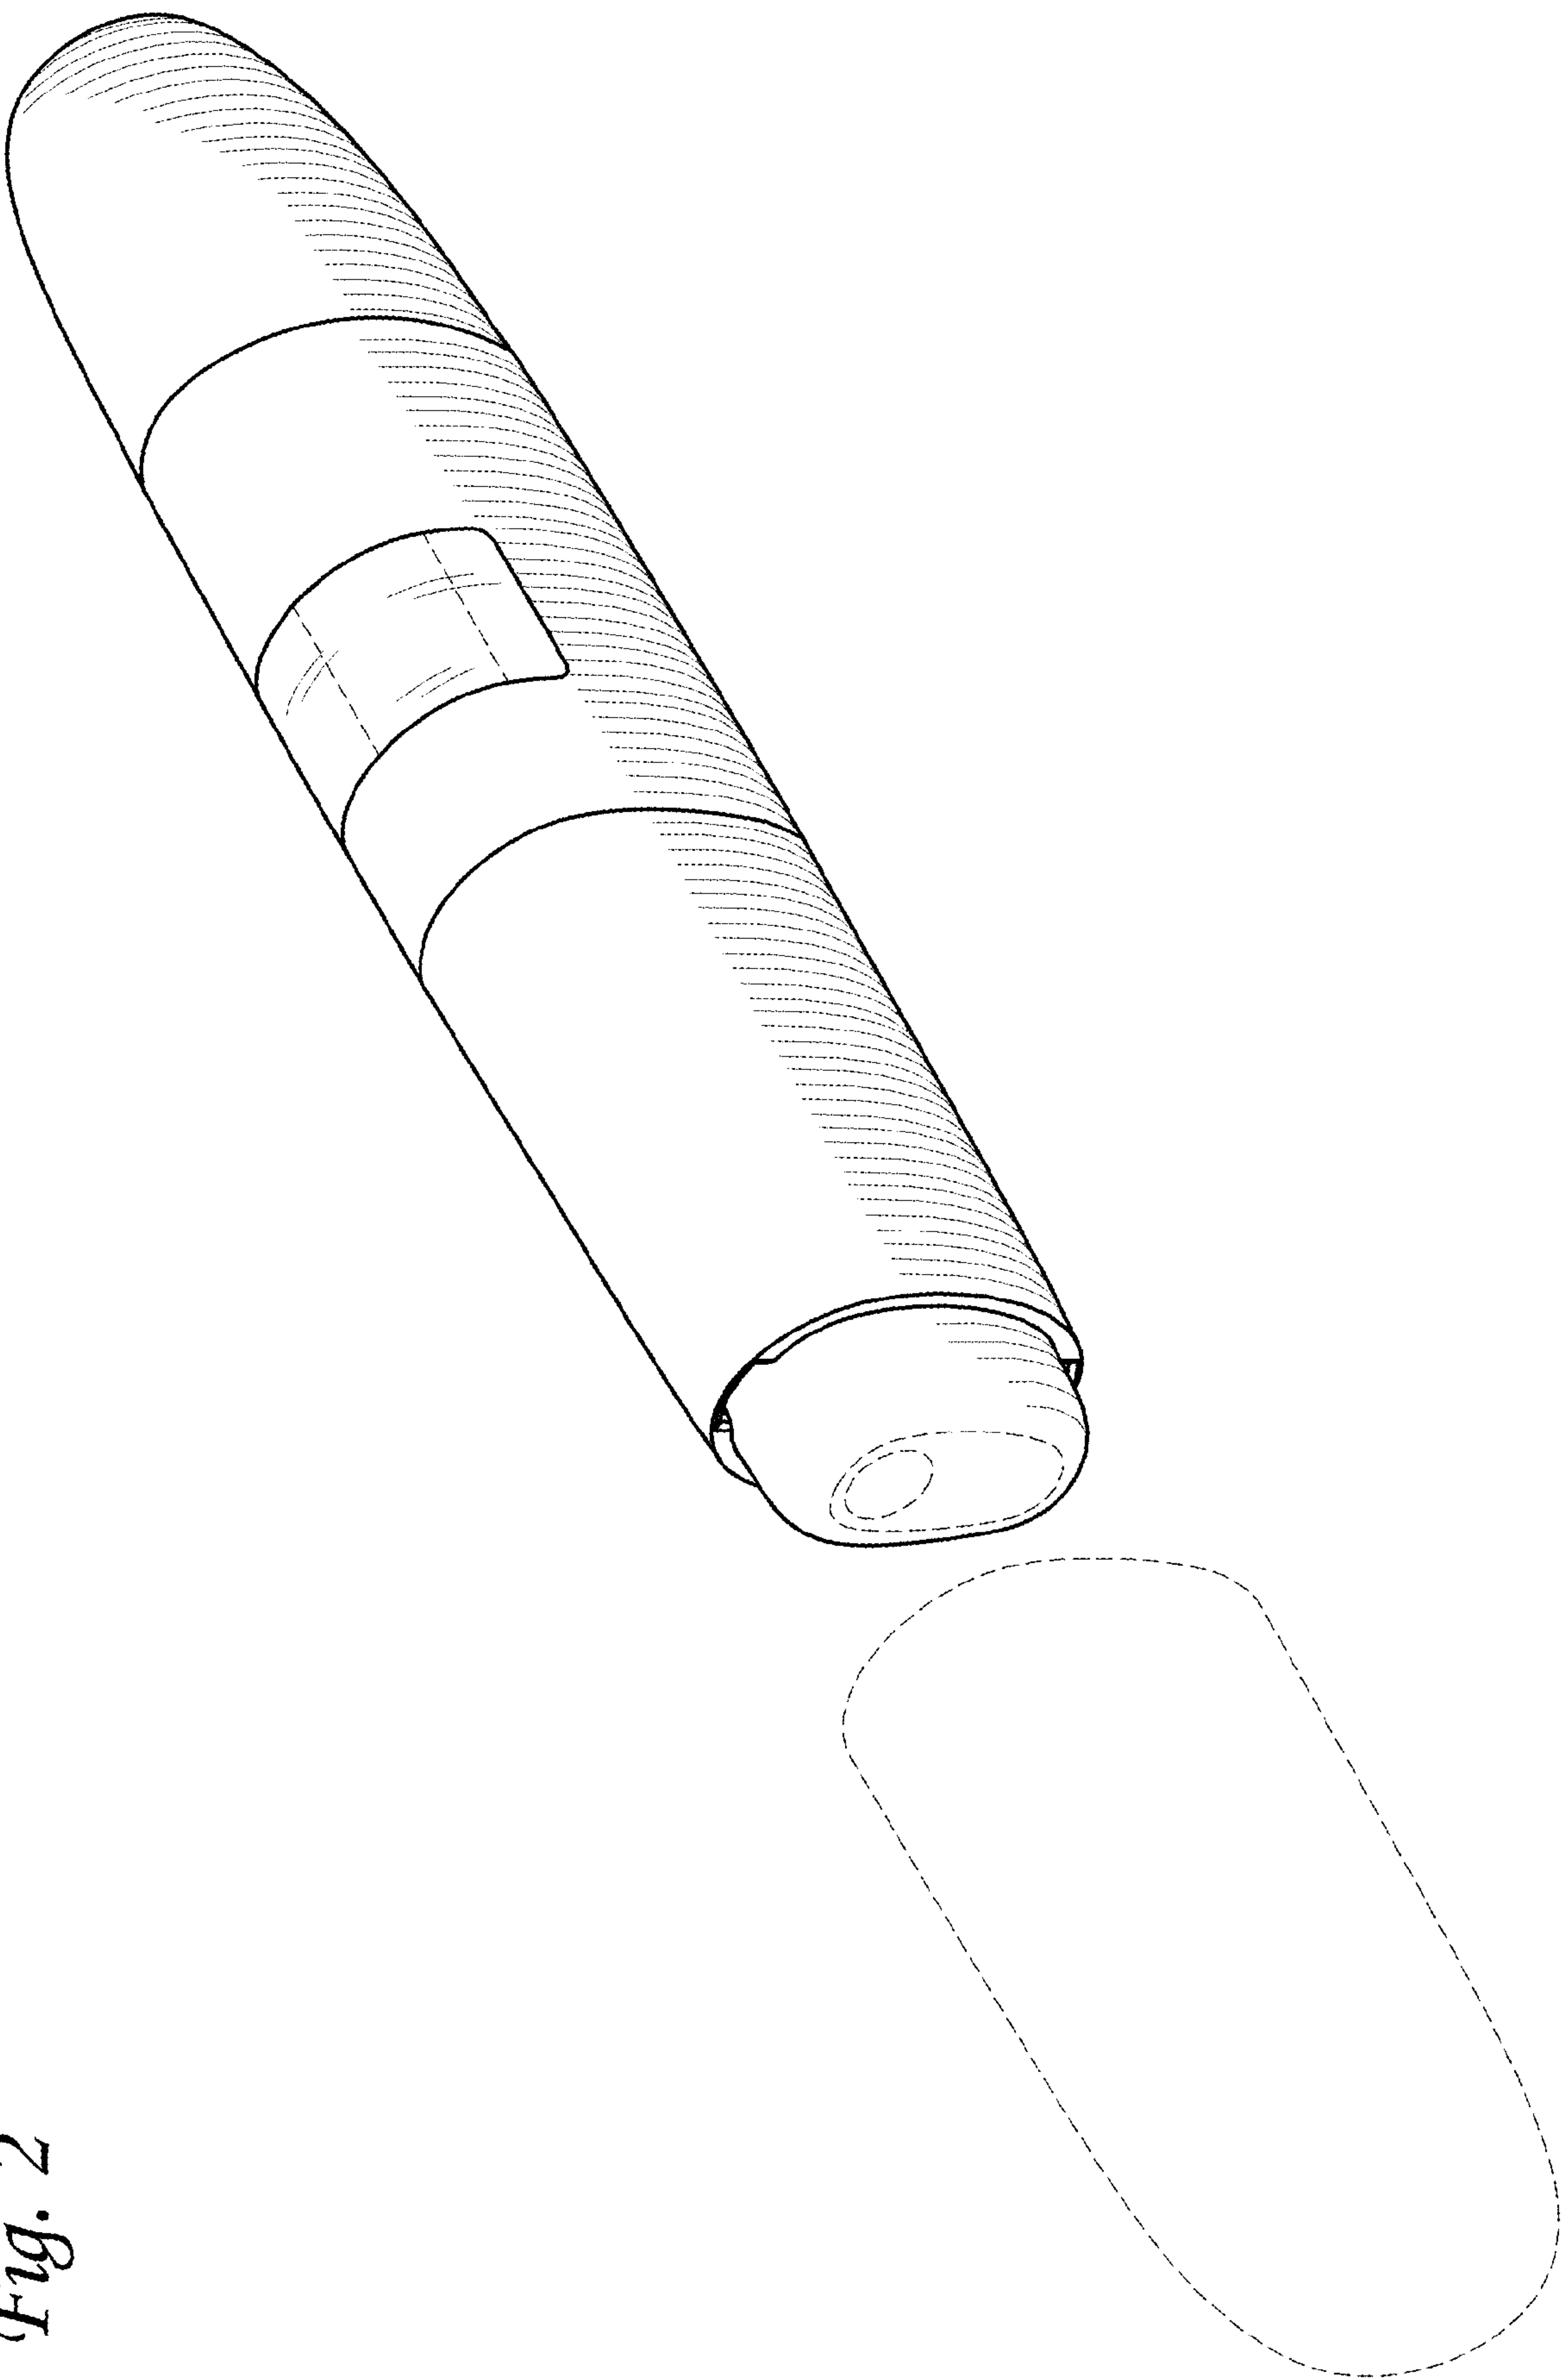


Fig. 2

Fig. 3

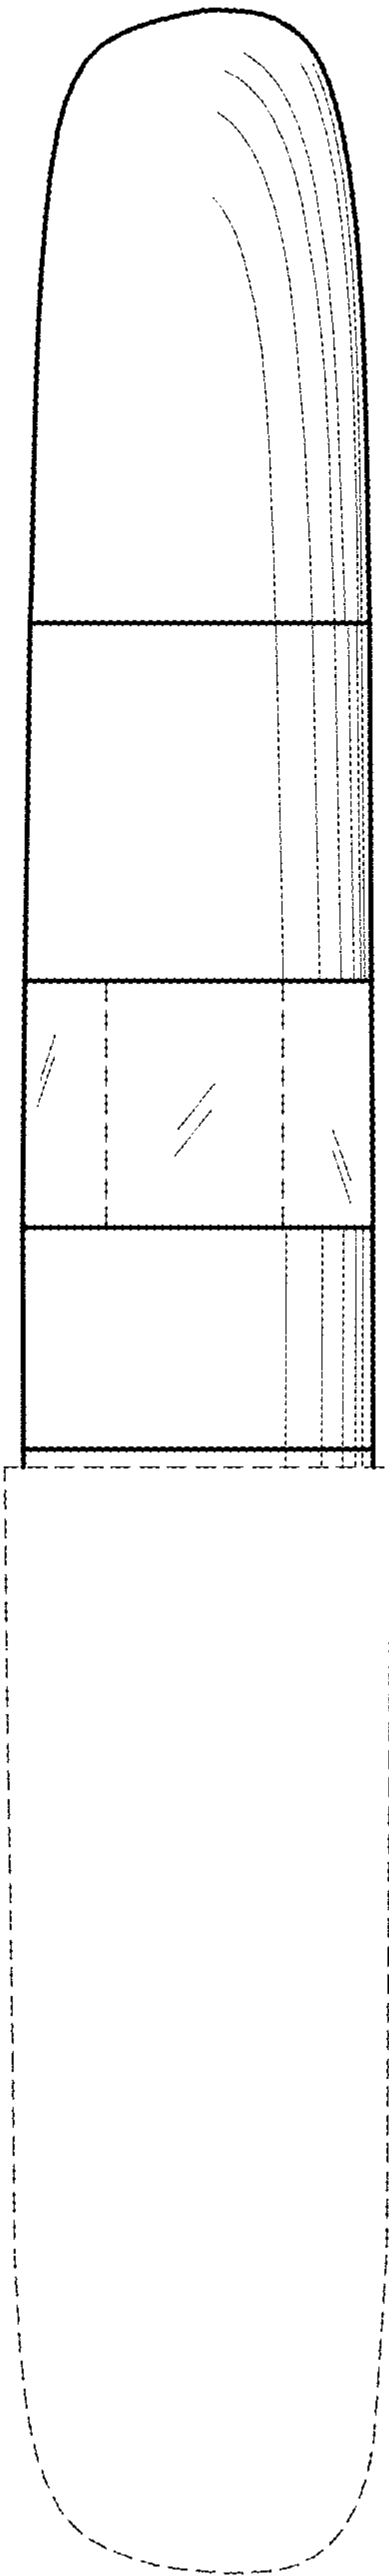


Fig. 4

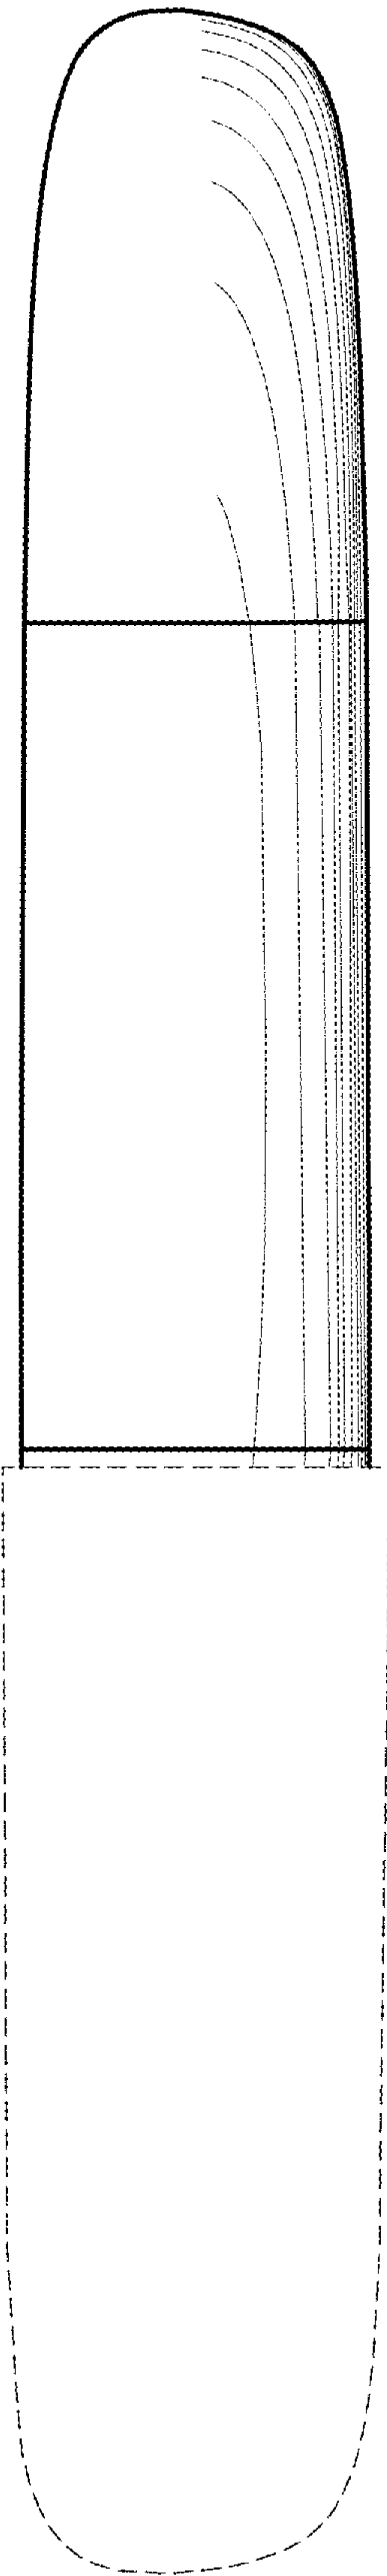


Fig. 5

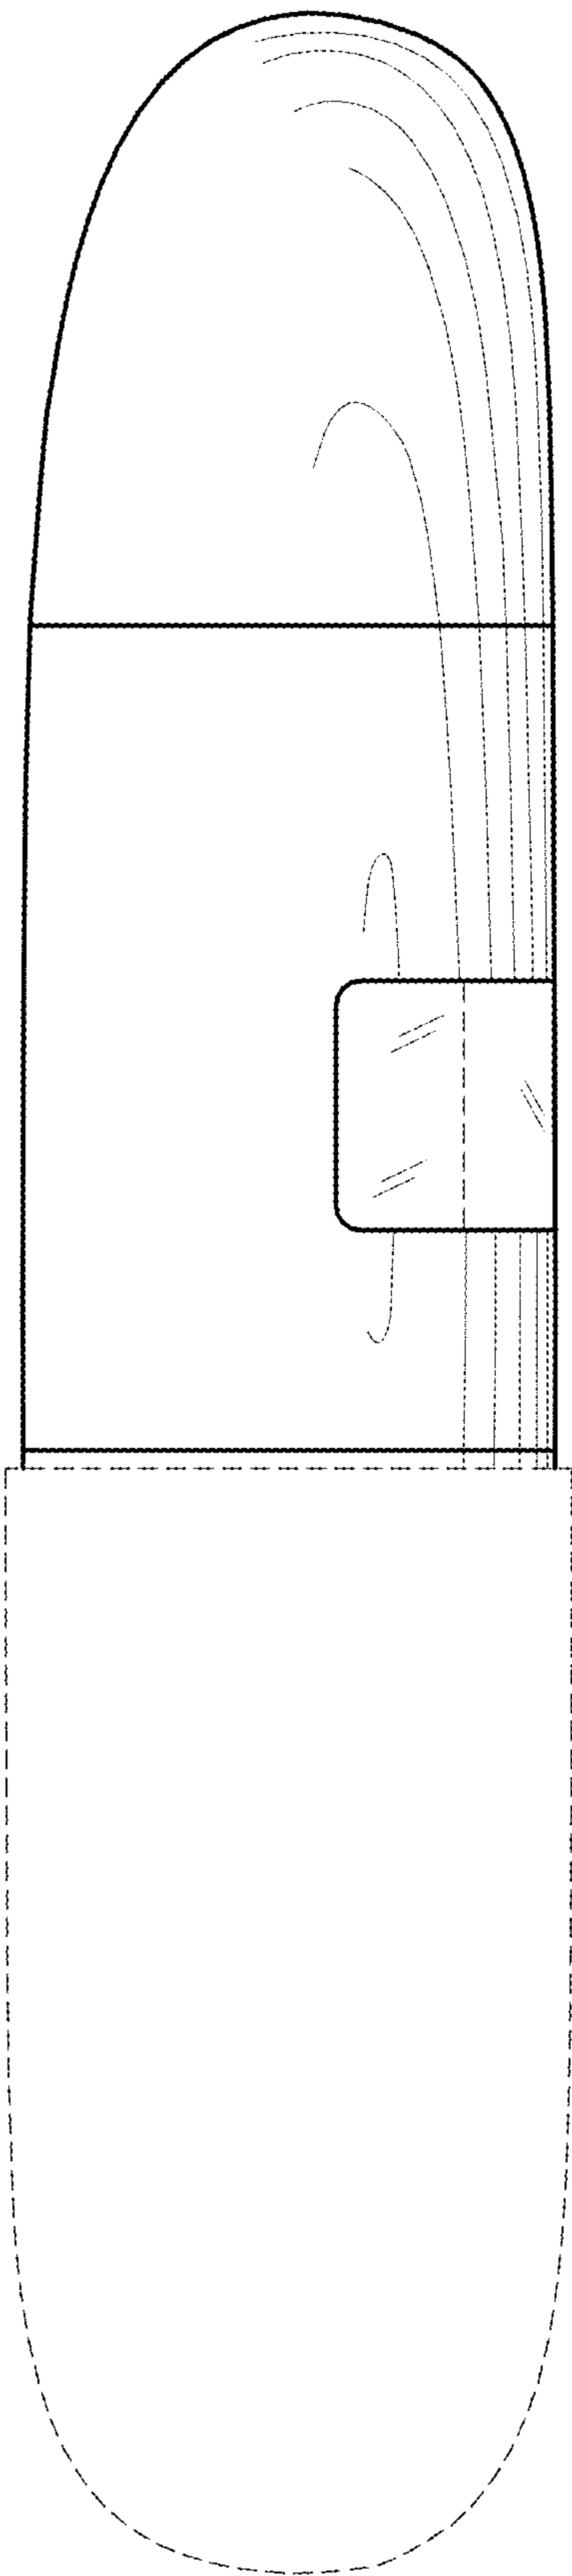


Fig. 6

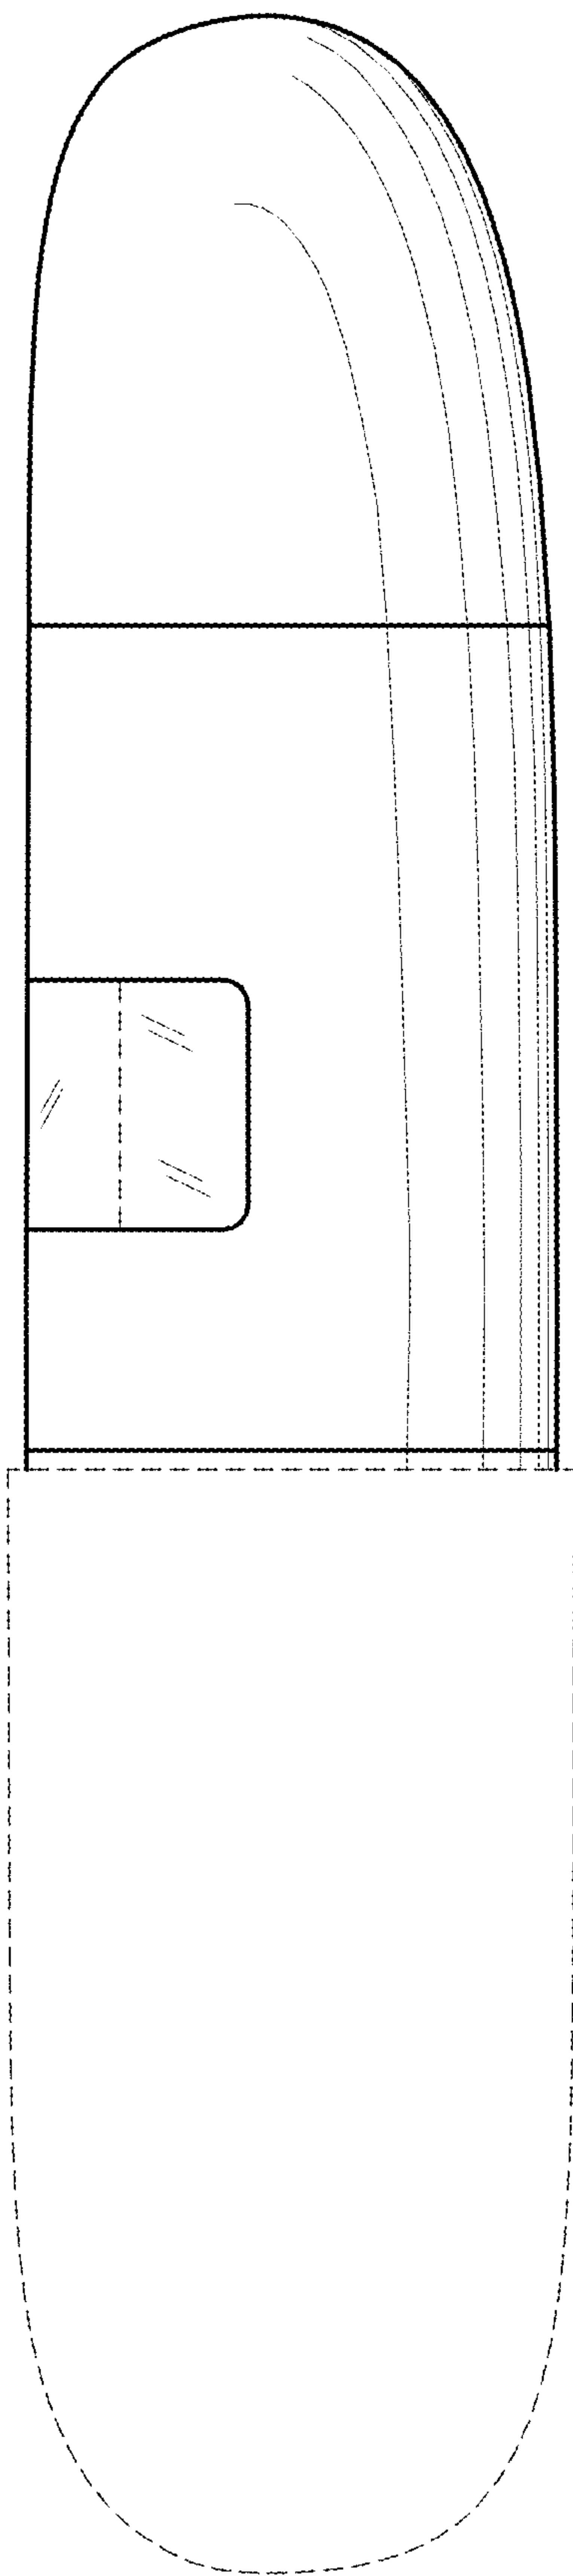


Fig. 7

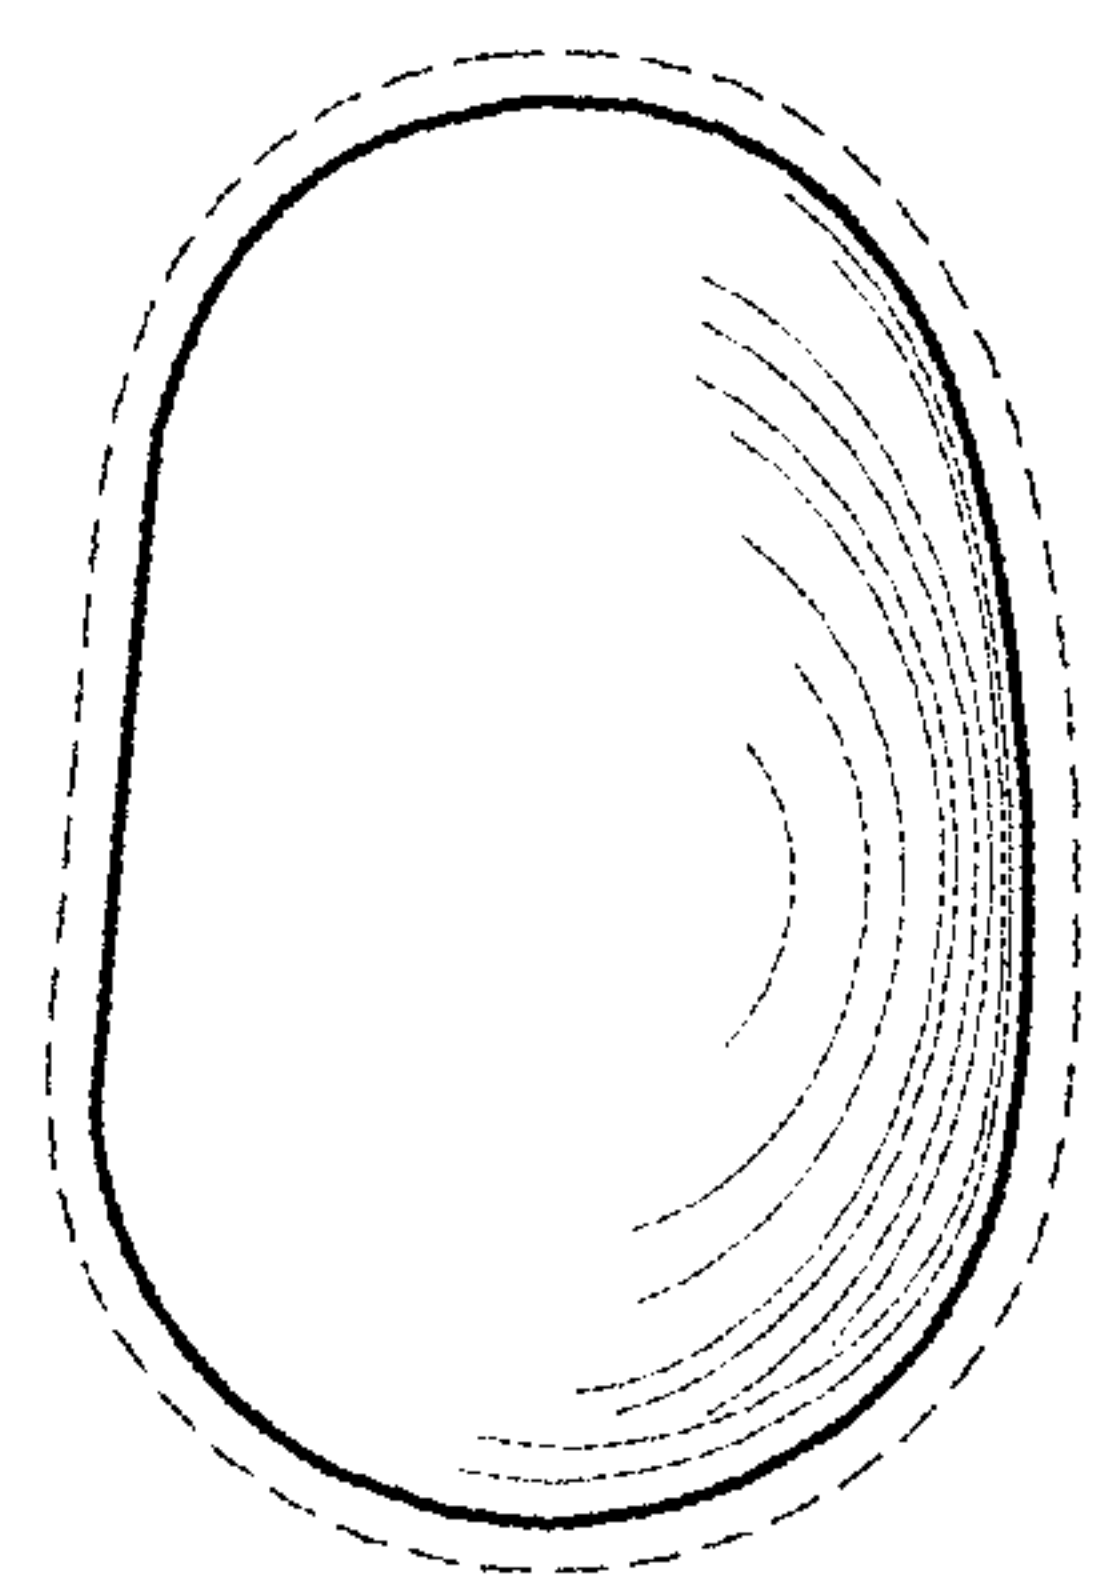


Fig. 8

