



US0D1050478S

(12)

United States Design Patent

McAteer et al.

(10)

Patent No.:

US D1,050,478 S

(45)

Date of Patent:

** Nov. 5, 2024

(54) PLATELET-RICH PLASMA ACTIVATION DEVICE

(71) Applicant: Curative Sound, LLC, Carmel, IN (US)

(72) Inventors: Jeffrey Phillip McAteer, Carmel, IN (US); Geoffrey N. Barber, New Castle, IN (US); Randal Douglas Wood, New Palestine, IN (US); Matthew C. Haws, Noblesville, IN (US); James V. Olson, Jr., Indianapolis, IN (US)

(73) Assignee: Curative Sound, LLC, Carmel, IN (US)

(**) Term: 15 Years

(21) Appl. No.: 29/864,891

(22) Filed: Jun. 27, 2022

(51) LOC (14) Cl. 24-02

(52) U.S. Cl. USPC D24/216

(58) Field of Classification Search USPC D24/107, 108, 130, 133, 186, 216, 231, D24/232; D10/81 CPC G01N 2035/00306; G01N 2030/027; G01N 21/76; G01N 2035/0029; G01N 35/0029 See application file for complete search history.

(56) References Cited

U.S. PATENT DOCUMENTS

D266,189 S * 9/1982 Safianoff D24/117

D480,137 S * 9/2003 Nilsson D24/108

D627,081 S * 11/2010 Giraud D24/216

D658,307 S * 4/2012 Recchi D24/216

D921,918 S * 6/2021 Eriksson D24/216

(Continued)

FOREIGN PATENT DOCUMENTS

CN 303370981 * 9/2015

CN 308168962 * 8/2023

(Continued)

OTHER PUBLICATIONS

“LinkedIn: Lance Liberti, MBA.” Found online May 3, 2024 at linkedin.com. Reference dated Jan. 24, 2022. Retrieved from https://www.linkedin.com/pulse/photoactivation-platelet-rich-plasma-lance-liberti-mba.*

(Continued)

Primary Examiner — Kendra Leslie Hamilton

Assistant Examiner — Elizabeth S Struble

(74) Attorney, Agent, or Firm — Maginot, Moore & Beck

(57) CLAIM

The ornamental design for a platelet-rich plasma activation device as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of a platelet-rich plasma activation device showing our new design;

FIG. 2 is a front side elevational view of the platelet-rich plasma activation device of FIG. 1;

FIG. 3 is a rear side elevational view of the platelet-rich plasma activation device of FIG. 1;

FIG. 4 is a right side elevational view of the platelet-rich plasma activation device of FIG. 1;


FIG. 5 is a left side elevational view of the platelet-rich plasma activation device of FIG. 1;

FIG. 6 is a top plan view of the platelet-rich plasma activation device of FIG. 1; and,

FIG. 7 is a bottom plan view of the platelet-rich plasma activation device of FIG. 1.

The dashed broken lines shown in the drawings depict portions of the platelet-rich plasma activation device that form no part of the claimed design. The dash-dot-dash broken lines shown in the drawings define the bounds of the claimed design and form no part of the claimed design.

1 Claim, 7 Drawing Sheets

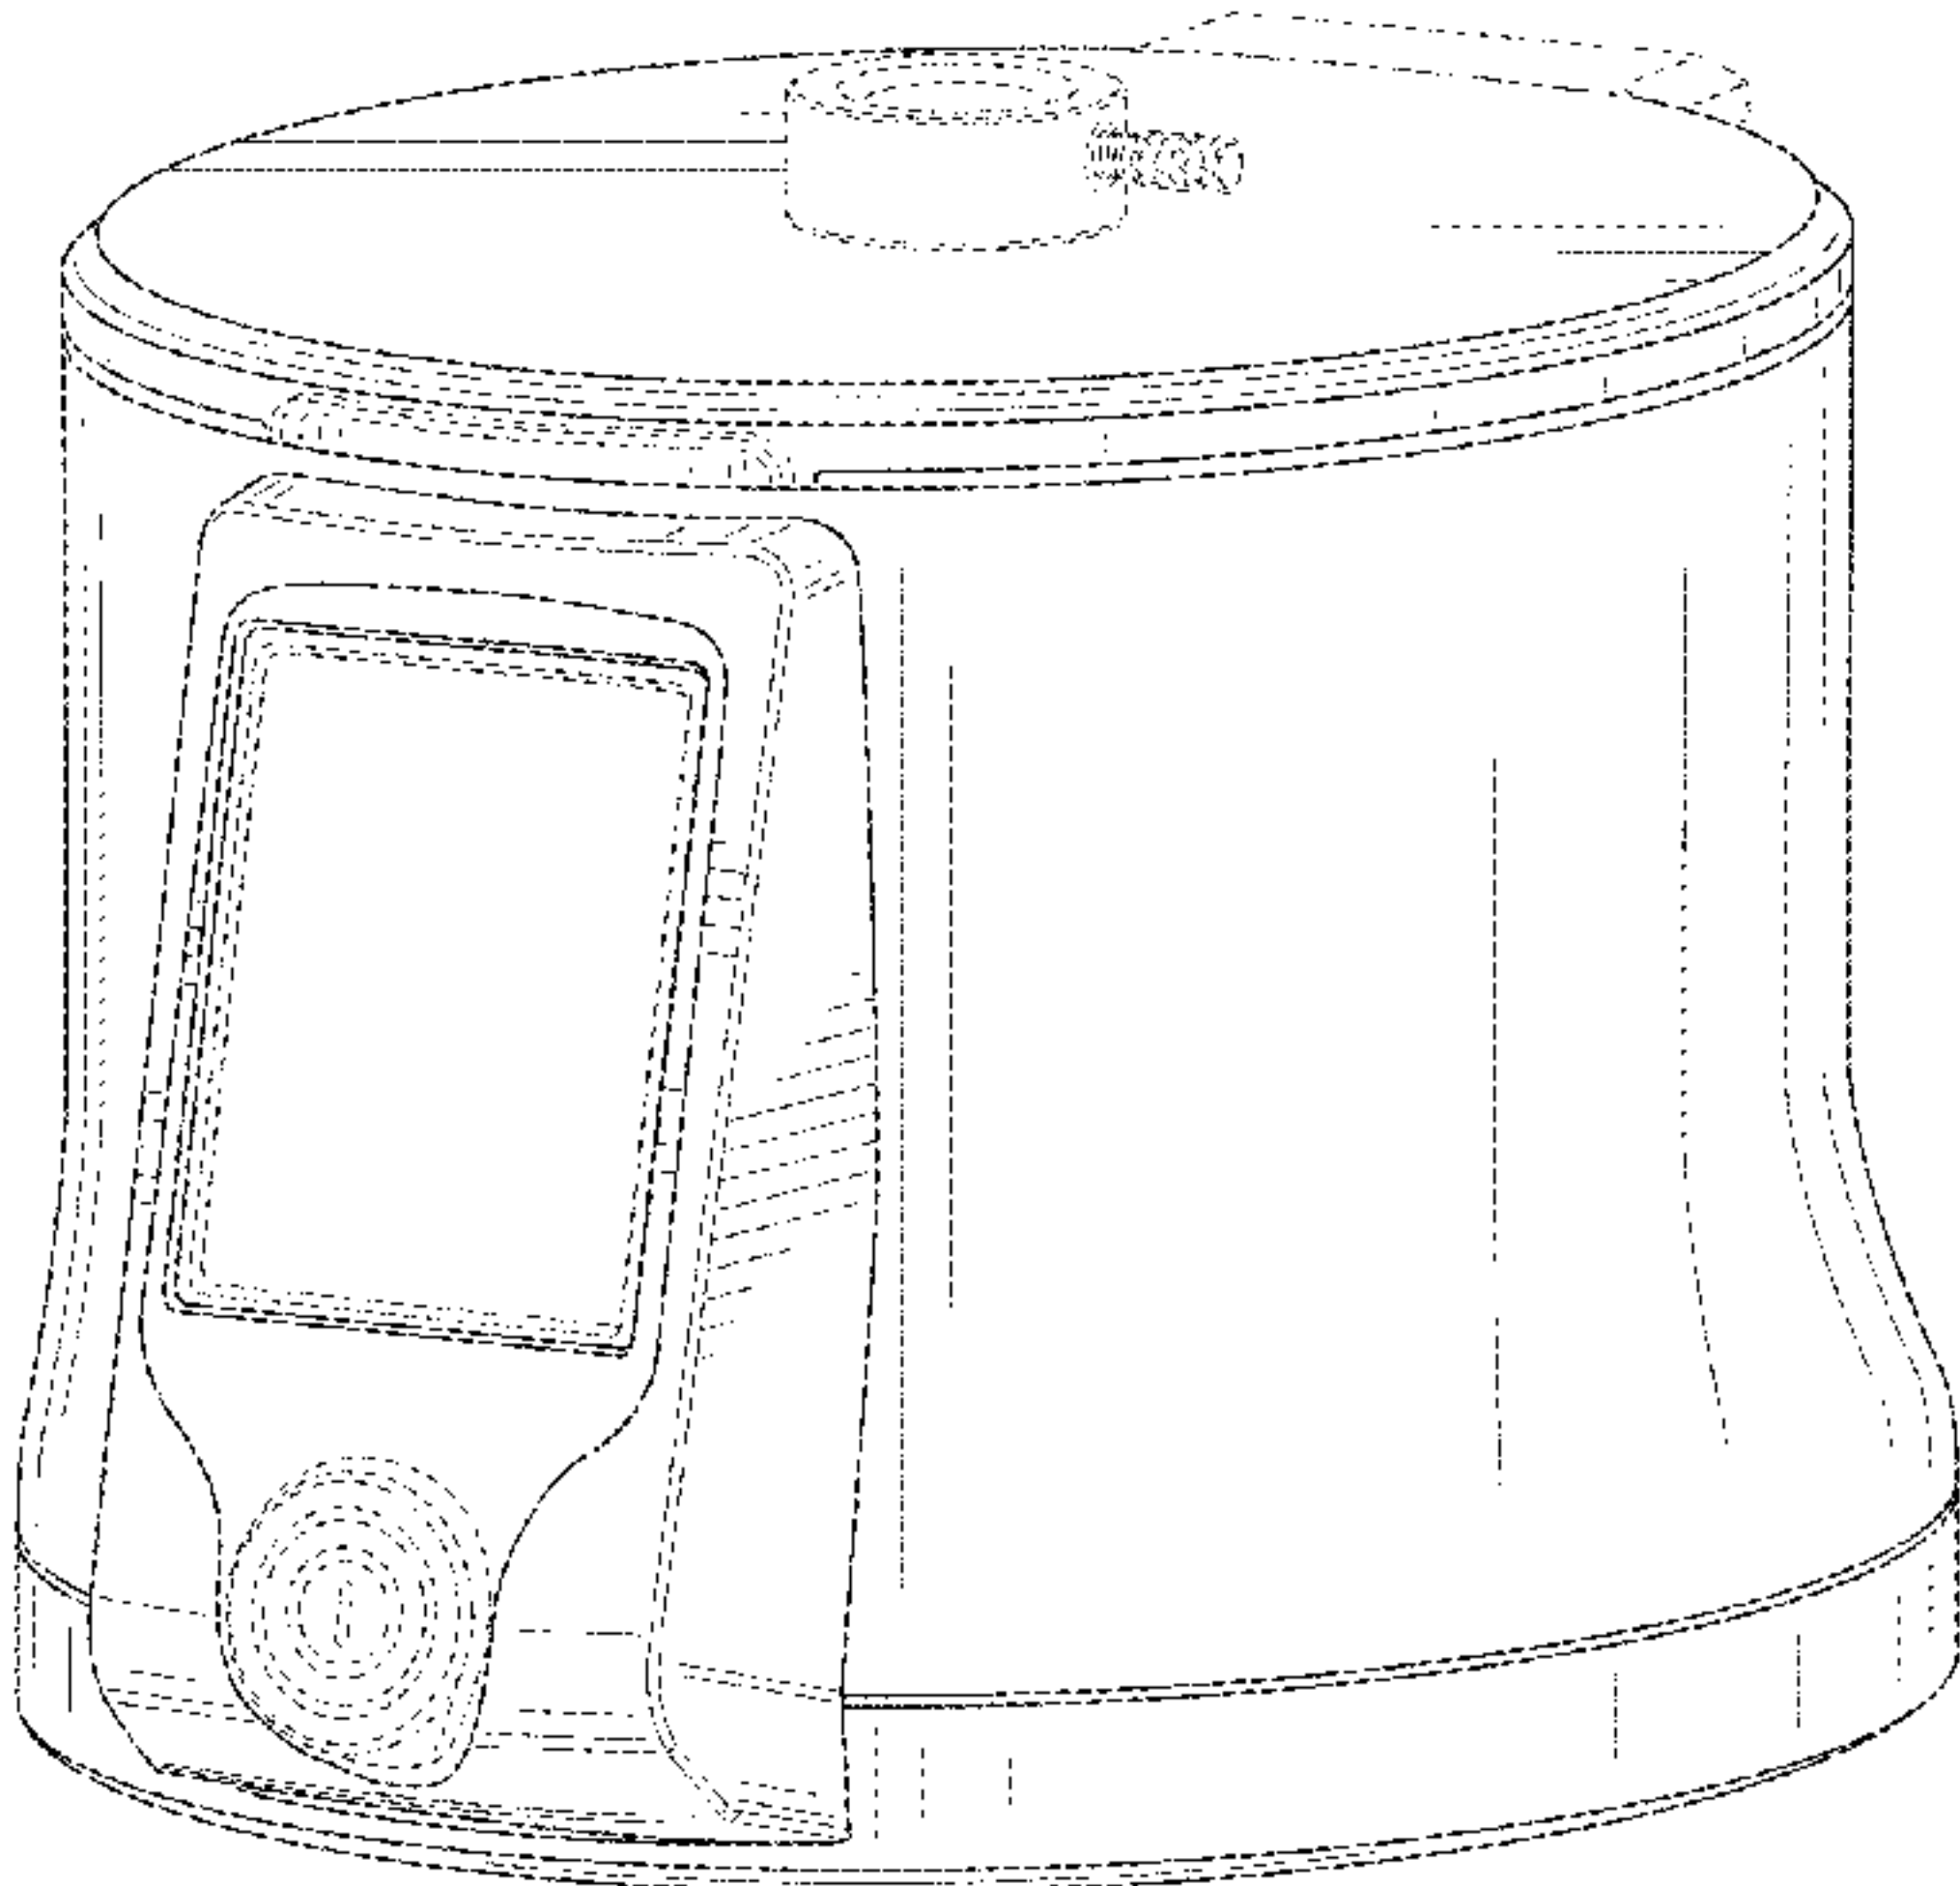

(56)

References Cited

OTHER PUBLICATIONS

U.S. PATENT DOCUMENTS

D925,759 S * 7/2021 Suzuki D24/216
D963,882 S * 9/2022 Birdsall D24/216
D977,138 S * 1/2023 Crockett D24/216
D1,001,266 S * 10/2023 Proctor D24/107
D1,012,899 S * 1/2024 Chen D24/231
2002/0049401 A1 * 4/2002 Ghelli B01D 61/58
604/6.14
2021/0086001 A1 * 3/2021 Hoffman A61H 1/00
2023/0172623 A1 * 6/2023 McAteer A61B 17/22
600/437

FOREIGN PATENT DOCUMENTS

CN 308305628 * 11/2023
CN 308452667 * 2/2024

“Soko: Extracorporeal Shockwave Therapy Machine.” Found online May 3, 2024 at amazon.com. Reference dated Sep. 20, 2023. Retrieved from <https://www.amazon.com/SOKO-Extracorporeal-Shockwave-Physical-Treatment/dp/B0CJFPQWYN>.
“German Journal of Sports Medicine: Case Report.” Found online May 3, 2024 at germanjournalsportsmedicine.com. Reference dated Apr. 2023. Retrieved from <https://www.germanjournalsportsmedicine.com/archive/archive-2023/issue-2/use-of-combined-shockwave-therapy-and-platelet-rich-plasma-injection-for-management-of-chron>.
“East Coast Podiatry: Extracorporeal Shockwave Therapy.” Found online May 3, 2024 at youtube.com. Reference dated Sep. 7, 2024. Retrieved from <https://www.youtube.com/watch?v=Uprz-p4dAH8>.

* cited by examiner

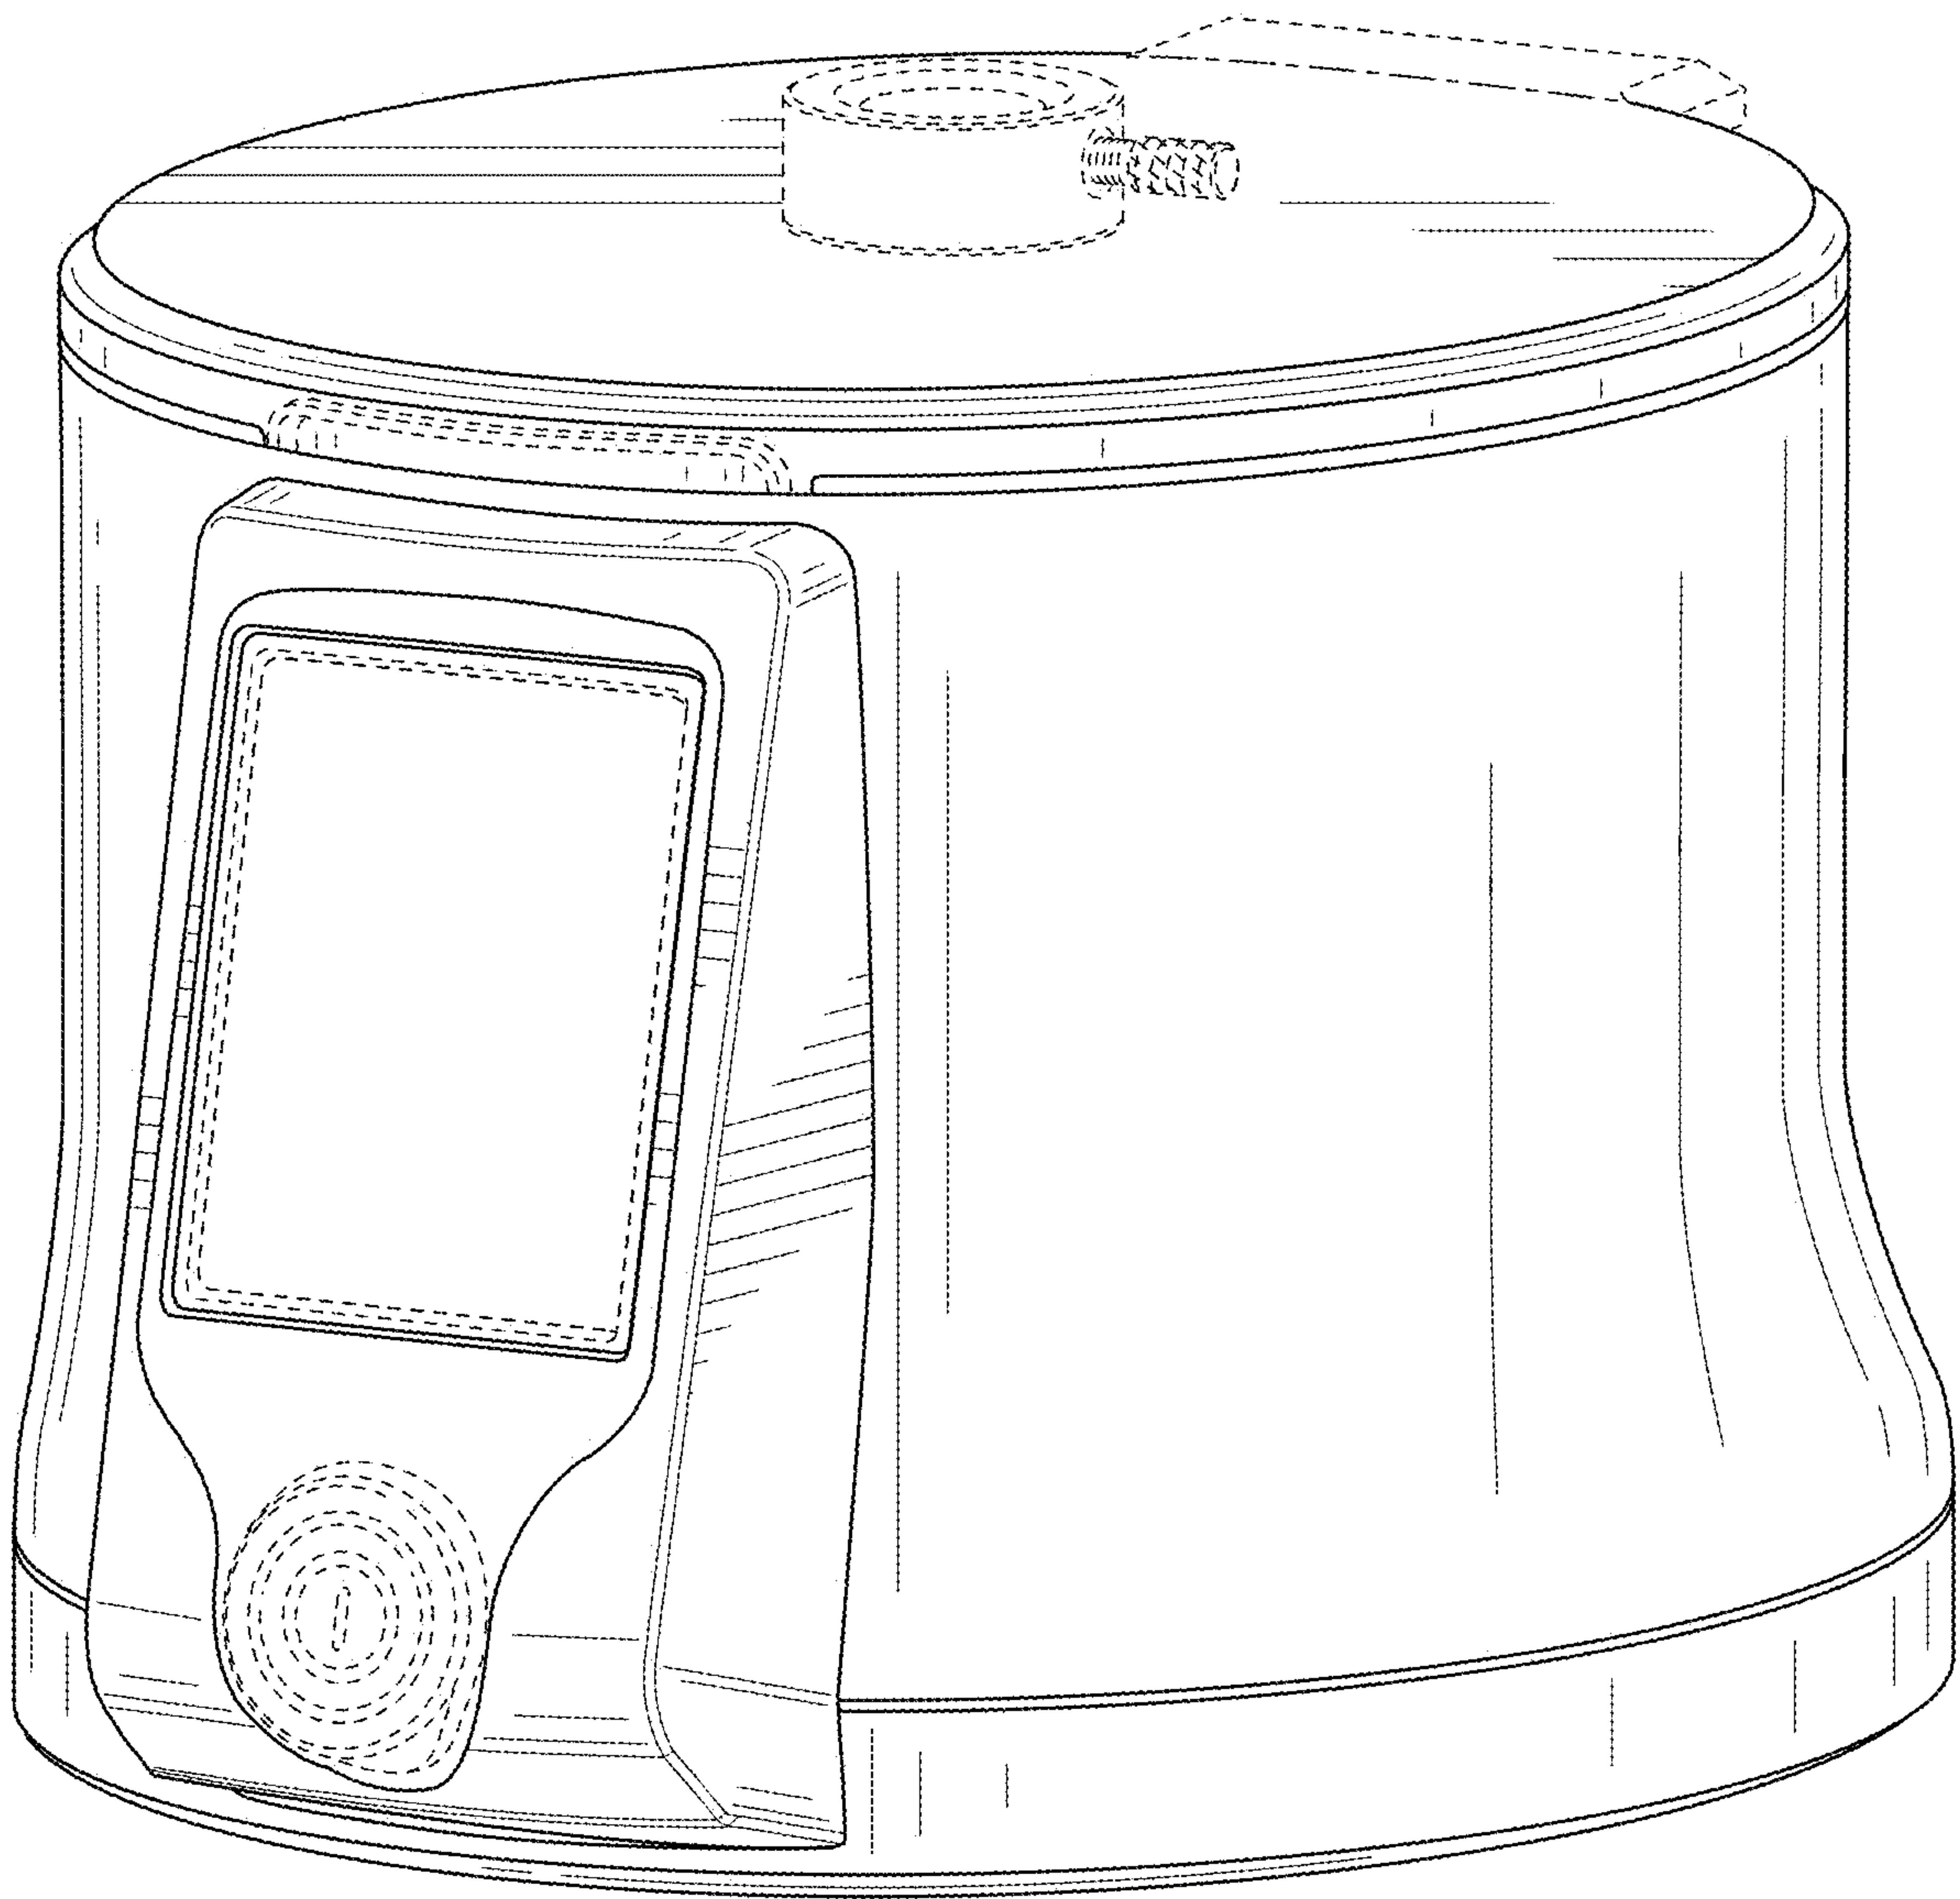


FIG. 1

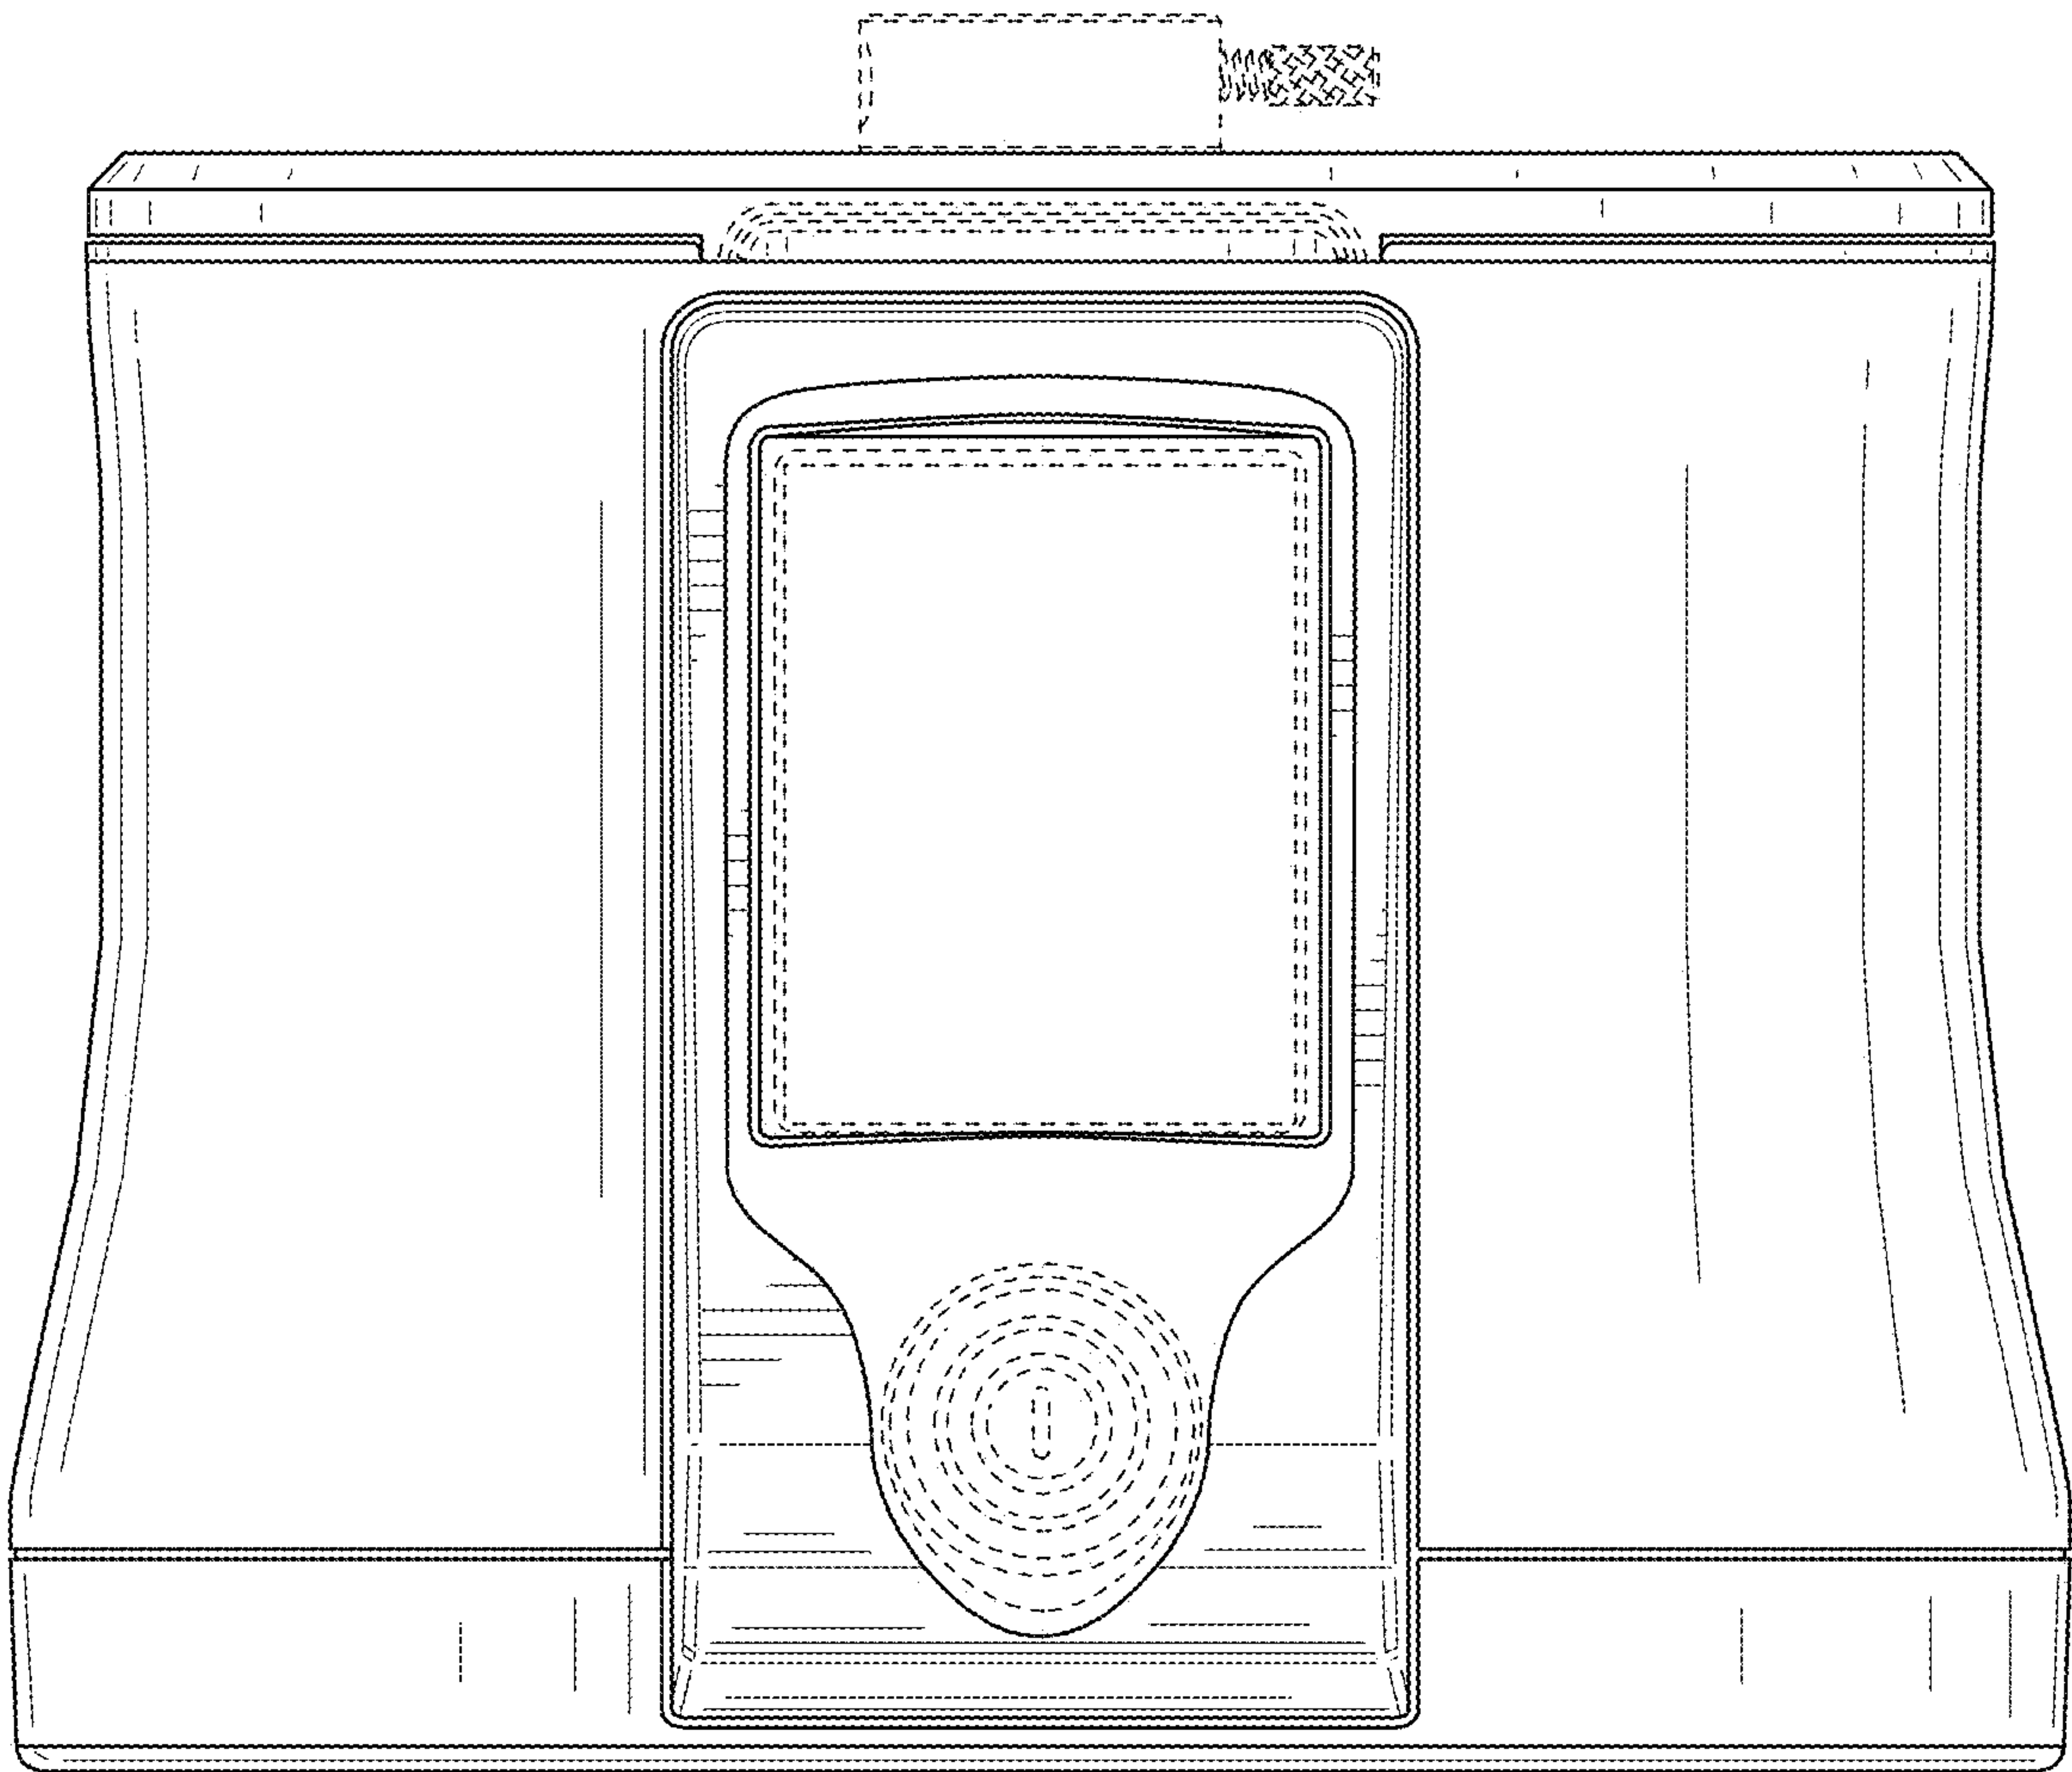


FIG. 2

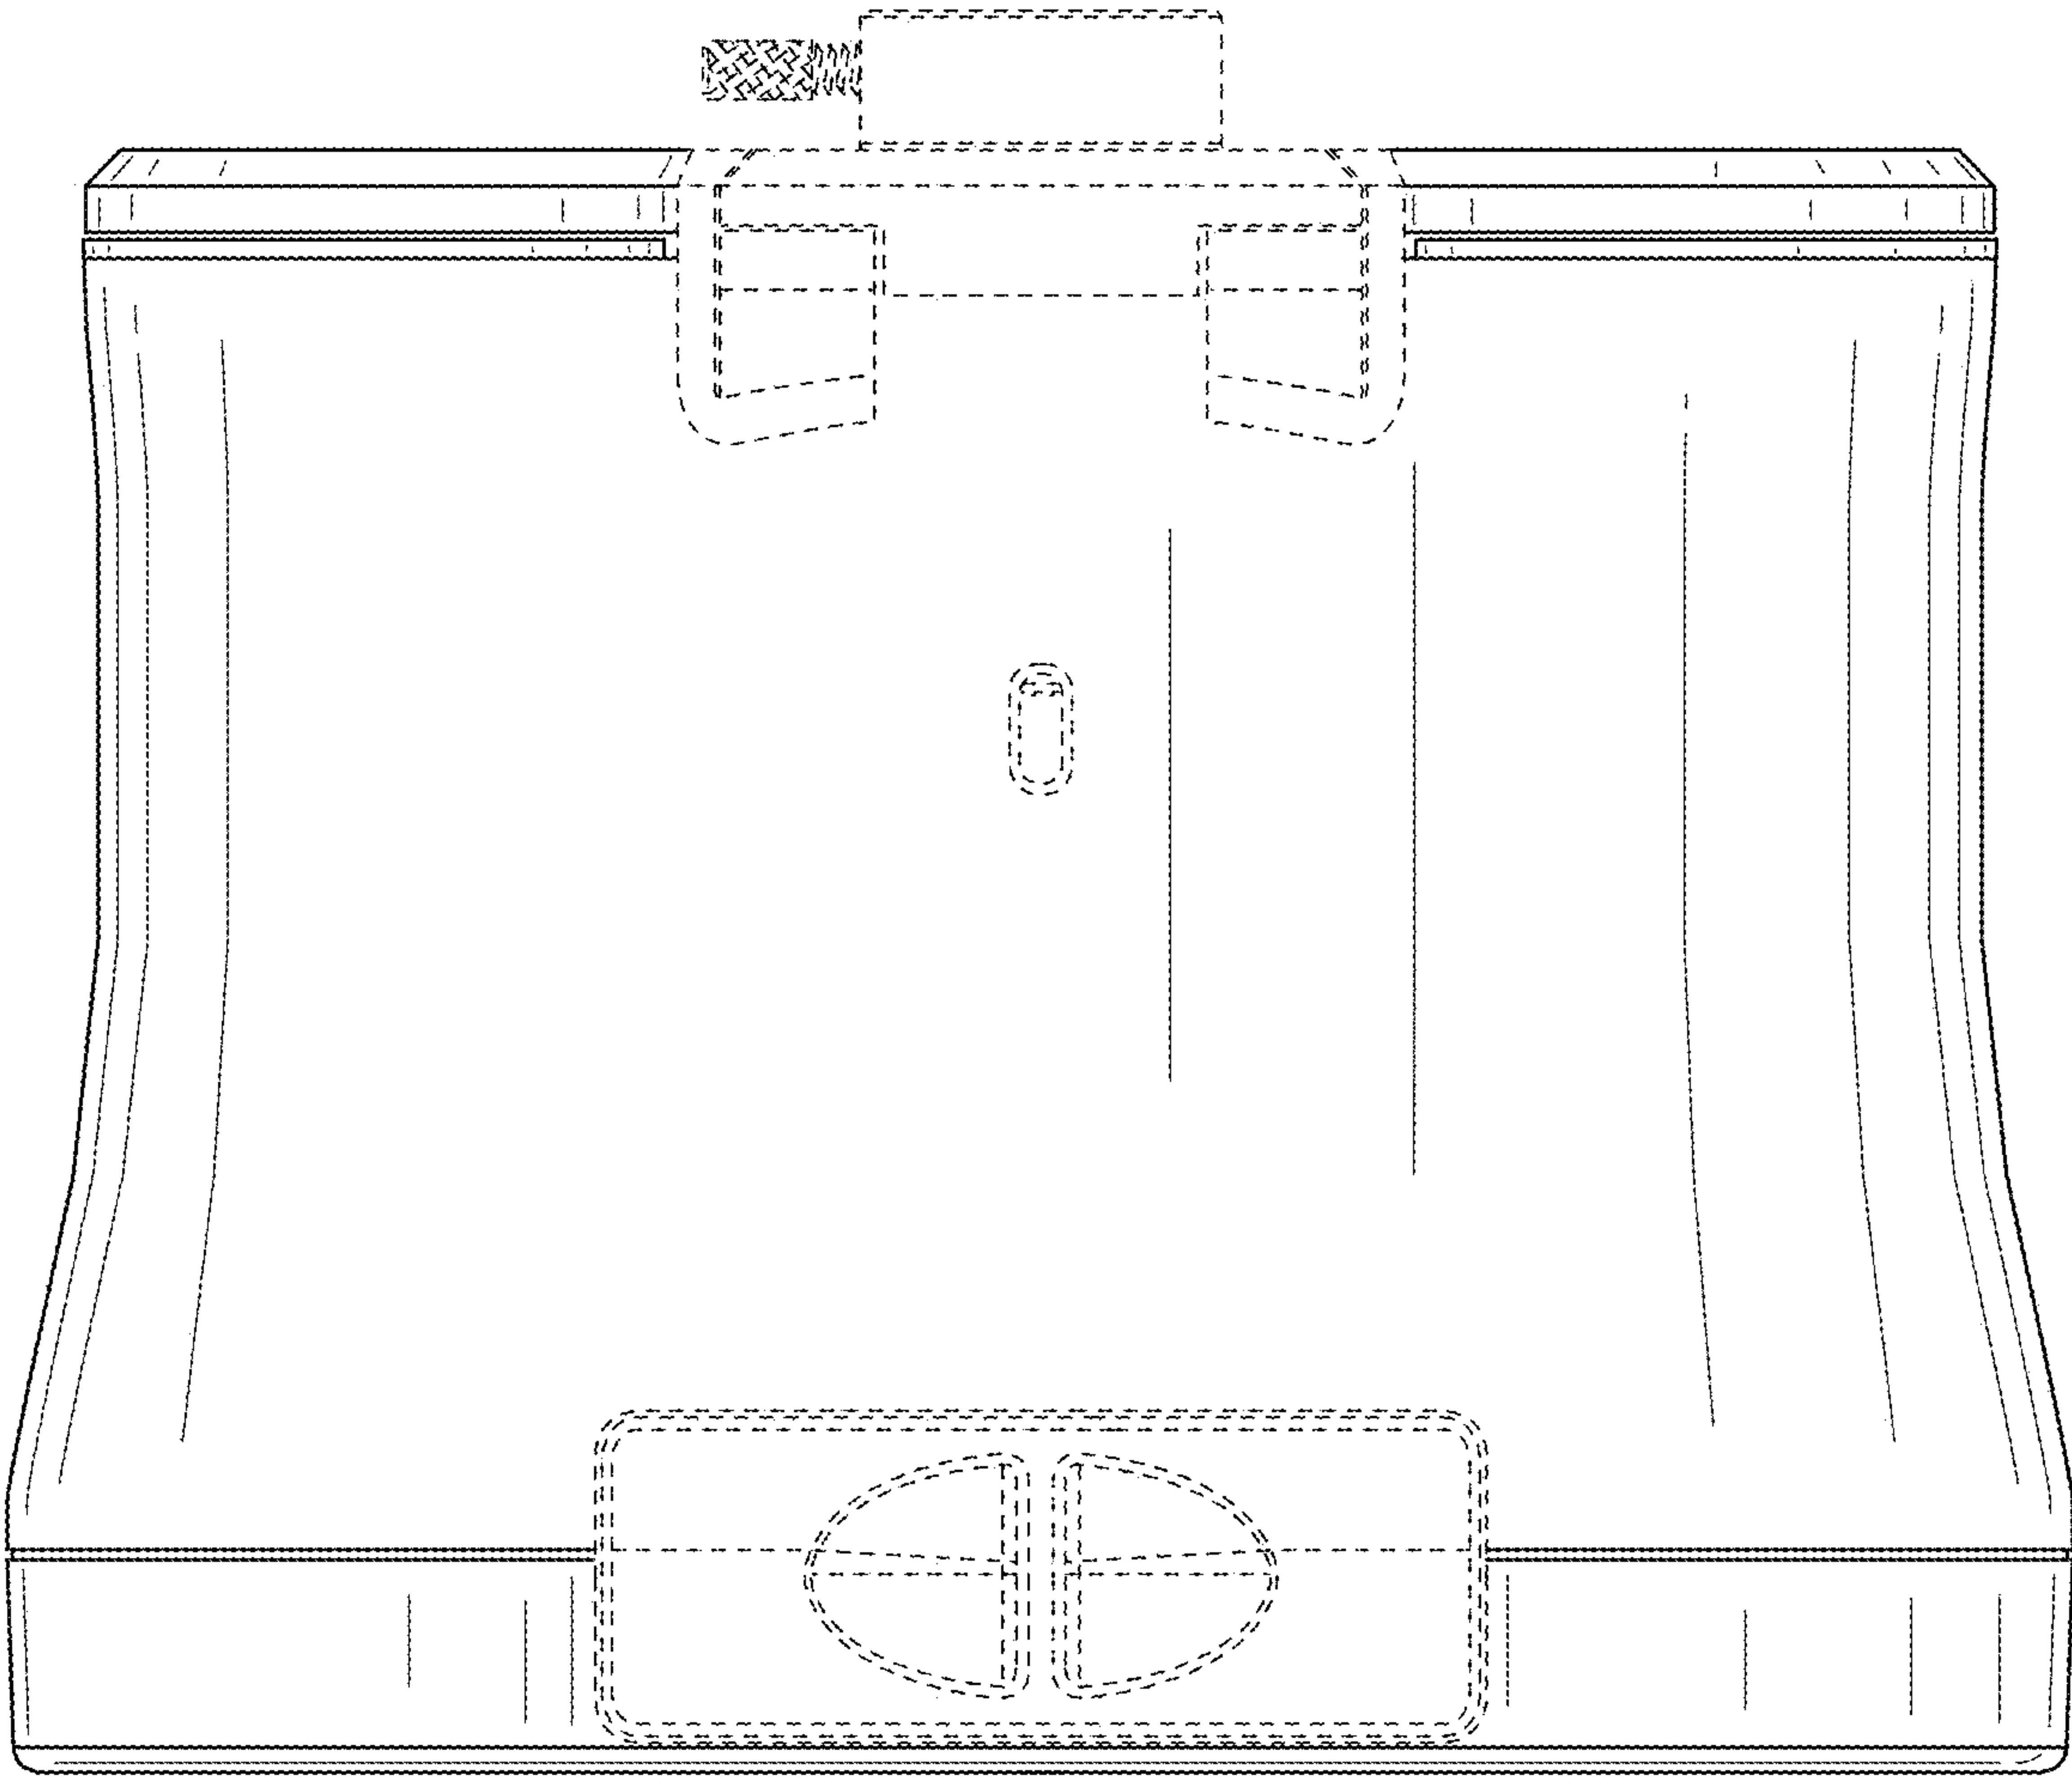


FIG. 3

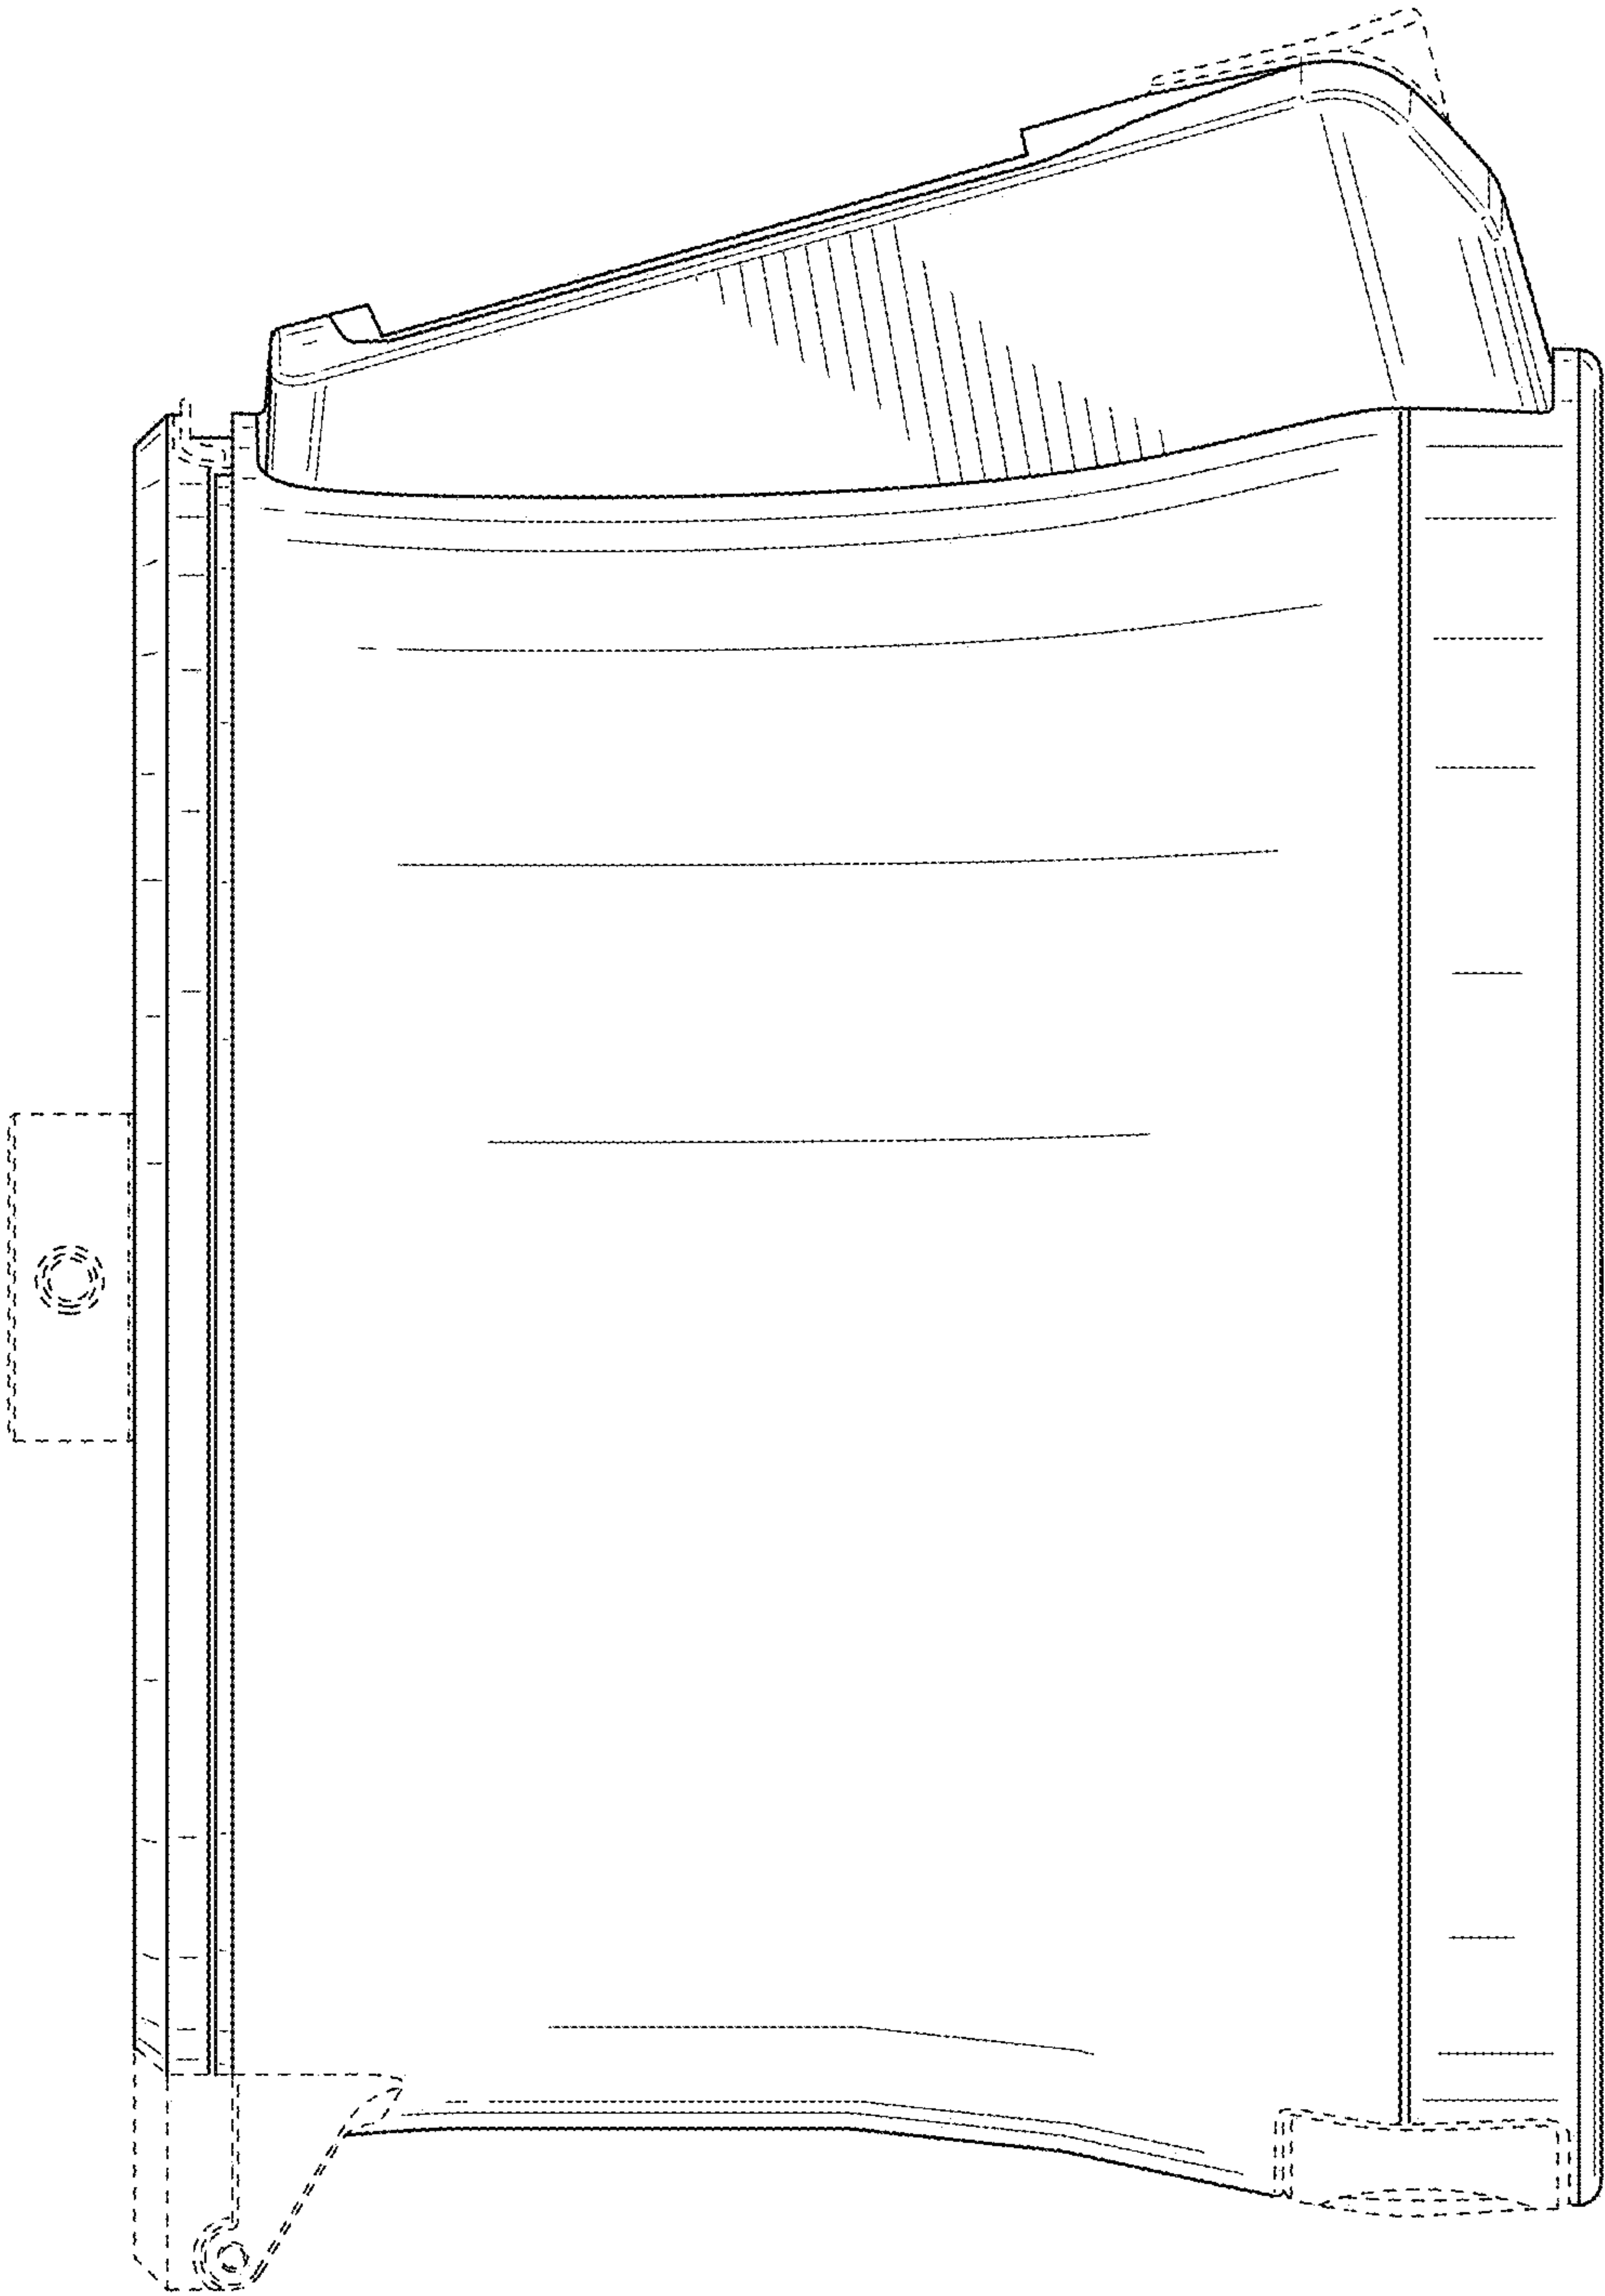


FIG. 4

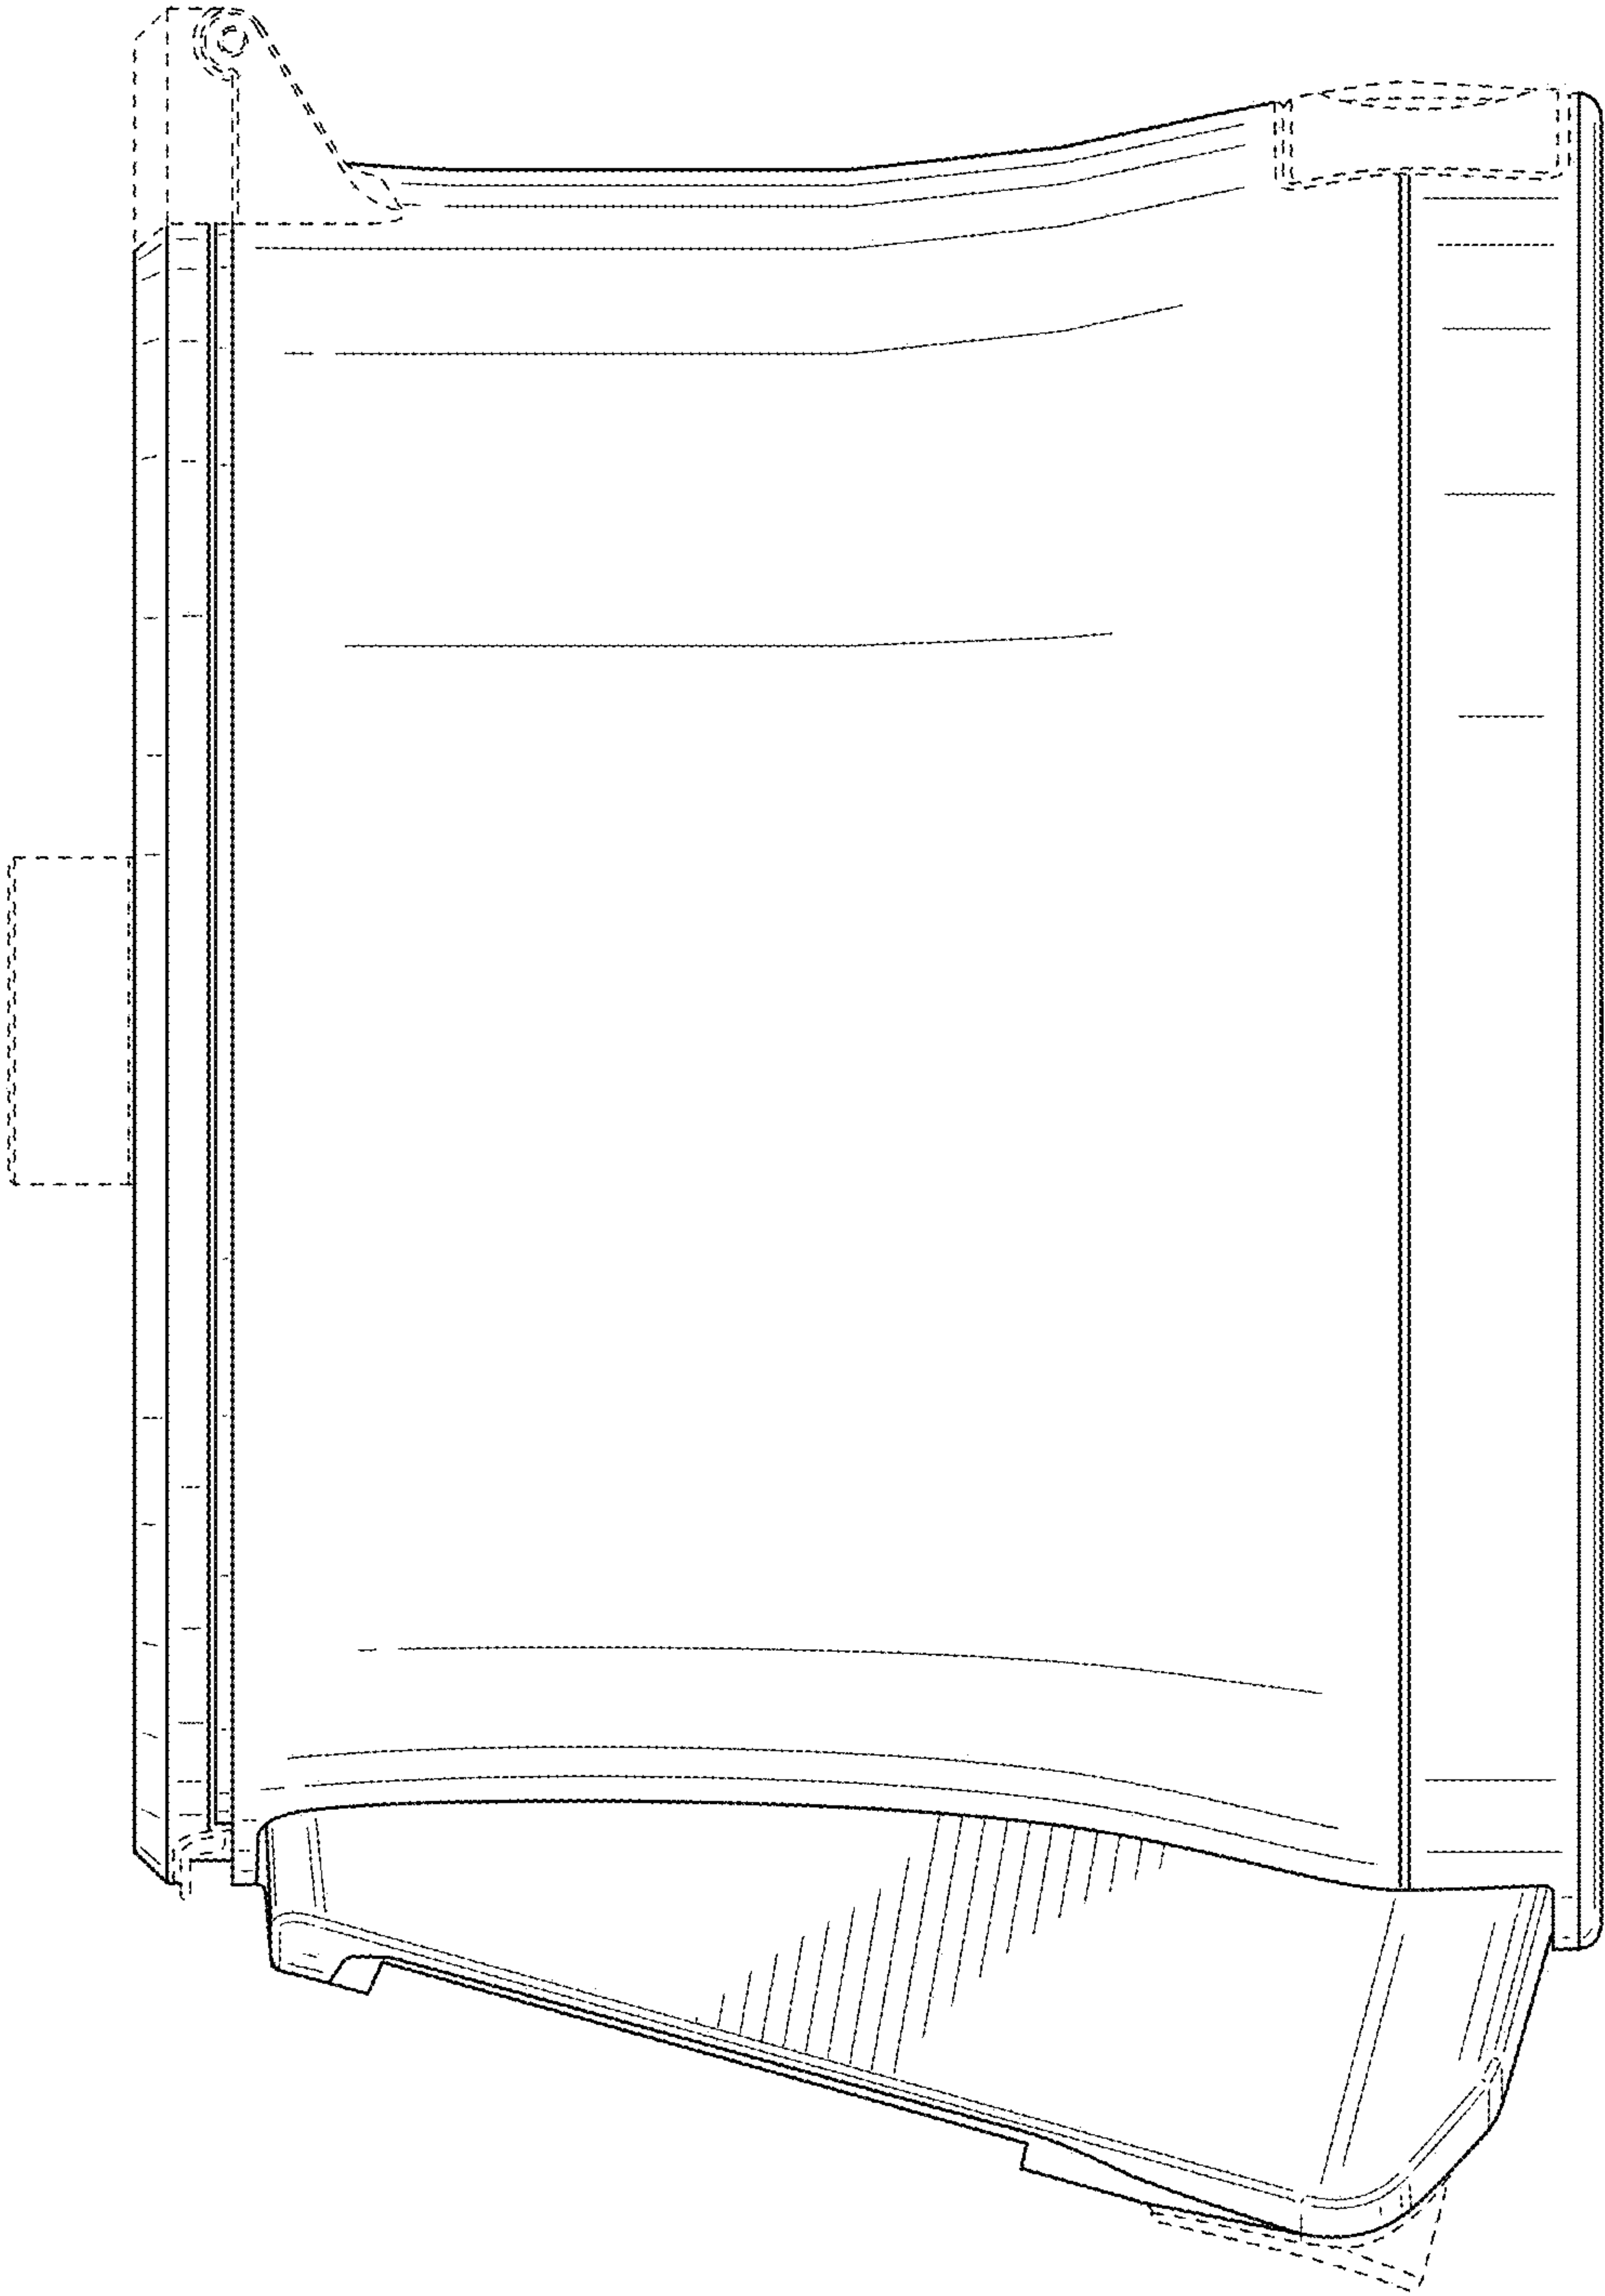


FIG. 5

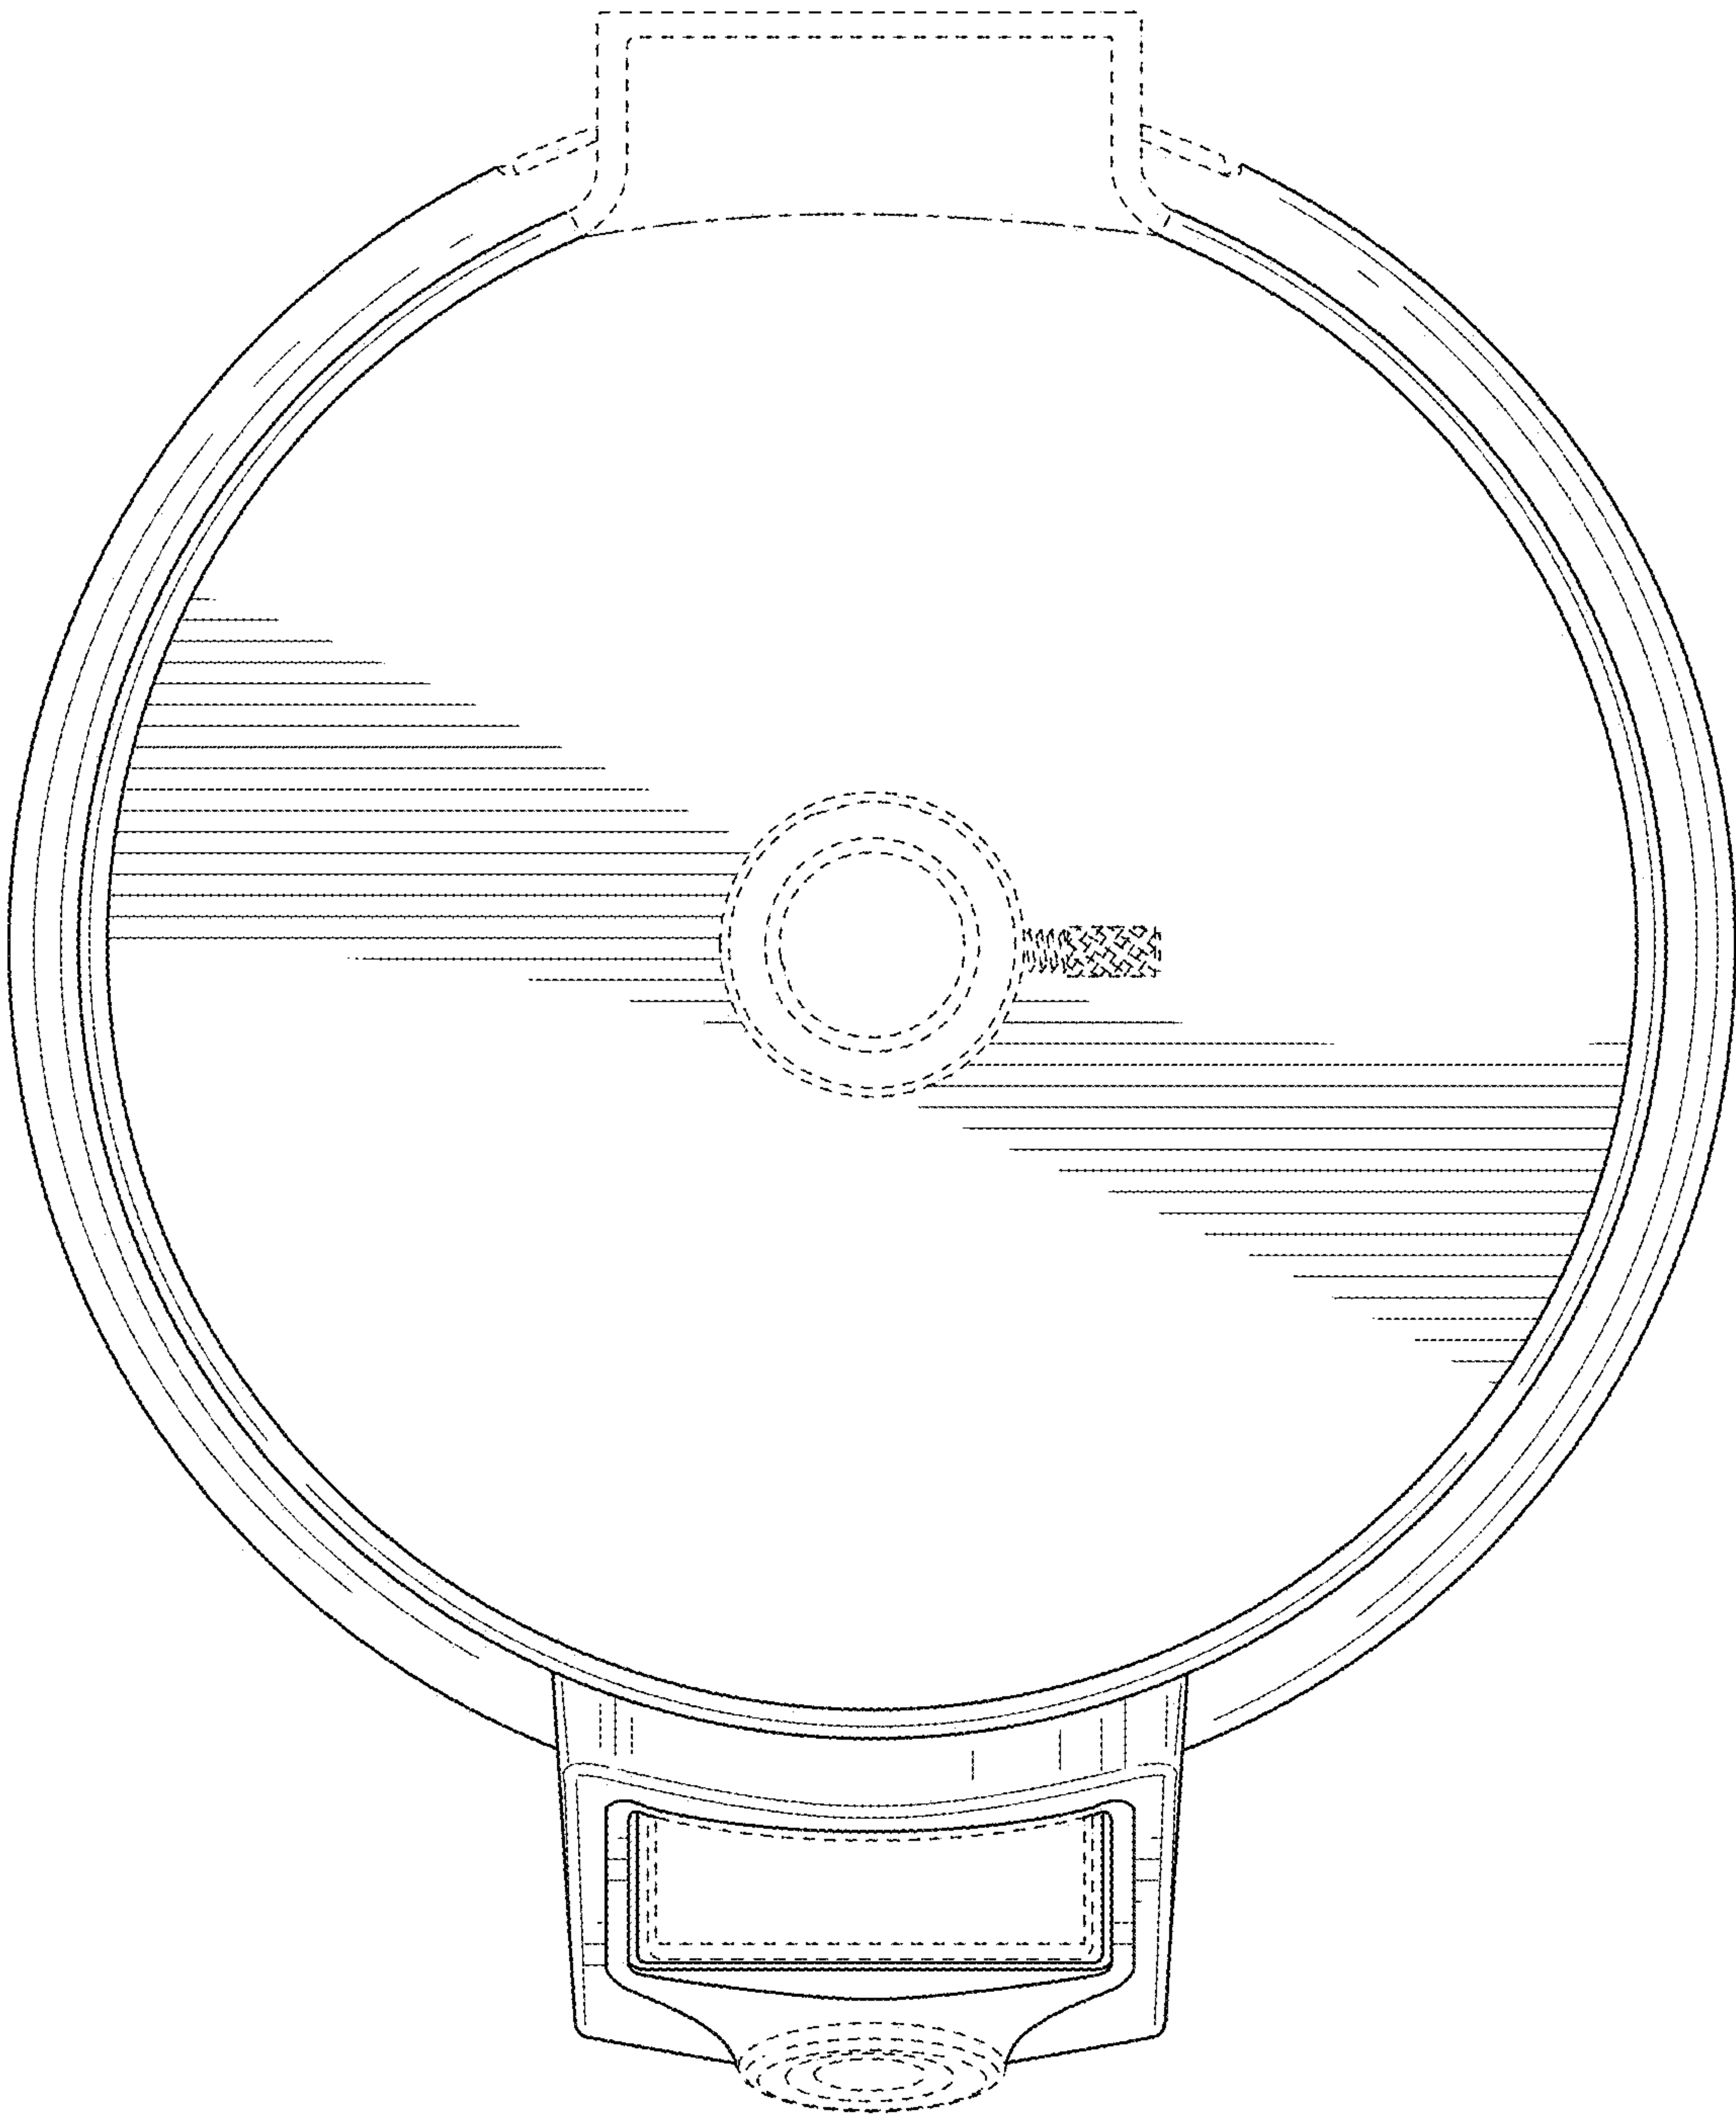


FIG. 6

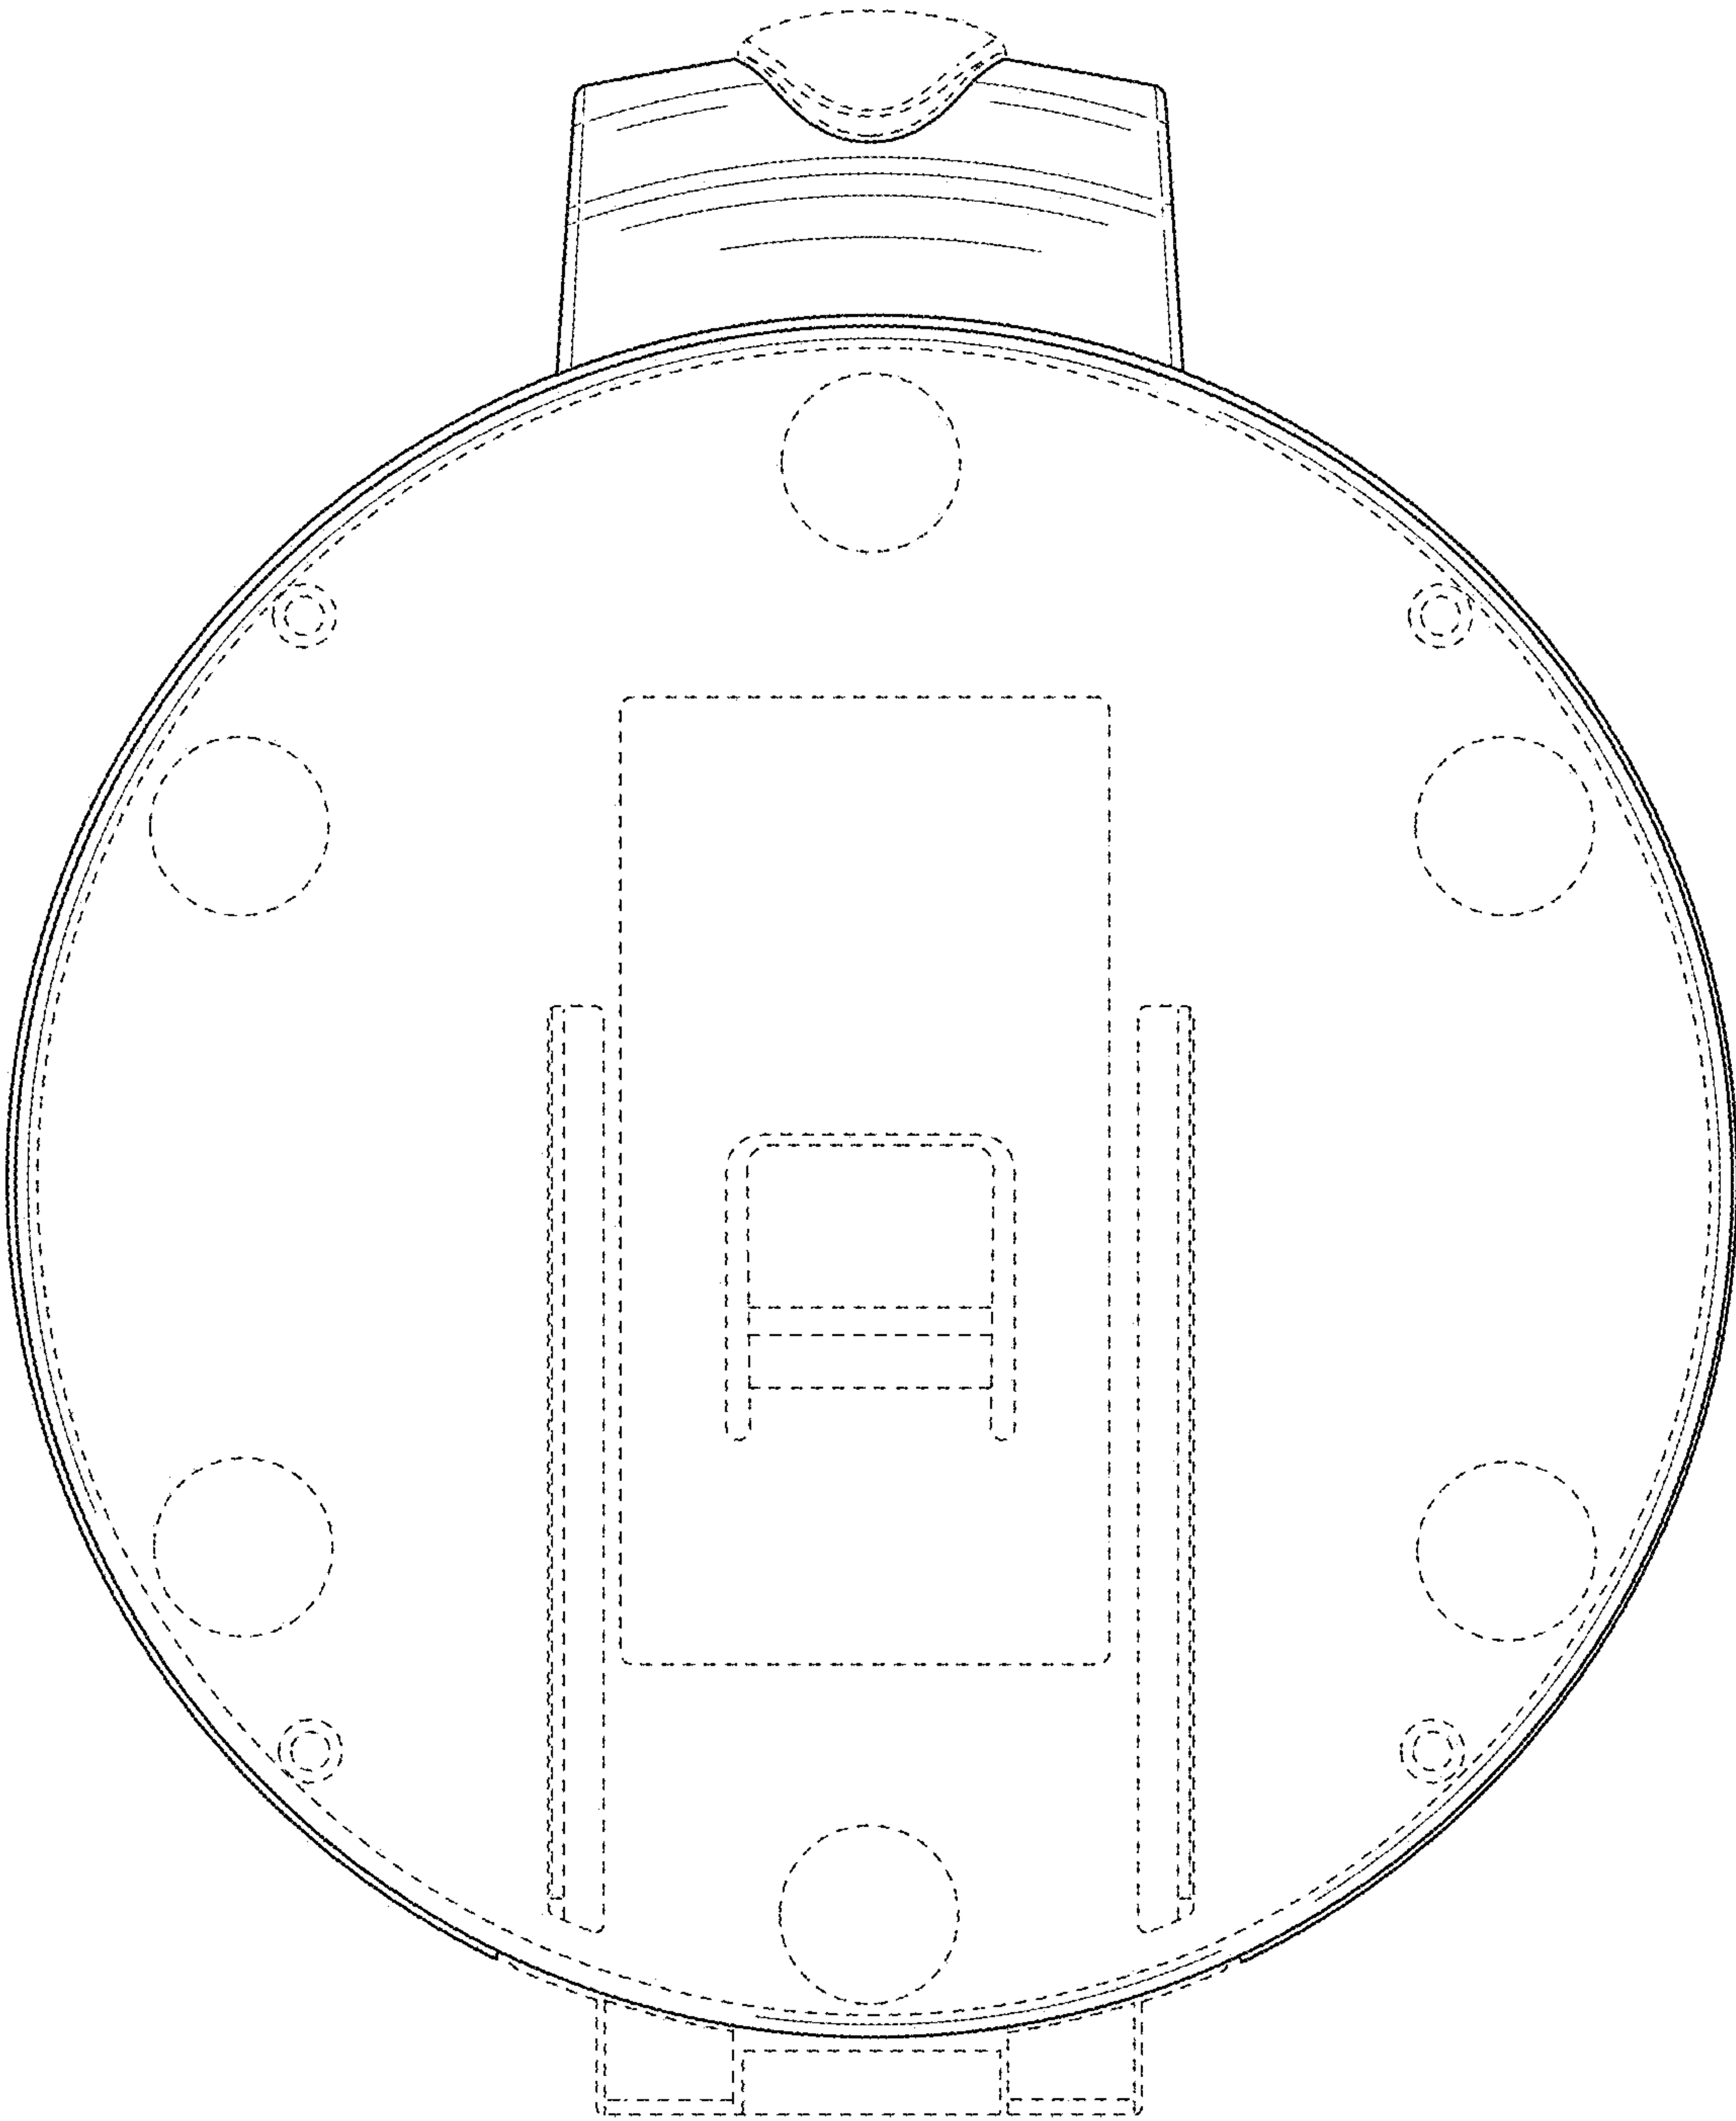


FIG. 7