



US0D1052105S

(12)

United States Design Patent

Fathi et al.

(10)

Patent No.:

US D1,052,105 S

(45)

Date of Patent:

** Nov. 19, 2024

(54) INSTRUMENT FOR MANIPULATING REAGENT DROPLETS

(71) Applicant: Nuclera Ltd, Cambridge (GB)

(72) Inventors: Saeed Fathi, Cambridge (GB); Dean Parkin, Cambridge (GB); Jonathan Wells, Cambridge (GB)

(73) Assignee: Nuclera Ltd, Cambridge (GB)

(**) Term: 15 Years

(21) Appl. No.: 35/517,437

(22) Filed: Dec. 19, 2022

(80) Hague Agreement Data

Int. Filing Date: Dec. 19, 2022
Int. Reg. No.: DM/229143
Int. Reg. Date: Dec. 19, 2022
Int. Reg. Pub. Date: Jun. 9, 2023

(30) Foreign Application Priority Data

Jun. 21, 2022 (GB) 6215109
(51) LOC (14) Cl. 24-02
(52) U.S. Cl.
USPC D24/216
(58) Field of Classification Search
USPC D24/216, 217, 107, 185, 186, 219, 231,
D24/232, 233, 234, 169, 209, 210, 218;
D10/81

(Continued)

(56) References Cited

U.S. PATENT DOCUMENTS

D201,166 S * 5/1965 Power D24/217
D229,220 S * 11/1973 Pulos et al. D32/1
(Continued)

FOREIGN PATENT DOCUMENTS

CN 304191077 * 6/2017
CN 307980927 * 4/2023

OTHER PUBLICATIONS

Automatic Dry Biochemical Analyzer, [site visited Mar. 21, 2024].
Available from Internet. URL: <https://www.aliexpress.us/item/3256806058036598.html> (Year: 2024).*

Primary Examiner — T Chase Nelson
Assistant Examiner — Kelly L Gross
(74) Attorney, Agent, or Firm — McCarter & English, LLP

(57) CLAIM


The ornamental design for an instrument for manipulating reagent droplets as shown and described.

DESCRIPTION

FIG. 1.1 is a front view of an instrument for manipulating reagent droplets, showing our new design;
FIG. 1.2 is a left side view of the embodiment shown in FIG. 1.1;
FIG. 1.3 is a right side view of the embodiment shown in FIG. 1.1;
FIG. 1.4 is a back view of the embodiment shown in FIG. 1.1;
FIG. 1.5 is a top view of the embodiment shown in FIG. 1.1;
FIG. 1.6 is a bottom view of the embodiment shown in FIG. 1.1; and
FIG. 1.7 is a perspective view of the embodiment shown in FIG. 1.1.

The claimed design concerns an instrument for manipulating reagent droplets; The key features lie in the appearance of the product; No particular color or shade is claimed. The broken lines shown in the figures are for the purpose of illustrating portions of the instrument for manipulating reagent droplets and form no part of the claimed design.

1 Claim, 7 Drawing Sheets

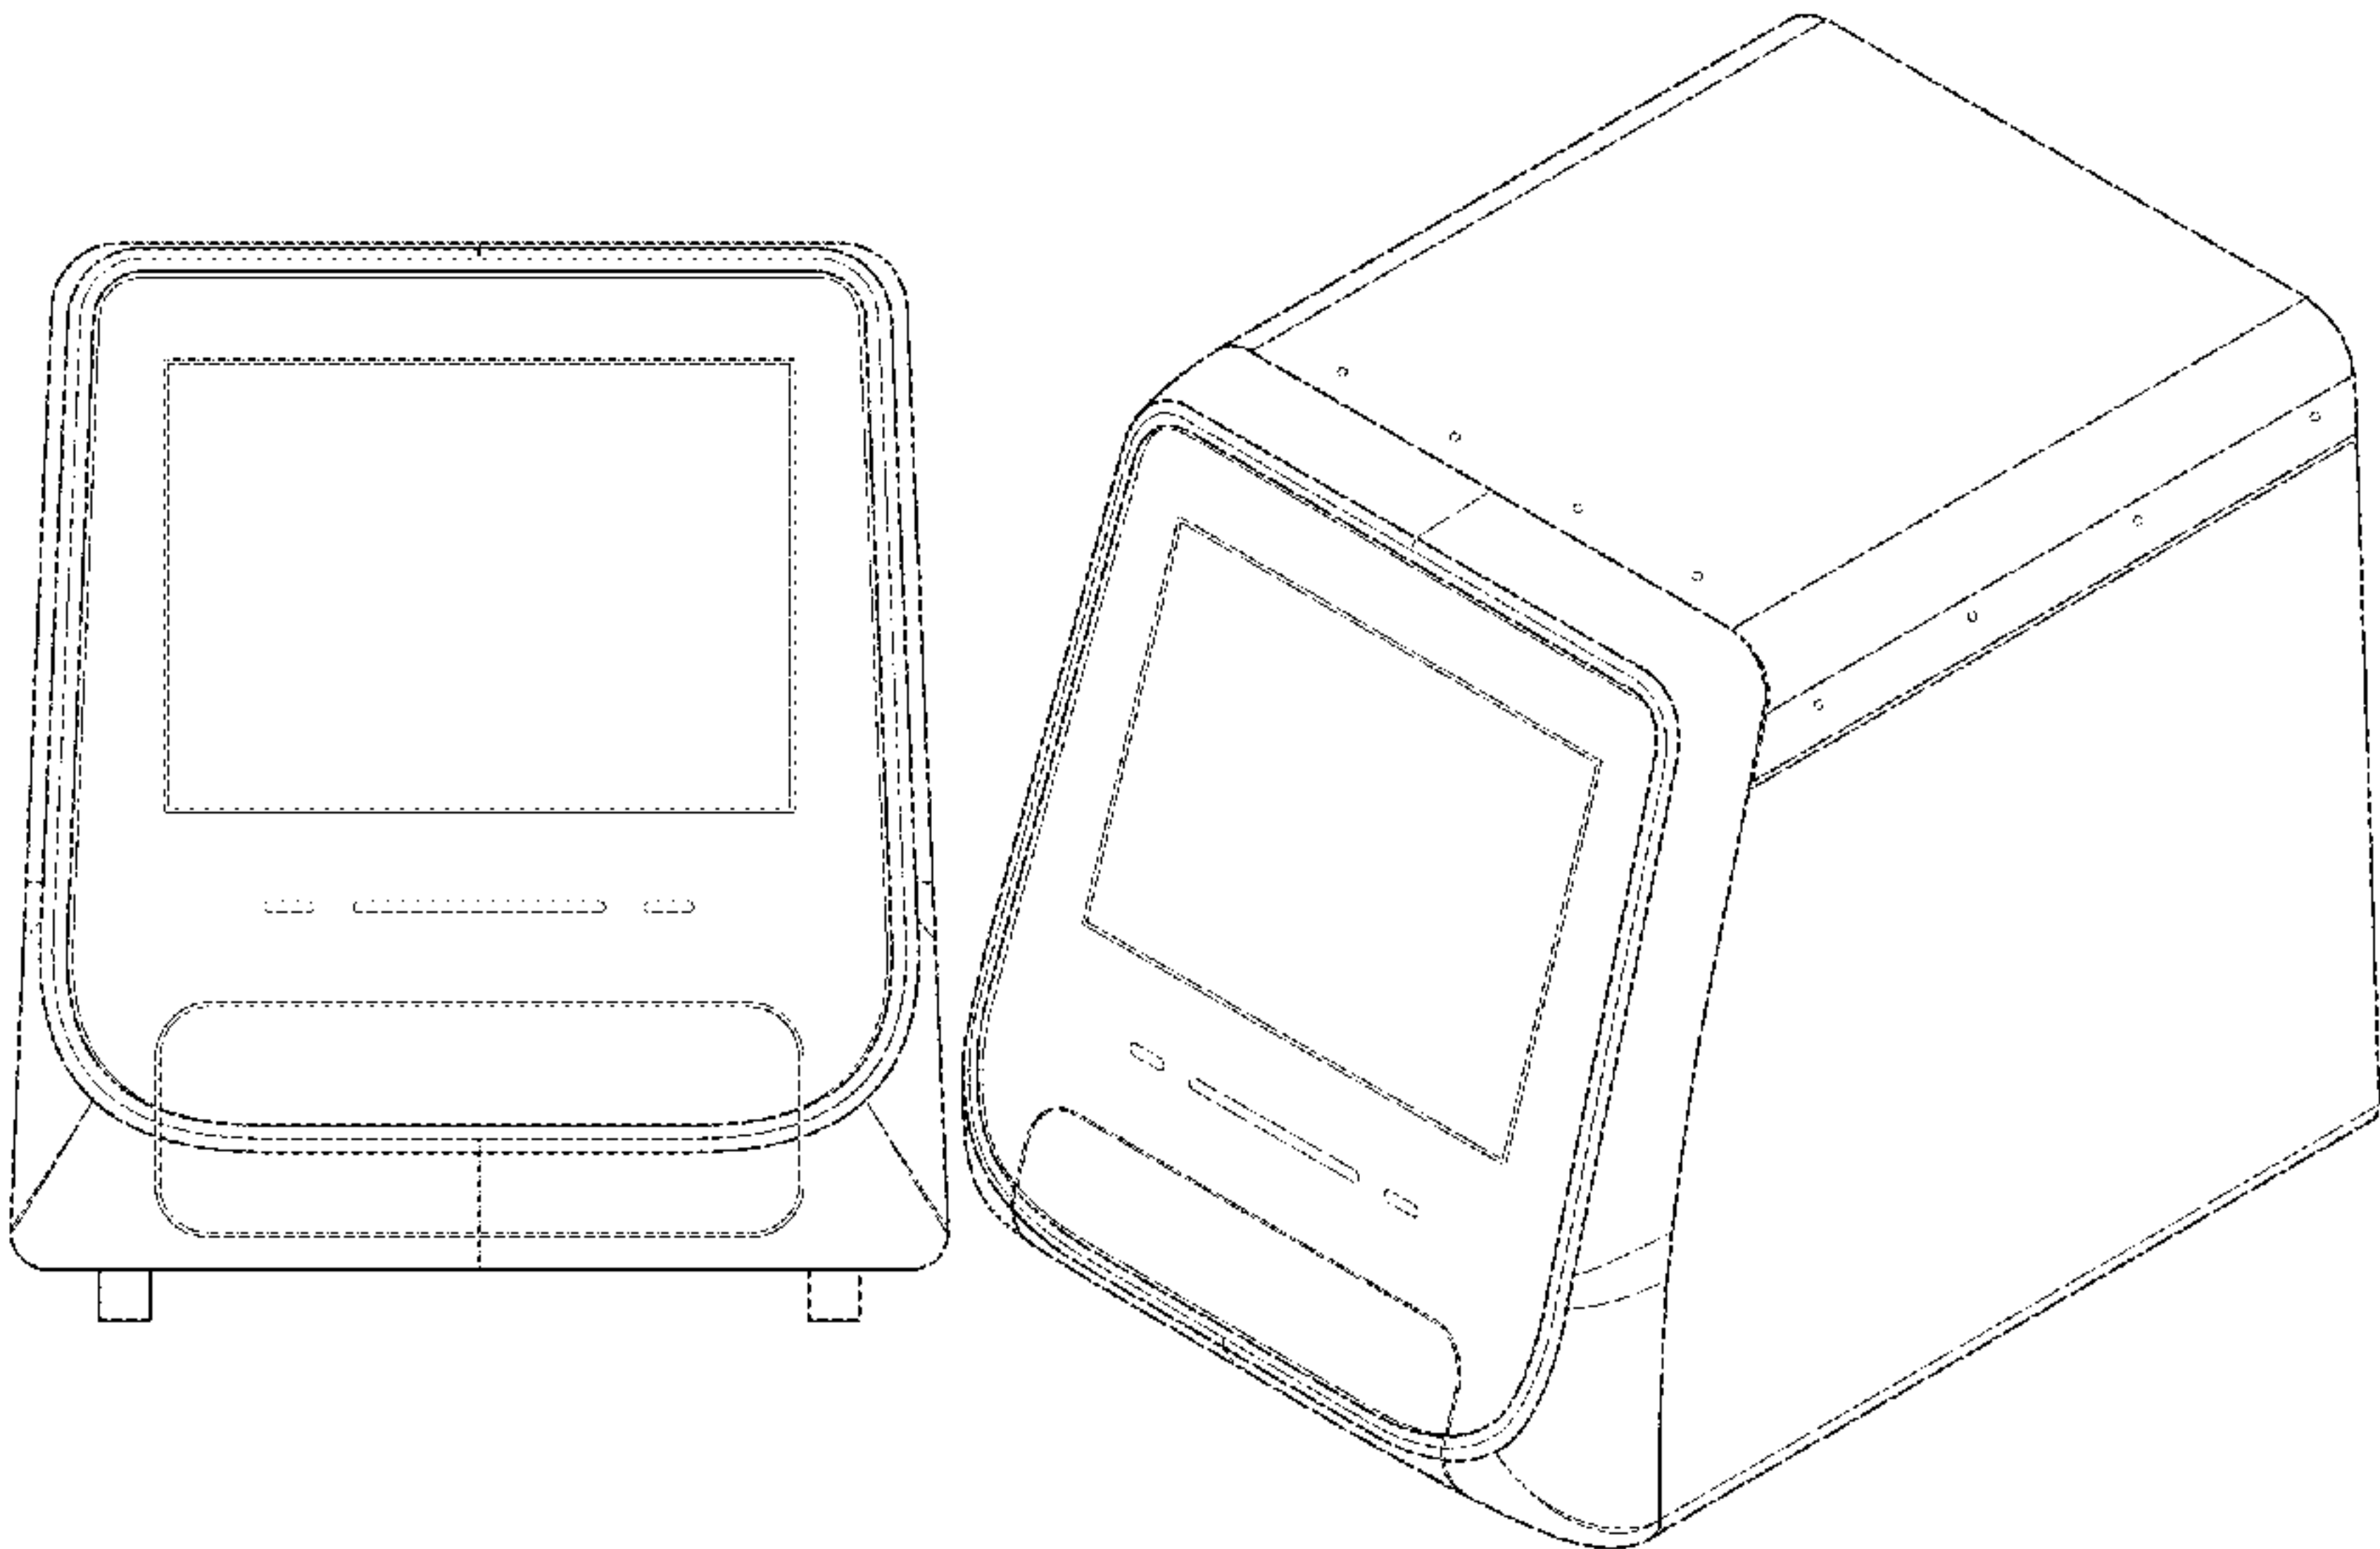

(58) **Field of Classification Search**

CPC G01N 2035/00306; G01N 2035/00326;
G01N 2035/00336; G01N 2030/027;
G01N 21/76; G01N 33/50; G01N 35/025
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D266,151 S * 9/1982 Dawson D24/232
D487,517 S * 3/2004 Cudworth D24/217
D537,951 S * 3/2007 Okamoto D24/233
D556,914 S * 12/2007 Okamoto D24/233
D561,349 S * 2/2008 Levin D24/232
D579,540 S * 10/2008 Hochman D24/107
D588,276 S * 3/2009 Isozaki D24/232
D640,378 S * 6/2011 Okawa D24/186
D653,764 S * 2/2012 Macemon D24/216
D670,402 S * 11/2012 Shibata D24/216
D682,441 S * 5/2013 Kim D24/216
D687,968 S * 8/2013 Trigg D24/232
D688,804 S * 8/2013 Kim D24/216
D693,019 S * 11/2013 Isozaki D24/216
D703,343 S * 4/2014 Biswas D24/217
D704,348 S * 5/2014 Shibata D24/216
D704,350 S * 5/2014 Lau D24/217
D717,966 S * 11/2014 Elson D24/217
D719,671 S * 12/2014 Nishikawa D24/232
D729,405 S * 5/2015 Ramstad D24/233
D730,535 S * 5/2015 Gutmann D24/216
D740,434 S * 10/2015 Isozaki D24/216
D744,880 S * 12/2015 Smith D24/232
D761,142 S * 7/2016 Golta D24/216
D774,205 S * 12/2016 Grace D24/169
D775,365 S * 12/2016 Mathers D24/232
D782,058 S * 3/2017 Wan D24/216
D784,549 S * 4/2017 Brooks D24/216
D794,211 S * 8/2017 Ang D24/232
D796,358 S * 9/2017 Abbott D24/186
D815,754 S * 4/2018 Morkos D24/232
D817,509 S * 5/2018 McMullin D24/216
D818,146 S * 5/2018 Tanaka D24/216
D819,225 S * 5/2018 Mead D24/233
D825,776 S * 8/2018 Quick D24/232
D825,777 S * 8/2018 Quick D24/232
D830,210 S * 10/2018 Ihara D24/216
D850,310 S * 6/2019 Kang D24/216
D850,956 S * 6/2019 Barton D24/216
D854,188 S * 7/2019 Schaeken D24/232

D864,415 S * 10/2019 Norton D24/232
D865,220 S * 10/2019 Davidson D24/232
D870,311 S * 12/2019 Kang D24/216
D870,576 S * 12/2019 Kang D24/216
D870,917 S * 12/2019 Kang D24/232
D871,605 S * 12/2019 Kang D24/232
D872,298 S * 1/2020 Kang D24/232
D872,603 S * 1/2020 Fushida D24/216
D874,017 S * 1/2020 Jenoski D24/216
D875,963 S * 2/2020 Gruen D24/216
D881,405 S * 4/2020 Hussey D24/216
D883,510 S * 5/2020 Neuman D24/216
D883,515 S * 5/2020 Jenoski D24/232
D884,901 S * 5/2020 Tam D24/232
D887,295 S * 6/2020 Carney D10/81
D887,296 S * 6/2020 Stone D24/216
D890,357 S * 7/2020 Zanon D24/217
D890,361 S * 7/2020 Nüesch D24/232
D892,352 S * 8/2020 Huang D24/232
D907,245 S * 1/2021 Rateike D24/232
D908,911 S * 1/2021 Reavis, Jr. D24/216
D914,231 S * 3/2021 Ong D24/216
D914,905 S * 3/2021 Wade D24/216
D921,920 S * 6/2021 Rotach D24/232
D922,600 S * 6/2021 Upsdell D24/216
D922,605 S * 6/2021 Berkeley D24/217
D923,197 S * 6/2021 Allegoren D24/232
D923,200 S * 6/2021 Luther D24/233
D931,118 S * 9/2021 Lee D24/232
D932,047 S * 9/2021 Hölbl D24/216
D932,929 S * 10/2021 Stone D24/216
D936,706 S * 11/2021 Swatosch D15/7
D937,433 S * 11/2021 Sugie D24/158
D942,037 S * 1/2022 Mathers D24/232
D942,039 S * 1/2022 Luther D24/233
D953,563 S * 5/2022 Mataka D24/186
D953,564 S * 5/2022 Kim D24/217
D954,288 S * 6/2022 Wade D24/216
D961,115 S * 8/2022 Karnieli D24/232
D962,473 S * 8/2022 Wu D24/232
D964,593 S * 9/2022 Grimmel D24/232
D969,339 S * 11/2022 Sugie D24/219
D978,378 S * 2/2023 Sugie D24/232
D982,181 S * 3/2023 Tanaka D24/232
D990,346 S * 6/2023 Stone D24/216
D992,140 S * 7/2023 Clottu D24/217
D1,008,044 S * 12/2023 Chipperfield D10/81
D1,009,273 S * 12/2023 Chun D24/185

* cited by examiner

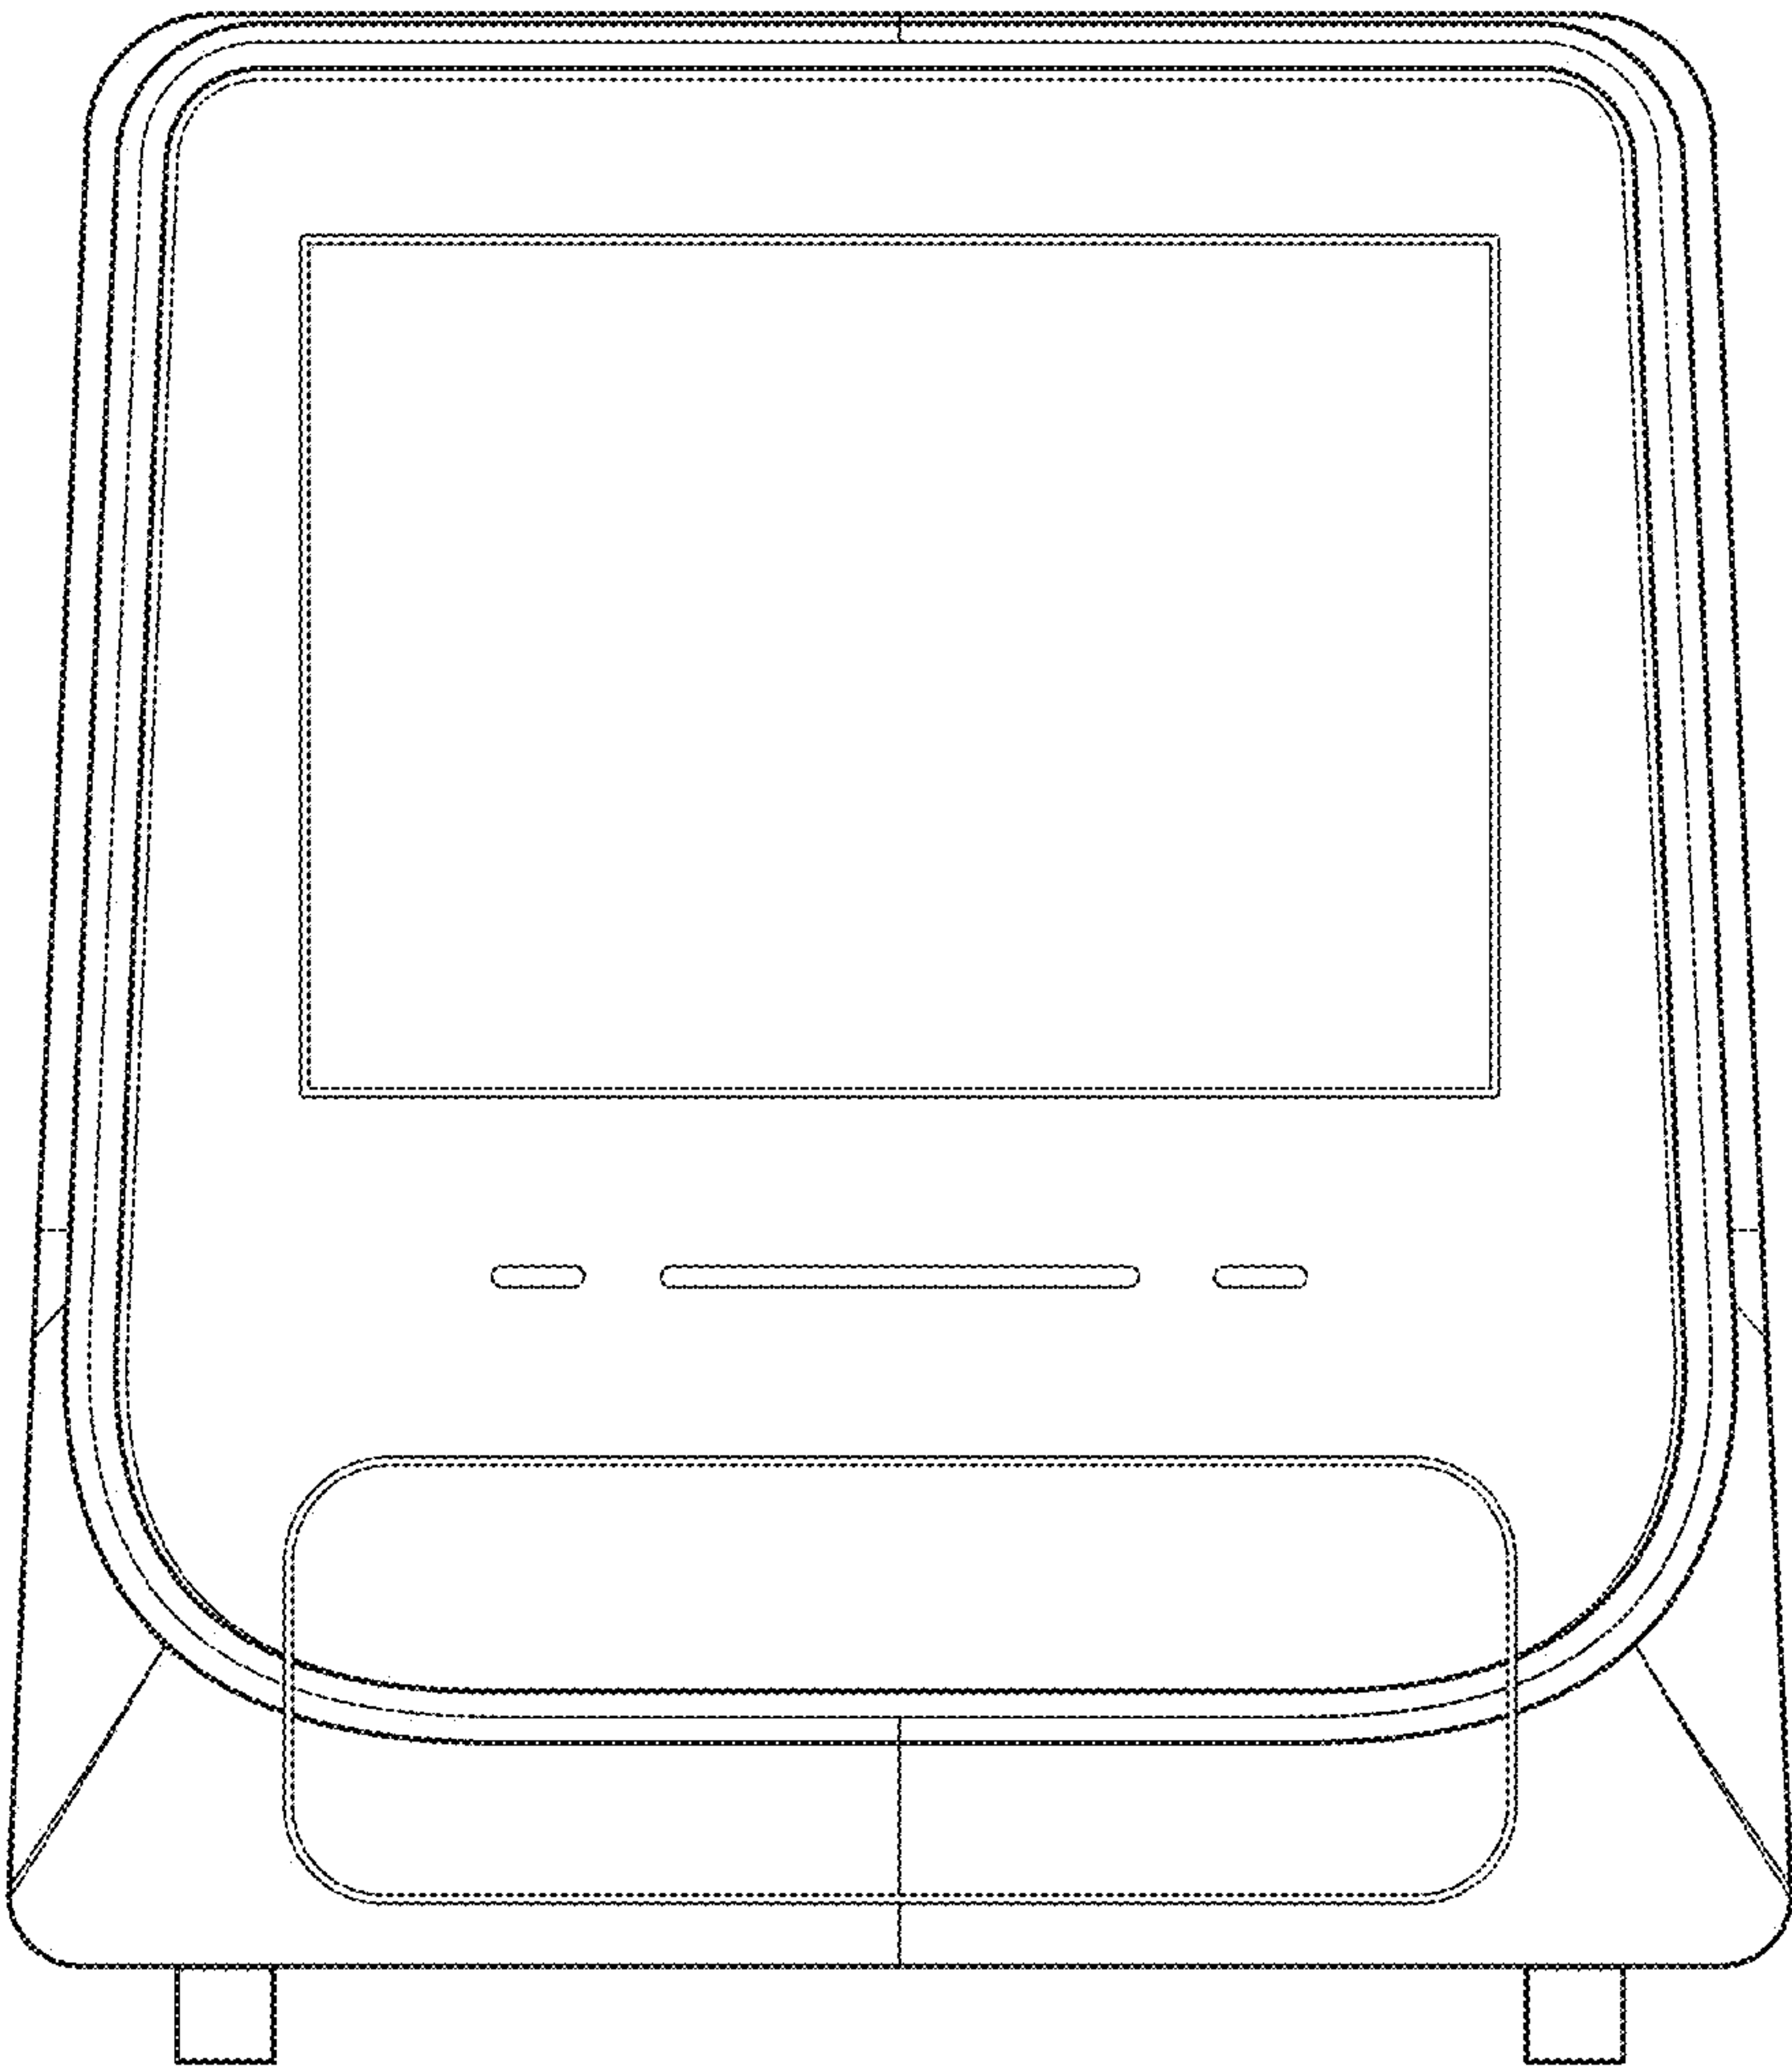


FIG. 1.1

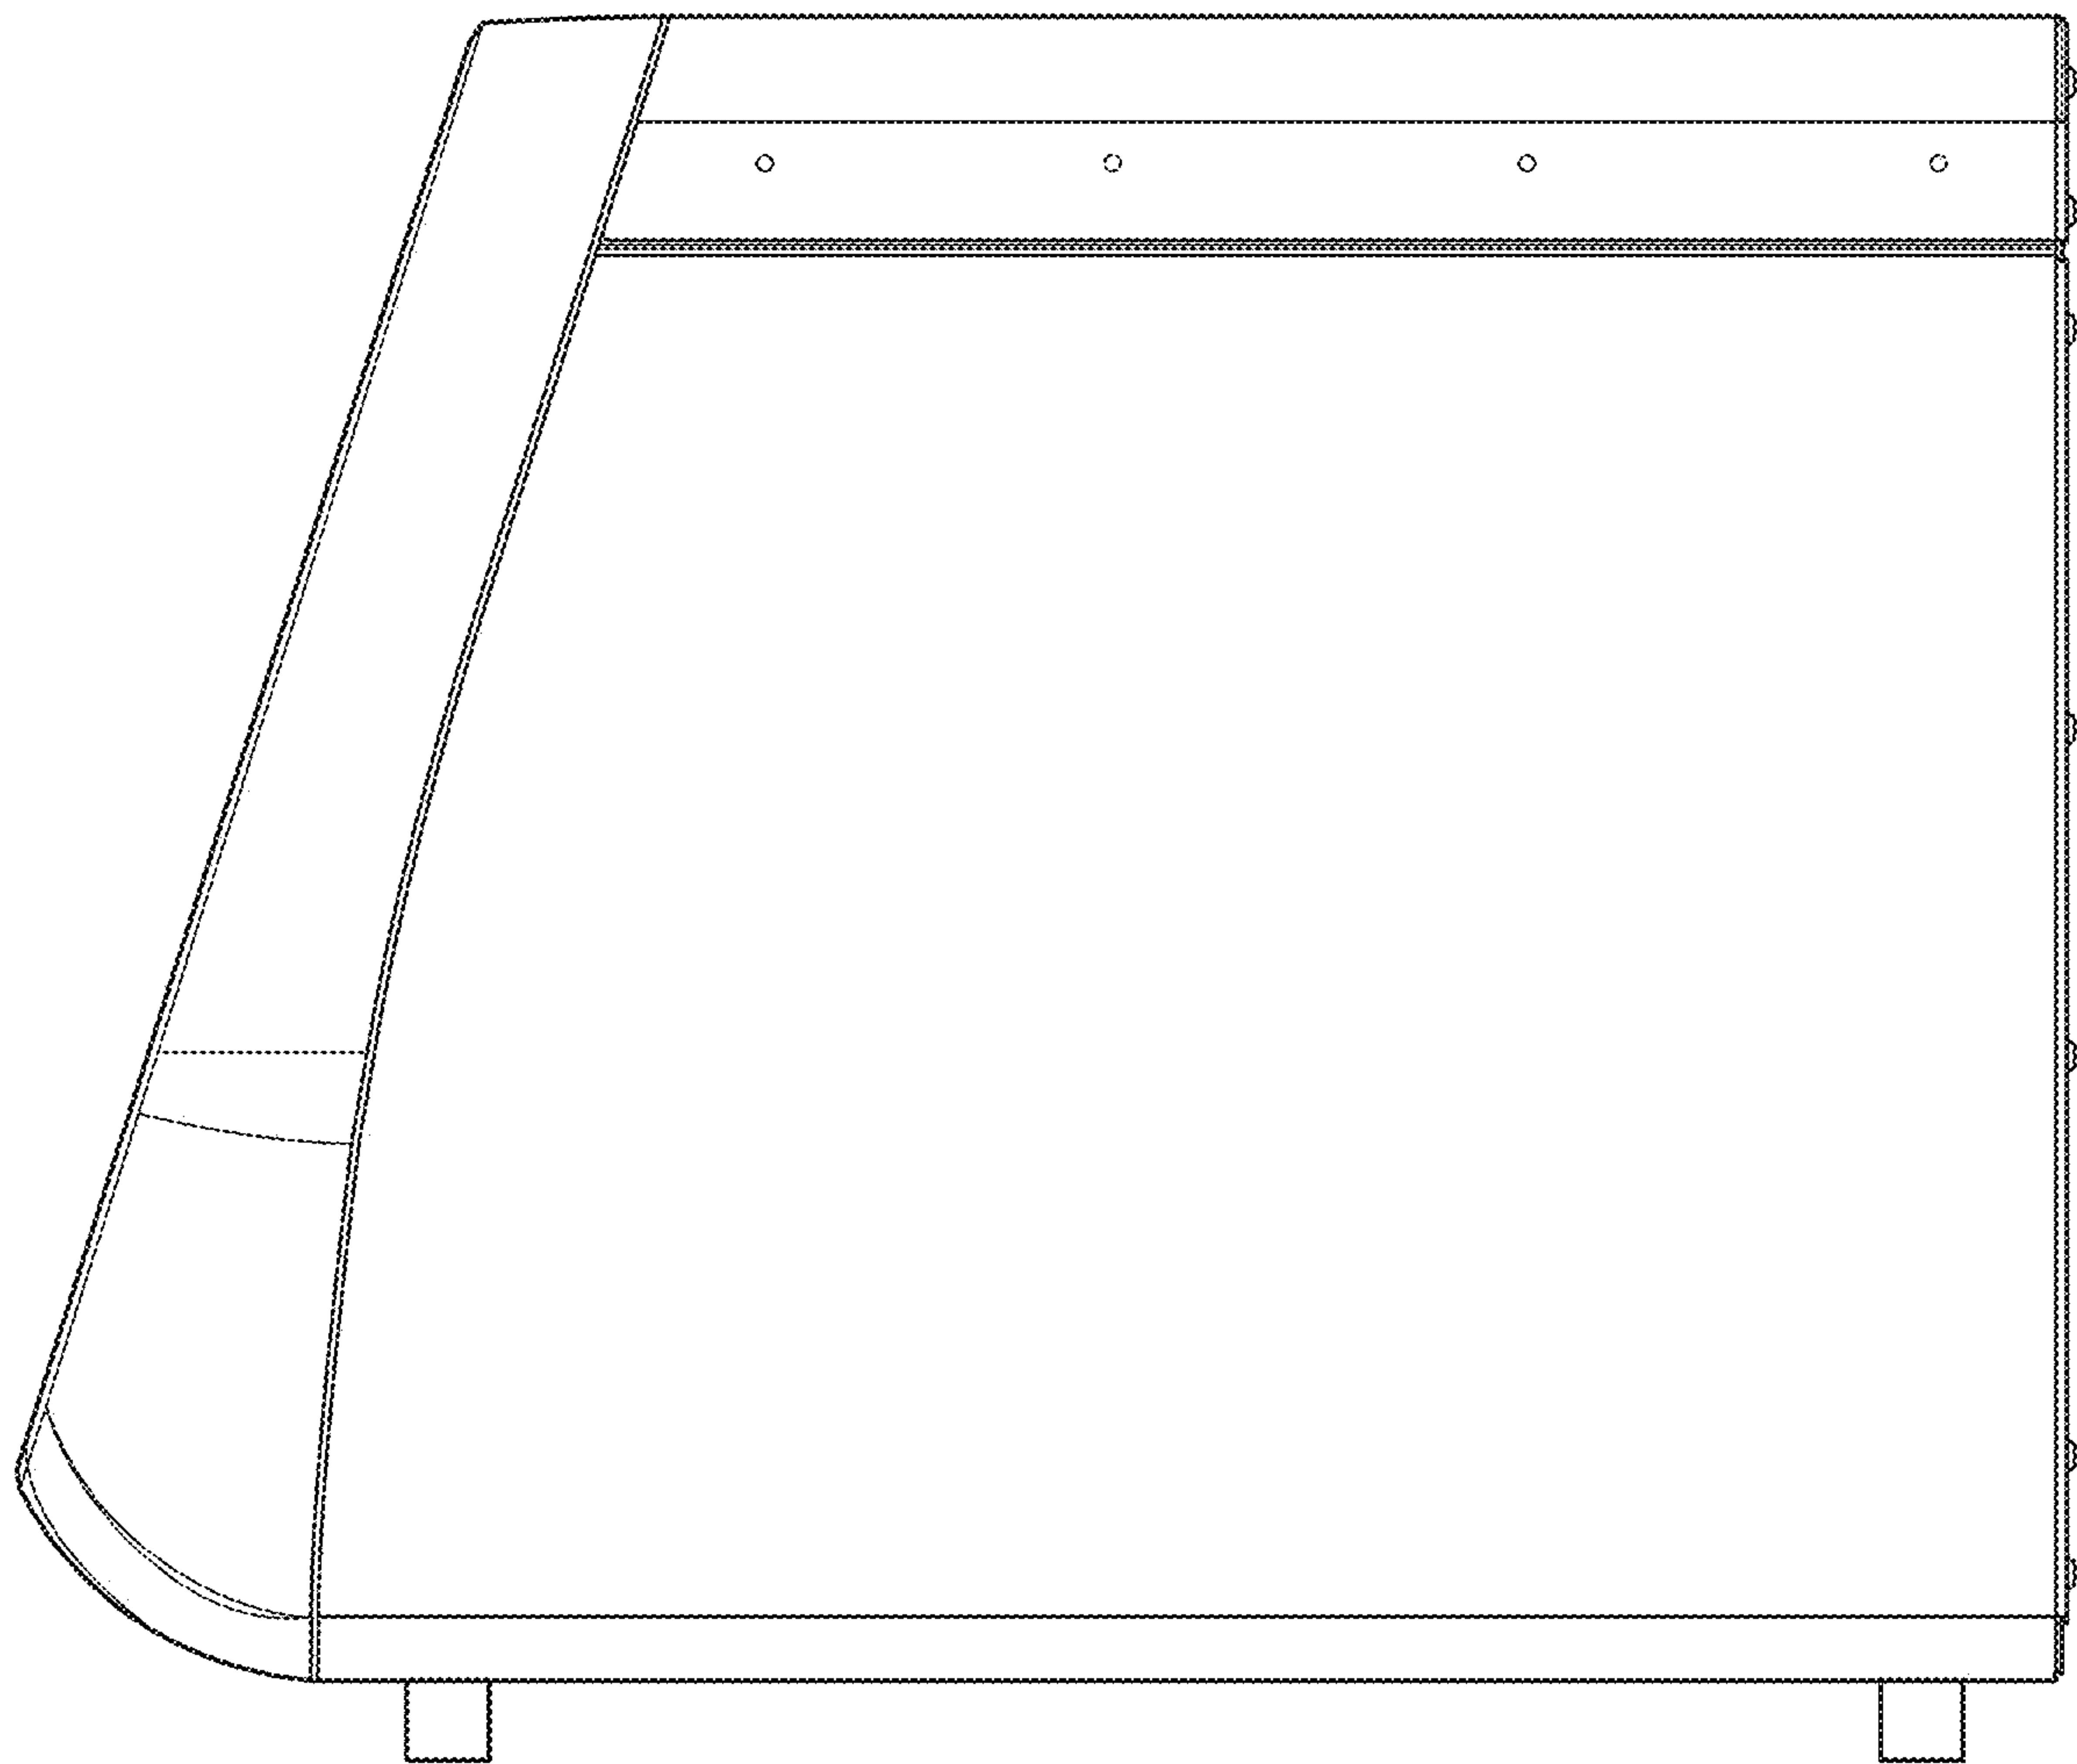


FIG. 1.2

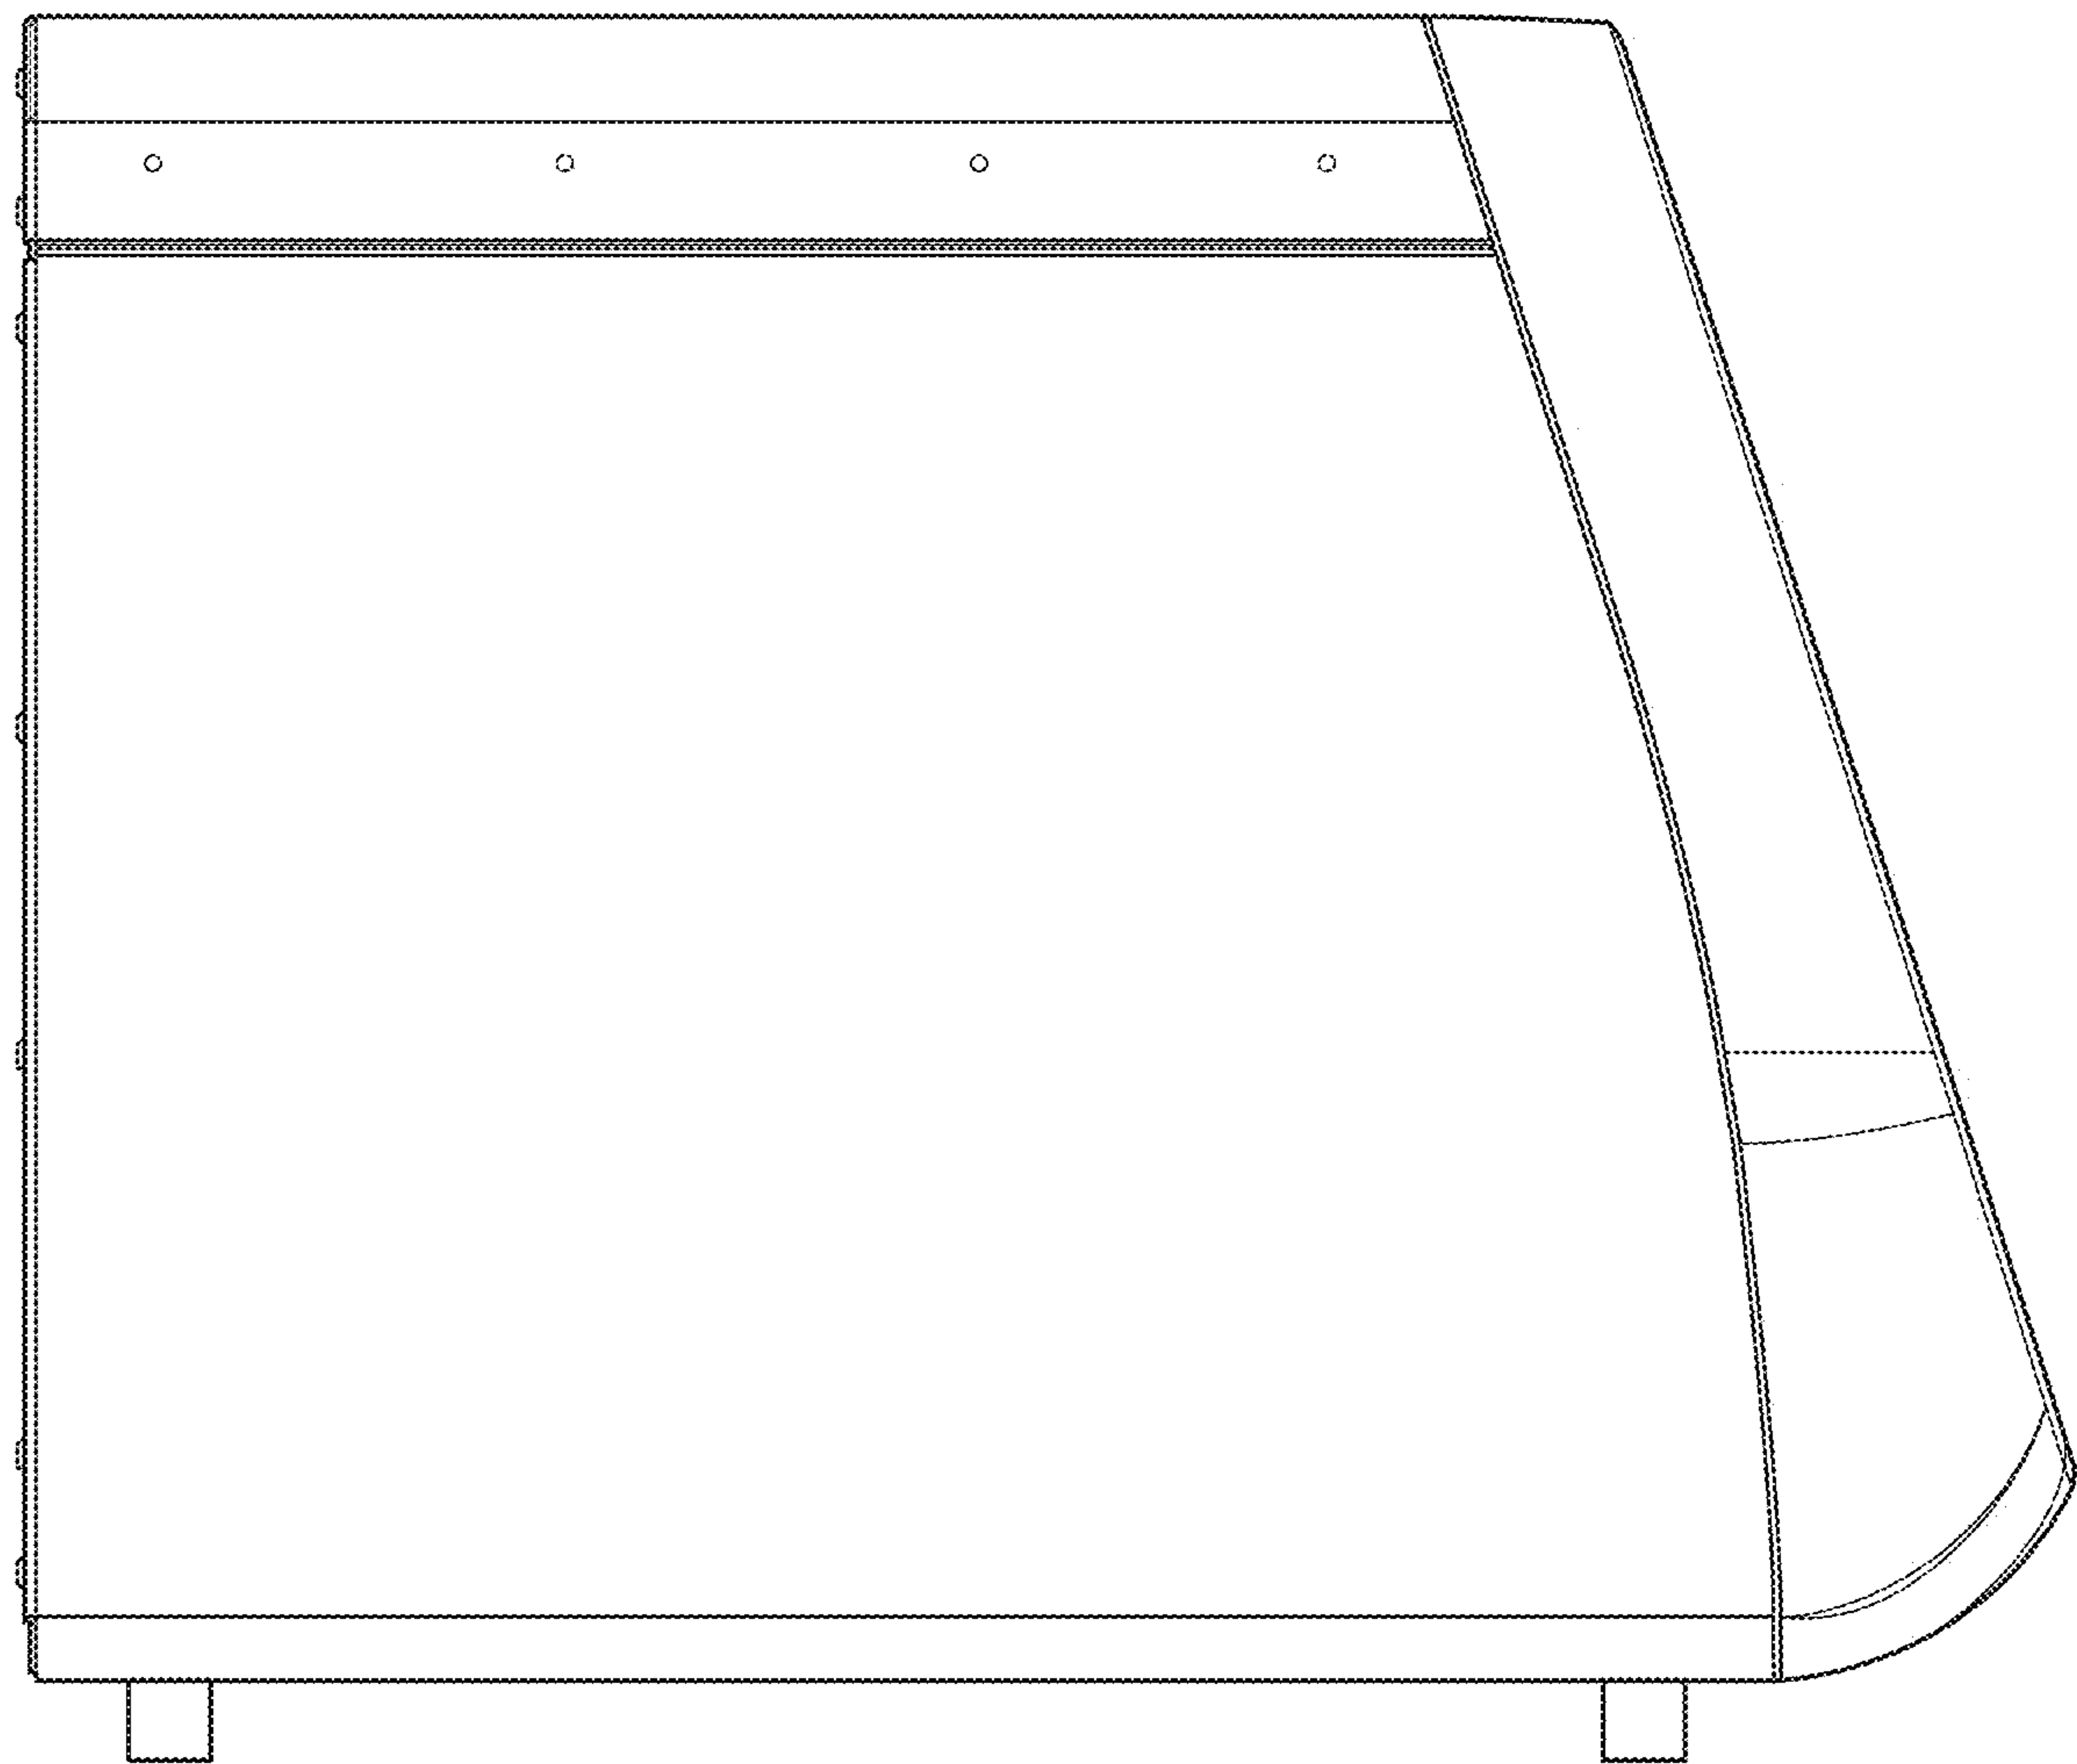


FIG. 1.3

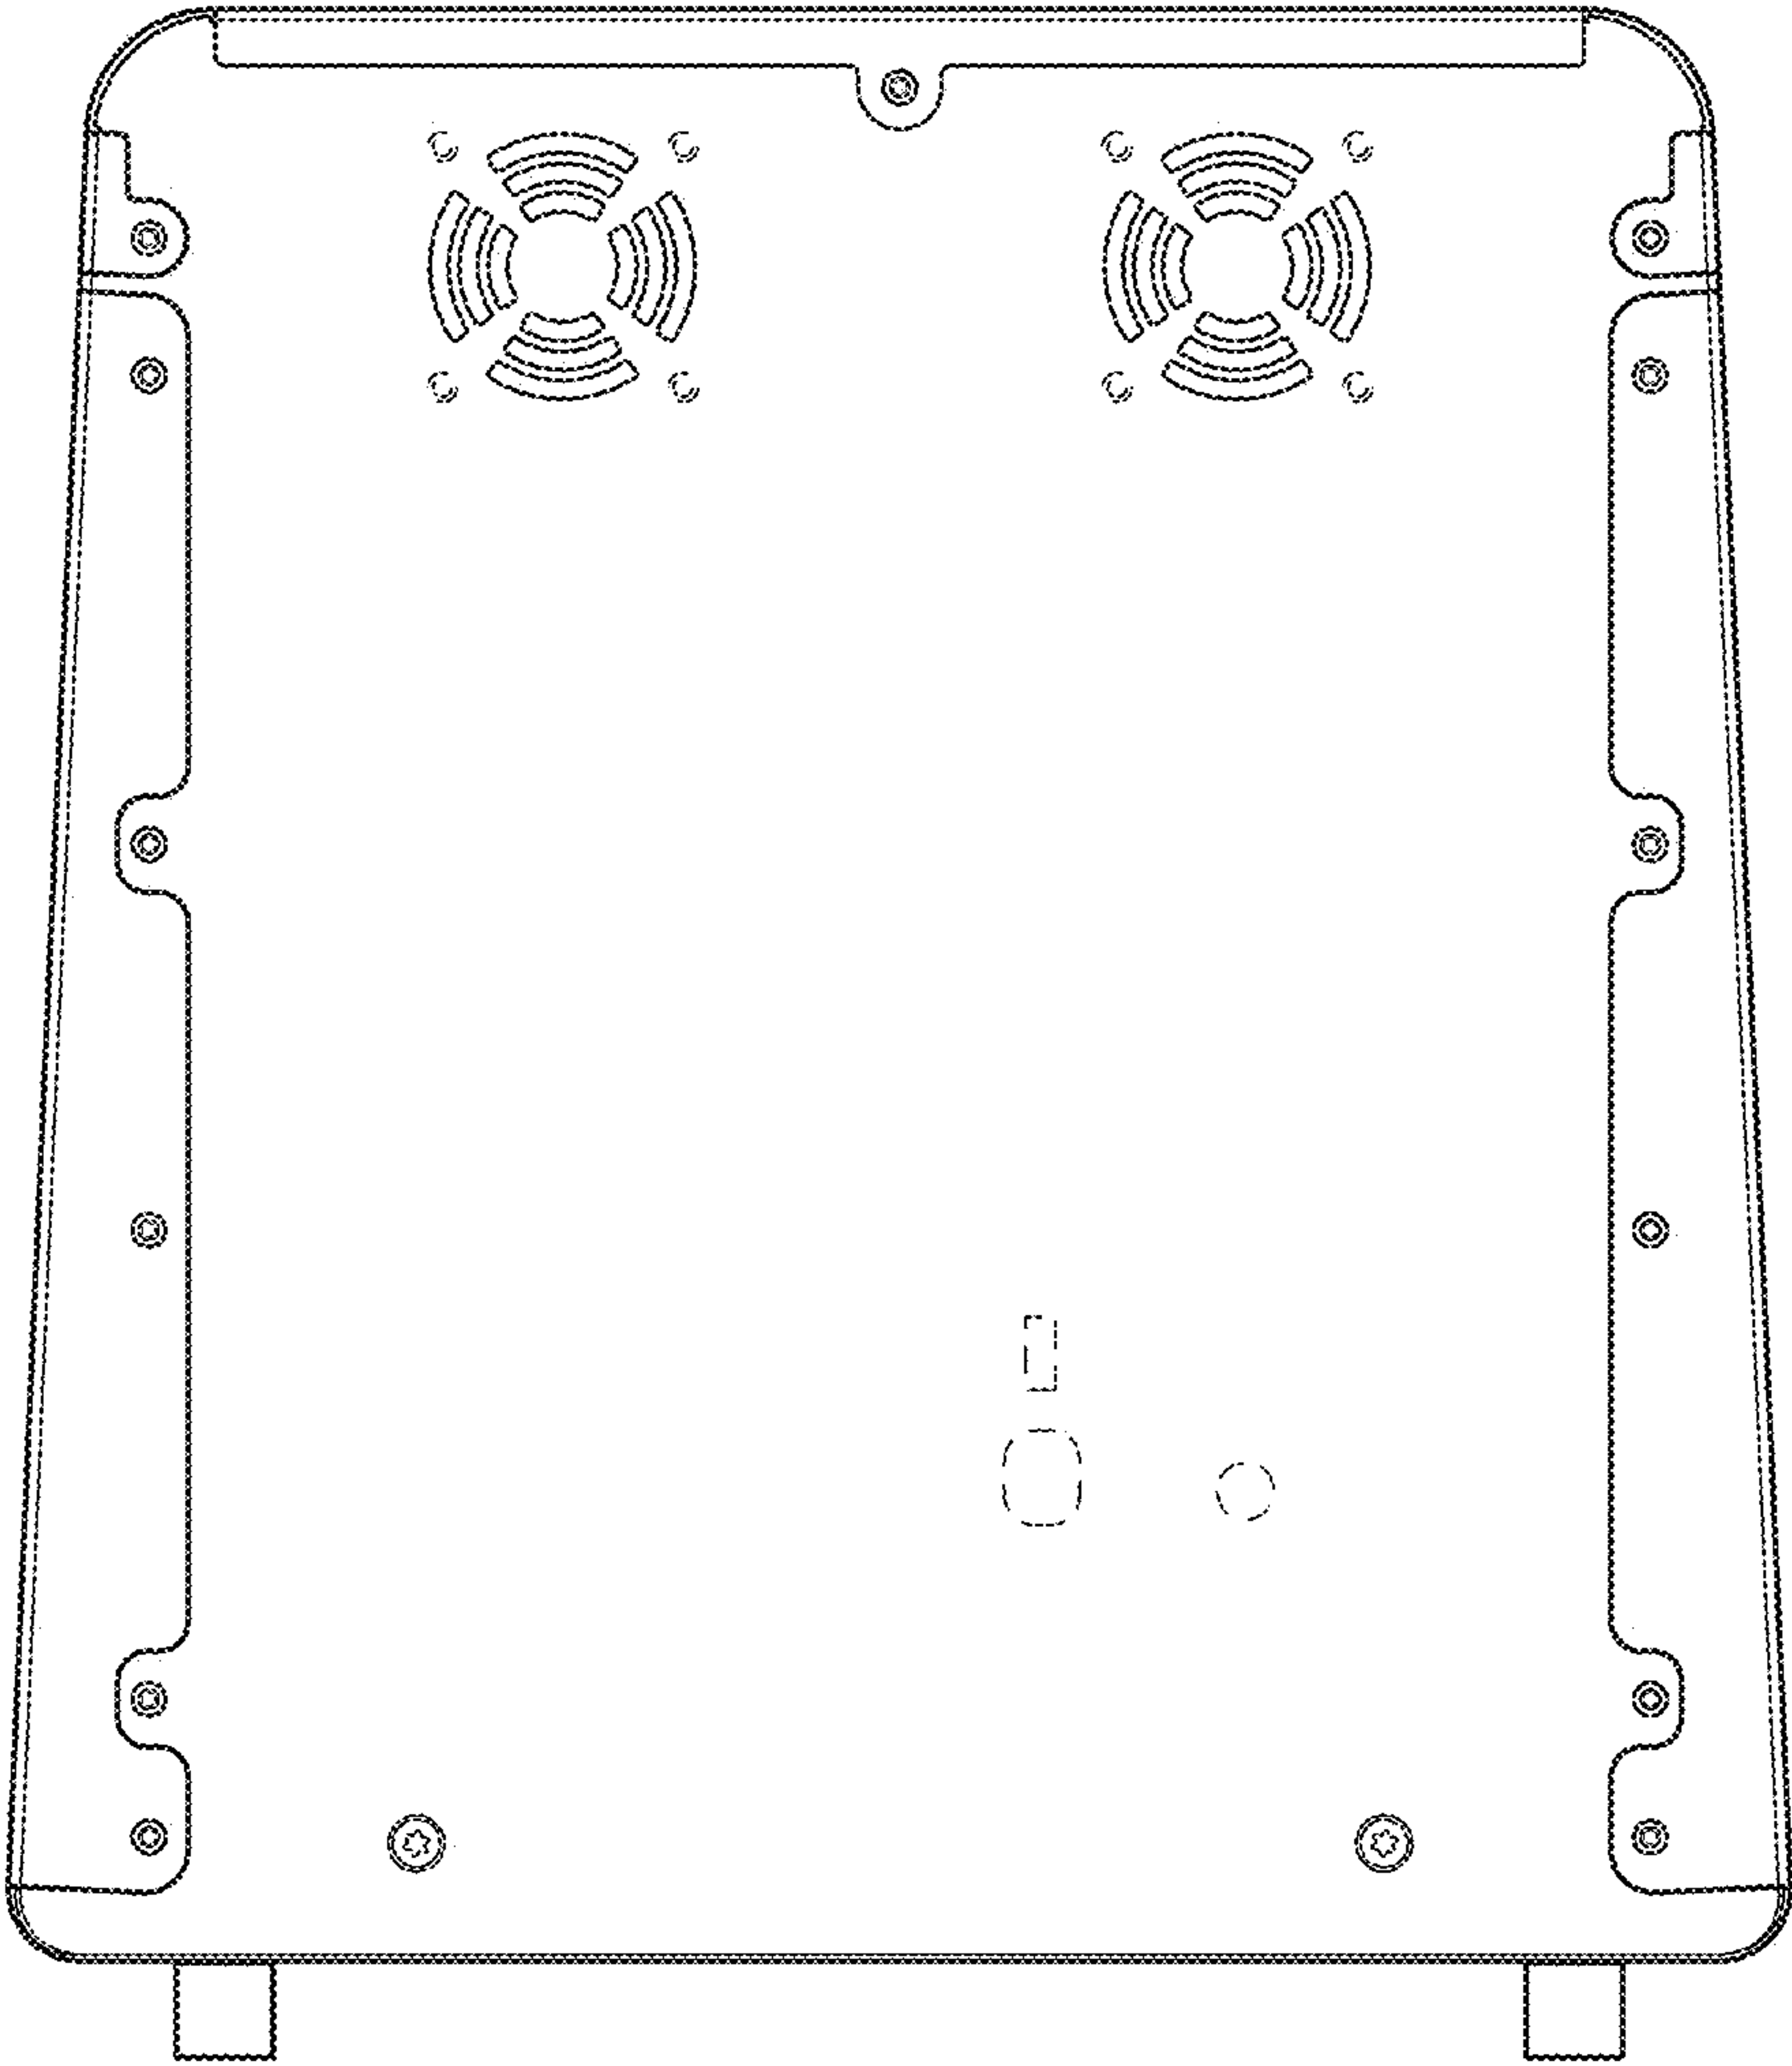


FIG. 1.4

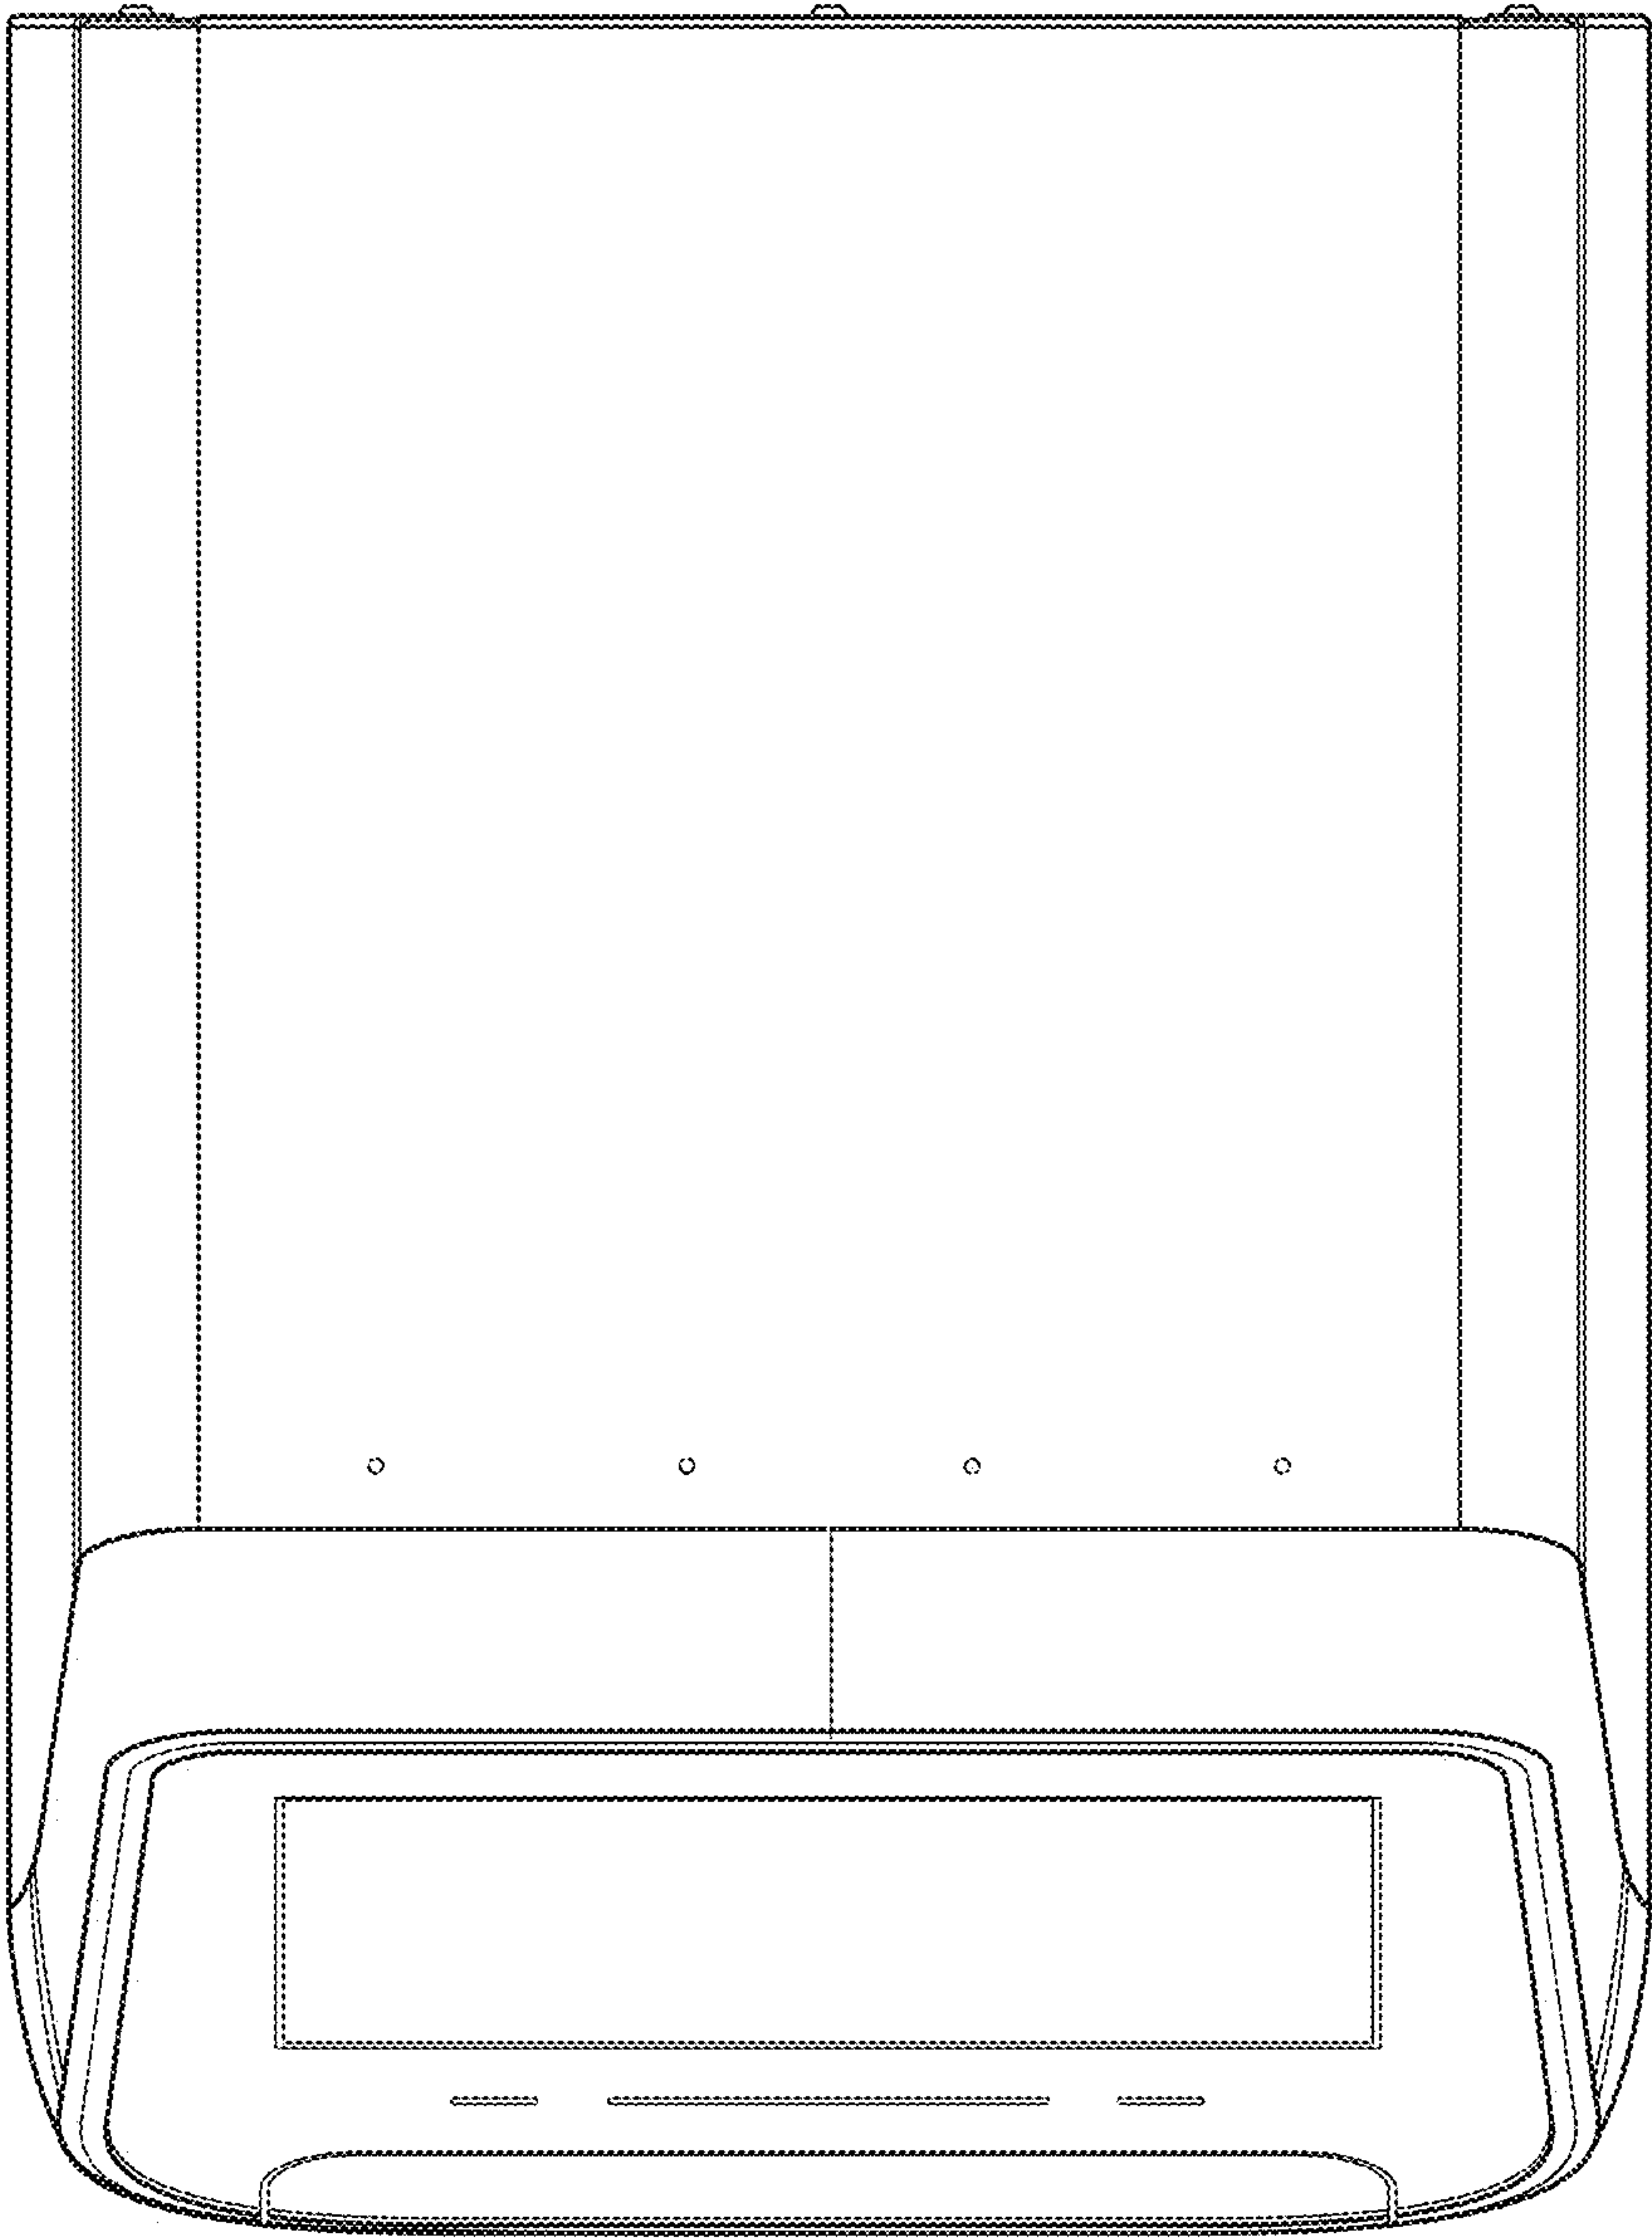


FIG. 1.5

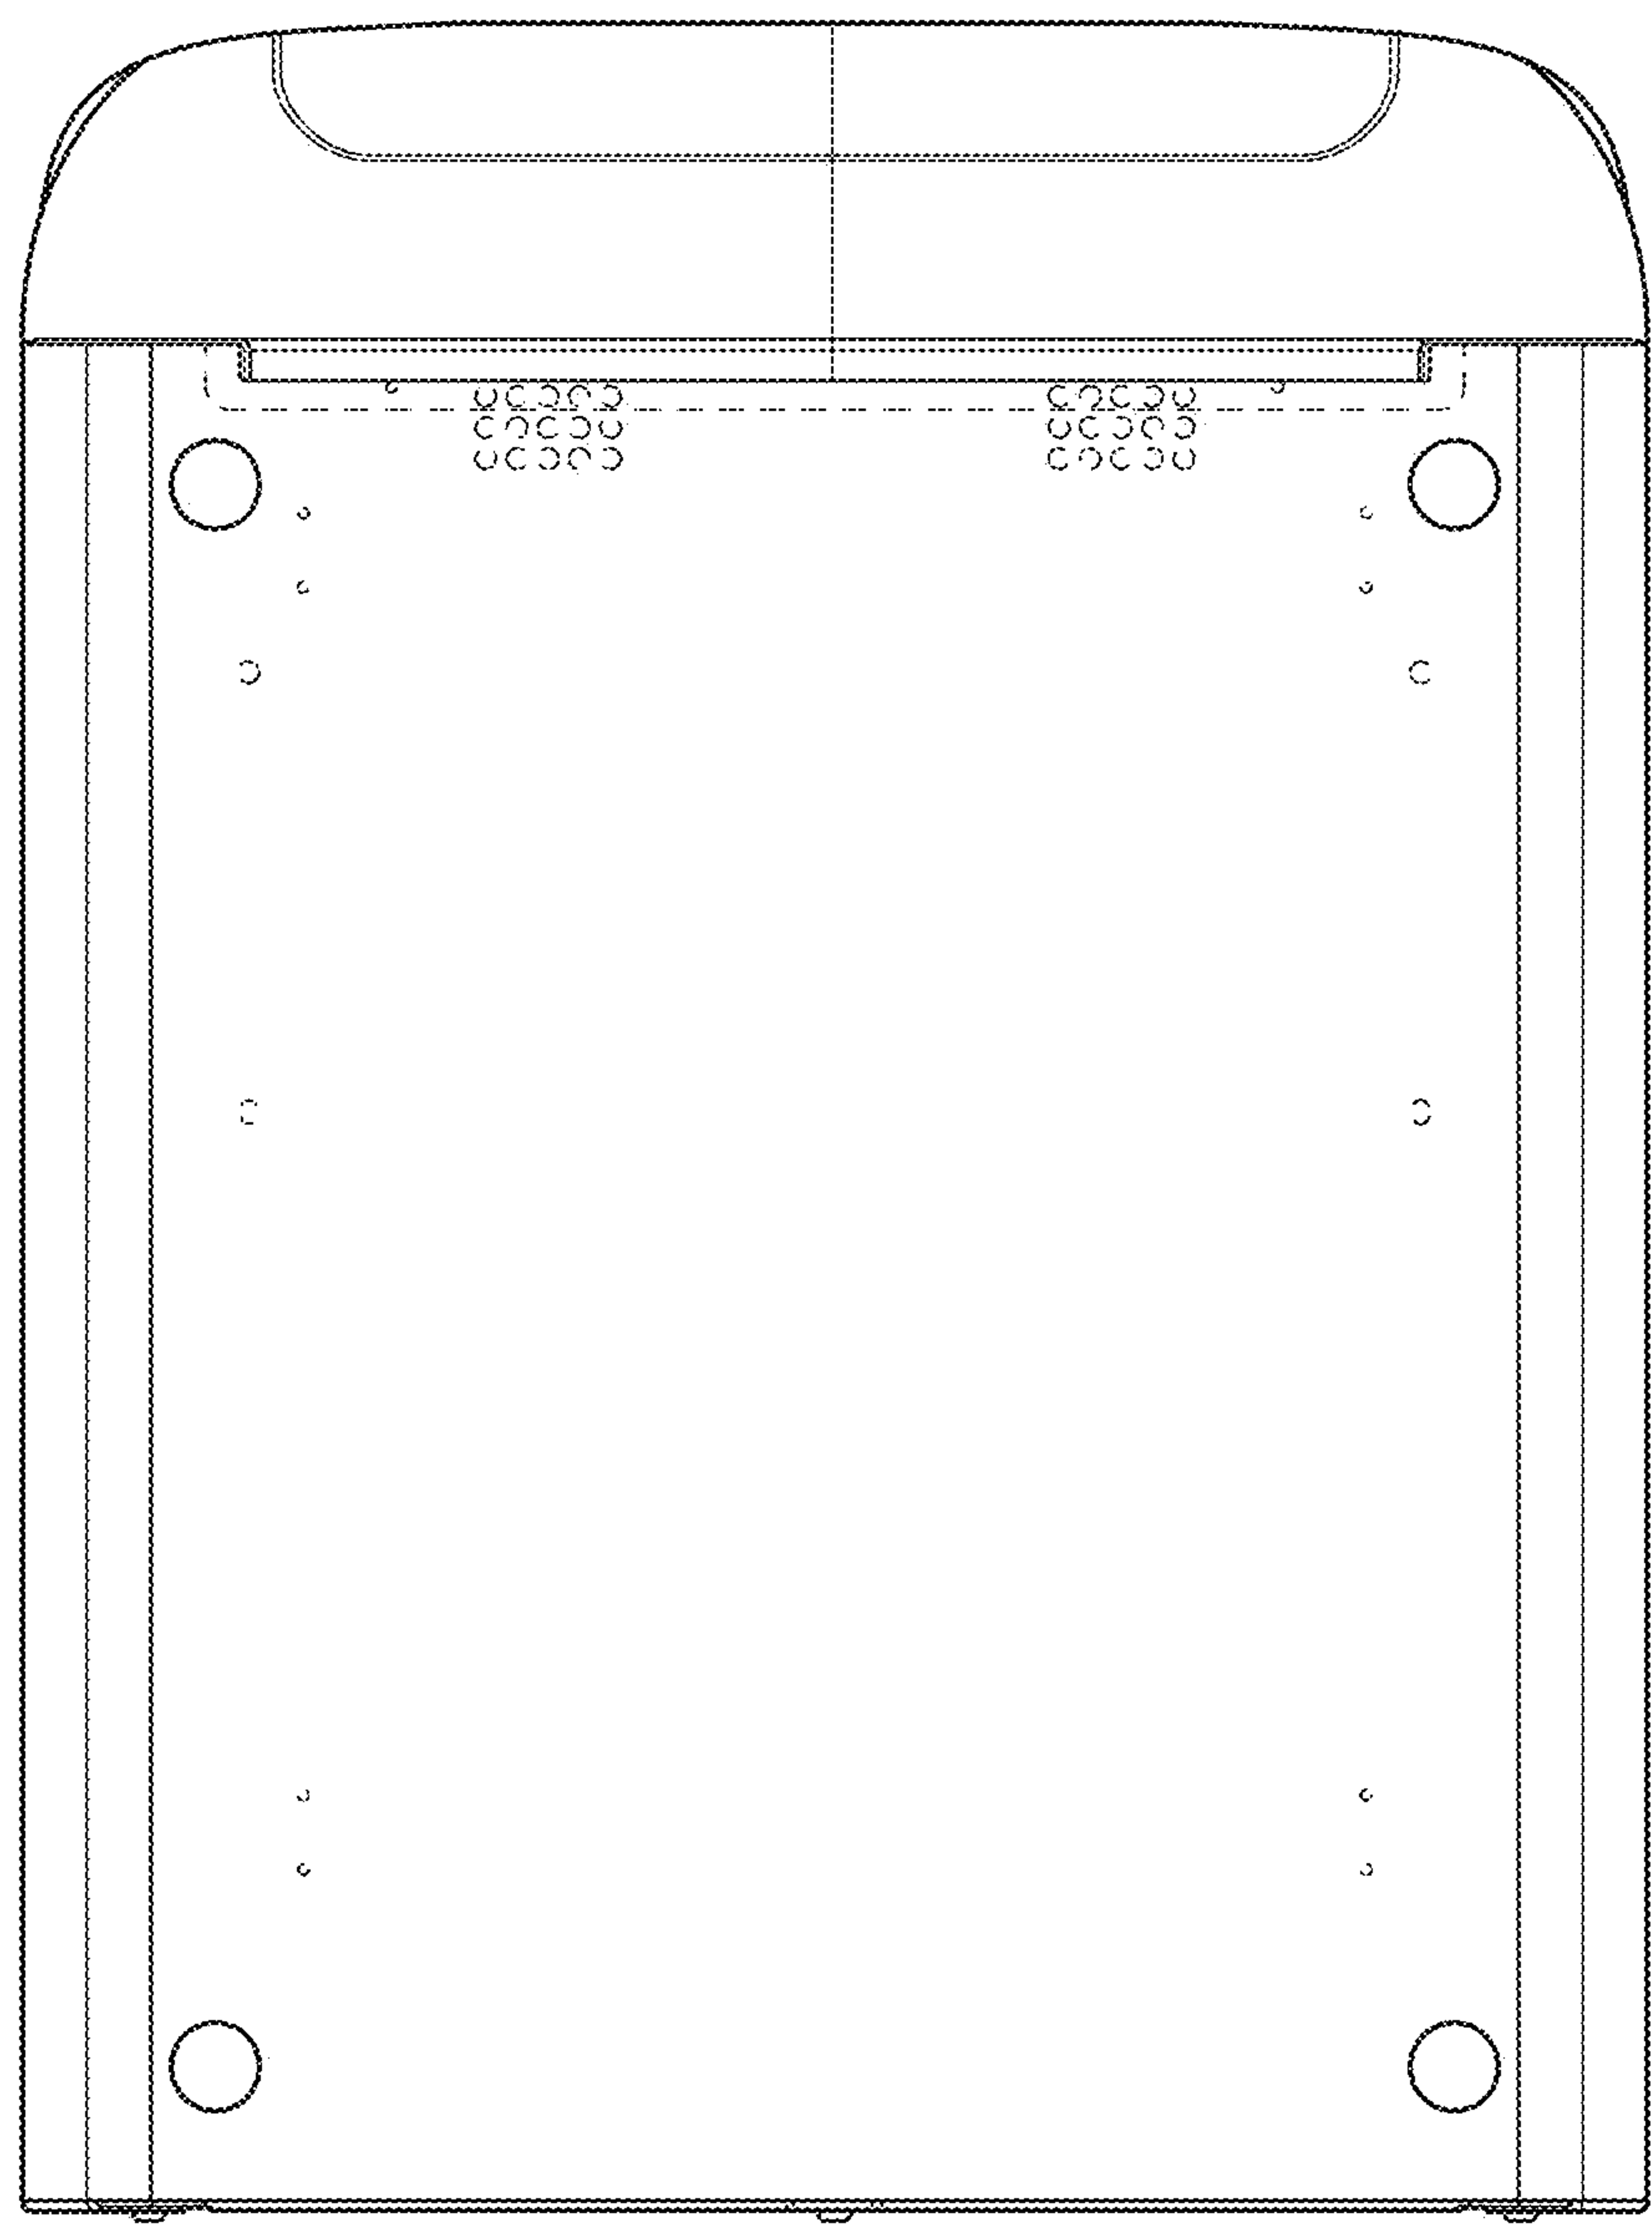


FIG. 1.6

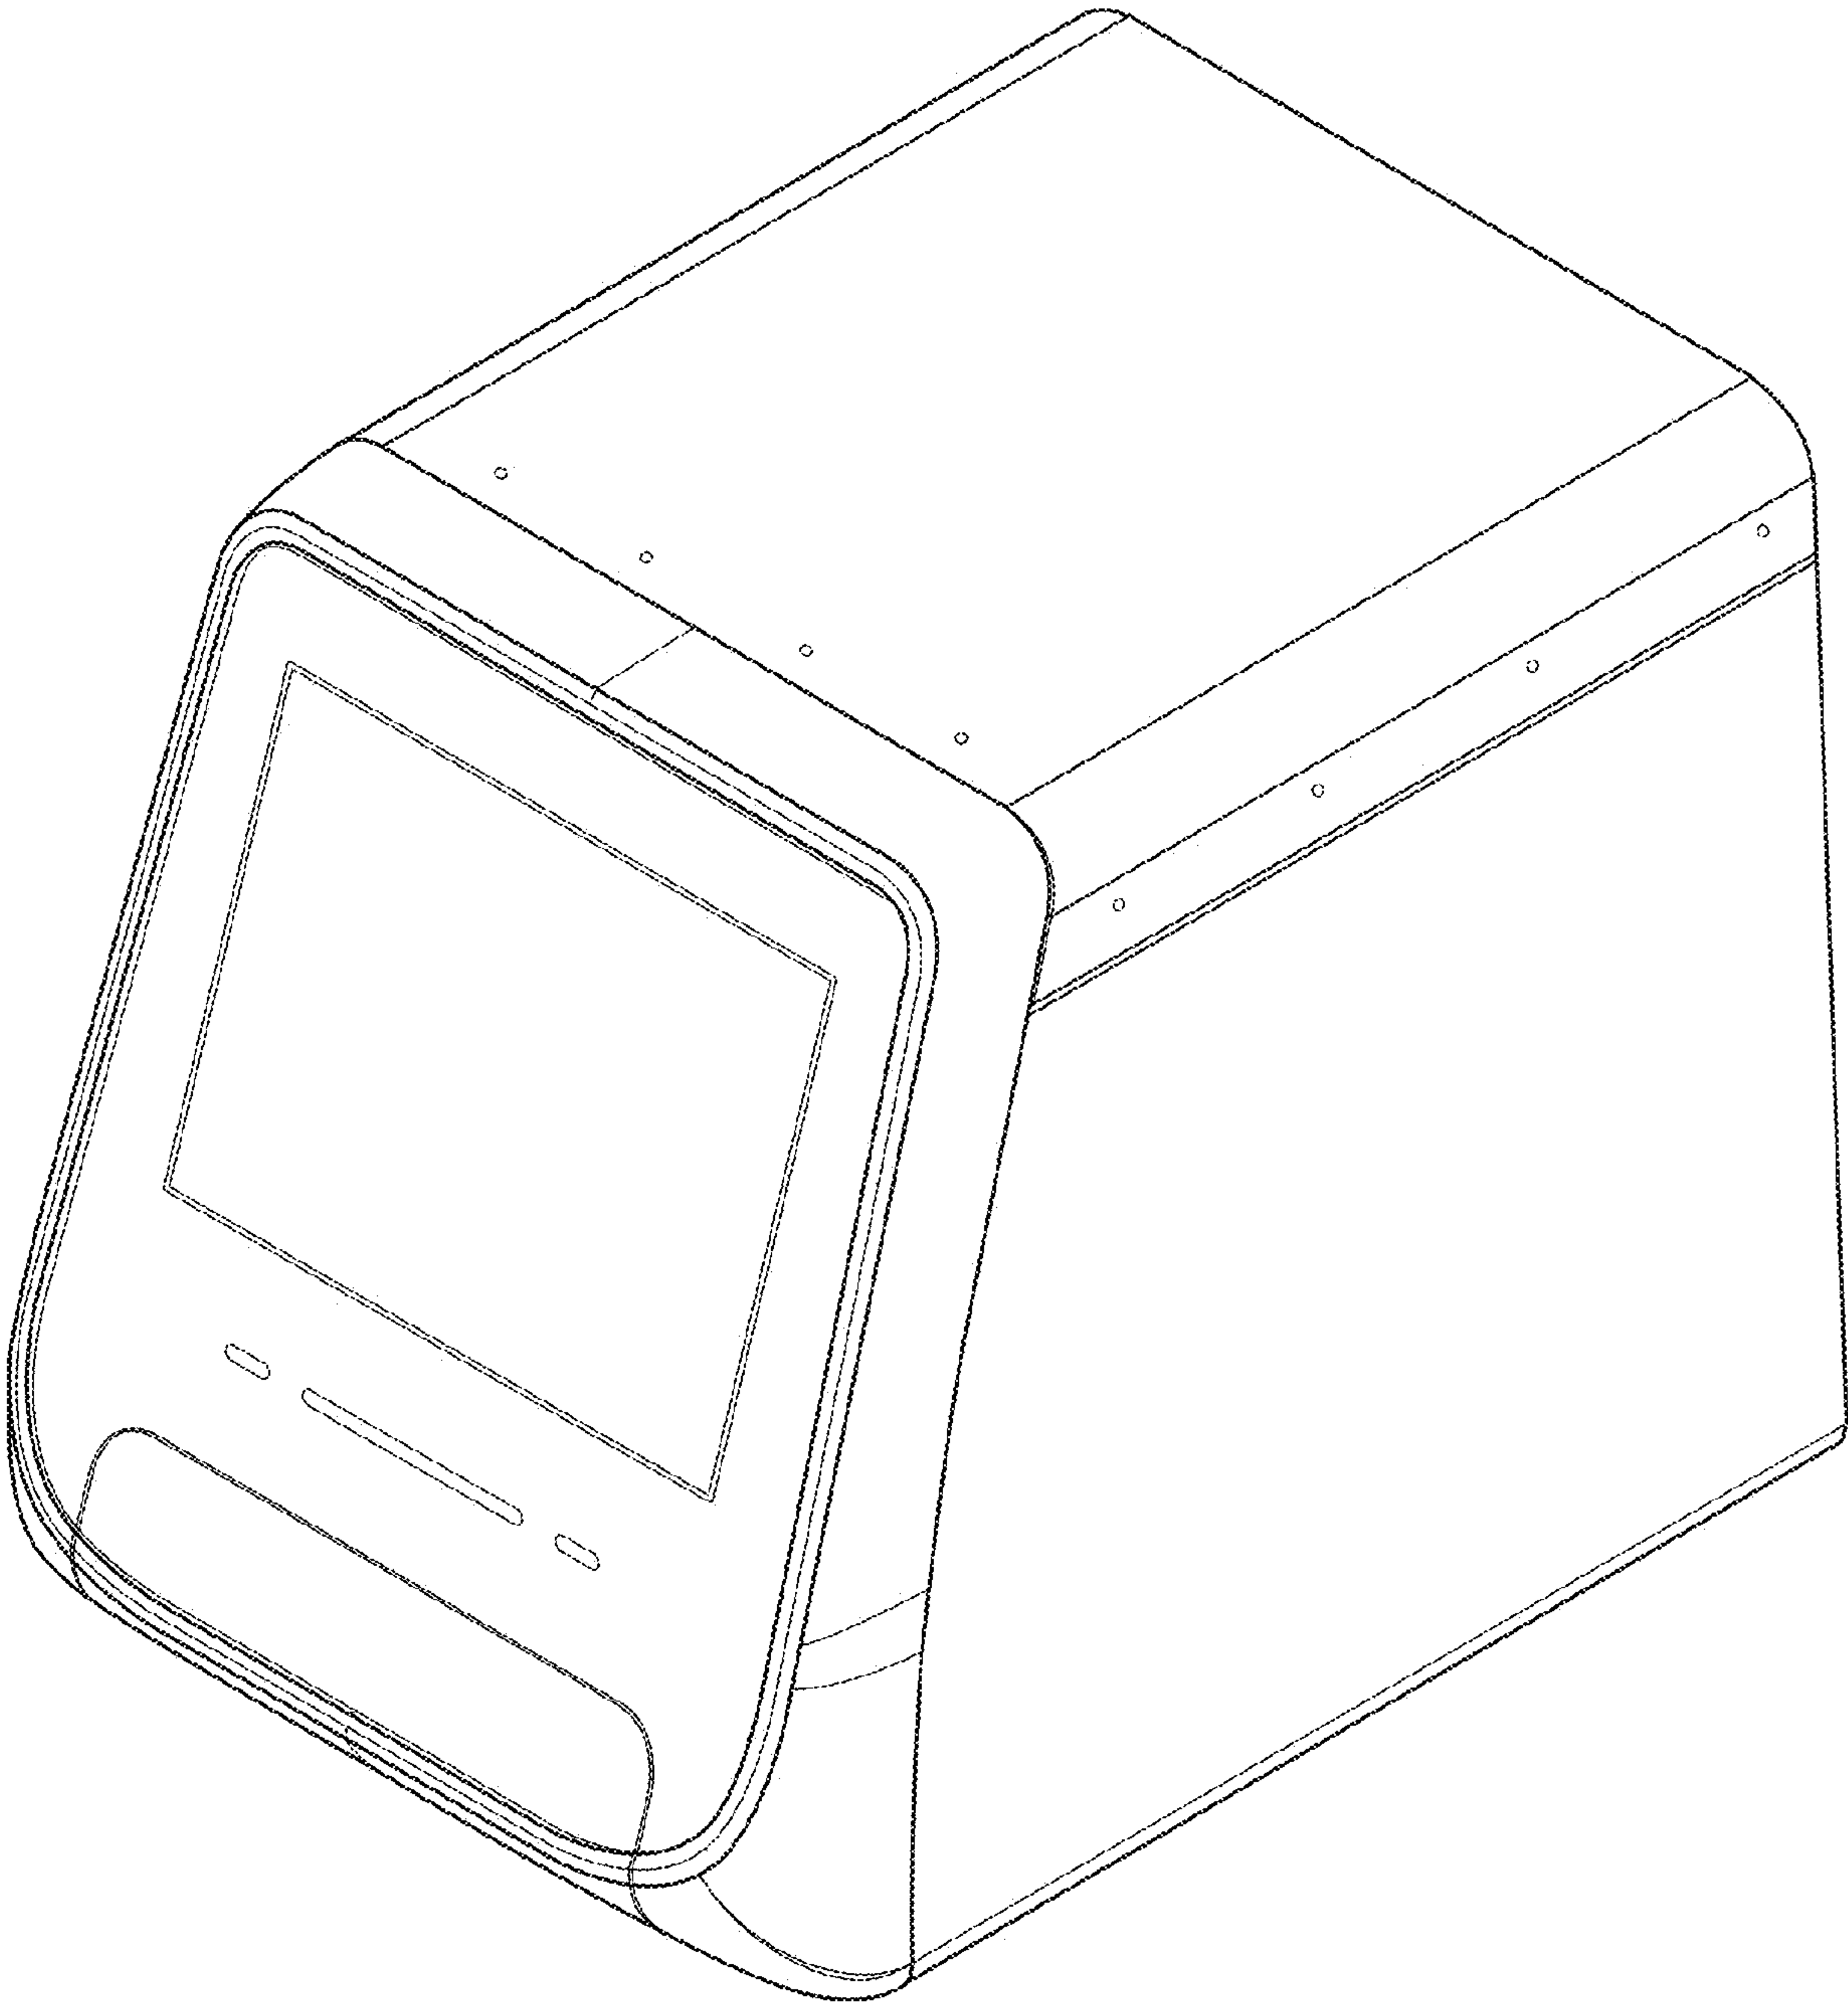


FIG. 1.7