



US0D1054027S

(12)

United States Design Patent

Held et al.

(10)

Patent No.:

US D1,054,027 S

(45)

Date of Patent:

** Dec. 10, 2024

(54)

ENDOSCOPE HANDLE

(71)

Applicant:

OLYMPUS Winter & Ibe GmbH,
Hamburg (DE)

(72)

Inventors:

Fred Held, Hamburg (DE); Thomas
Maerzke, Hamburg (DE); Alrun
Thuemen, Hamburg (DE)

(73)

Assignee:

OLYMPUS WINTER & IBE GMBH,
Hamburg (DE)

D795,424 S * 8/2017 Sloss D24/138
D798,445 S * 9/2017 Heni D24/133
D818,122 S * 5/2018 Oberkircher D24/144
D835,170 S * 12/2018 Pilz D16/130
D841,160 S * 2/2019 Cranfield D24/138
D844,137 S * 3/2019 Sun D24/138
D852,358 S * 6/2019 Matuschek D24/138
D864,388 S * 10/2019 Barber D24/133
D874,647 S * 2/2020 Cranfield D24/138
D919,804 S * 5/2021 Cole D24/133

(Continued)

(**) Term:

15 Years

(21)

Appl. No.:

29/856,113

(22)

Filed:

Oct. 11, 2022

(30)

Foreign Application Priority Data

Apr. 14, 2022 (EM) 008938948.1

(51)

LOC (14) Cl.

24-02

(52)

U.S. Cl.

USPC D24/138

(58)

Field of Classification Search

USPC D24/108, 111, 112, 118, 117, 127, 130,
D24/133, 135, 137, 138, 141, 143, 144,
D24/148, 152, 153, 154, 170, 176, 179,
D24/216, 222; D16/130, 132, 136, 200,
D16/202–206, 208, 218, 219
CPC A61B 1/00172; A61B 1/00009; A61B
1/00042; A61B 1/00043; A61B 1/00057;
A61B 1/00066; A61B 1/00105; A61B
1/00117; A61B 1/00128; A61B 1/00165;
A61B 1/00181; A61B 1/00183; A61B
1/0052
See application file for complete search history.

(57)

OTHER PUBLICATIONS

Endoeye 3D Medical device, posted at ifdesign.com, posting date
Dec. 30, 2018, retrieved Oct. 28, 2023, online, URL:https://ifdesign.
com/en/winner-ranking/project/endoeye-3d/235134 (Year: 2018).*

(Continued)

Primary Examiner — Jennifer L Rempfer
Assistant Examiner — Michelle Marquart Christeon
(74) Attorney, Agent, or Firm — Scully, Scott, Murphy &
Presser, P.C.

(57)

CLAIM

The ornamental design for an endoscope handle as shown
and described.

DESCRIPTION

FIG. 1 is an enlarged front view of an endoscope handle
showing our new design;
FIG. 2 is a top plan view thereof;
FIG. 3 is a bottom view thereof;
FIG. 4 is a left-side view thereof, the right-side view being
a mirror image thereof; and,
FIG. 5 is a perspective view thereof.
The broken lines shown in the drawings illustrate portions of
the endoscope handle that form no part of the claimed
design.


(56)

References Cited

U.S. PATENT DOCUMENTS

D745,670 S * 12/2015 Czupalla D24/138
D779,053 S * 2/2017 Kobida D24/108

1 Claim, 5 Drawing Sheets

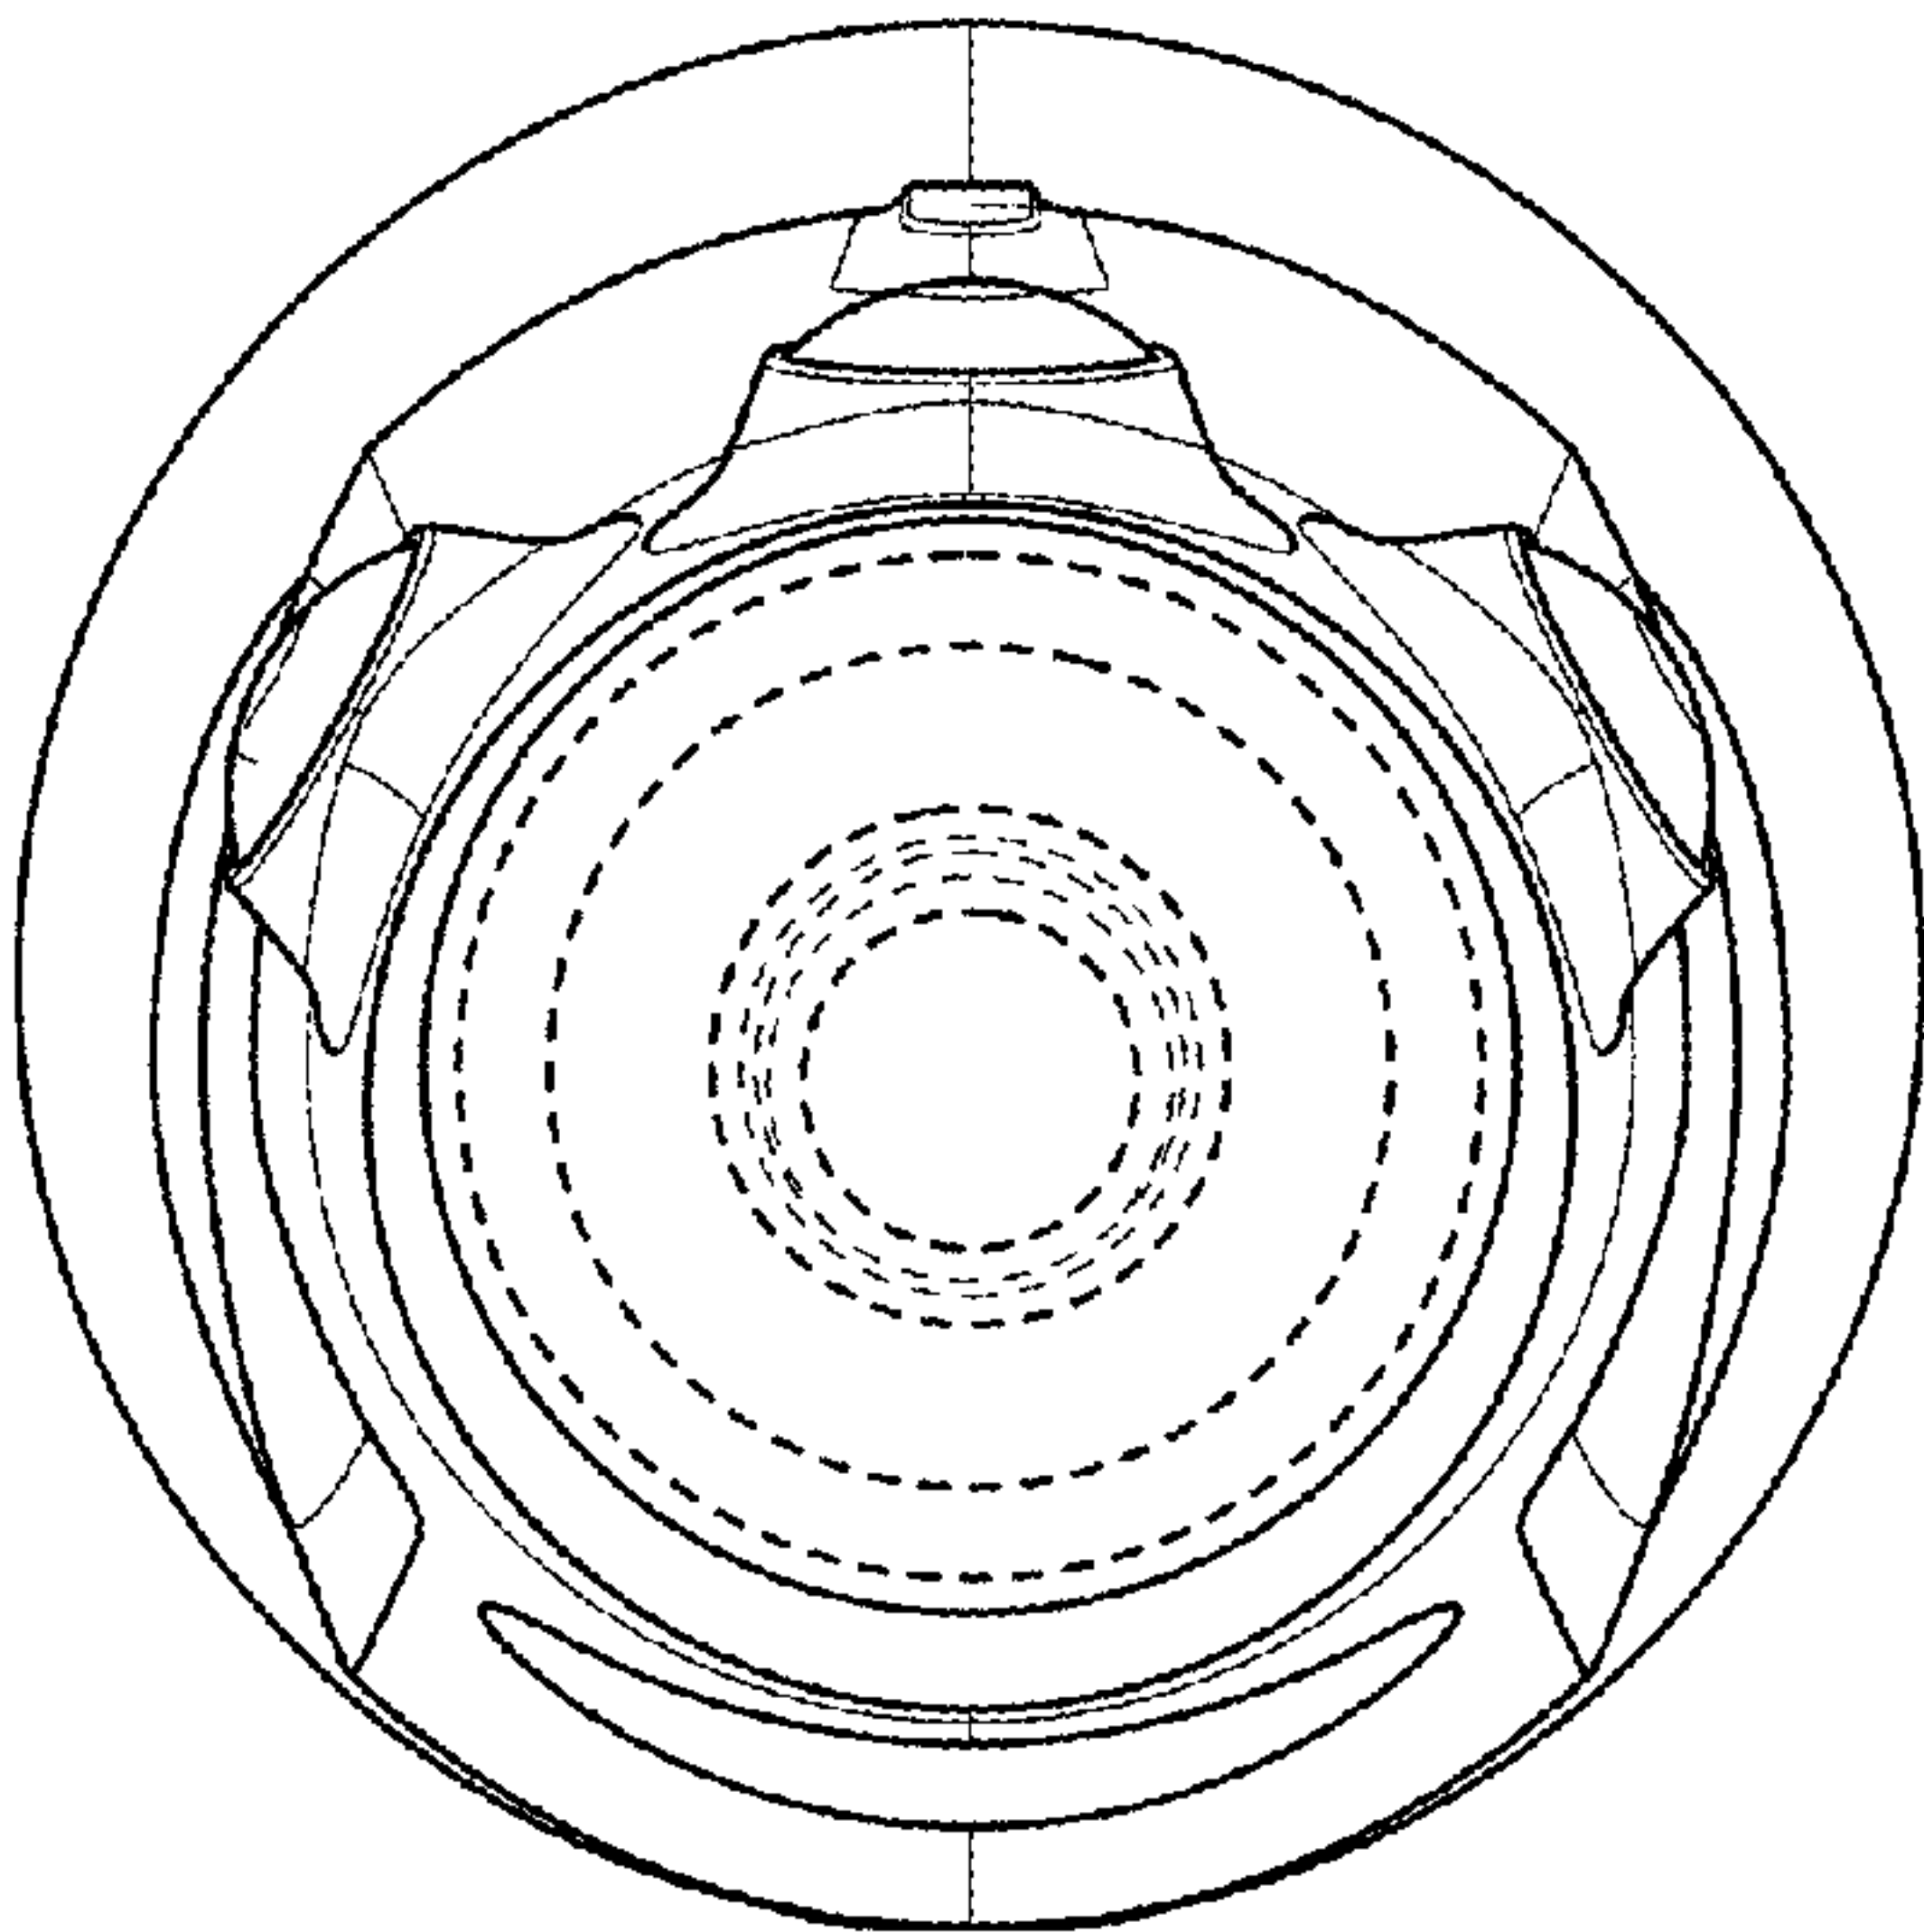

(56) **References Cited**

U.S. PATENT DOCUMENTS

D956,969 S * 7/2022 Bast D24/133
2015/0343121 A1 * 12/2015 Kobida A61M 1/7411
604/187

OTHER PUBLICATIONS

Olympus Visera Elite II 3D, posted at ifdesign.com, posting date Jun. 30, 2021, retrieved Oct. 28, 2023, online, URL:<https://www.youtube.com/watch?v=lskCd6dfZvA&t=65s> (Year: 2021).*

Endoeye HDII catalog, posted at medfau.com, posting date unavailable, retrieved Oct. 28, 2023, online, URL:<chrome-extension://efaidnbmnnnibpcajpcglclefindmkaj/https://medfau.com/wp-content/uploads/2021/05/endoeye-hd-5mm.pdf>(Year: 2023 (Year: 2023)).*

Red Dot Group, “Red Dot Design Award Endoeye” published 2014; Olympus Winter & Ibe GmbH.

HD Endoeye High definition digital videolaparoscope—resolutionary imaging, Endoeye, Olympus Europa Holding GMBH, 2013.

Video Telescope, Endoeye HD II, Olympus, Copyright 2020 Olympus Winter & Ibe GmbH.

* cited by examiner

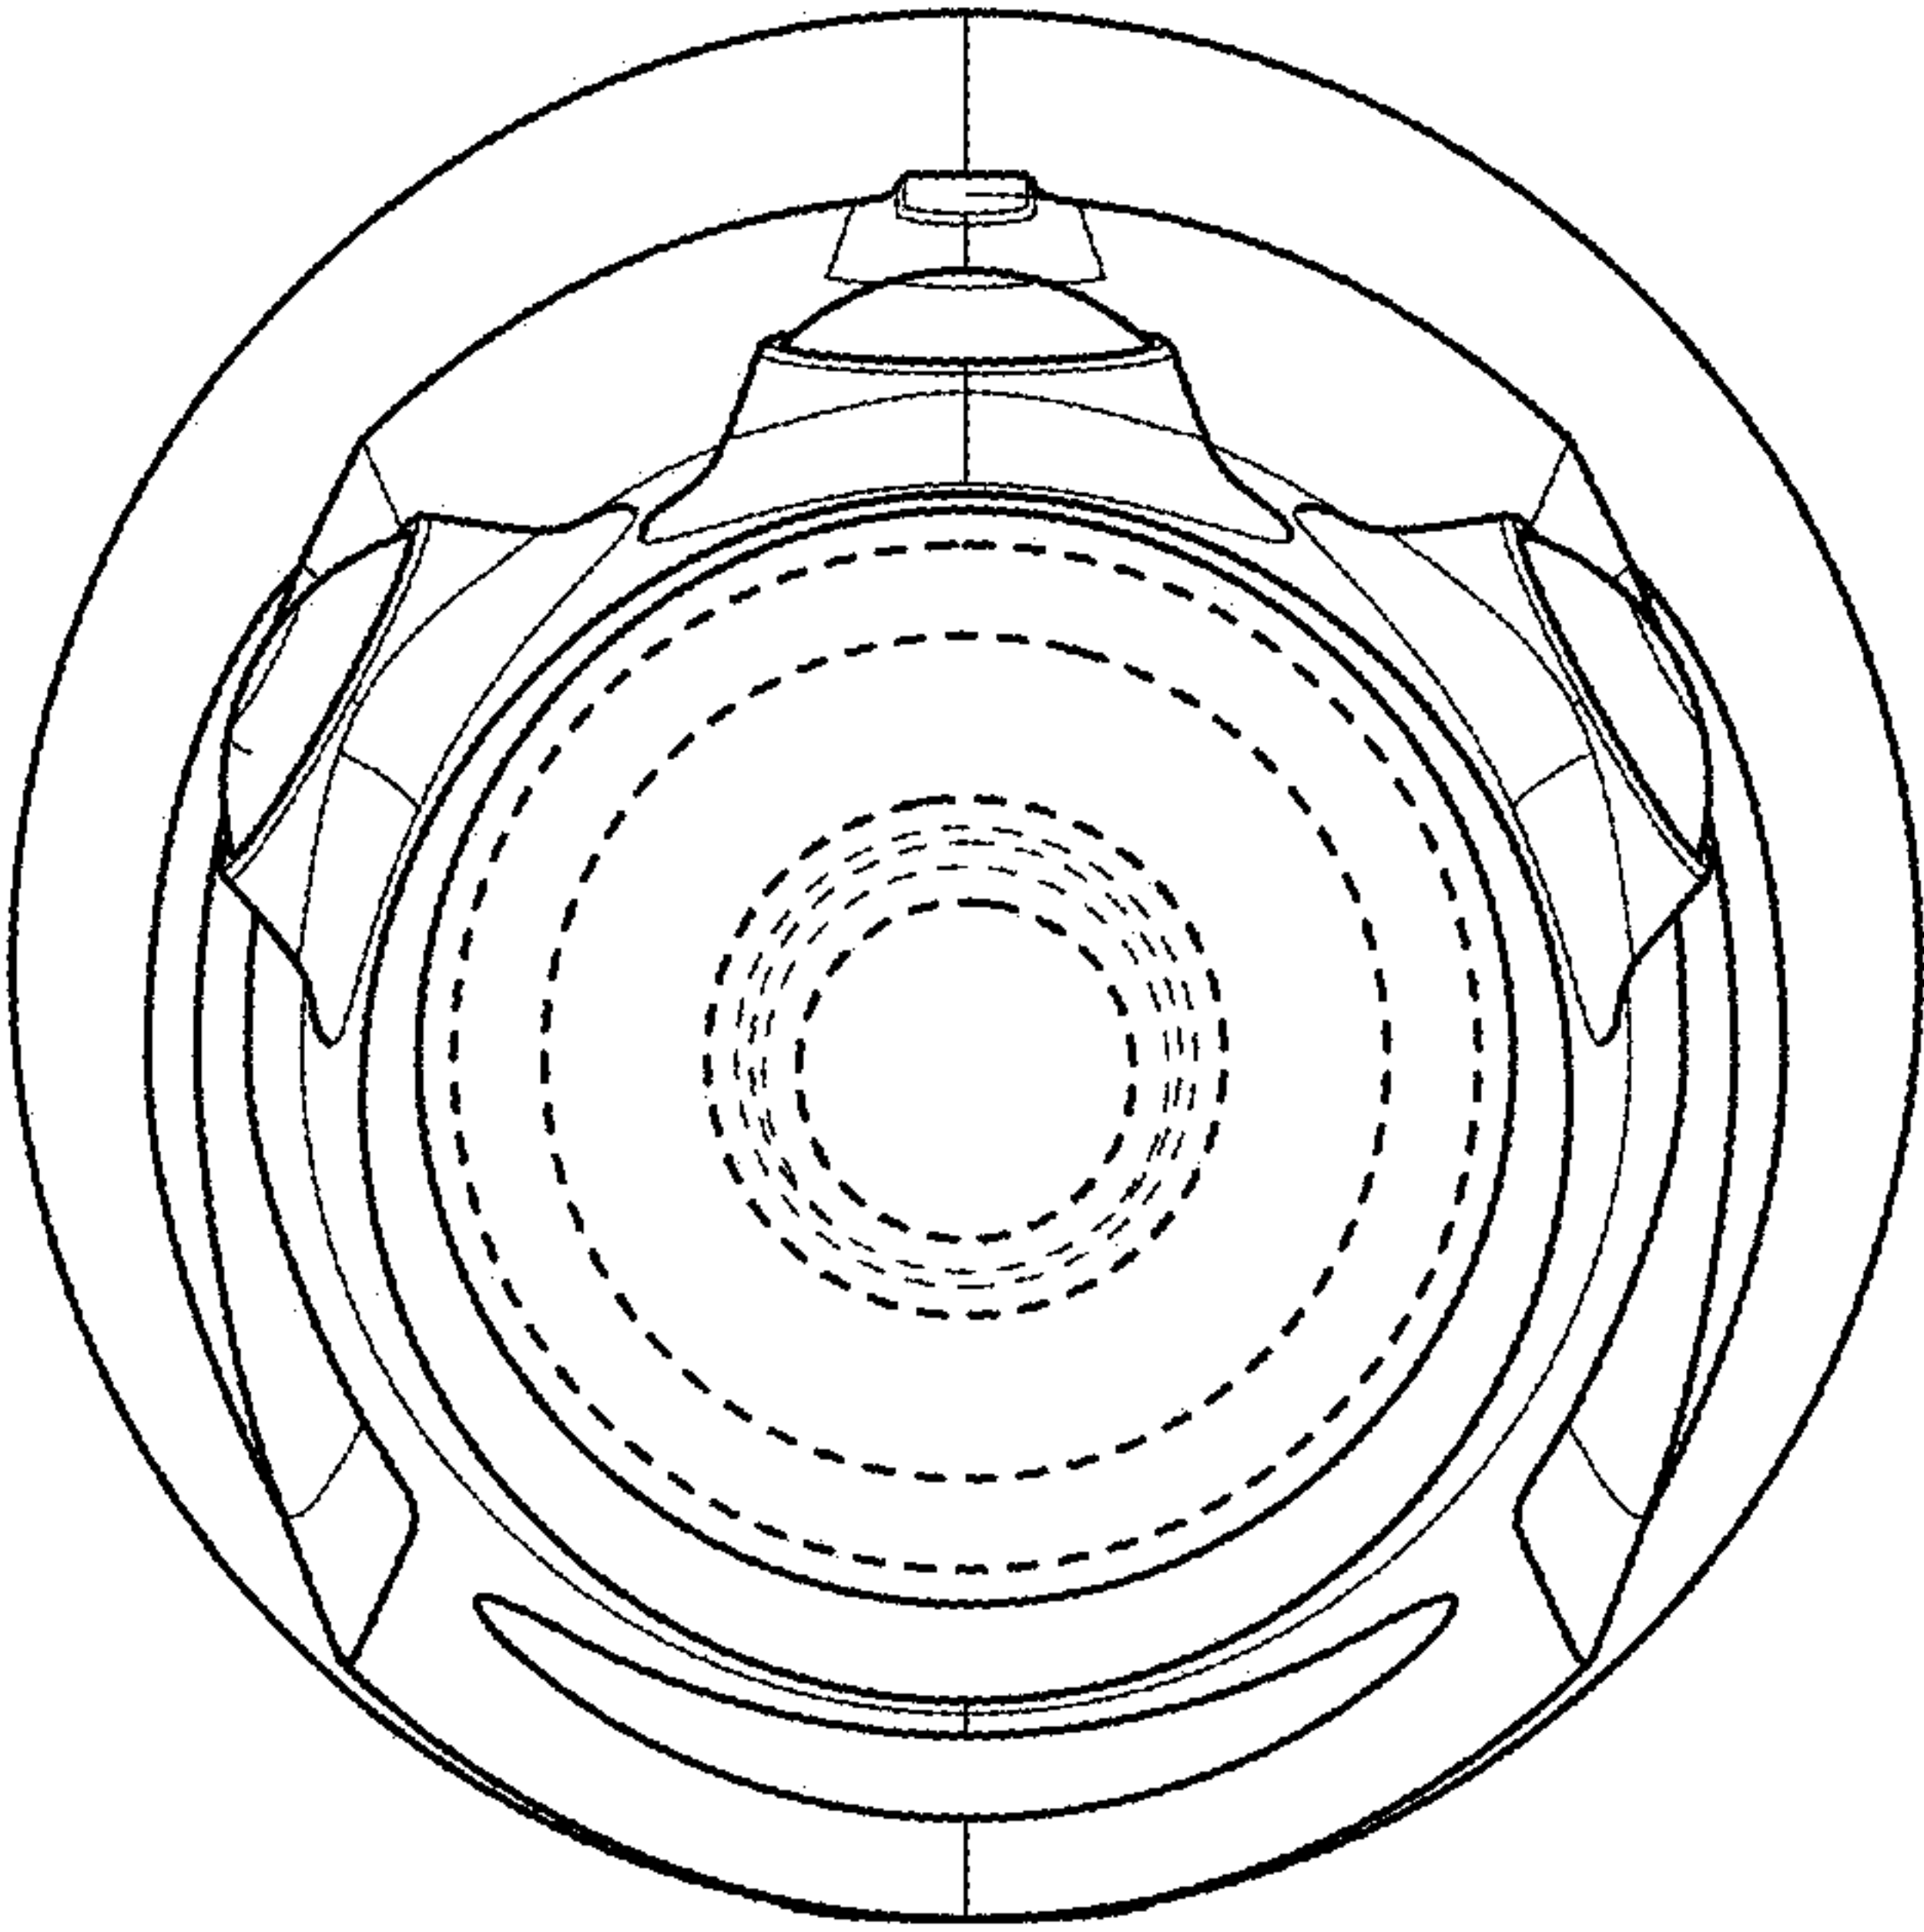


FIG. 1

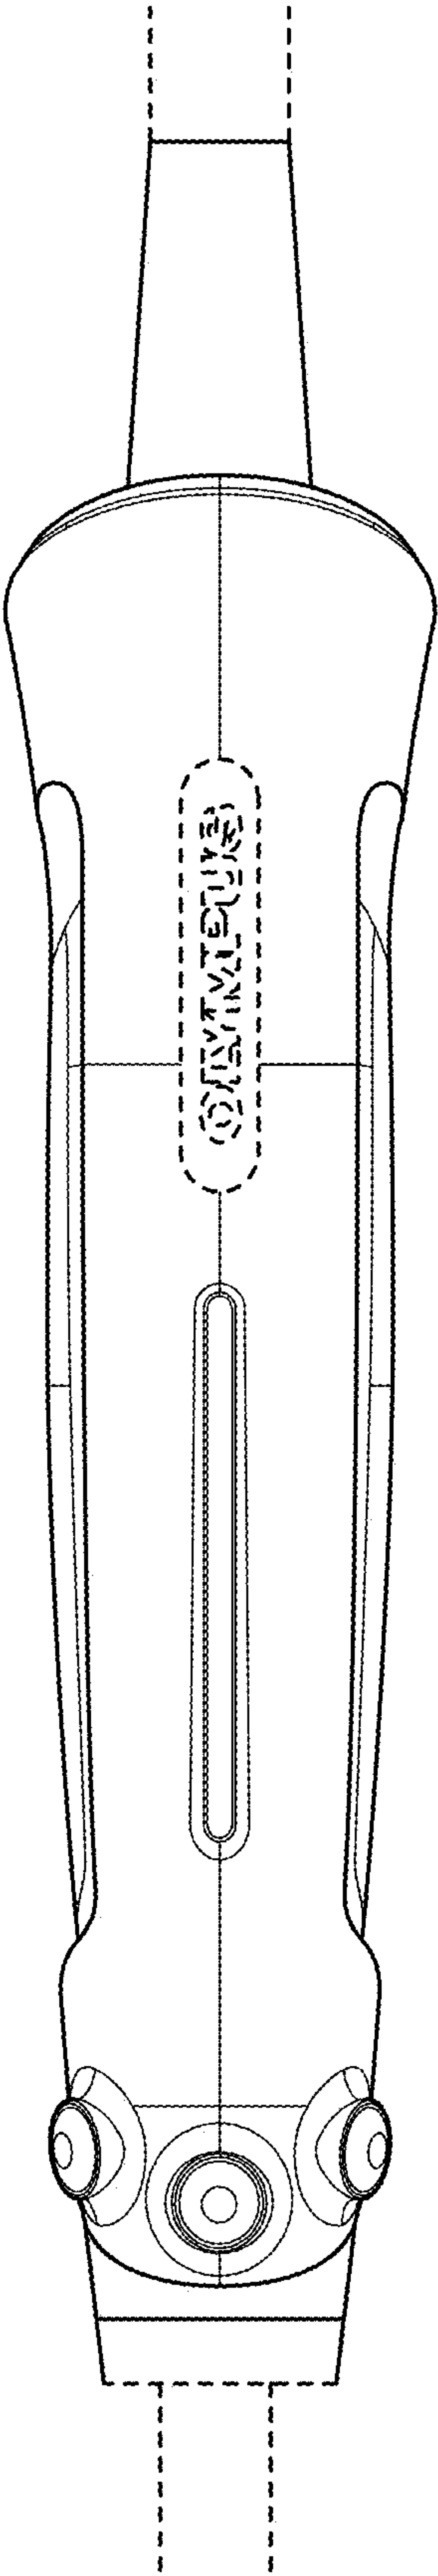


FIG. 2

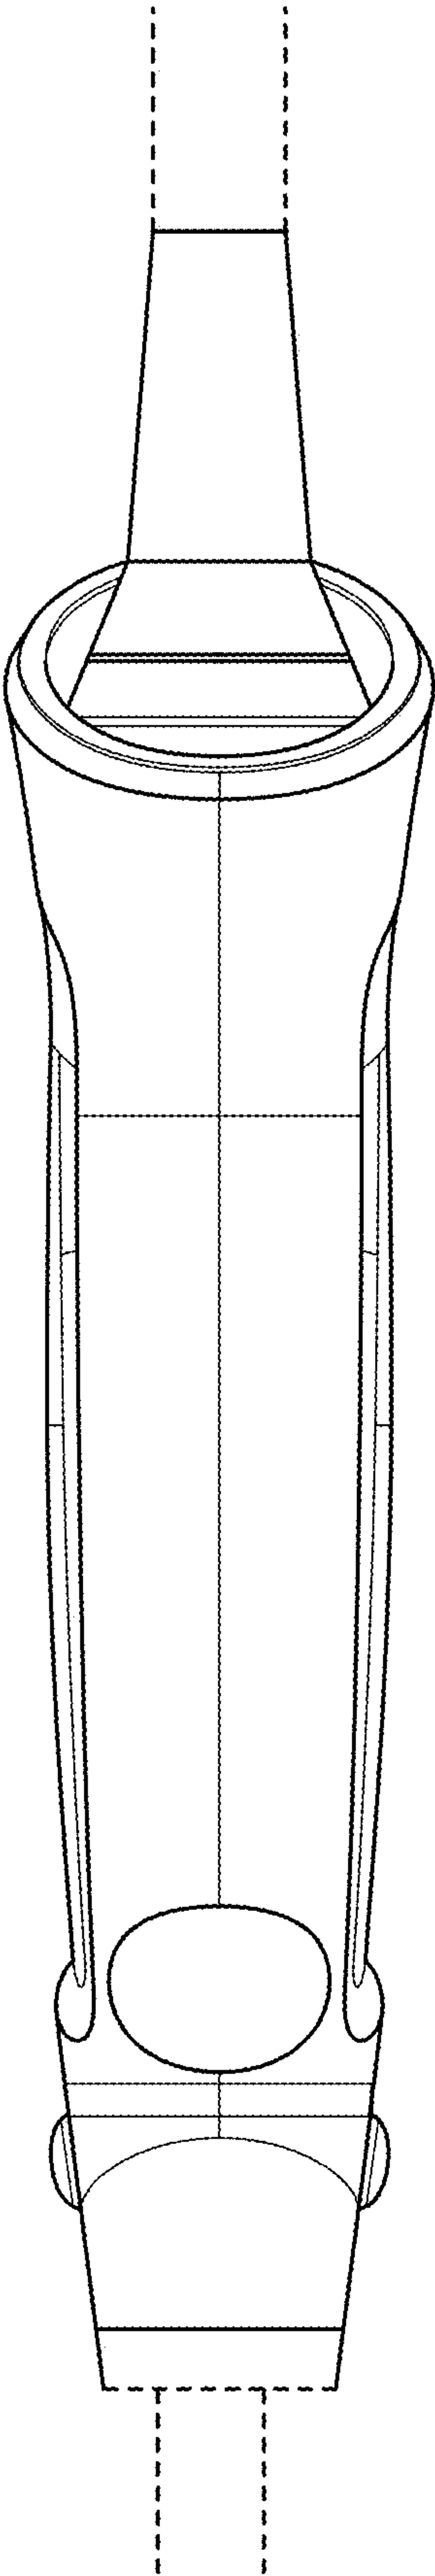


FIG. 3

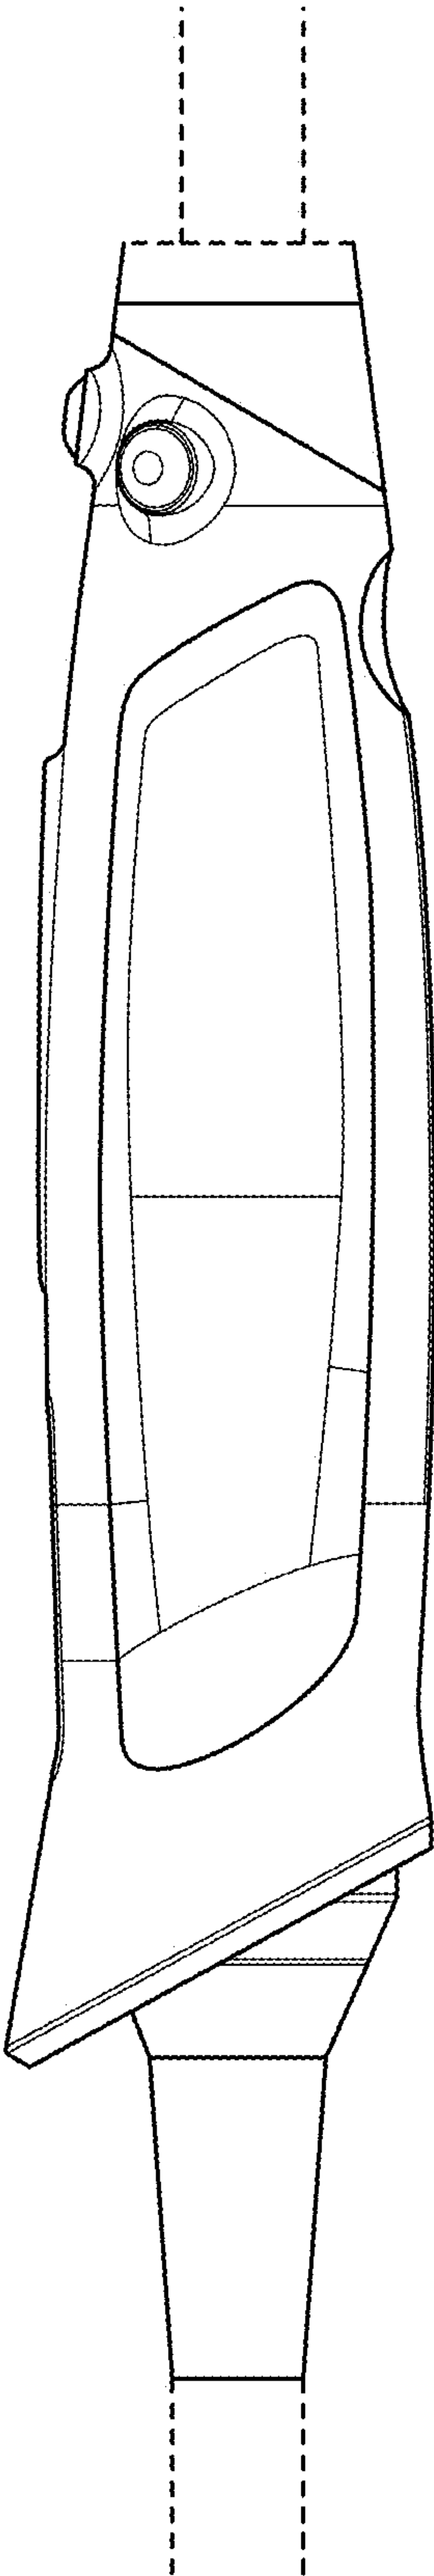


FIG. 4

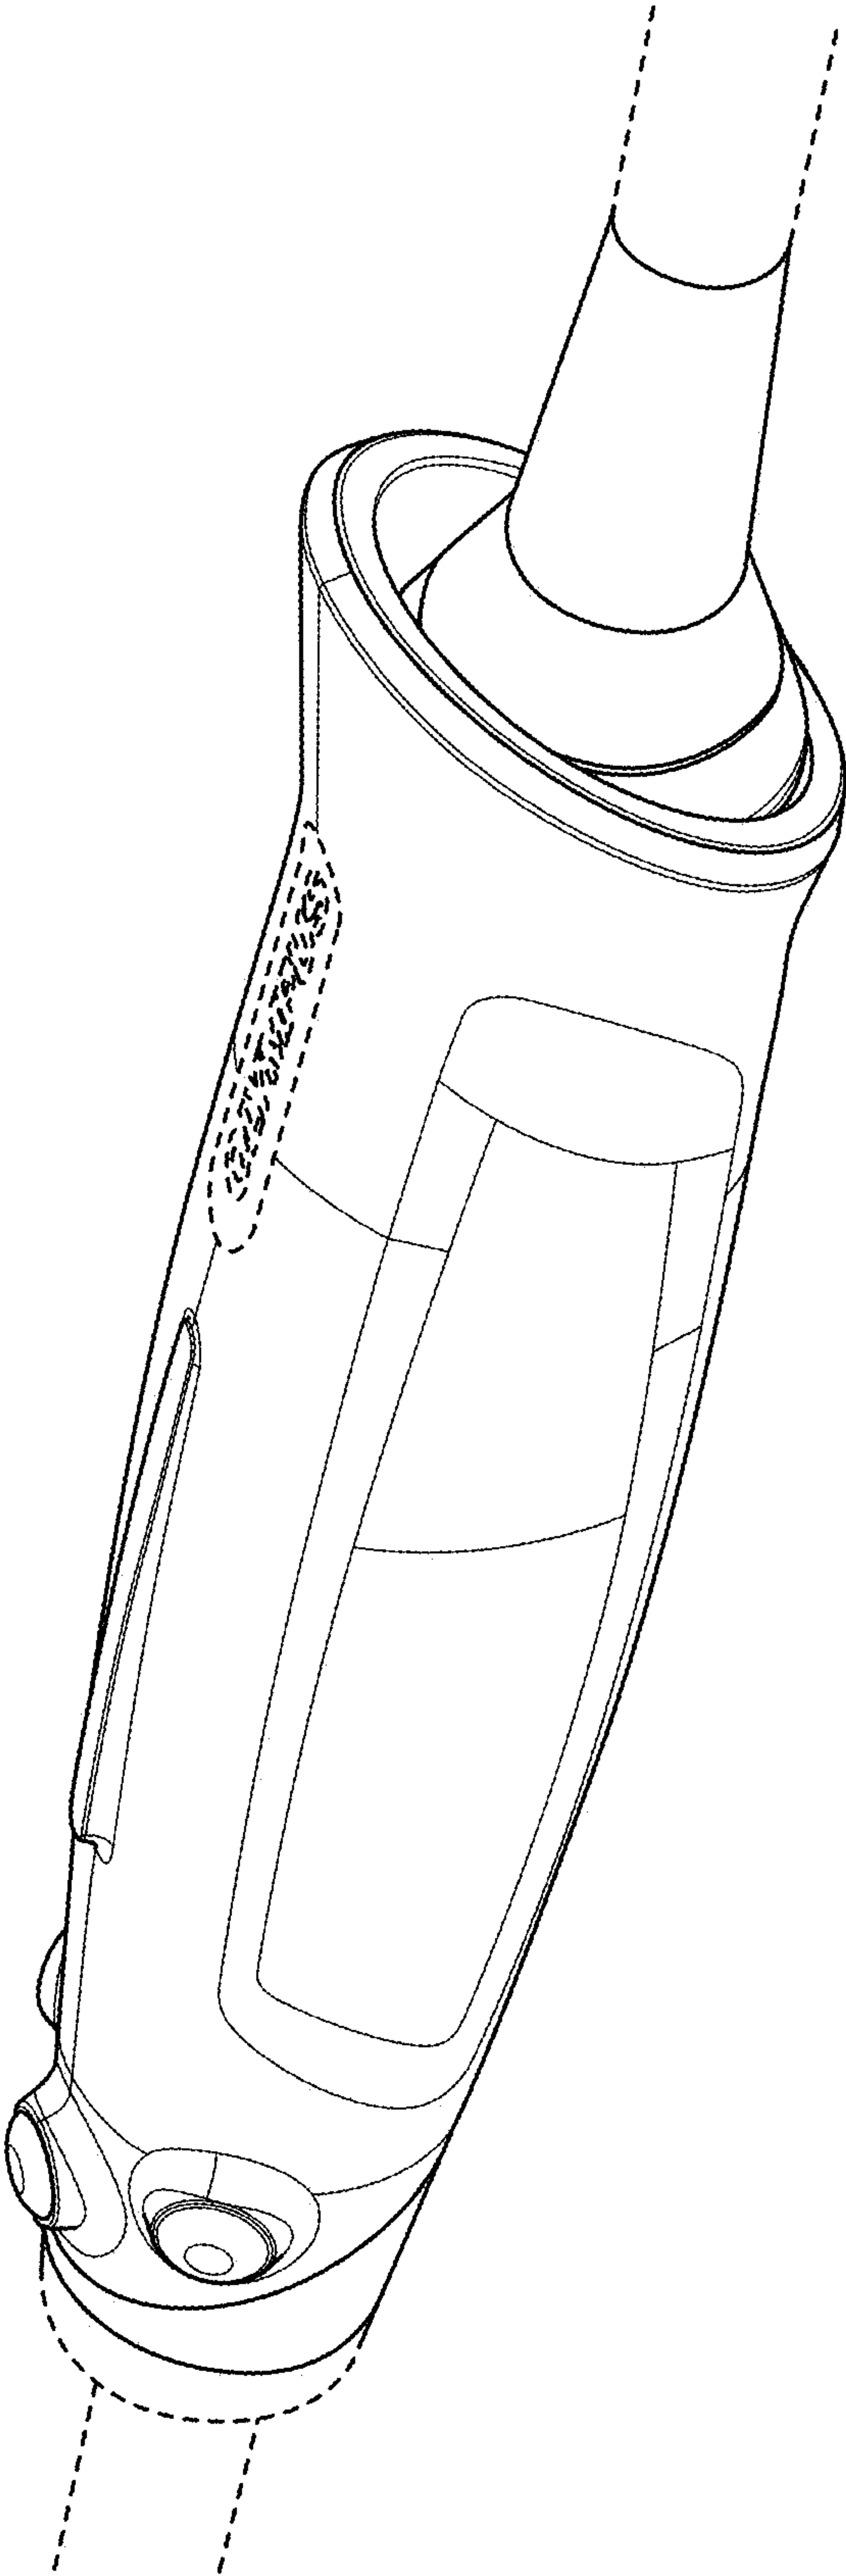


FIG. 5