



US0D1054582S

(12)

United States Design Patent

Luther et al.

(10) Patent No.:

US D1,054,582 S

(45) Date of Patent:

** Dec. 17, 2024

(54) ELECTROPORATION PROCESSING DEVICE

(71) Applicant: MaxCyte, Inc., Gaithersburg, MD (US)

(72) Inventors: James William Luther, Milan (IT);
Bertold Engler, Altensteig (DE);
Andrea Besana, Seveso (IT); Thomas
Alan Peach, Milan (IT); Frank
Modica, Silver Spring, MD (US);
Nicholas Chopas, Germantown, MD
(US)

(73) Assignee: MaxCyte, Inc., Rockville, MD (US)

(**) Term: 15 Years

(21) Appl. No.: 29/791,748

(22) Filed: Feb. 3, 2022

Related U.S. Application Data

(63) Continuation of application No. 29/734,300, filed on
May 11, 2020, now Pat. No. Des. 944,410.

(51) LOC (14) Cl. 24-02

(52) U.S. Cl.
USPC D24/216

(58) Field of Classification Search
USPC D24/107, 185, 186, 216, 224, 231, 232,
D24/233; D10/81
CPC A61N 1/327; A61N 1/0412; B01L 2200/16;
B01L 2200/18; B01L 2300/0809; B01L
3/502; B01L 3/523
See application file for complete search history.

(56) References Cited

U.S. PATENT DOCUMENTS

D445,509 S 7/2001 Berndt et al.
6,773,669 B1 8/2004 Holaday et al.
D564,100 S * 3/2008 O'Banion D24/216

D630,765 S 1/2011 Winkenbach et al.
D672,466 S * 12/2012 Kravitz D24/216
D711,549 S 8/2014 Trump
(Continued)

FOREIGN PATENT DOCUMENTS

CN 304579343 * 4/2018
CN 305871200 * 6/2020
KR 3012451580002 * 1/2024

OTHER PUBLICATIONS

"MaxCyte: Small-scale Ruo Processing Assemblies." Found online
Apr. 12, 2024 at maxcyte.com. Reference dated Mar. 27, 2023.
Retrieved from <https://maxcyte.com/processing-assemblies/static-ruo-small/>.*

(Continued)

Primary Examiner — Kendra Leslie Hamilton

Assistant Examiner — Elizabeth S Struble

(74) Attorney, Agent, or Firm — Finnegan, Henderson,
Farabow, Garrett & Dunner LLP

(57) CLAIM


The ornamental design for an electroporation processing
device, as shown and described.

DESCRIPTION

FIG. 1 is a front, top, right perspective view of an elec-
troporation processing device, showing the new design;
FIG. 2 is a rear, bottom, left perspective thereof;
FIG. 3 is a left view thereof;
FIG. 4 is a rear view thereof;
FIG. 5 is a front view thereof;
FIG. 6 is a top view thereof; and,
FIG. 7 is a bottom view thereof.

The broken lines of equal-length depict portions of the
electroporation processing device that form no part of the
claimed design.

1 Claim, 7 Drawing Sheets

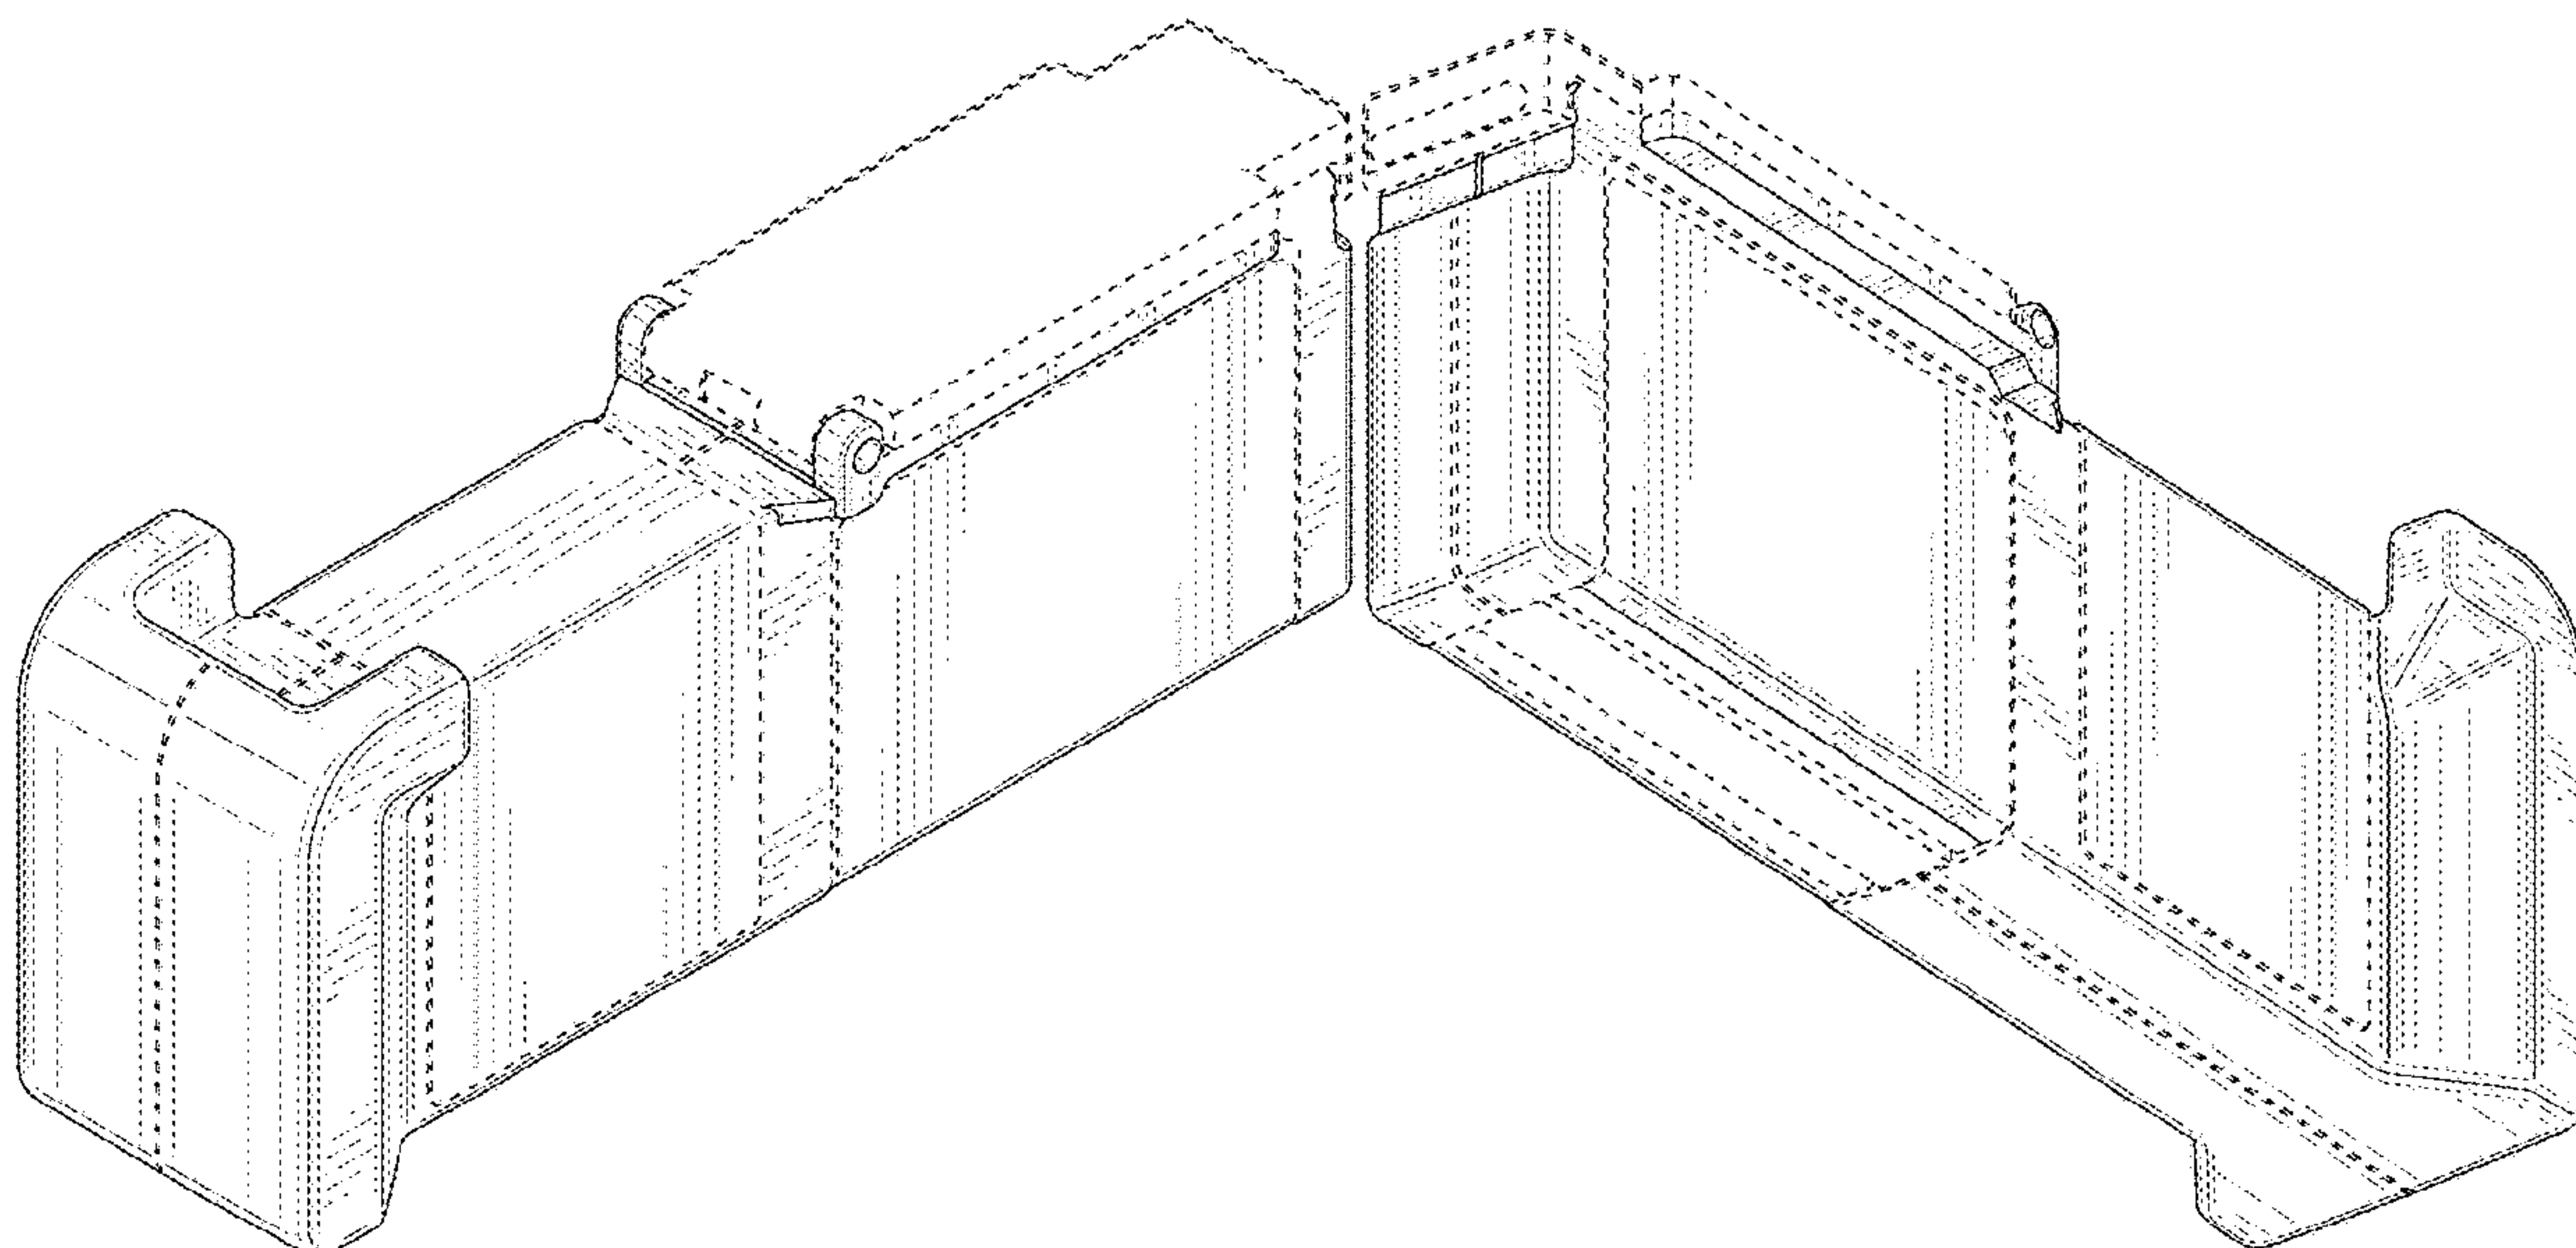

(56)

References Cited

U.S. PATENT DOCUMENTS

D714,459 S * 9/2014 Develon D24/216
D717,438 S 11/2014 Lin et al.
D718,473 S 11/2014 Benarieh et al.
D843,006 S * 3/2019 Huang D24/216
D857,913 S * 8/2019 LiCalzi D24/216
D858,790 S * 9/2019 Hsu D24/216
D922,600 S * 6/2021 Upsdell D24/216
D923,200 S 6/2021 Luther et al.
D931,493 S 9/2021 Darbyshire et al.
D943,760 S * 2/2022 Luther D24/216
D944,410 S * 2/2022 Luther D24/216
D960,385 S * 8/2022 Schubert D24/186
2003/0180939 A1 * 9/2003 Kaste C12M 35/02
435/809
2004/0197883 A1 10/2004 Dzekunov et al.
2006/0245970 A1 11/2006 Lee
2007/0128708 A1 * 6/2007 Gamelin C12M 41/44
435/173.6
2020/0290037 A1 9/2020 Salomon et al.

2021/0106987 A1 4/2021 Lind et al.
2021/0123009 A1 4/2021 Yeo et al.
2021/0348109 A1 * 11/2021 Modica C12M 35/02

OTHER PUBLICATIONS

“BTX Online: AgilePulse Max Large Volume Transfectin System.” Found online Apr. 12, 2024 at [btxonline.com](https://www.btxonline.com). Reference dated <https://www.btxonline.com/agilepulse-max-large-volume-transfection-system.html>.
“BTX Online: ECM 630 Exponential Decay Wave Electroporation System.” Found online Apr. 12, 2024 at [btxonline.com](https://www.btxonline.com). Reference dated Mar. 17, 2017. Retrieved from <https://www.btxonline.com/ecm-630-exponential-decay-wave-electroporation-system.html>.
“Science Direct: Tolerability of Two Sequential Electroporation Treatments Using MedPulser DNA Deliver System in Healthy Adults.” Found online Apr. 12, 2024 at [sciencedirect.com](https://www.sciencedirect.com). Reference dated May 2009. Retrieved from <https://www.sciencedirect.com/science/article/pii/S1525001616317932>.

* cited by examiner

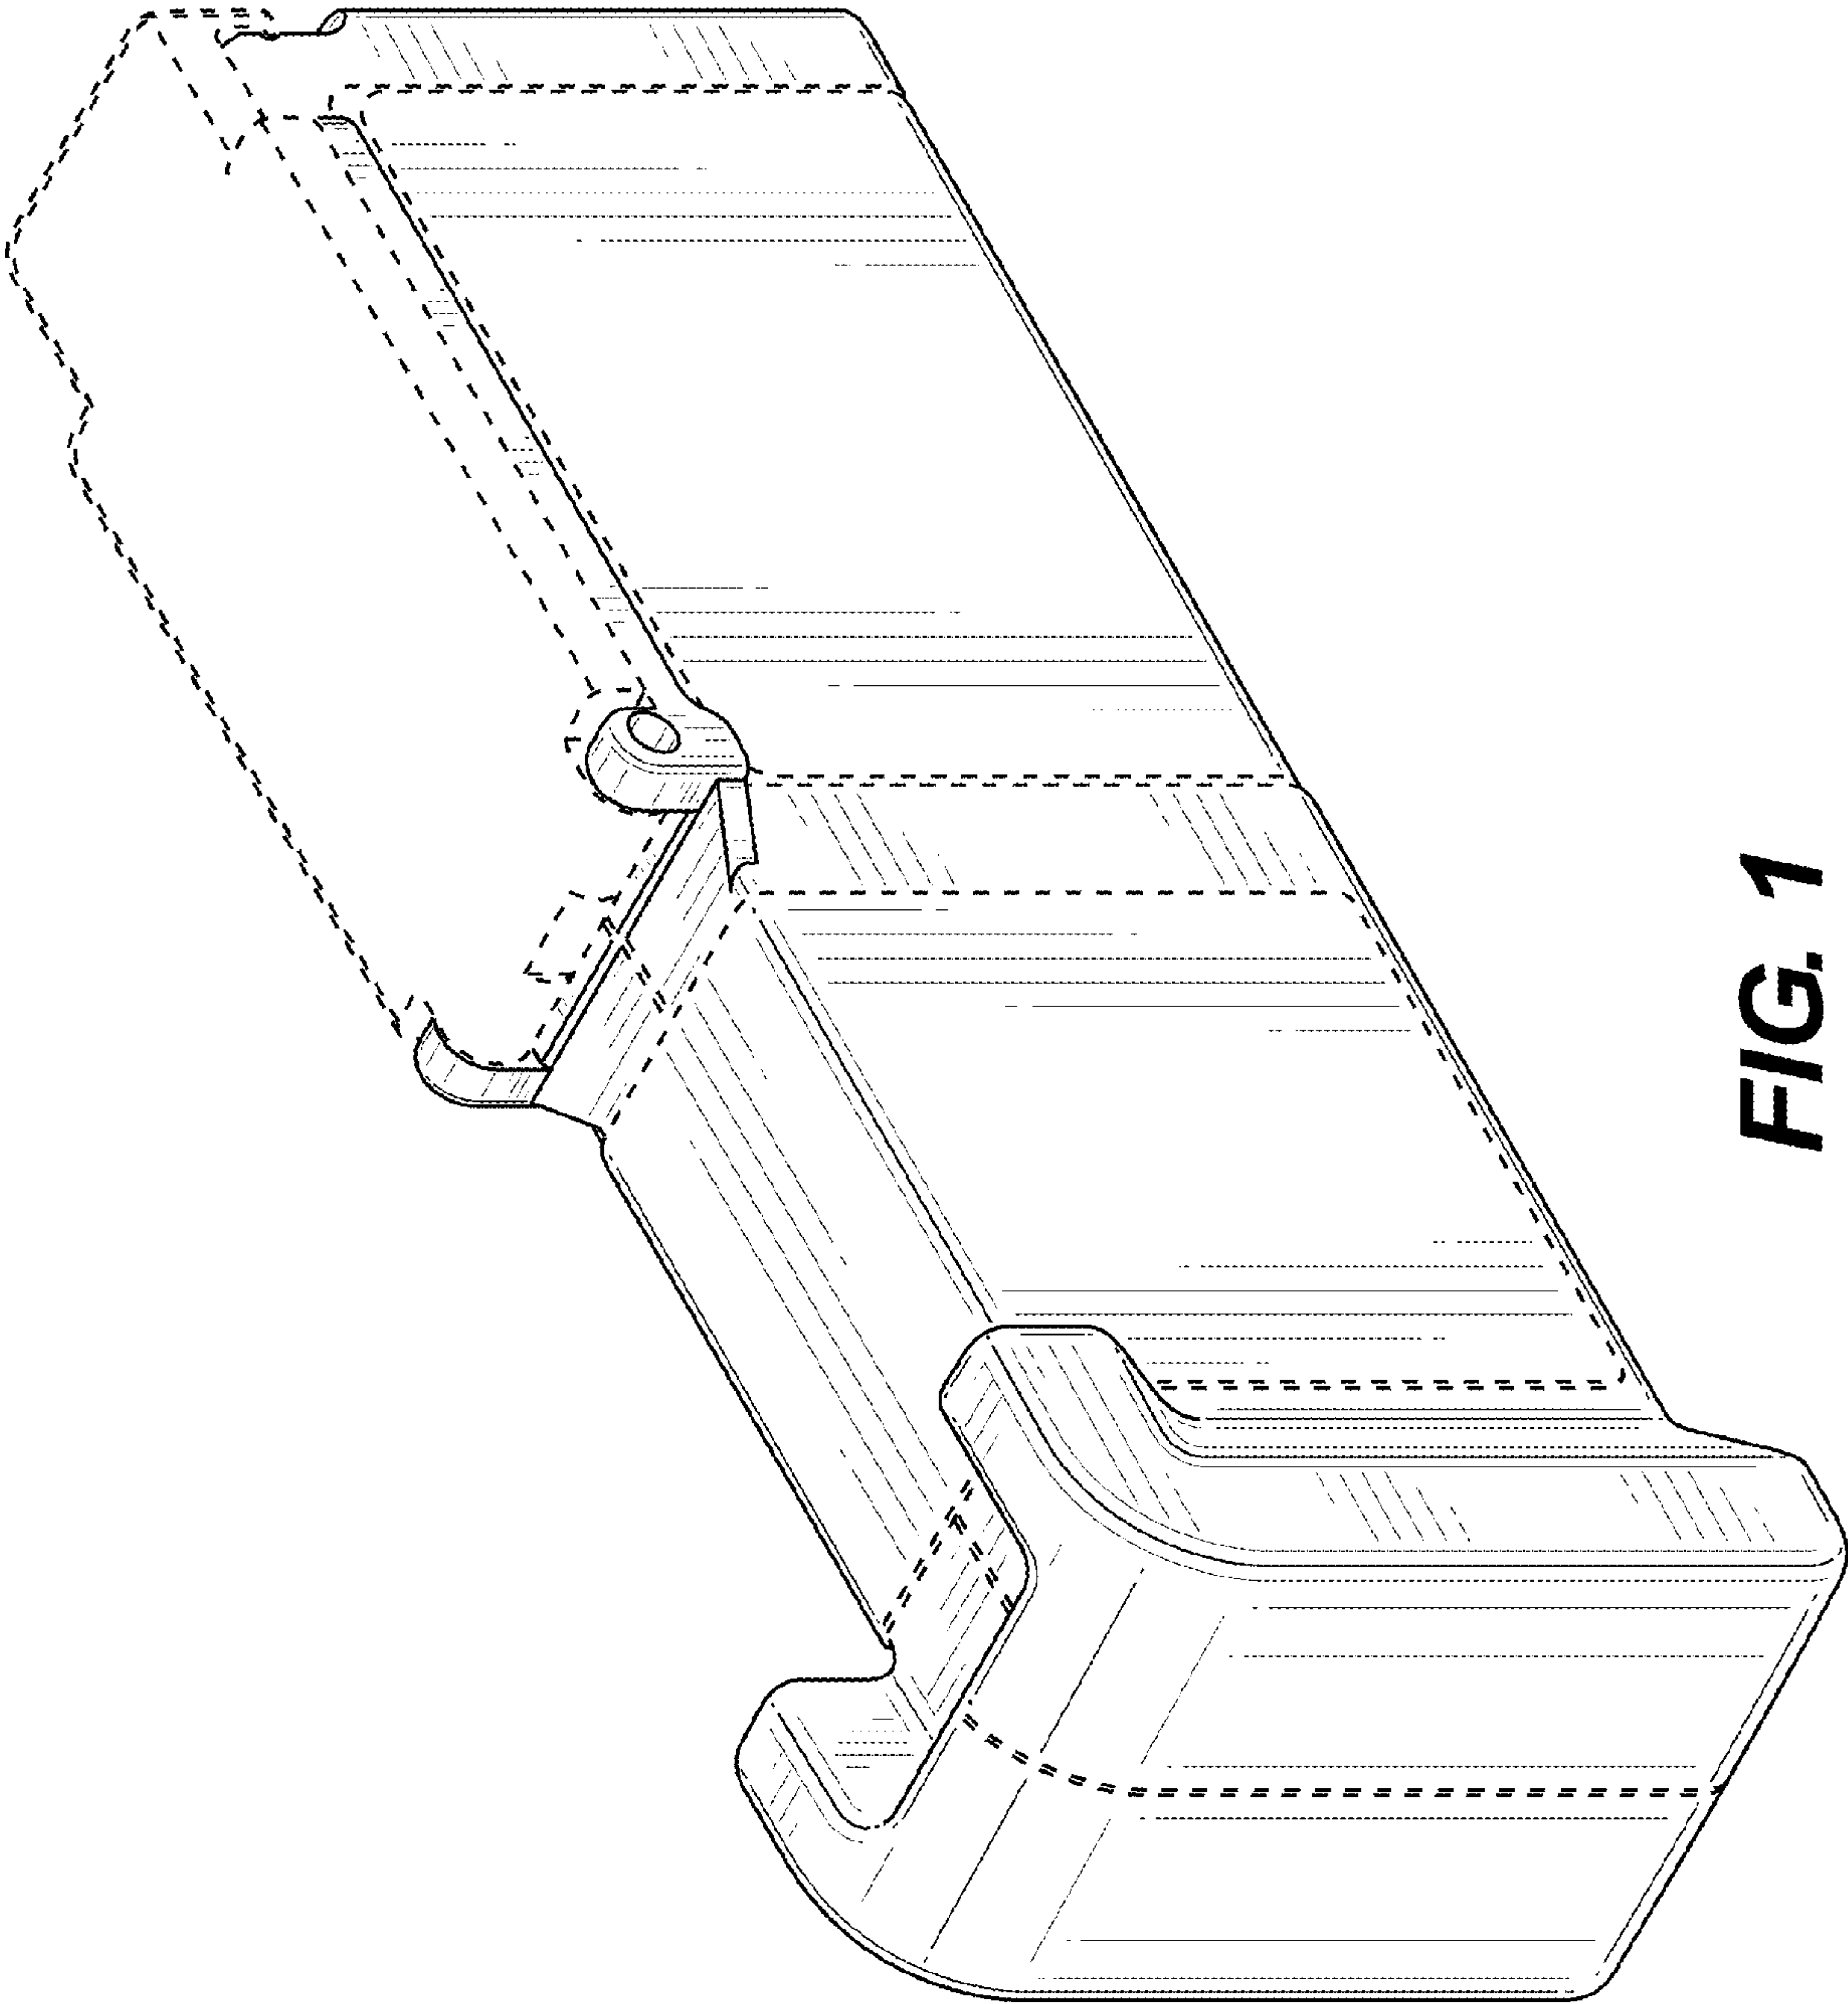


FIG. 1

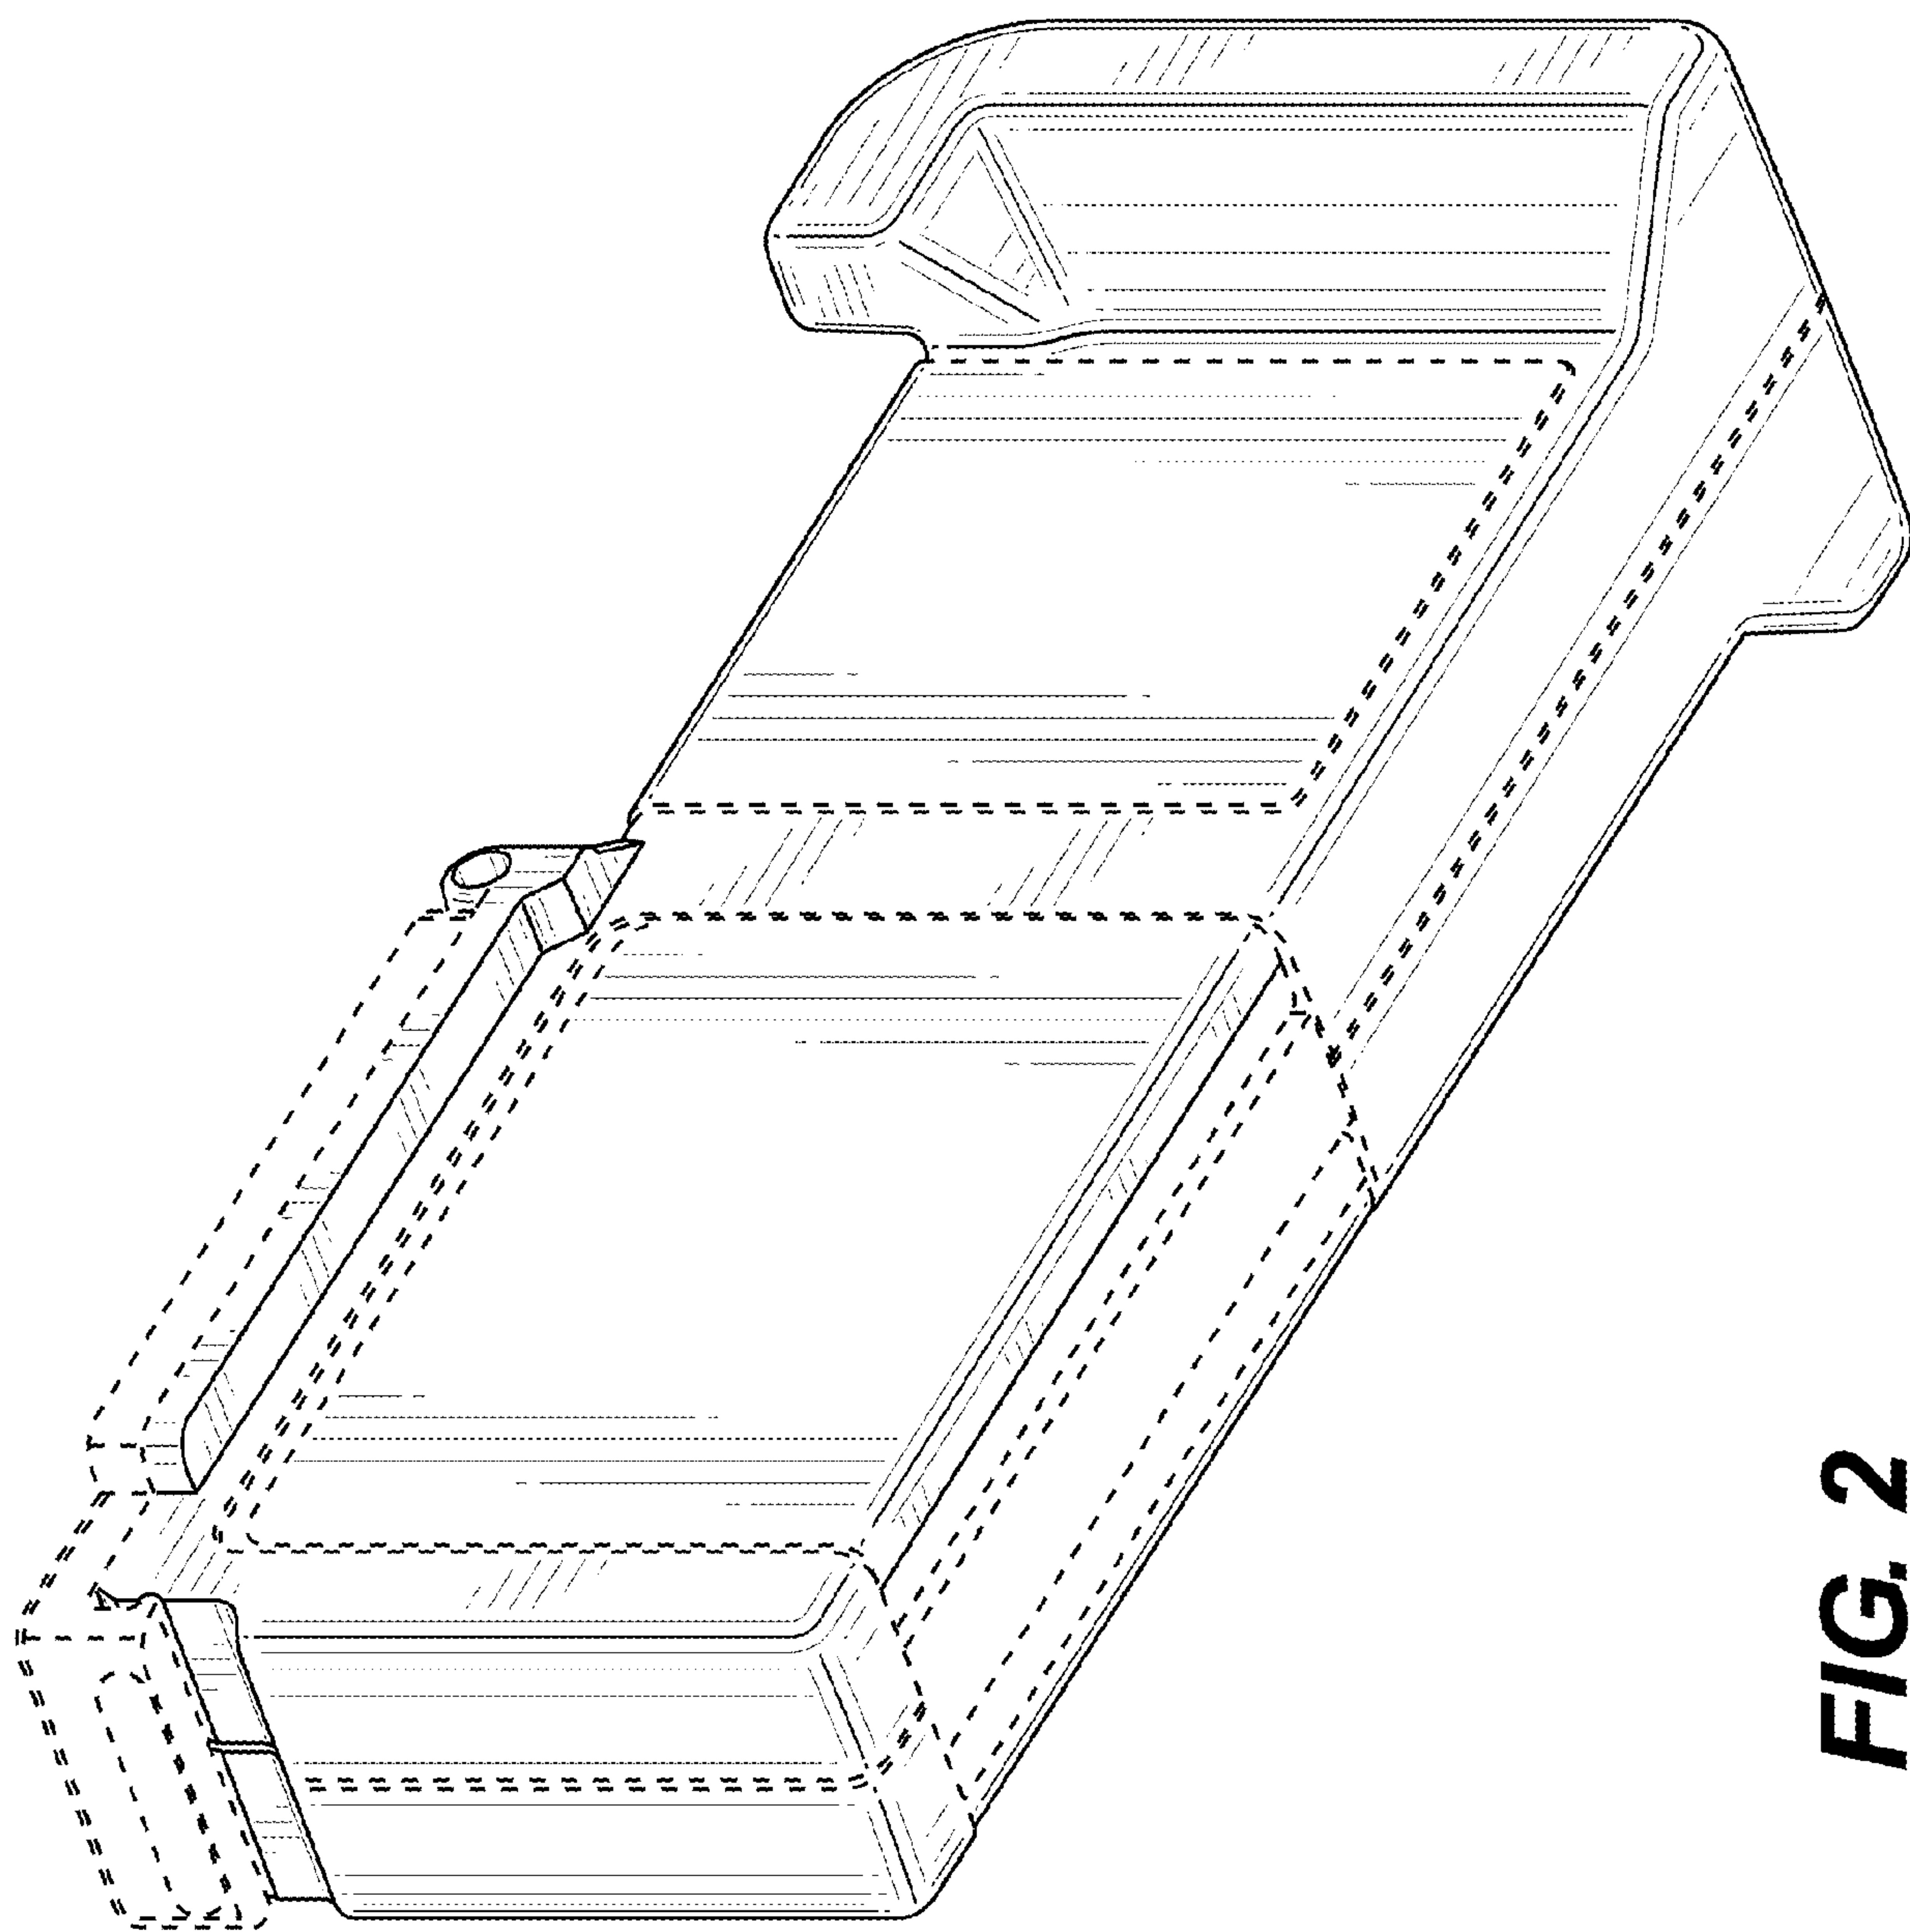


FIG. 2

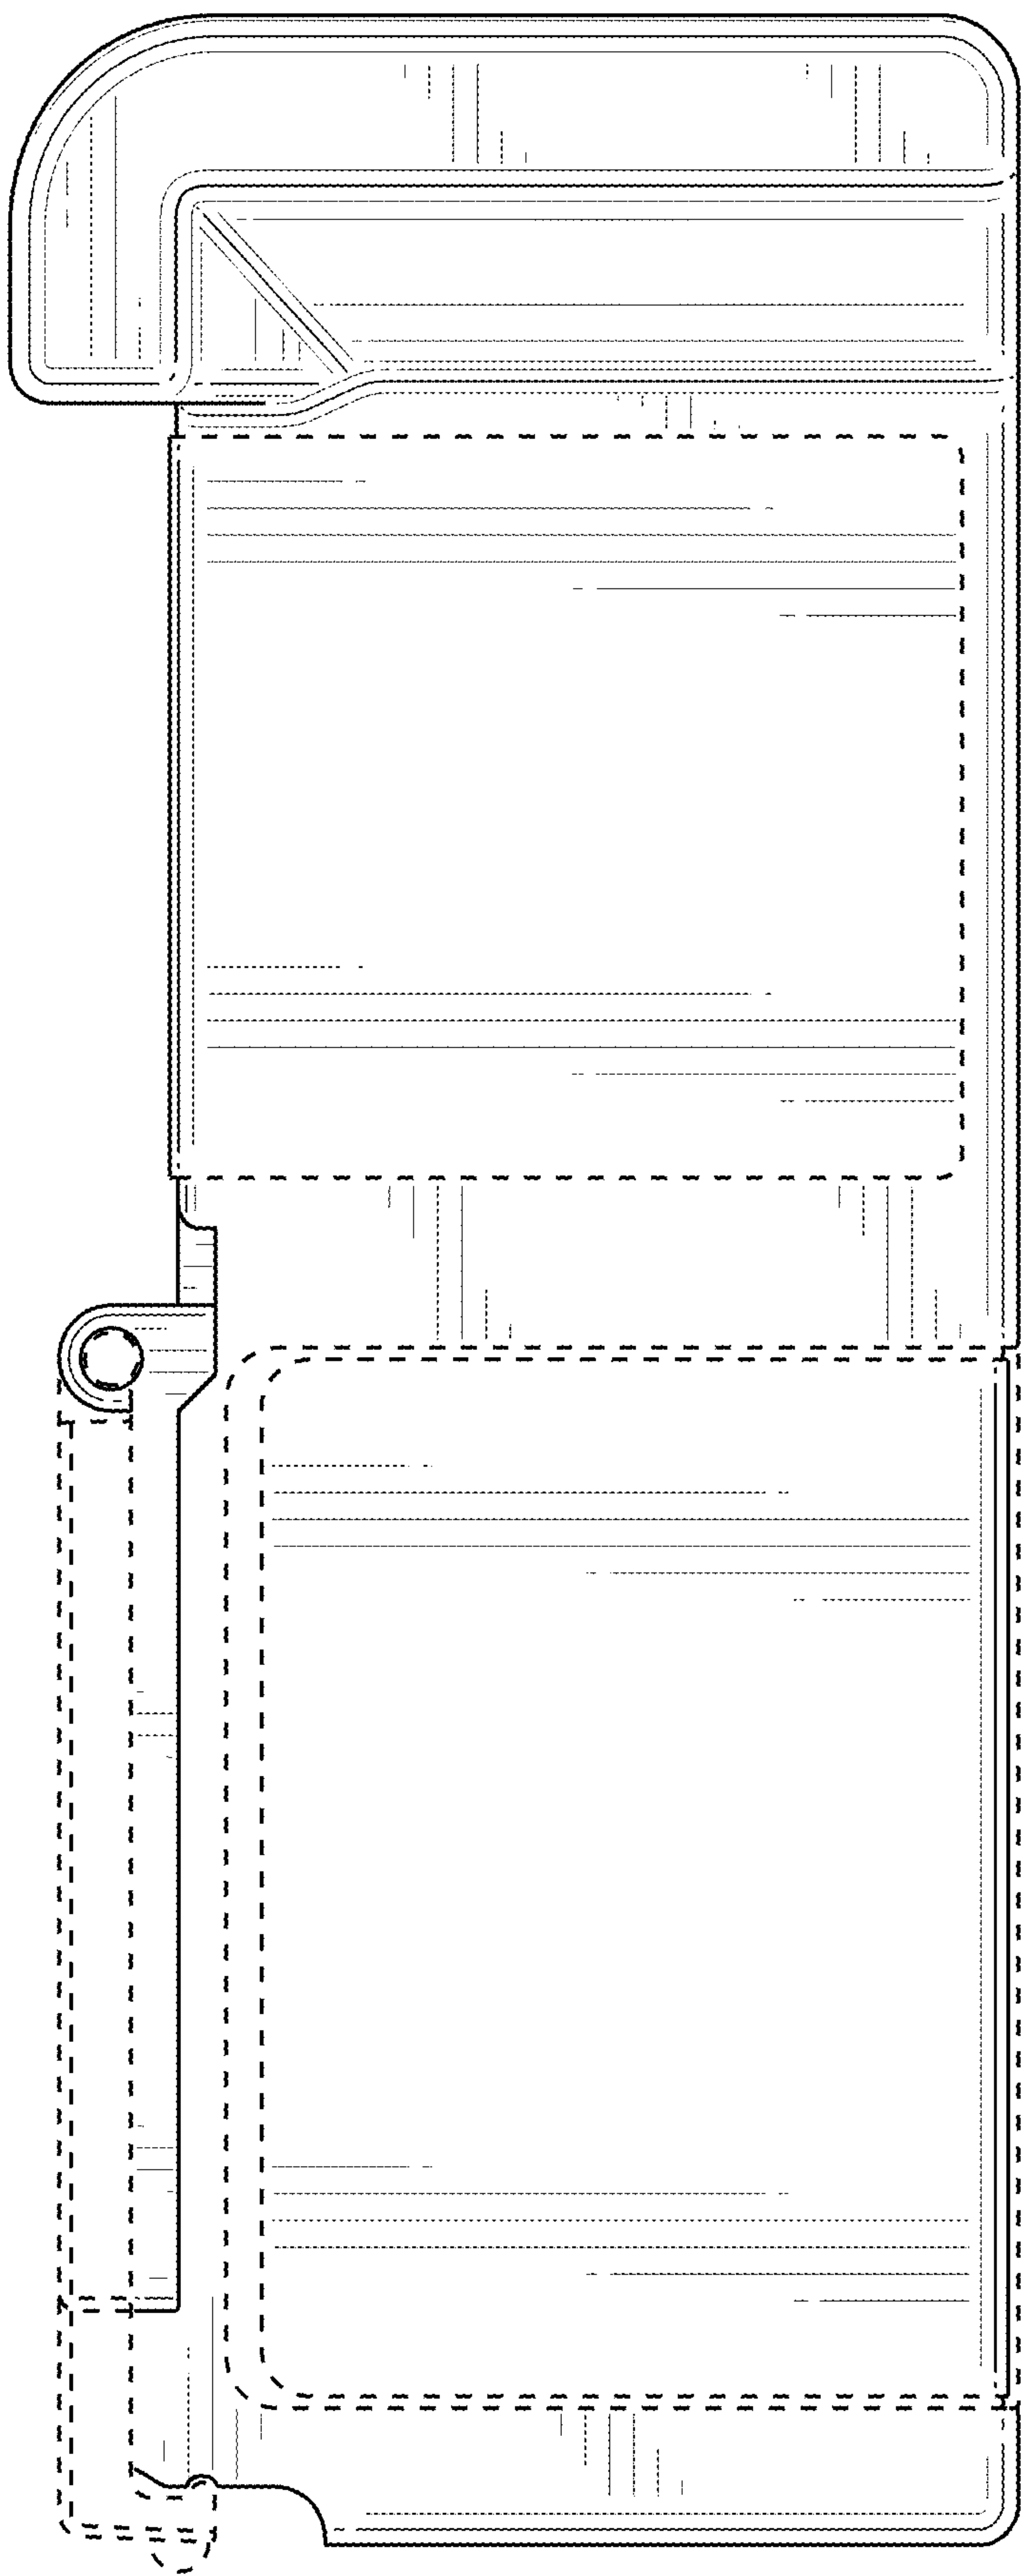


FIG. 3

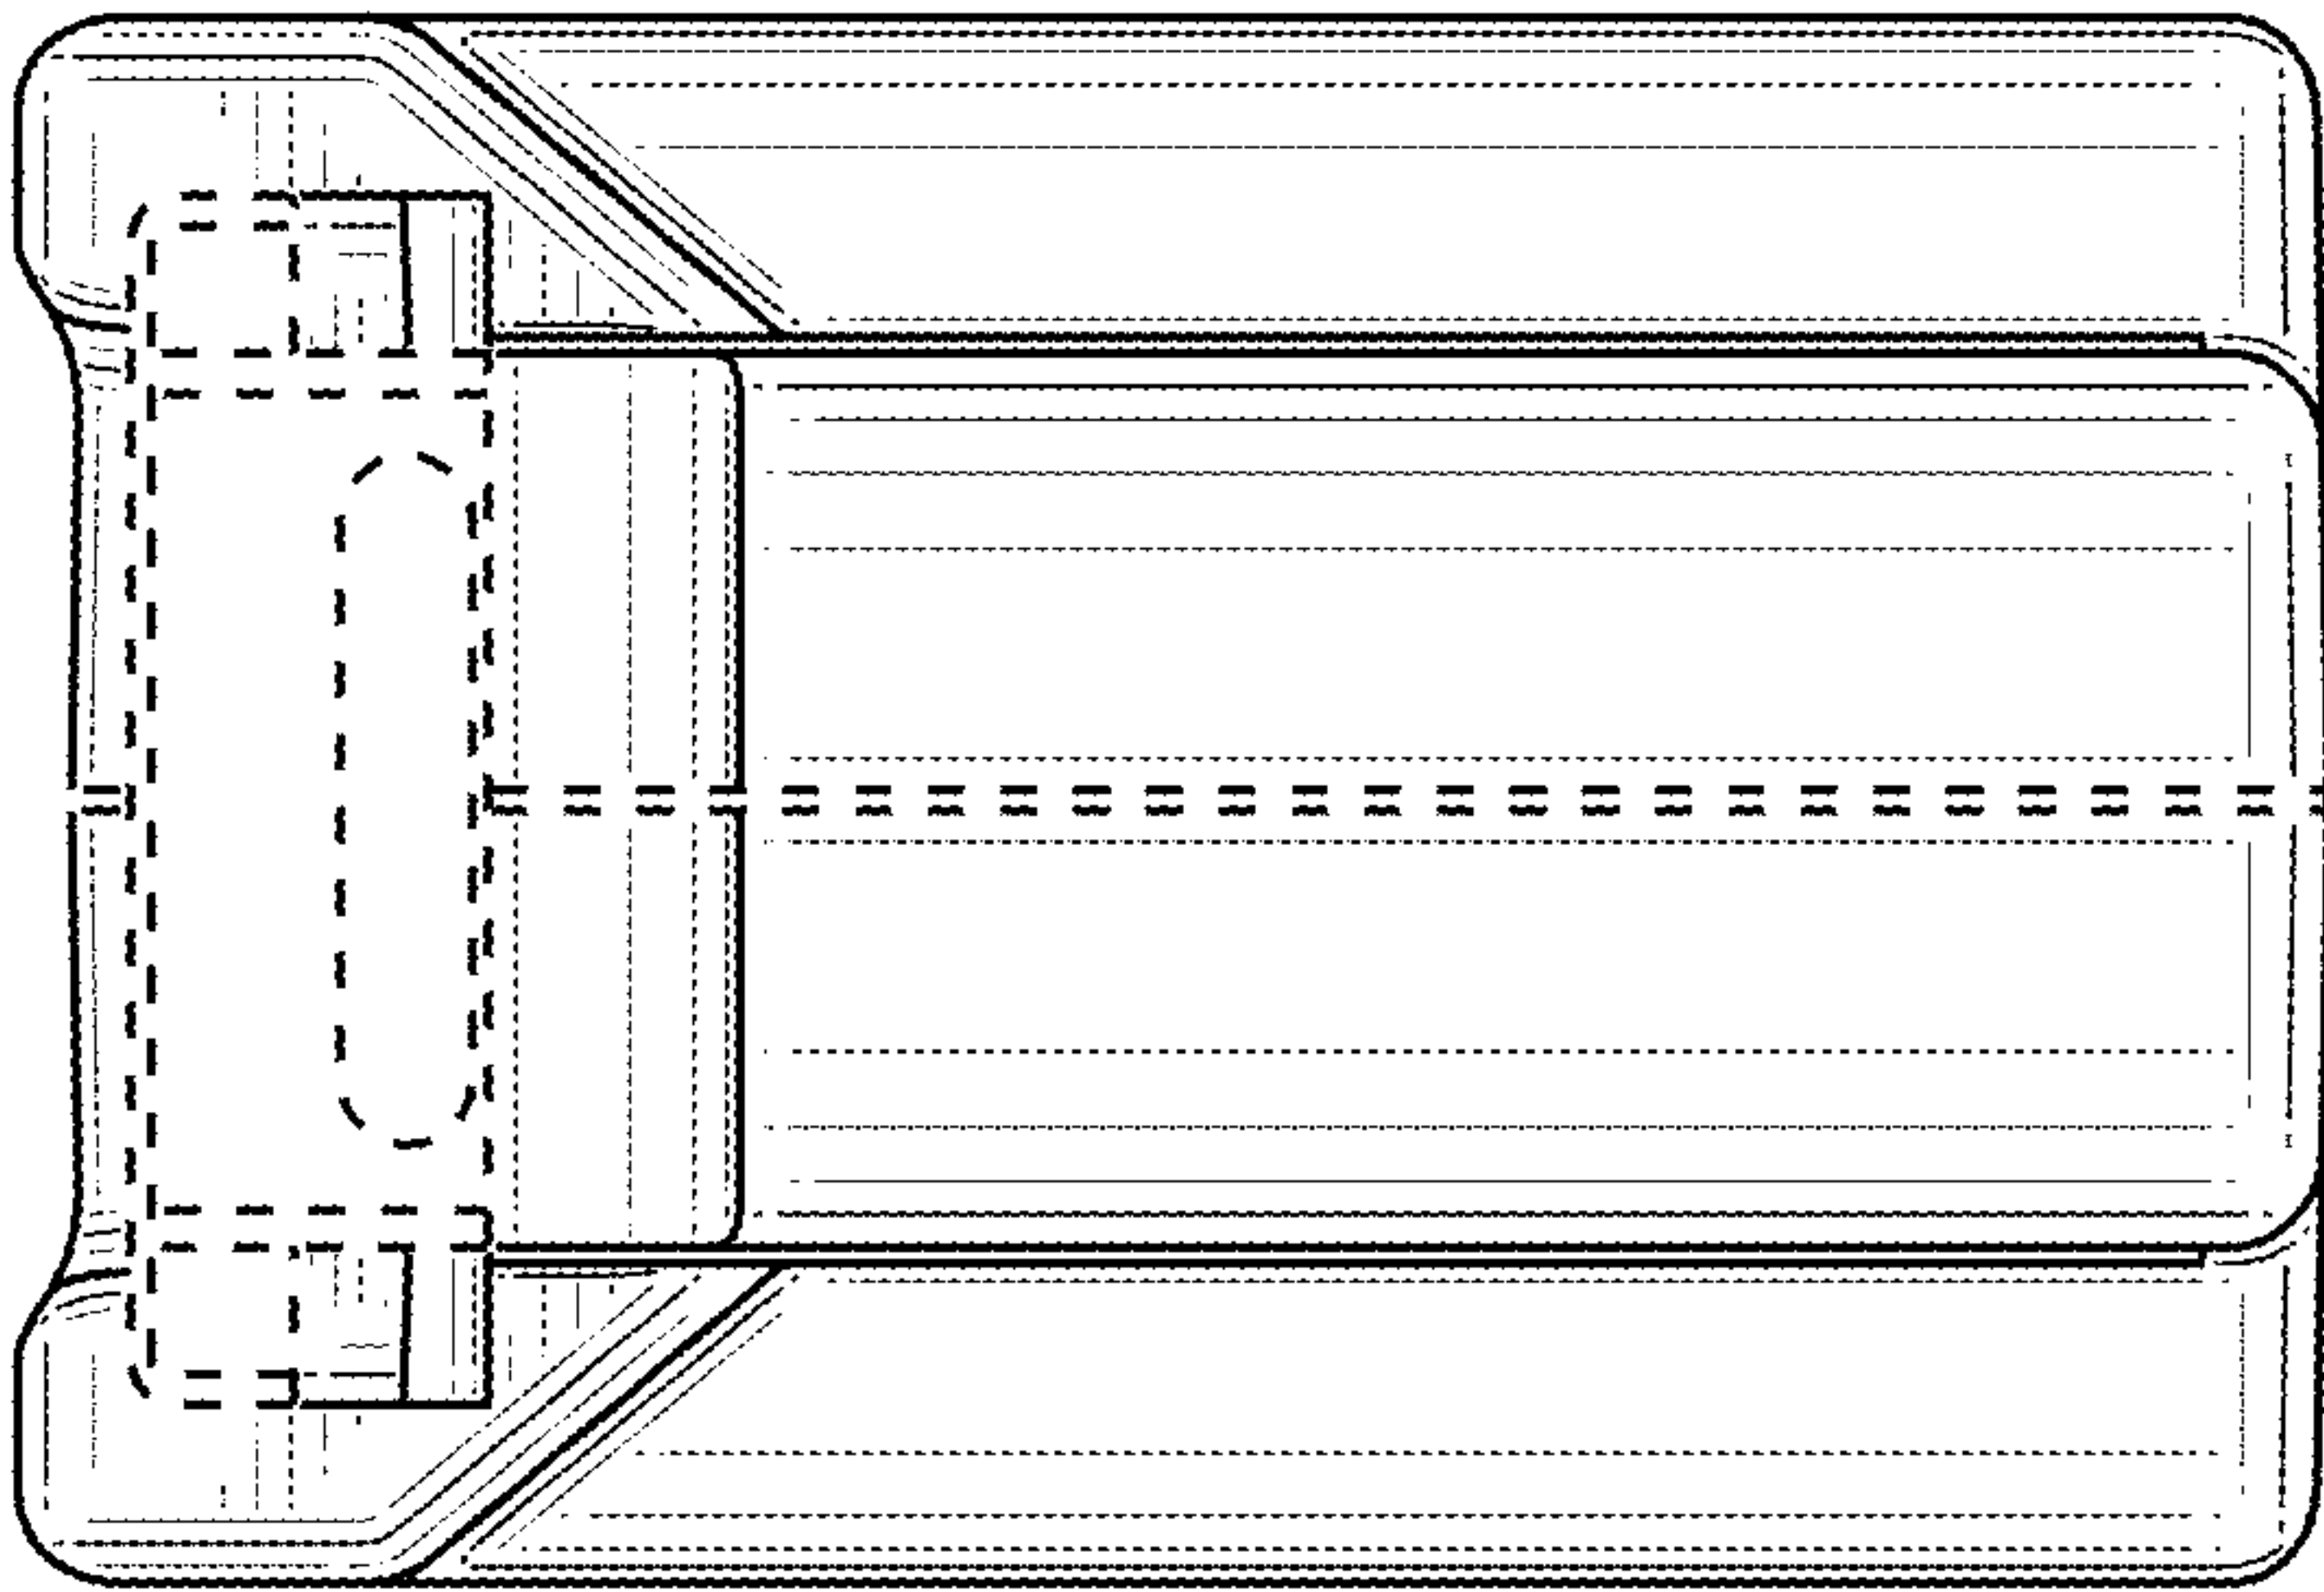


FIG. 4

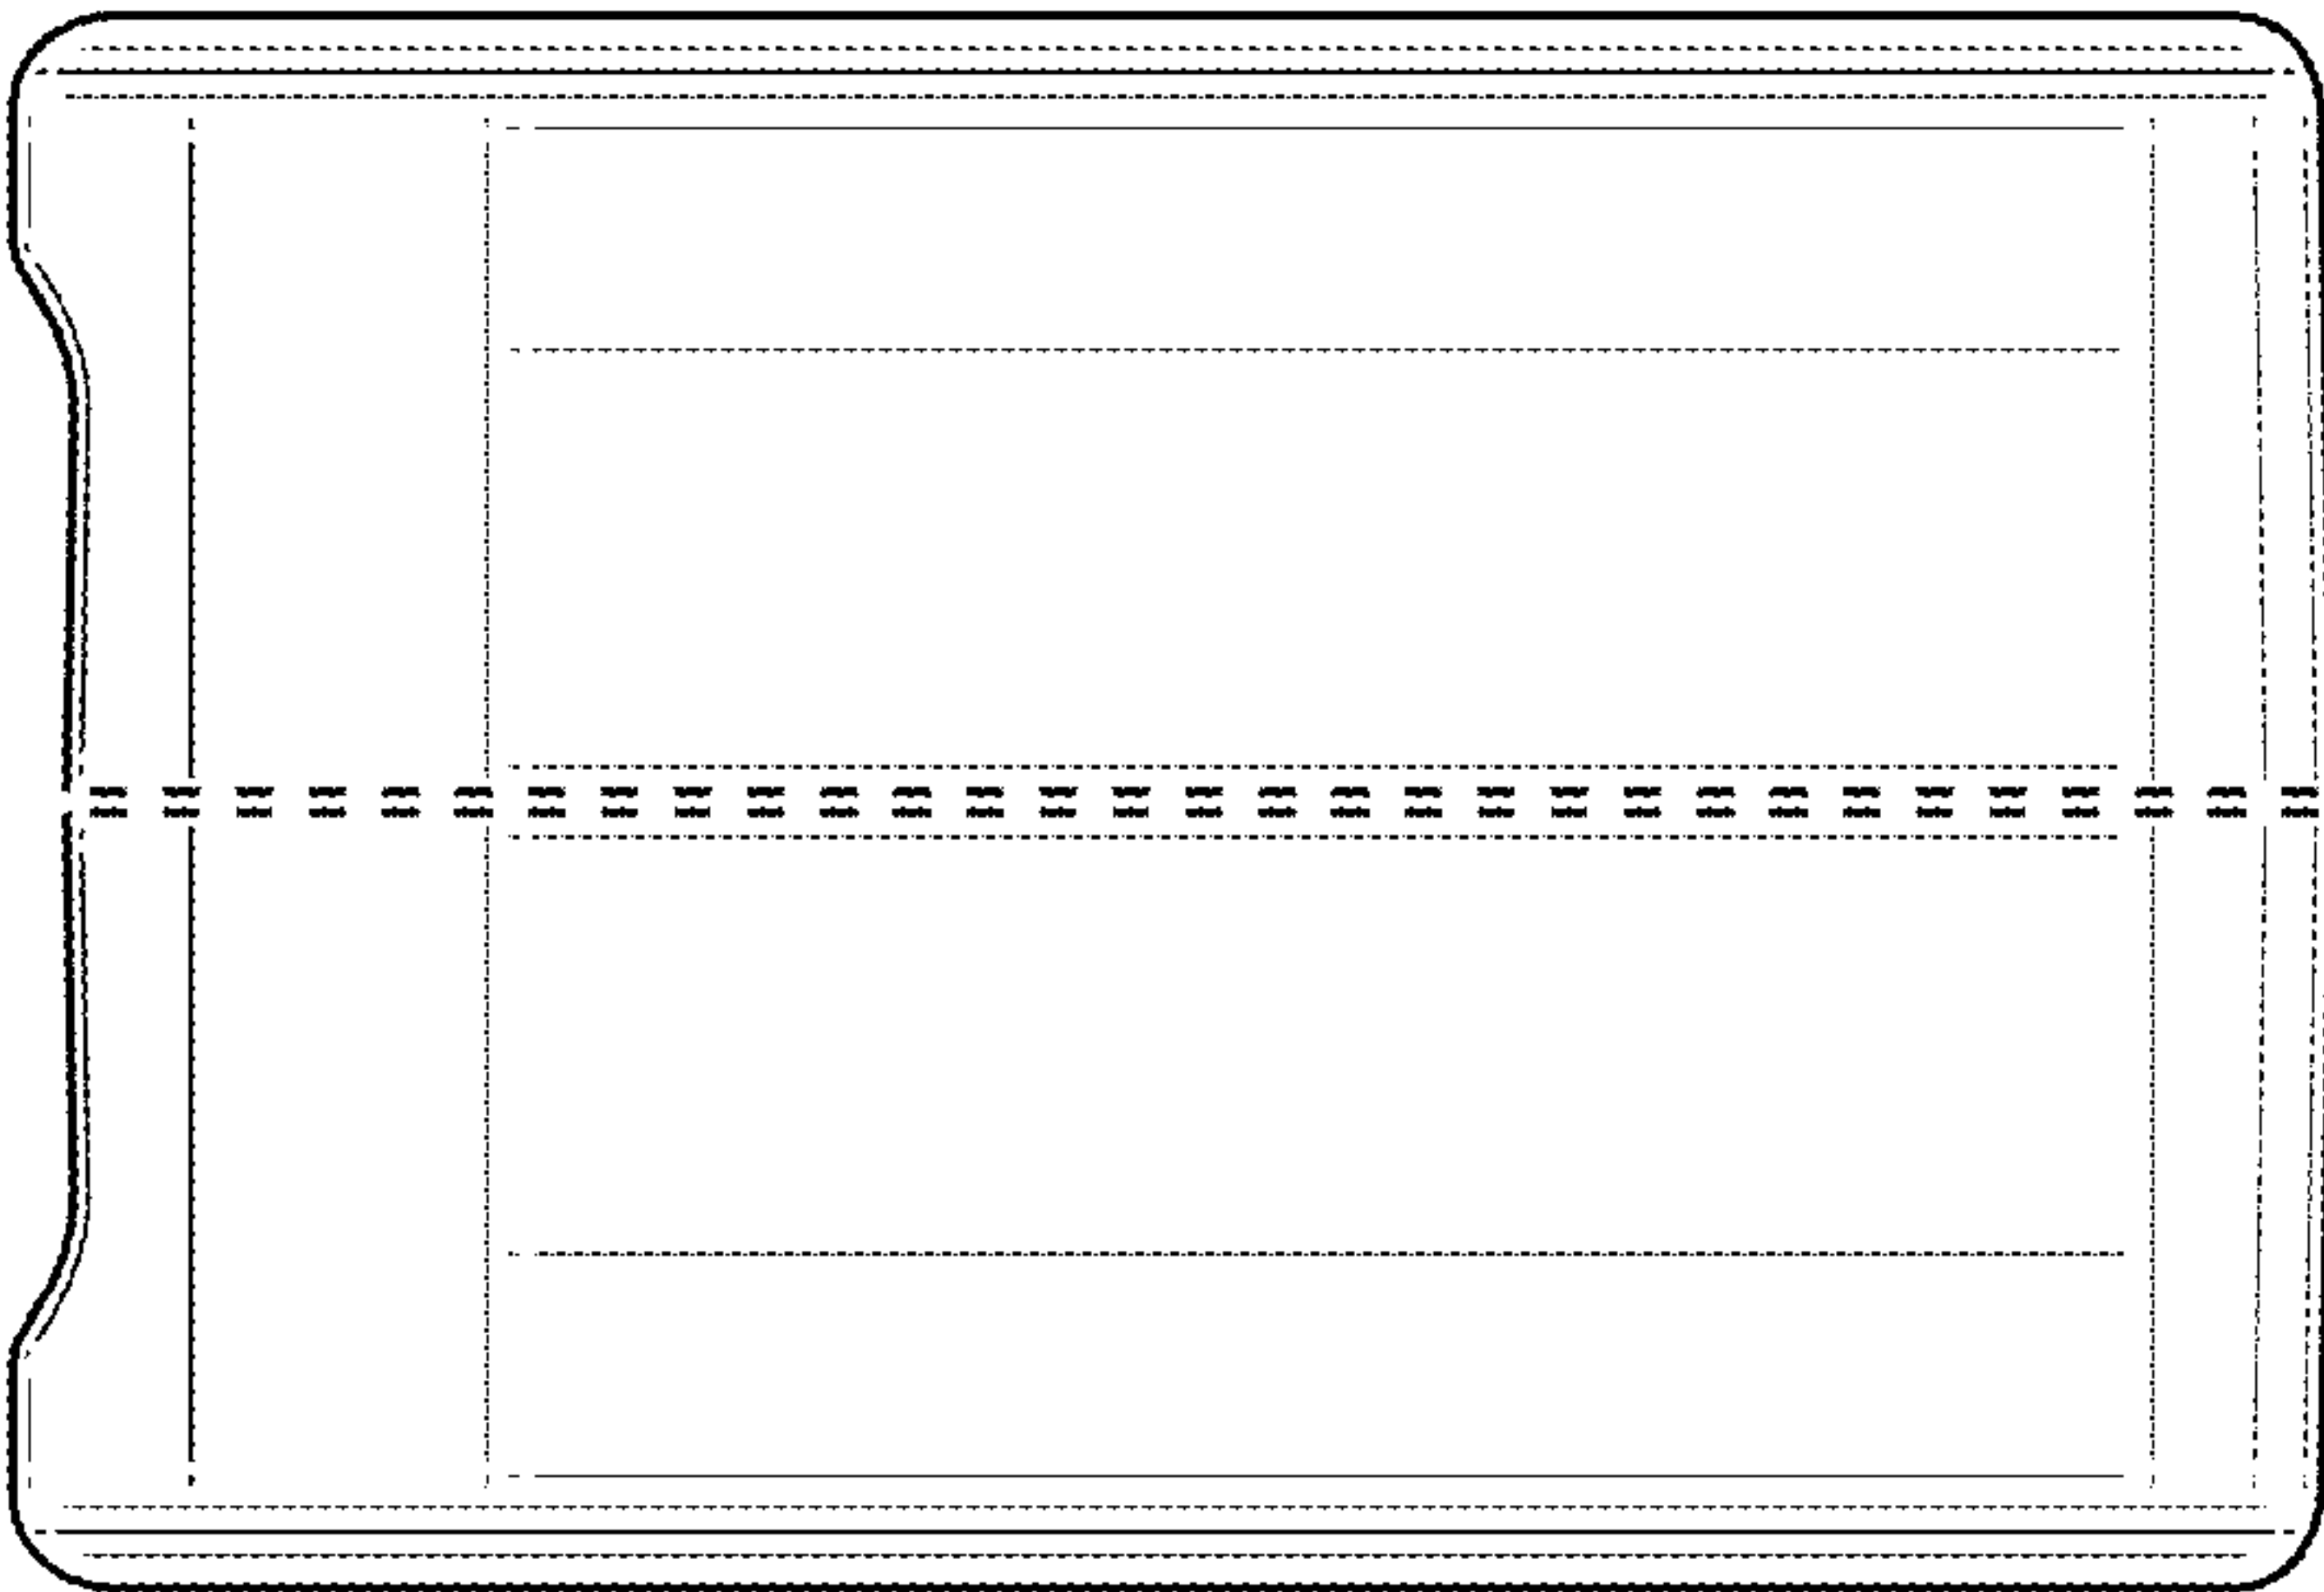


FIG. 5

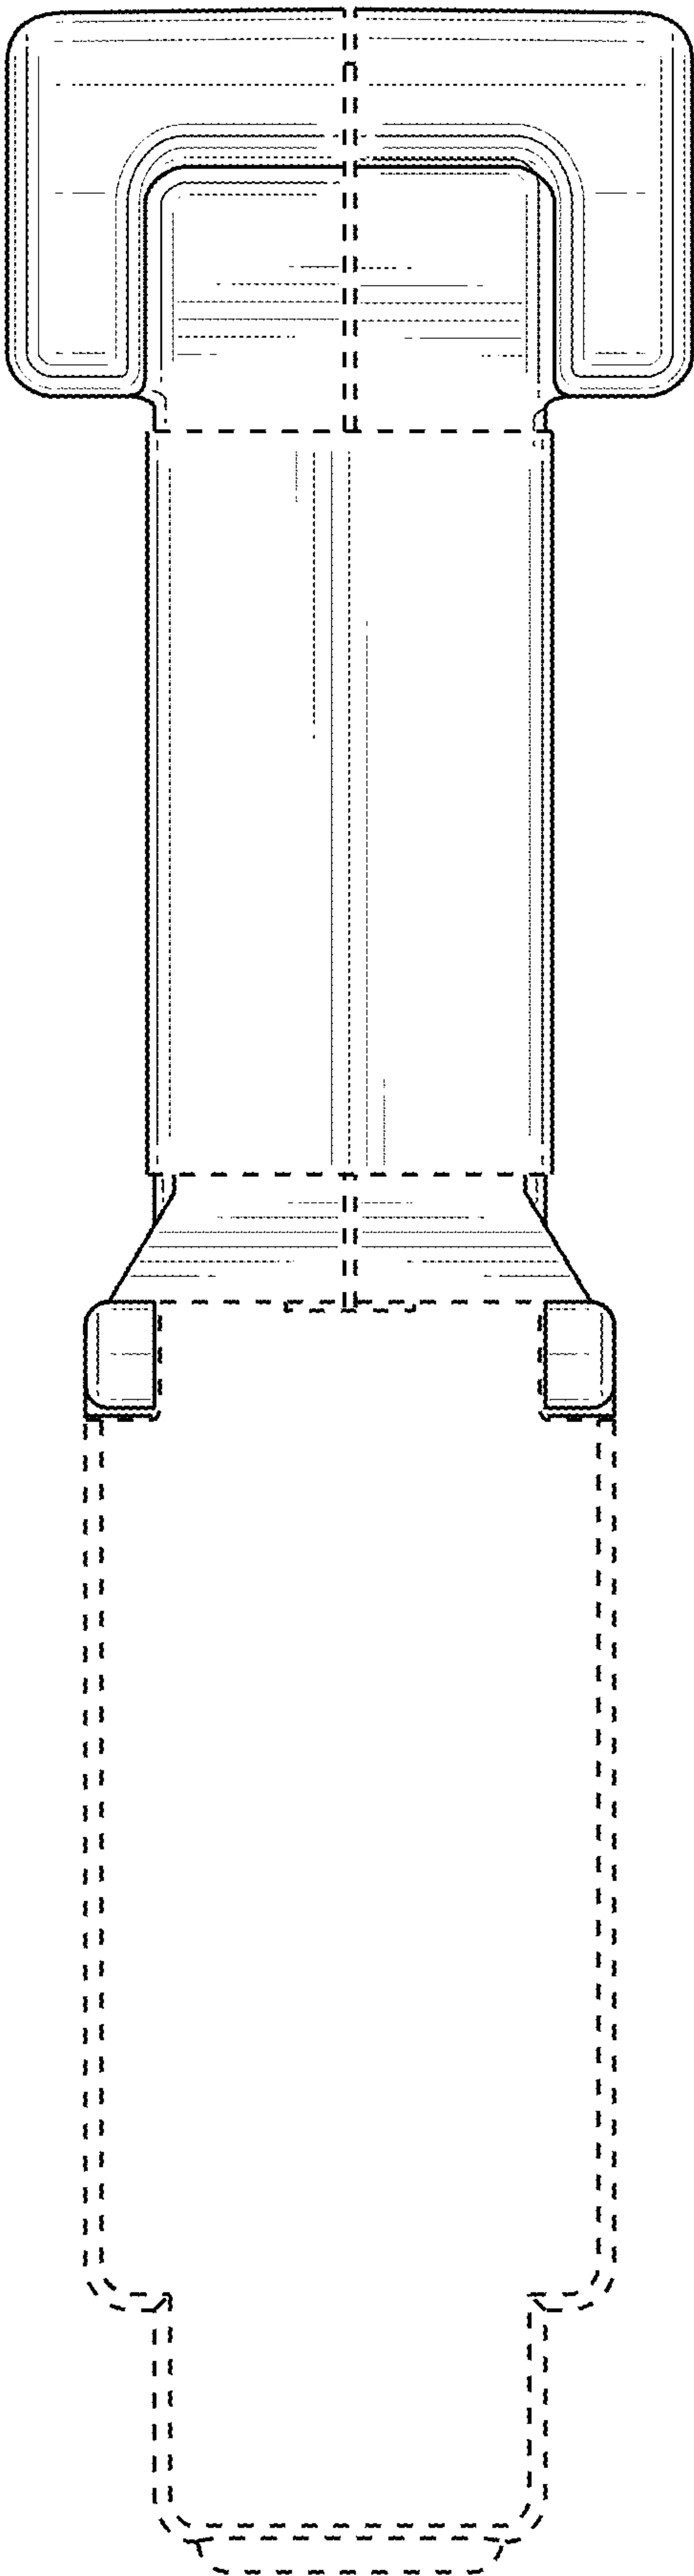


FIG. 6

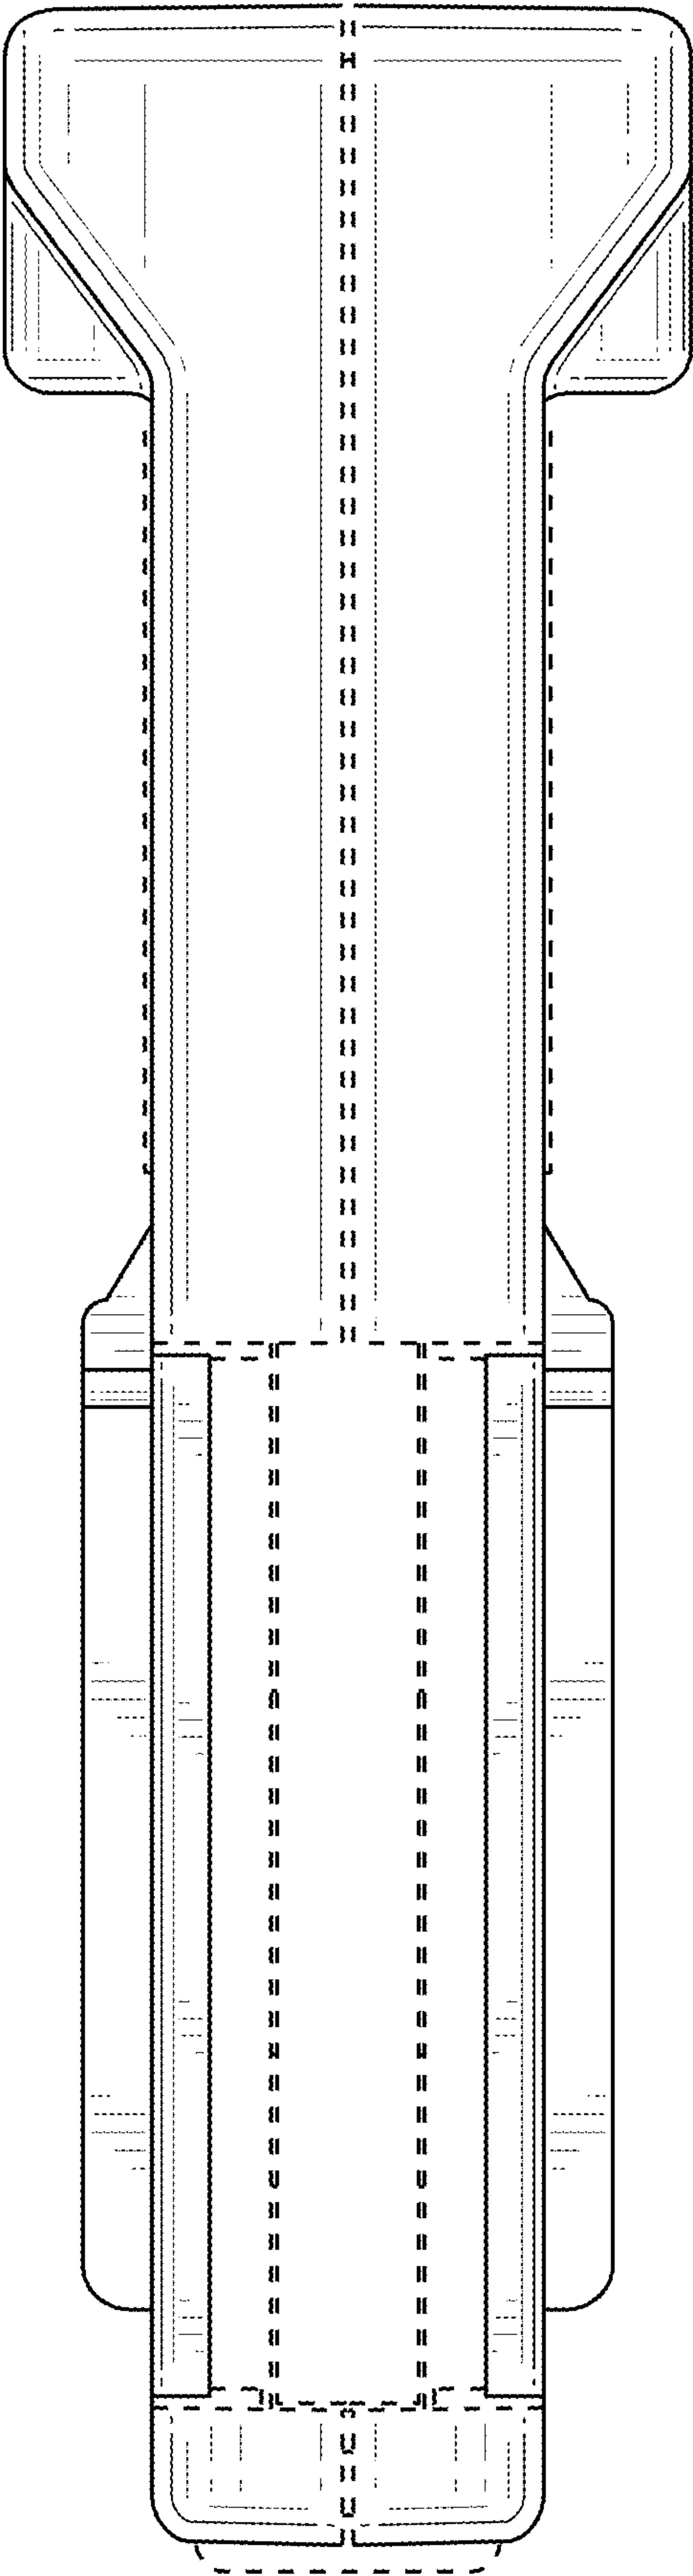


FIG. 7