



US0D1058848S

(12)

United States Design Patent

Boggess et al.

(10)

Patent No.:

US D1,058,848 S

(45)

Date of Patent:

** Jan. 21, 2025

(54) STERILIZATION CART

(71) Applicant: **STERIS Corporation**, Mentor, OH (US)

(72) Inventors: **Joshua Boggess**, Chardon, OH (US);
Dale J. Kitchen, Chardon, OH (US);
Nathan Pohl, Wickliffe, OH (US);
Michael St. Onge, Erie, PA (US);
Michael A. Varcho, Mentor, OH (US);
Joseph R. Regimbald, Chicago, IL (US)

(73) Assignee: **STERIS Corporation**, Mentor, OH (US)

(**) Term: **15 Years**

(21) Appl. No.: **29/911,791**

(22) Filed: **Sep. 8, 2023**

(51) **LOC (15) Cl.** **24-01**

(52) **U.S. Cl.**
USPC **D24/217**

(58) **Field of Classification Search**
USPC D24/118, 121, 207, 216, 217, 218, 219,
D24/220, 224, 232; D3/303, 294;
D9/420, 423

(Continued)

(56) **References Cited**

U.S. PATENT DOCUMENTS

D108,508 S * 2/1938 Finn D24/217
D117,720 S * 11/1939 Newman D24/217
(Continued)

OTHER PUBLICATIONS

AMSCO Surgical Case Cart, [site visited Nov. 12, 2024]. Available from Internet. URL: <https://www.steris.com/healthcare/products/sterile-processing-department-accessories/surgical-instrument-case-carts> (Year: 2024).*

Primary Examiner — T Chase Nelson
Assistant Examiner — Kelly L Gross
(74) Attorney, Agent, or Firm — Schwegman Lundberg & Woessner, P.A.

(57) **CLAIM**
The ornamental design for a sterilization cart, as shown and described.

DESCRIPTION

FIG. 1 is a top, front, left perspective view of a first embodiment of a sterilization cart (such as a mobile or movable cart for sterilizing medical or other equipment), showing our new design;
FIG. 2 is a top, front, right perspective view thereof;
FIG. 3 is a top, rear, right perspective view thereof;
FIG. 4 is a top, rear, left perspective view thereof;
FIG. 5 is a bottom, front, left perspective view thereof;
FIG. 6 is a bottom, front, right perspective view thereof;
FIG. 7 is a bottom, rear, right perspective view thereof;
FIG. 8 is a bottom, rear, left perspective view thereof;
FIG. 9 is a front view thereof;
FIG. 10 is a rear view thereof;
FIG. 11 is a right side view thereof;
FIG. 12 is a left side view thereof;
FIG. 13 is a top view thereof; and,
FIG. 14 is a bottom view thereof.
FIG. 15 is a top, front, left perspective view of a second embodiment of a sterilization cart (such as a mobile or movable cart for sterilizing medical or other equipment), showing our new design;
FIG. 16 is a top, front, right perspective view thereof;
FIG. 17 is a top, rear, right perspective view thereof;
FIG. 18 is a top, rear, left perspective view thereof;
FIG. 19 is a bottom, front, left perspective view thereof;
FIG. 20 is a bottom, front, right perspective view thereof;
FIG. 21 is a bottom, rear, right perspective view thereof;
FIG. 22 is a bottom, rear, left perspective view thereof;
FIG. 23 is a front view thereof;
FIG. 24 is a rear view thereof;
FIG. 25 is a right side view thereof;
FIG. 26 is a left side view thereof;
FIG. 27 is a top view thereof: and,
(Continued)

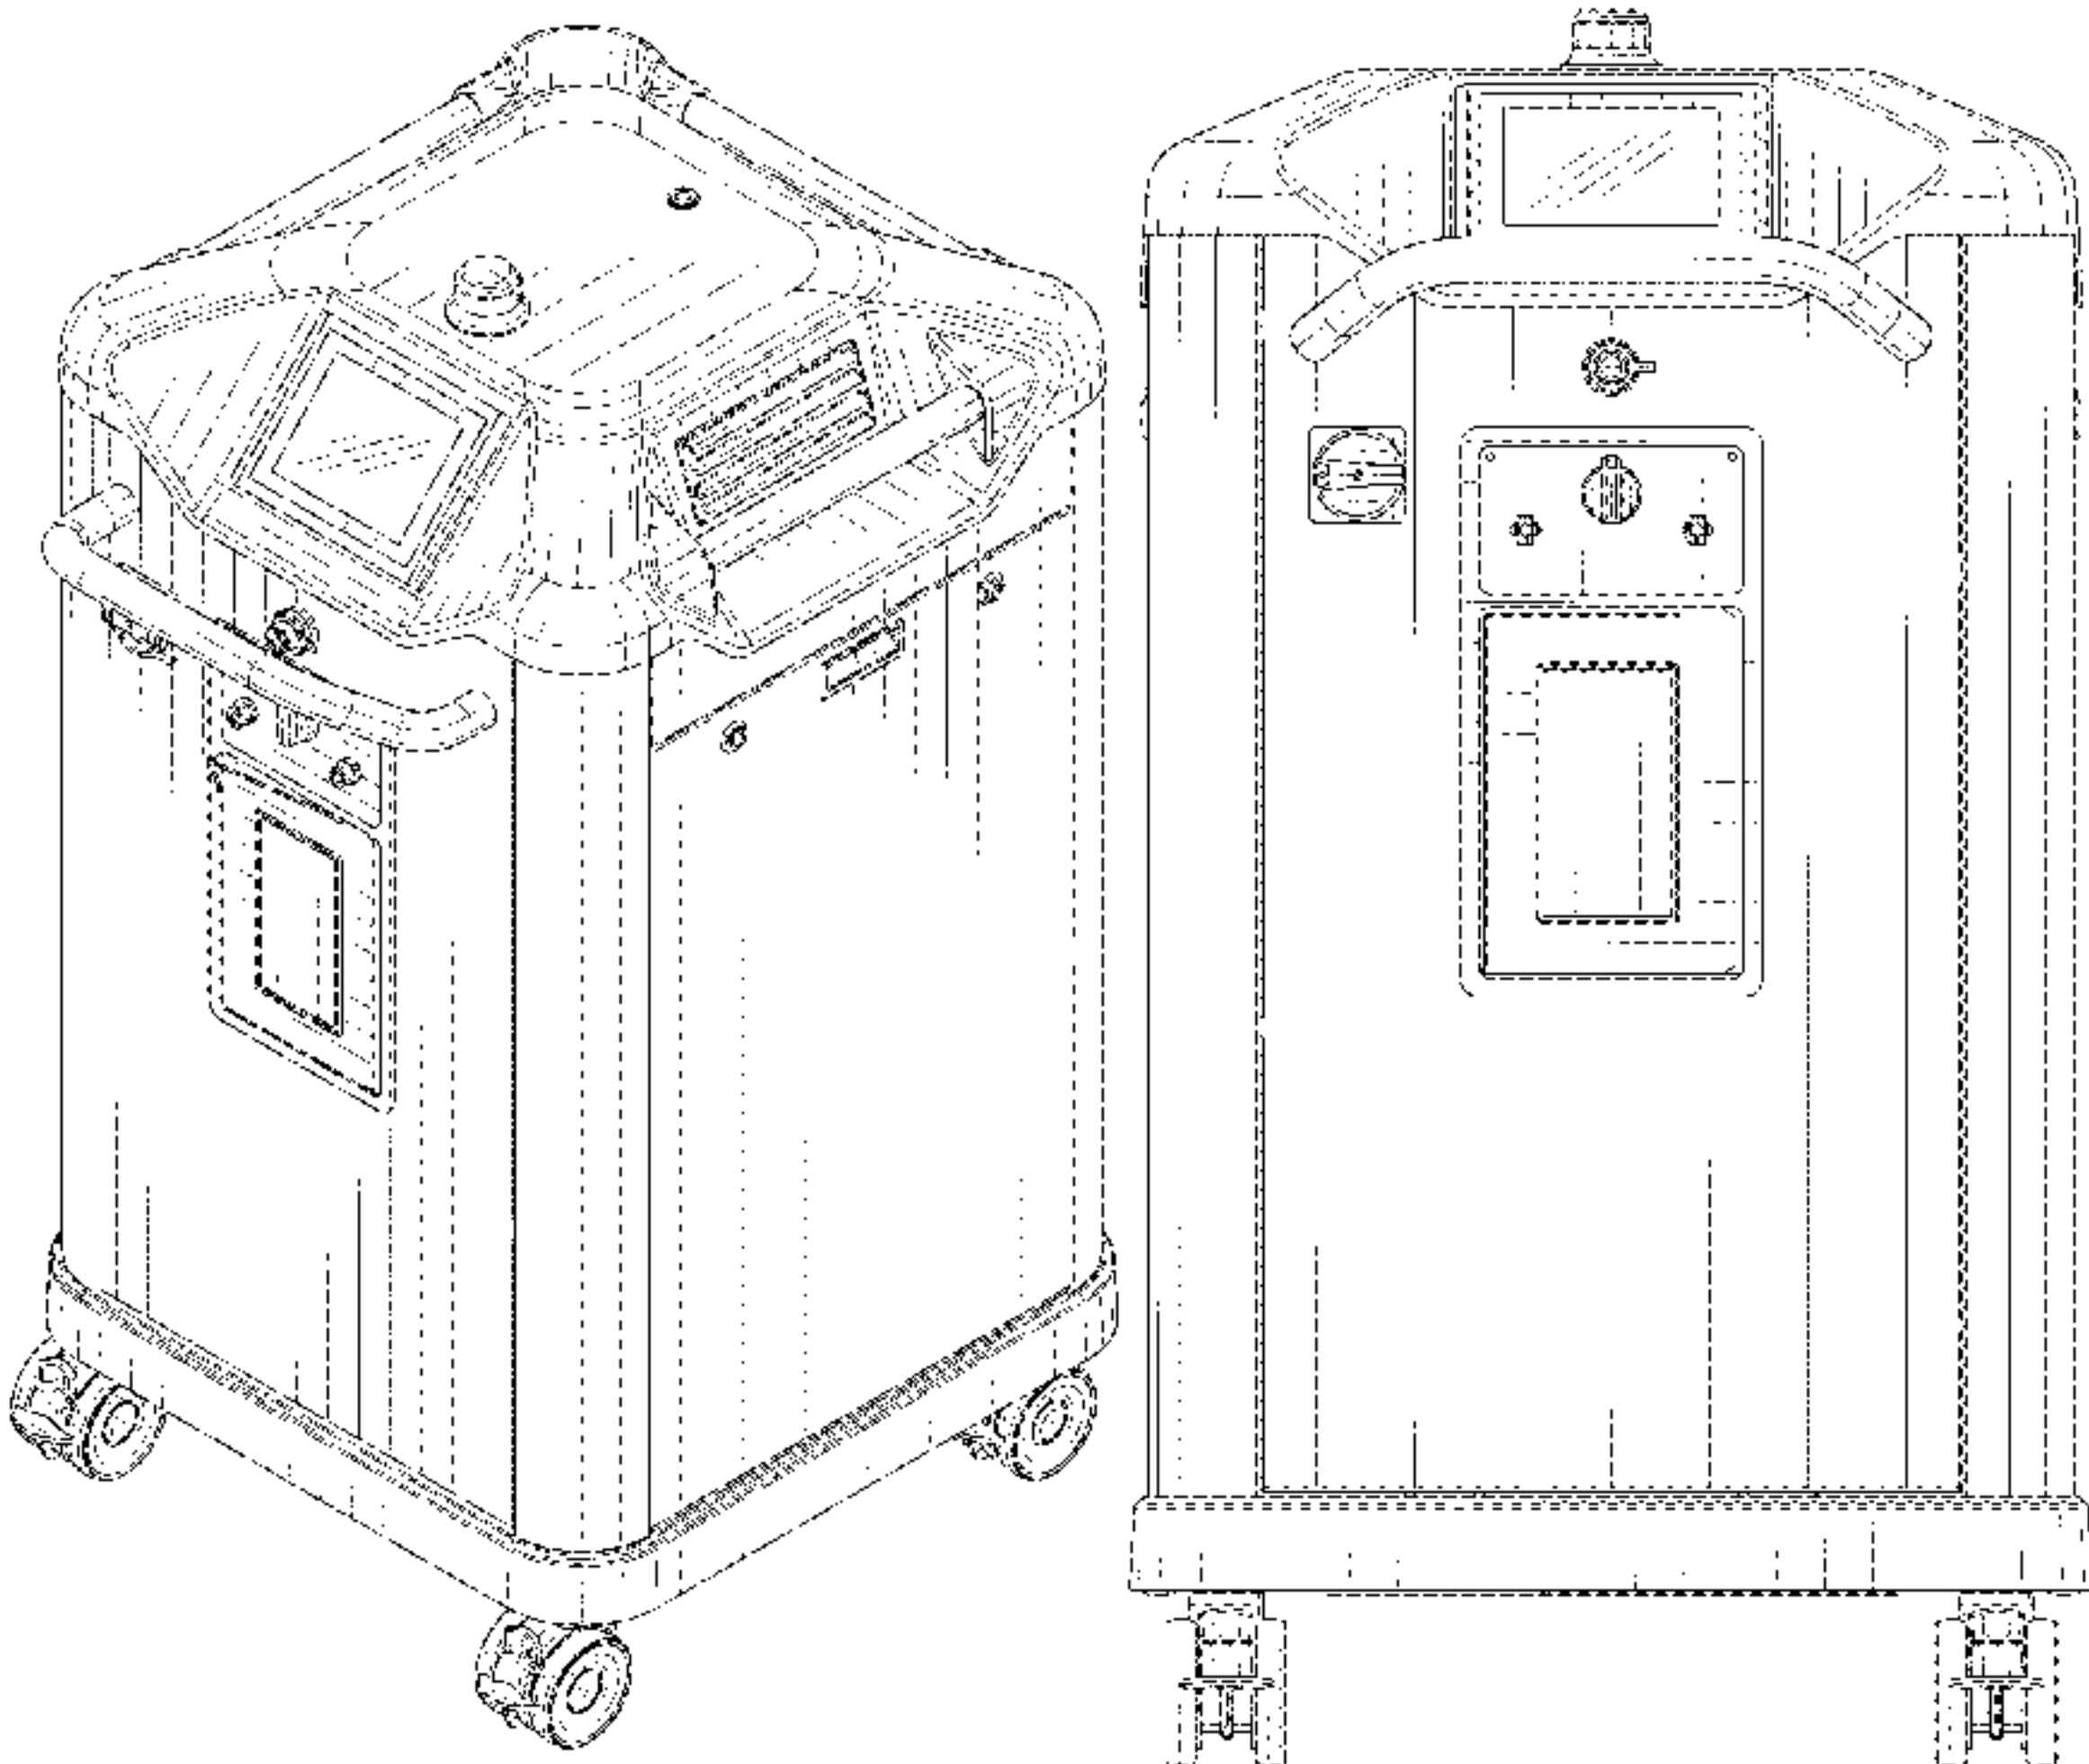


FIG. 28 is a bottom view thereof.
The shade lines show surface contour.
The broken lines depict unclaimed portions of the sterilization cart, and the broken lines form no part of the claimed design.

1 Claim, 28 Drawing Sheets

(58) **Field of Classification Search**
CPC A61L 2202/122; A61L 2202/10; A61L 2202/11; A61L 2202/14; A61L 2202/23; A61L 2202/24; A61L 2202/182; A61L 2/26; A61L 2/24; A61L 2/17; A61L 2/18; A61L 2/025
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

2,467,337 A * 4/1949 Schnell A61L 2/00 99/413
D176,310 S * 12/1955 Schulz D24/217
D207,517 S * 4/1967 Perkins D24/217
D235,933 S * 7/1975 Wyse D24/217
3,994,684 A * 11/1976 Tomasulo A61L 2/07 422/26

D264,123 S * 4/1982 Brendgord D24/217
D275,031 S * 8/1984 Moyse D24/232
D305,261 S * 12/1989 Hobbs D24/217
D319,309 S * 8/1991 Taylor D24/217
D347,696 S * 6/1994 Tominaga D24/217
D379,519 S * 5/1997 Carter D24/217
D502,546 S * 3/2005 Shin D6/534
D546,473 S * 7/2007 Xu D24/217
D616,563 S * 5/2010 Huck D24/217
D703,343 S * 4/2014 Biswas D24/217
D776,293 S * 1/2017 Cerasi D24/217
D822,845 S * 7/2018 Shimobayashi D24/217
D822,846 S * 7/2018 Shimobayashi D24/217
D824,533 S * 7/2018 Shimobayashi D24/217
D841,831 S * 2/2019 Shimobayashi D24/217
D846,141 S * 4/2019 Shimobayashi D24/217
D873,434 S * 1/2020 Xie D24/217
D890,357 S * 7/2020 Zanon D24/217
D898,218 S * 10/2020 Hickey D24/217
D908,238 S * 1/2021 Cavada, Jr. D24/217
D930,181 S * 9/2021 Milliff D24/217
D957,667 S * 7/2022 Shimobayashi D24/217
D977,139 S * 1/2023 Lai D24/217
D992,140 S * 7/2023 Clottu D24/217
D1,018,892 S * 3/2024 Zargaryan D24/217
D1,038,551 S * 8/2024 Cho D15/199
D1,046,193 S * 10/2024 Marker D24/232
D1,049,423 S * 10/2024 Allegoren D24/232
2011/0291372 A1 * 12/2011 Stryker B62B 3/005 280/47.35
2024/0279868 A1 * 8/2024 Pease D06F 73/00

* cited by examiner

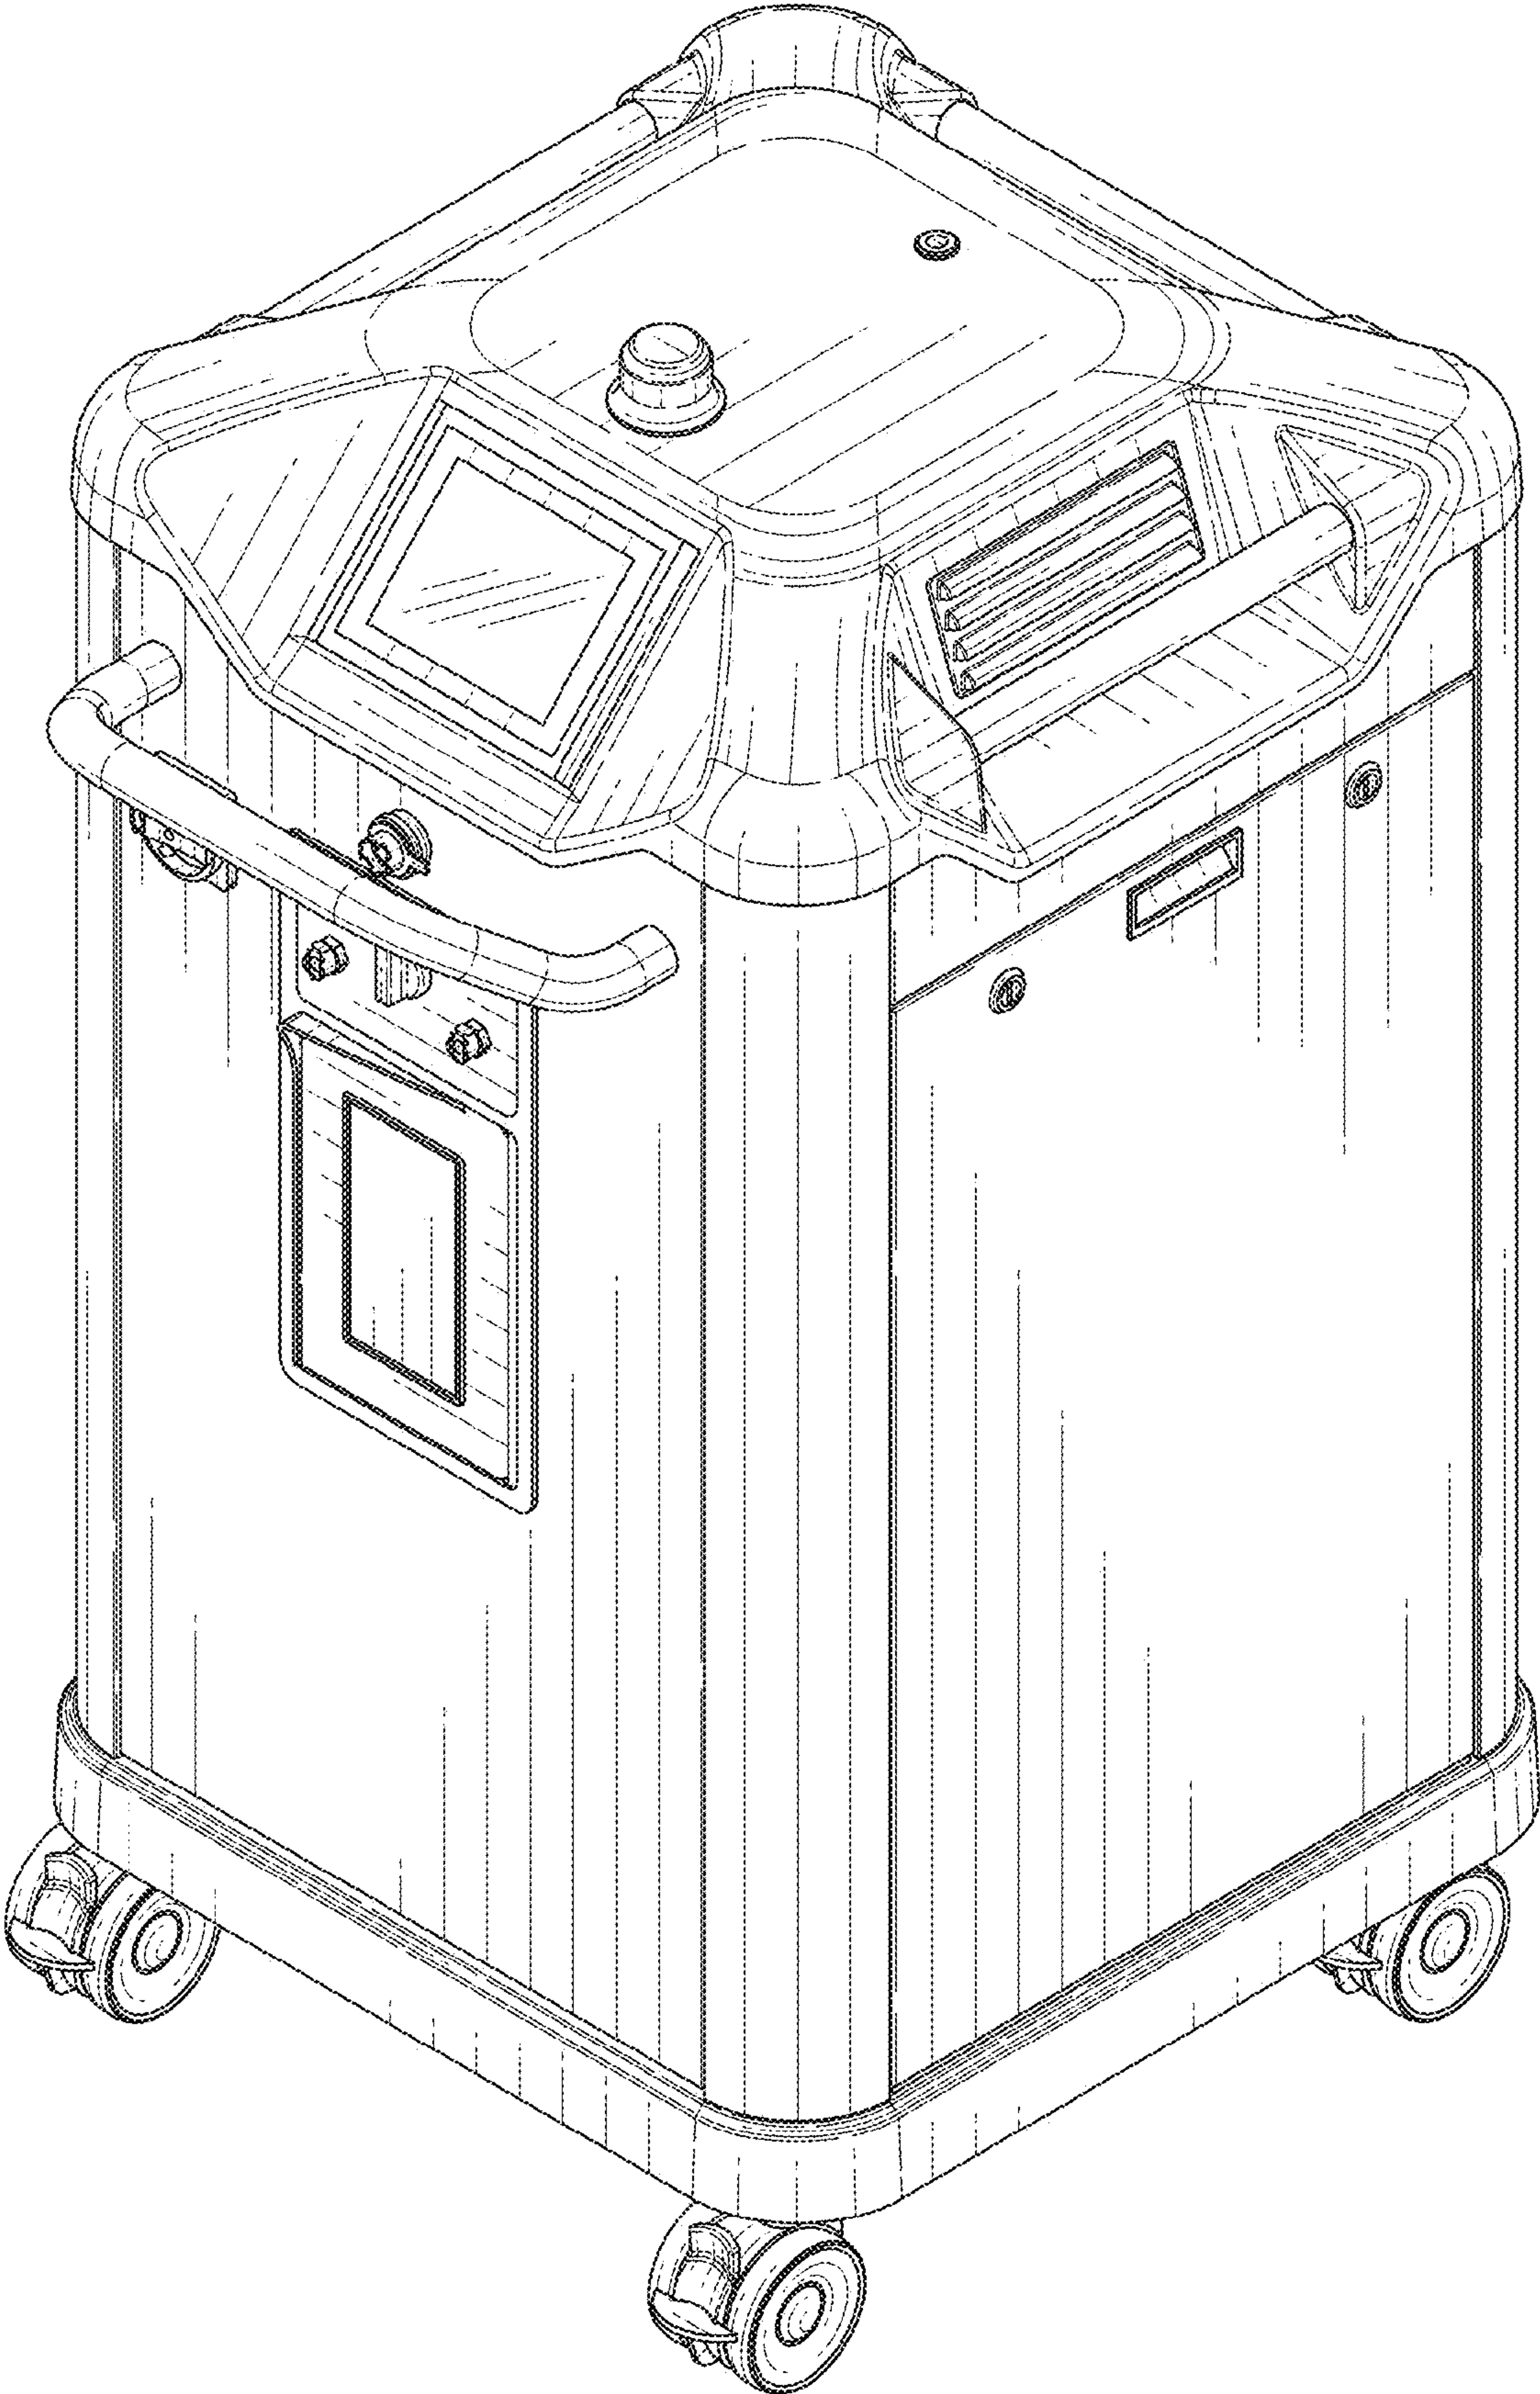


FIG. 1

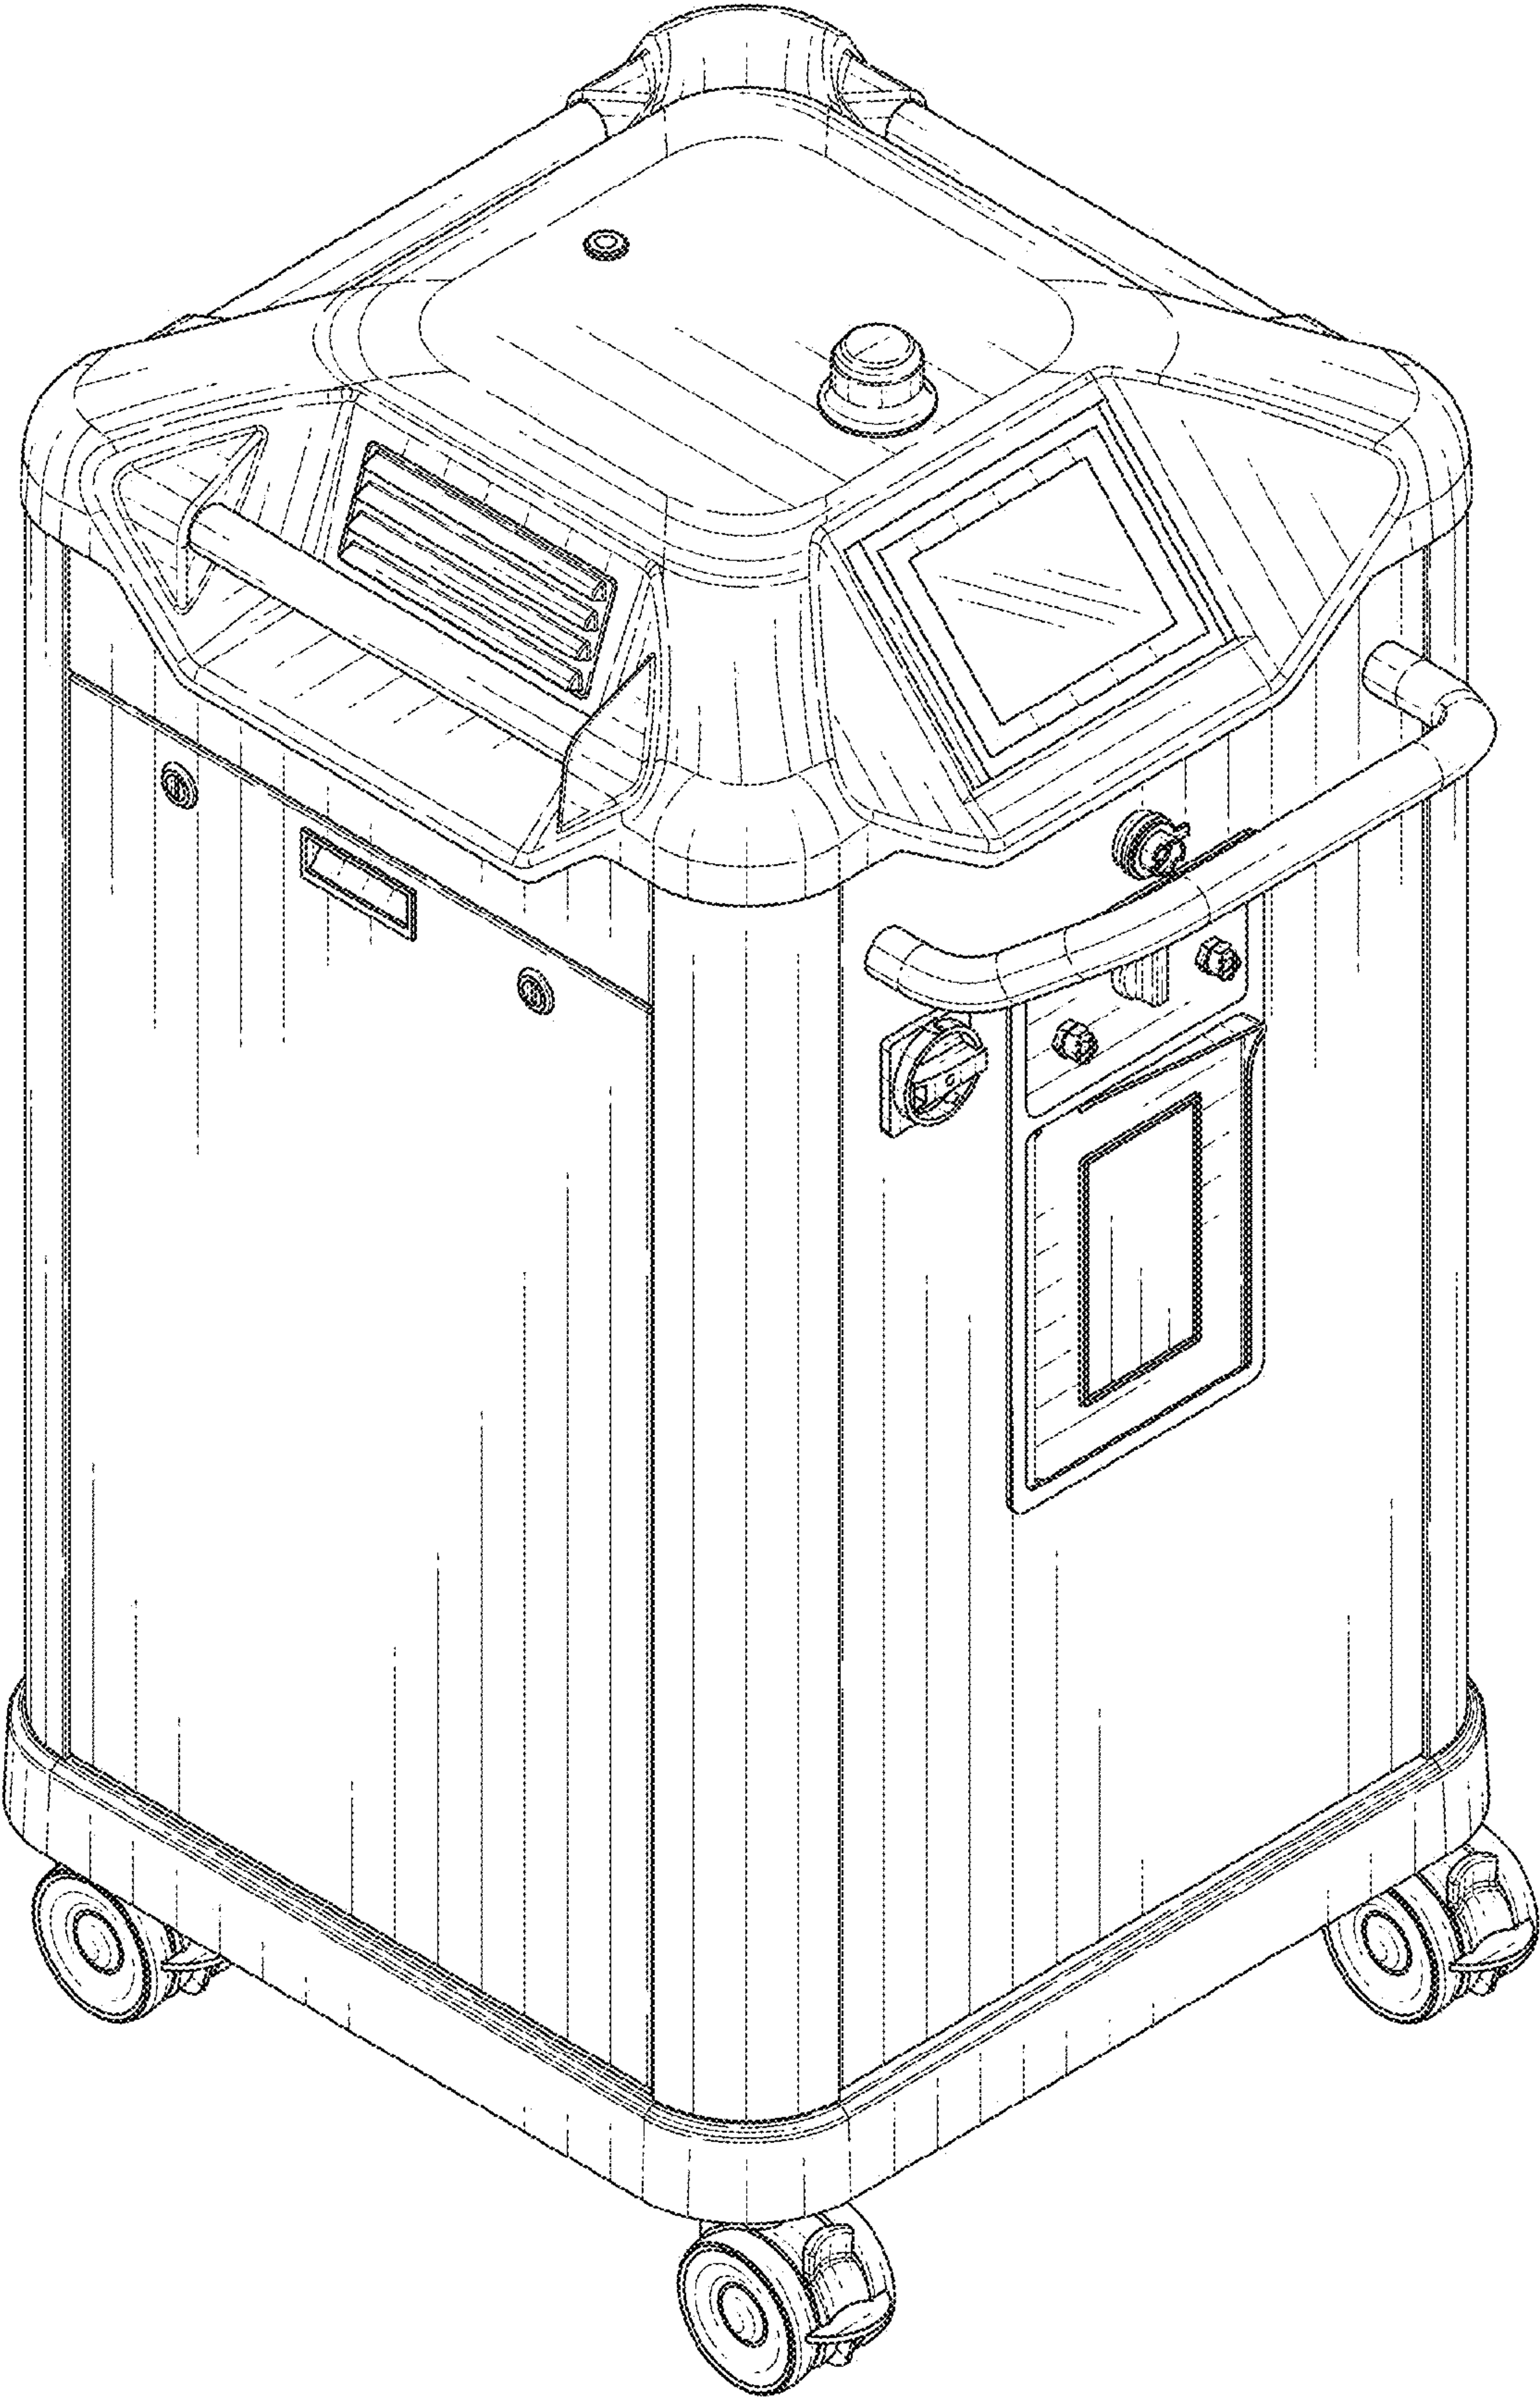


FIG. 2

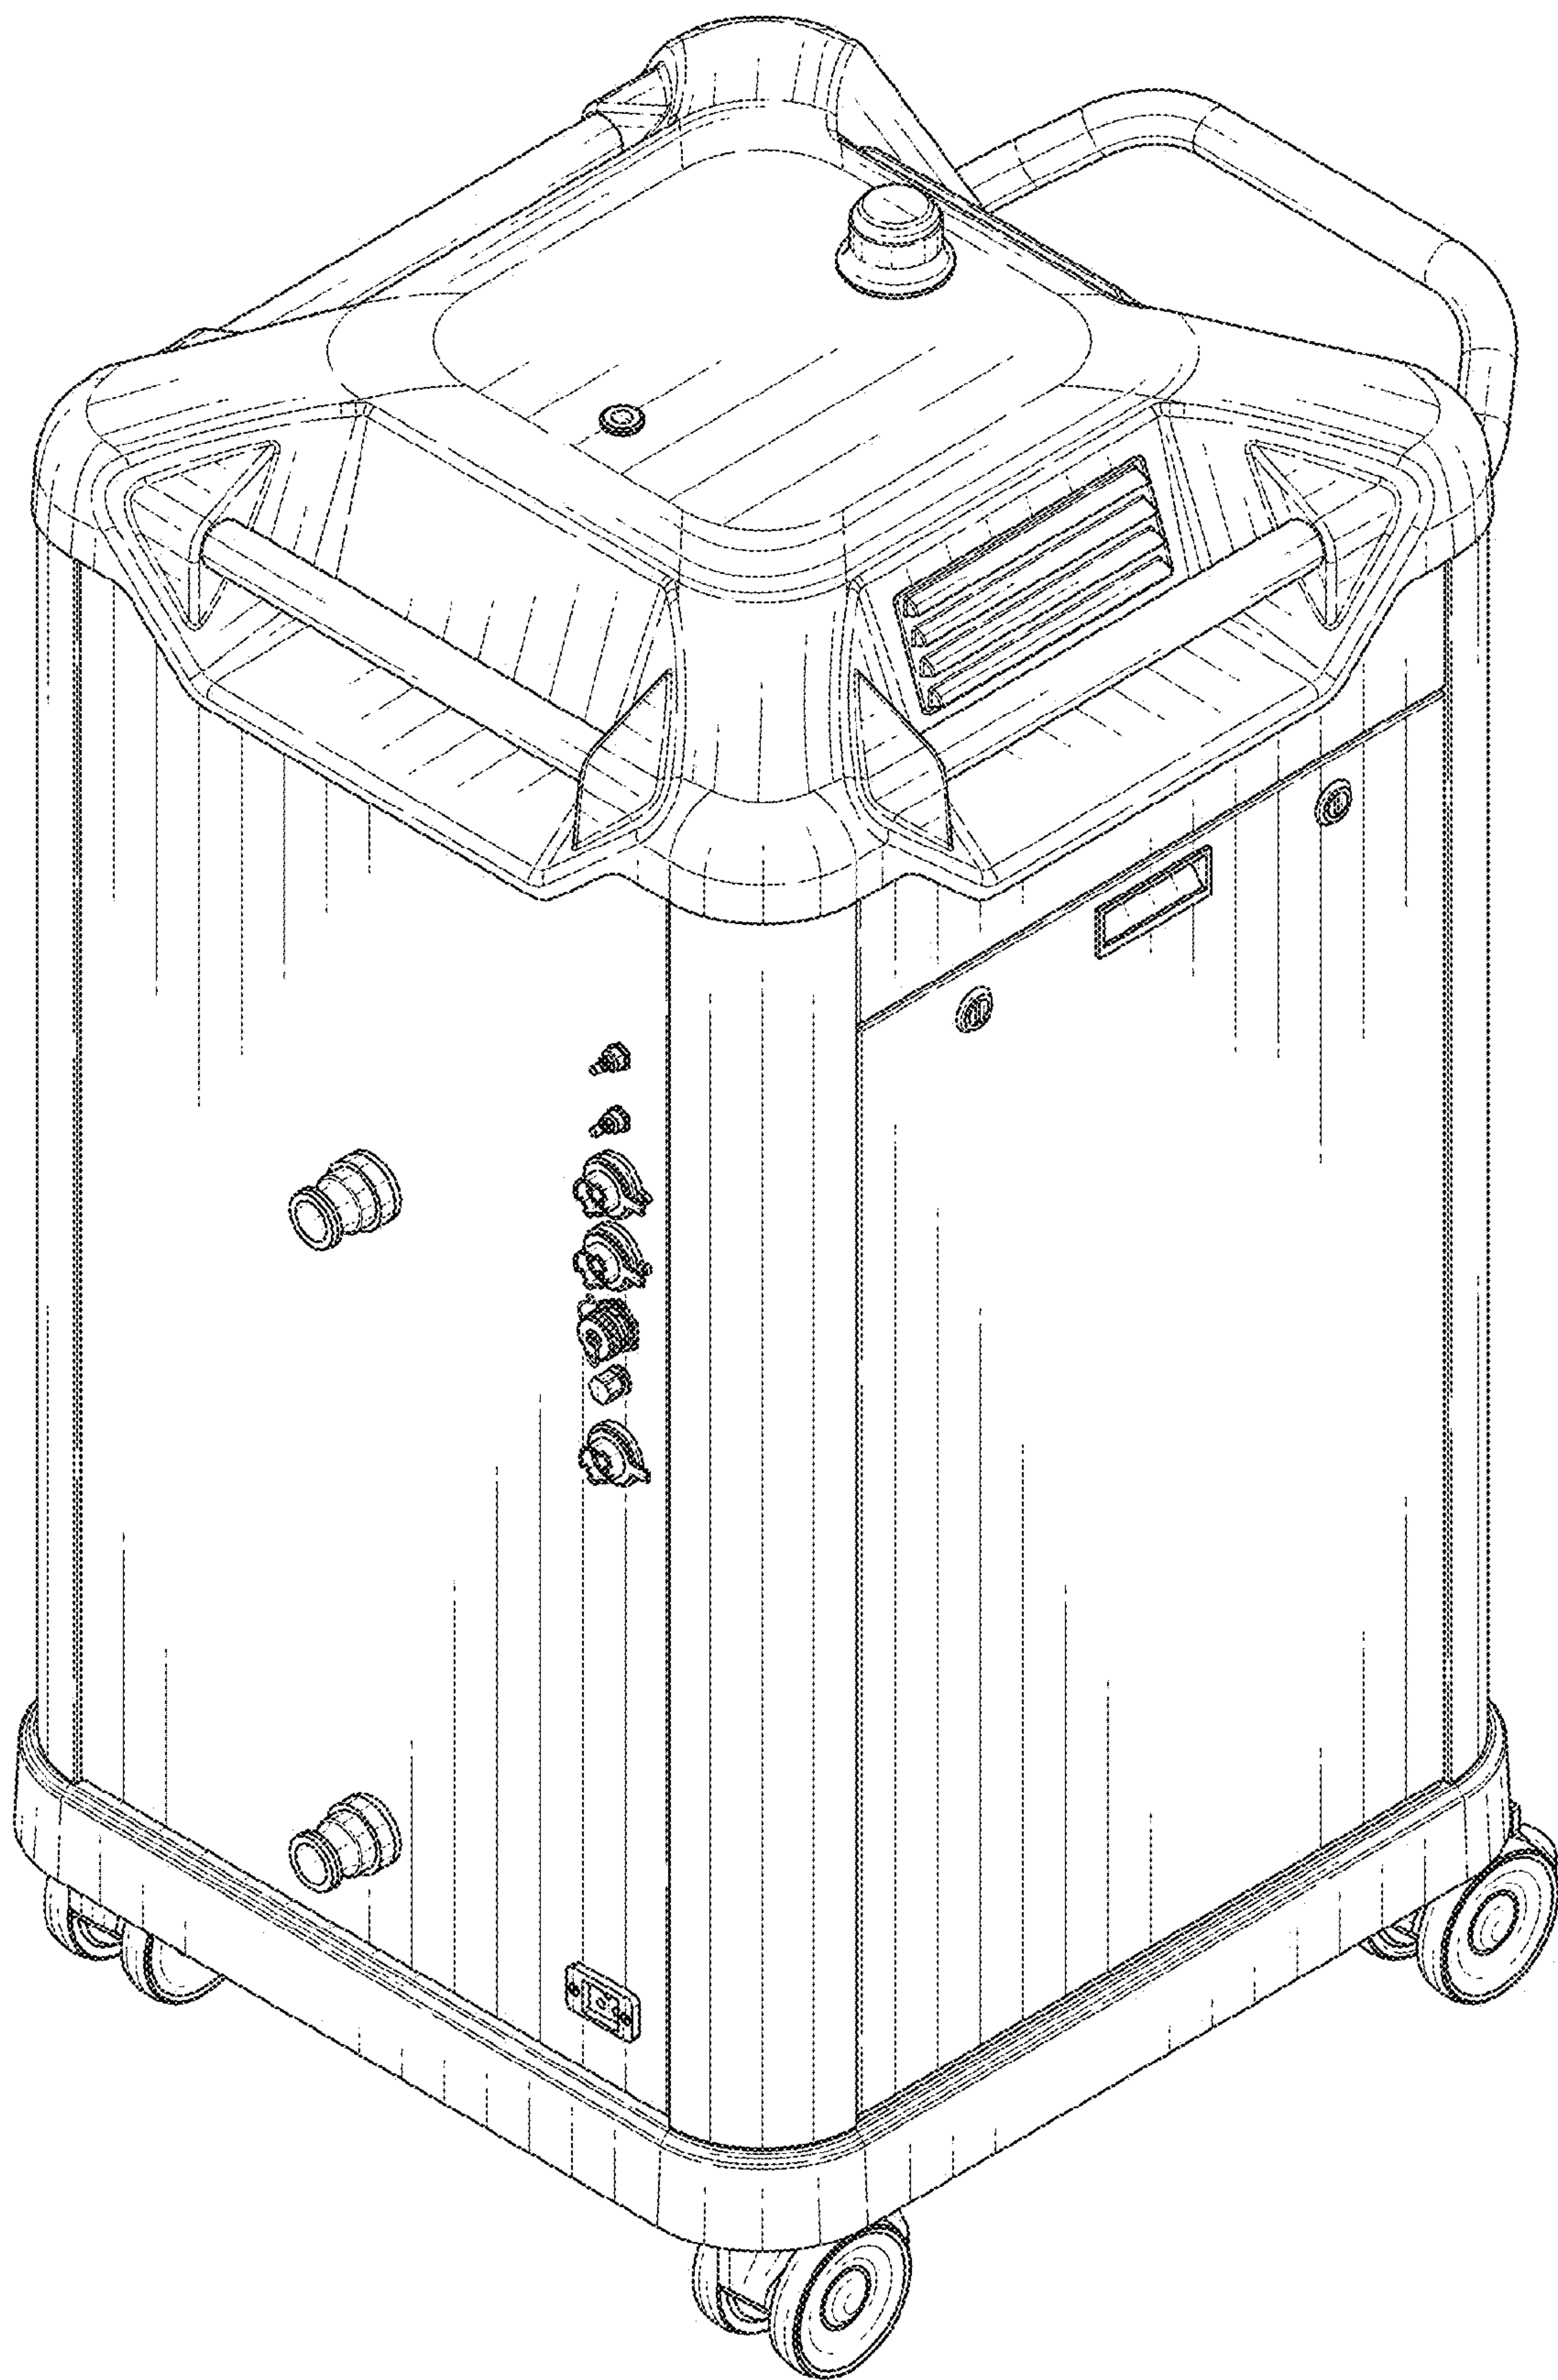


FIG. 3

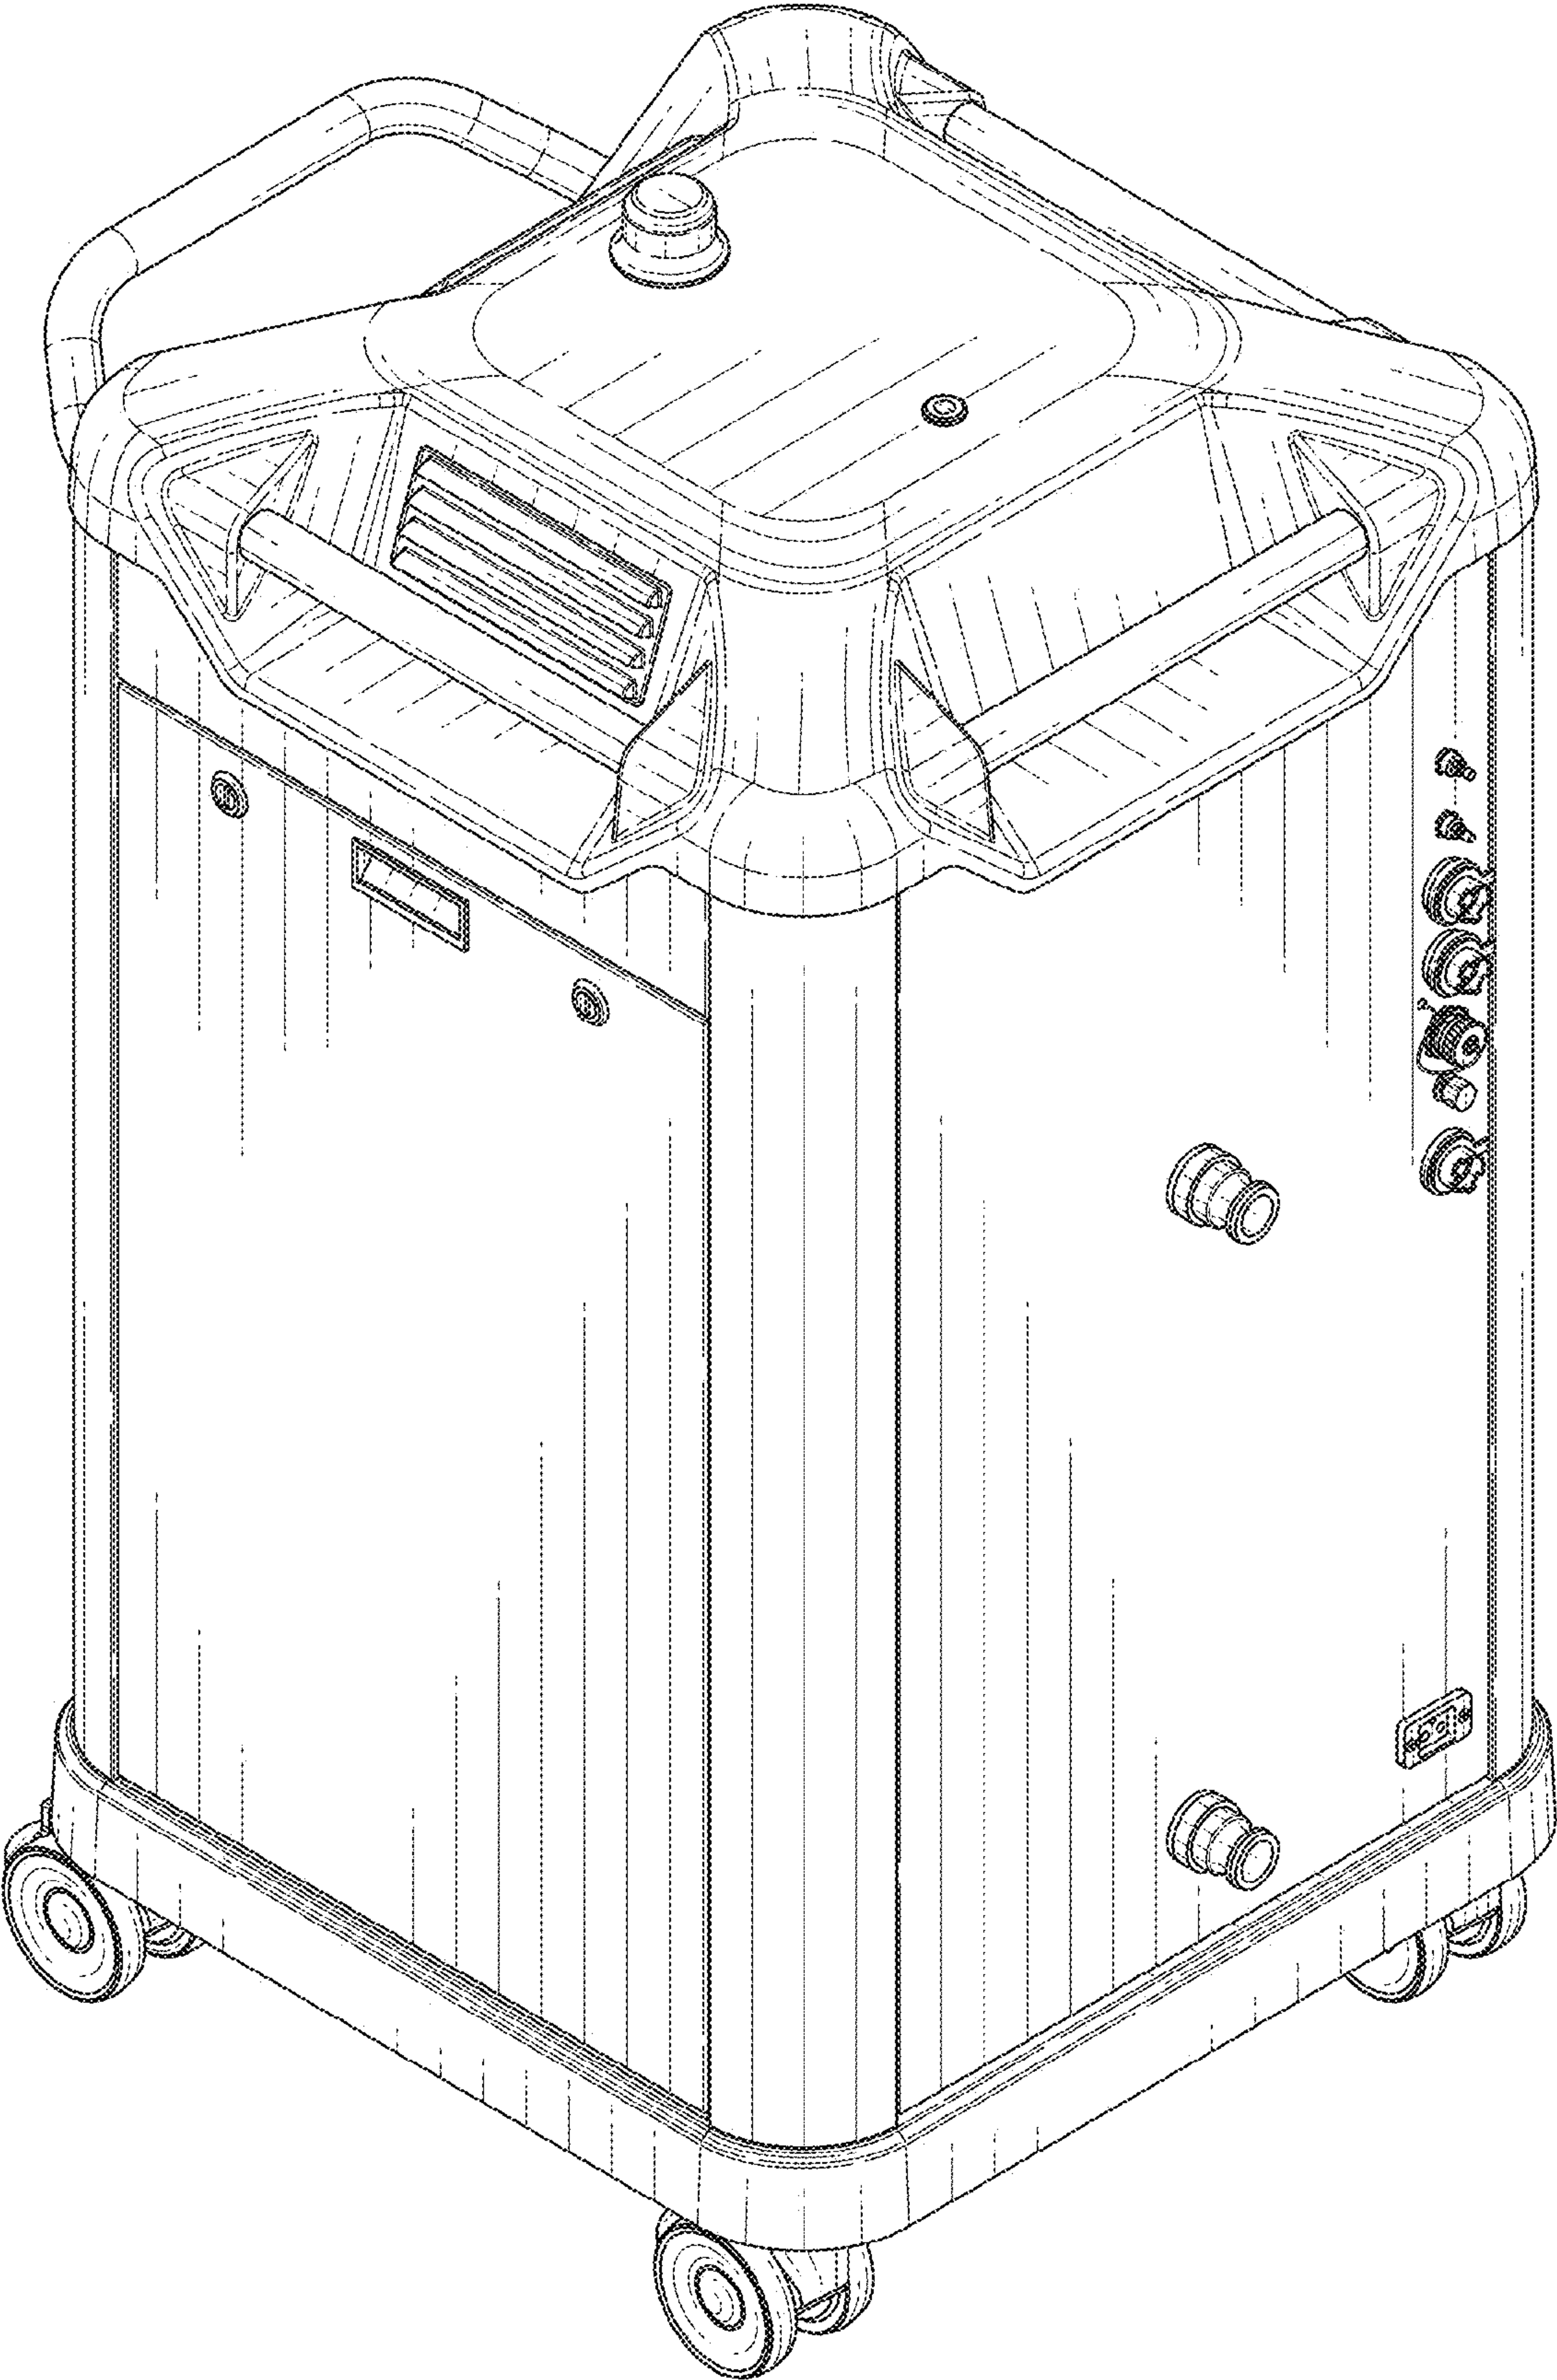


FIG. 4

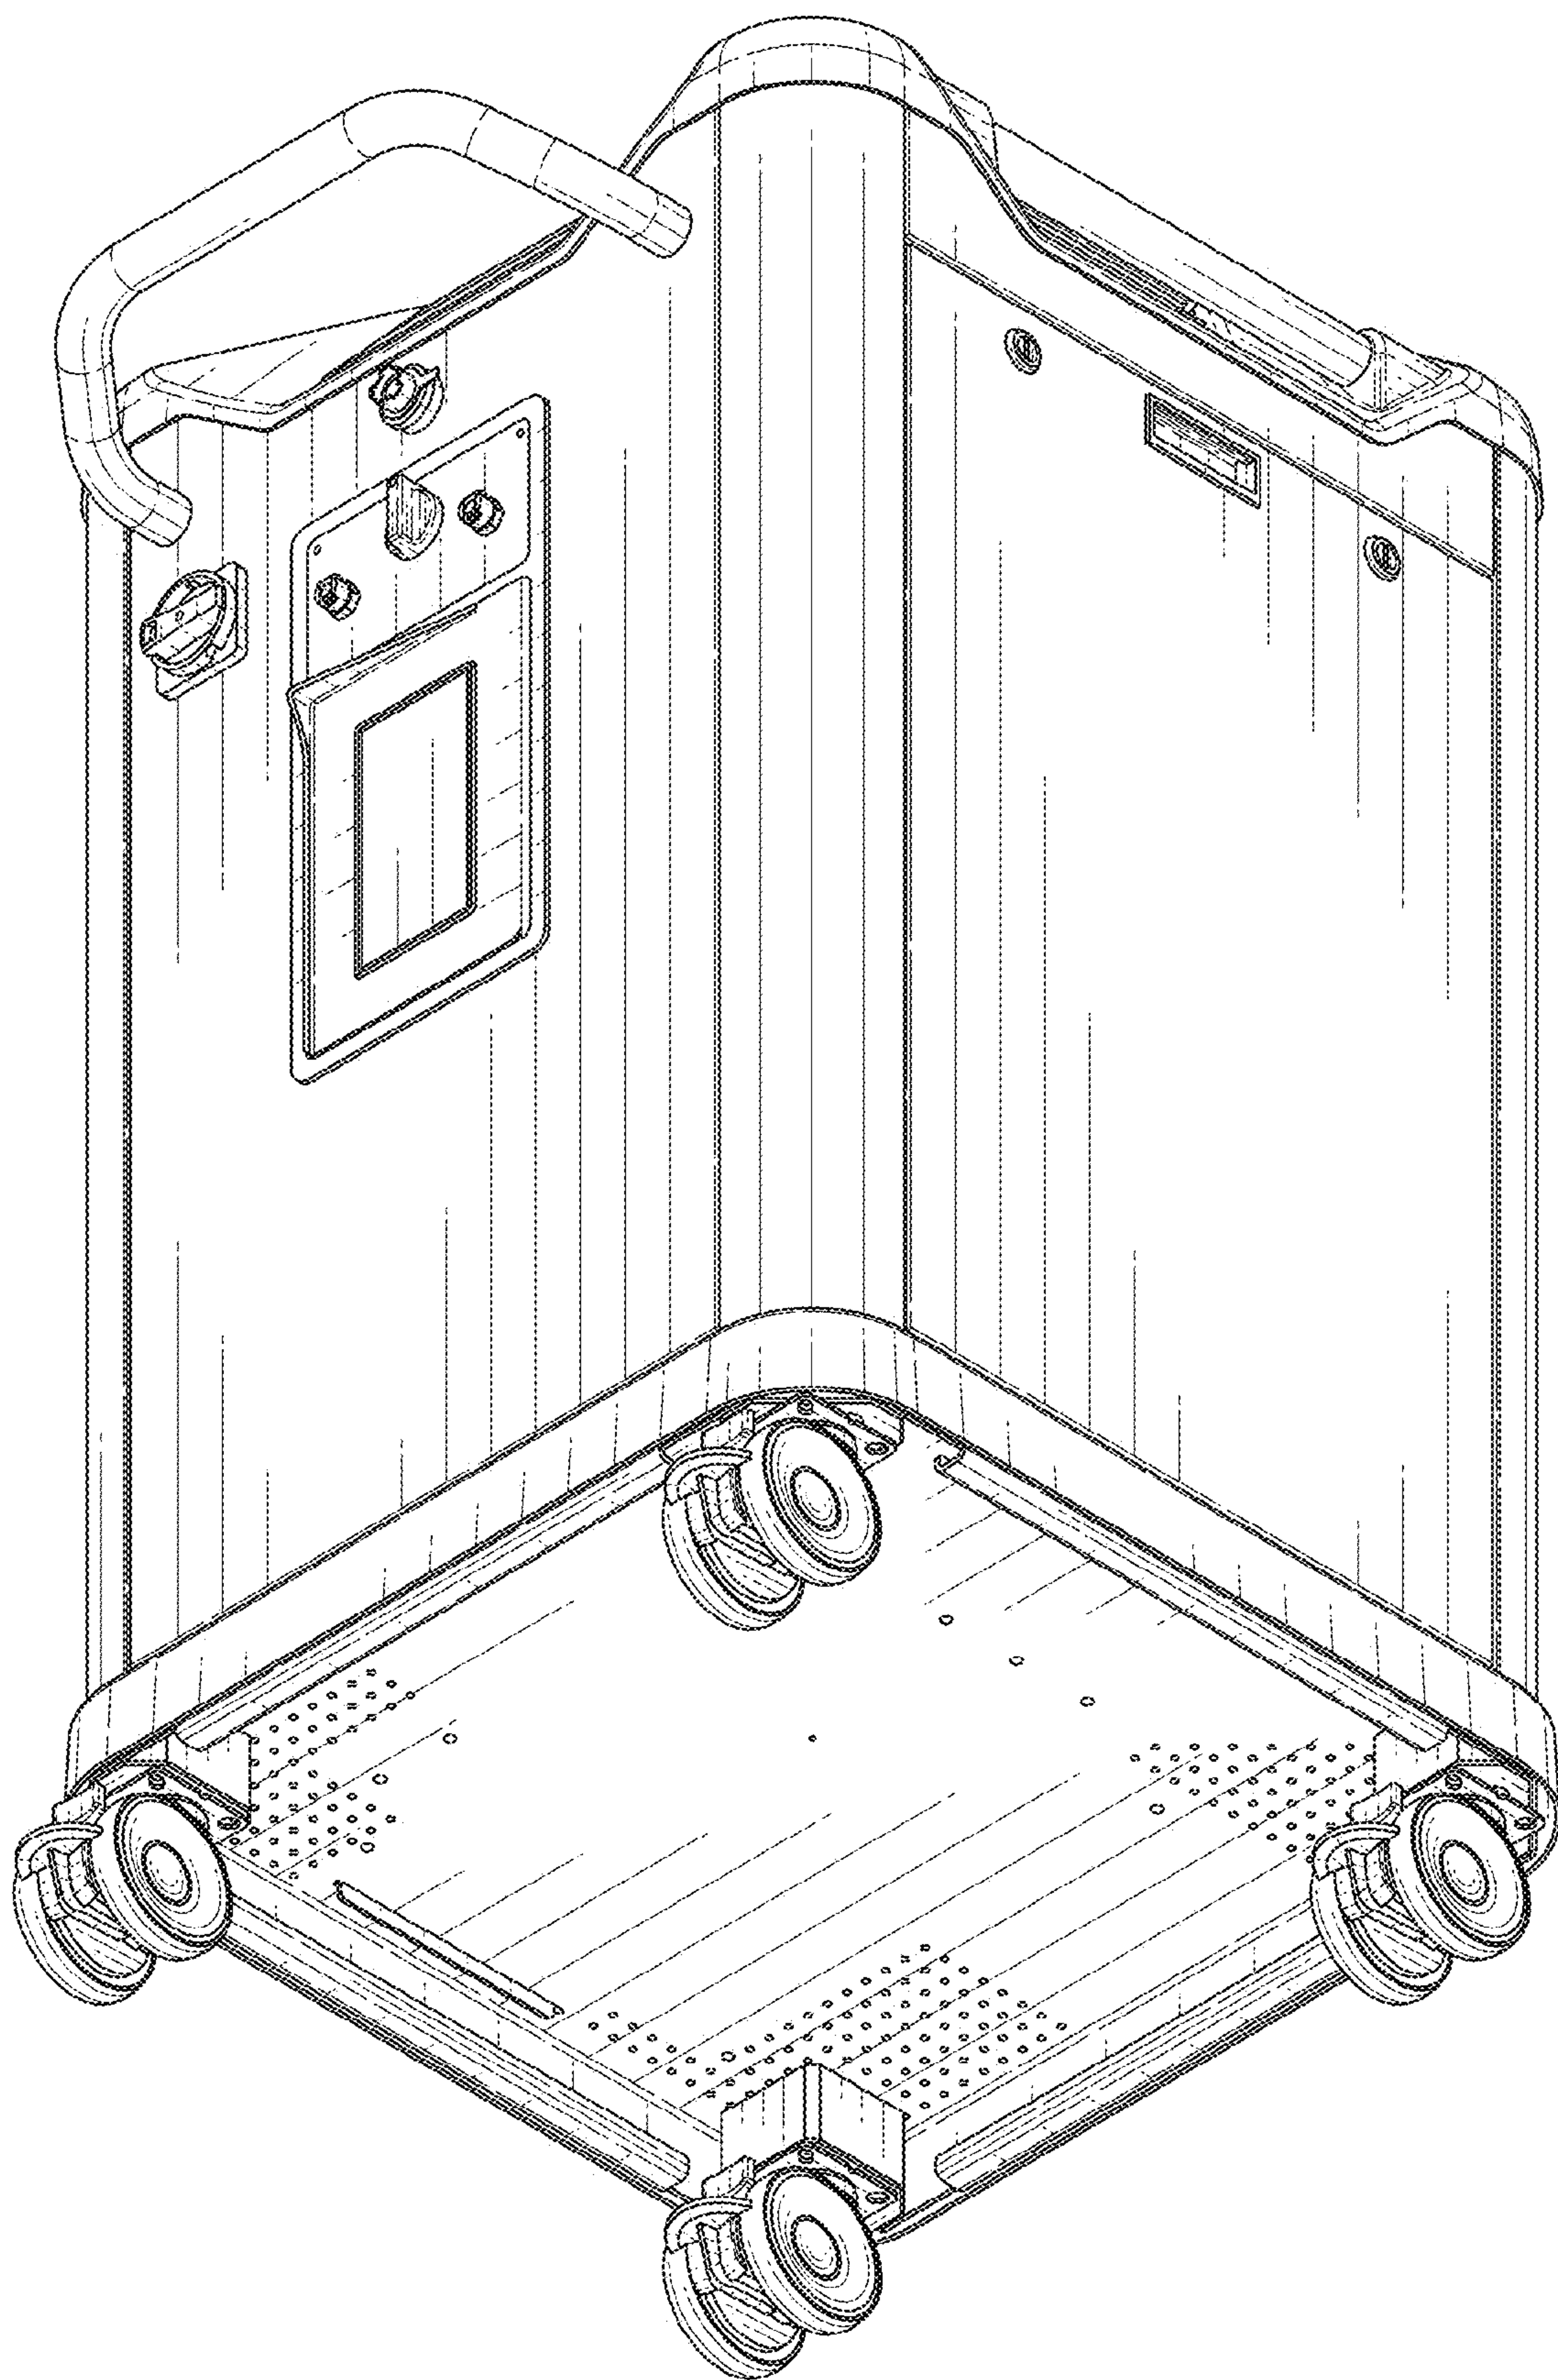


FIG. 5

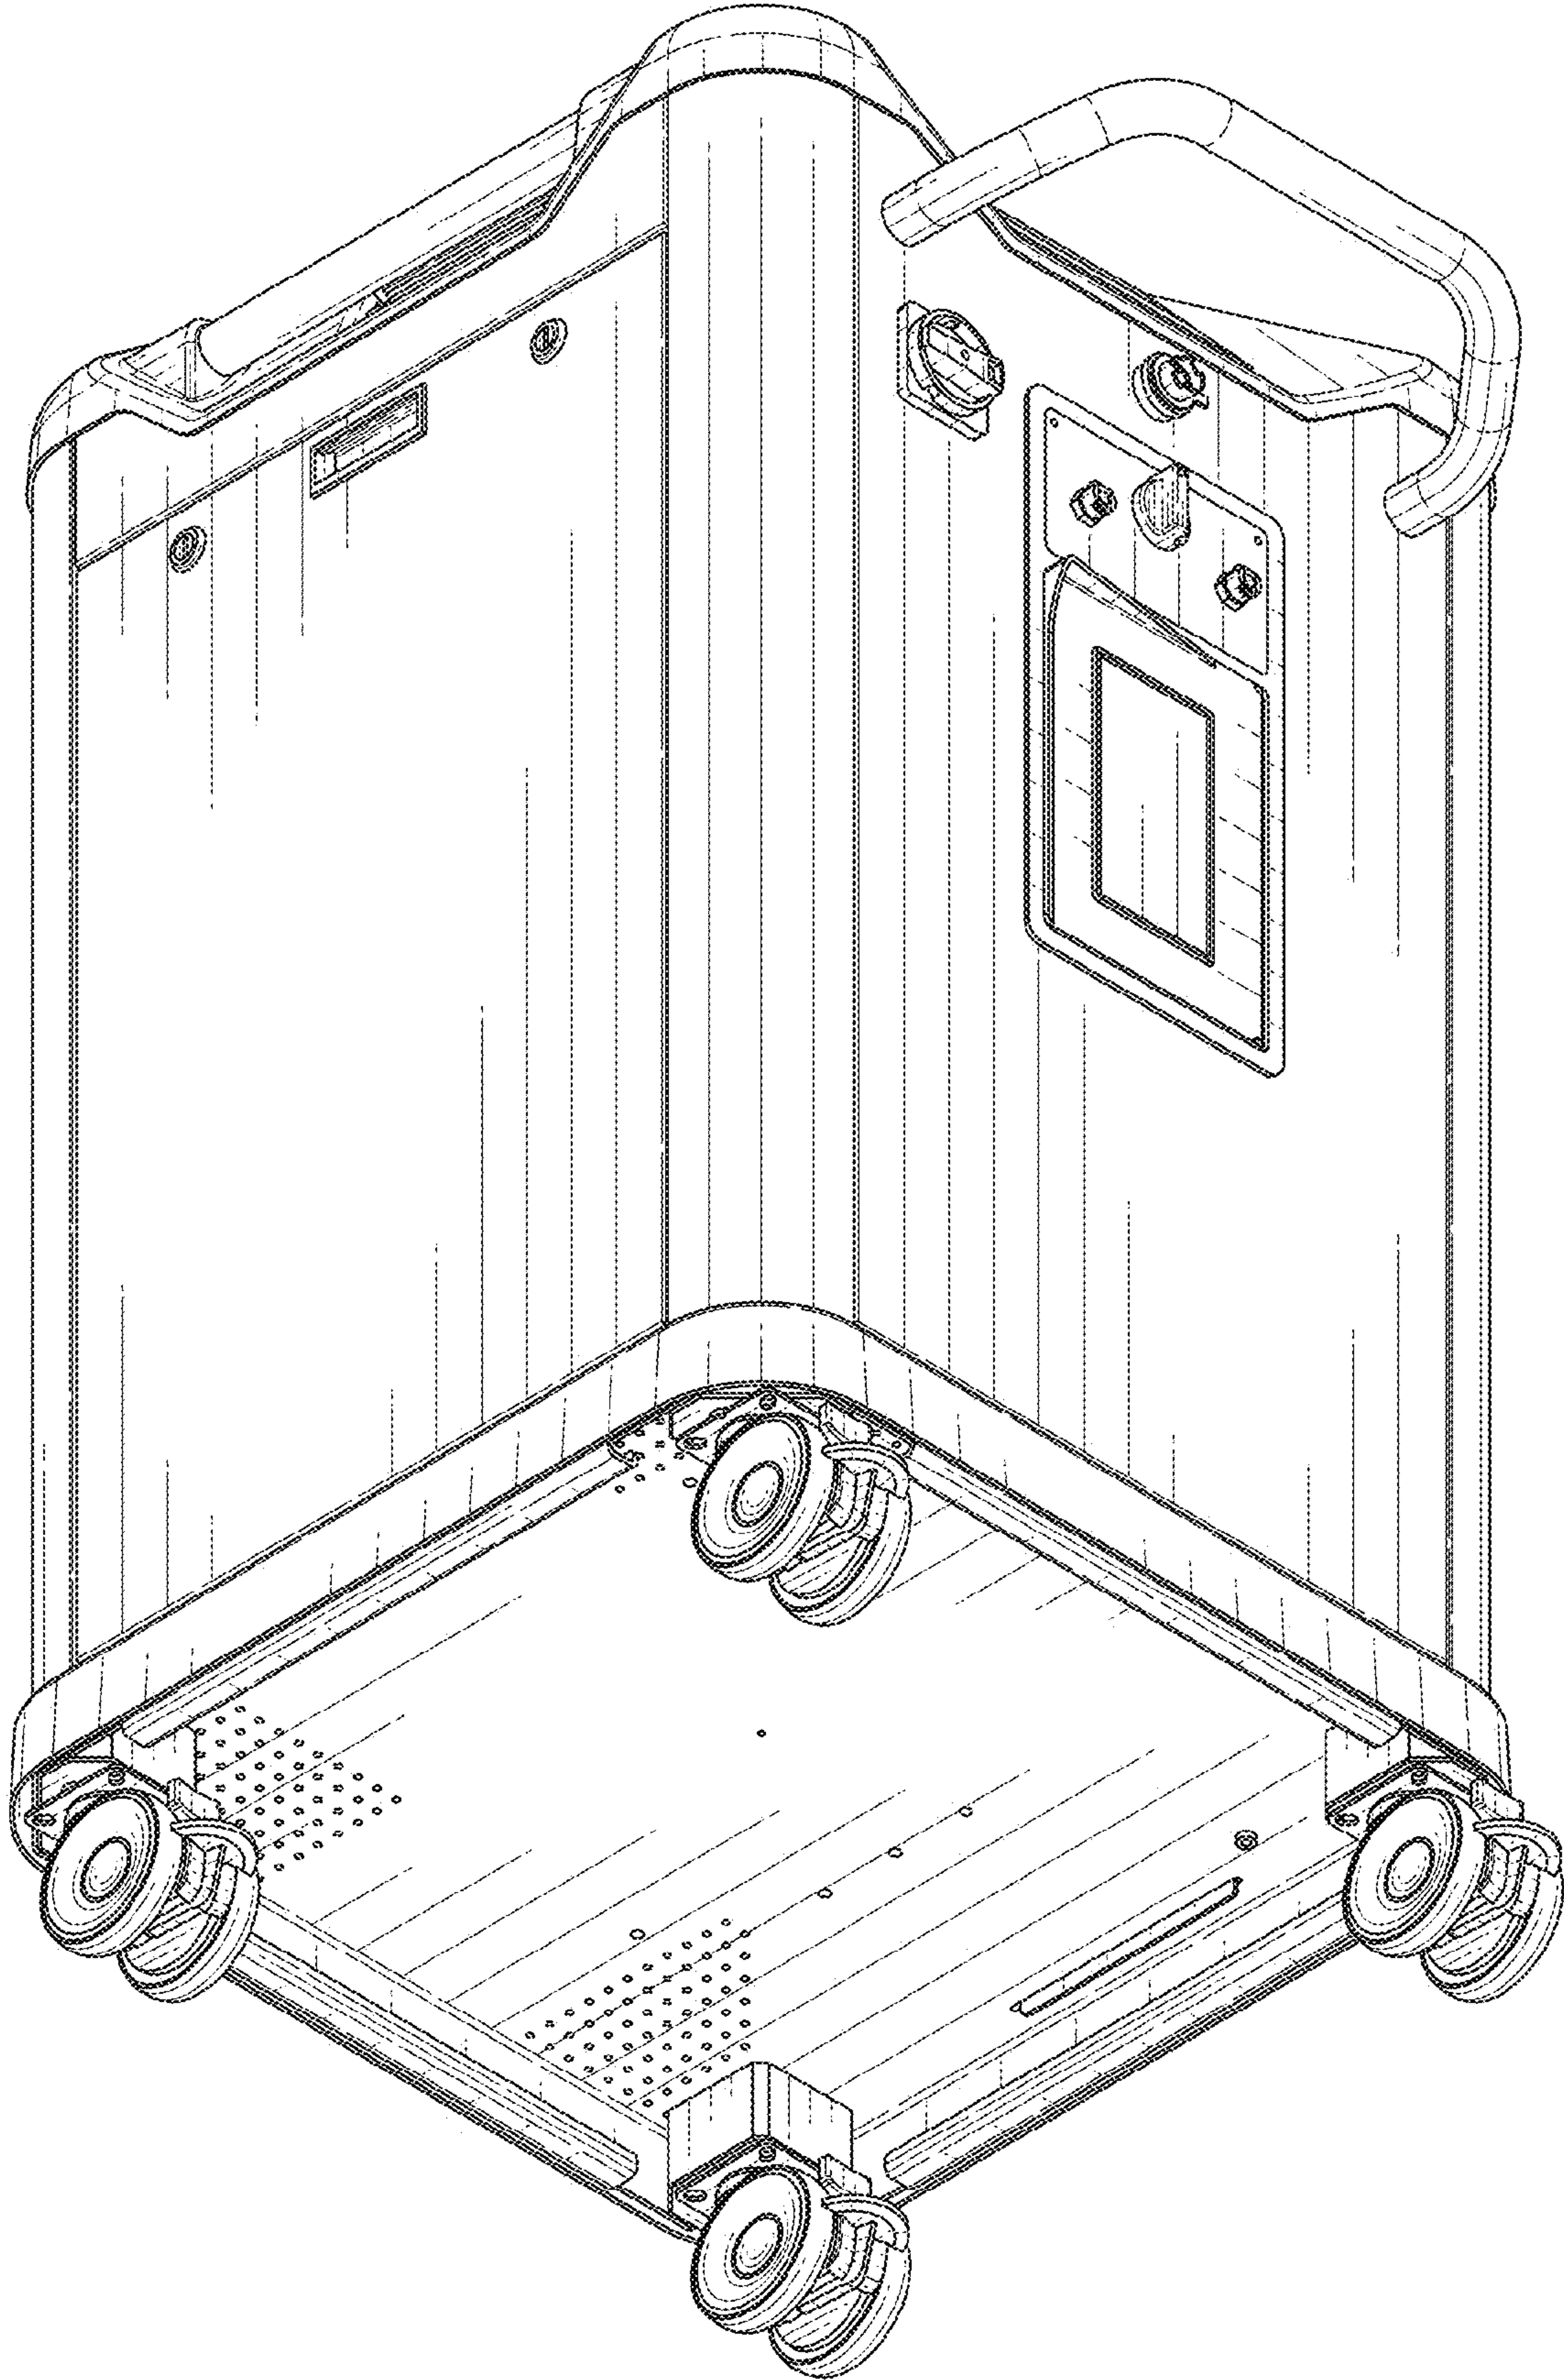


FIG. 6

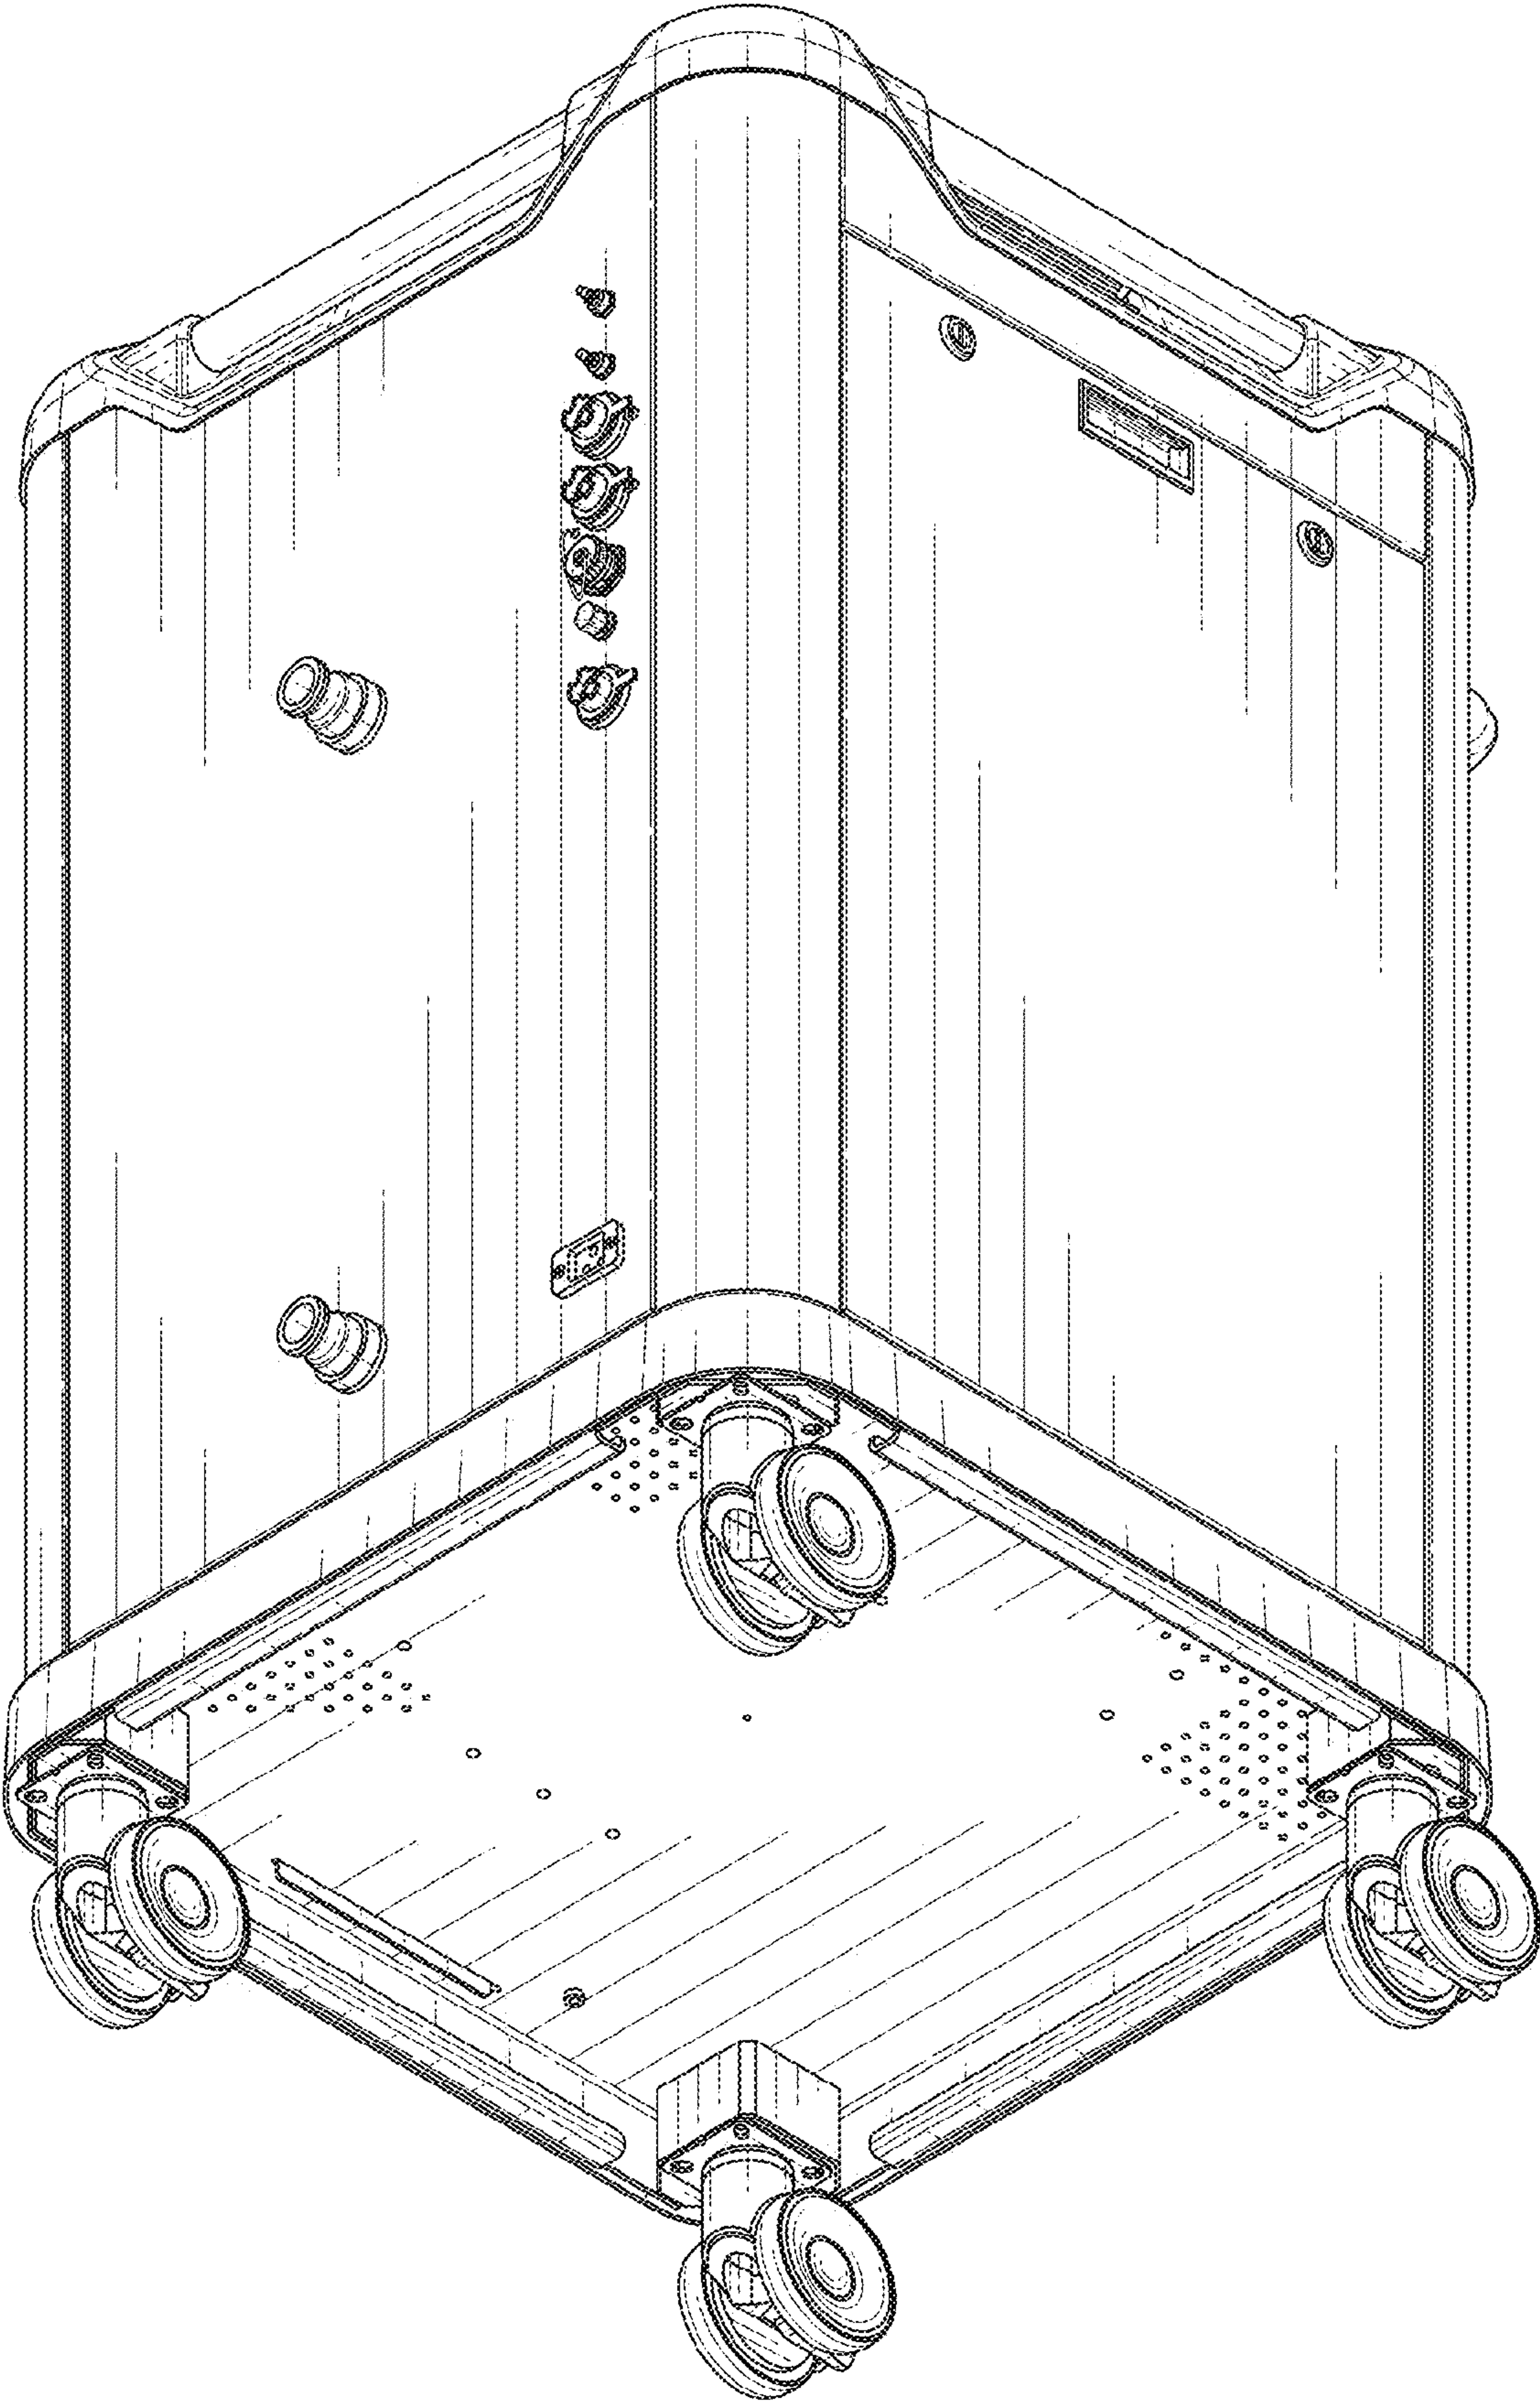


FIG. 7

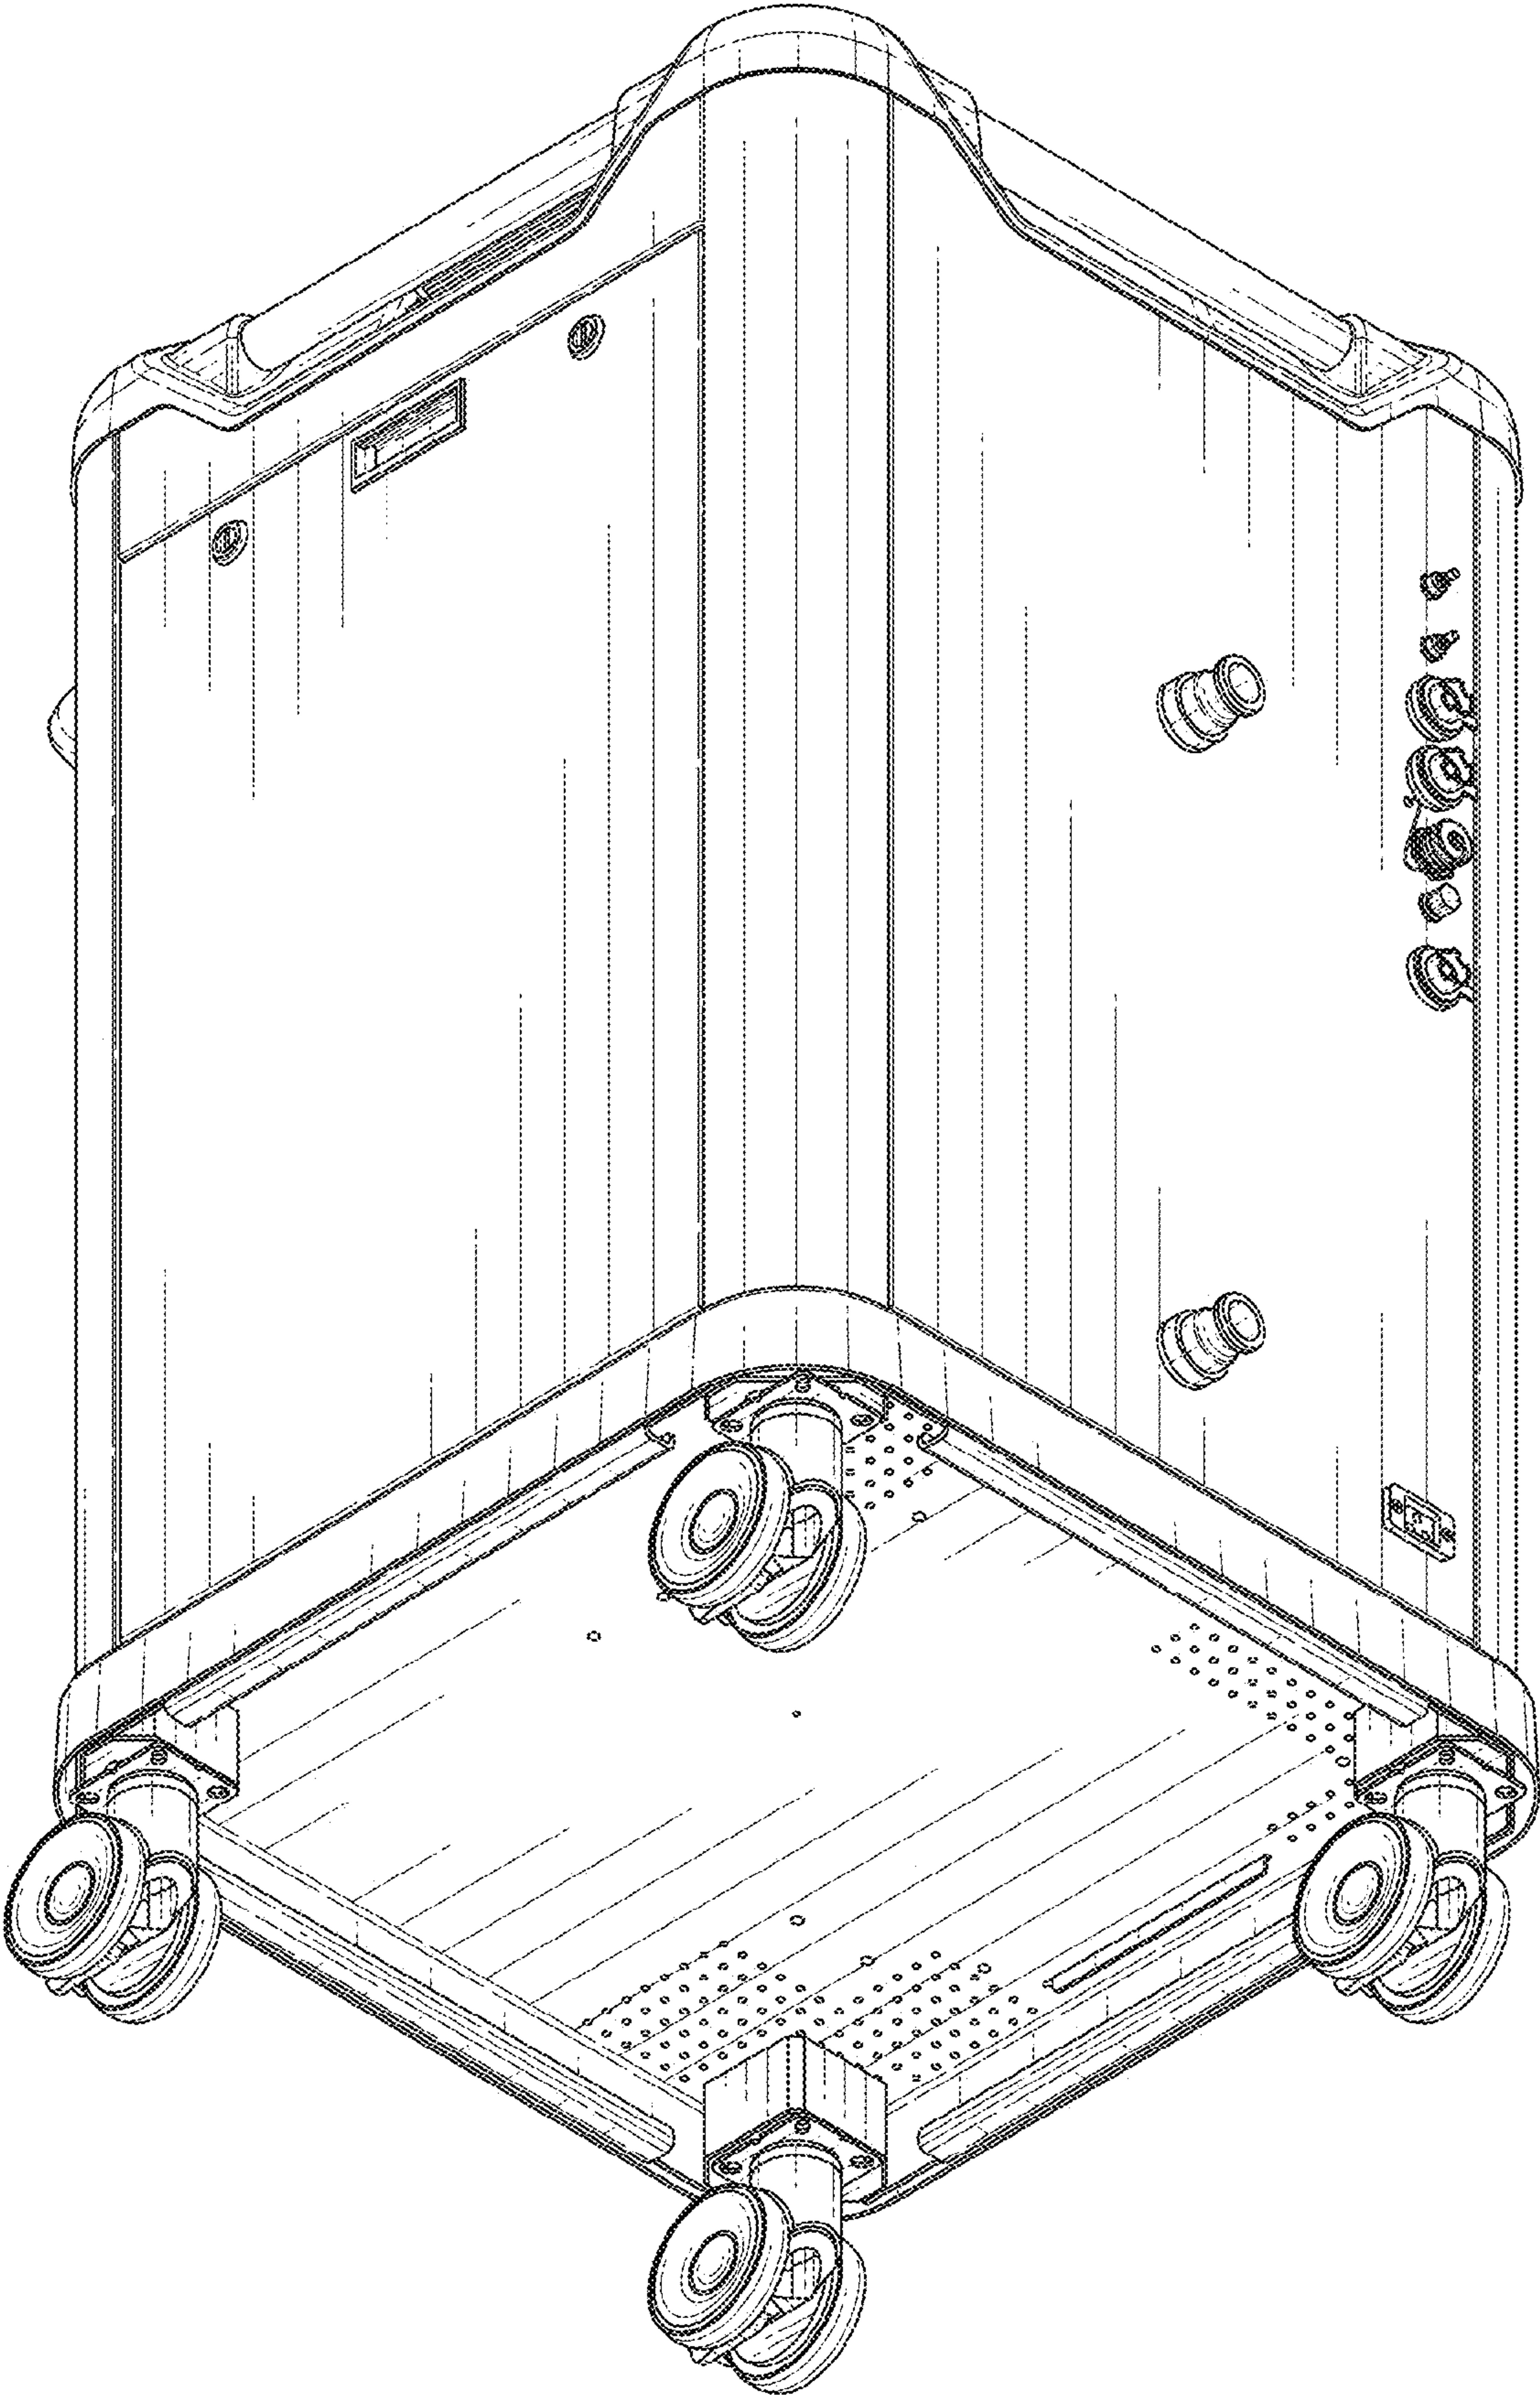


FIG. 8

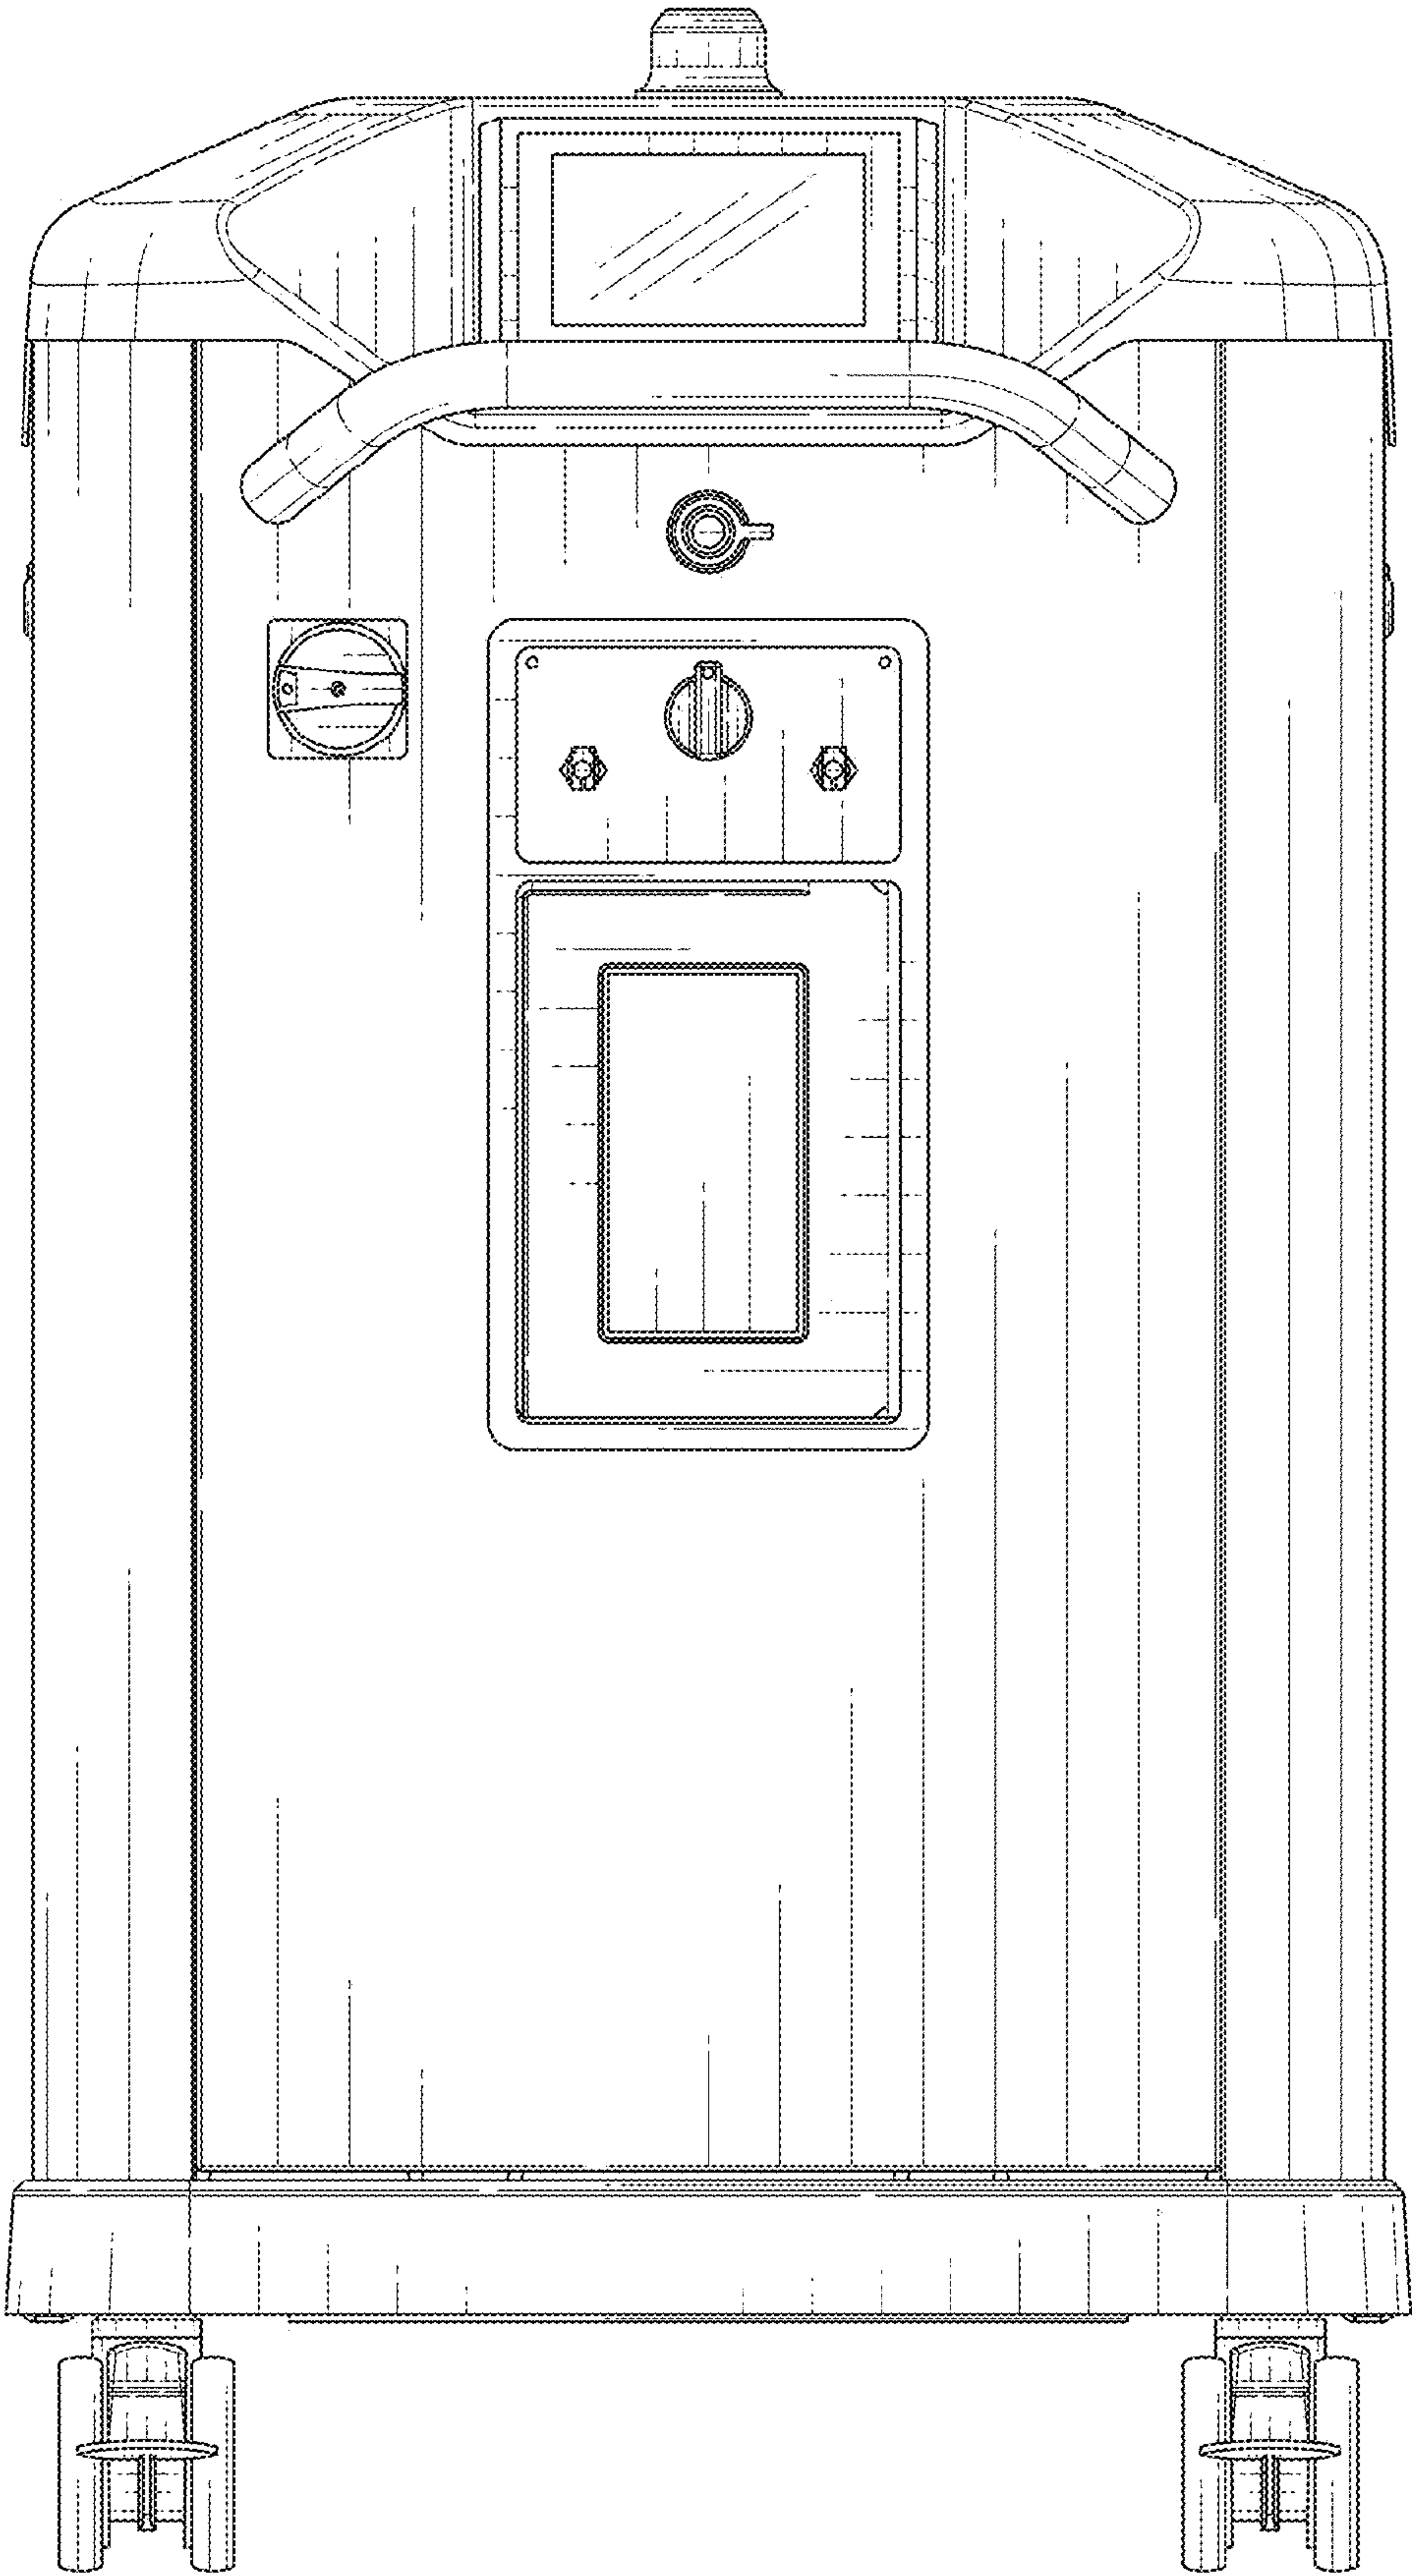


FIG. 9

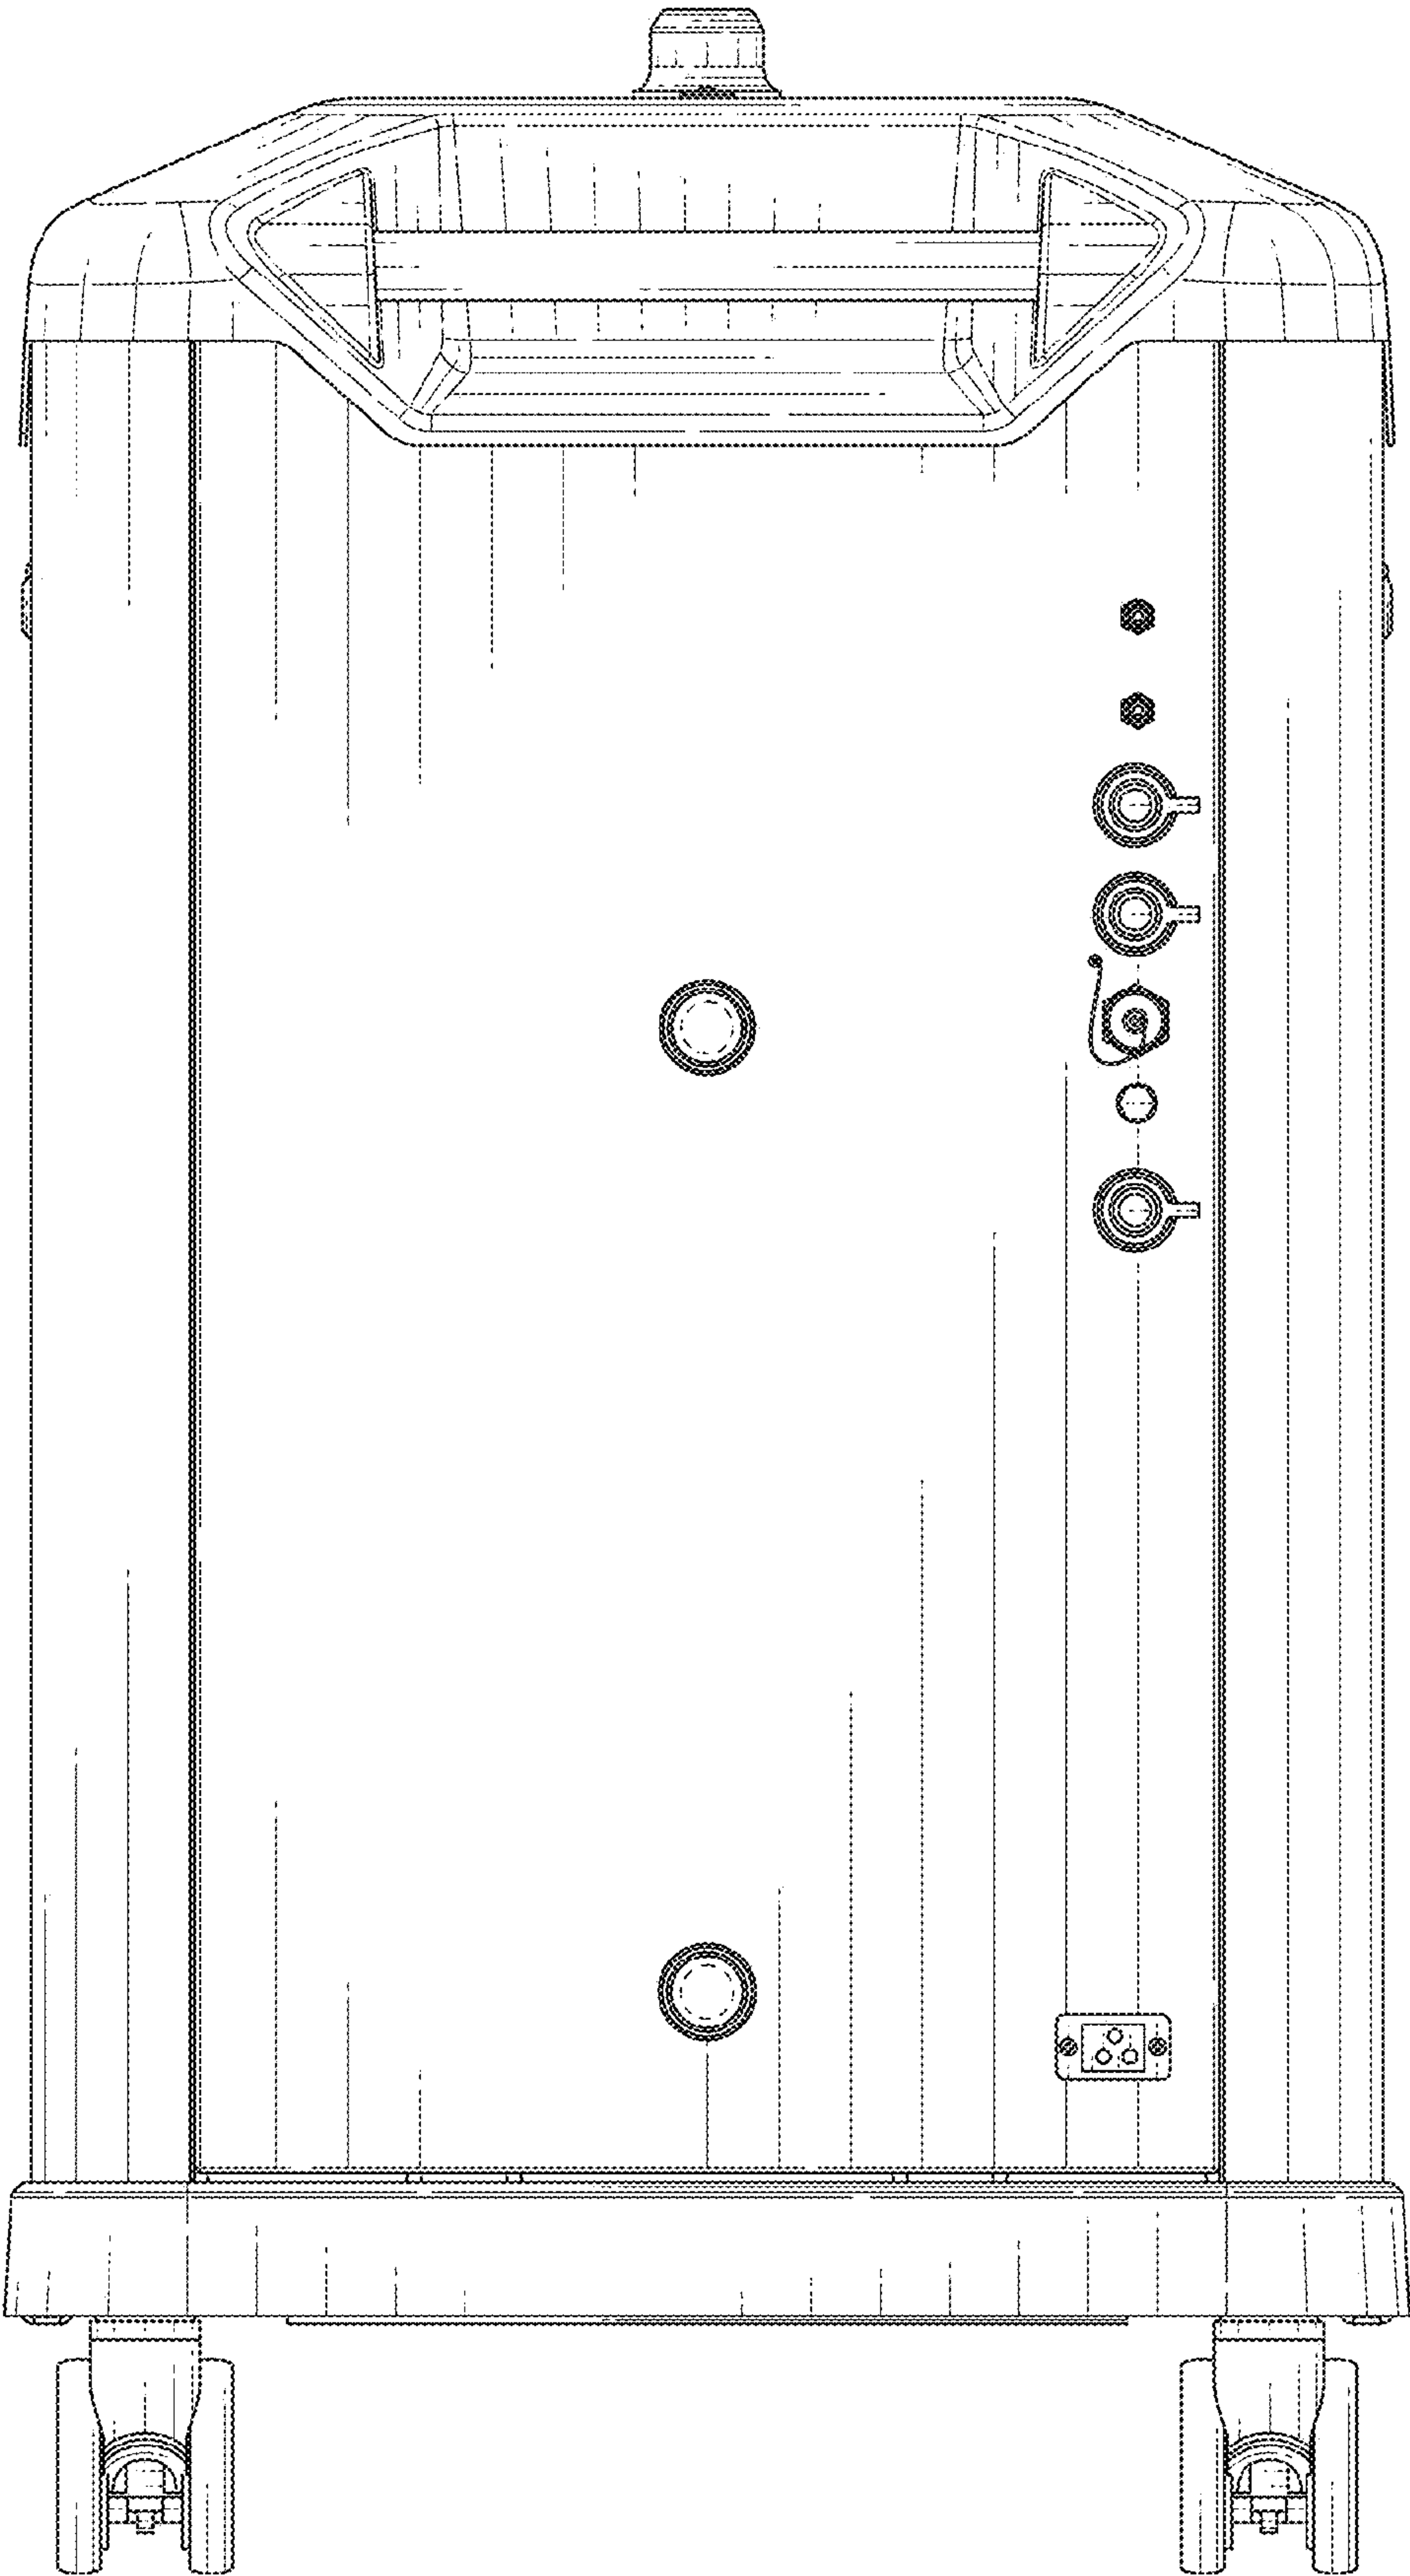


FIG. 10

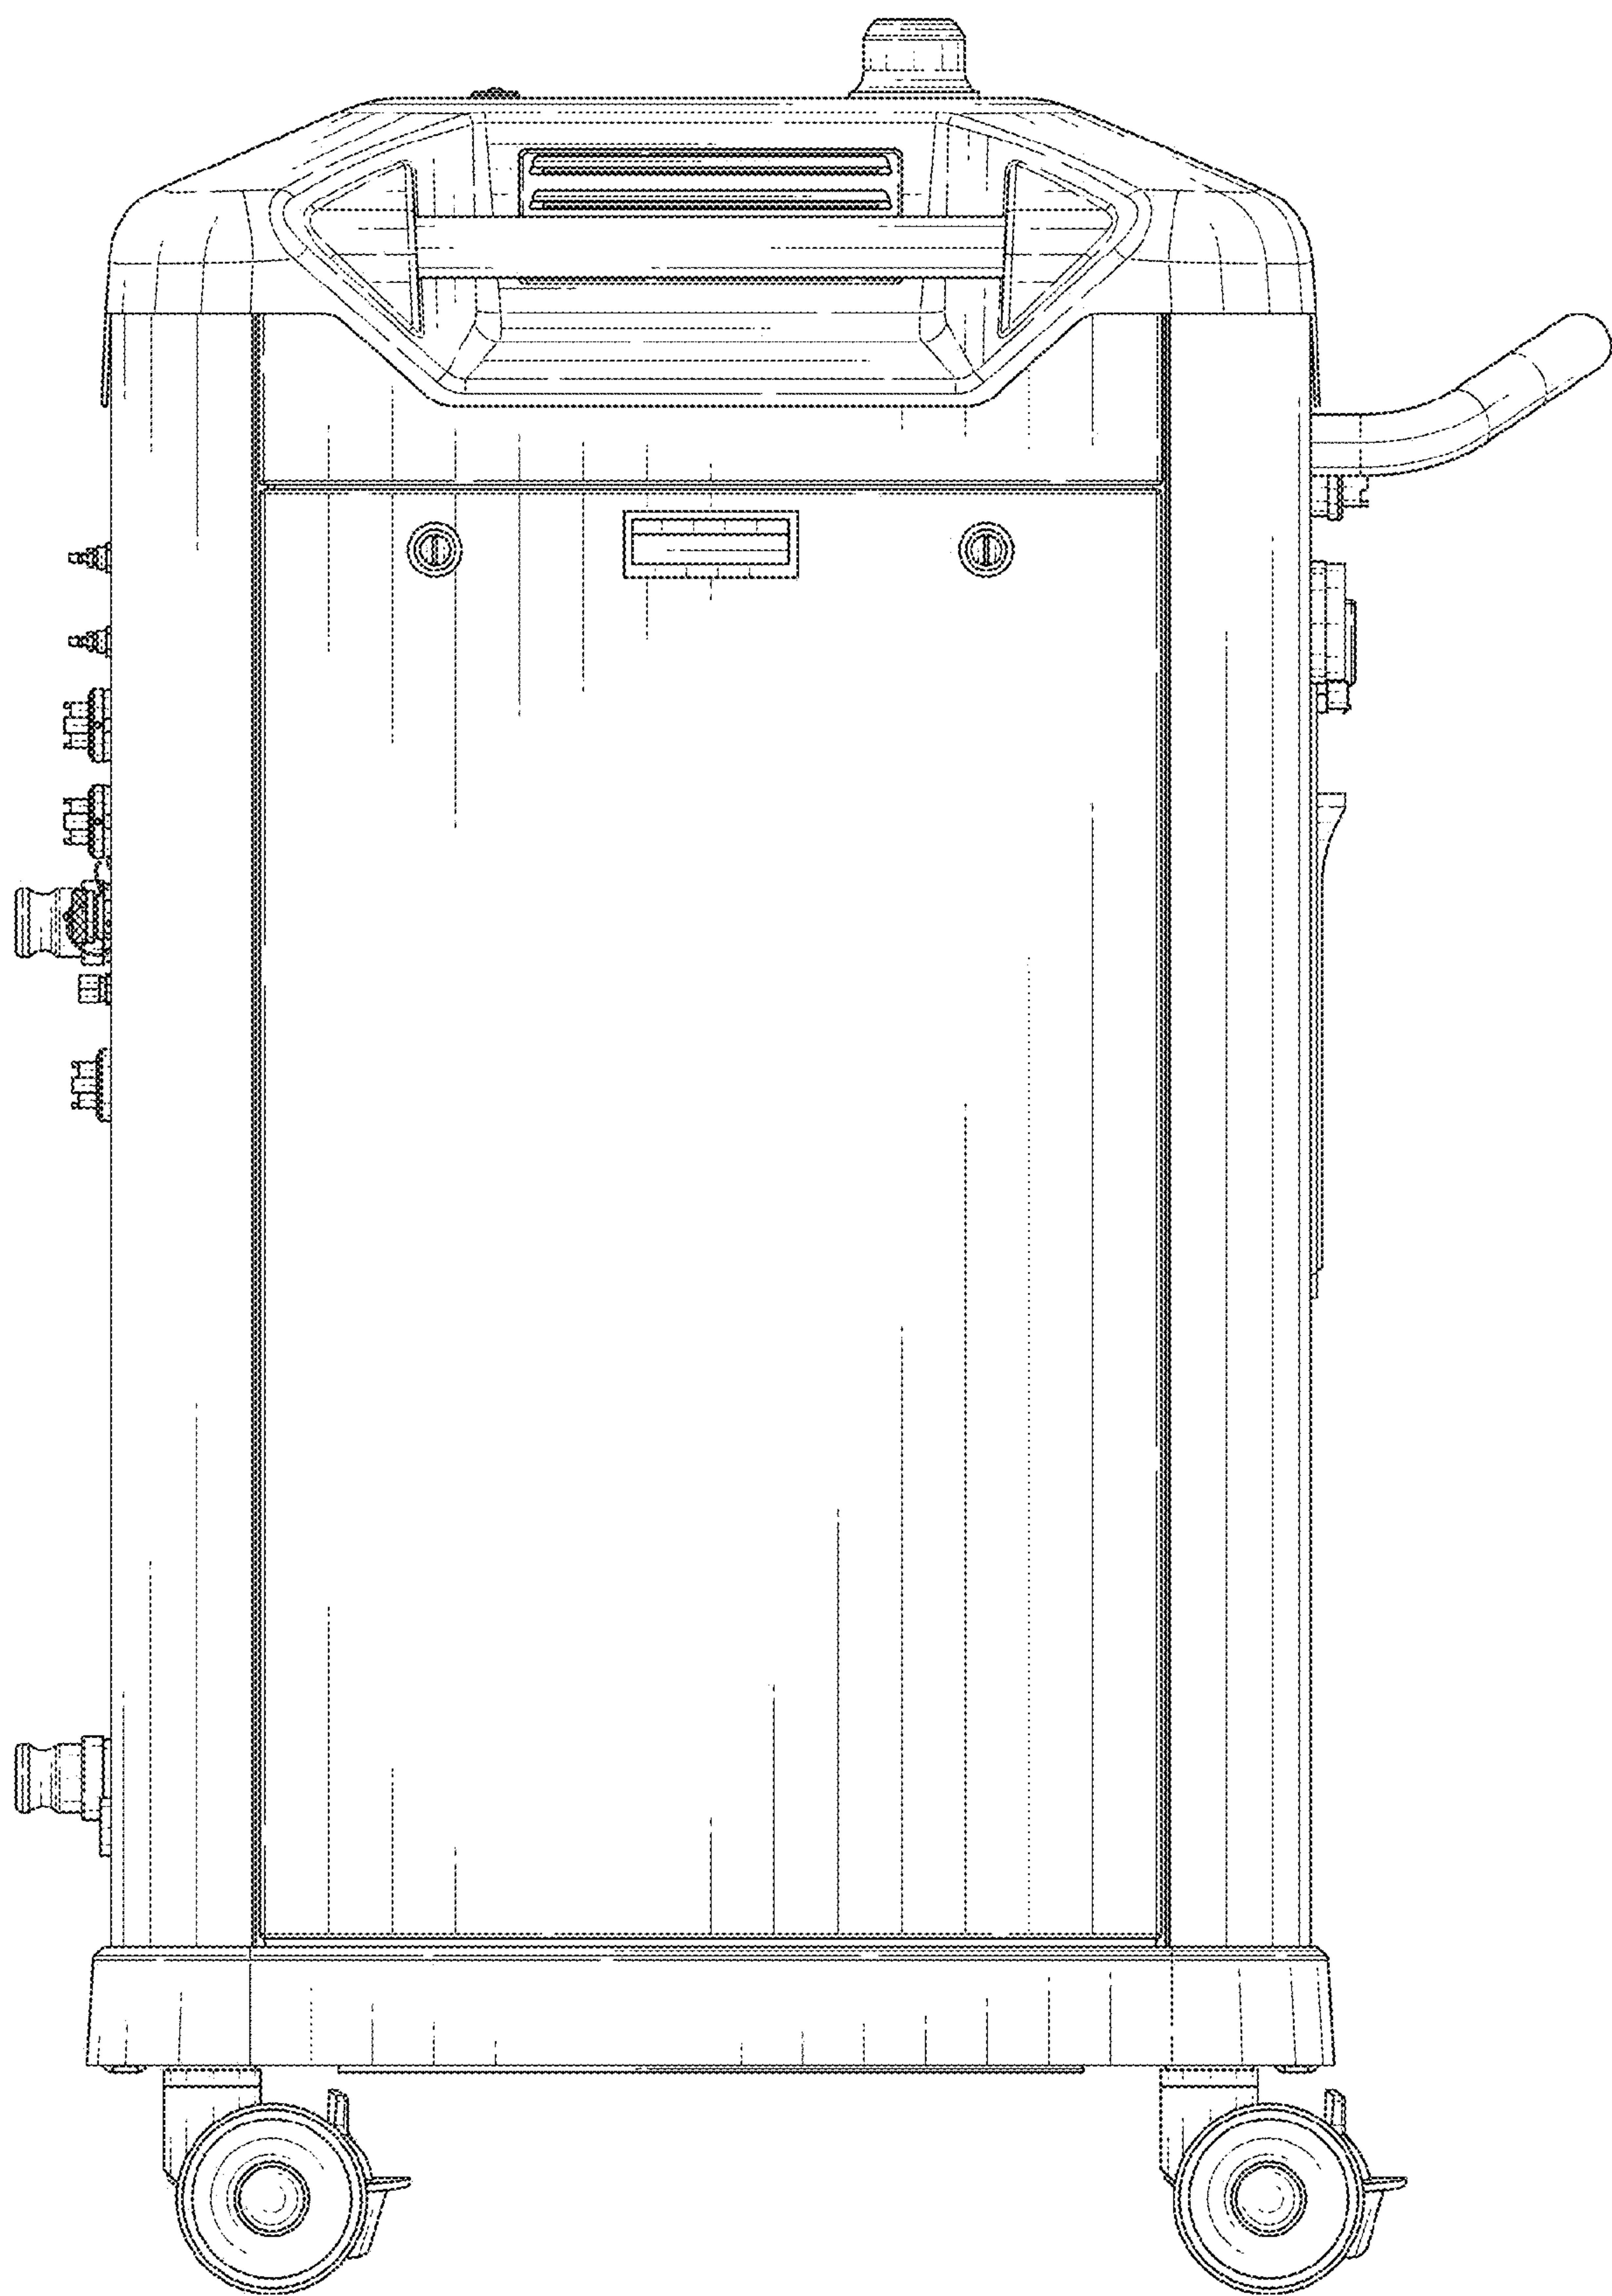


FIG. 11

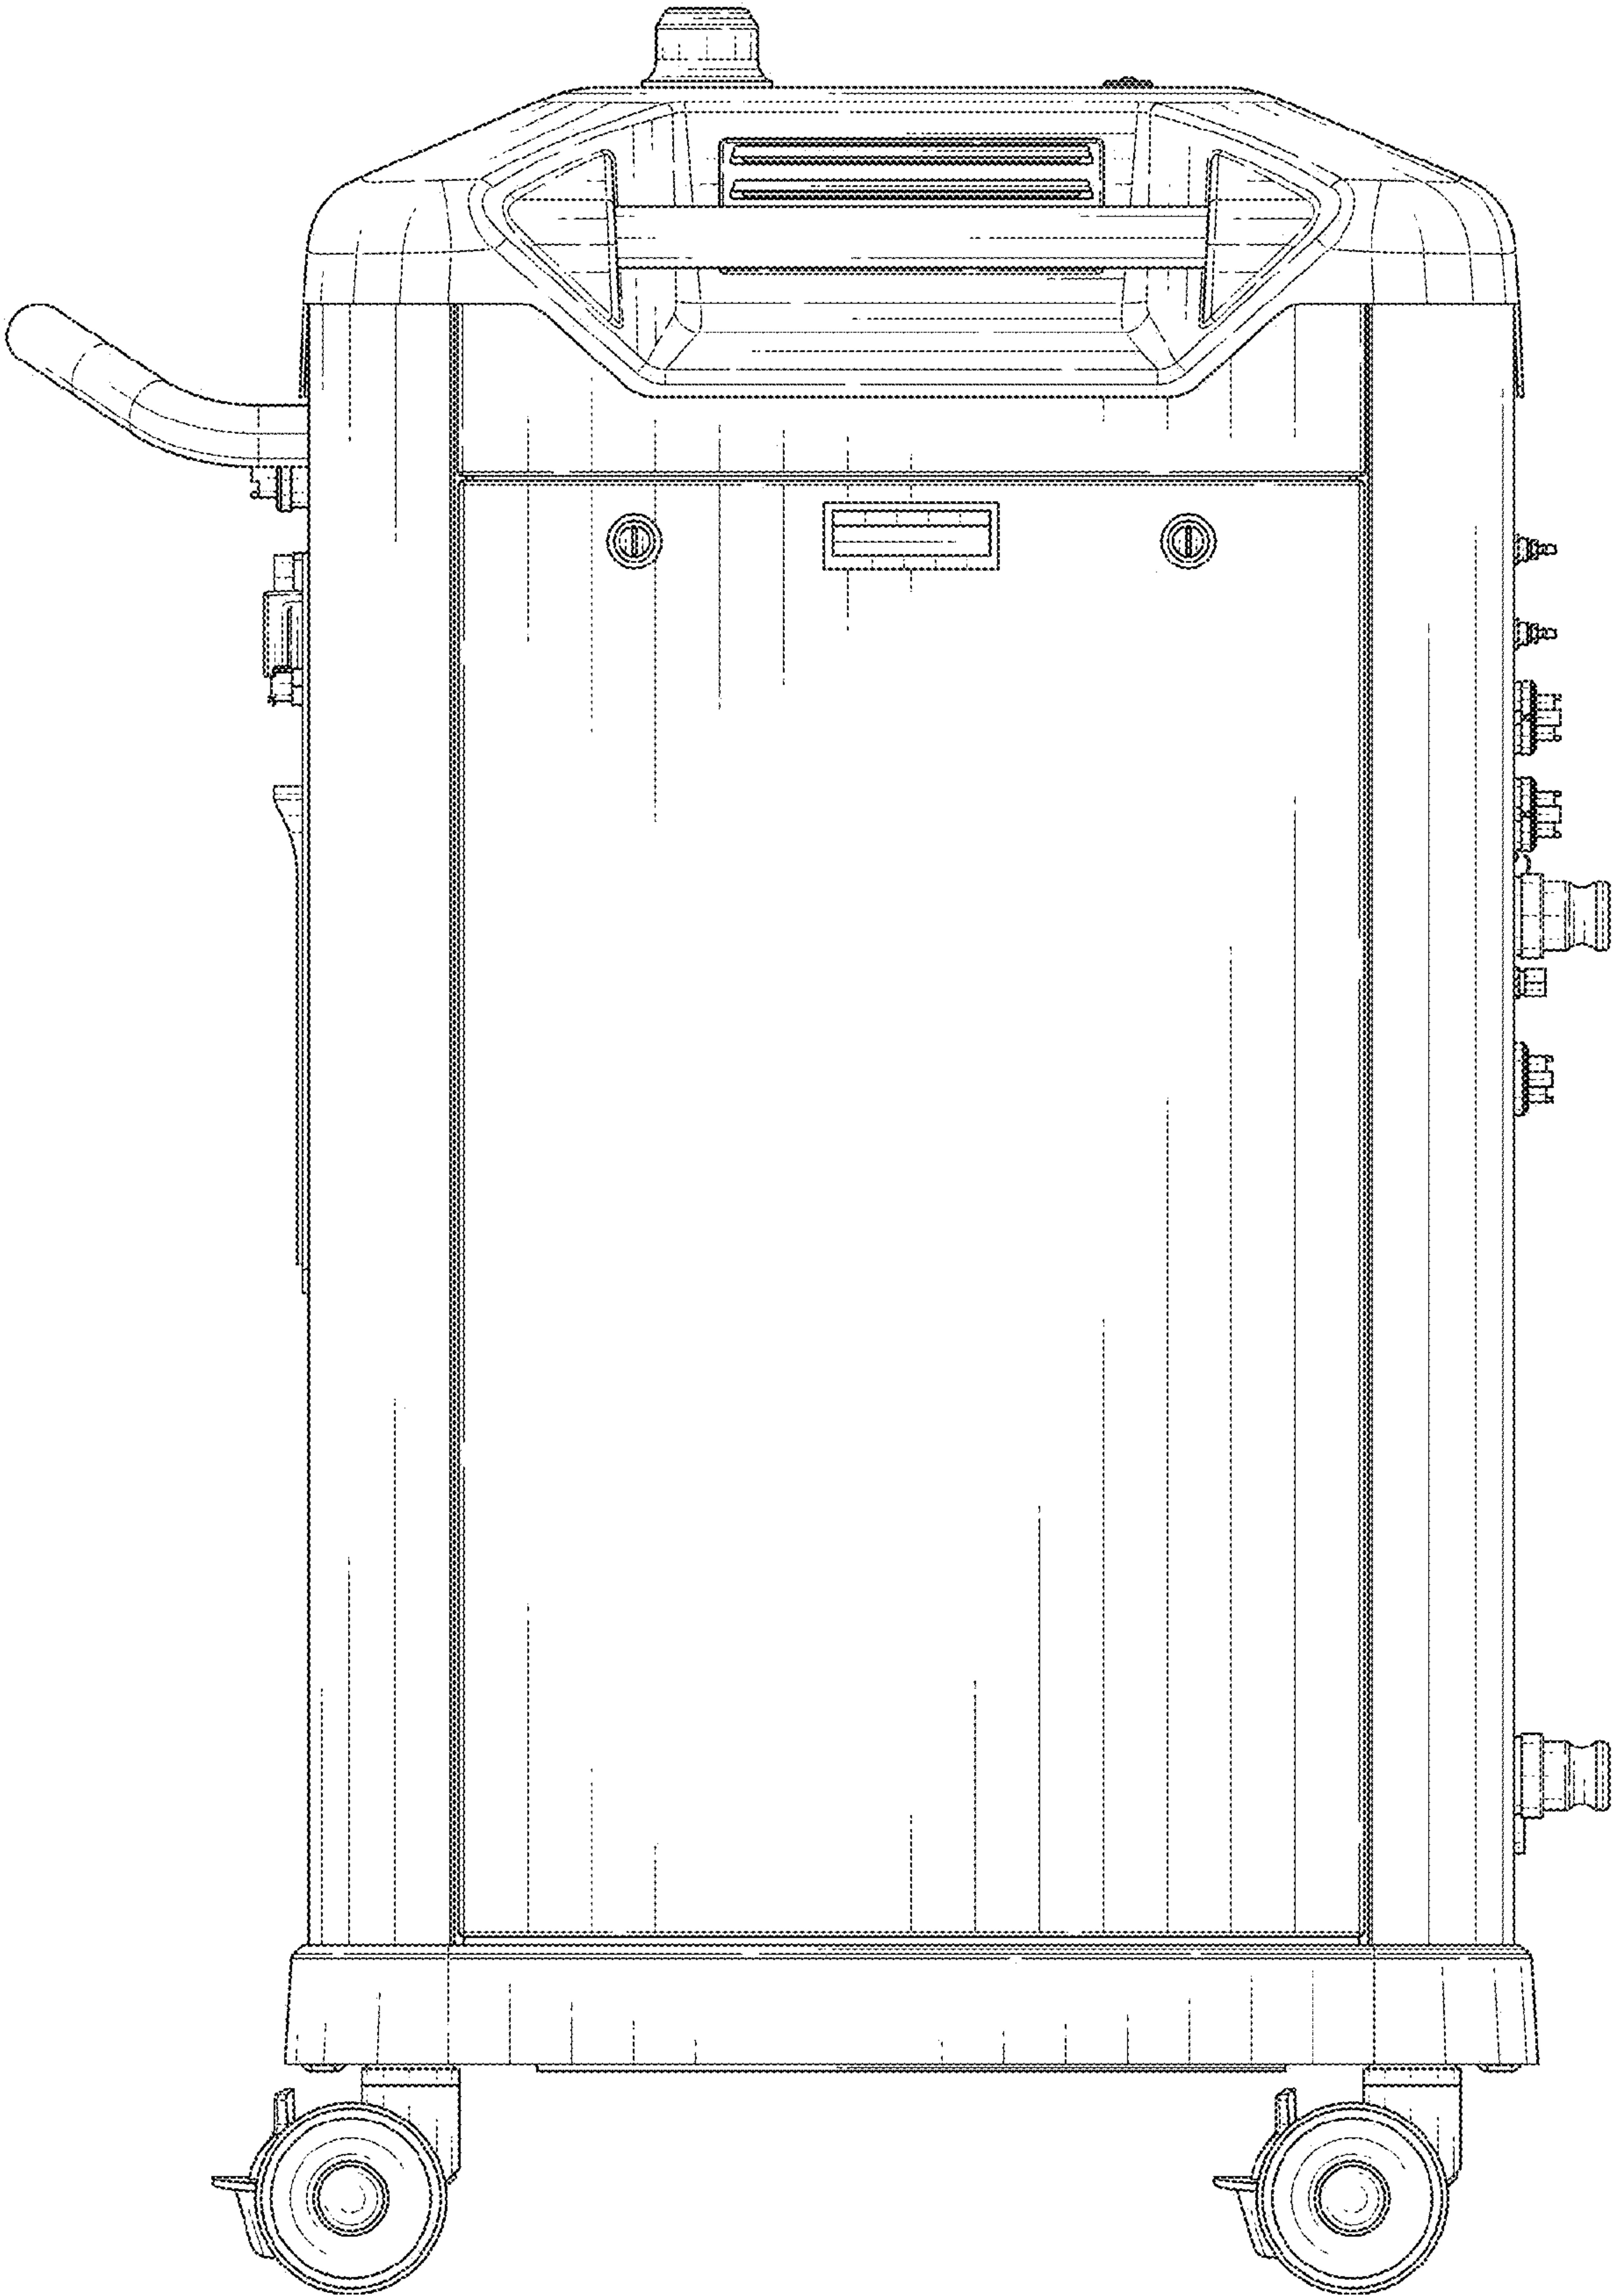


FIG. 12

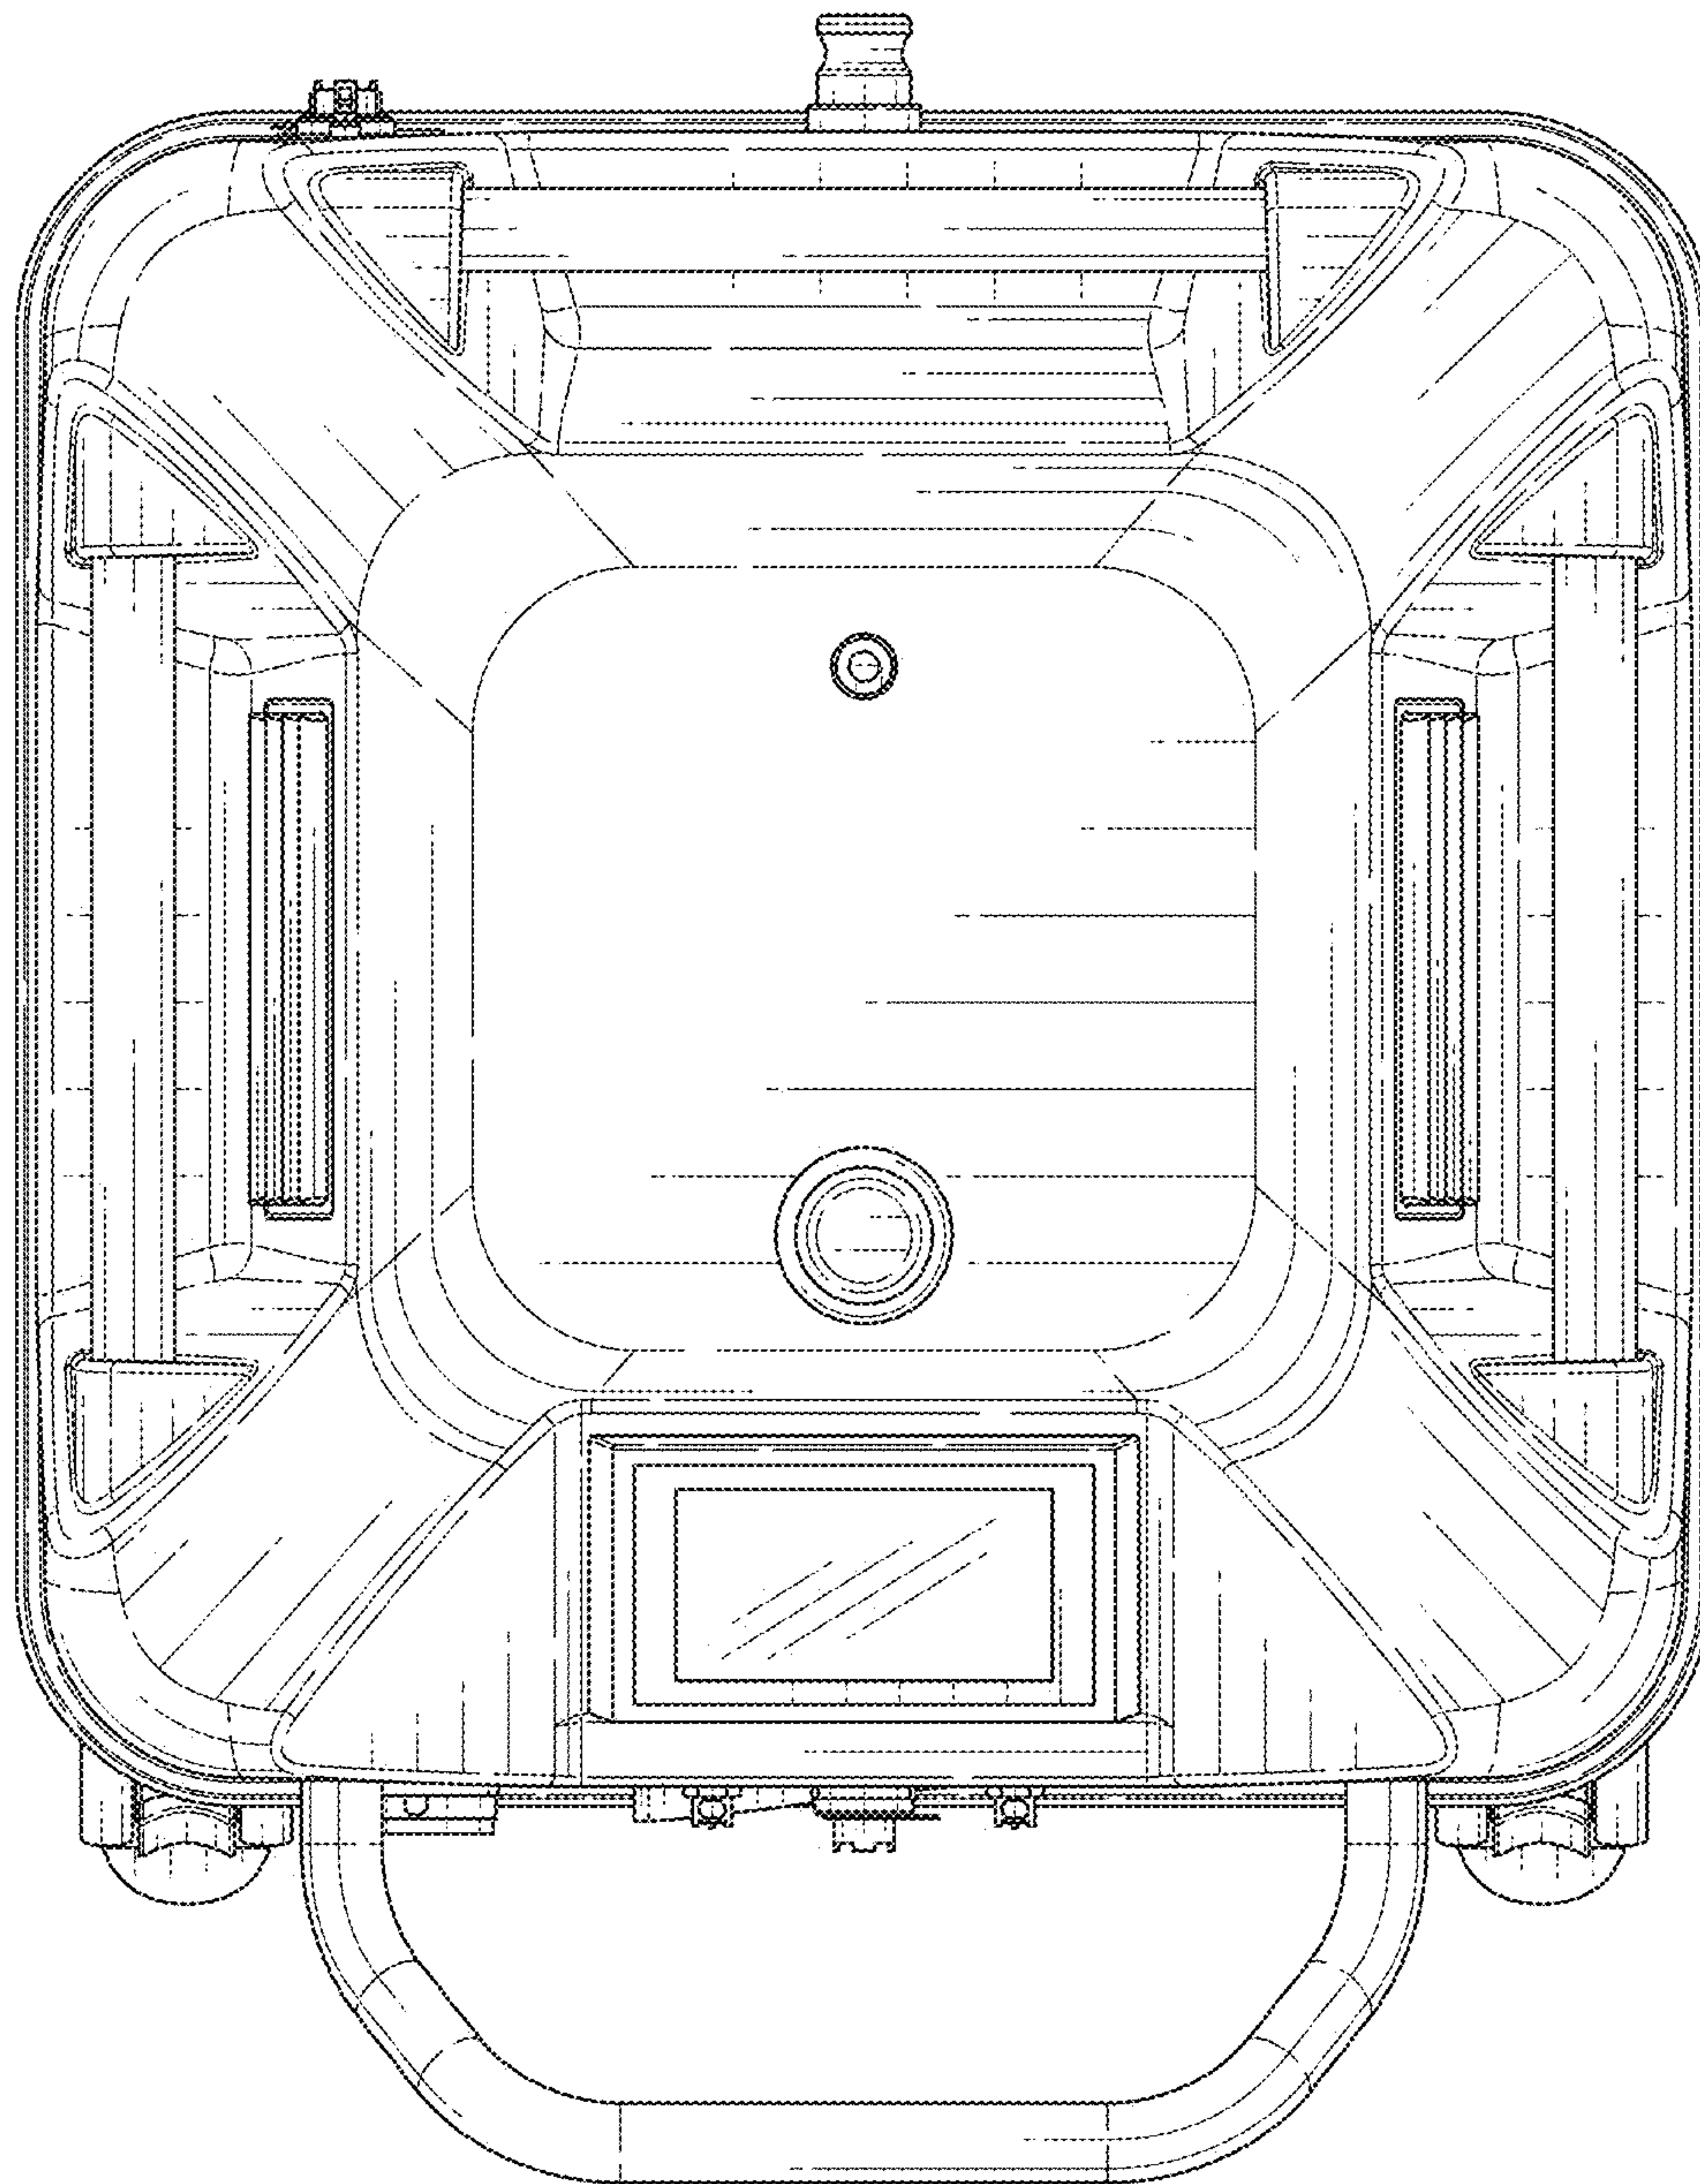


FIG. 13

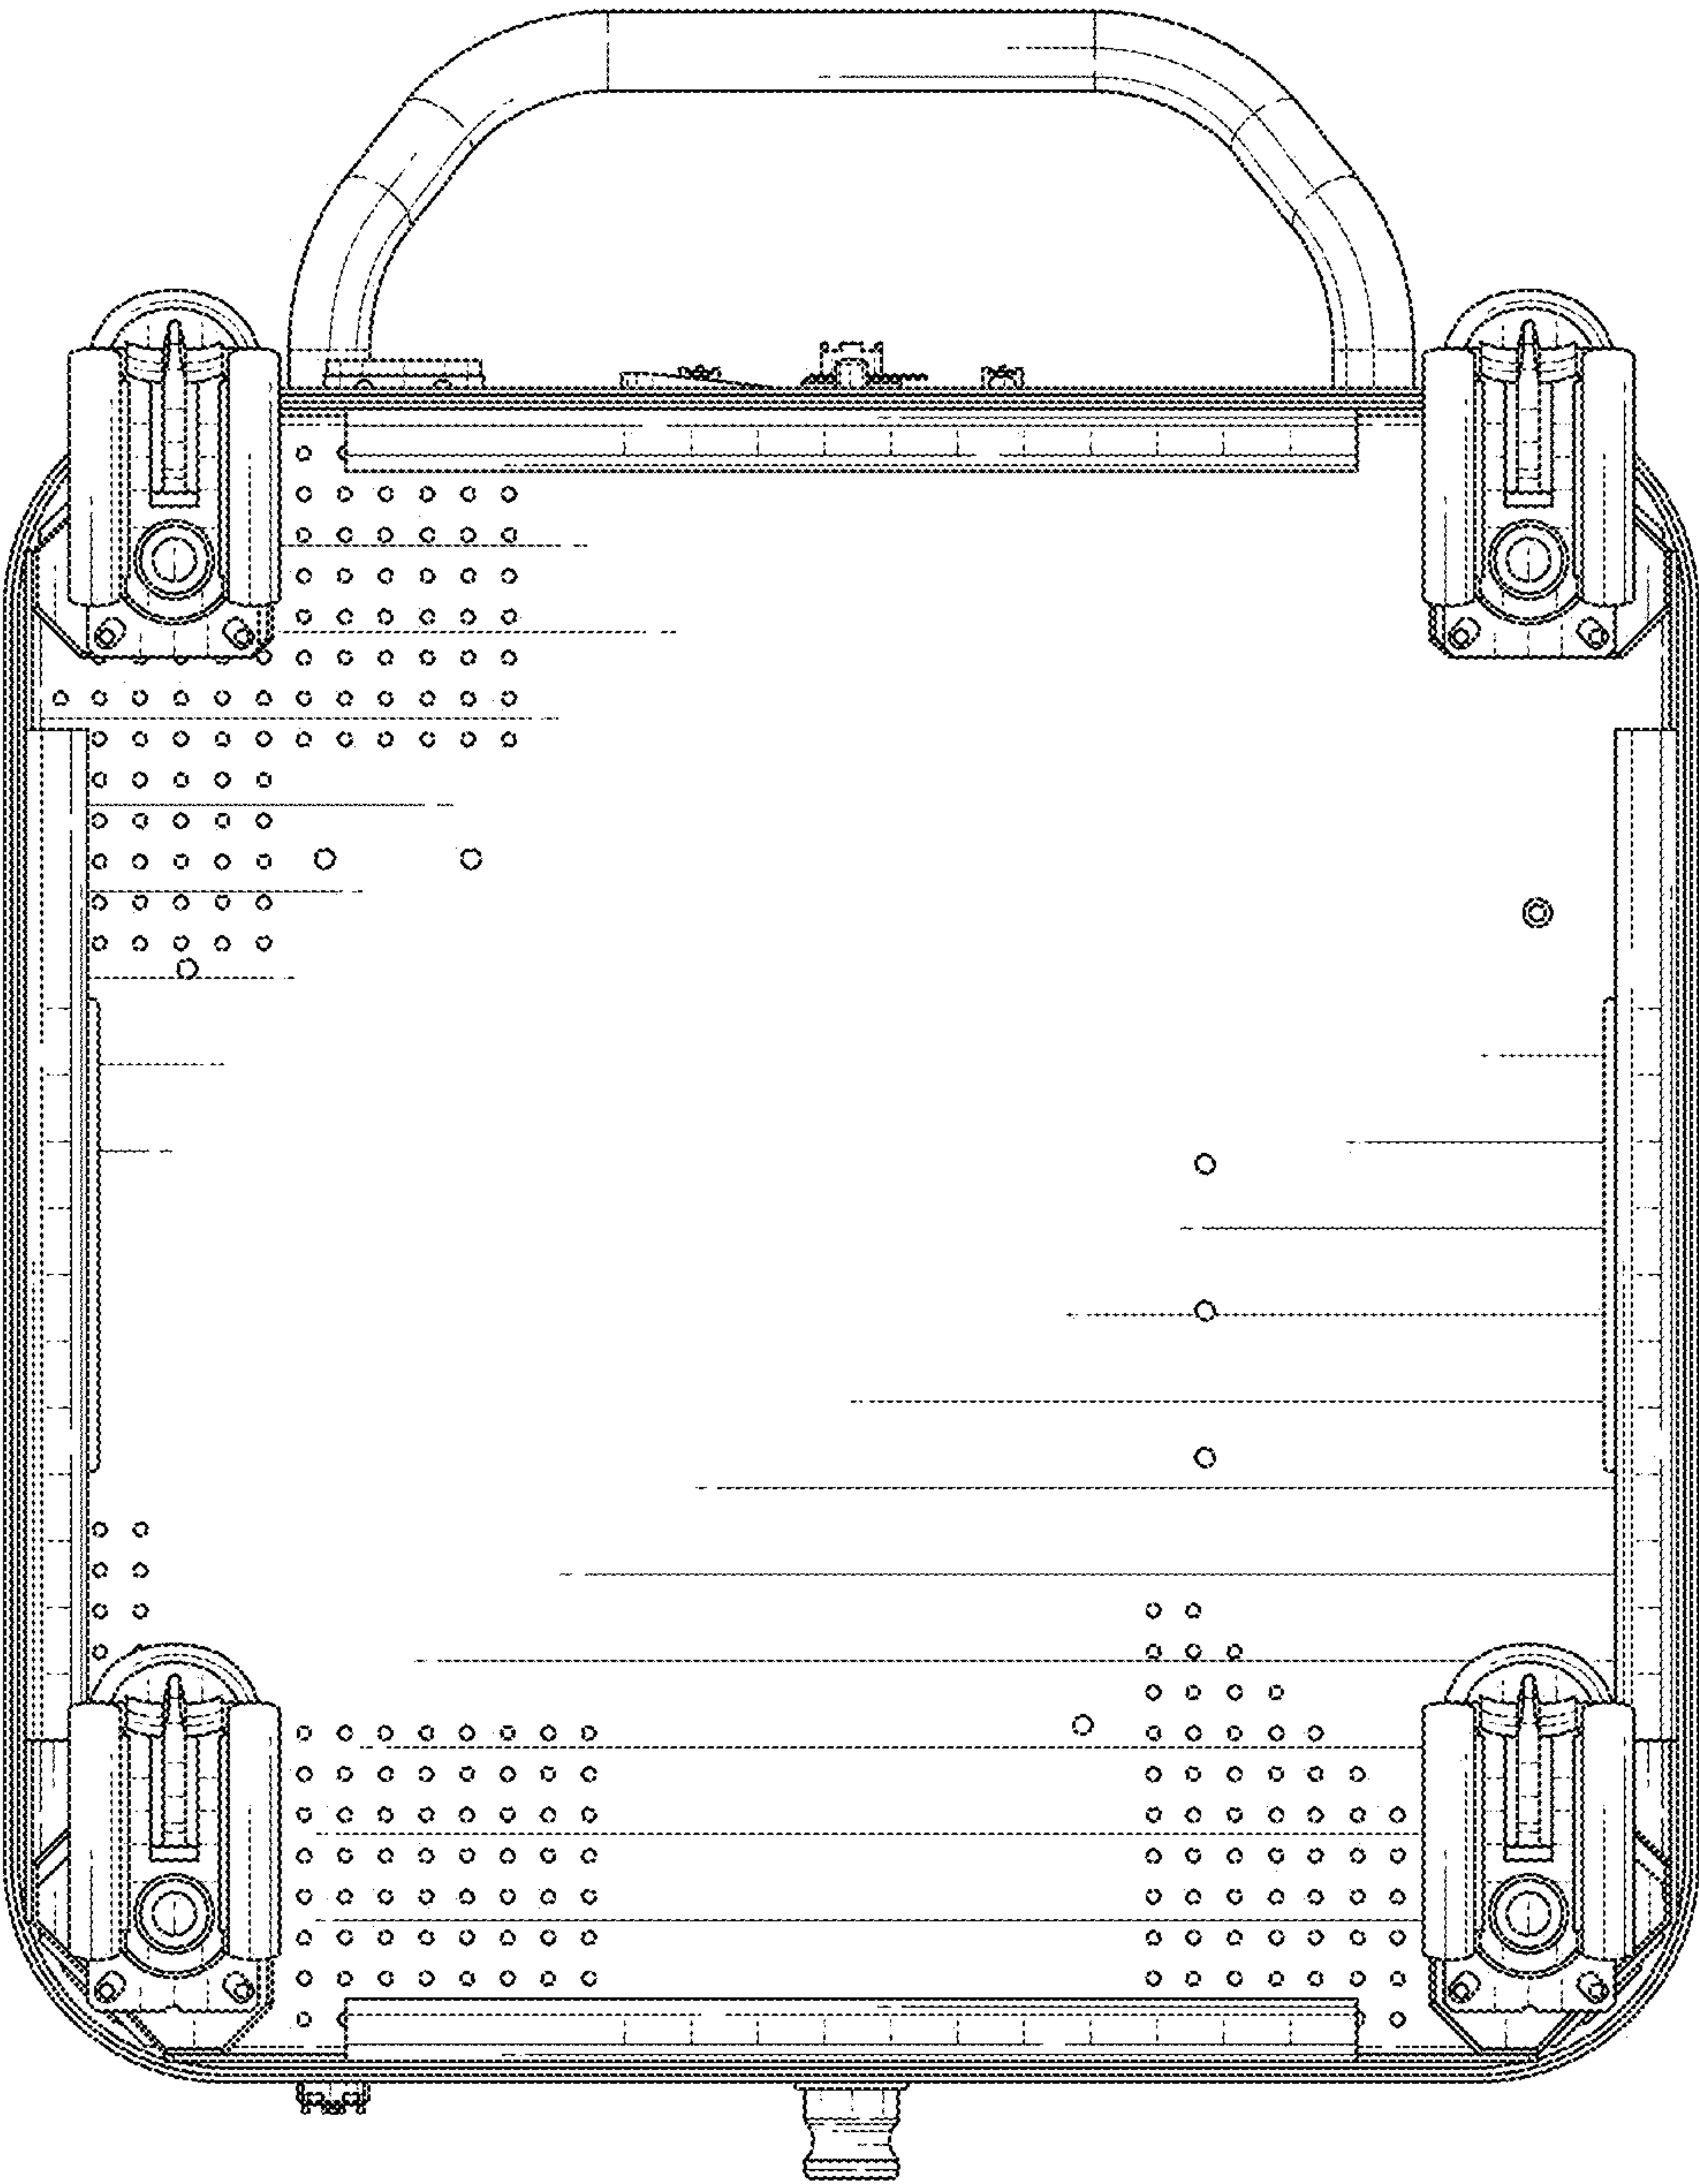


FIG. 14

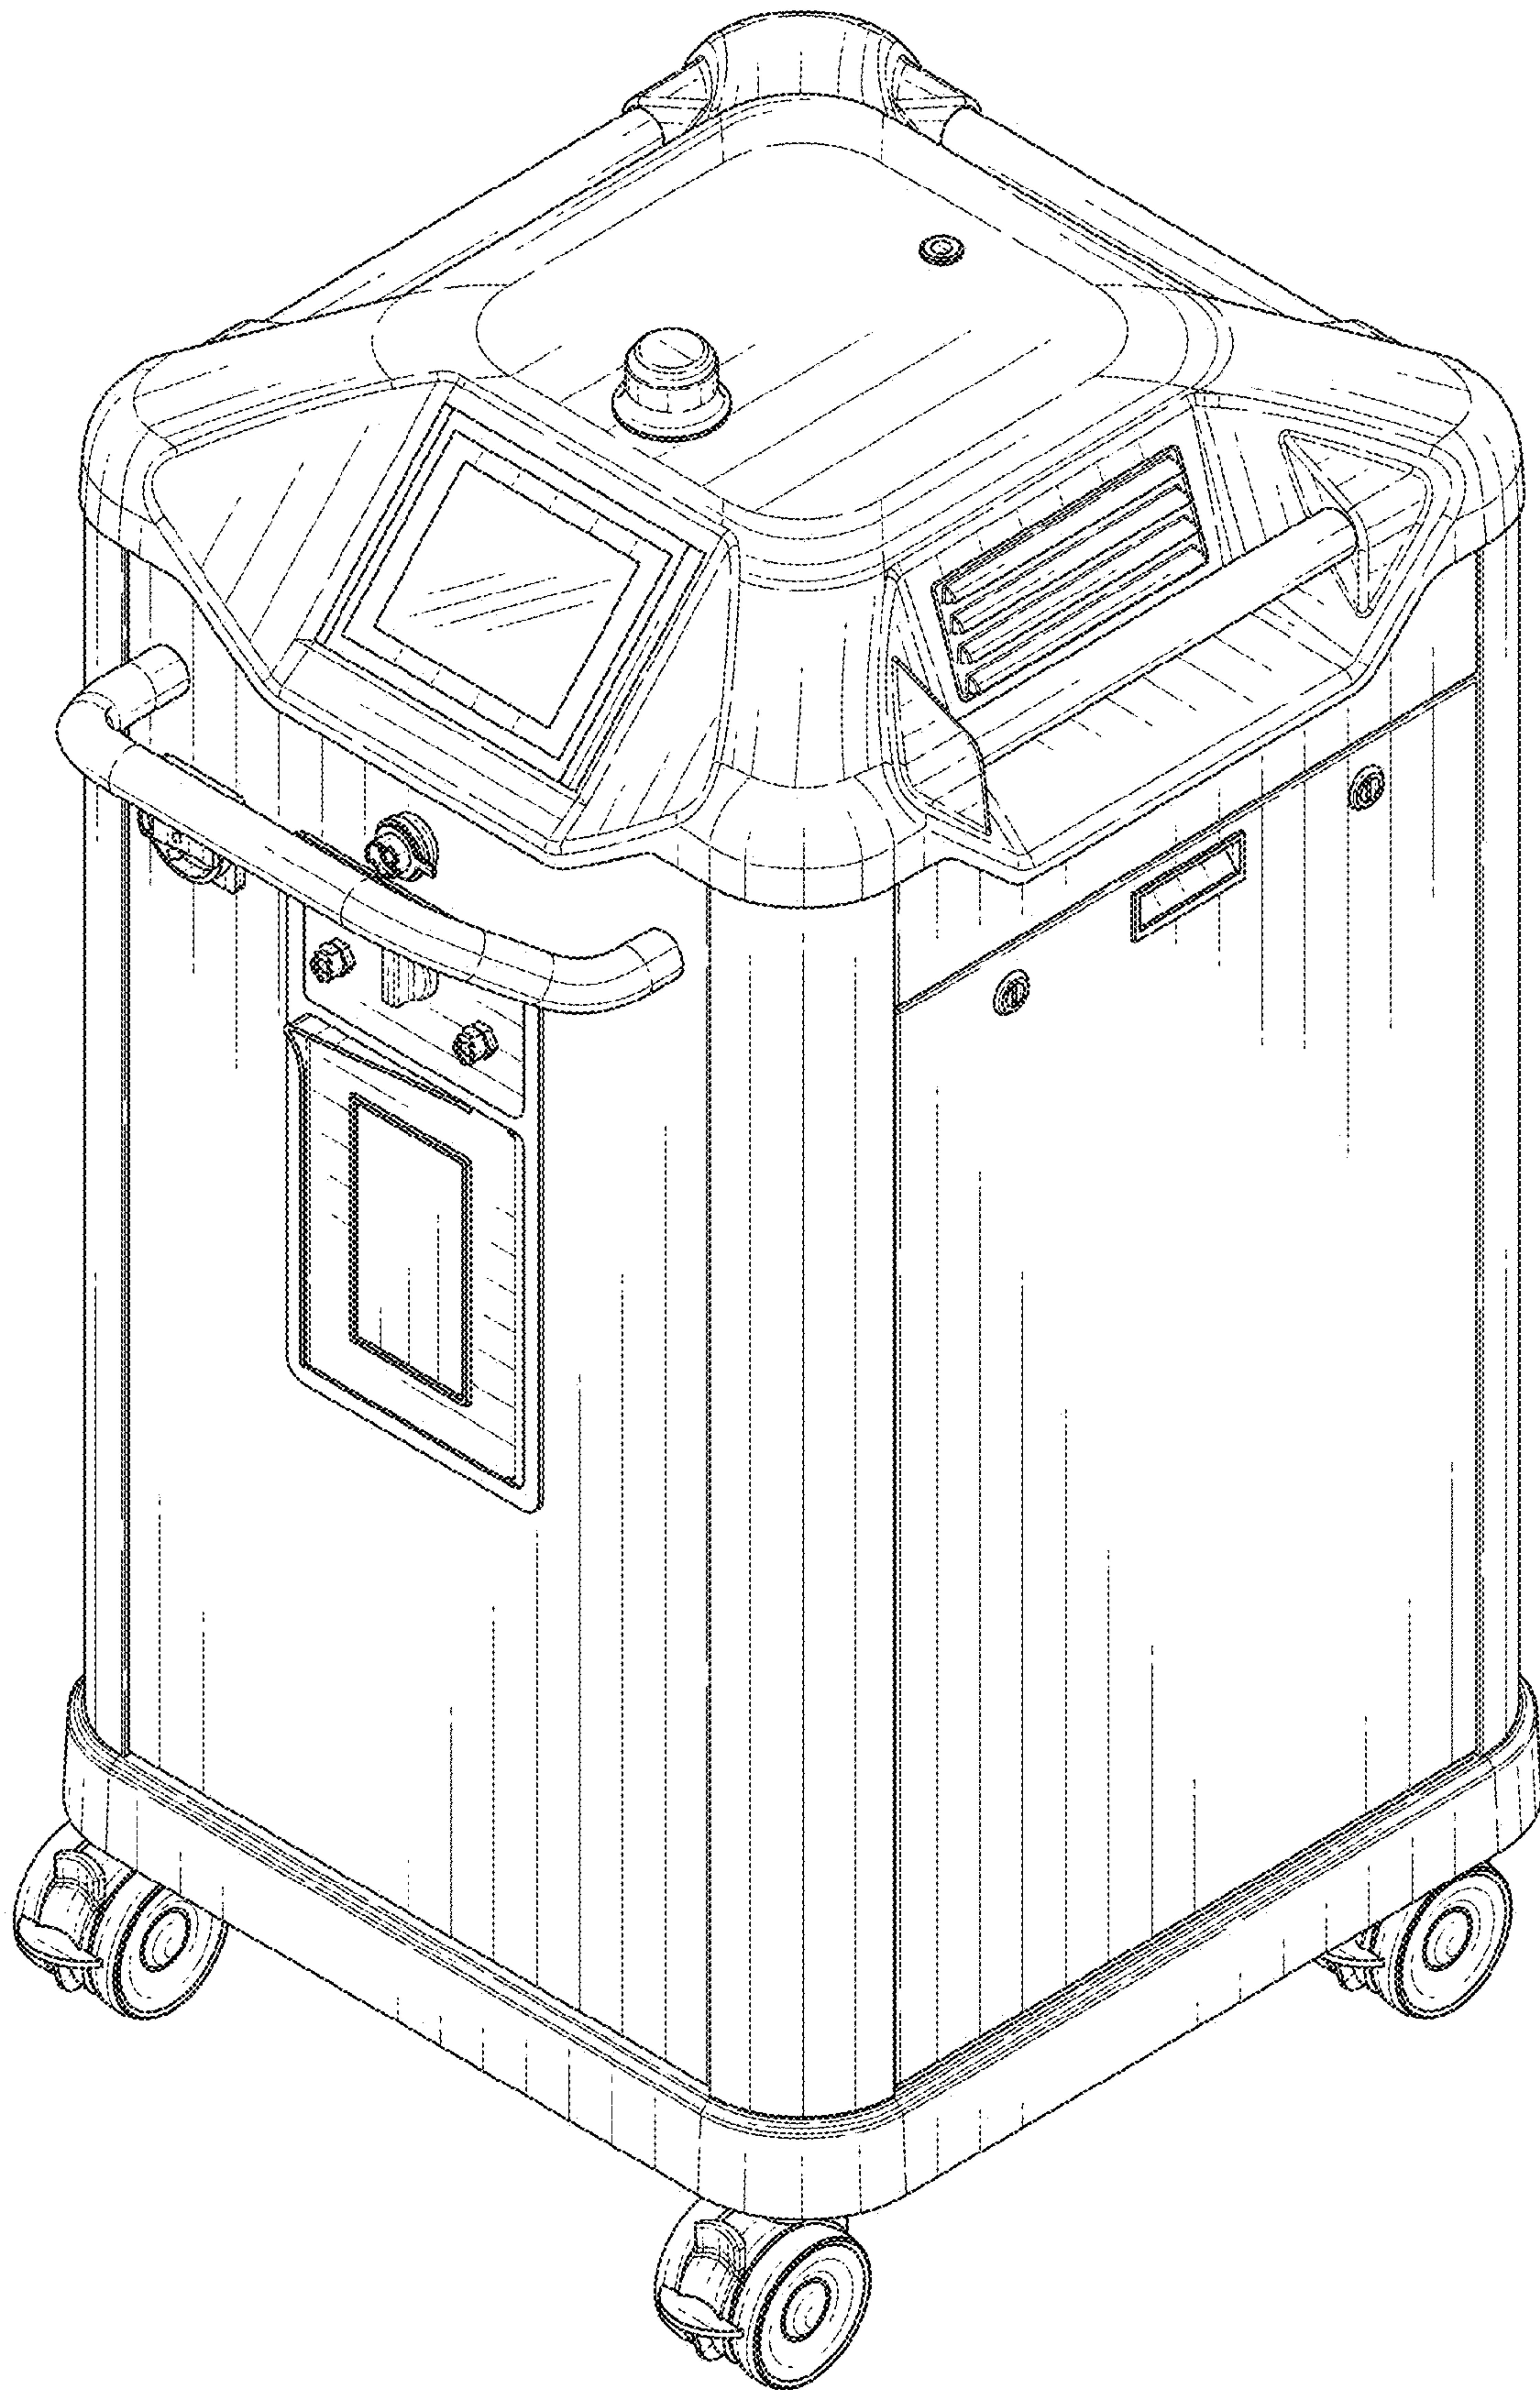


FIG. 15

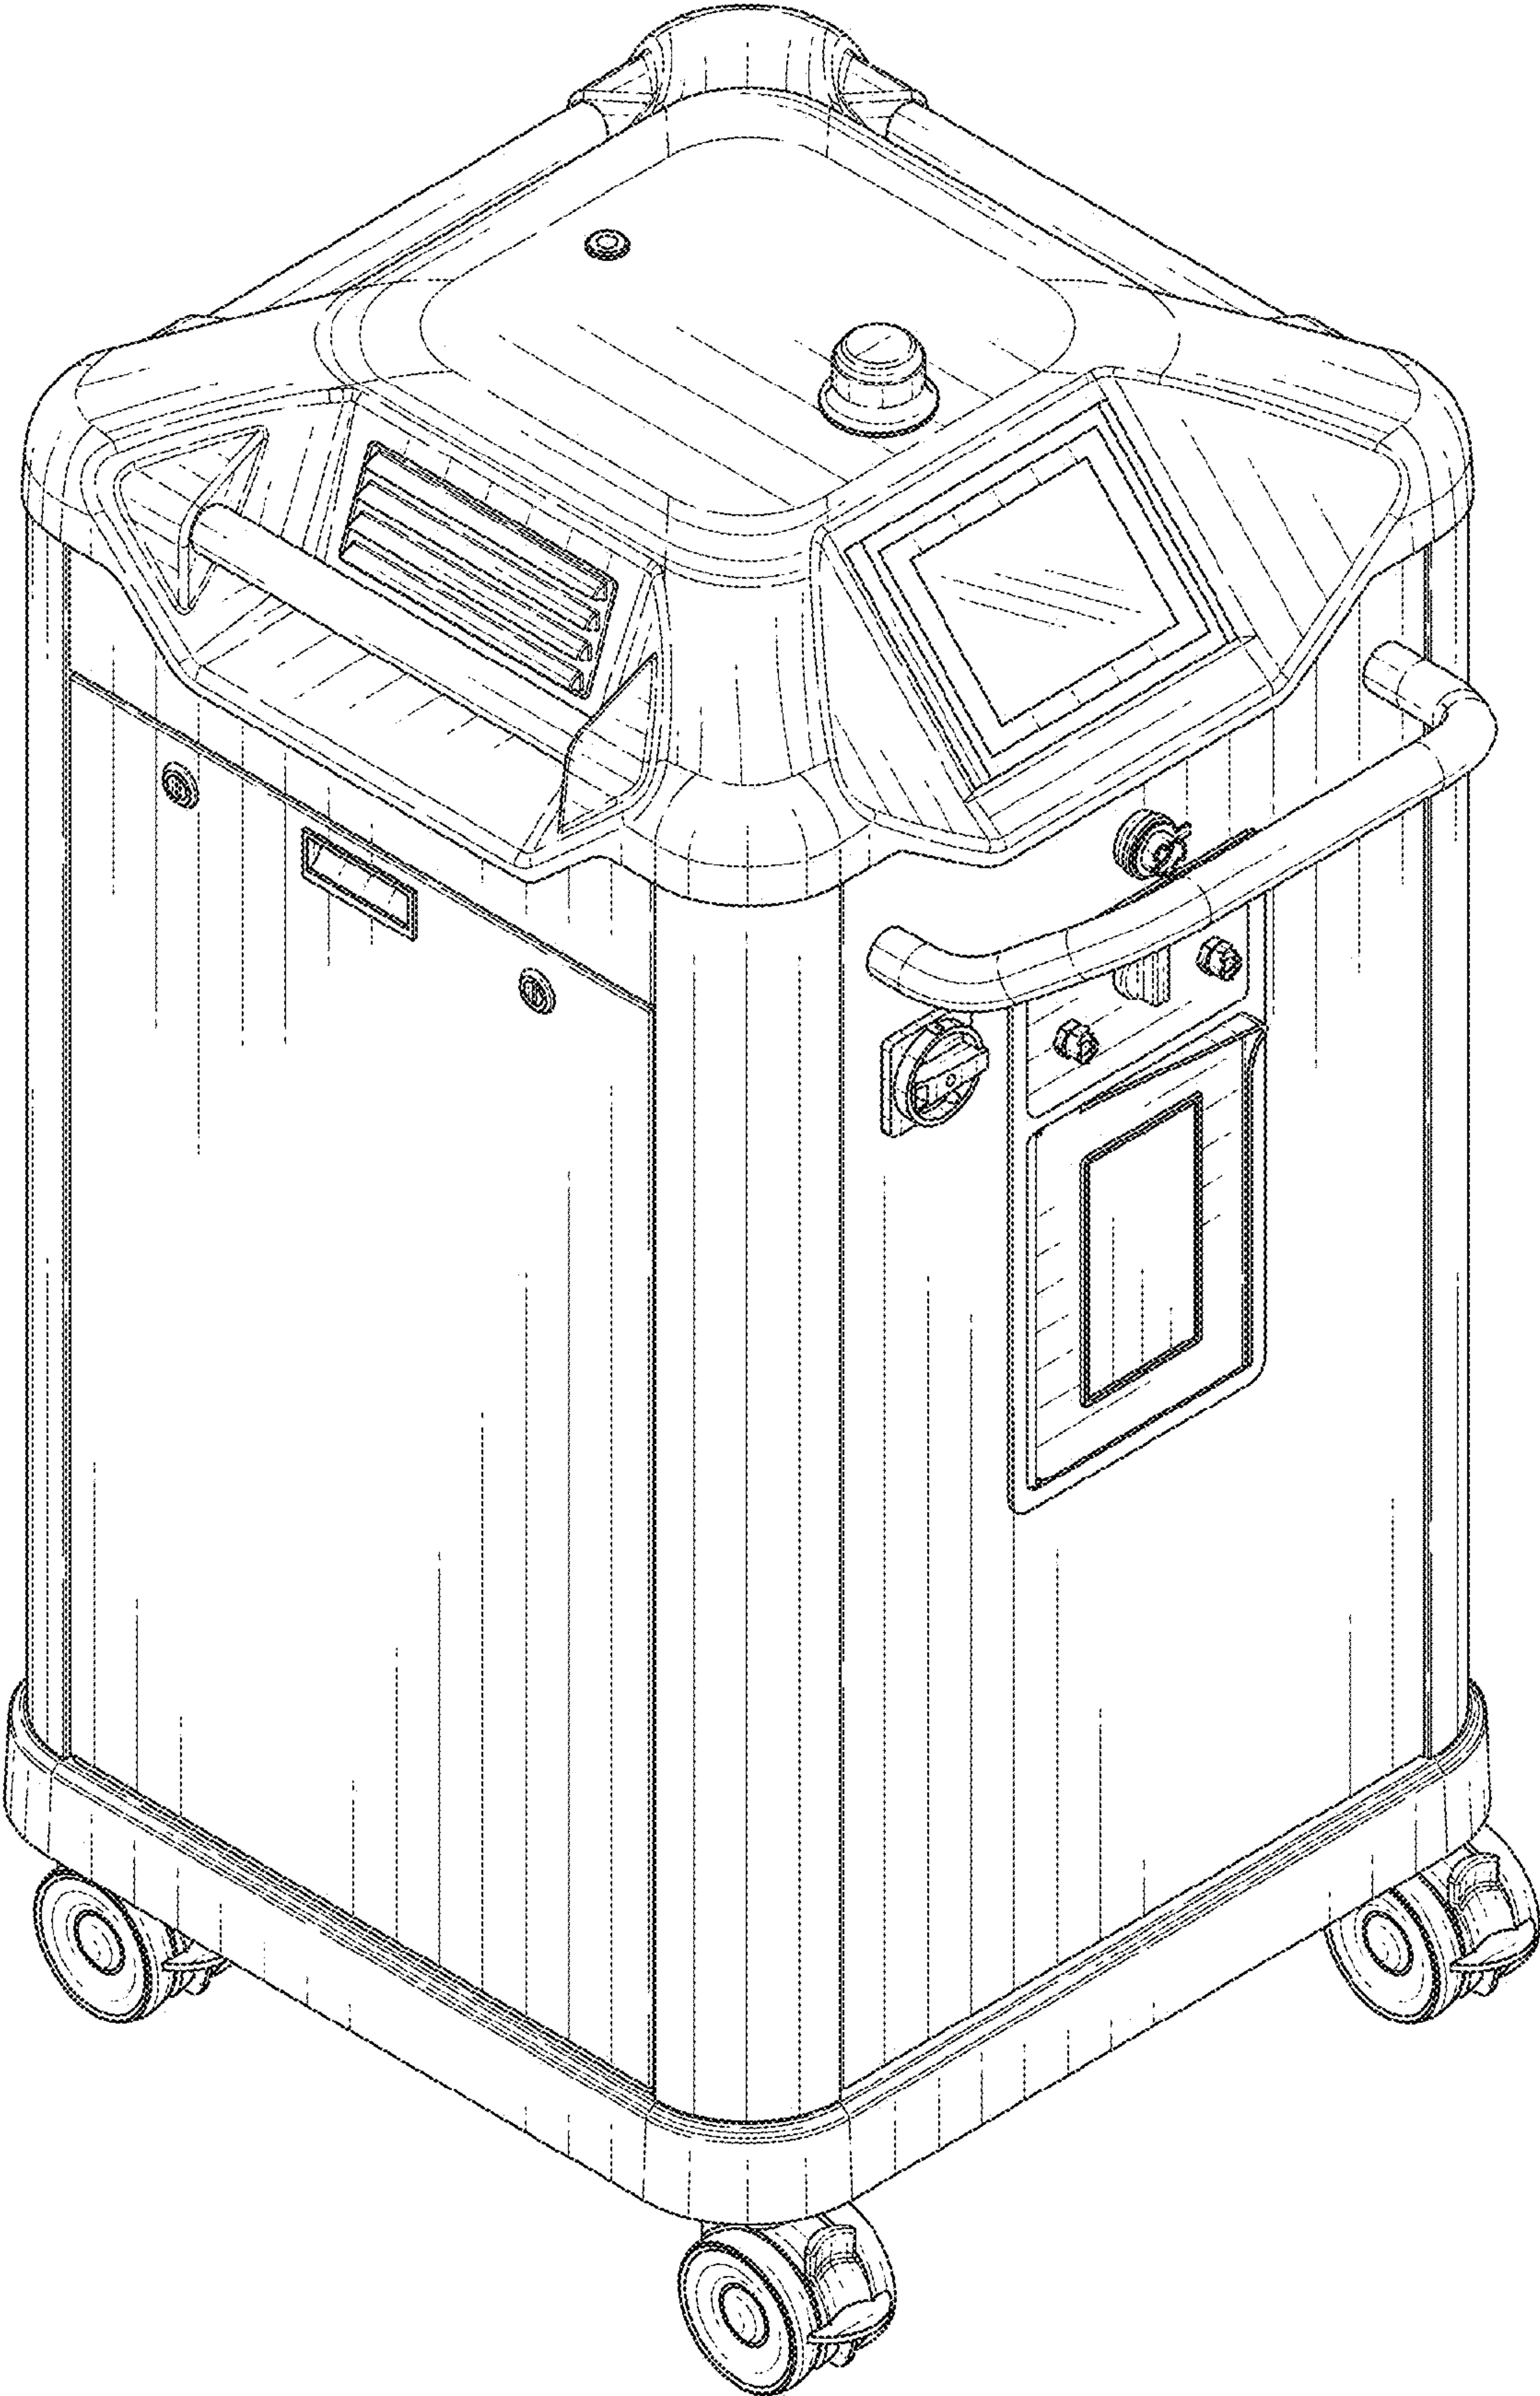


FIG. 16

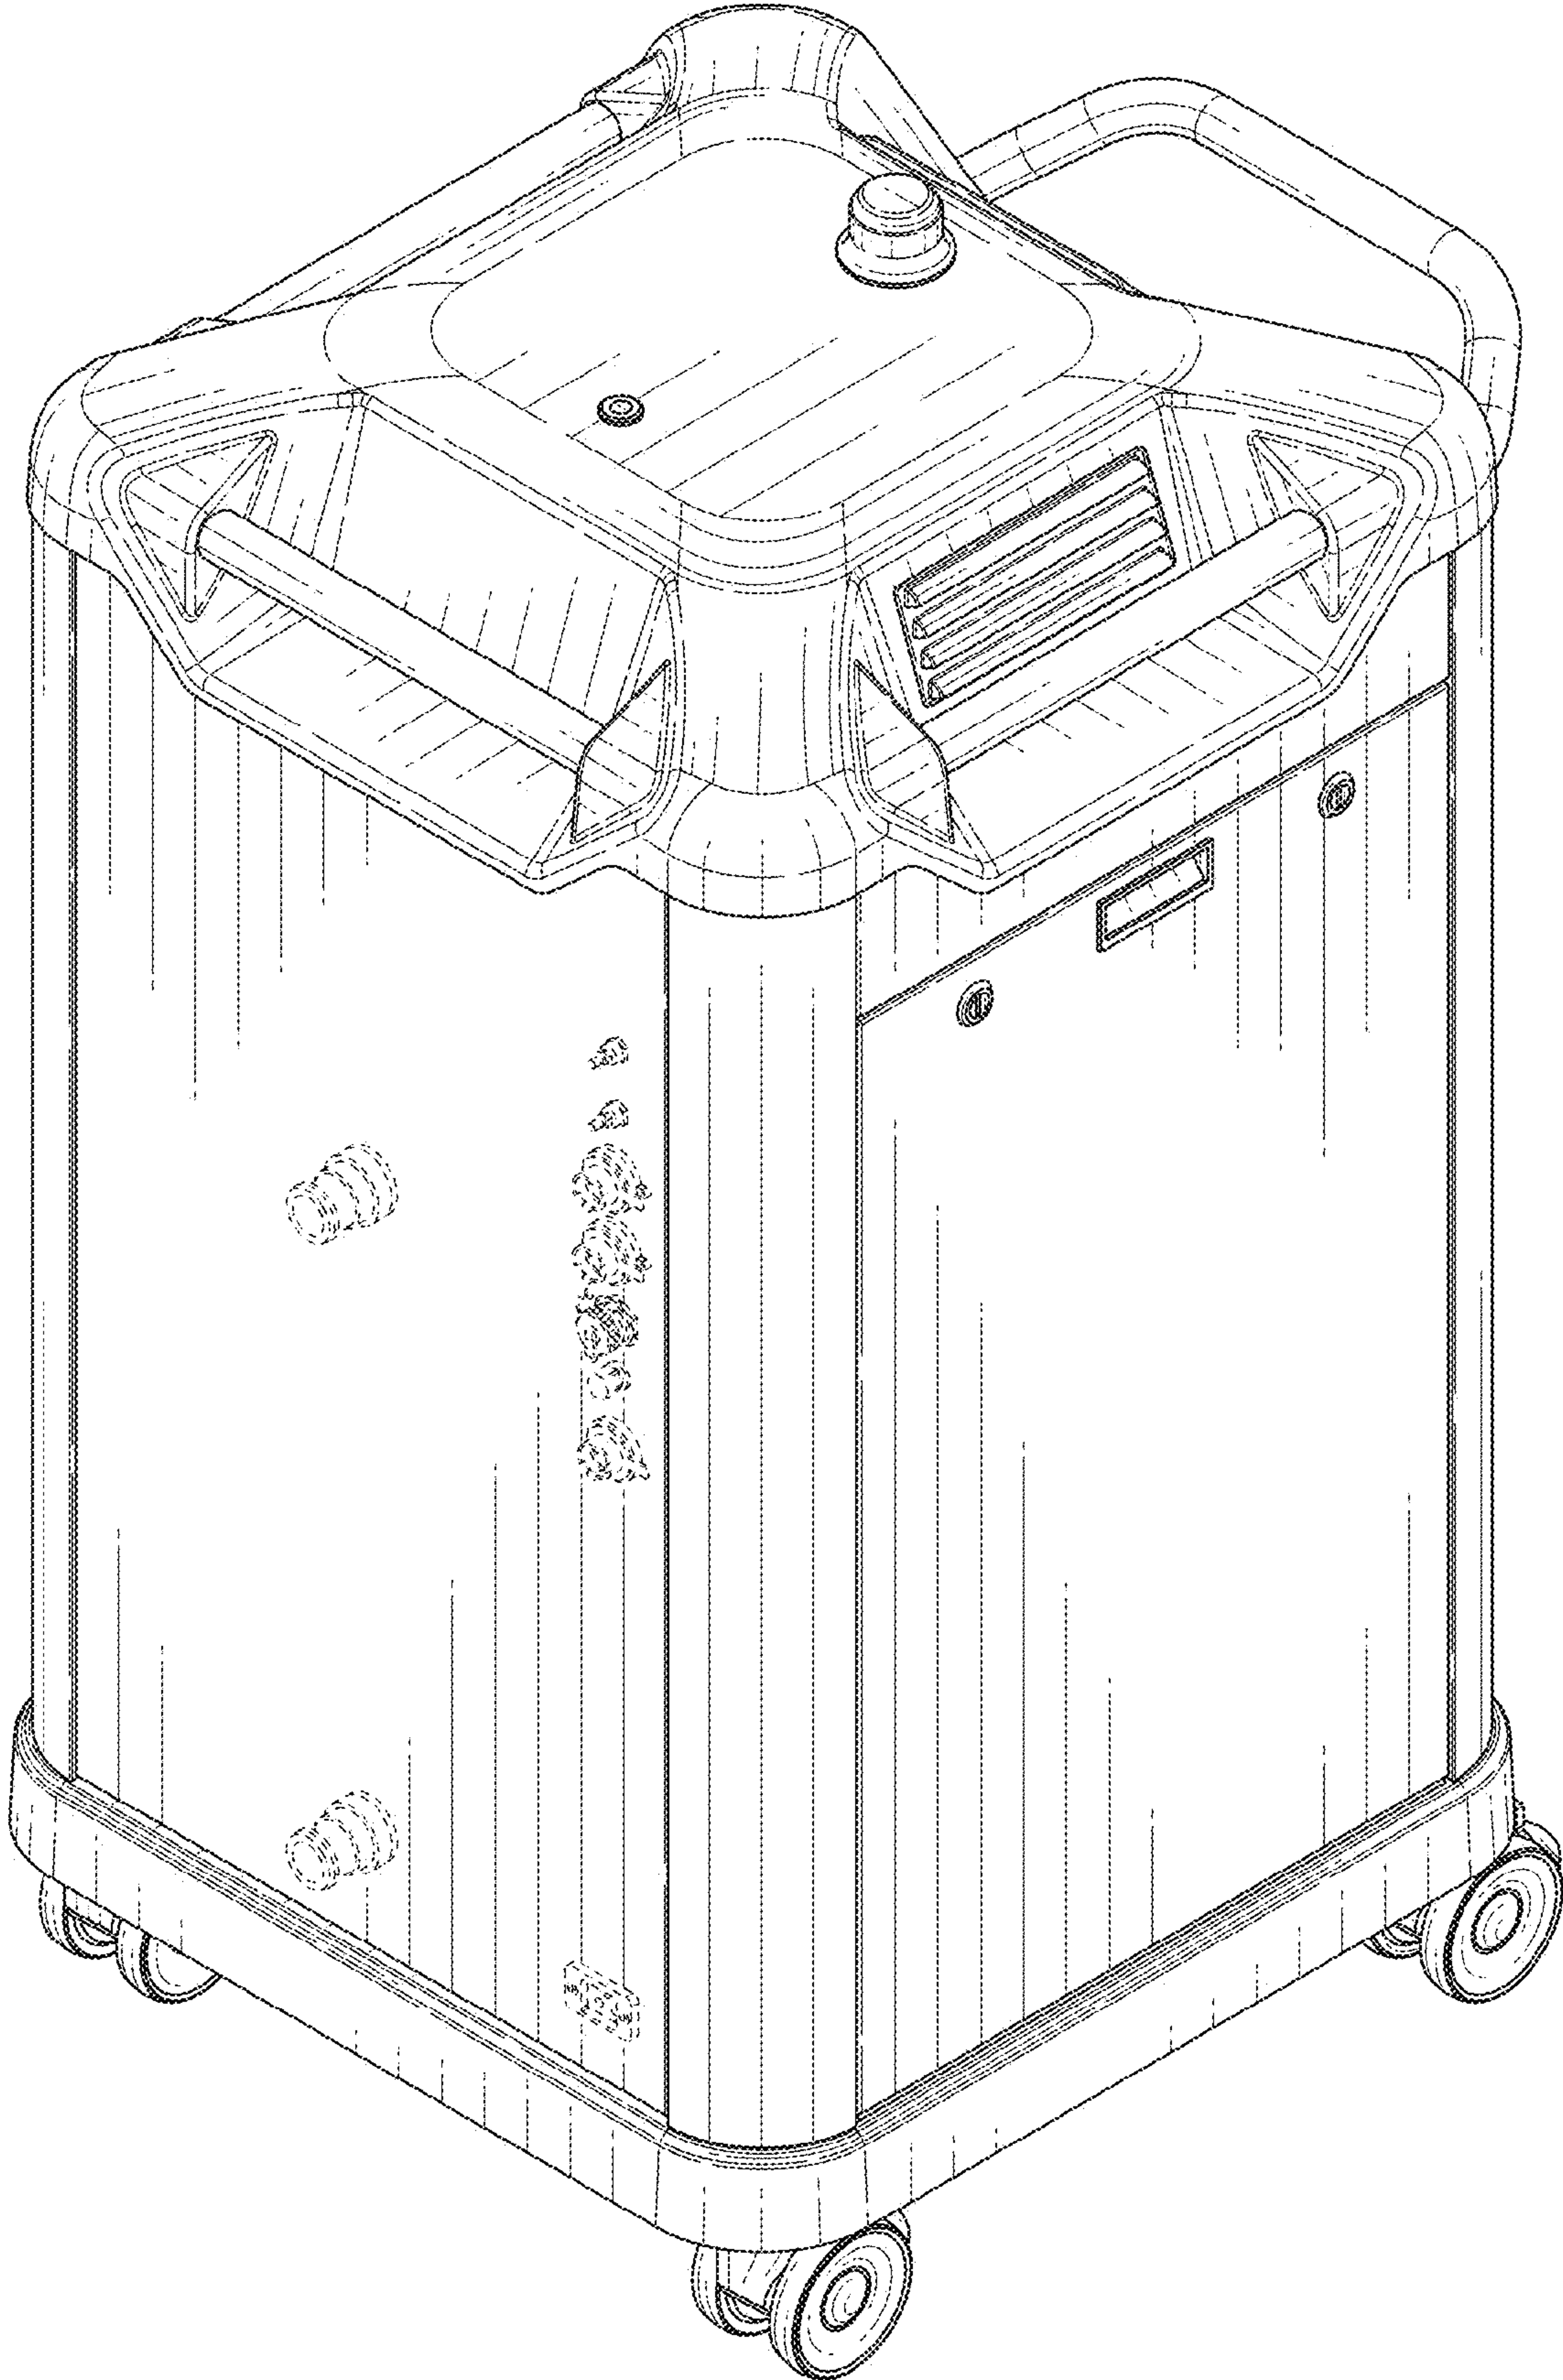


FIG. 17

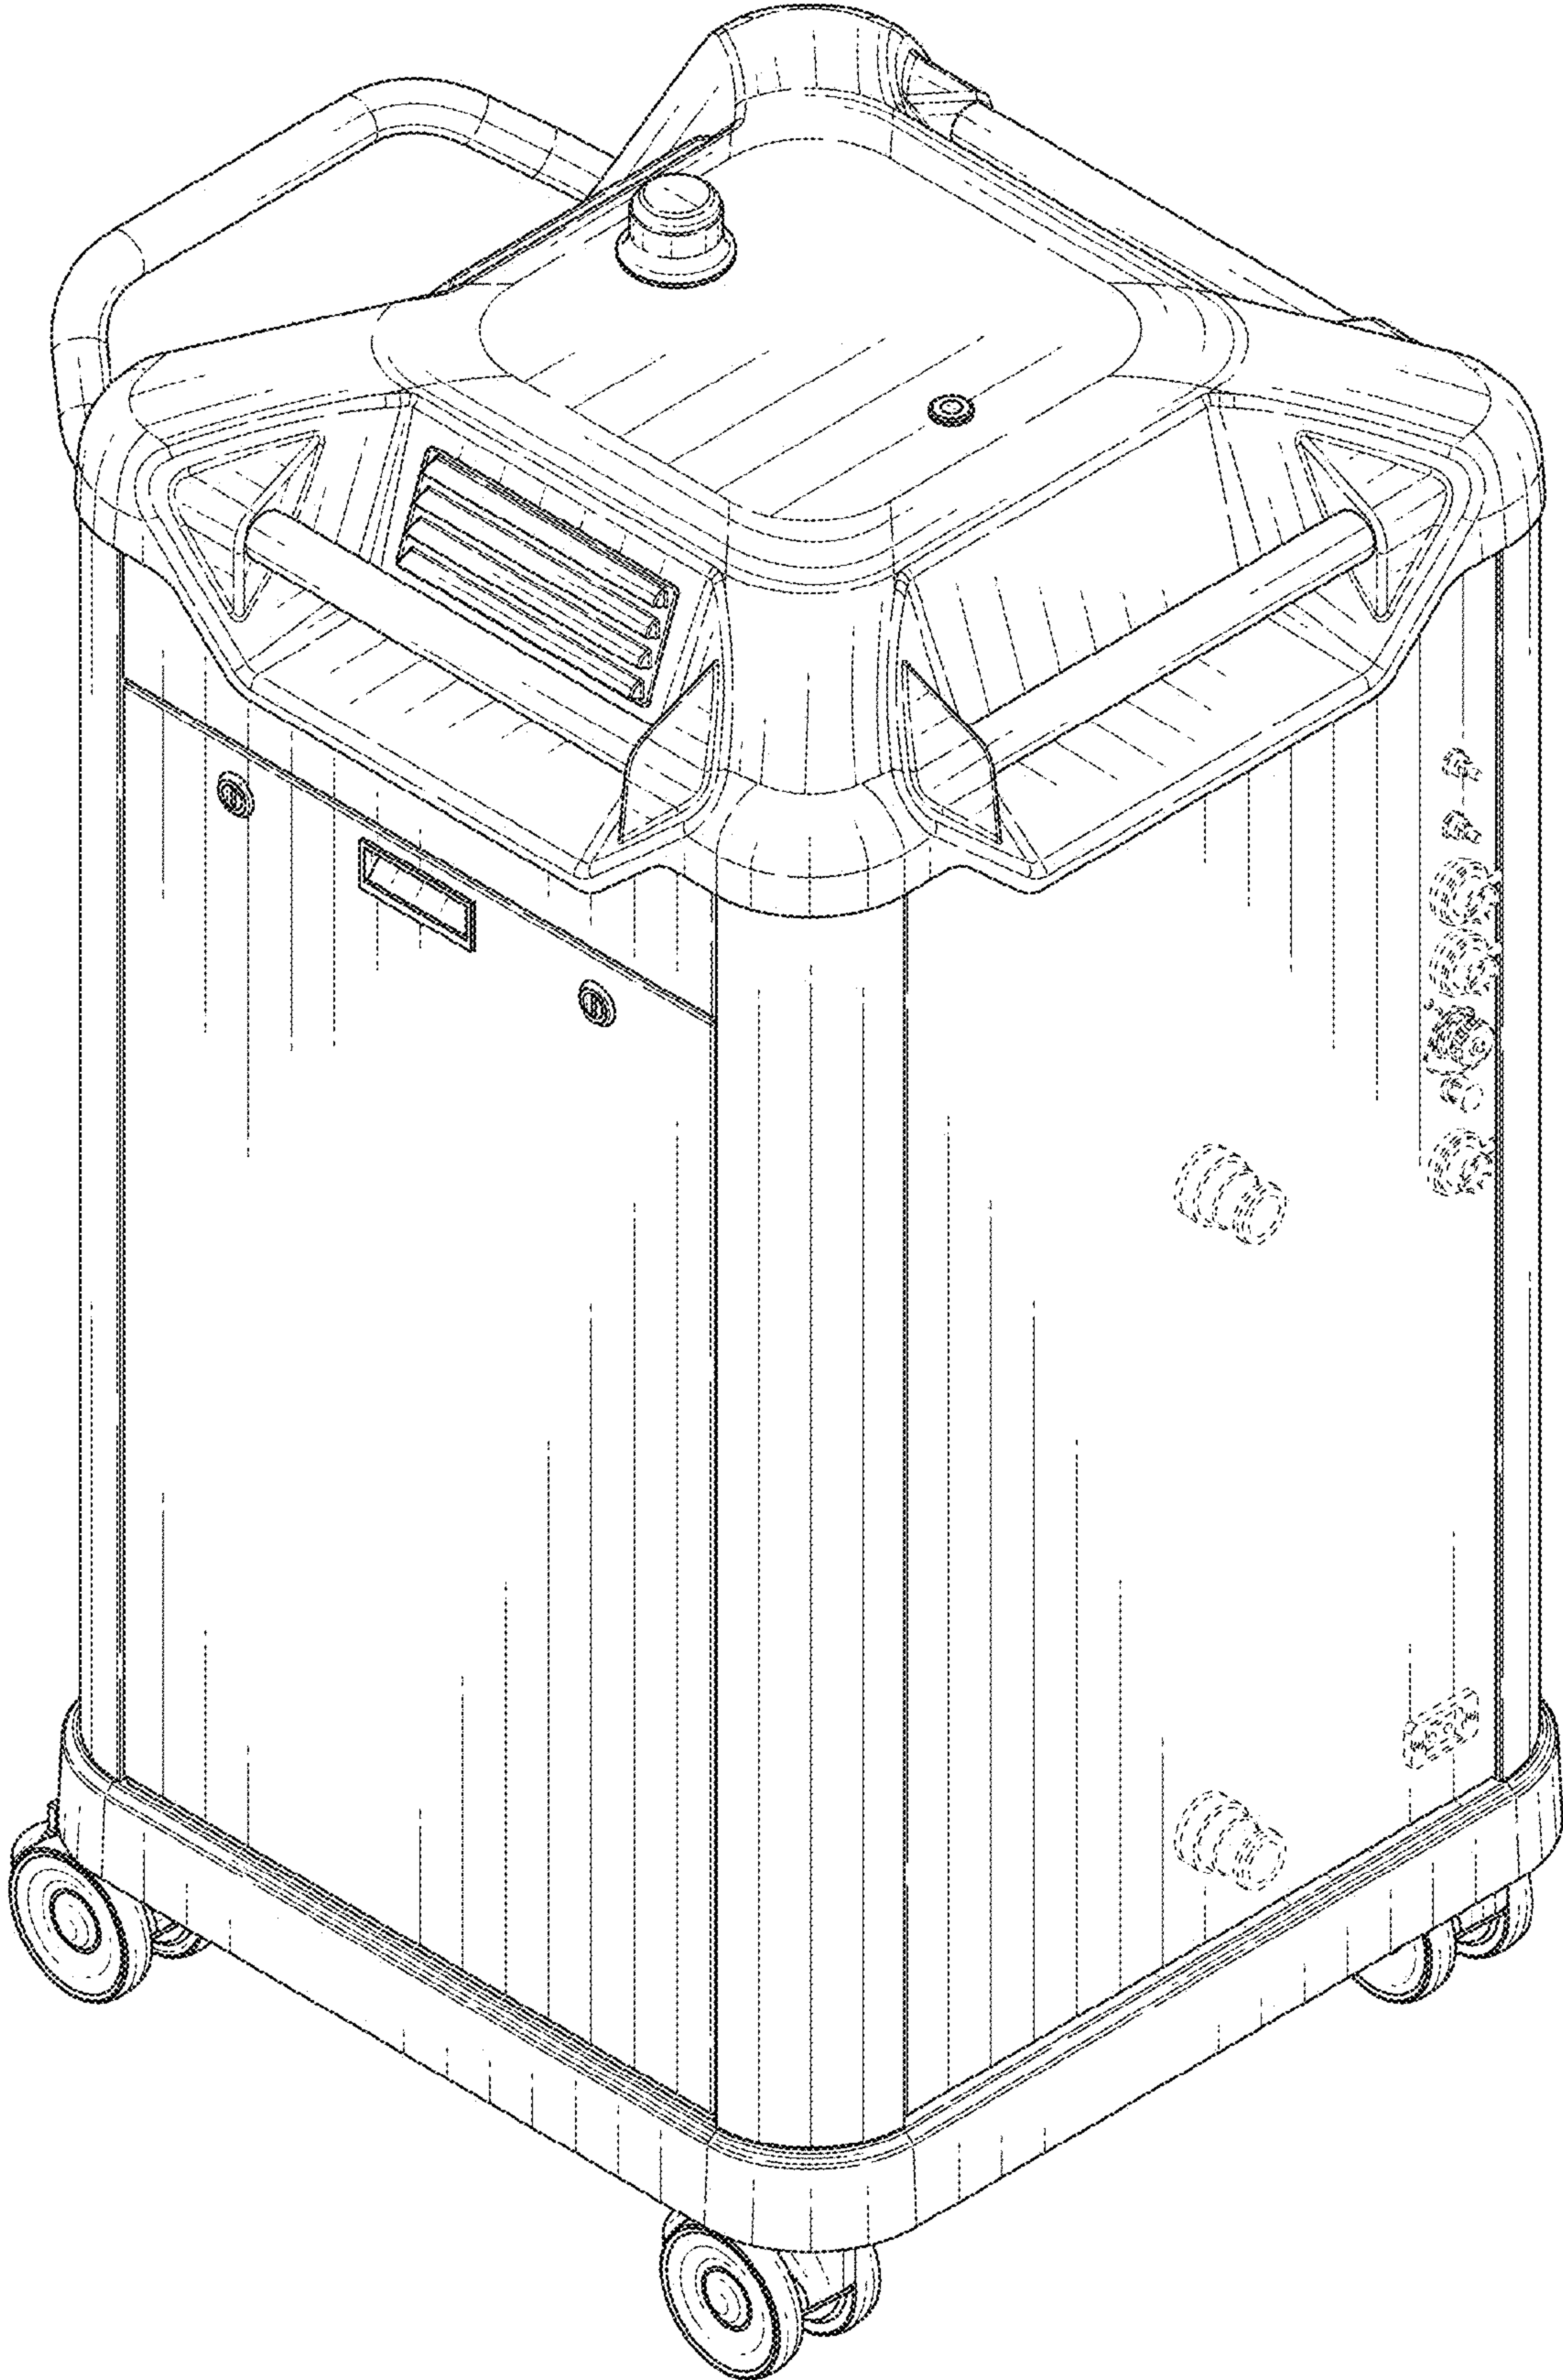


FIG. 18

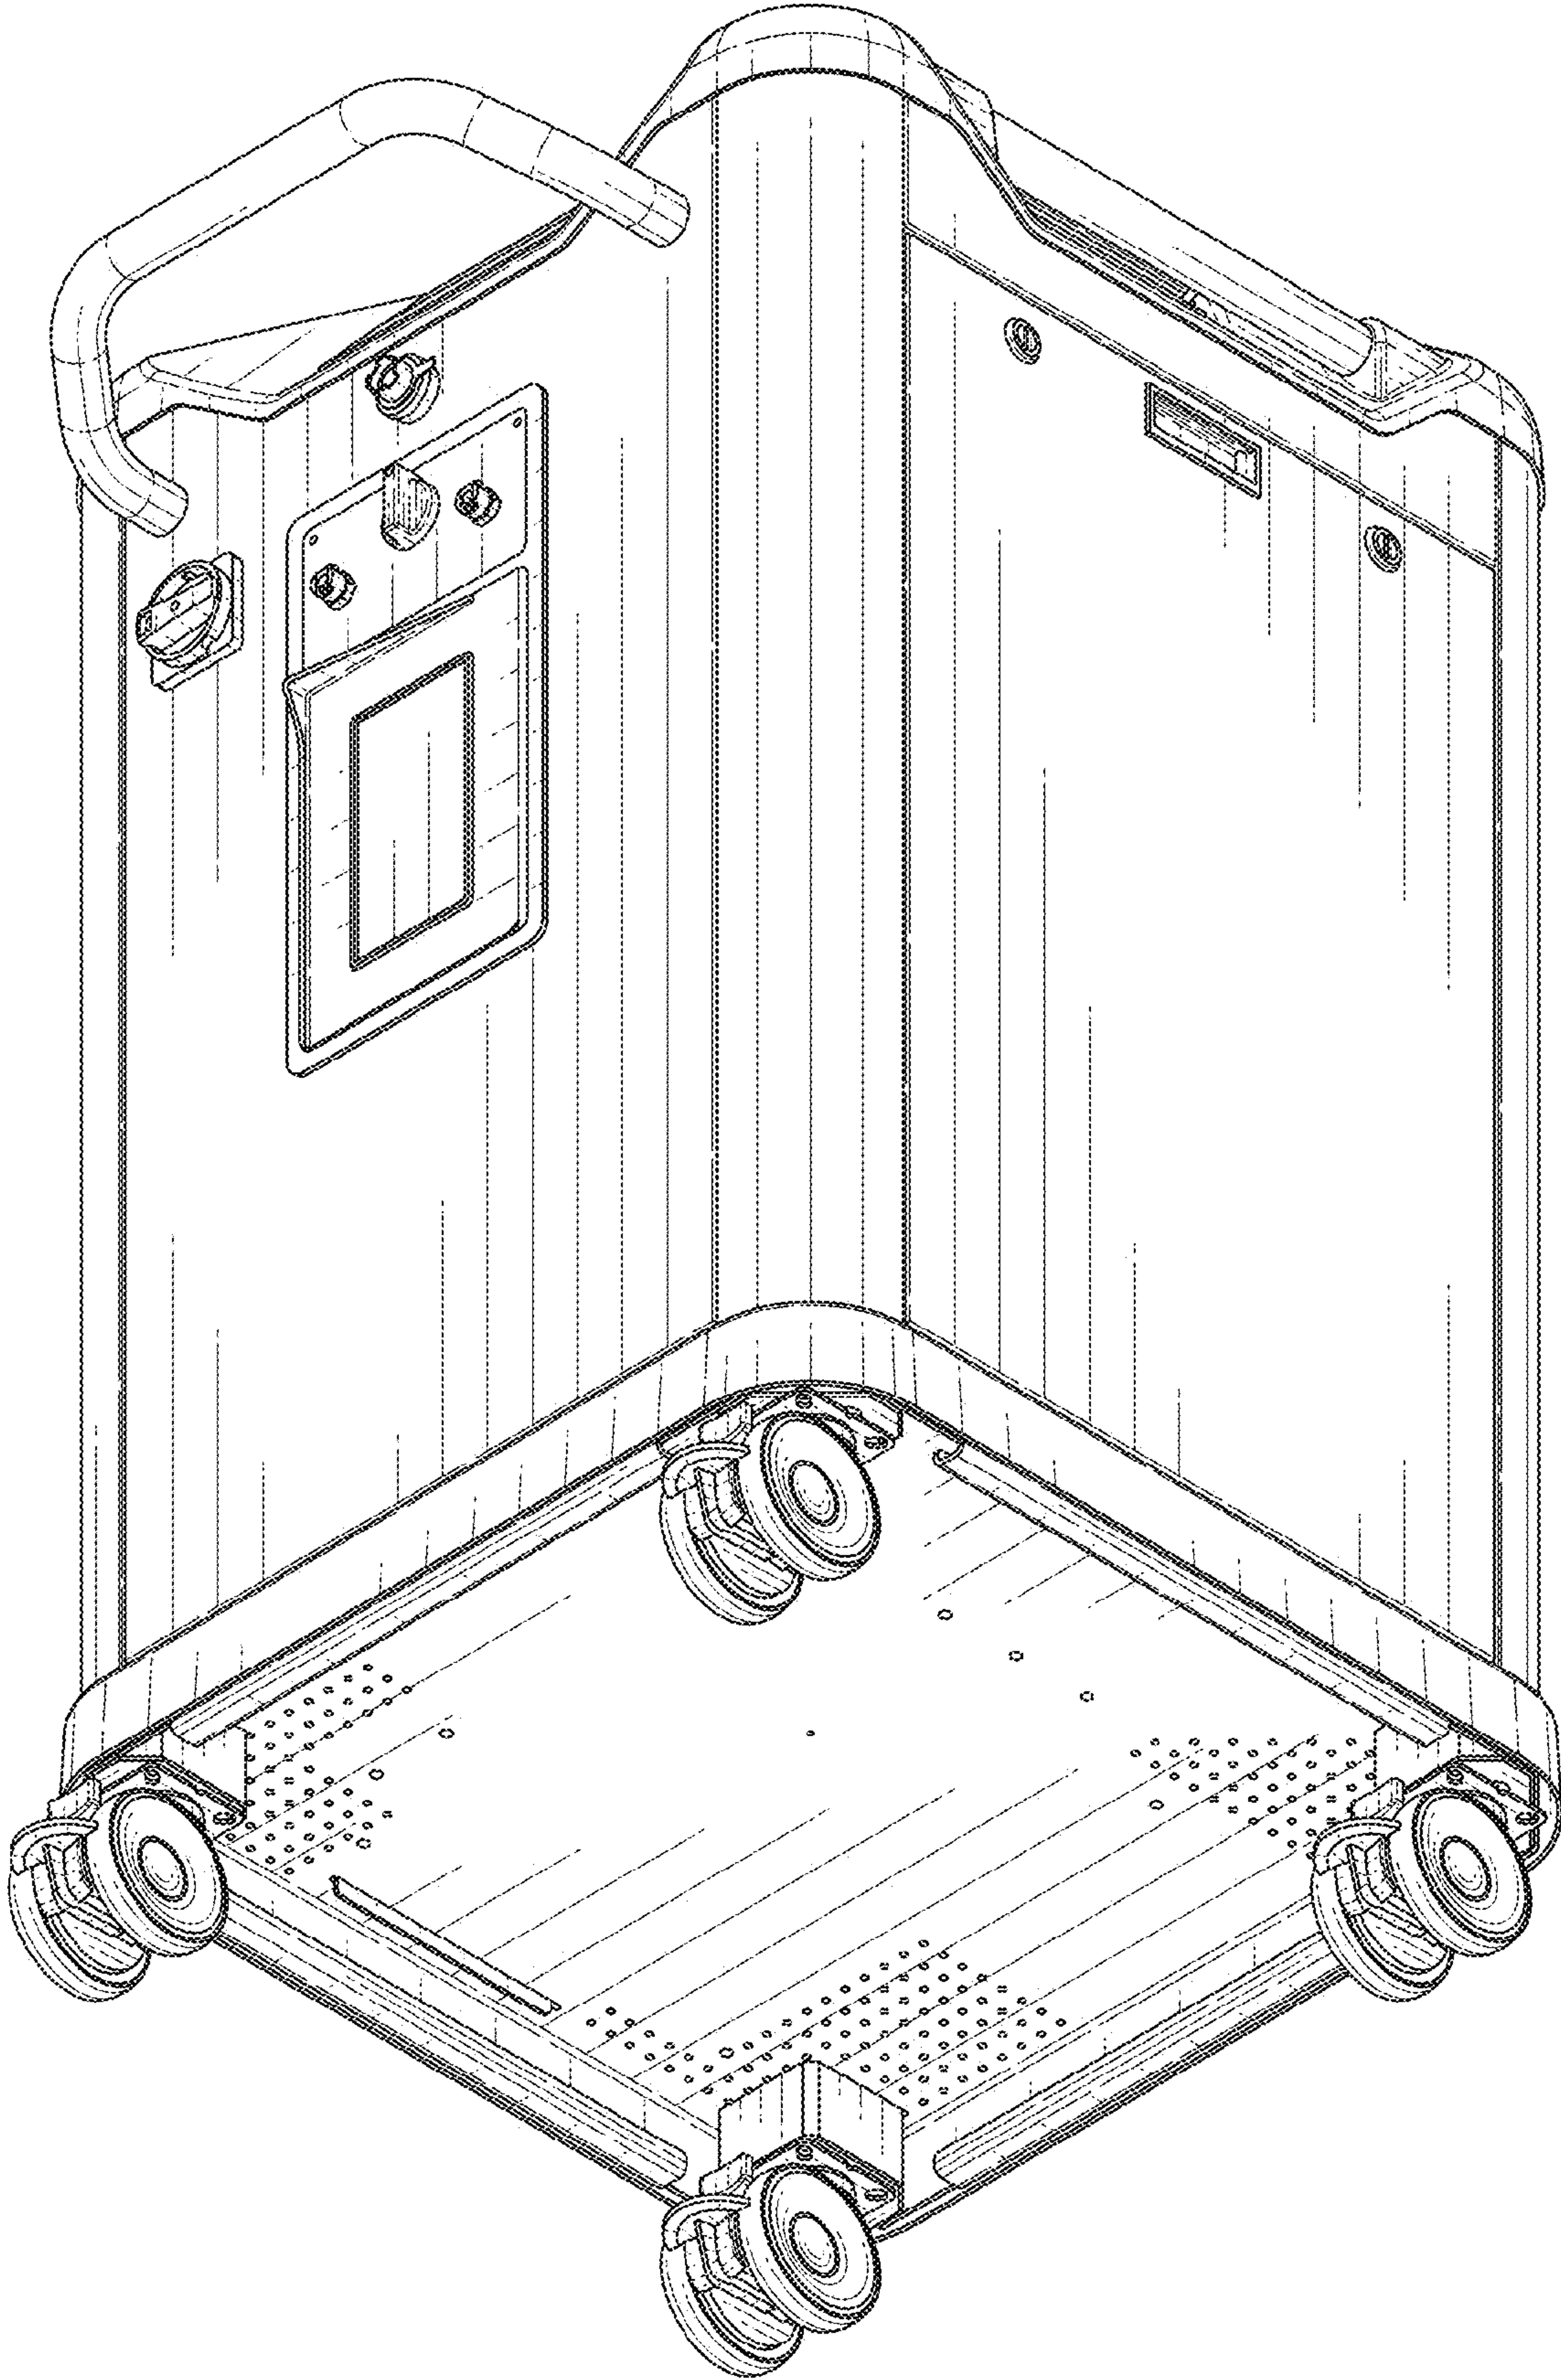


FIG. 19

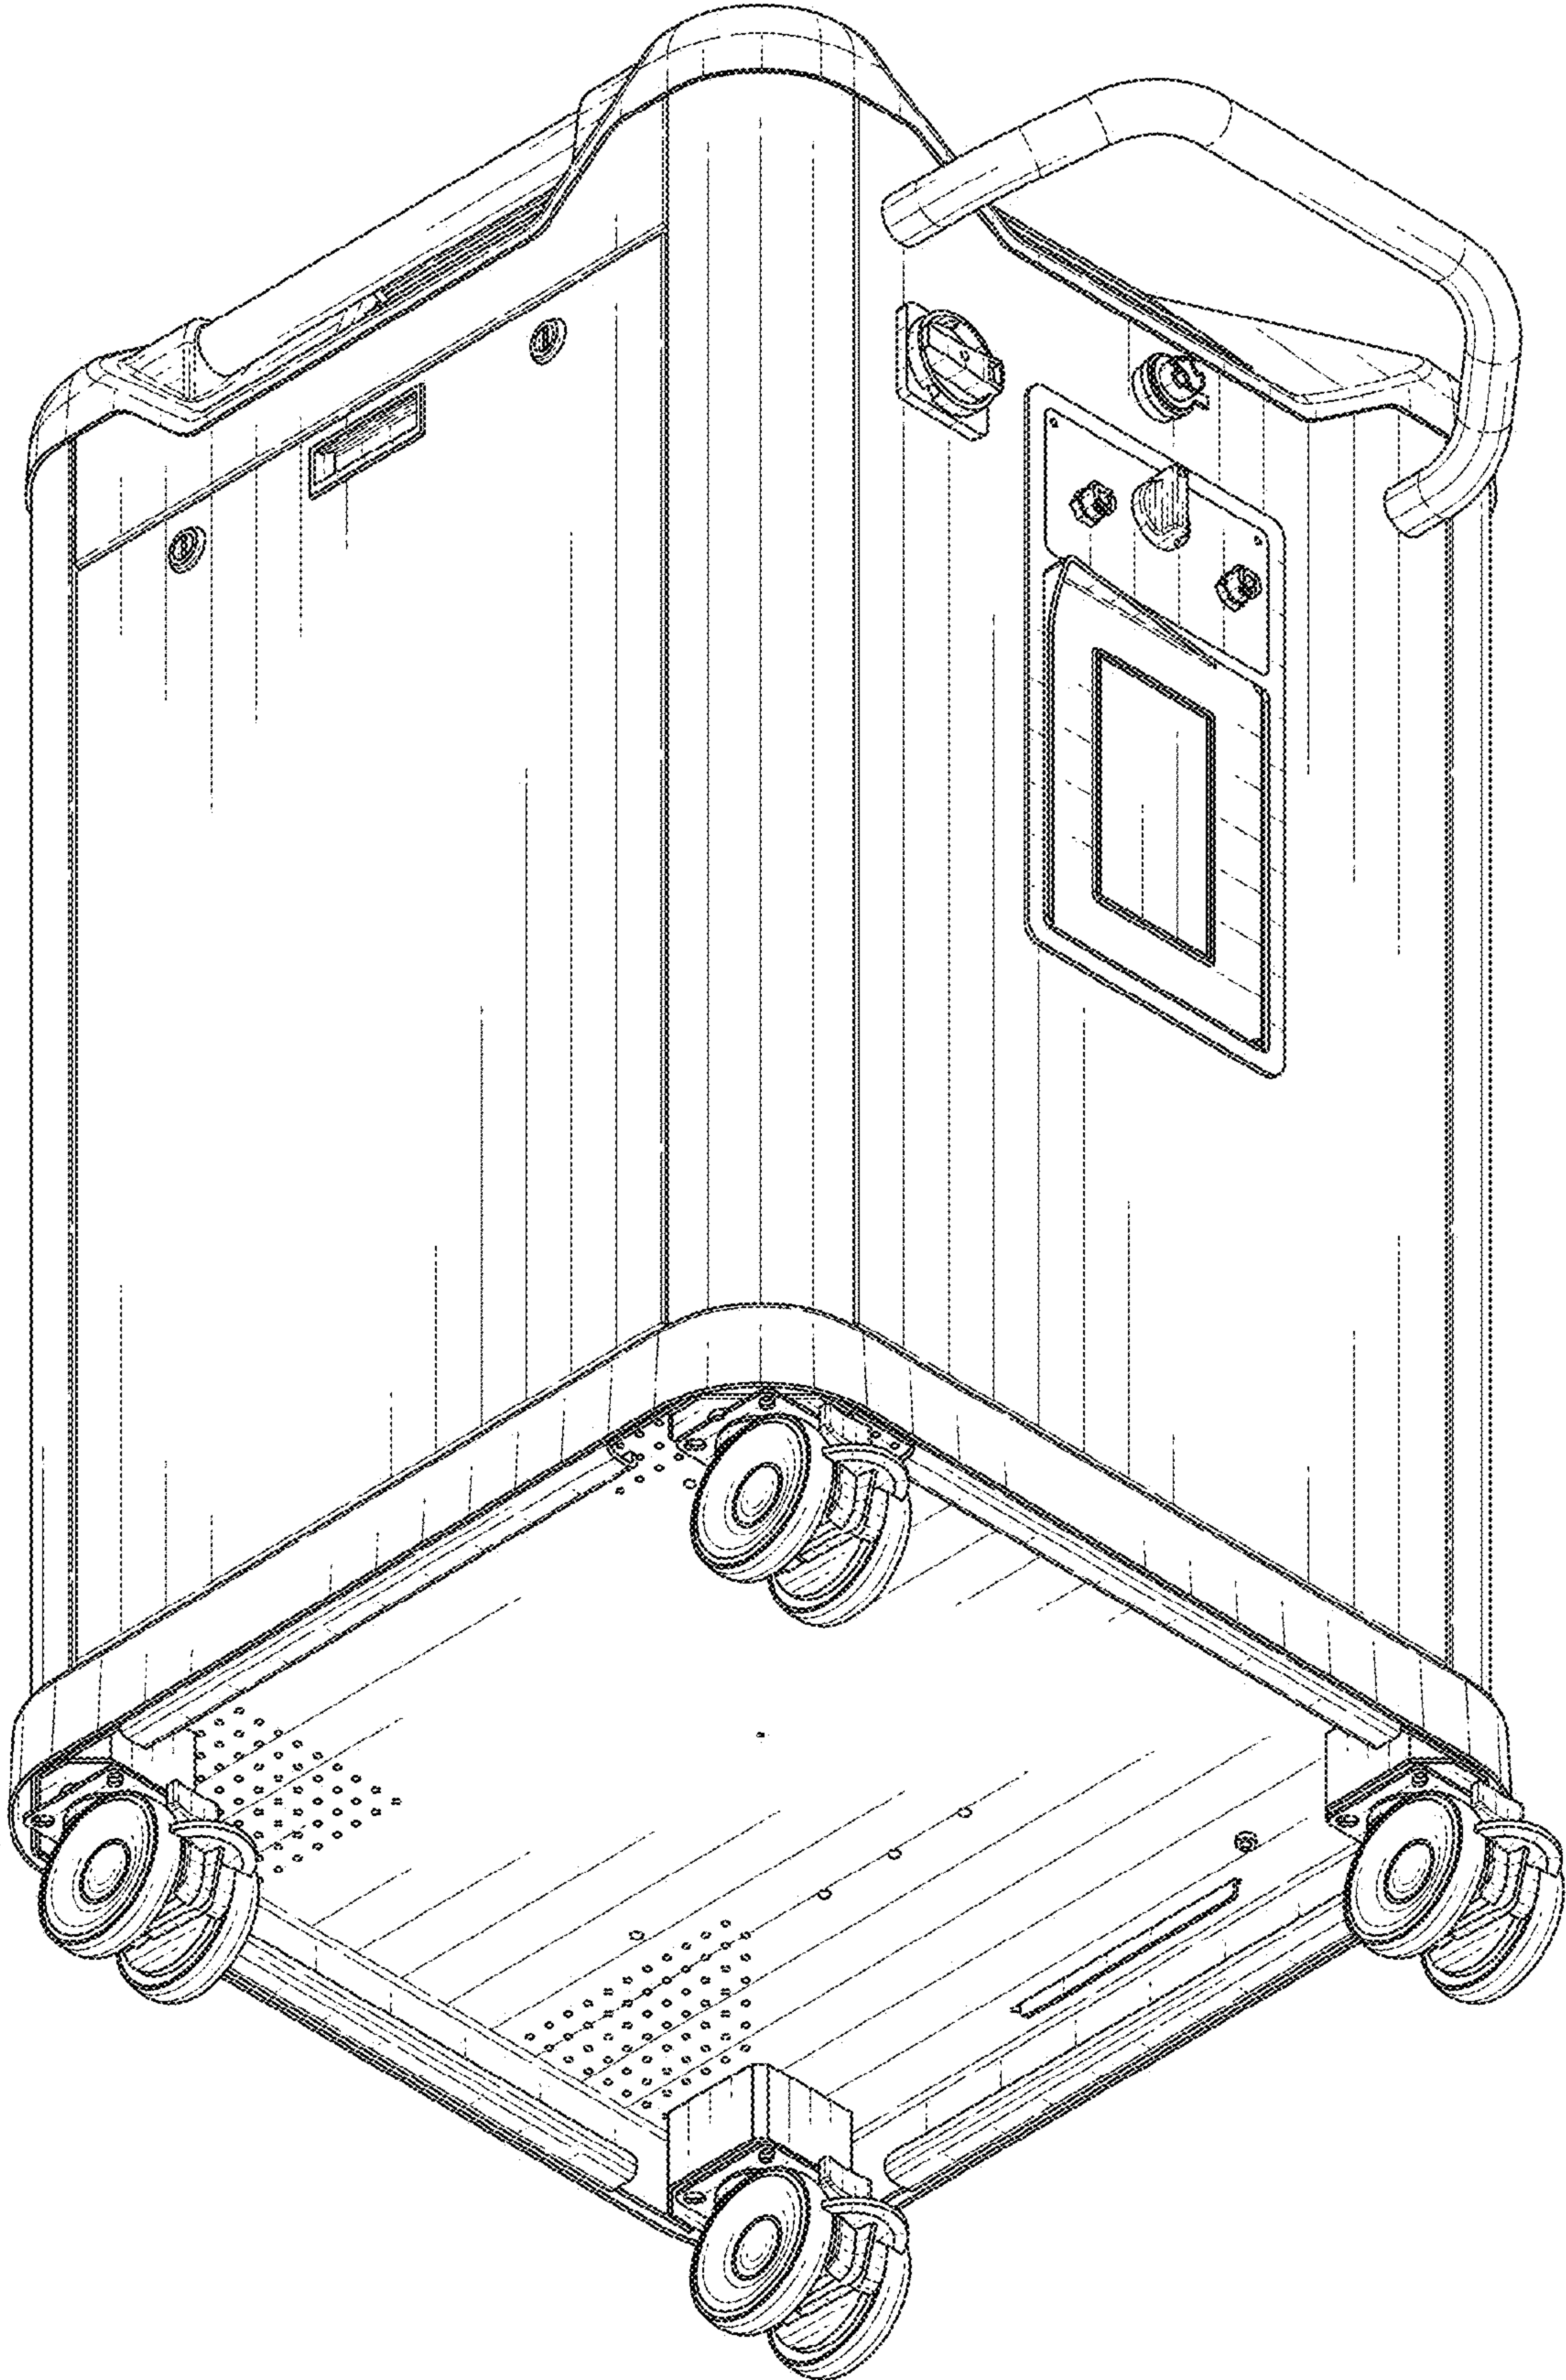


FIG. 20

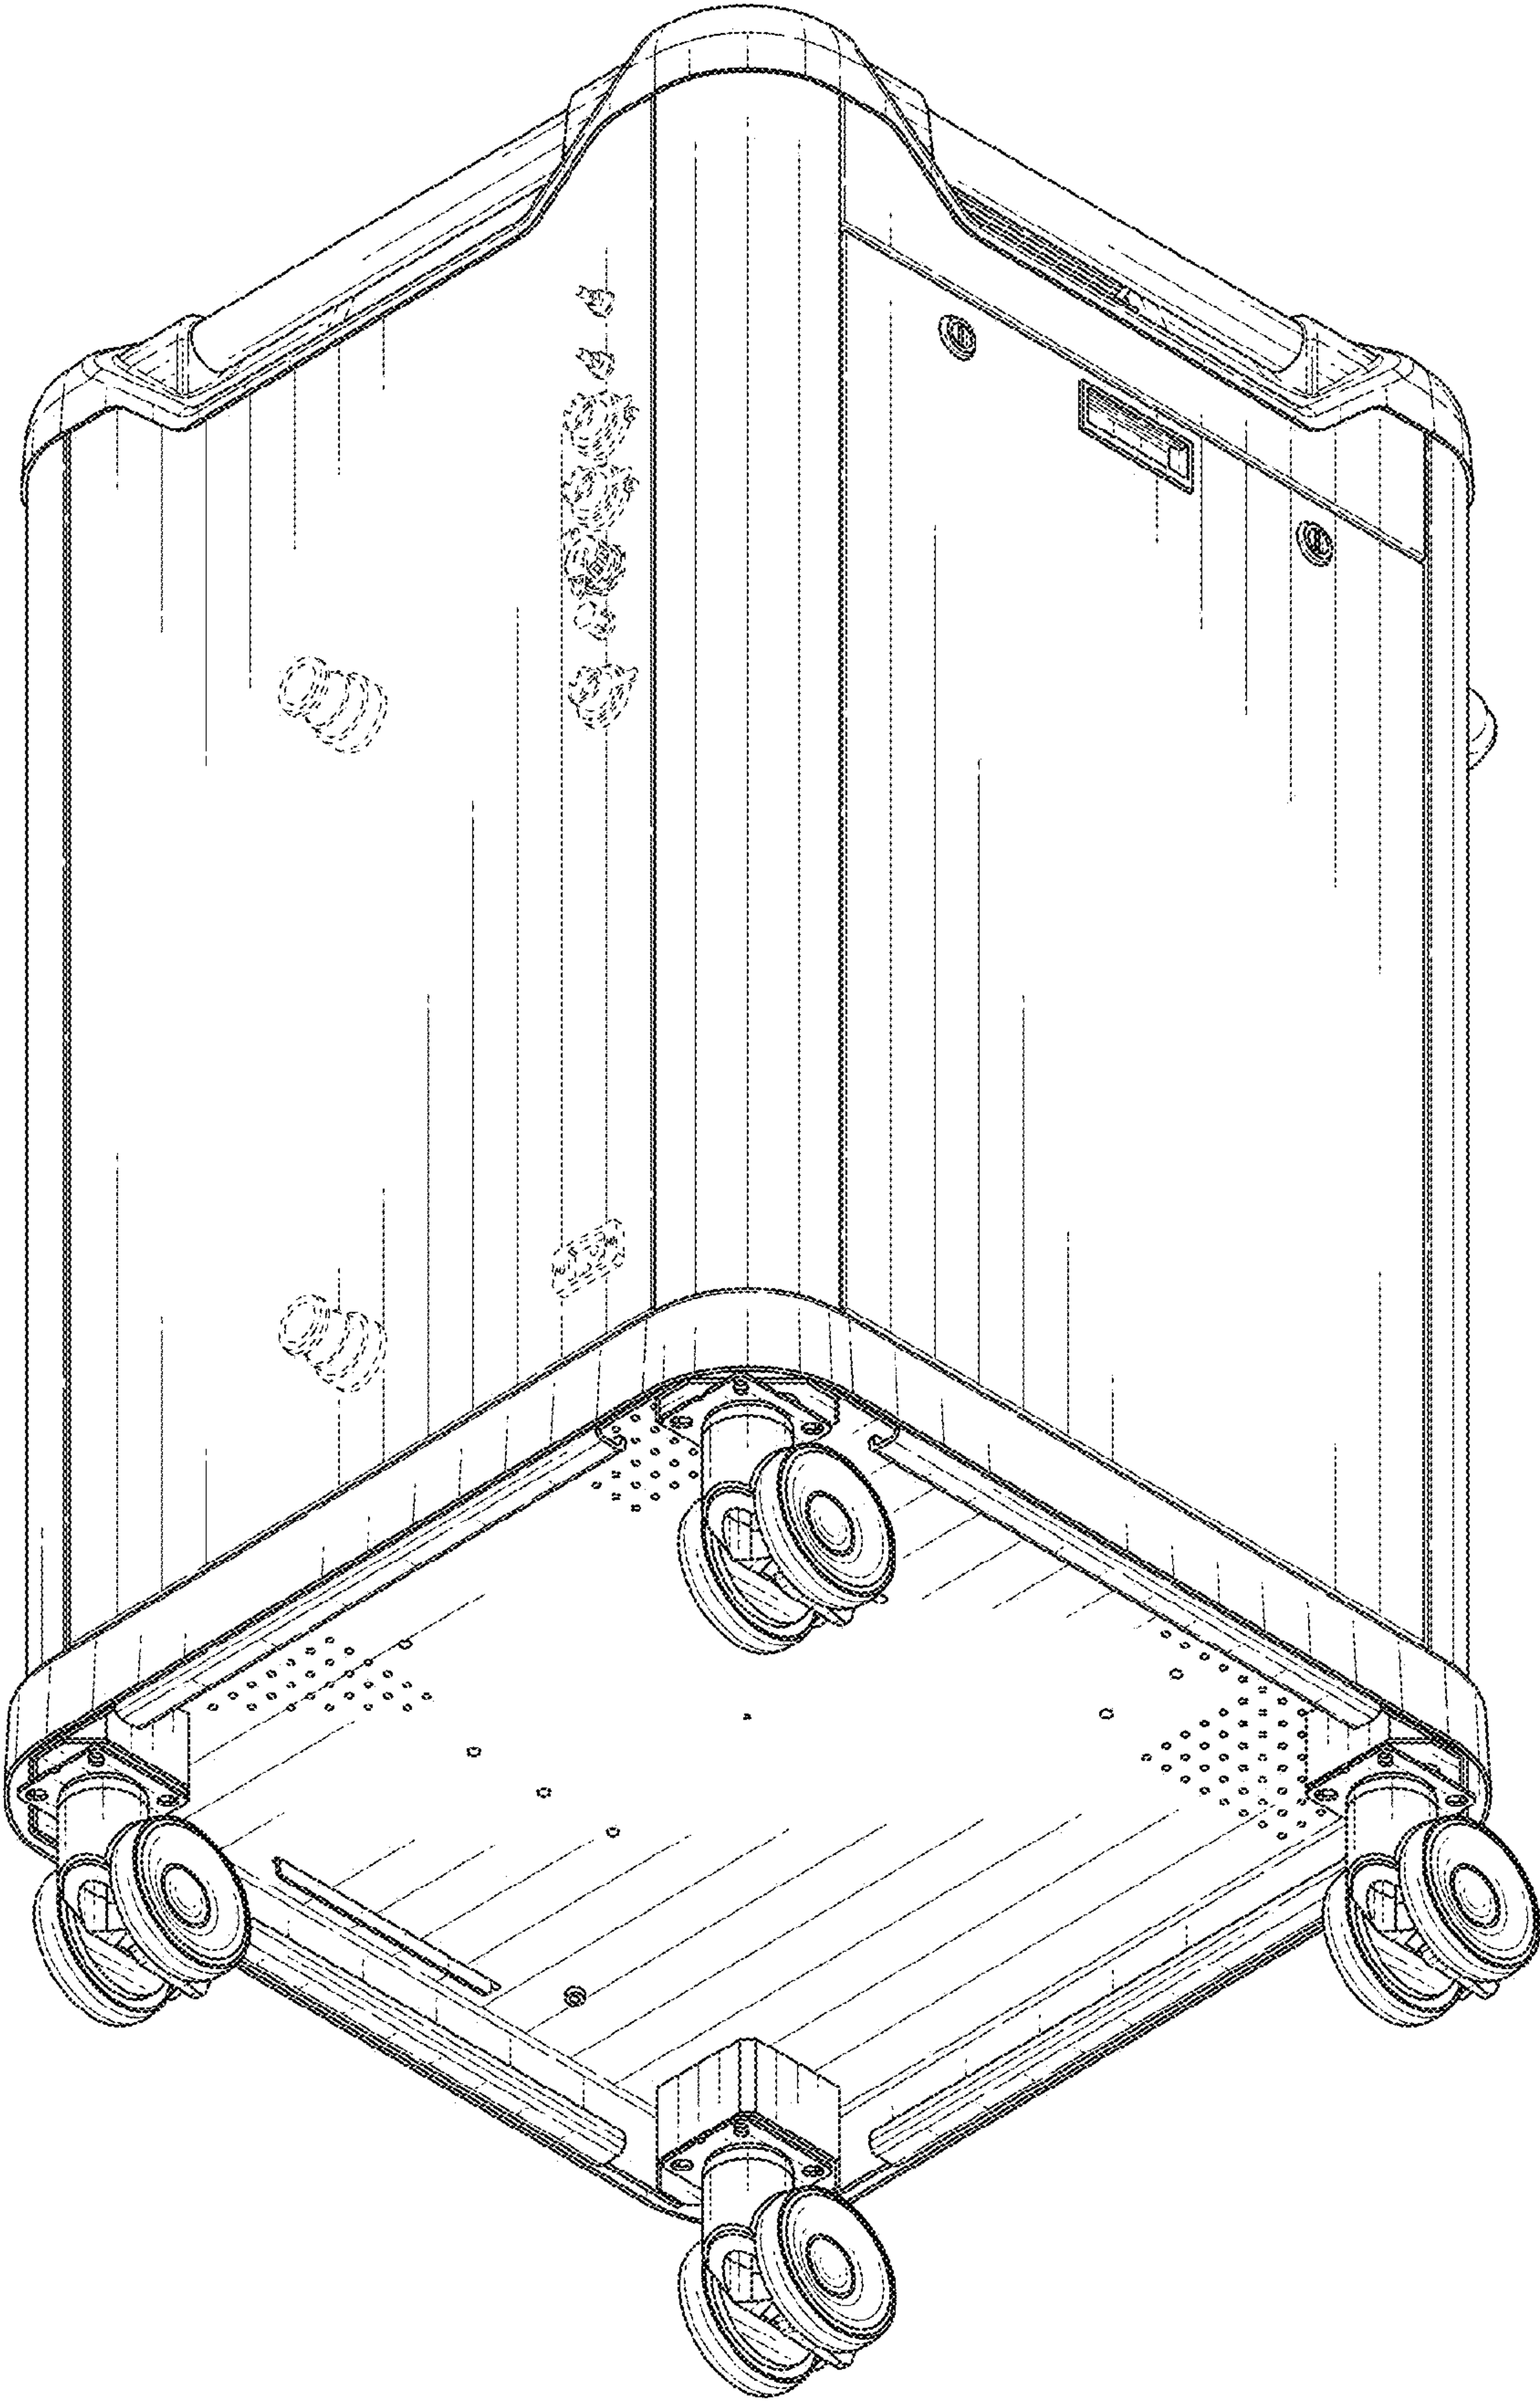


FIG. 21

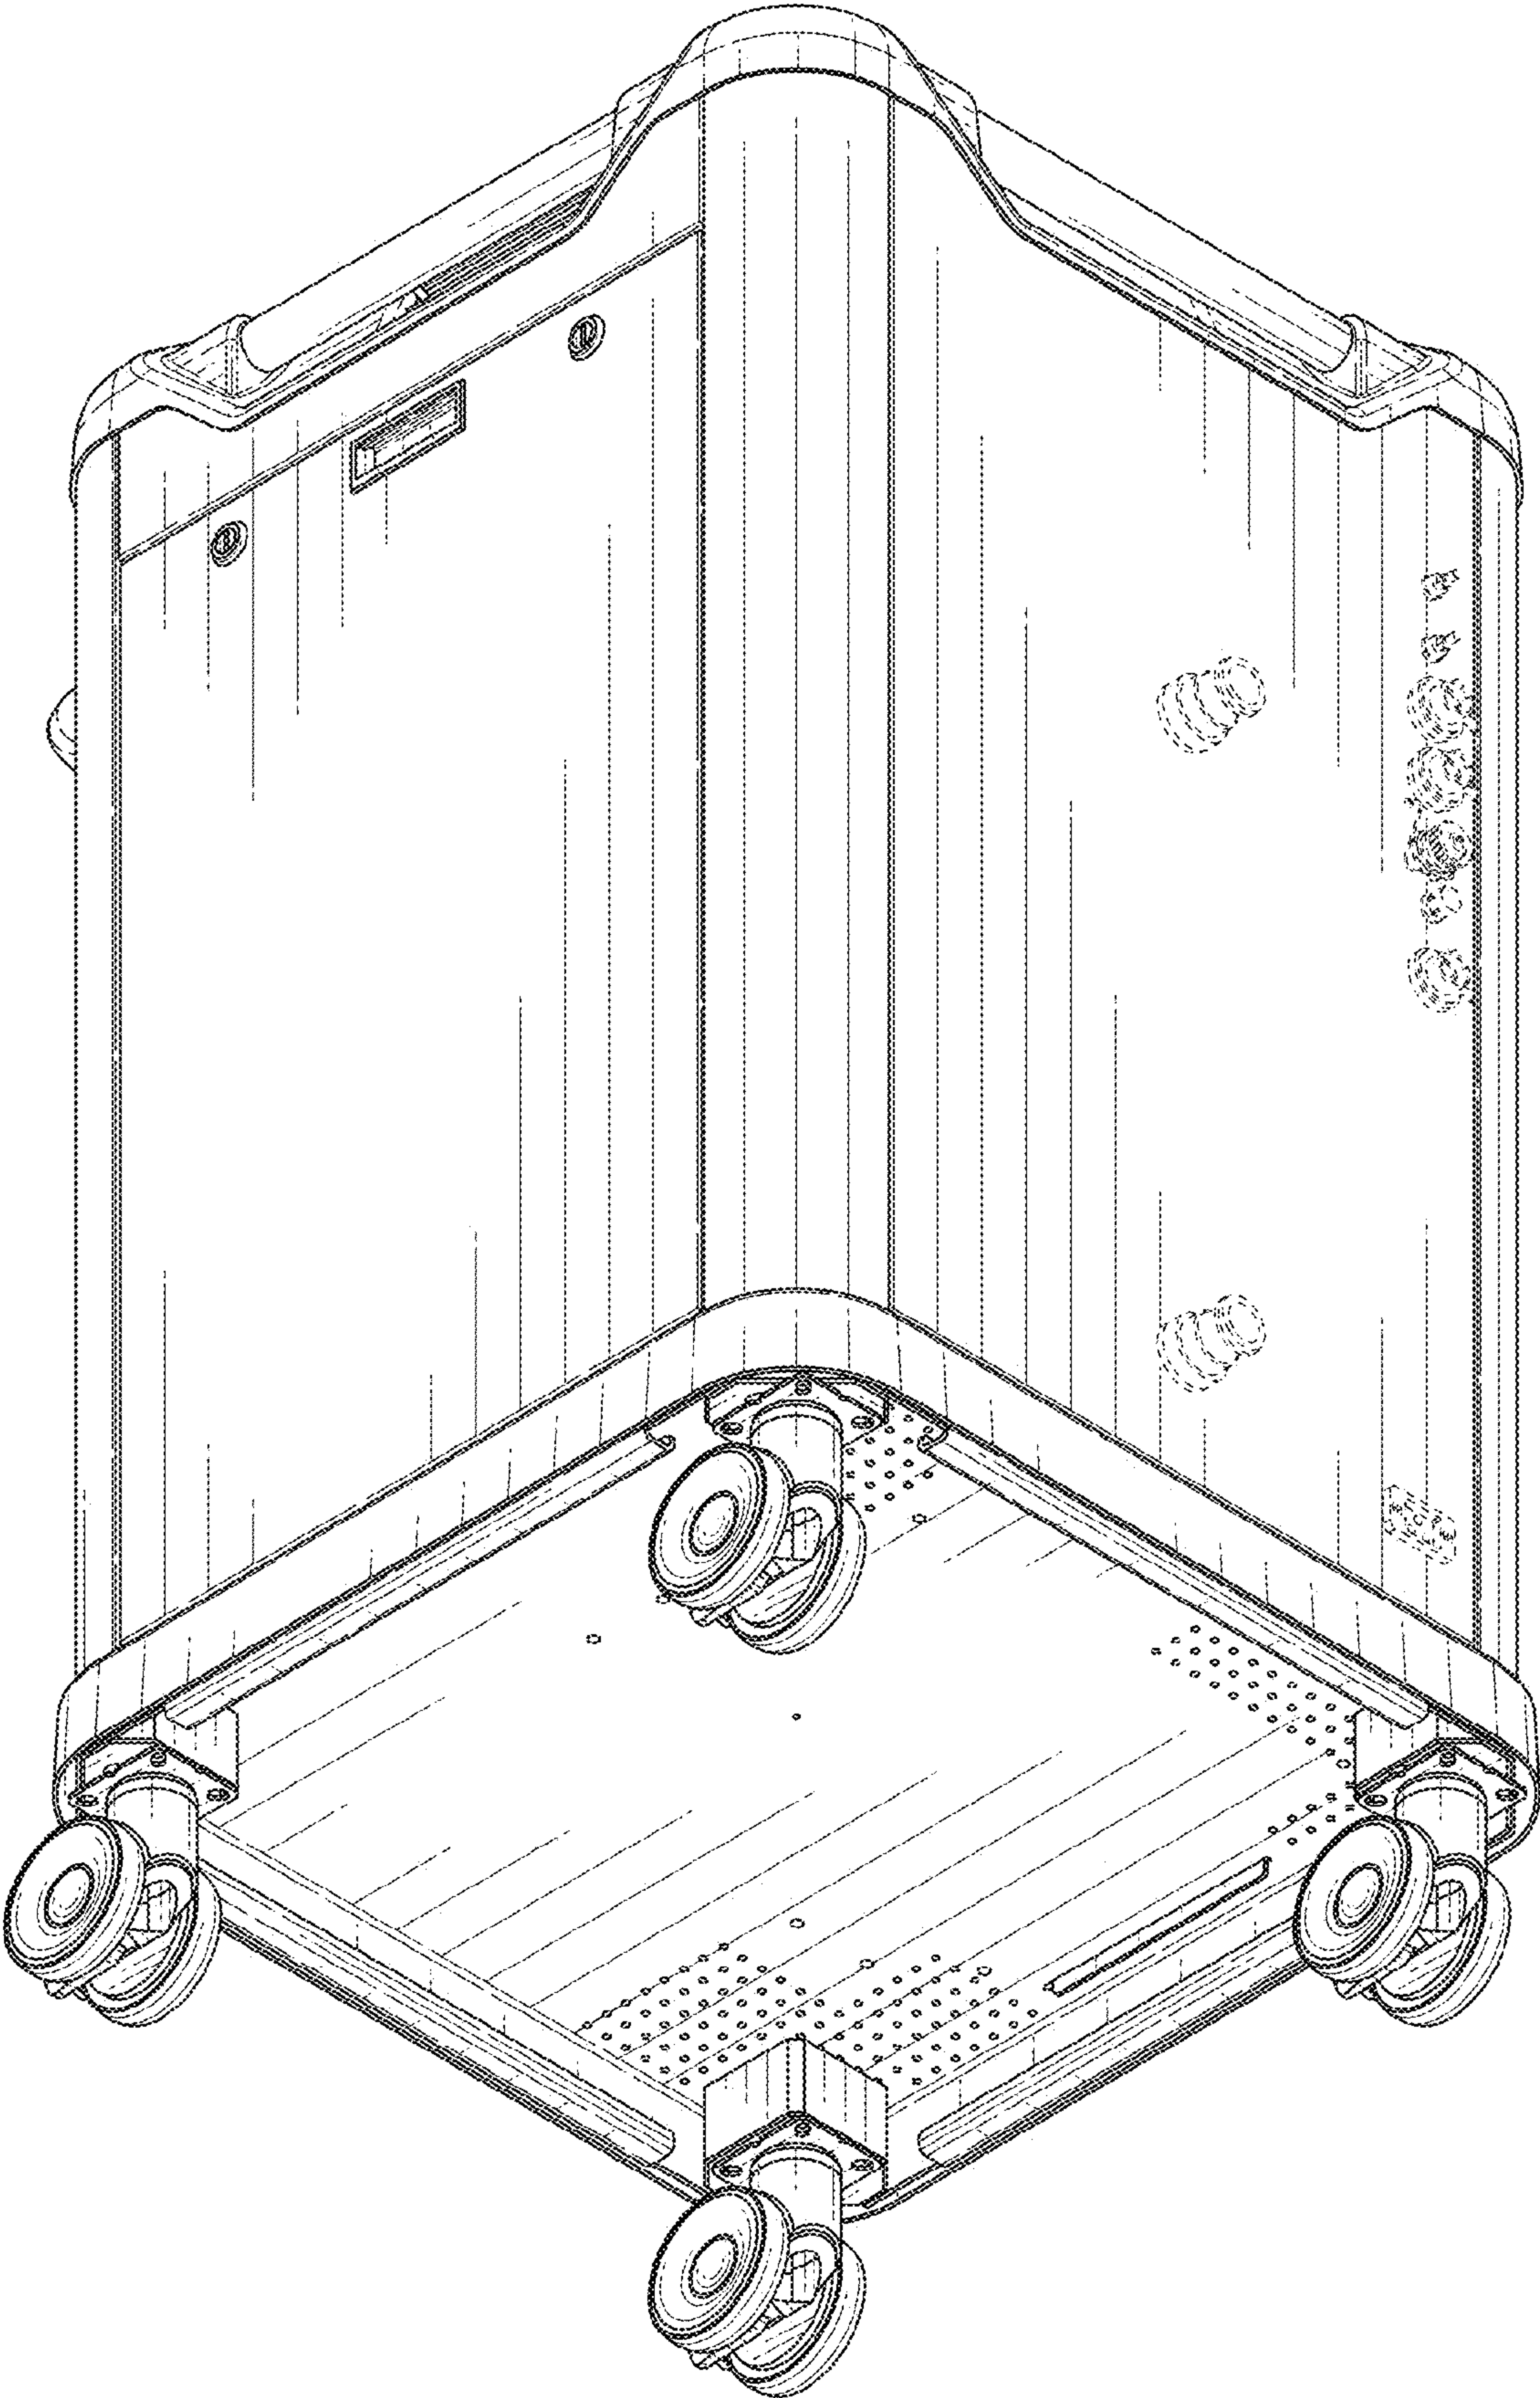


FIG. 22

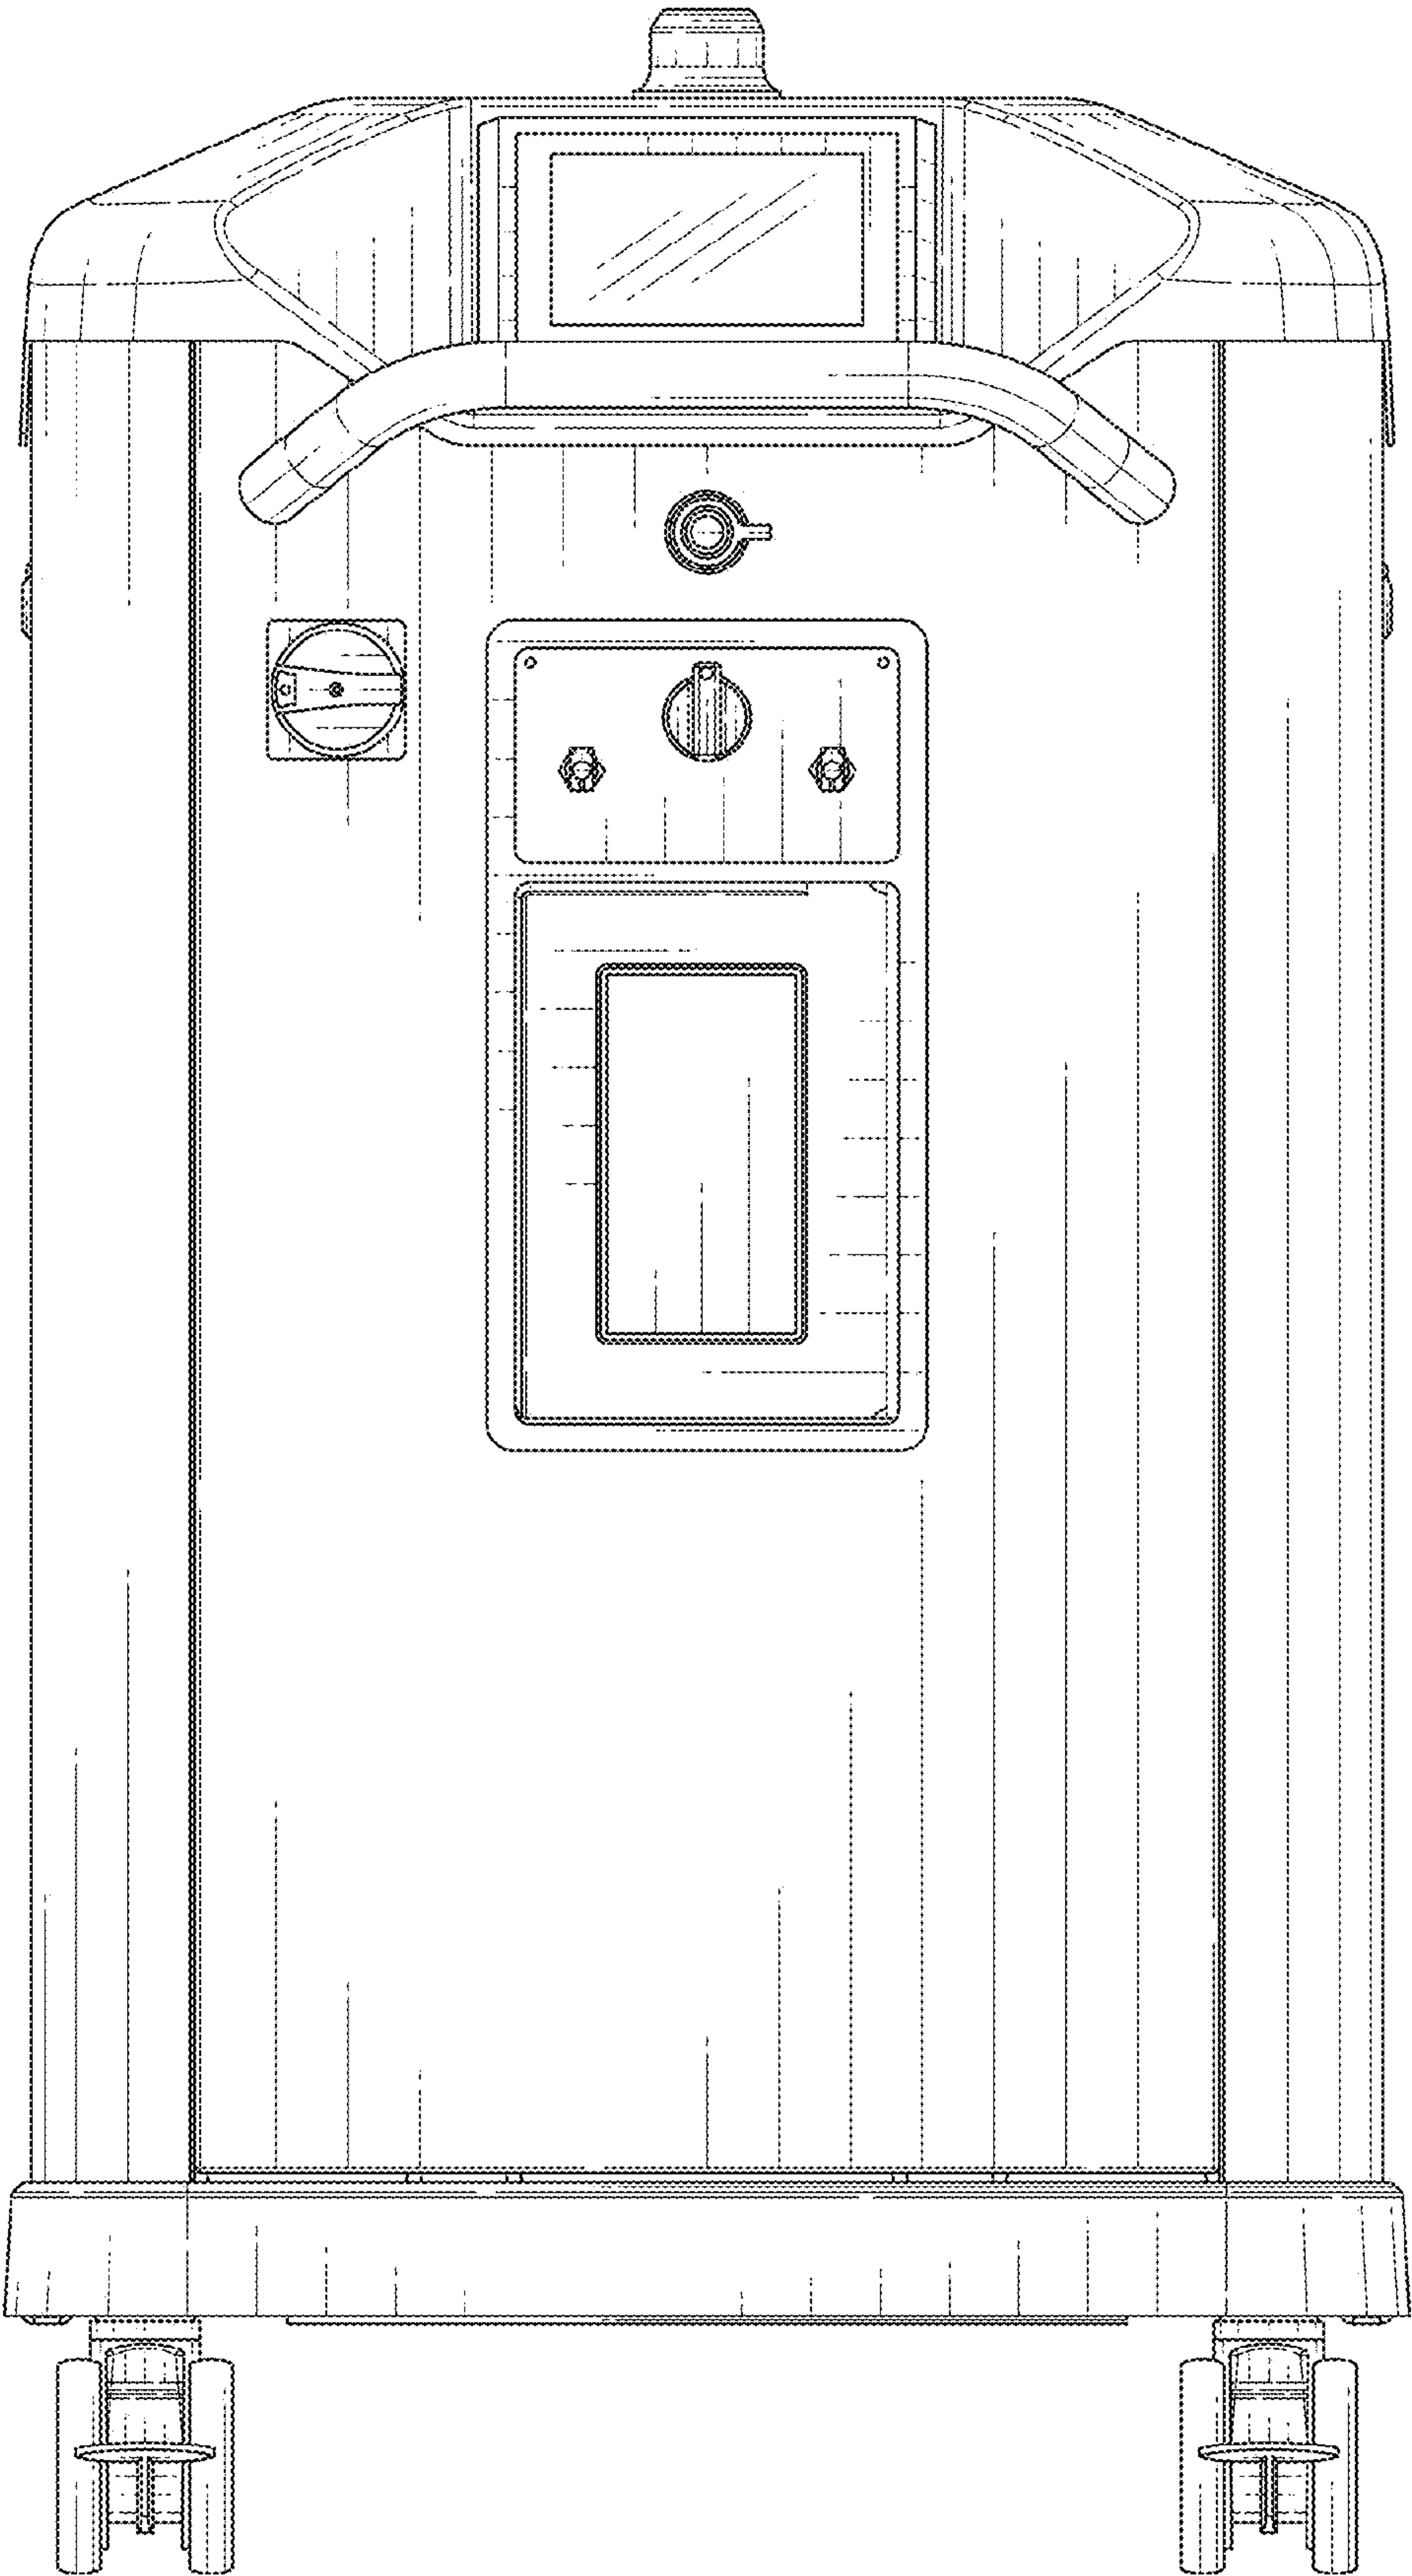


FIG. 23

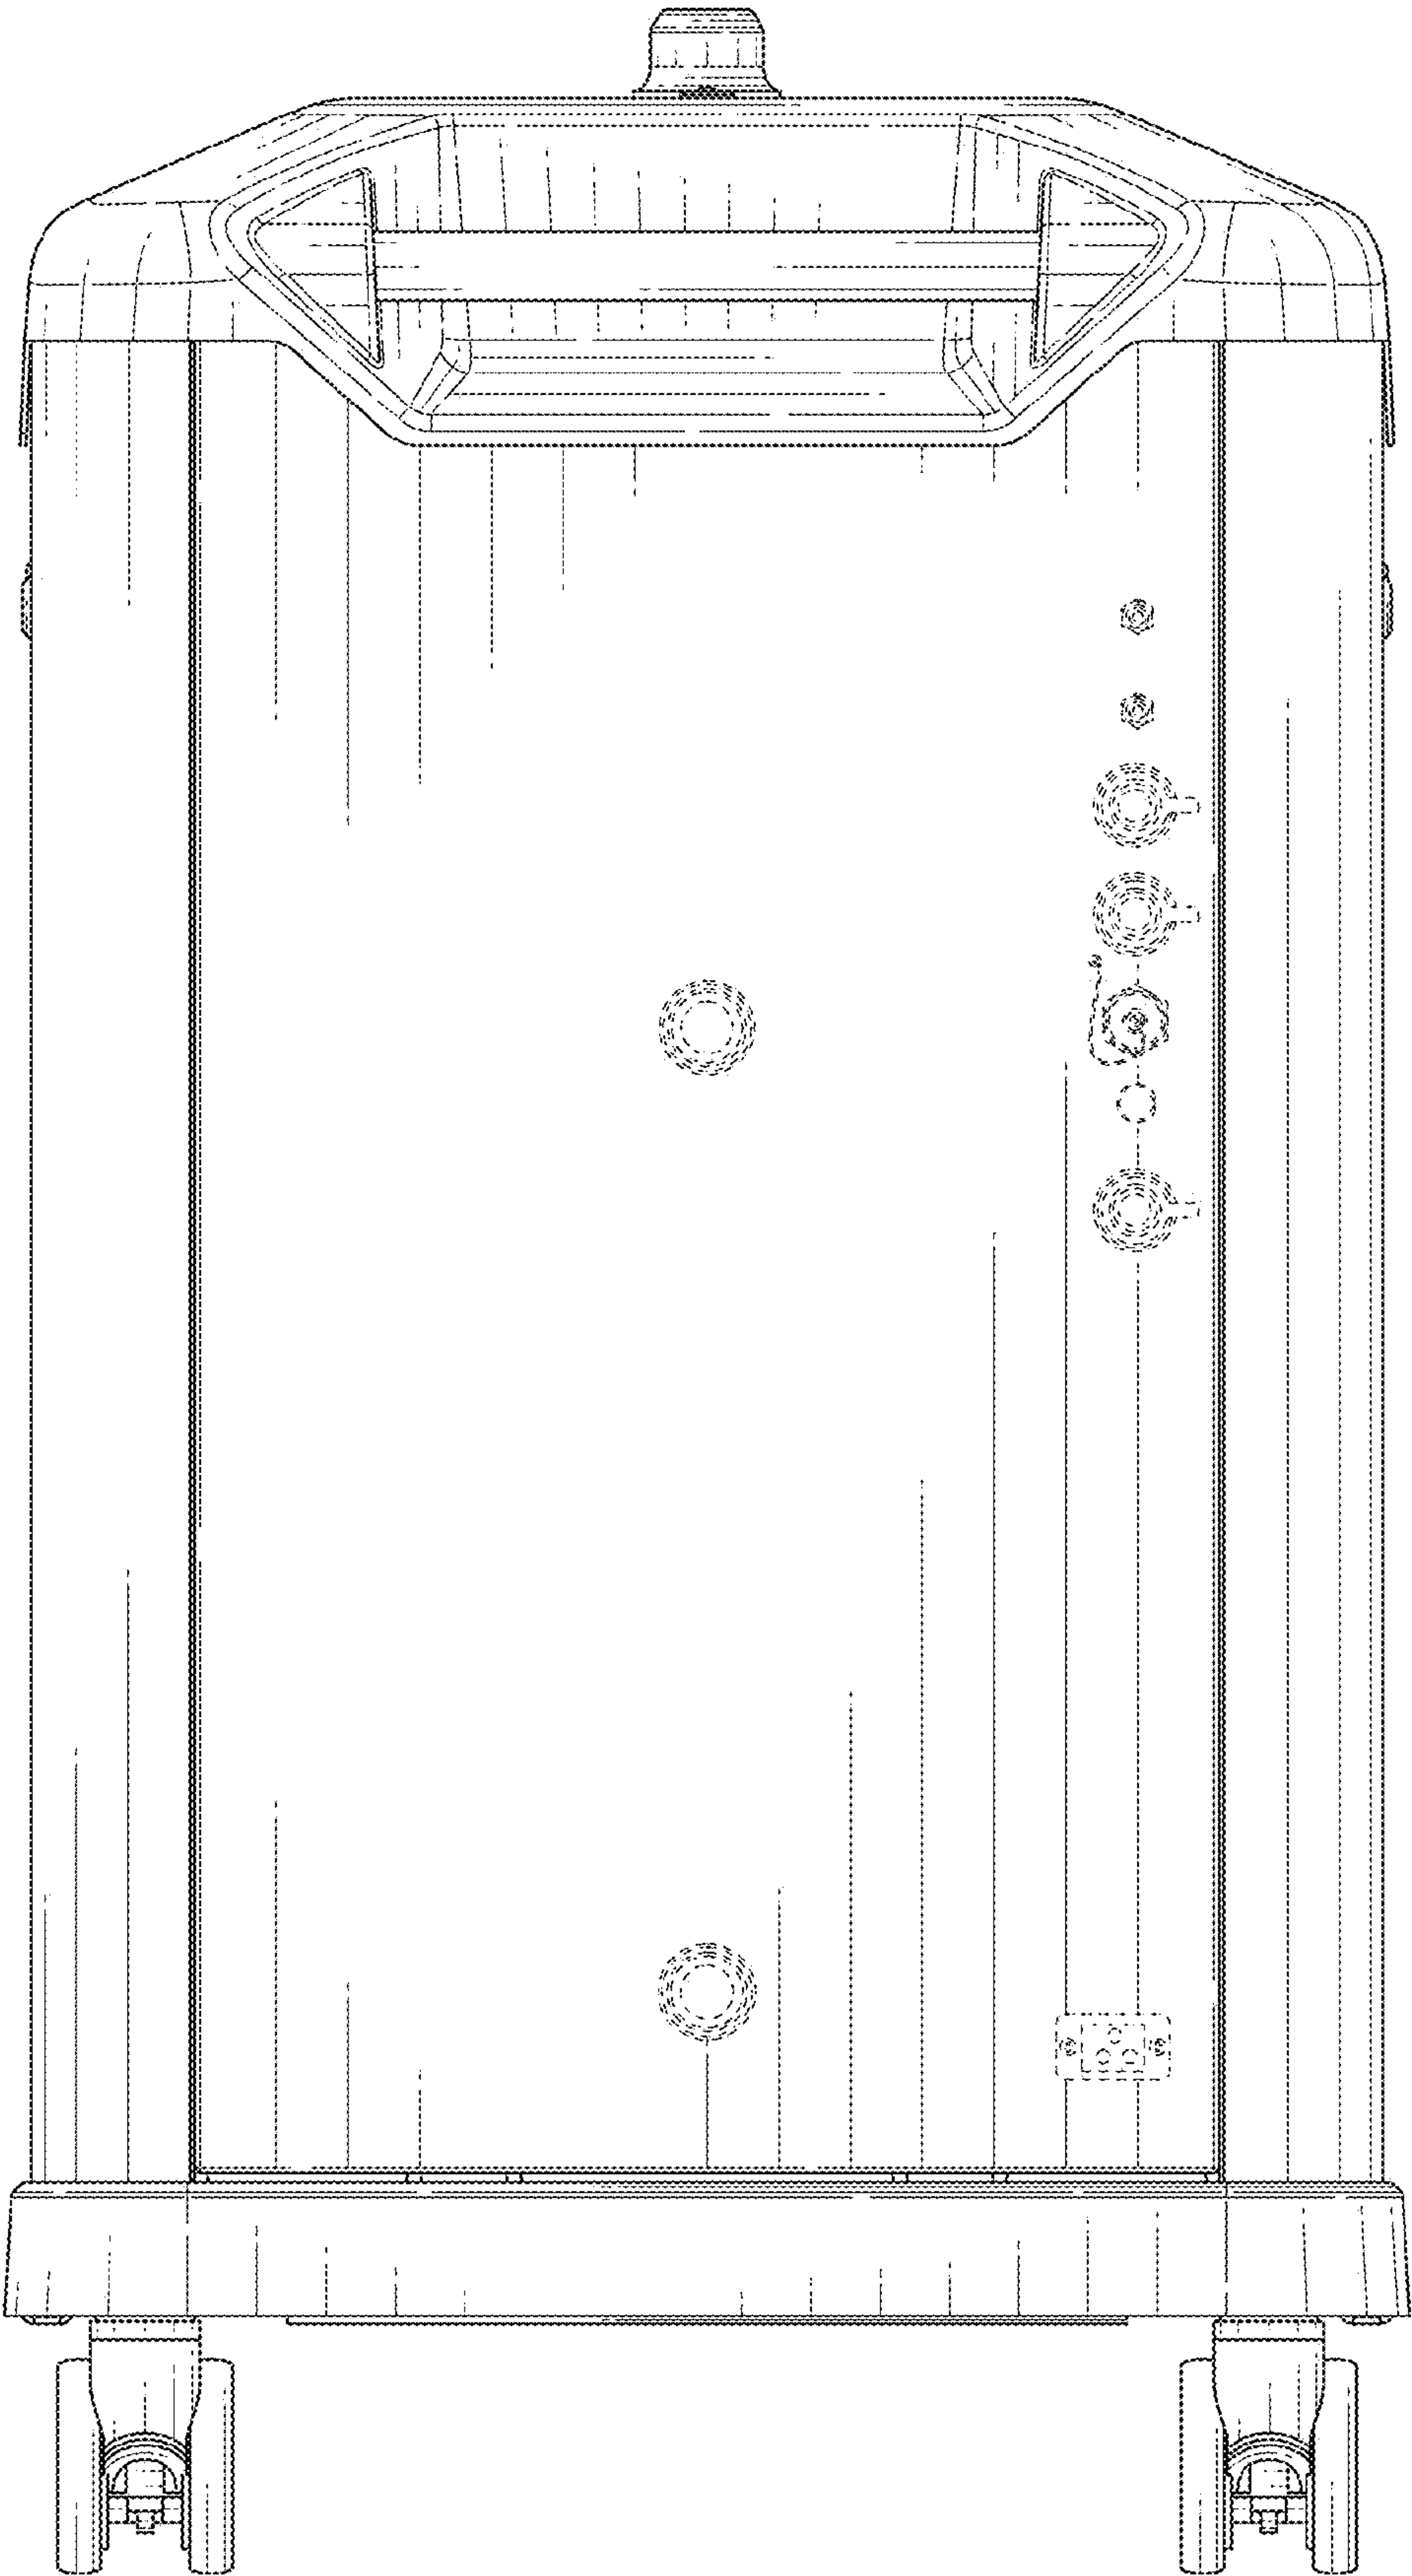


FIG. 24

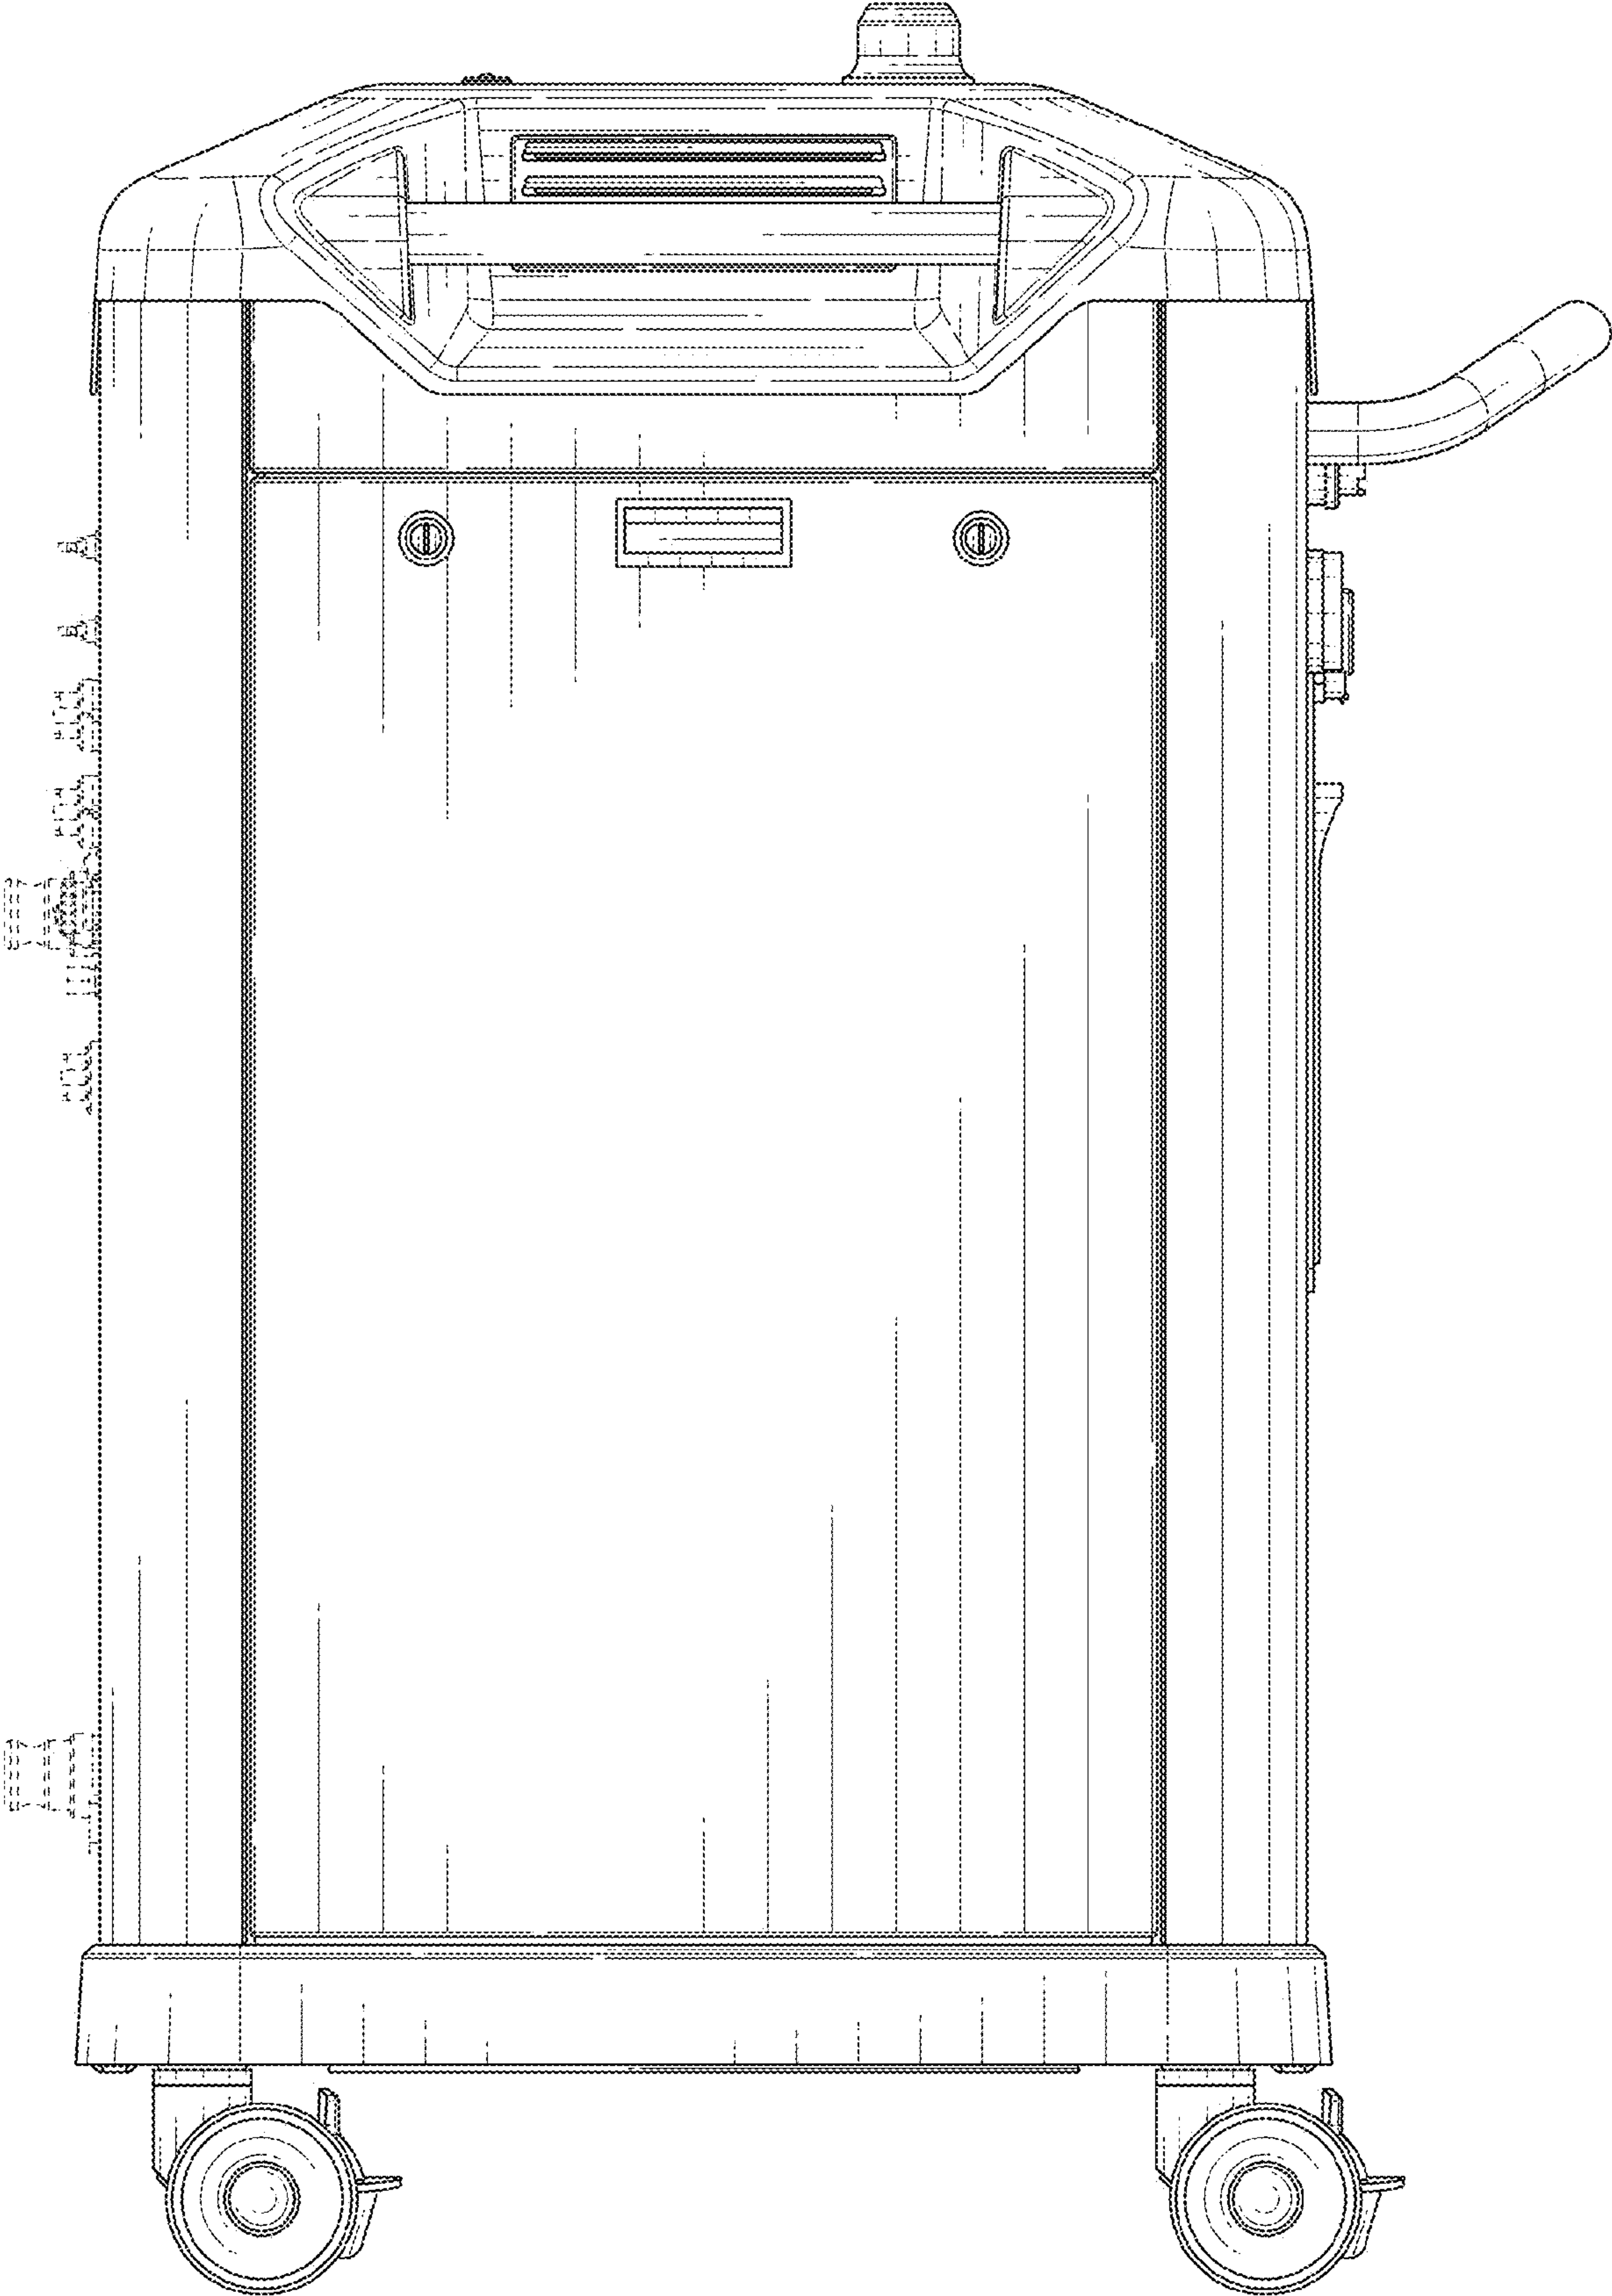


FIG. 25

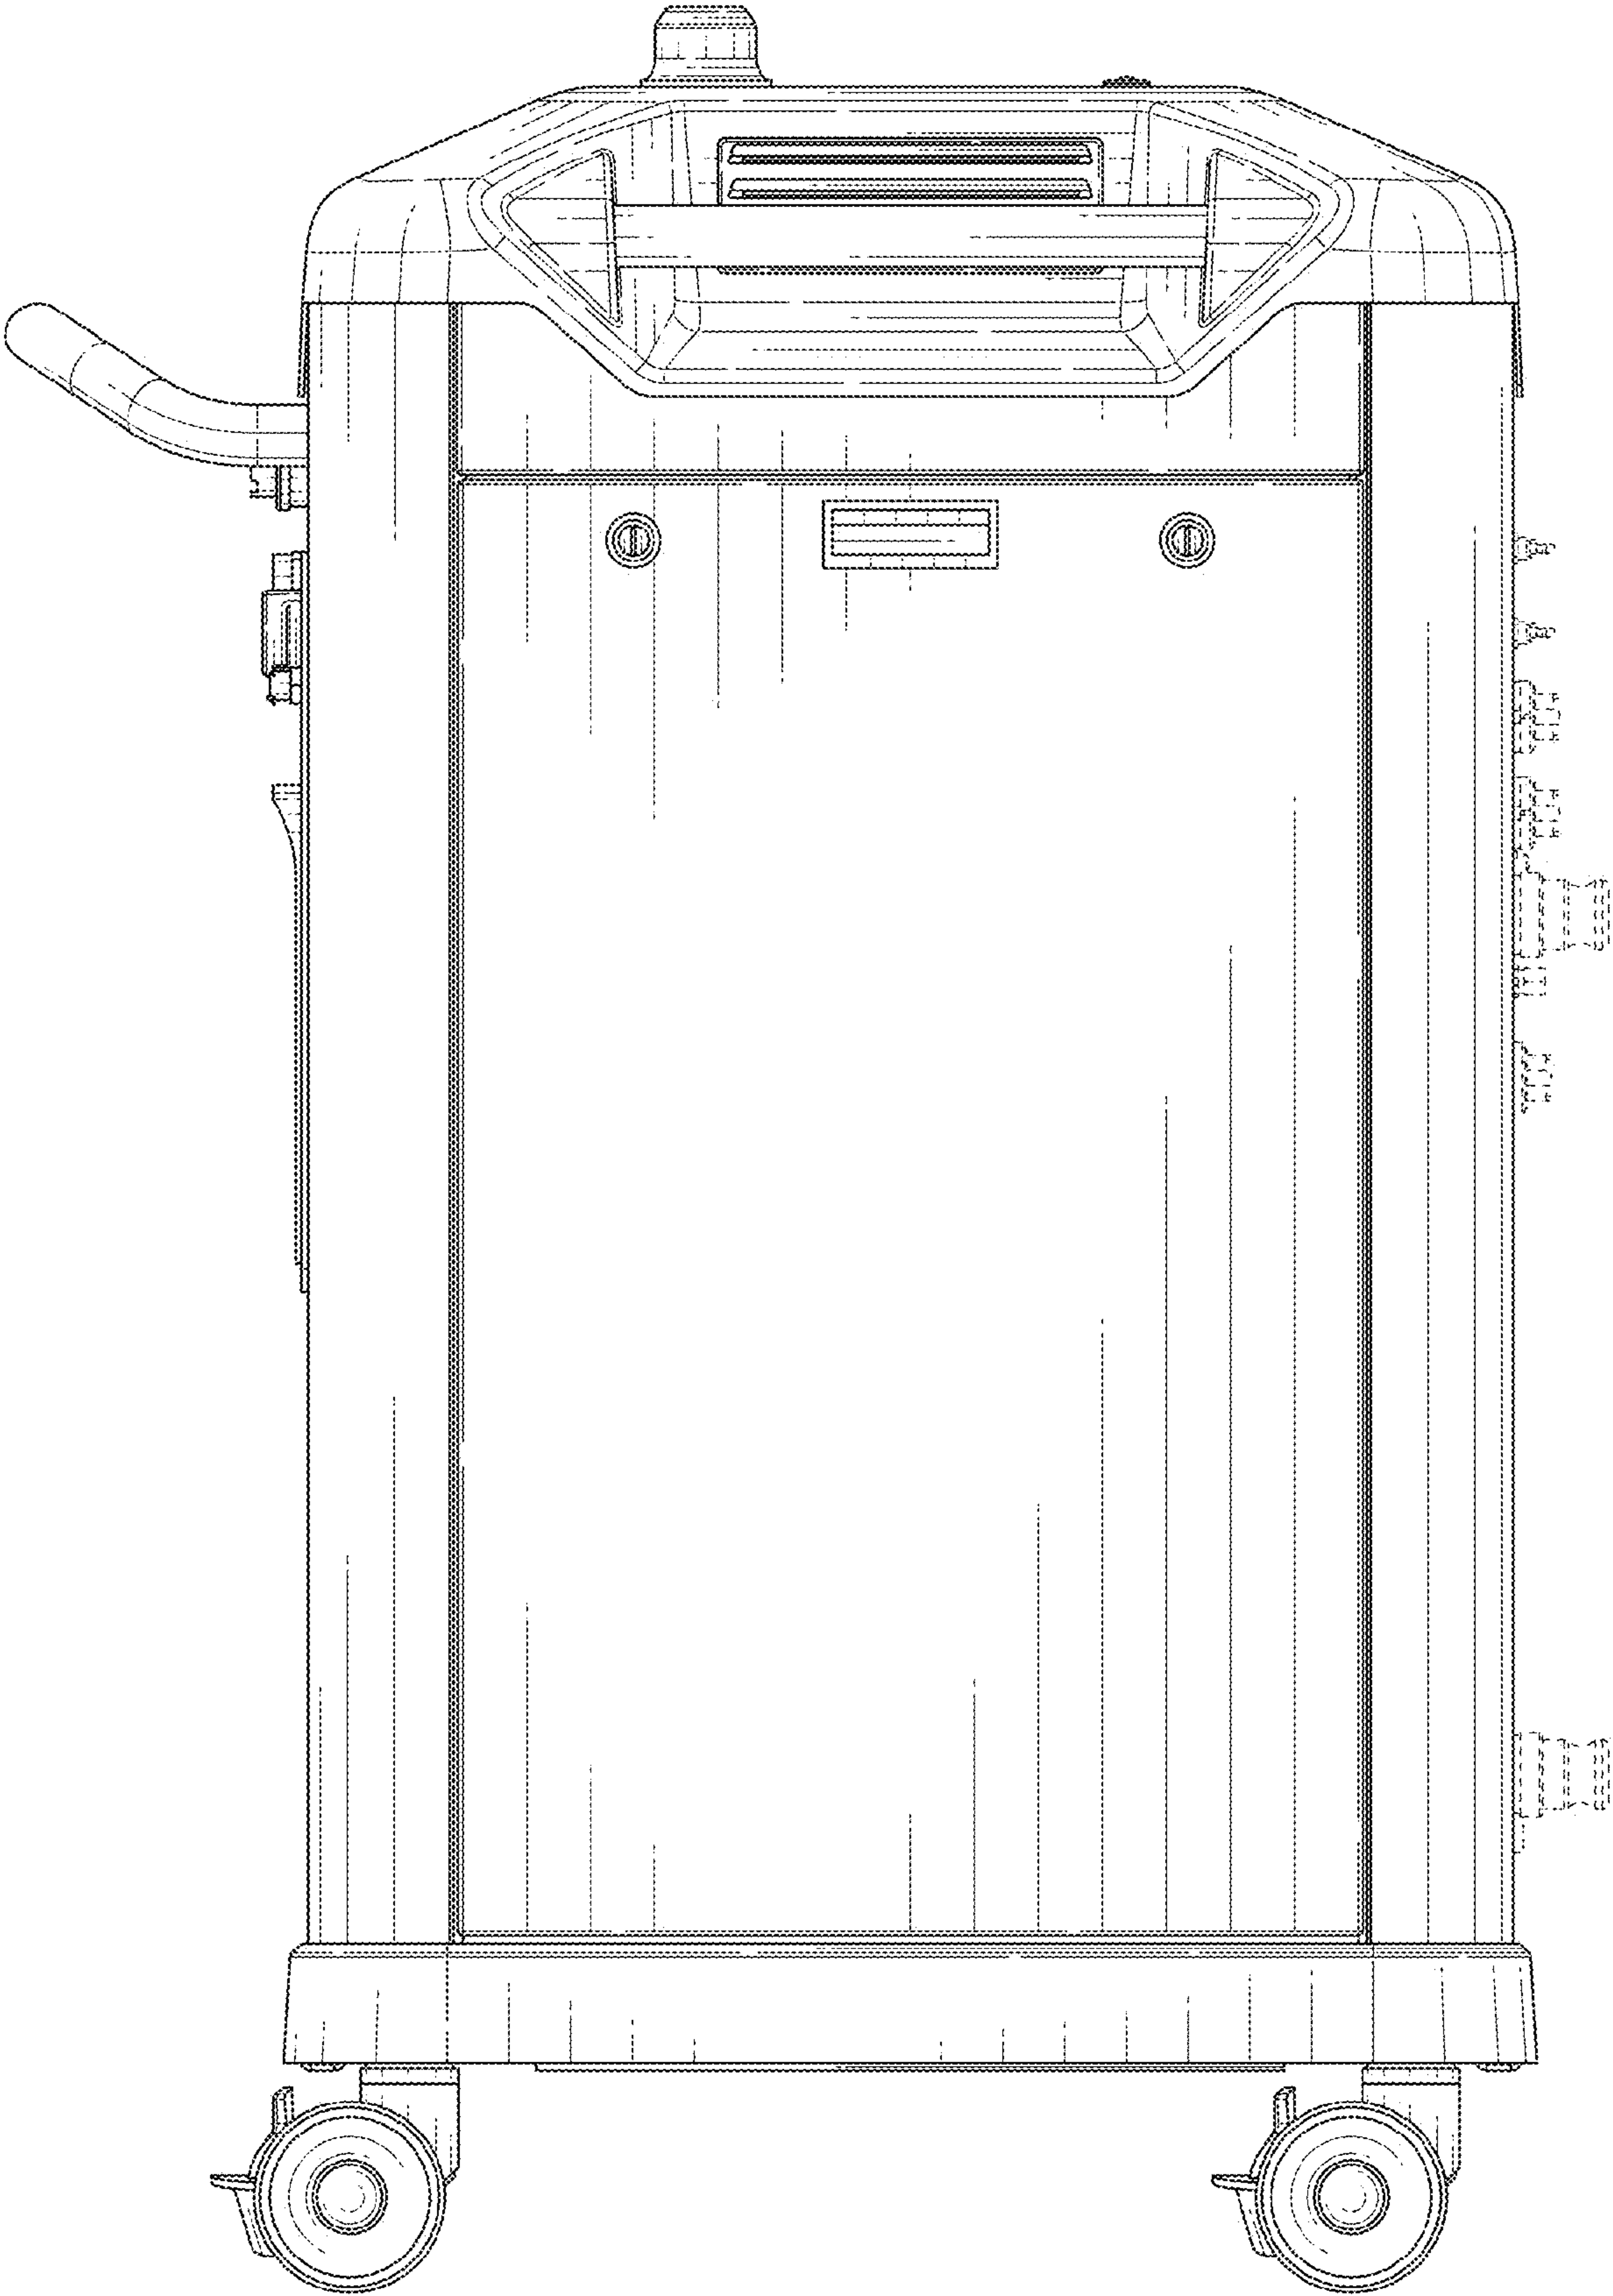


FIG. 26

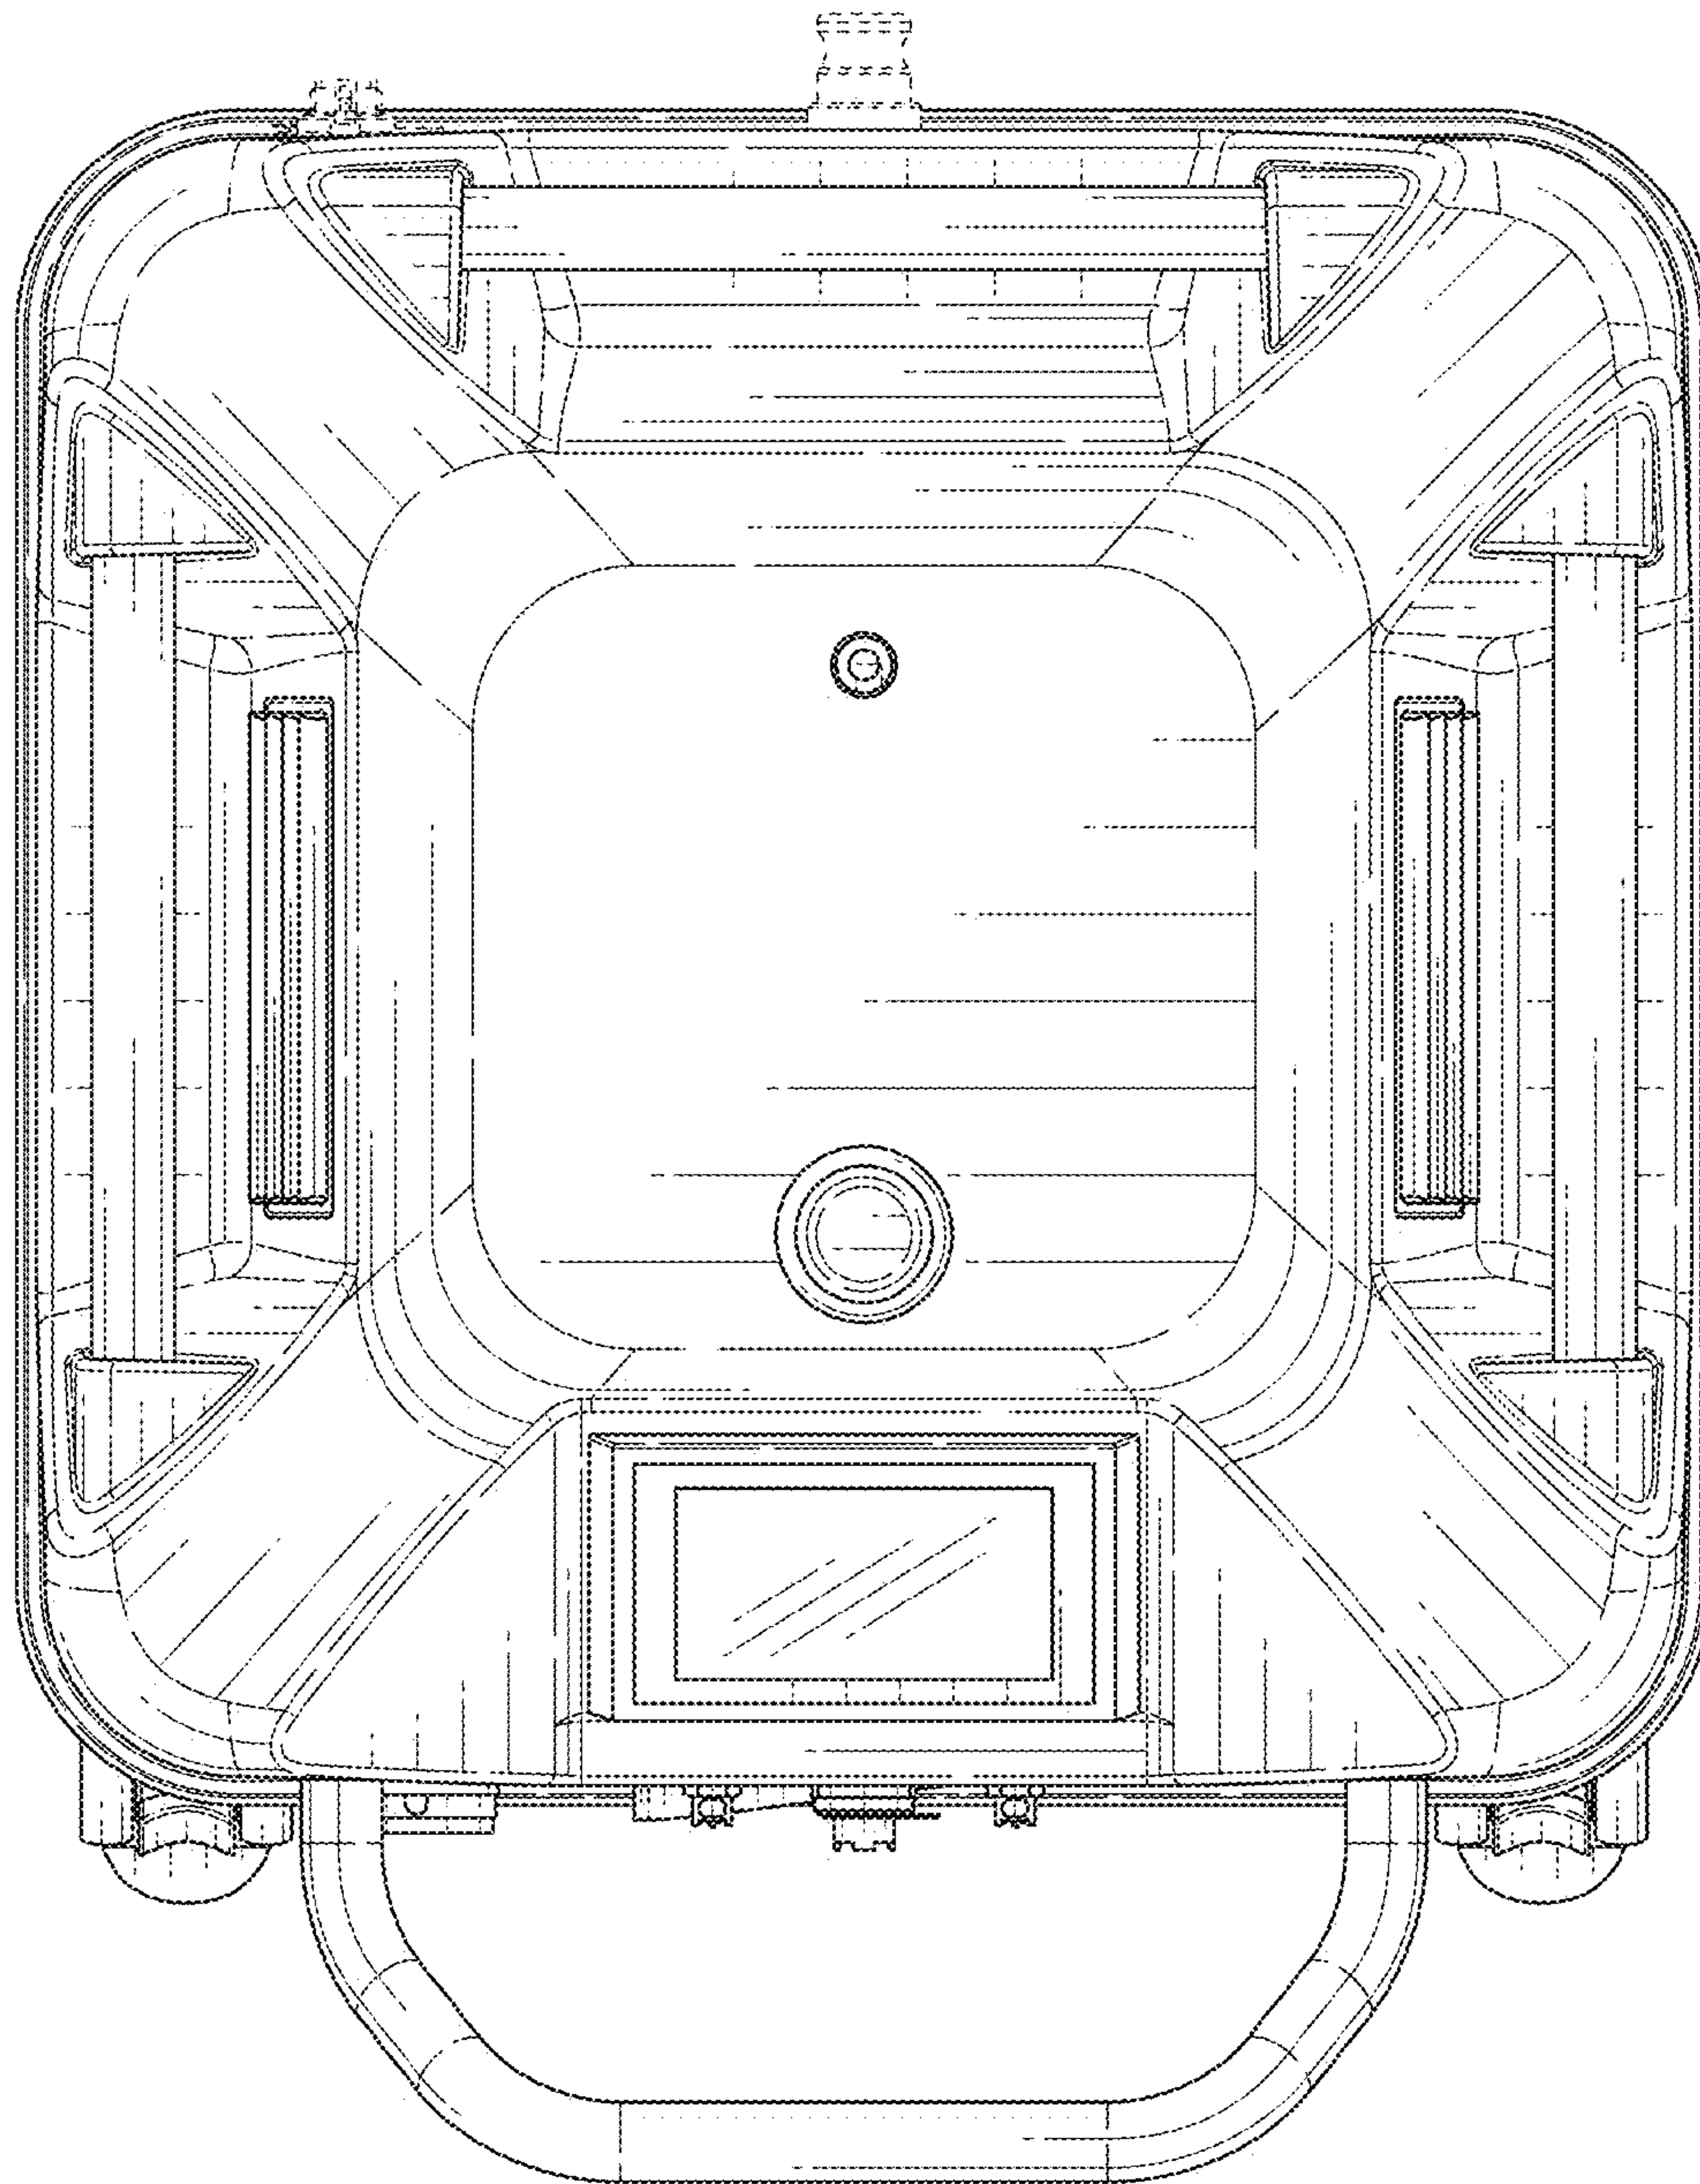


FIG. 27

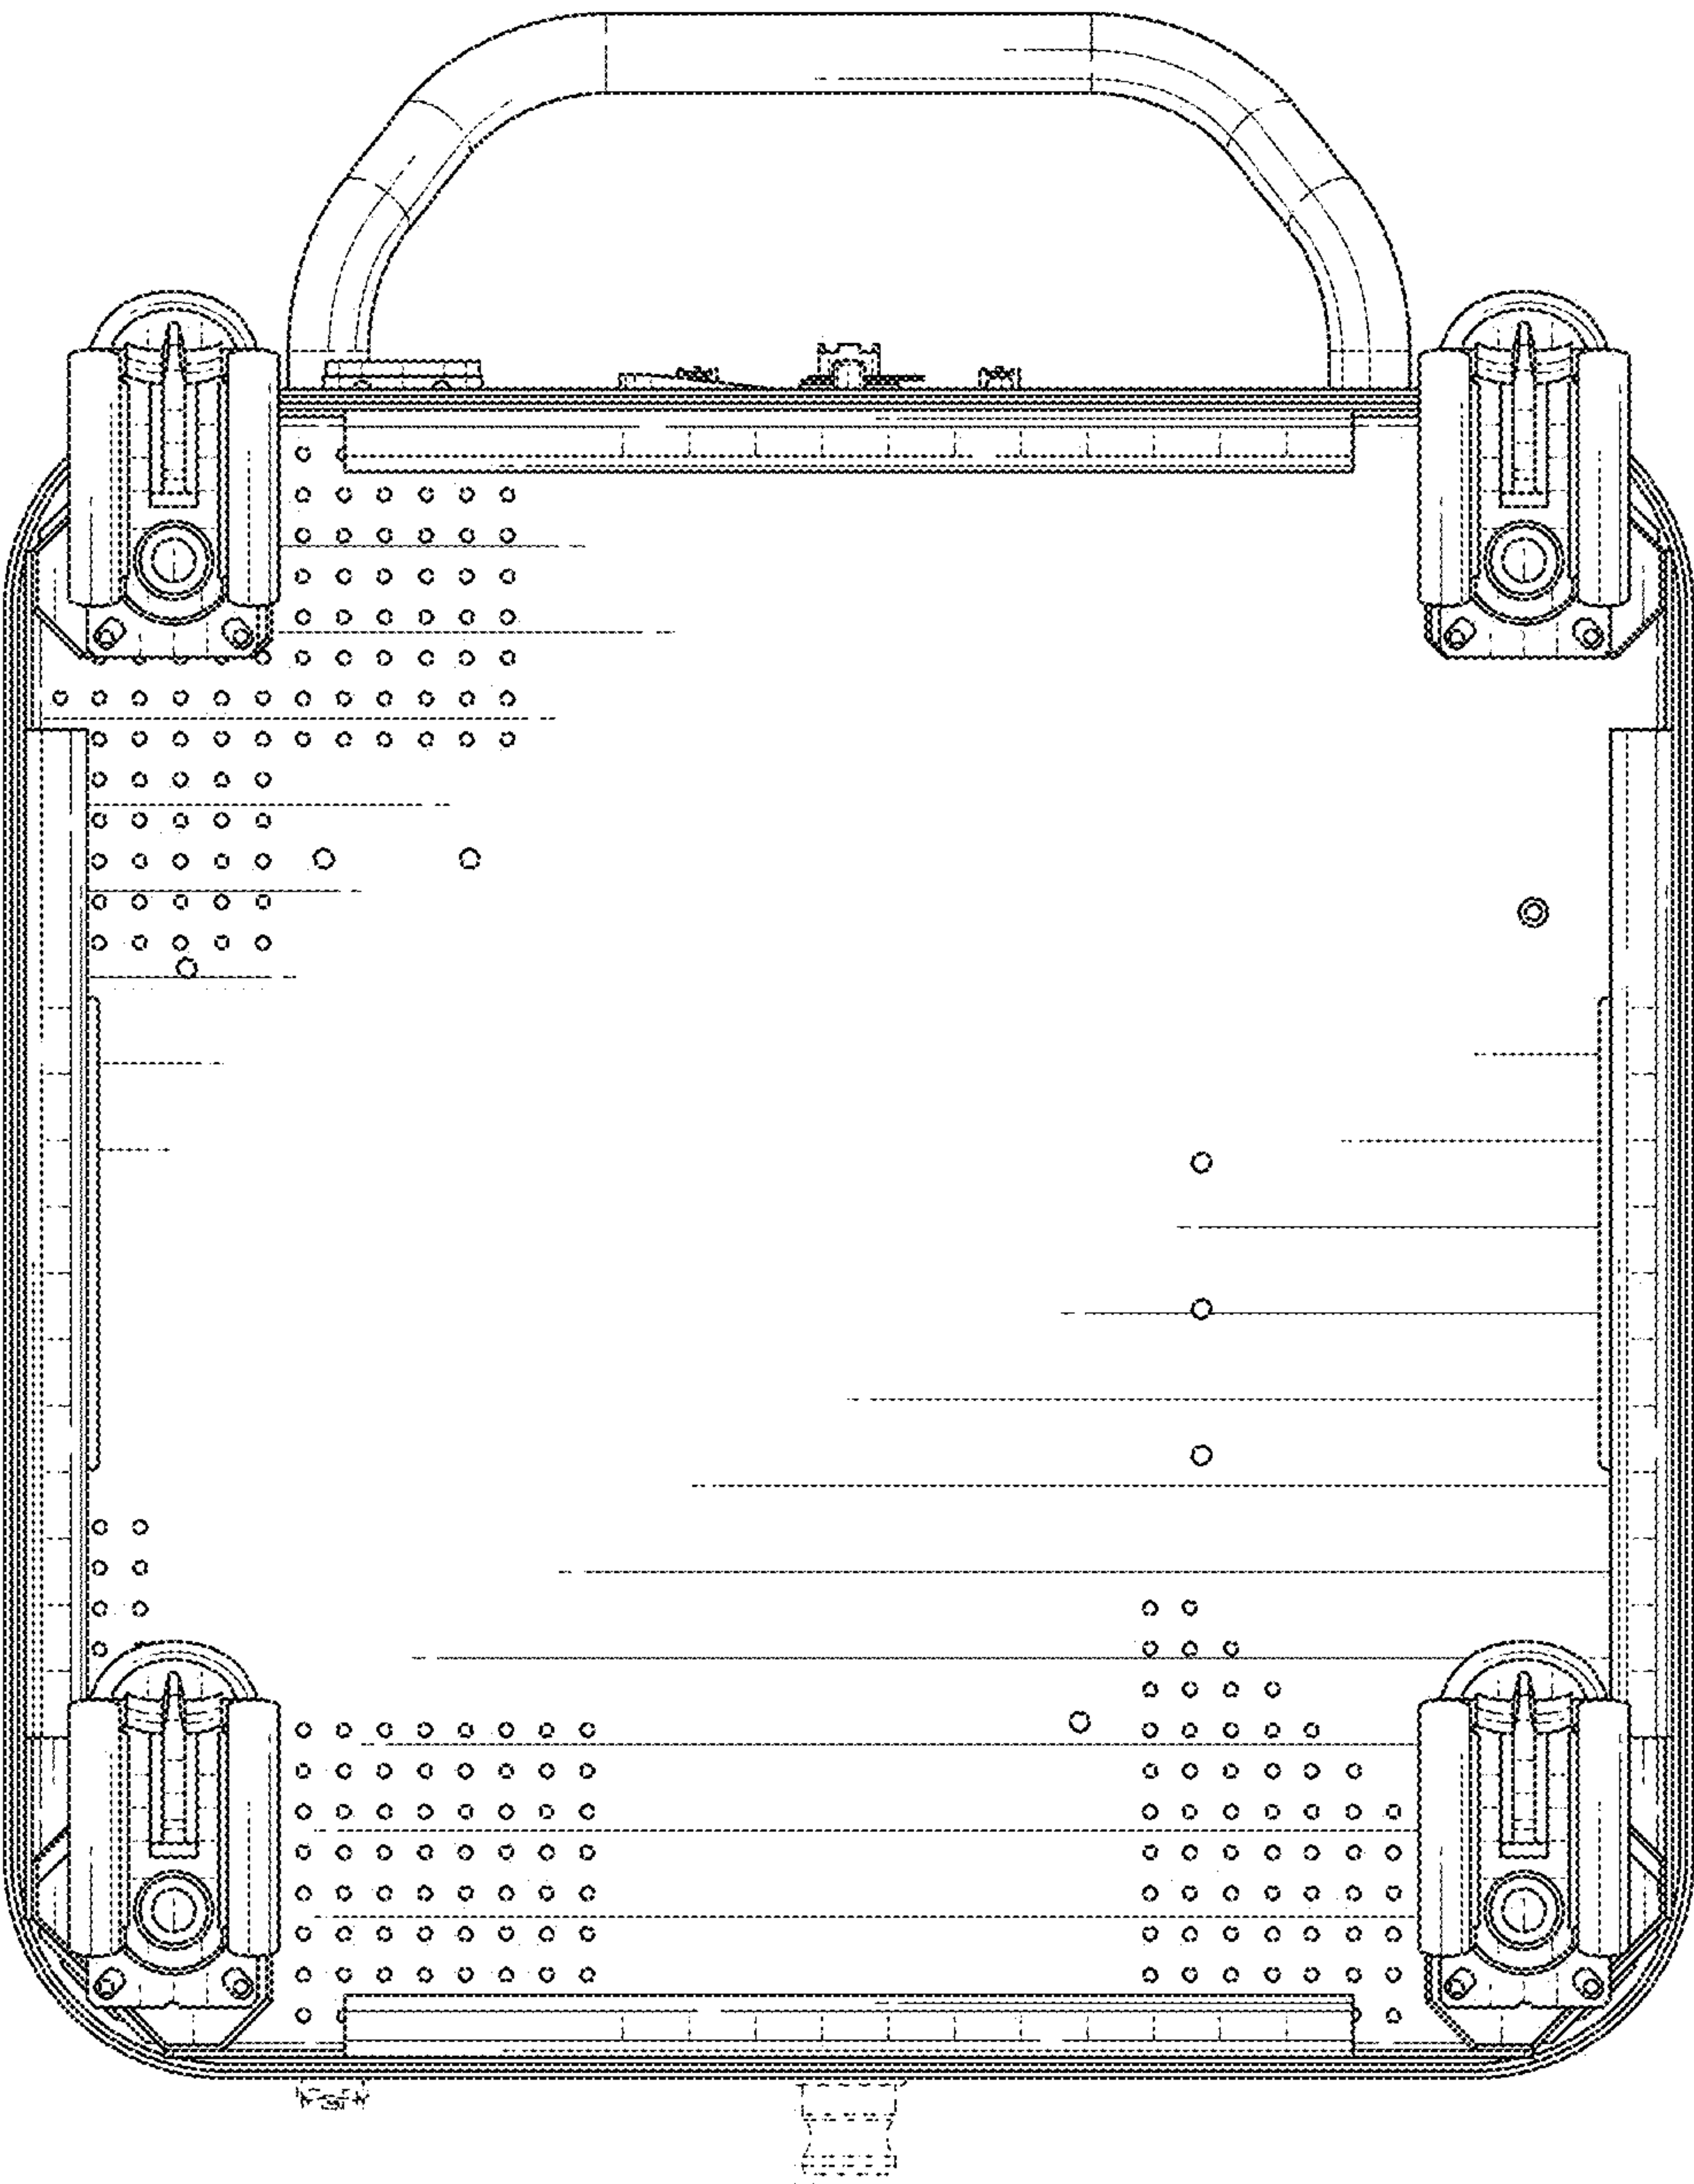


FIG. 28