



US0D1061453S

(12)

United States Design Patent

Duke et al.

(10)

Patent No.:

US D1,061,453 S

(45)

Date of Patent:

** Feb. 11, 2025

(54) **HAND CONTROLLER APPARATUS FOR MEDICAL DEVICE**

(71) Applicant: **Titan Medical Inc.**, Toronto (CA)

(72) Inventors: **Jonathan Bradley Duke**, Louisville, CO (US); **Chad Clayton Walters**, Apex, NC (US); **Olivier Franck Currat**, Louisville, CO (US); **Eric Collins**, Louisville, CO (US)

(73) Assignee: **Titan Medical Inc.**, Toronto (CA)

(**) Term: **15 Years**

(21) Appl. No.: **29/865,565**

(22) Filed: **Aug. 1, 2022**

Related U.S. Application Data

(62) Division of application No. 29/668,353, filed on Oct. 30, 2018, now Pat. No. Des. 963,596.

(51) **LOC (15) Cl.** **14-03**

(52) **U.S. Cl.**
USPC **D13/168; D24/133**

(58) **Field of Classification Search**
USPC D13/168; D24/186, 168, 133, 144;
D14/205, 218, 412; D21/333
CPC A61B 34/30; A61B 34/75; A61B 34/76
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

4,980,626	A	12/1990	Hess
5,290,386	A	3/1994	Trudeau
5,482,409	A	1/1996	Dunning
5,741,113	A	4/1998	Bacchi
6,587,750	B2	7/2003	Gerbi et al.
8,353,897	B2	1/2013	Doyle

(Continued)

FOREIGN PATENT DOCUMENTS

CN	102973321	A	3/2013
CN	103687701	A	3/2014

(Continued)

OTHER PUBLICATIONS

Analog Devices, "Integrated AMR Angle Sensor and Signal Conditioner," Data Sheet ADA4571, Rev. 0, 2014, 21 pages.
(Continued)

Primary Examiner — T Chase Nelson
Assistant Examiner — Kelly L Gross
(74) *Attorney, Agent, or Firm* — Knobbe, Martens, Olson & Bear LLP


(57) **CLAIM**

The ornamental design for a hand controller apparatus for a medical device, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of a hand controller apparatus for a medical device.
FIG. 2 is a front view of the hand controller apparatus of FIG. 1.
FIG. 3 is a rear view of the hand controller apparatus of FIG. 1.
FIG. 4 is a left side view of the hand controller apparatus of FIG. 1.
FIG. 5 is a right side view of the hand controller apparatus of FIG. 1.
FIG. 6 is a top plan view of the hand controller apparatus of FIG. 1; and,
FIG. 7 is a bottom plan view of the hand controller apparatus of FIG. 1.
The broken lines depict portions of the hand controller apparatus for a medical device that form no part of the claimed design.

1 Claim, 5 Drawing Sheets

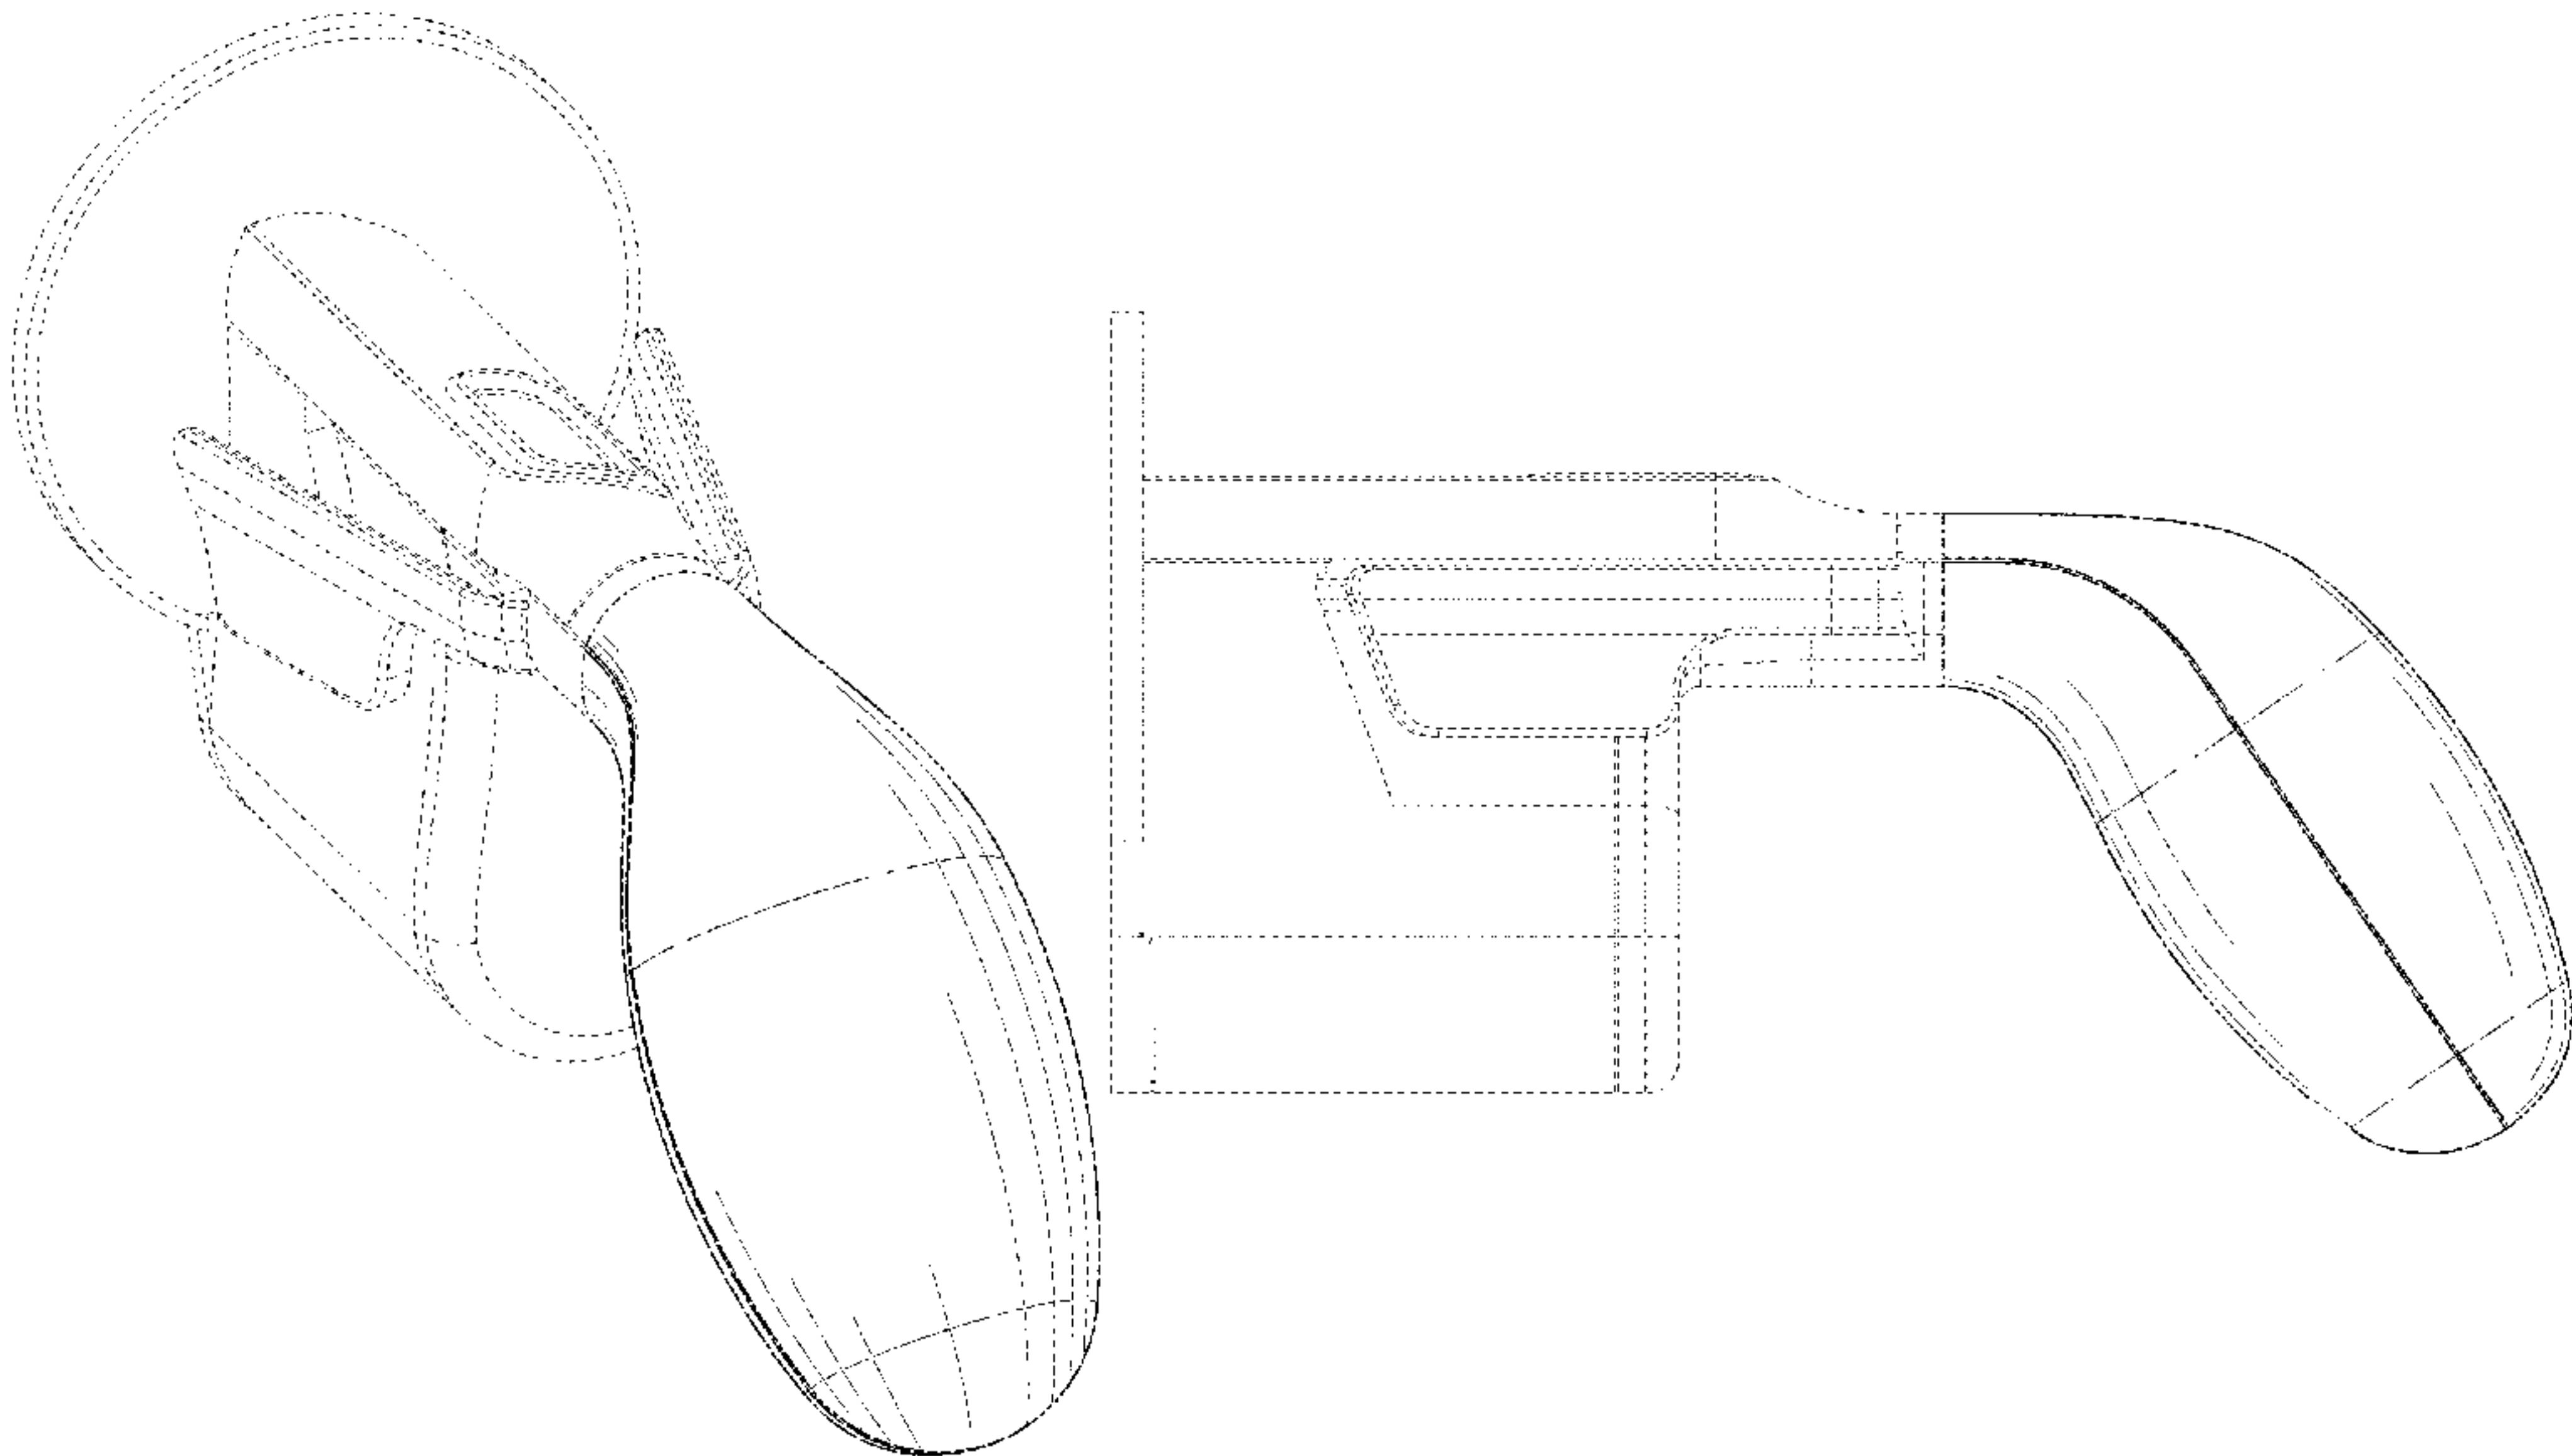

(56)

References Cited**U.S. PATENT DOCUMENTS**

8,638,057 B2 1/2014 Goldberg et al.
D813,203 S 3/2018 Hardi
D817,300 S 5/2018 Bristol
D840,360 S 2/2019 Scott
10,426,561 B1 10/2019 Kelly et al.
D867,309 S 11/2019 Detering
D882,529 S 4/2020 Scott
D900,042 S 10/2020 Scott
D905,164 S * 12/2020 Adams D21/333
10,875,182 B2 12/2020 Wang
D910,845 S 2/2021 Kwon
D963,596 S * 9/2022 Duke D13/168
D995,485 S * 8/2023 Chen D14/218
D995,638 S * 8/2023 O'Doherty D21/566
D1,003,256 S * 10/2023 Peralta D13/168
D1,005,484 S * 11/2023 Treen D24/133
D1,010,590 S * 1/2024 Li D10/50
D1,013,879 S * 2/2024 Murray D14/428
D1,017,802 S * 3/2024 Behrendt D24/133
D1,017,803 S * 3/2024 Behrendt D24/133
D1,018,536 S * 3/2024 Wang D14/218
D1,018,843 S * 3/2024 Behrendt D24/133
D1,020,665 S * 4/2024 Gasta D13/168
D1,025,356 S * 4/2024 Treen D24/133
D1,025,951 S * 5/2024 Mai D14/205
D1,028,230 S * 5/2024 Payne D24/133
D1,028,911 S * 5/2024 Li D13/168
D1,029,111 S * 5/2024 Ritchie D14/412
D1,029,251 S * 5/2024 Ueda D24/138
D1,029,274 S * 5/2024 Bechtel D24/186
D1,031,196 S * 6/2024 Lin D32/51
D1,031,674 S * 6/2024 Song D13/168
D1,036,552 S * 7/2024 Wei D21/333
D1,038,046 S * 8/2024 PrevotEAU D14/218
D1,038,132 S * 8/2024 Zhang D14/412
D1,039,053 S * 8/2024 Lin D21/333
D1,039,505 S * 8/2024 Zhou D13/168
D1,039,618 S * 8/2024 Wu D21/333
D1,040,771 S * 9/2024 Huang D14/218
D1,042,638 S * 9/2024 Qiu D14/218
2003/0045900 A1 3/2003 Hahnen
2008/0232932 A1 9/2008 Jinno
2009/0058342 A1 3/2009 Nihei
2010/0080669 A1 4/2010 Labonville et al.
2010/0161129 A1 6/2010 Costa
2010/0318059 A1 12/2010 Farritor
2011/0020779 A1 1/2011 Hannaford
2011/0077478 A1 3/2011 Freeman
2011/0118748 A1 5/2011 Itkowitz
2012/0234893 A1 9/2012 Schuchkmann
2013/0211590 A1 8/2013 Diolaiti et al.
2014/0276931 A1 9/2014 Parihar
2015/0025549 A1 1/2015 Kilroy
2015/0080924 A1 3/2015 Stulen et al.
2016/0066913 A1 3/2016 Swayze et al.
2017/0151013 A1 6/2017 Kappus

2017/0225337 A1 8/2017 Schaible et al.
2017/0361225 A1 12/2017 Goslin
2017/0367777 A1 12/2017 Kralicky et al.
2018/0168758 A1 6/2018 Lutzow et al.
2018/0271607 A1 9/2018 Kralicky et al.
2020/0129249 A1 4/2020 Kelly
2024/0164771 A1 * 5/2024 Wenchell, Jr. A61B 17/068
2024/0252232 A1 * 8/2024 Sims A61B 18/1445

FOREIGN PATENT DOCUMENTS

WO WO 2013/018934 A1 2/2013
WO WO 2016/201544 A1 12/2016
WO WO 2017/177547 A1 10/2017
WO WO 2017/210501 A1 12/2017
WO WO 2018/217435 A1 11/2018

OTHER PUBLICATIONS

Azoteq (Pty) Ltd, "IQS550/572/525-B000—Capacitive Trackpad/Touchscreen Controller," IQS5xx-B000 Trackpad Datasheet, Revision 2.0, Nov. 2016, 79 pages.
Integrated Device Technology, Inc., "IDT Inductive Position Sensors," 2017, 13 pages.
Integrated Device Technology, Inc., "Inductive Position Sensor IC," ZMID5201/02/03 Datasheet, Jun. 22, 2018, 33 pages.
Integrated Device Technology, Inc., "ZMID520x Evaluation Kit User Manual," Dec. 10, 2017, 39 pages.
Integrated Device Technology, Inc., "ZMID520x Inductive Position Sensor Family," Product Overview, 2018, 2 pages.
Integrated Device Technology, Inc., "ZMID520xMARC13001 Arc Application Module User Manual," Dec. 12, 2017, 15 pages.
International Search Report and Written Opinion mailed Feb. 7, 2020 in International Application No. PCT/US2019/058170, in 8 pages.
Intuitive Surgical, "da Vinci SP," downloaded on Oct. 9, 2018 from <https://www.intuitivesurgical.com/sp/>, in 5 pages.
Kasemsadeh, "LDC1612/LDC1614 Linear Position Sensing," Application Report SNOA931, Texas Instruments, Apr. 2015, 14 pages.
Microchip Technology Inc., "AT42QT1011 Data Sheet," 2017, 31 pages.
MPS, "14-Bit, Digital, Contactless Angle Sensor with ABZ Incremental & PWM Outputs," MagAlpha MA730, Rev. 1.01, Oct. 13, 2017, 27 pages.
SMSC, "8 Channel Capacitive Touch Sensor with 8 LED Drivers," CAP1188 Datasheet, Revision 1.32, Jan. 5, 2012, 93 pages.
Texas Instruments, "DRV2605L 2- to 5.2-V Haptic Driver for LRA and ERM with Effect Library and Smart-Loop Architecture," May 2014, Revised Mar. 2018, 70 pages.
Texas Instruments, "LDC1612, LDC1614 Multi-Channel 28-Bit Inductance to Digital Converter (LDC) for Inductive Sensing," Dec. 2014, Revised Mar. 2018, 65 pages.

* cited by examiner

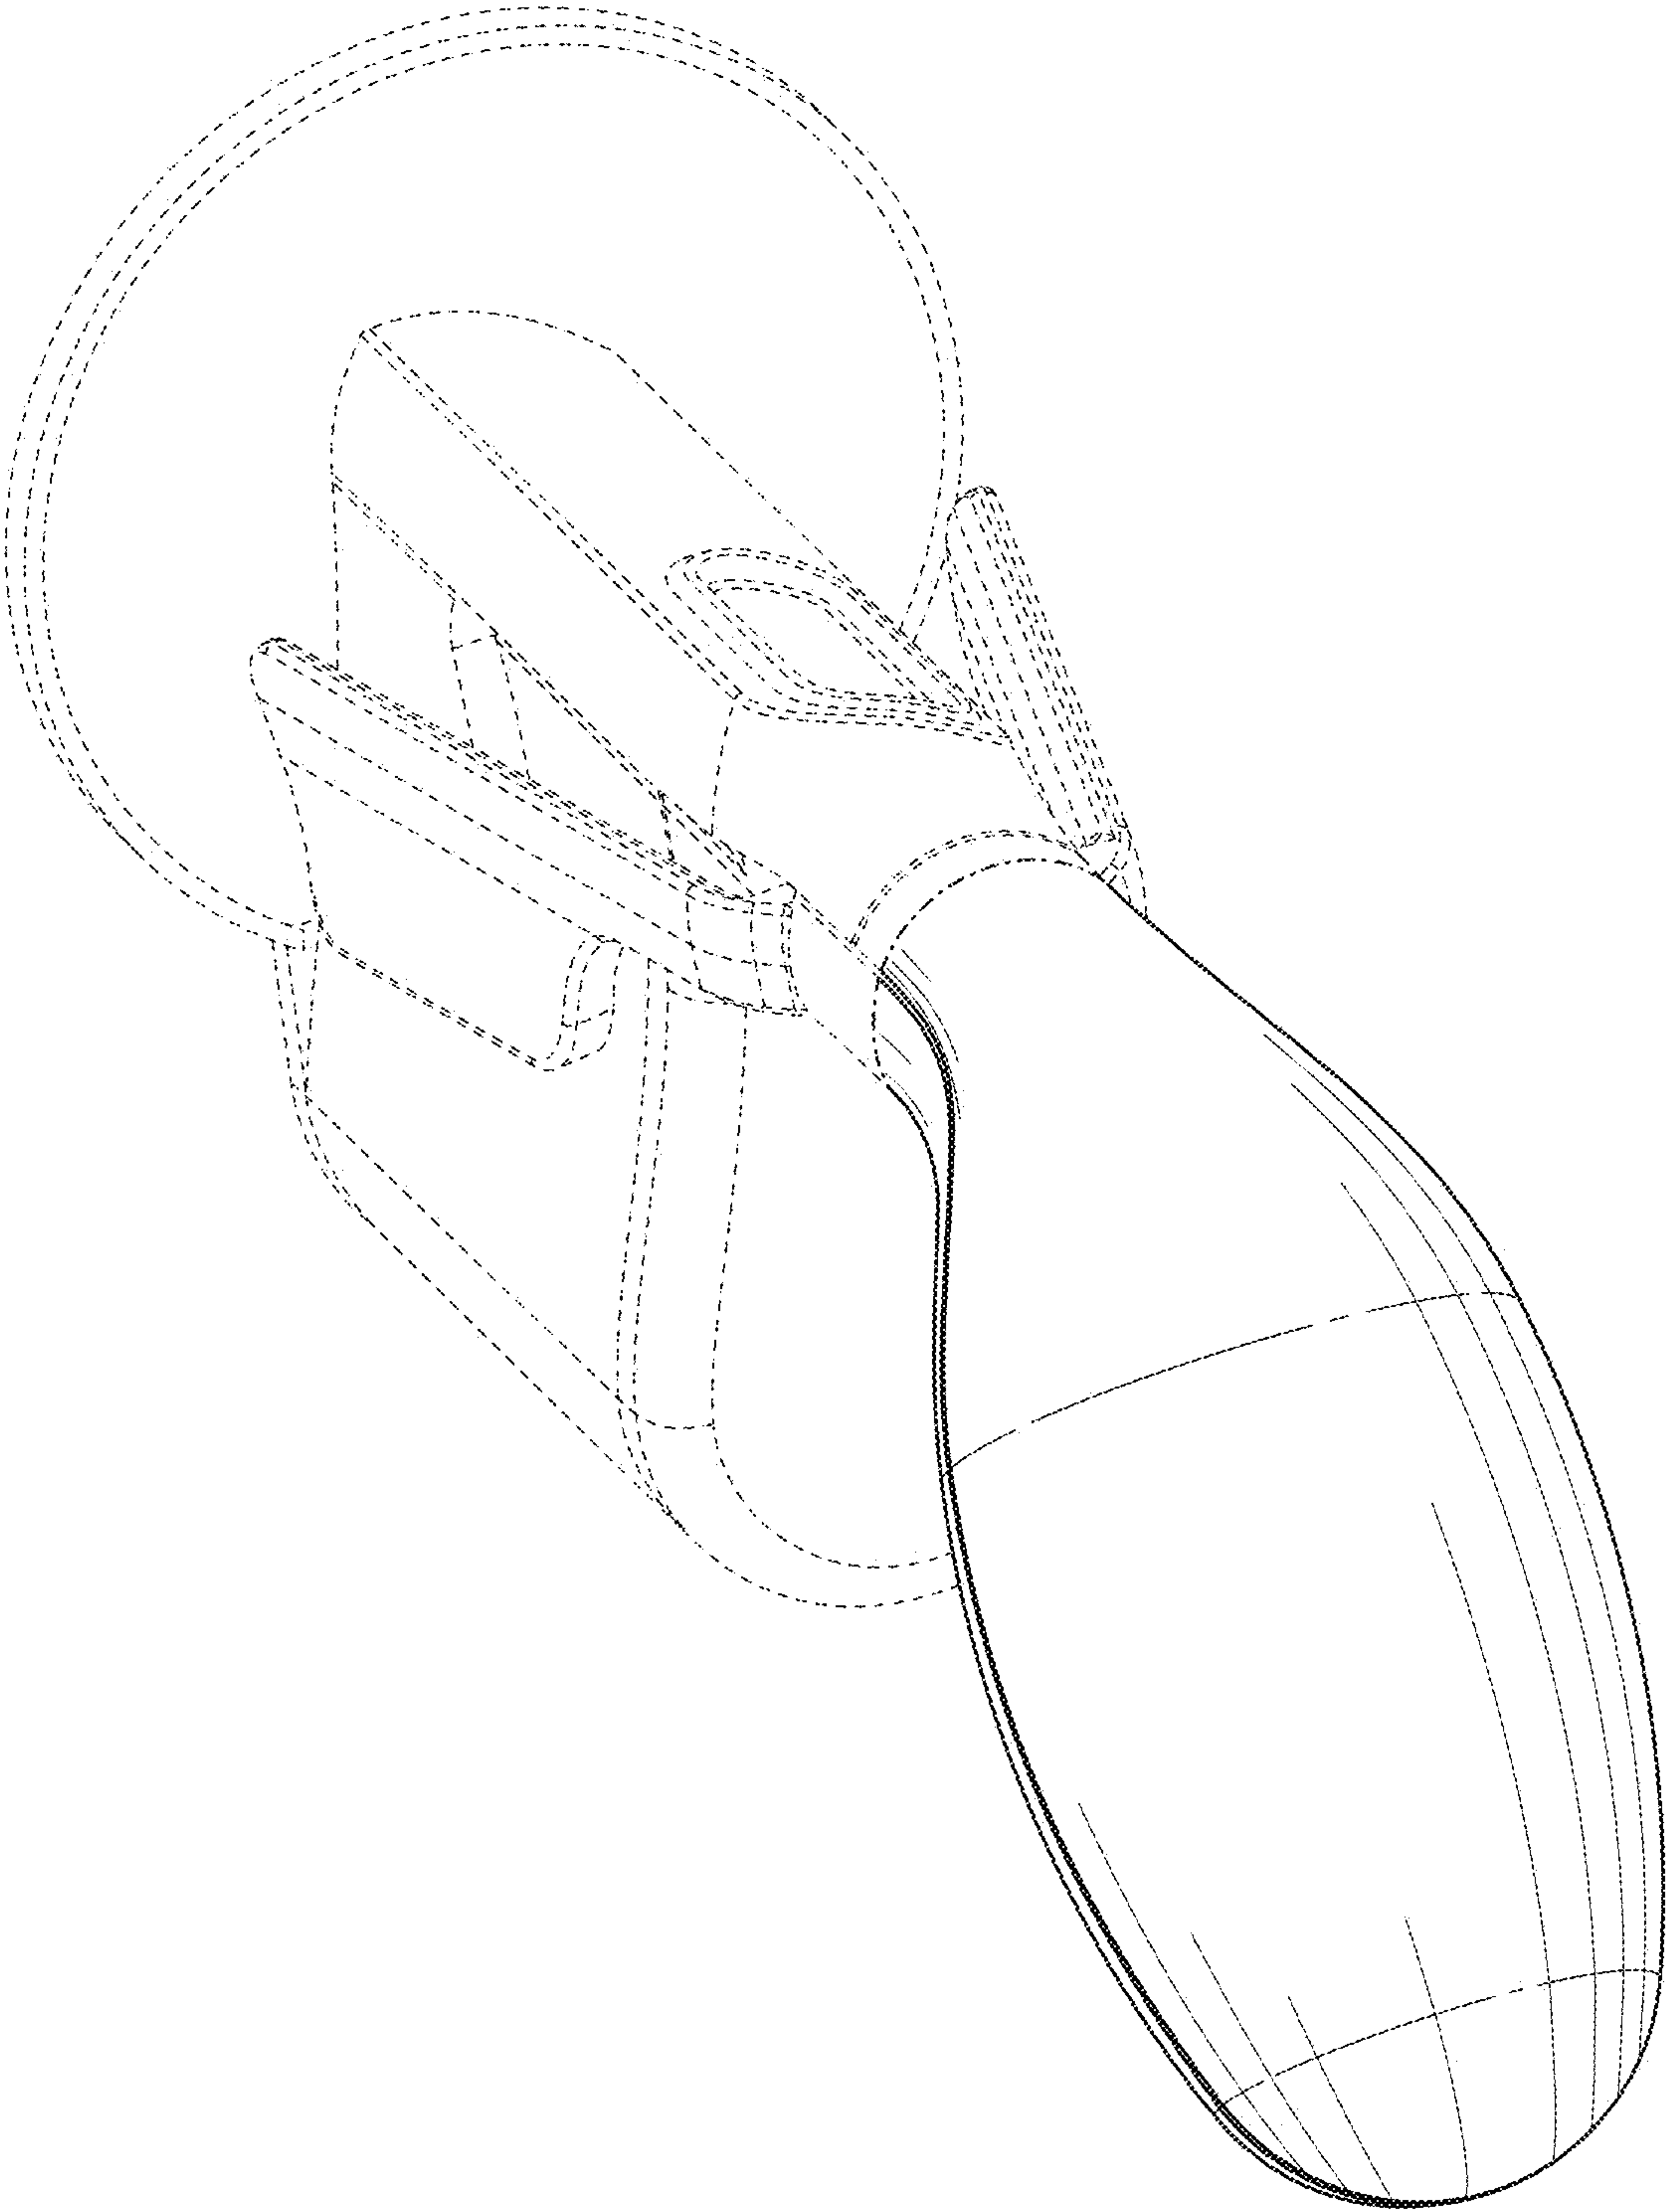


FIG. 1

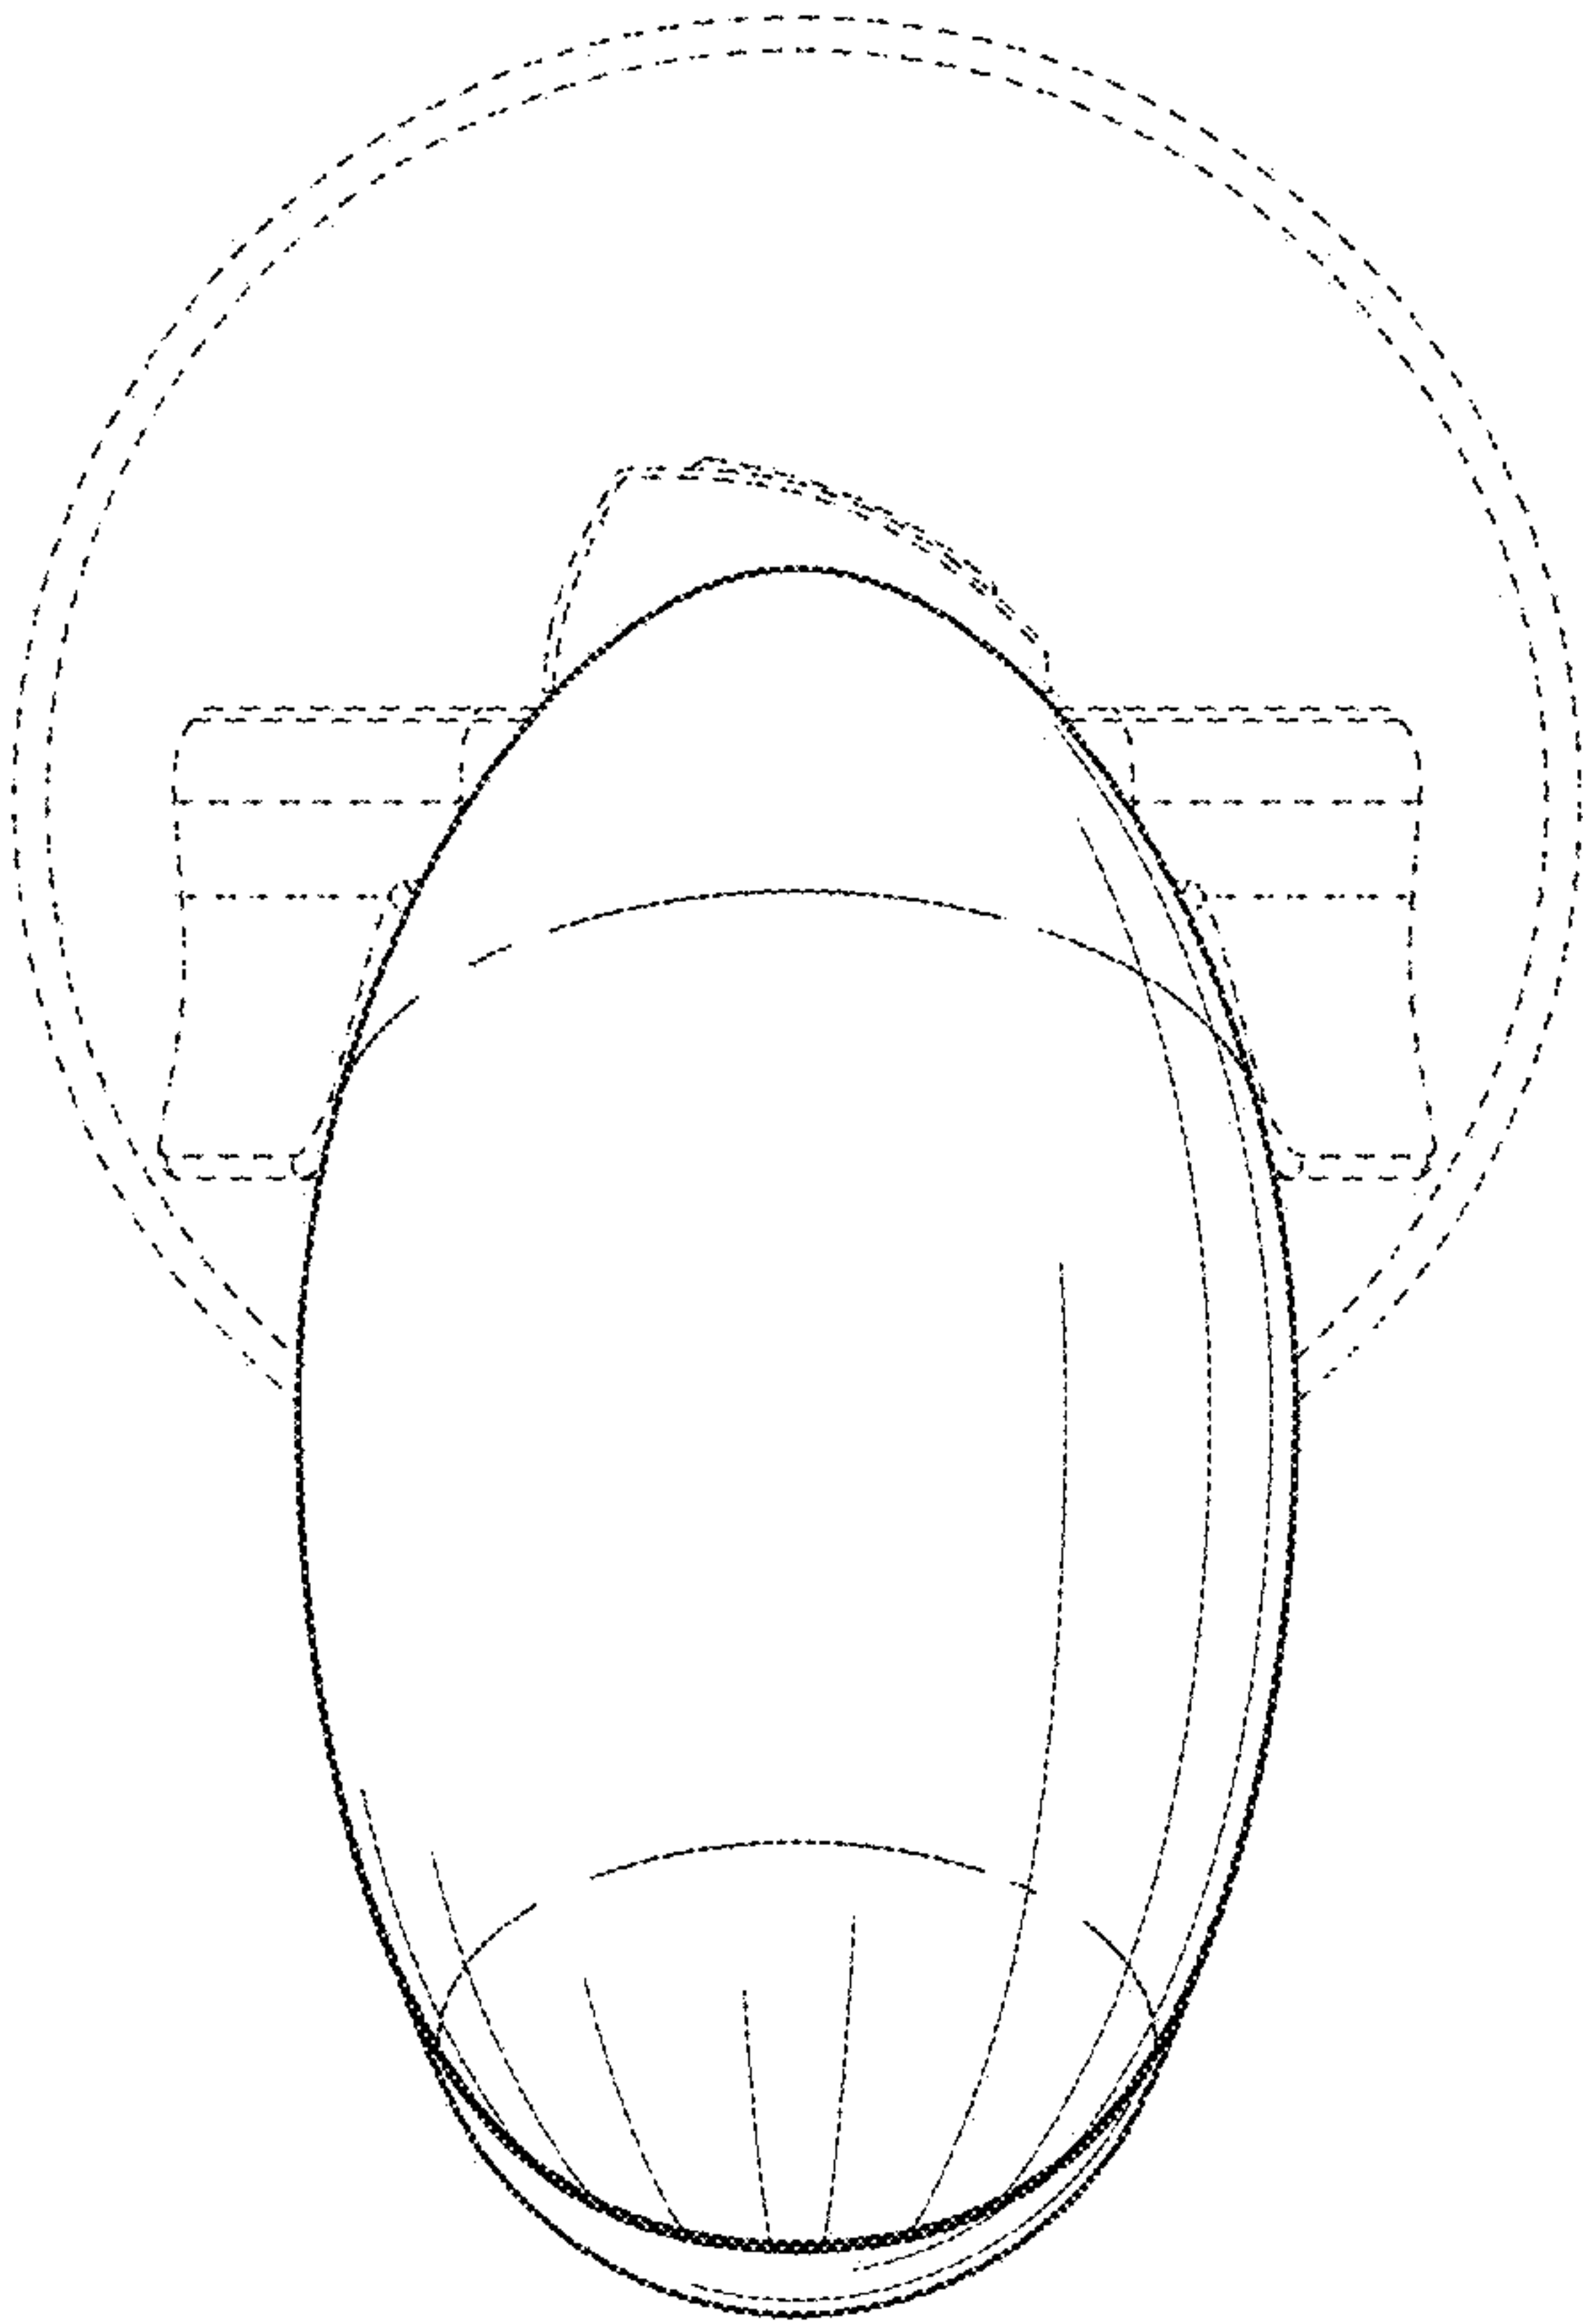


FIG. 2

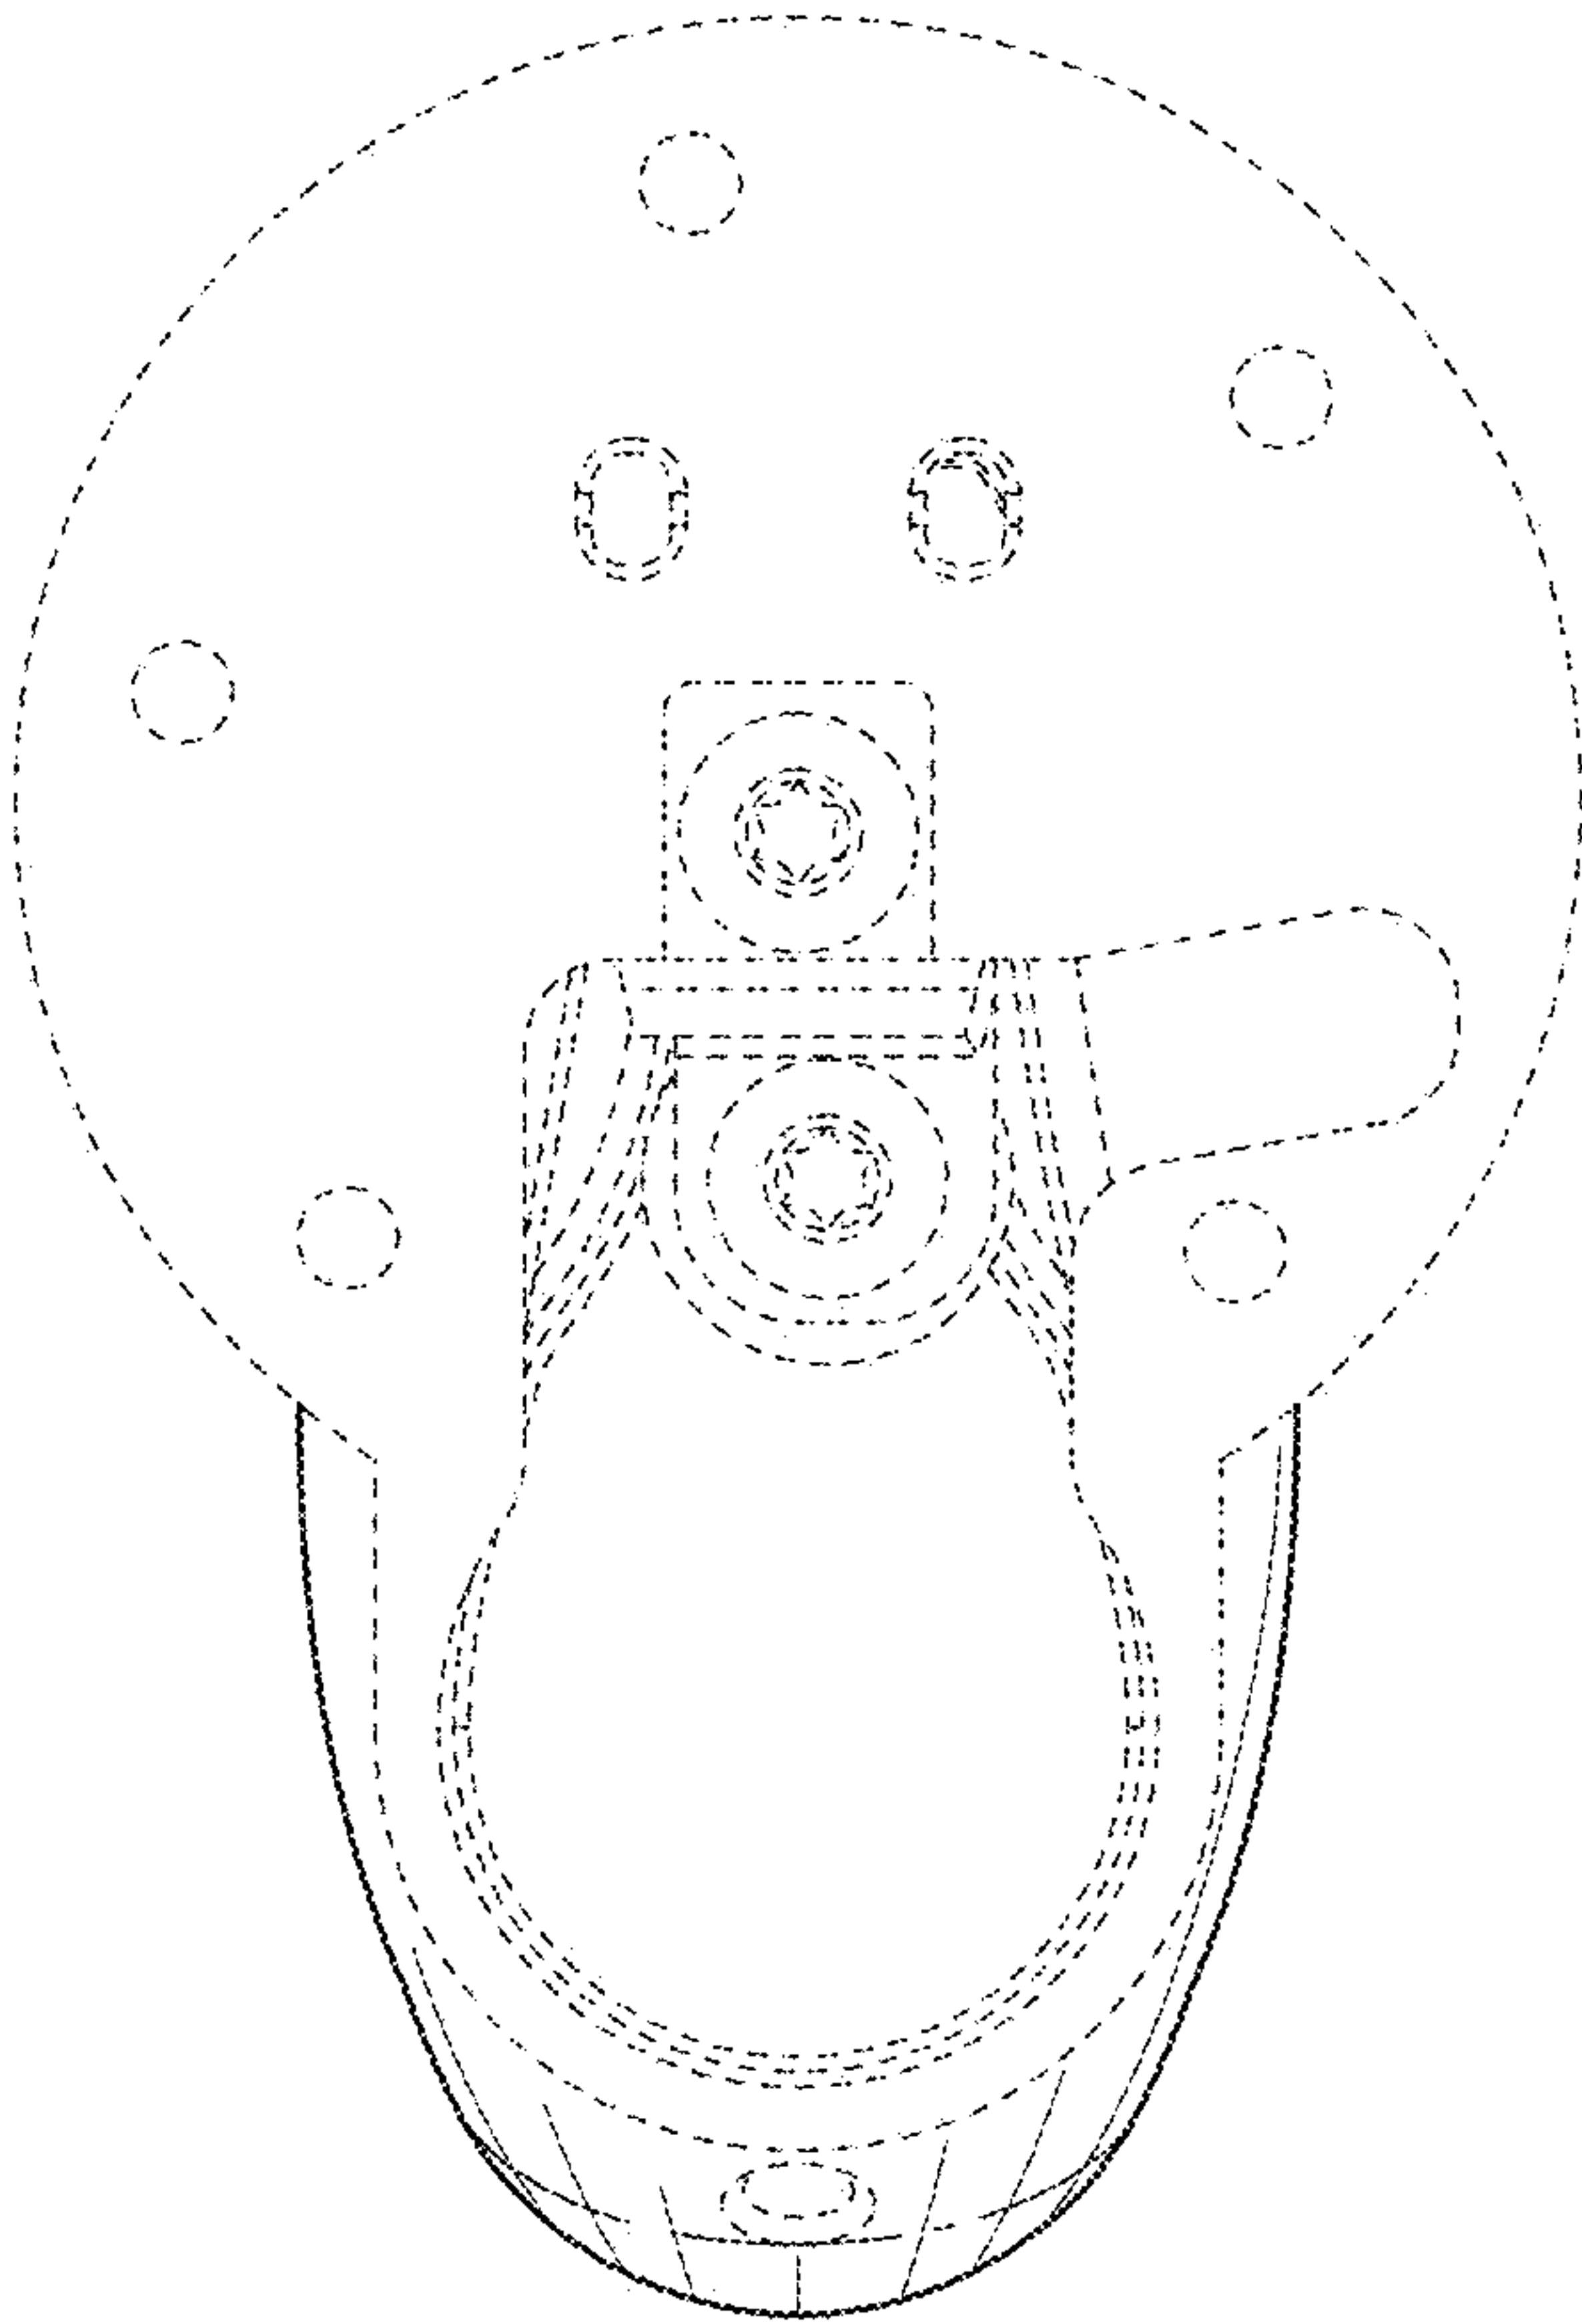


FIG. 3

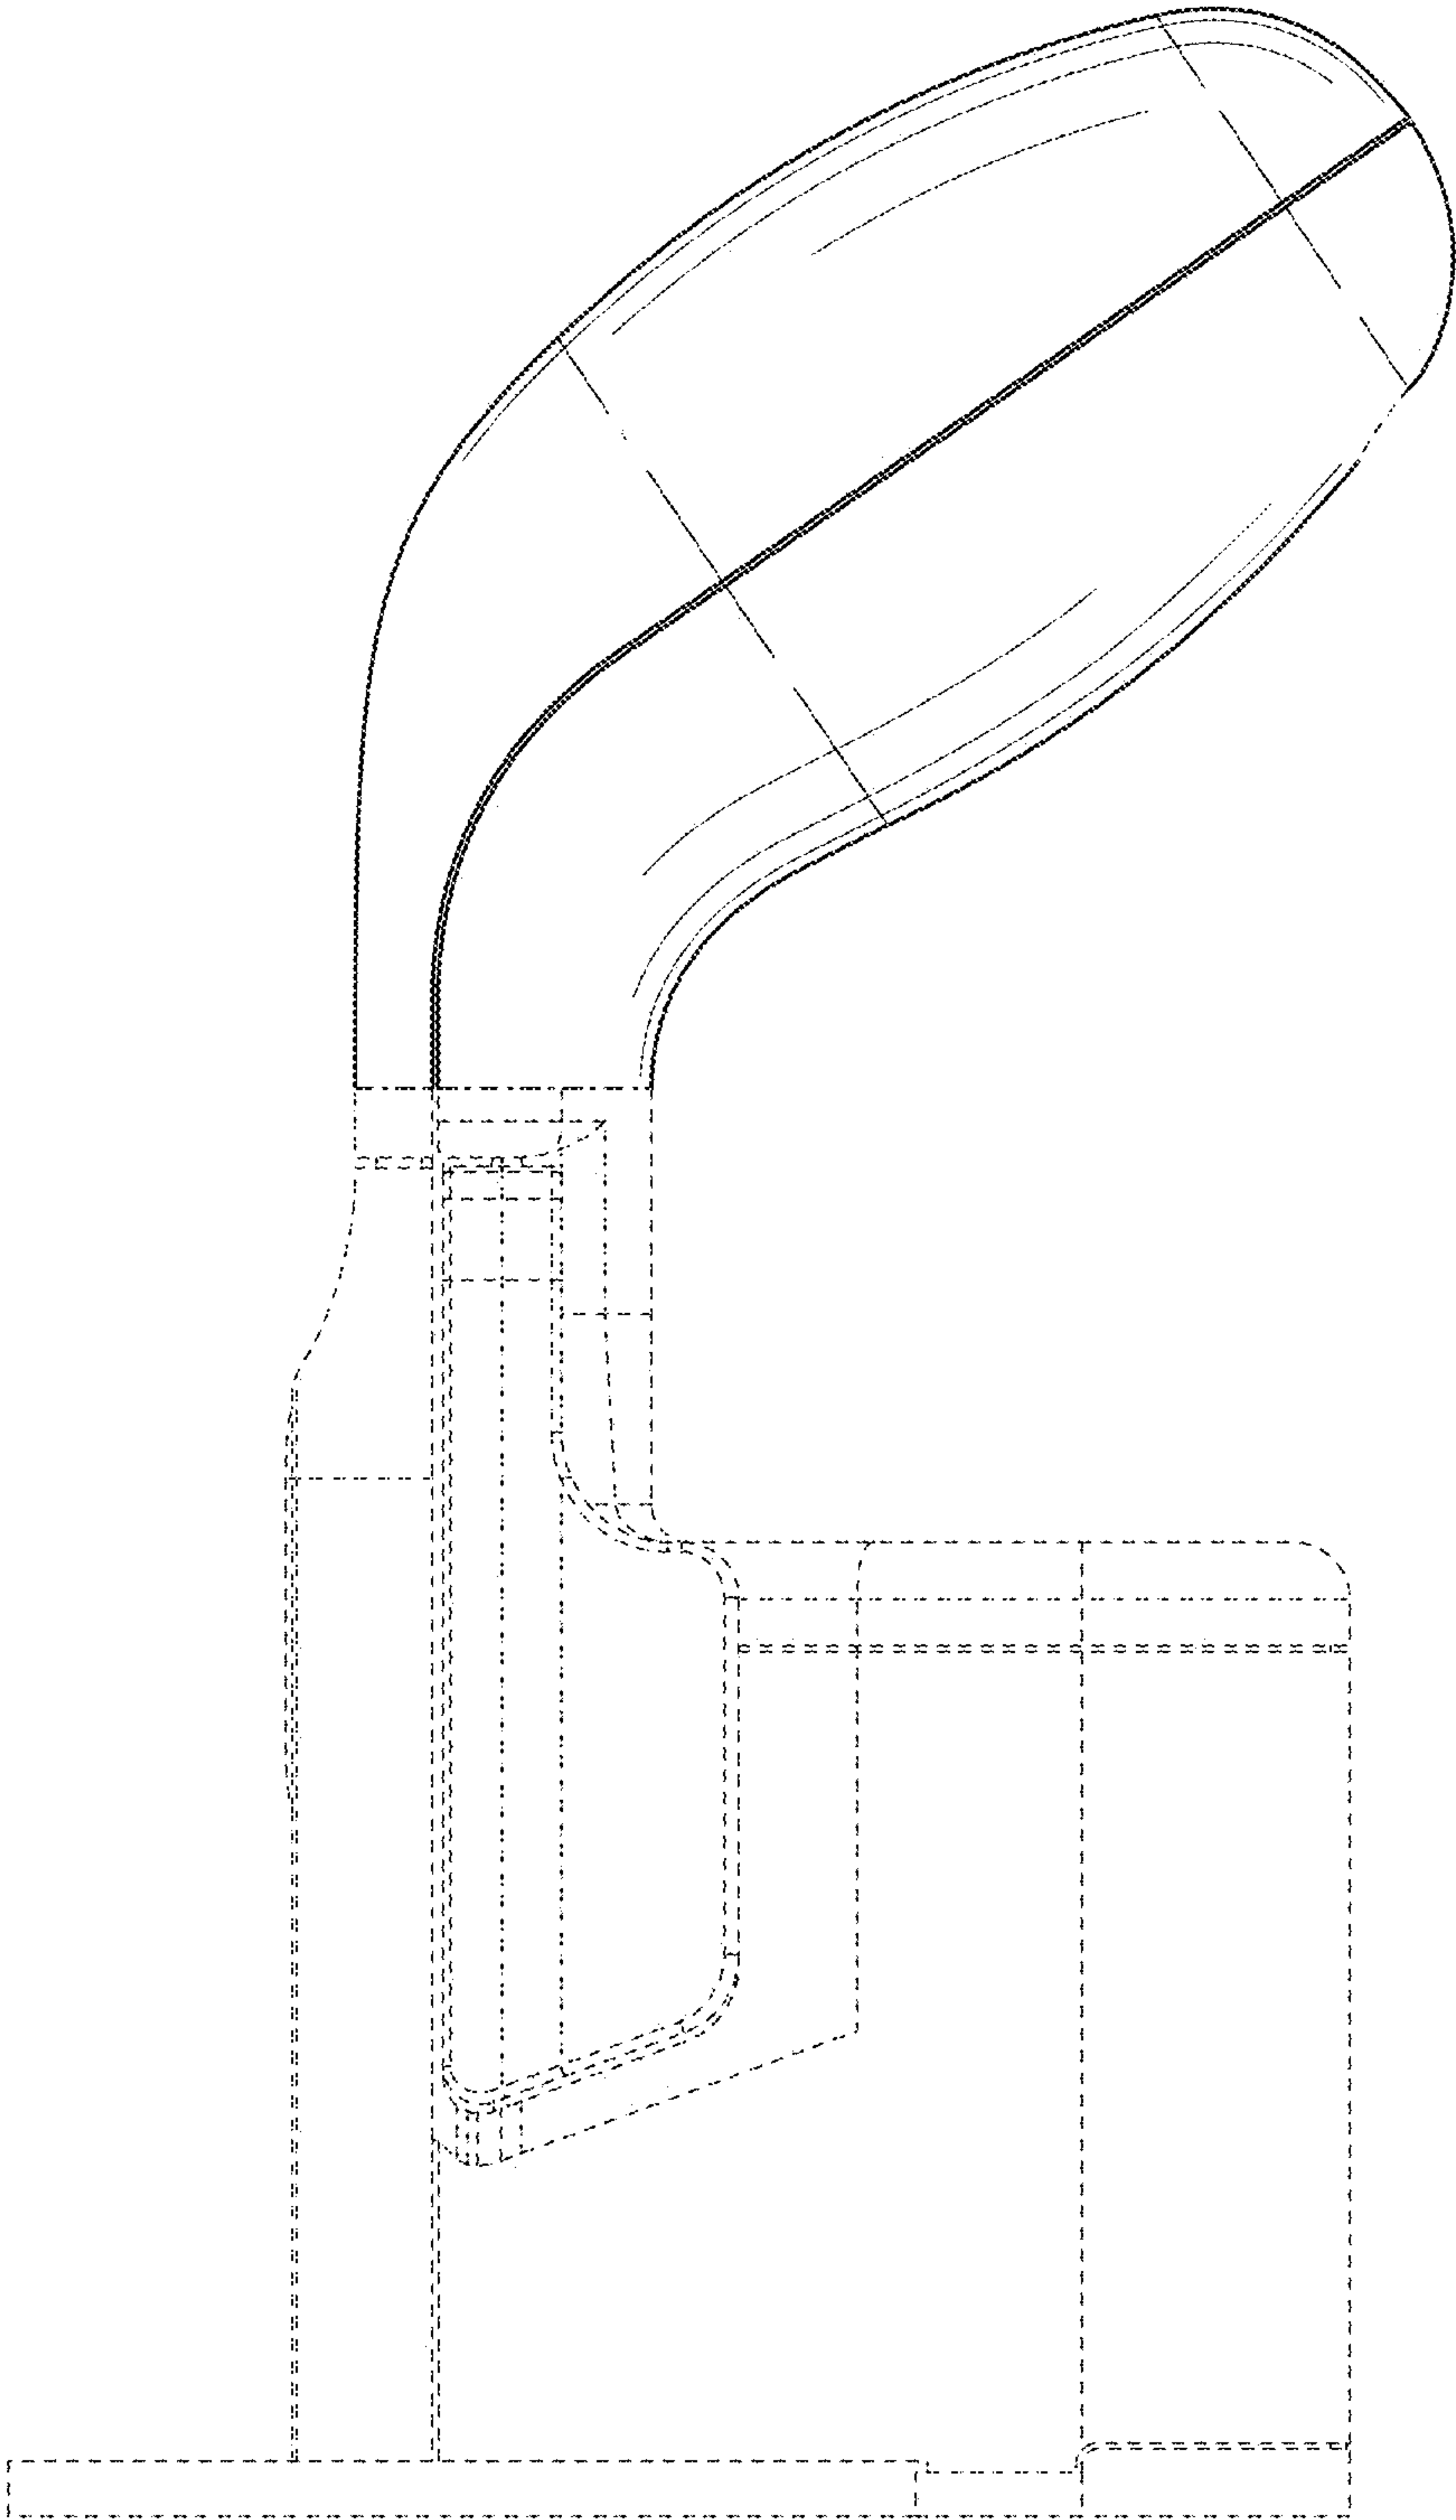


FIG. 4

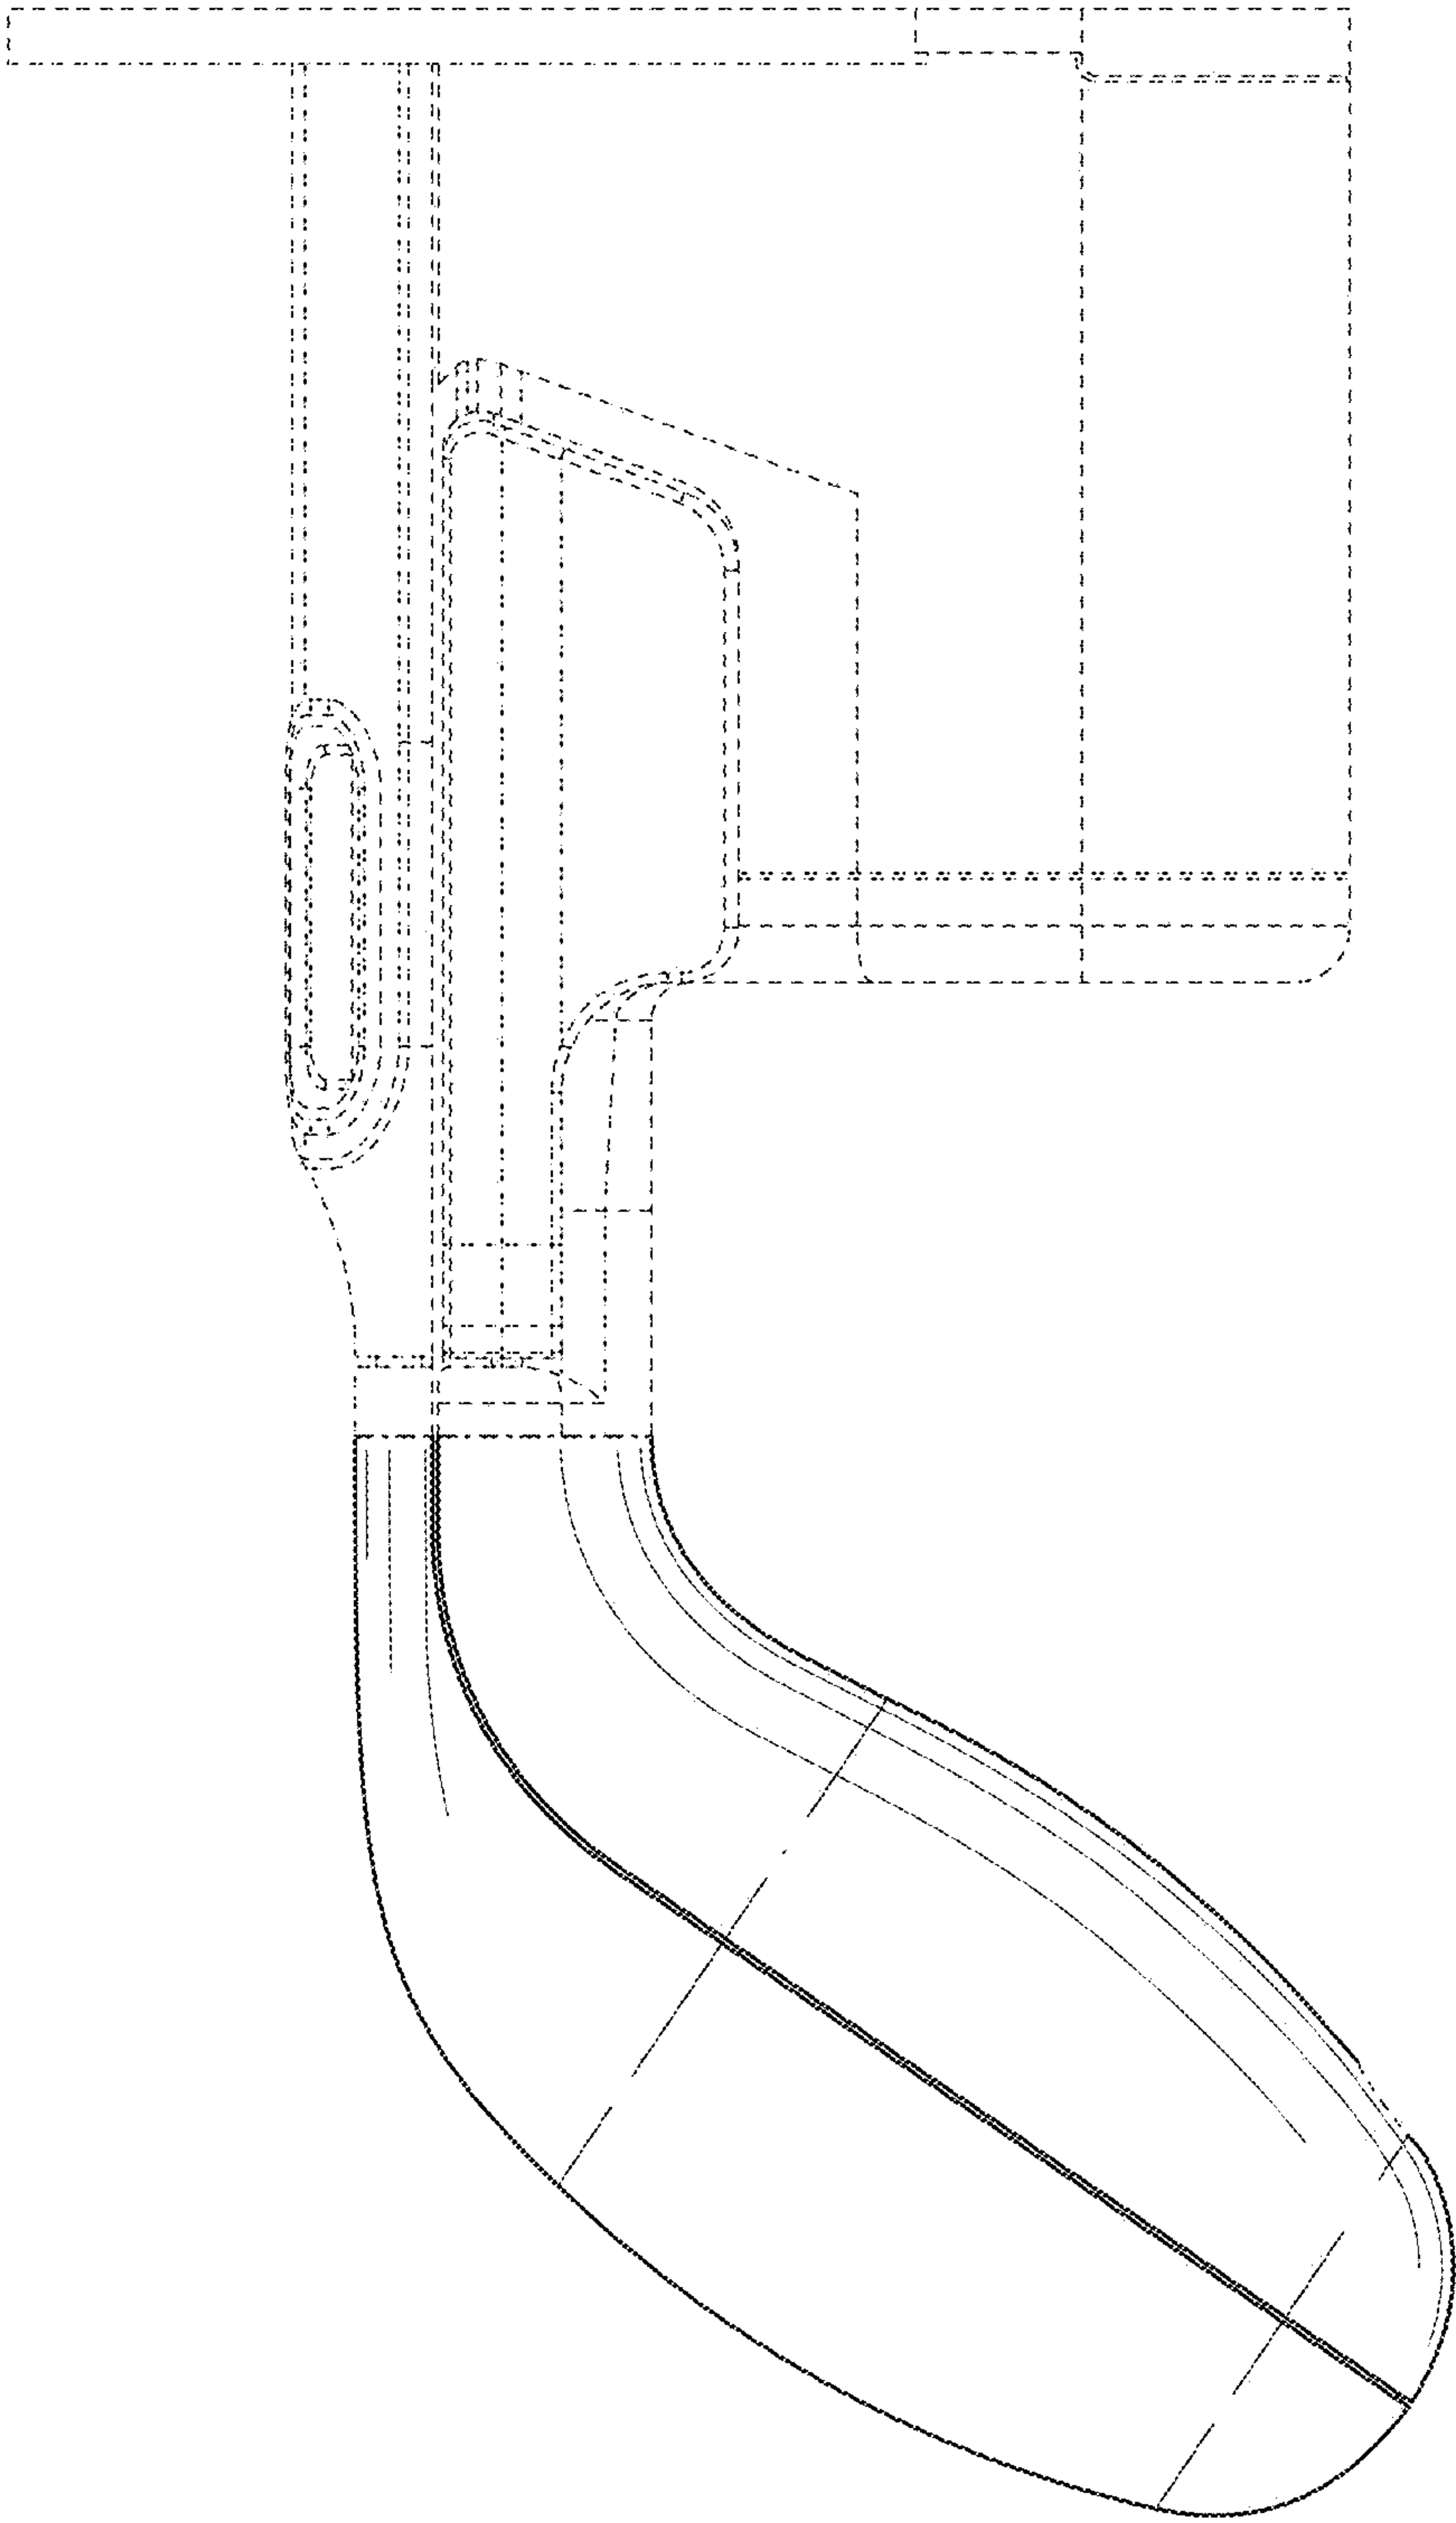


FIG. 5

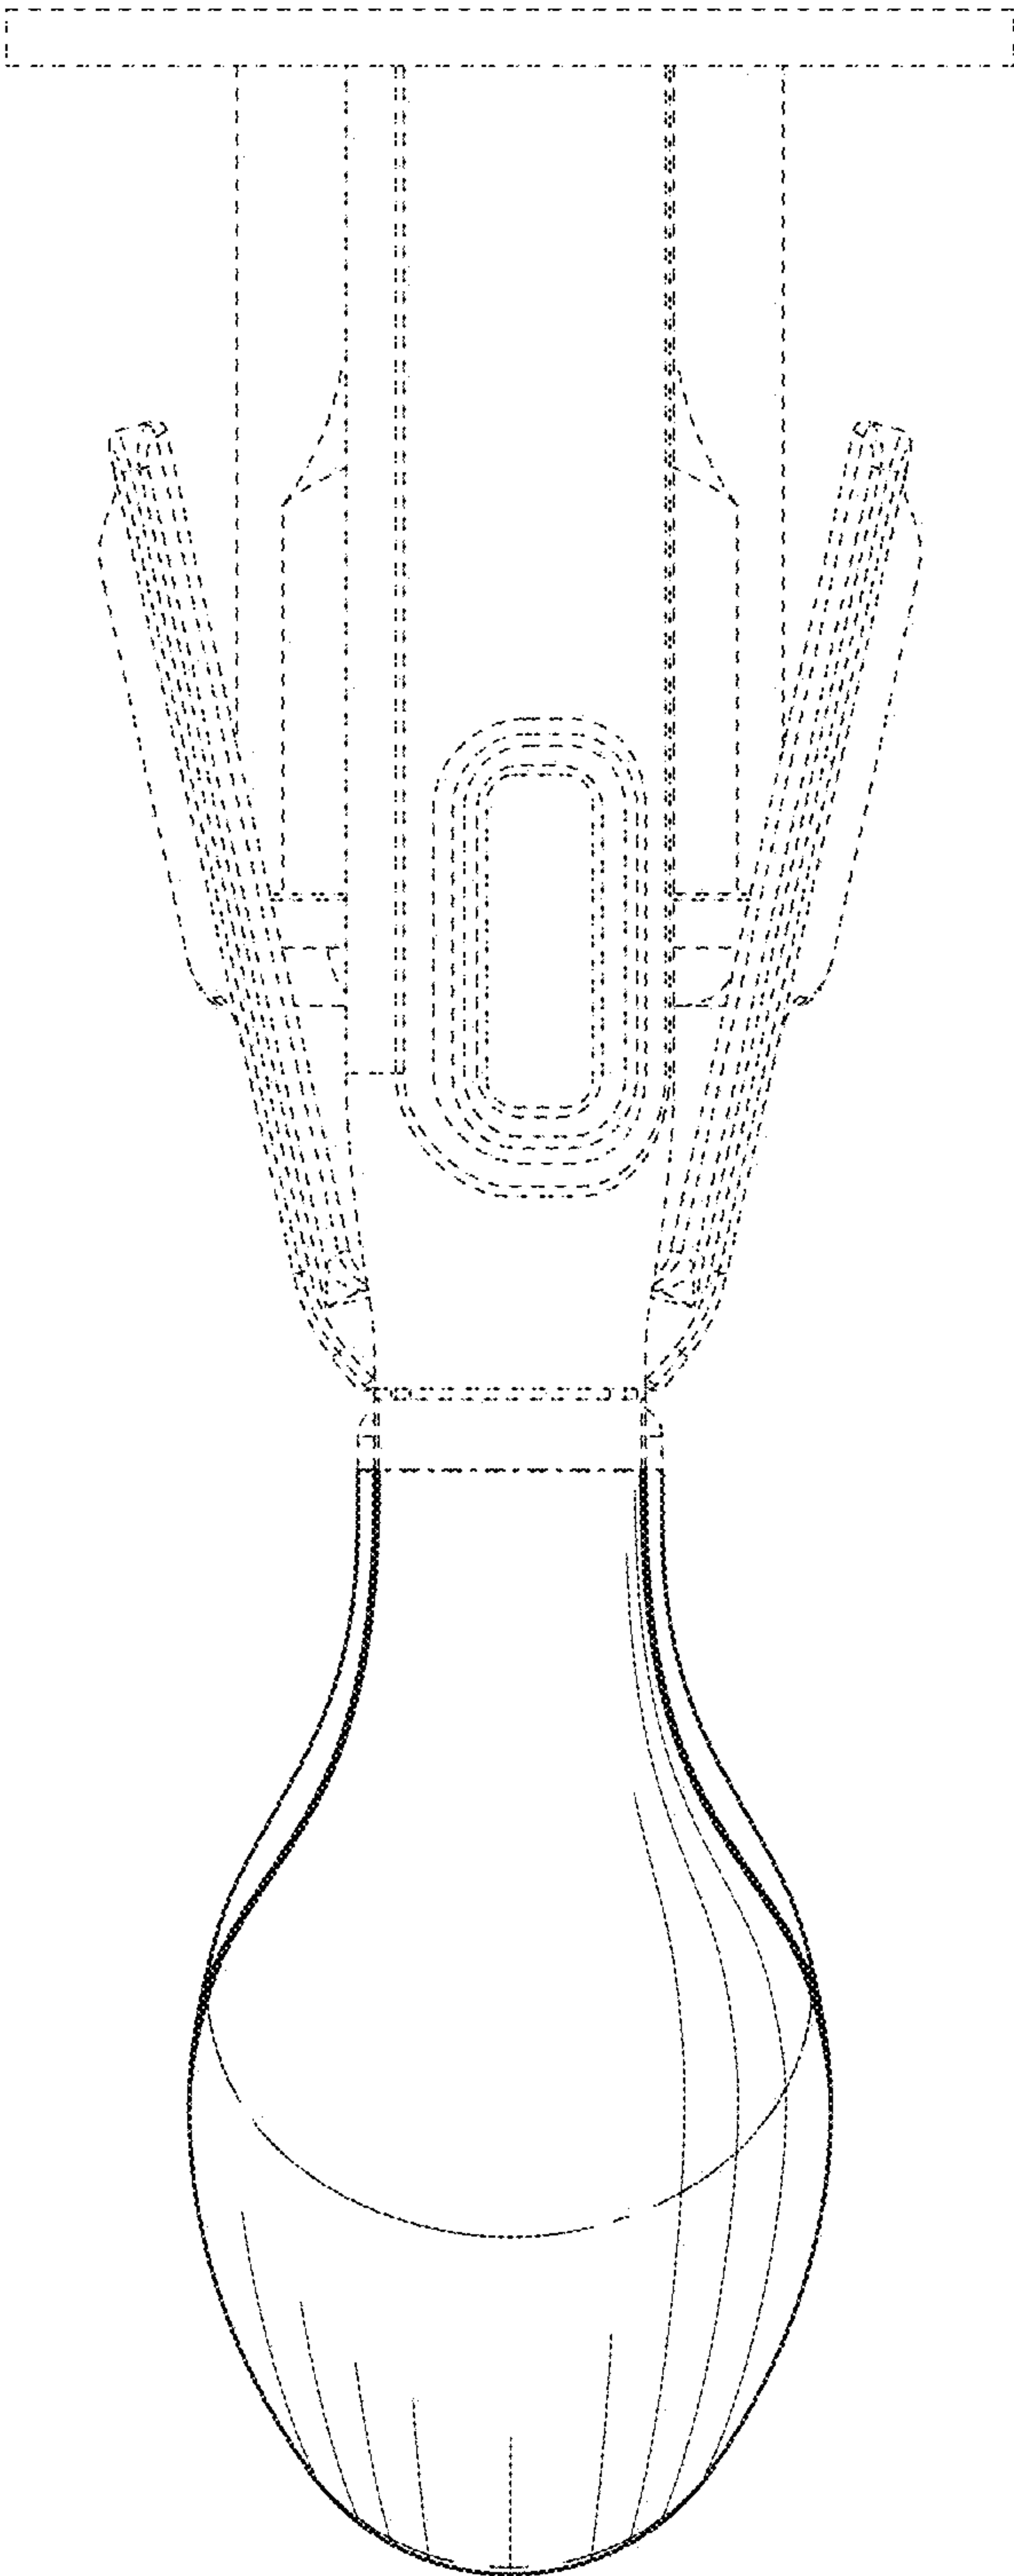


FIG. 6

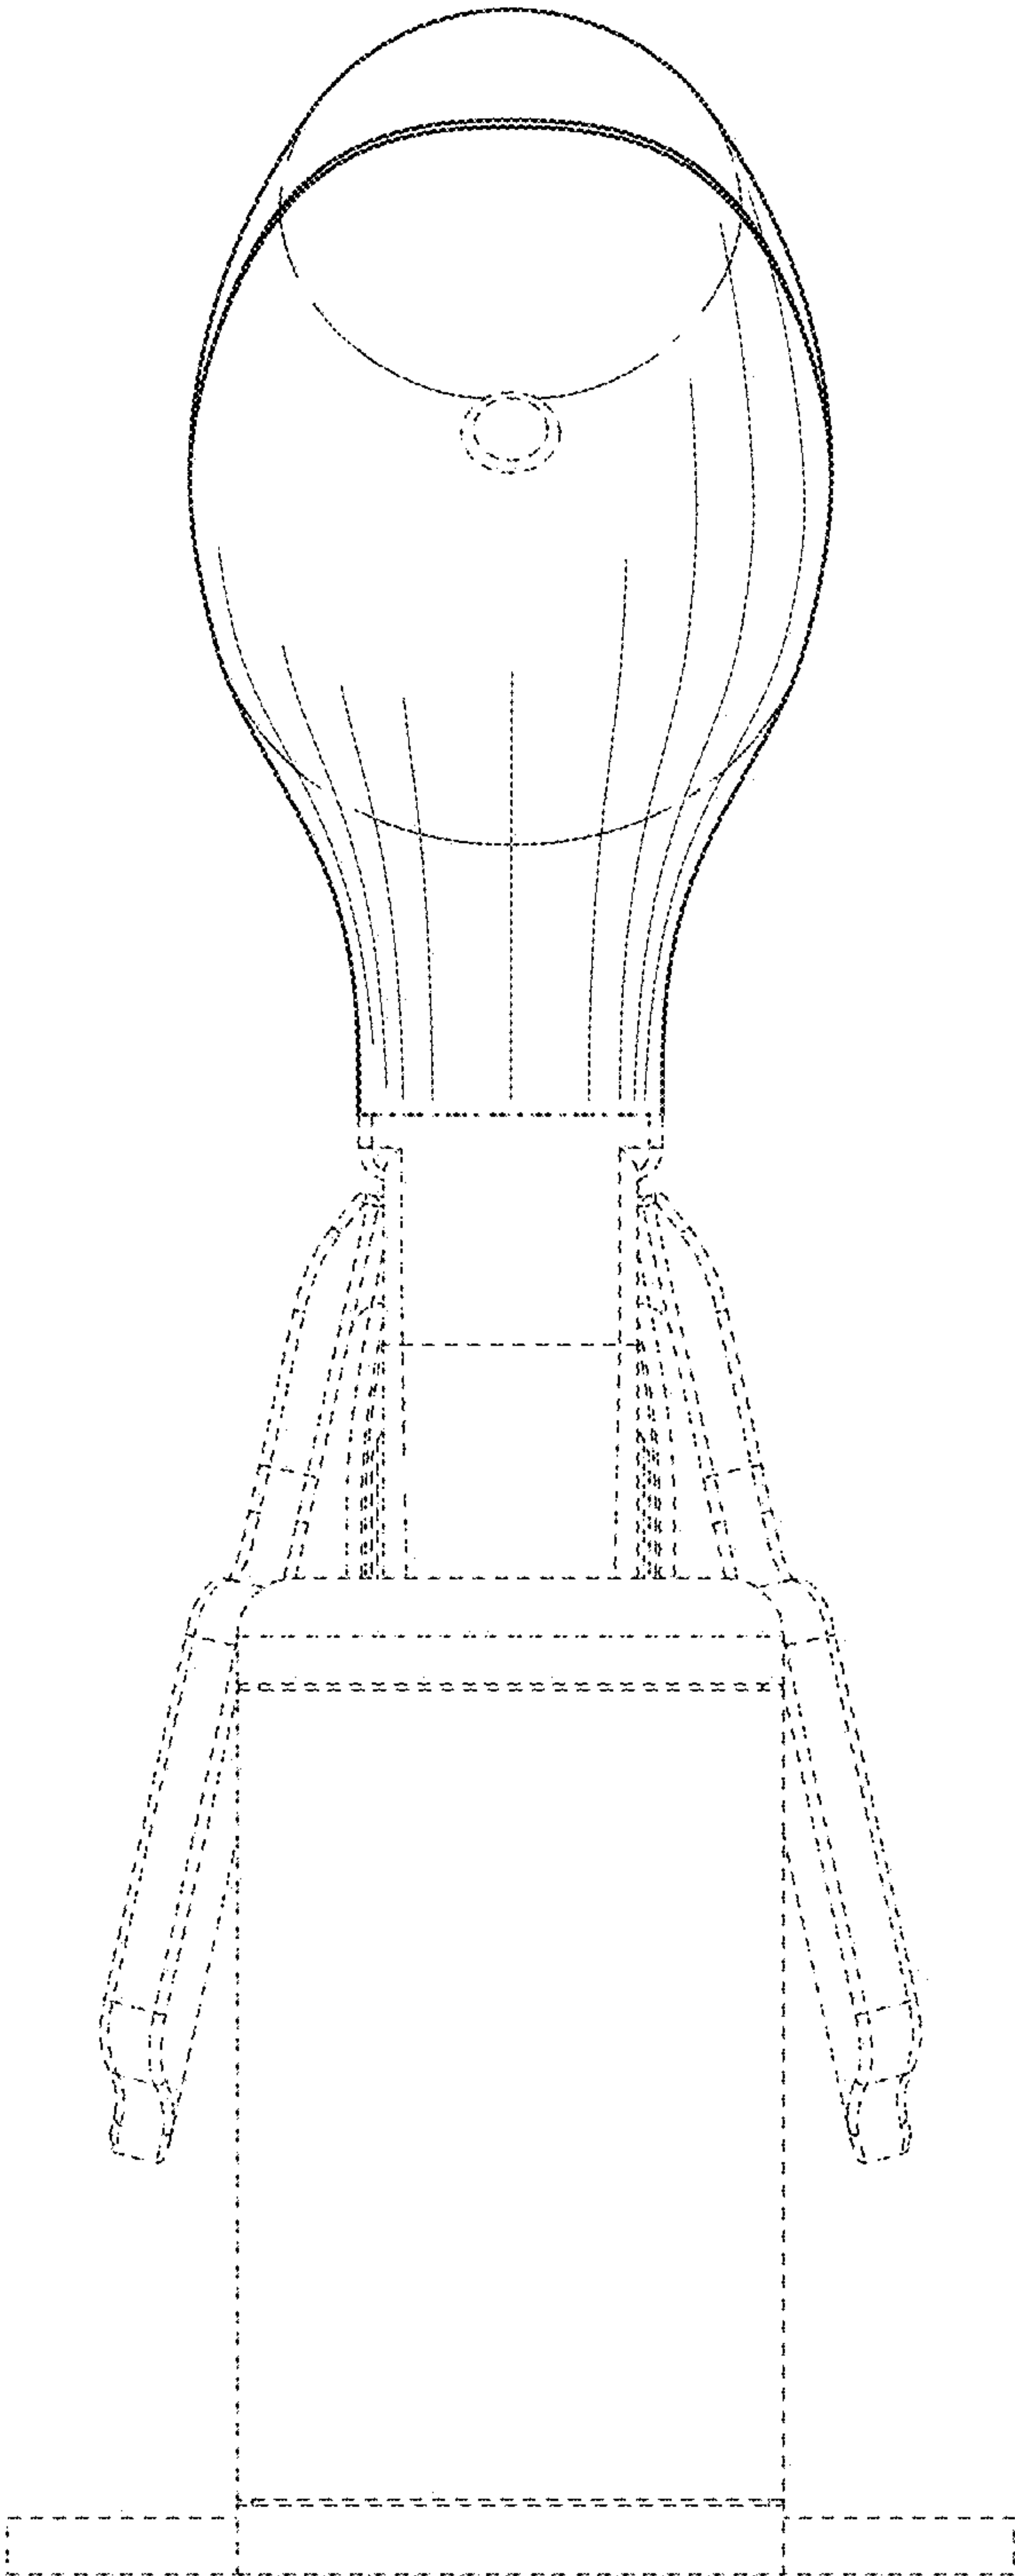


FIG. 7