



US0D1070110S

(12) **United States Design Patent** (10) **Patent No.: US D1,070,110 S**  
**Kraus et al.** (45) **Date of Patent: \*\* \*Apr. 8, 2025**

(54) **WATER BATH FOR MEDICAL AND SCIENTIFIC USE**

(71) Applicant: **PFM Medical GMBH**, Cologne (DE)

(72) Inventors: **Steffen Kraus**, Sandhausen (DE);  
**Erwin Schneider**, Nussloch (DE)

(73) Assignee: **PFM MEDICAL GMBH** (DE)

(\*) Notice: This patent is subject to a terminal disclaimer.

(\*\*) Term: **15 Years**

(21) Appl. No.: **29/812,658**

(22) Filed: **Oct. 22, 2021**

(30) **Foreign Application Priority Data**

Apr. 22, 2021 (EM) ..... 008512701-0001

Apr. 22, 2021 (EM) ..... 008512701-0002

(51) **LOC (15) Cl.** ..... **24-02**

(52) **U.S. Cl.**  
USPC ..... **D24/216**

(58) **Field of Classification Search**

USPC ..... D24/107, 121, 185, 186, 216, 217, 219,  
D24/220, 201, 202, 223, 224, 225, 227,  
D24/229, 230, 231, 232; D10/81

(Continued)

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

4,322,029 A \* 3/1982 Gropper ..... B04B 7/00  
494/47

D275,033 S \* 8/1984 Postlewait ..... D24/217  
(Continued)

**FOREIGN PATENT DOCUMENTS**

CN 307849528 \* 2/2023

CN 308227924 \* 9/2023

(Continued)

**OTHER PUBLICATIONS**

“IVYX Scientific: Digital Water Bath.” Found online 12/202/2023 at amazon.com. Reference dated Jun. 24, 2019. Retrieved from <https://www.amazon.com/IVYX-Scientific-Digital-Laboratory-RT-100°C/dp/B07T81P5KN/>.\*

(Continued)

*Primary Examiner* — Kendra Leslie Hamilton

*Assistant Examiner* — Elizabeth S Struble

(74) *Attorney, Agent, or Firm* — Lisa E. Geary; Eckert  
Seamans Cherin & Mellott, LLC

(57) **CLAIM**

The ornamental design for water bath for medical and scientific use, as shown and described.

**DESCRIPTION**

FIG. 1 is a top, front, and right-side perspective view of apparatus and equipment for doctors, hospitals and laboratories according to a first embodiment of the present invention;

FIG. 2 is a top, rear, and right-side perspective view of the apparatus and equipment shown in FIG. 1;

FIG. 3 is a front elevational view of the apparatus and equipment shown in FIG. 1;

FIG. 4 is a rear elevational view of the apparatus and equipment shown in FIG. 1;

FIG. 5 is a right-side elevational view of the apparatus and equipment shown in FIG. 1;



FIG. 6 is a left-side elevational view of the apparatus and equipment shown in FIG. 1;

FIG. 7 is a top plan view of the apparatus and equipment shown in FIG. 1; and,

FIG. 8 is a bottom plan view of the apparatus and equipment shown in FIG. 1.

In the drawings, the right-side and left side elevational views of each embodiment are symmetrical. The surface shading, if any, illustrated in the drawings is provided merely to highlight the contour of the design; it is not intended to be illustrative of texture or gloss.

(Continued)

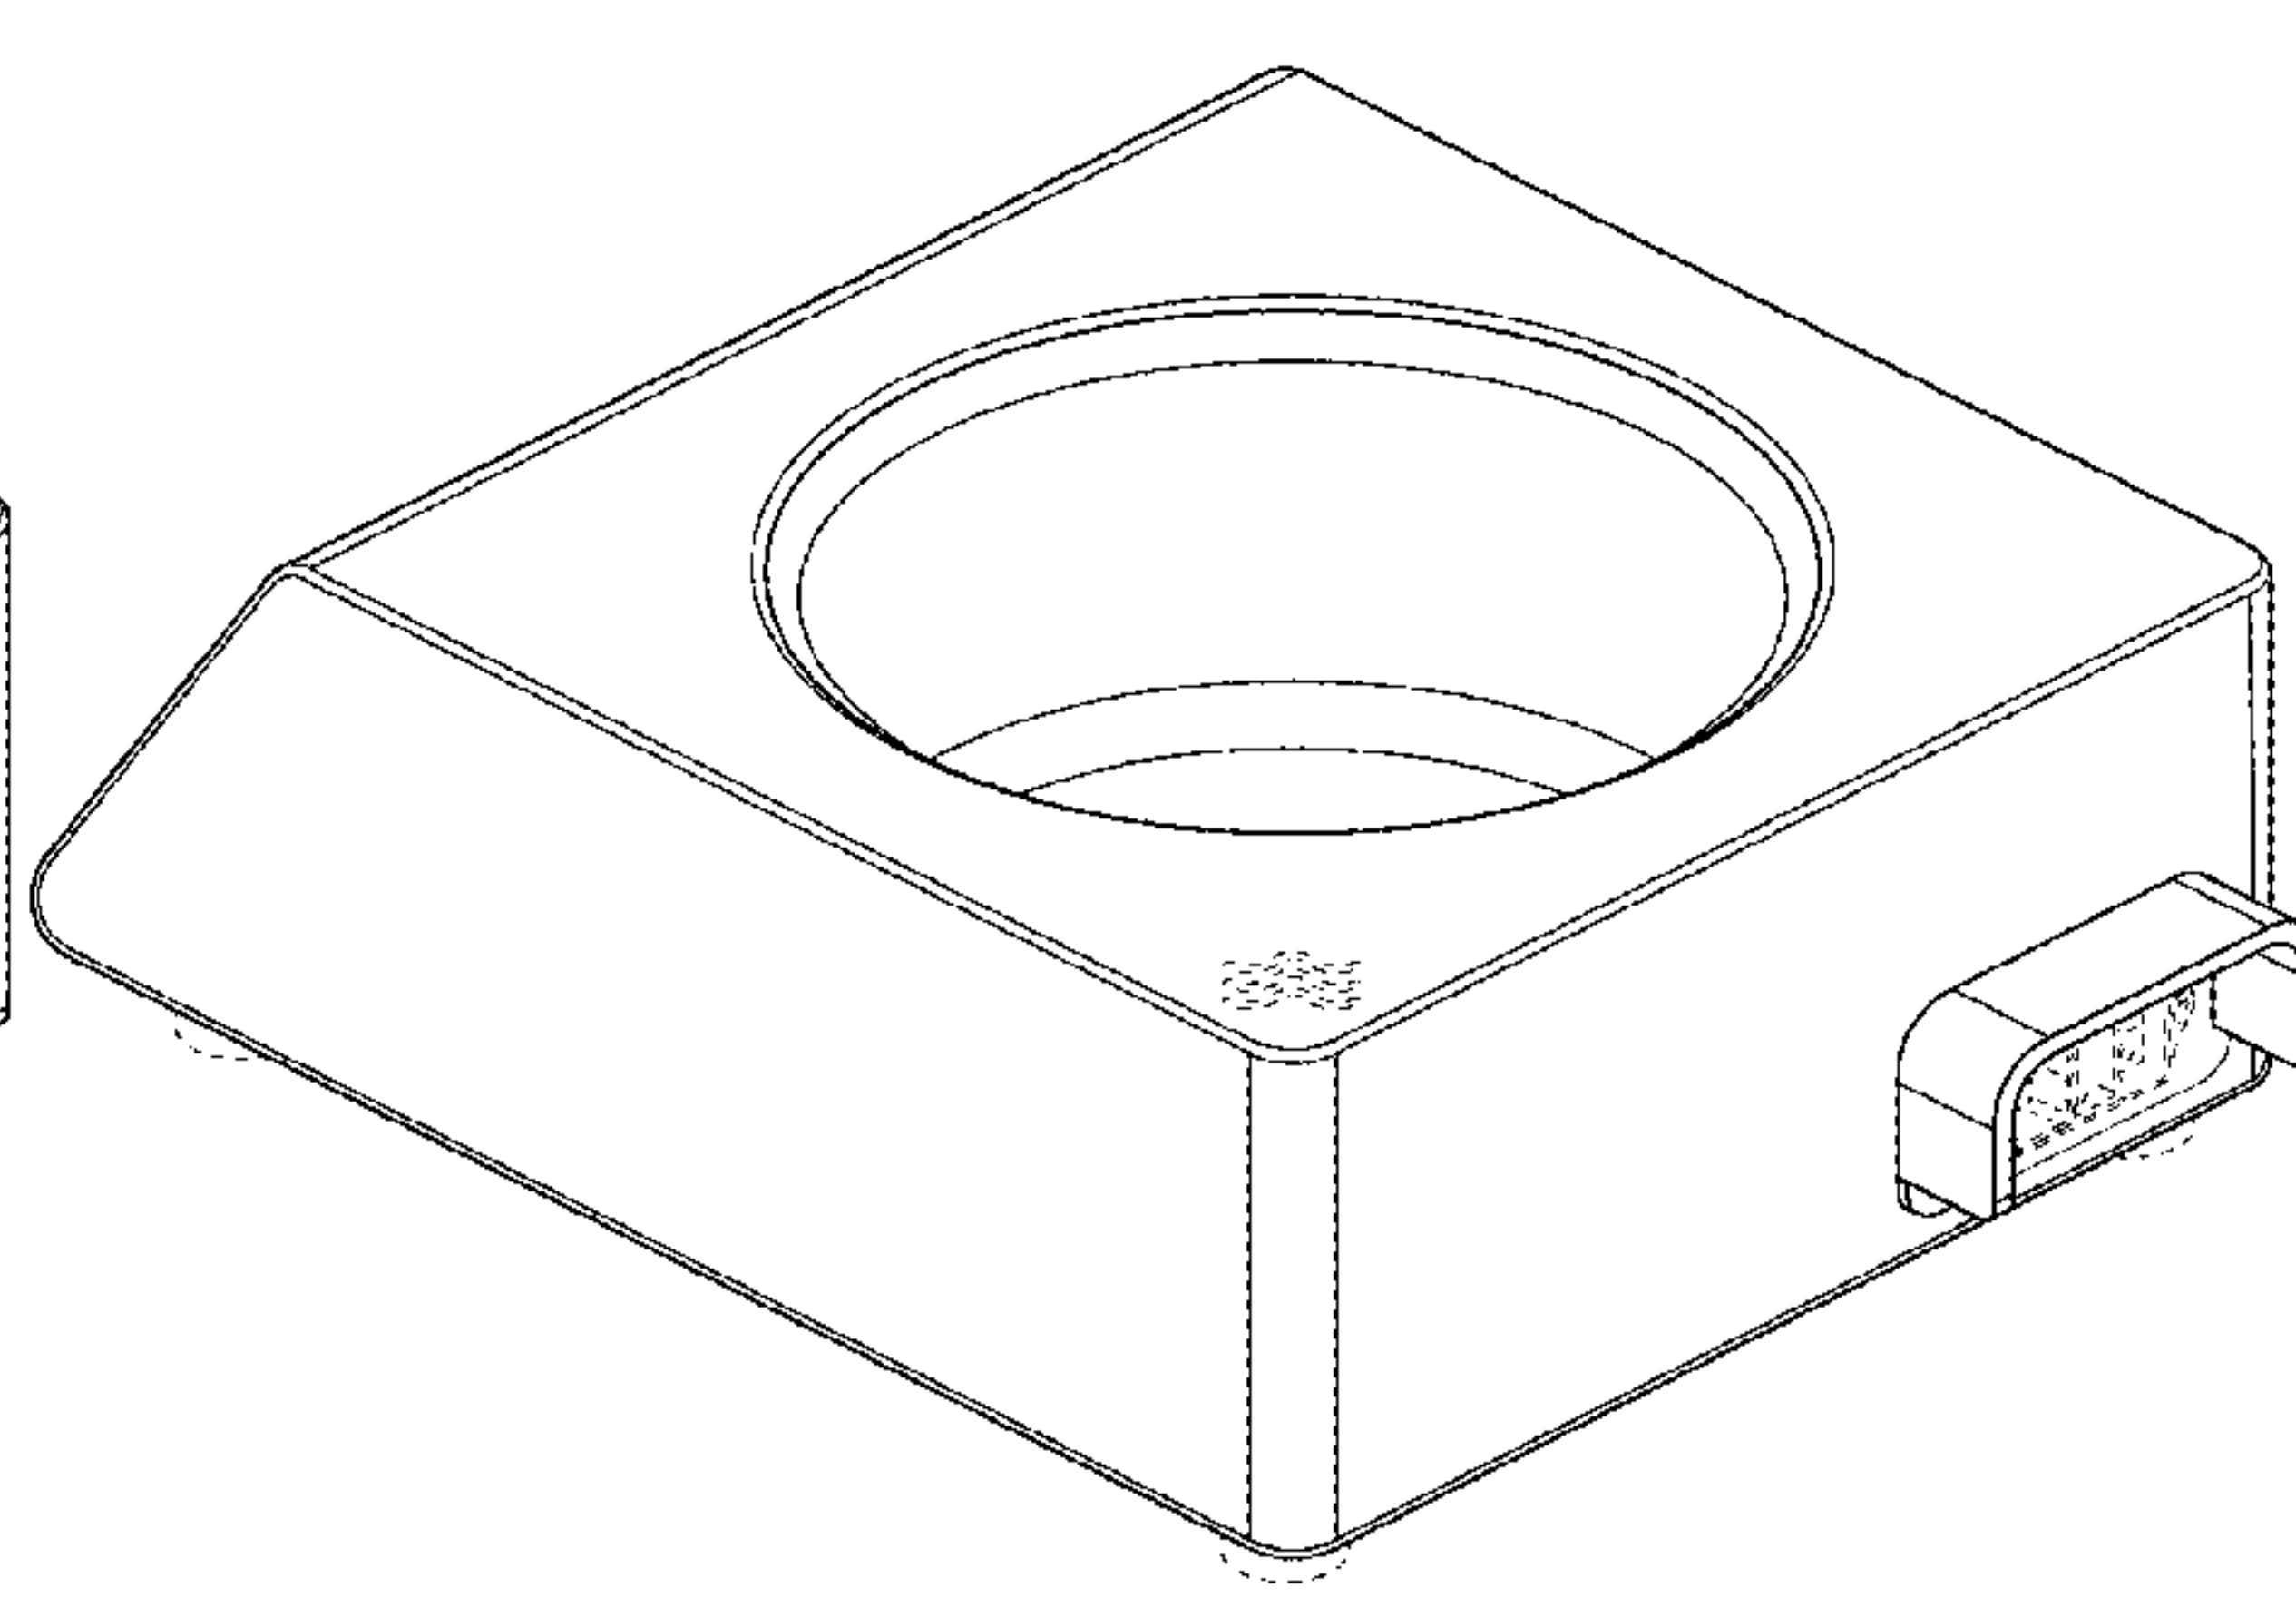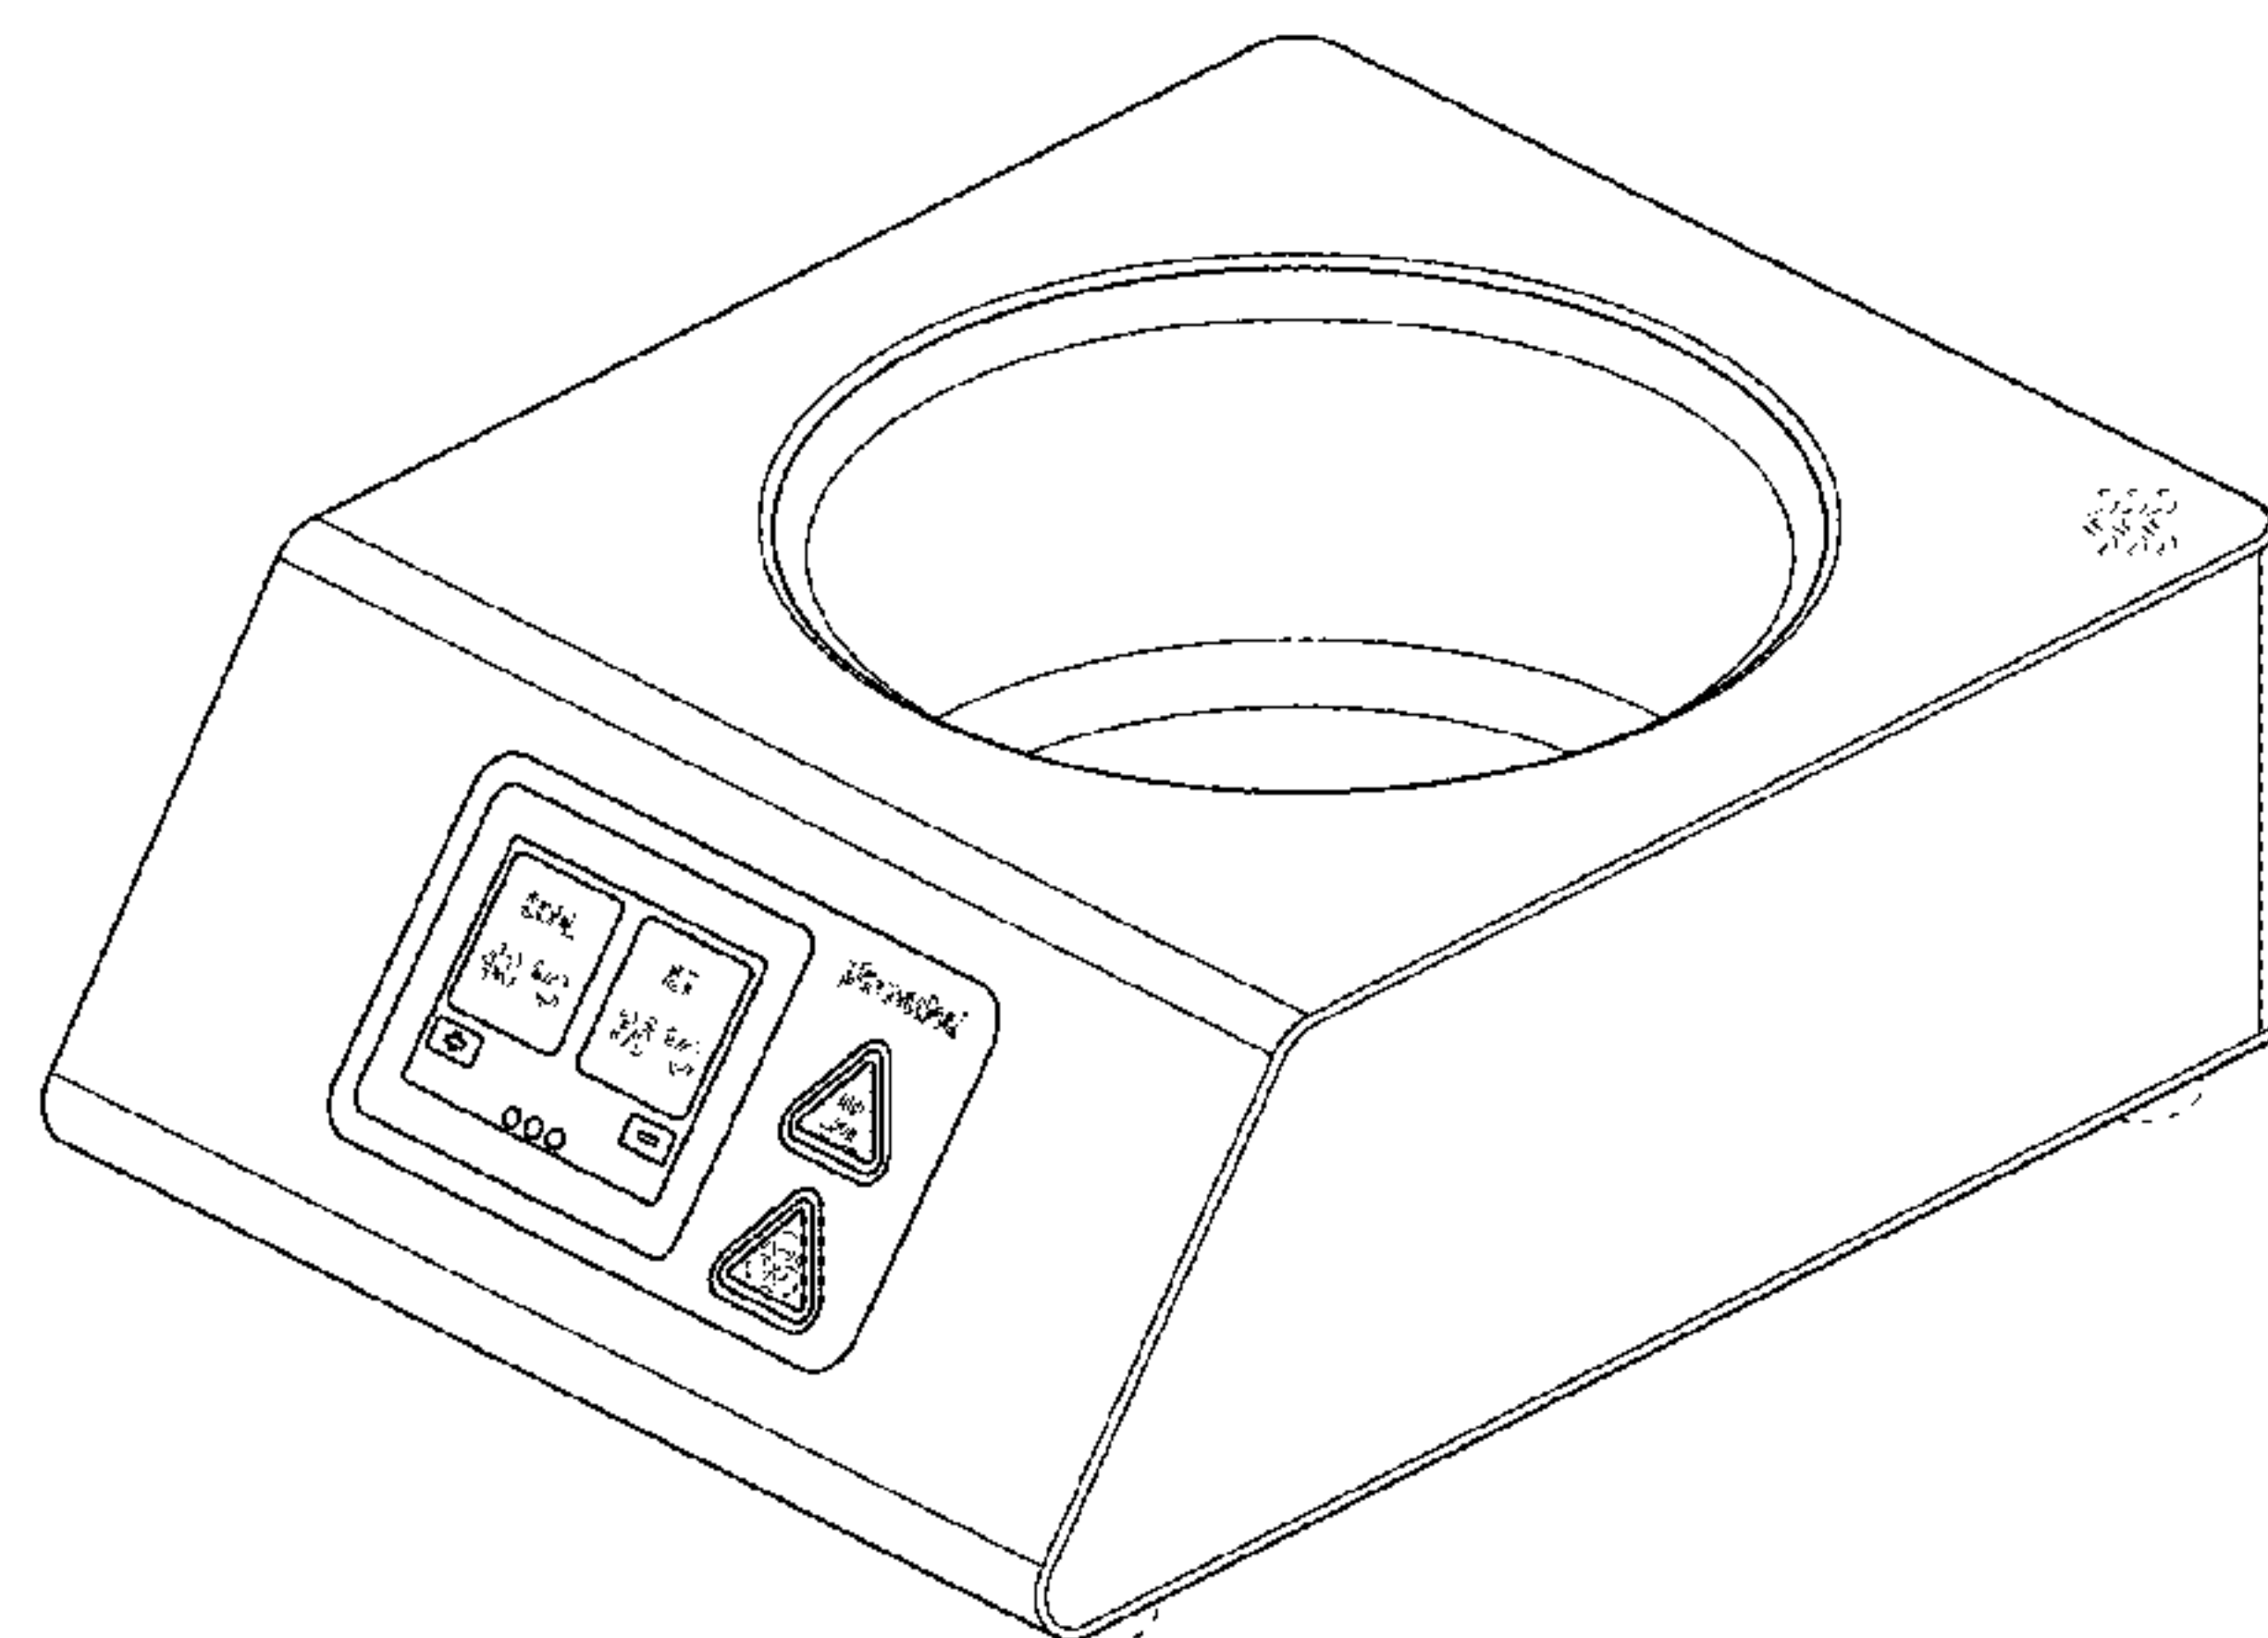

In the drawings, the equal-length broken lines depict portions of the water bath for medical and scientific use that form no part of the claimed design.

1 Claim, 8 Drawing Sheets

(58) Field of Classification Search

CPC ..... G01N 2035/00306; G01N 2035/00326;  
G01N 2035/00336; G01N 2030/027;  
G01N 21/6458; G01N 21/6484; G01N  
21/6486; G01N 21/76; G01N 35/025;  
G01N 21/0483; G01N 21/0303; G01N  
35/00029; G01N 35/00019; G01N  
21/6428; G01K 13/02; G01K 13/026;  
G01F 15/063; G01F 15/0755; G01F 1/68;  
B01L 7/02; B01L 7/04; B01L 7/50; B01L  
7/52

See application file for complete search history.

(56) References Cited

U.S. PATENT DOCUMENTS

D288,600 S \* 3/1987 Vander Hout ..... D24/217  
D449,548 S \* 10/2001 Goodman ..... D10/81  
D663,041 S \* 7/2012 Henssler ..... D24/219  
D701,616 S \* 3/2014 Schroer ..... D24/220

D733,312 S \* 6/2015 Schroer ..... D24/220  
10,046,327 B2 \* 8/2018 Schneider ..... A61B 17/30  
D839,443 S \* 1/2019 Stamm ..... D24/216  
D851,778 S \* 6/2019 Stamm ..... D24/216  
D971,437 S \* 11/2022 Shah ..... D24/232  
2011/0031232 A1 \* 2/2011 Kraus ..... F24H 1/185  
219/385  
2014/0259358 A1 \* 9/2014 Drury ..... A61H 33/601  
4/541.3

FOREIGN PATENT DOCUMENTS

GB 6263895 \* 2/2023  
JP D1737917 \* 3/2023

OTHER PUBLICATIONS

“Anzeser: Magnetic Stirrer.” Found online Dec. 20, 2023 at amazon.com. Reference dated Oct. 8, 2018. Retrieved from <https://www.amazon.com/ANZESER-Magnetic-Stirrer-Stirring-Capacity/dp/B07J59QVGQ/>.\*  
“Southern Labware: myFuge Mini.” Found online Dec. 20, 2023 at youtube.com. Reference dated Jul. 26, 2019. Retrieved from <https://www.youtube.com/watch?v=bDOng4gmBrY>.\*  
“Pfm medical: Rotary microtomes.” Found online Dec. 20, 2023 at youtube.com. Reference dated Feb. 13, 2017. Retrieved from <https://www.youtube.com/watch?v=O28rPXYzEBI>.\*

\* cited by examiner

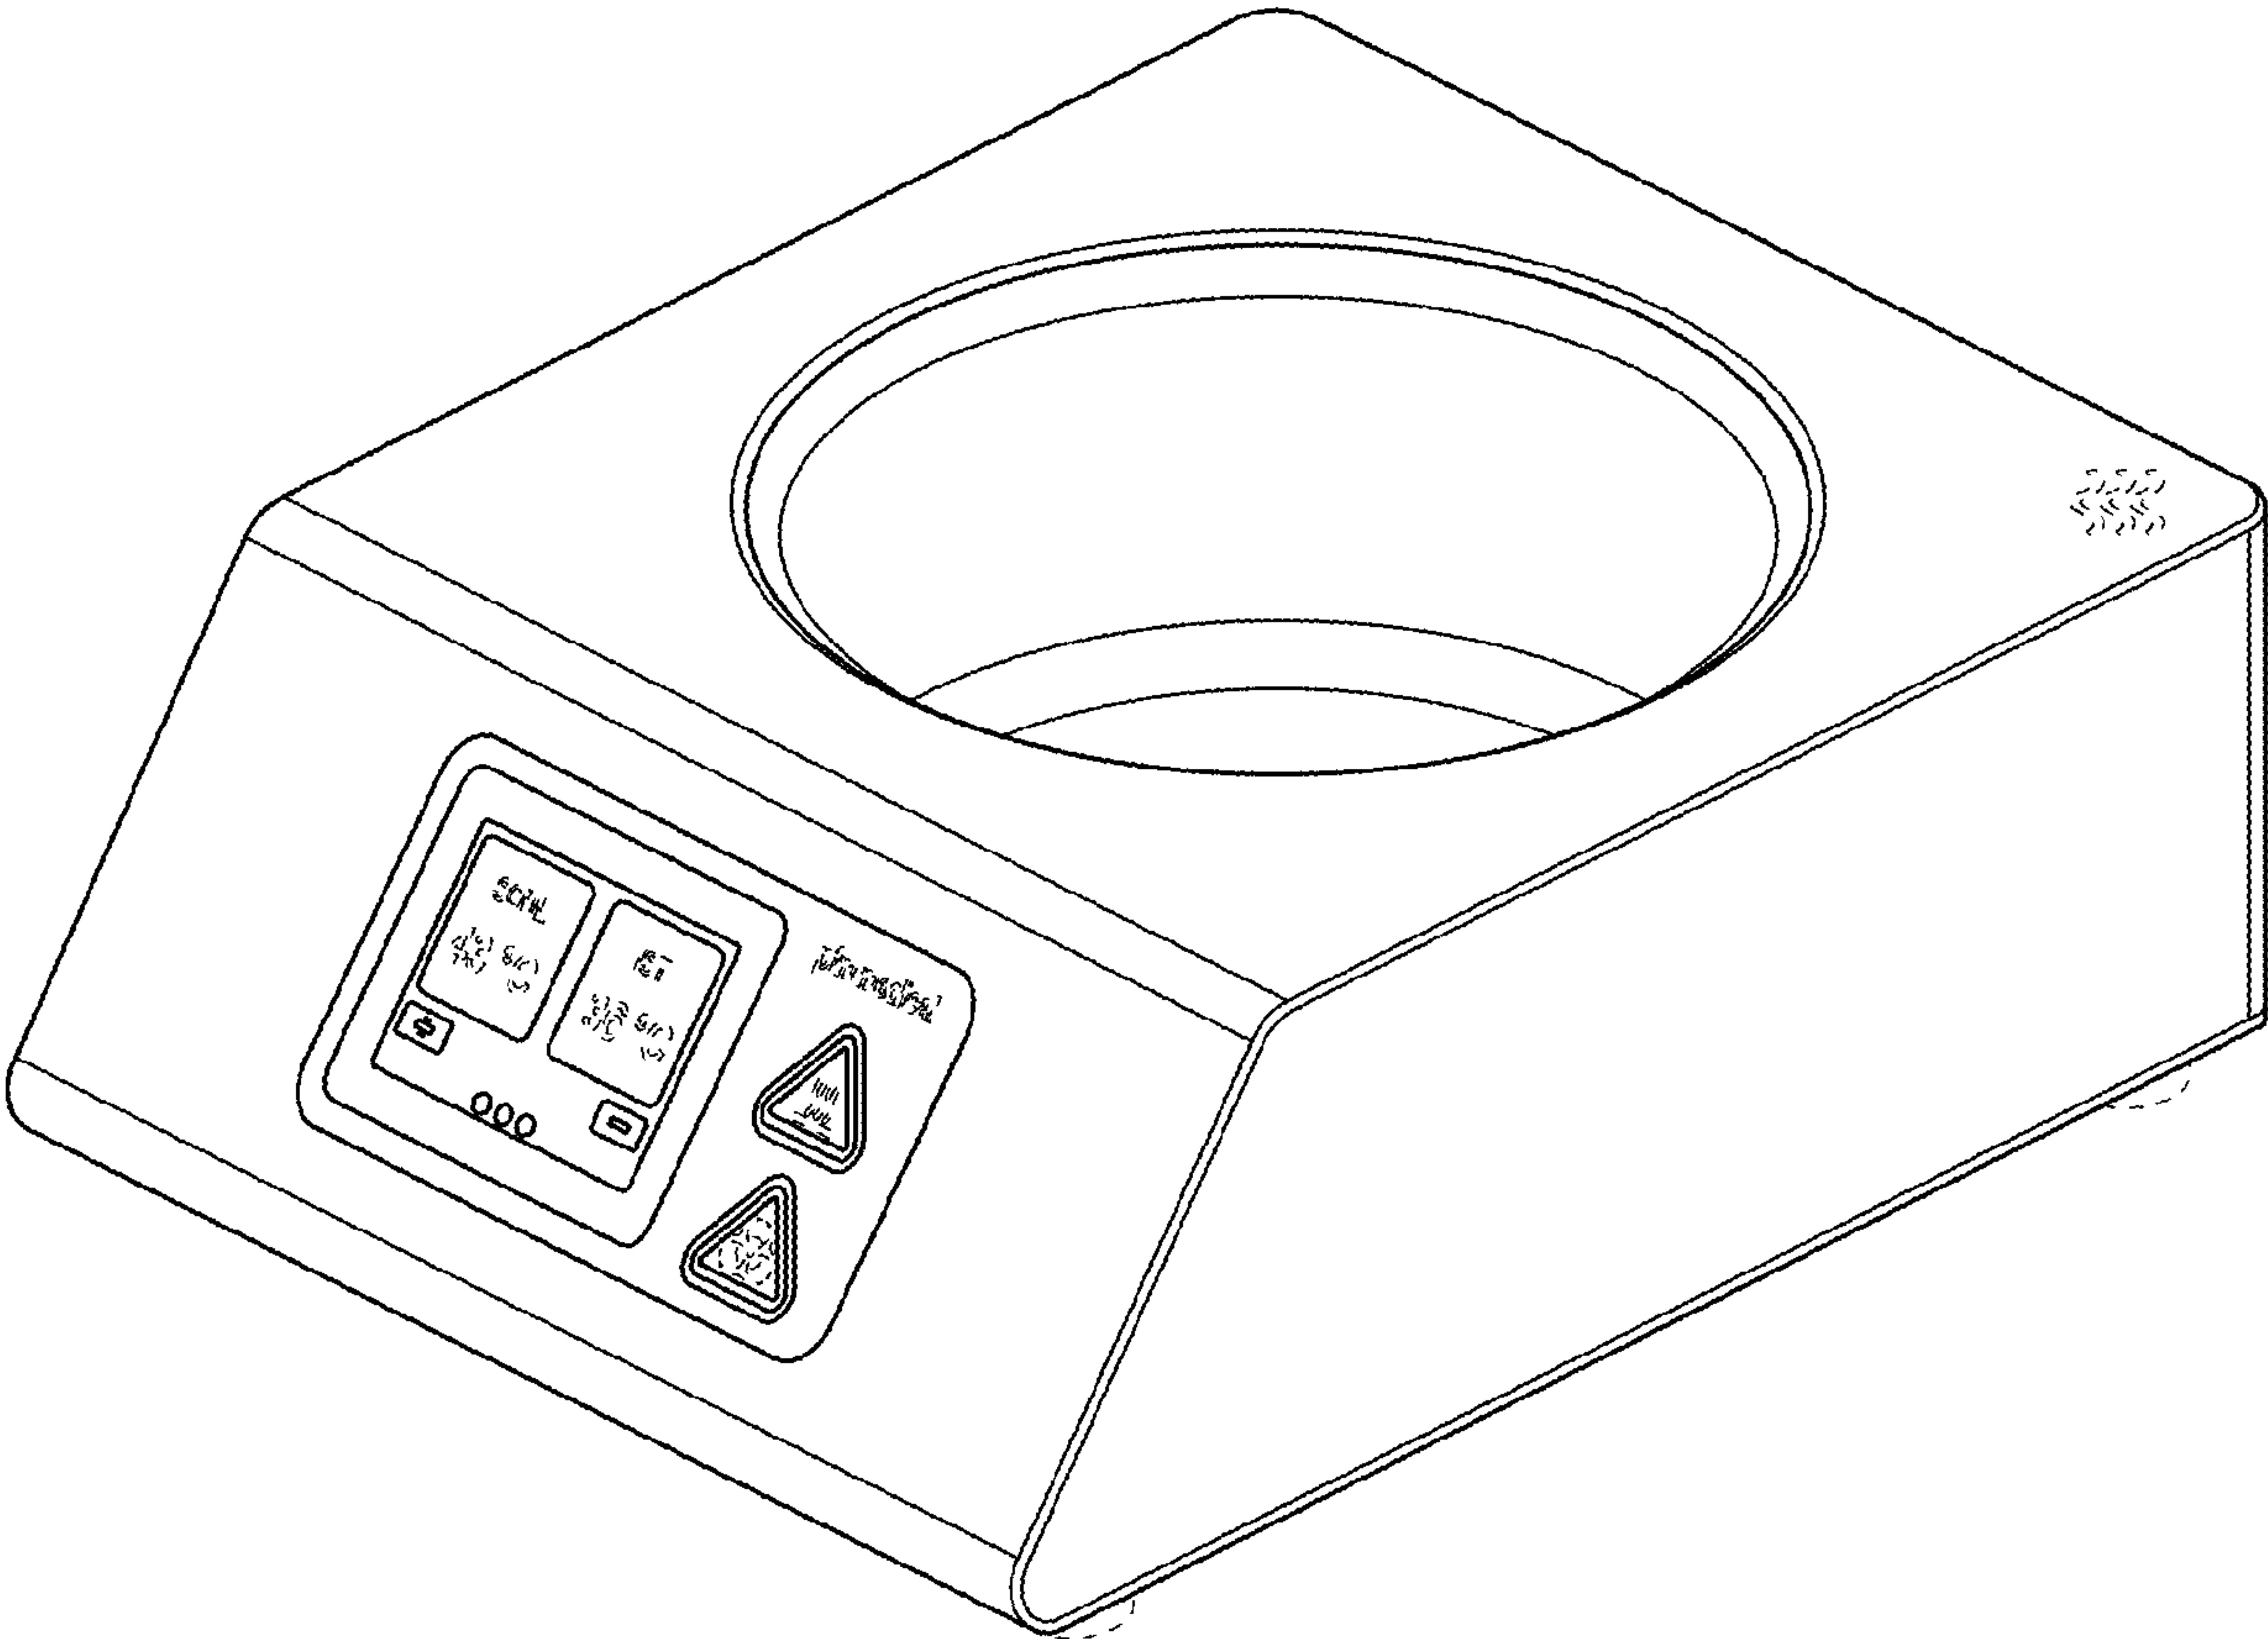


FIG. 1

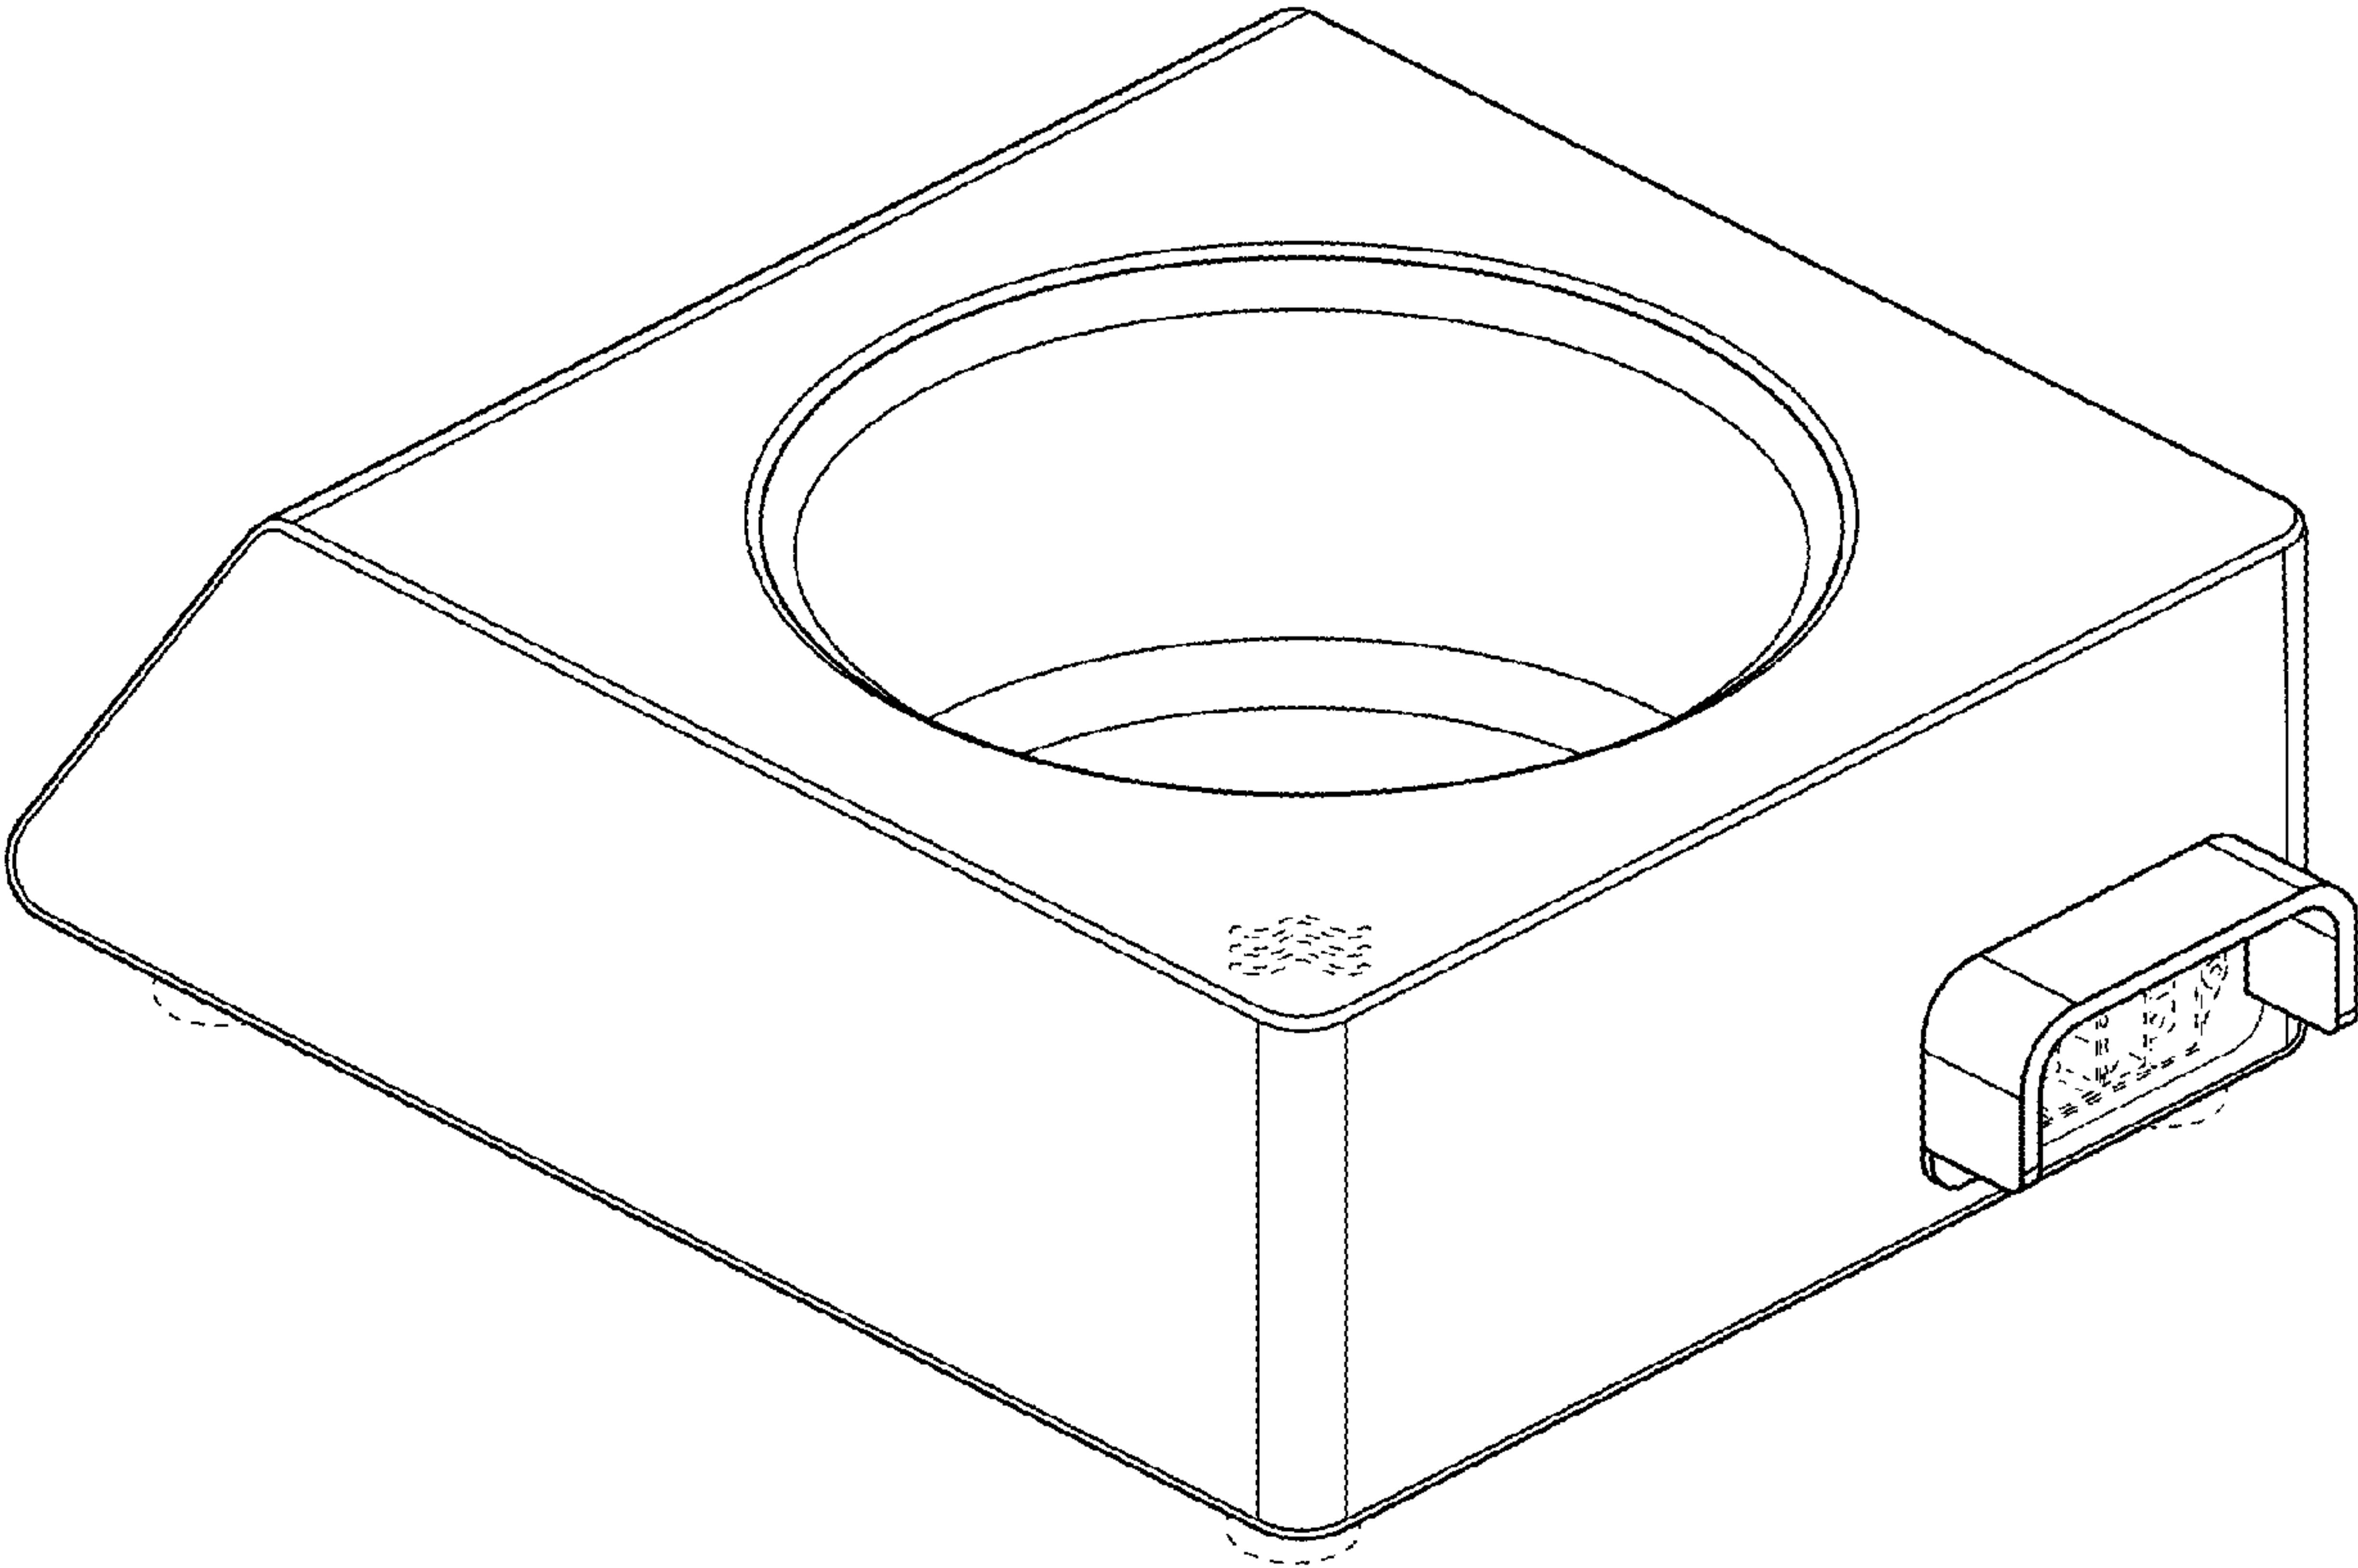


FIG. 2

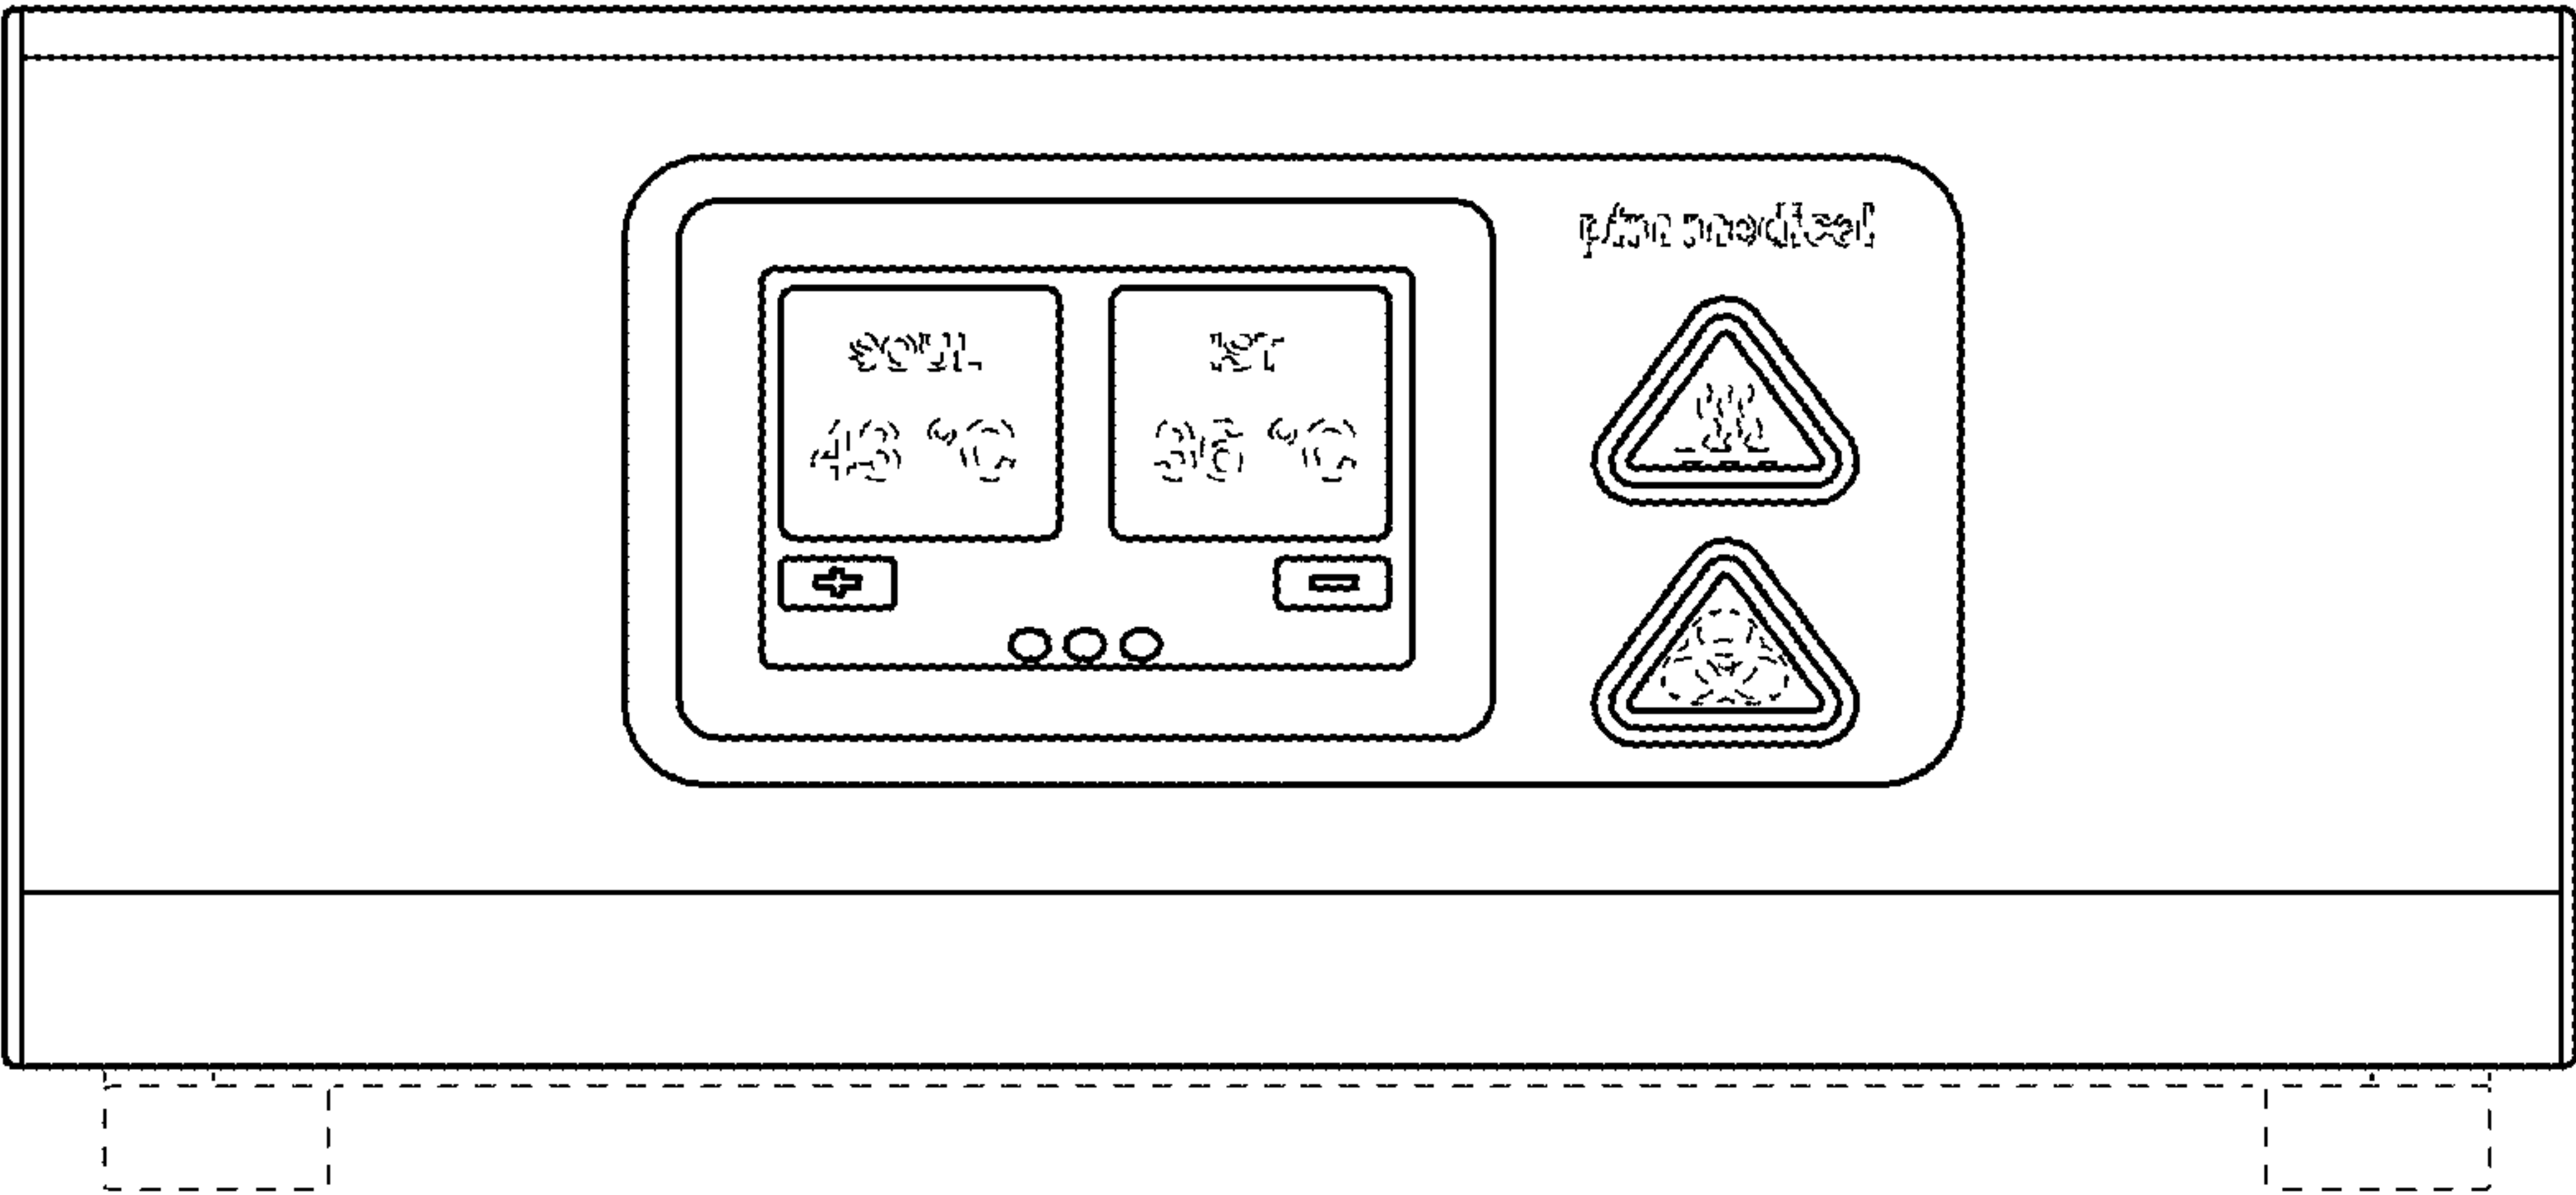


FIG. 3

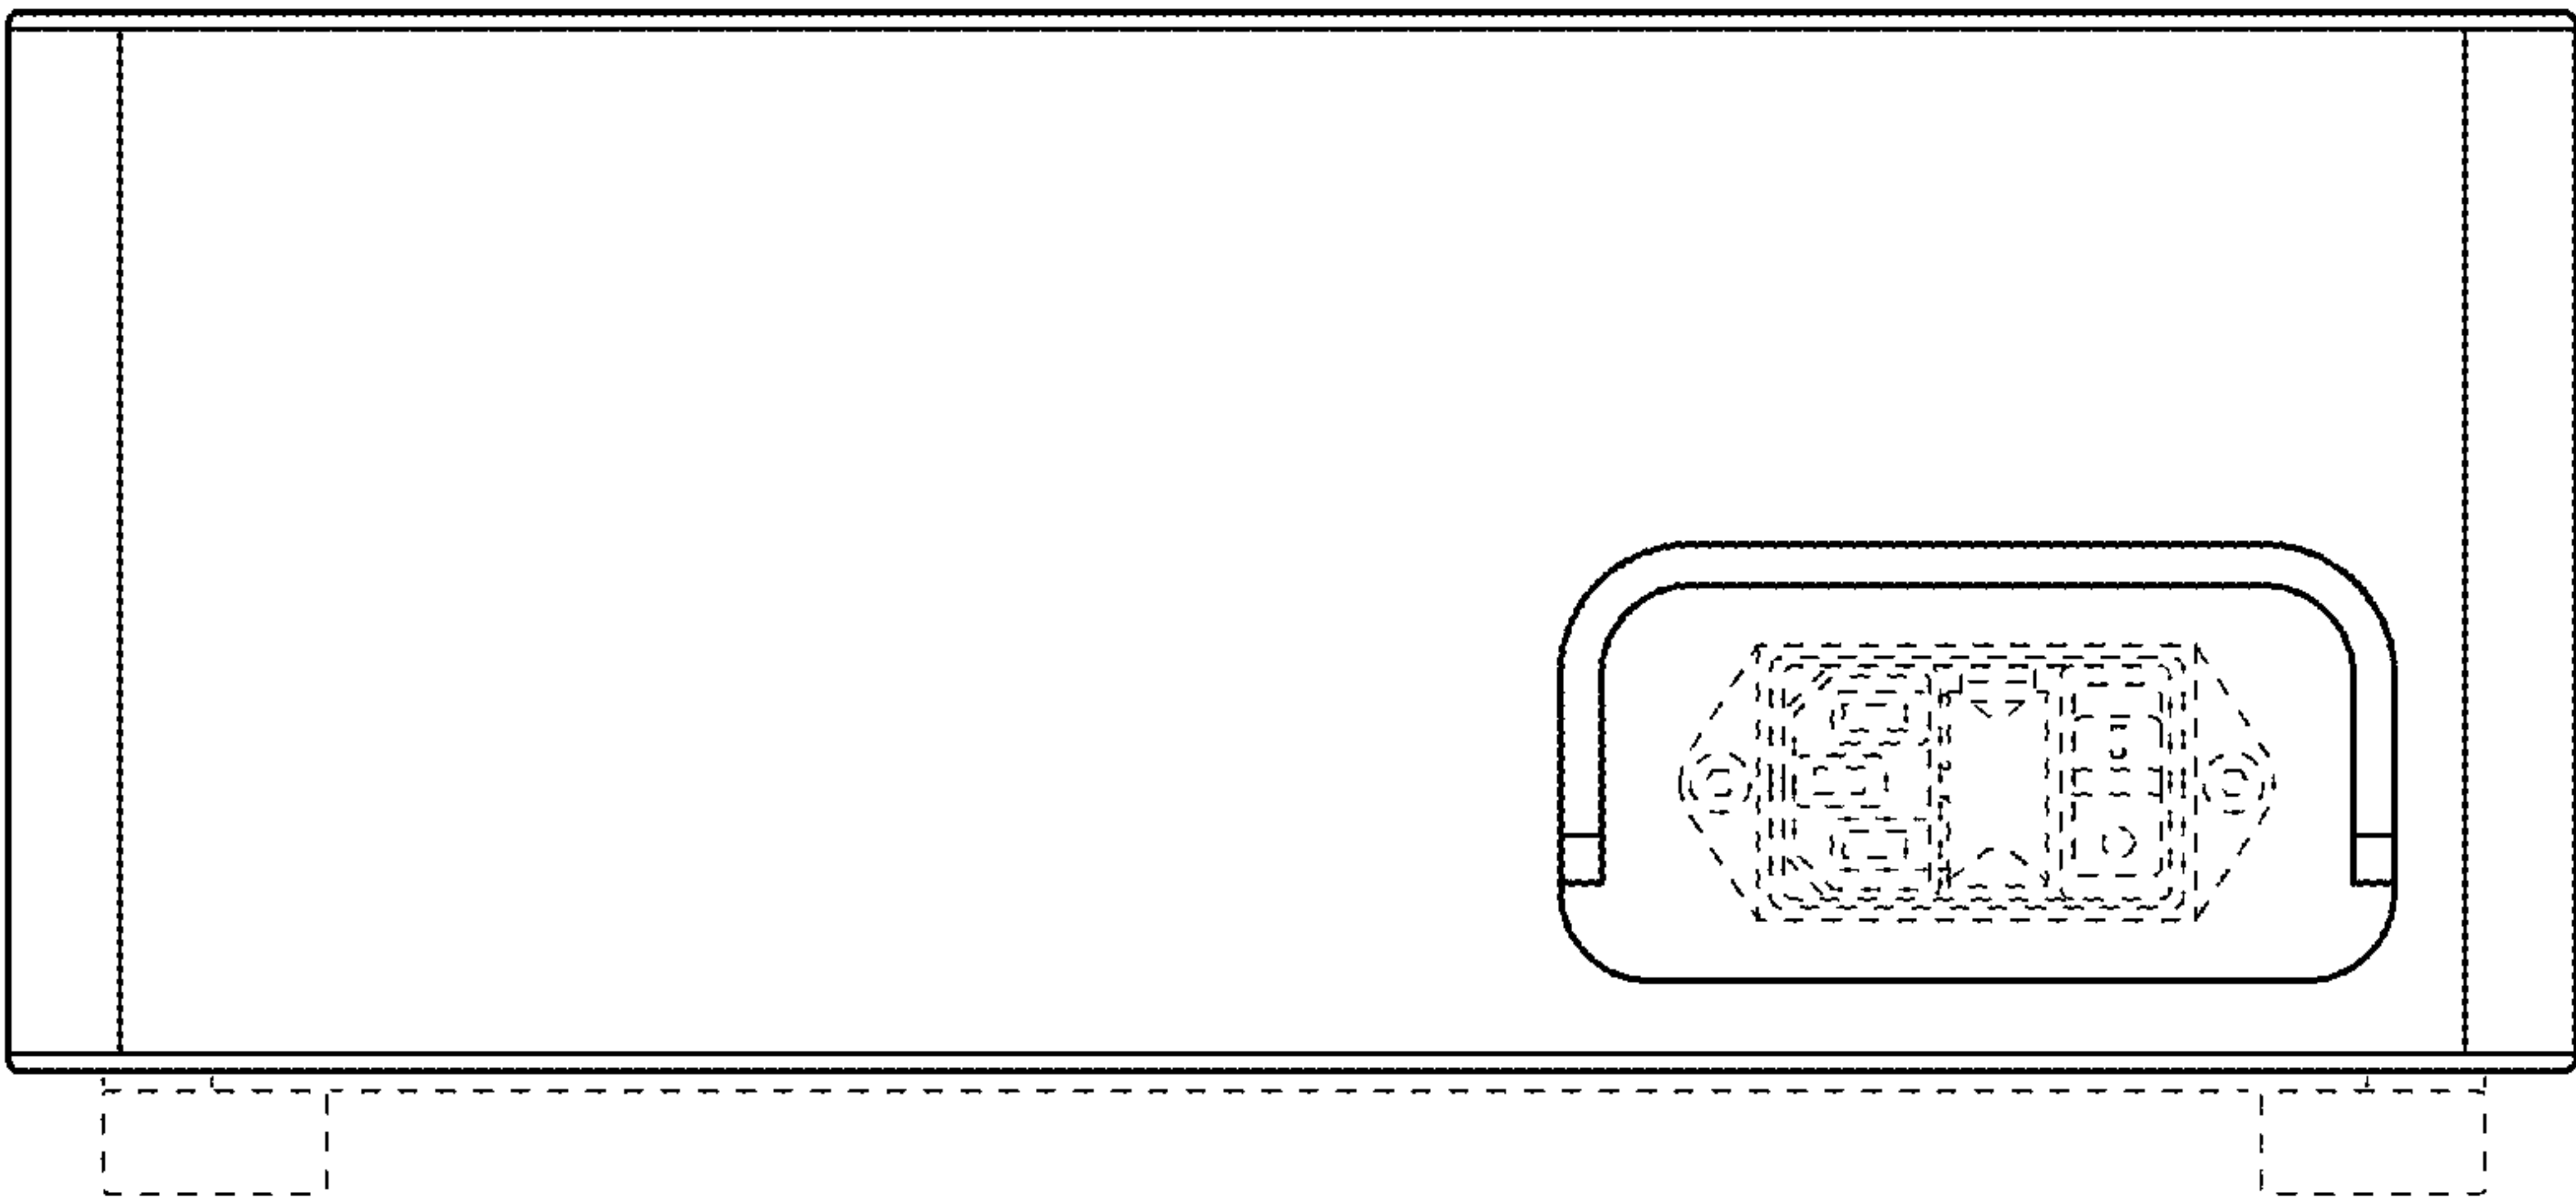


FIG. 4

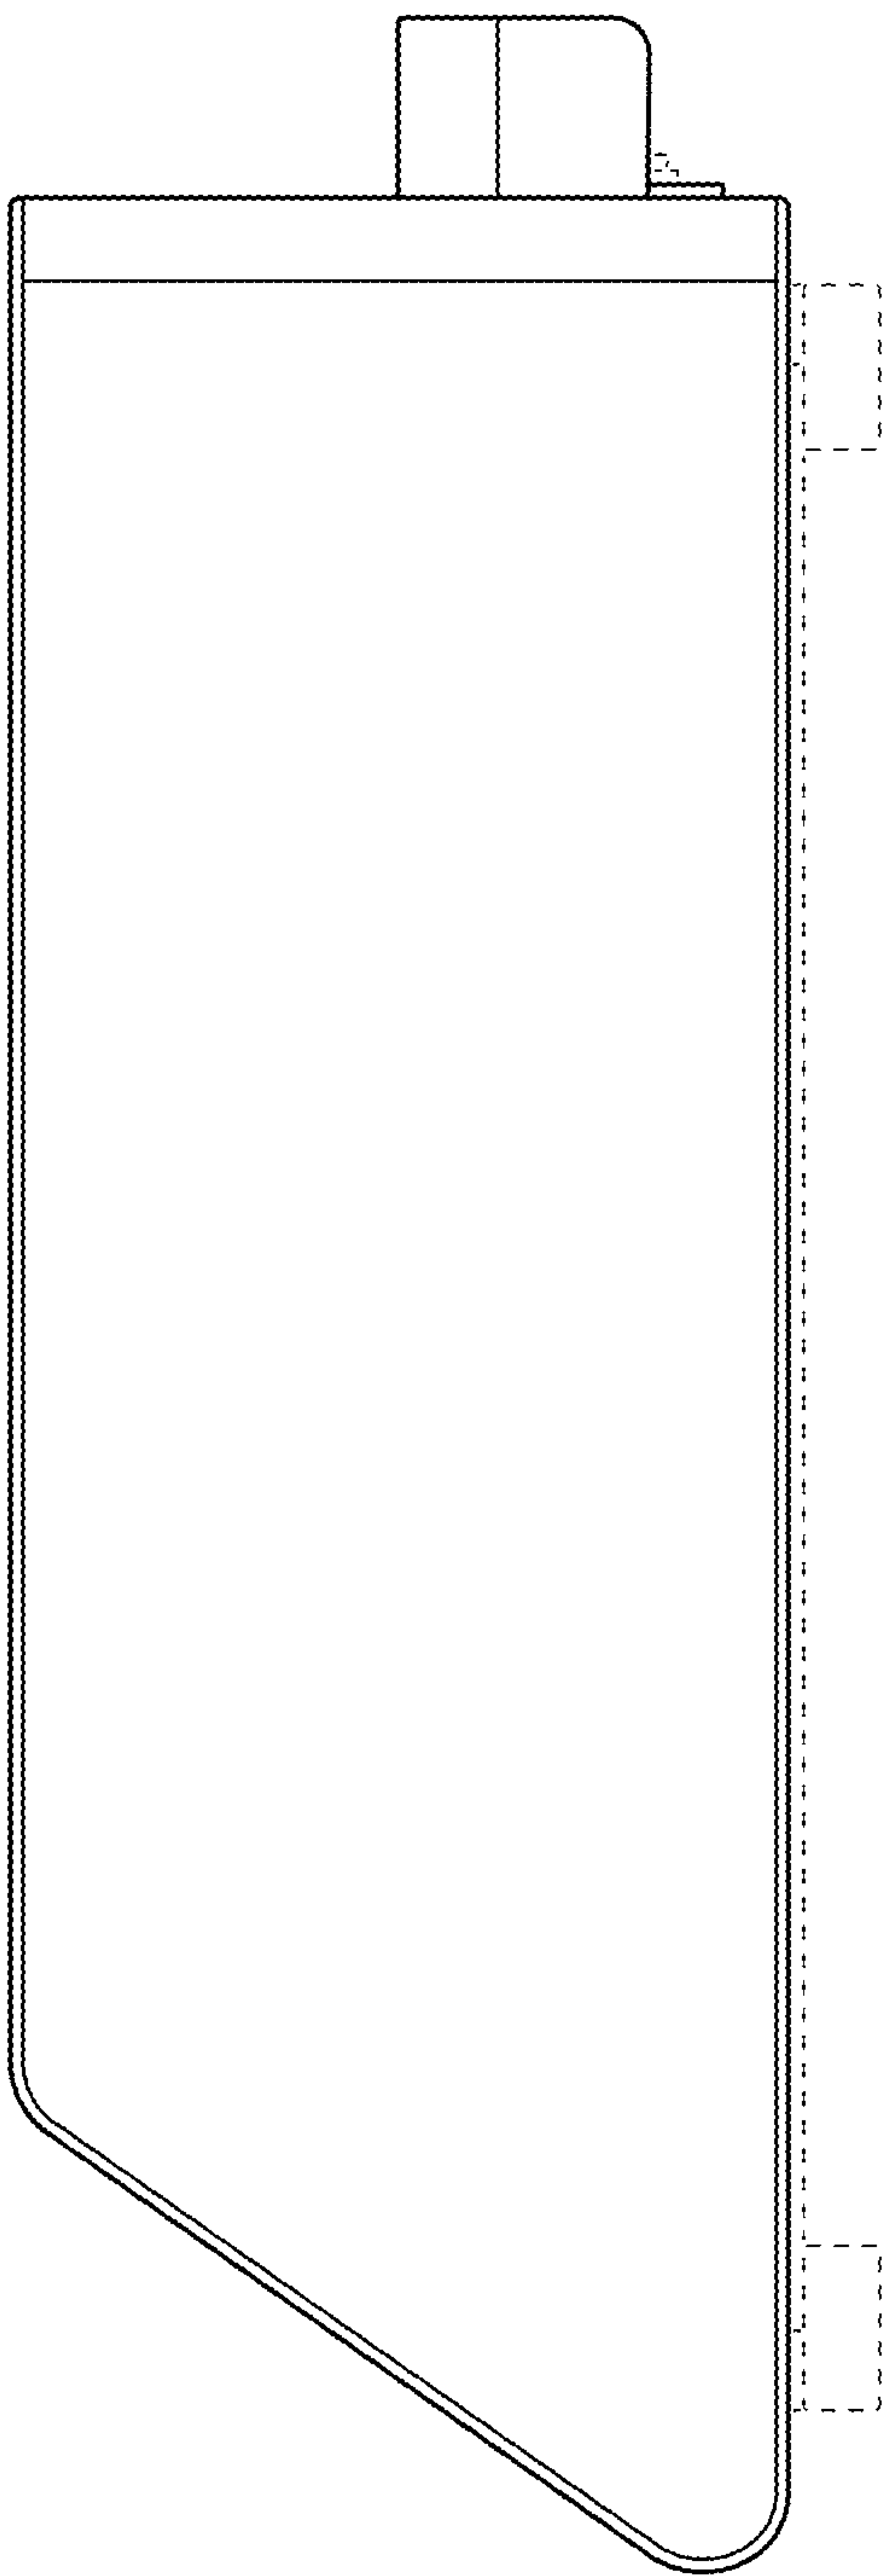


FIG. 5

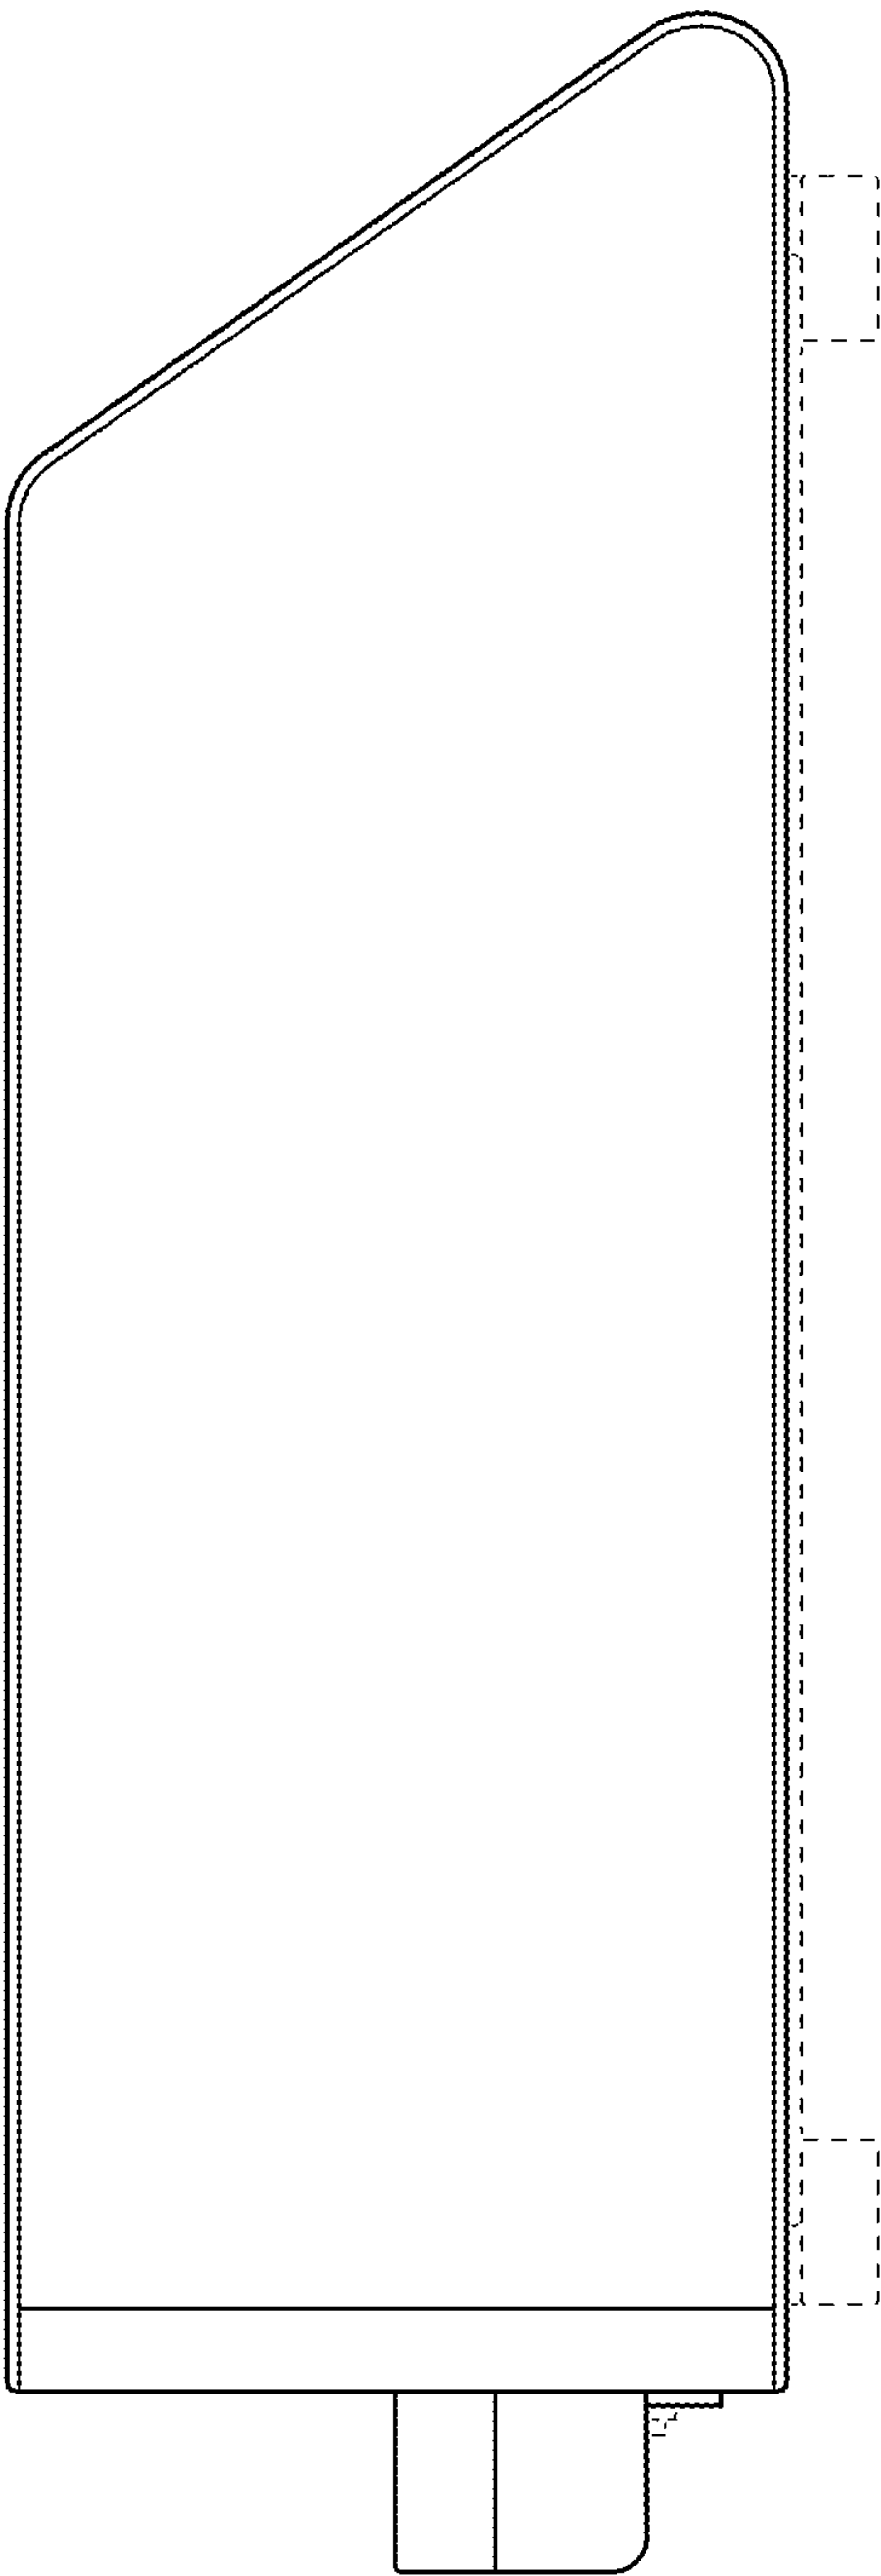


FIG. 6

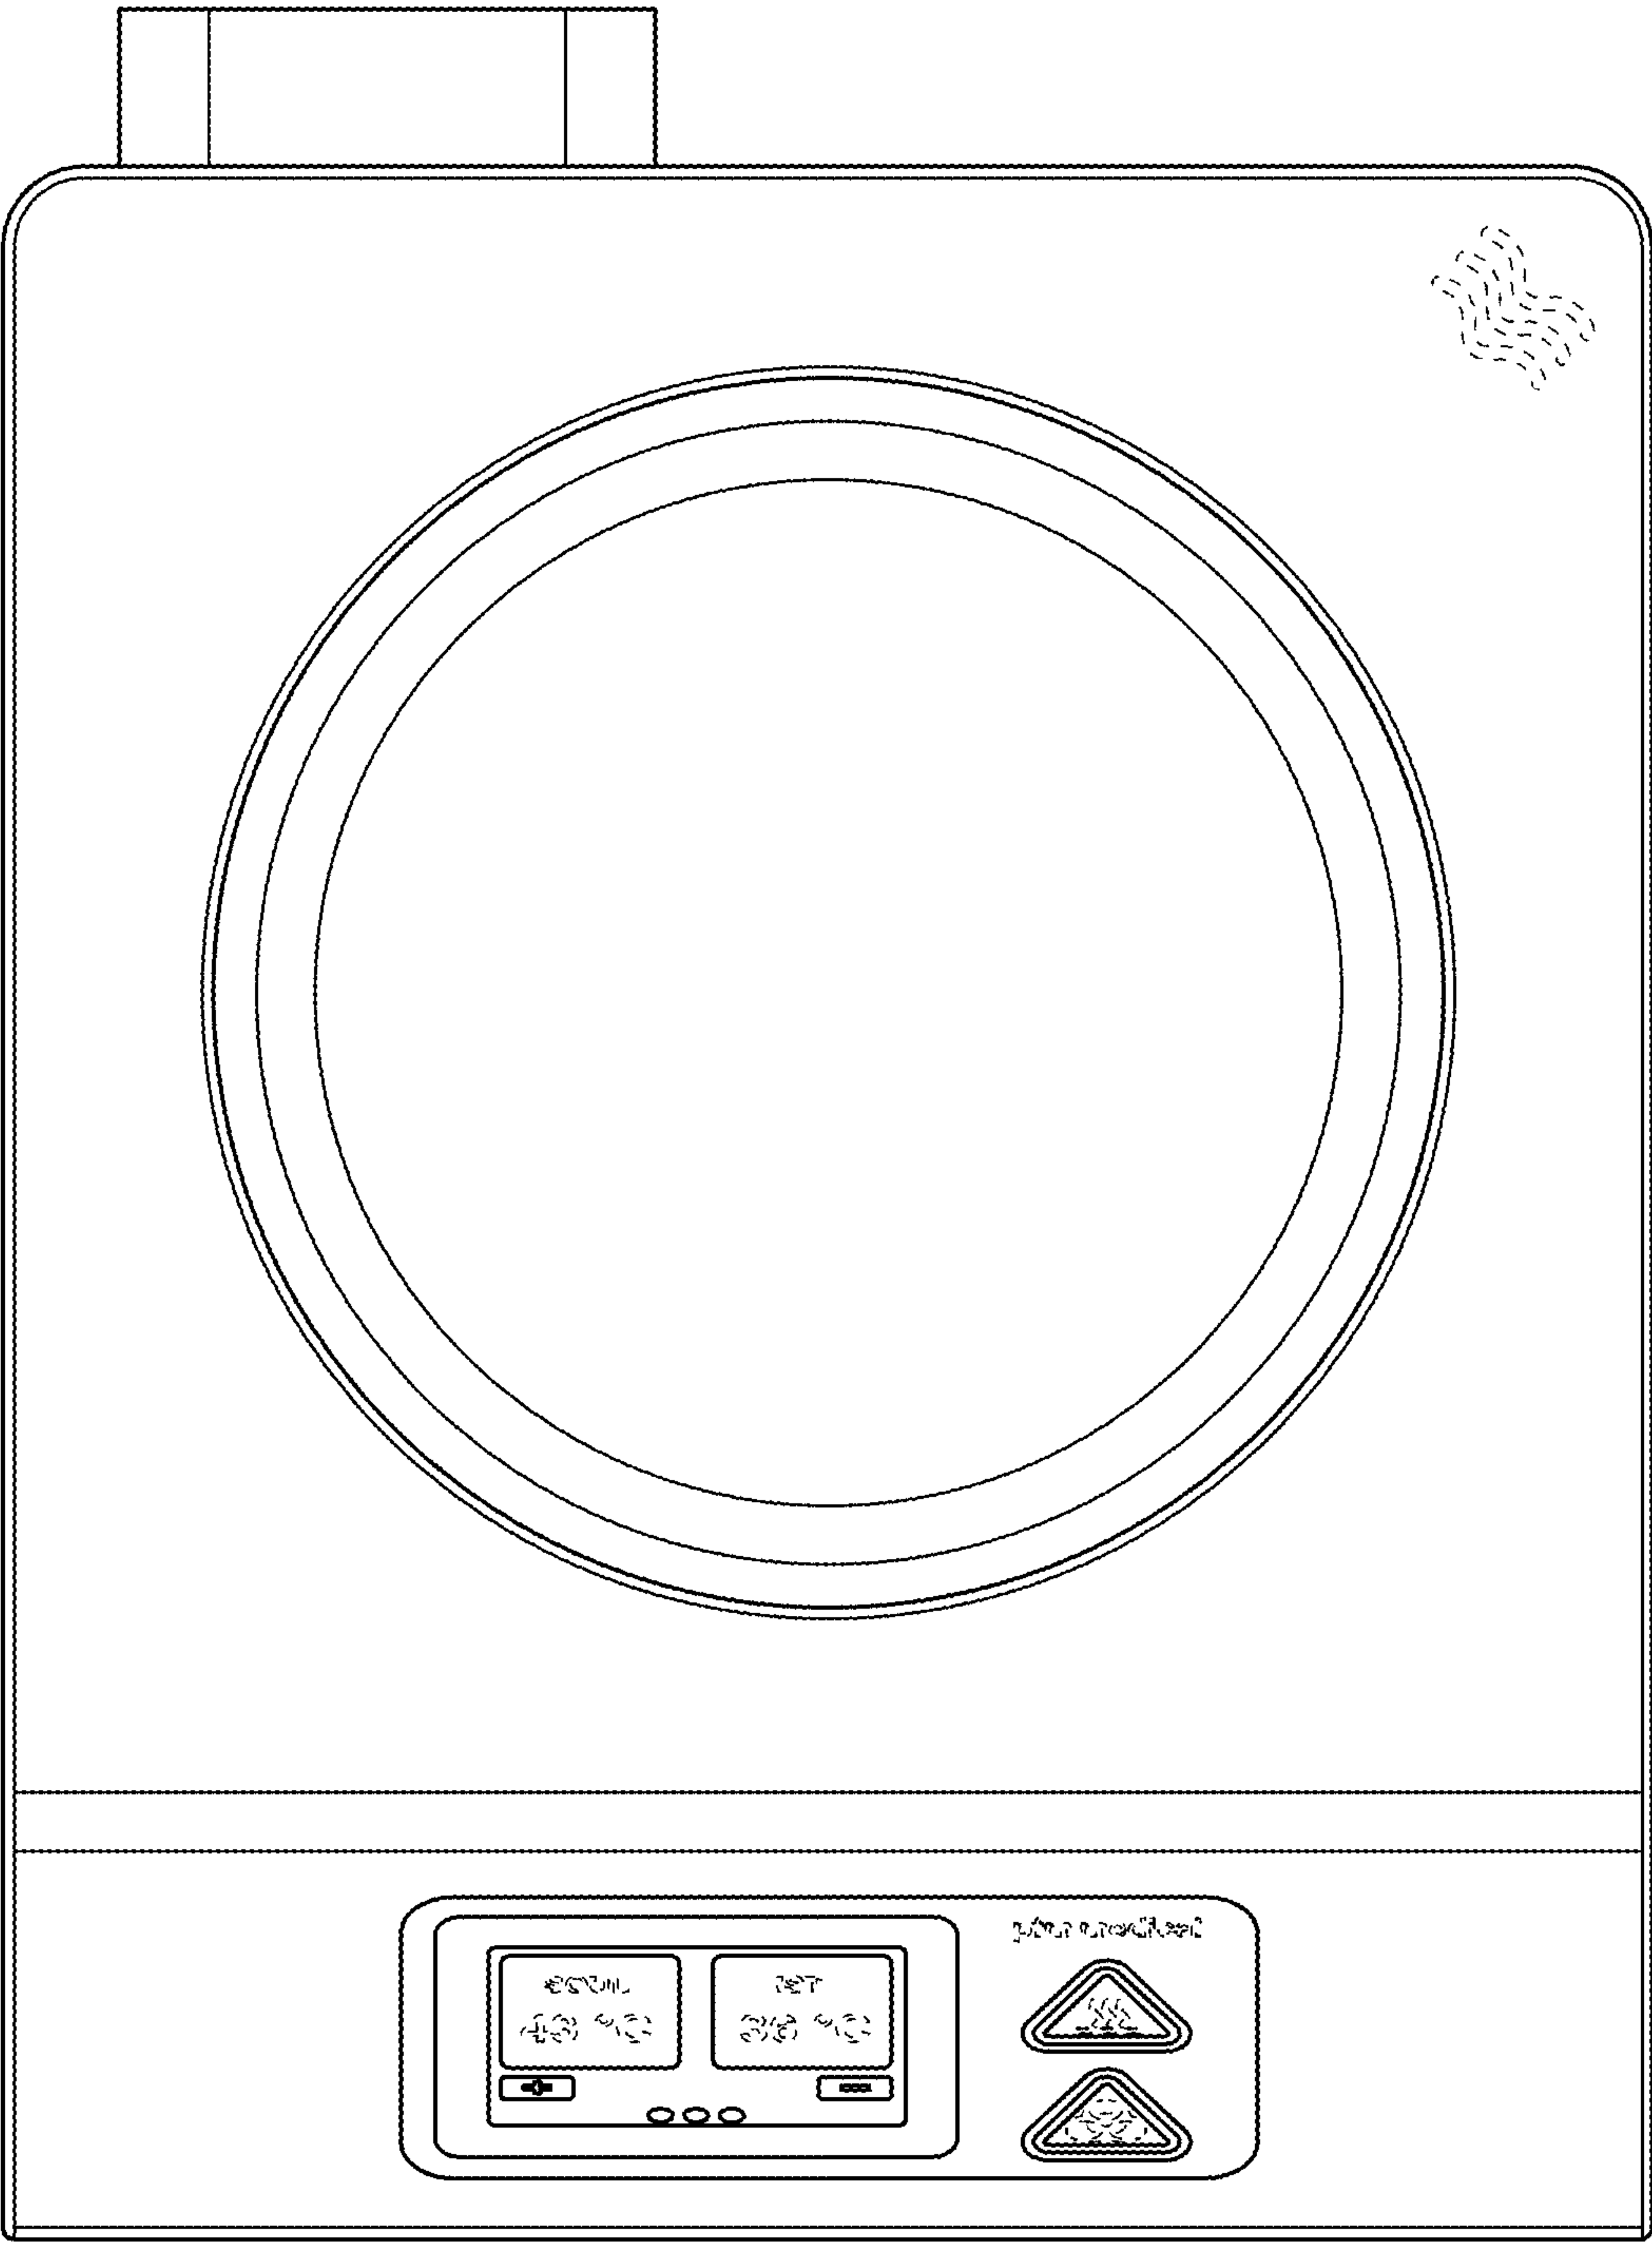


FIG. 7

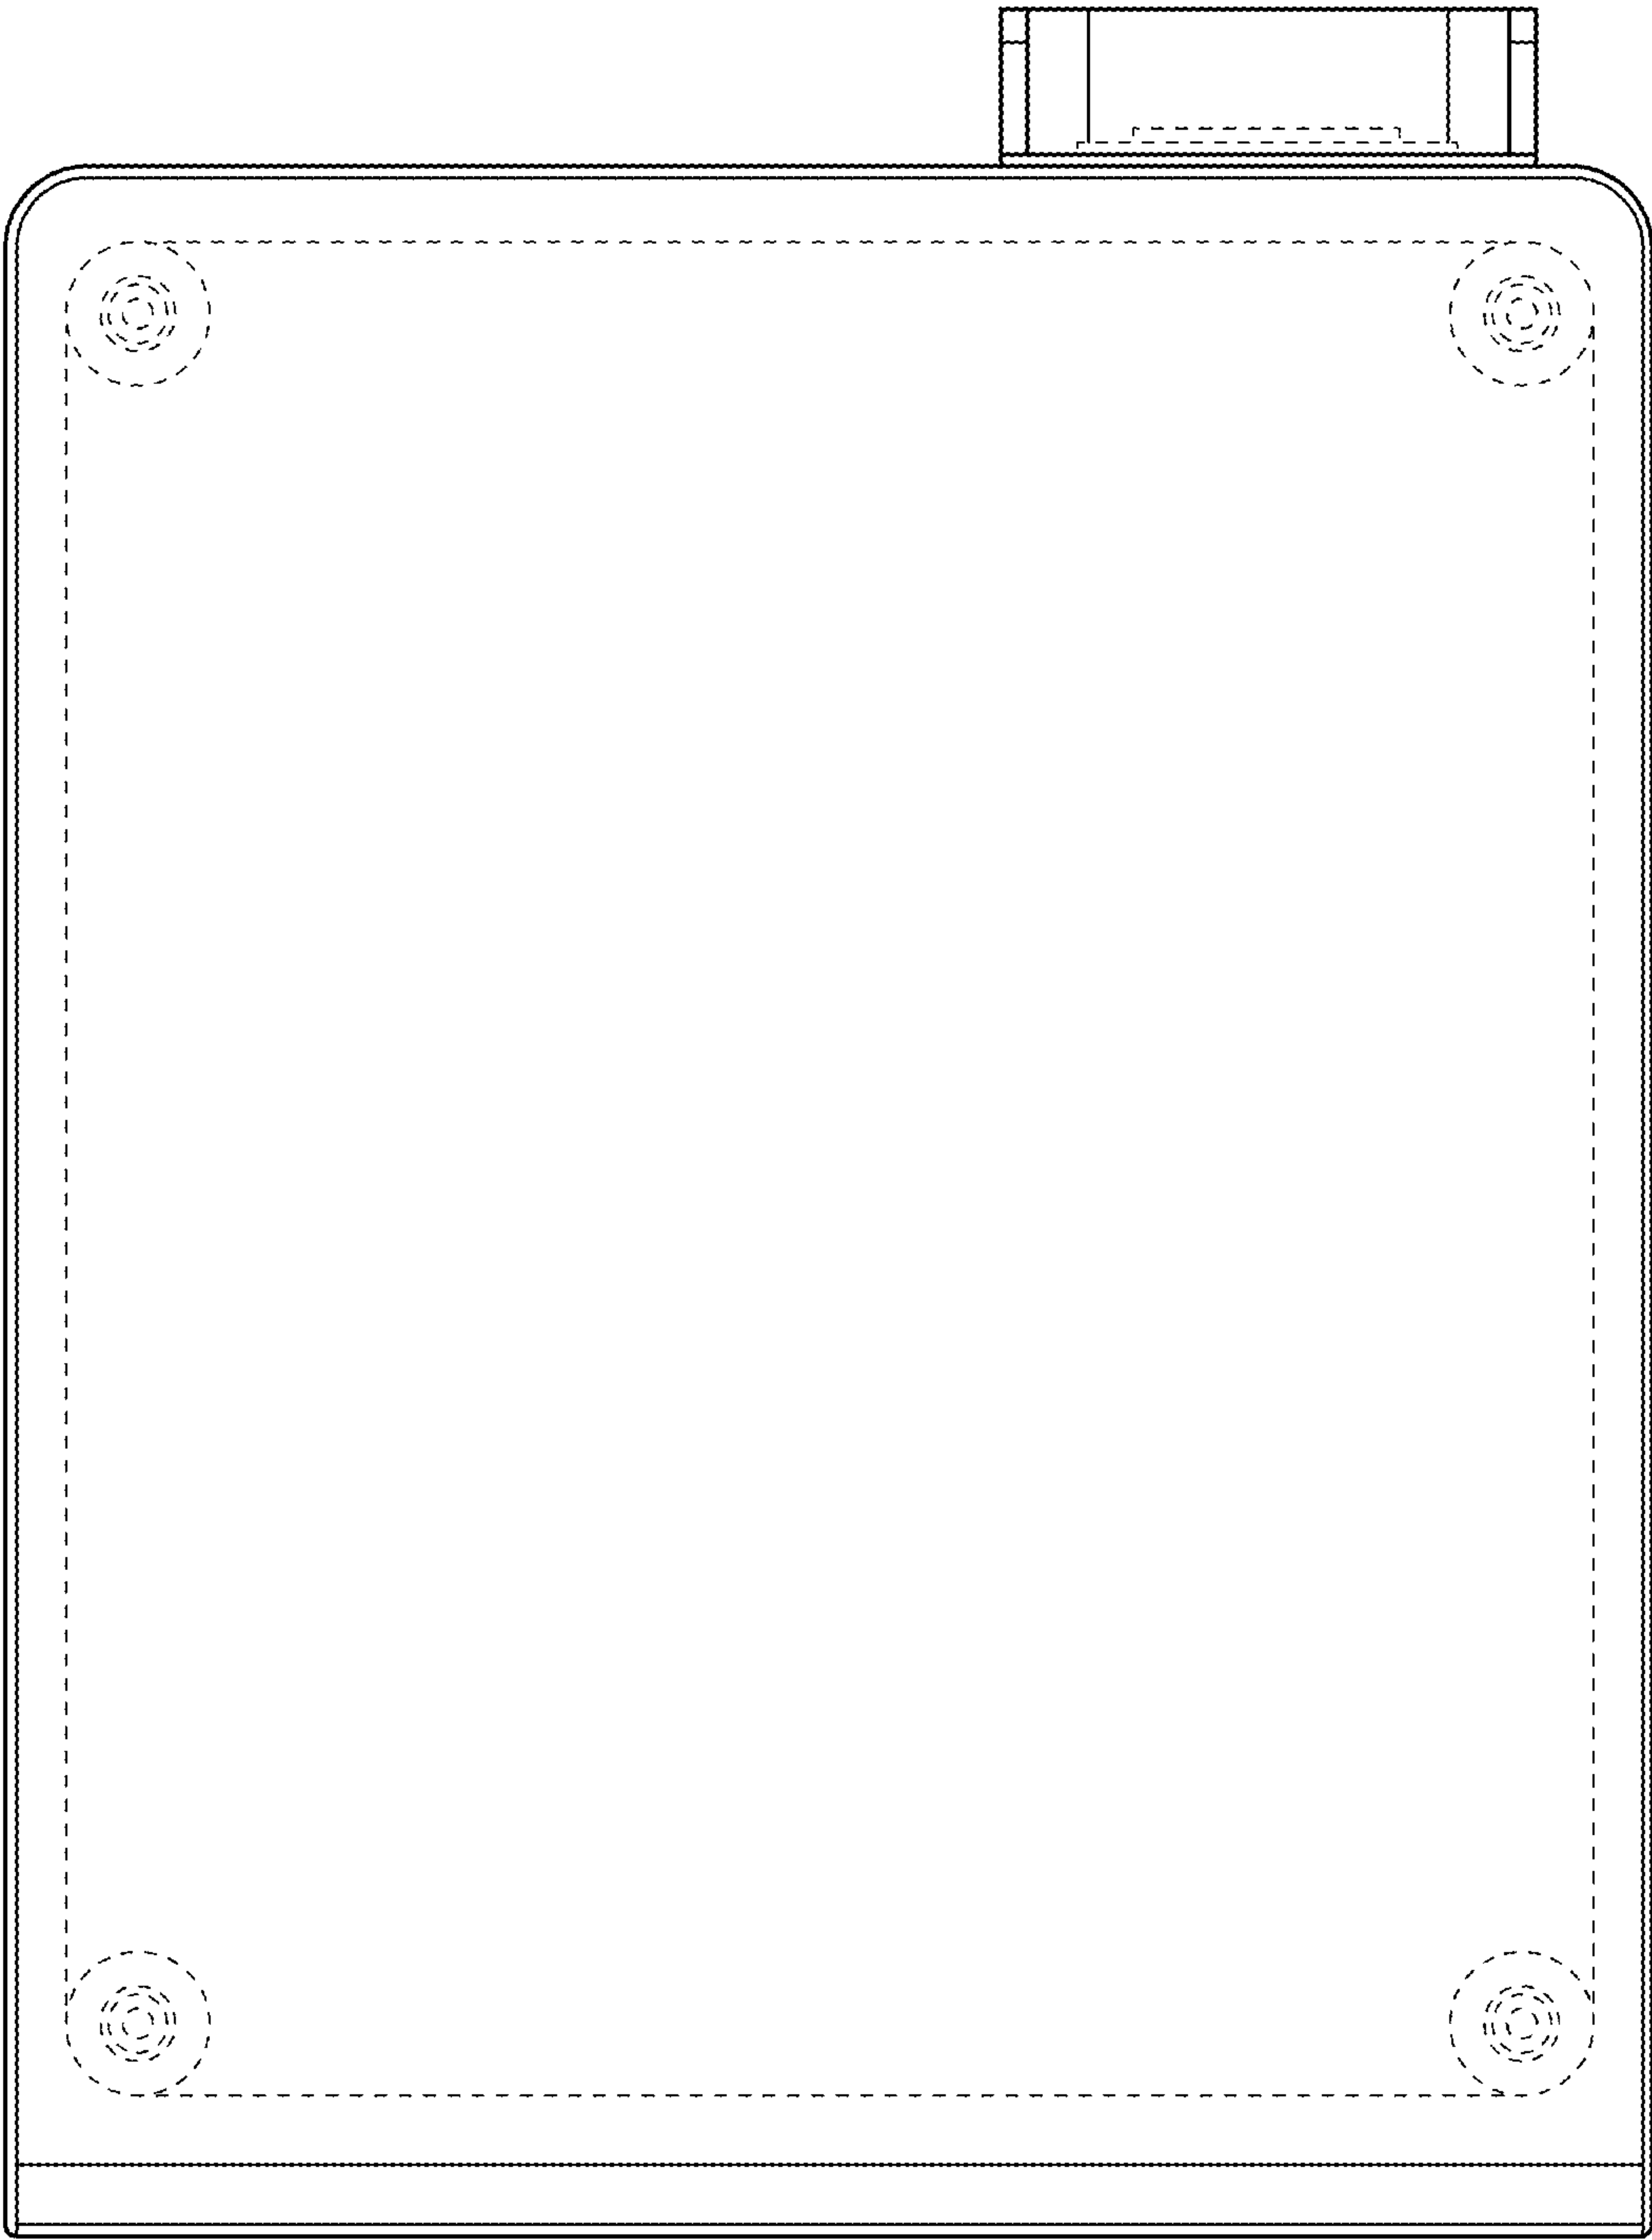


FIG. 8