

The break lines in FIGS. 1-7 indicate that the appearance of any portion of the embolization microcatheter for delivery of beads to peripheral vessels between the break lines forms no part of the claimed design.

1 Claim, 8 Drawing Sheets

(56) References Cited

U.S. PATENT DOCUMENTS

D861,156 S * 9/2019 Greenhalgh D24/108
D870,880 S * 12/2019 Hanson D24/112
11,129,960 B2 * 9/2021 Tal A61M 25/0051
D957,622 S * 7/2022 Oddo D24/110.4
D958,348 S * 7/2022 Balkovec D24/140
11,471,646 B2 * 10/2022 Tal A61L 29/126
D980,970 S * 3/2023 Virk D24/112
D980,971 S * 3/2023 Zarins D24/112
D980,972 S * 3/2023 Zarins D24/112
2013/0123752 A1 5/2013 Pursley
2021/0177430 A1 * 6/2021 Tal A61M 25/0051
2021/0196292 A1 * 7/2021 Vale A61M 25/0074
2022/0218358 A1 * 7/2022 Dagan A61N 5/1002
2023/0047163 A1 * 2/2023 Tal A61M 25/0054
2023/0277804 A1 * 9/2023 Dagan A61M 25/005
604/508
2023/0302254 A1 * 9/2023 Dagan A61M 25/0068

FOREIGN PATENT DOCUMENTS

IL 276416 B 8/2021
JP D1245407 * 7/2005

* cited by examiner

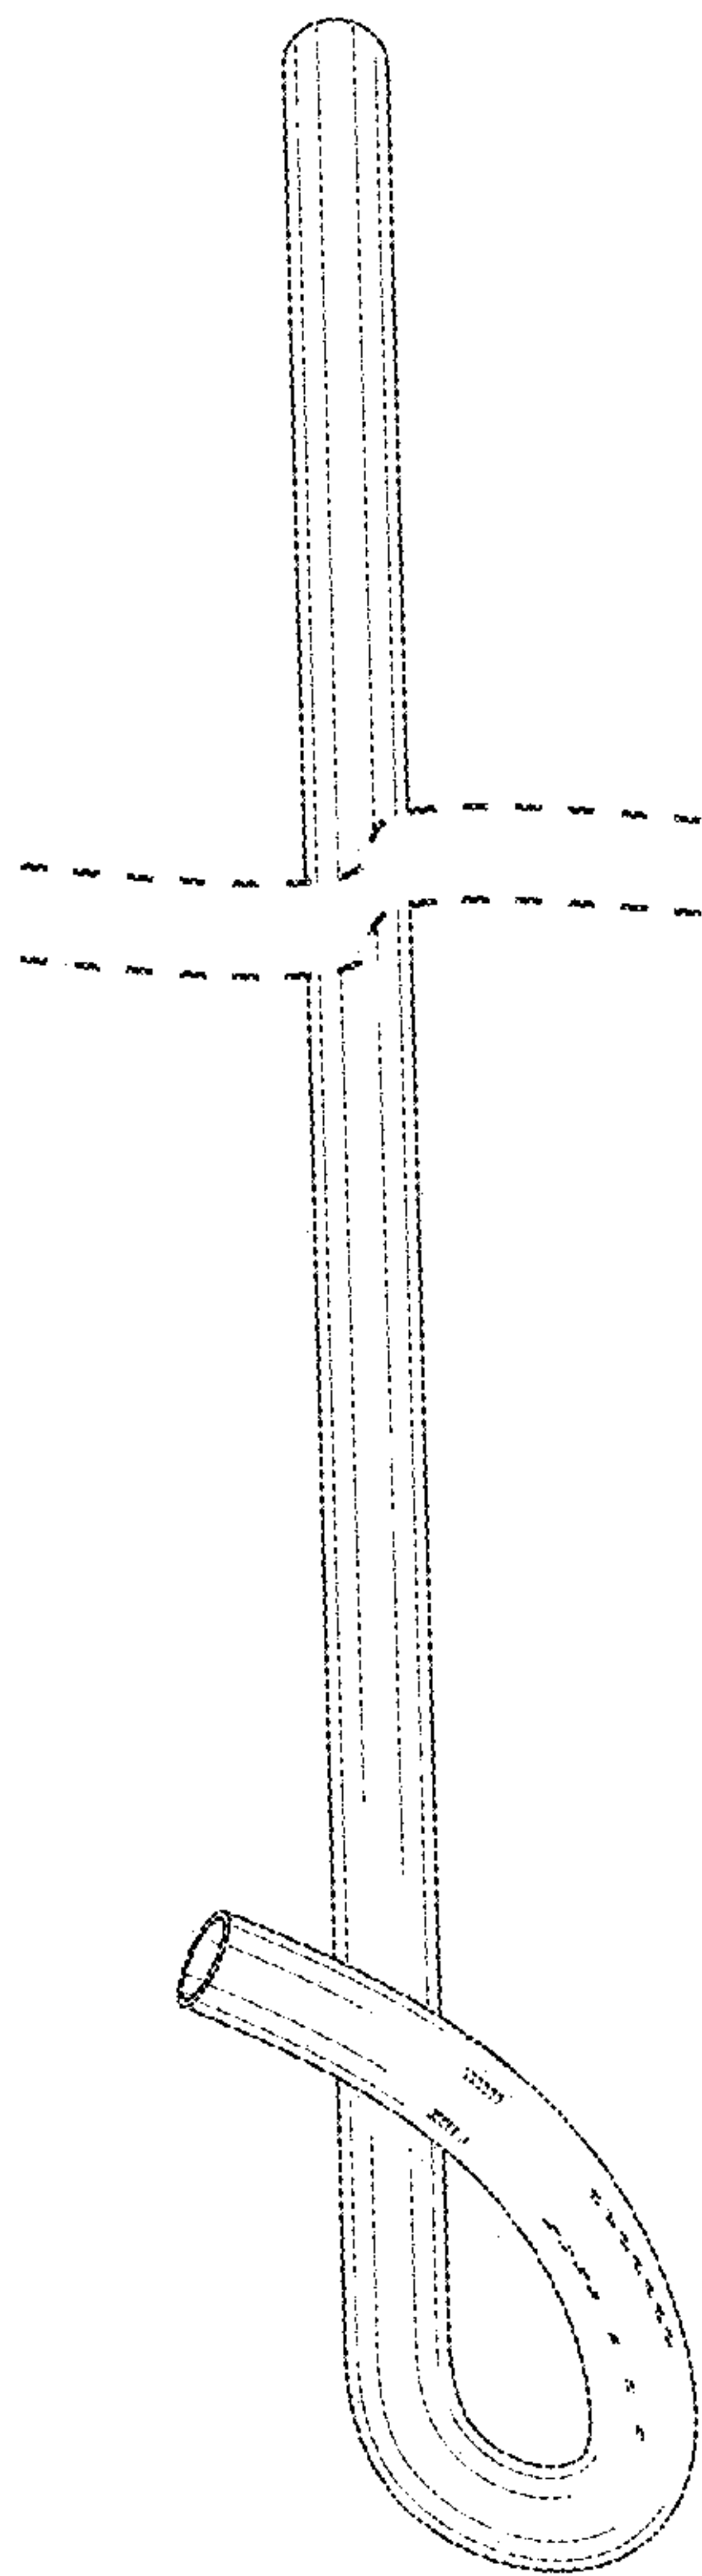


FIG. 1

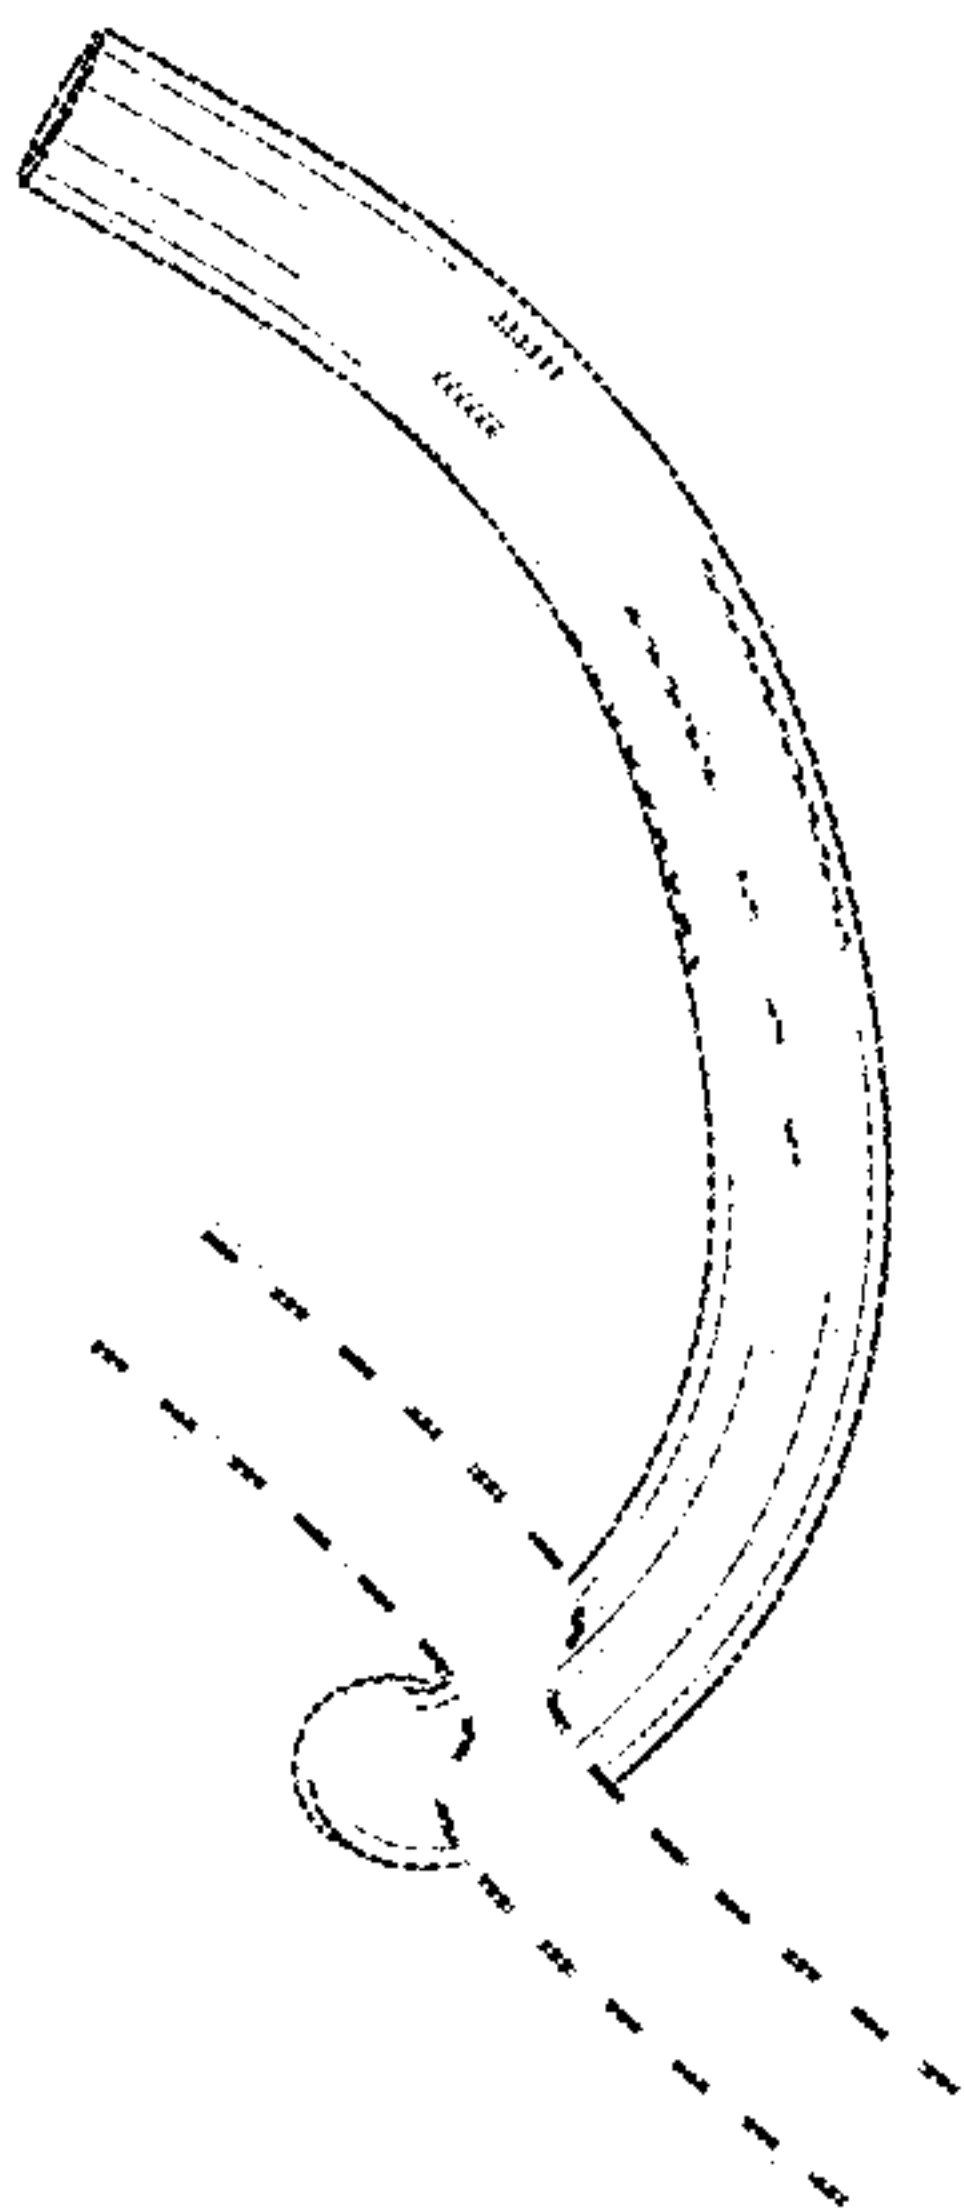


FIG. 2

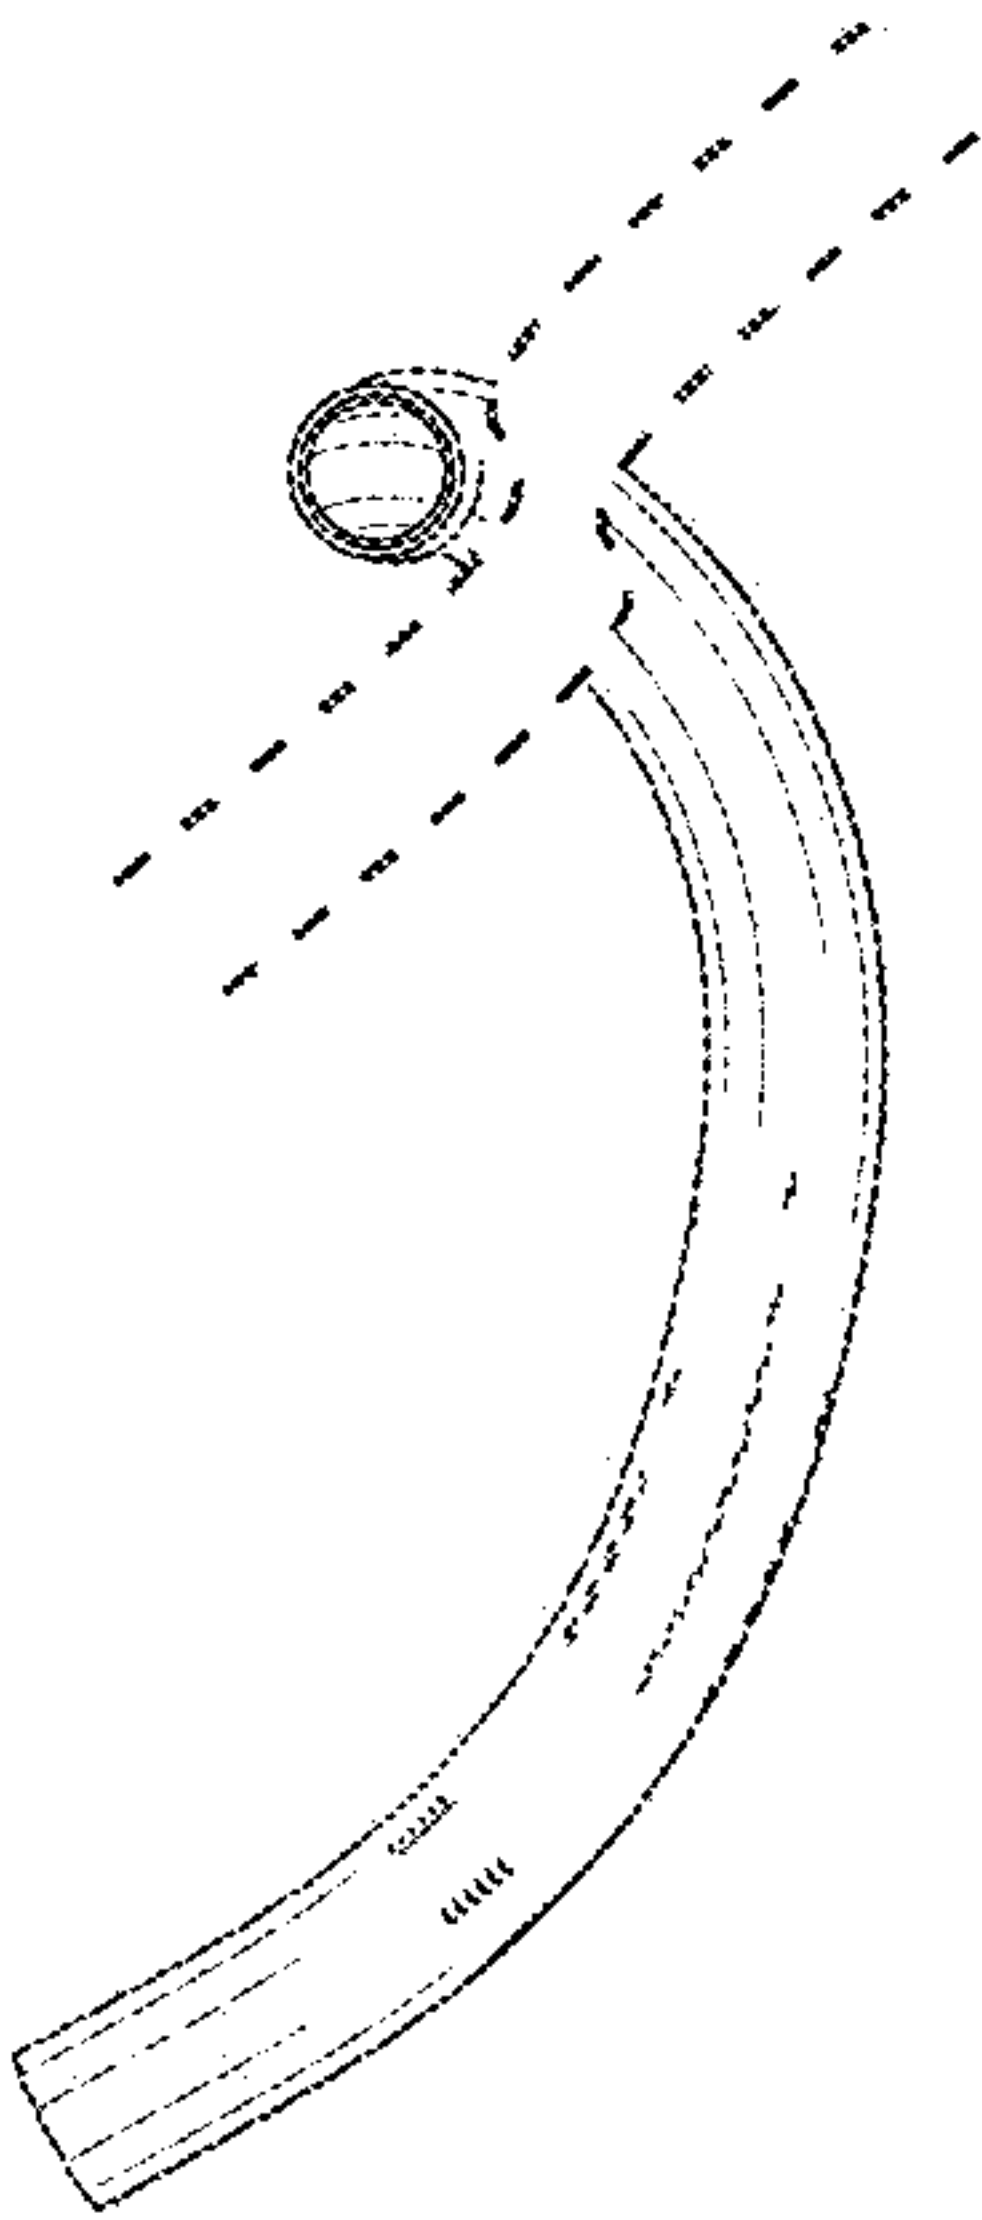


FIG. 3

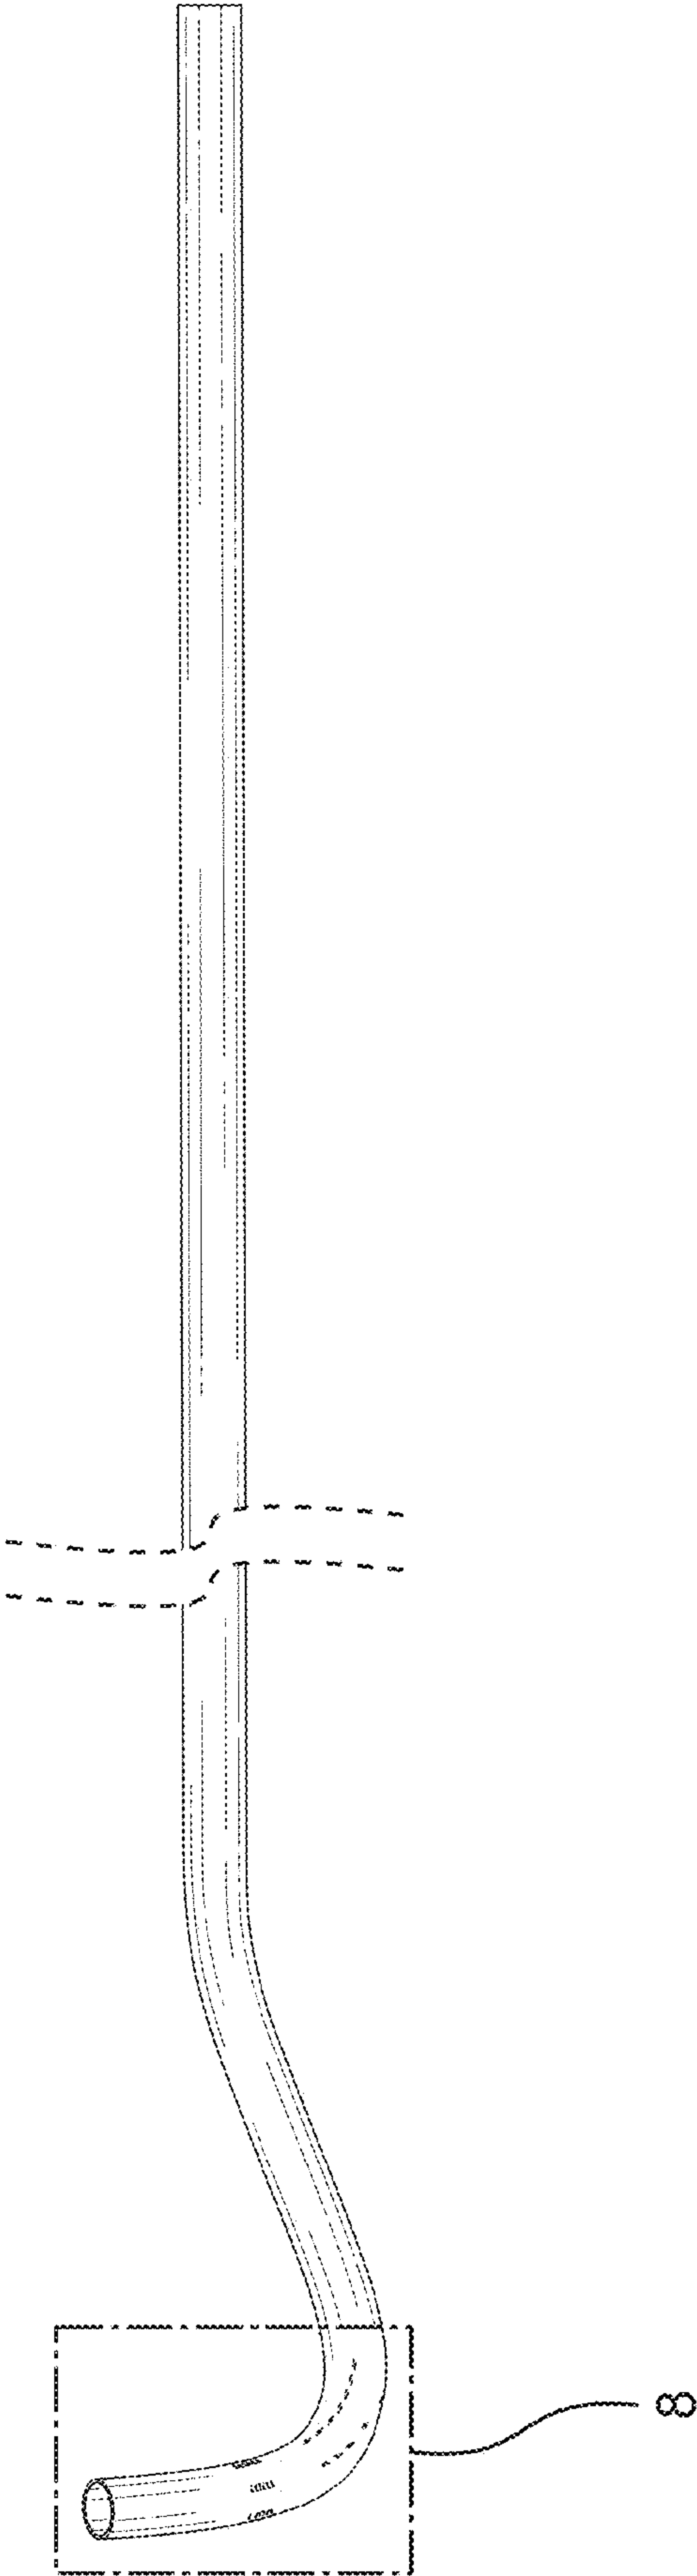


FIG. 4

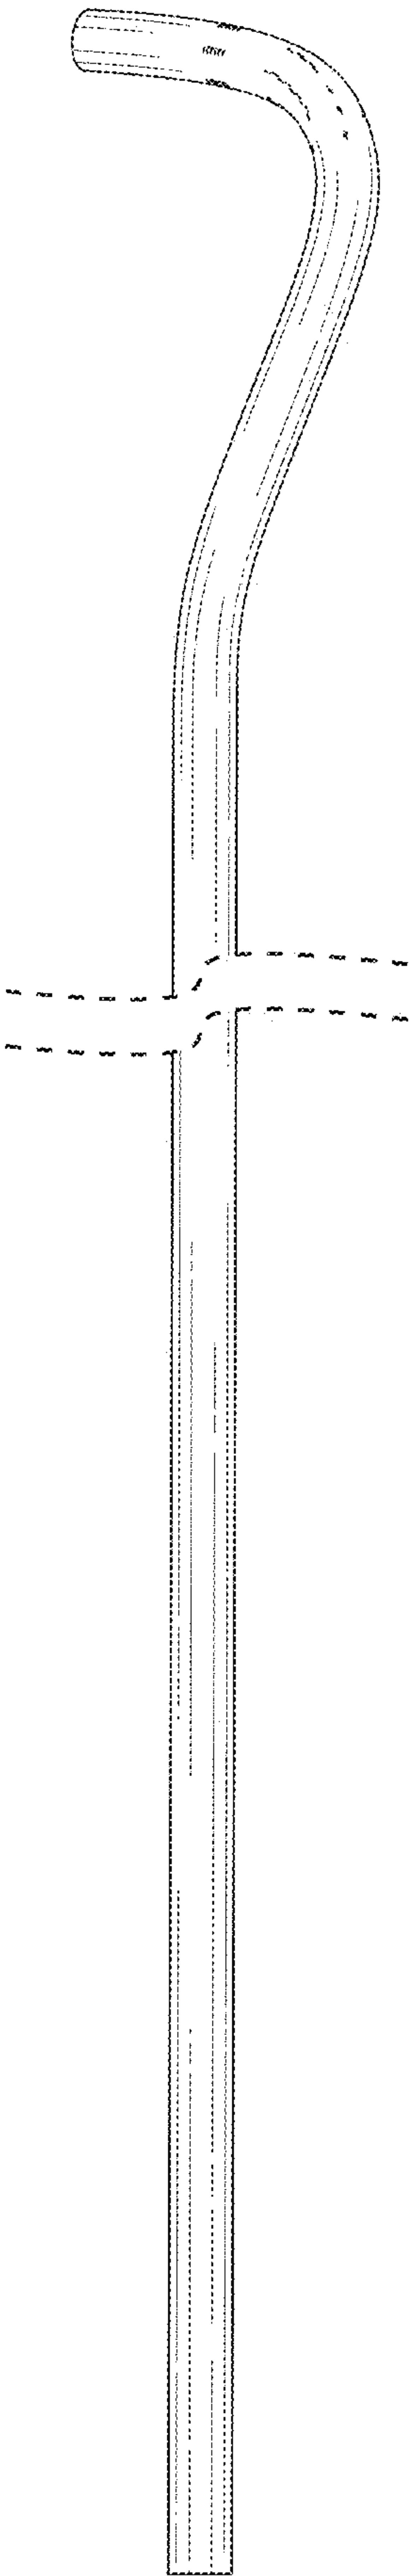


FIG. 5

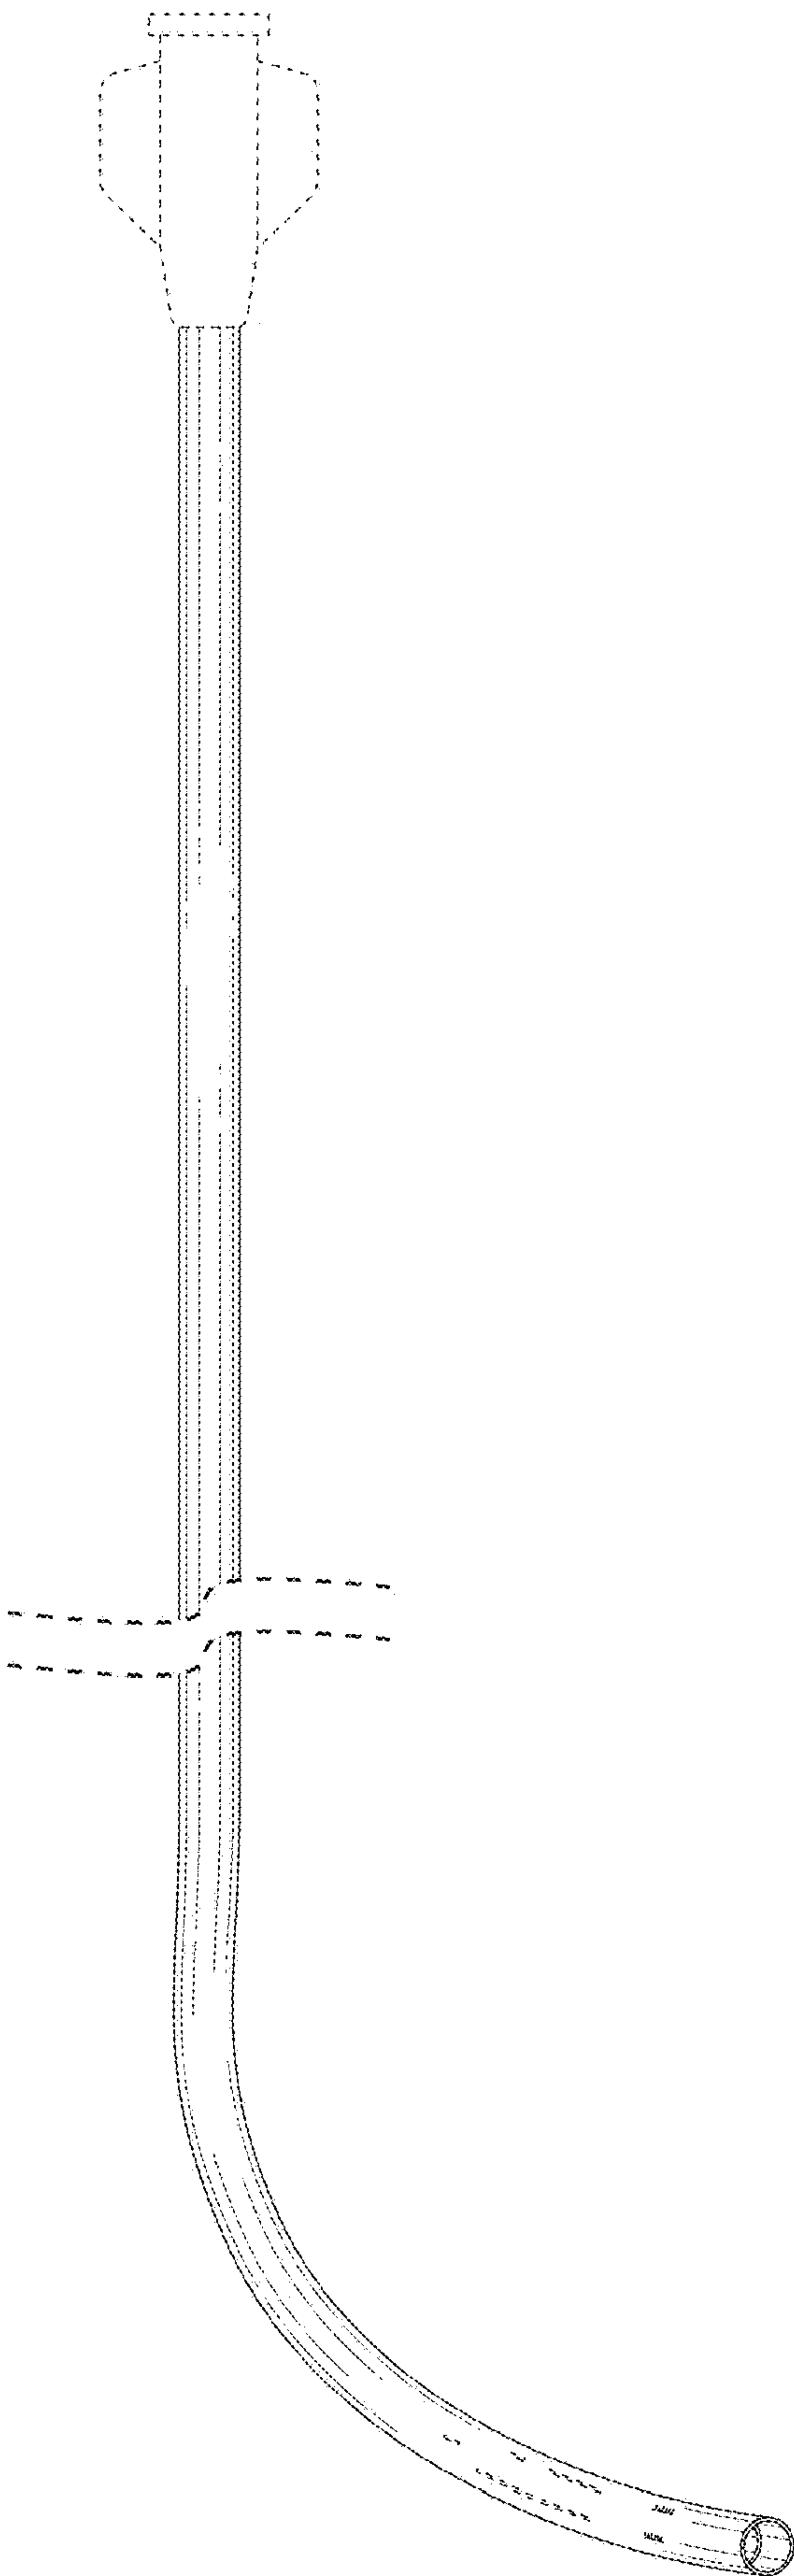


FIG. 6

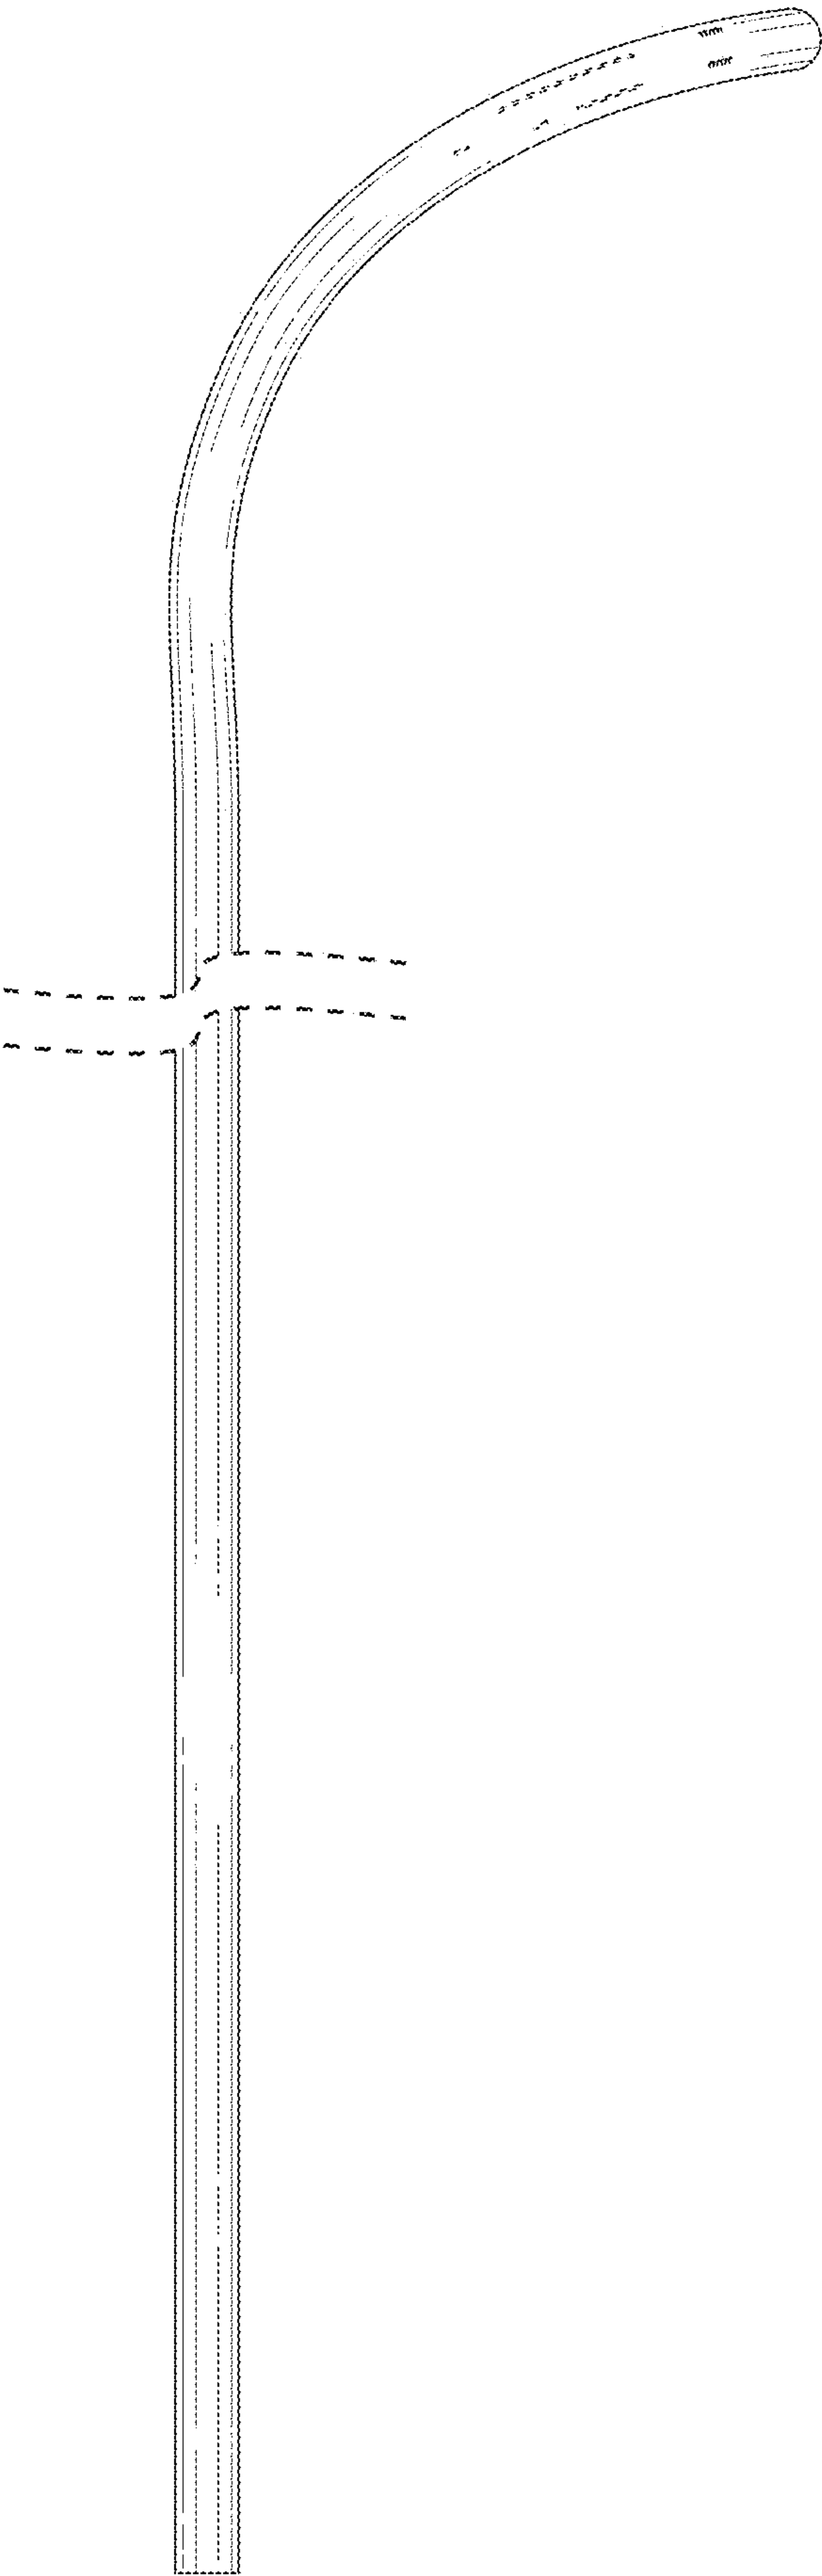


FIG. 7

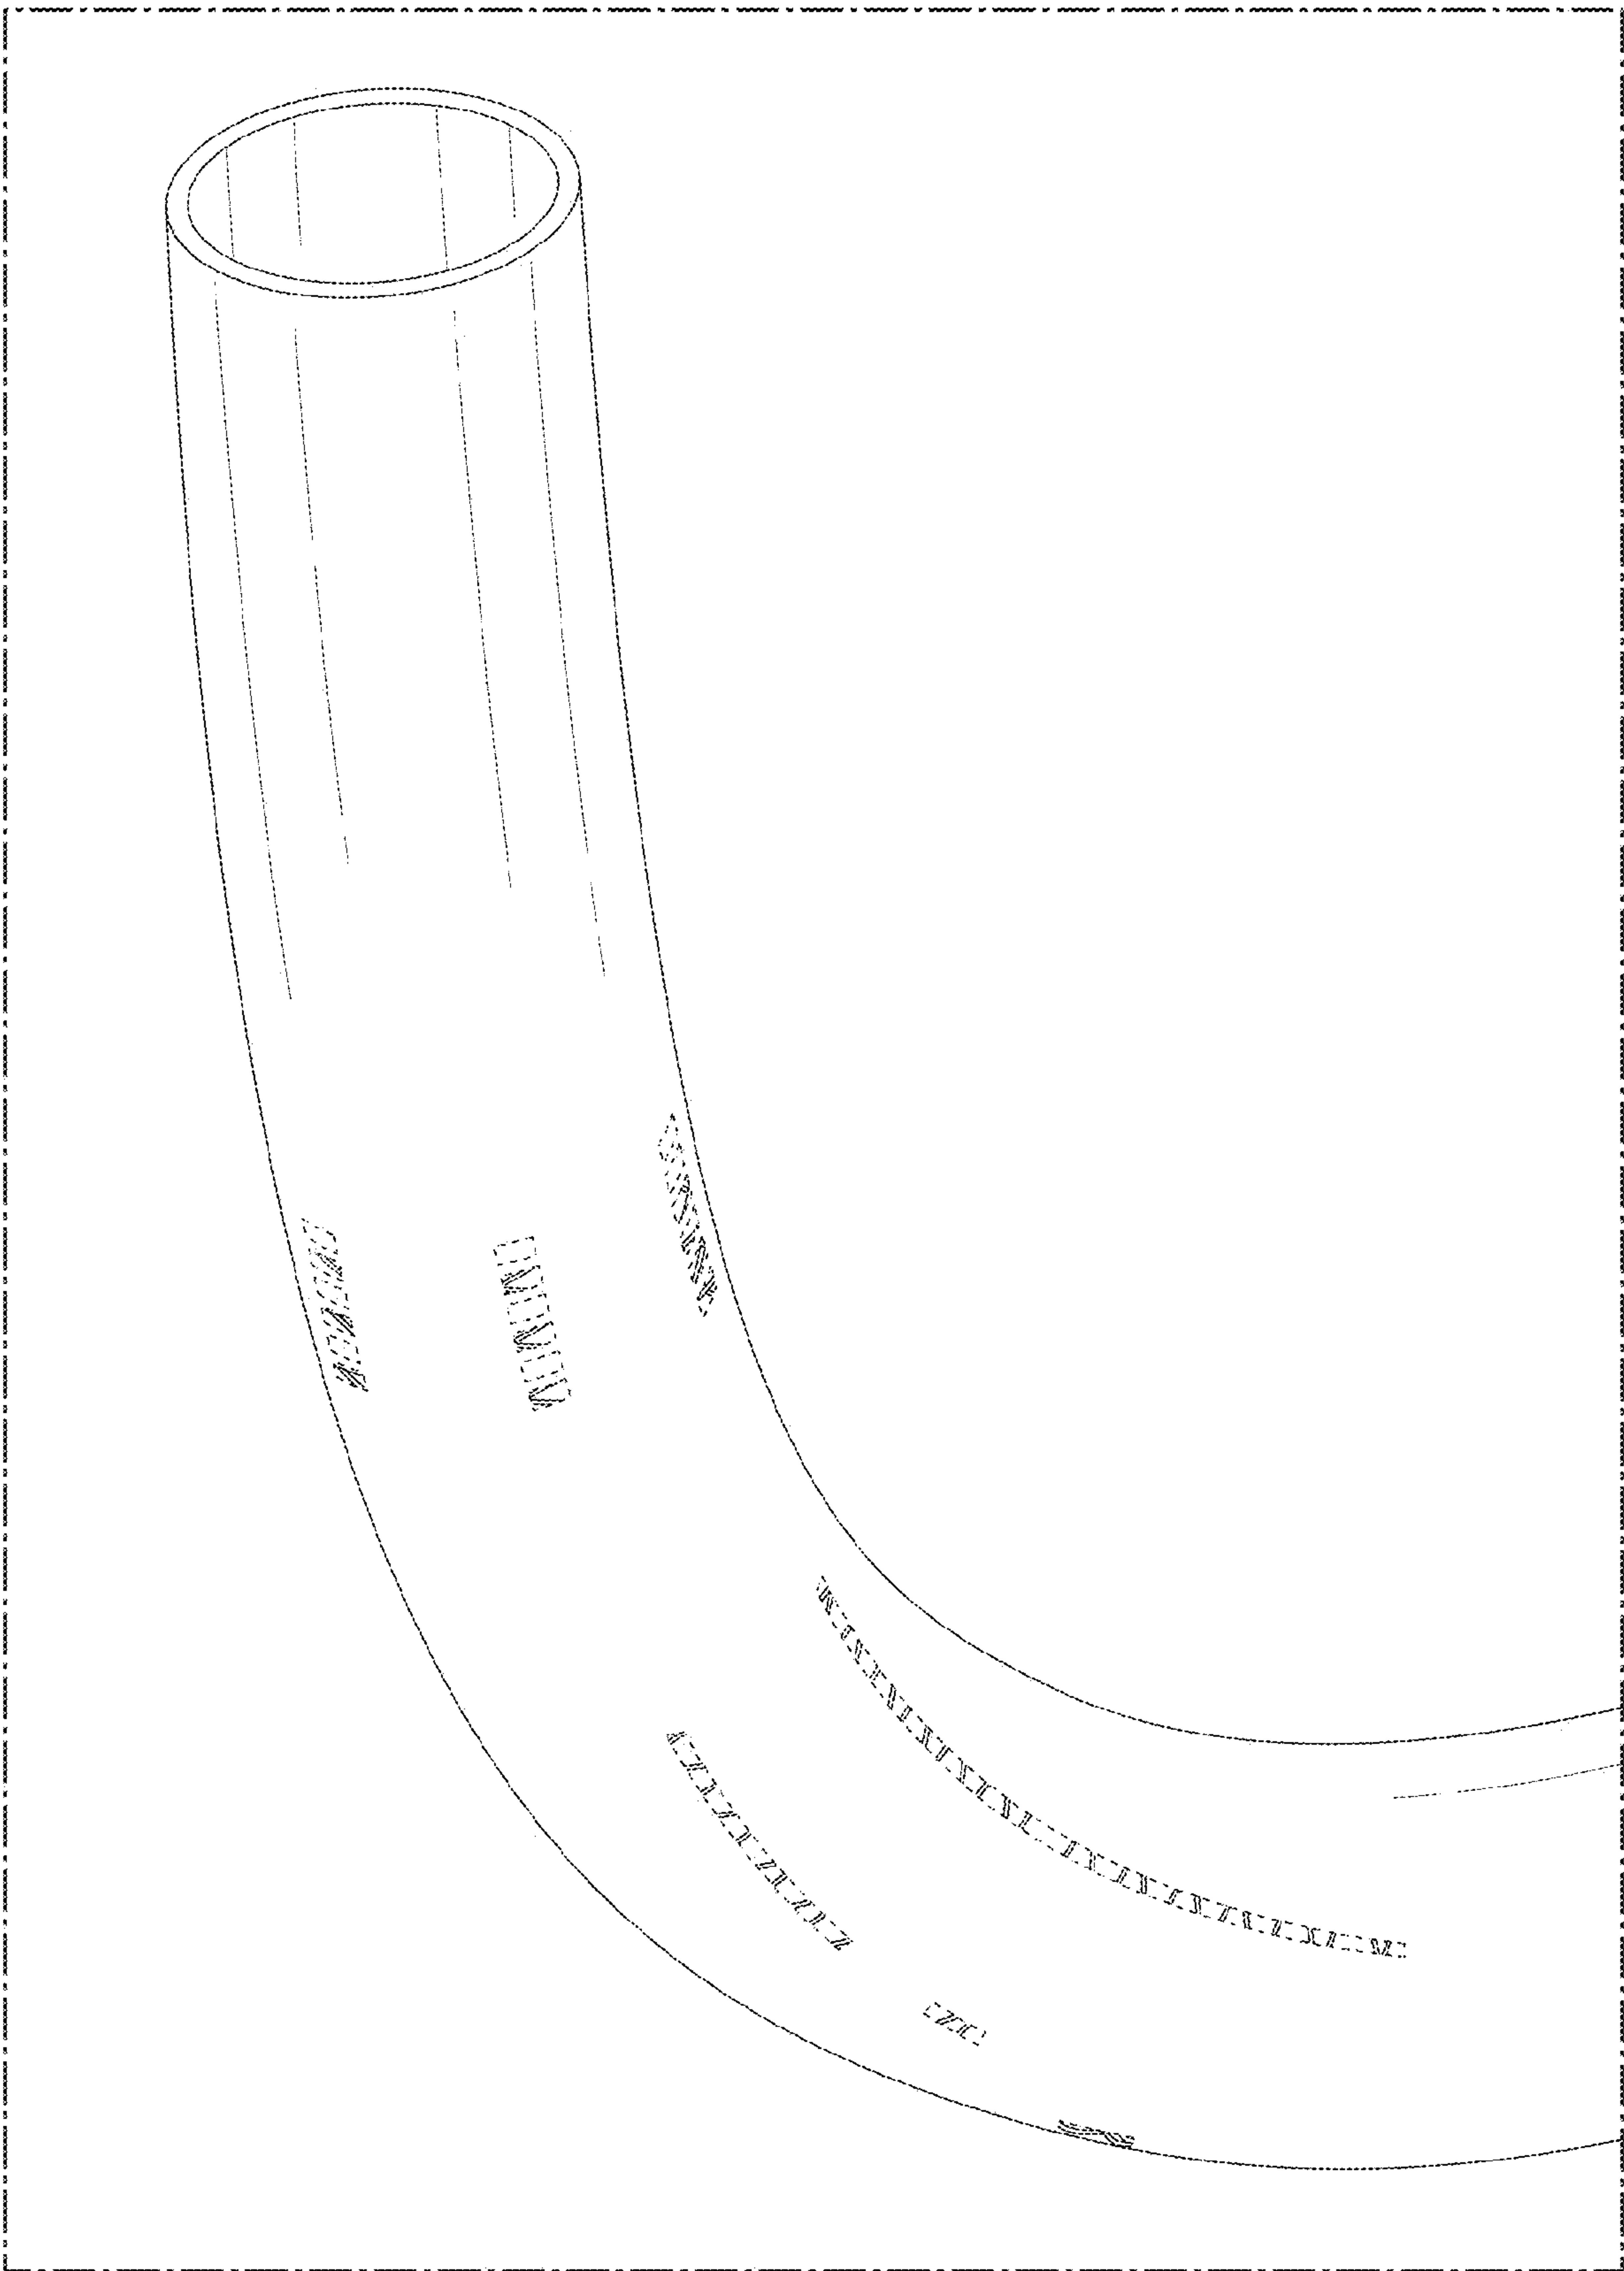


FIG. 8