



US0D1072272S

(12)

United States Design Patent

Luther et al.

(10)

Patent No.:

US D1,072,272 S

(45)

Date of Patent:

** Apr. 22, 2025

(54) ELECTROPORATION DEVICE

(71) Applicant: MaxCyte, Inc., Rockville, MD (US)

(72) Inventors: James William Luther, Milan (IT); Bertold Engler, Altensteig (DE); Andrea Besana, Seveso (IT); Thomas Alan Peach, Milan (IT)

(73) Assignee: Maxcyte, Inc., Rockville, MD (US)

(**) Term: 15 Years

(21) Appl. No.: 29/790,514

(22) Filed: Dec. 1, 2021

(51) LOC (15) Cl. 24-99

(52) U.S. Cl. USPC D24/233

(58) Field of Classification Search USPC D24/216, 222, 224, 225, 226, 227, 231, D24/232, 233 CPC .. B01D 57/02; C07K 1/26; C07K 1/24; B01L 3/0268; B01L 3/0275; B01L 3/5085; B01L 3/502707; B01L 9/52; G01N 27/447; G01N 27/44704; G01N 27/44756 See application file for complete search history.

(56) References Cited

U.S. PATENT DOCUMENTS

D430,304 S	*	8/2000	Oonuma	D24/232
D537,951 S	*	3/2007	Okamoto	D24/233
D546,761 S		7/2007	Schnackenberg	
D552,241 S		10/2007	Bromley et al.	
D567,761 S		4/2008	Waler et al.	
D574,771 S		8/2008	Flanigan et al.	
D620,886 S		8/2010	Flattinger et al.	
D621,523 S	*	8/2010	Onuma	D24/234
D693,928 S		11/2013	Chung et al.	
D712,352 S		9/2014	George et al.	
D712,833 S		9/2014	George et al.	
D728,121 S		4/2015	Cook et al.	

9,020,605 B2 4/2015 McCluskey et al.

D743,035 S 11/2015 Uozumi et al.

D759,250 S 6/2016 Engler

(Continued)

FOREIGN PATENT DOCUMENTS

CN 308419030 * 1/2024

CN 308441621 * 1/2024

(Continued)

OTHER PUBLICATIONS

“MaxCyte Inc: About Maxcyte’s Culture.” Found online Jan. 1, 2024 at youtube.com. Reference dated Jun. 27, 2023. Retrieved from https://www.youtube.com/watch?v=otJAn2r_Ri0.*

(Continued)

Primary Examiner — Kendra Leslie Hamilton

Assistant Examiner — Elizabeth S Struble

(74) Attorney, Agent, or Firm — Finnegan, Henderson, Farabow, Garrett & Dunner LLP

(57)


CLAIM

The ornamental design for an electroporation device, as shown and described.

DESCRIPTION

FIG. 1 is a front, top, right perspective view of an electroporation device, showing the new design; FIG. 2 is a rear, bottom, left perspective thereof; FIG. 3 is a front elevation view thereof; FIG. 4 is a rear elevation view thereof; FIG. 5 is a left side view thereof; FIG. 6 is a right side view thereof; FIG. 7 is a top plan view thereof; and, FIG. 8 is a bottom plan view thereof. The broken lines of even length depict portions of the electroporation device that form no part of the claimed design.

1 Claim, 8 Drawing Sheets

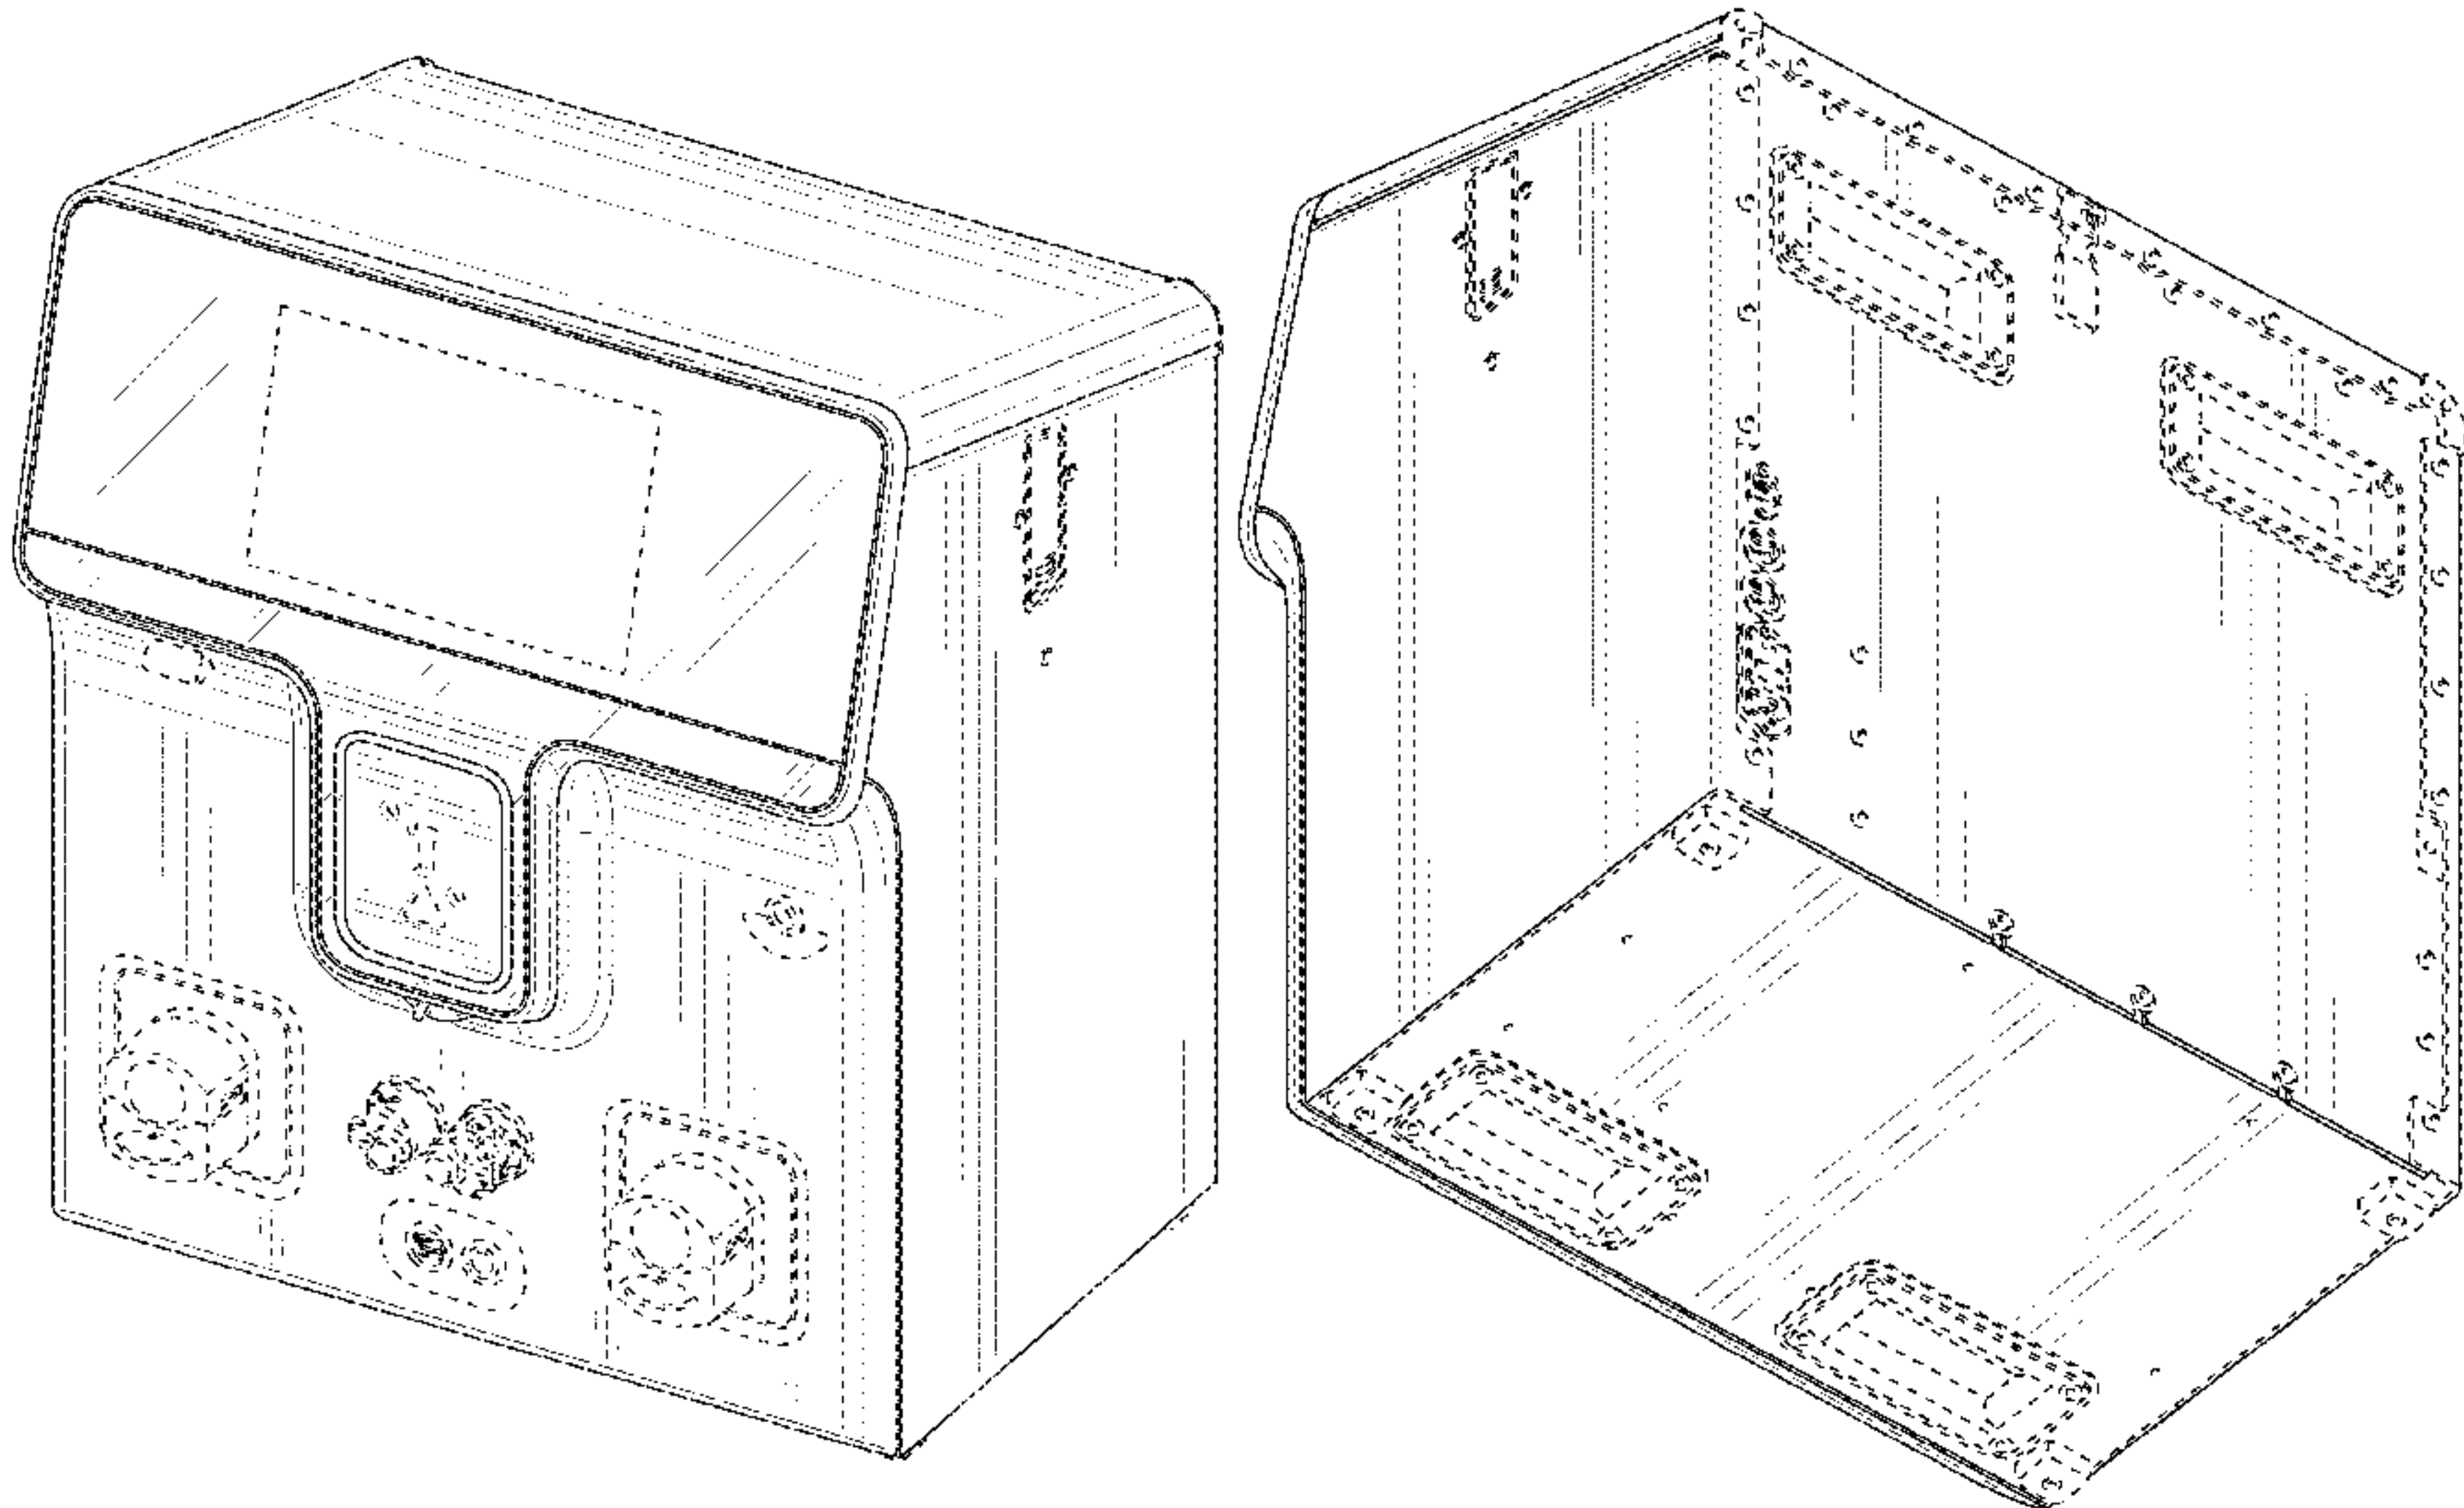

(56)

References Cited

OTHER PUBLICATIONS

U.S. PATENT DOCUMENTS

D821,601 S 6/2018 Henderson
D827,859 S * 9/2018 Mathers D24/232
D860,941 S 9/2019 Wheeler
D888,985 S * 6/2020 Hsieh D24/232
D906,536 S * 12/2020 Kozono D24/216
D923,199 S 6/2021 Luther et al.
D923,200 S 6/2021 Luther et al.
D965,816 S * 10/2022 Luther D24/233
D982,181 S * 3/2023 Tanaka D24/232
D984,293 S * 4/2023 Tam D10/75
D997,380 S * 8/2023 Garrido D24/234
2011/0297545 A1 * 12/2011 Latham G01N 27/44782
204/464
2016/0175619 A1 6/2016 Lee et al.
2018/0221882 A1 * 8/2018 Roberts G01N 27/44704
2022/0099624 A1 * 3/2022 Chang G01N 27/44756

FOREIGN PATENT DOCUMENTS

GB 6259922 * 2/2023
KR 3010220570000 9/2019
KR 3011203820000 7/2021
KR 3011278620000 9/2021

“www.bostonind.com: Qiagen QIAcube Connect DNA/RNA/
Protein Purification.” Found online Jan. 31, 2024 at youtube.com.
Reference dated Nov. 2, 2023. Retrieved fromhttps://www.youtube.com/watch?v=wrHQ-HCH_8o.
*
“Scilogex: Fastgel Gel Imaging System.” Found online Jan. 31,
2024 at youtube.com. Reference dated Feb. 13, 2020. Retrieved
from <https://www.youtube.com/watch?v=-2ksrexZ3tg>.
*
“MaxCyte: Understanding Flow Electroporation.” Found online
Jan. 31, 2024 at youtube.com. Reference dated Jun. 27, 2023.
Retrieved from<https://www.youtube.com/watch?v=BXXCenQGVC0>.
*

* cited by examiner

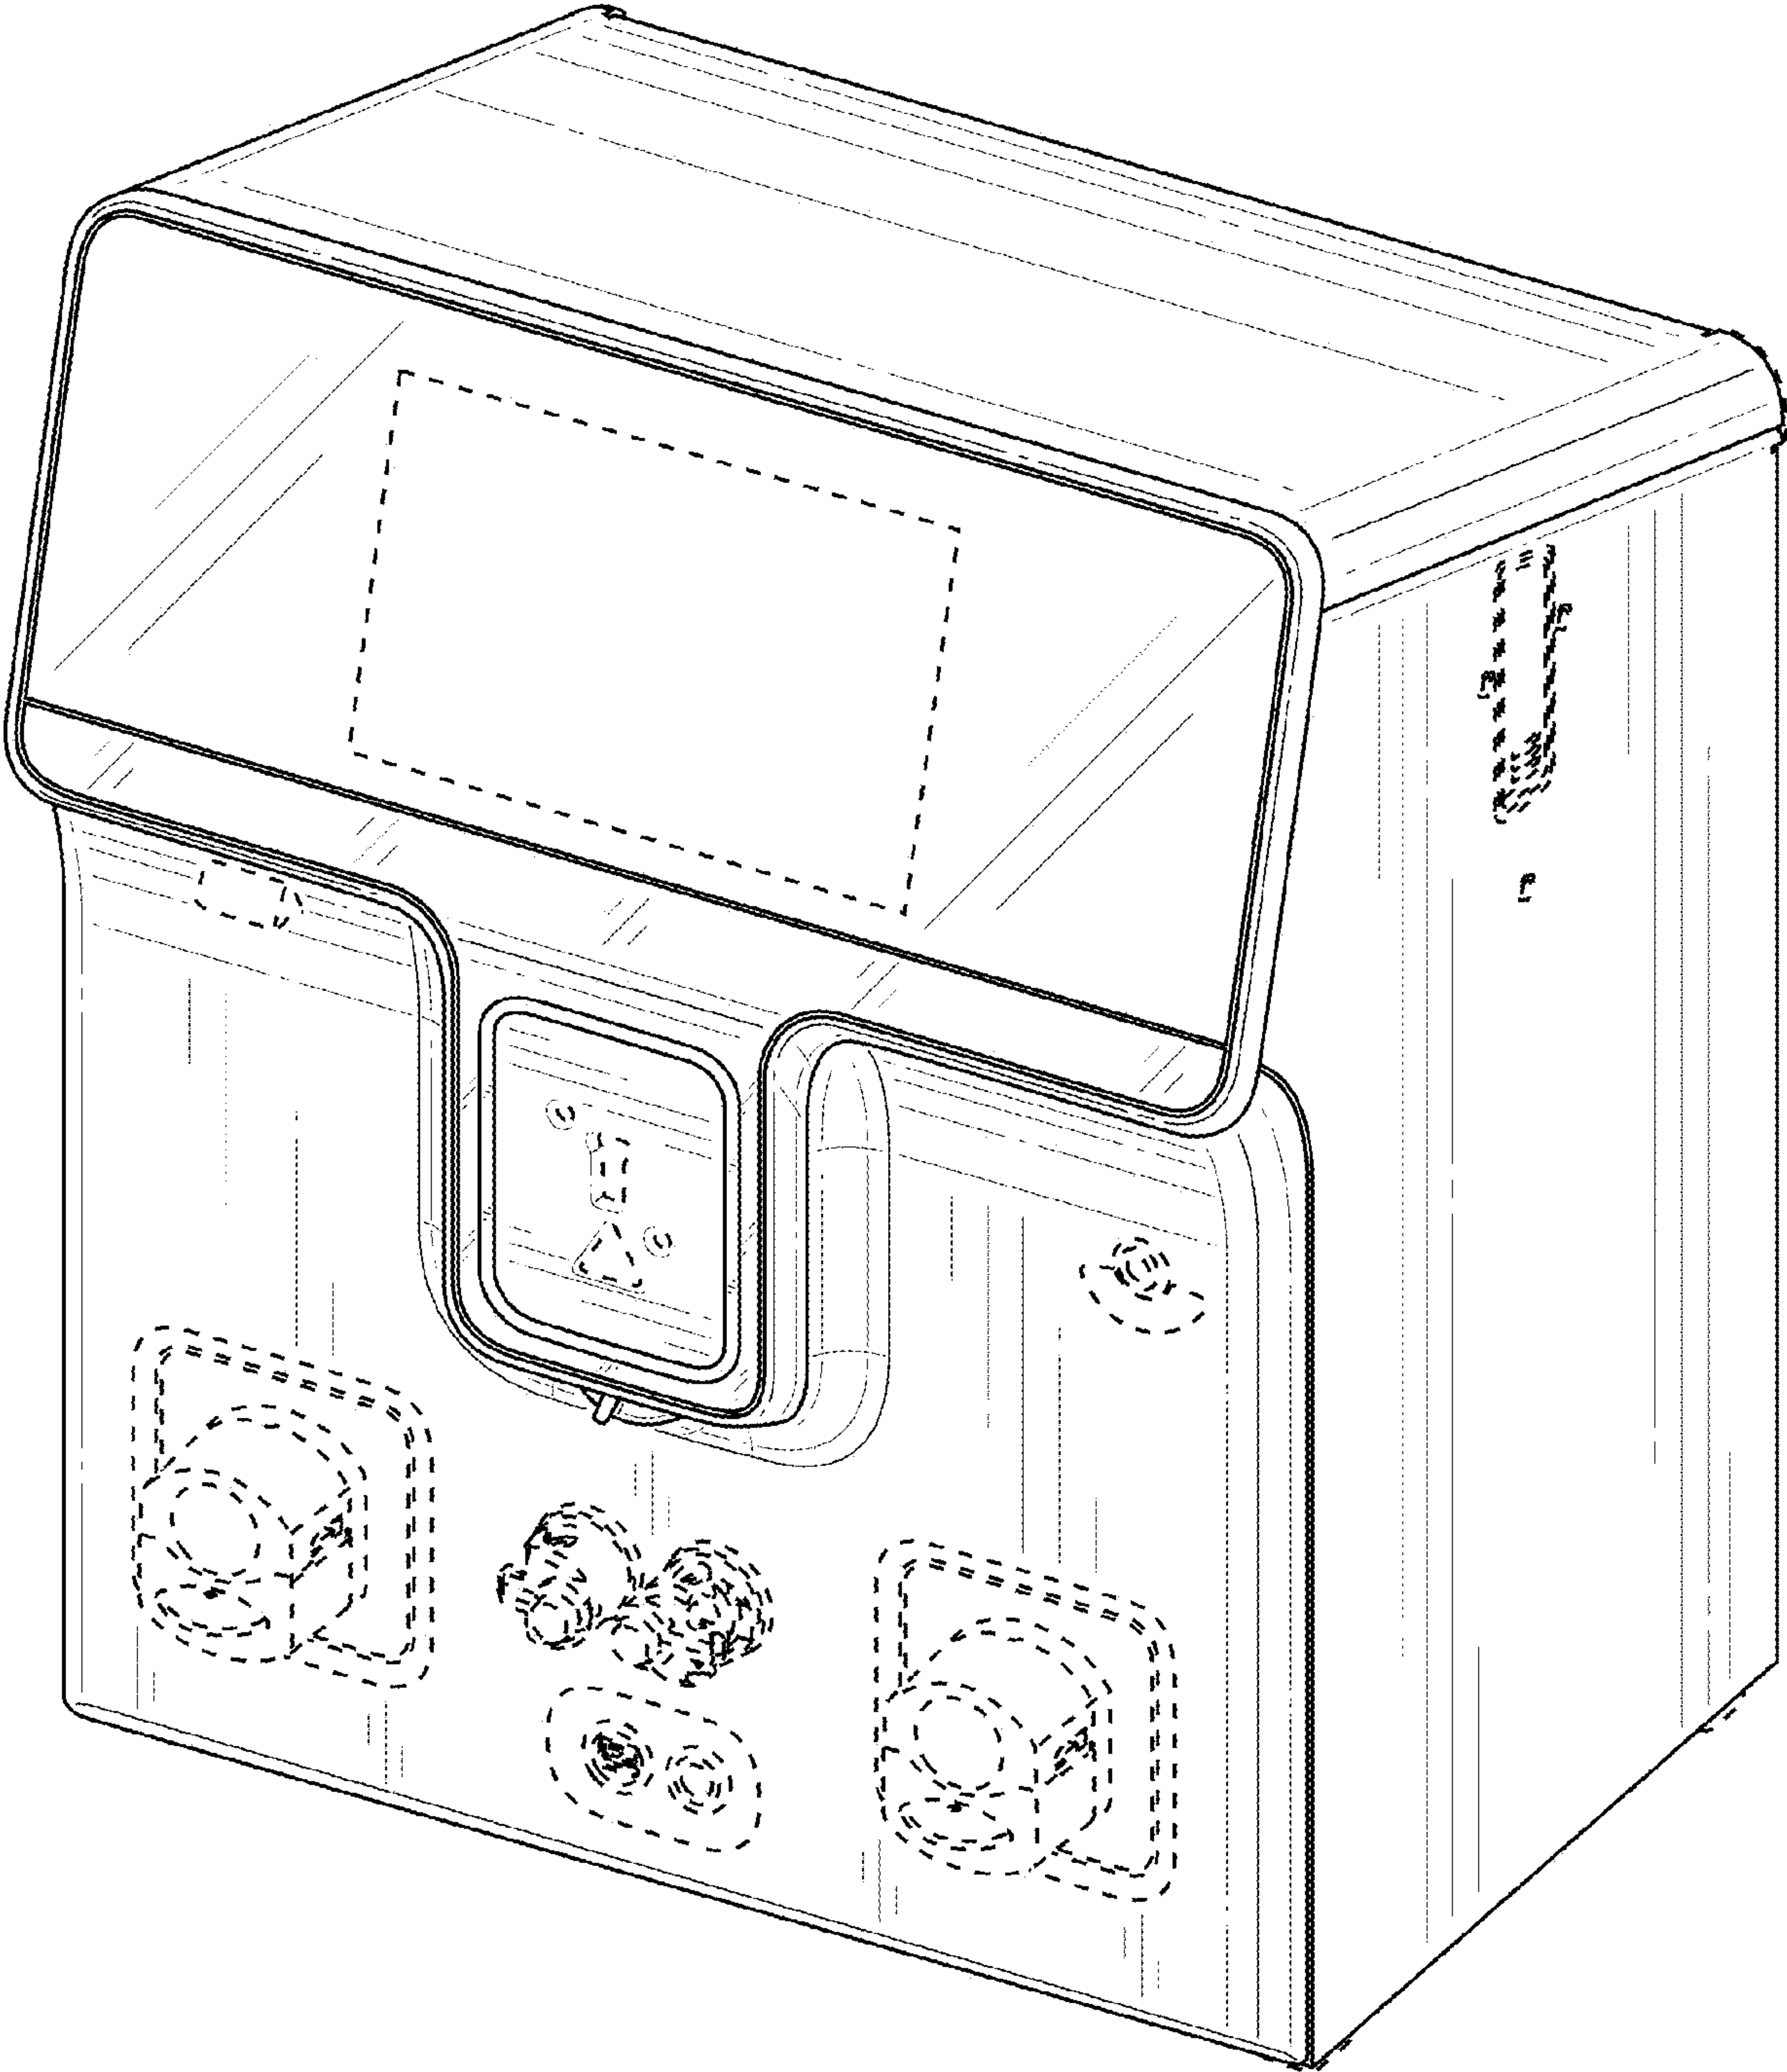


FIG. 1

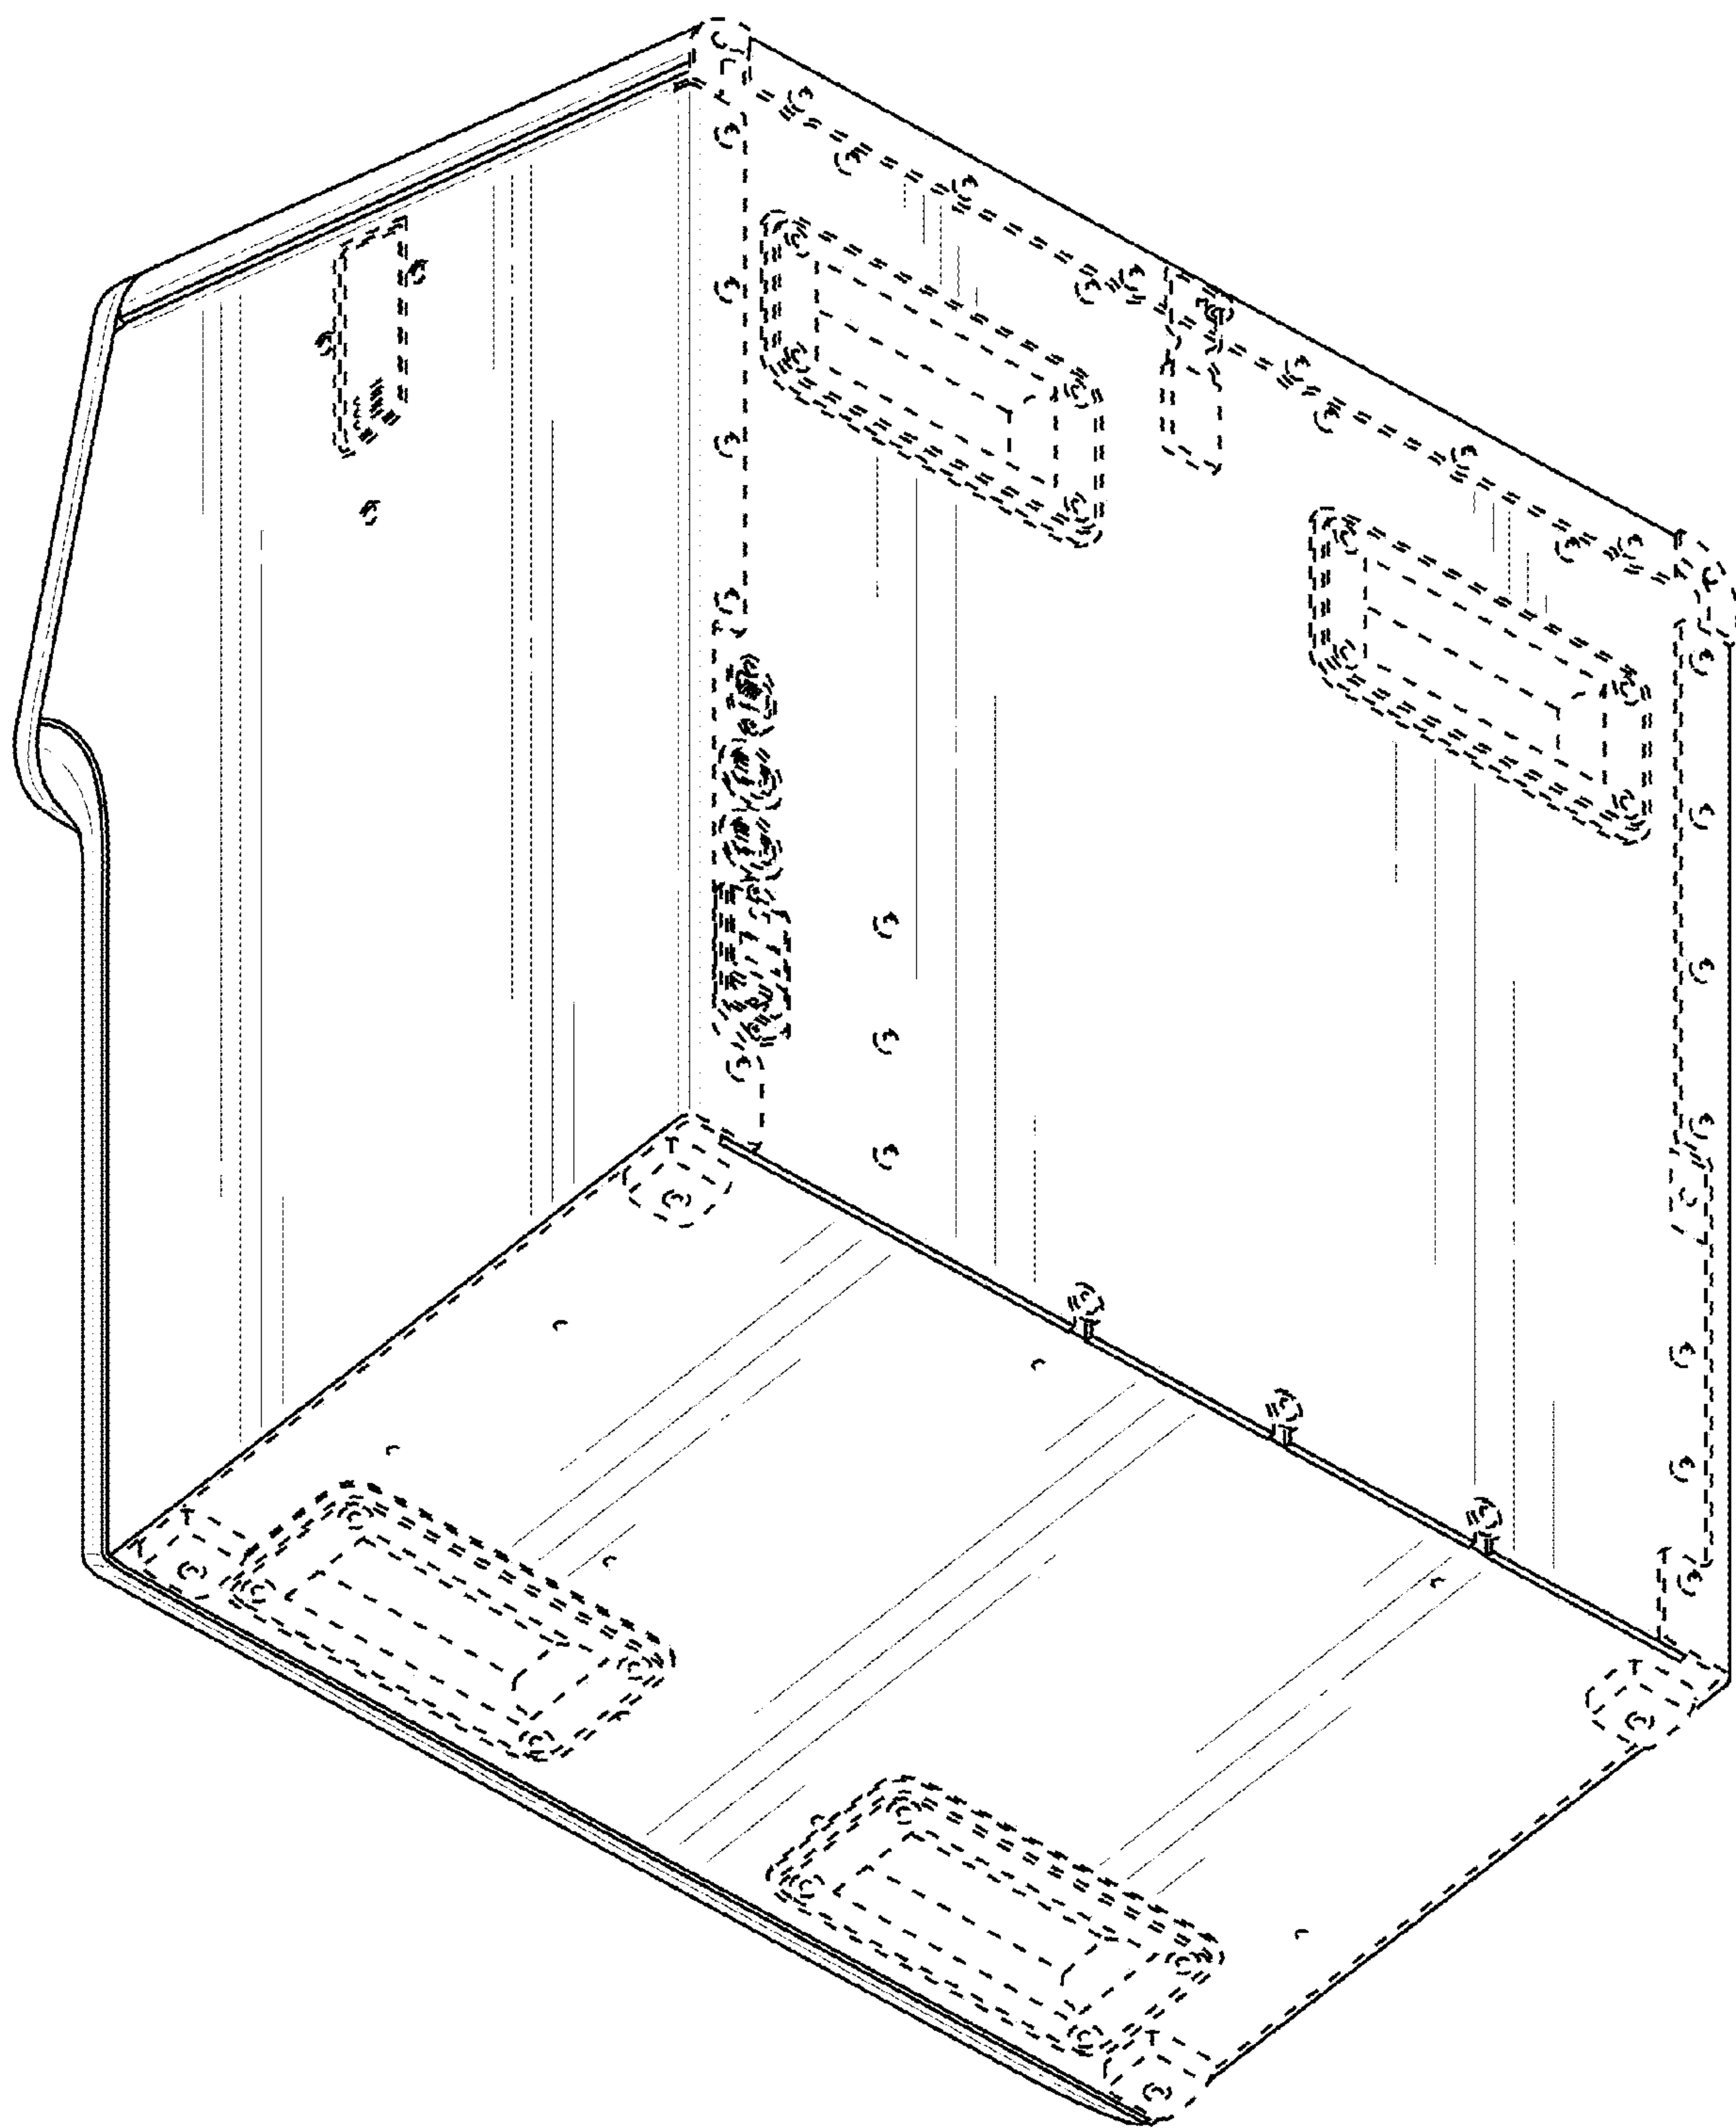


FIG. 2

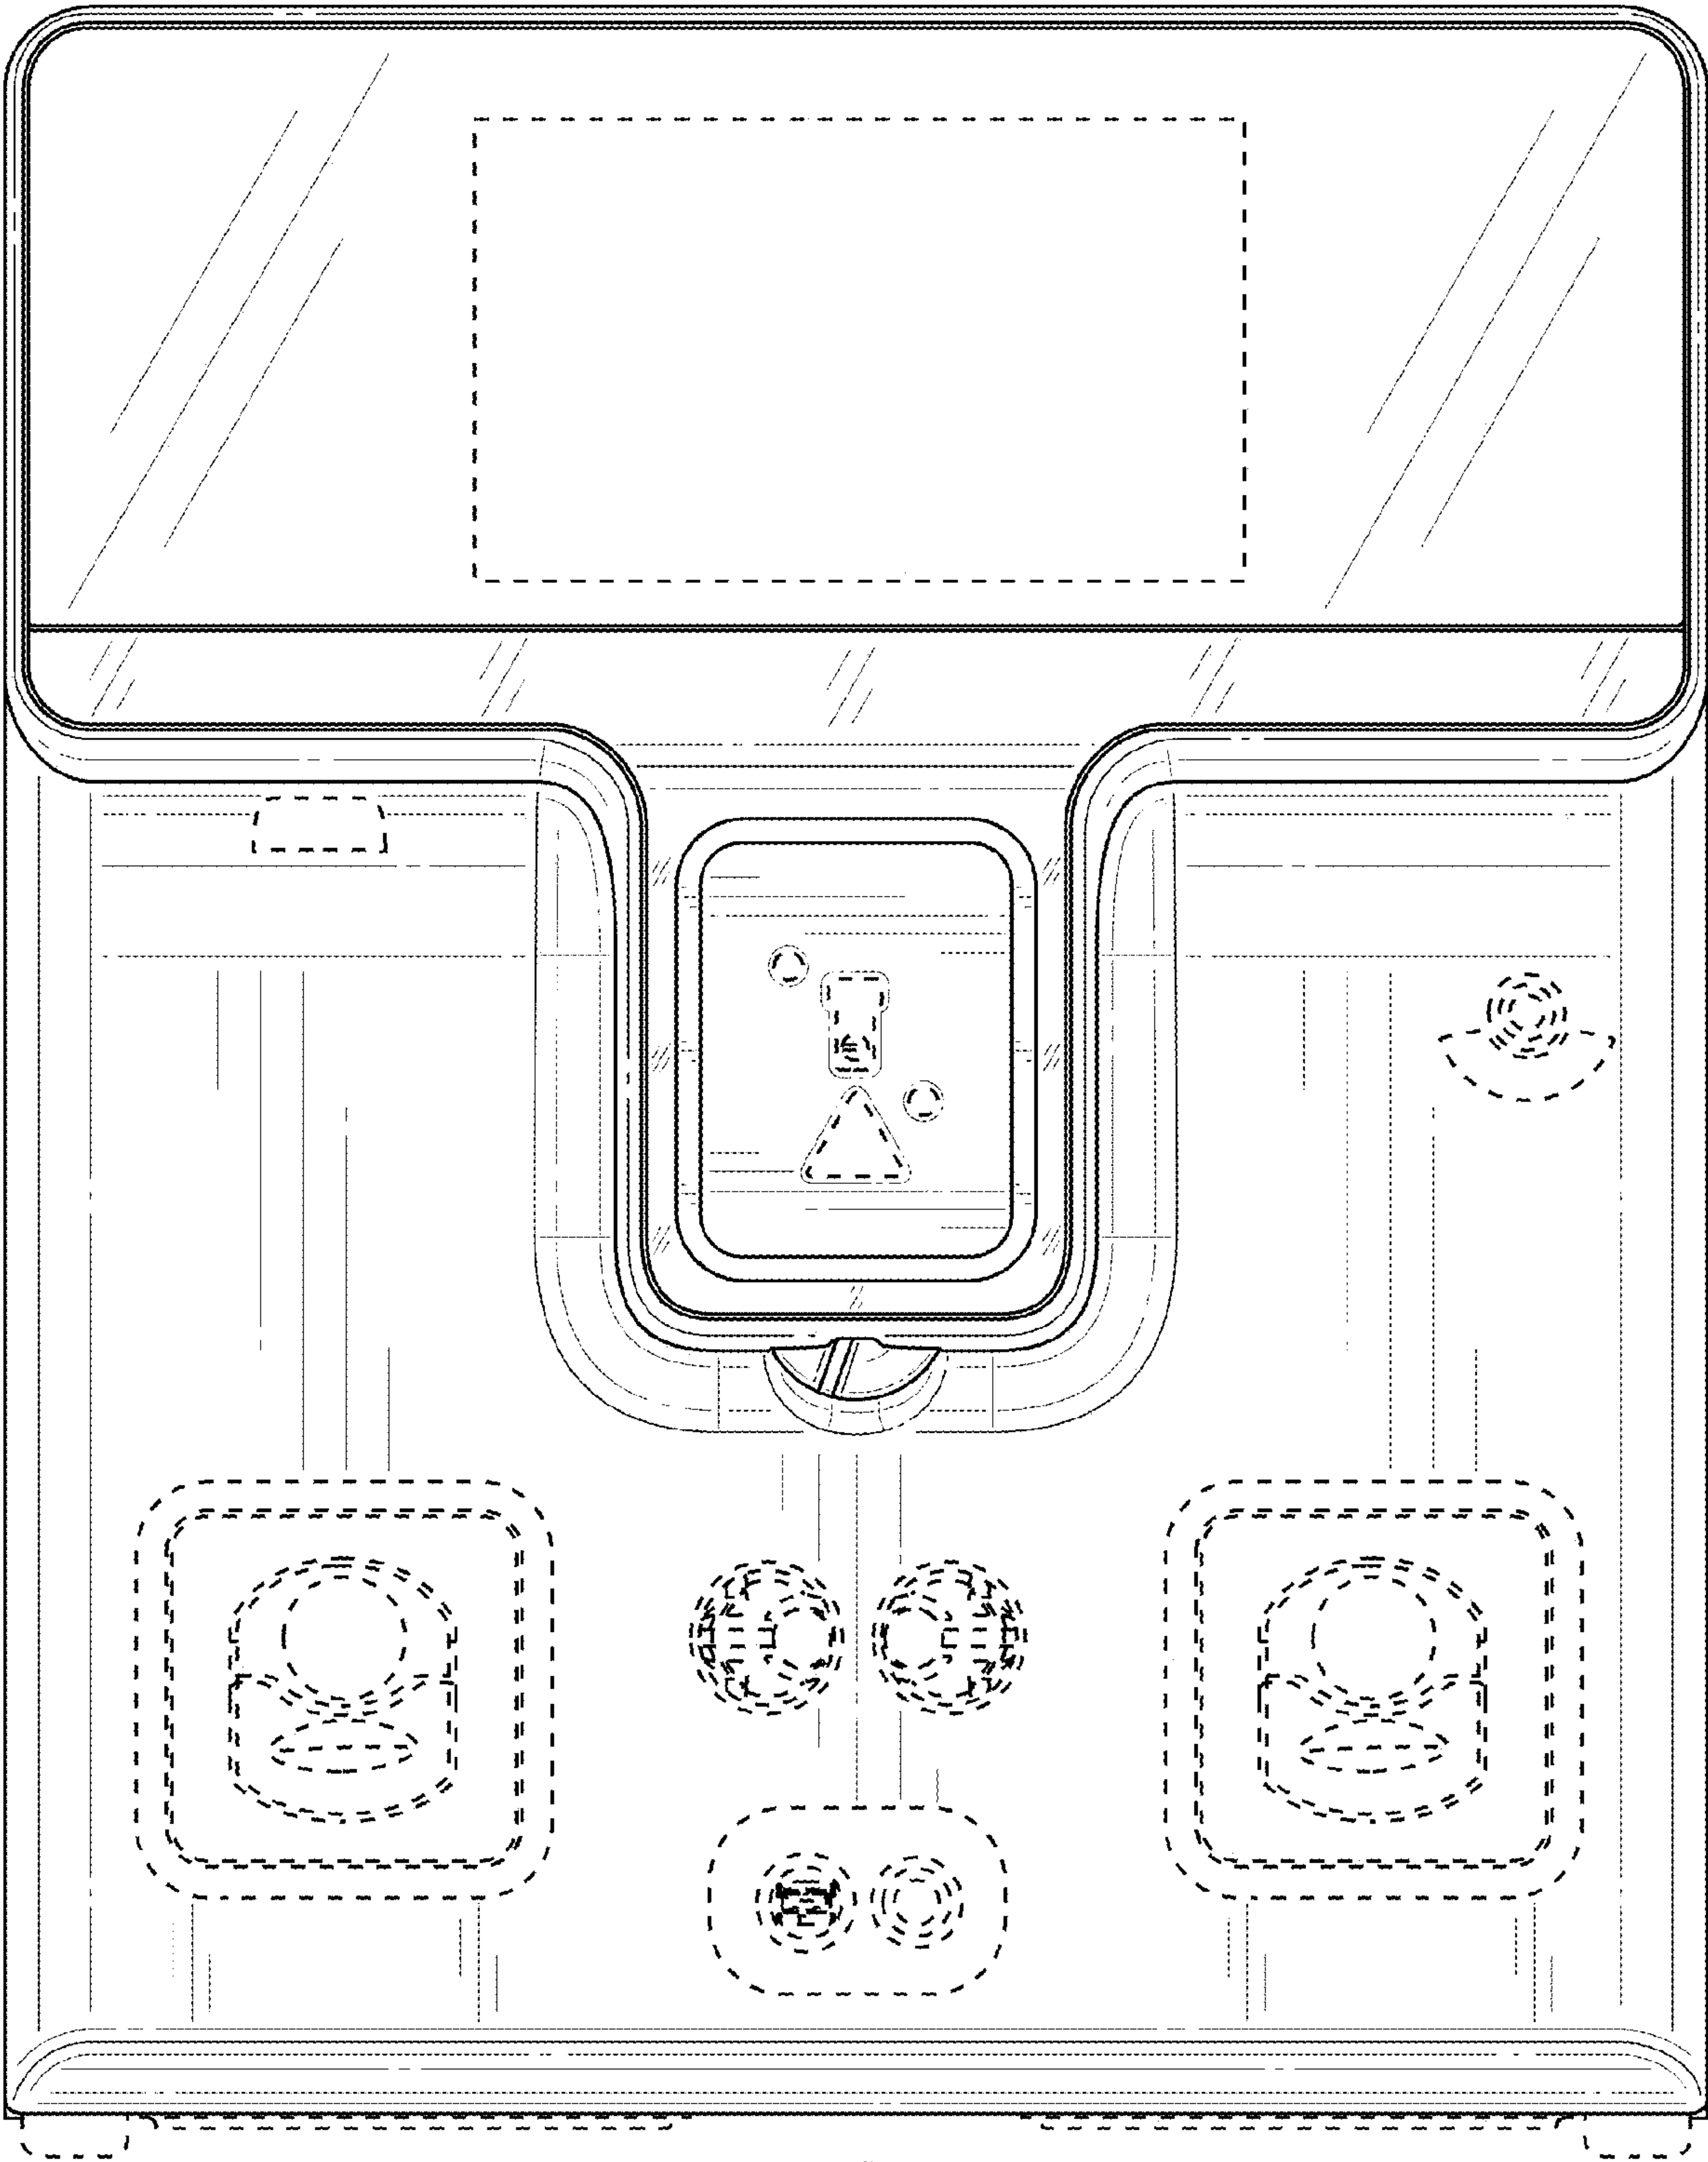


FIG. 3

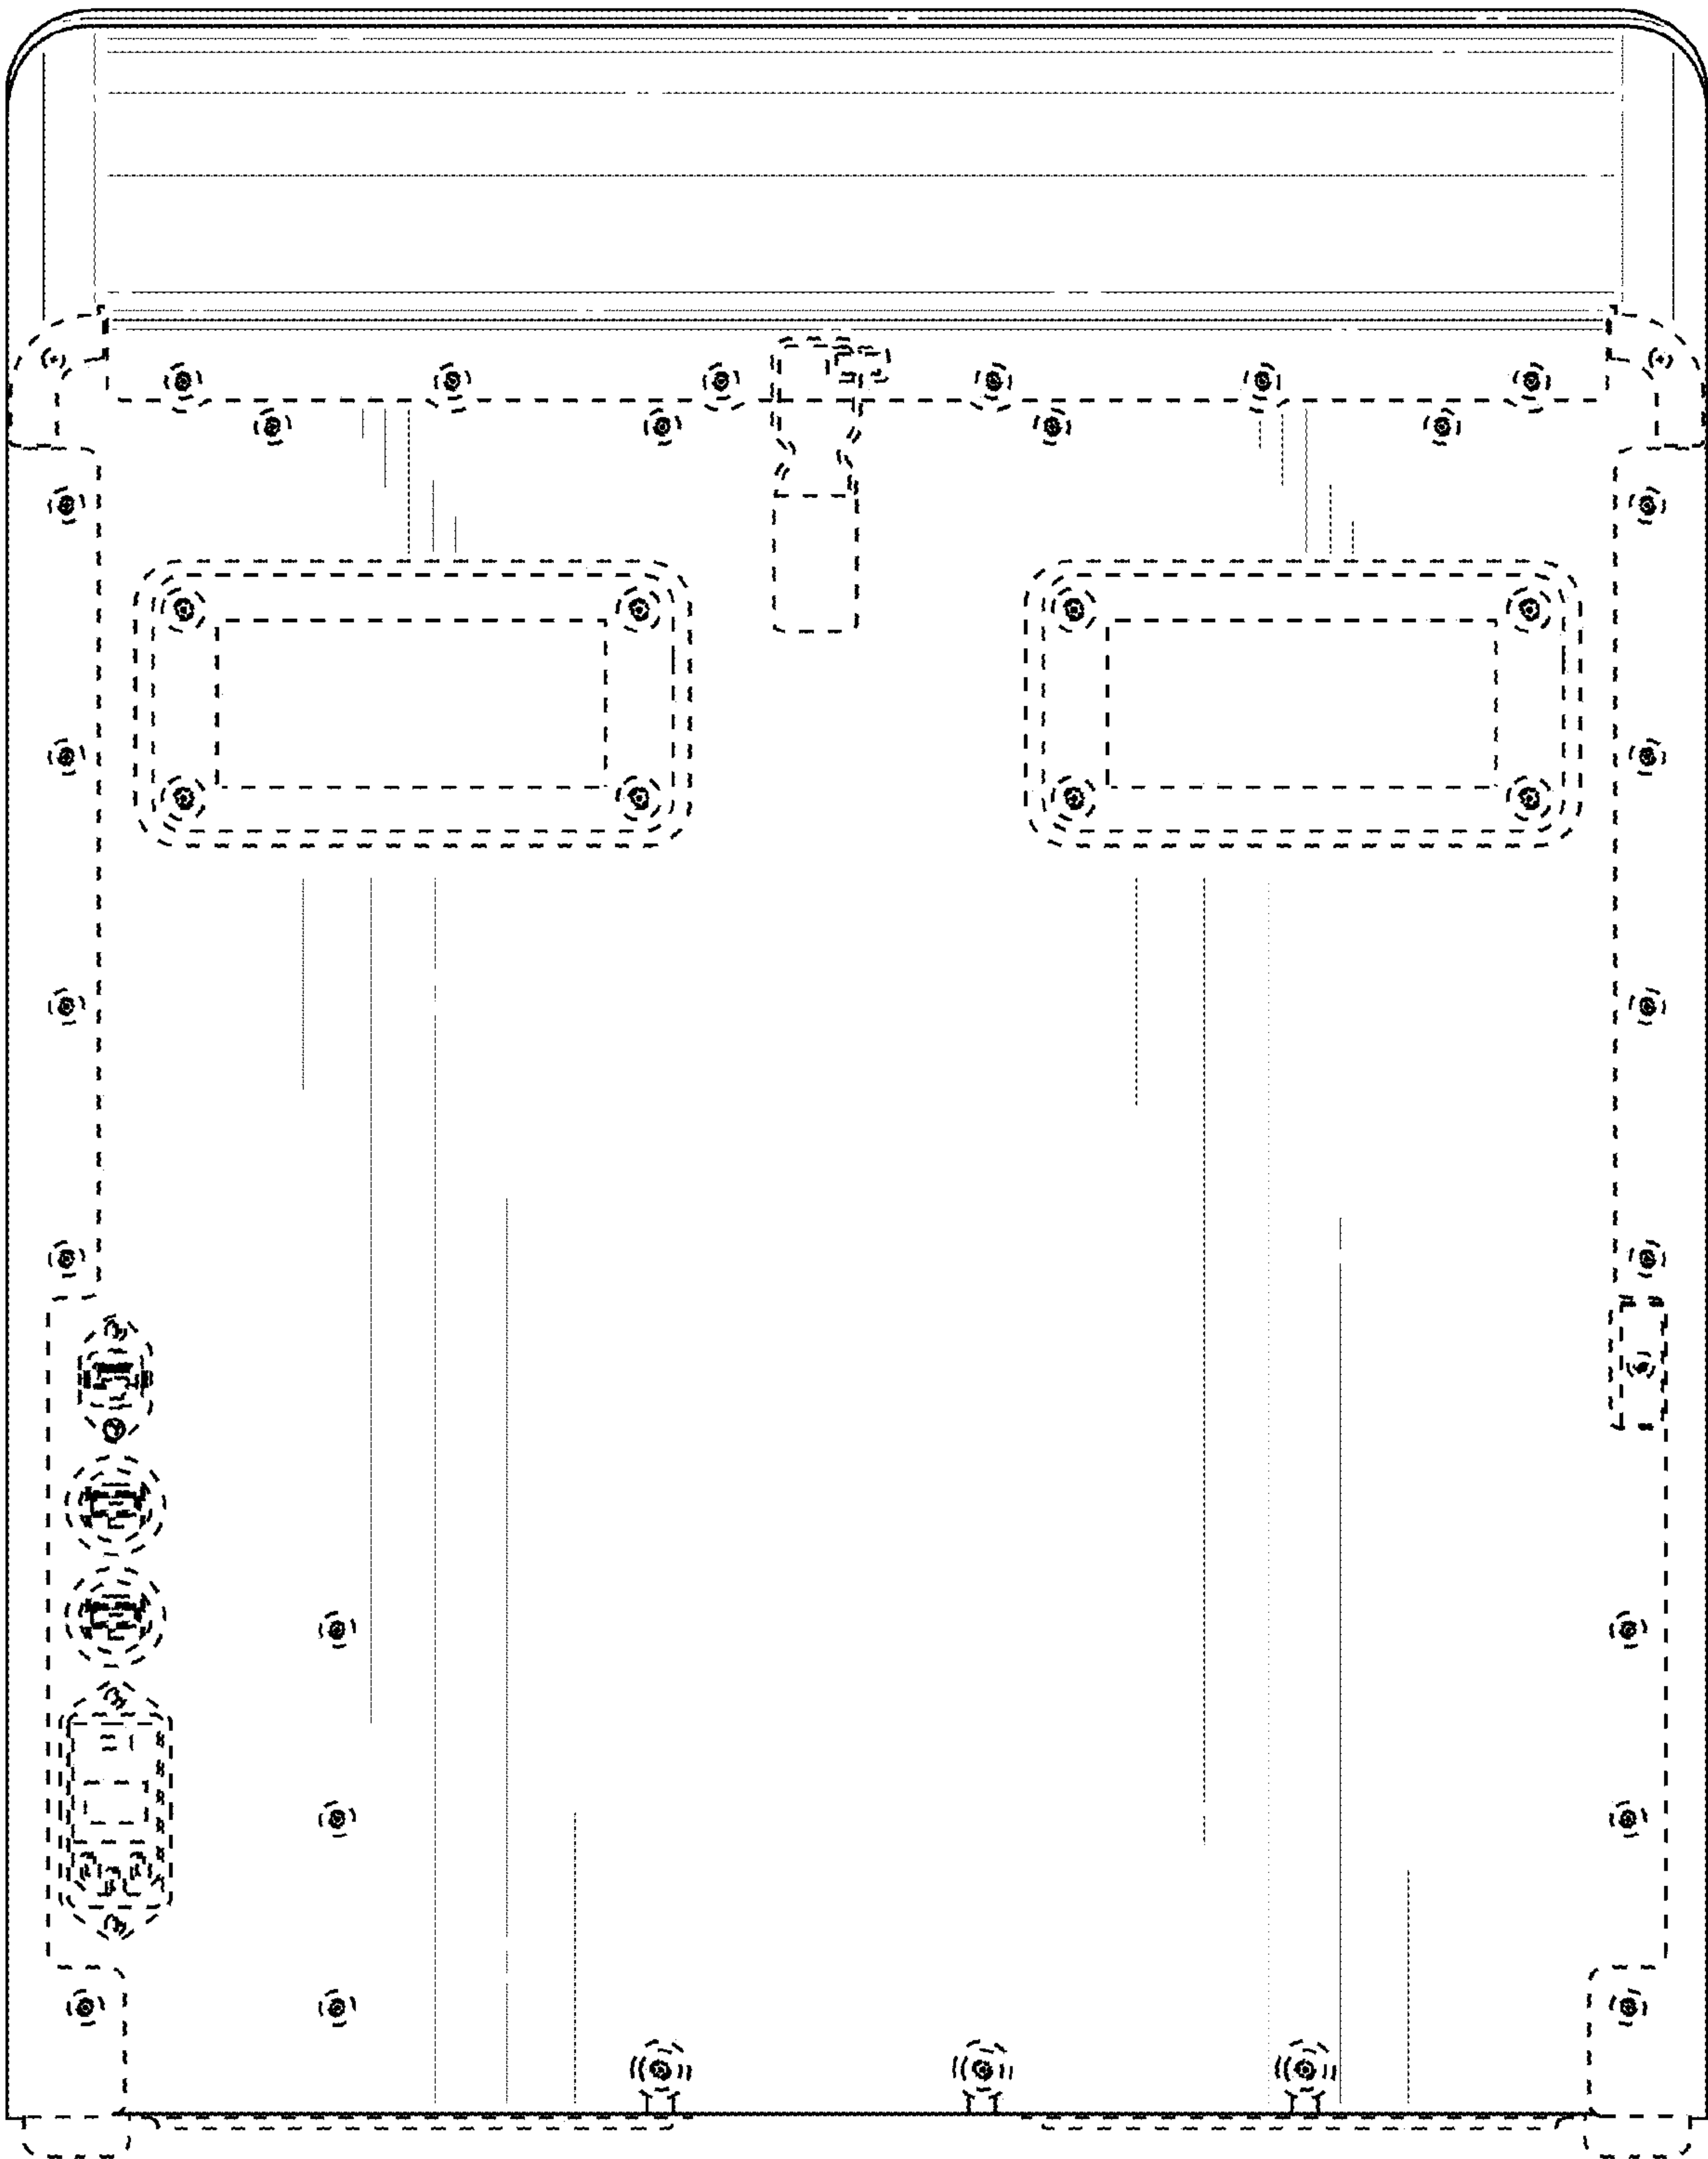


FIG. 4

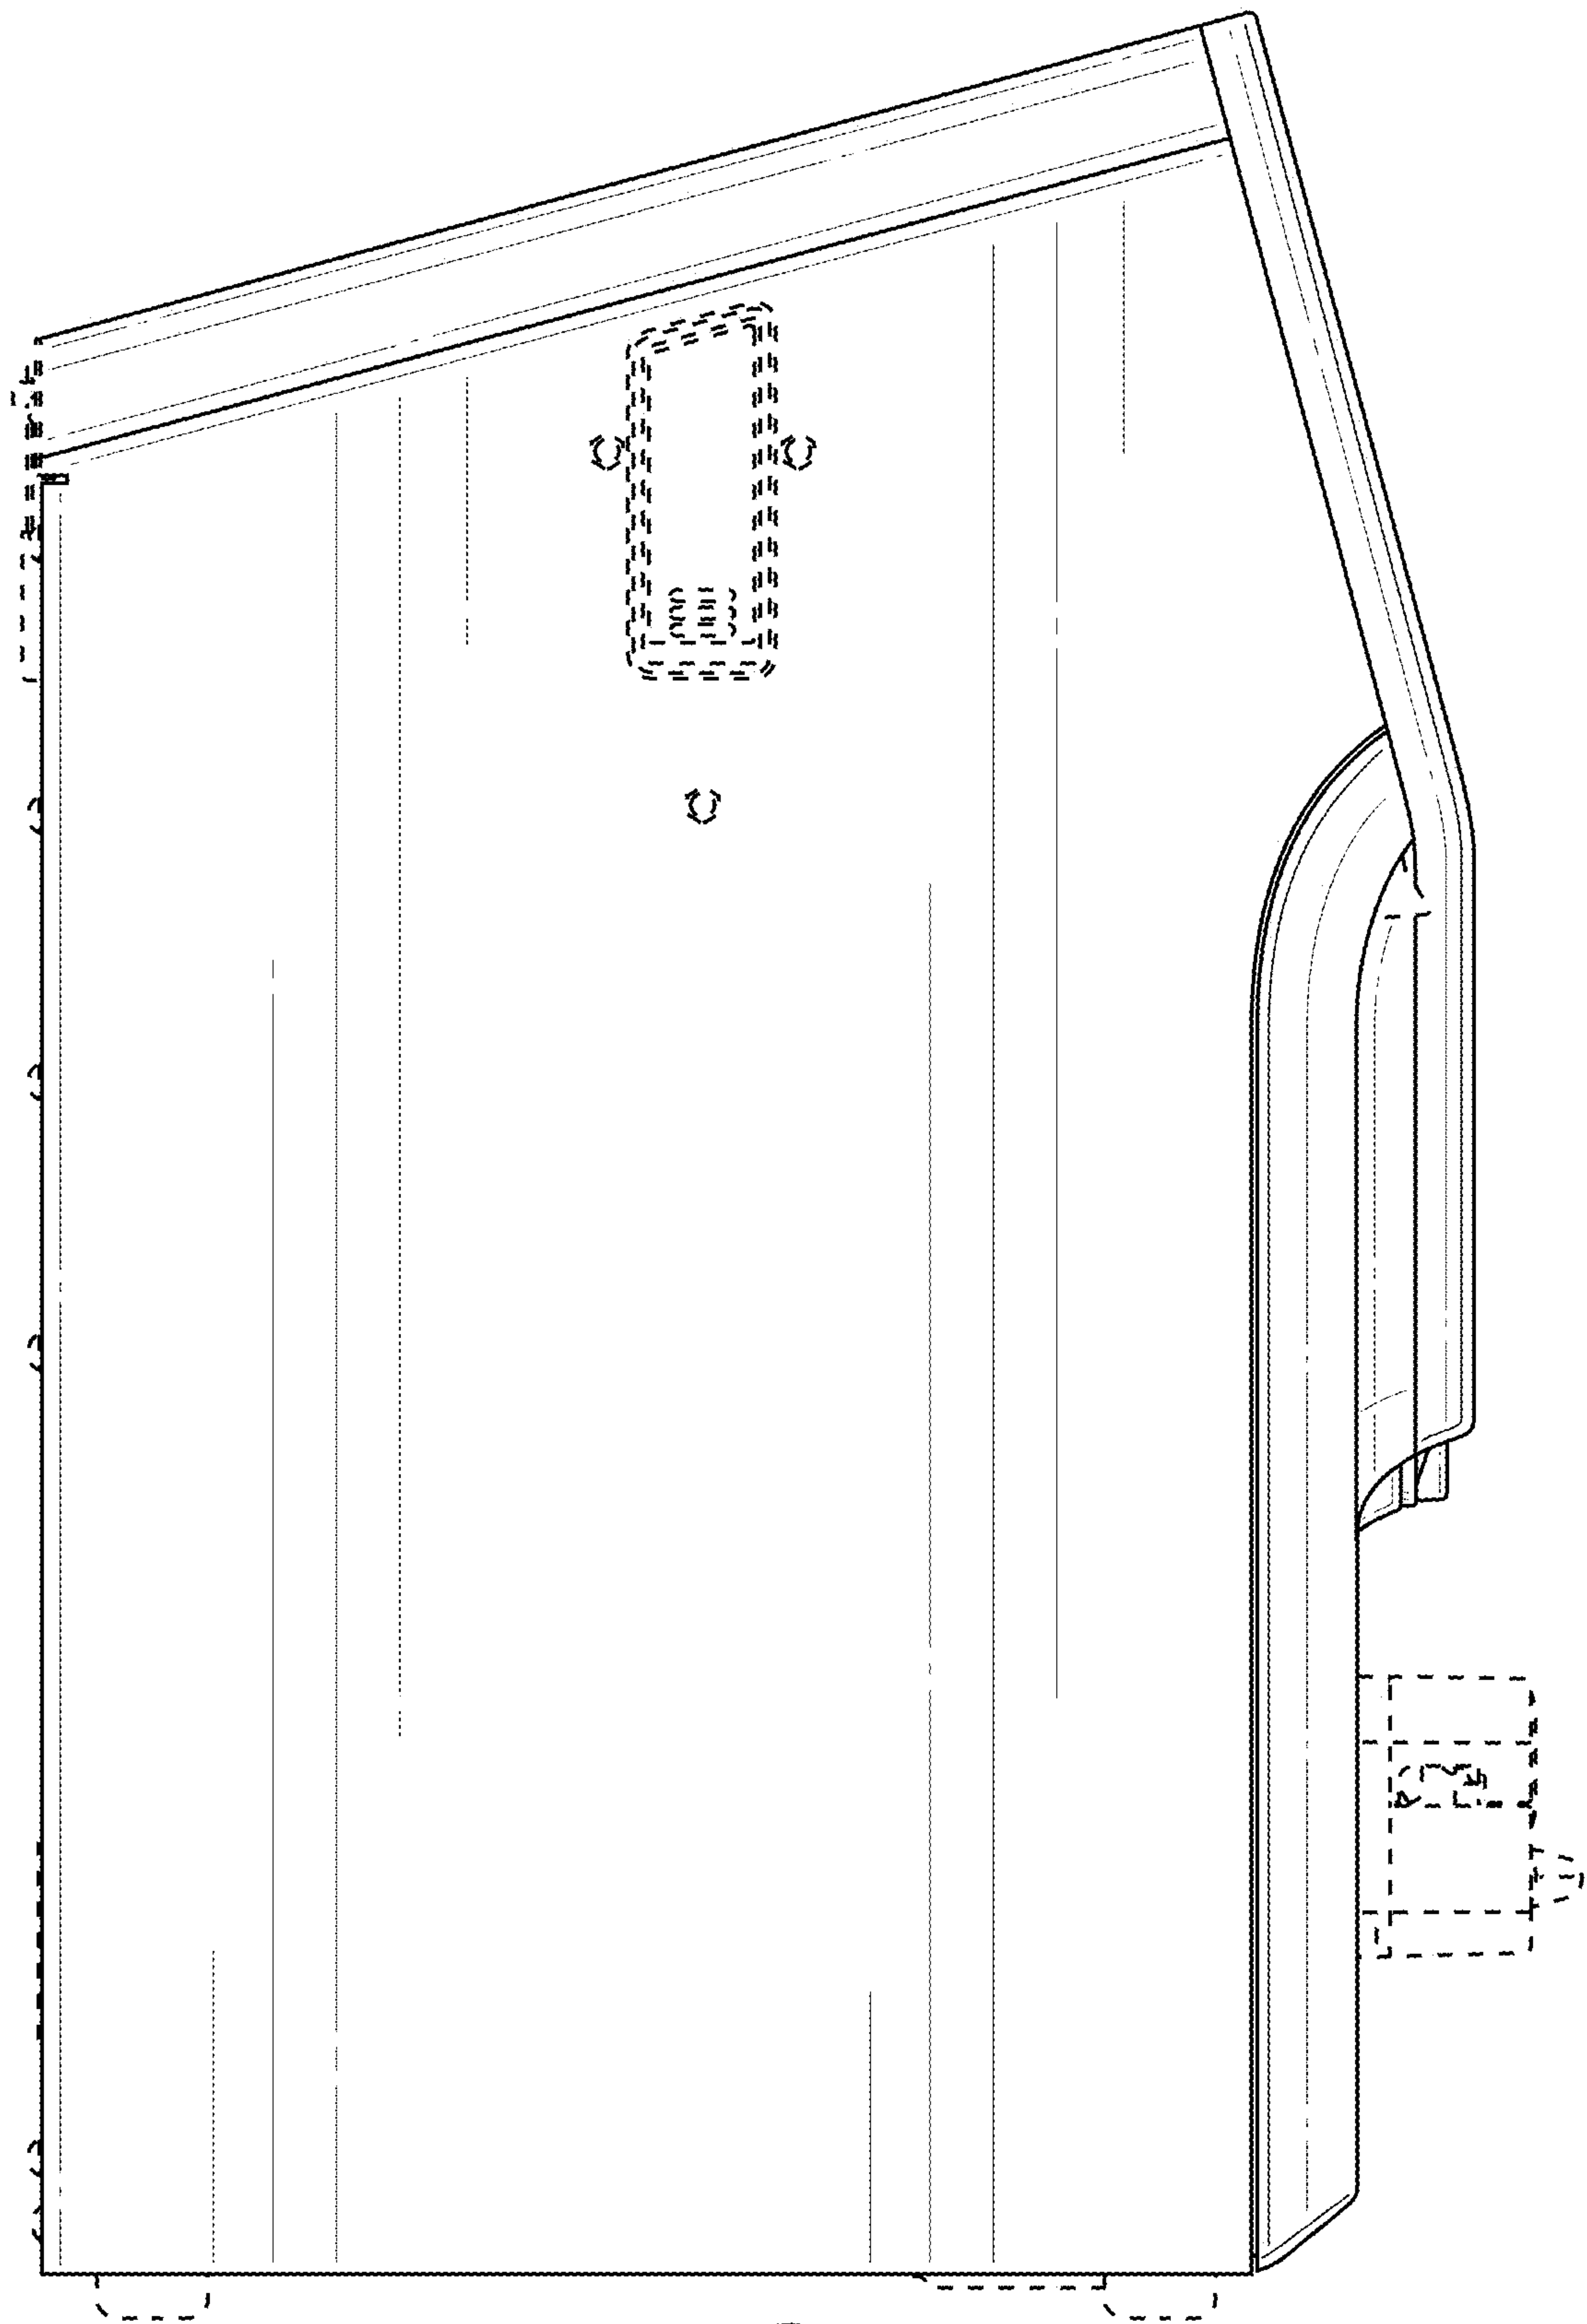


FIG. 5

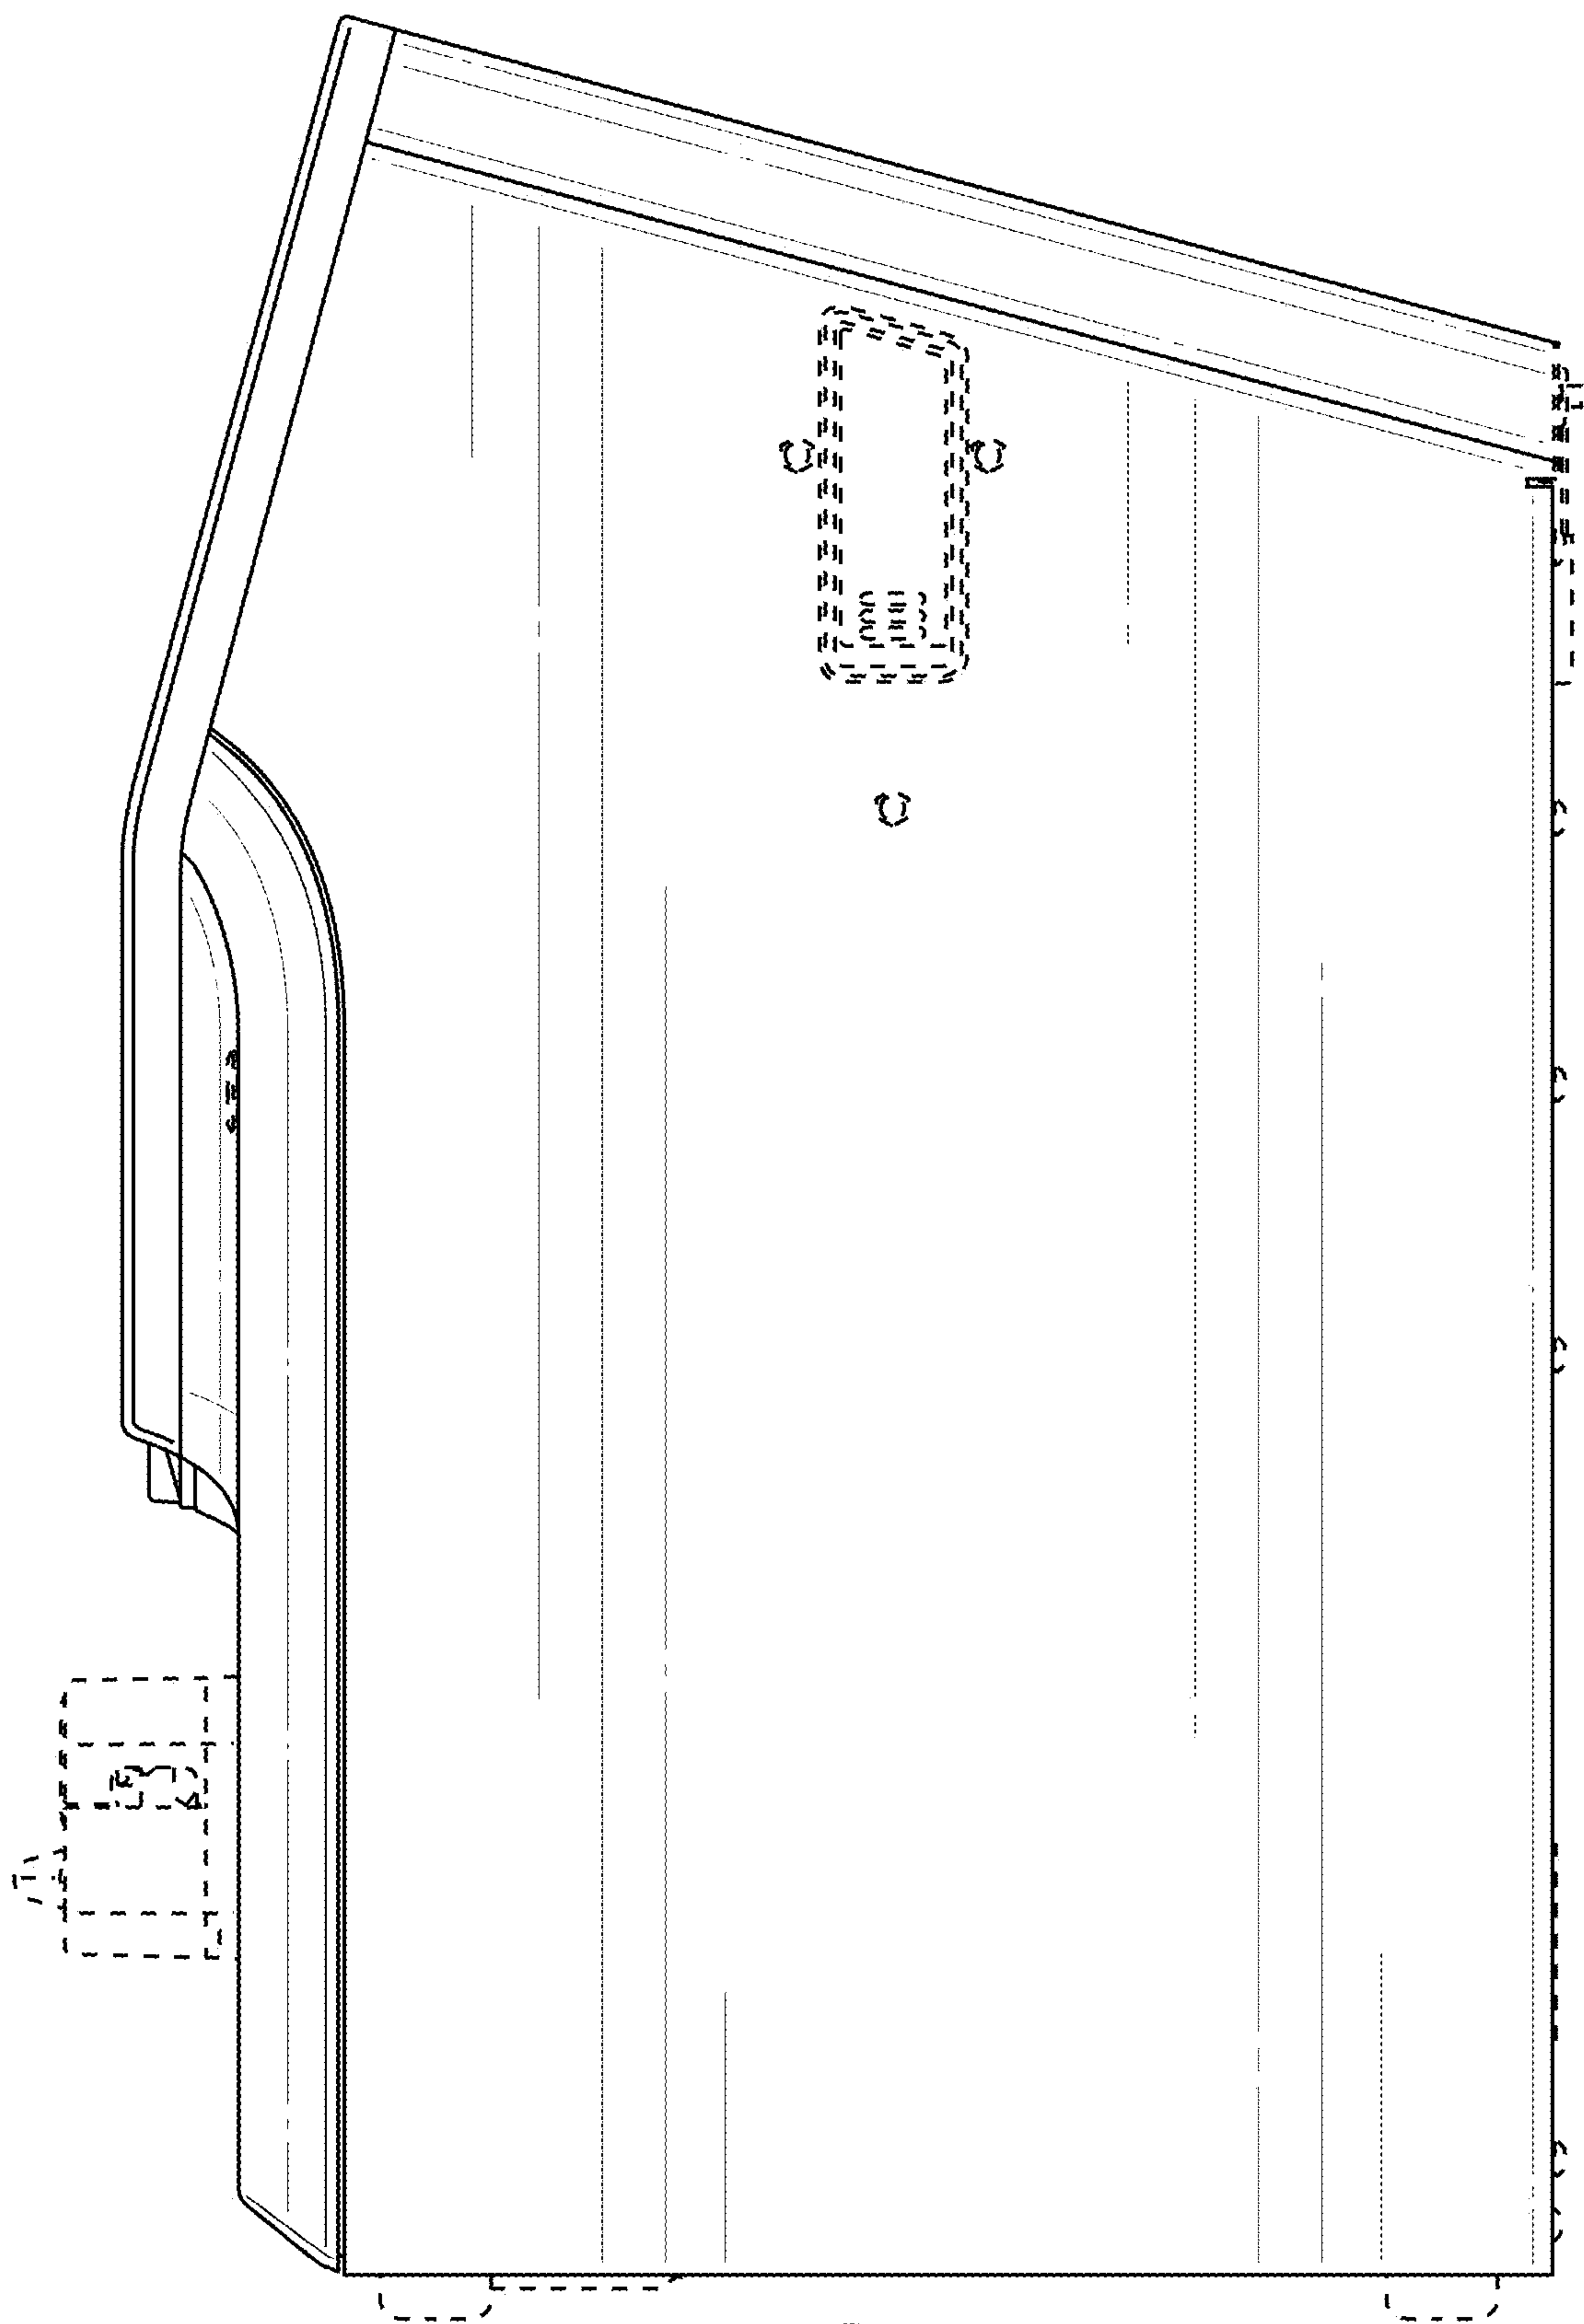


FIG. 6

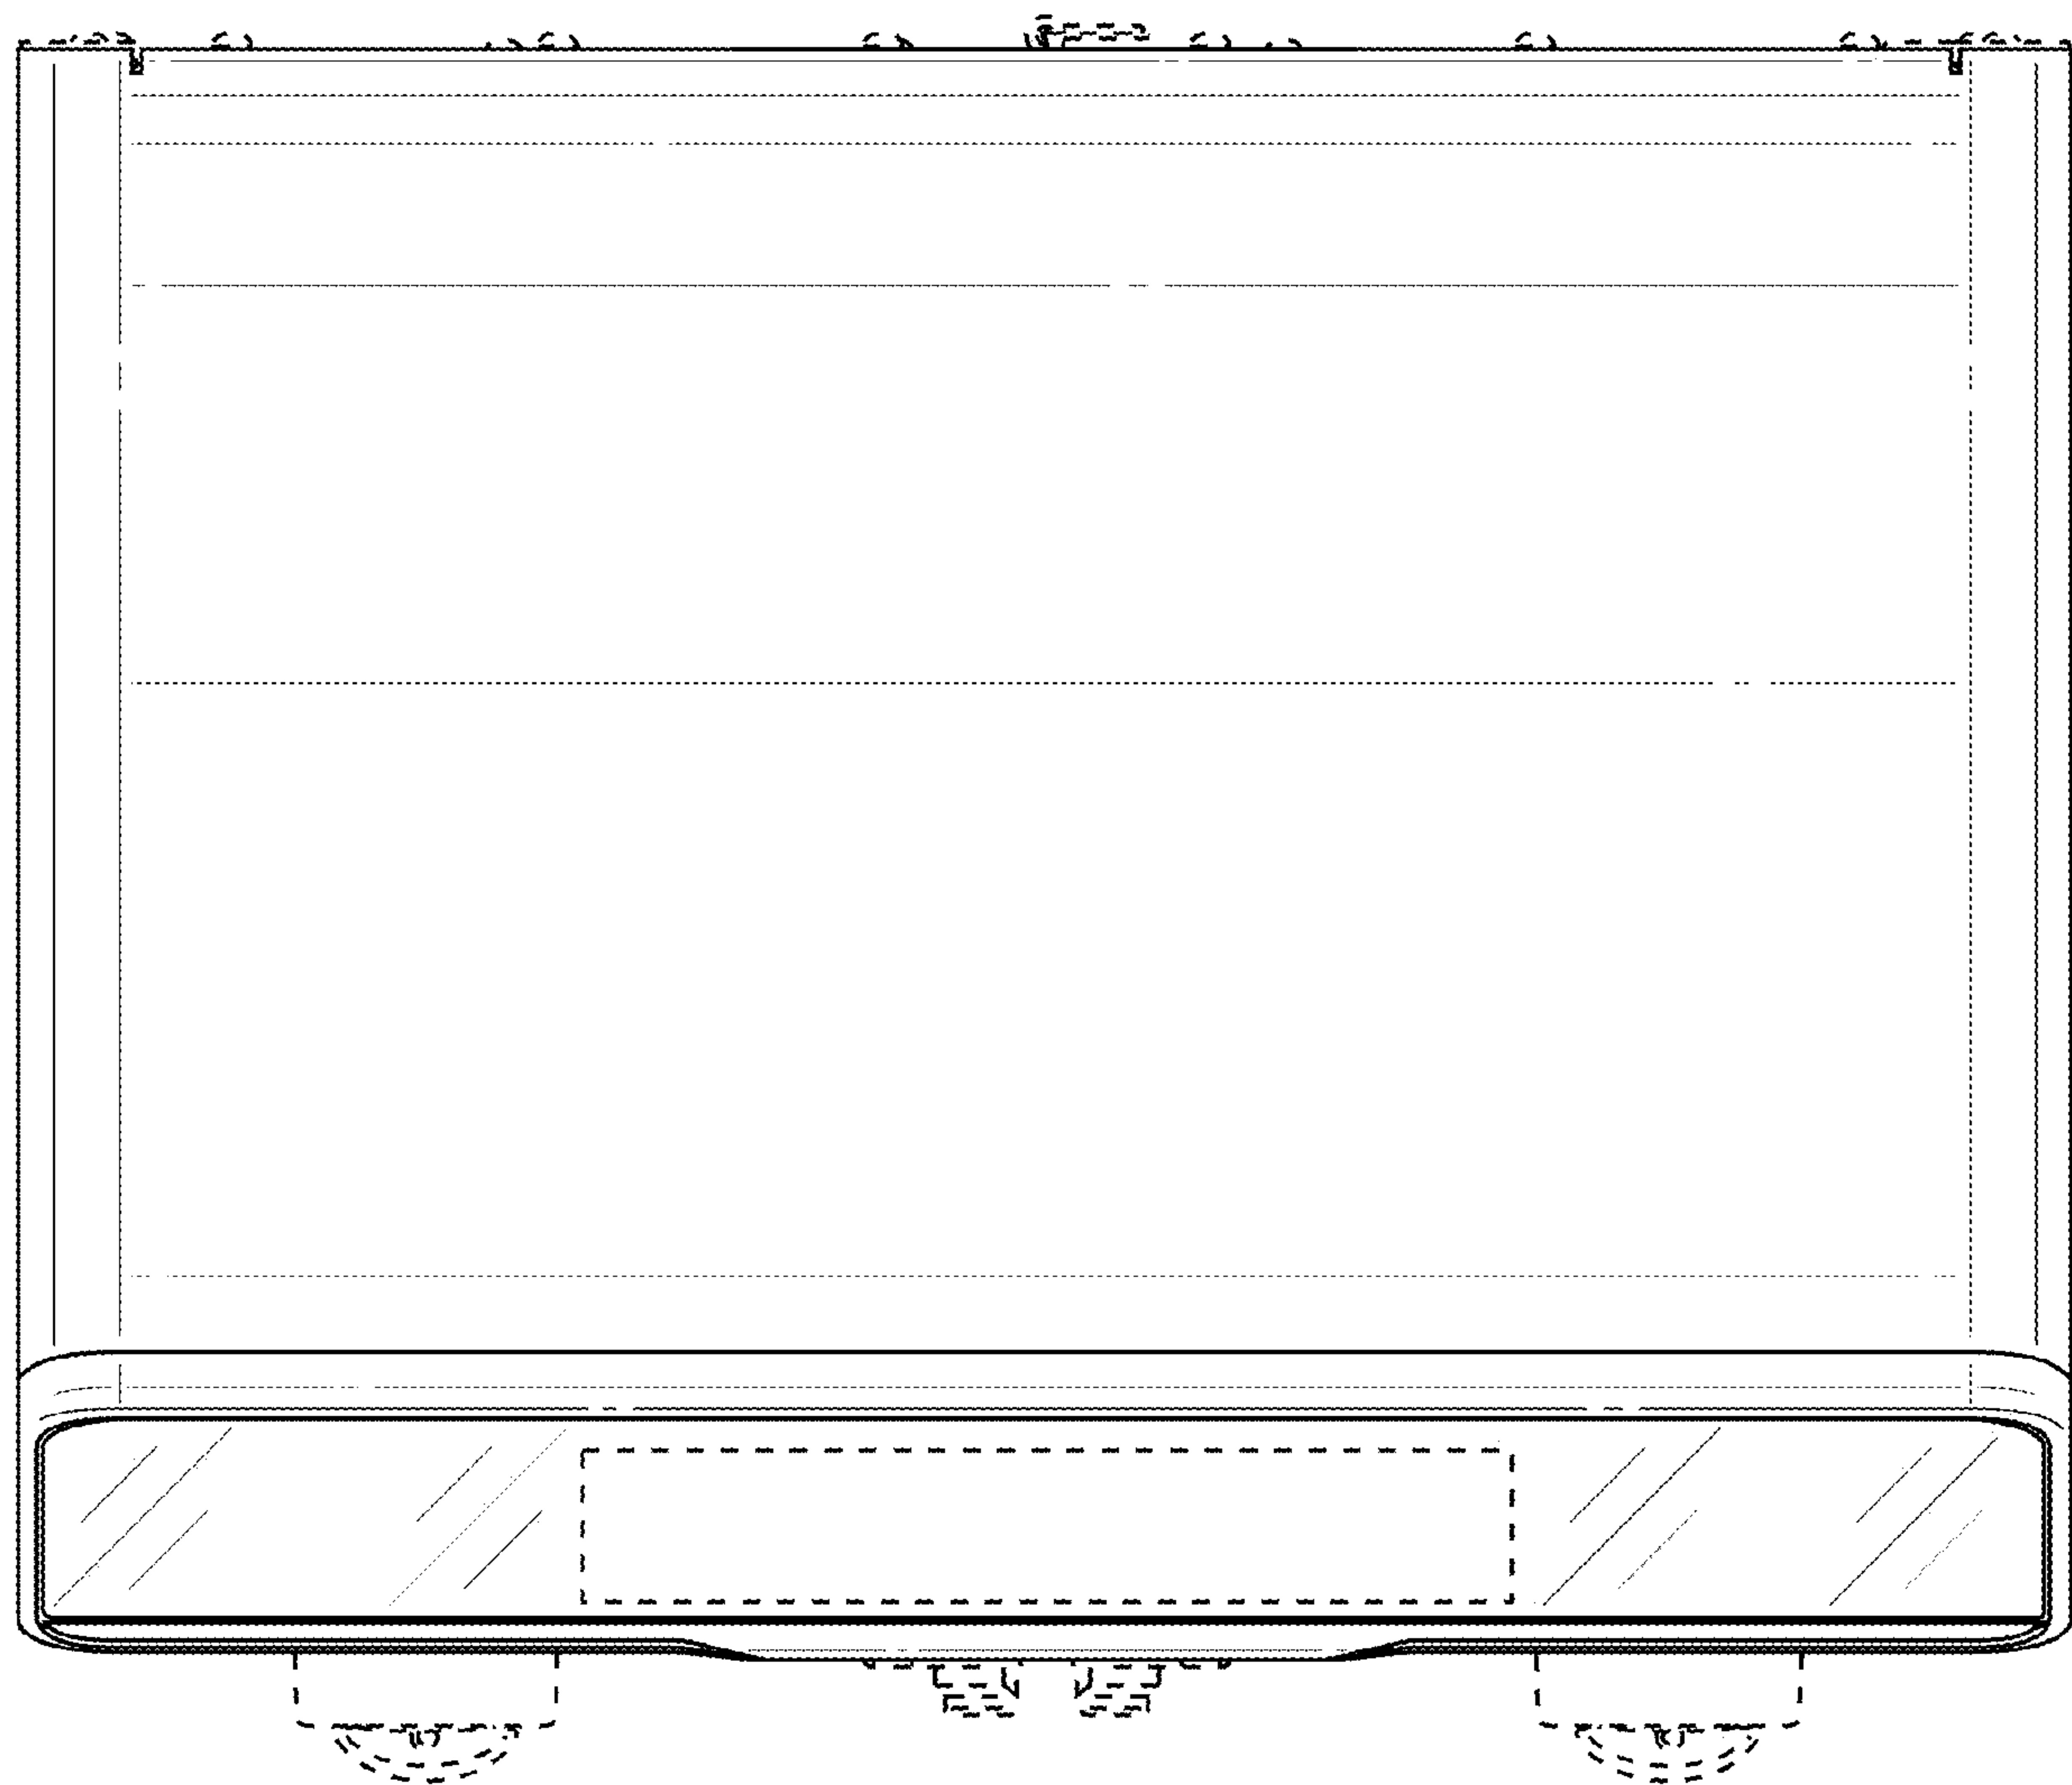


FIG. 7

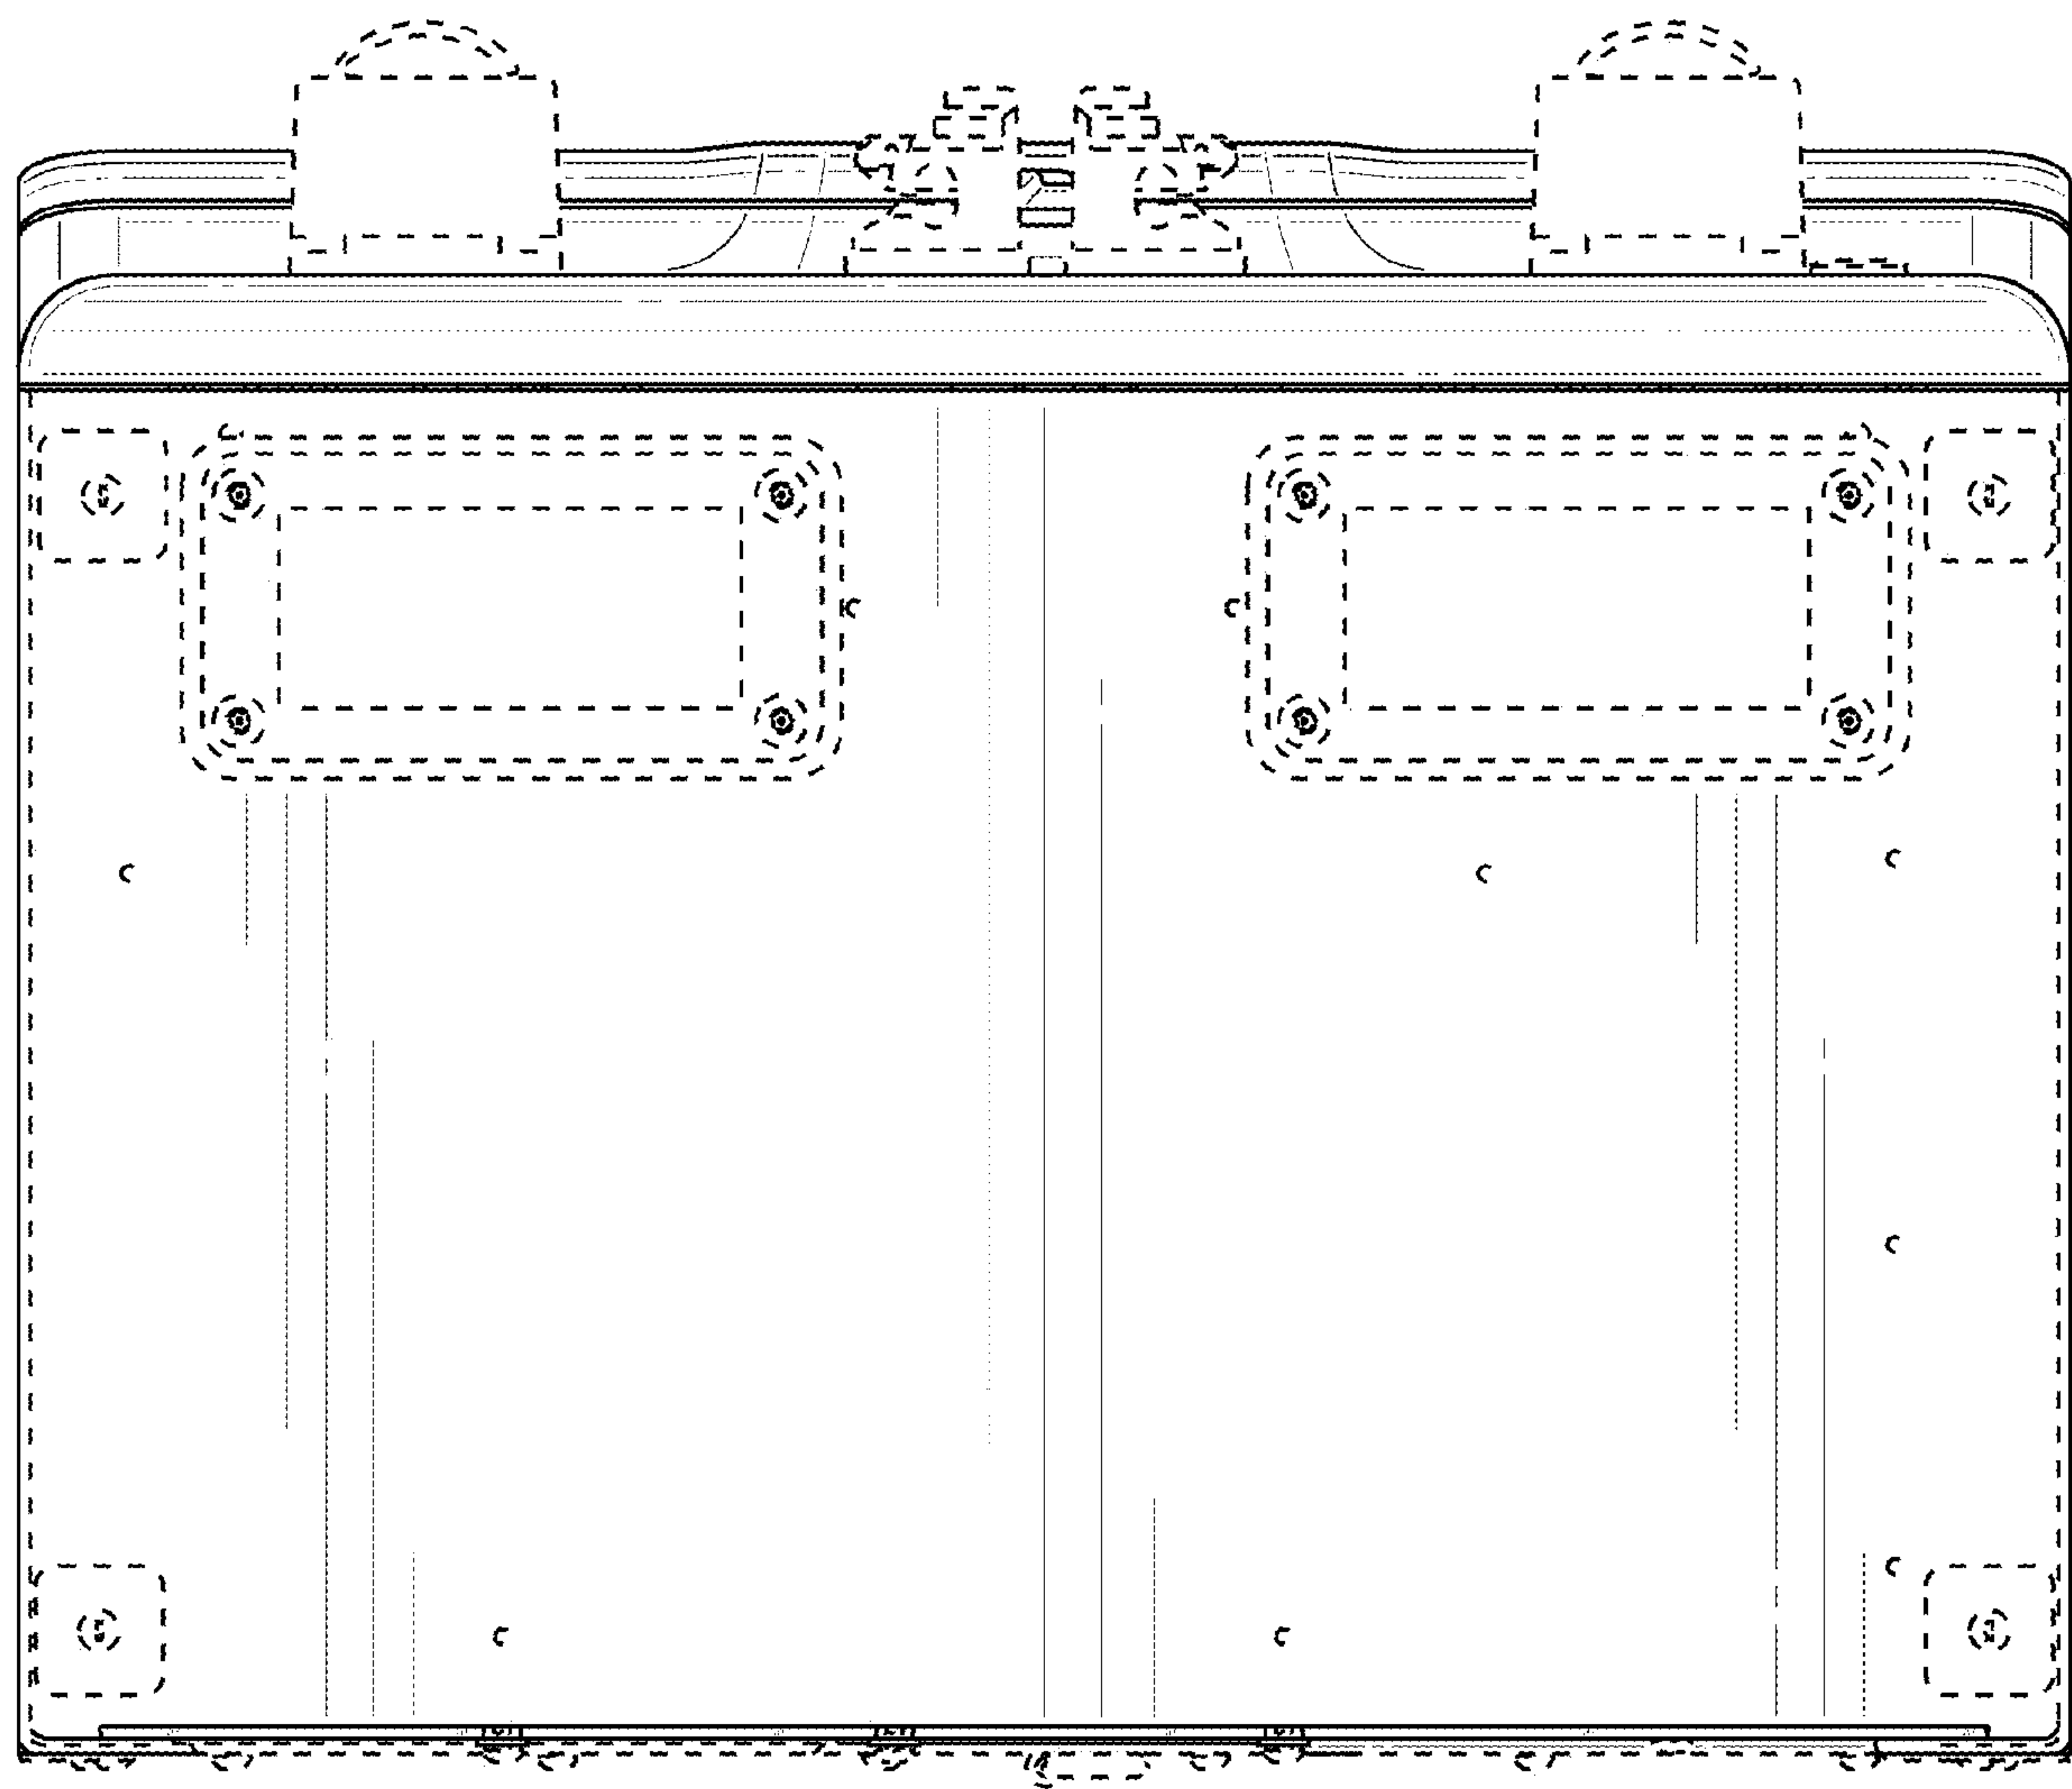


FIG. 8