



US0D1076107S

(12)

United States Design Patent
Hernandez

(10)

Patent No.: US D1,076,107 S

(45)

Date of Patent: ** May 20, 2025

- (54) ULTRASOUND TRANSDUCER HOUSING
- (71) Applicant: Lazaro Eduardo Hernandez, Cooper City, FL (US)
- (72) Inventor: Lazaro Eduardo Hernandez, Cooper City, FL (US)
- (**) Term: 15 Years
- (21) Appl. No.: 29/983,303
- (22) Filed: Jan. 9, 2025

Related U.S. Application Data

- (63) Continuation-in-part of application No. 29/973,198, filed on Nov. 14, 2024, which is a continuation-in-part of application No. 29/954,765, filed on Jul. 29, 2024, now Pat. No. Des. 1,055,291, which is a continuation-in-part of application No. 18/651,196, filed on Apr. 30, 2024, now Pat. No. 12,178,656, which is a continuation-in-part of application No. 18/471,150, filed on Sep. 20, 2023, which is a continuation-in-part of application No. 17/935,505, filed on Sep. 26, 2022, now Pat. No. 11,957,505, which is a continuation-in-part of application No. 17/210,013, filed on Mar. 23, 2021, now Pat. No. 11,457,889.
- (51) LOC (15) Cl. 24-01
- (52) U.S. Cl. D24/187
- (58) Field of Classification Search
- USPC D24/187, 185, 186, 133, 158, 127-129
- CPC A61B 8/06; A61B 8/08; A61B 8/42; A61B 8/4272; A61B 8/44; A61B 8/4433; A61B 8/4483; A61B 8/4494; A61B 8/52; A61B 8/5207; A61B 8/5215; A61B 8/5223; A61B 8/5238
- See application file for complete search history.

- (56) References Cited
- U.S. PATENT DOCUMENTS
- 4,796,632 A * 1/1989 Boyd A61B 8/4281 73/644
- D327,740 S 7/1992 Arioka et al.
- D360,035 S 7/1995 Miller et al.
- D376,126 S * 12/1996 Henderson D13/101
- D412,580 S * 8/1999 Kellstedt D24/187
- D630,756 S * 1/2011 Kitayama D24/187
- D669,181 S 10/2012 Prado
- D669,182 S 10/2012 Prado
- D692,564 S * 10/2013 Ninomiya D24/187
- (Continued)

Primary Examiner — Daniel J Domino
Assistant Examiner — Lee D. Starr


- (57) CLAIM
- The ornamental design for an ultrasound transducer housing, as shown and described.

DESCRIPTION

FIG. 1 is a top-front-left perspective view of an ultrasound transducer housing showing my new design;
FIG. 2 is a bottom-front-left perspective view thereof
FIG. 3 is a top-rear-right perspective view thereof;
FIG. 4 is a bottom-rear-right perspective view thereof;
FIG. 5 is a front elevational view thereof;
FIG. 6 is a rear elevational view thereof;
FIG. 7 is a top plan view thereof;
FIG. 8 is a bottom plan view thereof;
FIG. 9 is a right elevational view thereof;
FIG. 10 is a left elevational view thereof; and,
FIG. 11 is a top-rear-right perspective view thereof, wherein the ultrasound transducer housing is shown with a housing holder.

The broken lines showing a cable opening and a probe opening in FIGS. 2-4, 8, 9, and 11, and the broken lines showing a housing holder in FIG. 11 are included for the purpose of illustrating environmental structure and form no part of the claimed design.

1 Claim, 11 Drawing Sheets

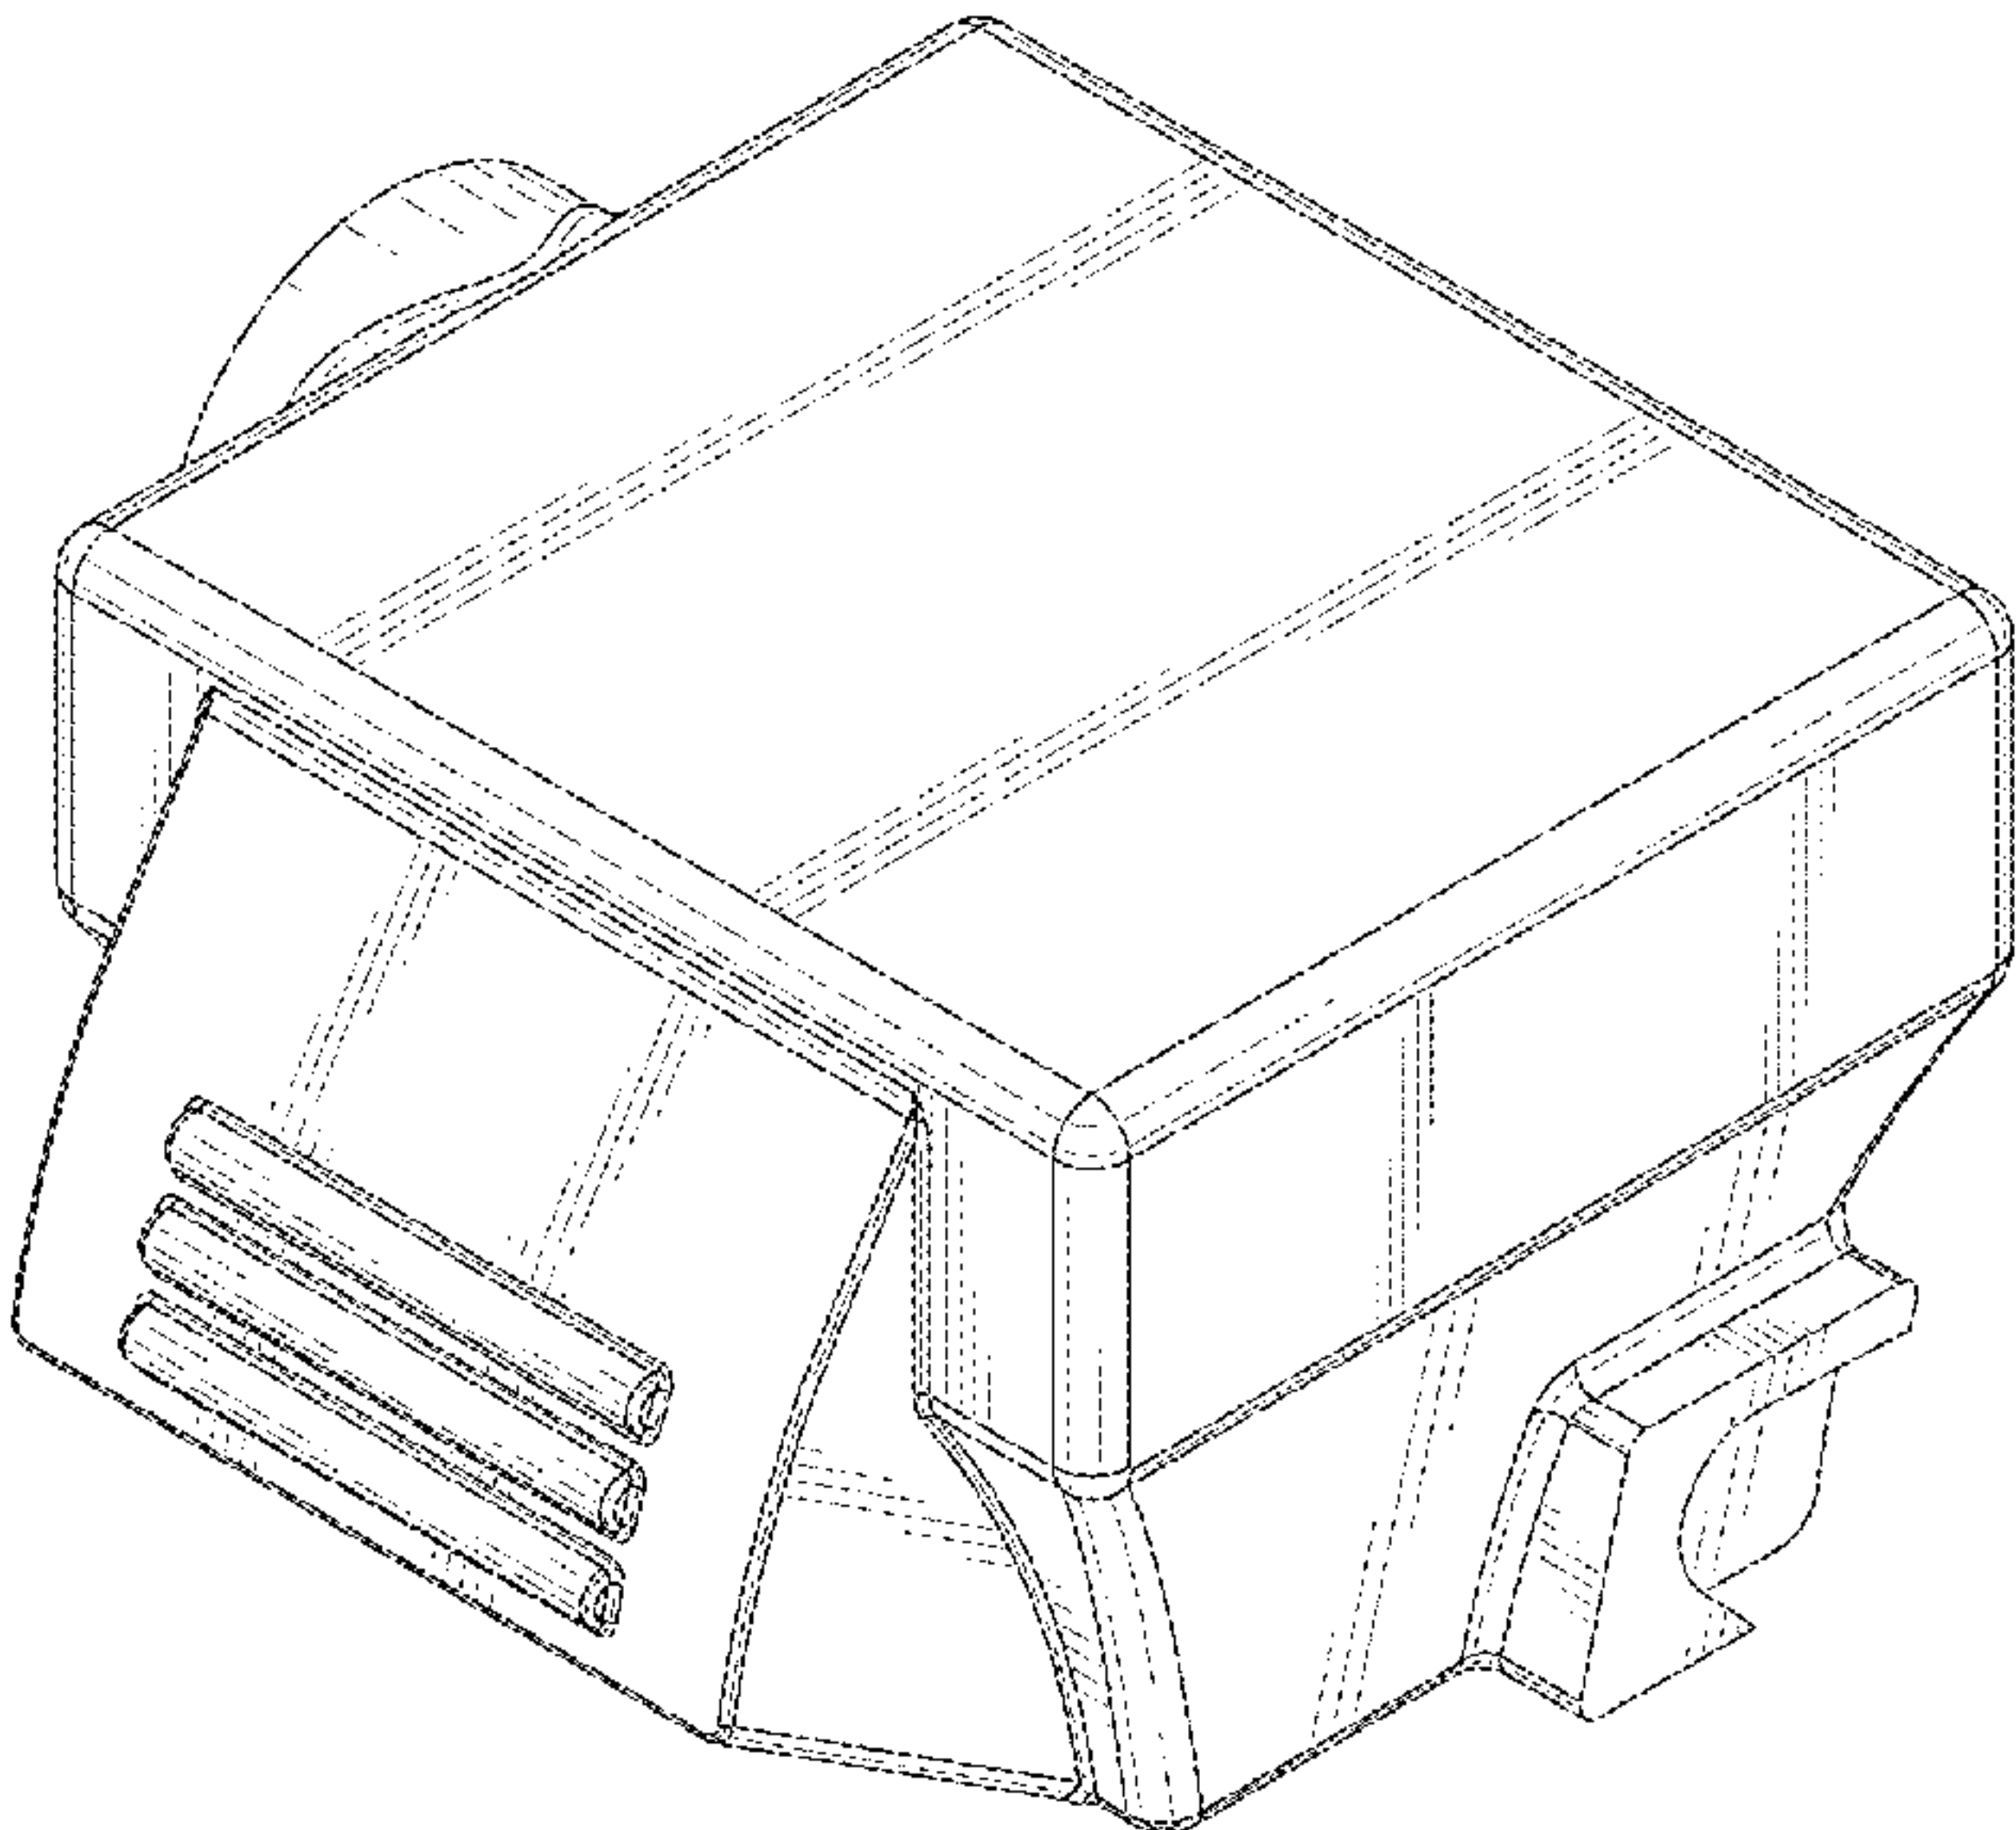

(56) **References Cited**

U.S. PATENT DOCUMENTS

D700,969	S	*	3/2014	Kim	D24/187
D743,040	S		11/2015	Corbett, III et al.	
D811,605	S		2/2018	Chang	
D861,178	S	*	9/2019	Emery	D24/187
D900,325	S	*	10/2020	Emery	D24/187
D1,055,291	S	*	12/2024	Hernandez	D24/187
2011/0112405	A1	*	5/2011	Barthe	A61B 8/467
					600/459
2013/0150715	A1	*	6/2013	Lacoste	A61B 8/4483
					600/439

* cited by examiner

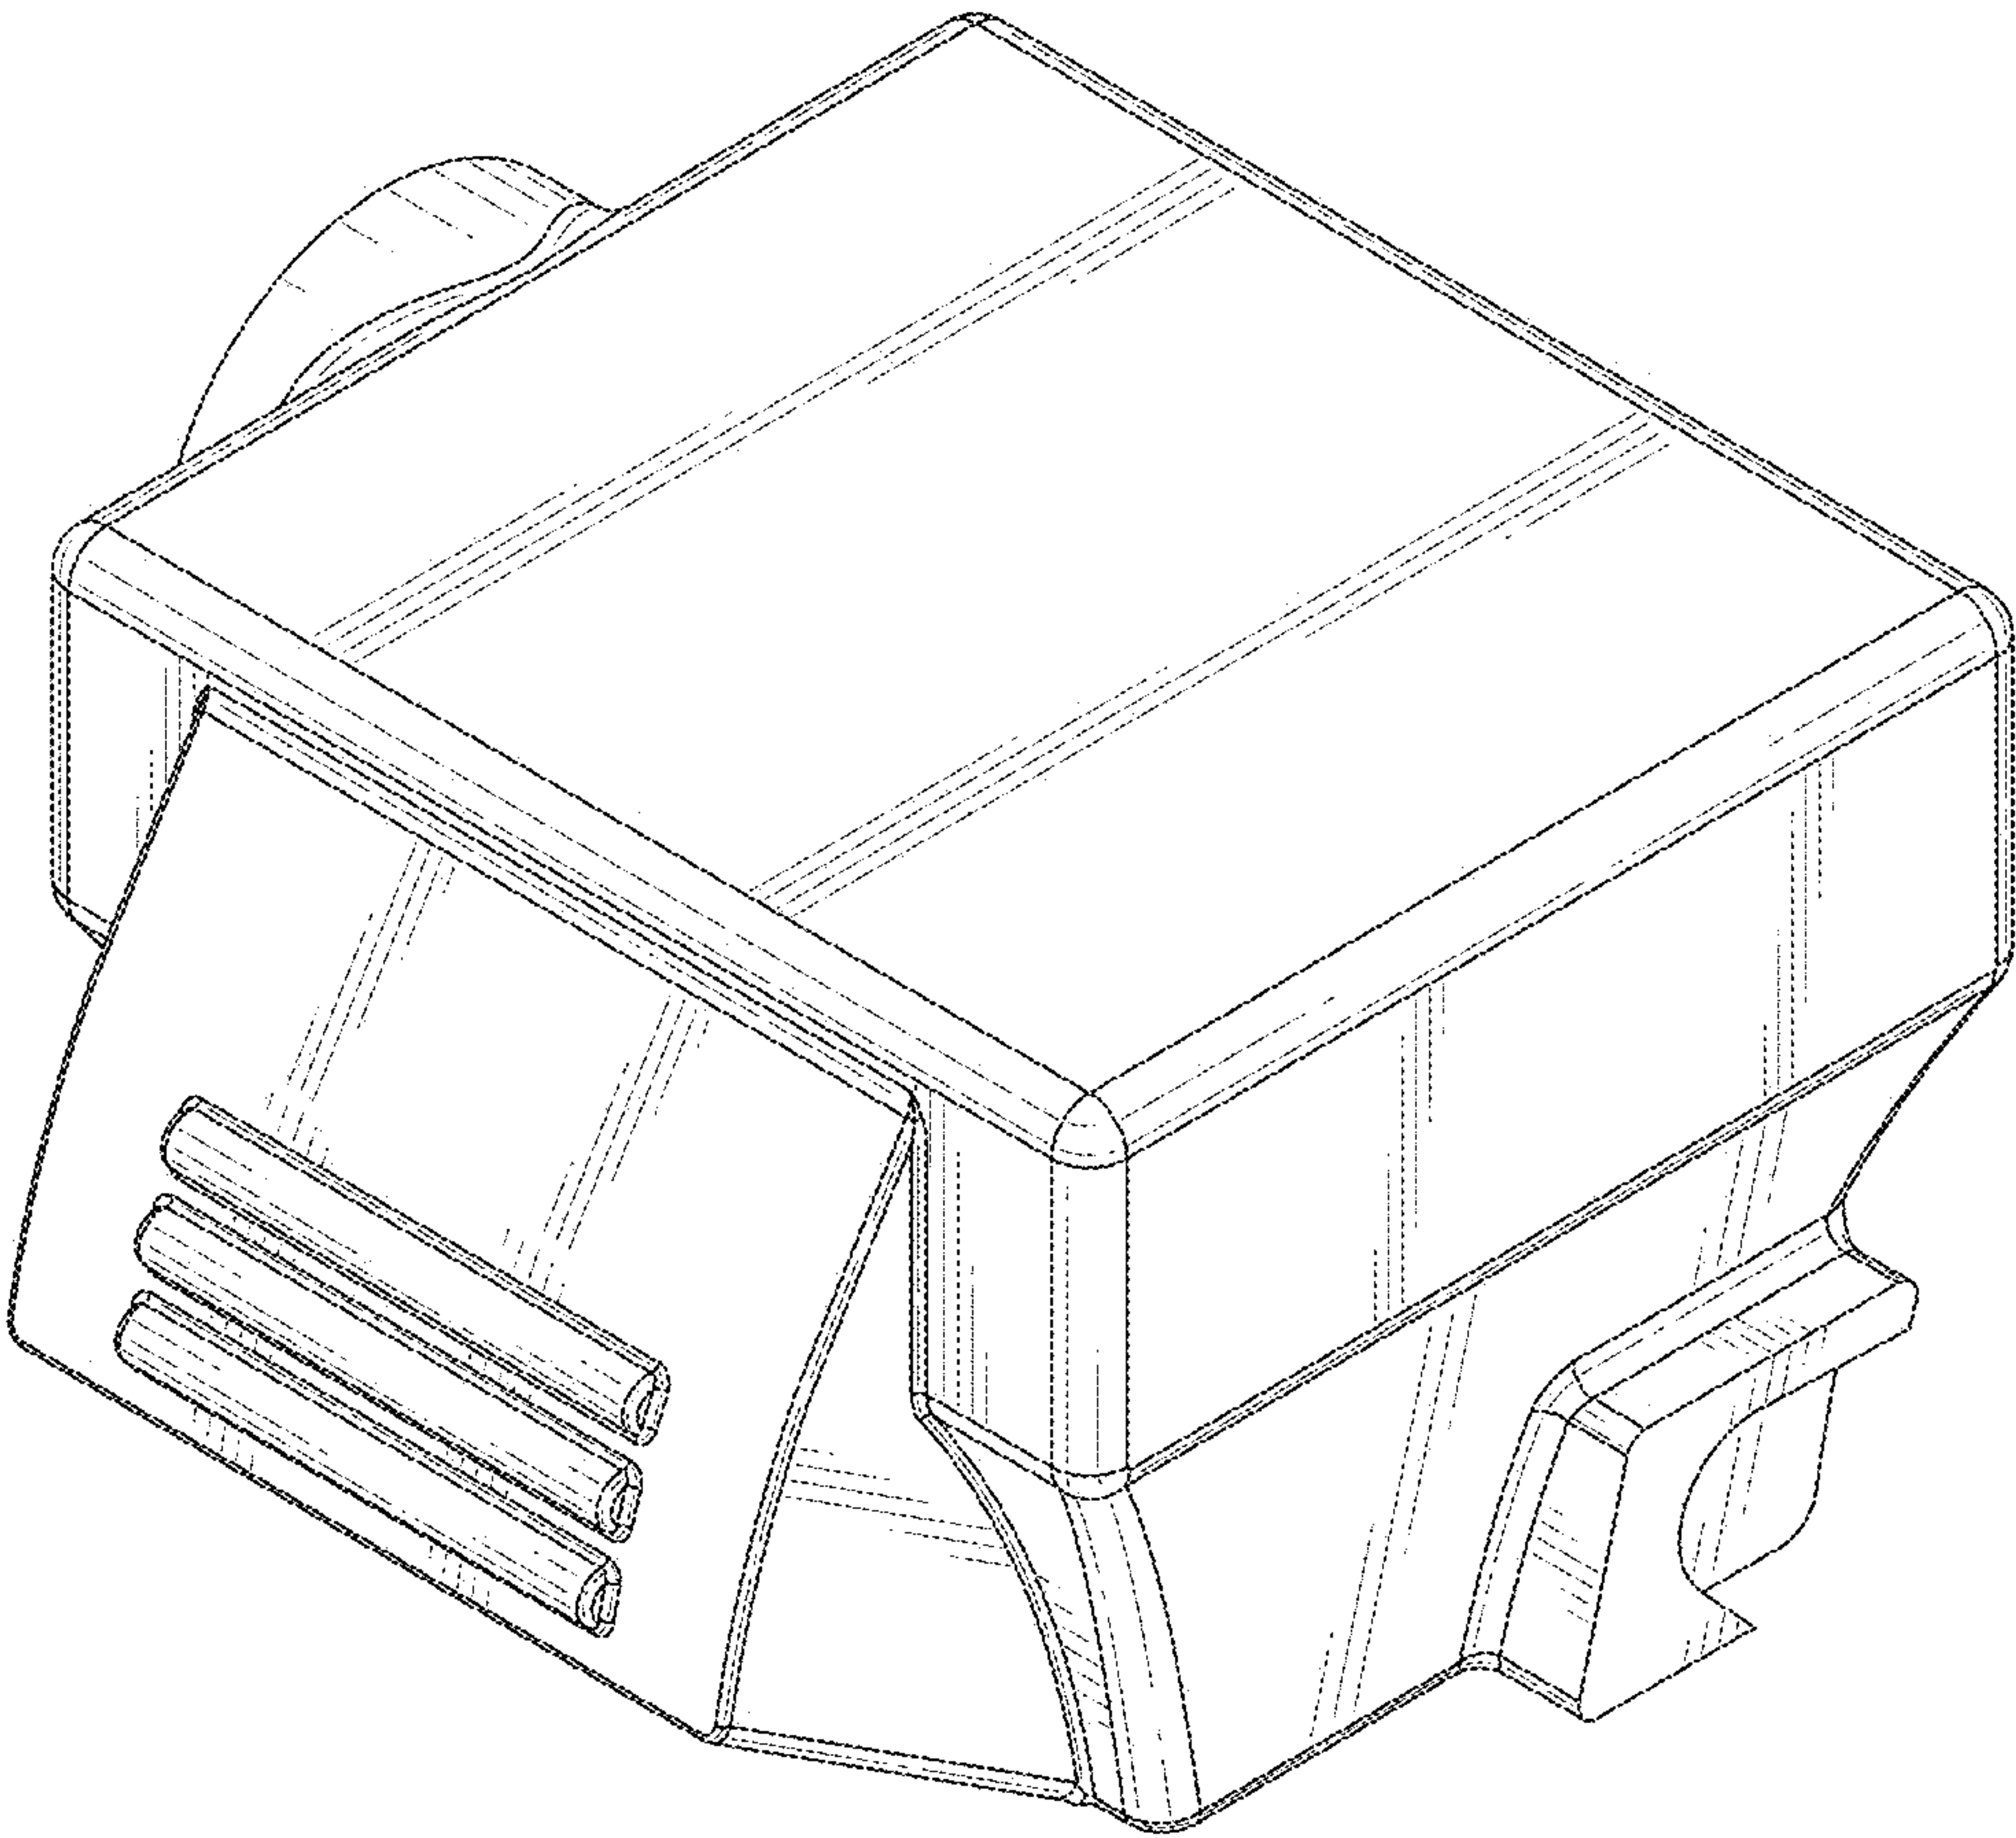


FIG. 1

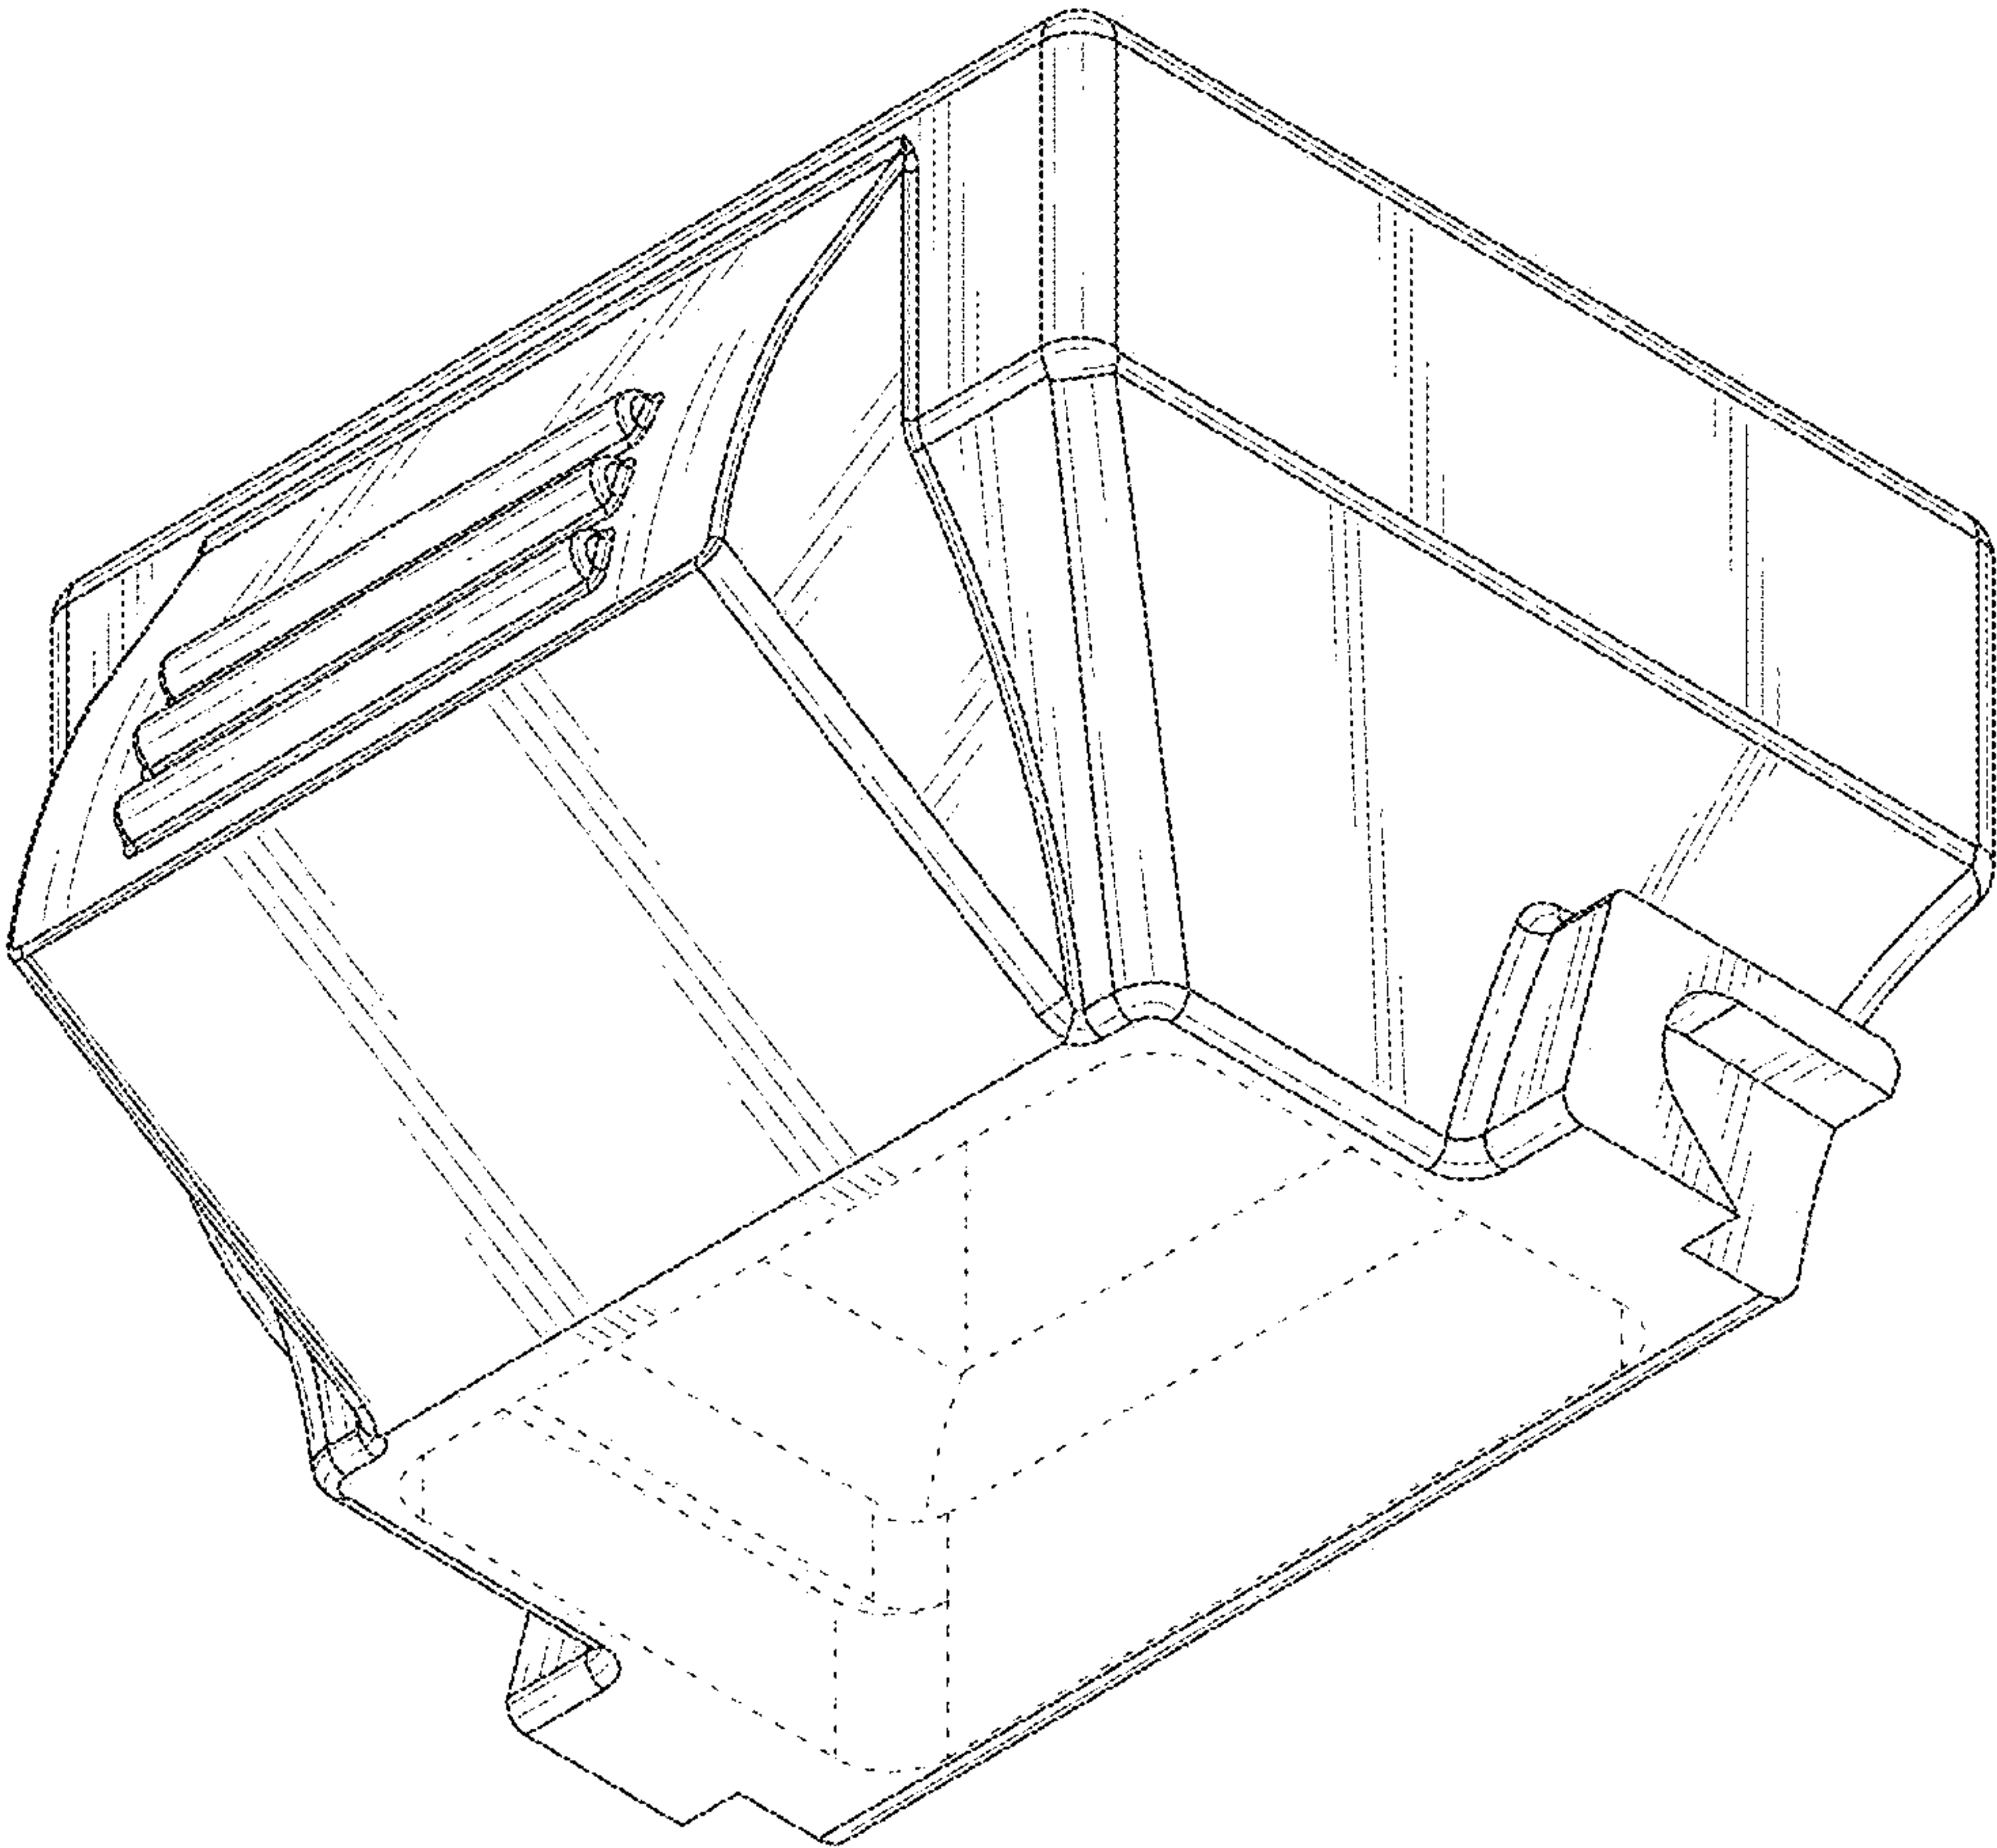


FIG. 2

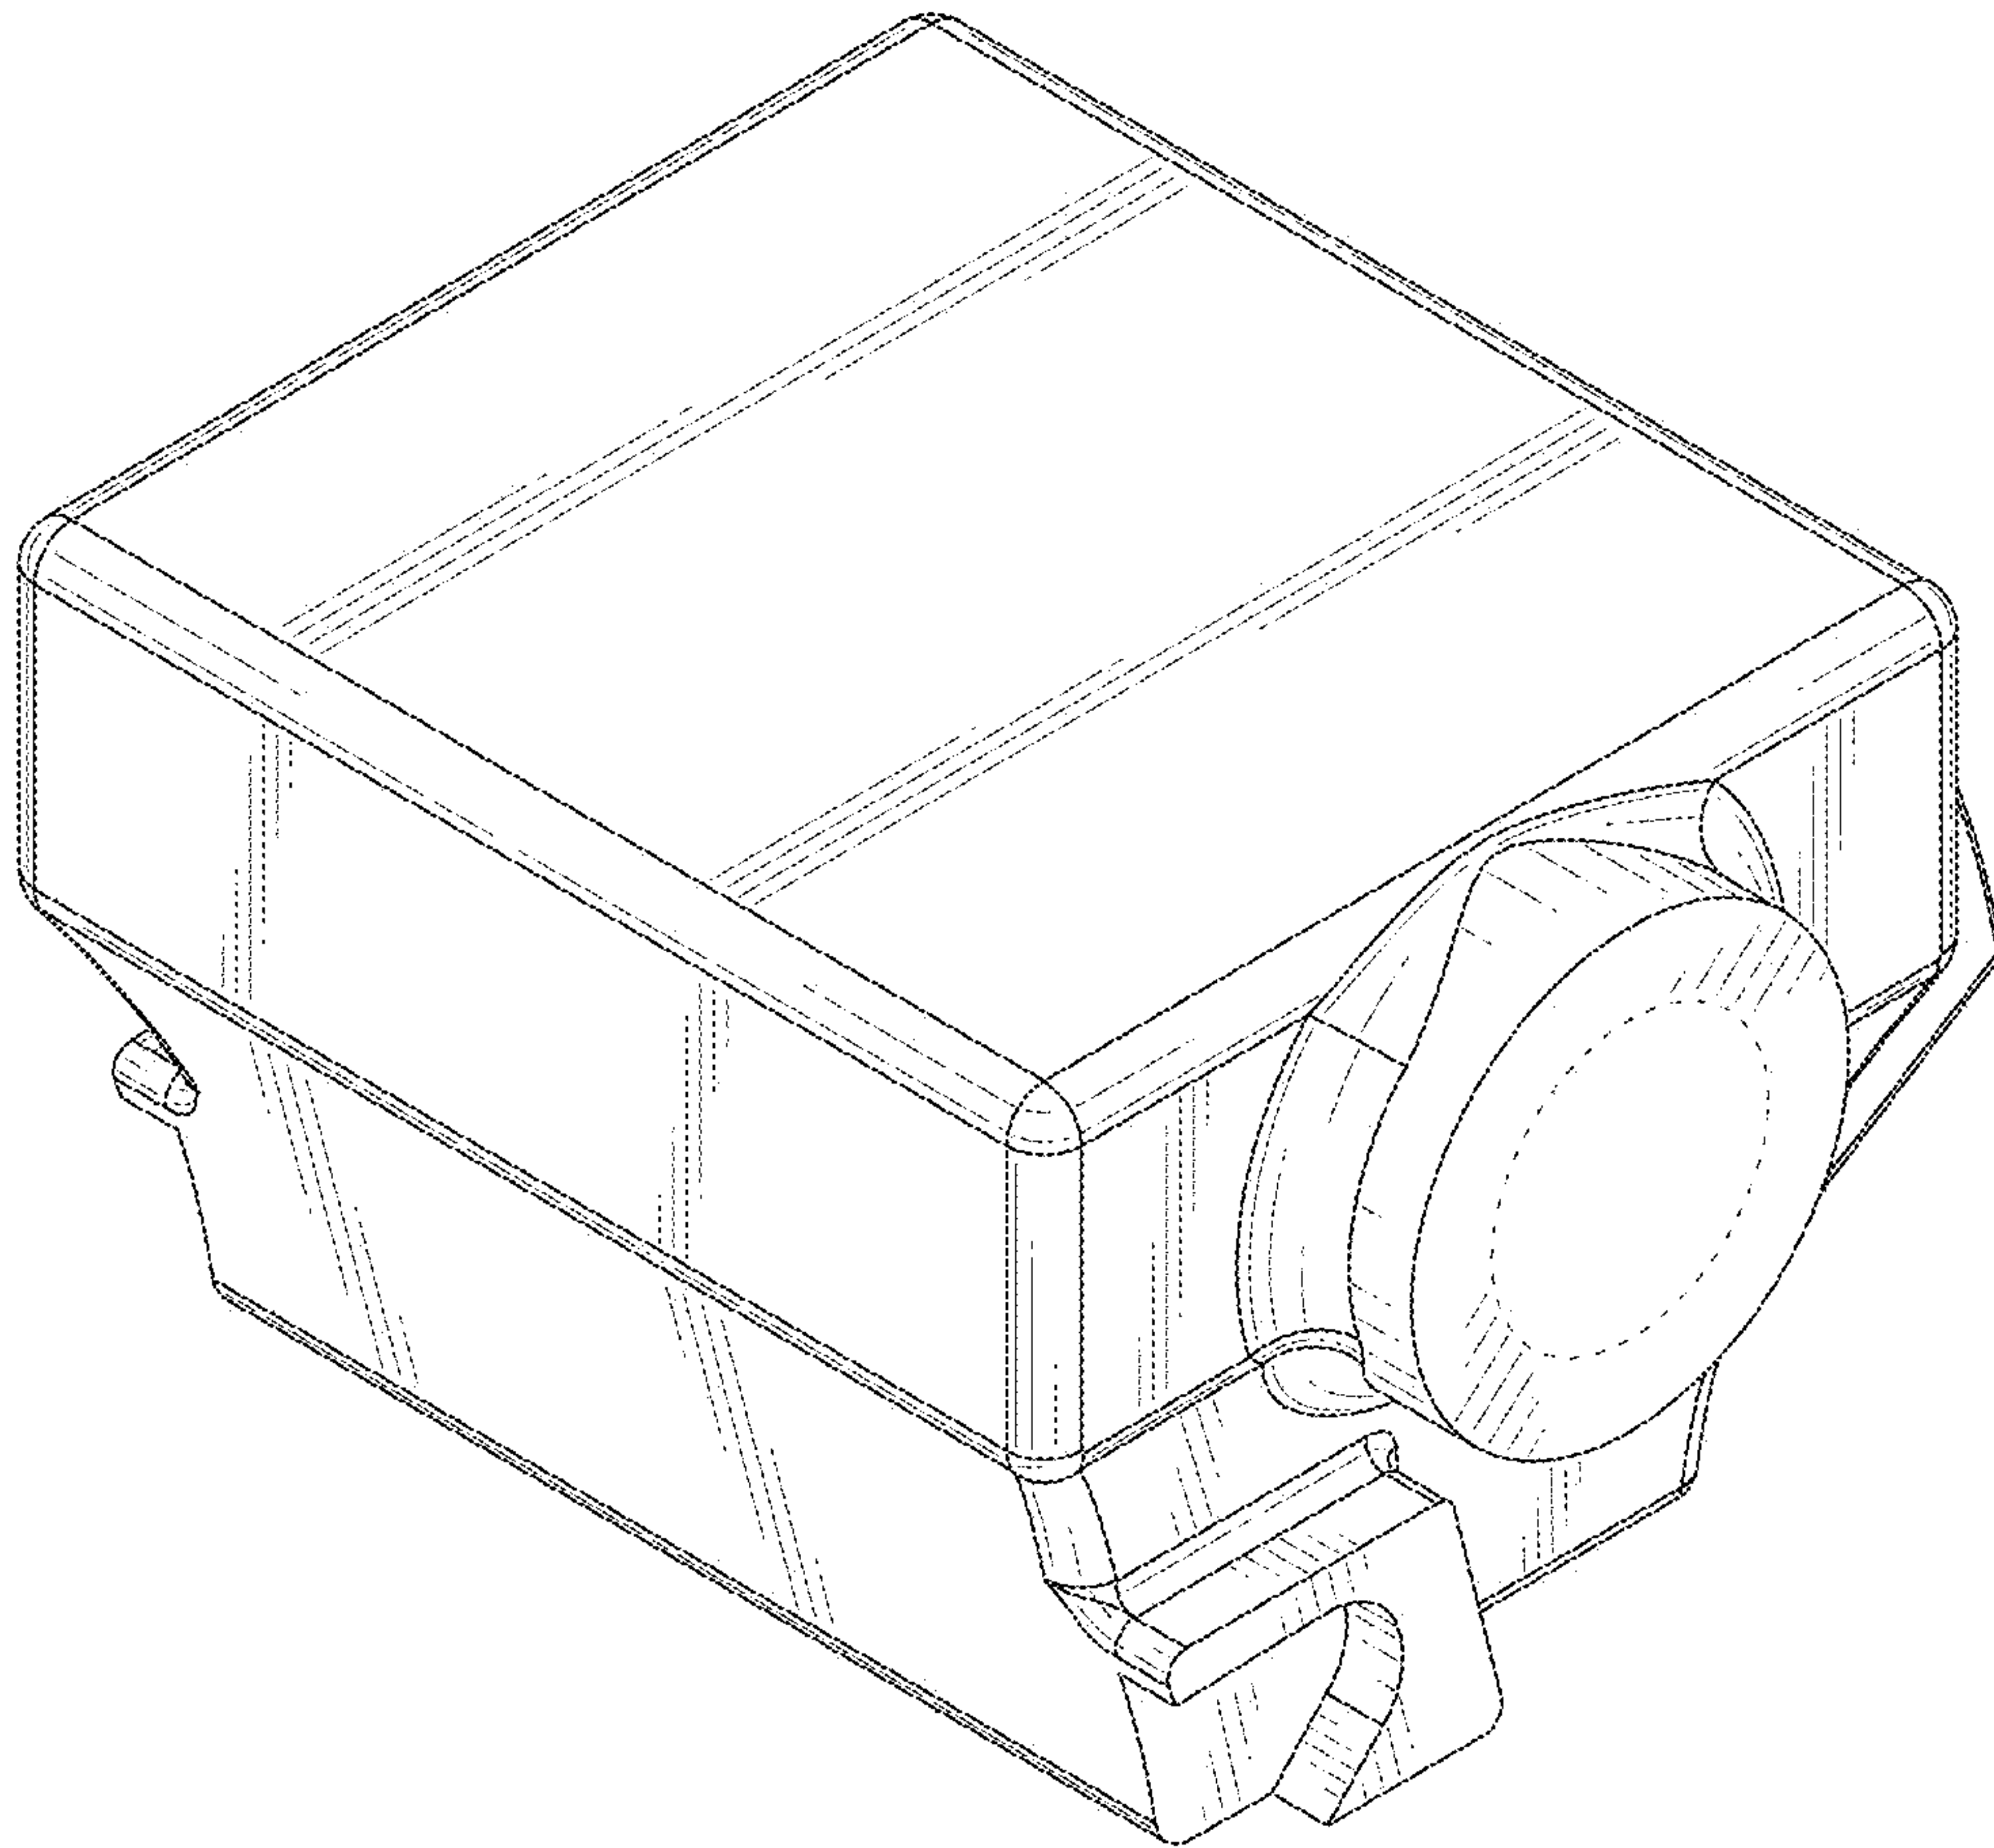


FIG. 3

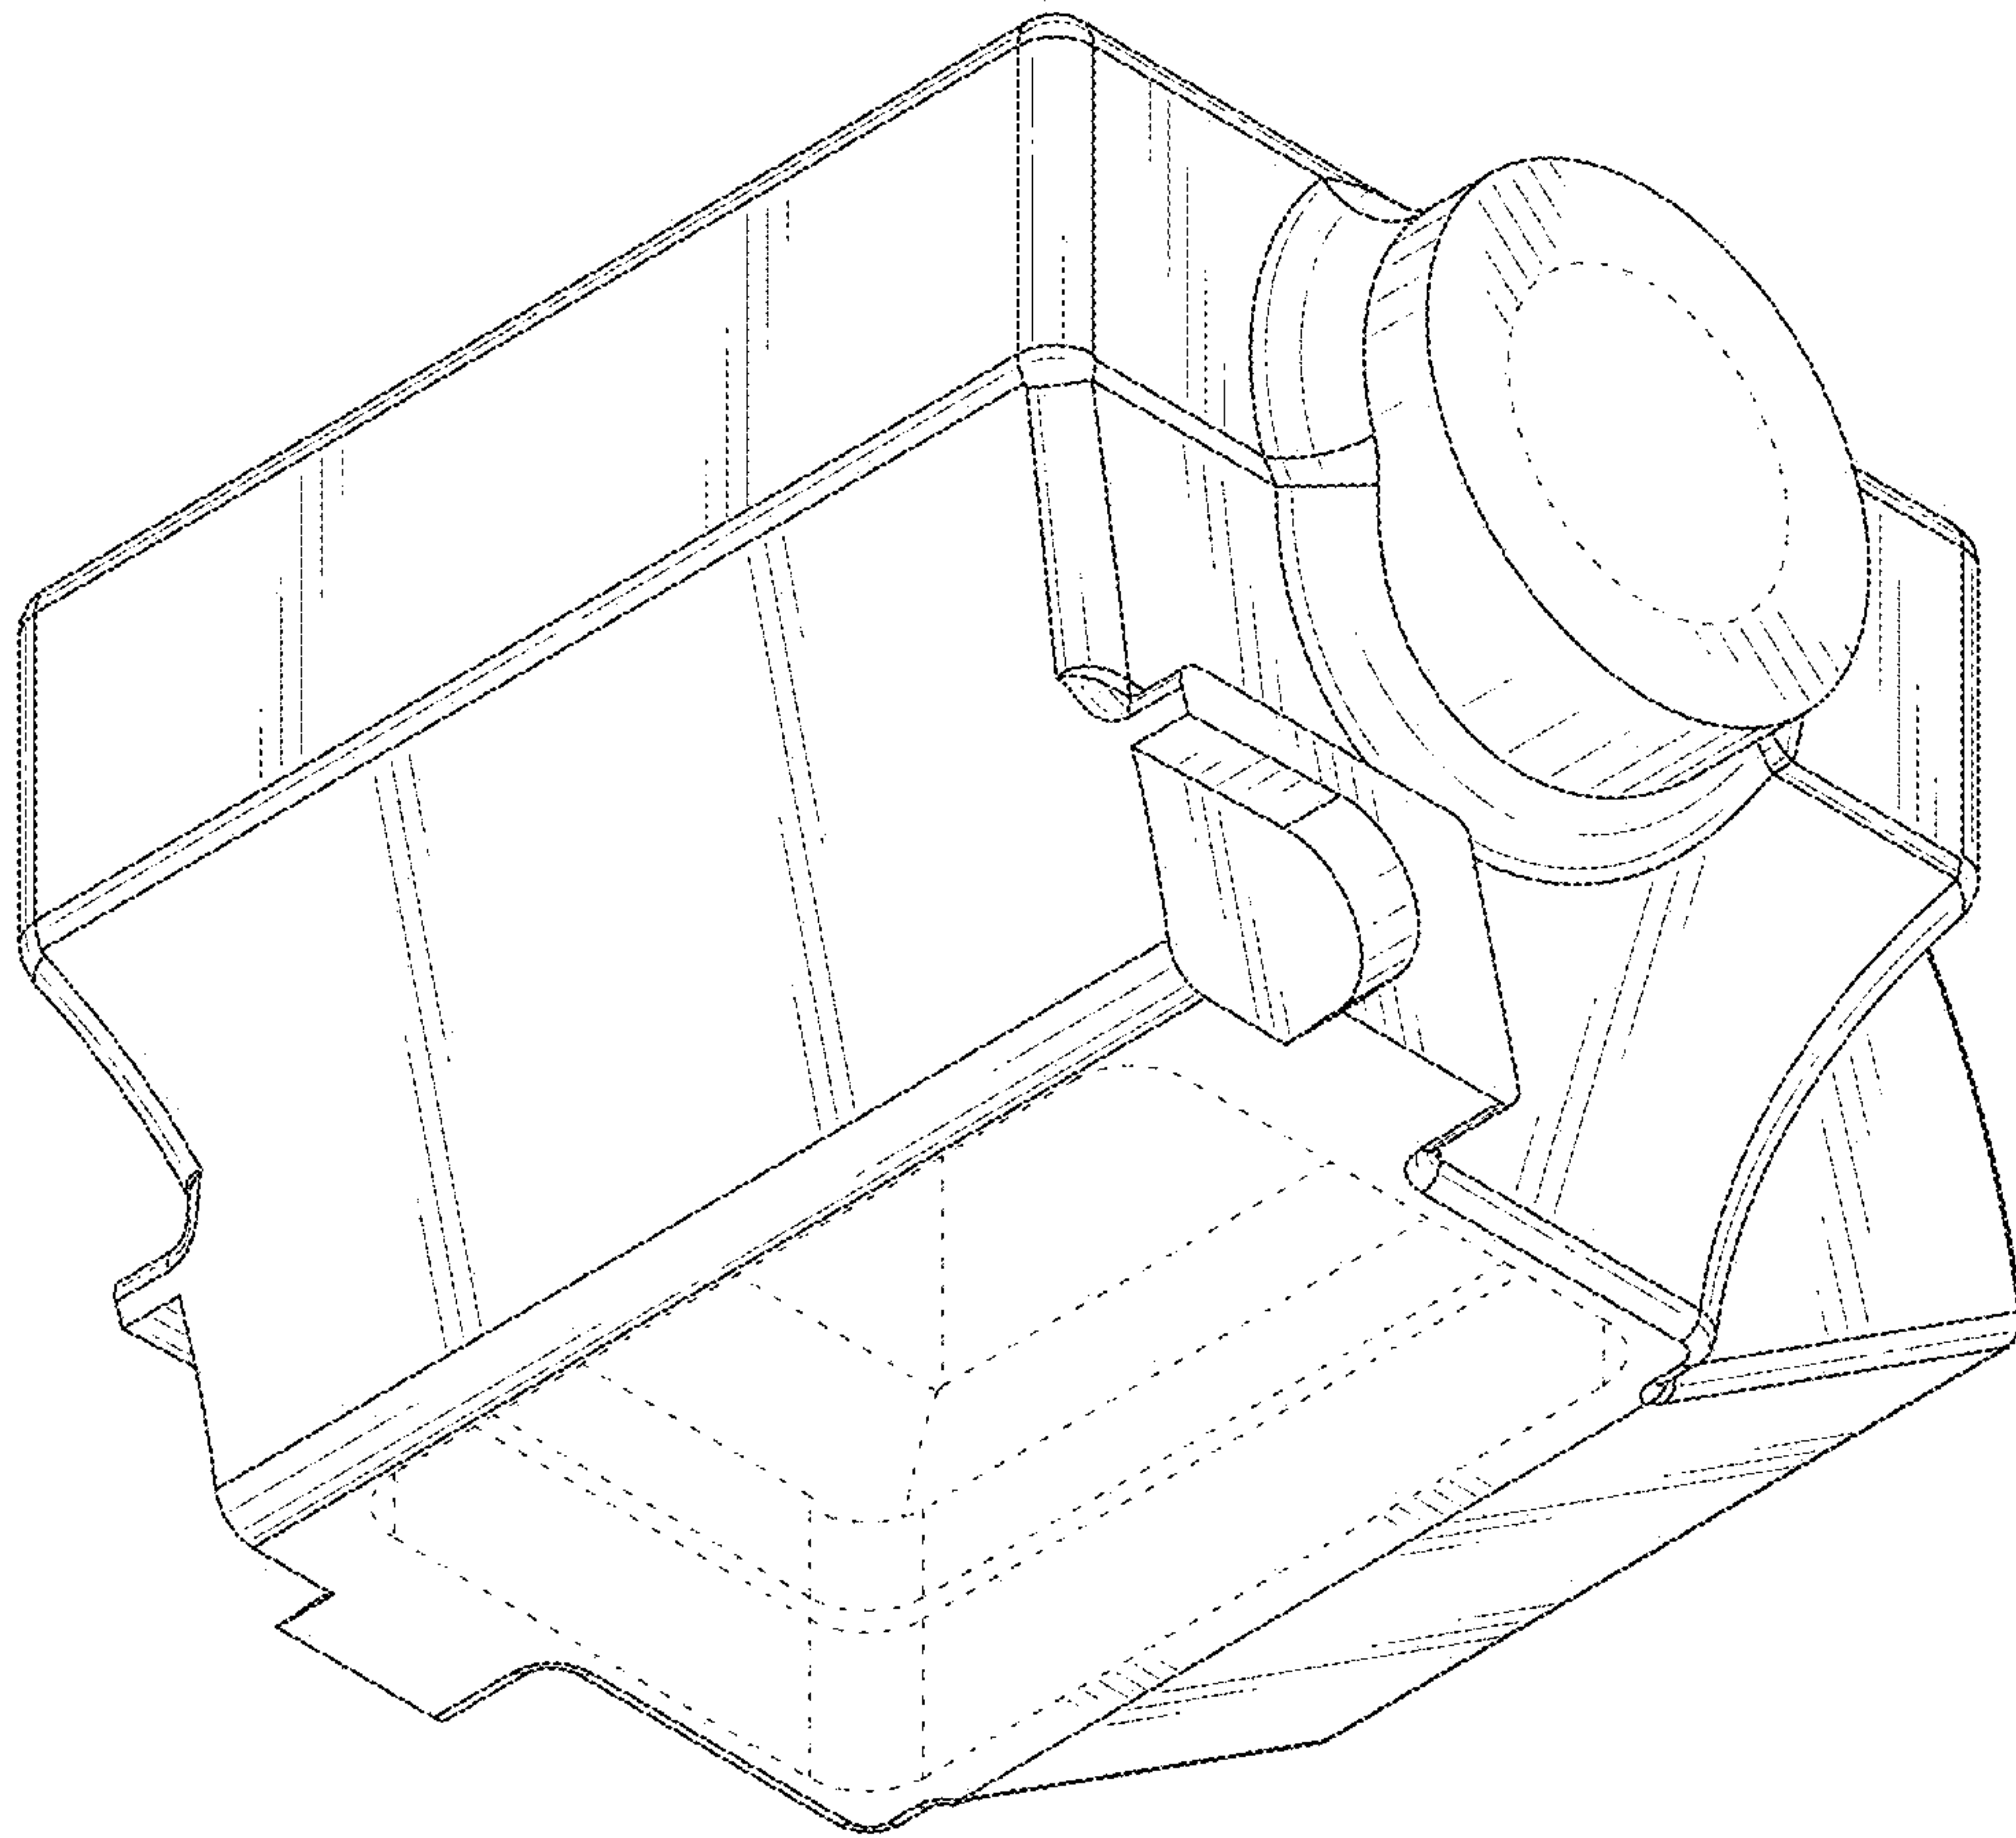


FIG. 4

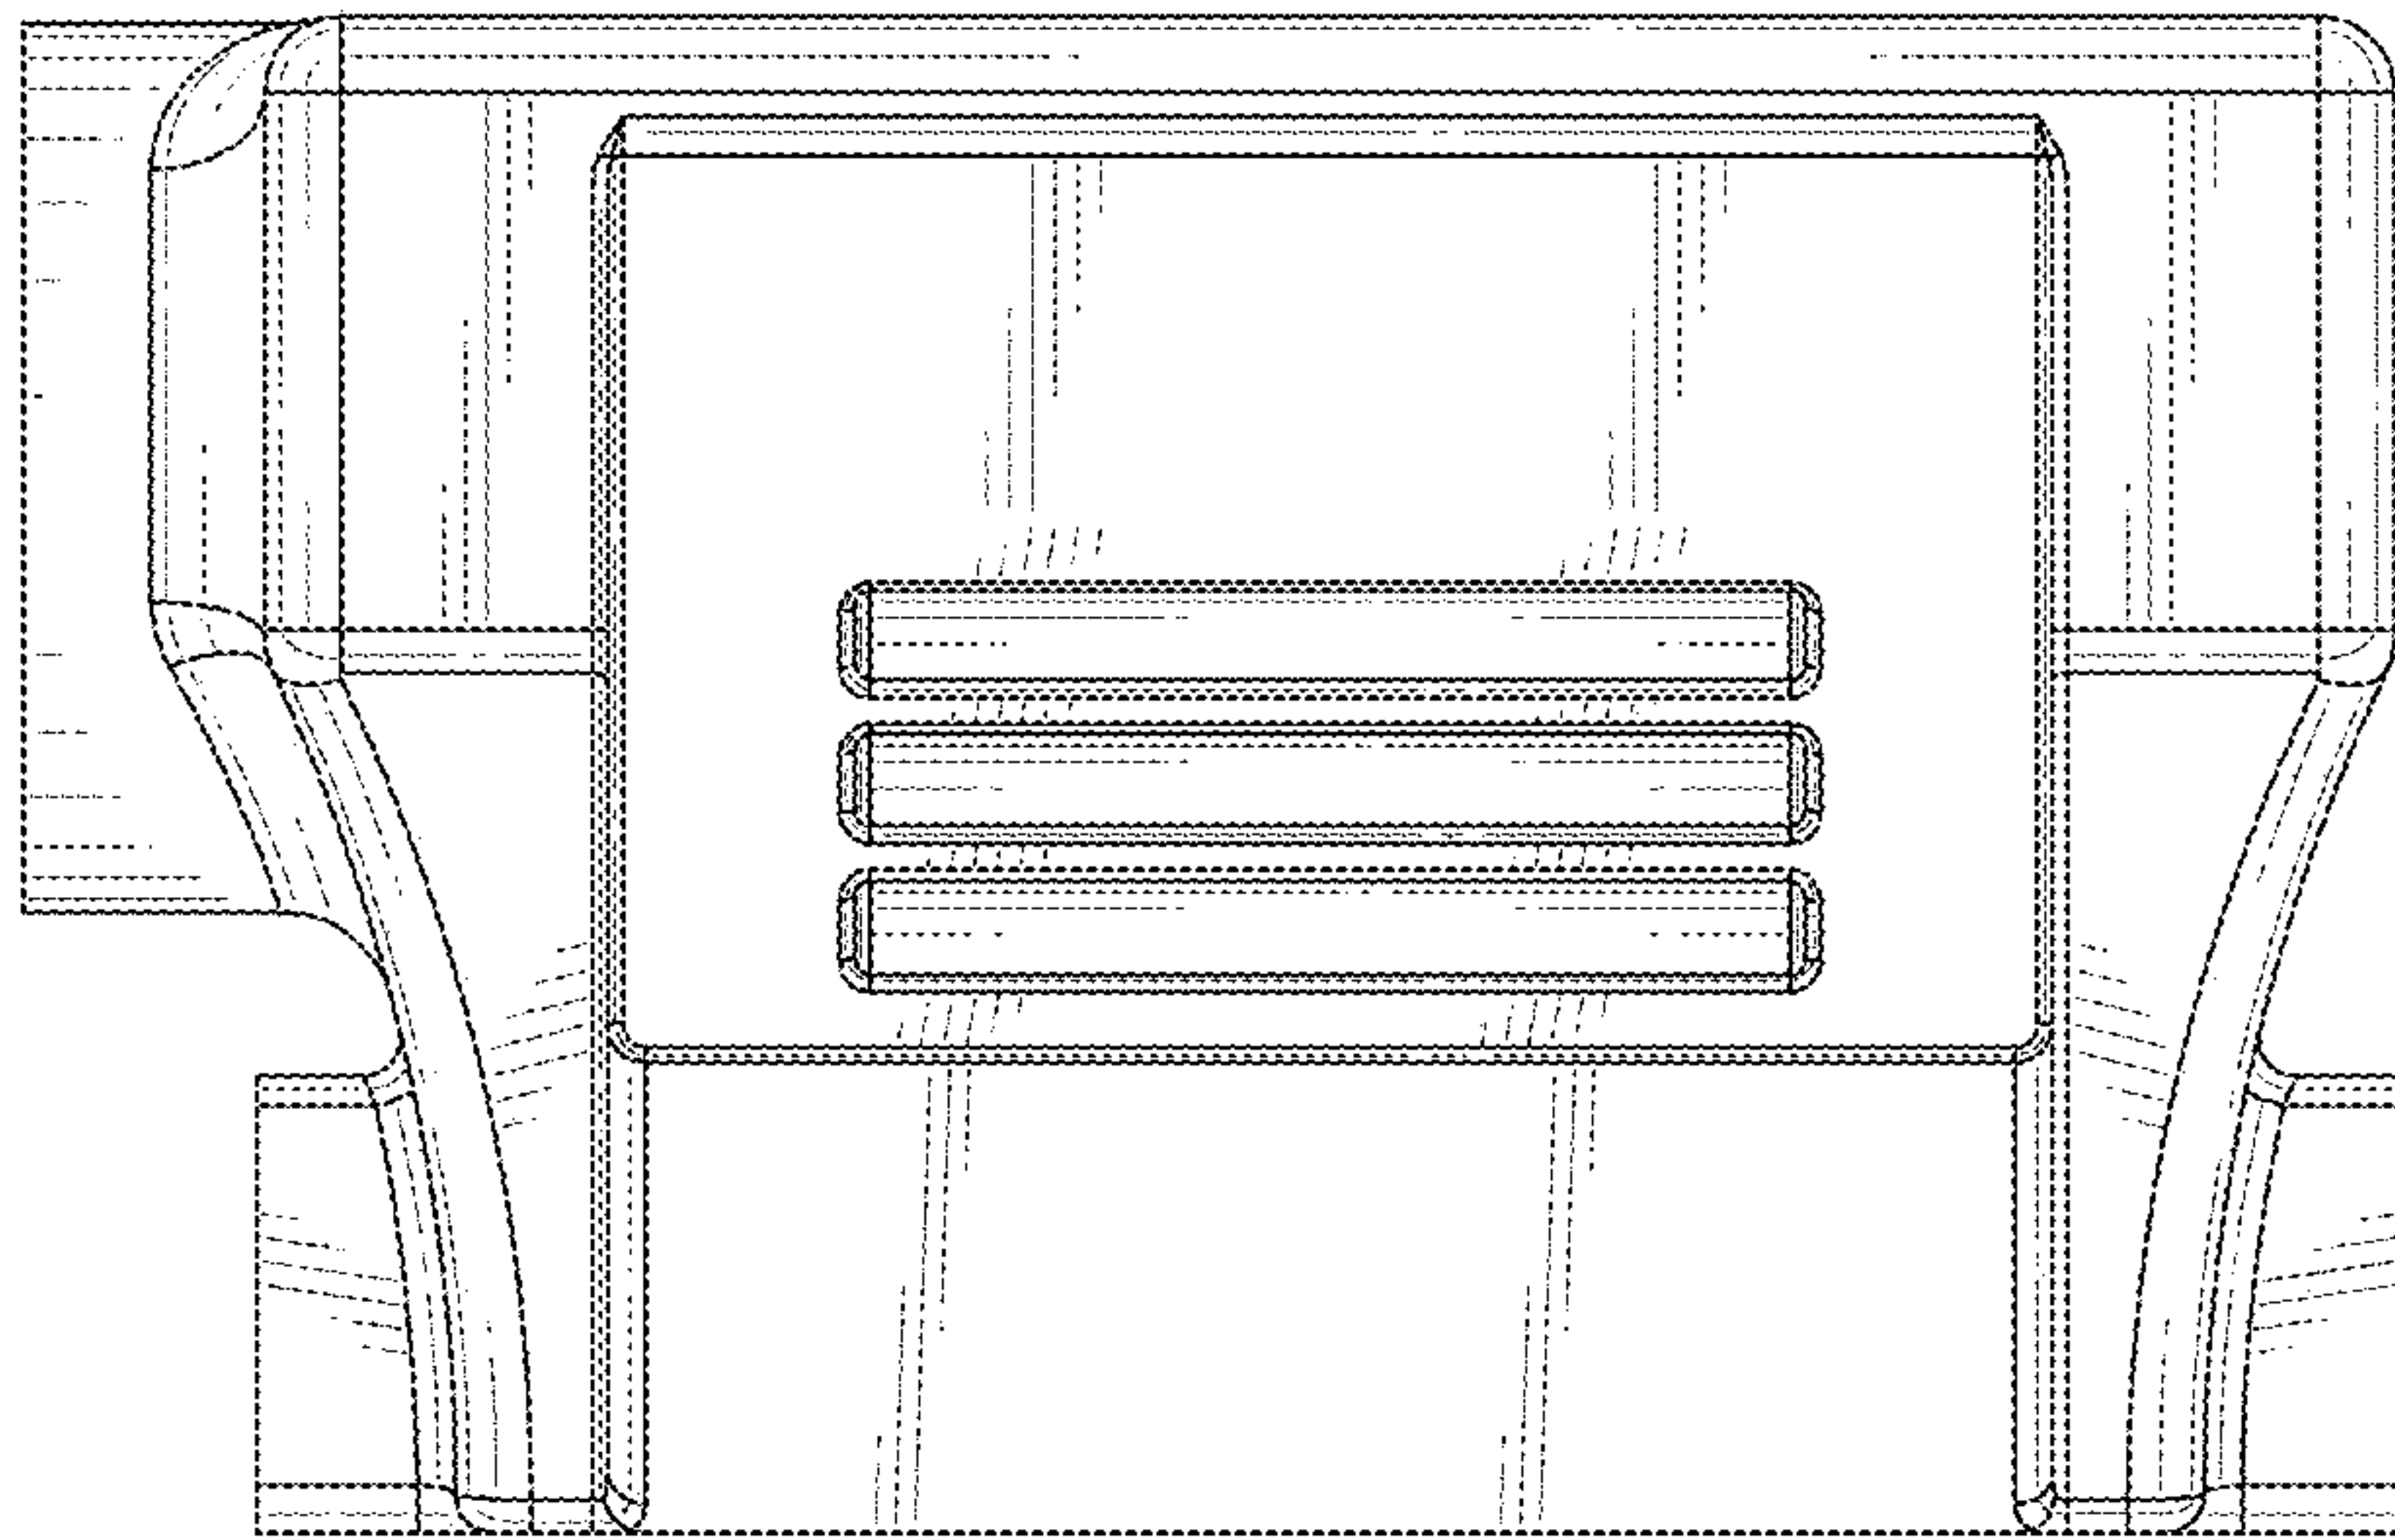


FIG. 5

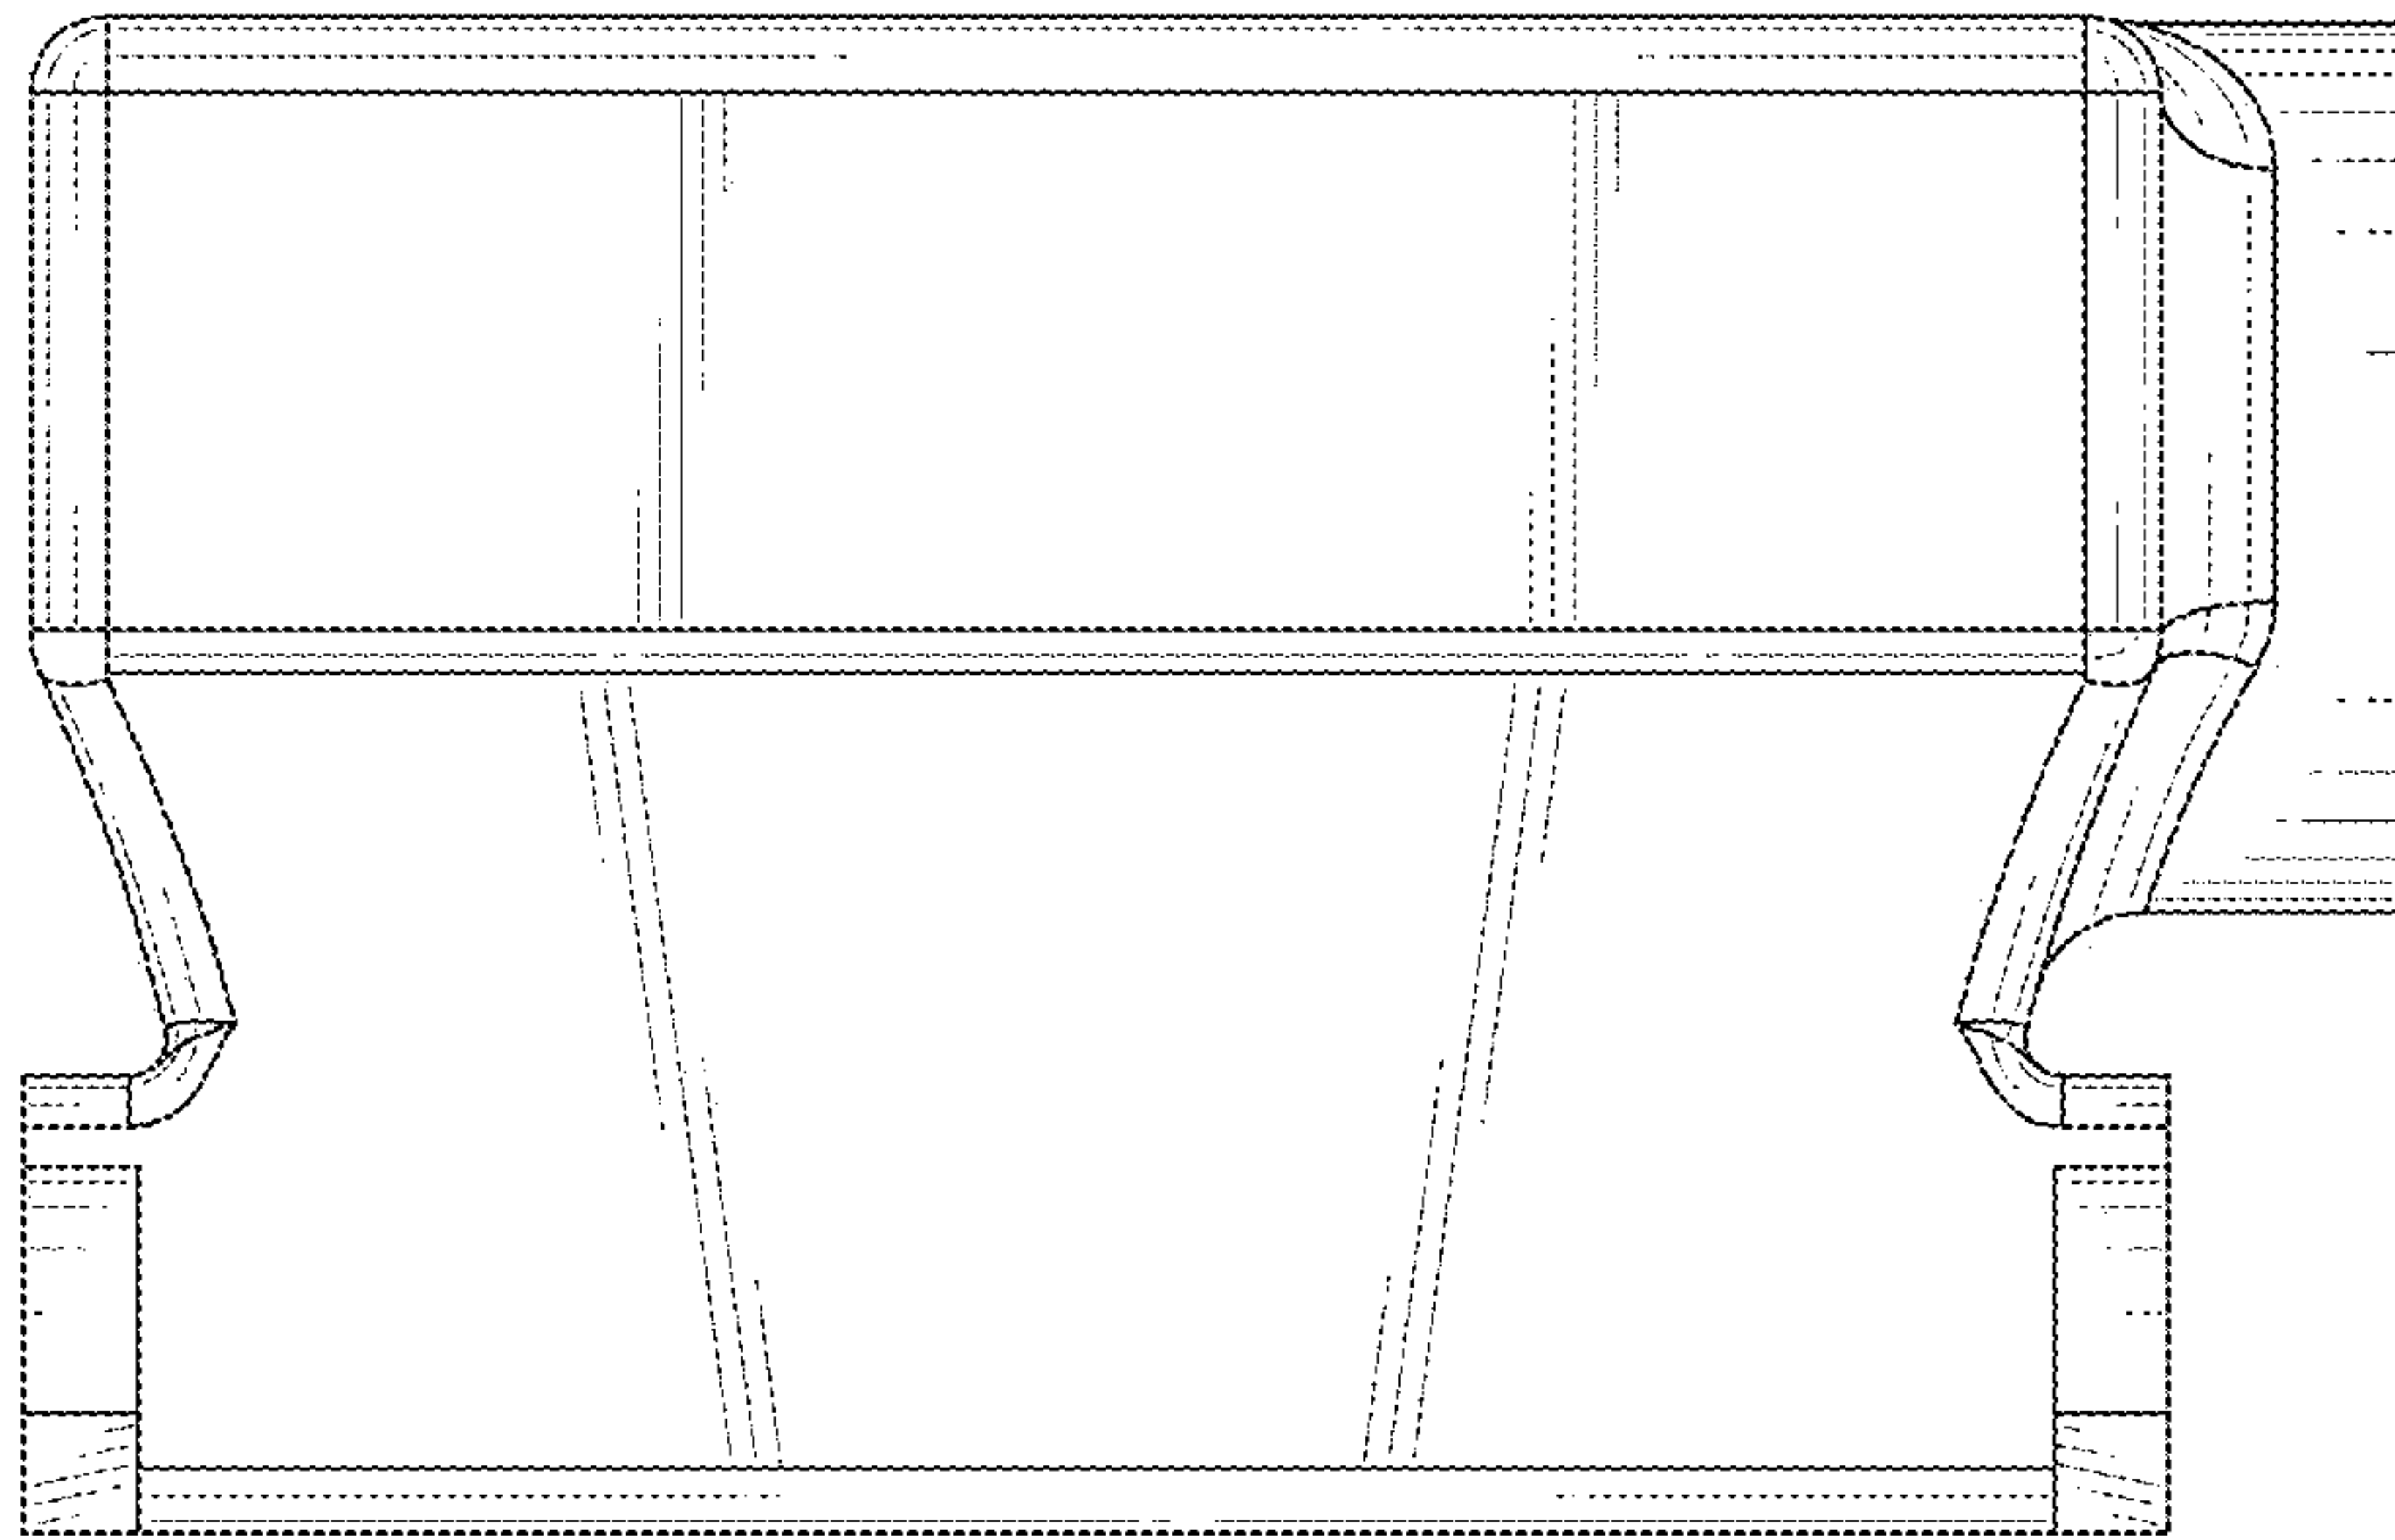


FIG. 6

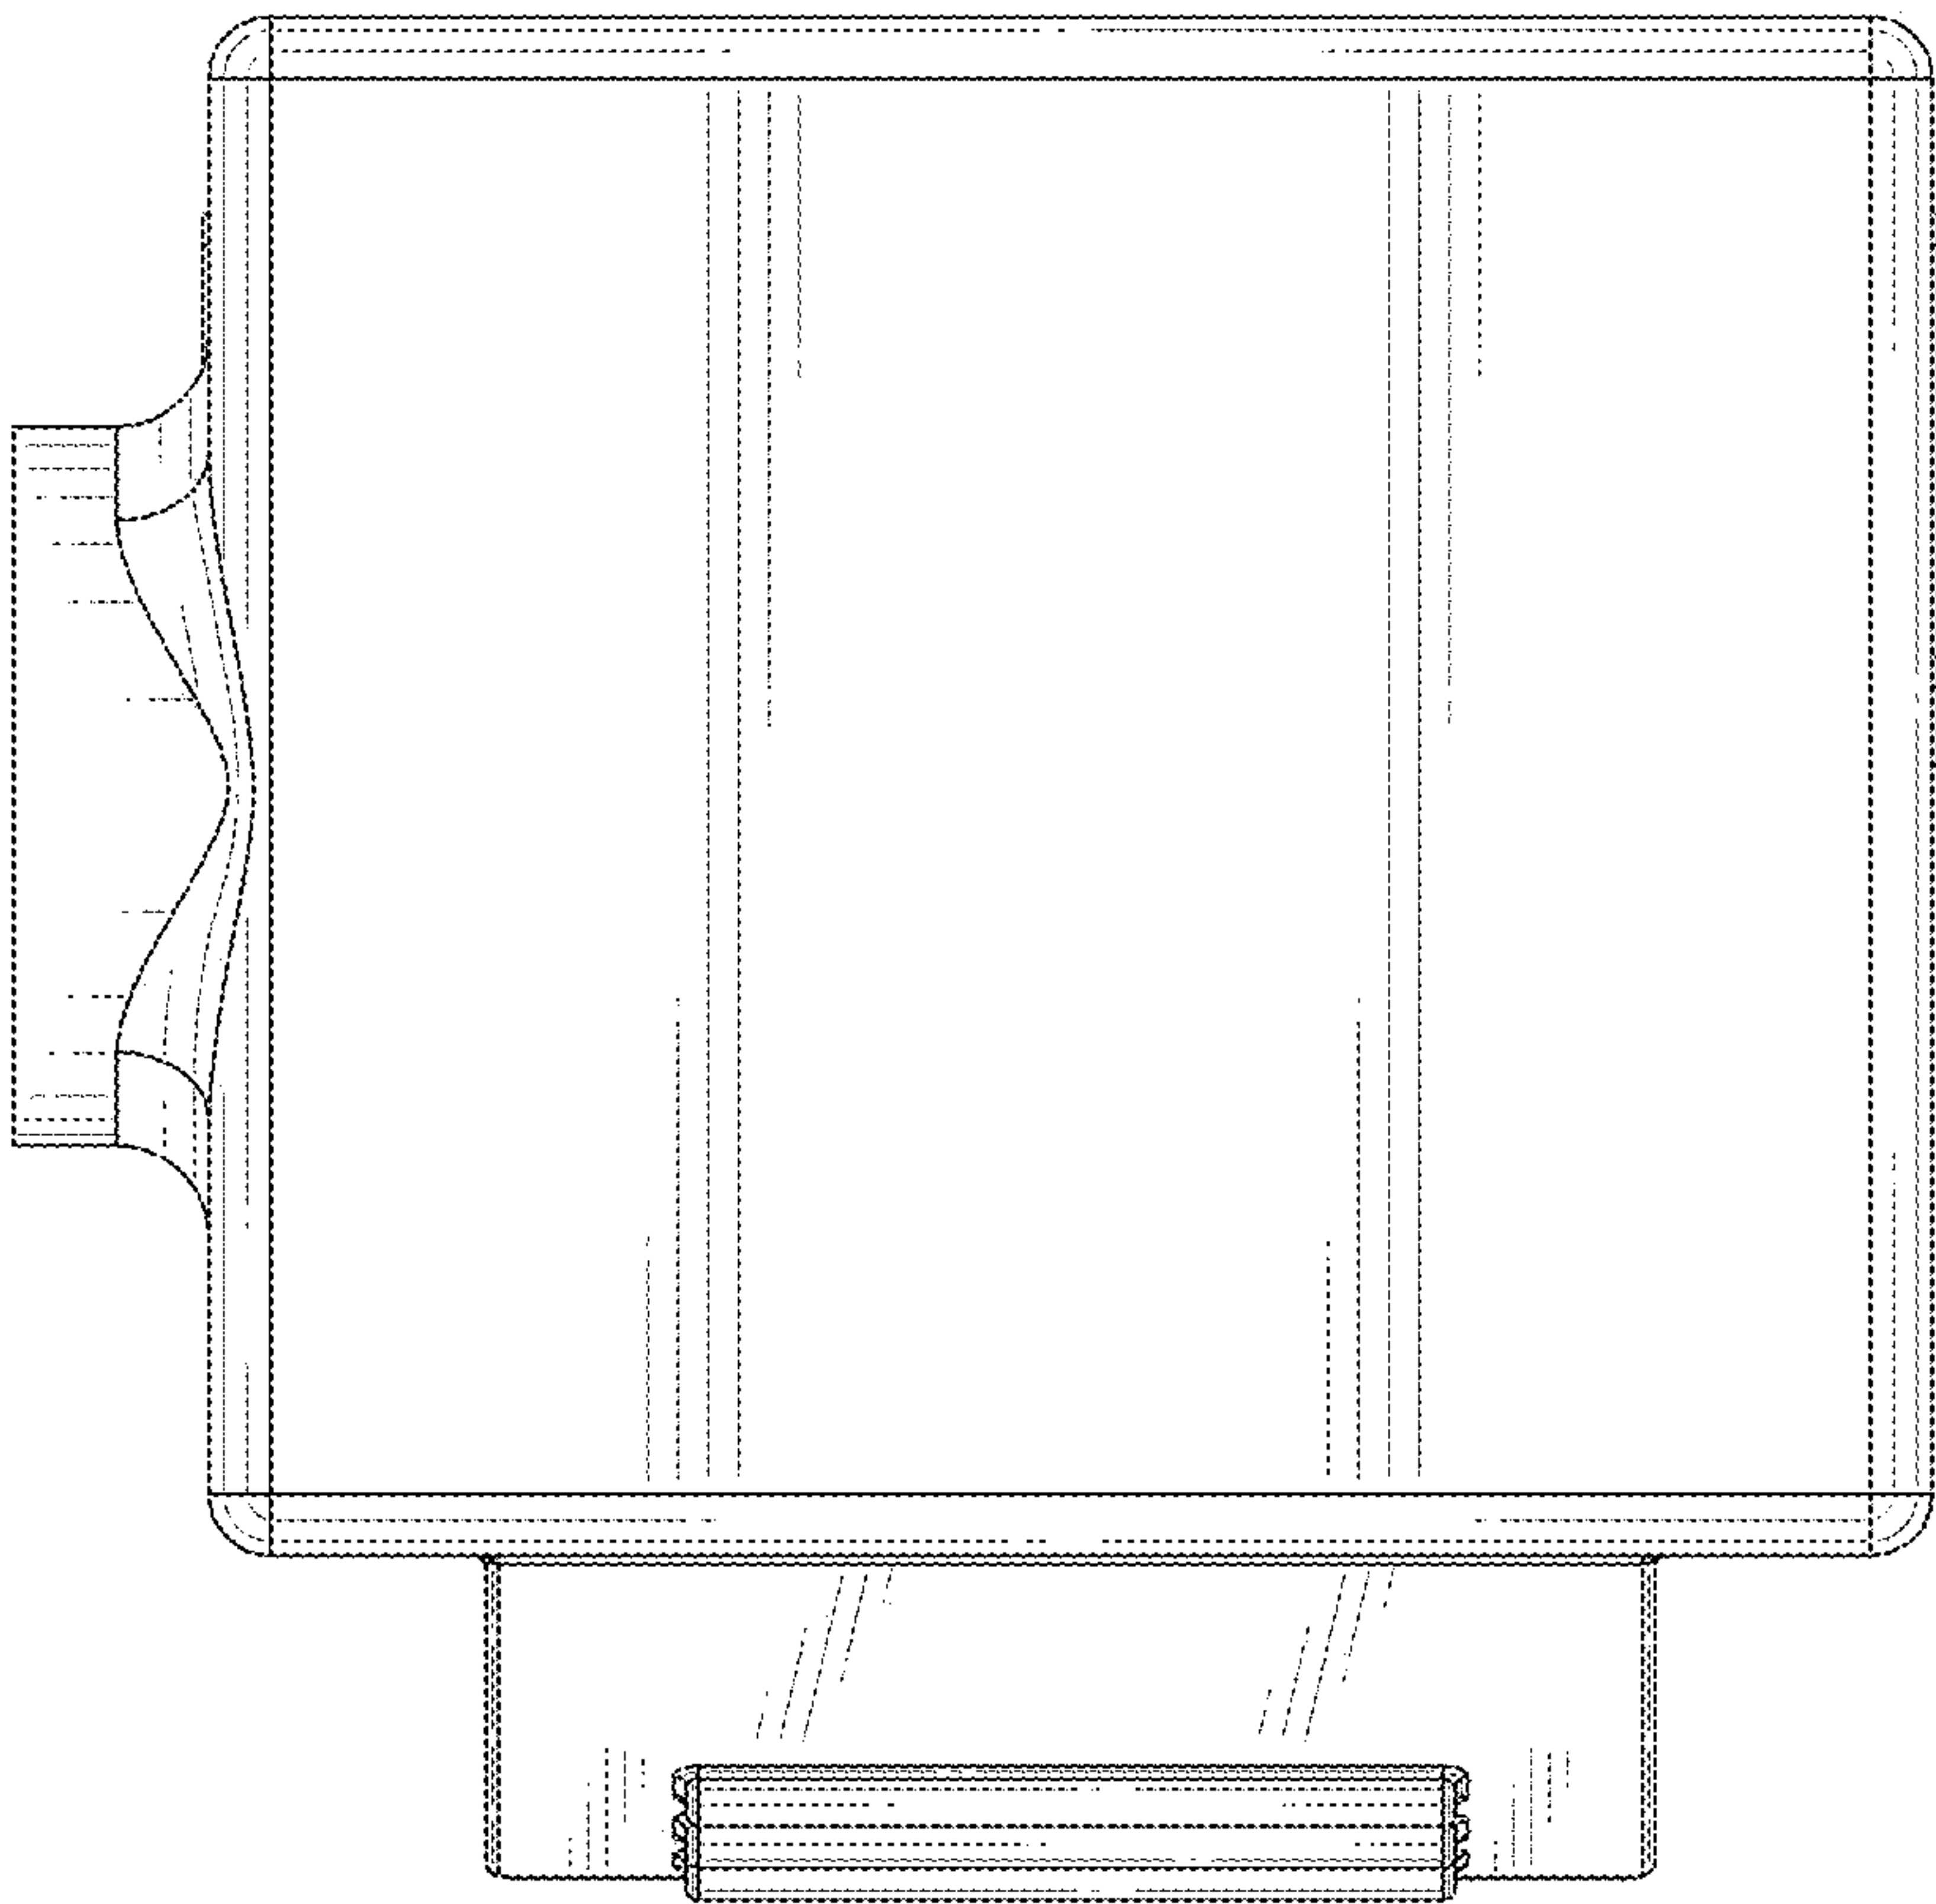


FIG. 7

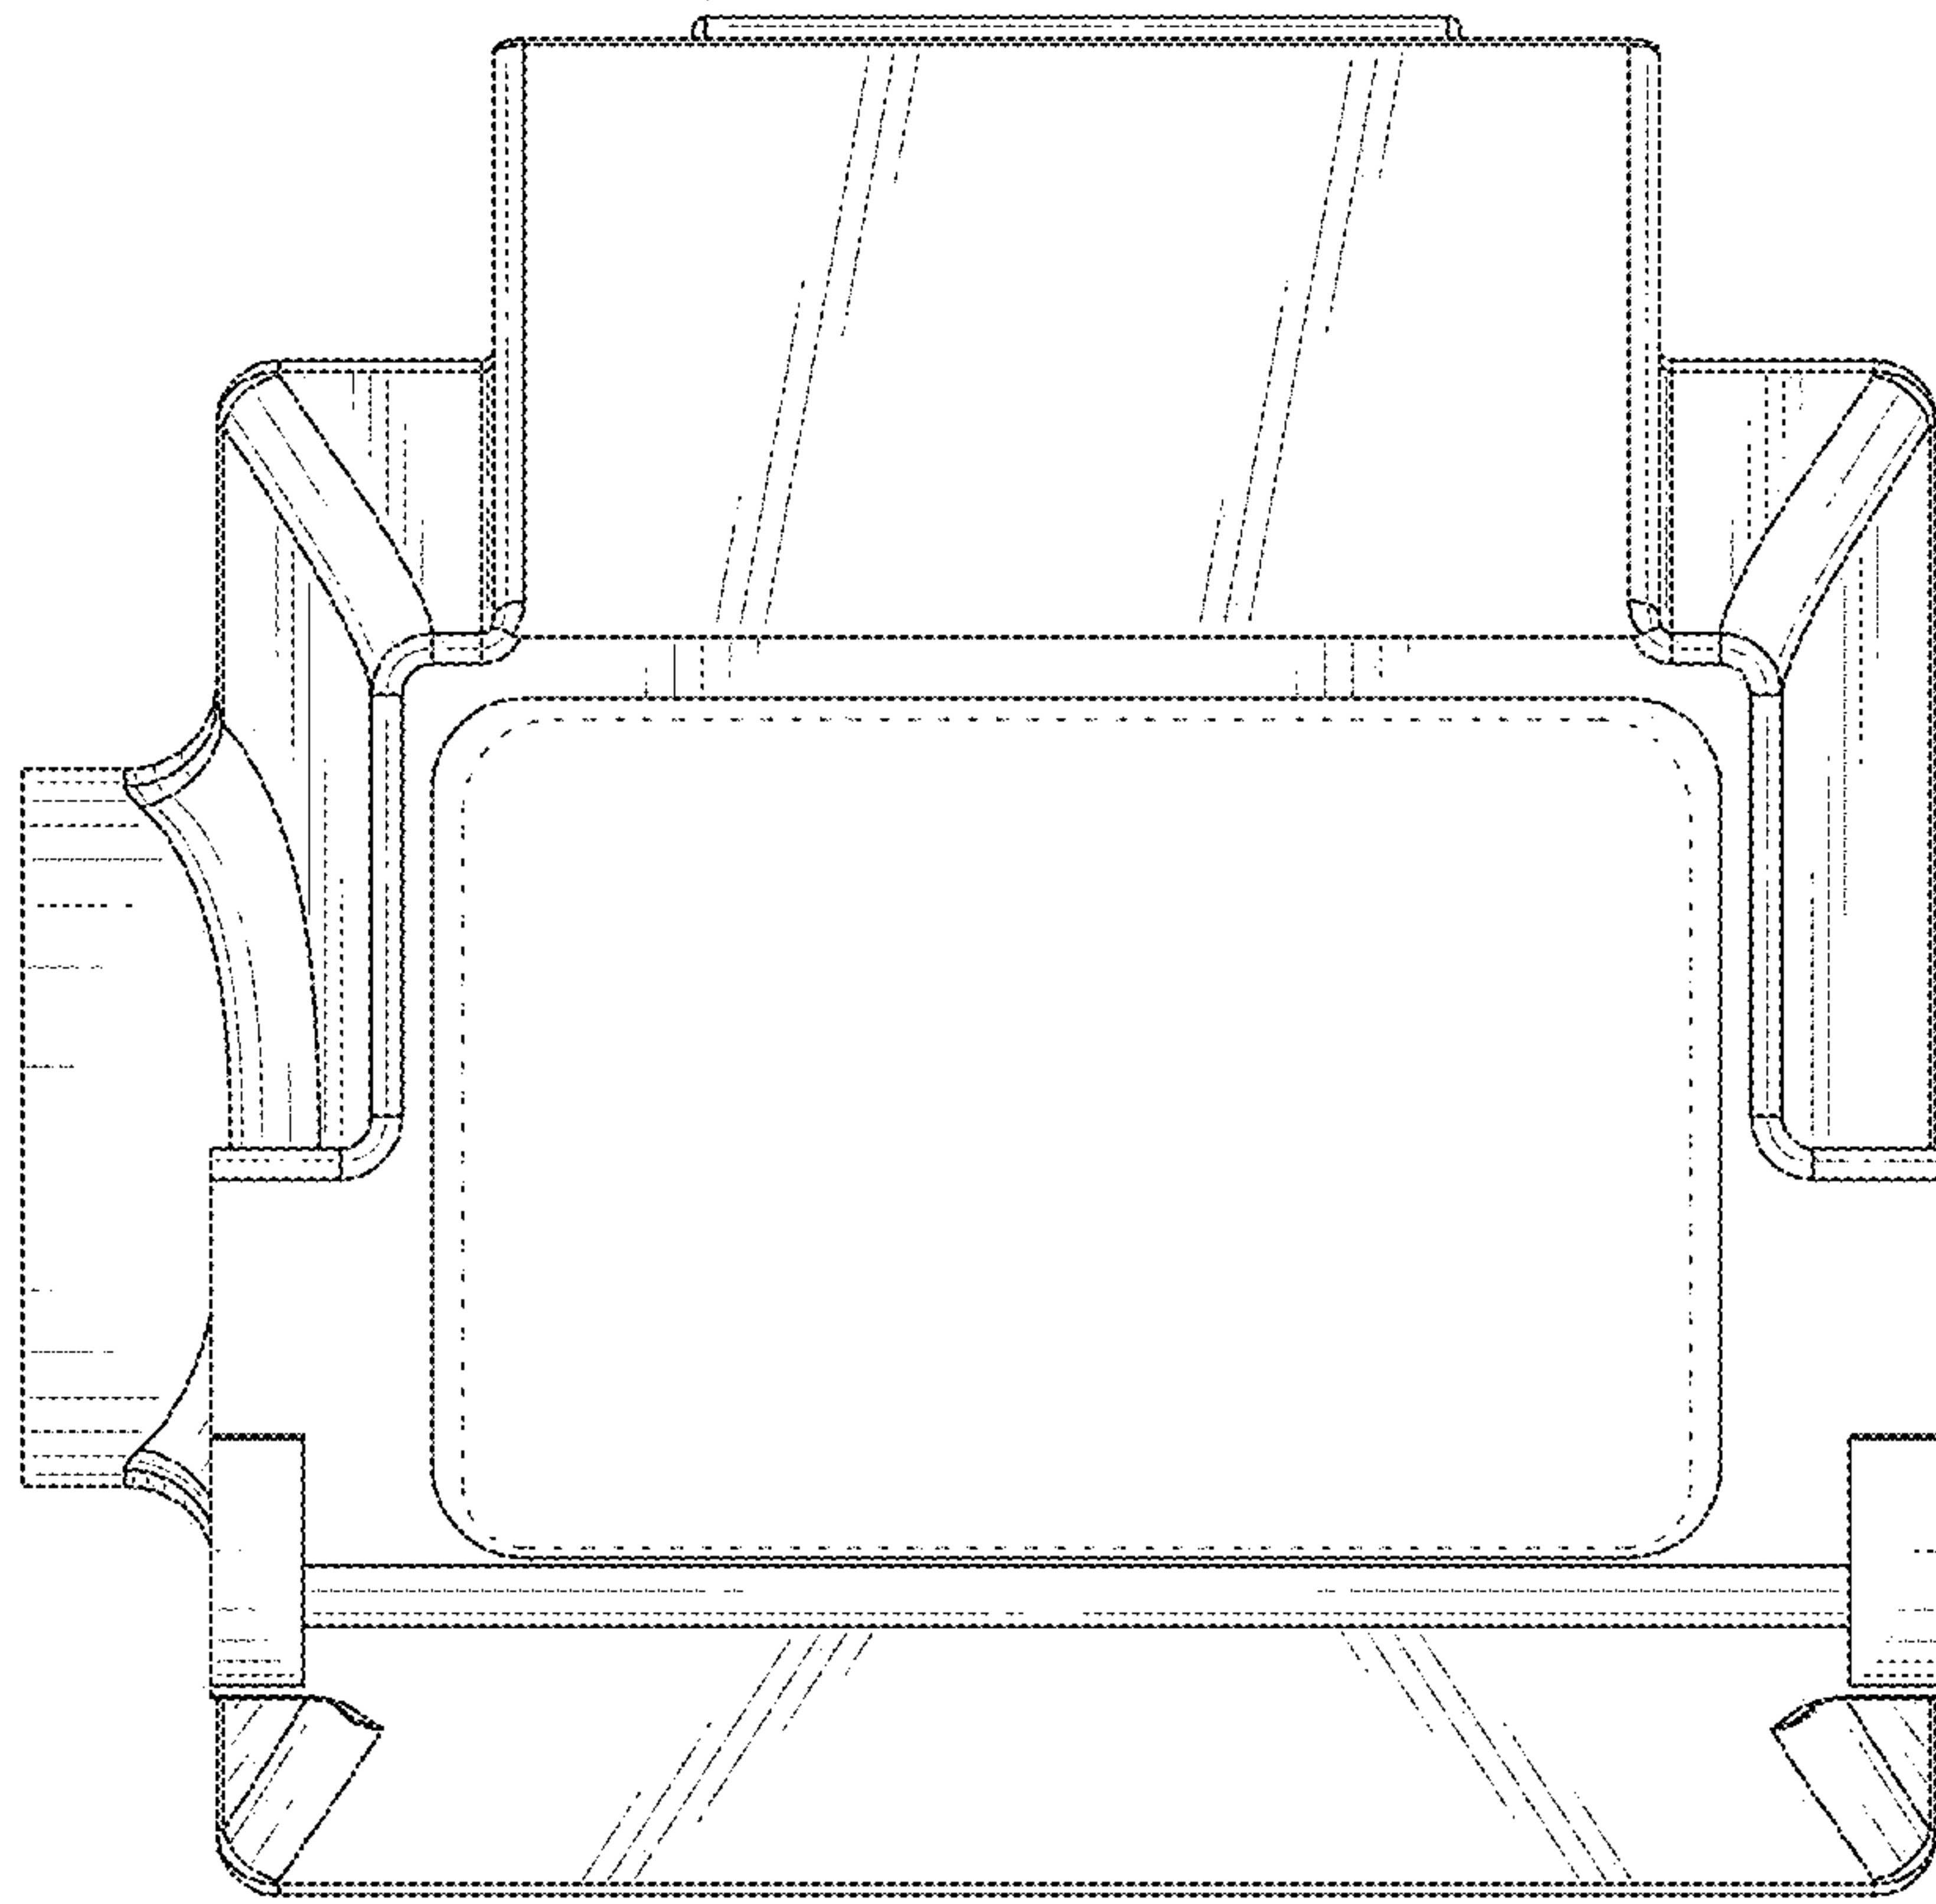


FIG. 8

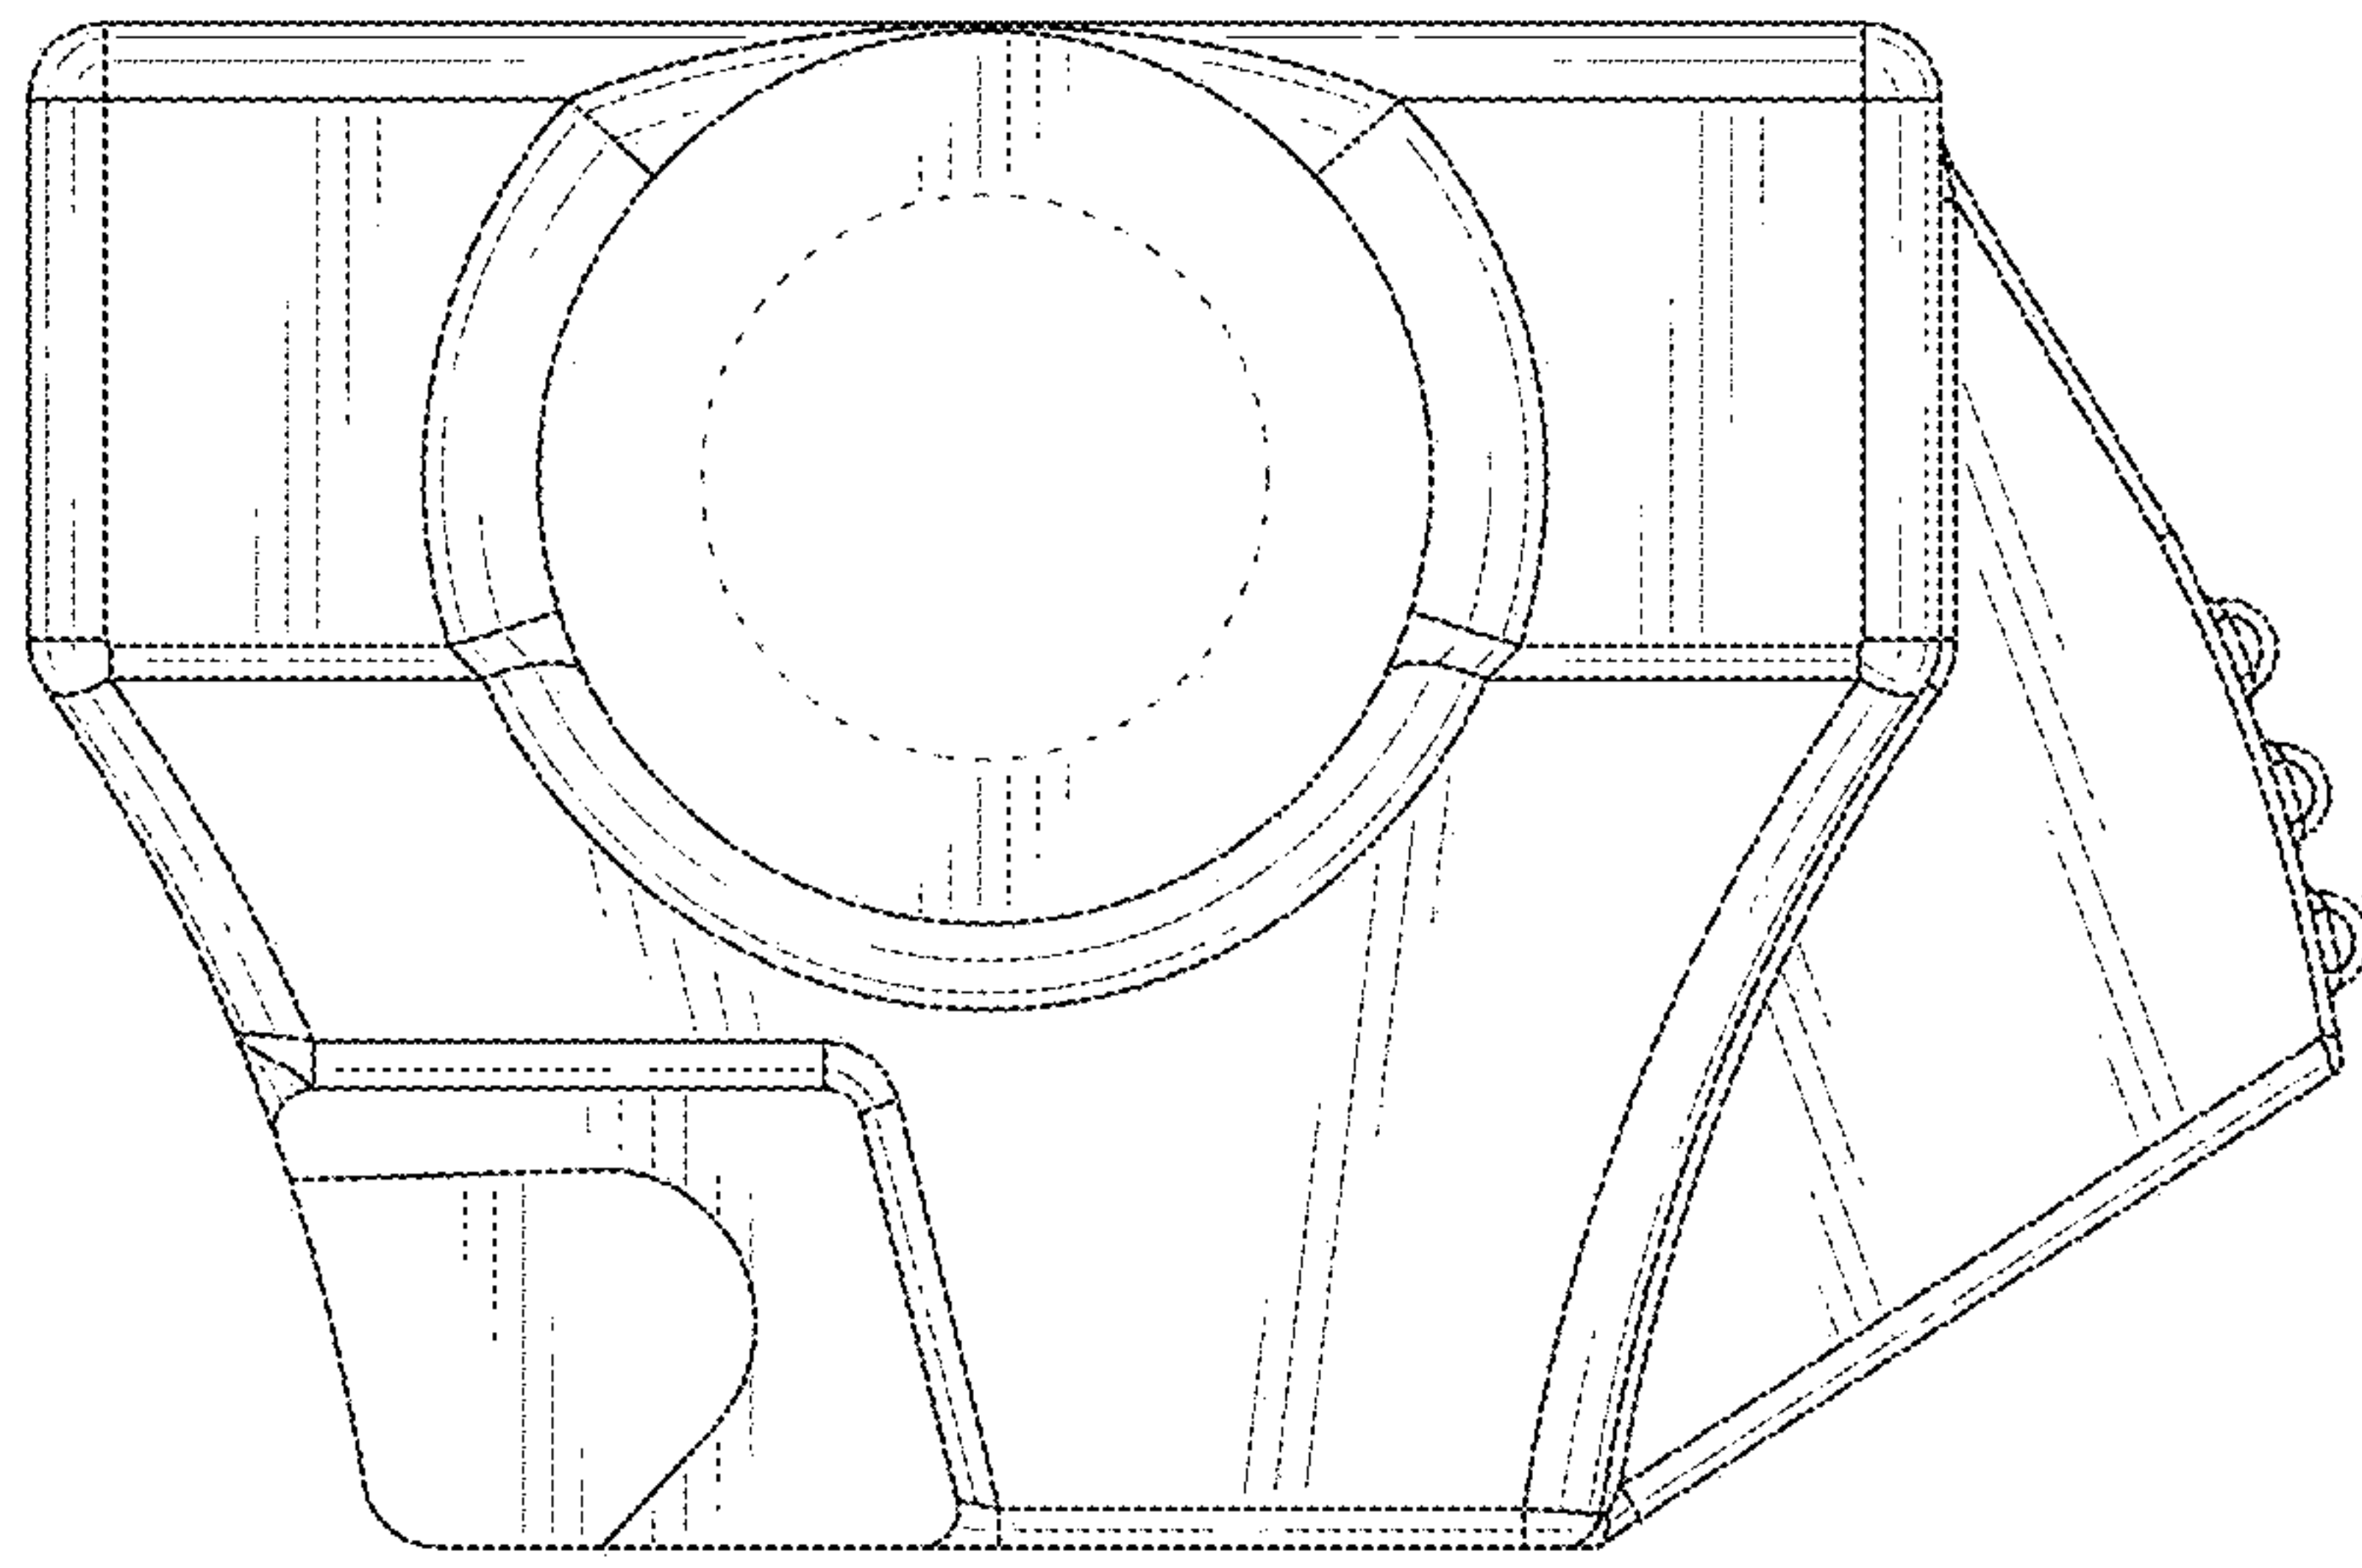


FIG. 9

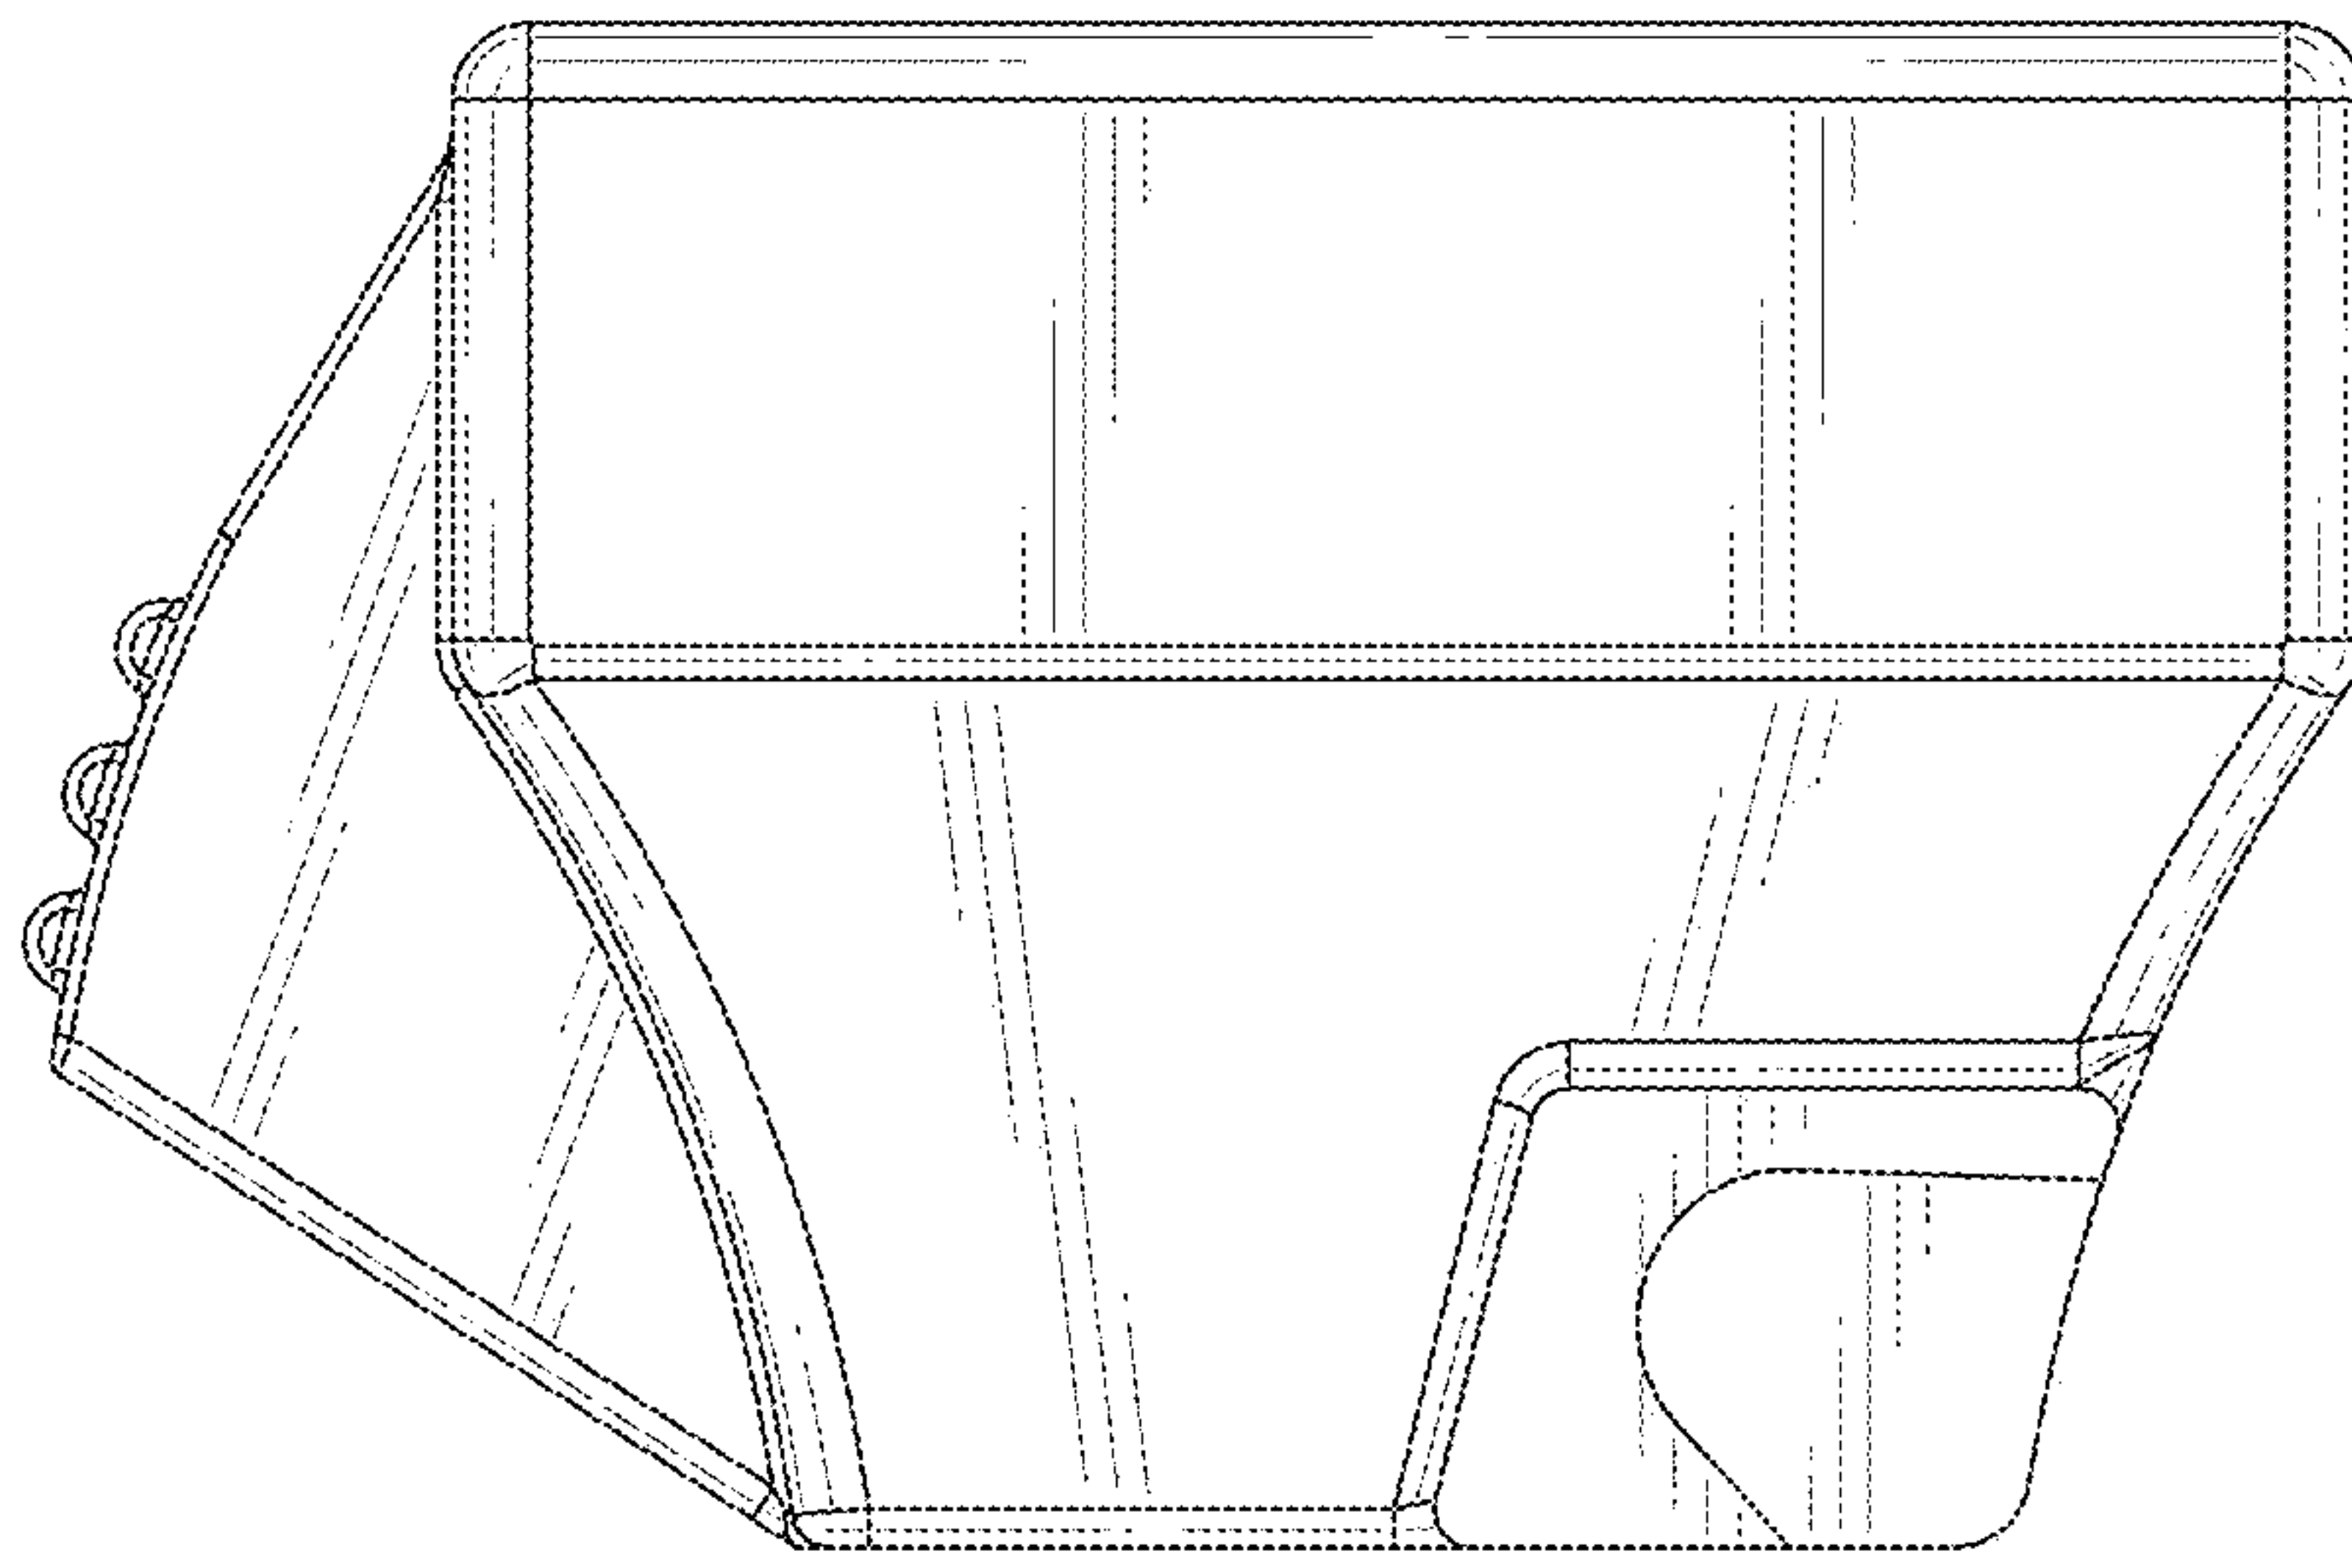


FIG. 10

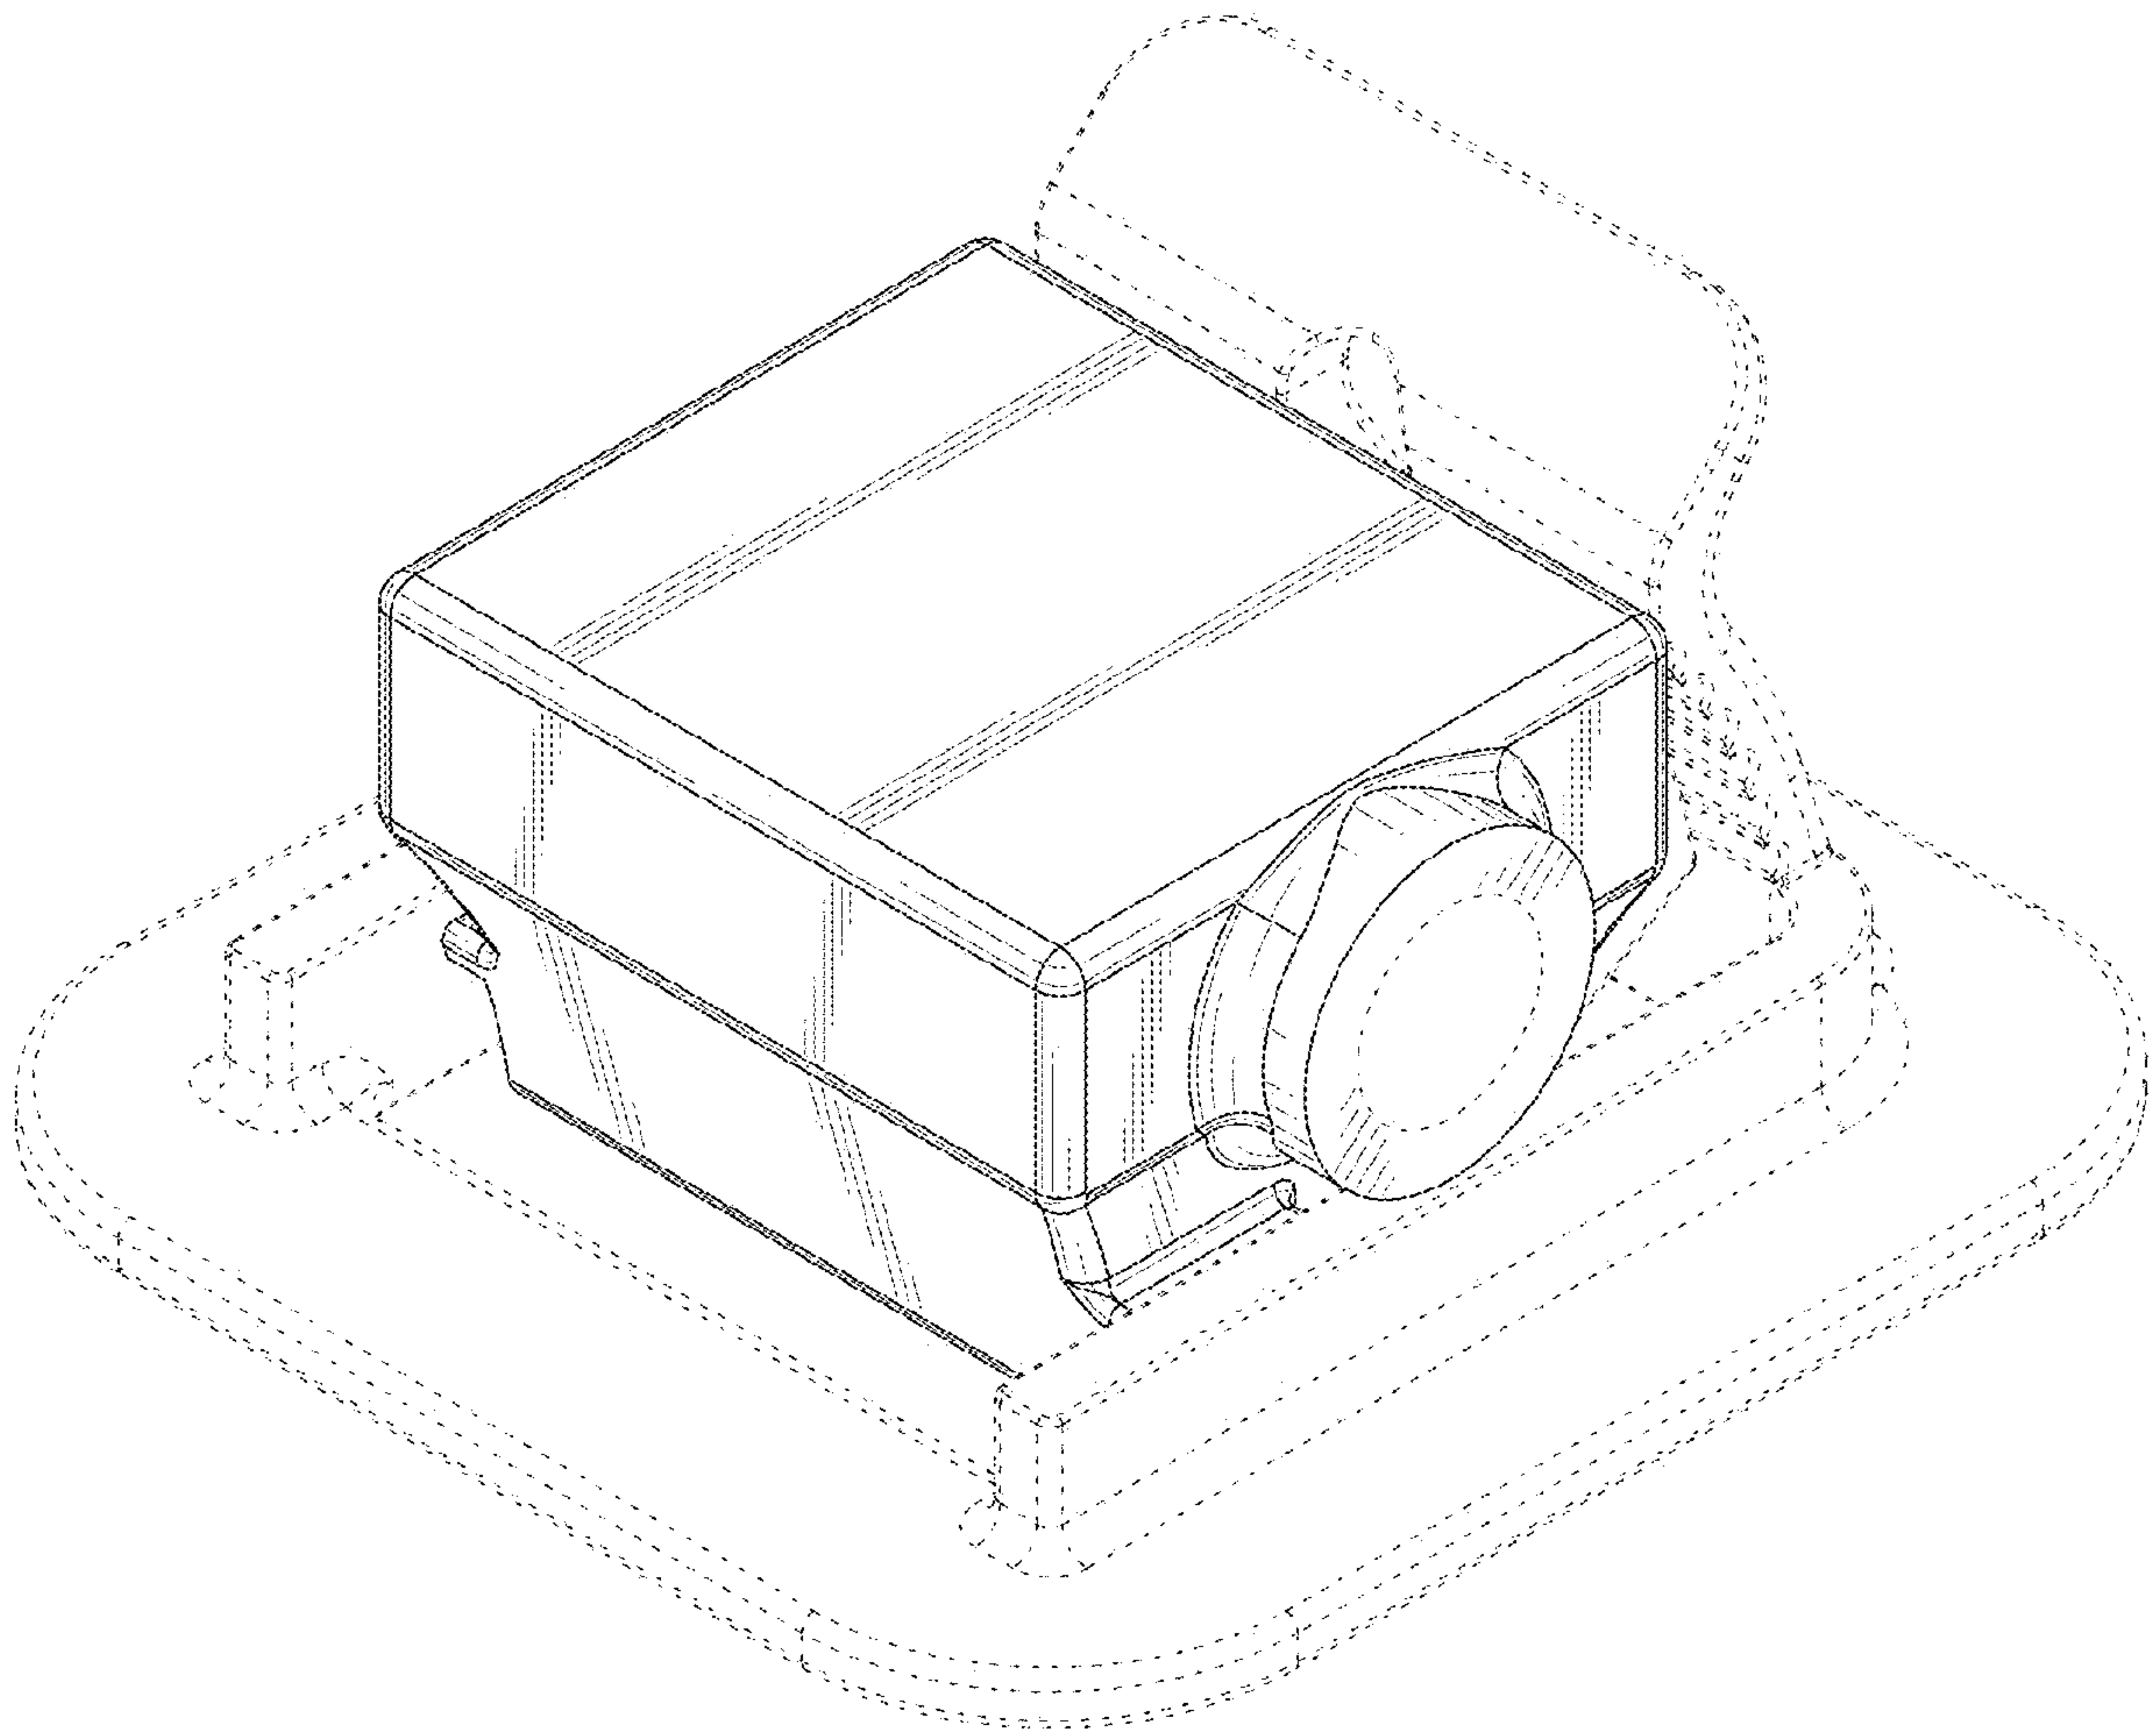


FIG. 11