

(12) **United States Design Patent**
Claudy et al.

(10) **Patent No.:** **US D1,076,136 S**

(45) **Date of Patent:** **** May 20, 2025**

(54) **DIAGNOSTIC DEVICE**

(71) Applicant: **EUROIMMUN Medizinische Labordiagnostika AG**, Luebeck (DE)

(72) Inventors: **Jonas Claudy**, Luebeck (DE); **Lars Warnecke**, Luebeck (DE); **Torsten Grün**, Luebeck (DE)

(73) Assignee: **EUROIMMUN Medizinische Labordiagnostika AG**, Luebeck (DE)

(**) Term: **15 Years**

(21) Appl. No.: **29/792,093**

(22) Filed: **Mar. 3, 2022**

(30) **Foreign Application Priority Data**

Sep. 6, 2021	(EM)	008673909-0001
Sep. 6, 2021	(EM)	008673909-0003
Sep. 6, 2021	(EM)	008673909-0005

(51) **LOC (15) Cl.** **24-02**

(52) **U.S. Cl.**
USPC **D24/216**

(58) **Field of Classification Search**
USPC D24/107, 108, 186, 206, 216, 217, 224, 224/226, 227, 231, 232

(Continued)

(56) **References Cited**

U.S. PATENT DOCUMENTS

D347,478 S	*	5/1994	Pinkney		D24/232
D491,272 S	*	6/2004	Alden		D24/232

(Continued)

FOREIGN PATENT DOCUMENTS

CN	306740017	*	8/2021
CN	308452632	*	2/2024
JP	D1590894	*	11/2017

OTHER PUBLICATIONS

“Medlab Series: Euroimmun at Medlab Middle East 2022.” Found online Mar. 28, 2024 at youtube.com. Reference dated Jan. 13, 2022. Retrieved from <https://www.youtube.com/watch?app=desktop&v=2EWKWvaLzPY>.*

(Continued)

Primary Examiner — Kendra Leslie Hamilton
Assistant Examiner — Elizabeth S Struble
(74) *Attorney, Agent, or Firm* — Grüneberg and Myers PLLC

(57) **CLAIM**

The ornamental design for a diagnostic device, as shown and described.

DESCRIPTION

The patent or application file contains at least one drawing executed in color. Copies of this patent or patent application publication with color drawing(s) will be provided by the Office upon request and payment of the necessary fee.

FIG. 1 is a front left perspective view of a first embodiment of a diagnostic device;

FIG. 2 is a front elevational view thereof;

FIG. 3 is a rear elevational view thereof;

FIG. 4 is a left elevational view thereof;

FIG. 5 is a right elevational view thereof;

FIG. 6 is a top plan view thereof;

FIG. 7 is a bottom plan view thereof;

FIG. 8 is a front left perspective view of a second embodiment of a diagnostic device;

FIG. 9 is a front elevational view thereof;

FIG. 10 is a rear elevational view thereof;

FIG. 11 is a left elevational view thereof;

FIG. 12 is a right elevational view thereof;

FIG. 13 is a top plan view thereof;

FIG. 14 is a bottom plan view thereof;

FIG. 15 is a front left perspective view of a third embodiment of a diagnostic device;

FIG. 16 is a front elevational view thereof;

FIG. 17 is a rear elevational view thereof;

FIG. 18 is a left elevational view thereof;

(Continued)

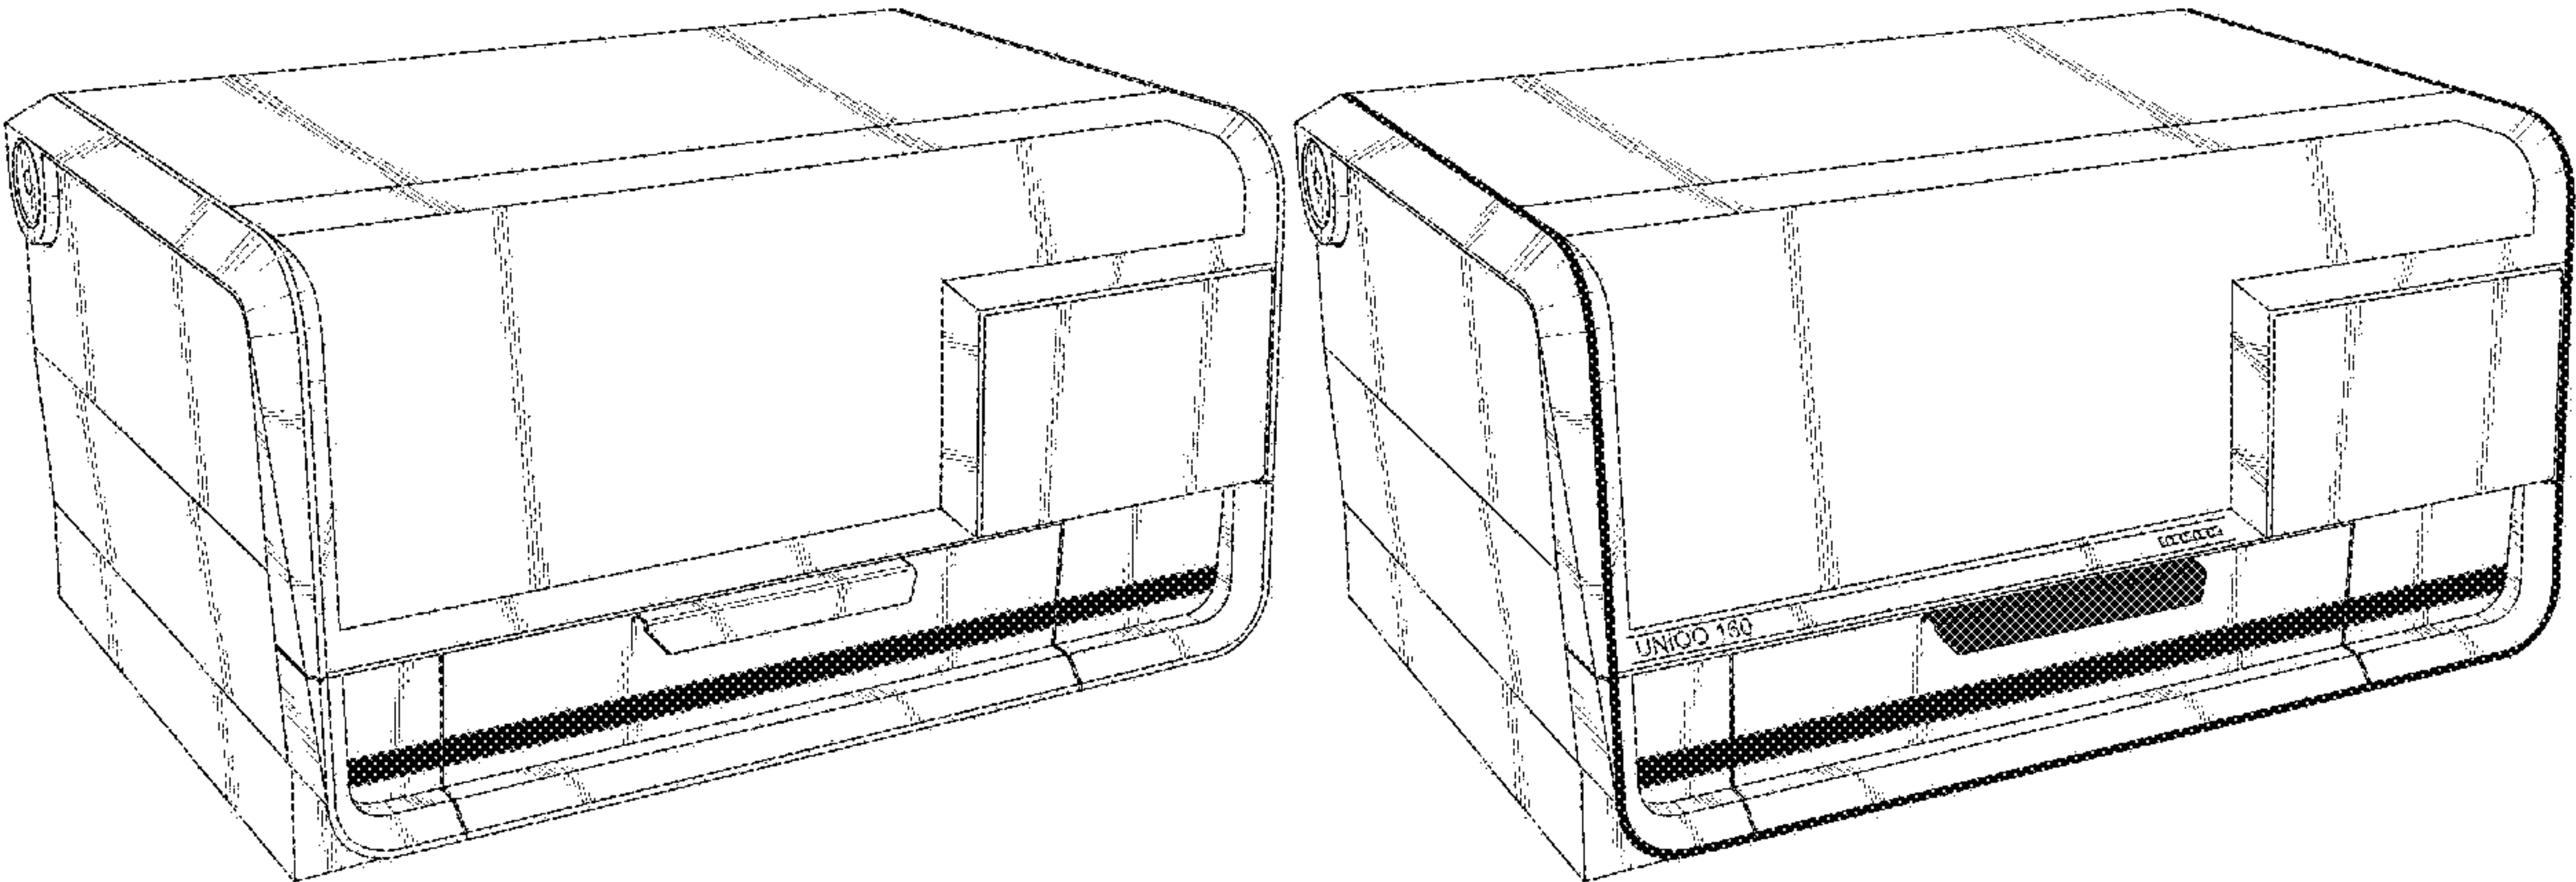


FIG. 19 is a right elevational view thereof;
FIG. 20 is a top plan view thereof; and,
FIG. 21 is a bottom plan view thereof.
In the drawings, the equal-length broken lines depict portions of the diagnostic device that form no part of the claimed design.

1 Claim, 21 Drawing Sheets
(3 of 21 Drawing Sheet(s) Filed in Color)

(58) Field of Classification Search

CPC .. B01L 3/021; B01L 3/058; B01L 3/52; B01L 3/5085; B01L 2200/16; B01L 3/5023; G01N 21/78; G01N 1/38; G01N 21/6428; G01N 33/50; G01N 33/49; C12M 23/08; C12M 23/14; C12M 23/44; C12M 23/46; C12M 23/48; C12M 23/58; A61J 1/2086; A61J 1/2096; A61J 1/2089; A61B 5/0006; A61B 5/0205

See application file for complete search history.

(56) References Cited

U.S. PATENT DOCUMENTS

D591,864 S *	5/2009	Schmidt	D24/216
D670,402 S *	11/2012	Shibata	D24/216
D687,141 S *	7/2013	Schneider	D24/111
D719,861 S *	12/2014	Kawai	D24/232
D850,310 S *	6/2019	Kang	D24/216
D874,017 S *	1/2020	Jenoski	D24/216
D896,981 S	9/2020	Gruen et al.	
D907,245 S	1/2021	Rateike et al.	
D914,230 S	3/2021	Kaffka et al.	
D936,855 S	11/2021	Huth et al.	
11,385,448 B2 *	7/2022	Okada	G02B 21/16
D1,019,440 S *	3/2024	Jablonski	D24/216
D1,019,441 S *	3/2024	Hasebe	D24/216
2017/0003310 A1 *	1/2017	Shohmi	G01N 35/00584
2022/0202648 A1 *	6/2022	Berger	B01F 23/565

OTHER PUBLICATIONS

“Medical Lab Management: Benchtop Instrument for Slide Processing.” Found online at medlabmag.com. Reference dated Oct. 2023. Retrieved from https://www.medlabmag.com/new_noteworthy/?noteid=1631.*
“Euroimmun: EUROArrayProcessor.” Found online Mar. 1, 2024 at youtube.com. Reference dated Apr. 14, 2022. Retrieved from https://www.youtube.com/watch?v=OC8apfQ_pb4.*
“Euroimmun Polska: EUROMicroblot.” Found online Mar. 28, 2024 at euroimmun.pl. Reference dated Oct. 24, 2022. Retrieved from <https://www.euroimmun.pl/mikrobloty-w-diagnostyce-boreliozy-nowosc/>.*
Huth et al., “Graphic designs[two-dimensional]”, Euroimmun Medizinische Labordiagnostika AG, Germany, filed Jun. 5, 2018, European Union Intellectual Property Organization design No. 005297595-0001.
Gruen et al., “Apparatus and installations for medical or laboratory diagnosis”, Euroimmun Medizinische Labordiagnostika AG, Germany, filed Jul. 20, 2018, European Union Intellectual Property Organization design Nos. 005508876-0001, 005508876-0002, 005508876-0003, 005508876-0004, 005508876-0005, 005508876-0006, 005508876-0007, 005508876-0008, 005508876-0009, 005508876-0010.
Grün et al., “Medical apparatus and equipment [fixed]”, Euroimmun Medizinische Labordiagnostika AG, Germany, filed Feb. 1, 2021, European Union Intellectual Property Organization design Nos. 008419618-0001, 008419618-0002, 008419618-0003, 008419618-0004, 008419618-0005, 008419618-0006, 008419618-0007, 008419618-0008, 008419618-0009.
Kaffka et al., “Medical apparatus and equipment”, Euroimmun Medizinische Labordiagnostika AG, Germany, filed Sep. 4, 2018, European Union Intellectual Property Organization design Nos. 005628583-0001, 005628583-0002, 005628583-0003, 005628583-0004, 005628583-0005, 005628583-0006, 005628583-0007, 005628583-0008, 005628583-0009, 005628583-0010.
Philipp Bartsch, “Medical apparatus and equipment [fixed]”, Euroimmun Medizinische Labordiagnostika AG, Germany, filed Apr. 9, 2018, European Union Intellectual Property Organization design Nos. 005226958-0001, 005226958-0002, 005226958-0003, 005226958-0004, 005226958-0005, 005226958-0006.
Rateike et al., “Apparatus and equipment for doctors, hospitals and laboratories”, Euroimmun Medizinische Labordiagnostika AG, Germany, filed Mar. 22, 2019, European Union Intellectual Property Organization design Nos. 006319323-0001, 006319323-0002, 006319323-0003, 006319323-0004.
U.S. Appl. No. 29/746,924, filed Aug. 18, 2020, Gruen et al.
U.S. Appl. No. 29/801,362, filed Jul. 28, 2021, Grün et al.

* cited by examiner

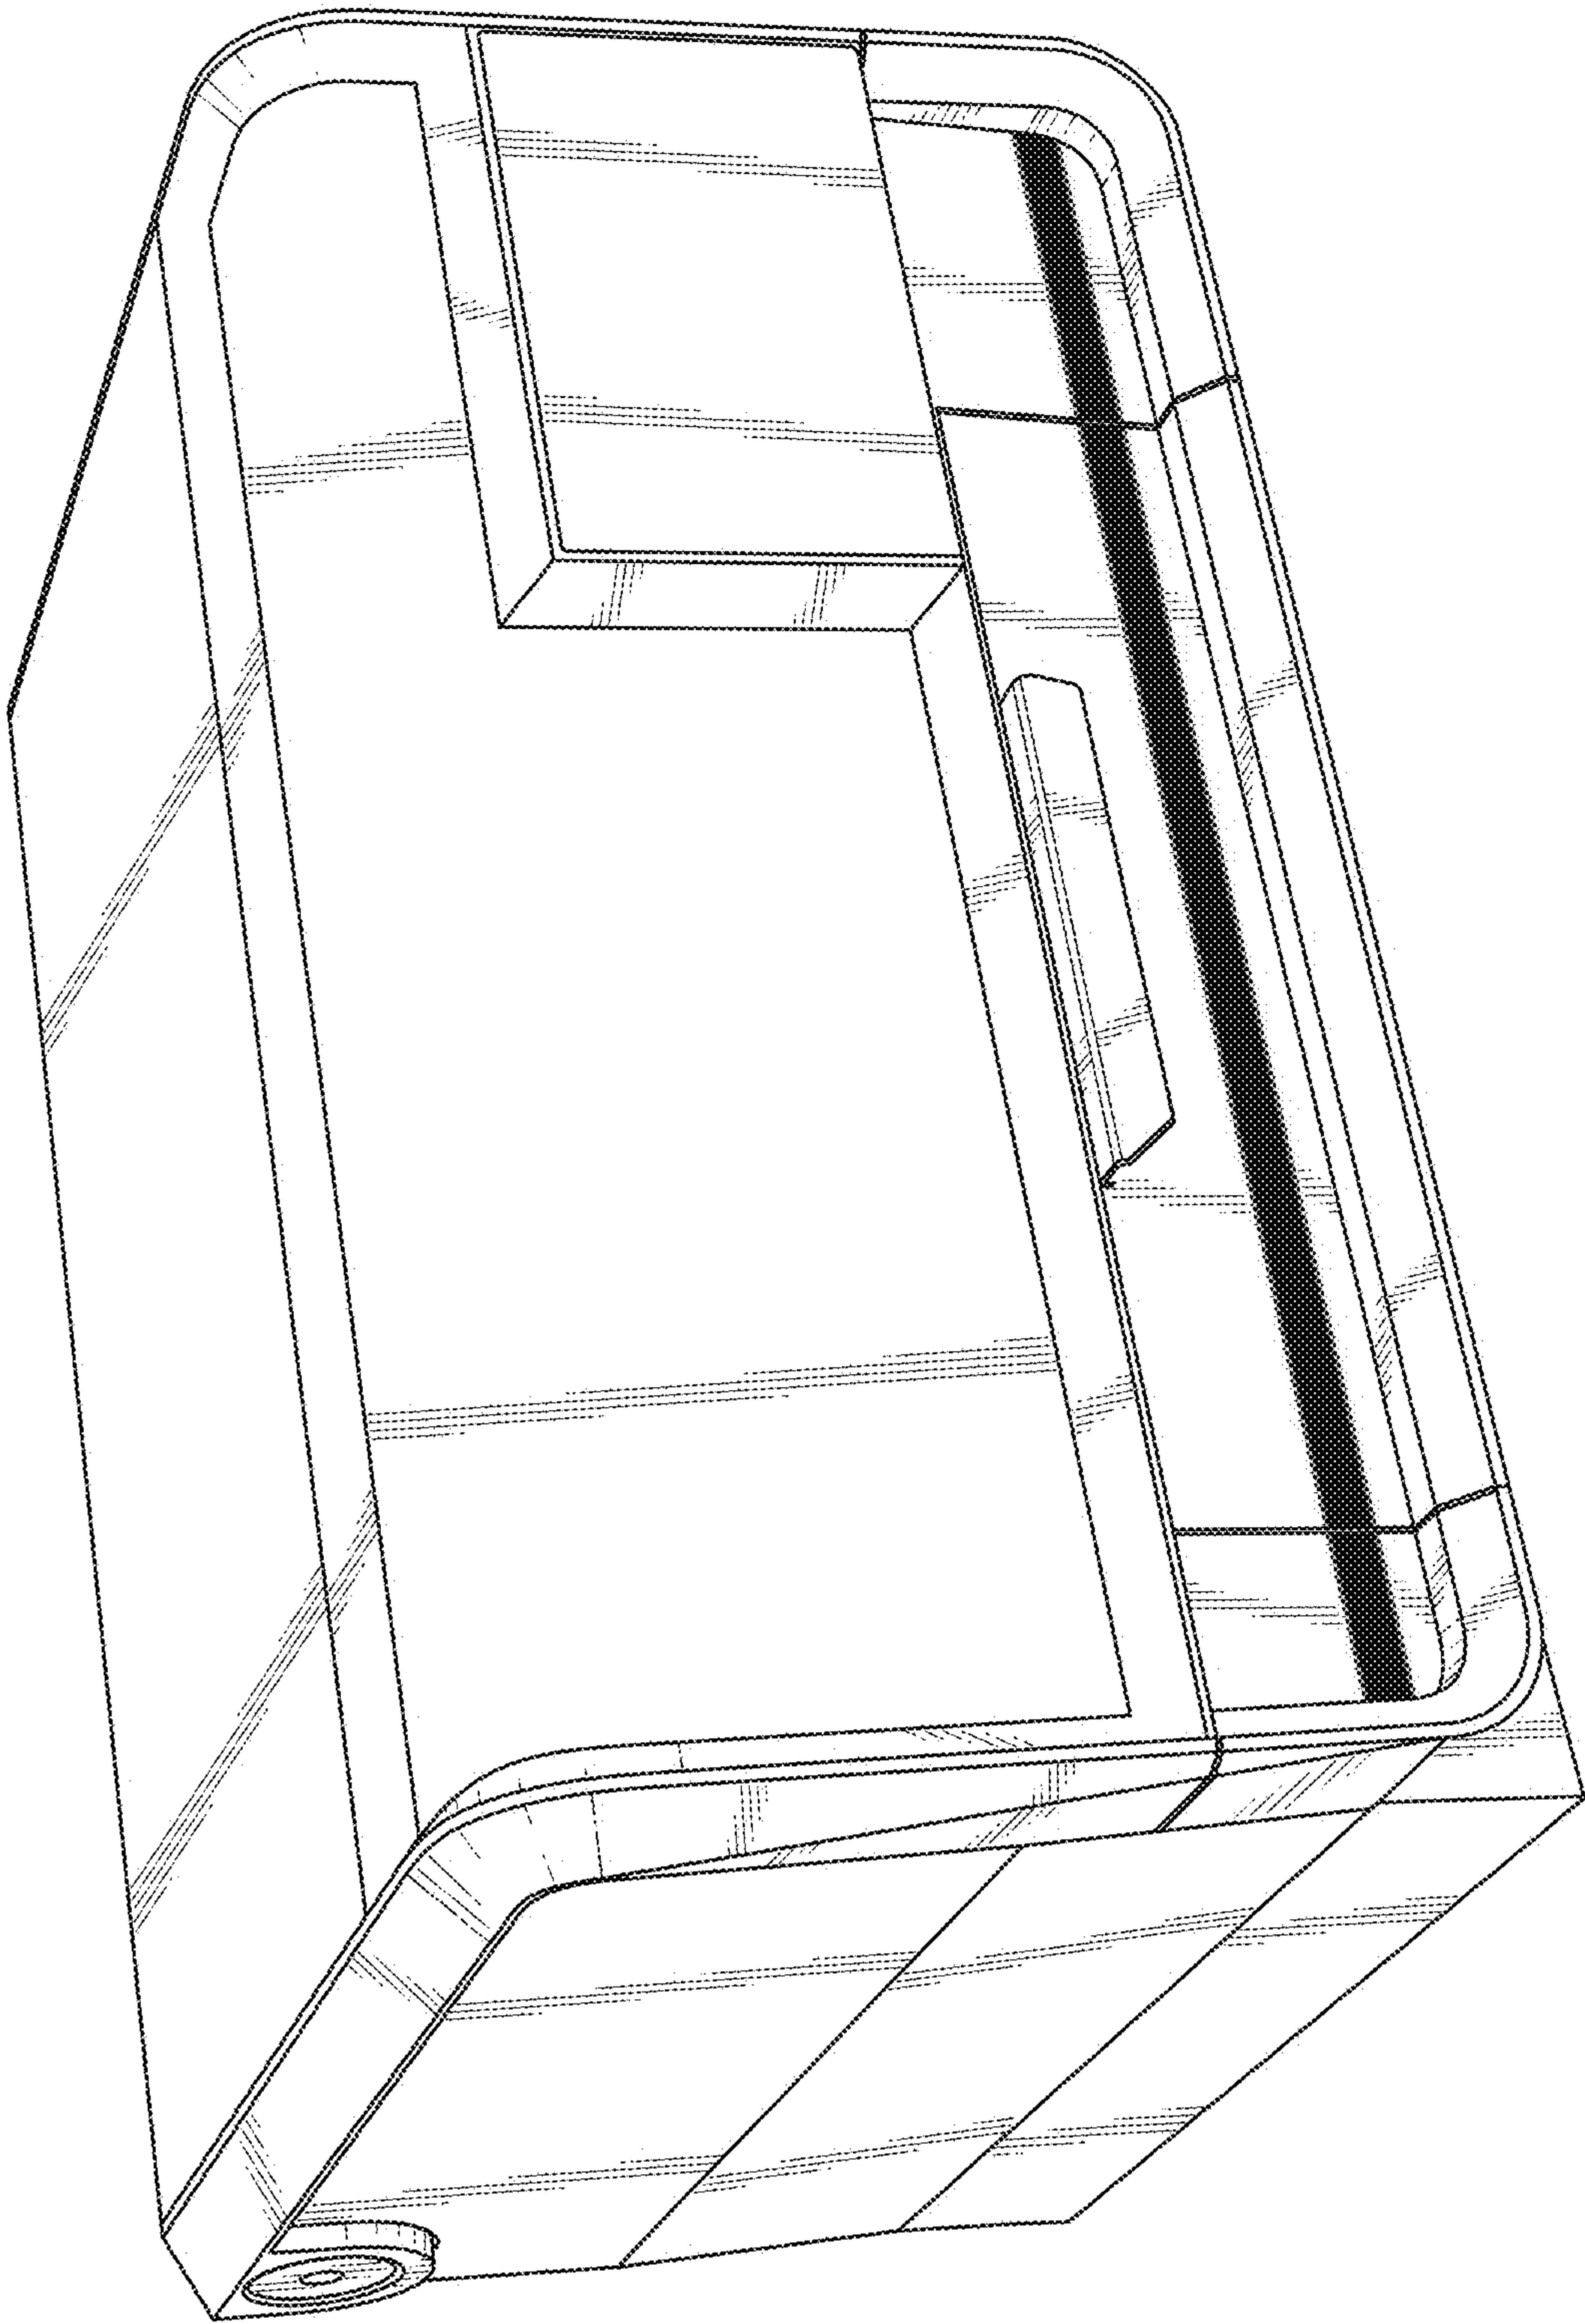


FIG. 1

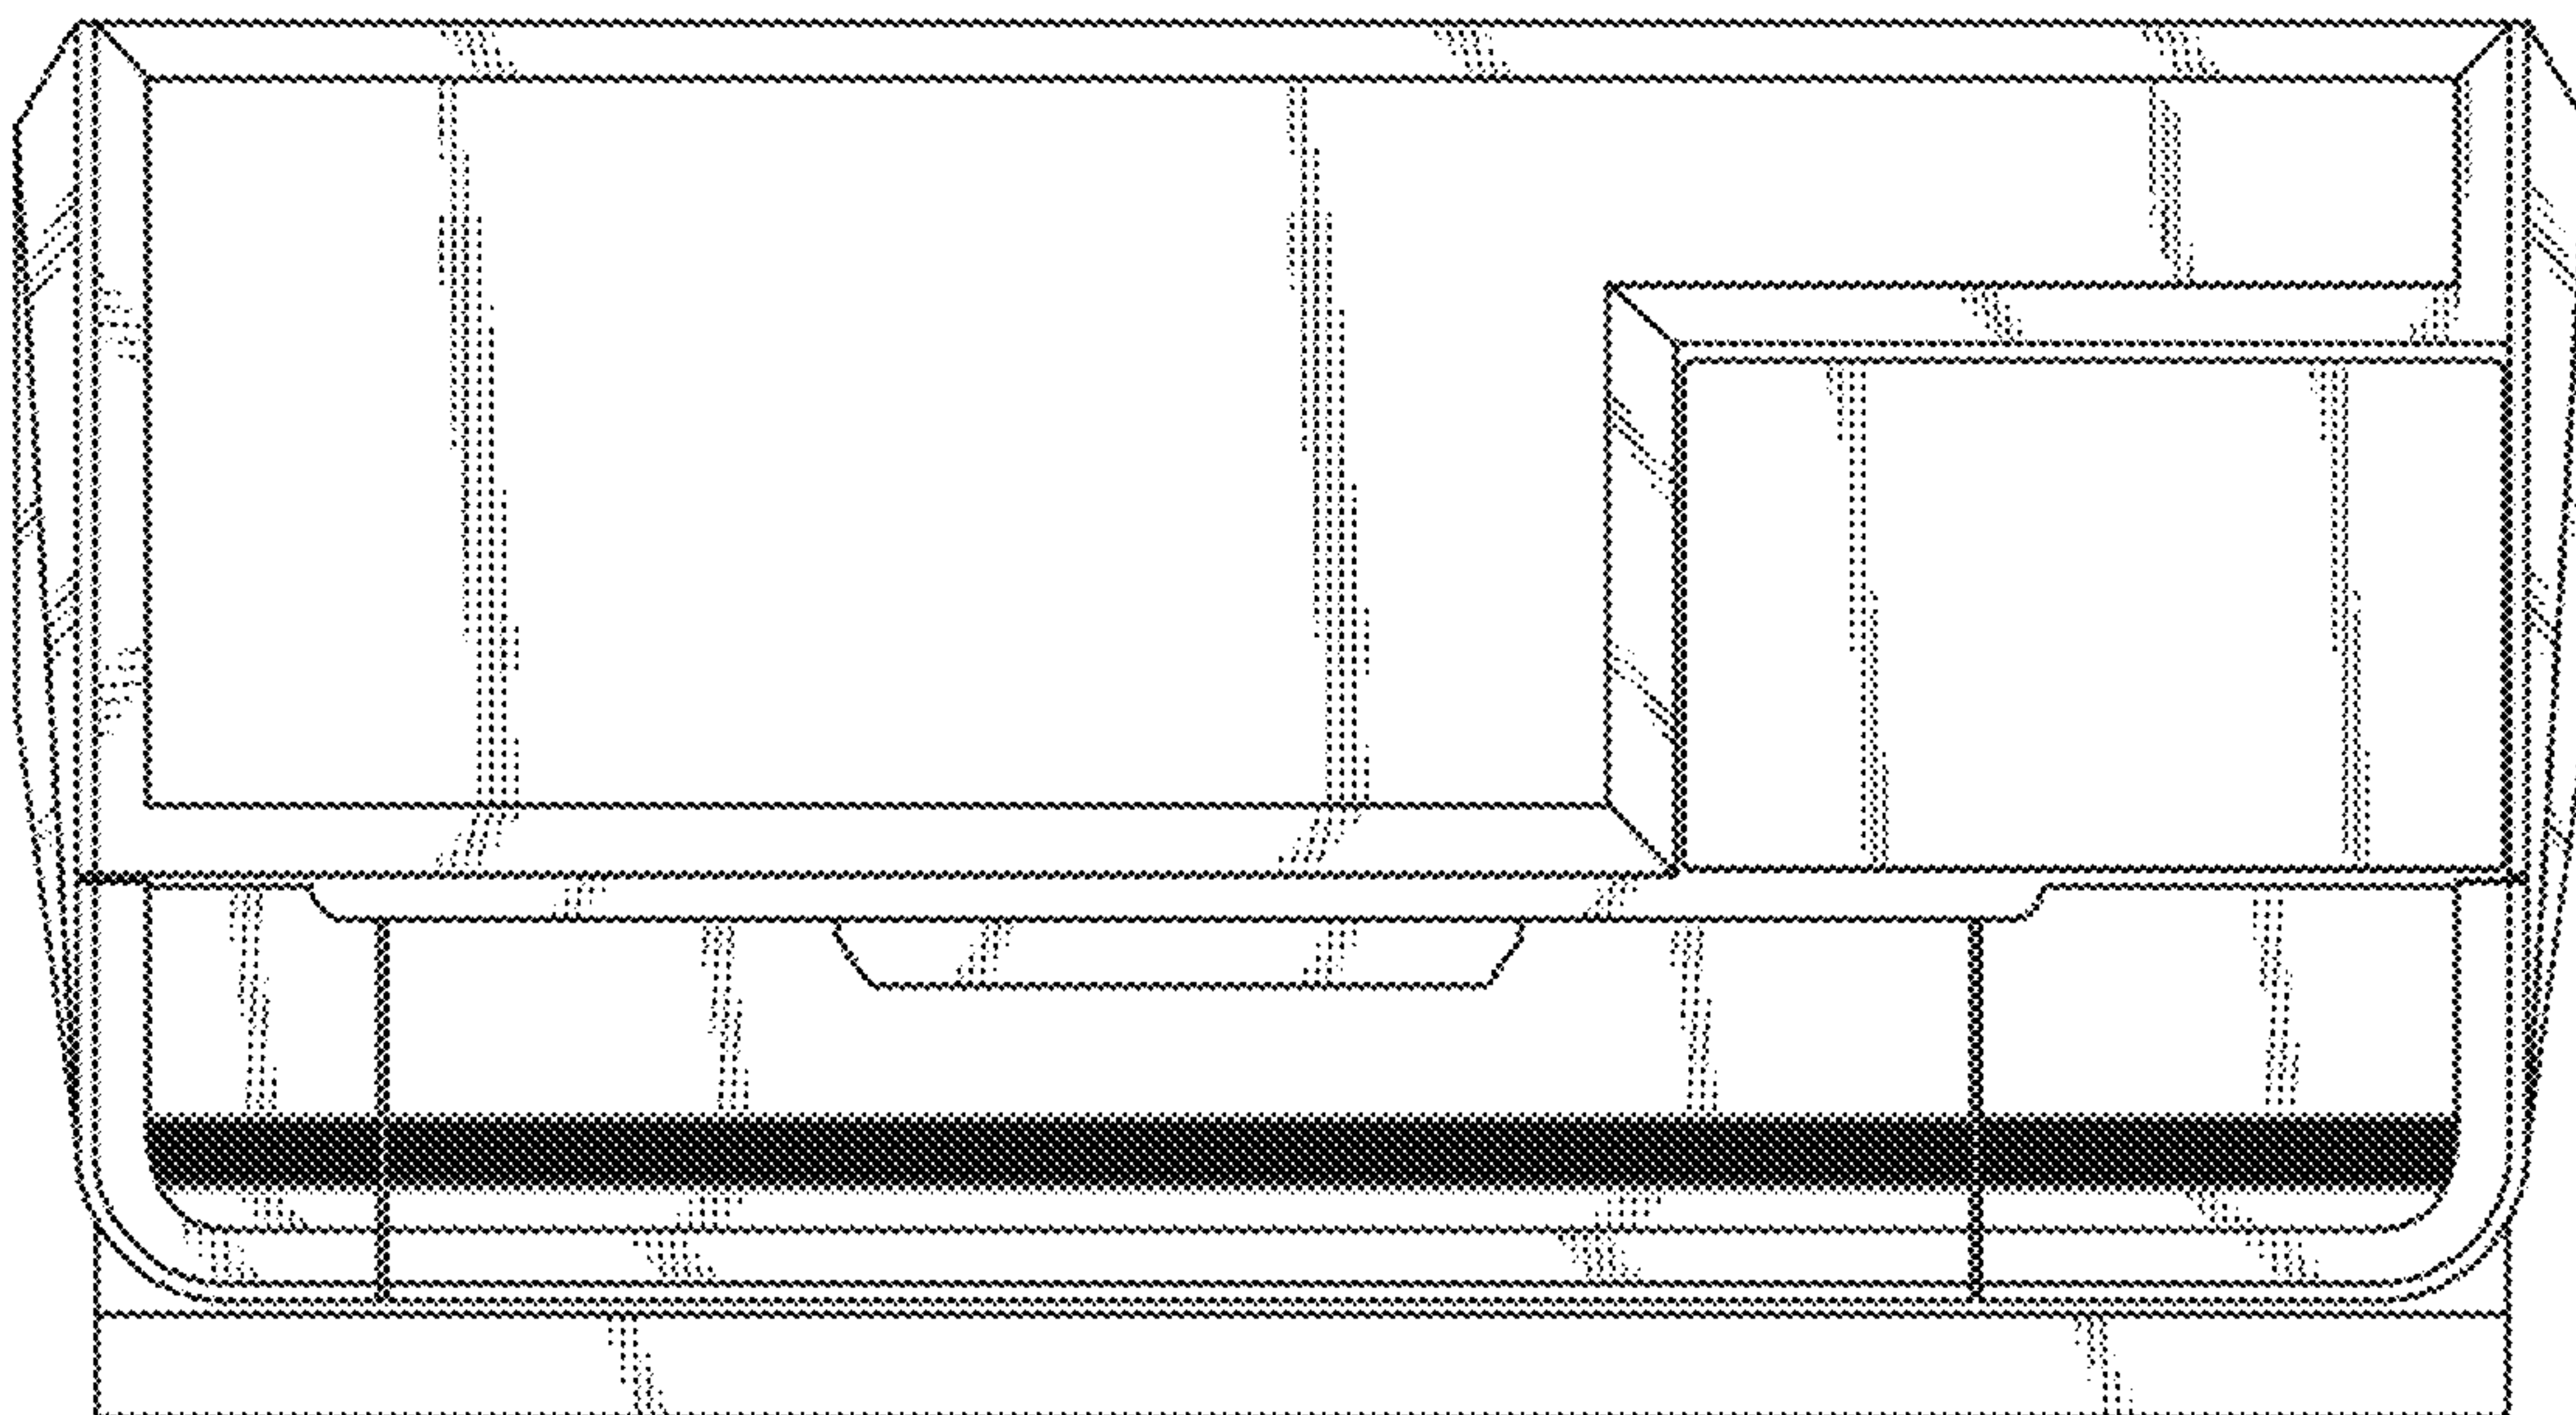


FIG. 2

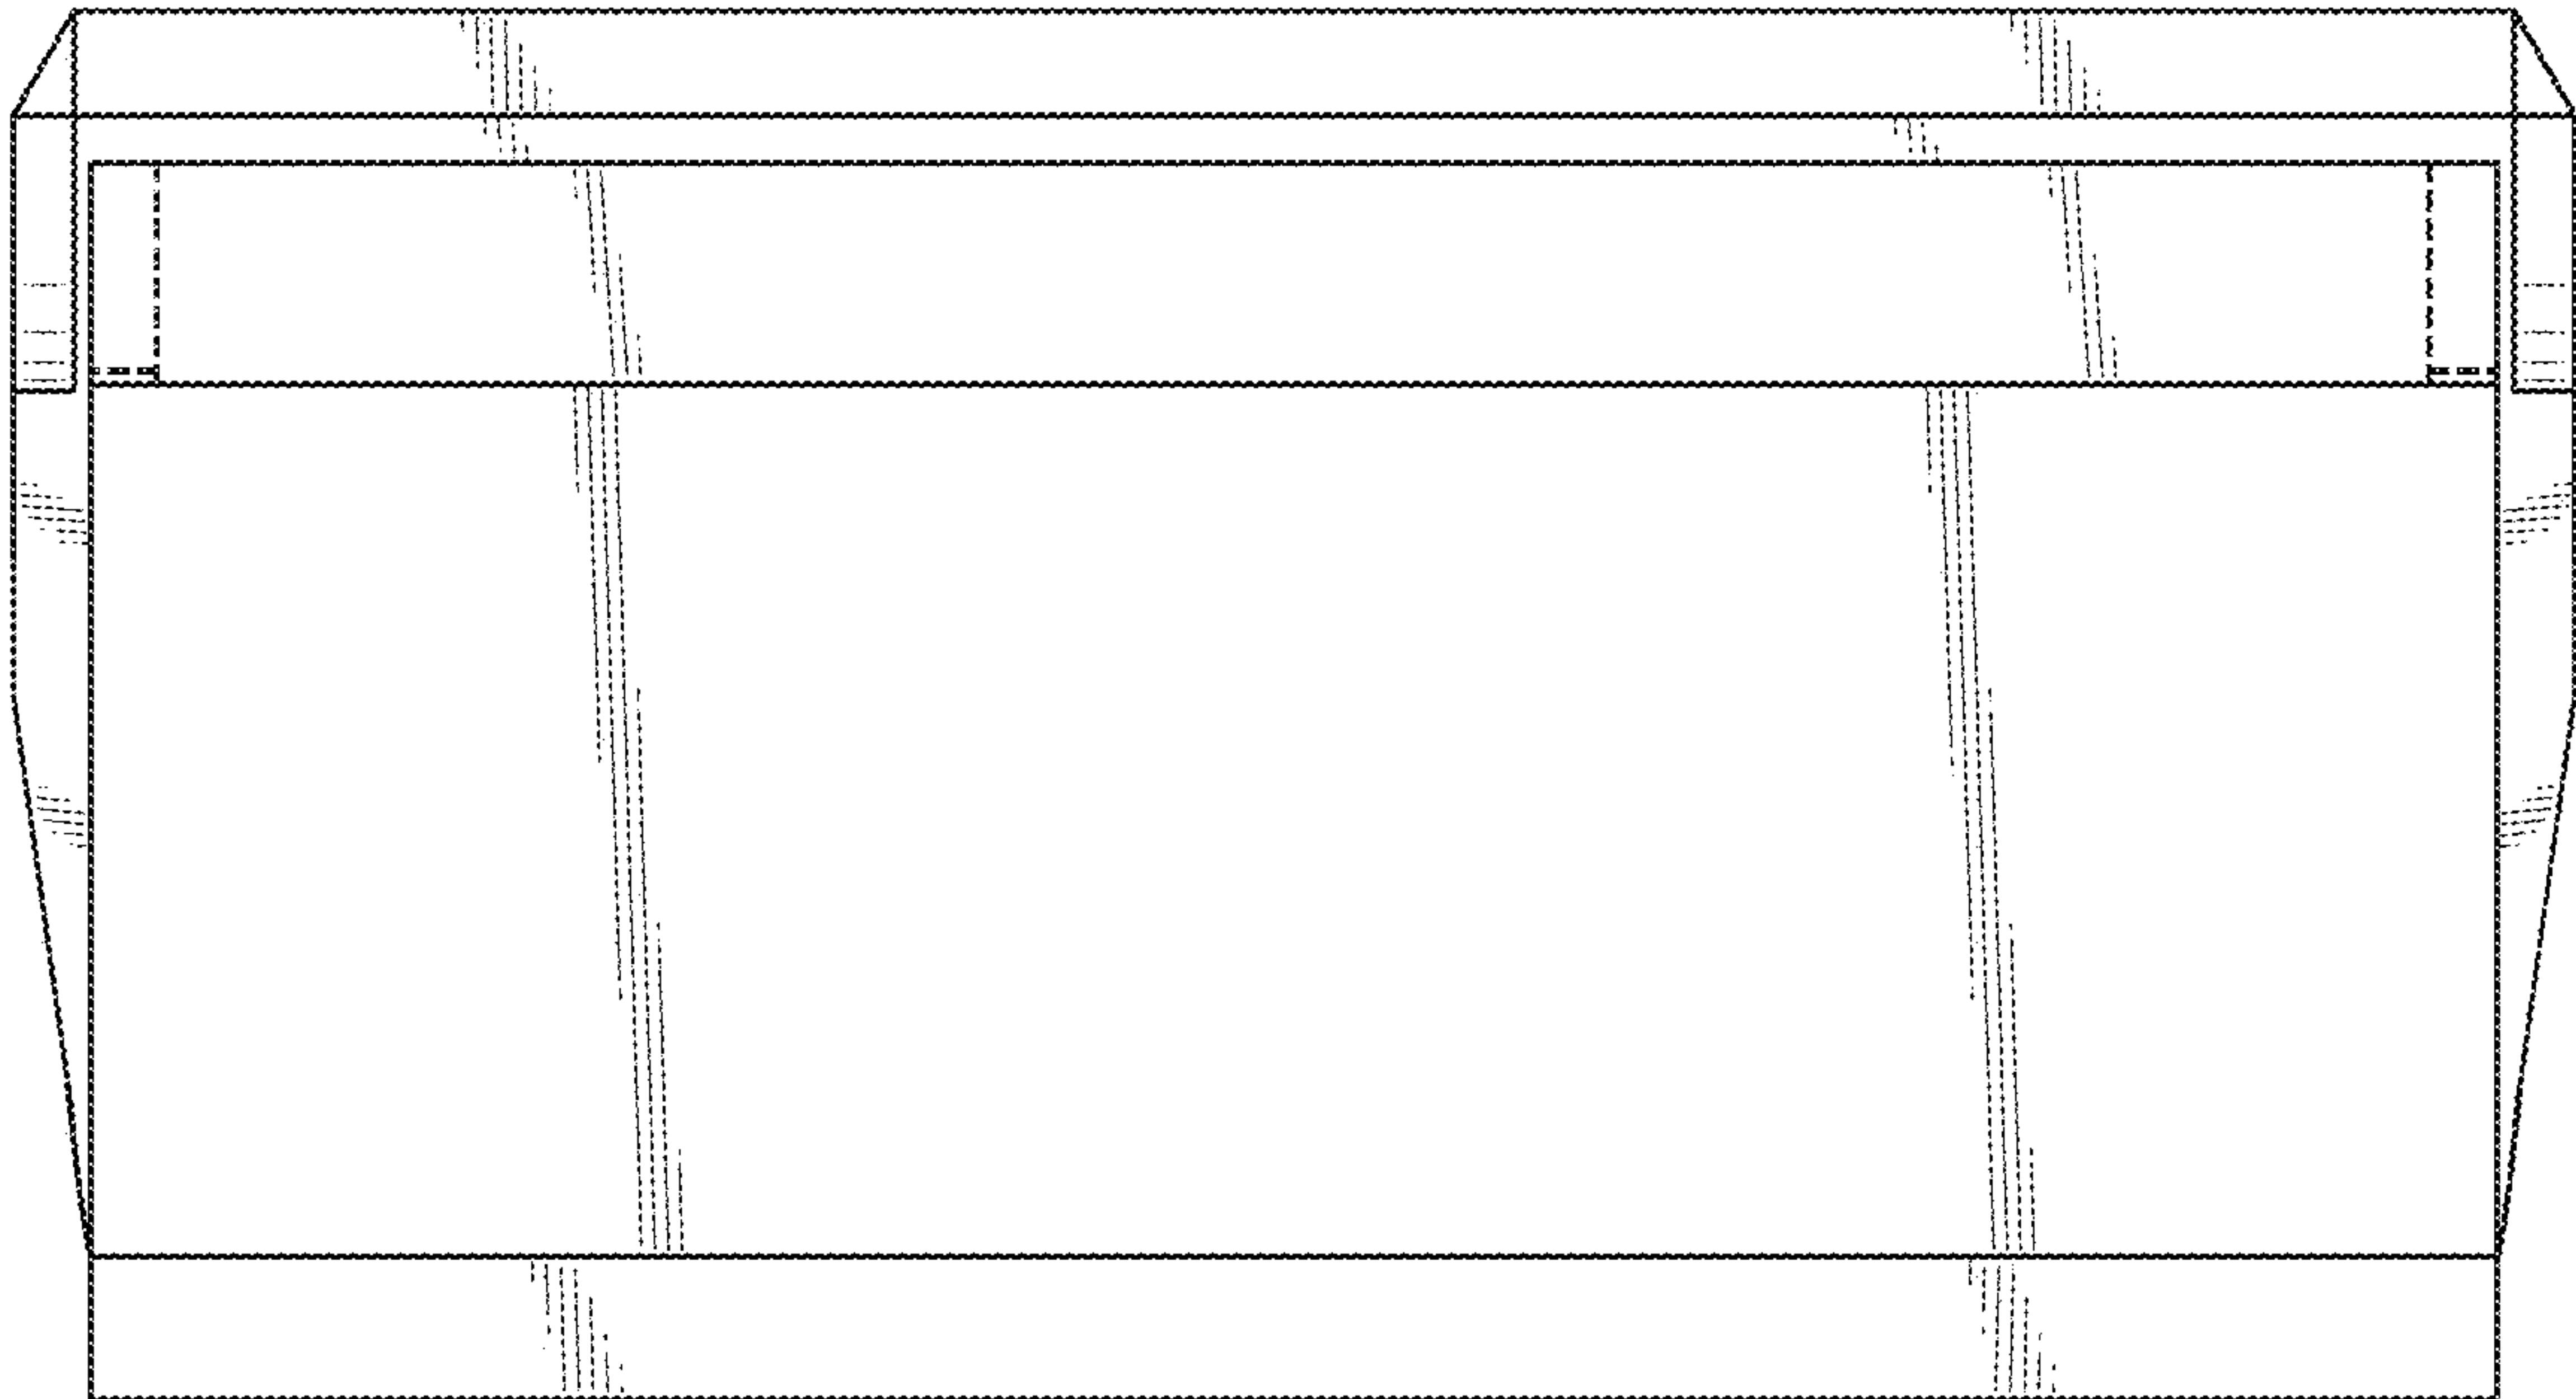


FIG. 3

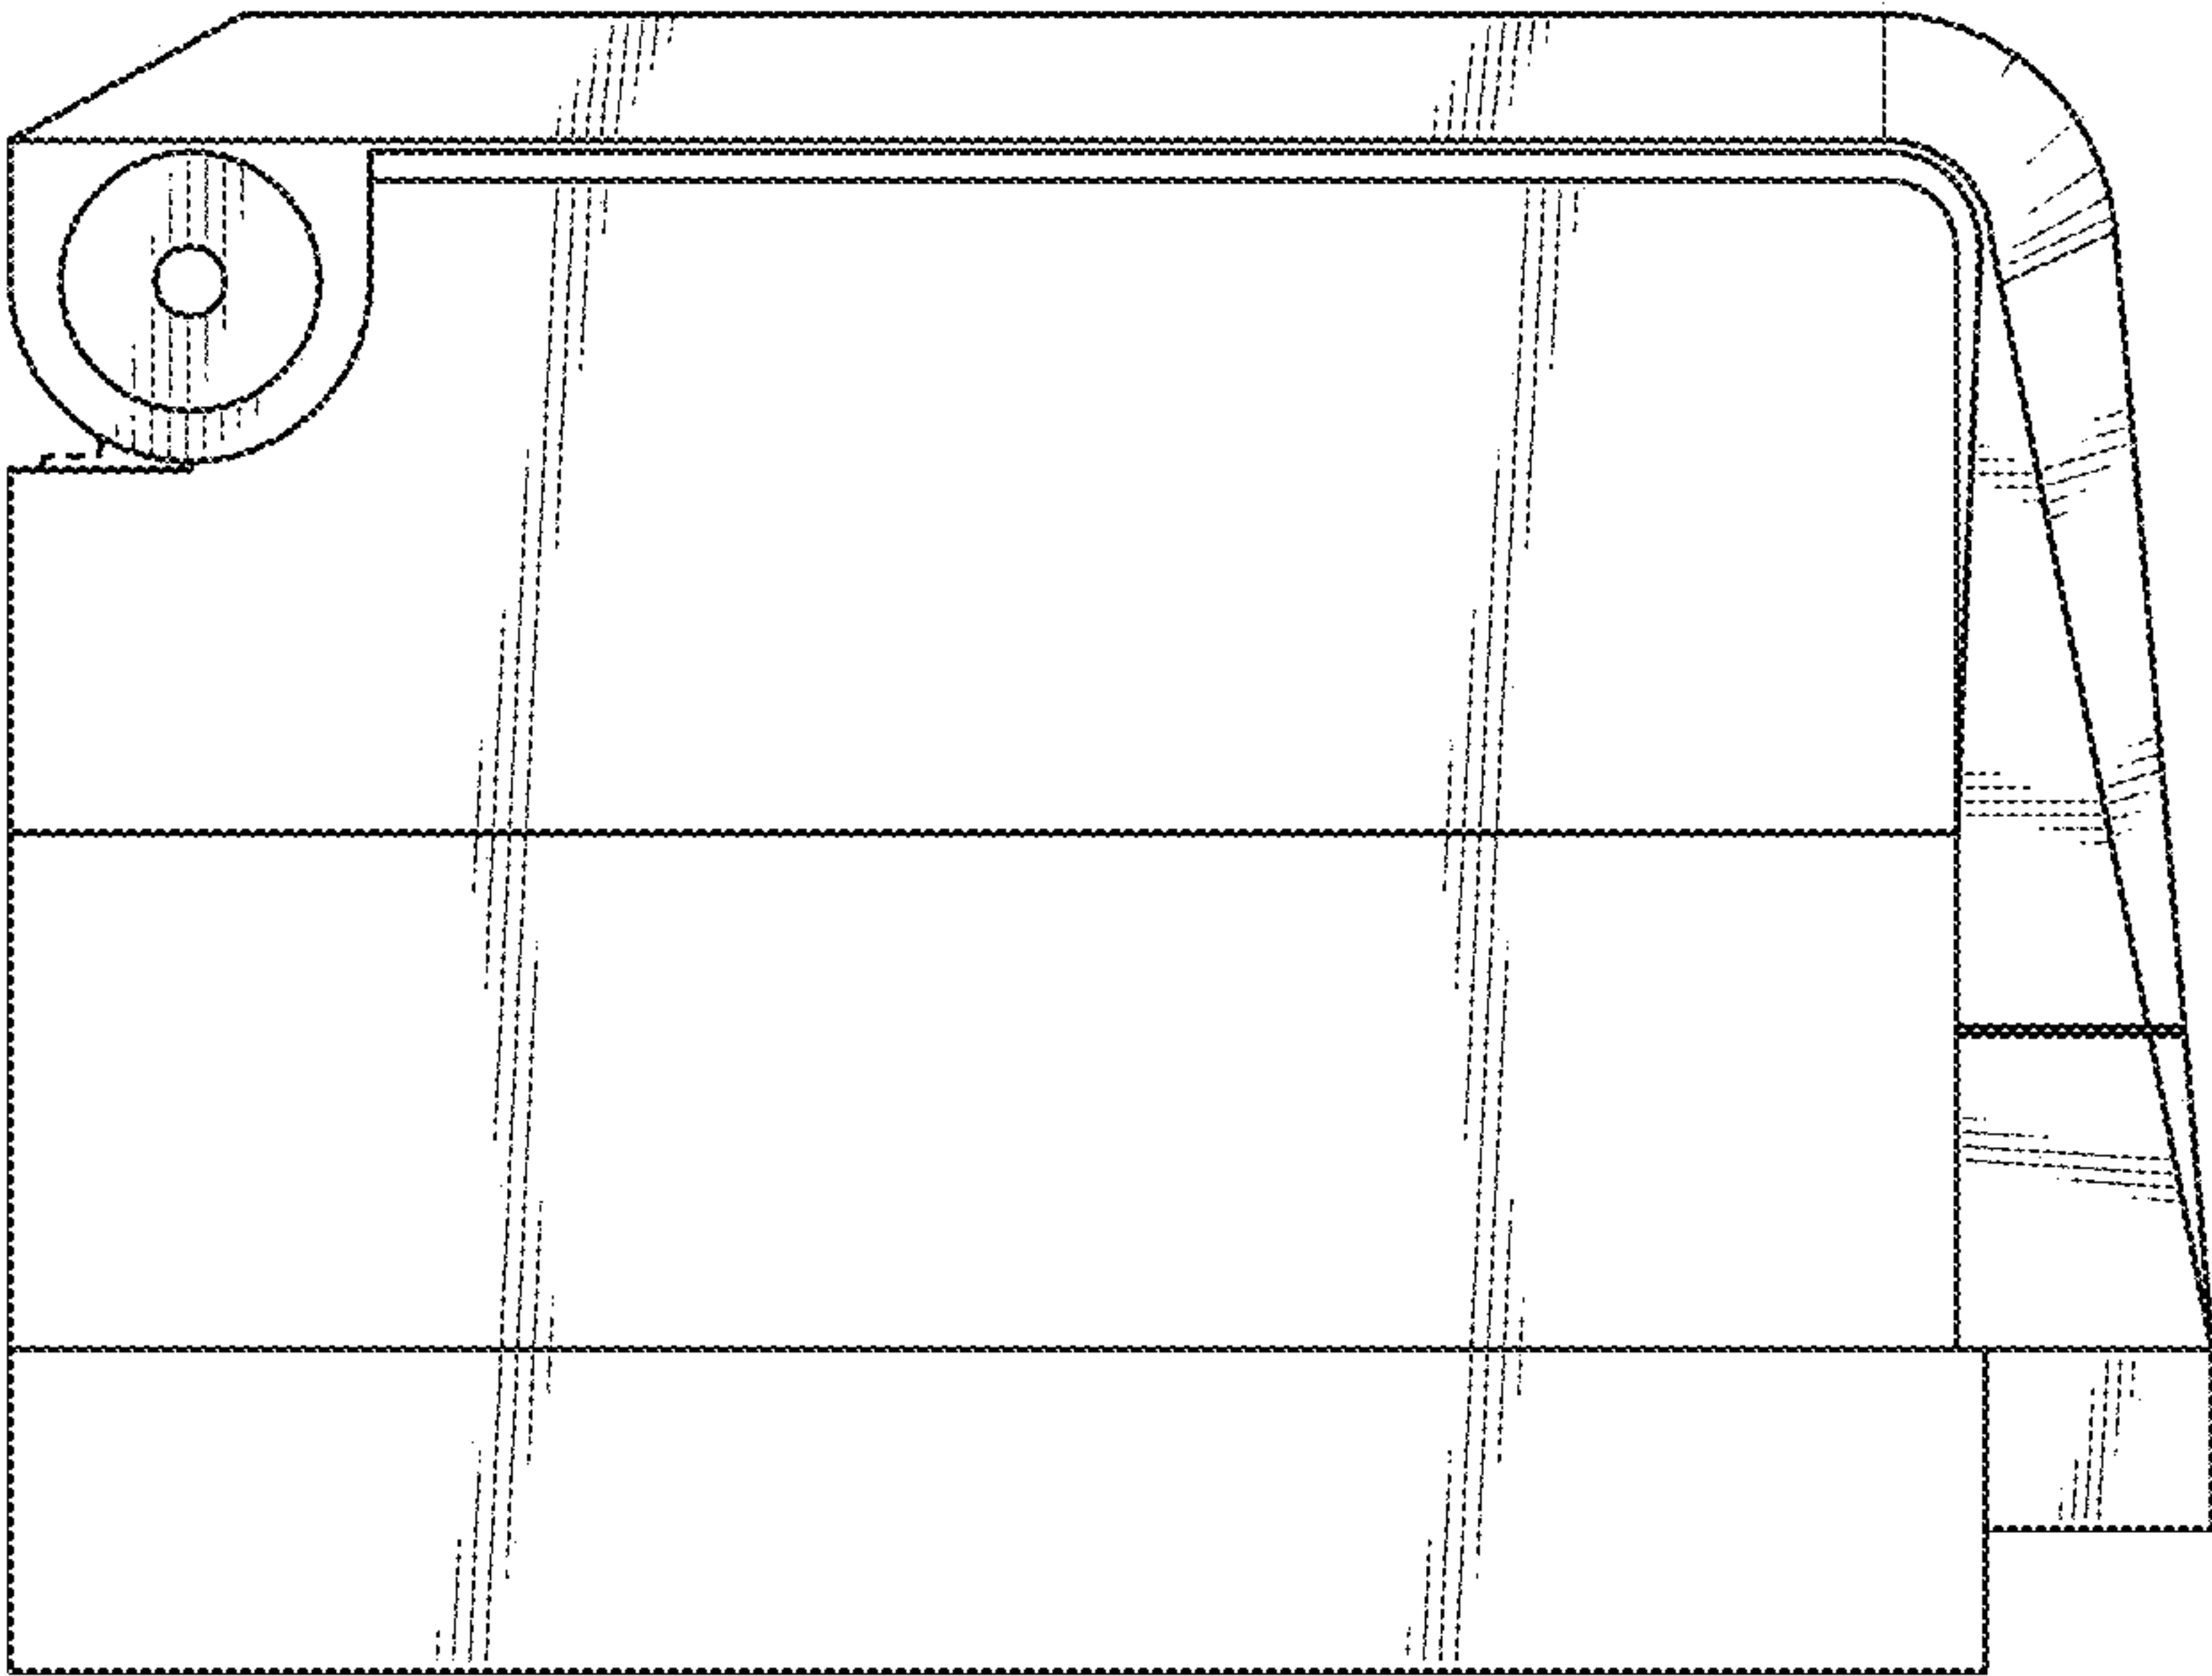


FIG. 4

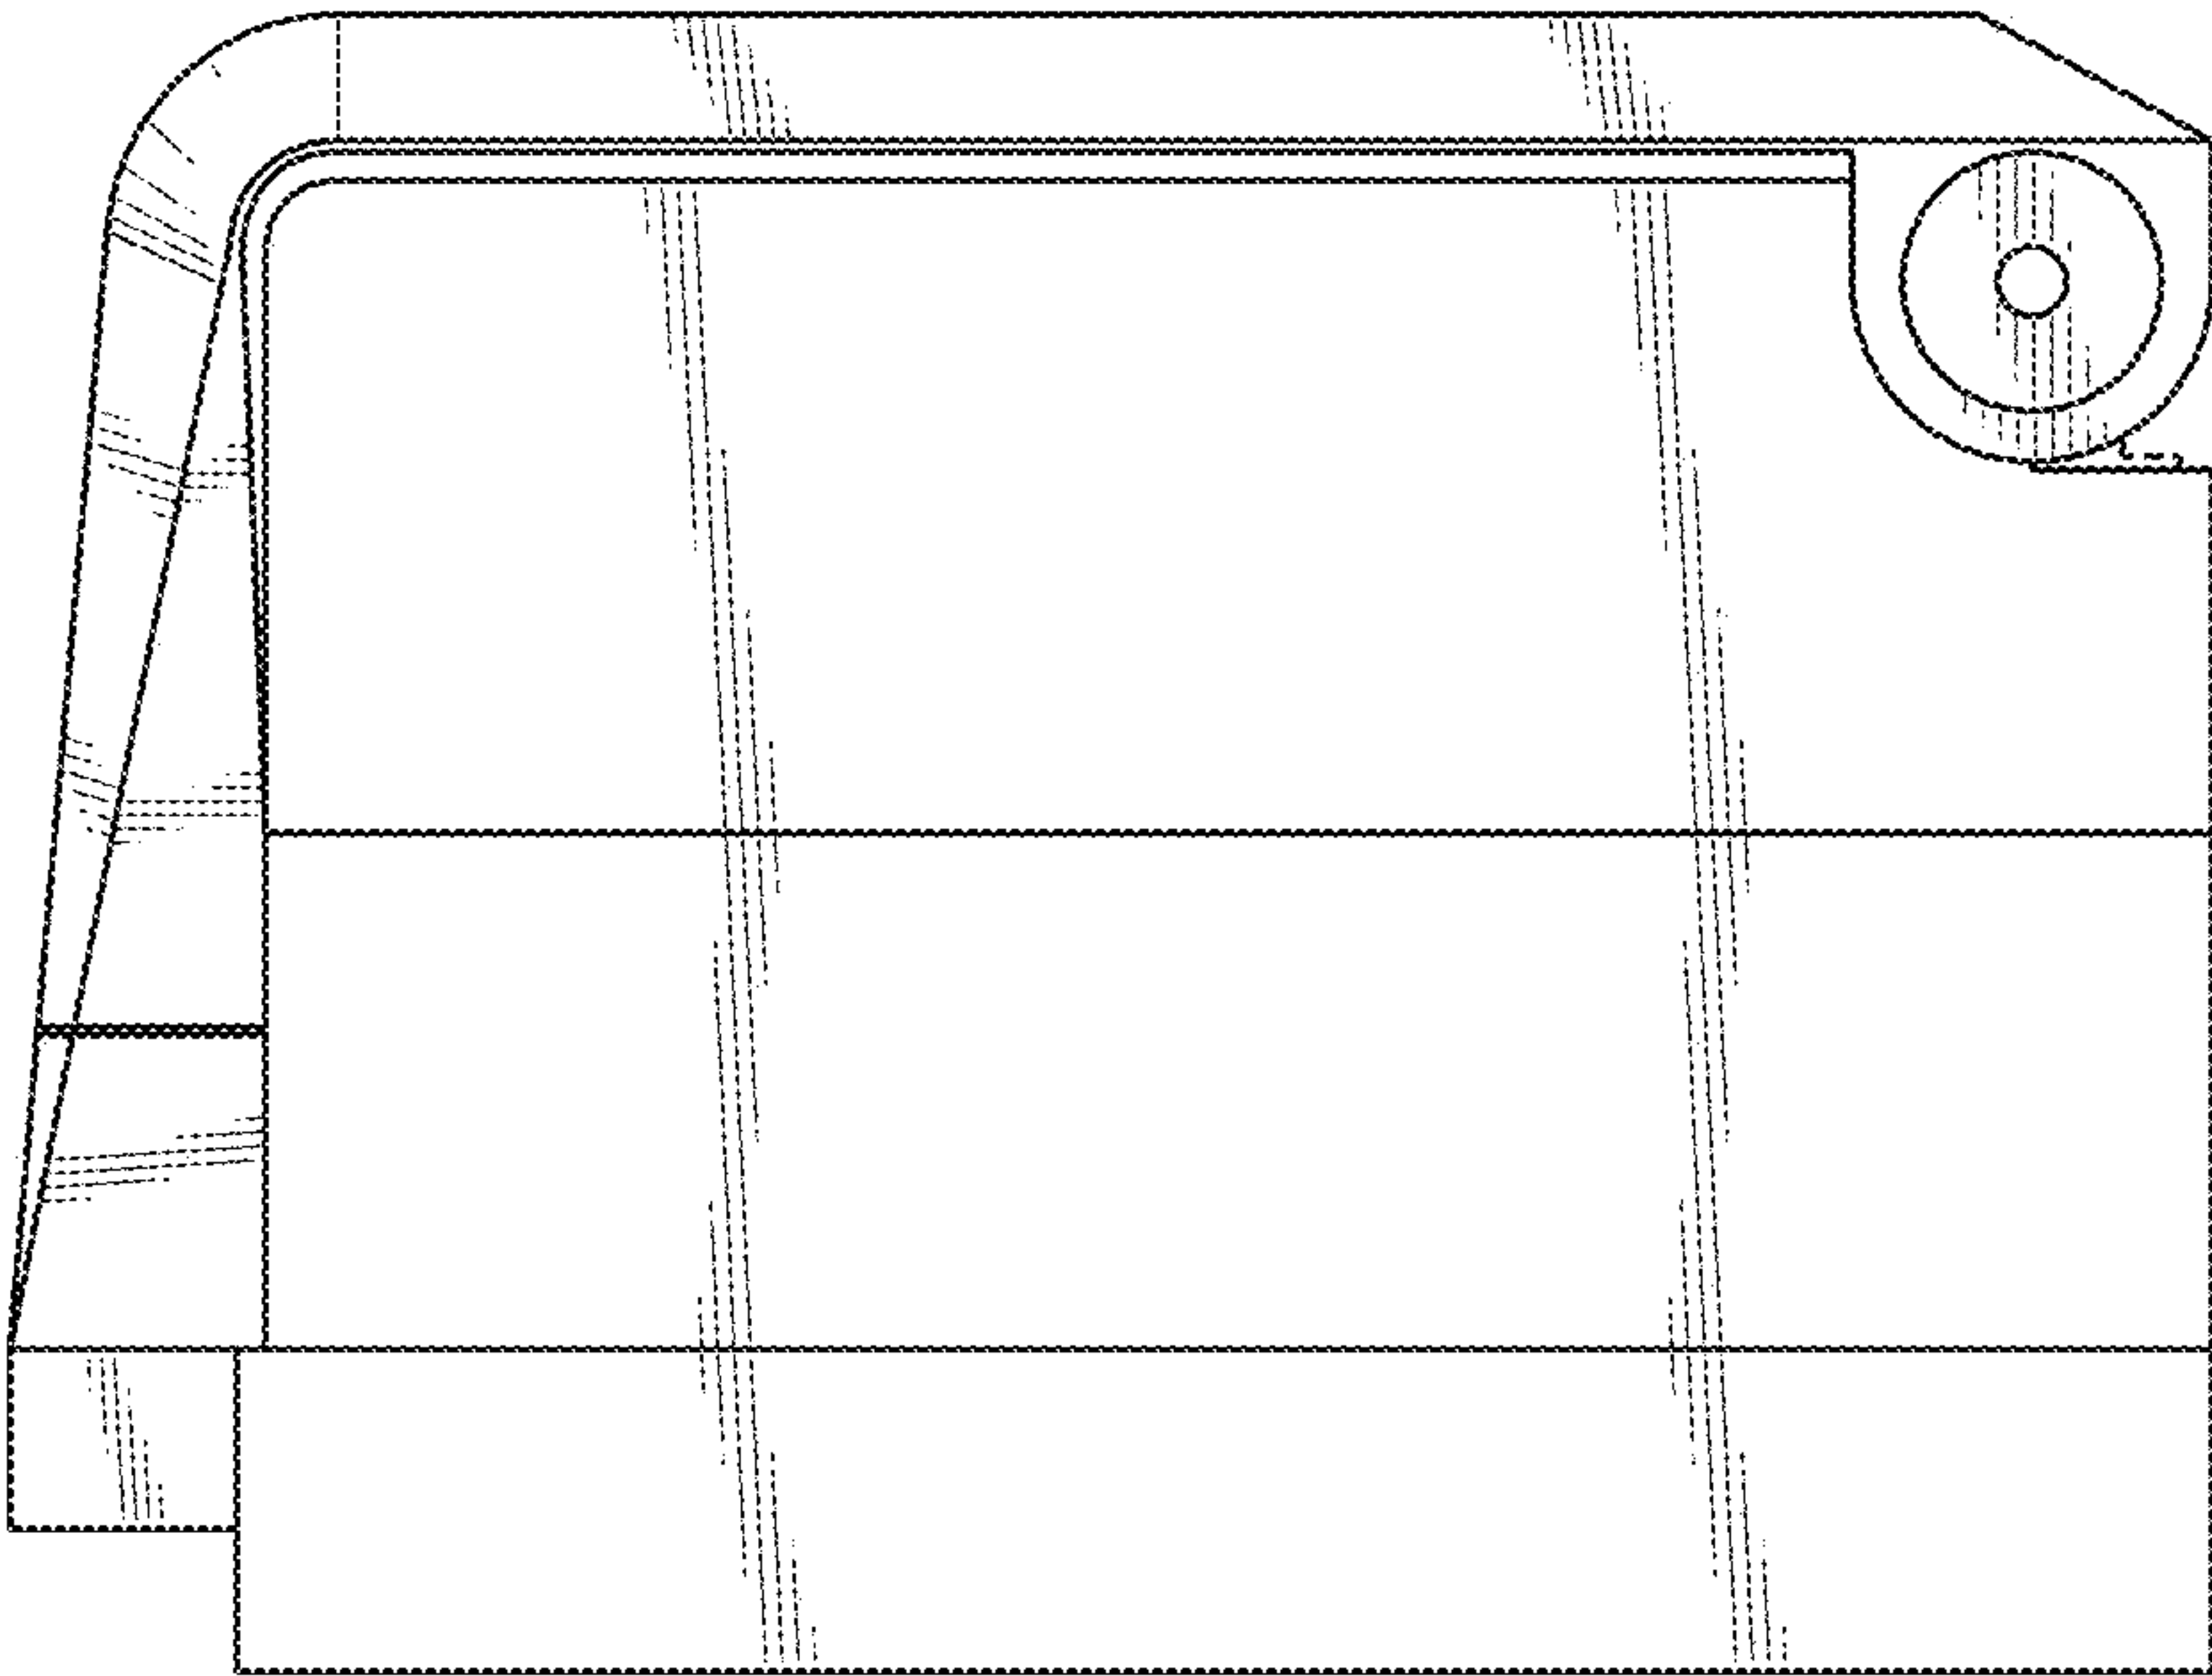


FIG. 5

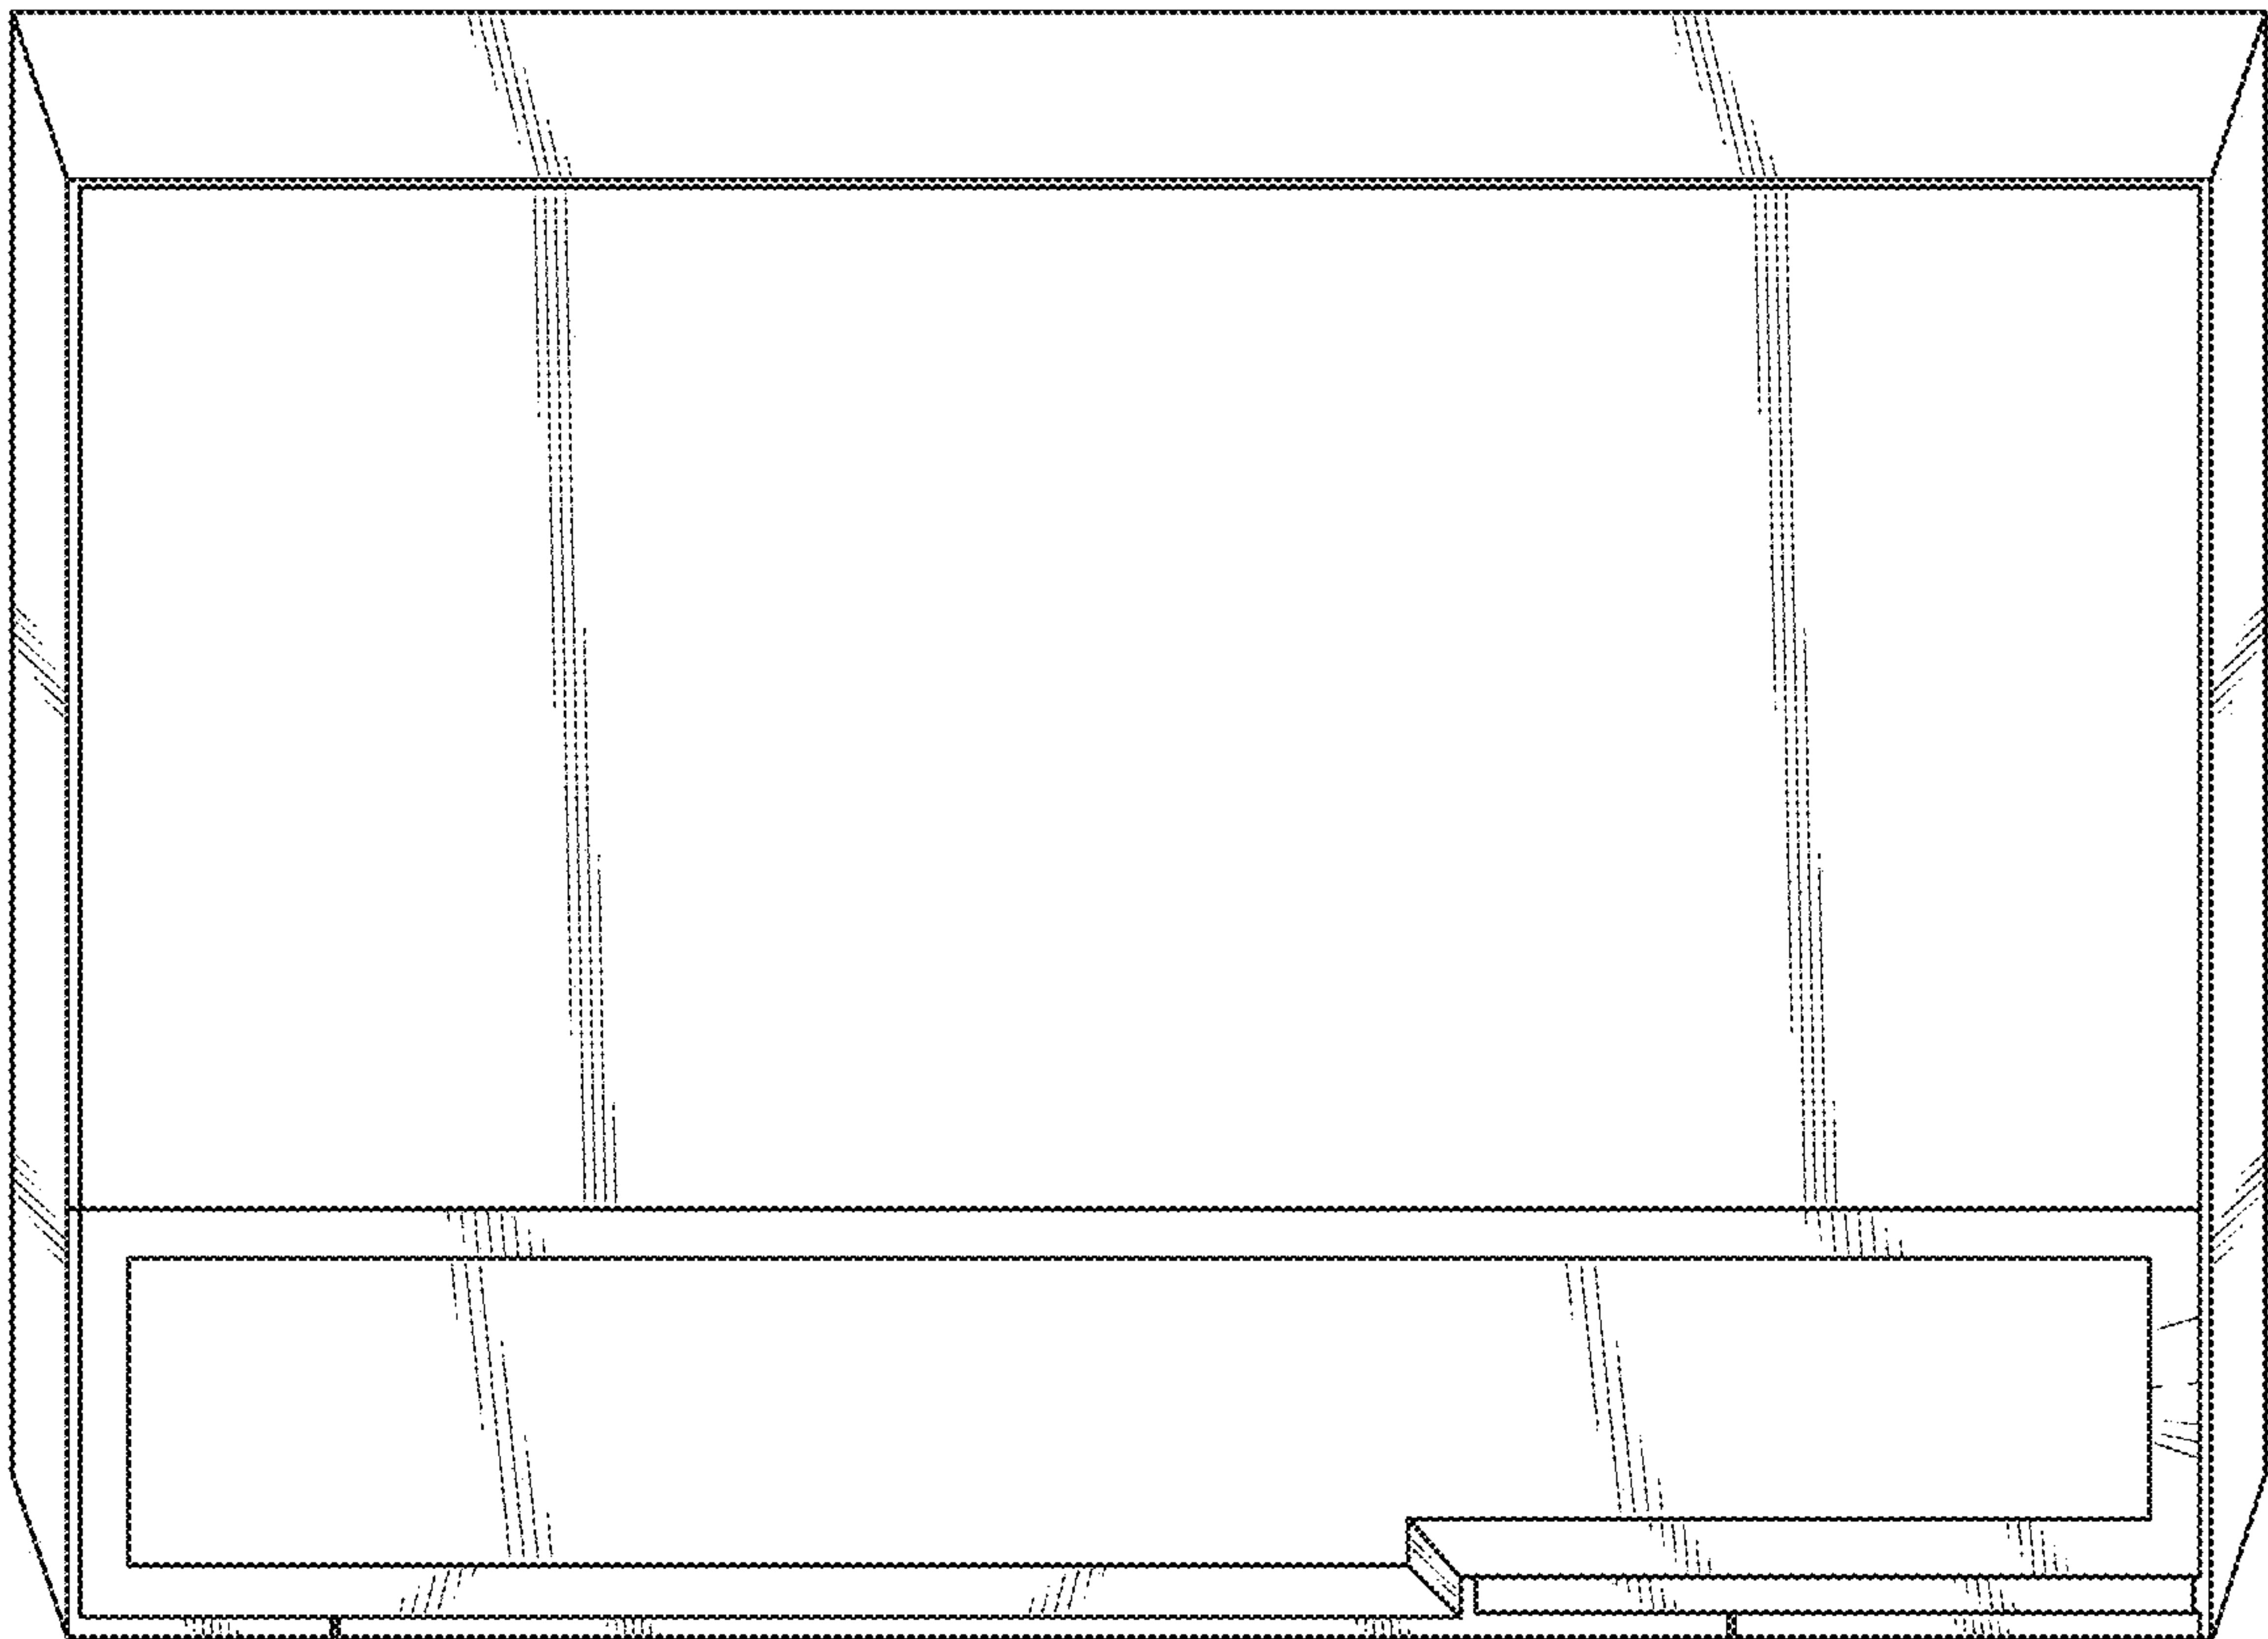


FIG. 6

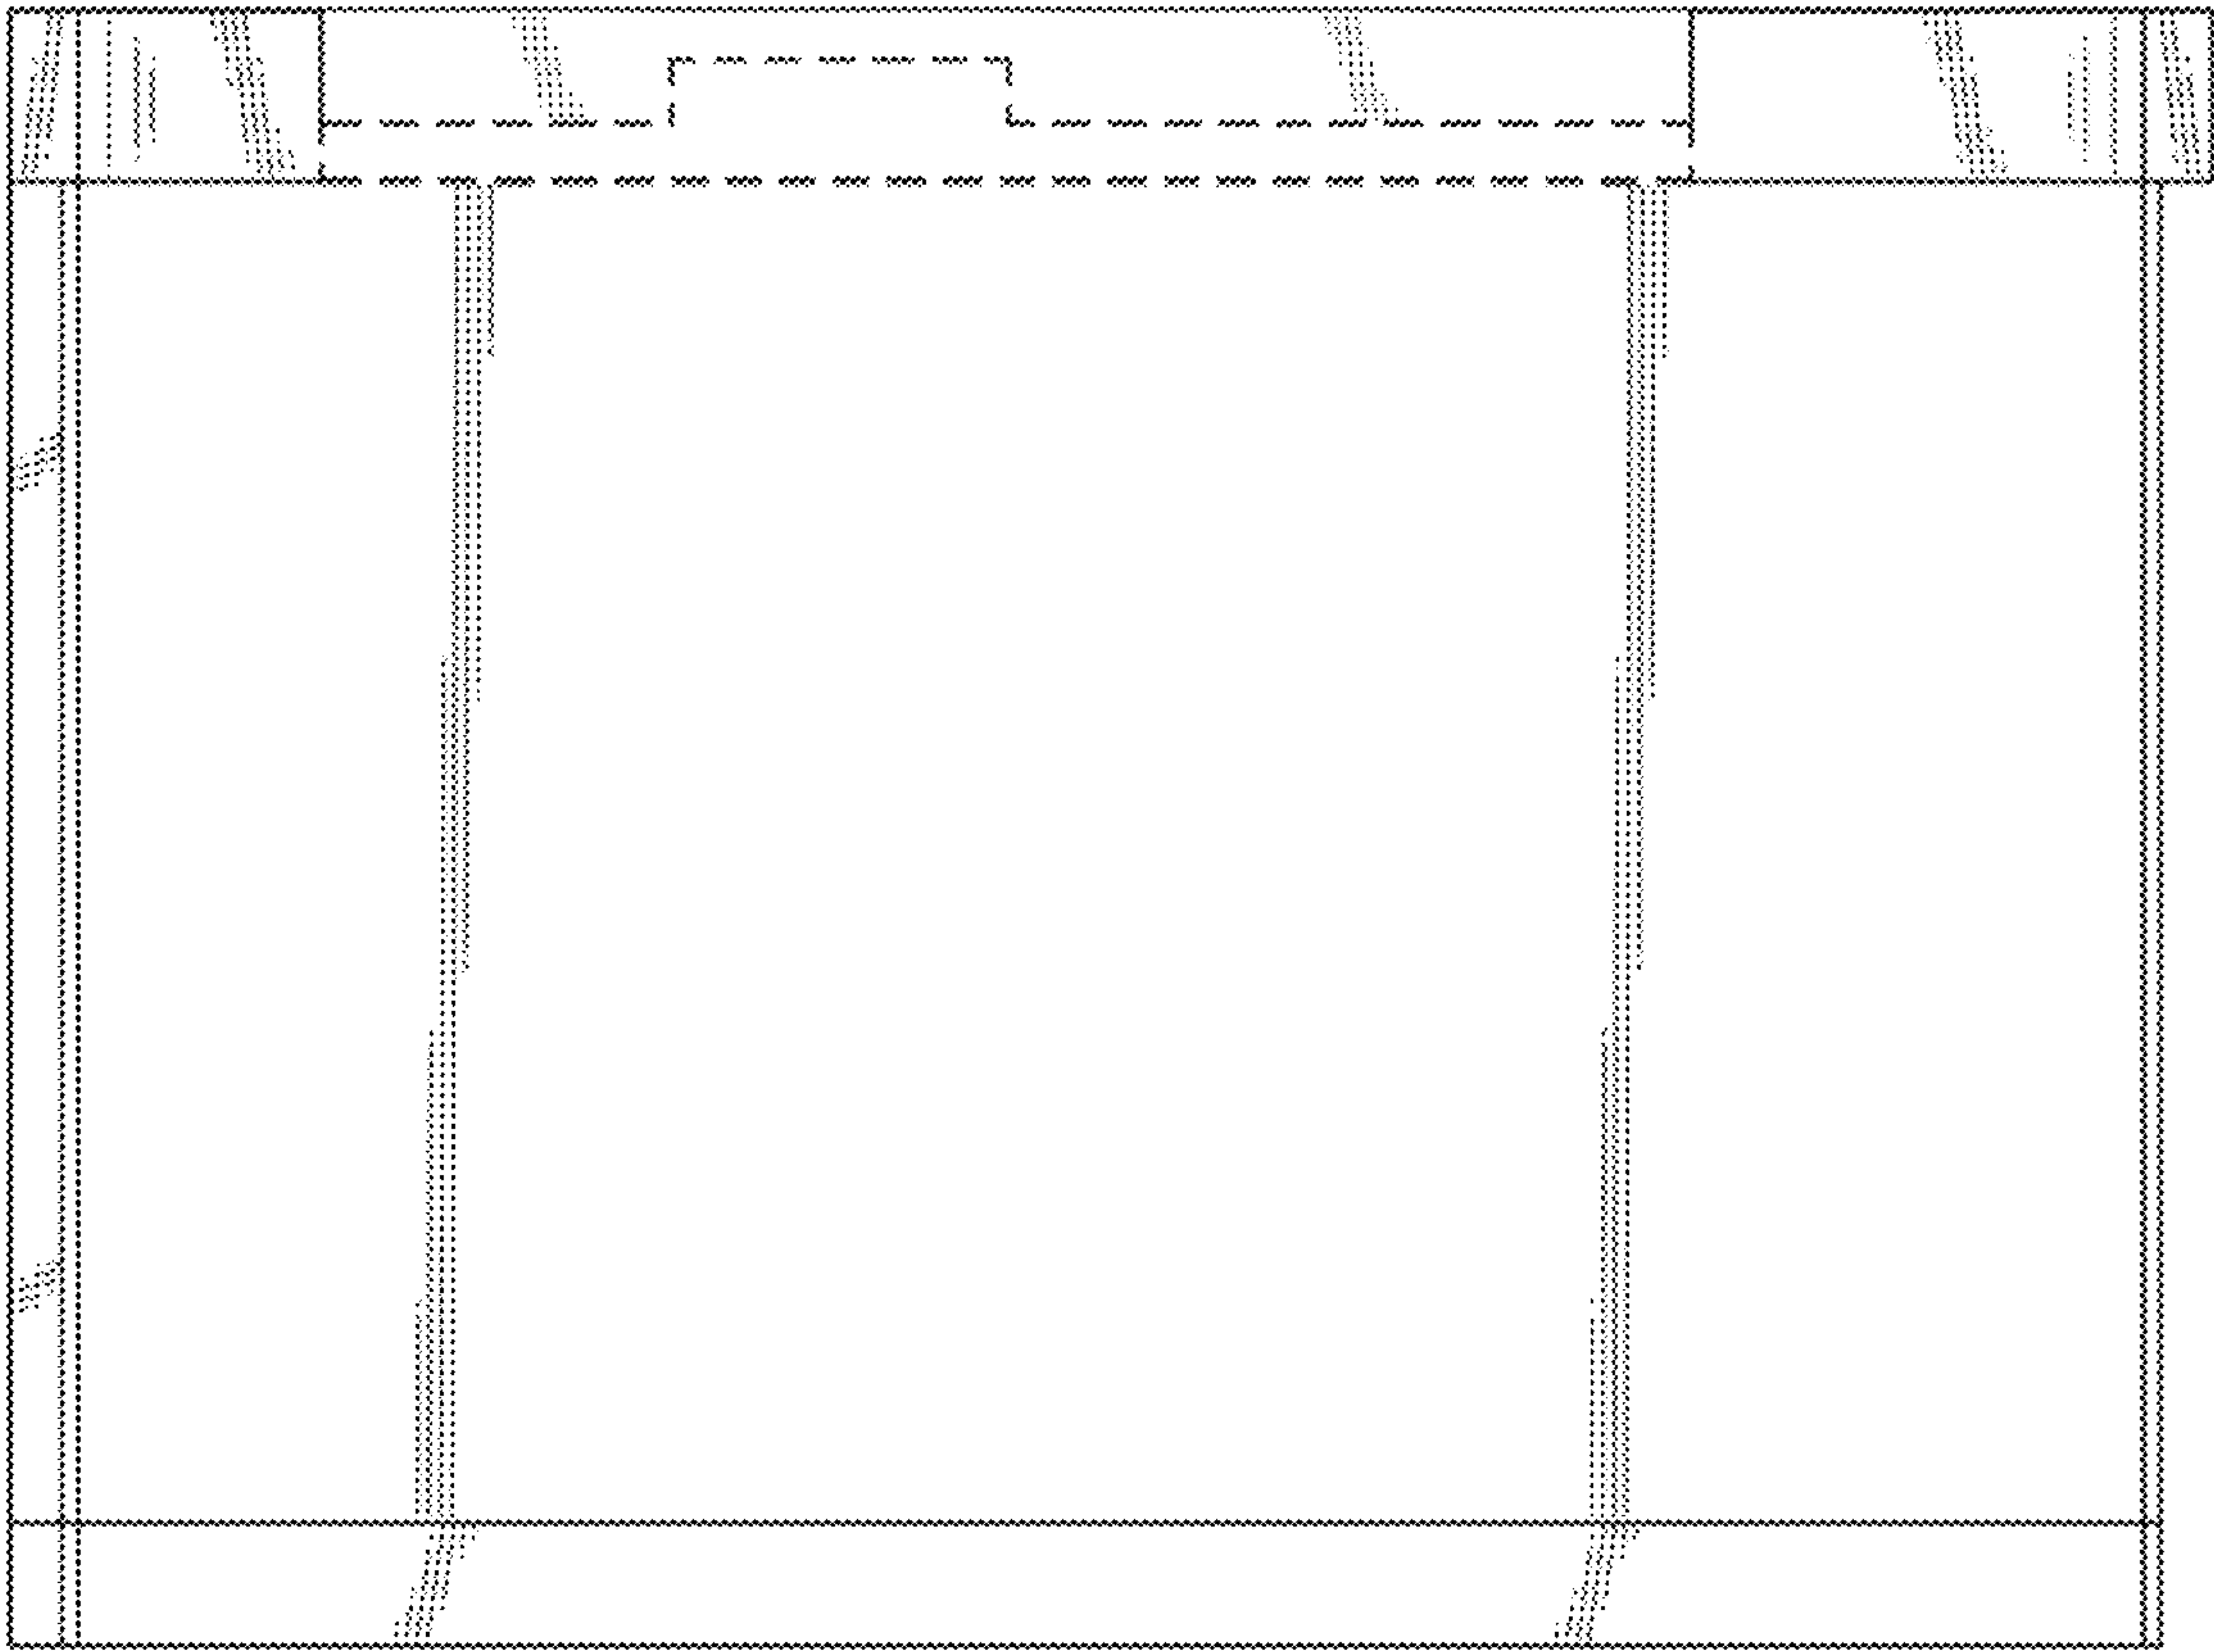


FIG. 7

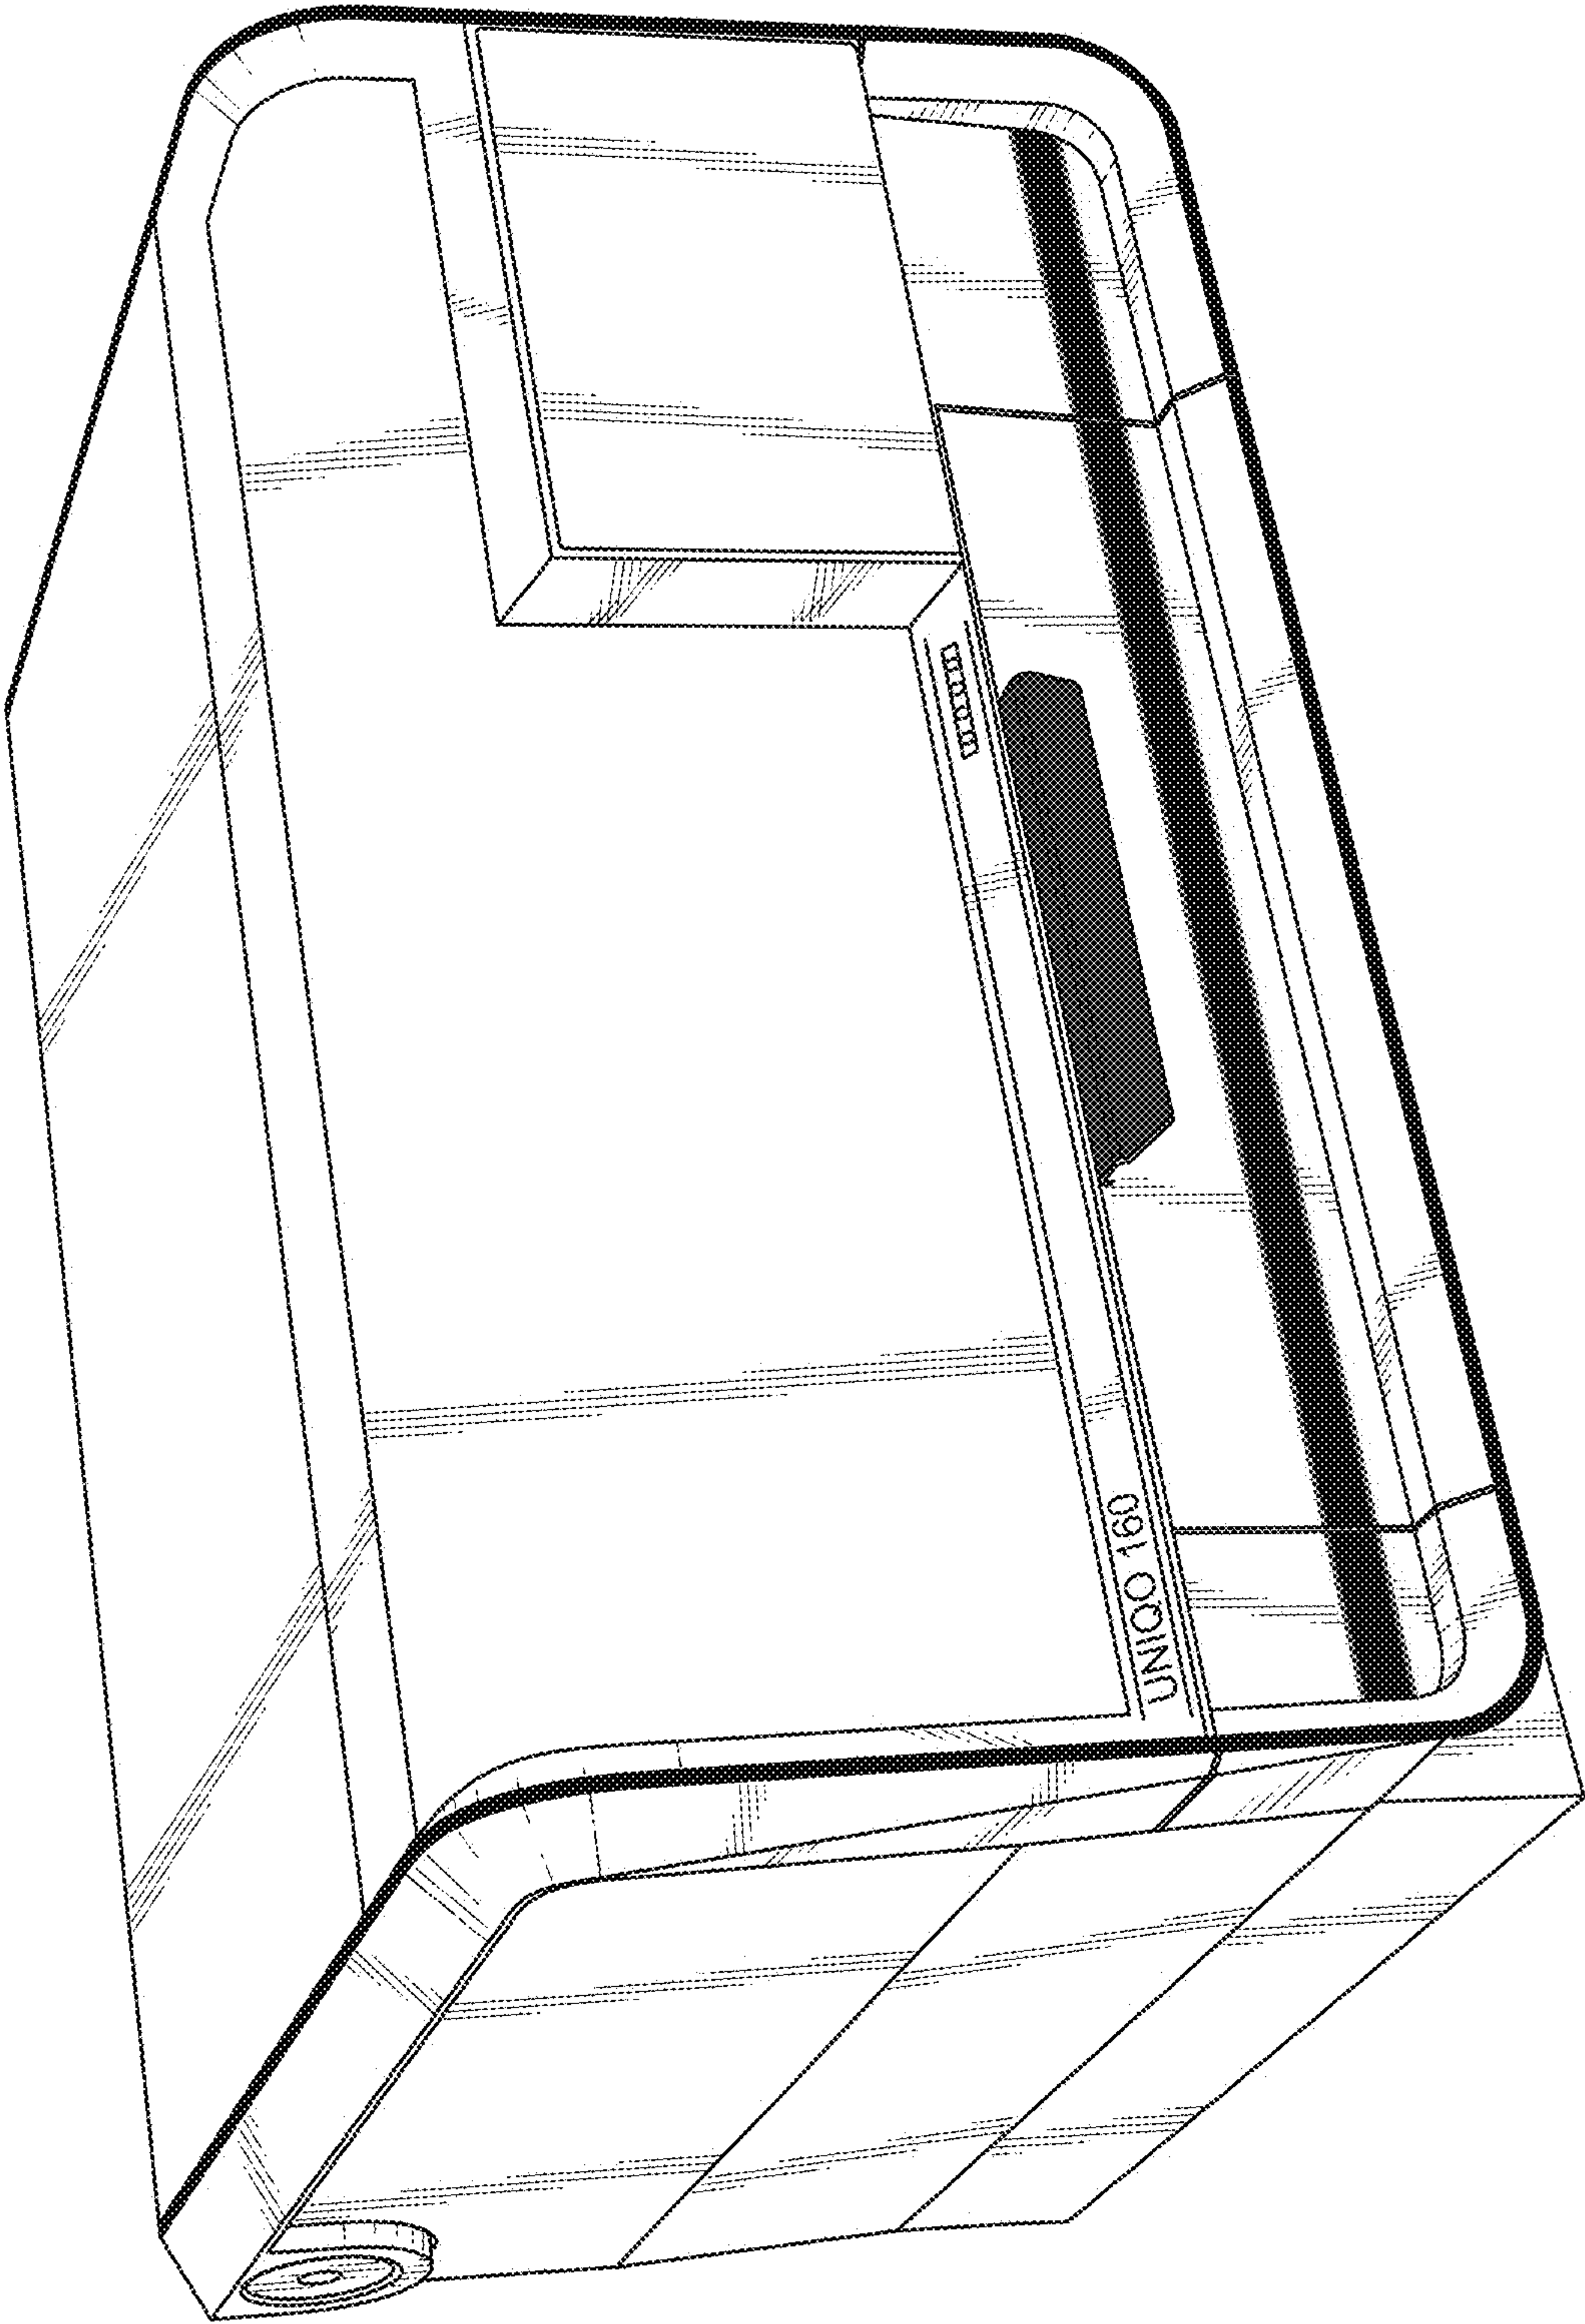


FIG. 8

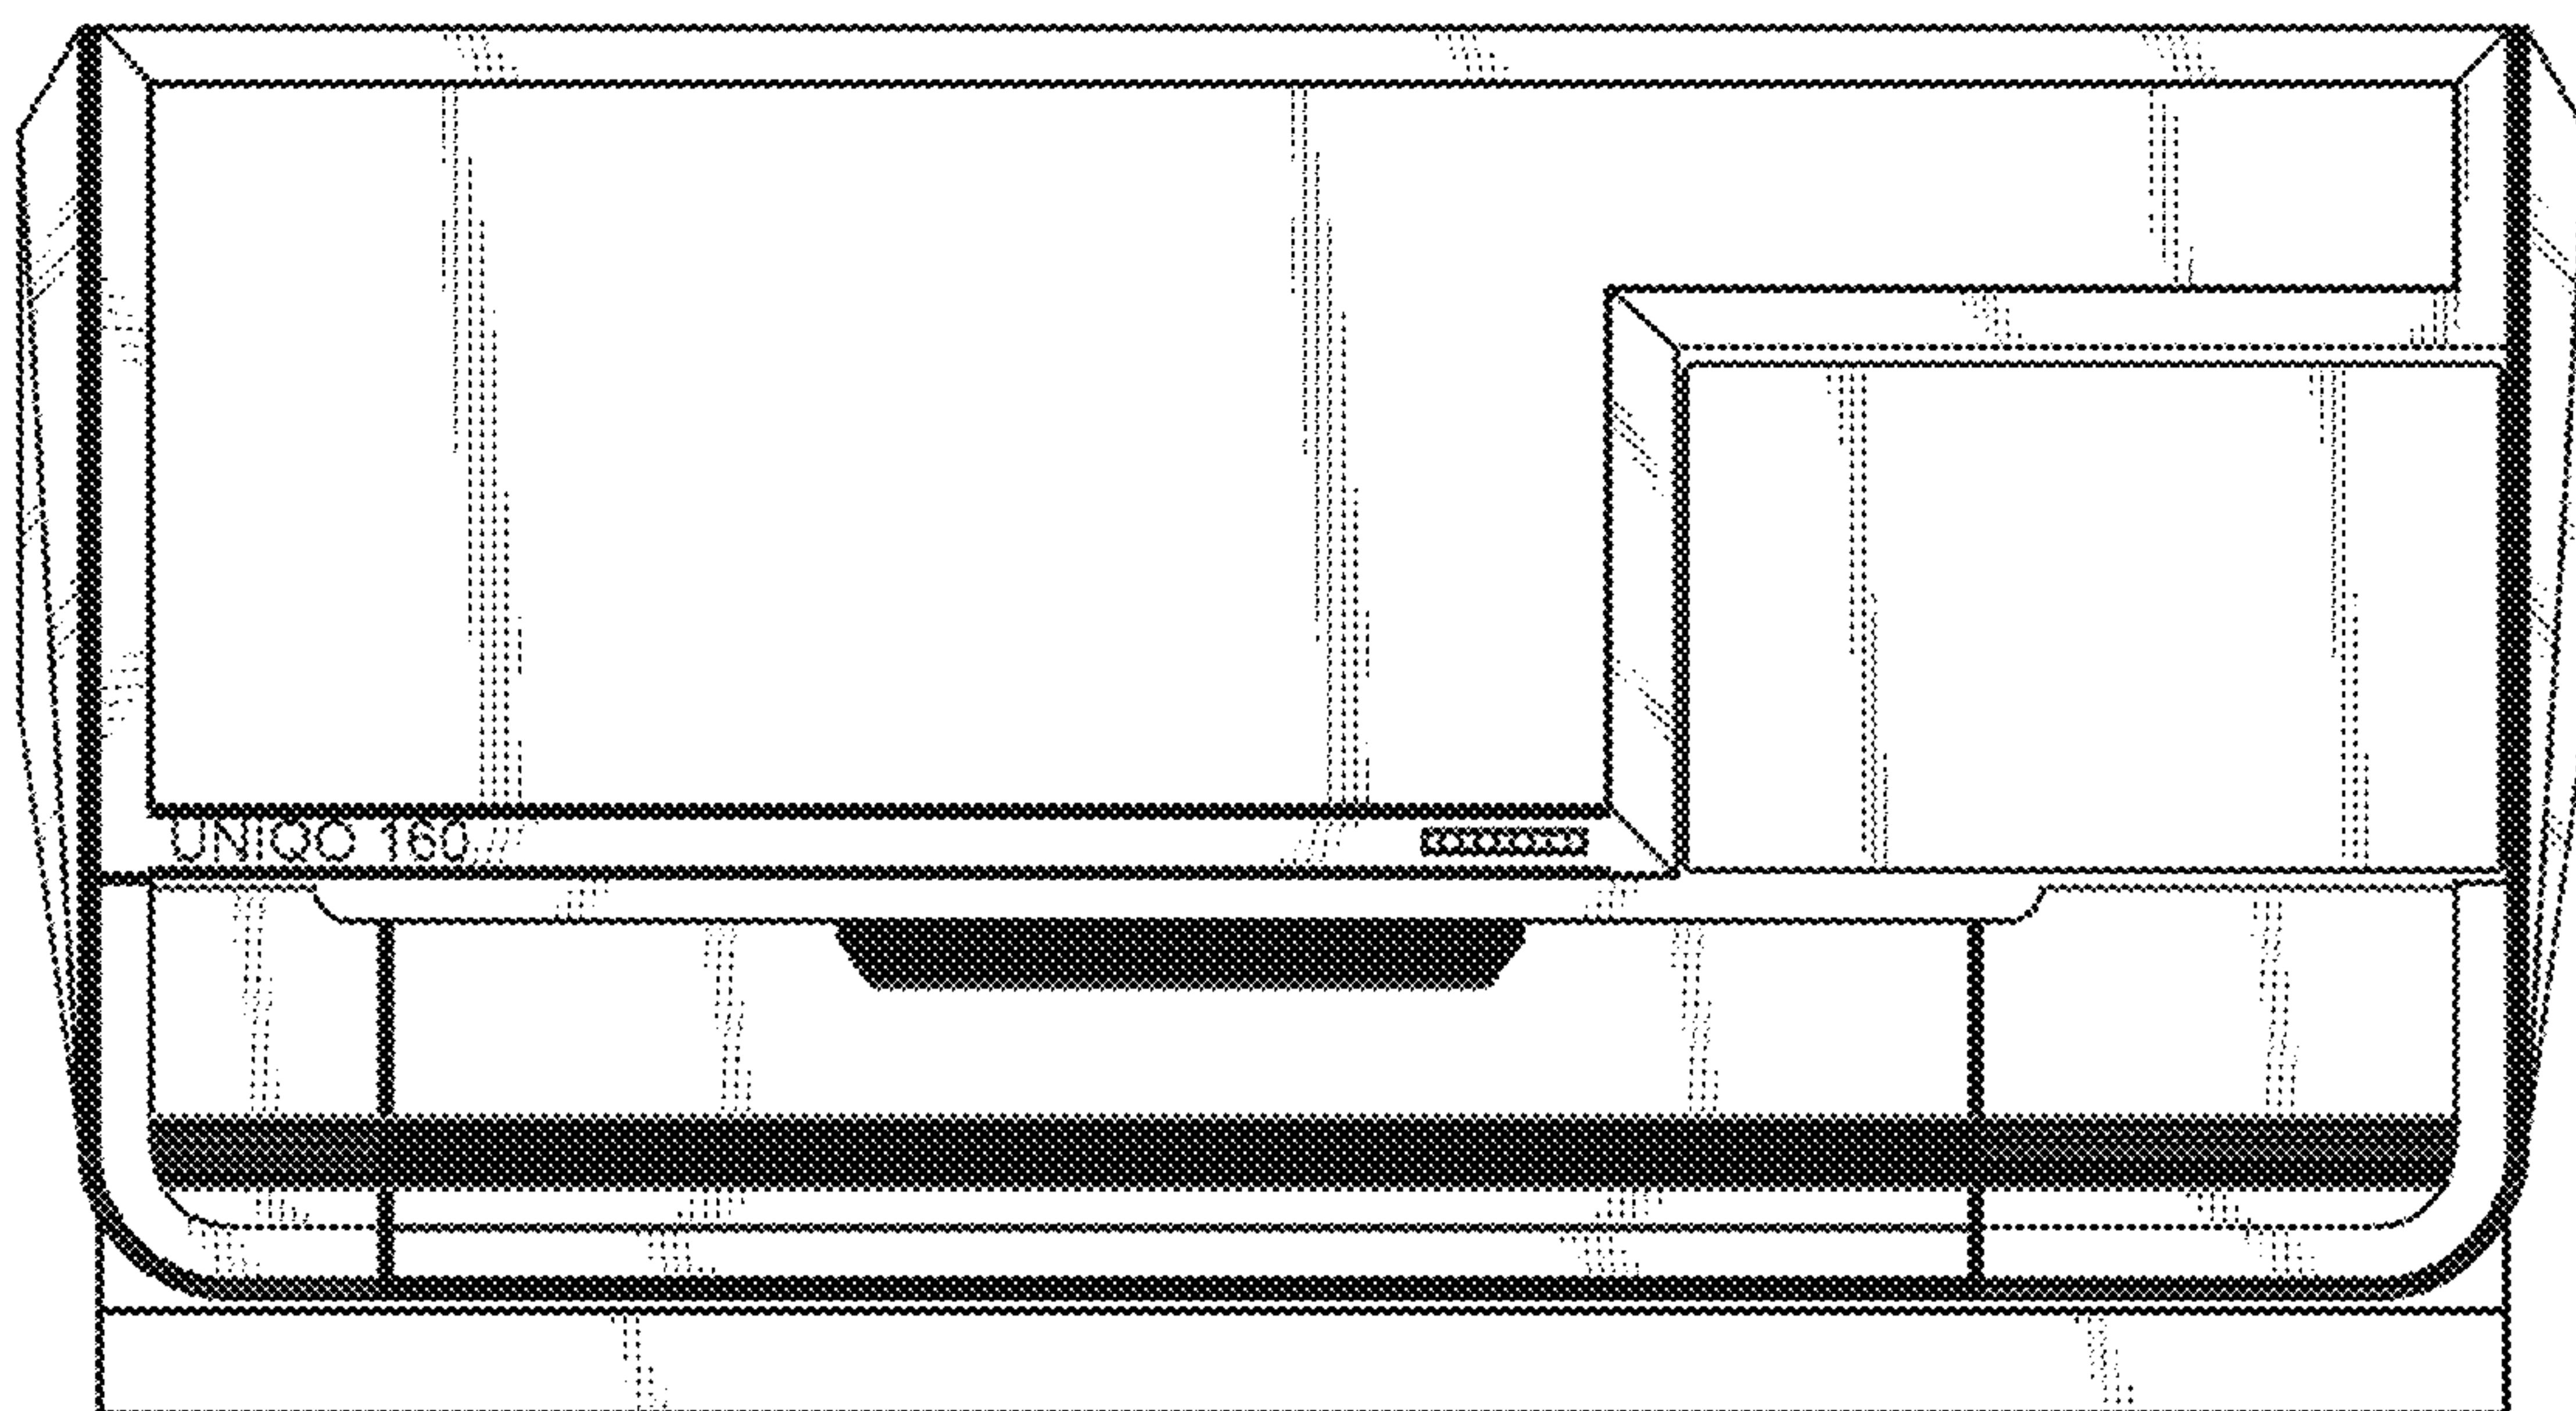


FIG. 9

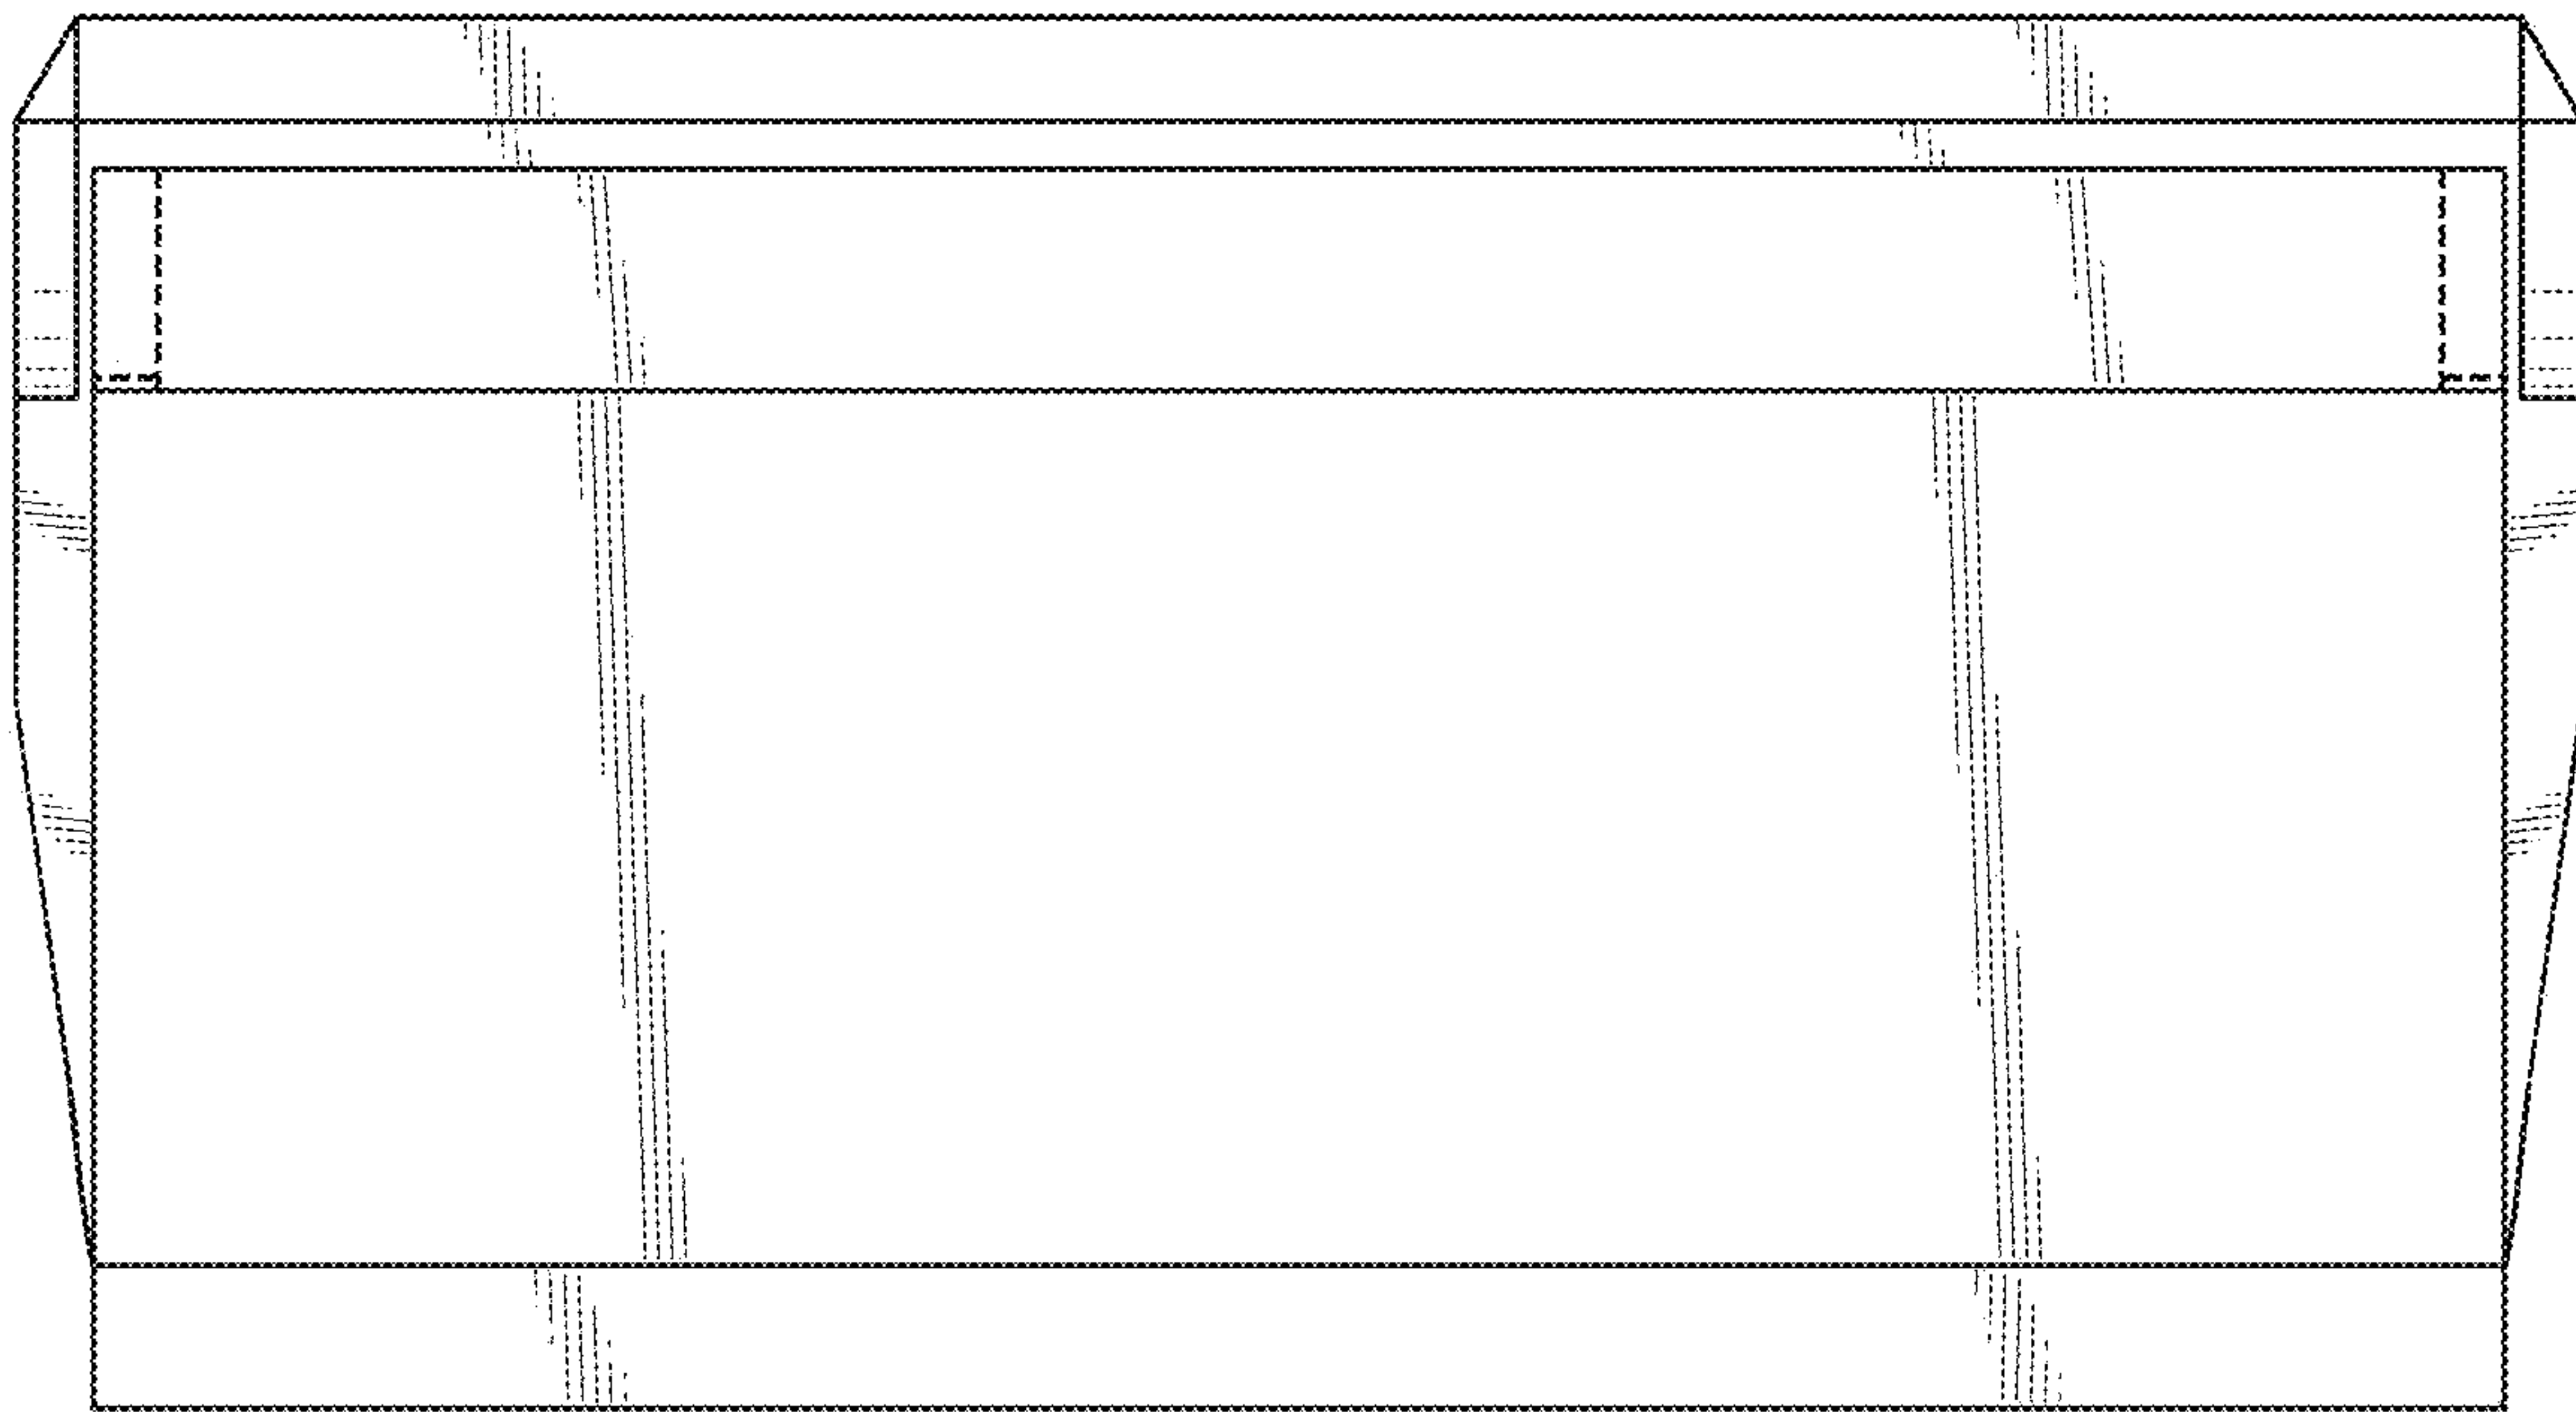


FIG. 10

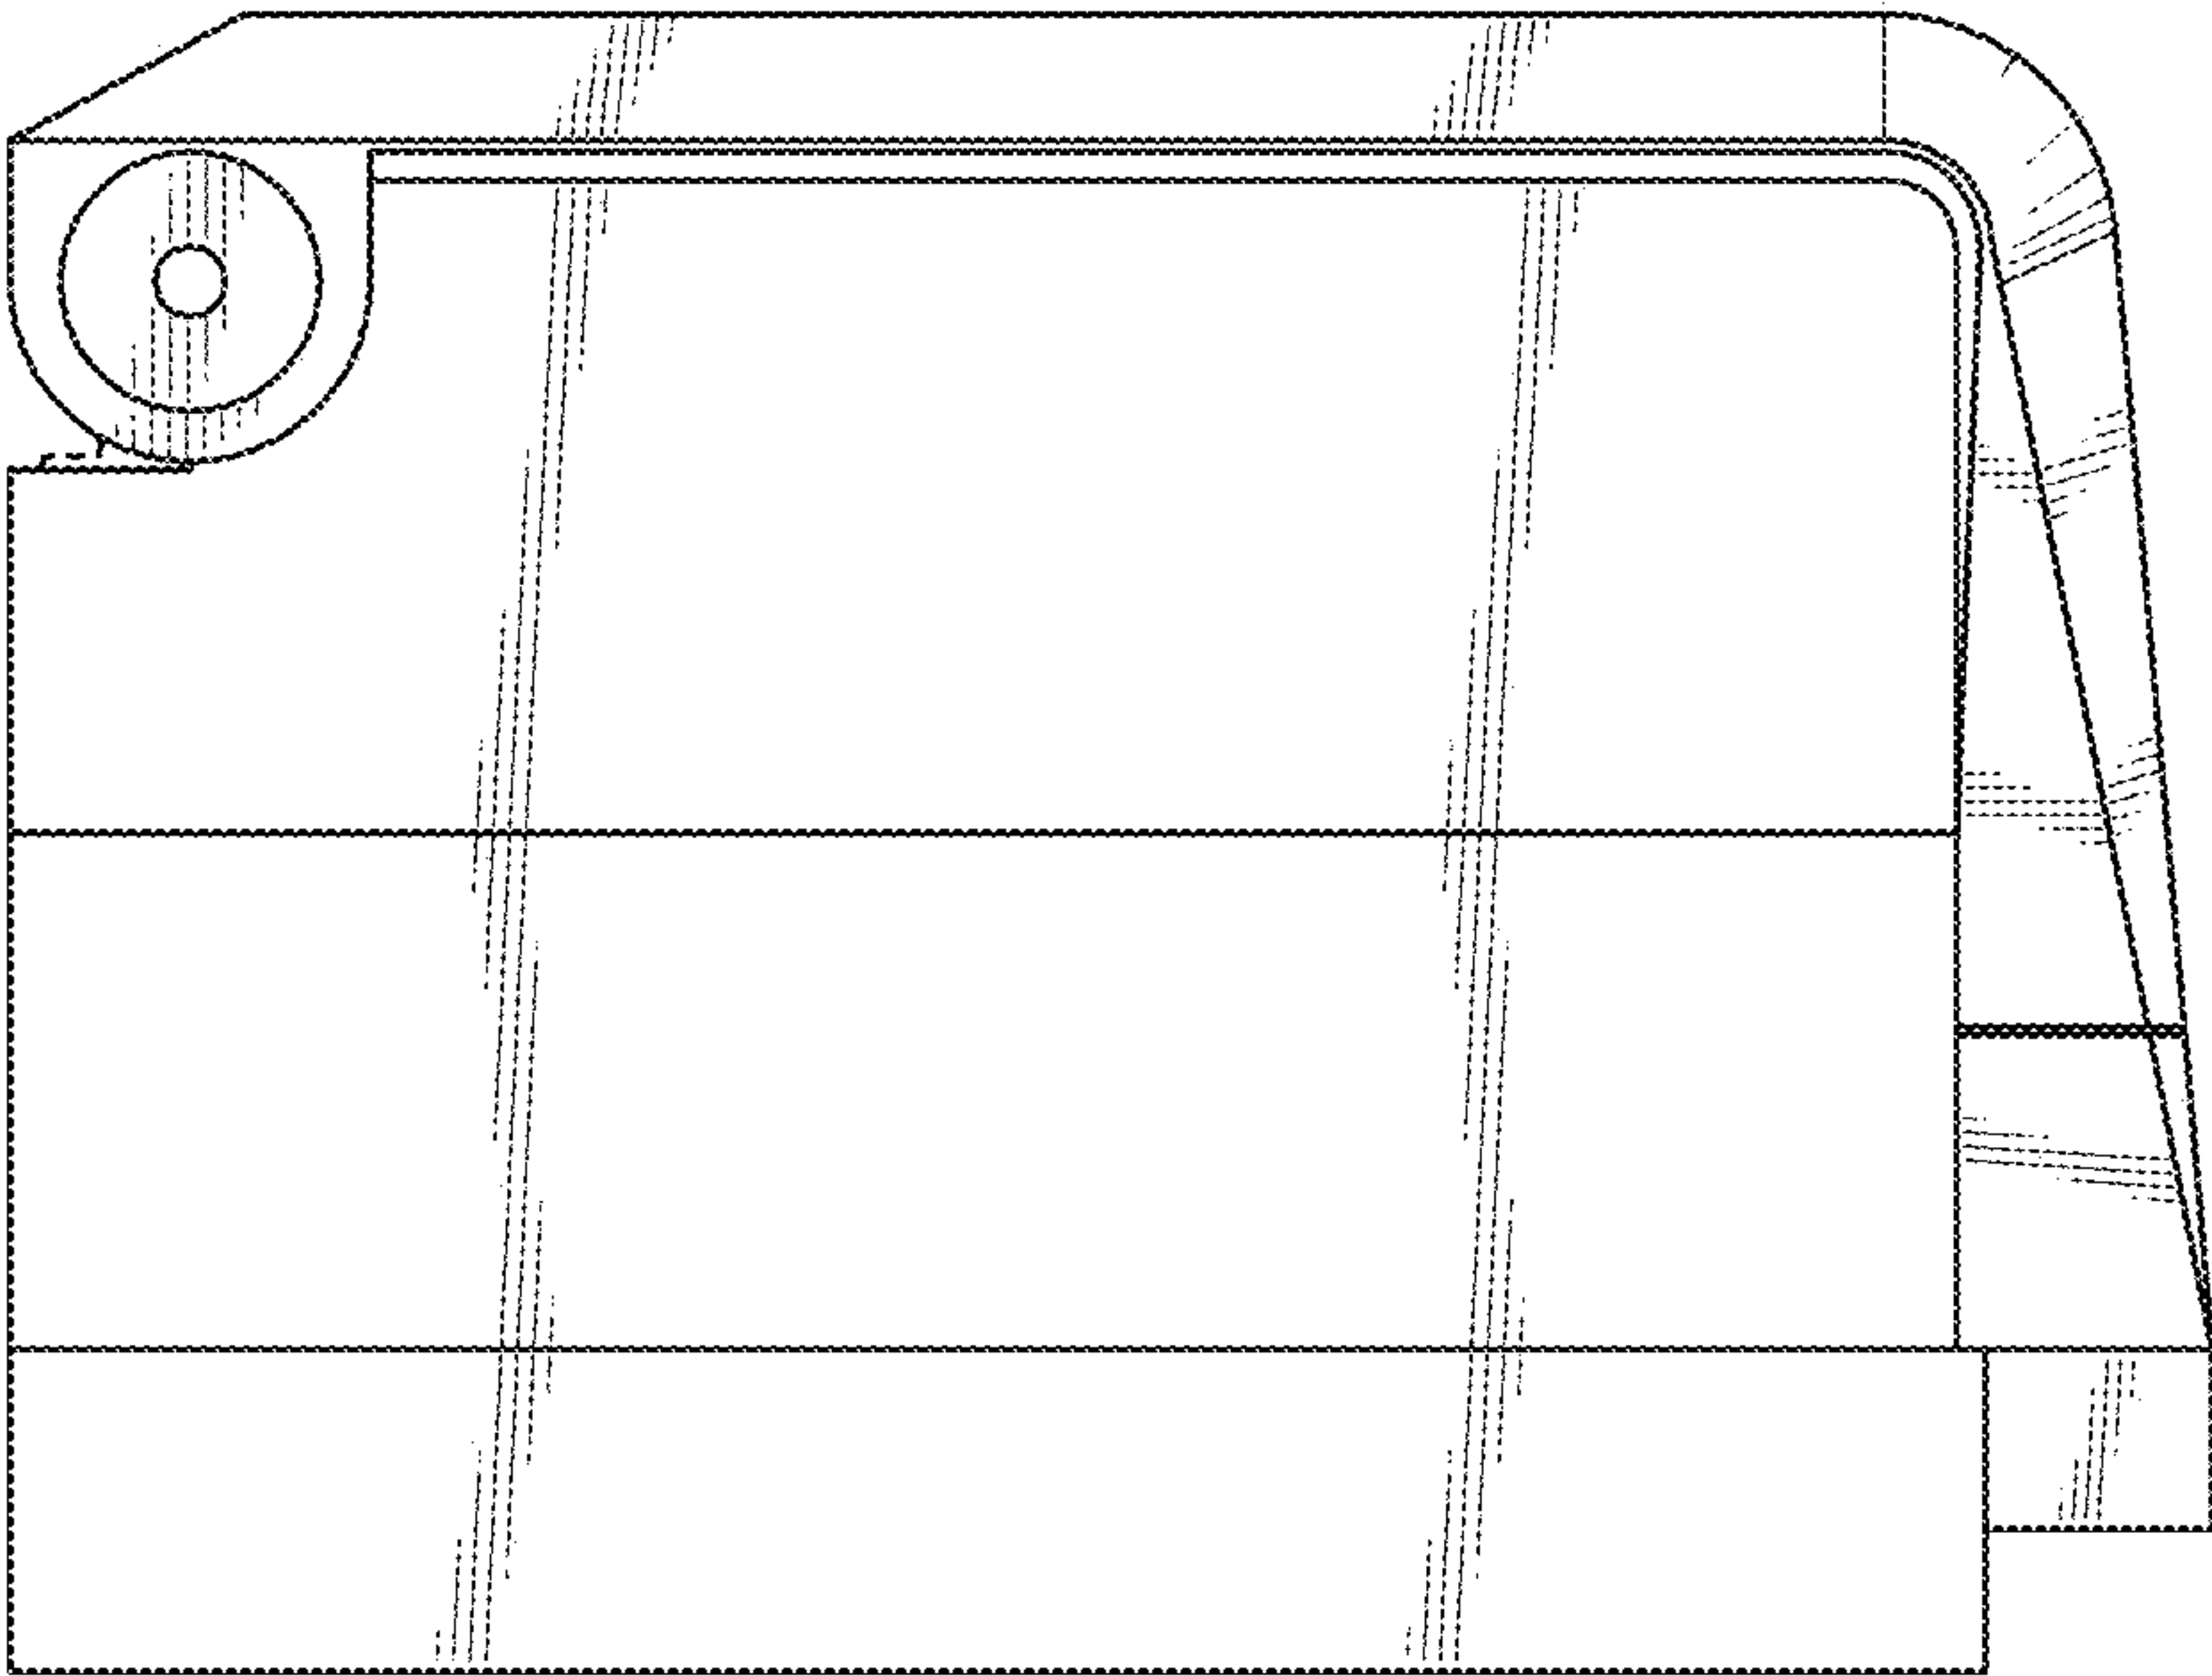


FIG. 11

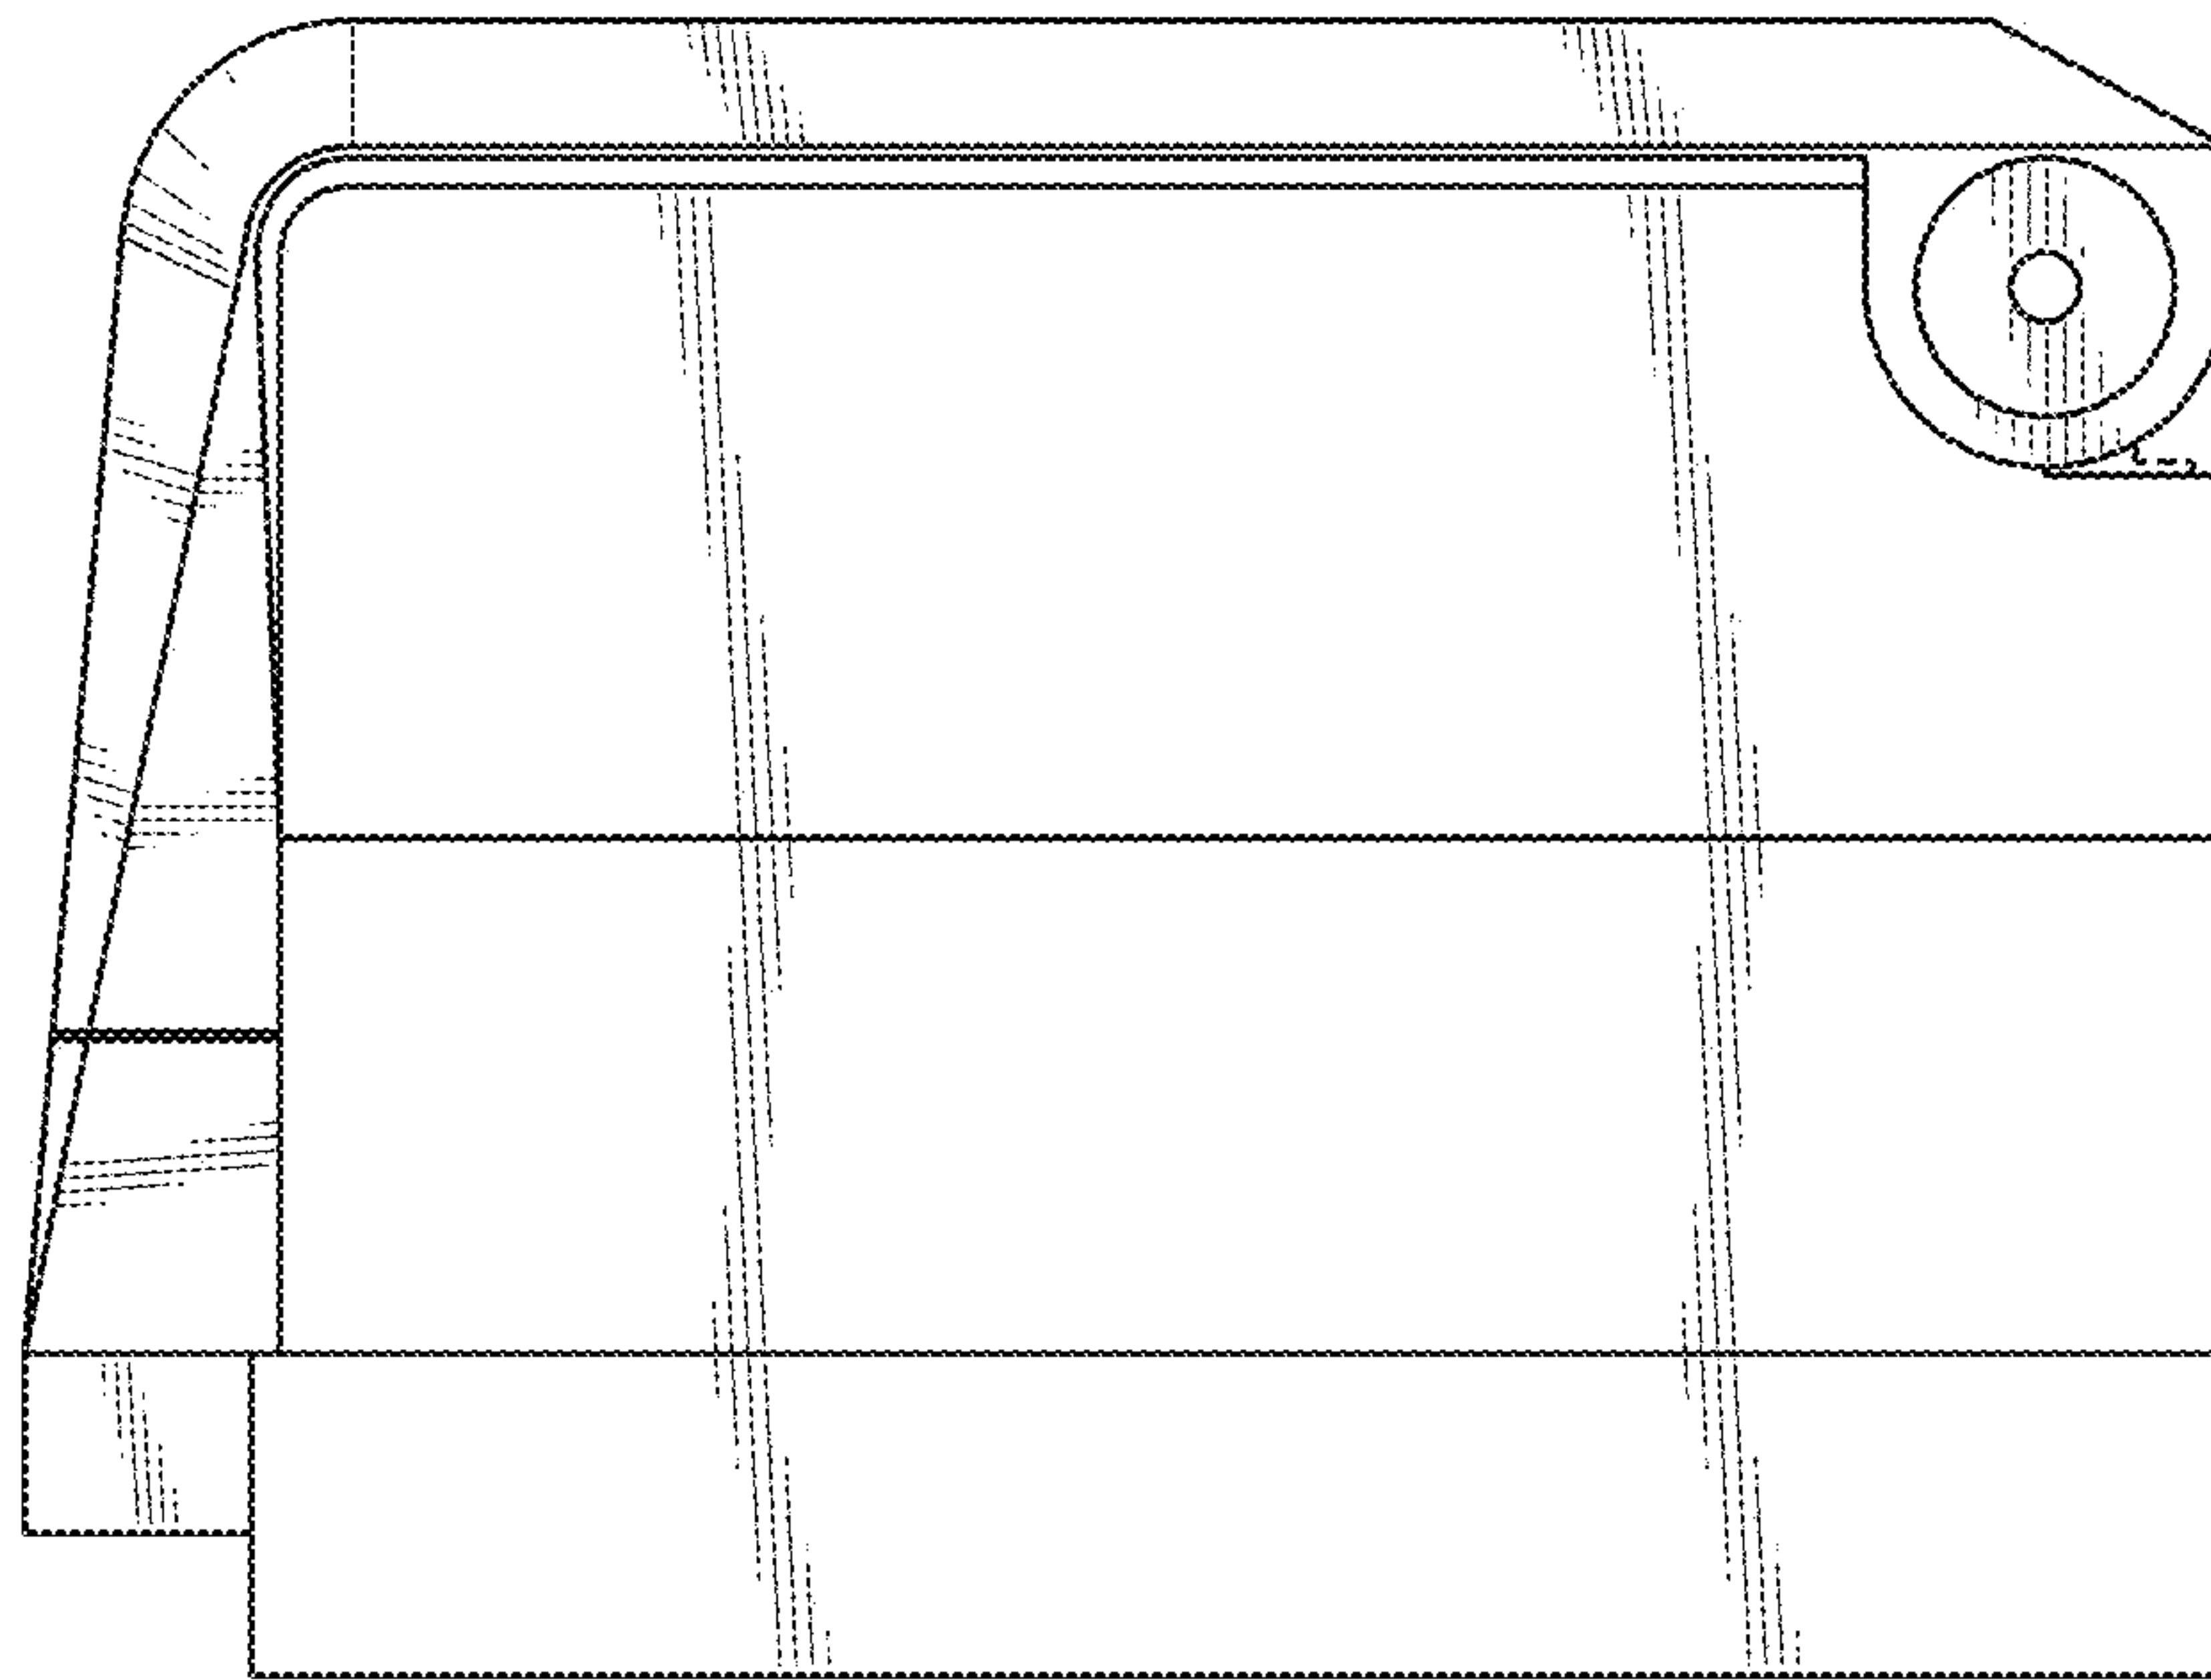


FIG. 12

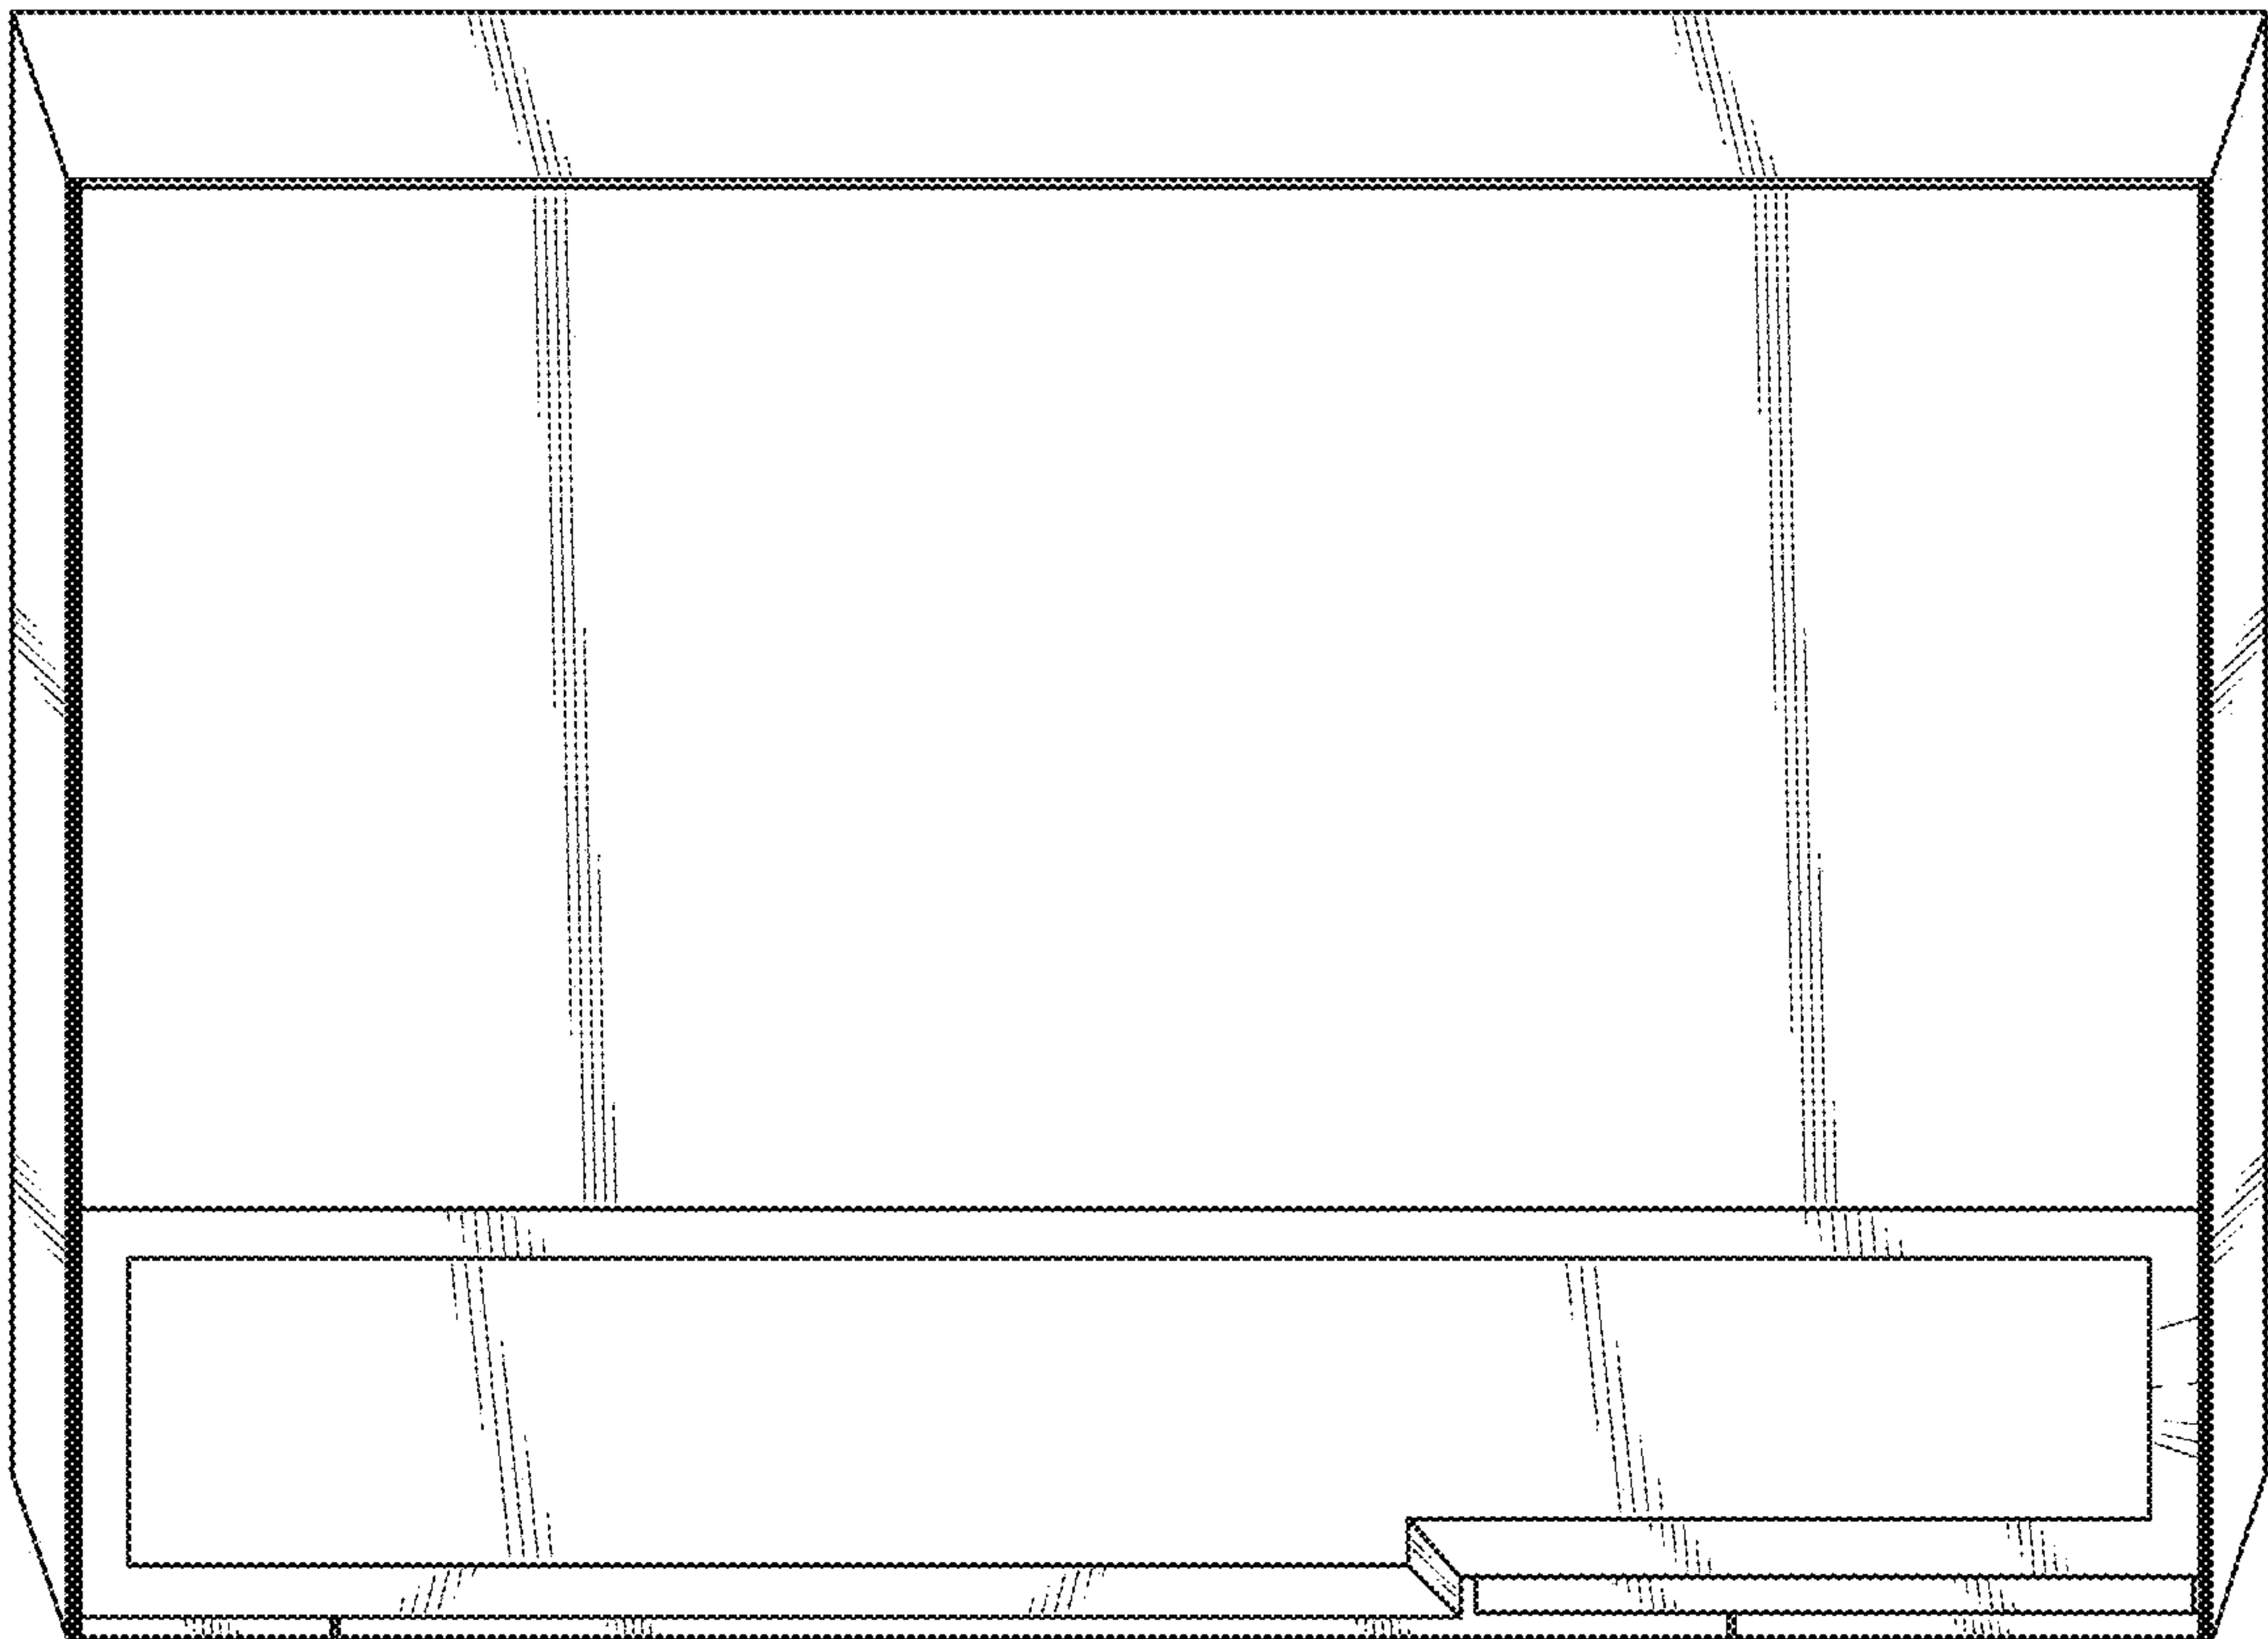


FIG. 13

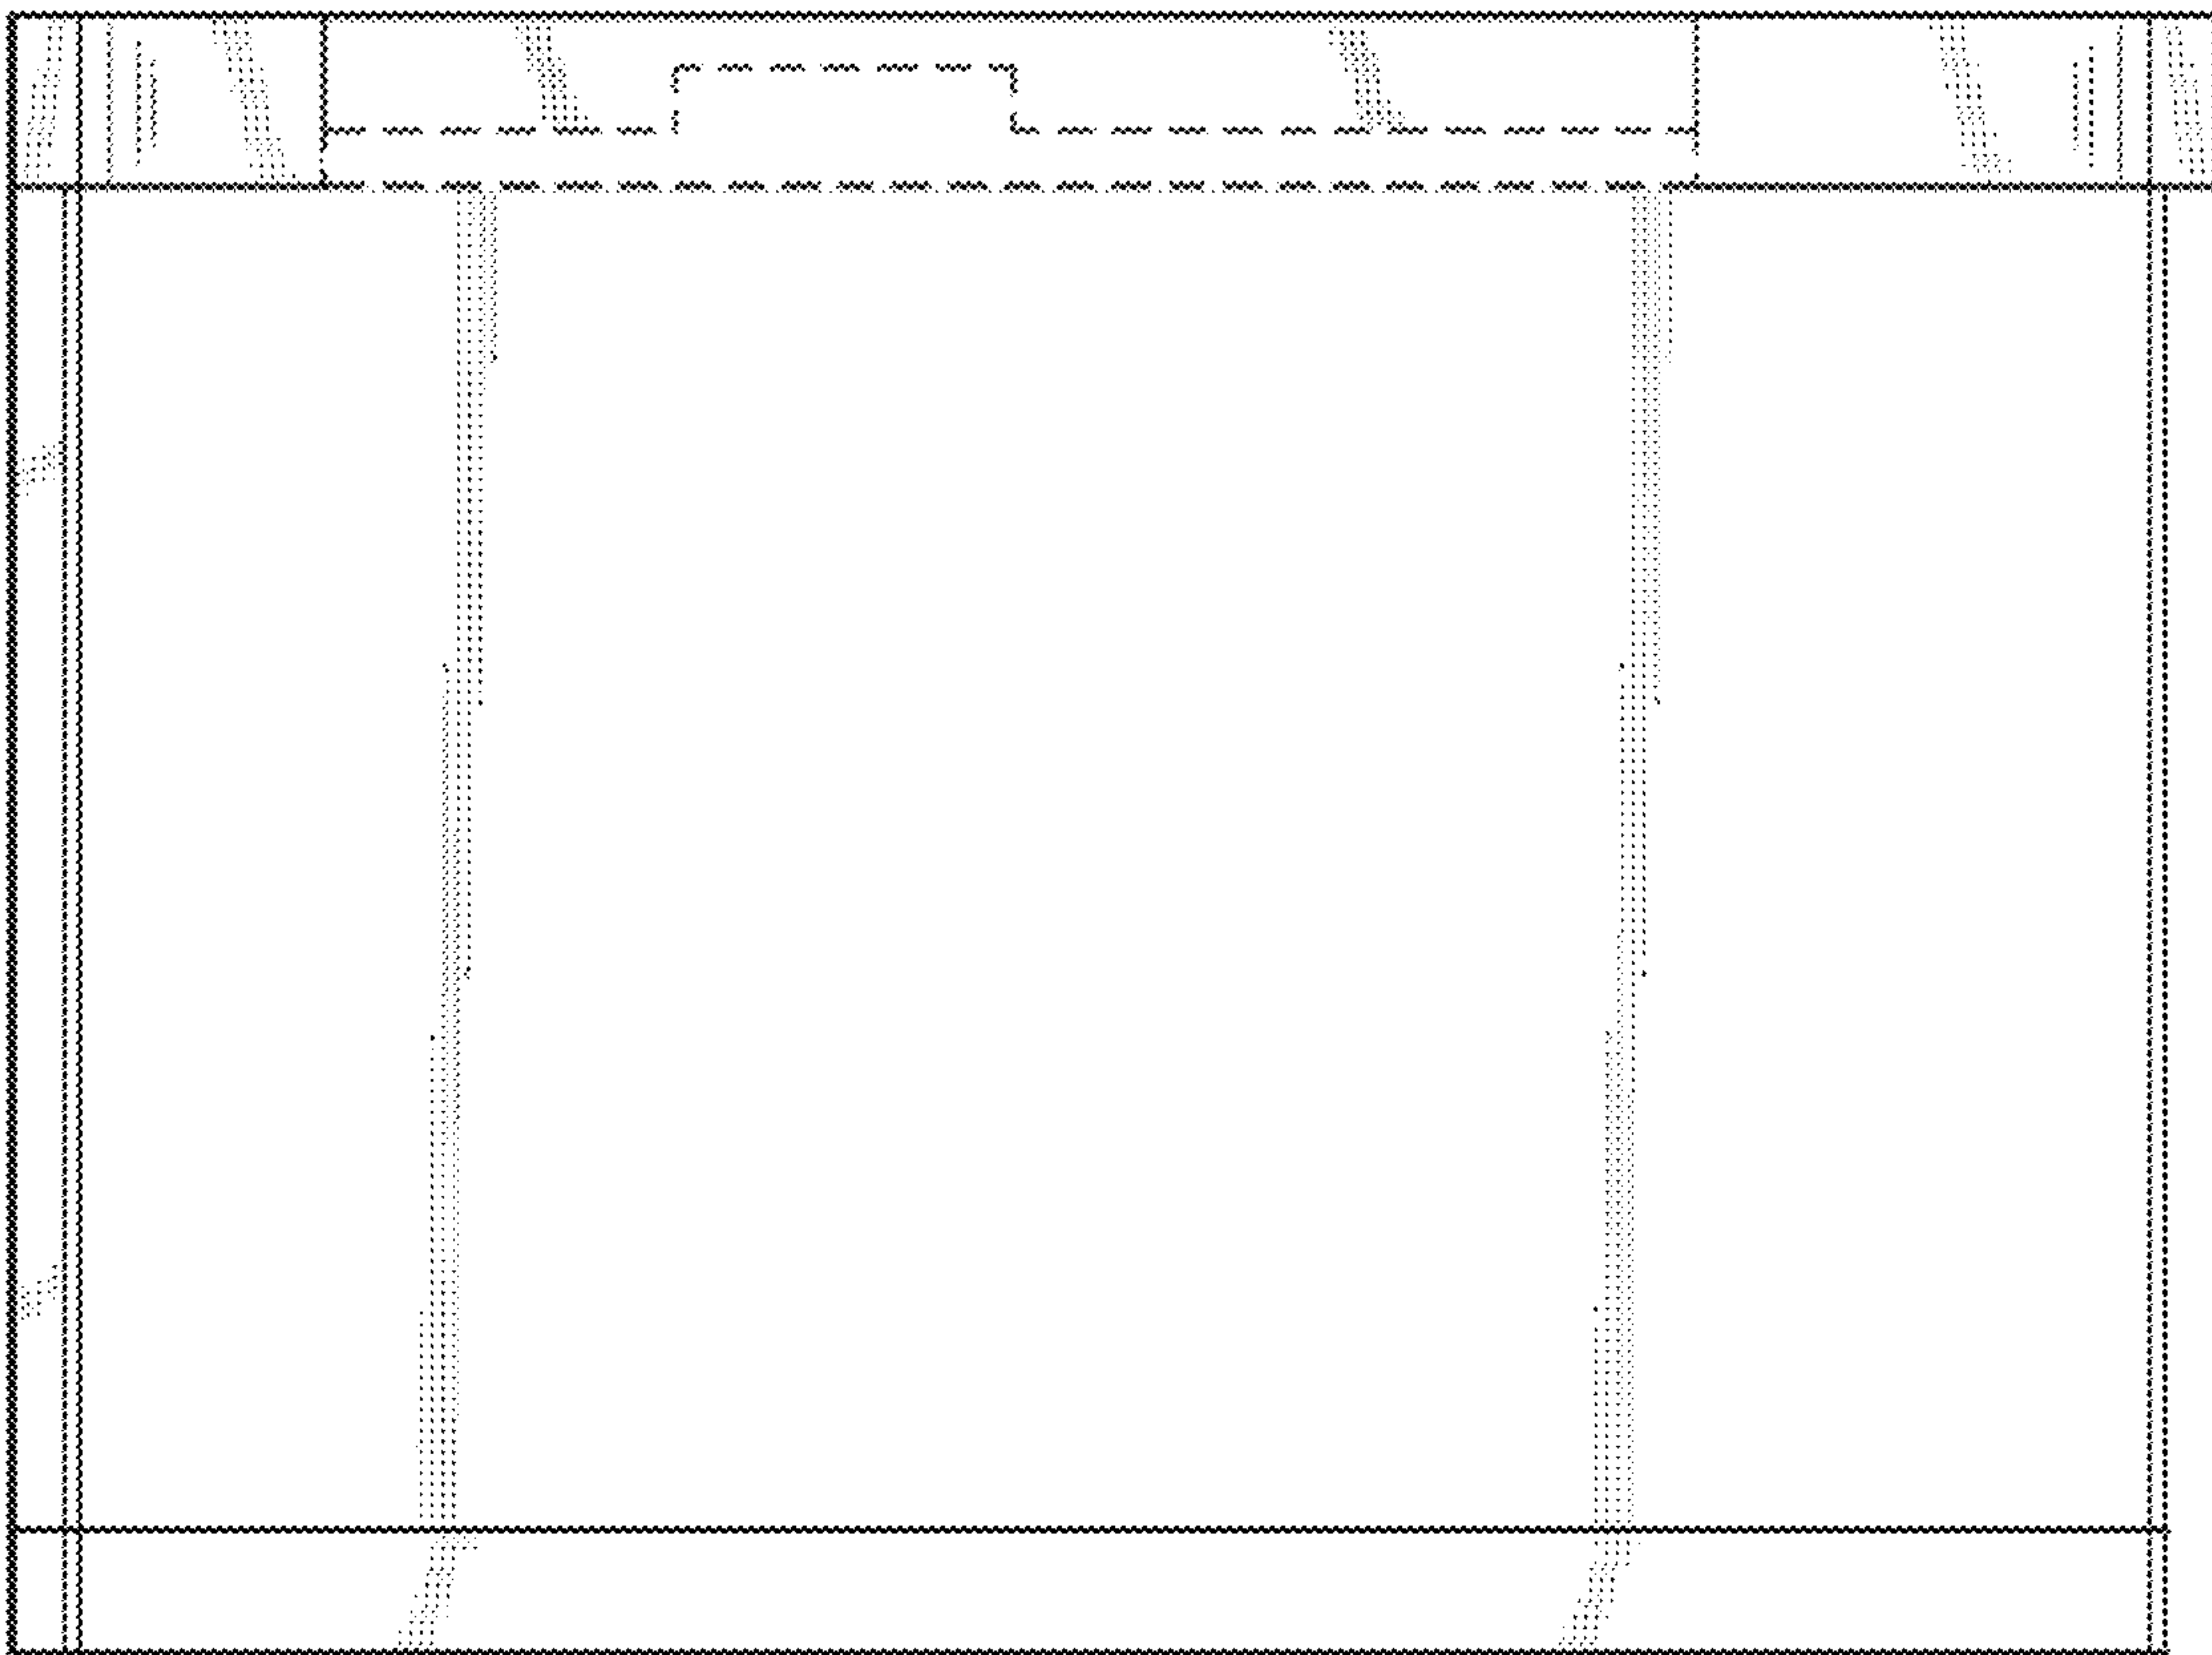


FIG. 14

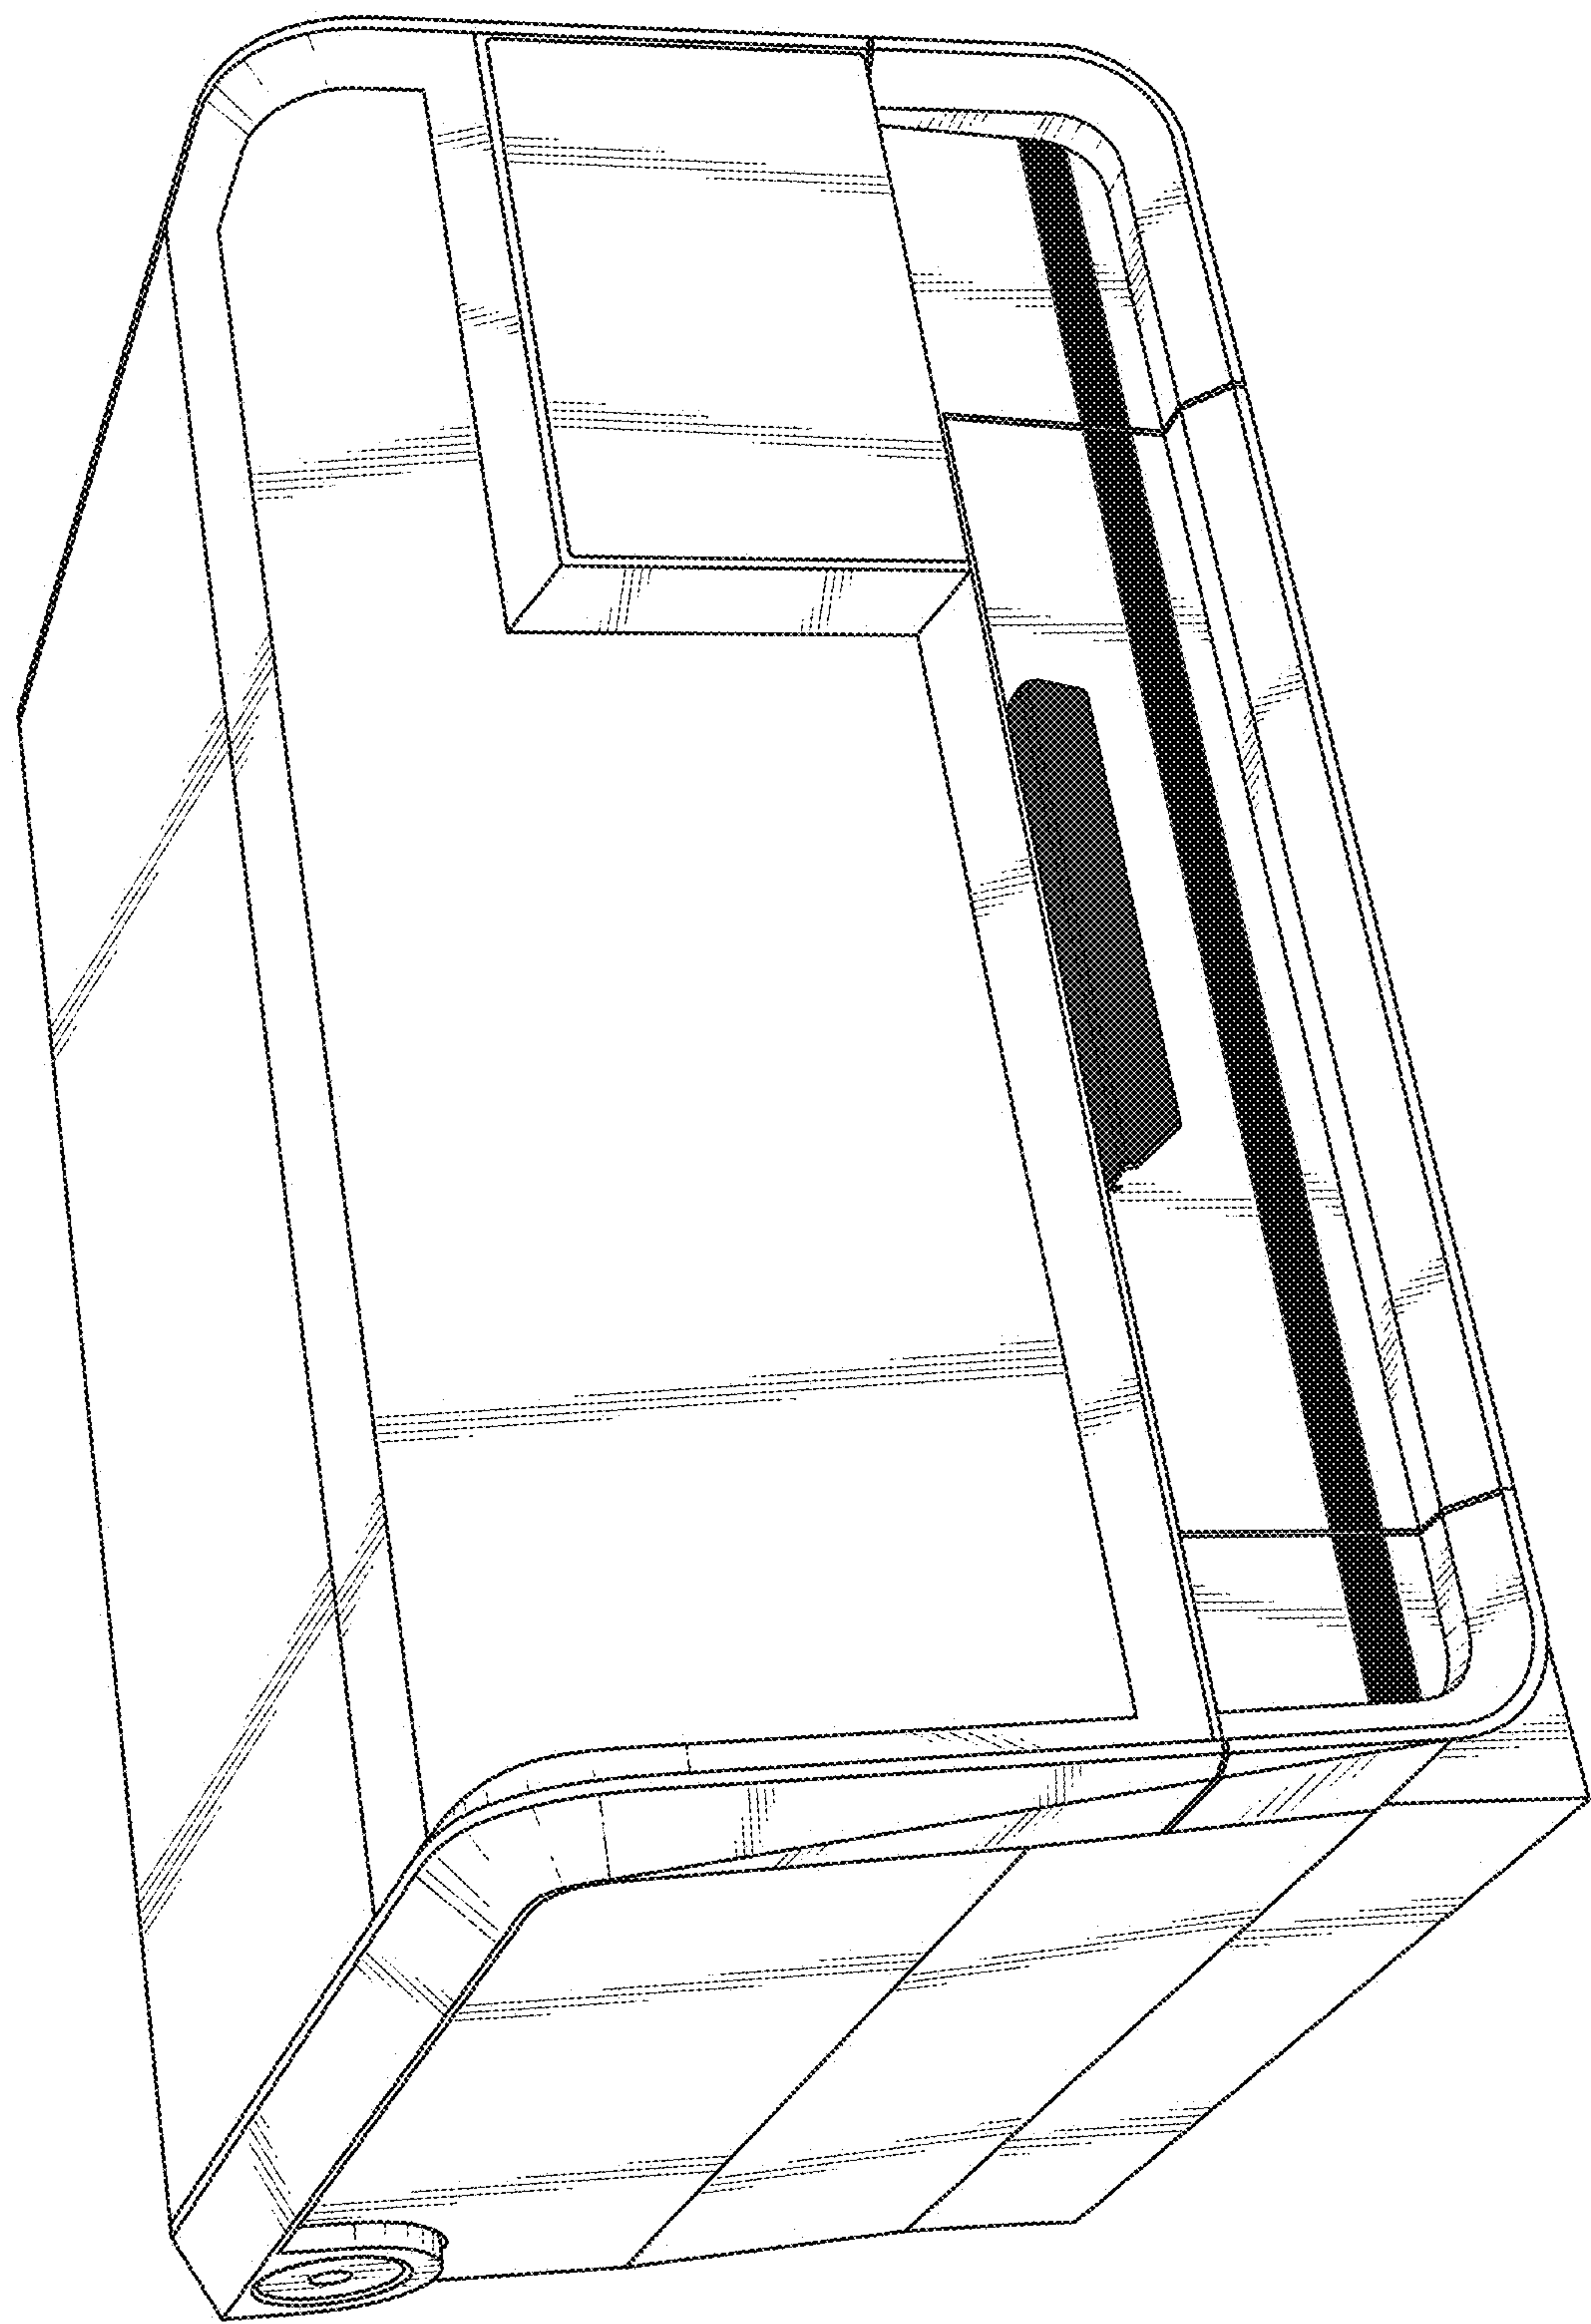


FIG. 15

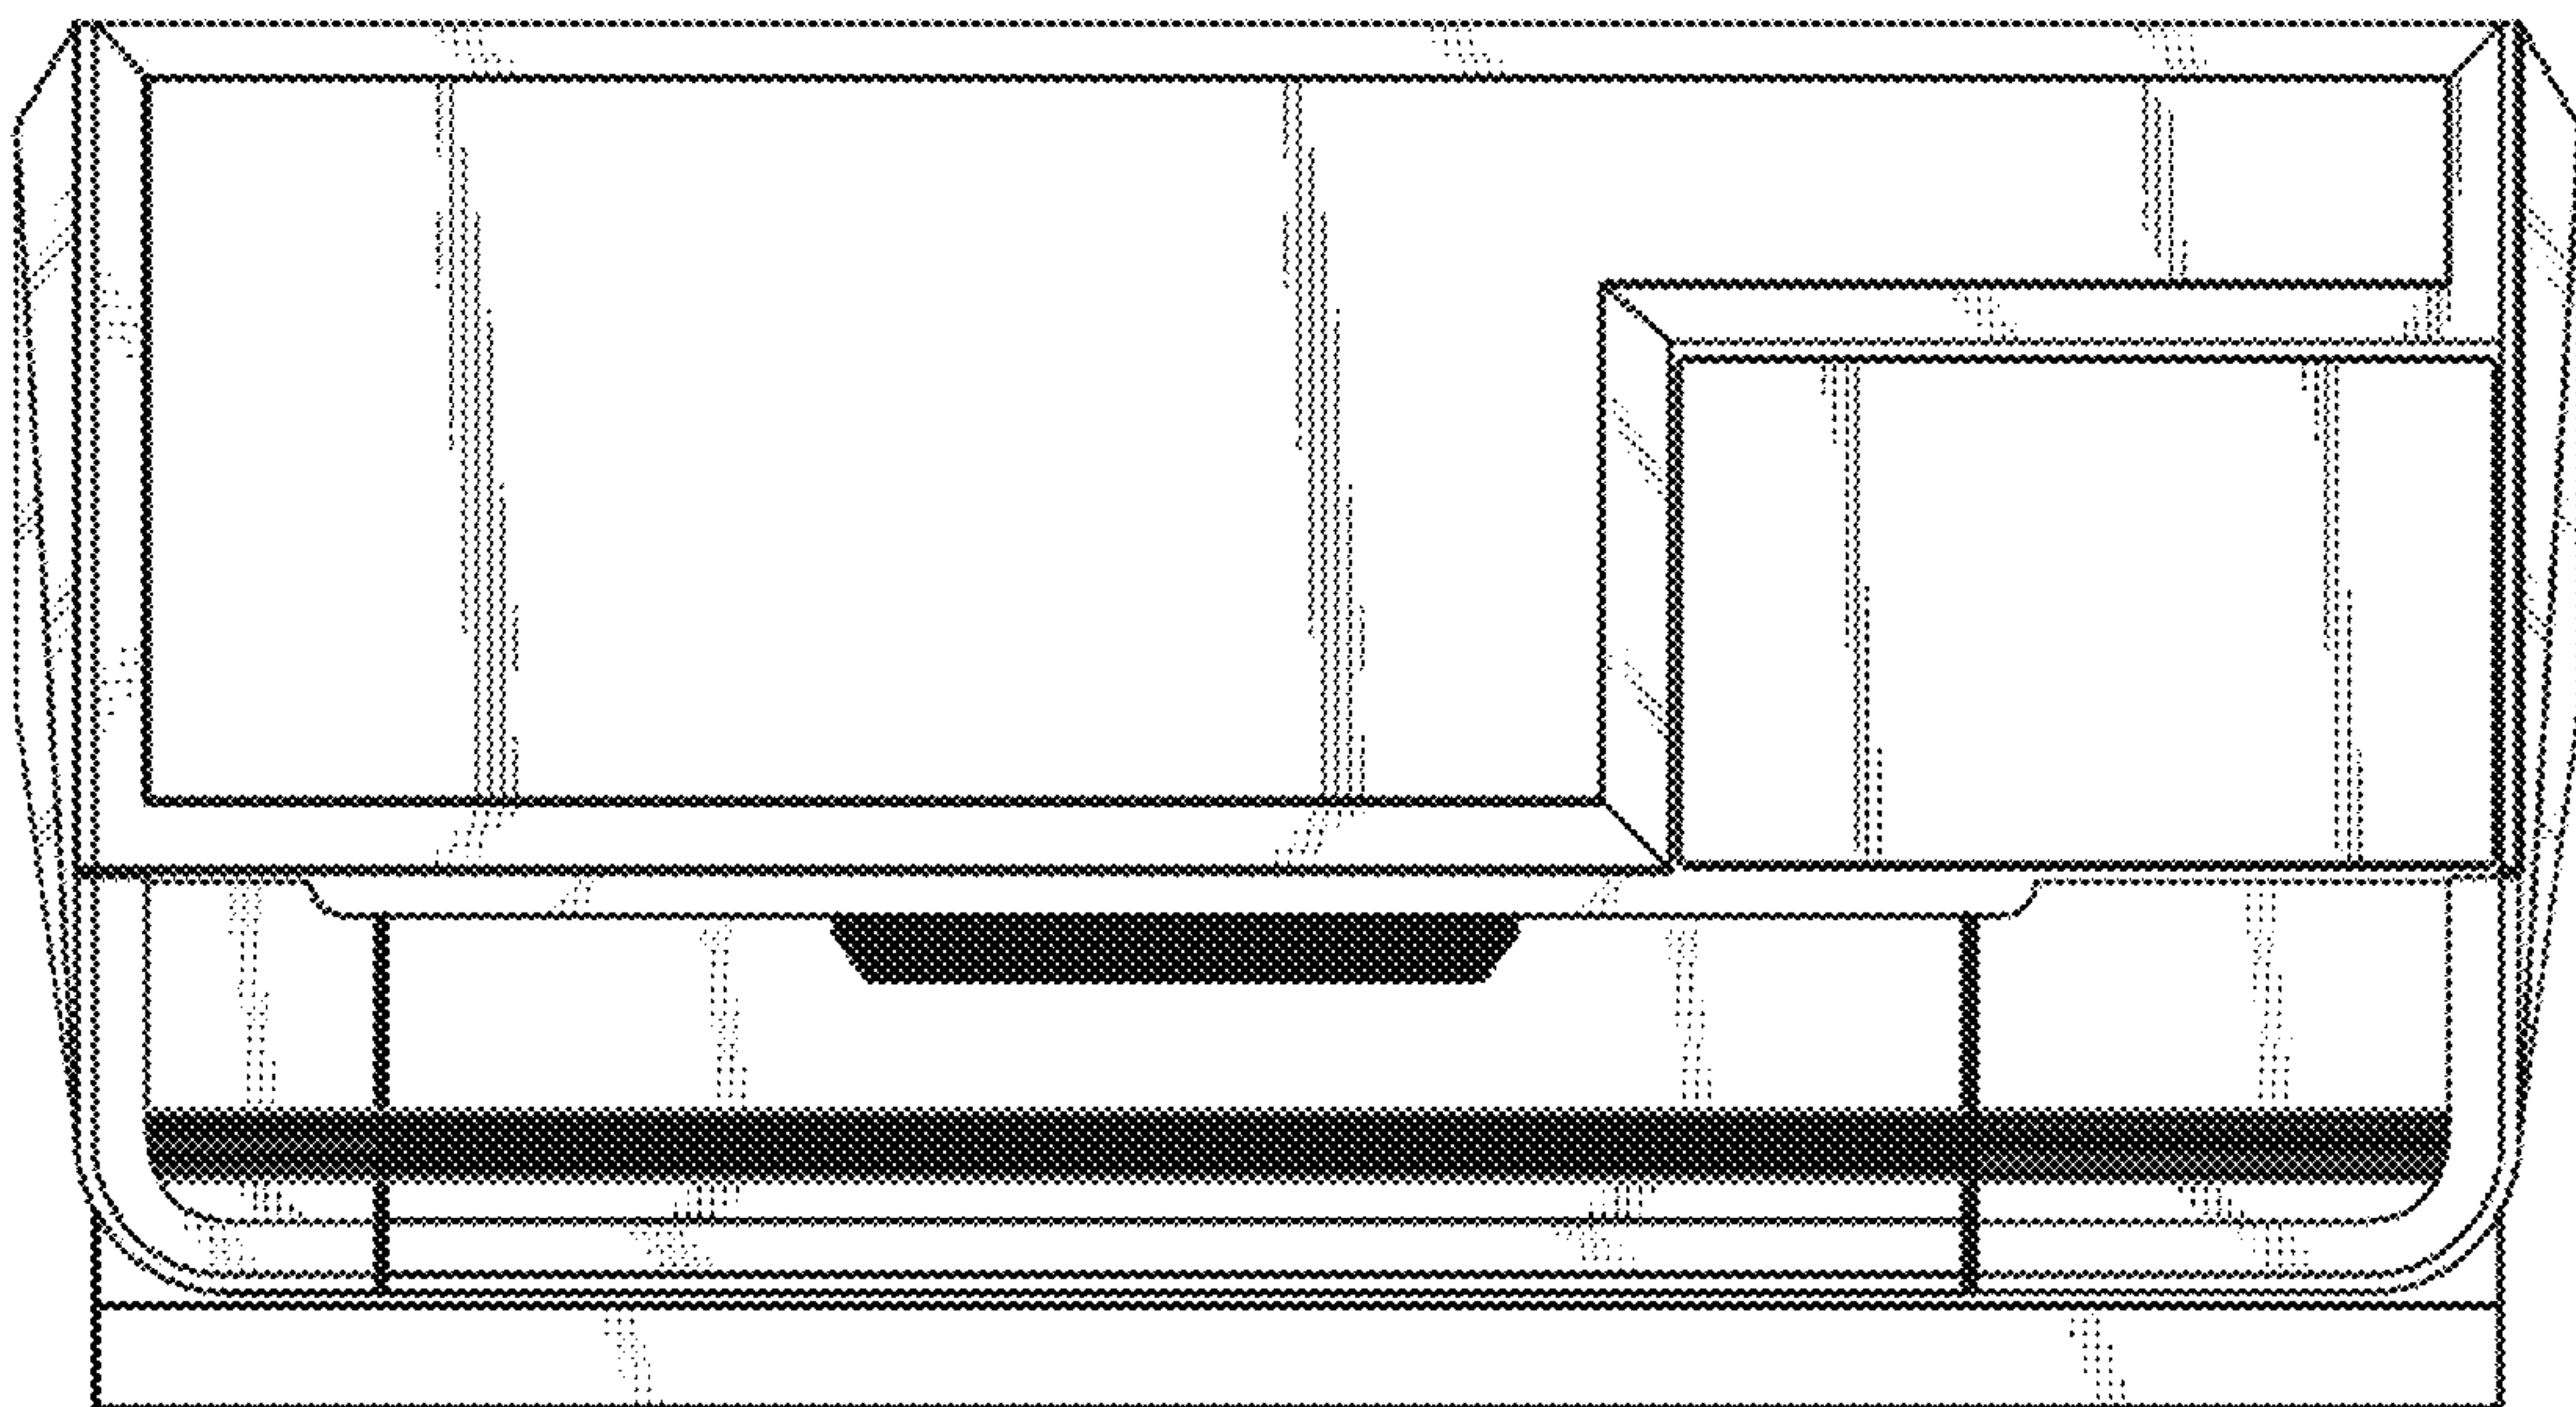


FIG. 16

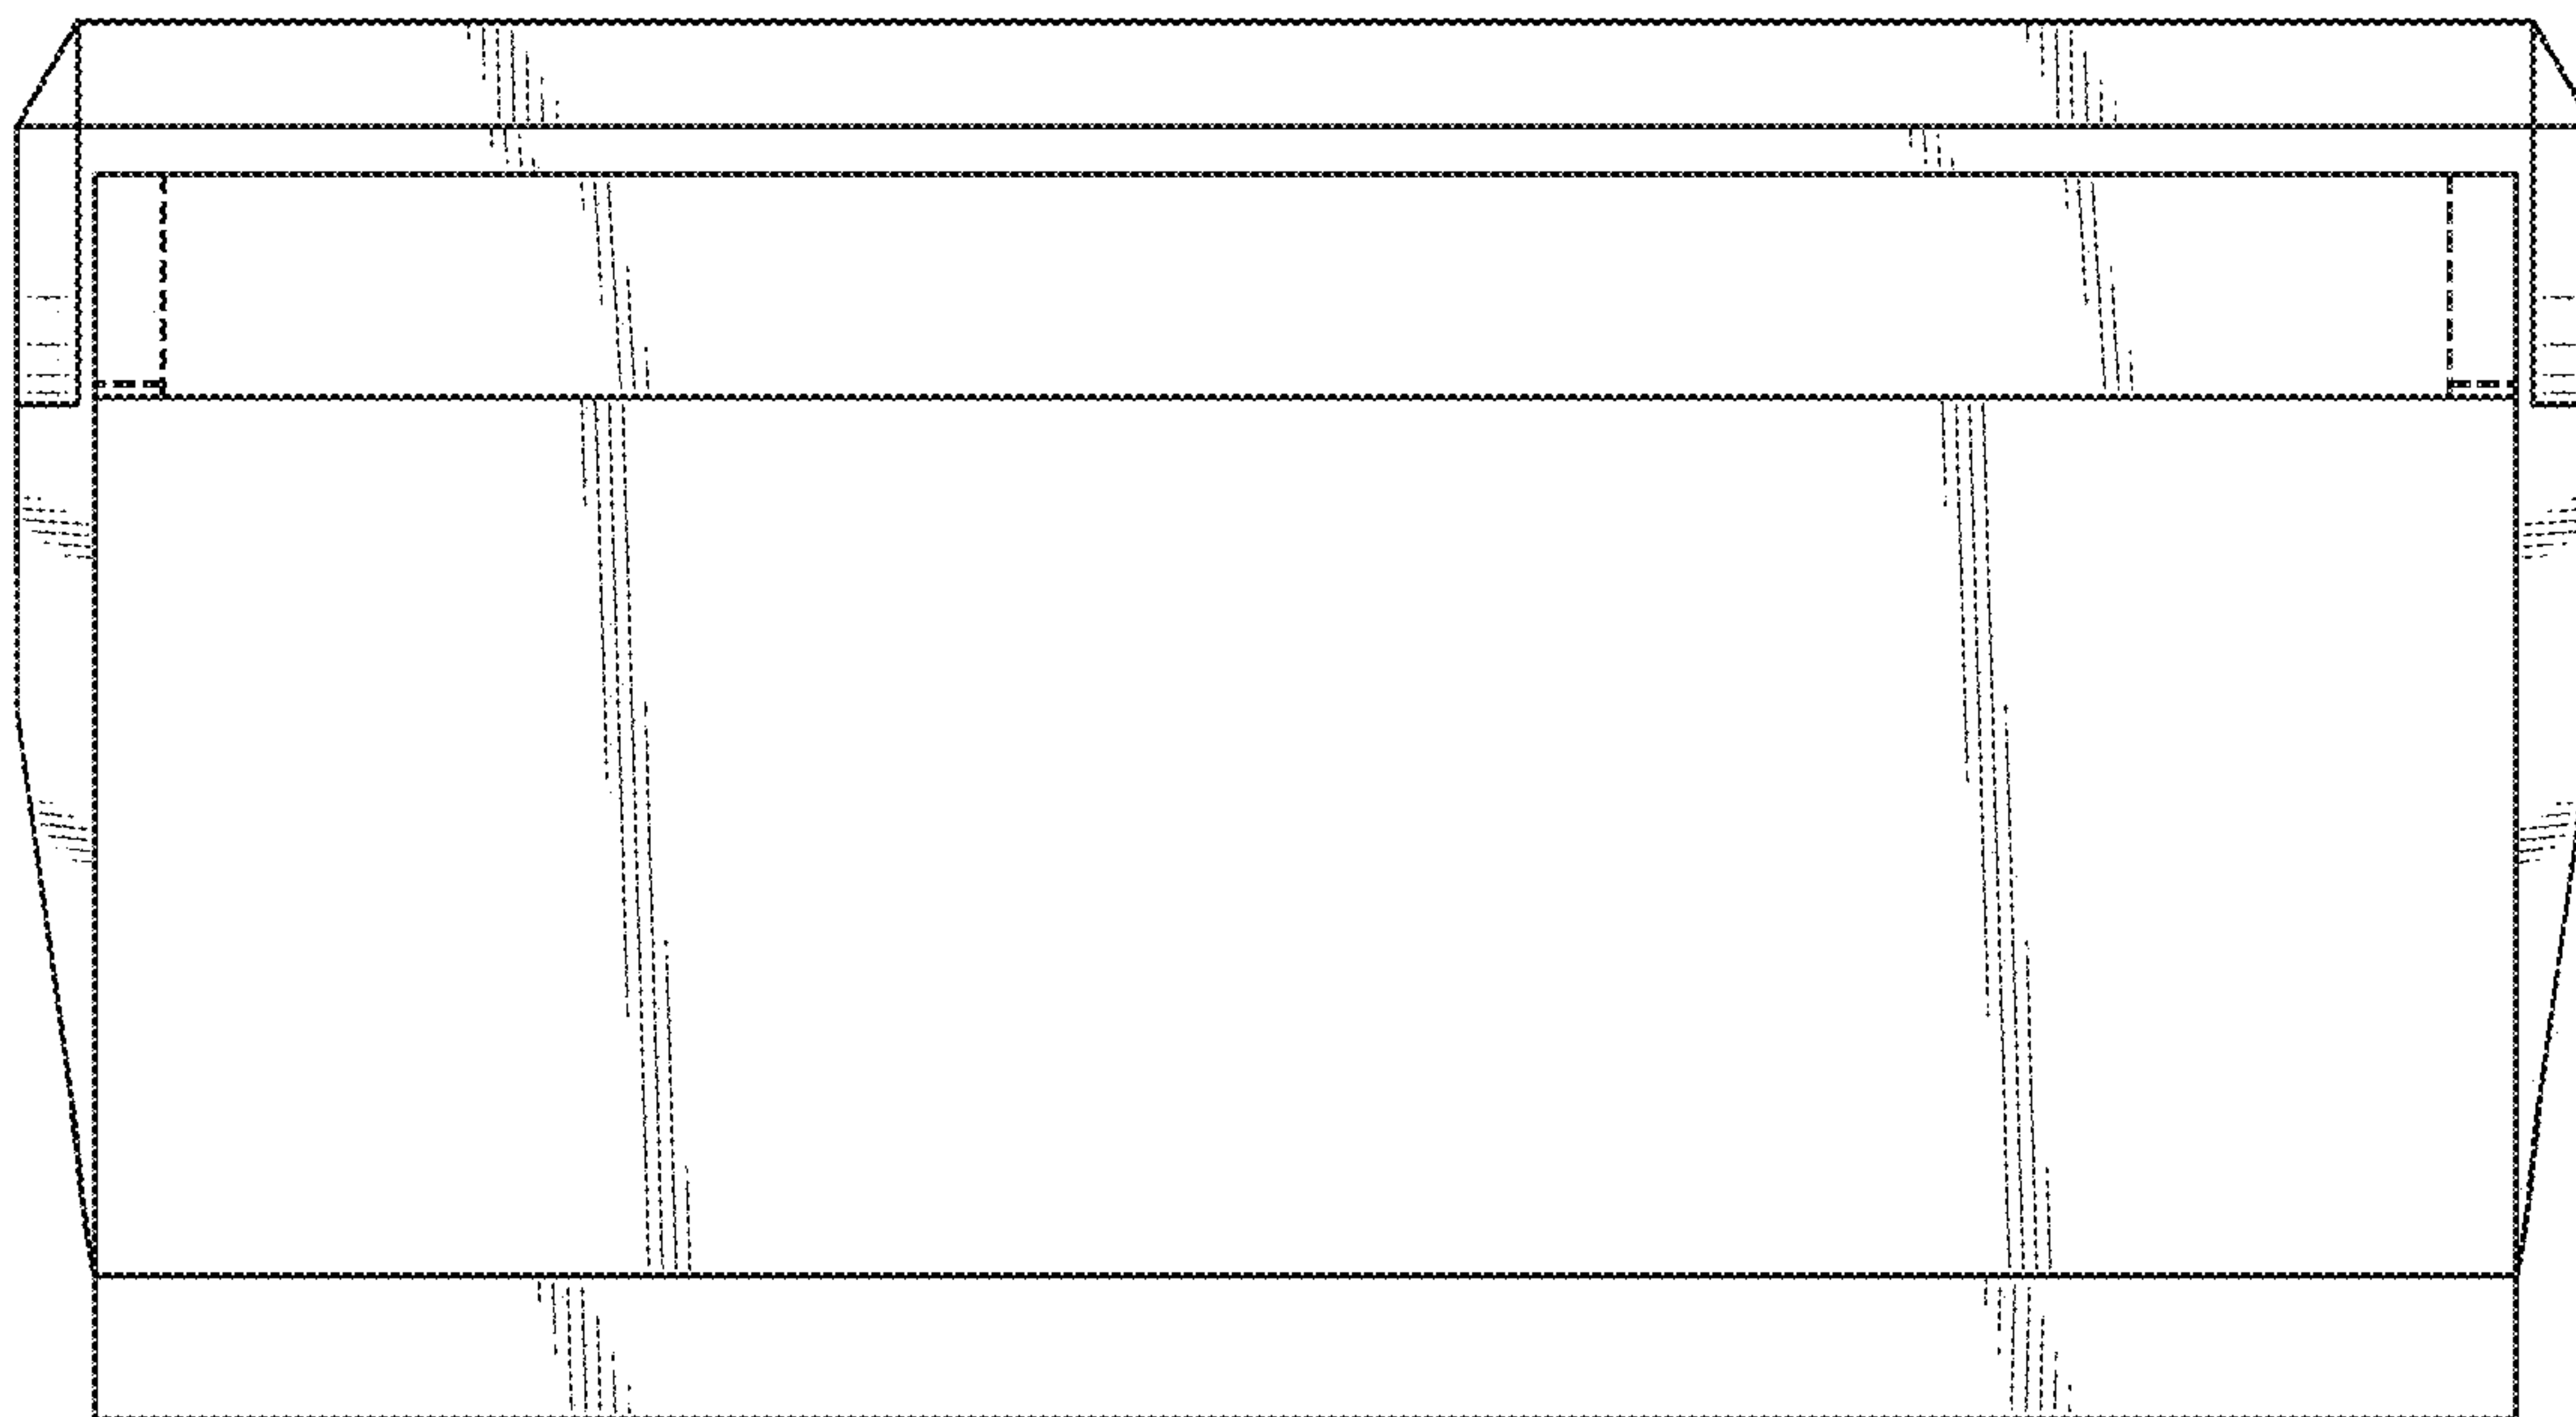


FIG. 17

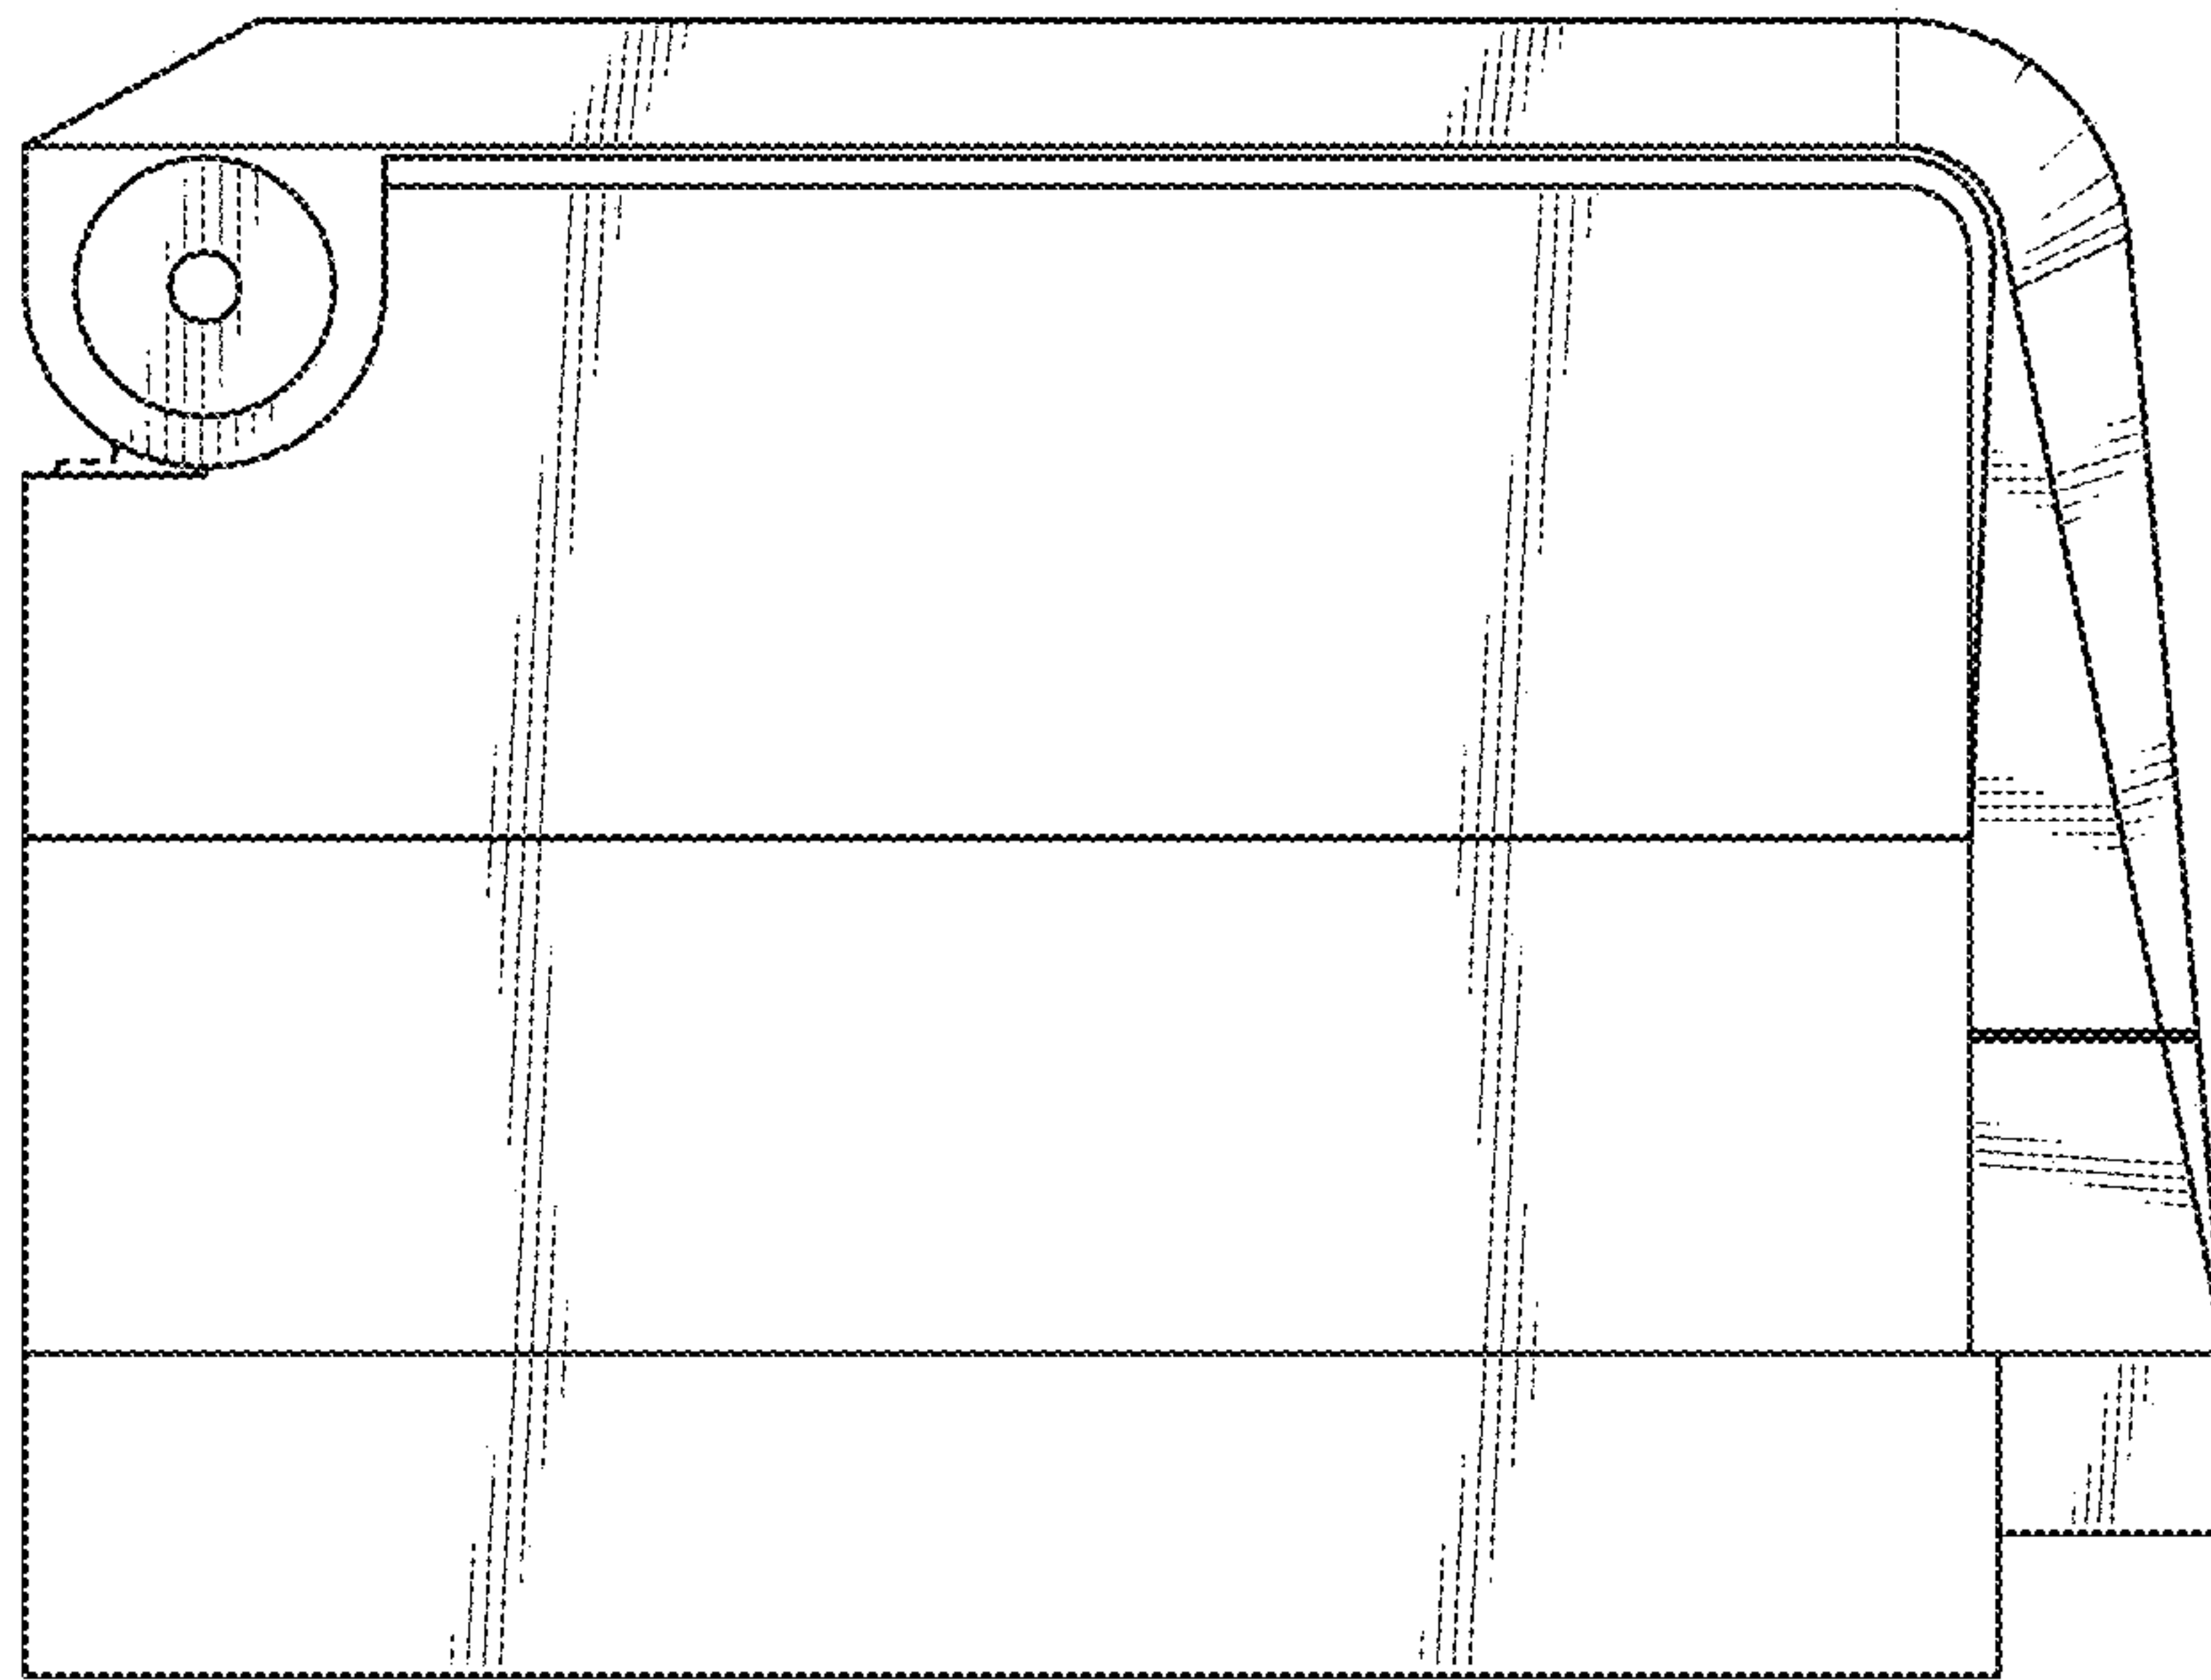


FIG. 18

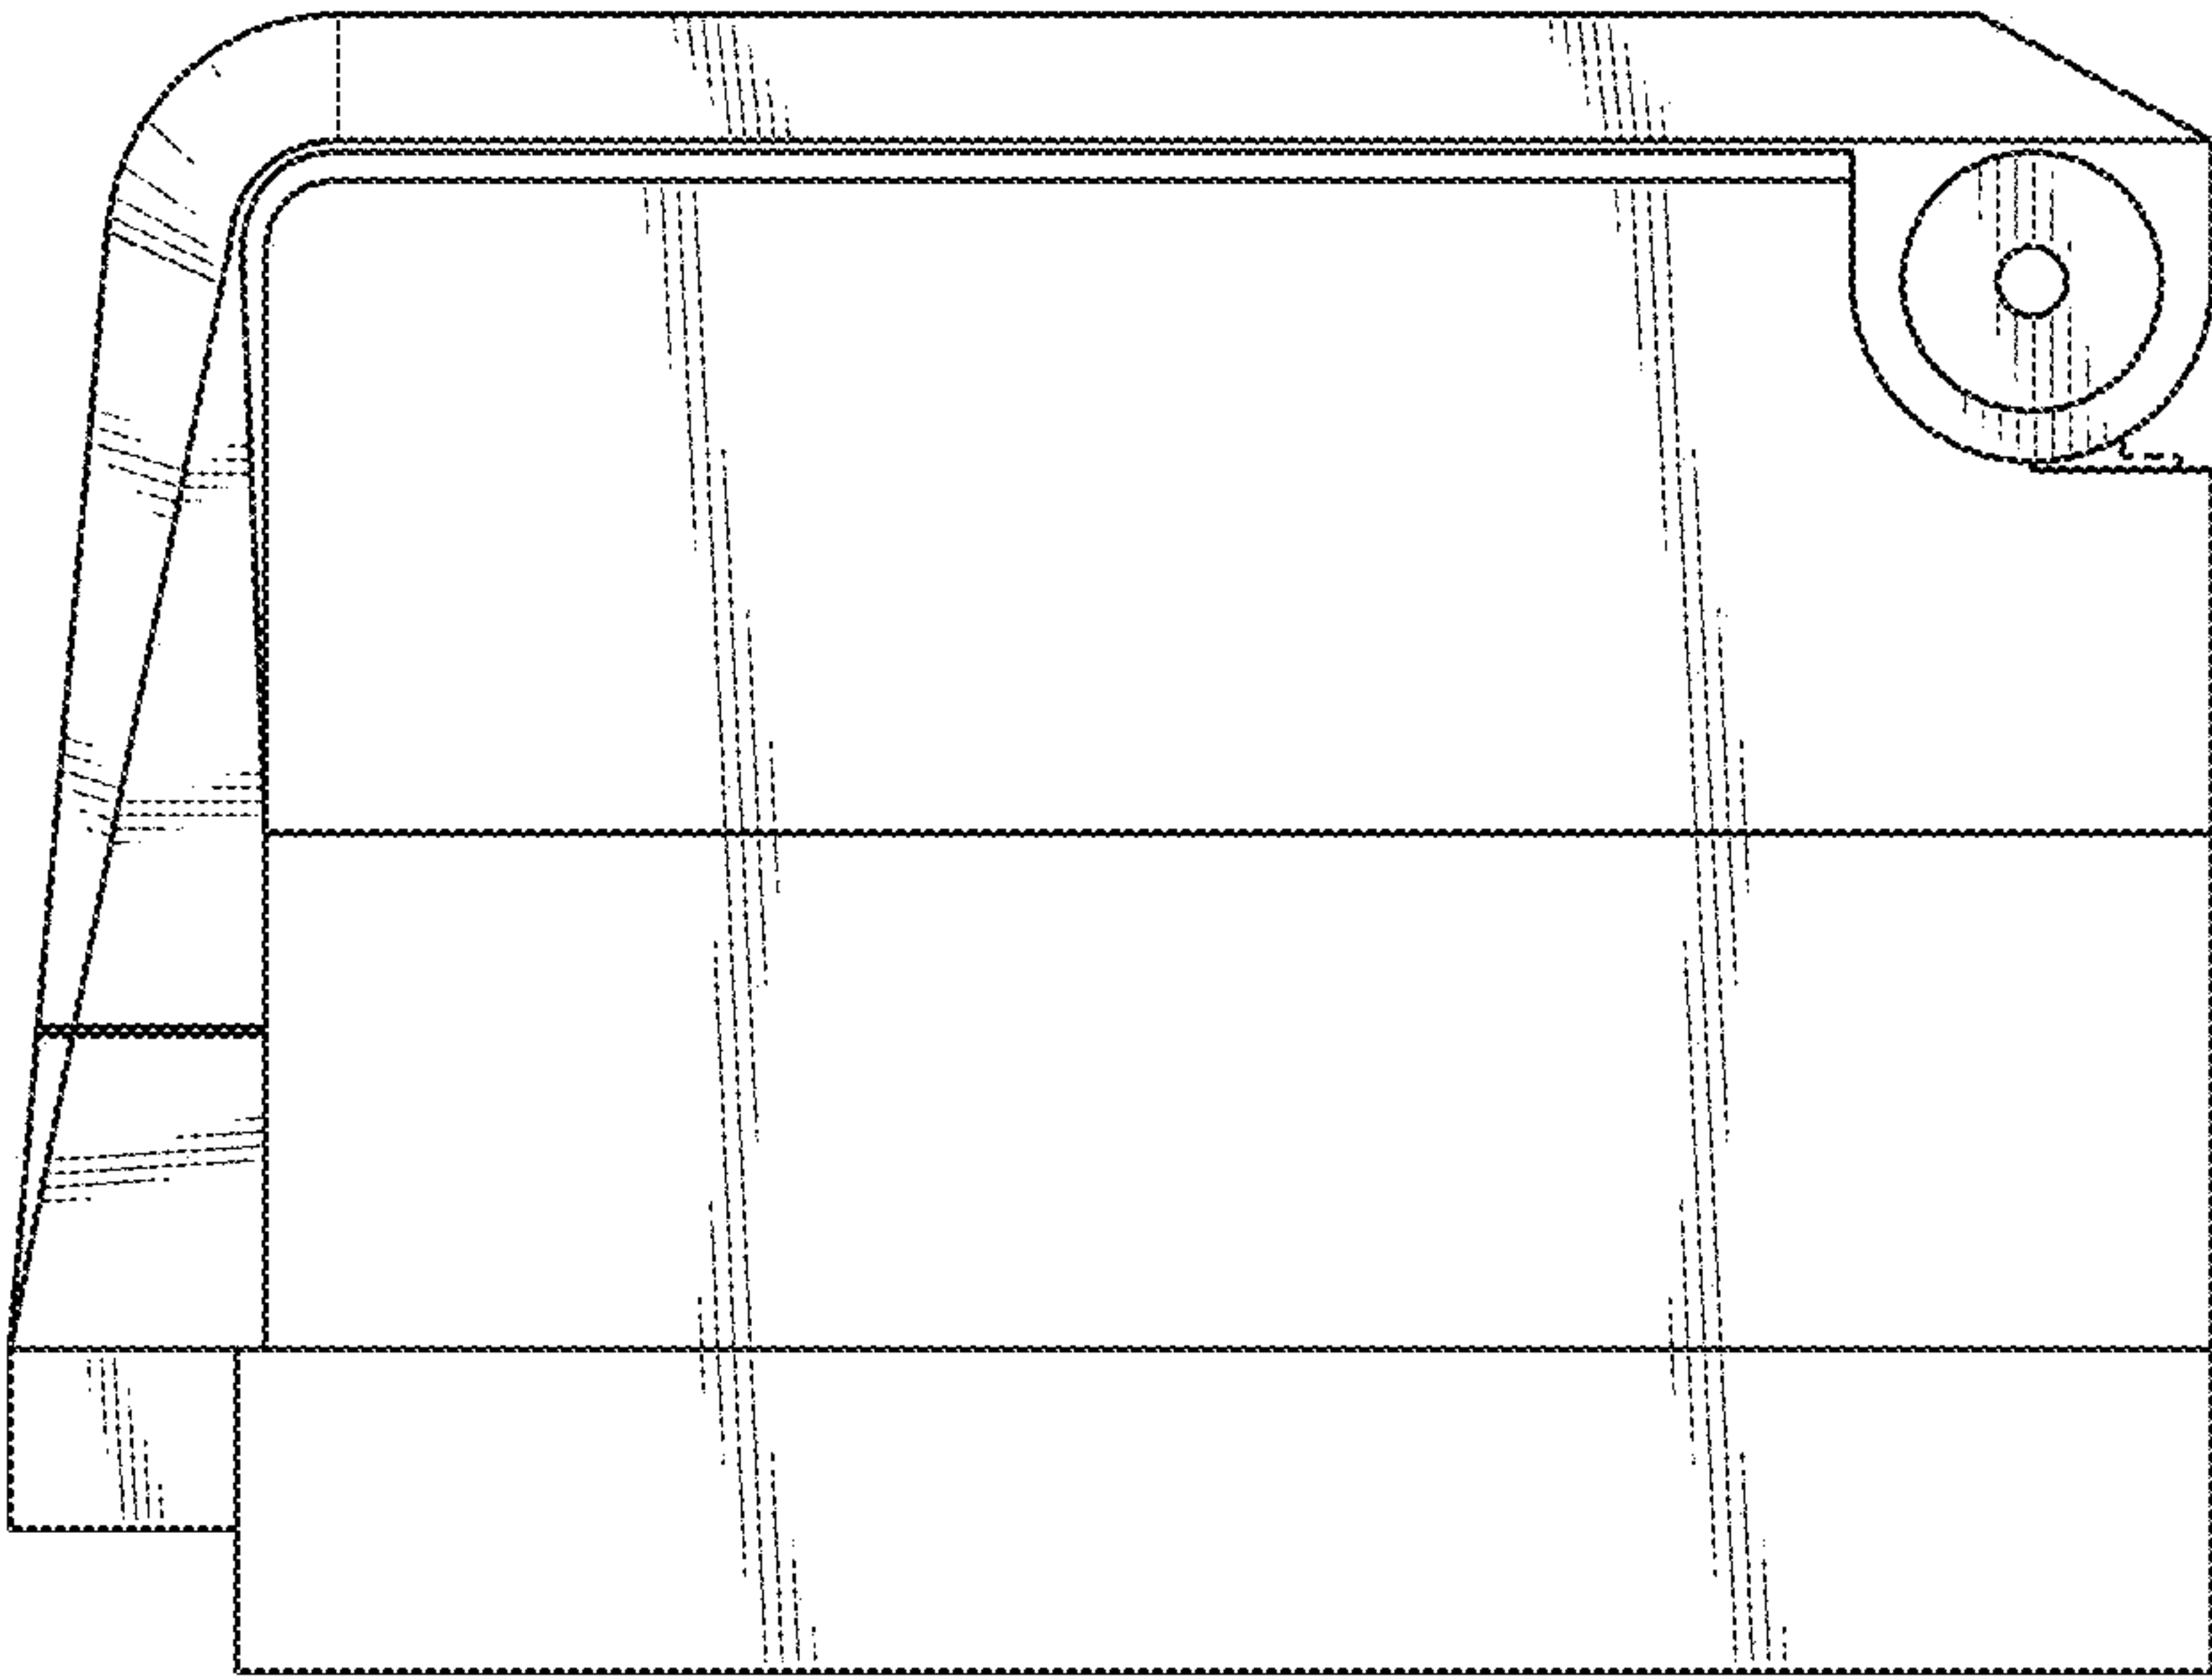


FIG. 19

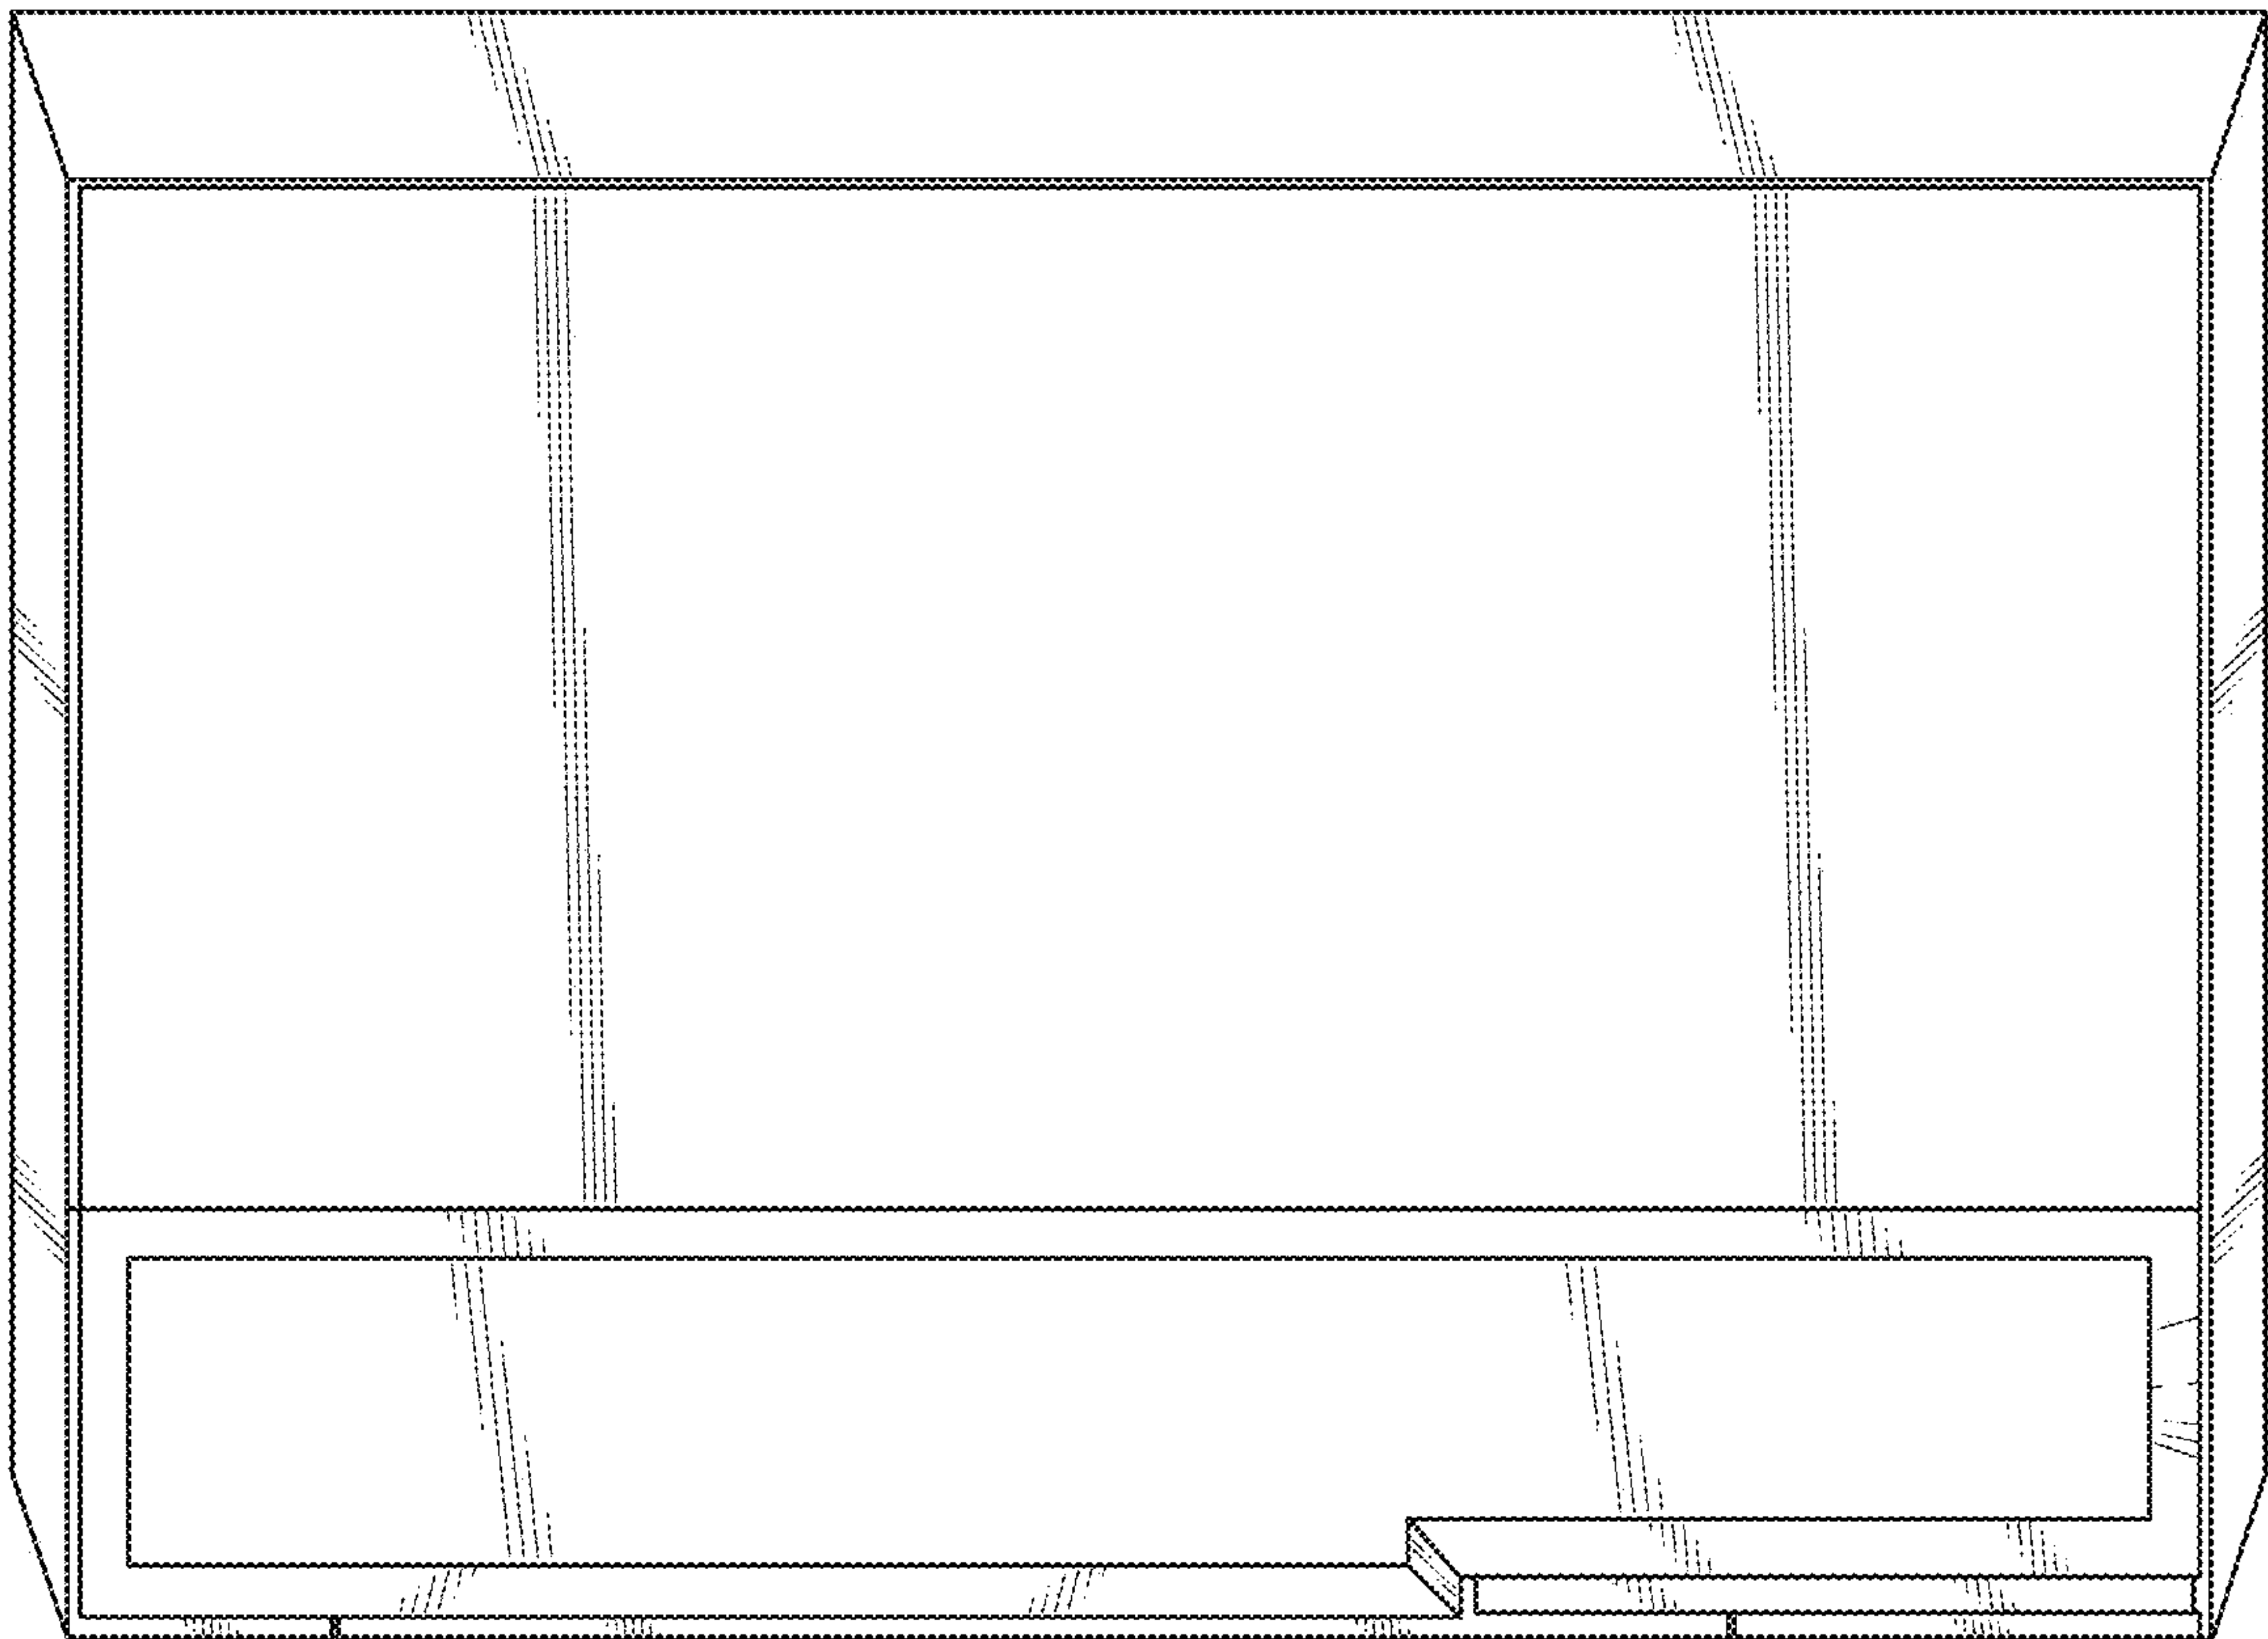


FIG. 20

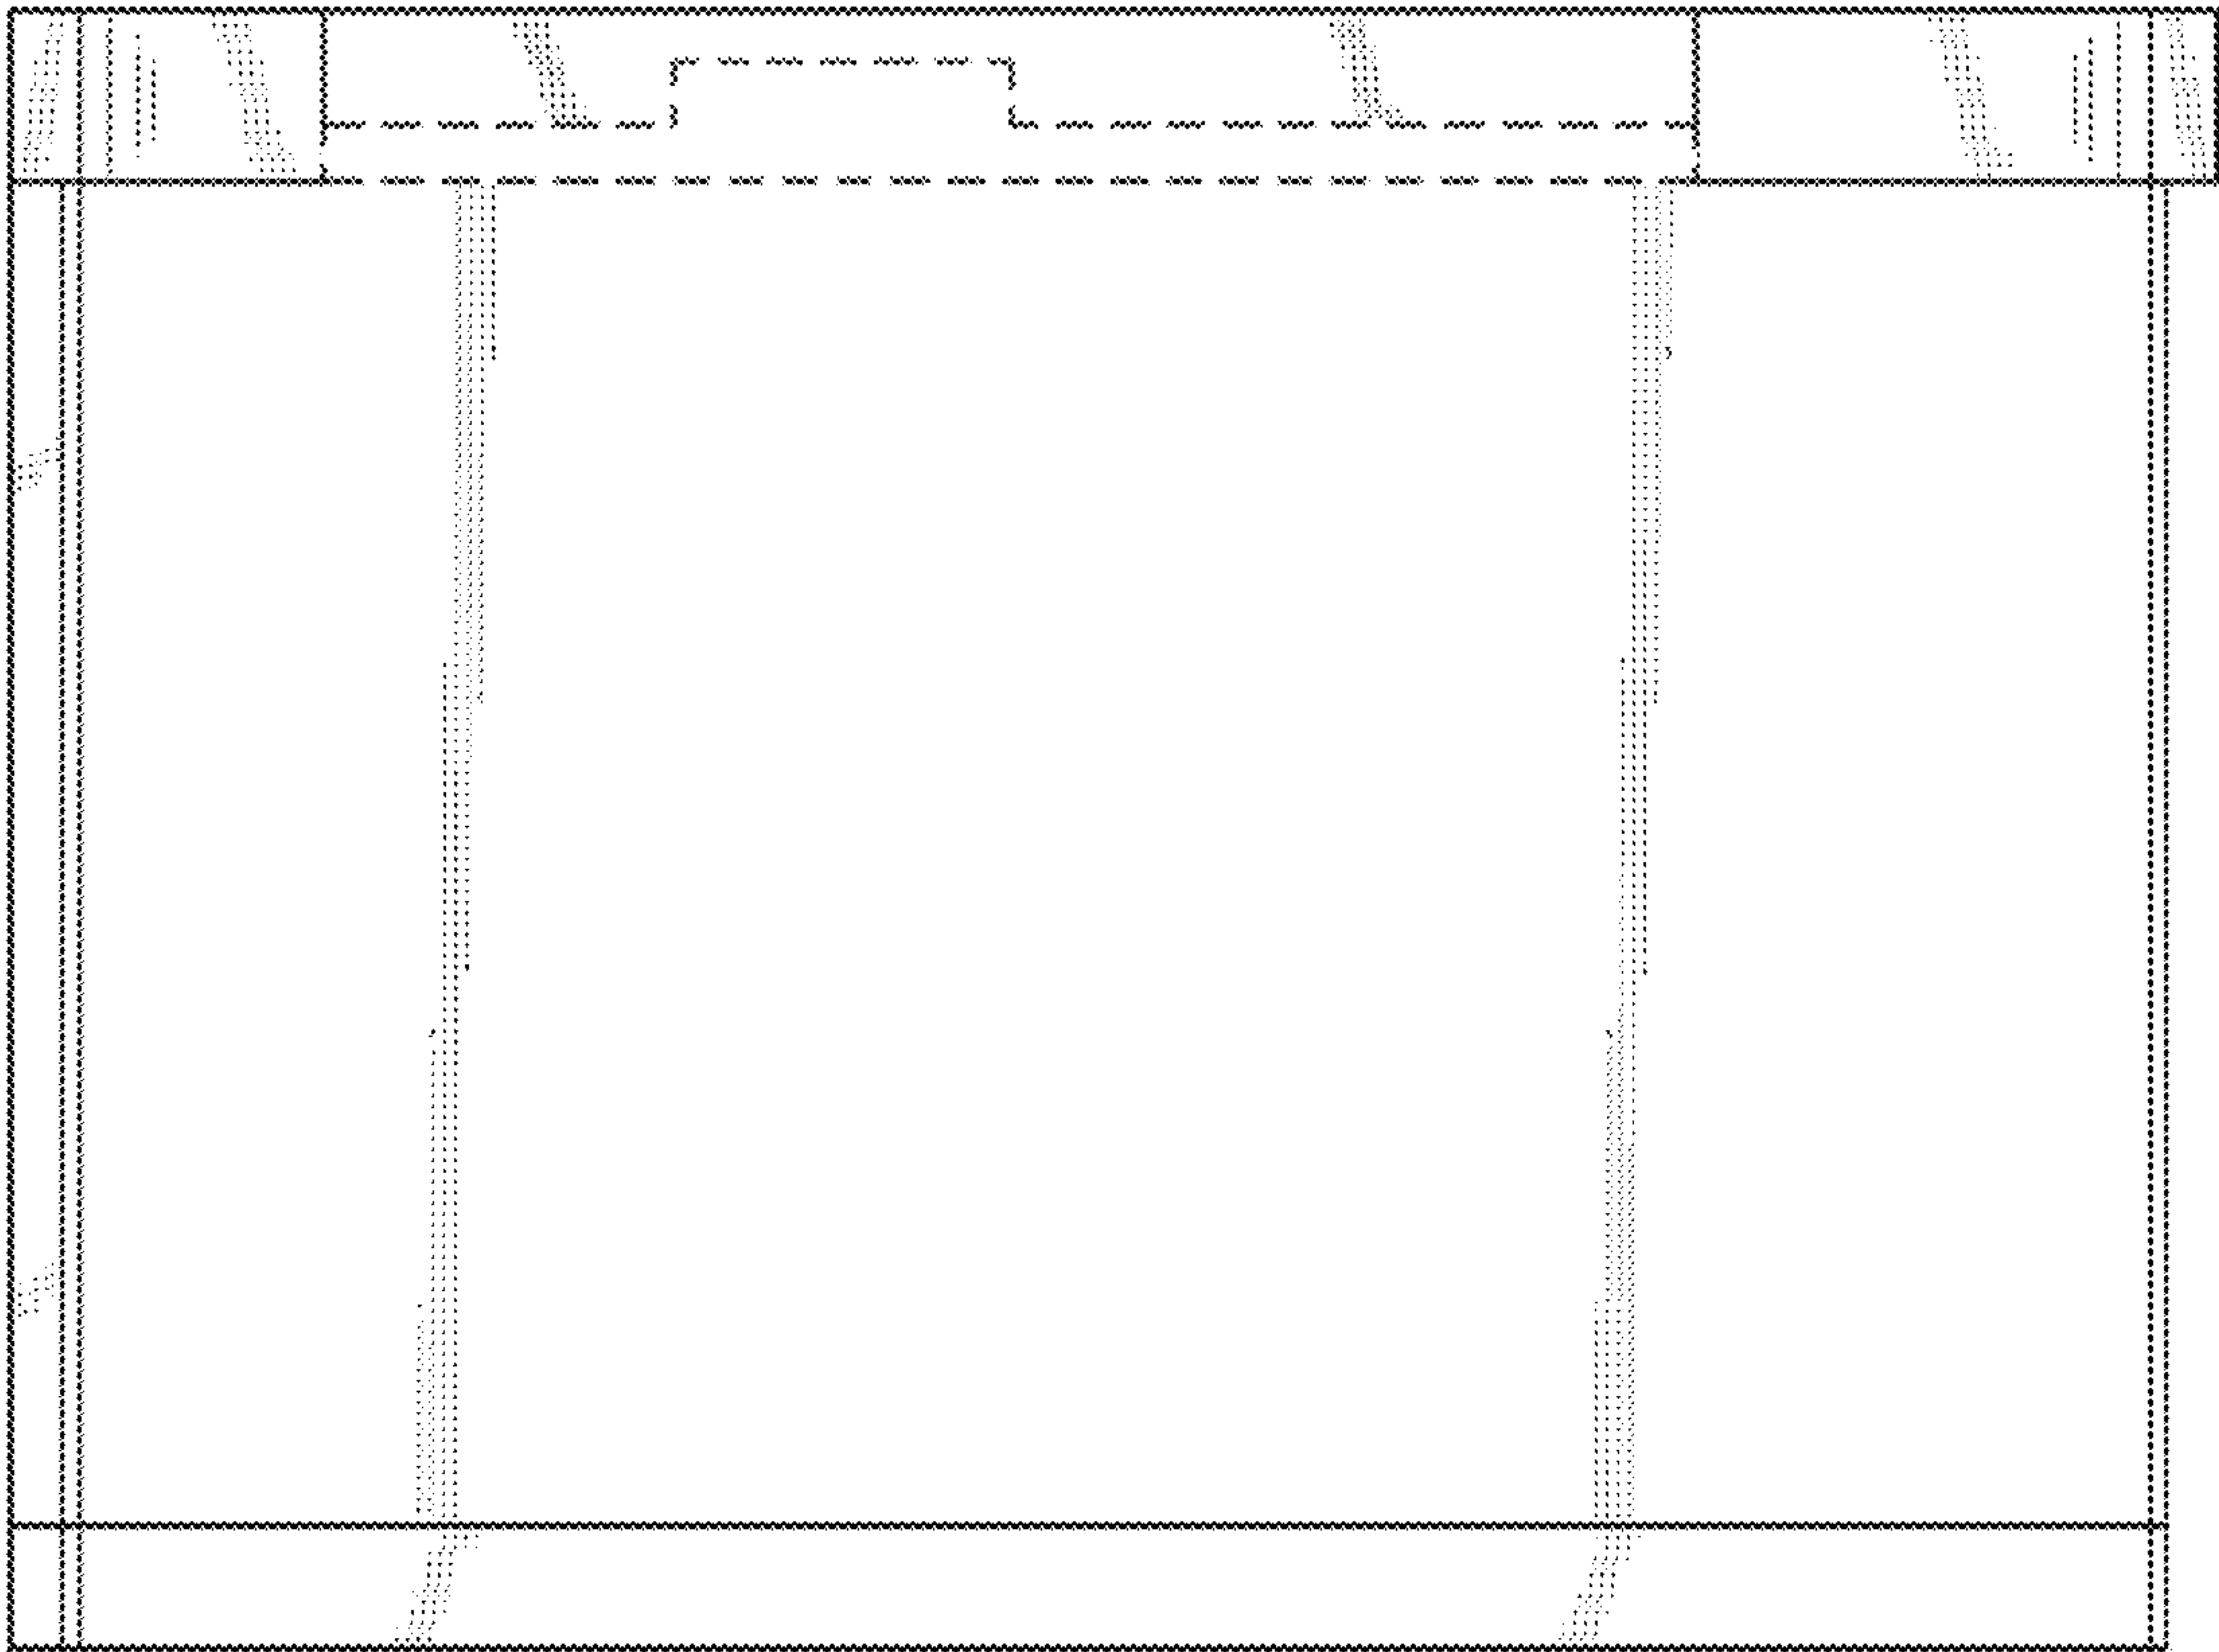


FIG. 21