



US0D1077690S

(12)

United States Design Patent

Liu et al.

(10)

Patent No.:

US D1,077,690 S

(45)

Date of Patent:

** Jun. 3, 2025

(54) ROLLING WALKER

(56) References Cited

(71) Applicant: **Zhejiang Medisite Medical Equipment Technology Co., Ltd.**, Hangzhou (CN)

(72) Inventors: **Zhikuo Liu**, Hangzhou (CN); **Liujiang Jiang**, Hangzhou (CN); **Zhixiang Fan**, Hangzhou (CN)

(73) Assignee: **Zhejiang Medisite Medical Equipment Technology Co., Ltd.**, Hangzhou (CN)

(**) Term: **15 Years**

(21) Appl. No.: **29/908,815**

(22) Filed: **Jan. 16, 2024**

U.S. PATENT DOCUMENTS

D721,620	S	1/2015	Huang	
D754,568	S *	4/2016	Wang	D12/130
9,849,057	B1 *	12/2017	Janeczek	A61G 5/0816
D834,458	S *	11/2018	Paterson	D12/130
D834,459	S *	11/2018	Wang	D12/130
10,588,814	B1 *	3/2020	Engel	A61M 21/00
D895,490	S	9/2020	Sakurai et al.	
D897,243	S *	9/2020	Tsai	D12/130

(Continued)

FOREIGN PATENT DOCUMENTS

CN	201430213160	*	3/2015
CN	201830690549.7	*	4/2019

(Continued)

OTHER PUBLICATIONS

Amazon—Best Sellers, posting date N/A [online], [retrieved Nov. 19, 2024]. Retrieved from internet, <https://www.amazon.com/Best-Sellers-Rolling-Walkers/zgbs/hpc/3776991> (Year: 2024).*

(Continued)

Primary Examiner — Garth Rademaker
Assistant Examiner — Aaron C Fowler
(74) *Attorney, Agent, or Firm* — Jose Cherson Weissbrot

(57) **CLAIM**
The ornamental design for a rolling walker, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of a rolling walker;
FIG. 2 is a front view thereof;
FIG. 3 is a rear view thereof;
FIG. 4 is a right side view thereof;
FIG. 5 is a left side view thereof;
FIG. 6 is a top view thereof; and,
FIG. 7 is a bottom view thereof.

1 Claim, 7 Drawing Sheets

Related U.S. Application Data

(63) Continuation-in-part of application No. 29/909,927, filed on Aug. 12, 2023, which is a continuation-in-part of application No. 29/879,806, filed on Jul. 12, 2023.

Foreign Application Priority Data


Dec. 28, 2023 (CN) 202330860717.3

(51) **LOC (15) Cl.** 12-12

(52) **U.S. Cl.**
USPC D12/130

(58) **Field of Classification Search**
USPC D3/7, 8; D12/128, 129, 130, 131, 133
CPC ... A61G 5/02; A61G 5/04; A61G 5/08; A61G 2200/36; A61G 2200/60; A47D 3/001; A47D 13/04; A47D 13/043

See application file for complete search history.

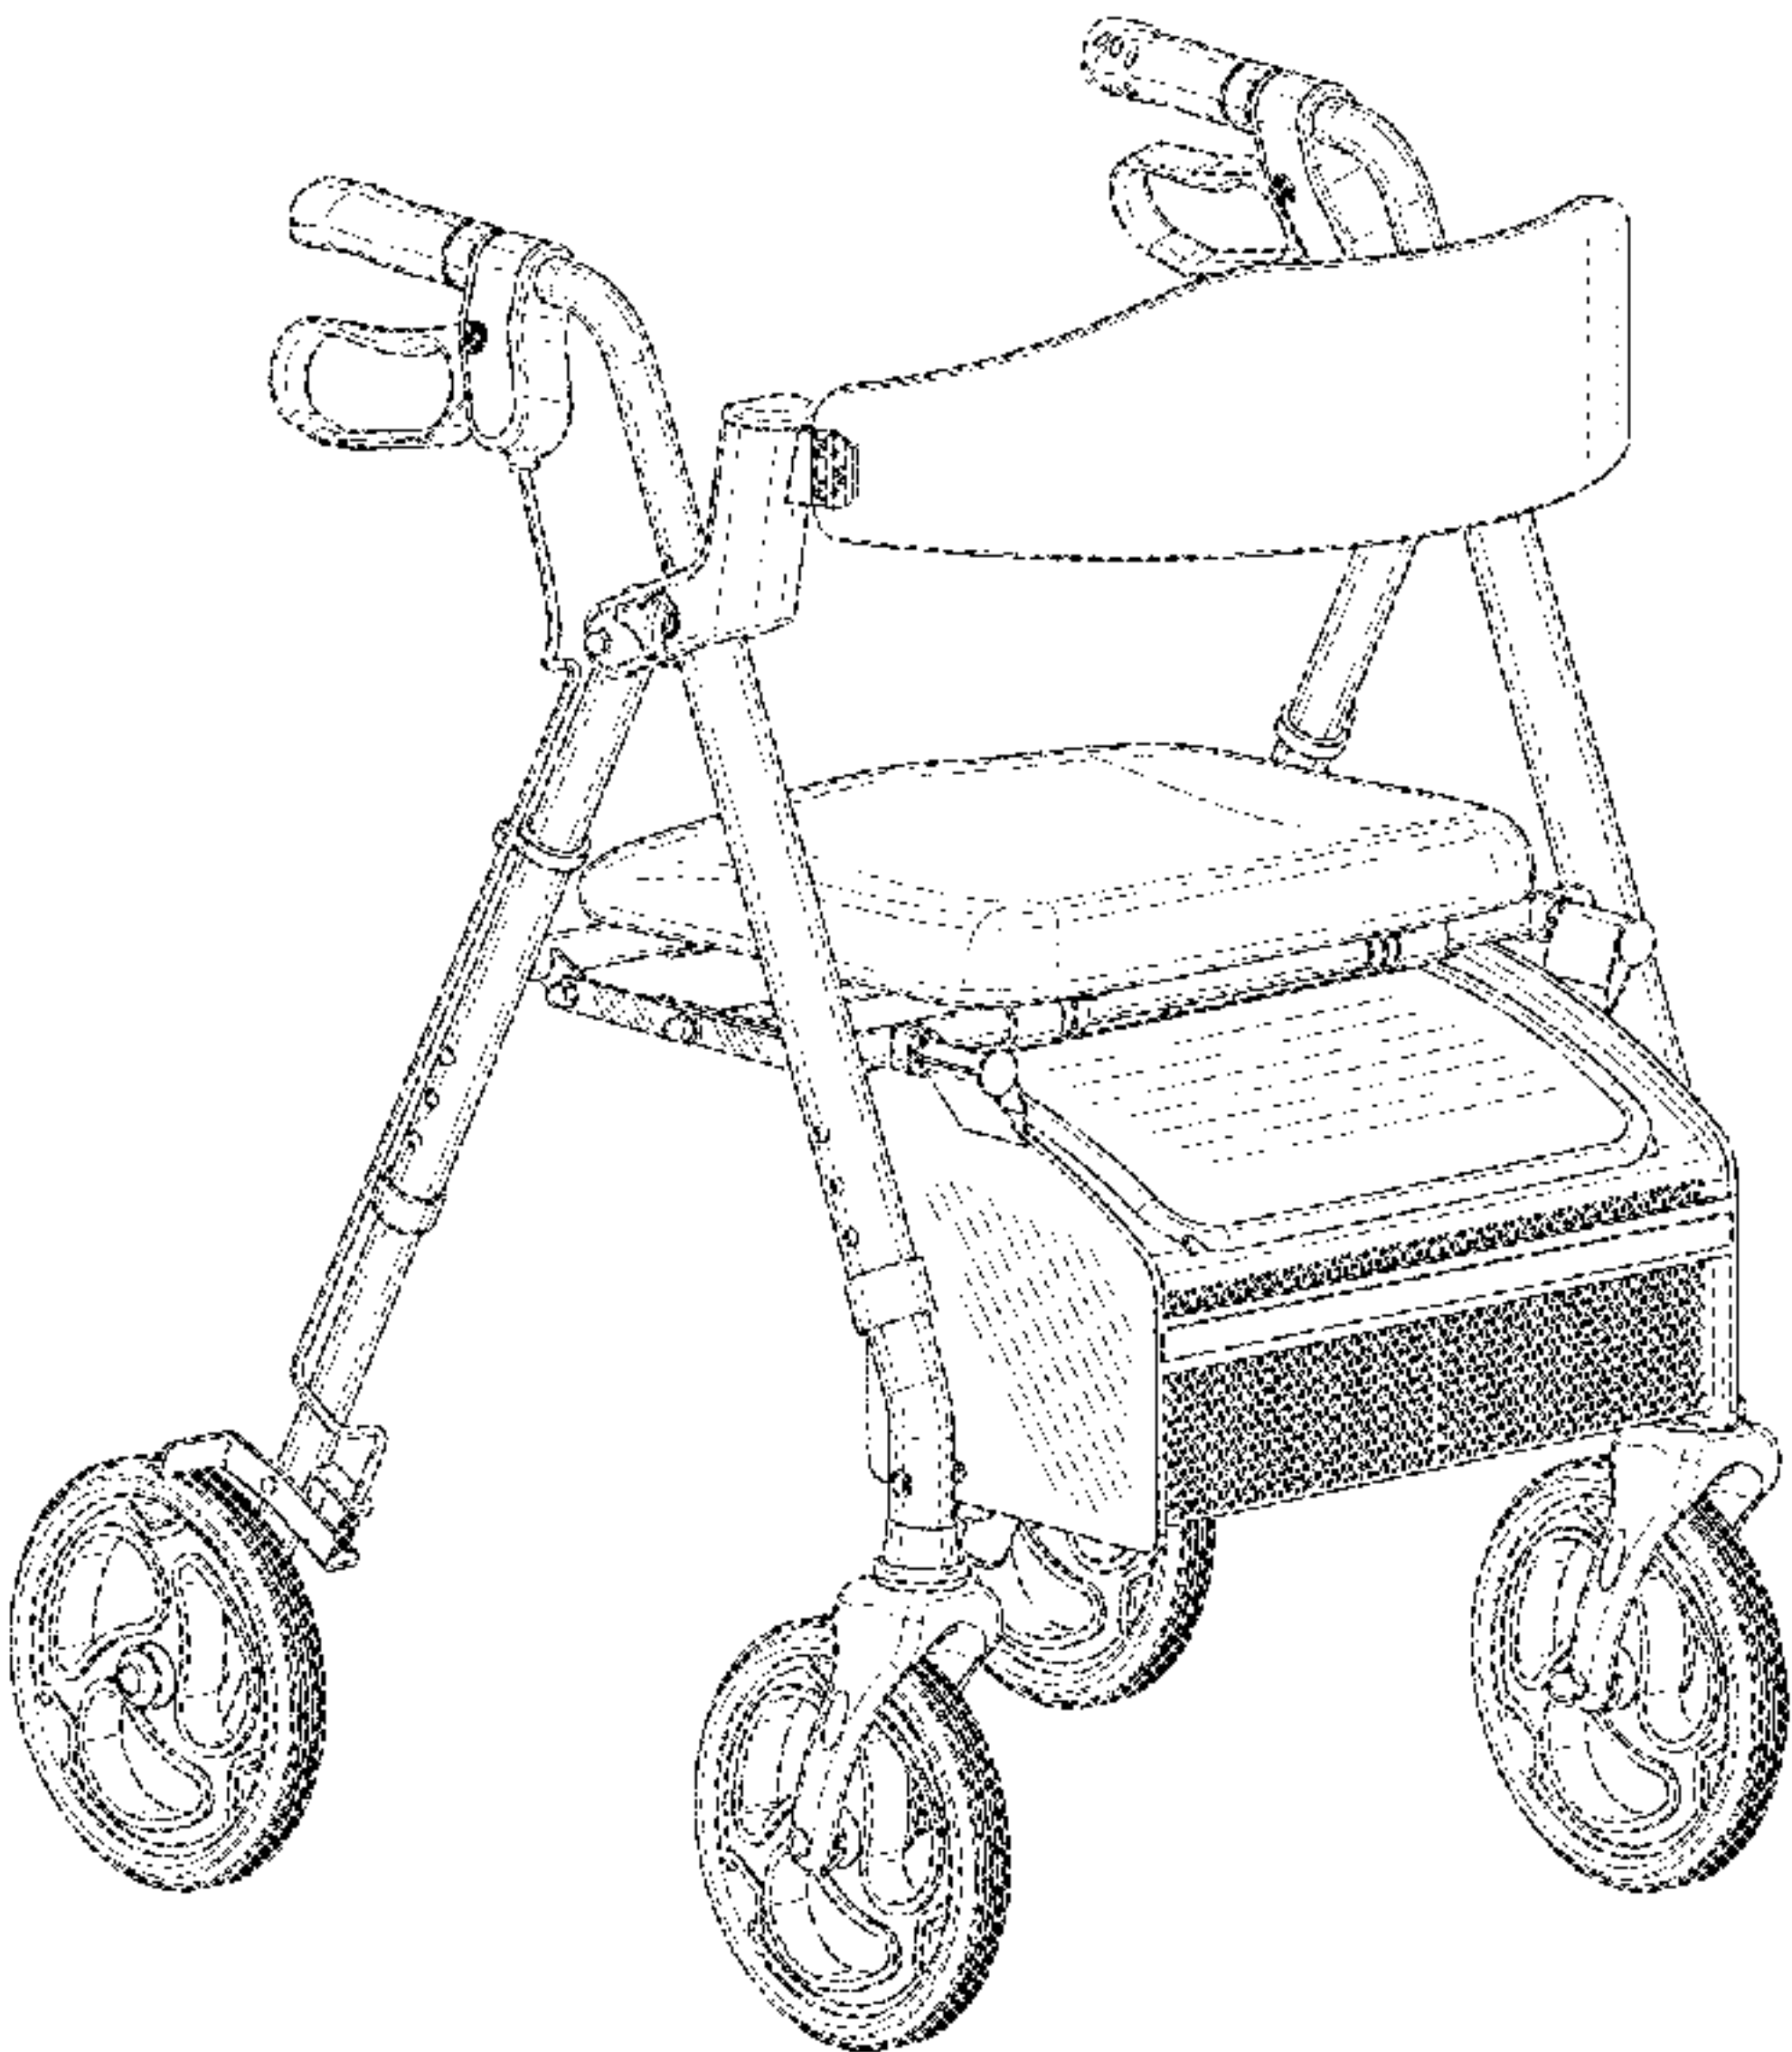

References Cited

D902,791	S	11/2020	Fellingham et al.	
D908,550	S *	1/2021	Berman	D12/130
D928,669	S *	8/2021	Bodman	D6/406.3
D929,910	S	9/2021	Sainz	
11,471,363	B1 *	10/2022	Semesnyei	A61H 3/04
D997,792	S *	9/2023	Berman	D12/130
D1,002,445	S *	10/2023	Wang	D12/130
D1,038,845	S	8/2024	Wang	
2013/0061893	A1 *	3/2013	Nilsson	A61G 5/1091 280/647
2014/0265188	A1 *	9/2014	Chang	A61G 5/101 280/47.4
2023/0028131	A1 *	1/2023	Hooworth	A61G 5/0841

CN	201930520838.7	*	2/2020
EM	015046808	*	1/2024
SE	2000/1476	*	1/2002

Amazon—Vocic, posted Nov. 23, 2023 [online], [retrieved Nov. 19, 2024]. Retrieved from internet, <https://www.amazon.com/VOCIC-Foldable-Rollator-Ergonomic-Adjustable/dp/B0CNWBPGG> (Year: 2023).*

Amazon—HZMedi, posted May 17, 2024 [online], [retrieved Nov. 19, 2024]. Retrieved from internet, <https://www.amazon.com/dp/B0D4DXGRMQ> (Year: 2024).*

Amazon—Homland, posted Aug. 14, 2024 [online], [retrieved Nov. 19, 2024]. Retrieved from internet, <https://www.amazon.com/HOMLAND-Foldable-Rollator-Adjustable-Lightweight/dp/B0DD3MTH3J> (Year: 2024).*

* cited by examiner



FIG. 1

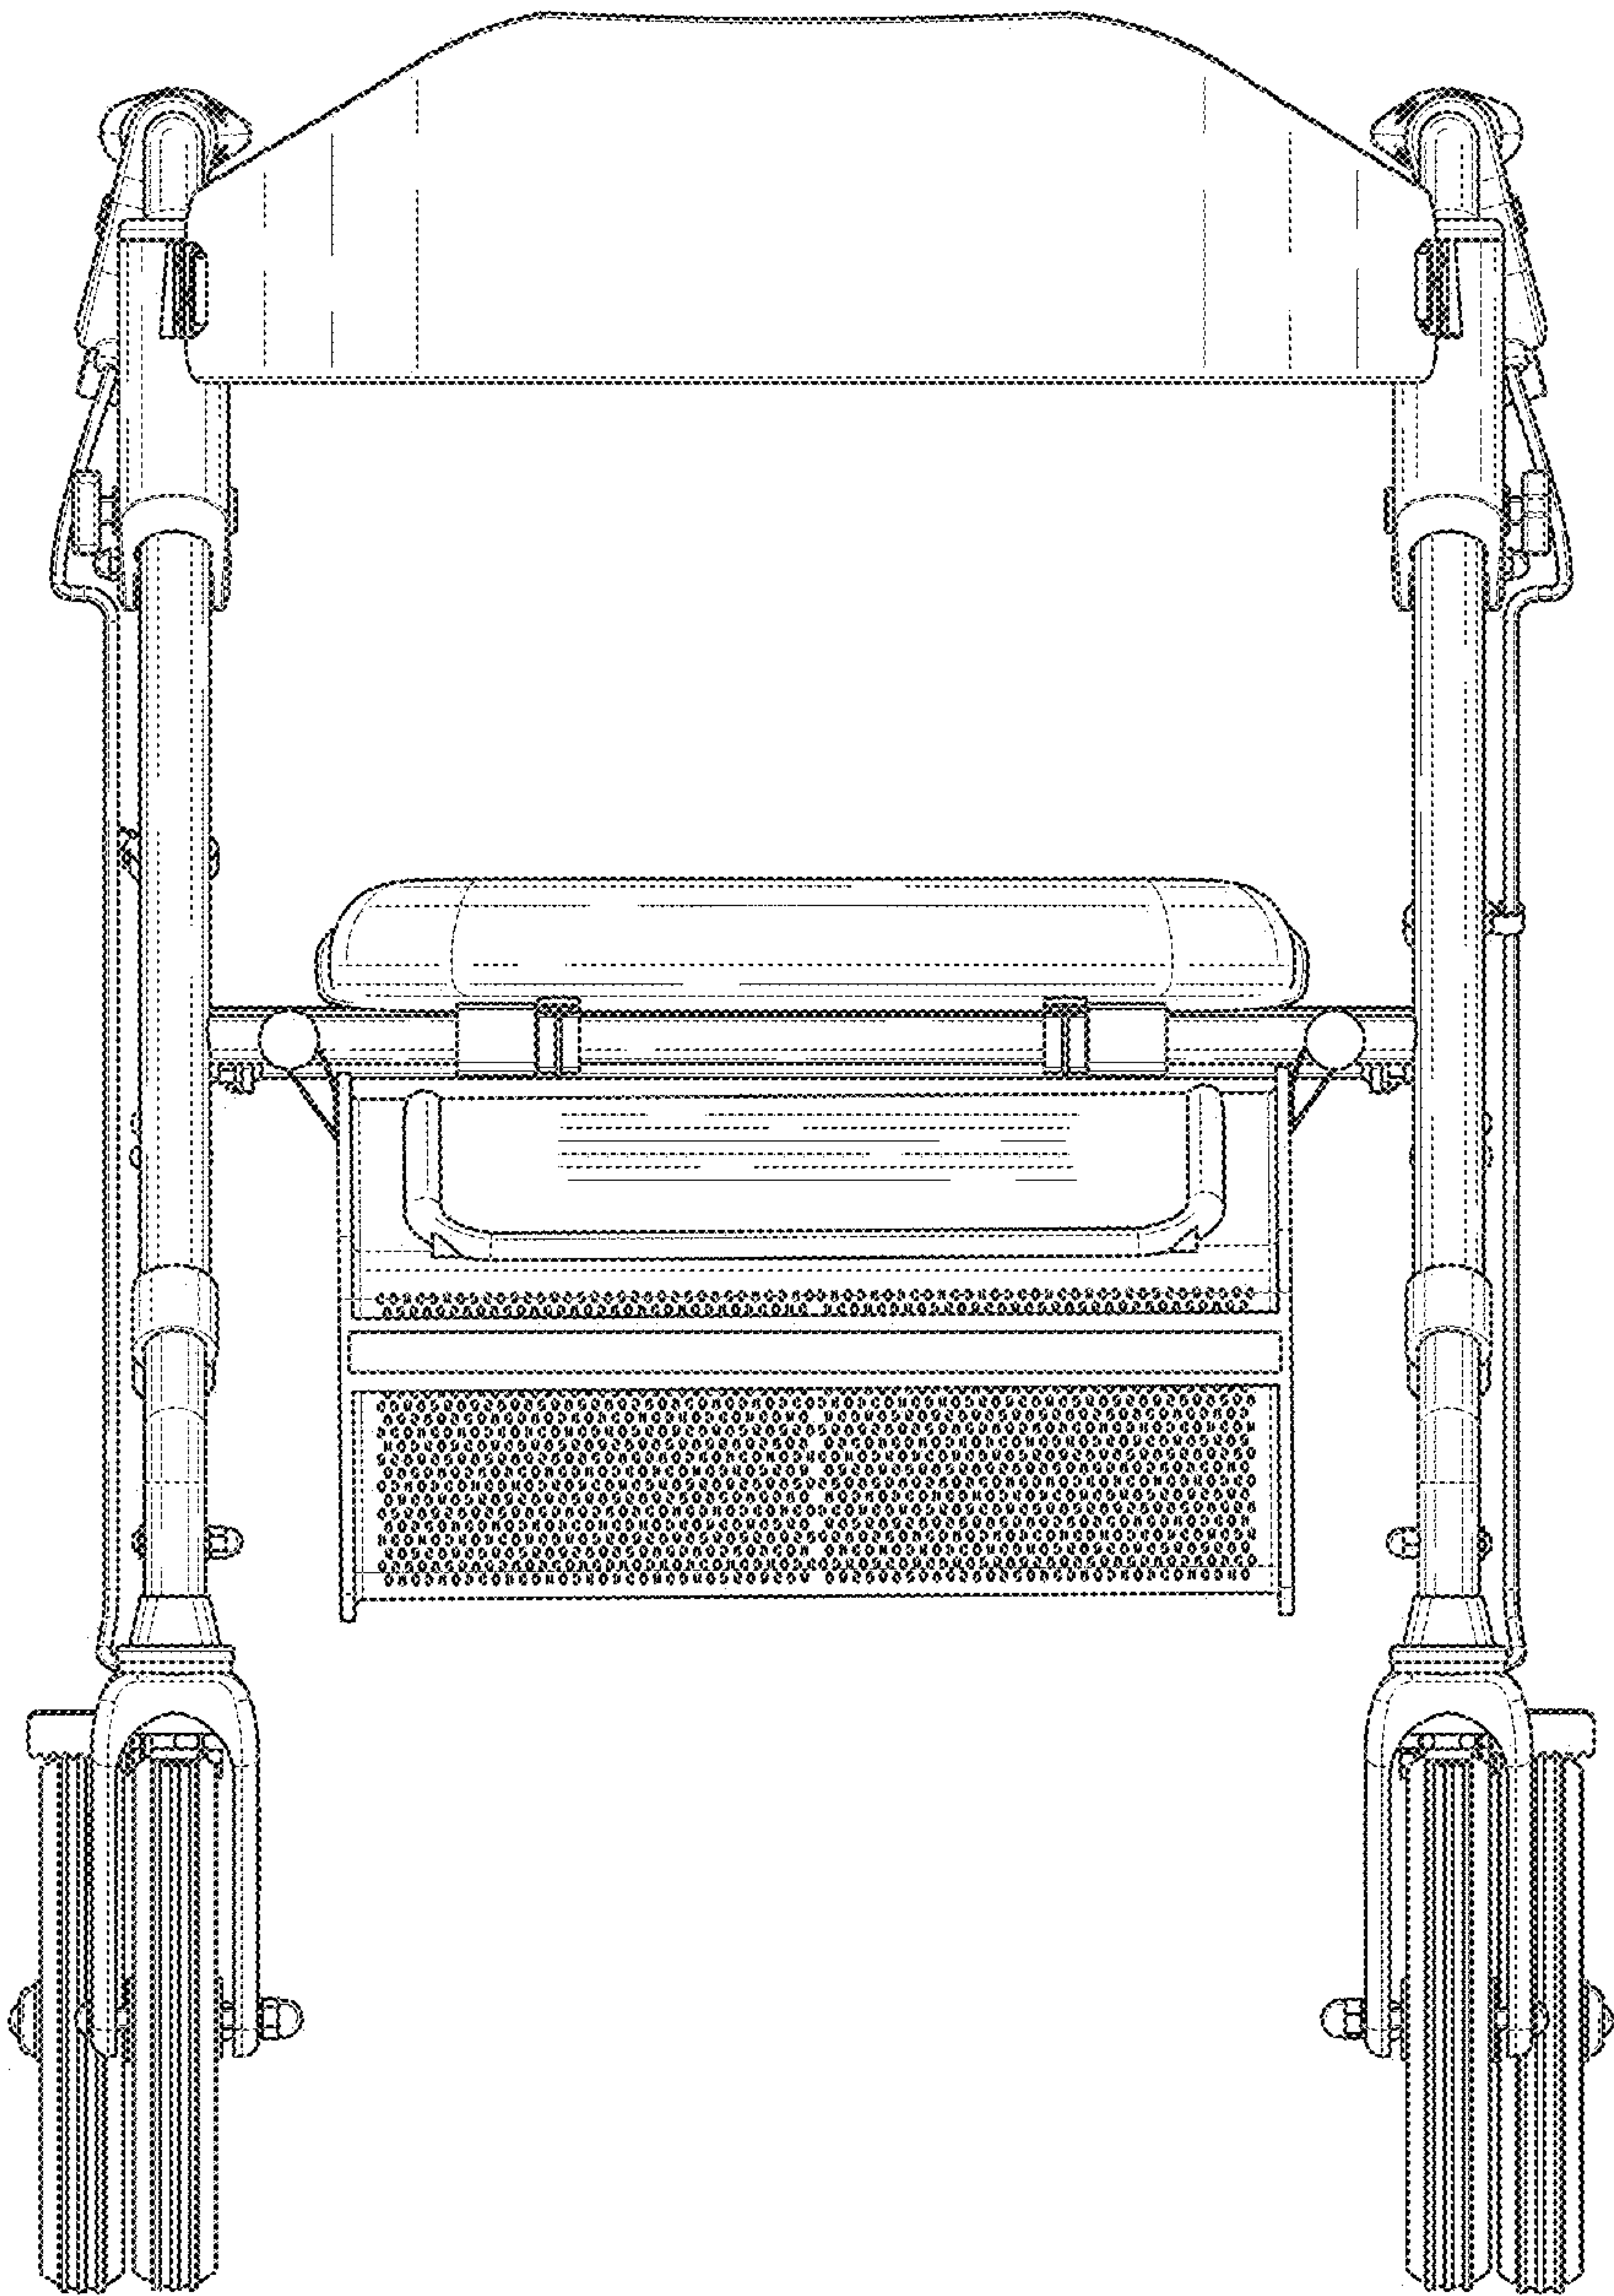


FIG. 2

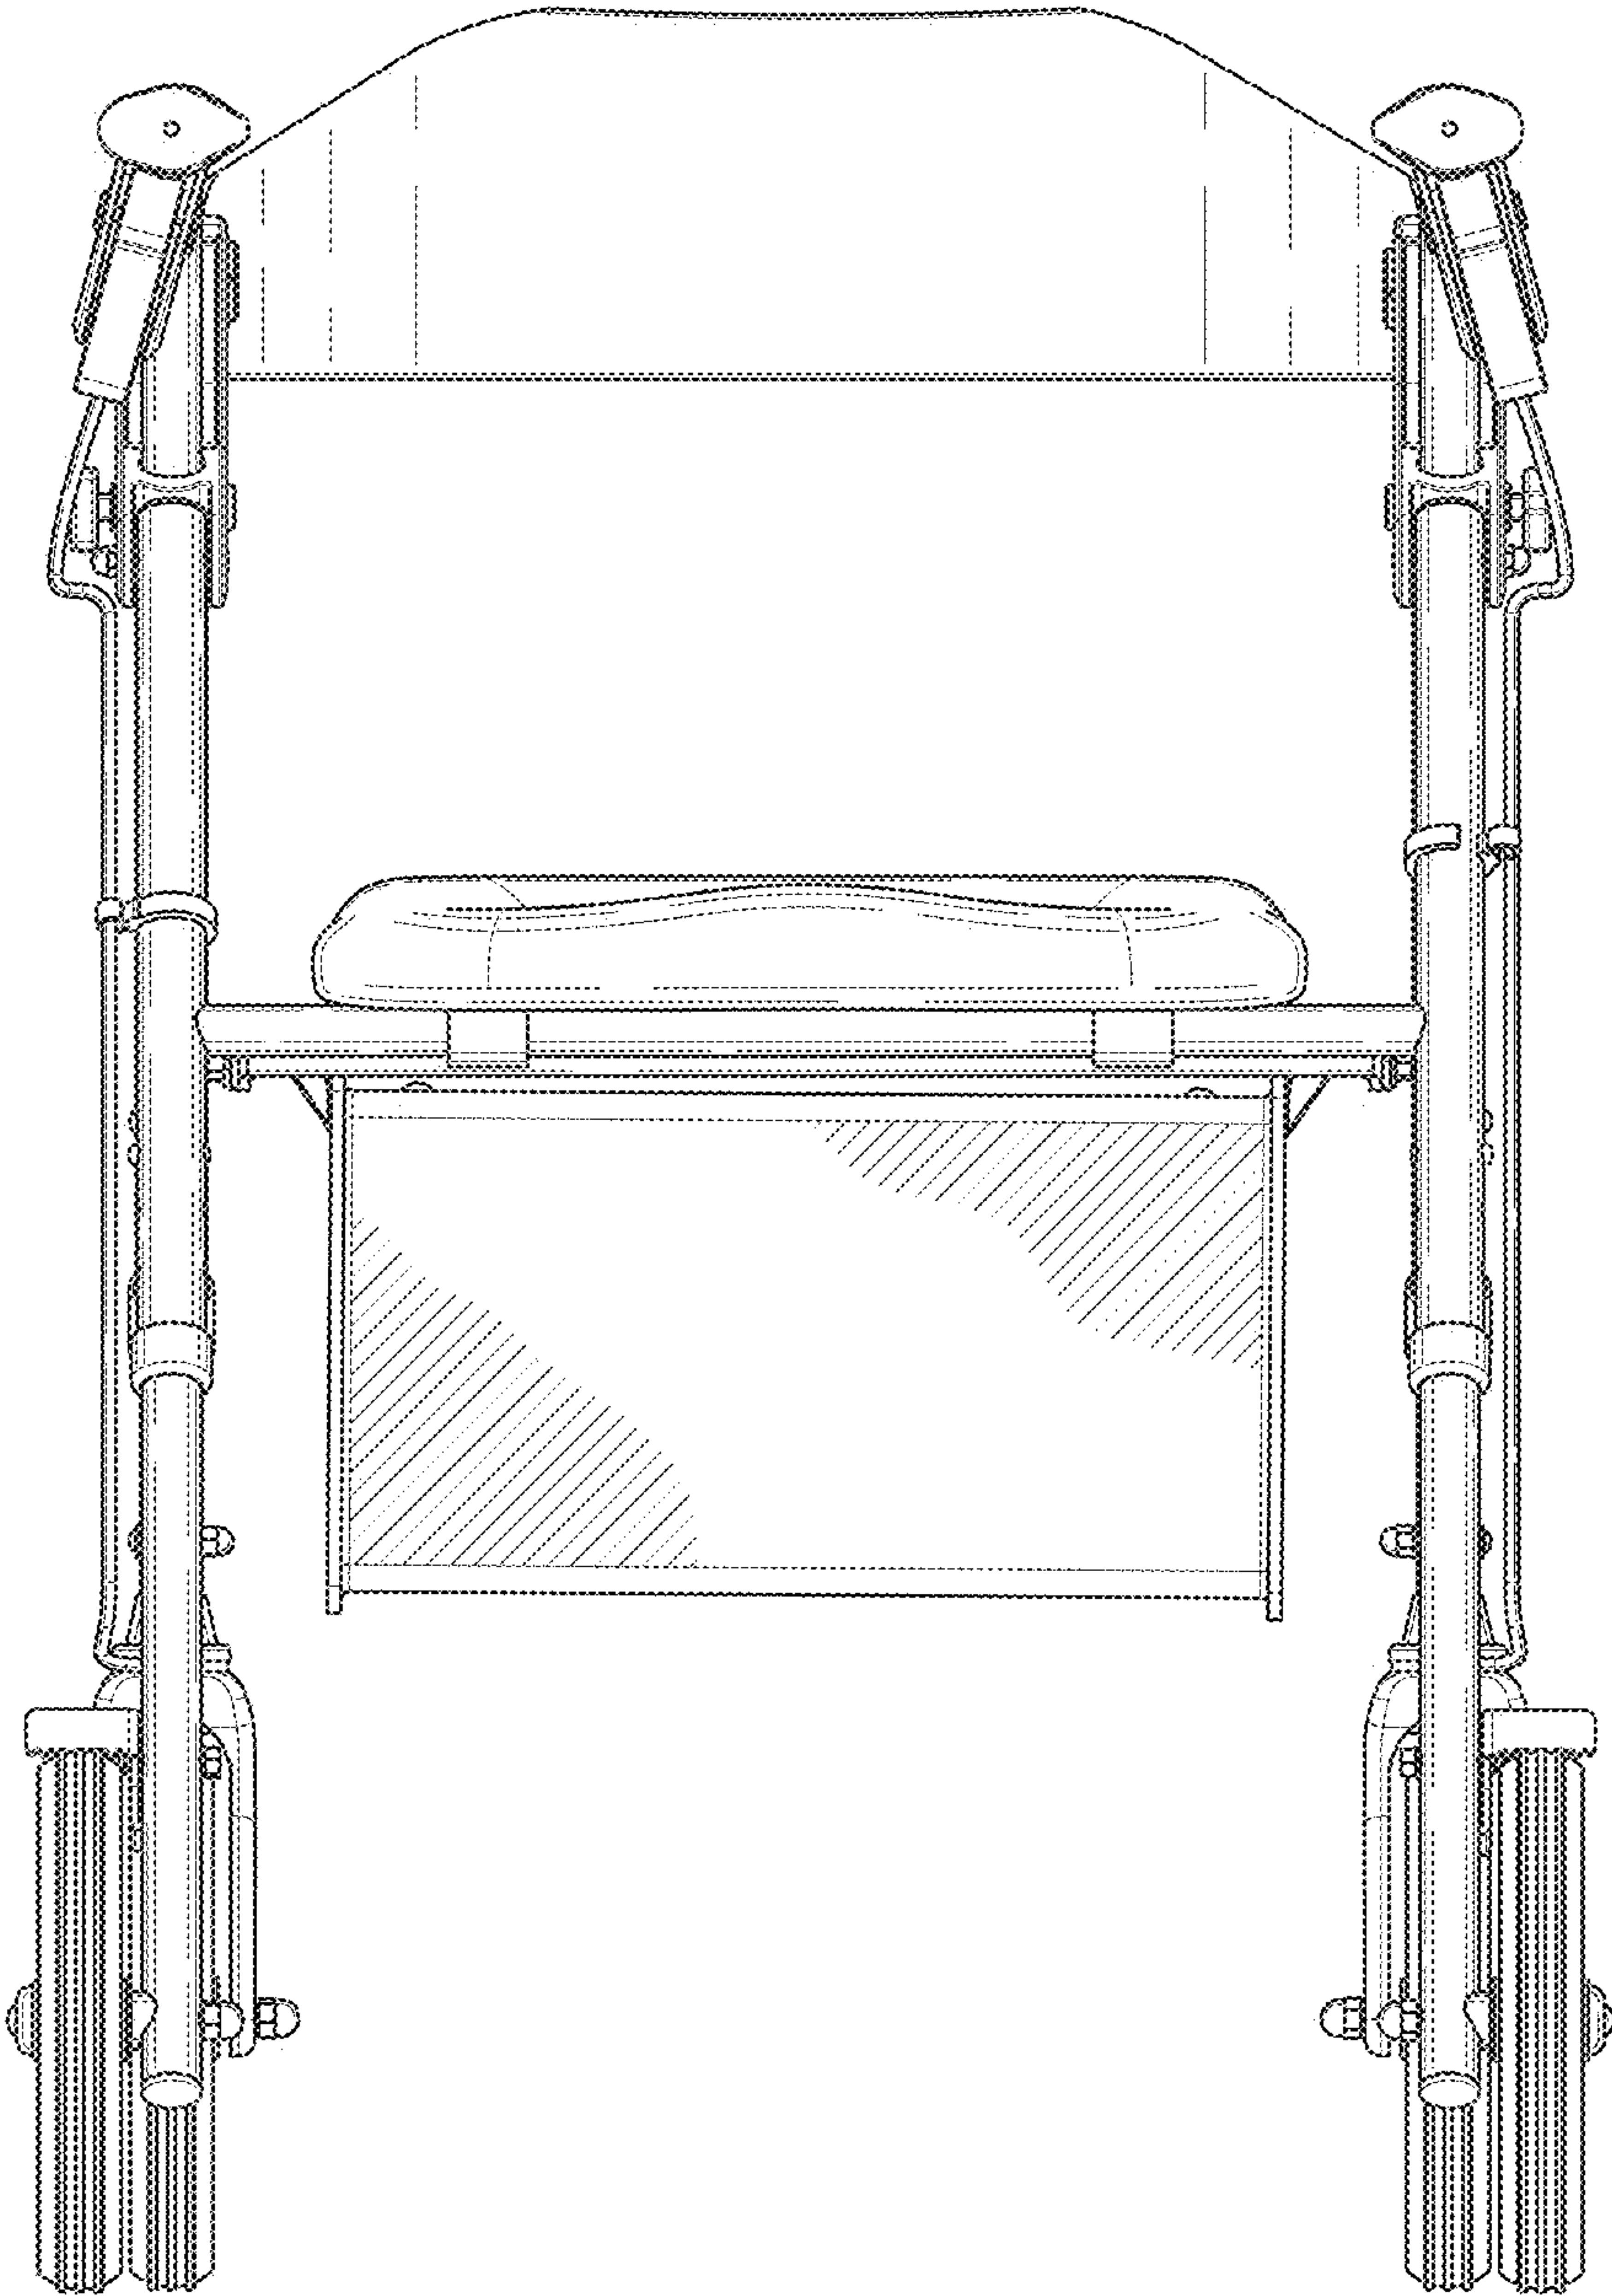


FIG. 3

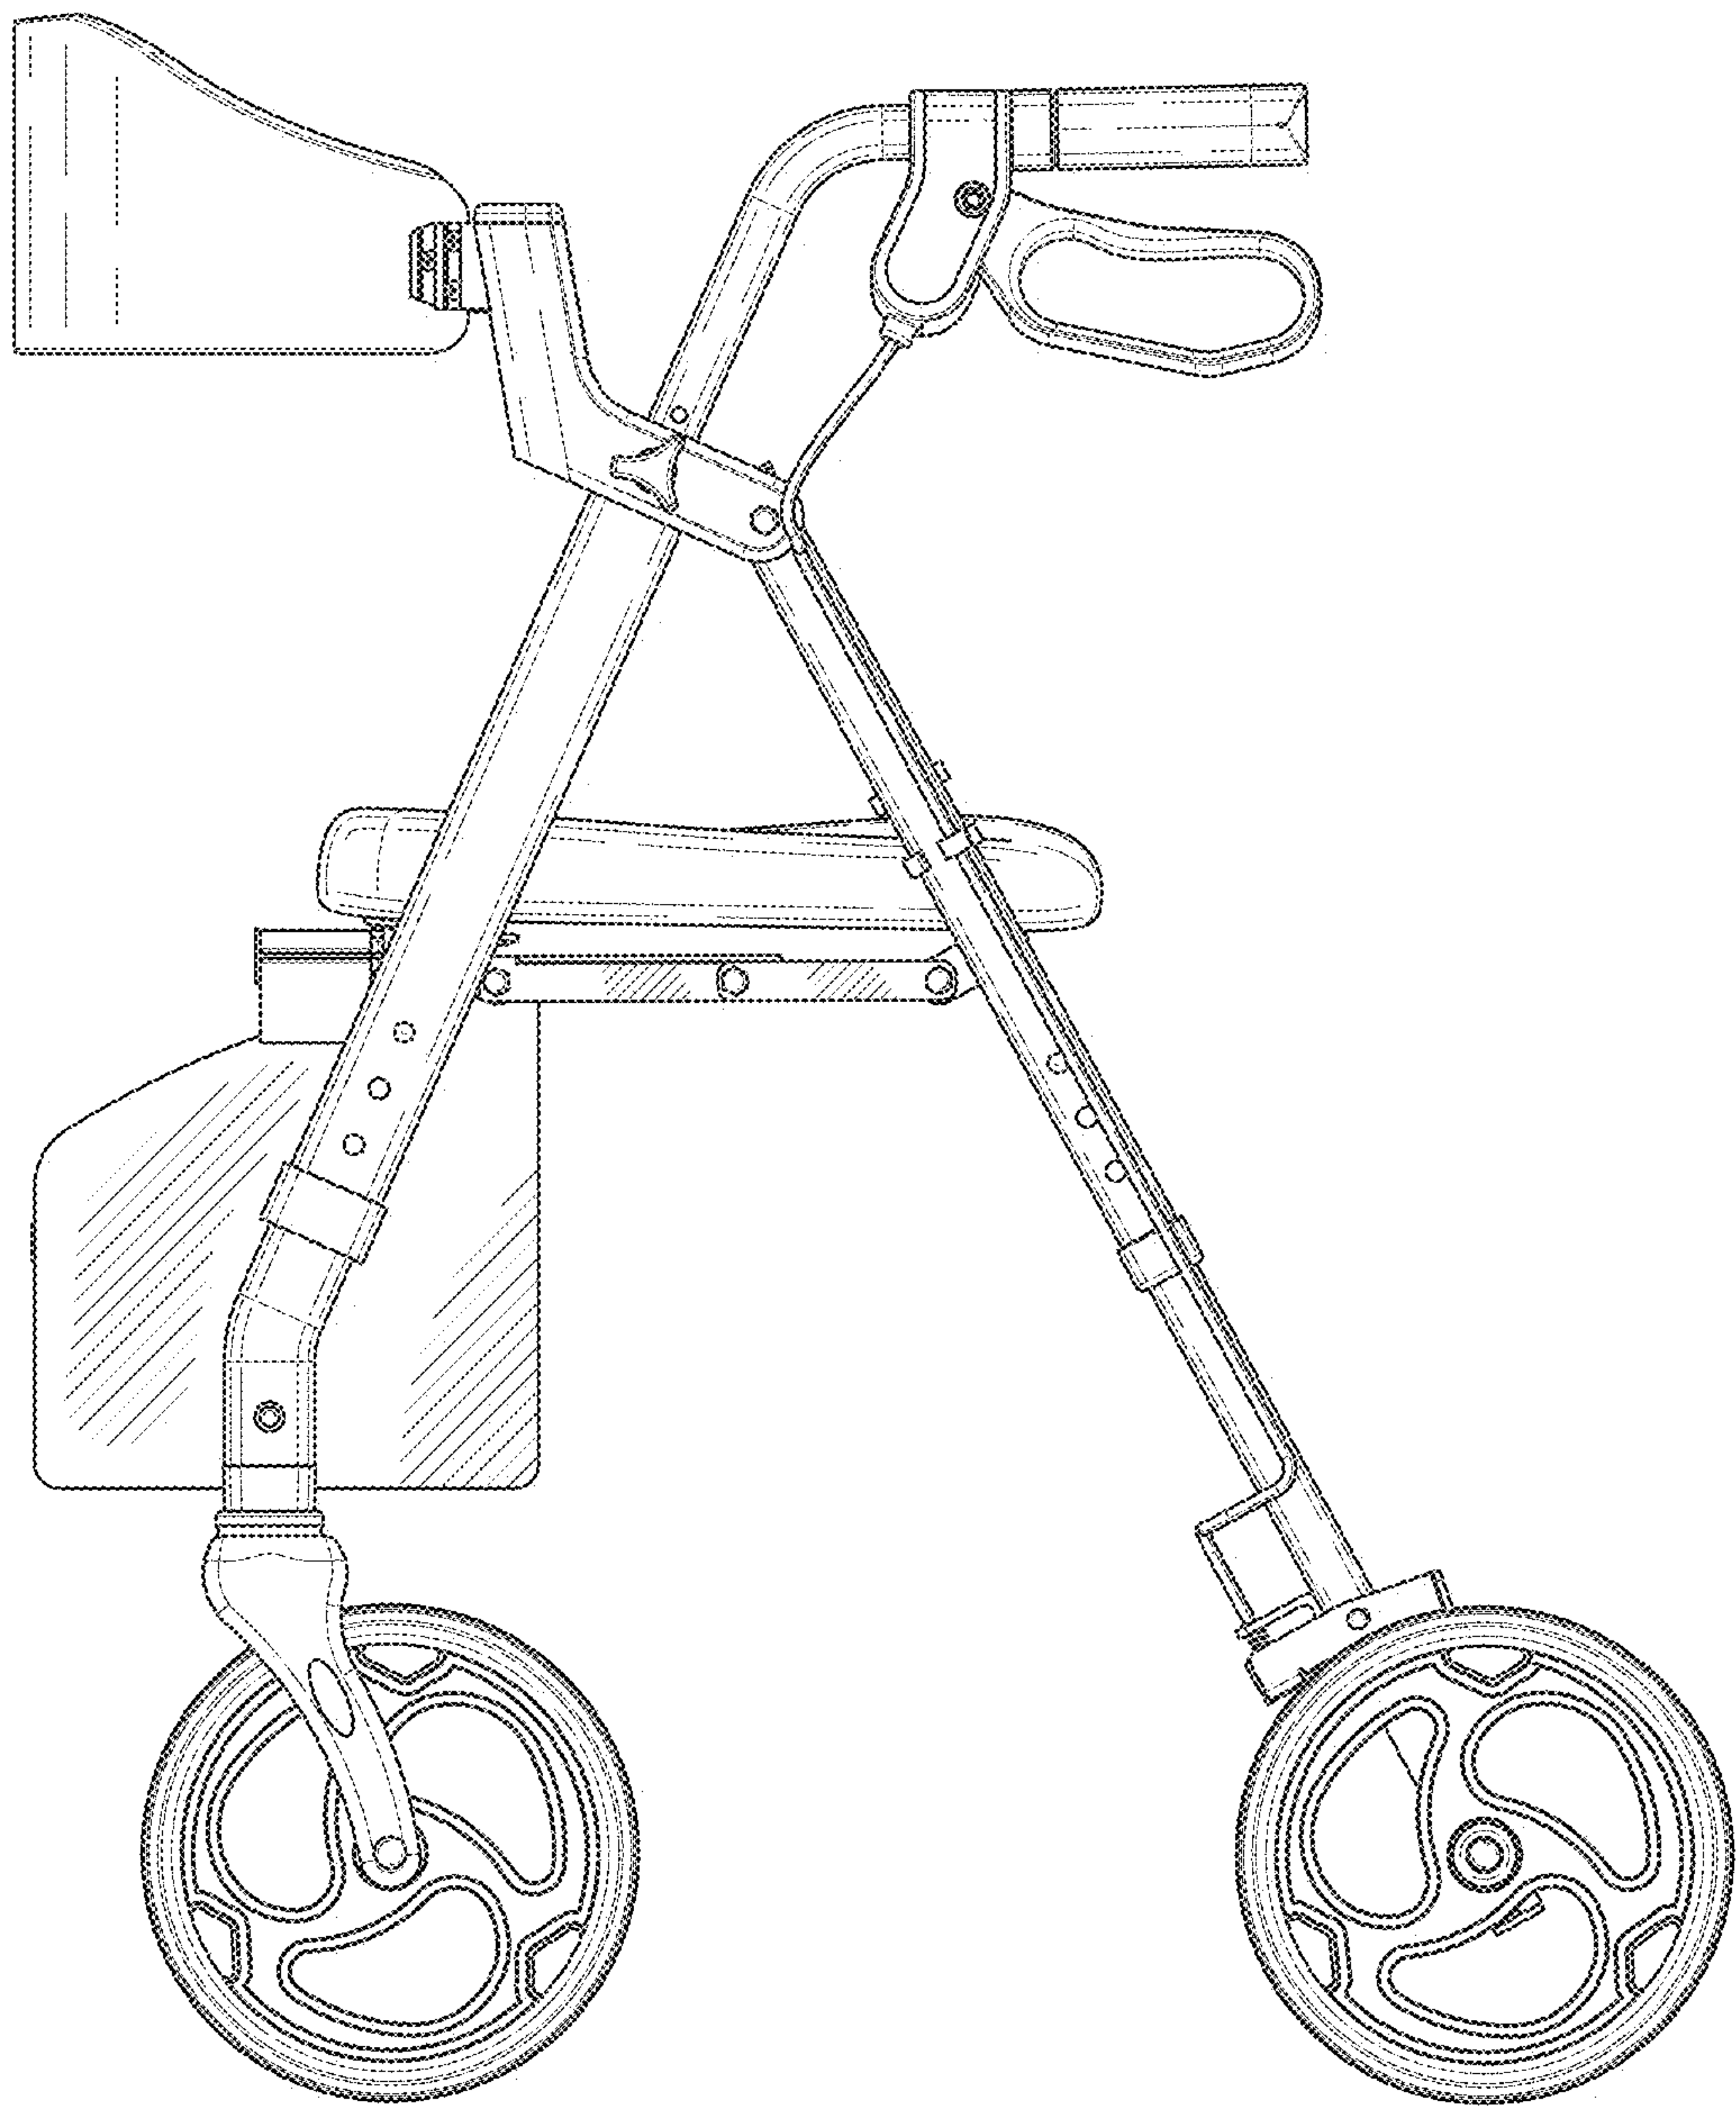


FIG. 4

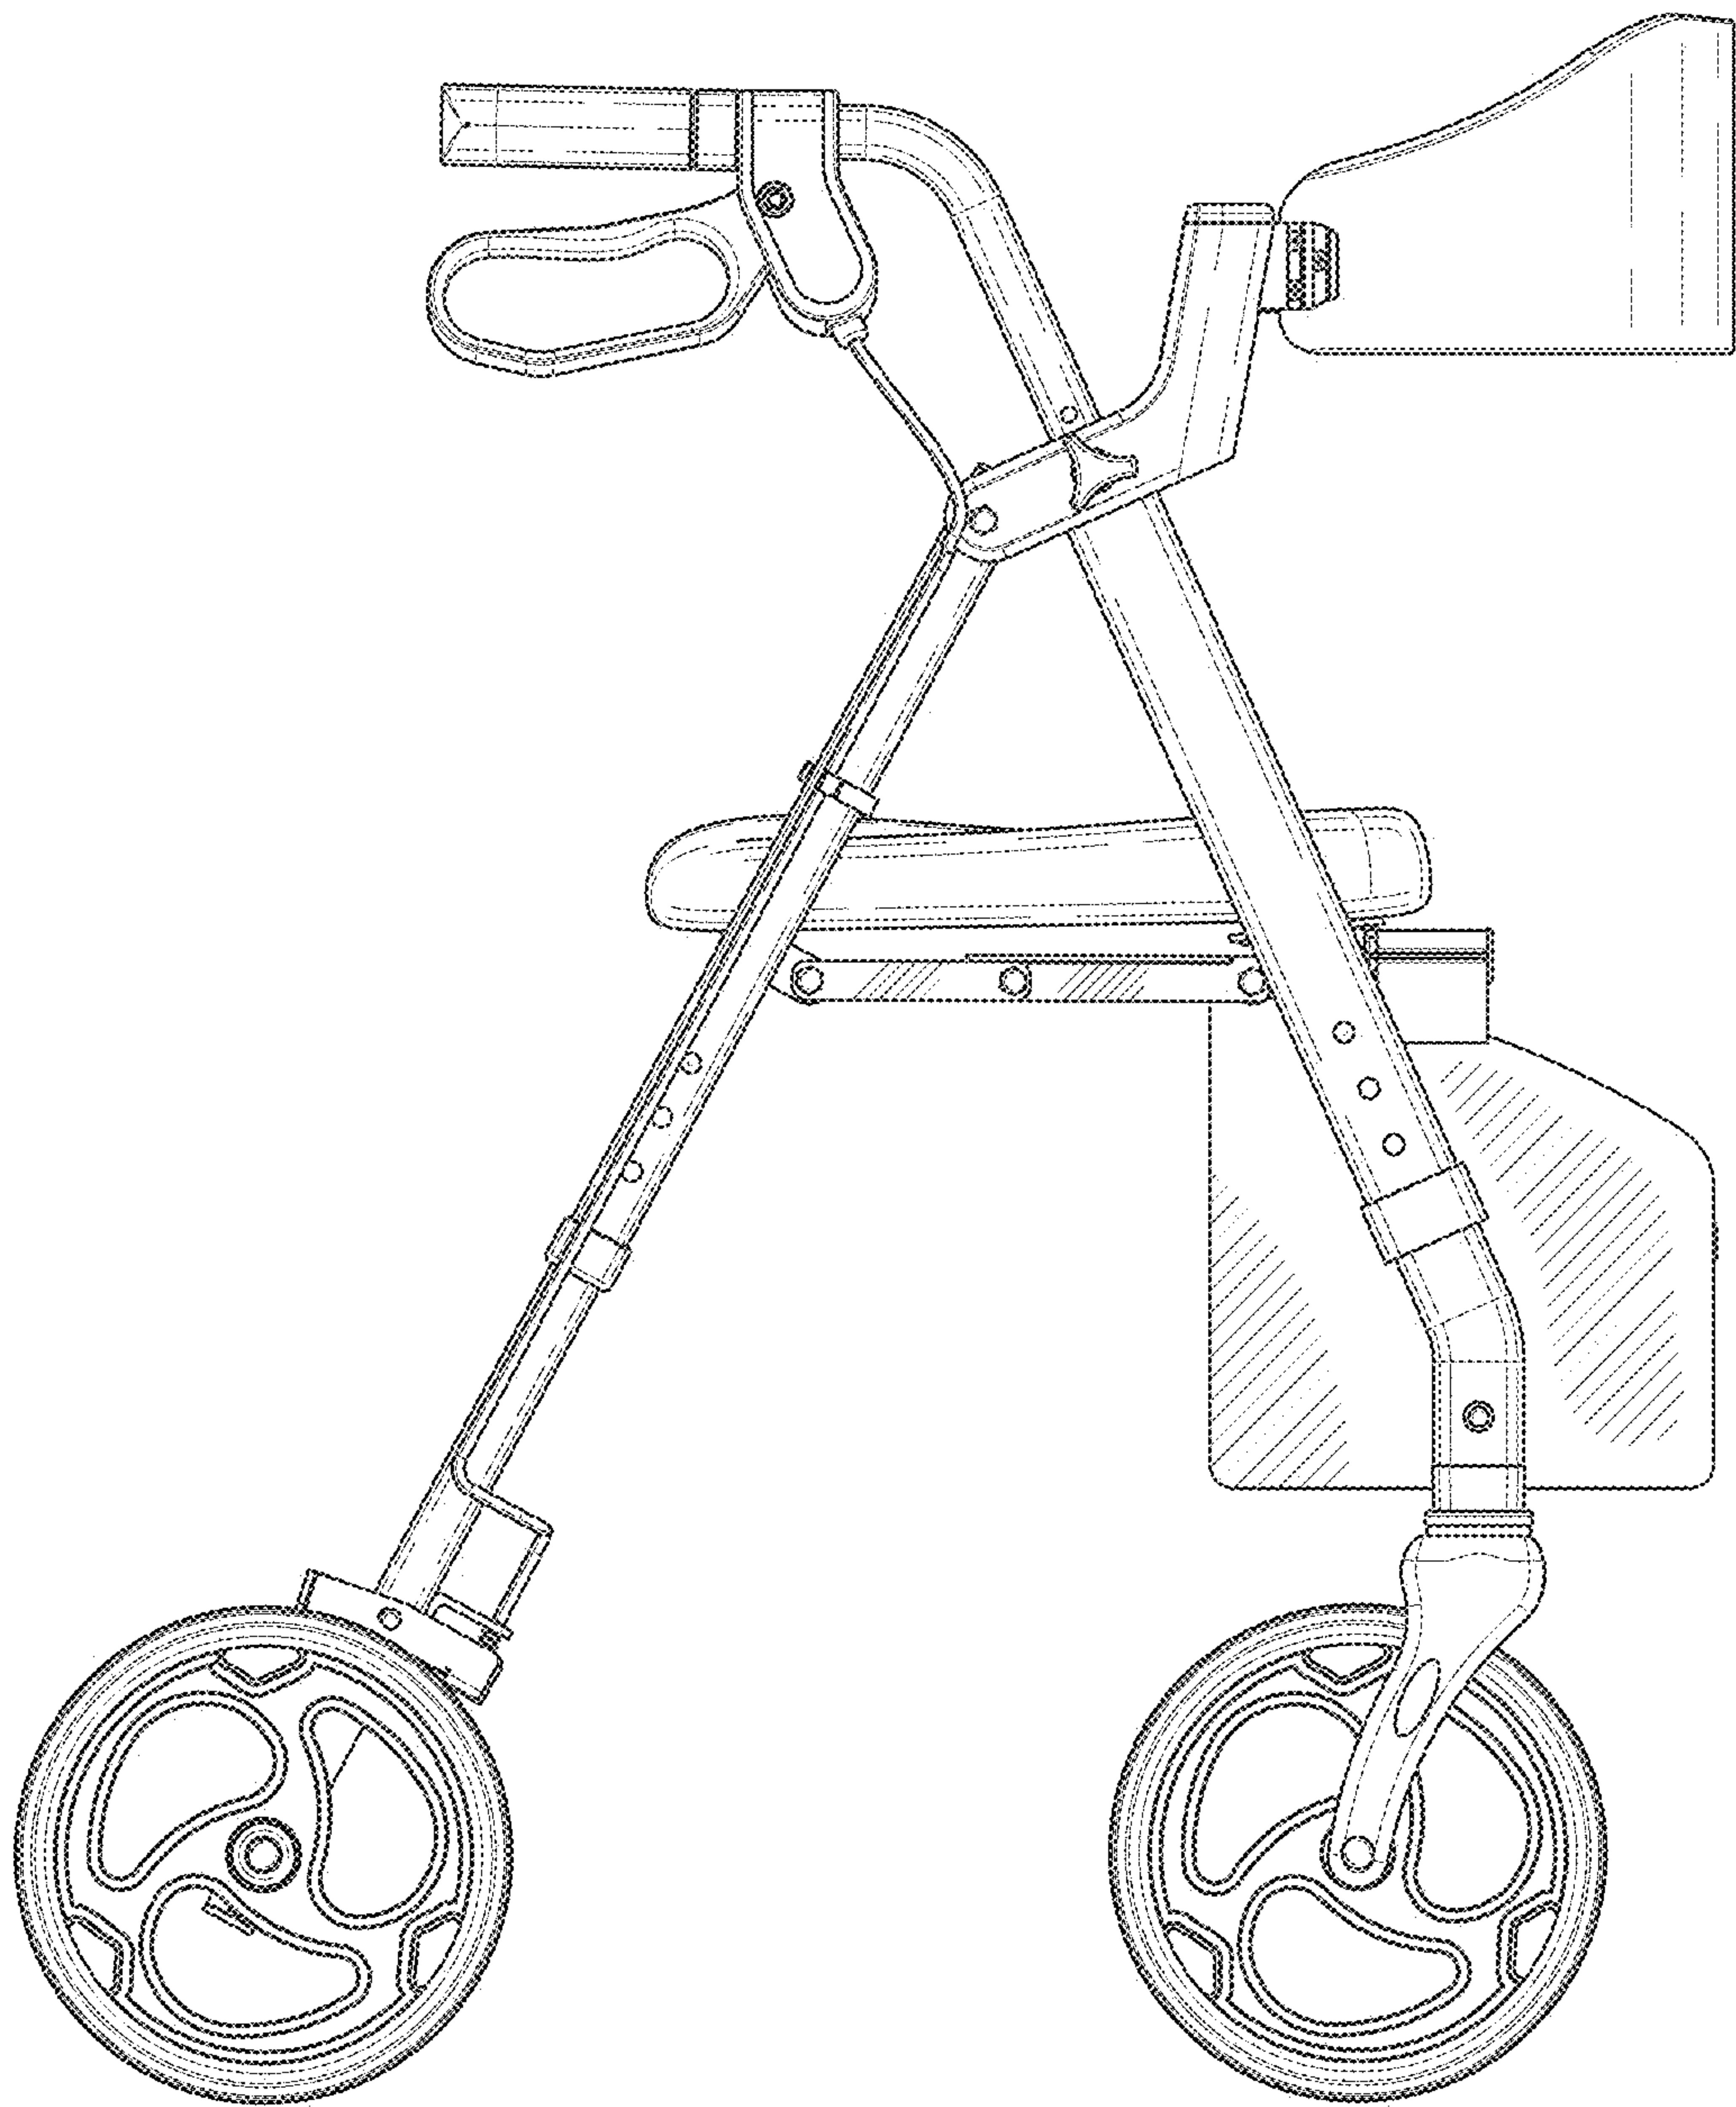


FIG. 5

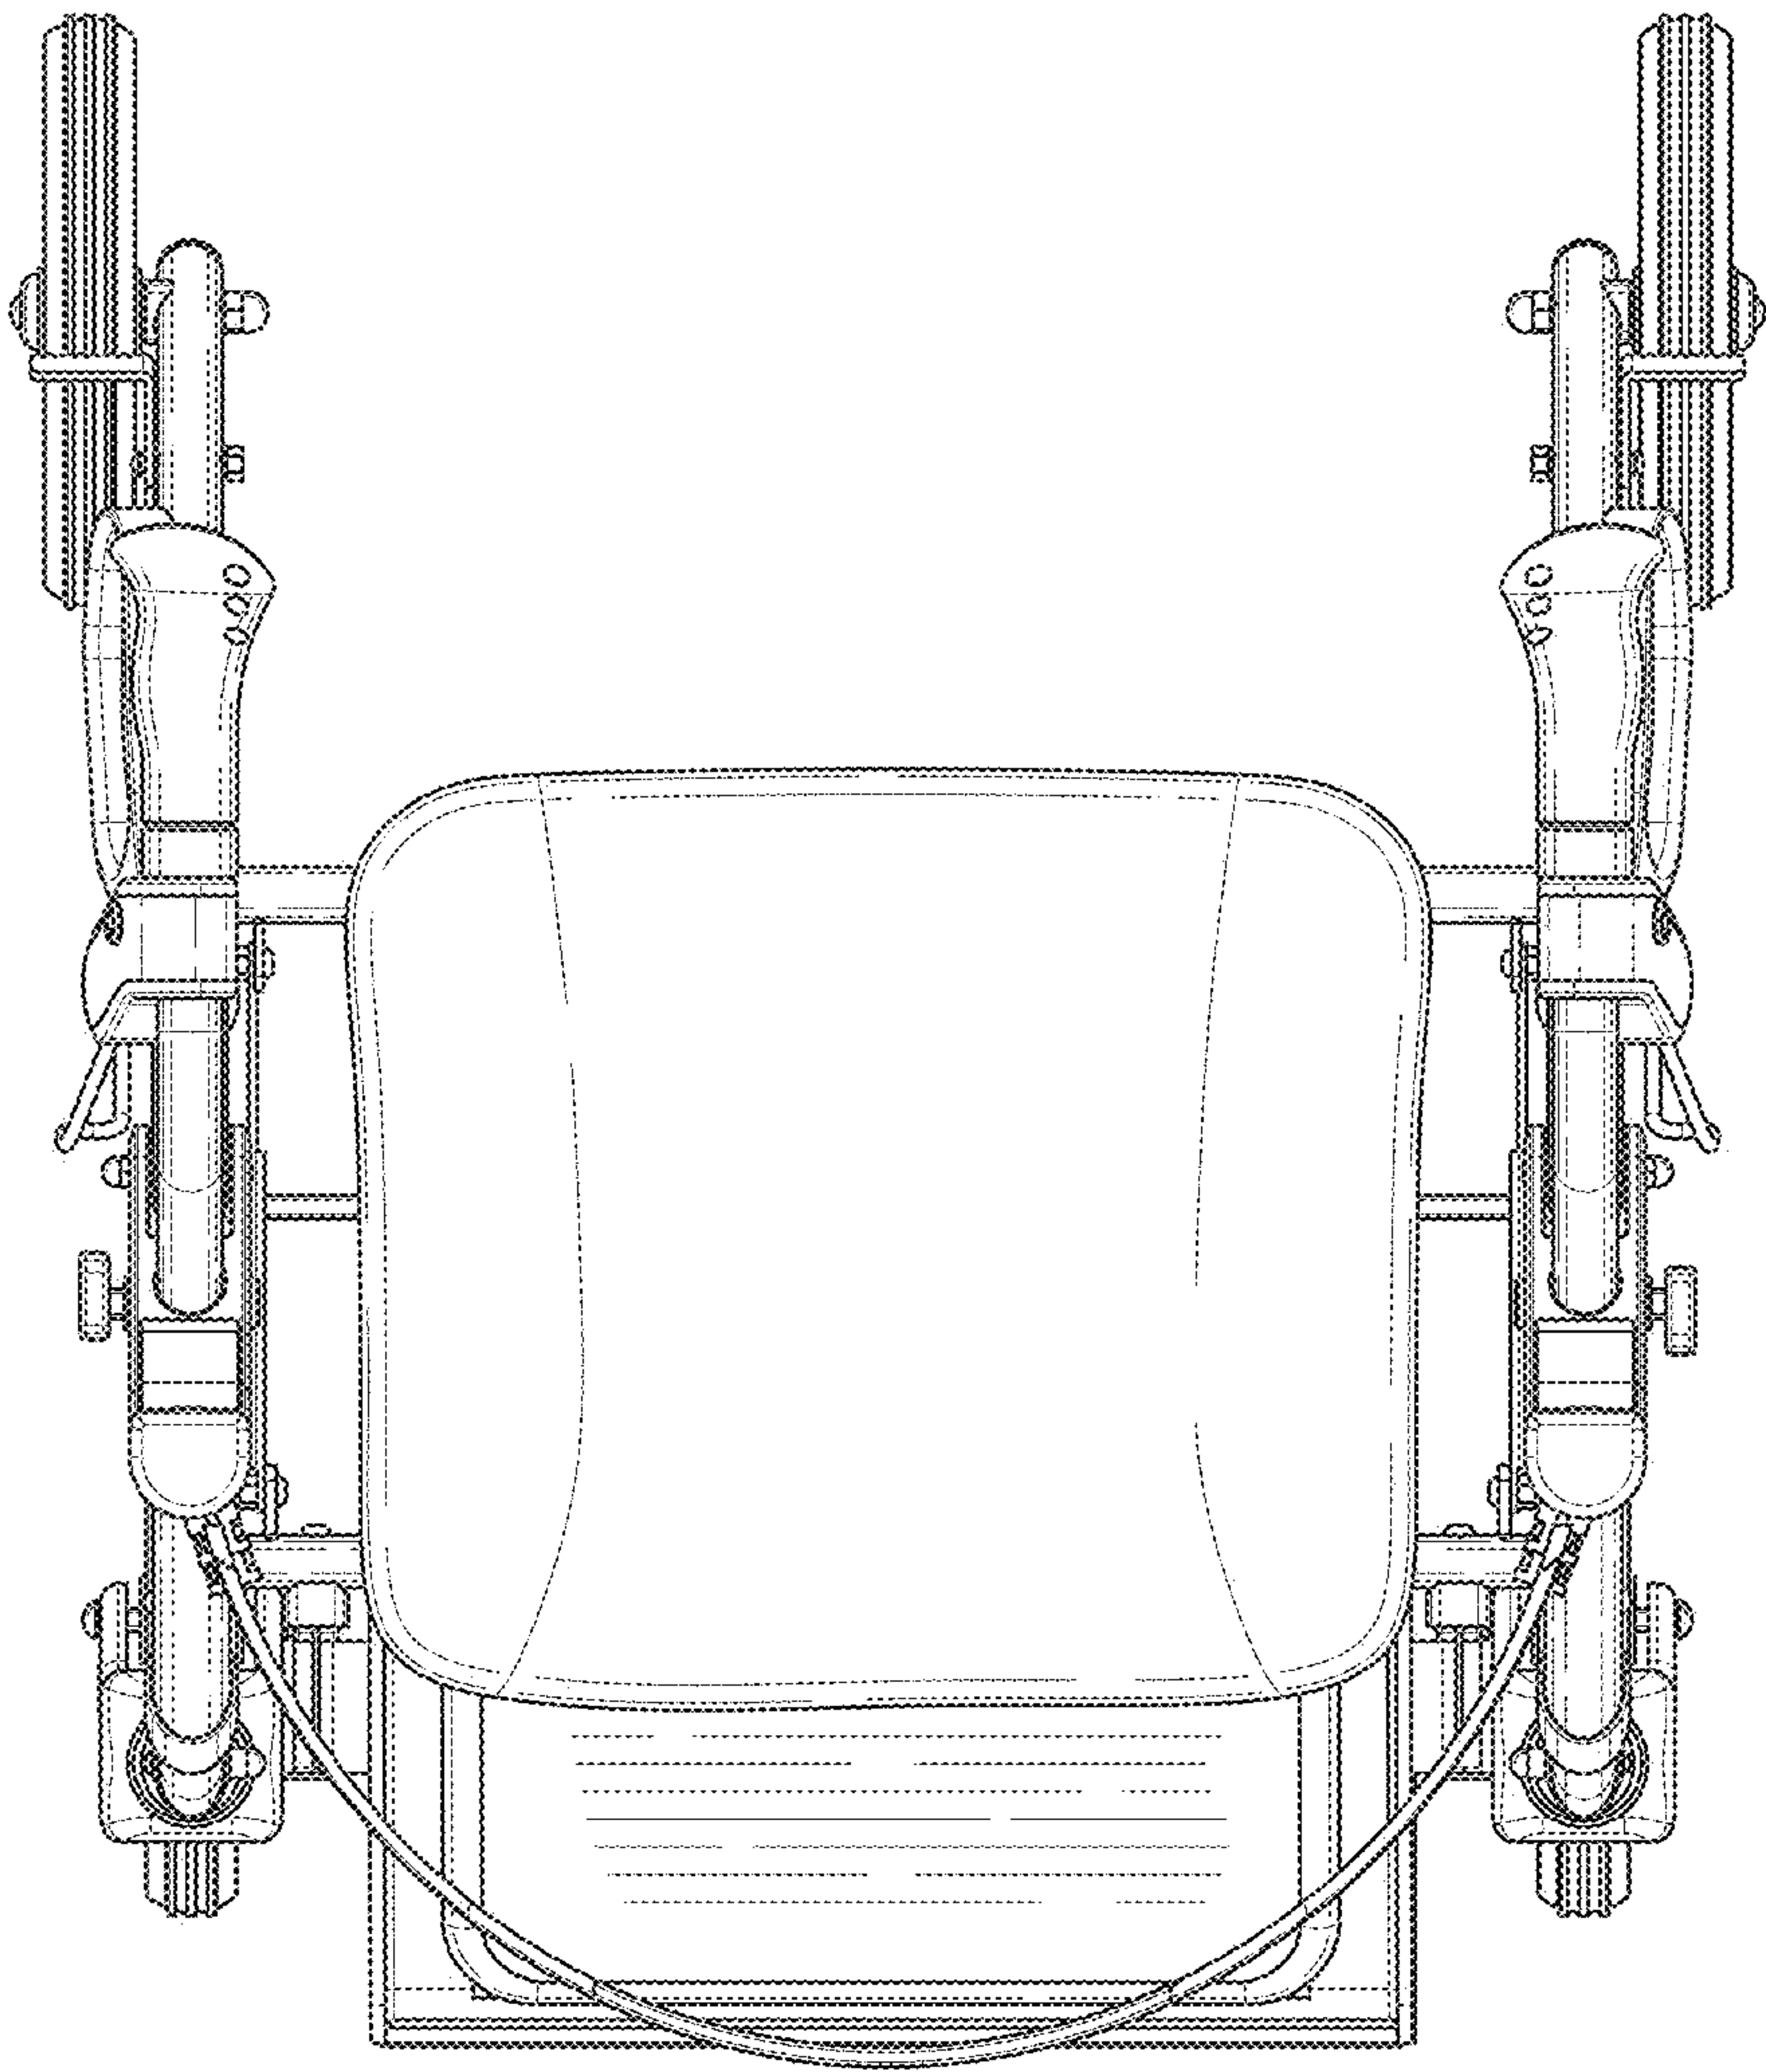


FIG. 6

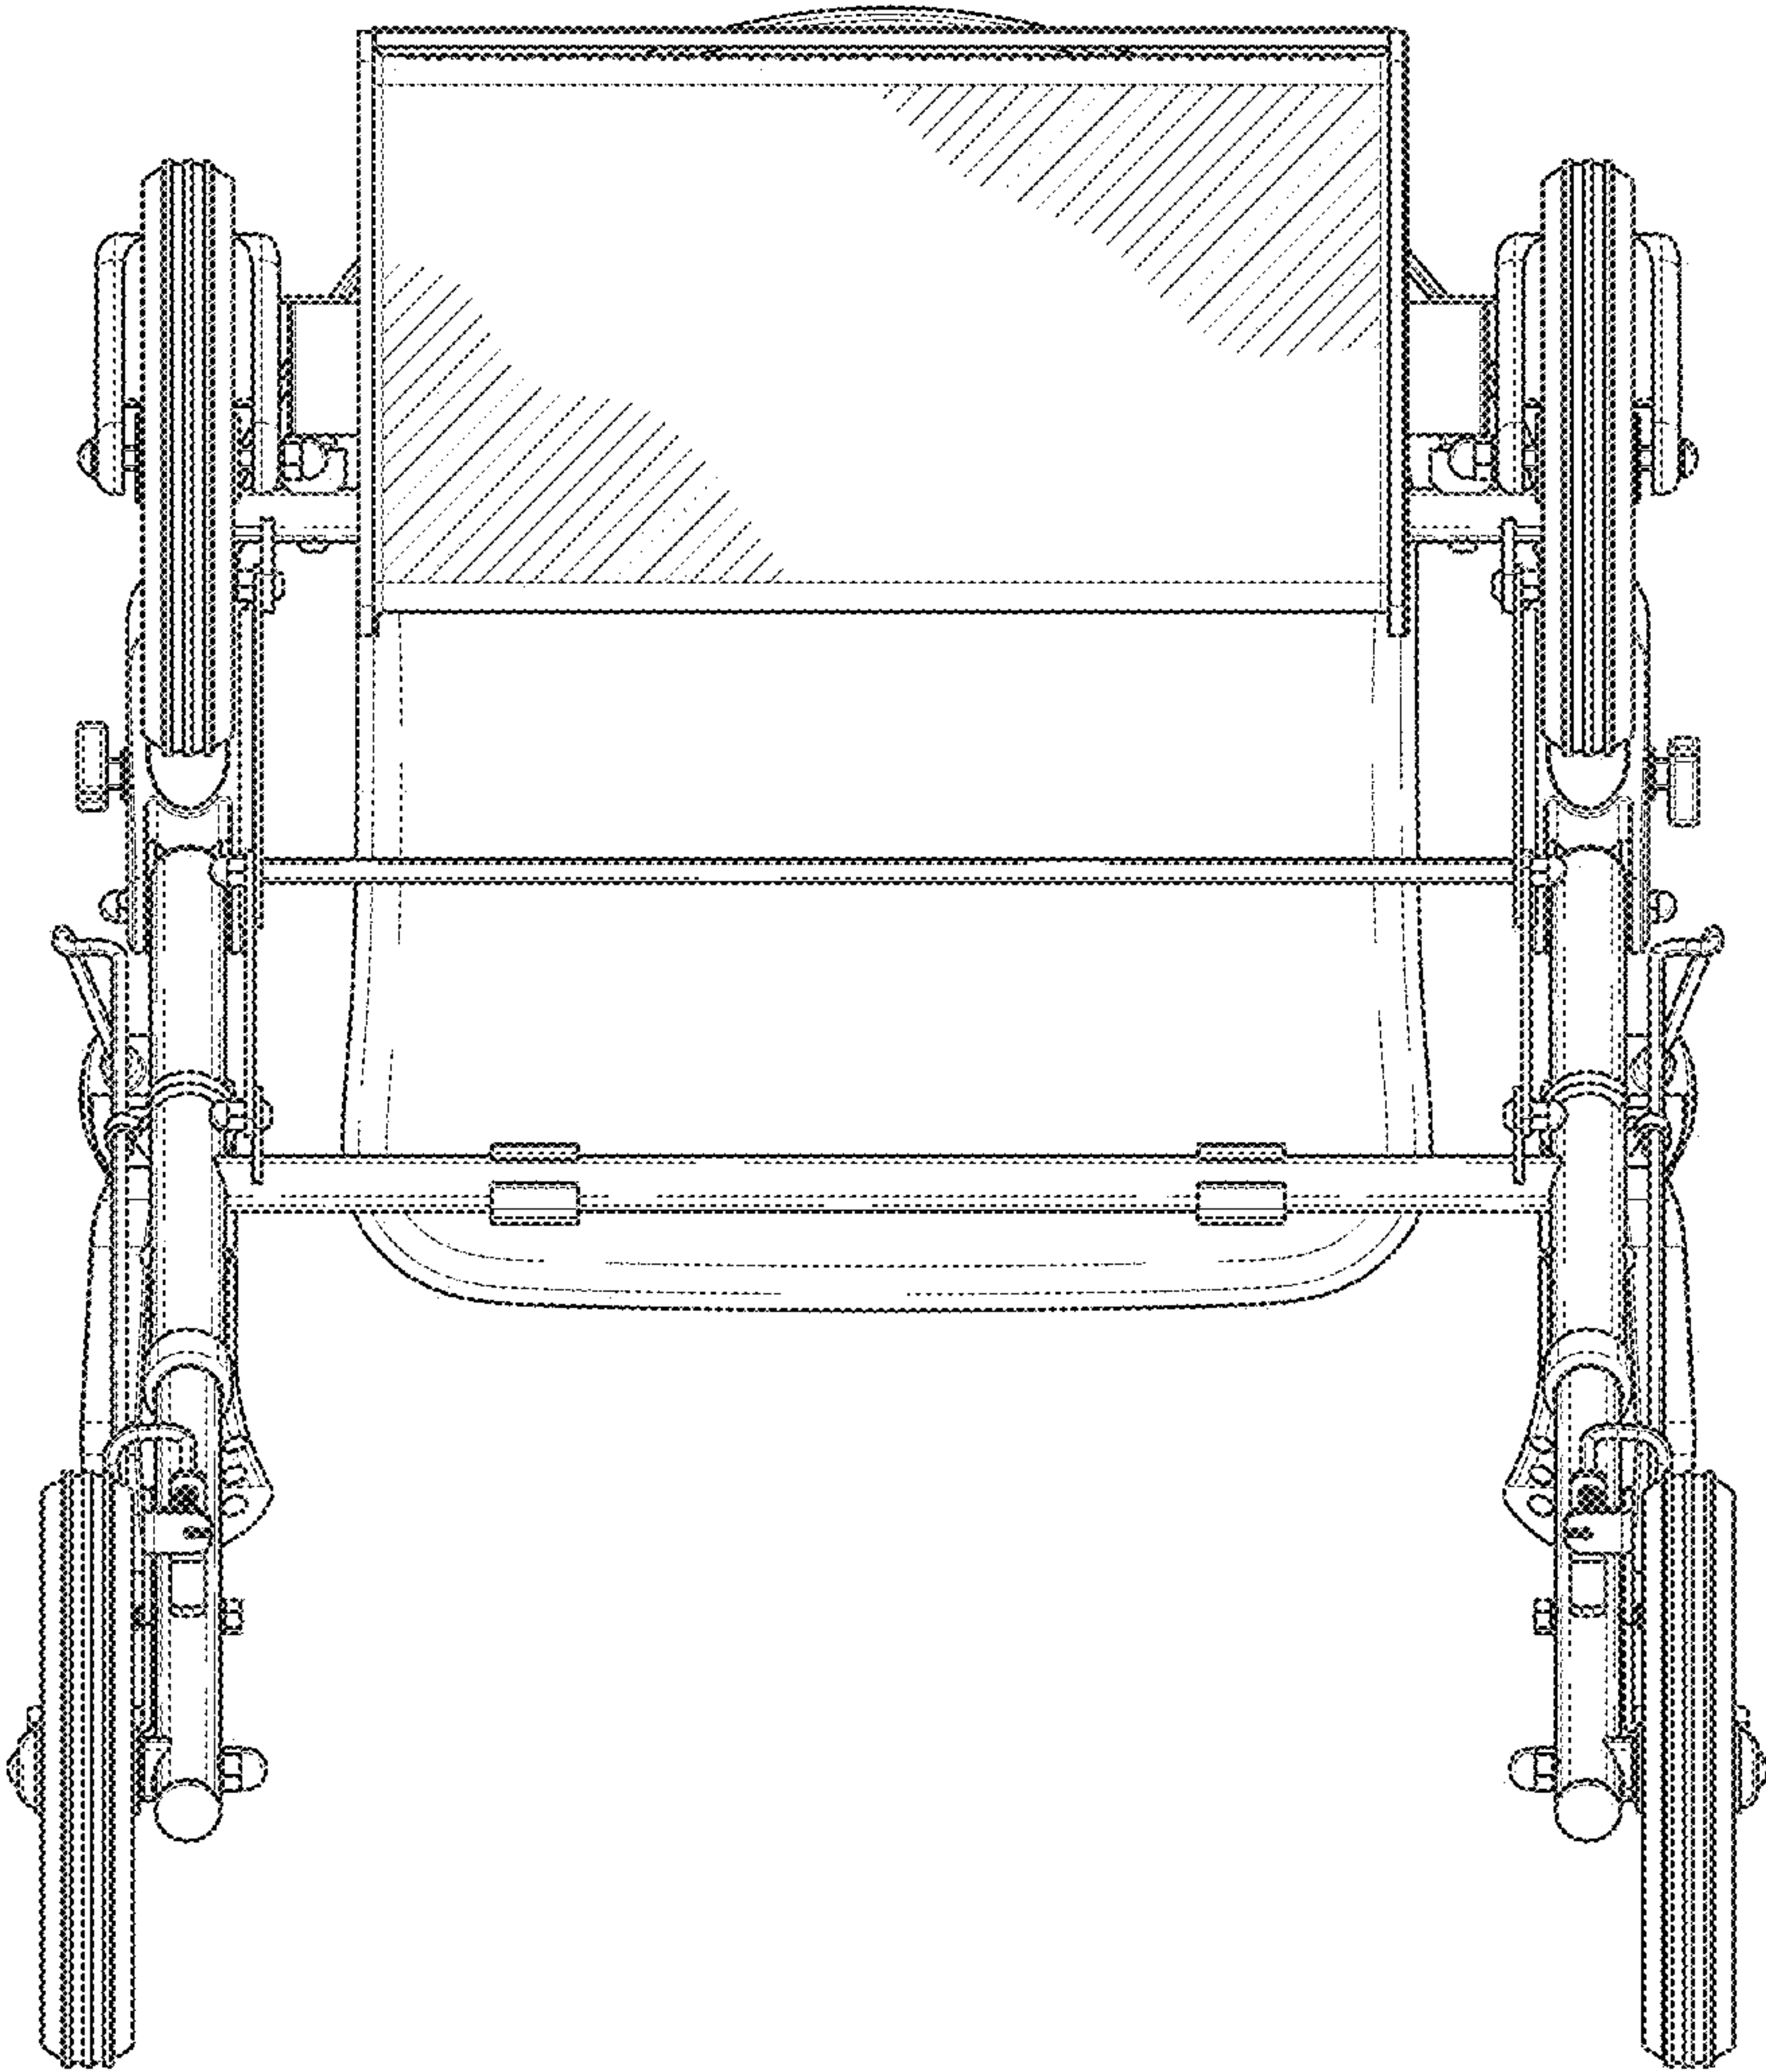


FIG. 7