



US0D1078082S

(12)

United States Design Patent

Comini et al.

(10)

Patent No.:

US D1,078,082 S

(45)

Date of Patent:

** Jun. 3, 2025

(54) MICROBIAL TESTING DEVICE

(71) Applicant: Merck Patent GmbH, Darmstadt (DE)

(72) Inventors: Fabrice Comini, Molsheim (FR); Hugo Ducros, Molsheim (FR)

(73) Assignee: MERCK PATENT GMBH, Darmstadt (DE)

(**) Term: 15 Years

(21) Appl. No.: 29/879,946

(22) Filed: Jul. 14, 2023

(51) LOC (15) Cl. 24-02

(52) U.S. Cl. D24/216

(58) Field of Classification Search

USPC D24/216, 217, 107, 185, 186, 219, 231, D24/232, 233, 234, 169, 209, 210, 218; D10/81

CPC G01N 2035/00306; G01N 2035/00326; G01N 2035/00336; G01N 2035/00039; G01N 2035/00049; G01N 2030/027; G01N 21/76; G01N 33/50; G01N 35/025; G01N 35/00029

See application file for complete search history.

(56) References Cited

U.S. PATENT DOCUMENTS

D253,427 S	*	11/1979	Ohie	D24/169
D270,371 S	*	8/1983	Lee	D24/220
D344,339 S	*	2/1994	Yoshikawa	D24/169
D370,979 S	*	6/1996	Pascale	D24/169
D453,780 S	*	2/2002	Evansic	D15/147
D537,951 S	*	3/2007	Okamoto	D24/233
D556,914 S	*	12/2007	Okamoto	D24/233
D579,540 S	*	10/2008	Hochman	D24/107
D598,036 S	*	8/2009	Bergstraesser	D15/147
D599,688 S	*	9/2009	Ito	D10/81
D603,972 S	*	11/2009	Petersen	D24/216
D607,569 S	*	1/2010	Yukikado	D24/186

D648,844 S	*	11/2011	Nelson	D24/185
D657,068 S	*	4/2012	Shibata	D24/216
D665,084 S	*	8/2012	Ishihara	D24/186
D673,295 S	*	12/2012	Motadel	D24/227
D678,530 S	*	3/2013	Khan	D24/186
D682,432 S	*	5/2013	Khan	D24/186
D682,441 S	*	5/2013	Kim	D24/216

(Continued)

FOREIGN PATENT DOCUMENTS

CN 308450369 * 2/2024

OTHER PUBLICATIONS

MAS-100 NT Ex, [site visited Aug. 21, 2024]. Available from Internet. URL: <https://www.sigmaaldrich.com/US/en/product/mm/109194> (Year: 2024).*

Primary Examiner — T Chase Nelson
Assistant Examiner — Kelly L Gross
(74) Attorney, Agent, or Firm — John A. Yirga, Esq.; Watts Law LLC


(57) CLAIM

The ornamental design for a microbial testing device as shown and described.

DESCRIPTION

FIG. 1 is a front, right perspective view of a microbial testing device showing the new design.
FIG. 2 is a front elevation view thereof.
FIG. 3 is a rear elevation view thereof.
FIG. 4 is a right side elevation view thereof.
FIG. 5 is a left side elevation view thereof.
FIG. 6 is a top plan view thereof; and,
FIG. 7 is a bottom plan view thereof.
The broken line in the drawings illustrate portions of the microbial testing device that form no part of the claimed design.

1 Claim, 7 Drawing Sheets

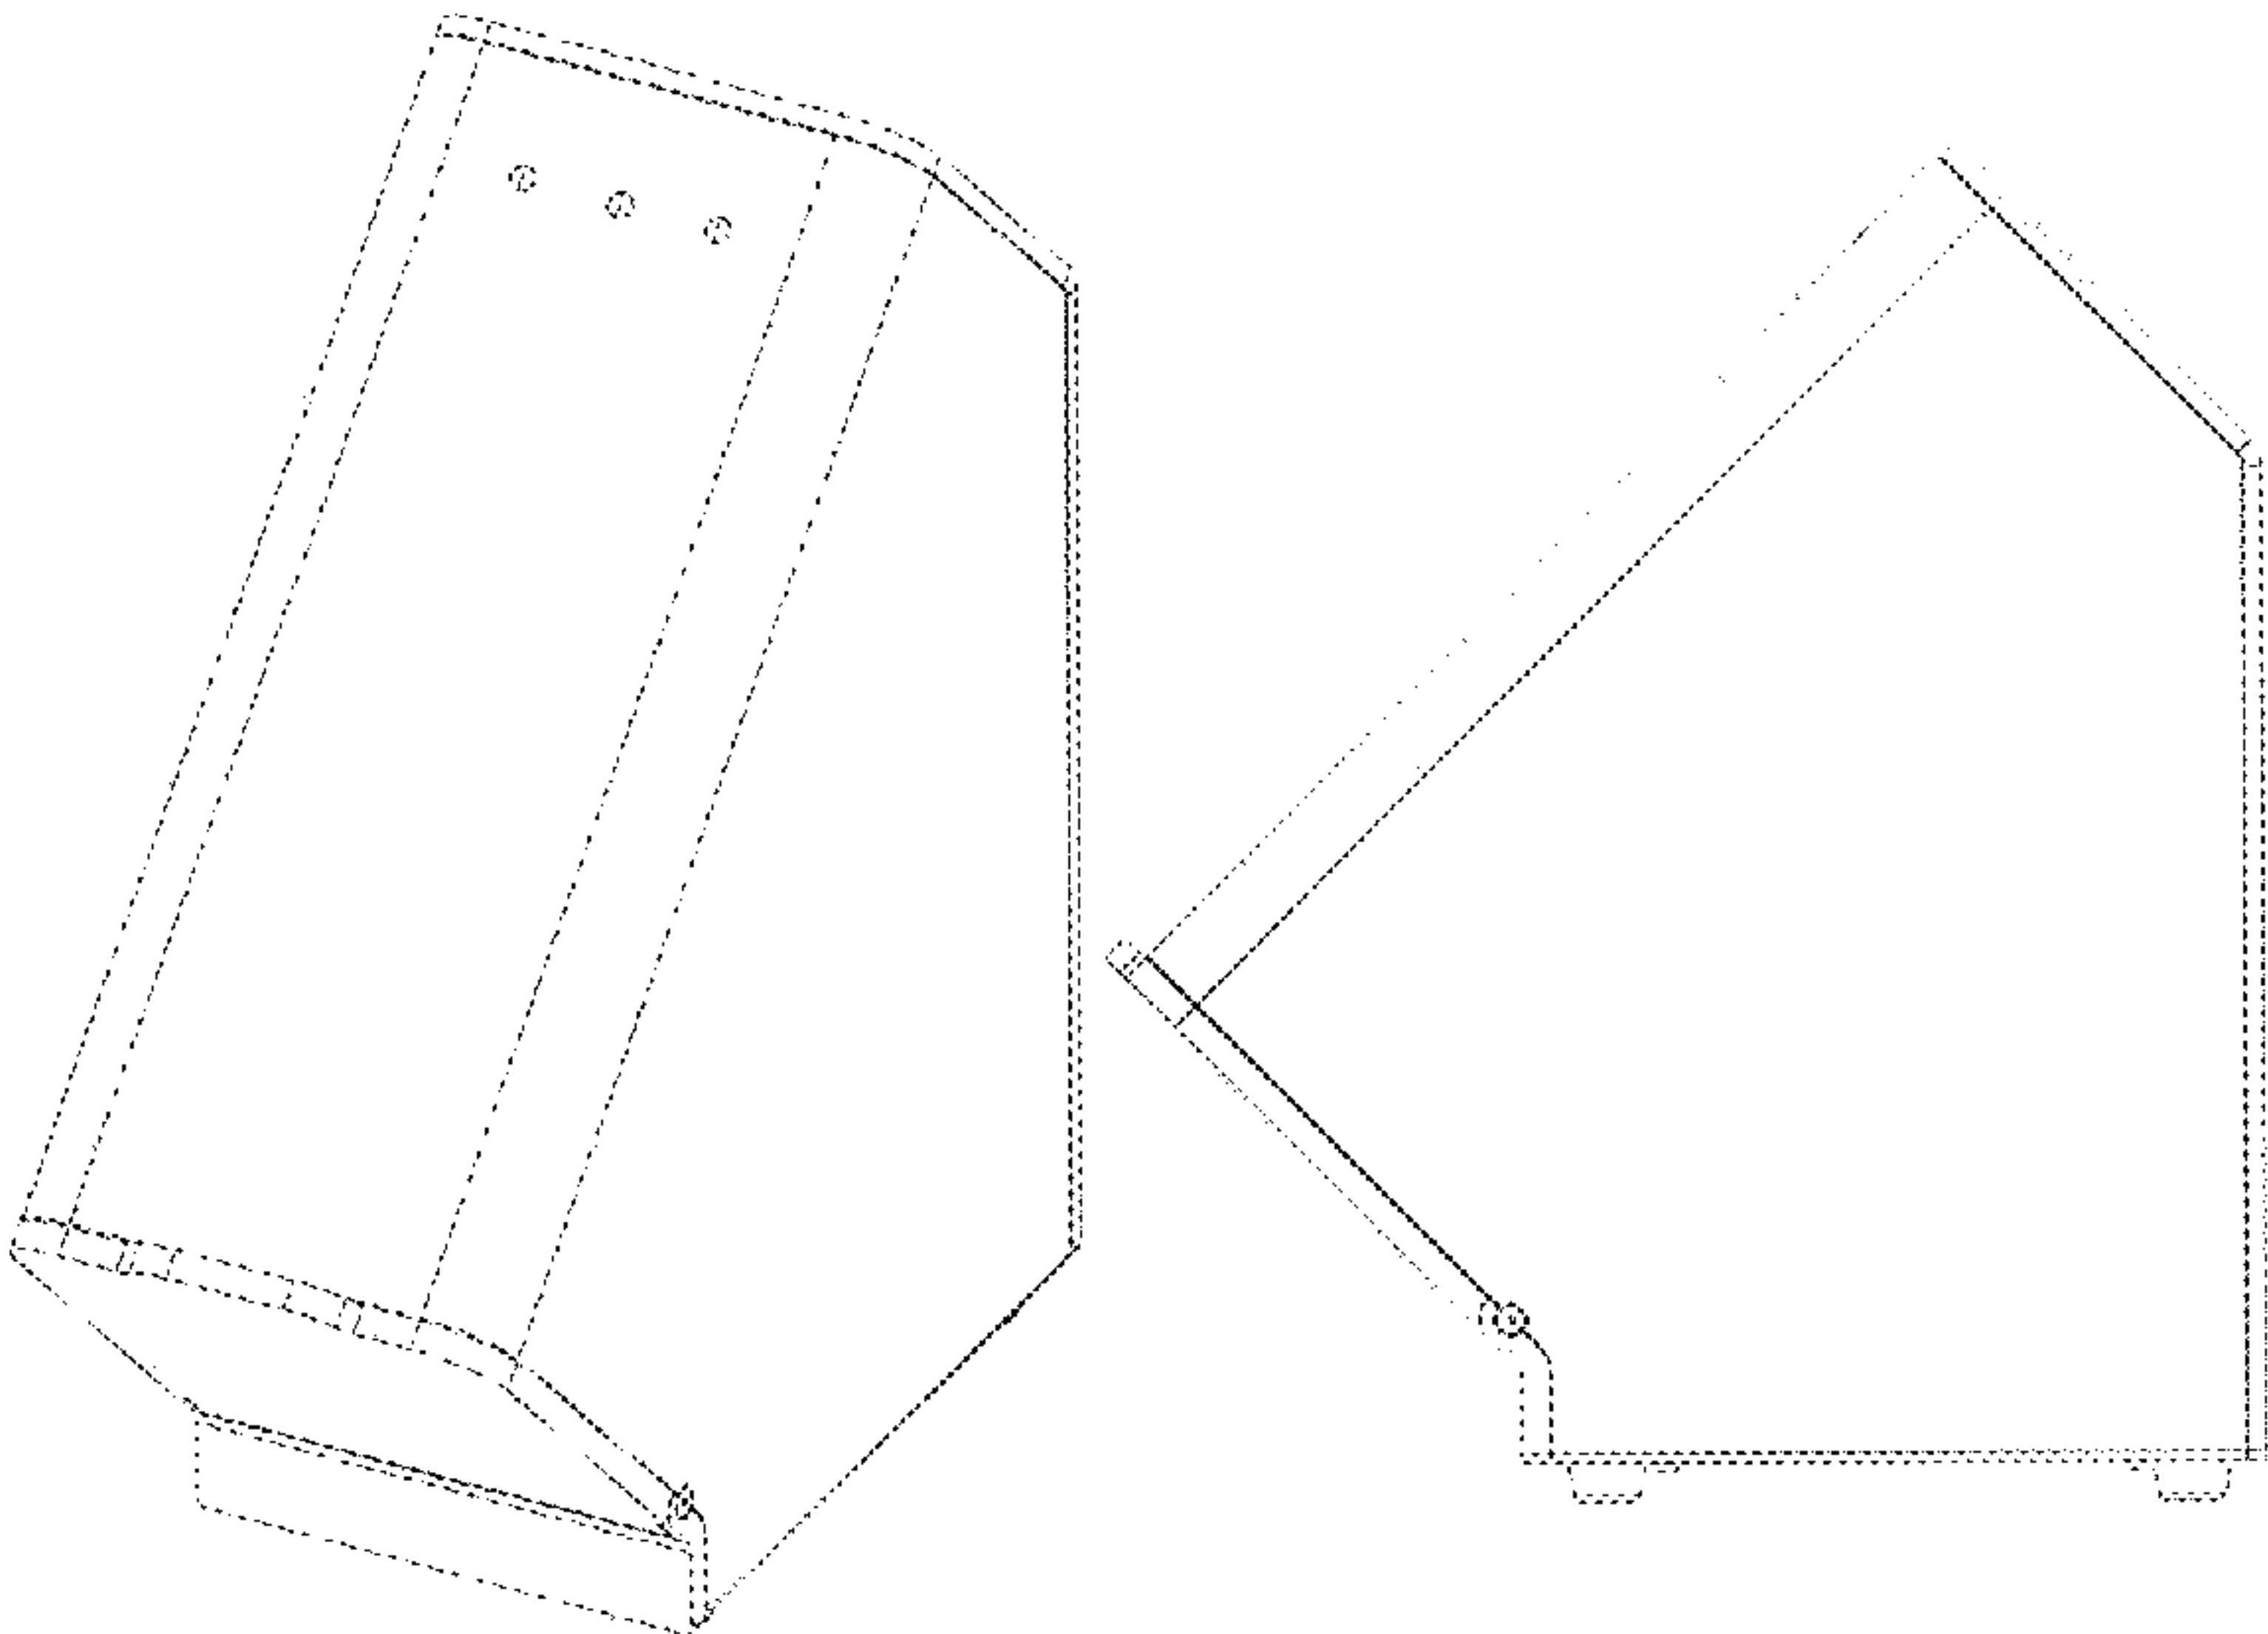

(56)

References Cited

U.S. PATENT DOCUMENTS

D684,270 S * 6/2013 Chang D24/216
D689,193 S * 9/2013 Shinohara D24/216
D694,899 S * 12/2013 Cook D24/216
D705,441 S * 5/2014 Chang D24/216
D712,066 S * 8/2014 Noda D24/232
D713,042 S * 9/2014 Gerber D24/185
D719,671 S * 12/2014 Nishikawa D24/232
D731,662 S * 6/2015 Khan D24/186
D762,748 S * 8/2016 Schönherr D15/122
D772,086 S * 11/2016 Schueren D24/234
D774,205 S * 12/2016 Grace D24/169
D785,198 S * 4/2017 Lemke D24/232
D809,948 S * 2/2018 Hirche D10/87
D818,146 S * 5/2018 Tanaka D24/216
D821,601 S * 6/2018 Henderson D24/169
D822,848 S * 7/2018 Lemke D24/232
D827,859 S * 9/2018 Mathers D24/232
D833,033 S * 11/2018 Foster D24/233
D835,281 S * 12/2018 Clifford D24/185
D835,293 S * 12/2018 Masuda D24/232
D843,007 S * 3/2019 Schulz D24/216
D848,880 S * 5/2019 Smith D24/234
D848,881 S * 5/2019 Huang D24/216

D865,220 S * 10/2019 Davidson D24/232
D869,310 S * 12/2019 Nagasawa D24/216
D870,576 S * 12/2019 Kang D24/216
D881,405 S * 4/2020 Hussey D24/216
D886,653 S * 6/2020 Sugie D24/216
D887,006 S * 6/2020 Frenkler D24/176
D887,295 S * 6/2020 Carney D10/81
D888,267 S * 6/2020 Salomon D24/216
D888,985 S * 6/2020 Hsieh D24/232
D892,352 S * 8/2020 Huang D24/232
D897,874 S * 10/2020 Carney D10/81
D907,211 S * 1/2021 Spurling D24/169
D907,795 S * 1/2021 Buie D24/216
D933,848 S * 10/2021 Shapiro D15/147
D942,039 S * 1/2022 Luther D24/233
D946,431 S * 3/2022 Blake D24/232
D963,499 S * 9/2022 Blake D24/232
D975,308 S * 1/2023 Frenkler D24/186
D979,094 S * 2/2023 Tortora D24/227
D982,181 S * 3/2023 Tanaka D24/232
D983,682 S * 4/2023 Lubjenka D24/232
D1,023,804 S * 4/2024 Blake D24/216
D1,031,080 S * 6/2024 Miya D3/203.1
D1,035,035 S * 7/2024 Freber D24/232
D1,035,857 S * 7/2024 Hochman D24/107
2024/0183869 A1 * 6/2024 Subramanian G01N 1/30

* cited by examiner

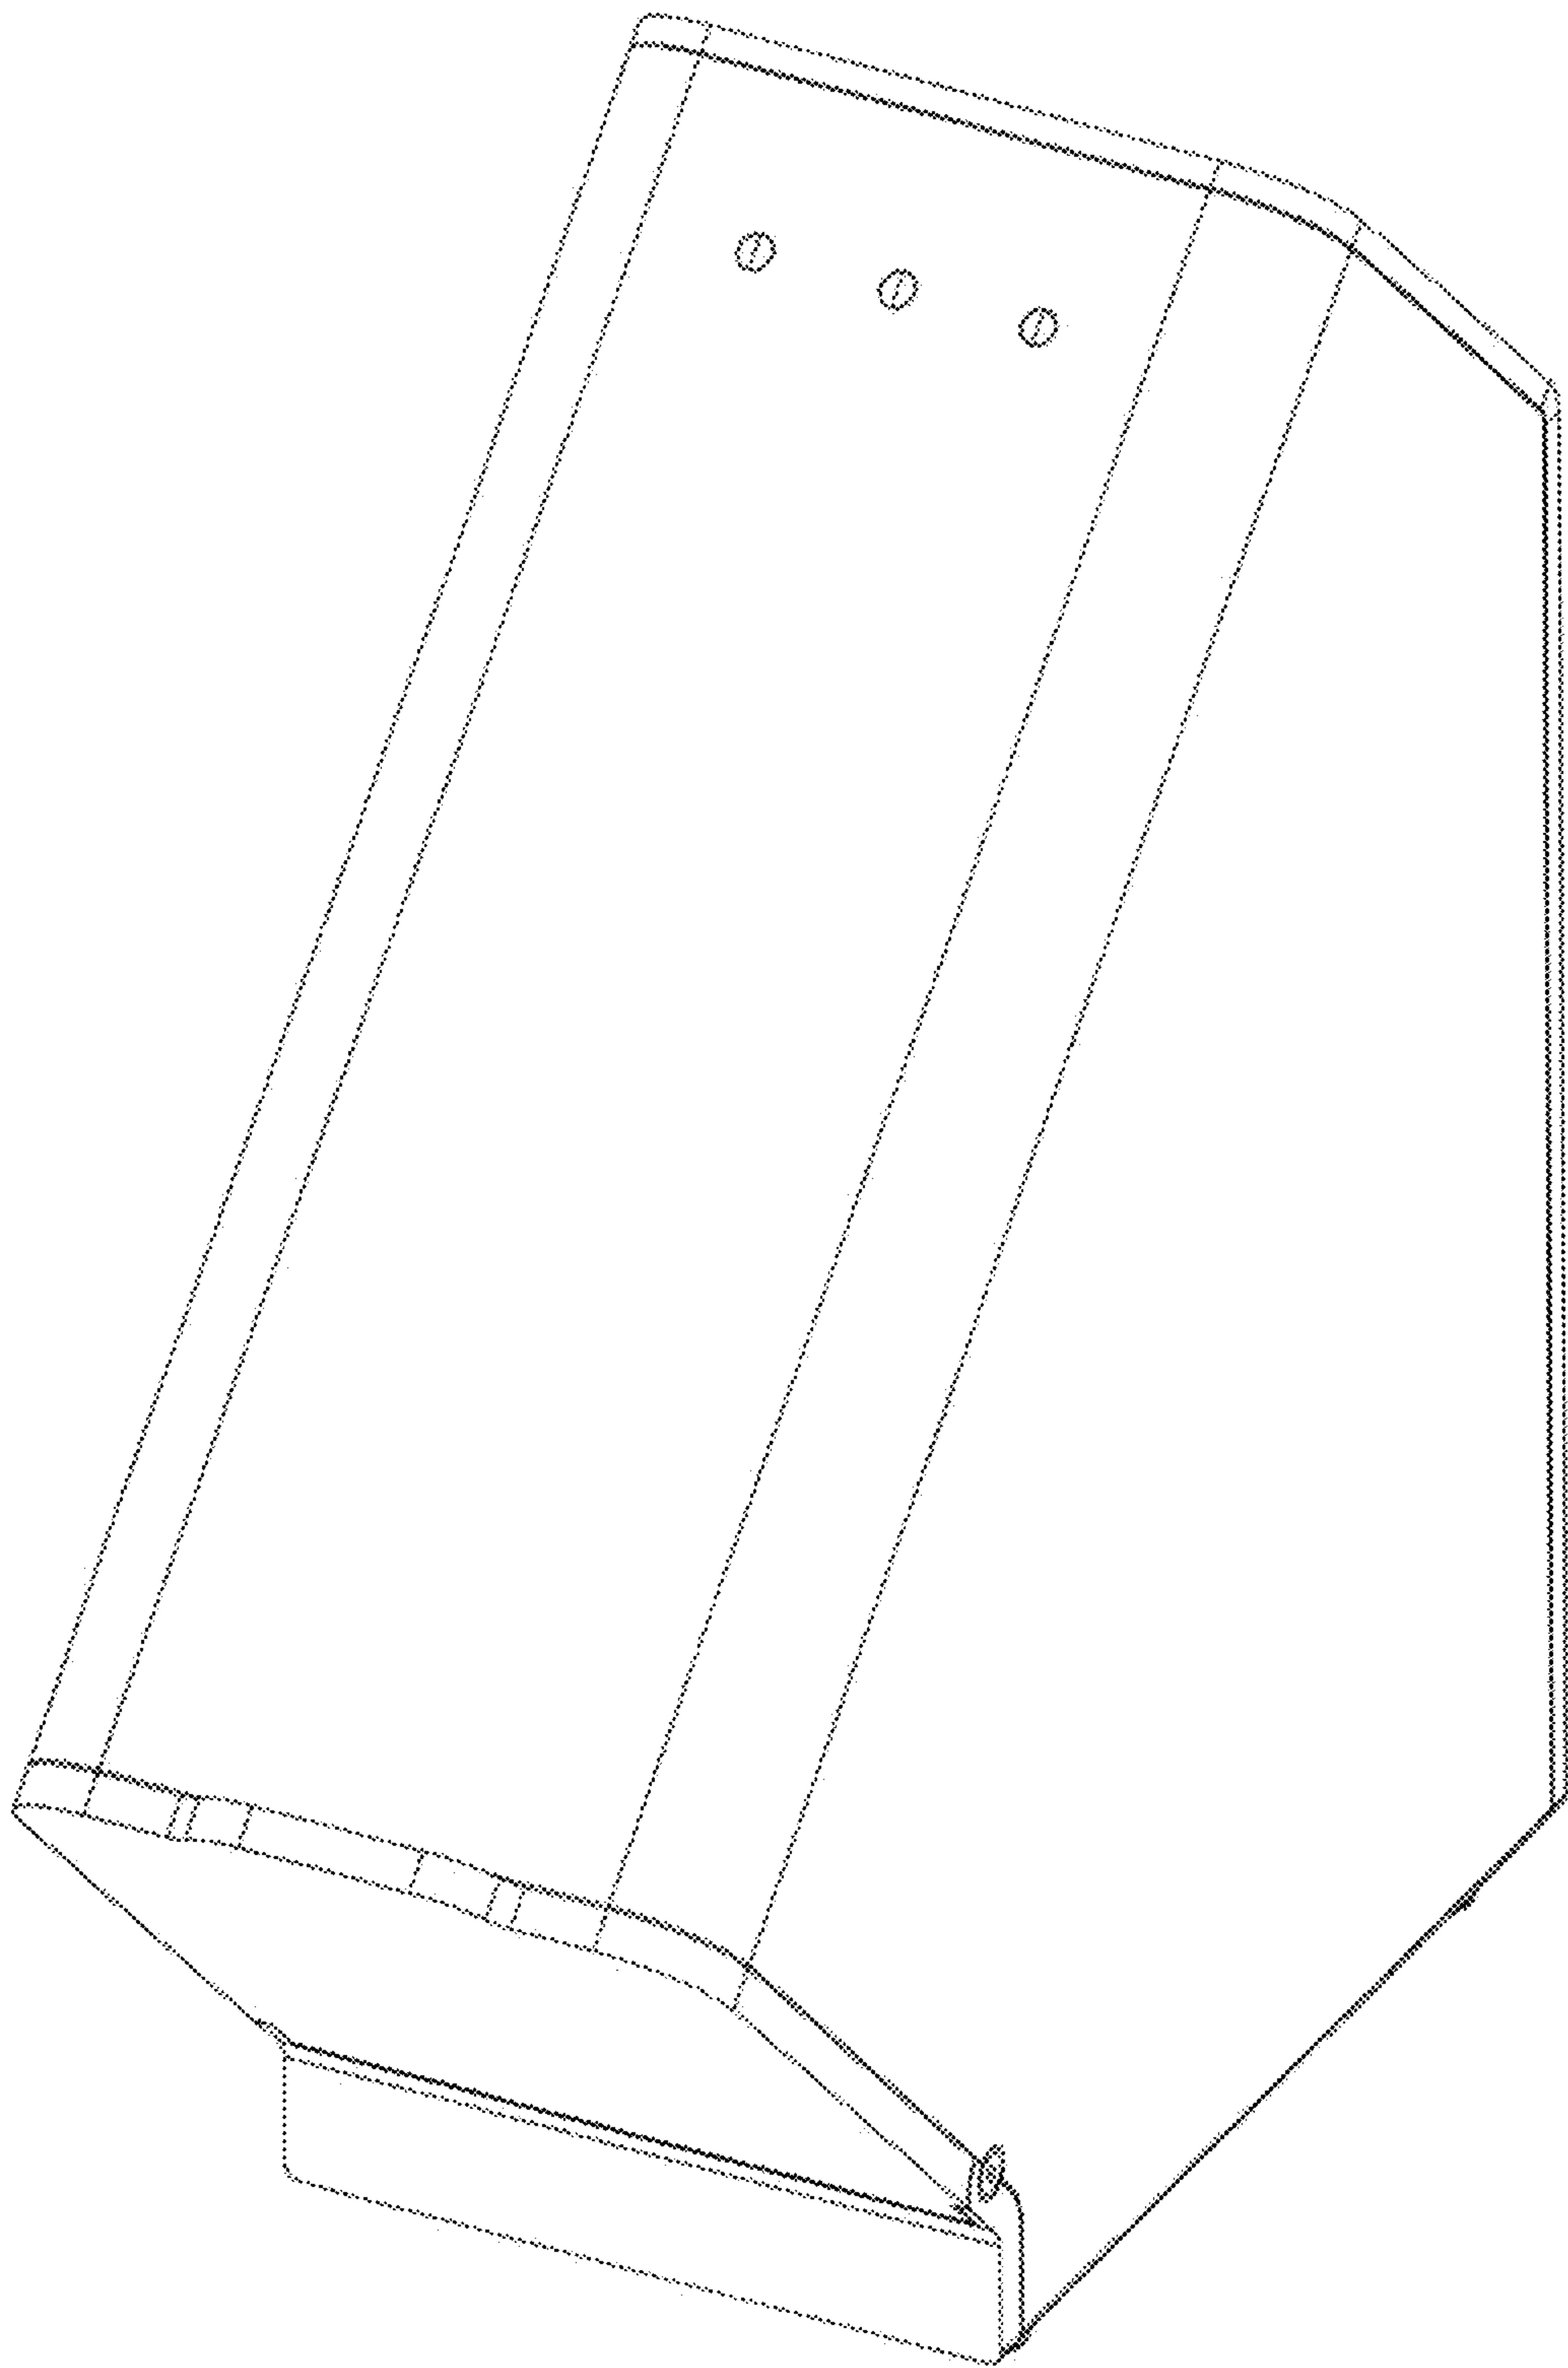


FIG. 1

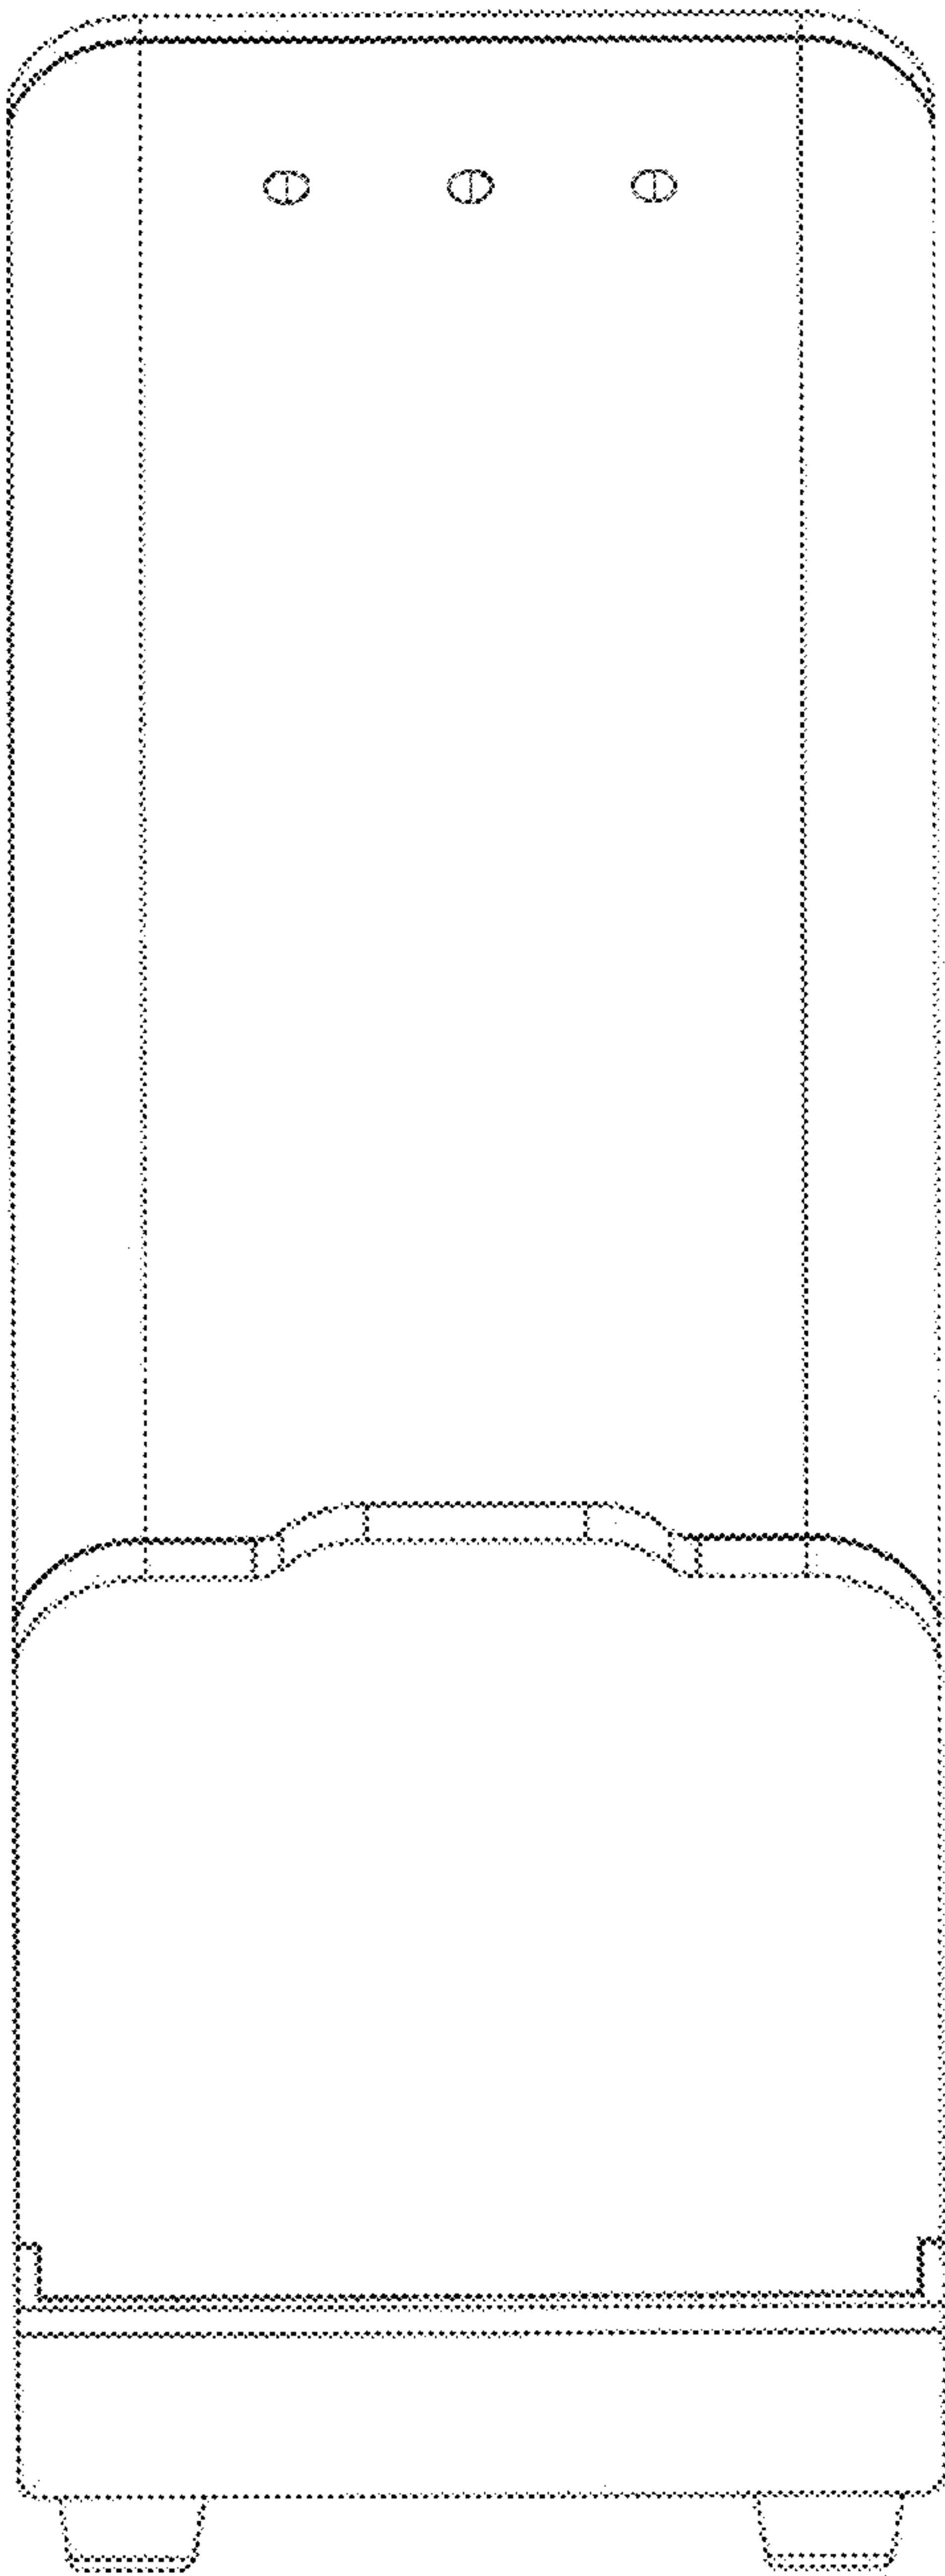


FIG. 2

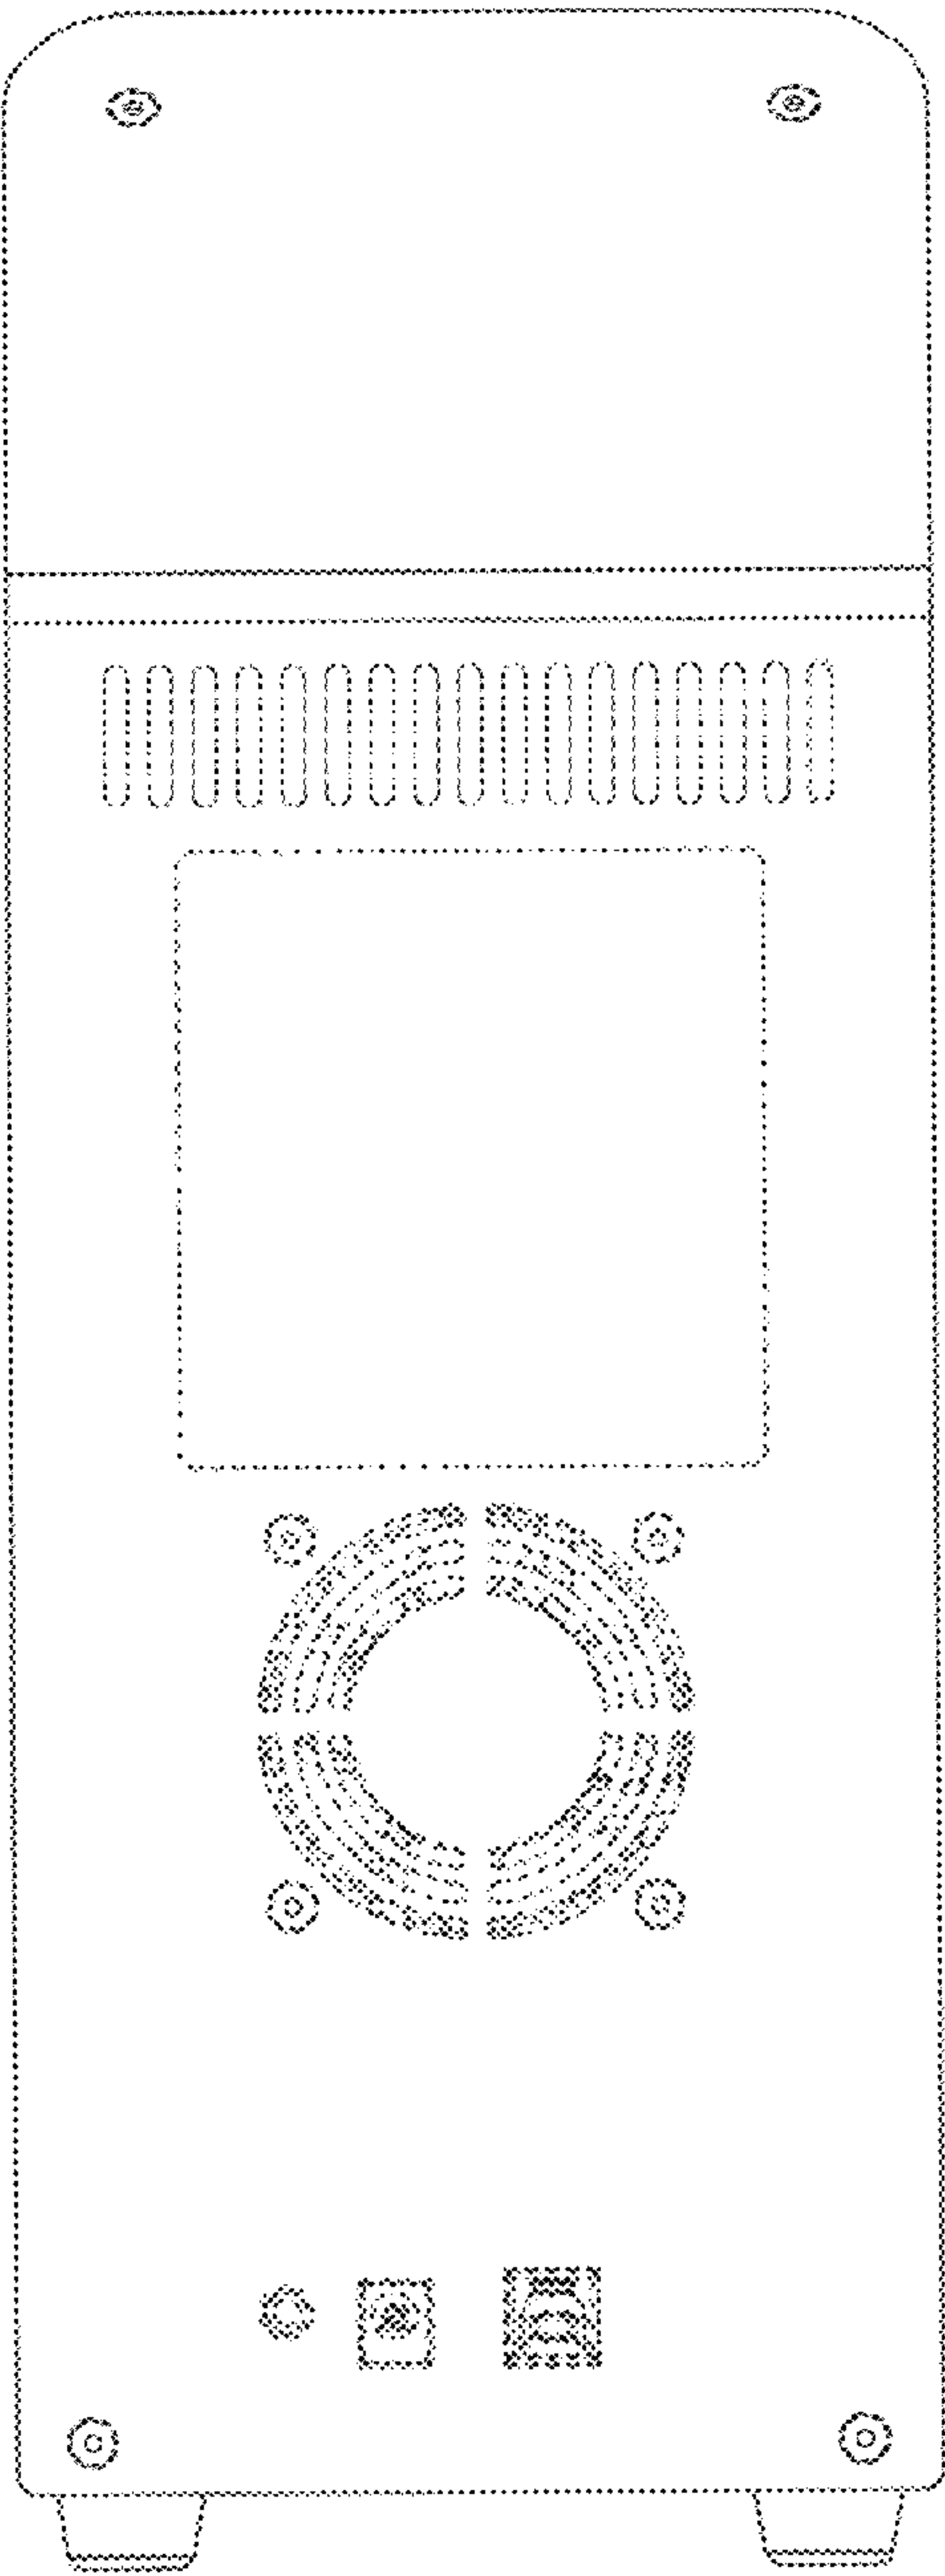


FIG. 3

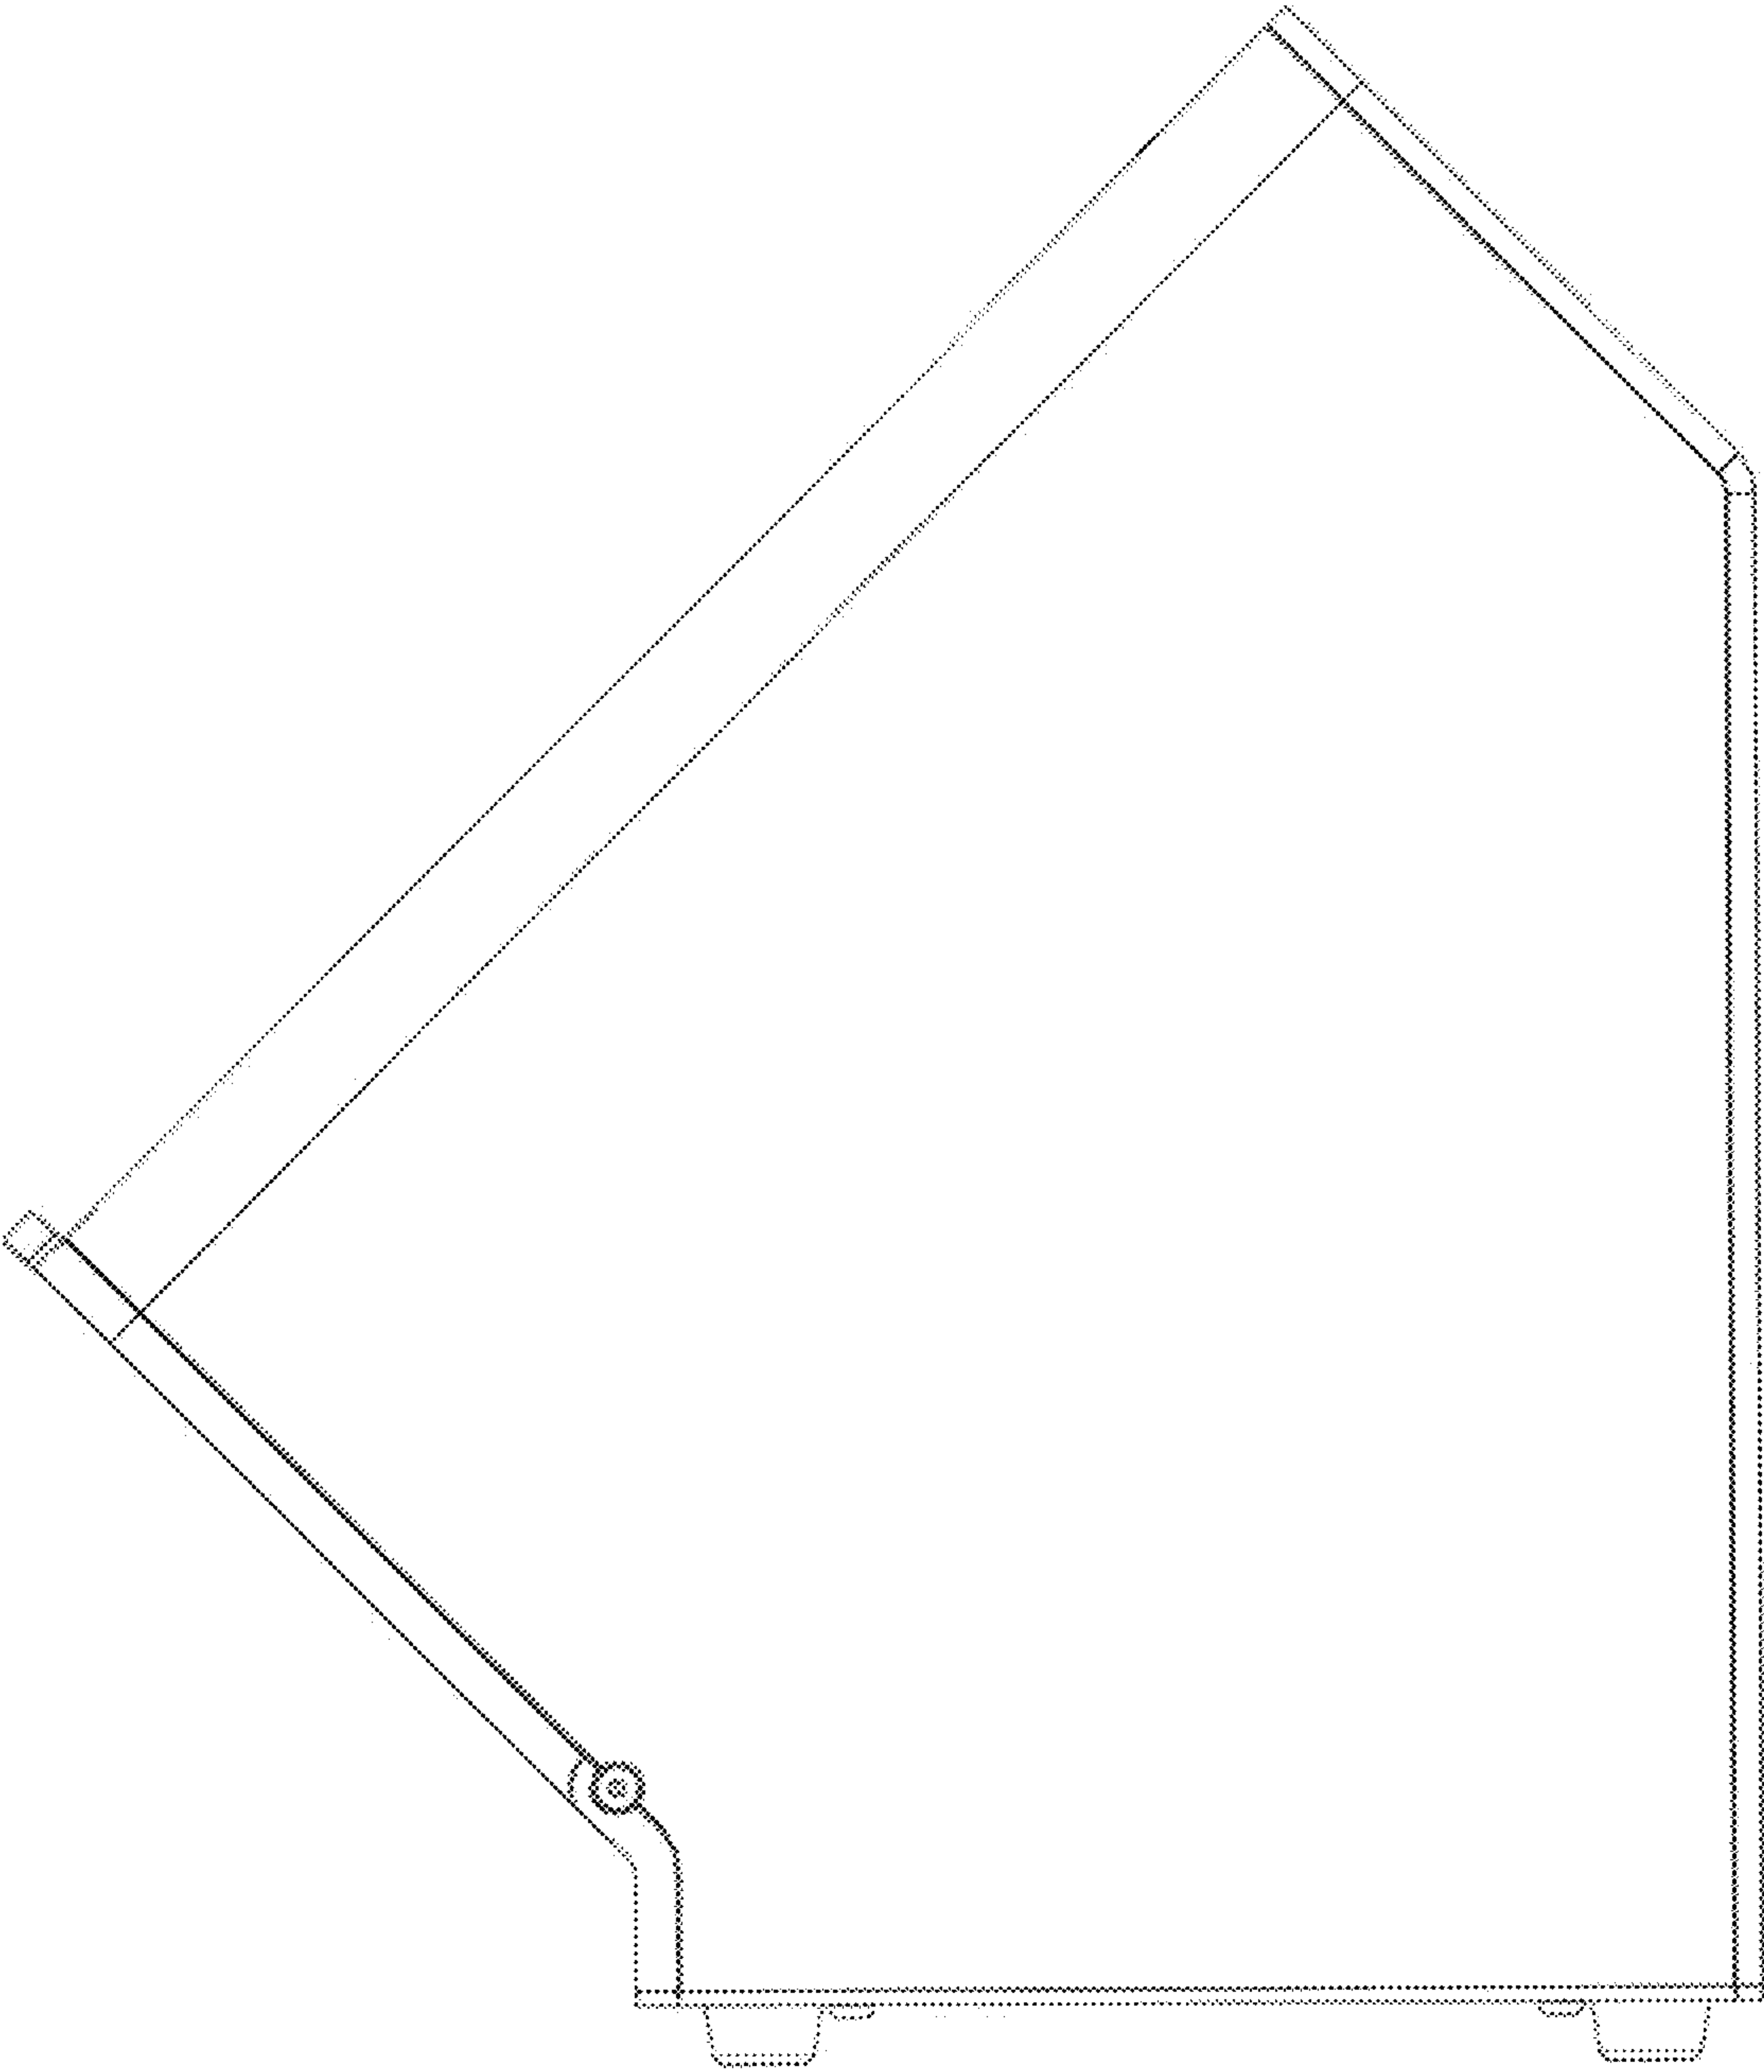


FIG. 4

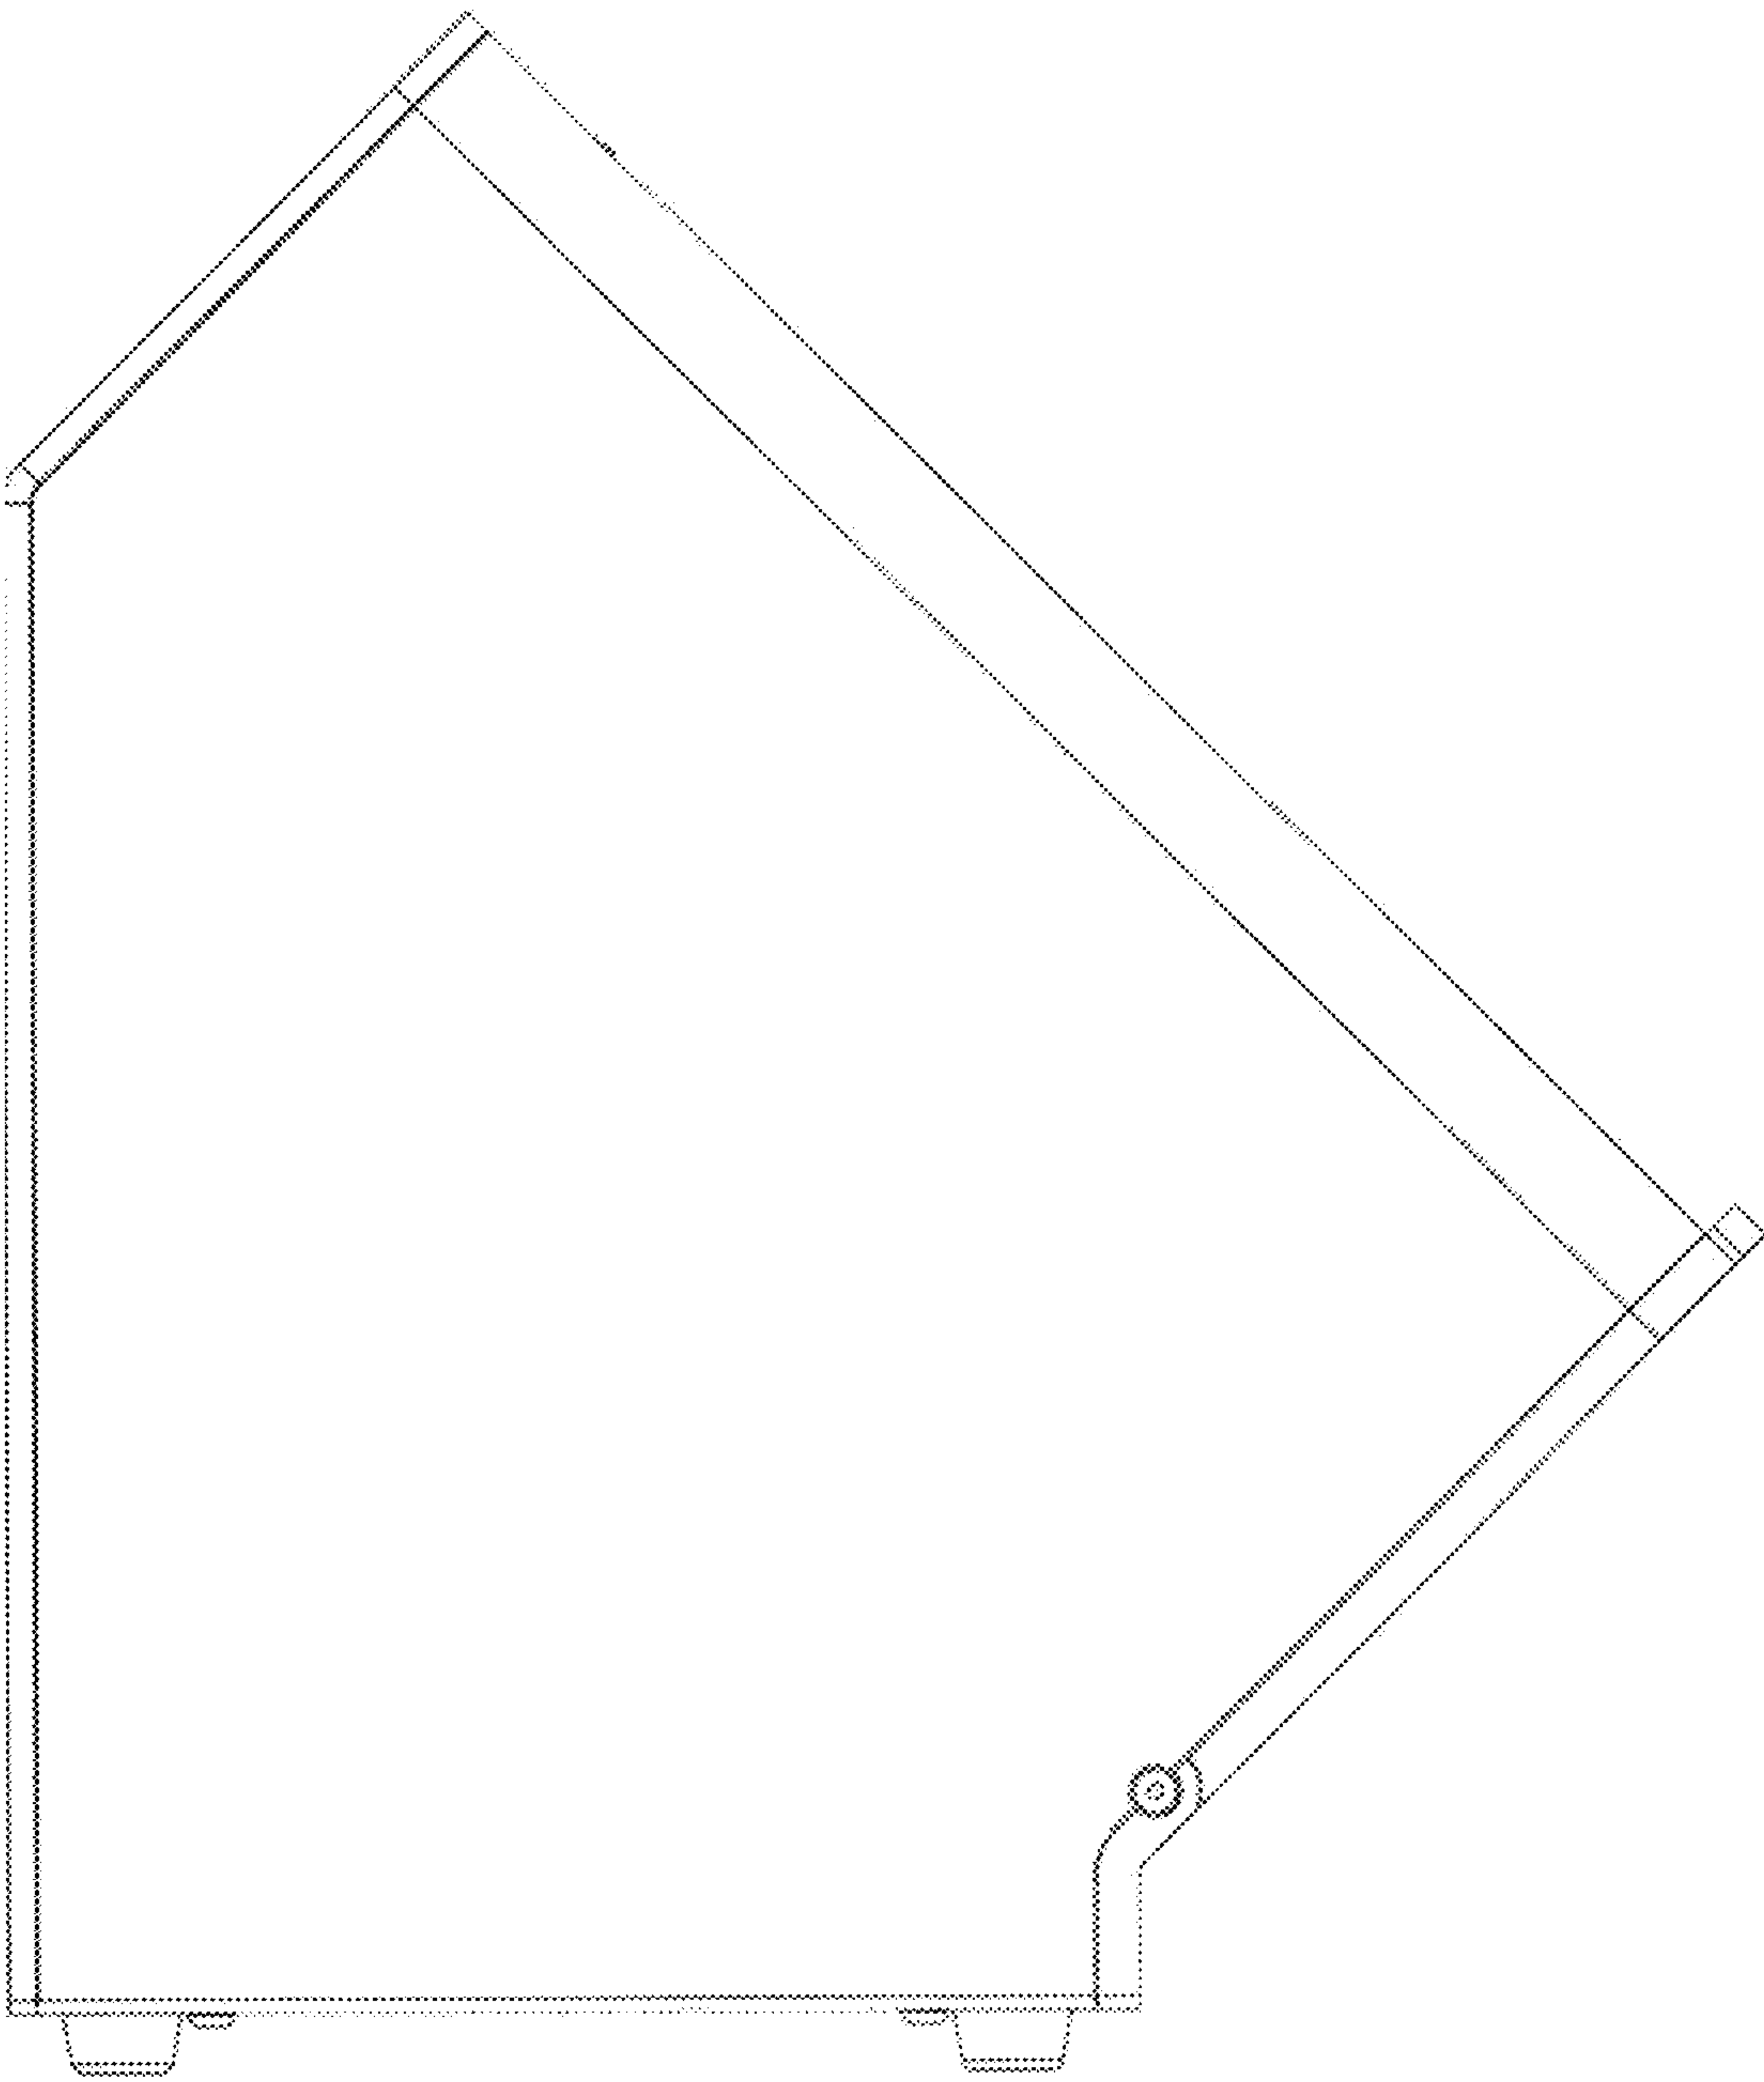


FIG. 5

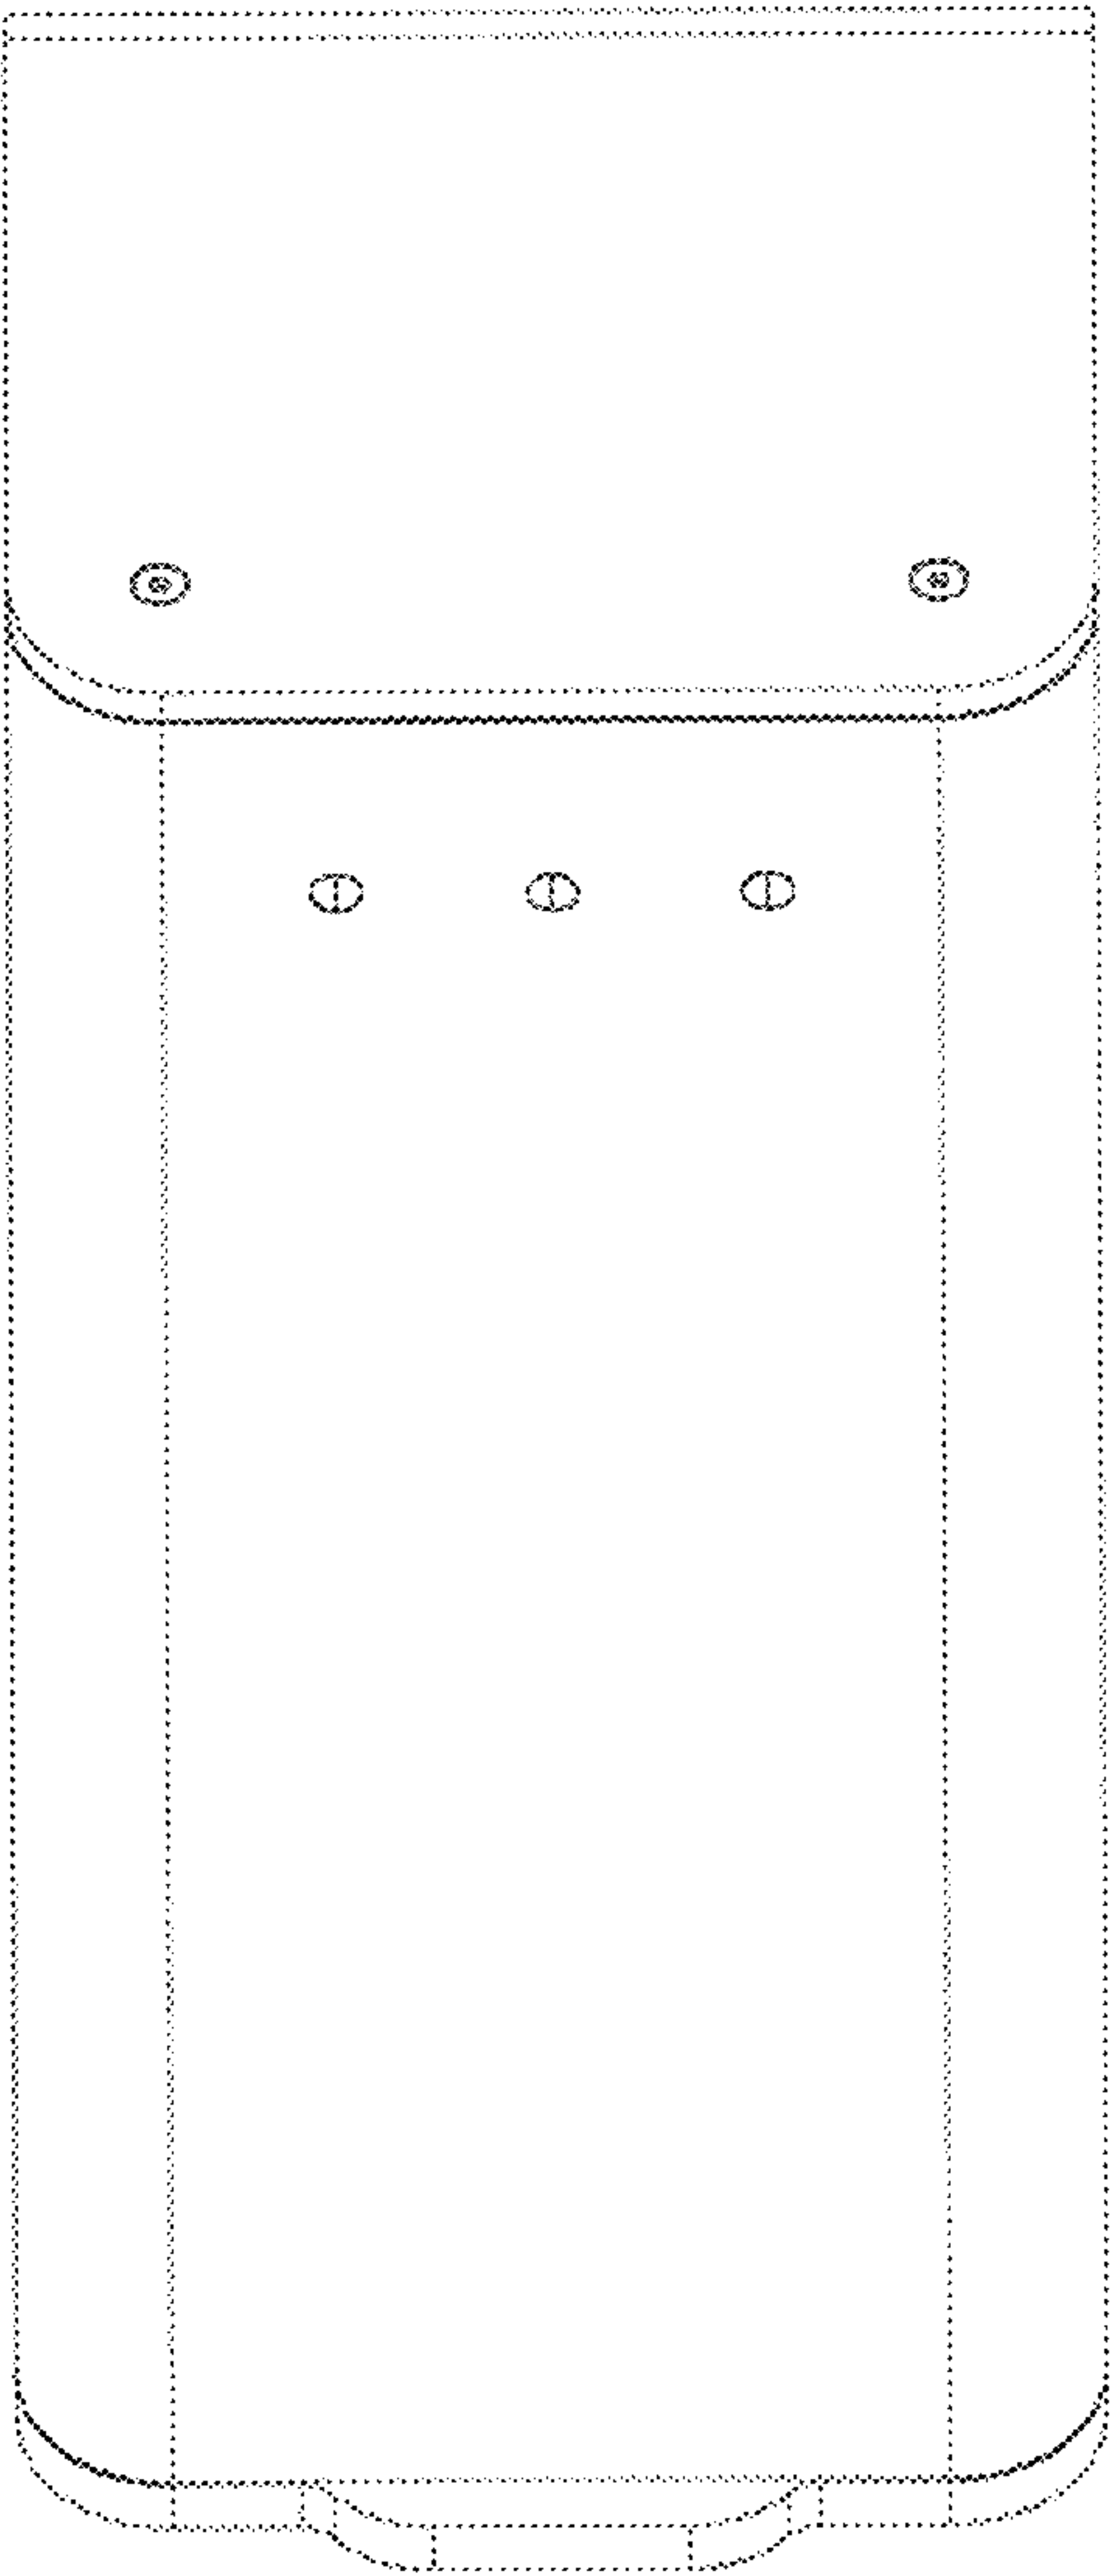


FIG. 6

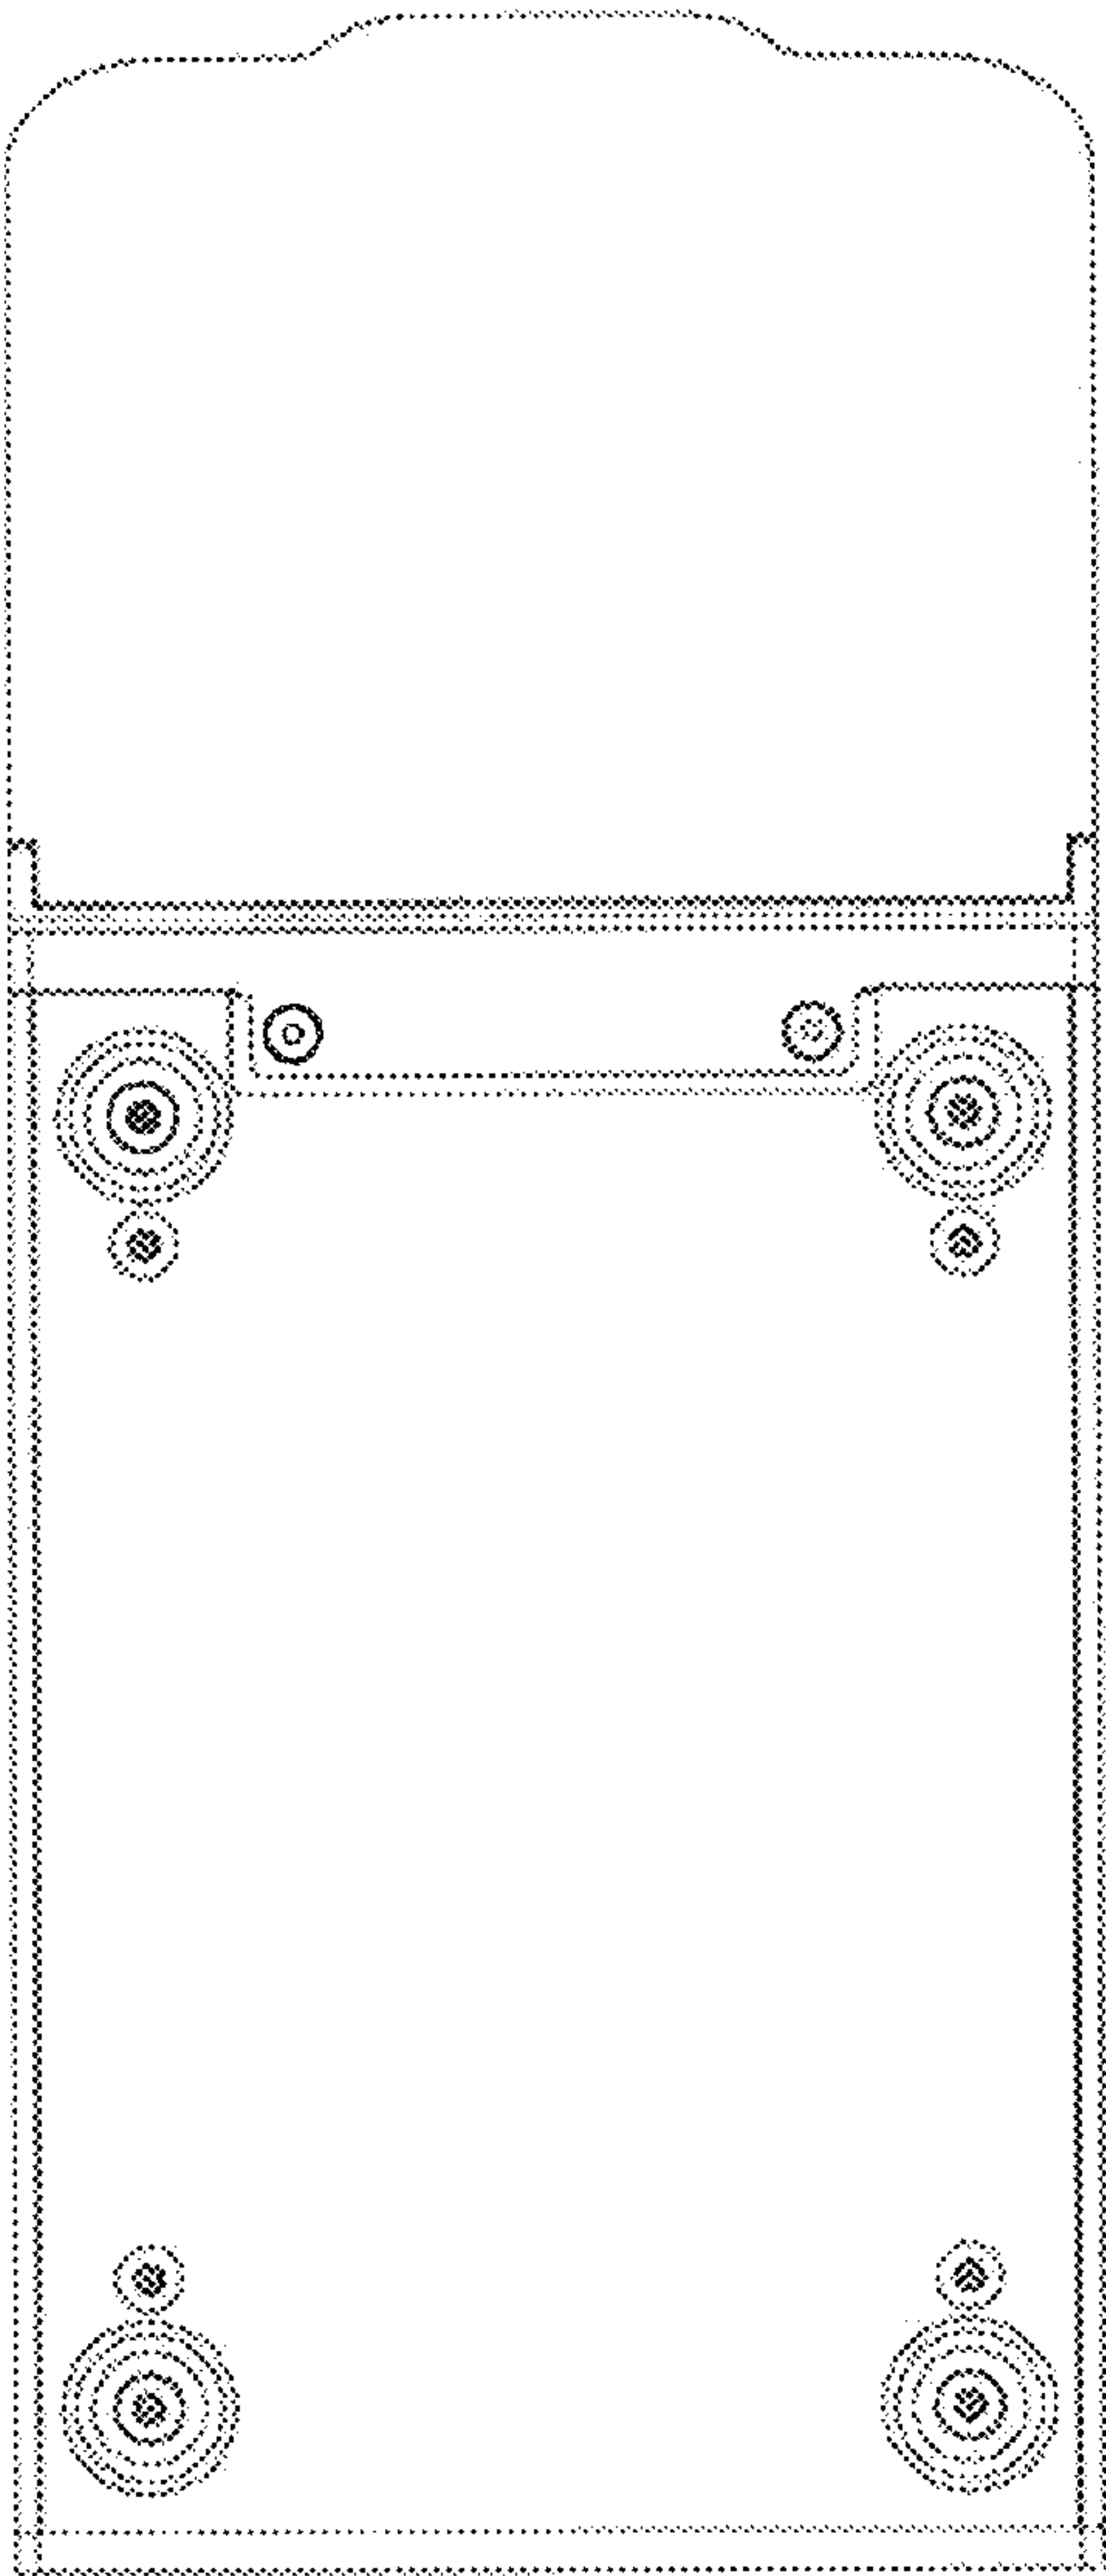


FIG. 7