

US0D1082024S

(12)

United States Design Patent

Li

(10)

Patent No.:

US D1,082,024 S

(45)

Date of Patent:

** Jul. 1, 2025

(54) COLD THERAPY SYSTEM

(71) Applicant: SHENZHEN BAOHUAYAO TECHNOLOGY CO., LTD., Guangdong (CN)

(72) Inventor: Xiong Li, Guangdong (CN)

(73) Assignee: SHENZHEN BAOHUAYAO TECHNOLOGY CO., LTD., Shenzhen (CN)

(**) Term: 15 Years

(21) Appl. No.: 29/986,035

(22) Filed: Jan. 17, 2025

(51) LOC (15) Cl. 24-01

(52) U.S. Cl. USPC D24/206

(58) Field of Classification Search USPC D24/107, 185, 200, 206–208, 209, D24/190–191, 231; D15/7, 80; D7/601, D7/603, 605, 607, 608, 629

(Continued)

(56) References Cited

U.S. PATENT DOCUMENTS

D348,733 S * 7/1994 Truelove D24/206

D590,064 S * 4/2009 Janisch D24/206

(Continued)

FOREIGN PATENT DOCUMENTS

CN 308458810 * 2/2024

CN 308676391 * 6/2024

CN 308881280 * 10/2024

OTHER PUBLICATIONS

BilnavyNew, Cold Therapy Machine, Published: Mar. 22, 2025, amazon.com, Retrieved from: https://www.amazon.com/Therapy-Machine-Portable-Surgery-Programmable/dp/B0F26D18VD/ref=sr_1_10 (Year: 2025).*

(Continued)

Primary Examiner — Jennifer L Rempfer

Assistant Examiner — Edward P Jones

(74) Attorney, Agent, or Firm — Daniel M. Cohn

(57) CLAIM

The ornamental design for a cold therapy system as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of a coolant reservoir of a cold therapy system showing my new design shown separately for ease of illustration;

FIG. 2 is another perspective view thereof;

FIG. 3 is a front elevational view thereof;

FIG. 4 is a rear elevational view thereof;

FIG. 5 is a left side elevational view thereof;

FIG. 6 is a right side elevational view thereof;

FIG. 7 is a top plan view thereof;

FIG. 8 is a bottom plan view thereof;

FIG. 9 is a perspective view of a pump unit of the cold therapy system shown separately for ease of illustration;

FIG. 10 is another perspective view thereof;

FIG. 11 is a front elevational view thereof;

FIG. 12 is a rear elevational view thereof;

FIG. 13 is a left side elevational view thereof;

FIG. 14 is a right side elevational view thereof;


FIG. 15 is a top plan view thereof;

FIG. 16 is a bottom plan view thereof;

FIG. 17 is a perspective view of the cold therapy system where the cold therapy system is in a configuration of use; and,

FIG. 18 is an enlarged view of portion 18 shown in FIG. 10. The dash-dash broken lines in the drawings depict portions of the cold therapy system that form no part of the claimed design. the dot-dash broken lines in FIGS. 10 and 18 represent boundaries of the enlarged portions and form no part of the claimed design. The cold therapy system is shown with a symbolic break in its length and the appearance of any portion of the cold therapy system between the break lines form no part of the claimed design.

1 Claim, 18 Drawing Sheets

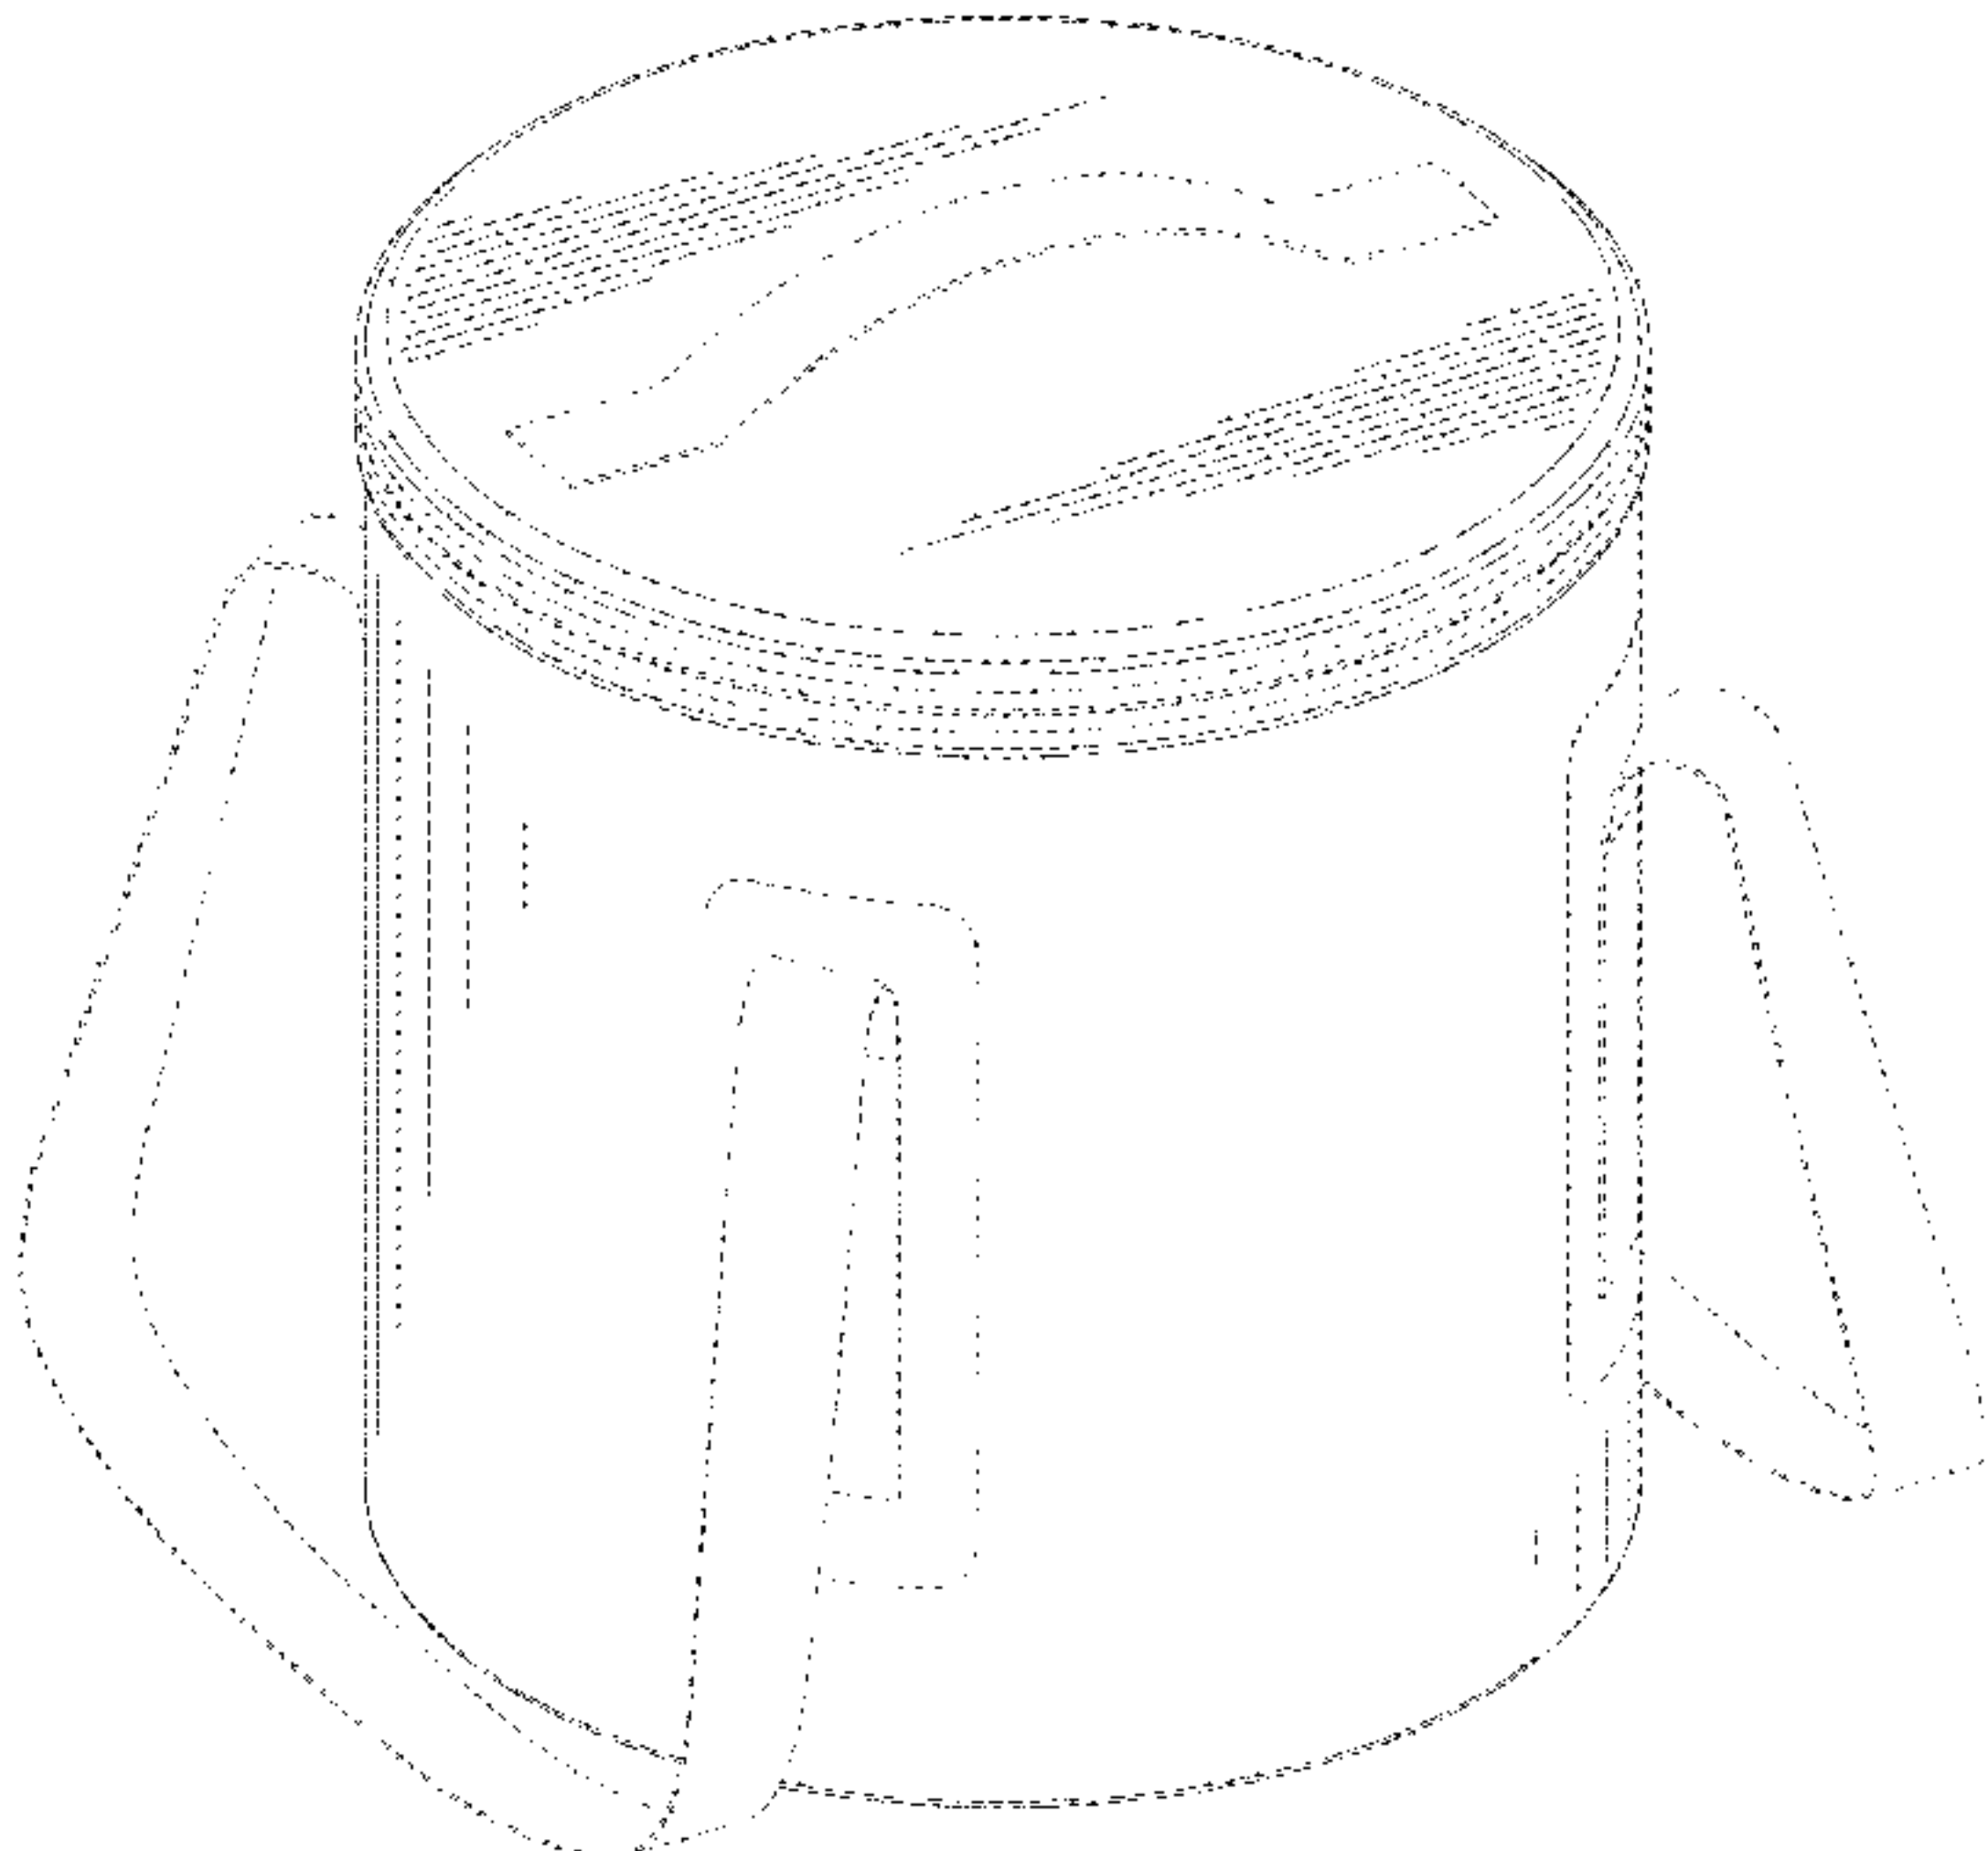

(58) **Field of Classification Search**
CPC A61F 7/00; A61F 7/10; A61F 7/02; A61F 7/08; A61F 7/0097; A61H 2201/02
See application file for complete search history.

(56) **References Cited**
U.S. PATENT DOCUMENTS

D620,763	S	*	8/2010	Meehan		D7/605
D829,244	S	*	9/2018	Sullivan		D15/79
D854,698	S		7/2019	Sivan		
D870,301	S		12/2019	Sivan		
D875,394	S	*	2/2020	Komatick		D6/601
D935,027	S	*	11/2021	Larrow		D24/167
D942,814	S	*	2/2022	Yao		D3/202
D963,872	S	*	9/2022	Zender		D24/206
D978,362	S	*	2/2023	Chen		D24/204
12,213,910	B1	*	2/2025	Dai		A61F 7/0085
D1,065,560	S	*	3/2025	Jiang		D24/185
2004/0068309	A1	*	4/2004	Edelman		A61F 7/02 607/104
2020/0352779	A1	*	11/2020	Graessle		A61F 7/02

OTHER PUBLICATIONS

Celpack, Portable Ice Therapy Machine for Post-Operative Recovery, Published: Feb. 25, 2025, amazon.com, Retrieved from: <https://www.amazon.com/Portable-Post-Operative-Recovery-Injuries-Swelling/dp/B0DYDQ64MZ> (Year: 2025).*

Cryoforce, Cryoforce Cold Therapy Machine, Published: Jul. 4, 2024, amazonca, Retrived from: <https://www.amazon.ca/CRYOFORCE-Programable-replacement-Post-Surgery-Universal/dp/B0D7V8LXFD> (Year: 2024).*

Kinryopy, Cold Therapy Machine with Programmable Timer, Portable Ice Machine for Knee After Surgery, Published: Jan. 11, 2025, amazon.com, Retrieved from: <https://www.amazon.com/Programmable-Portable-Replacement-Cryotherapy-Compression/dp/B0DSSMW086?th=1> (Year: 2025).*

“Cold Therapy Machine, Ice Machine for Knee Care After-Surgery, Knee Replacement Recovery Equipment Aids Pack, Cryotherapy System w/Compression Wrap Pad for Shoulder, Ankle, Foot, ACL Relief”, Retrieved Jan. 17, 2025. Retrieved from Internet, <https://www.amazon.com/dp/B0DHS35863>.

* cited by examiner

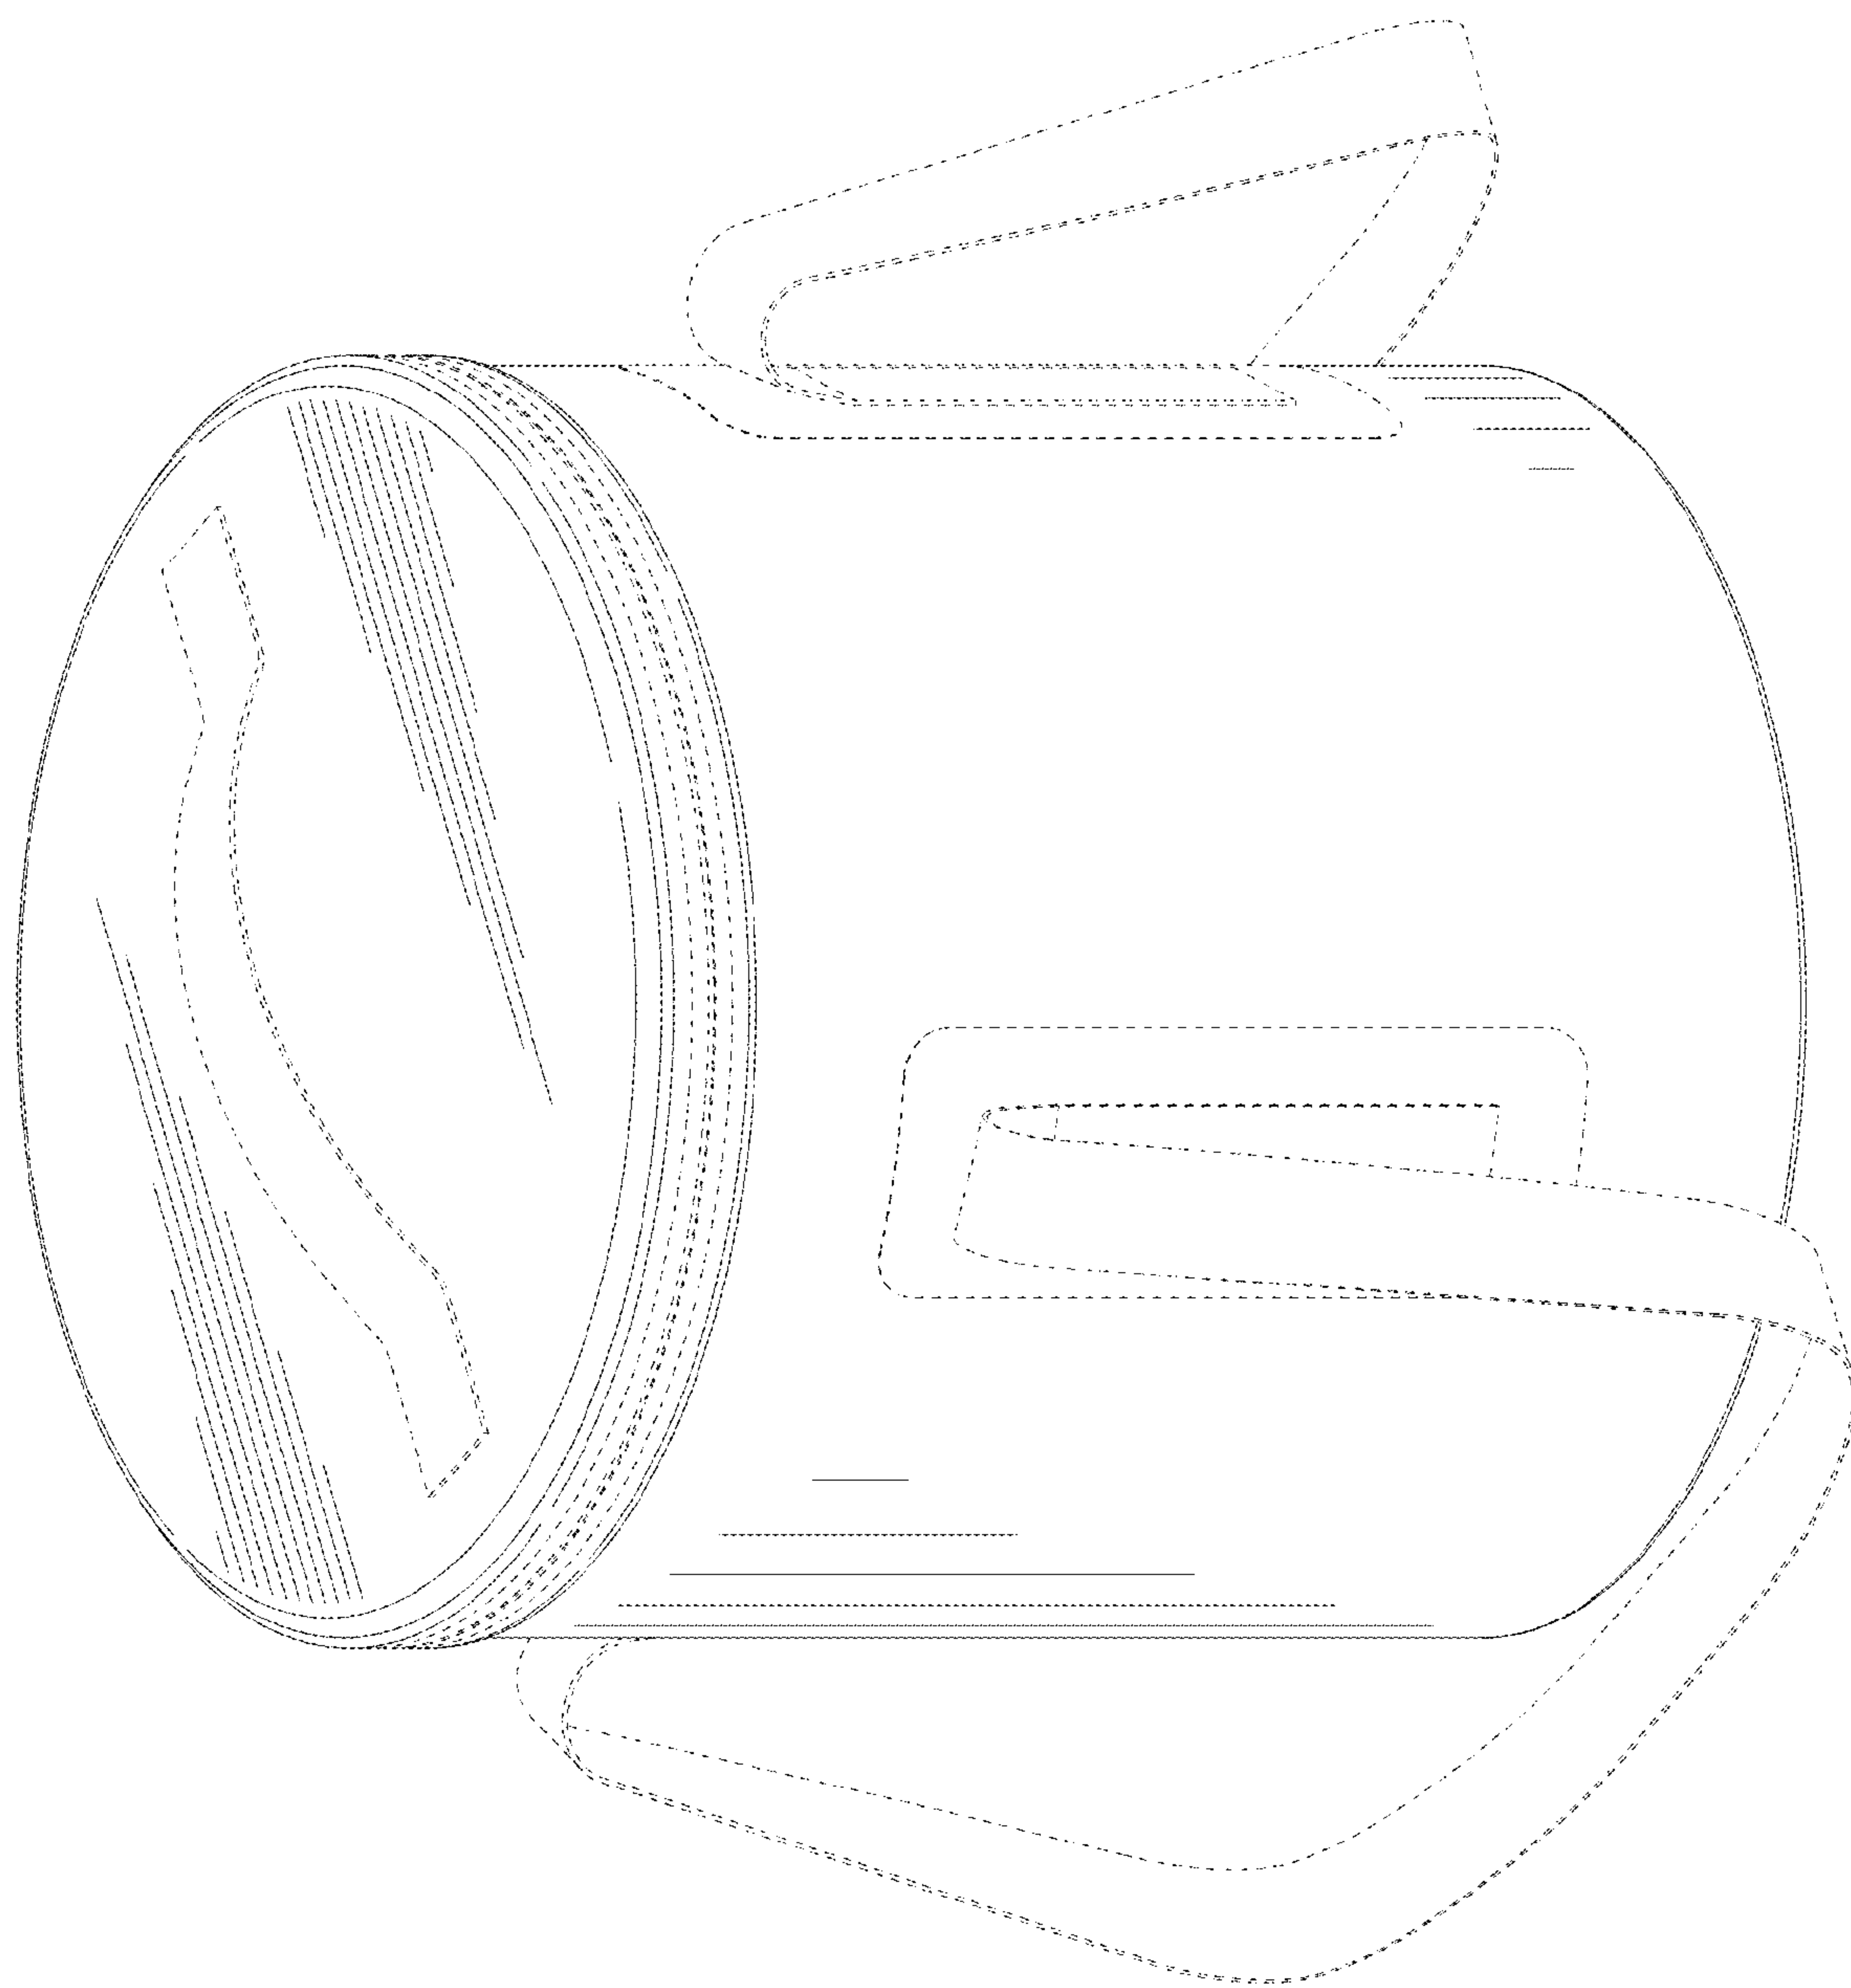


FIG. 1

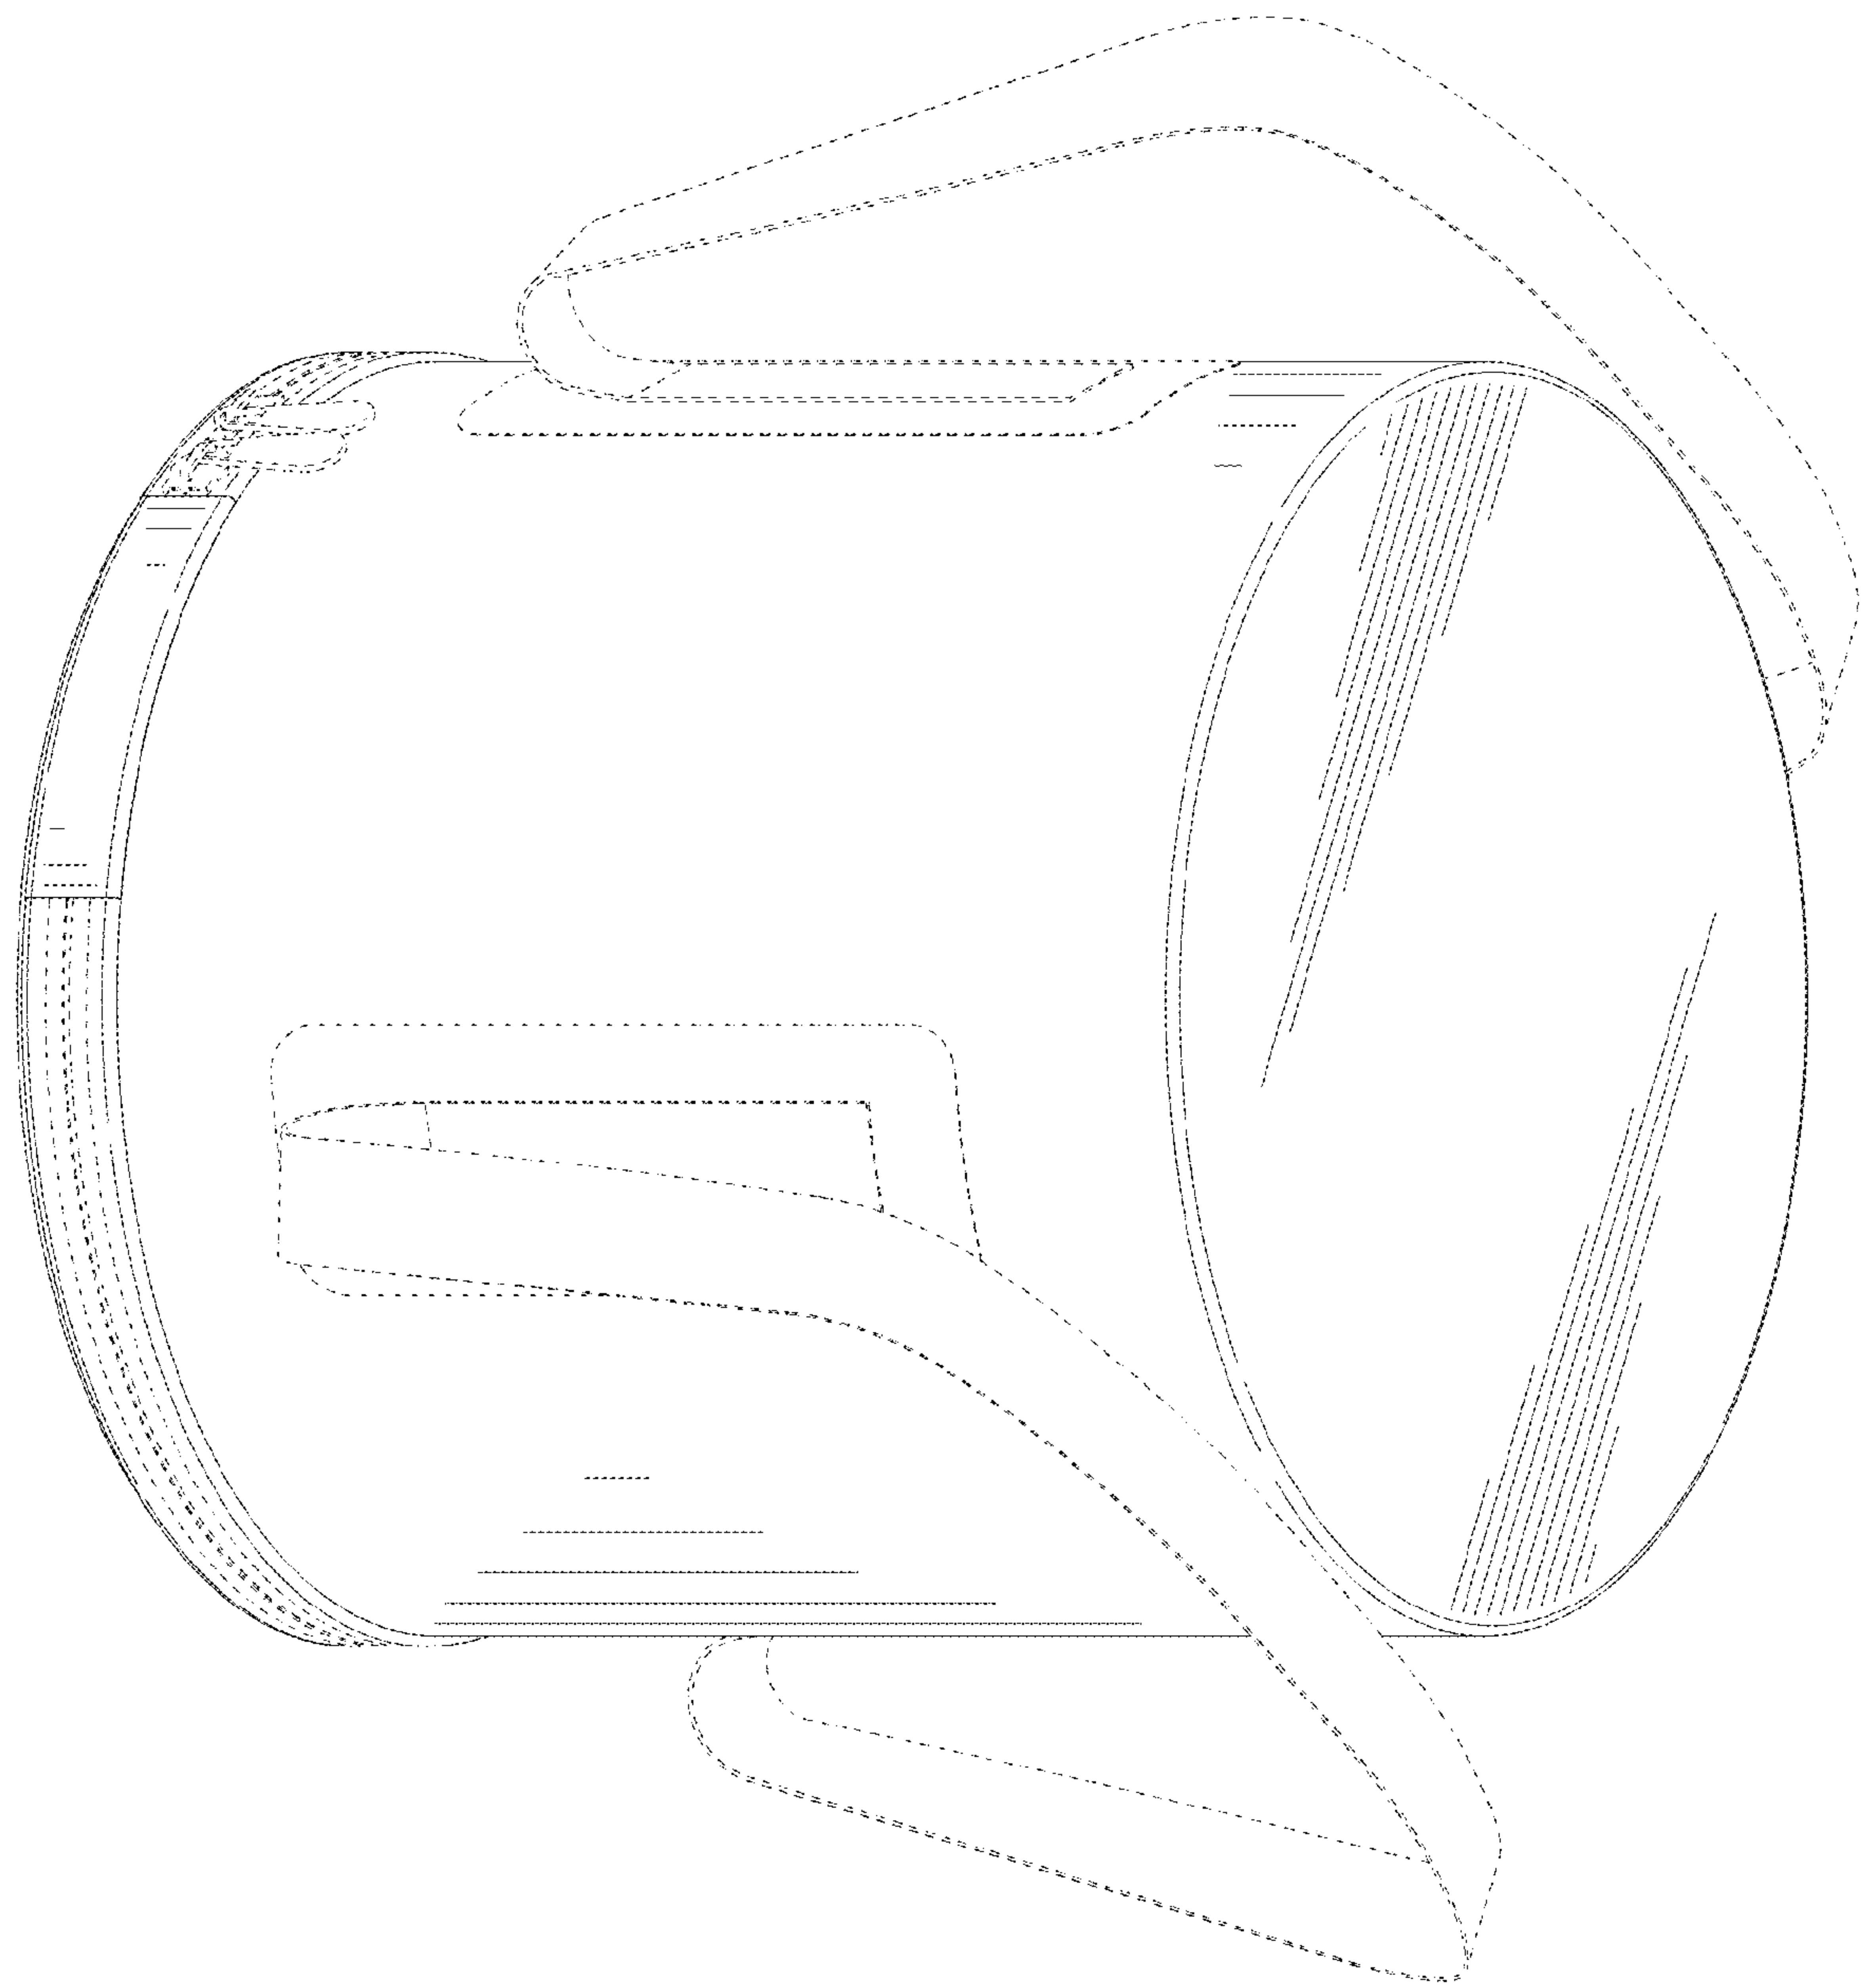


FIG. 2

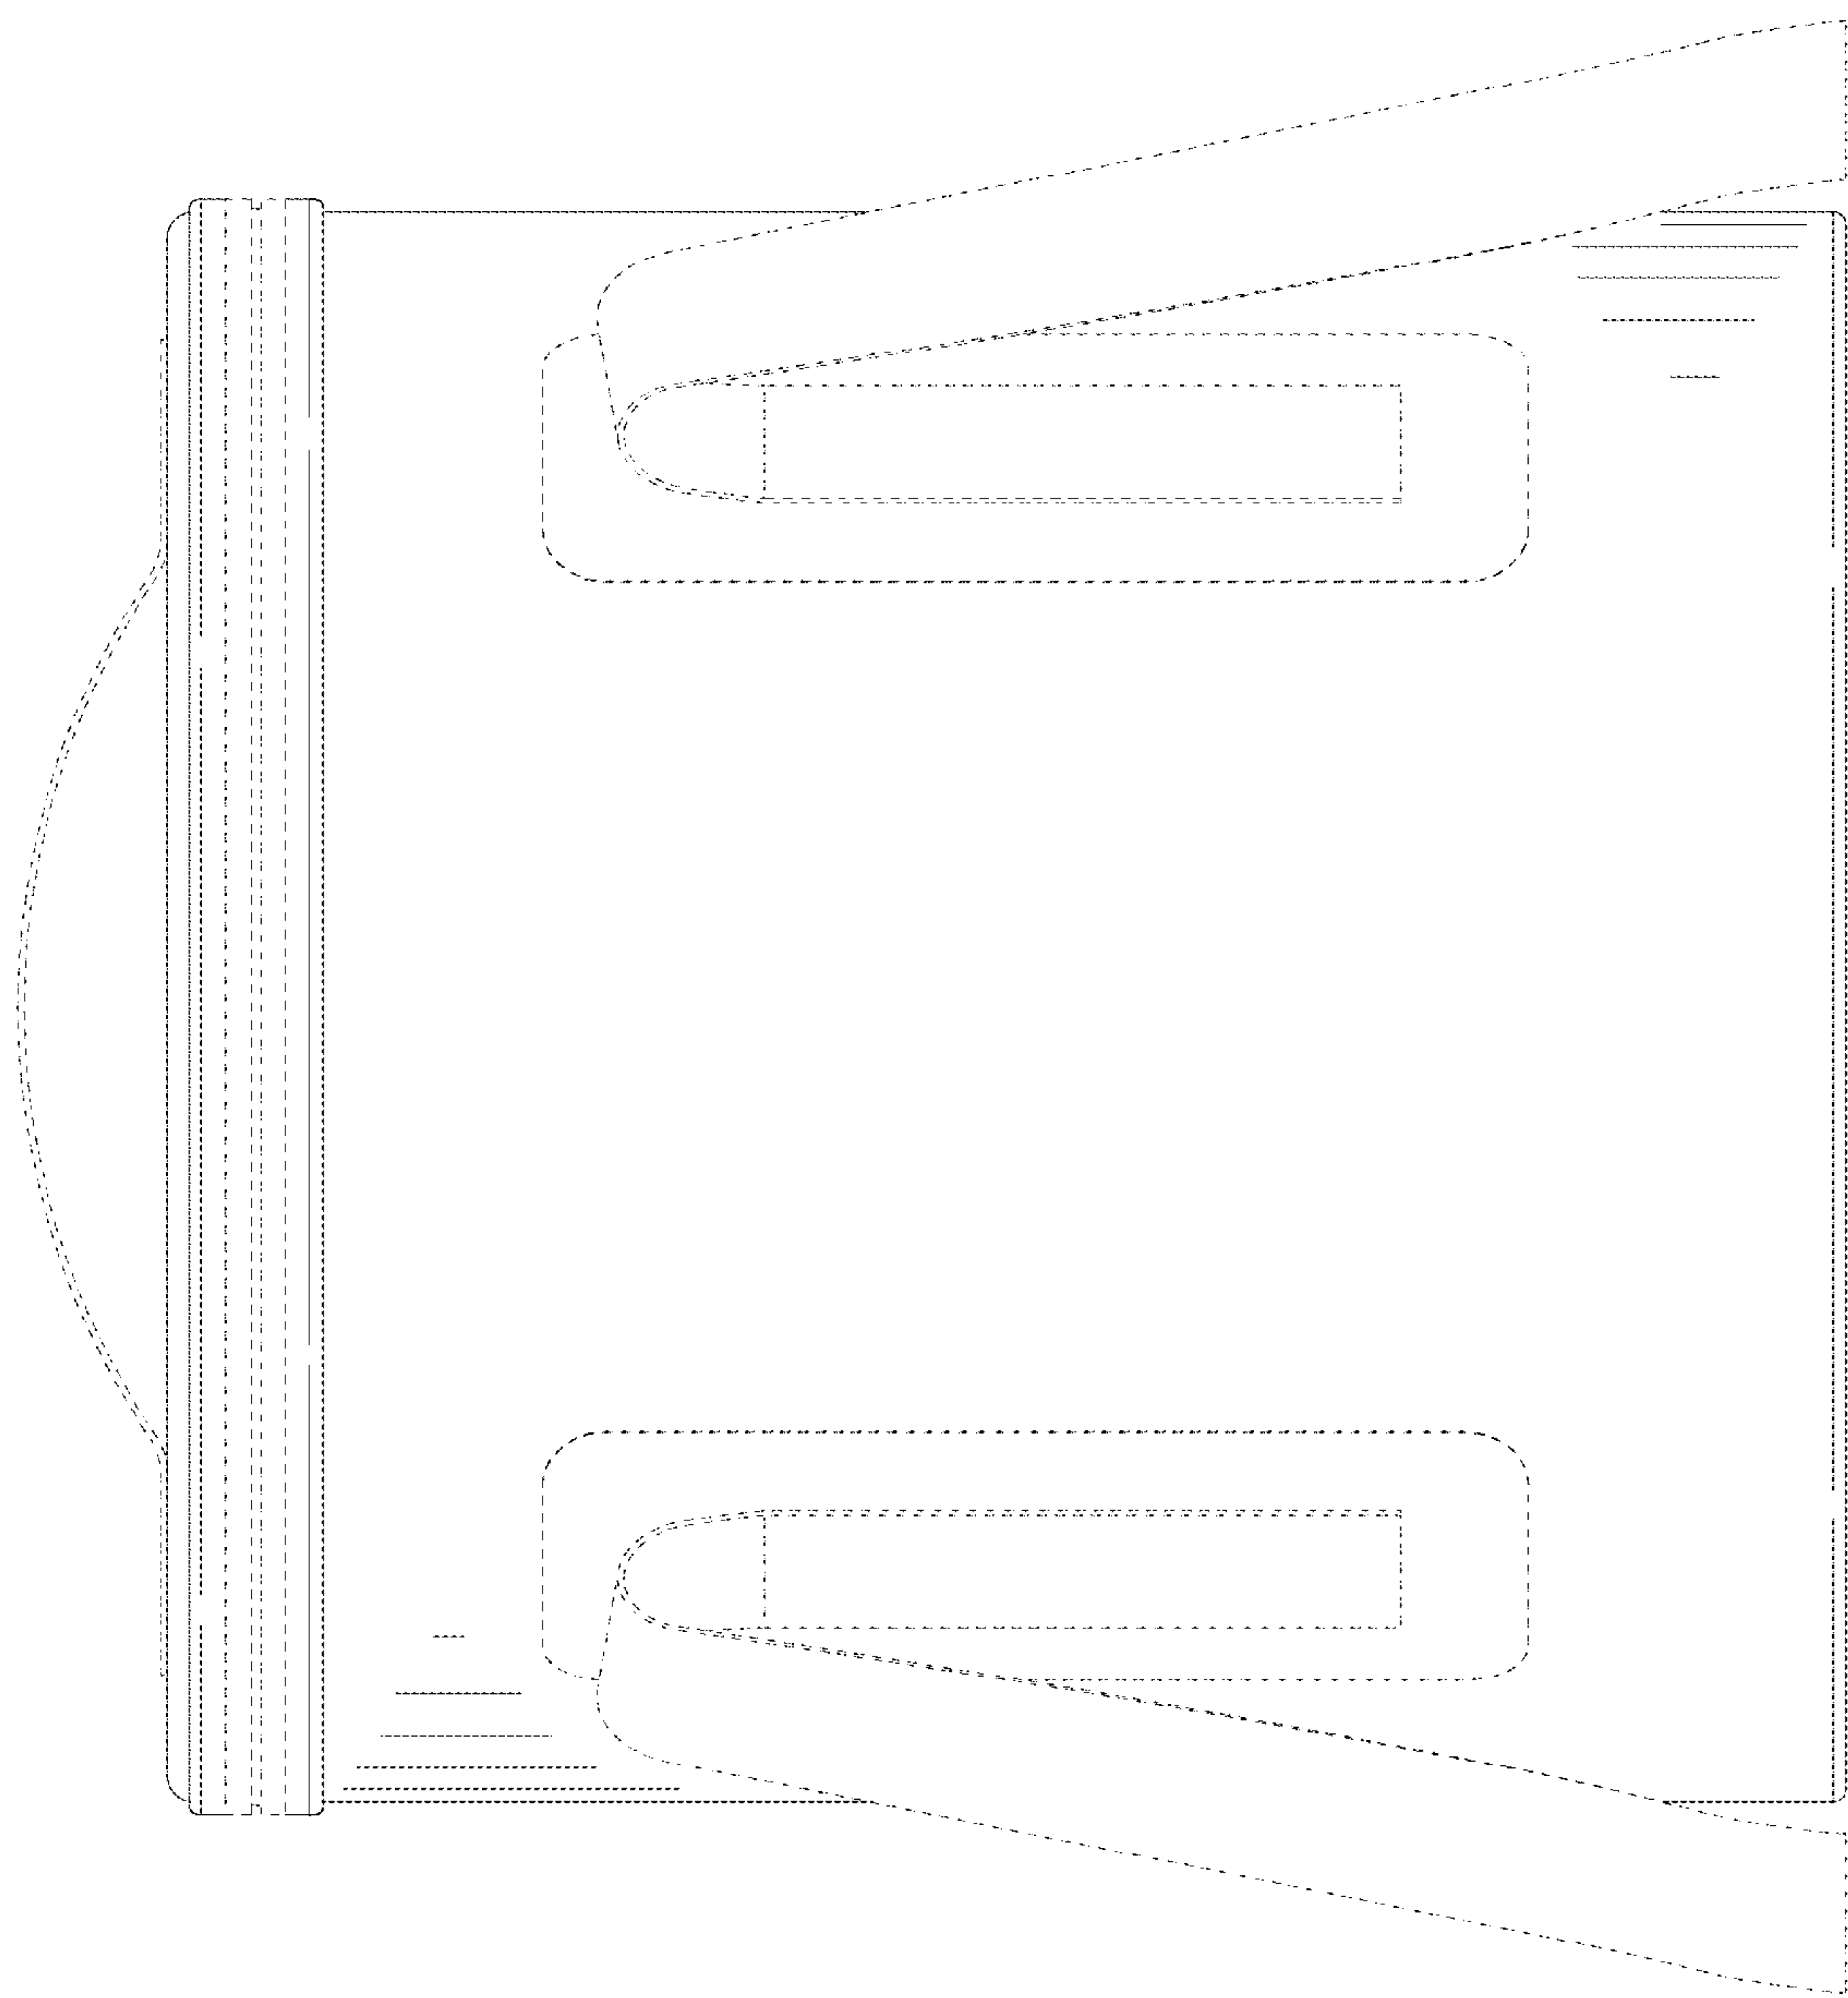


FIG. 3

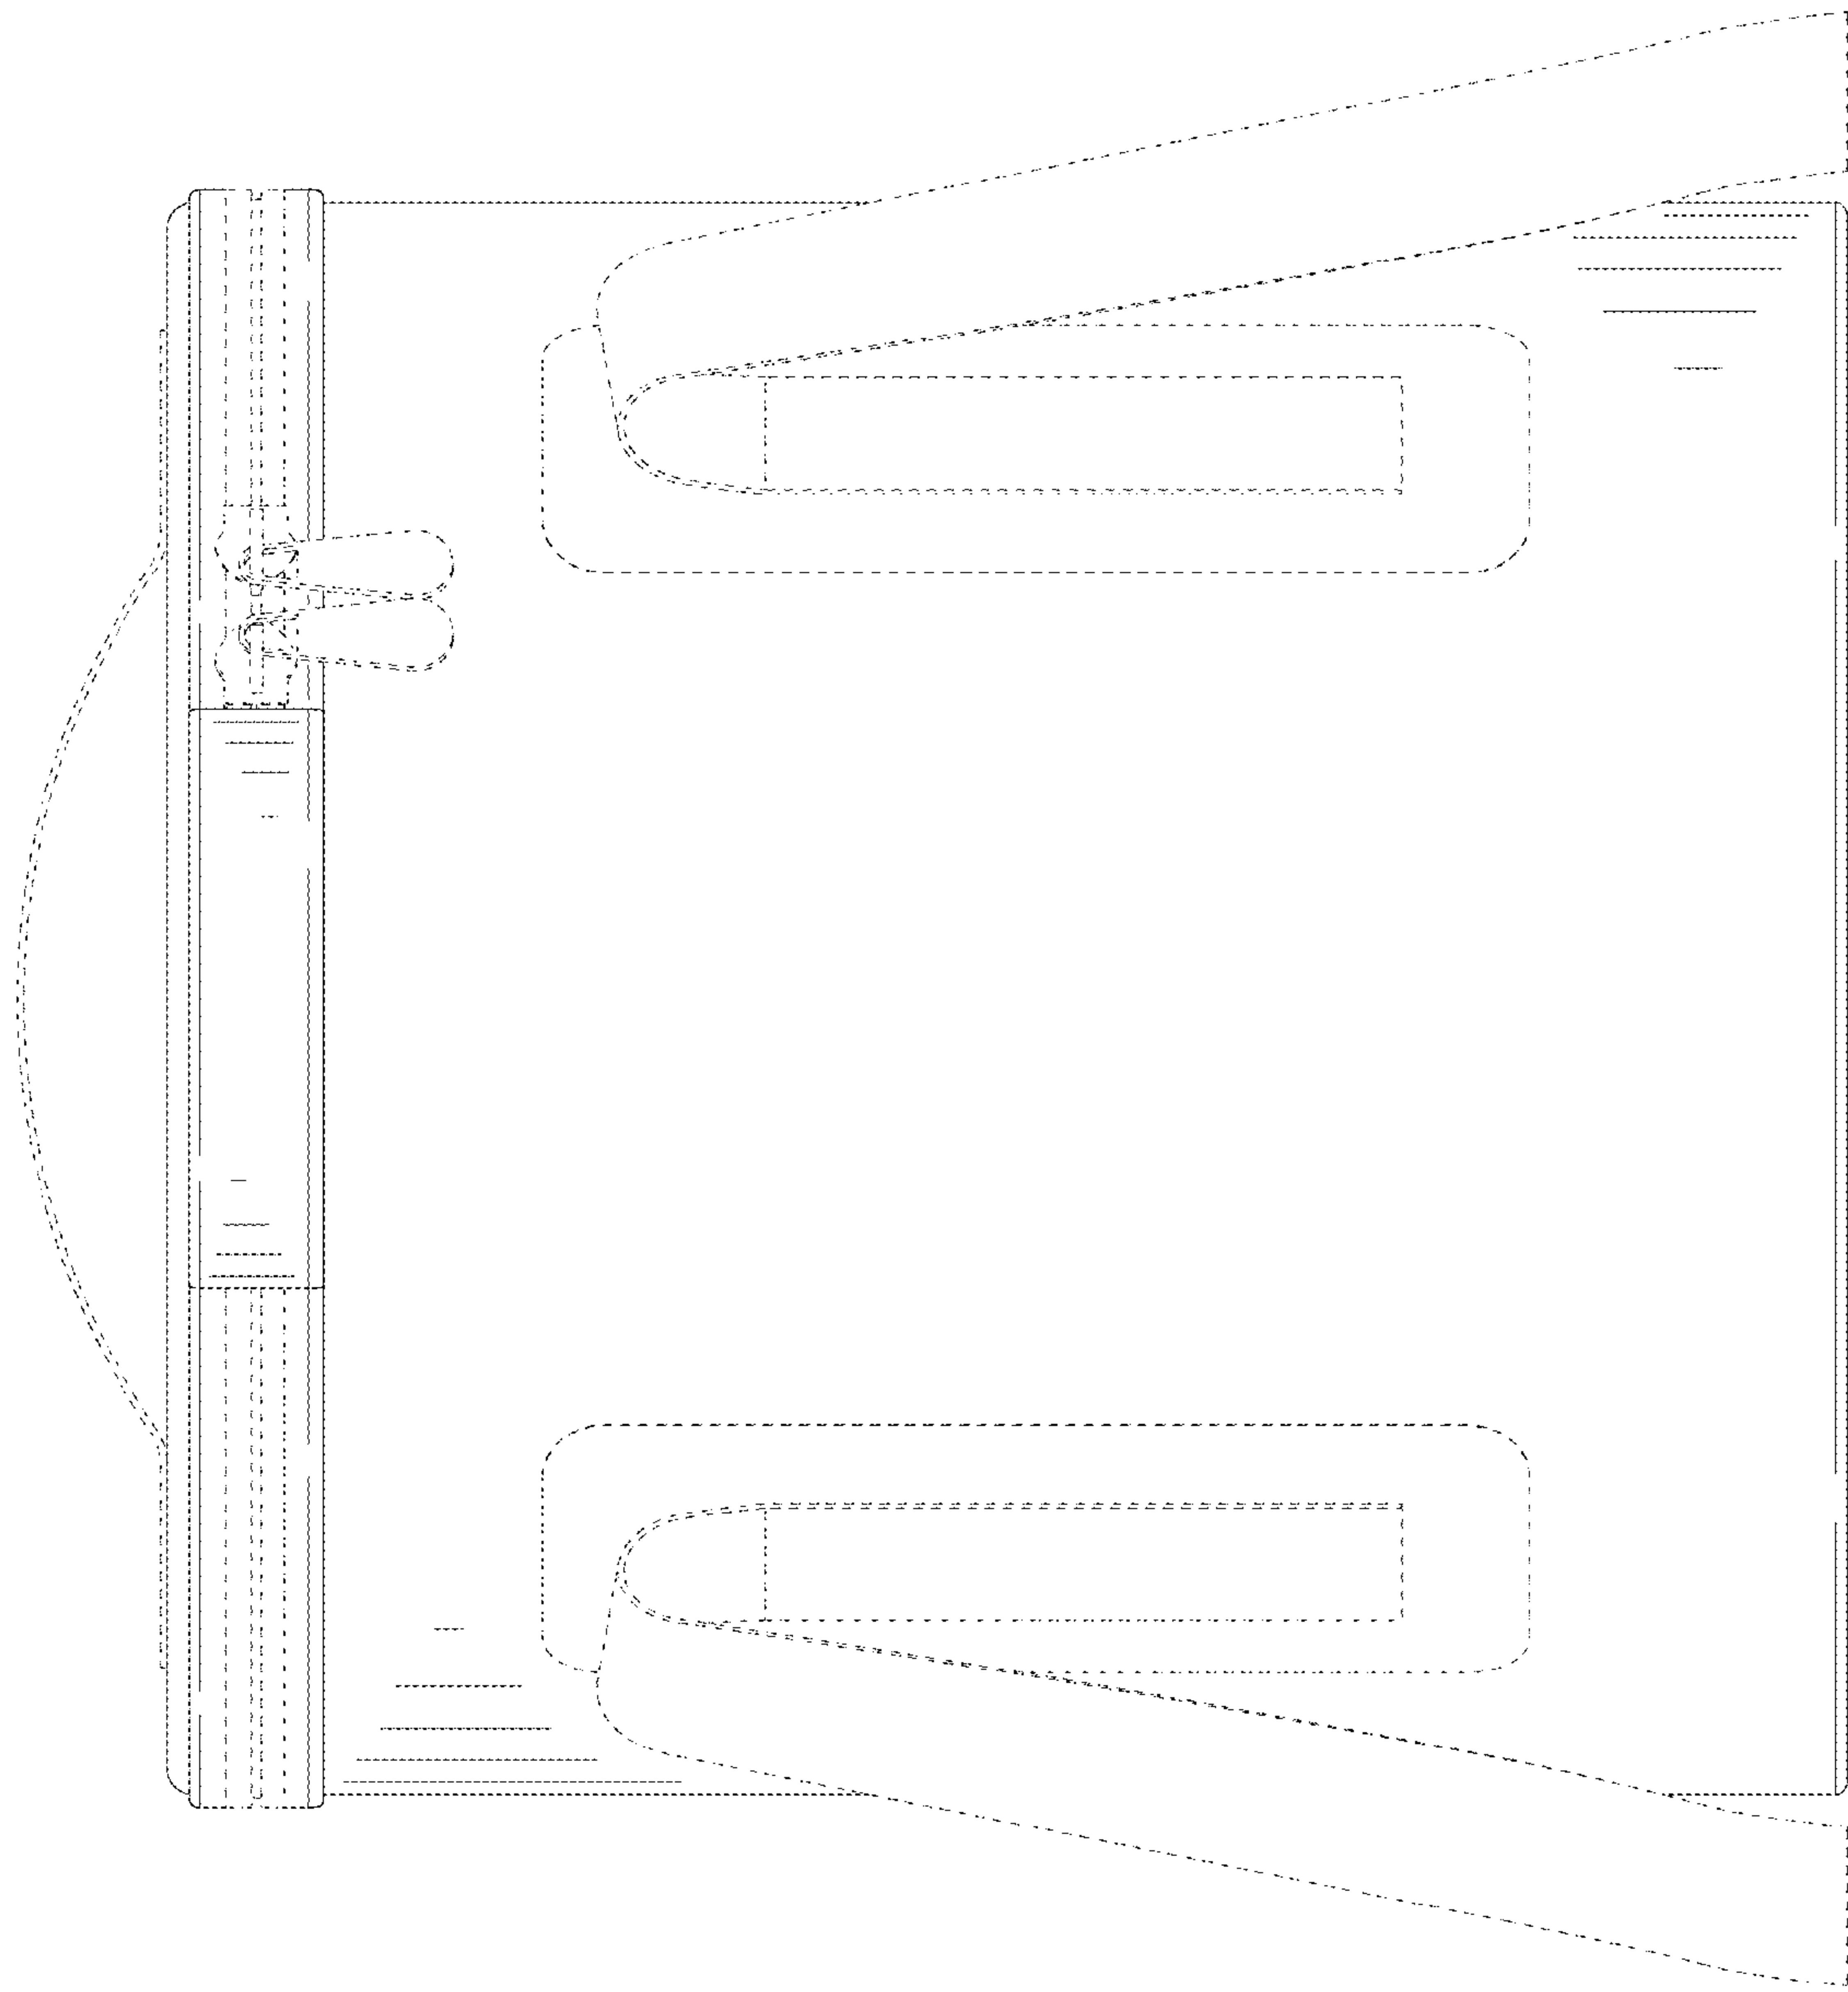


FIG. 4

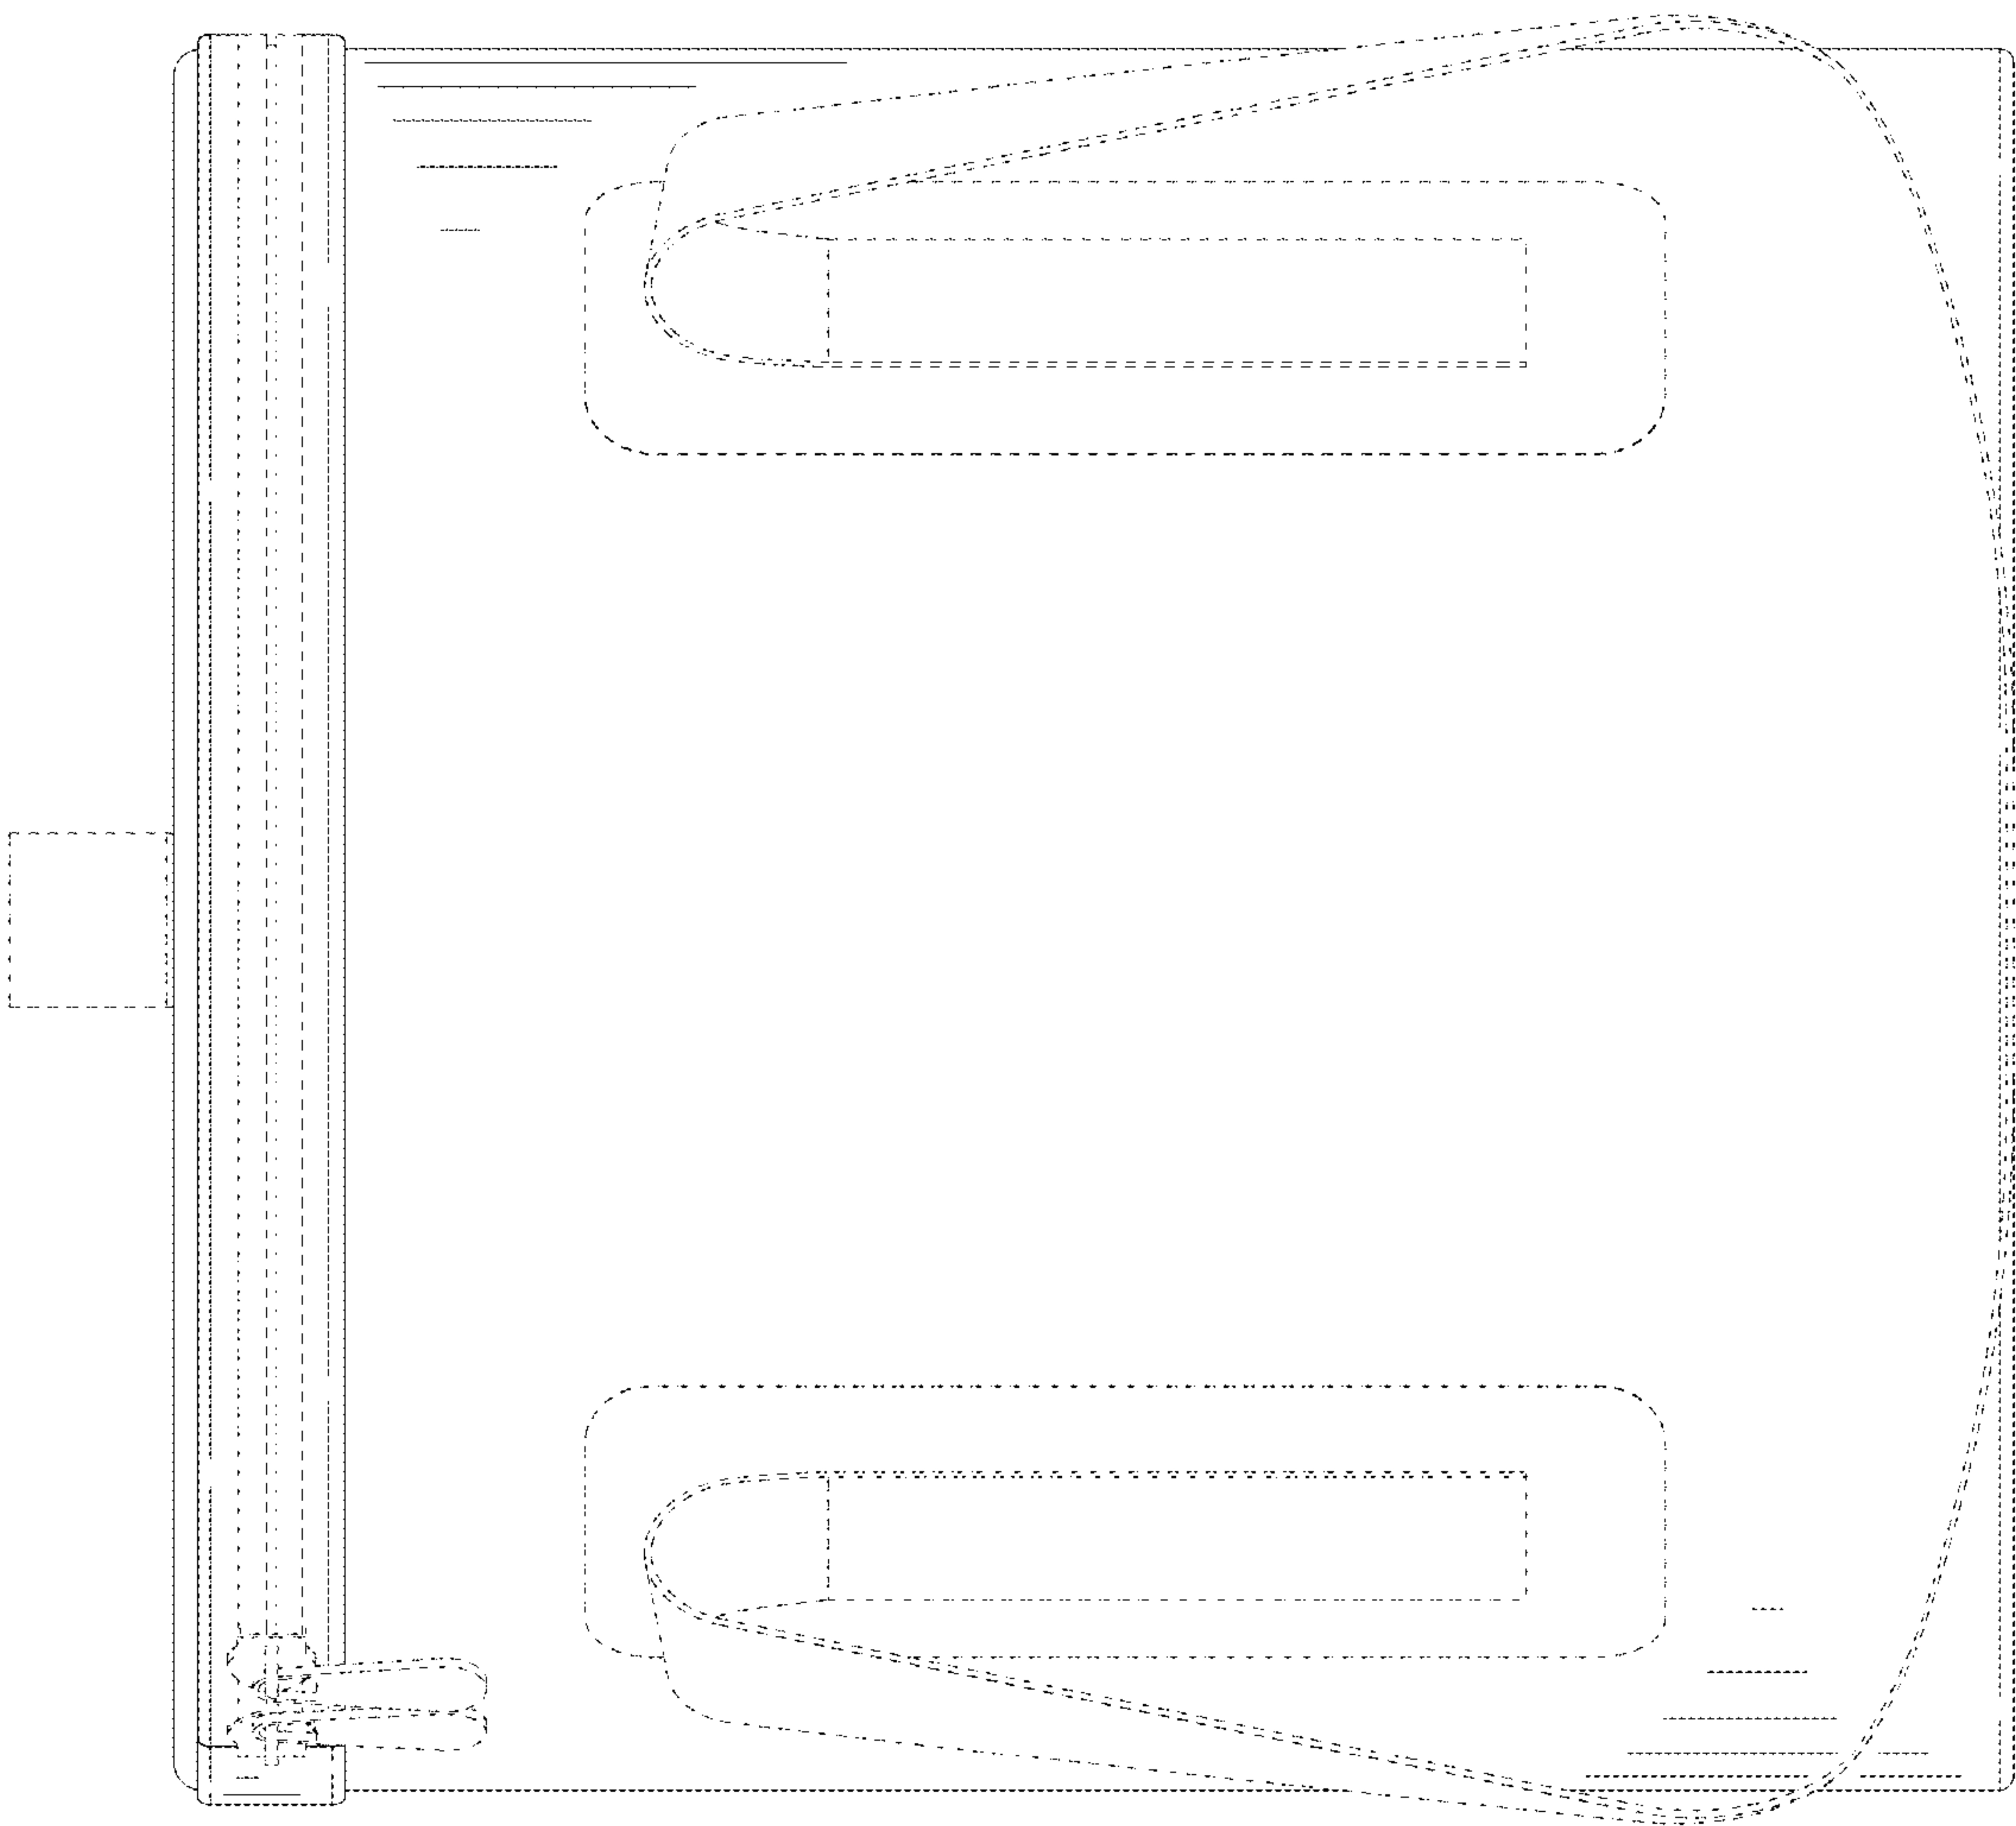


FIG. 5

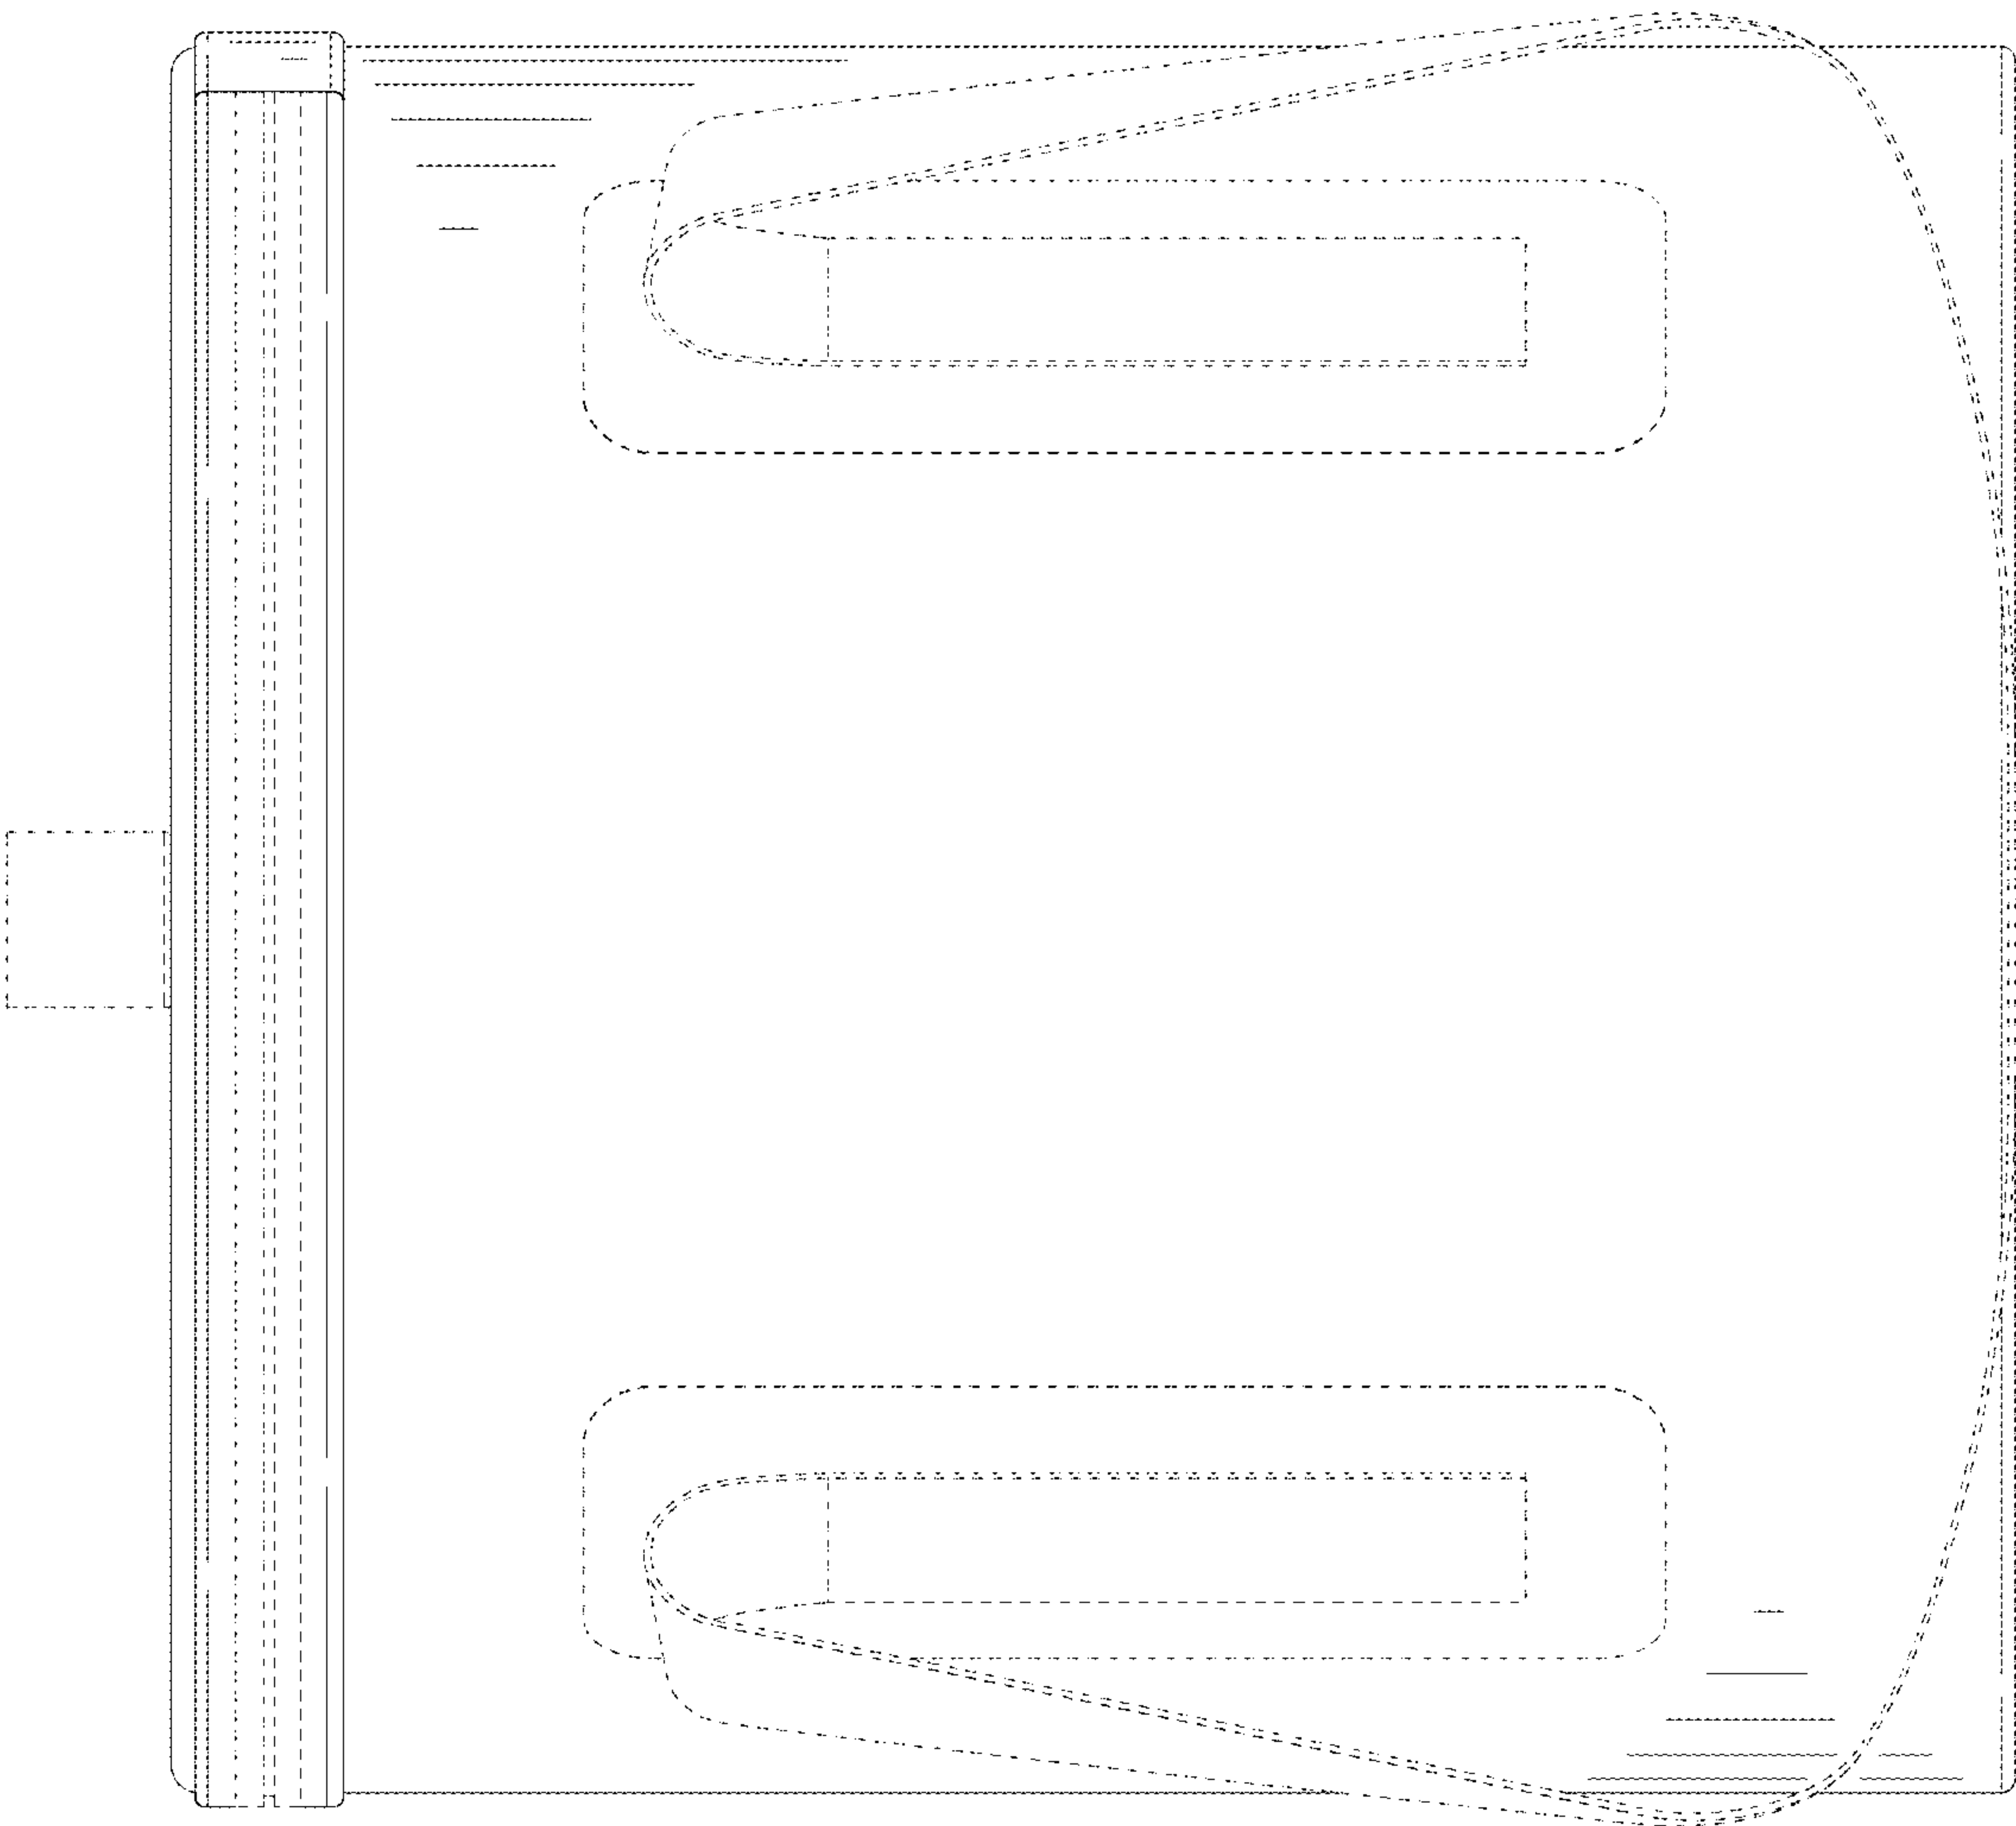


FIG. 6

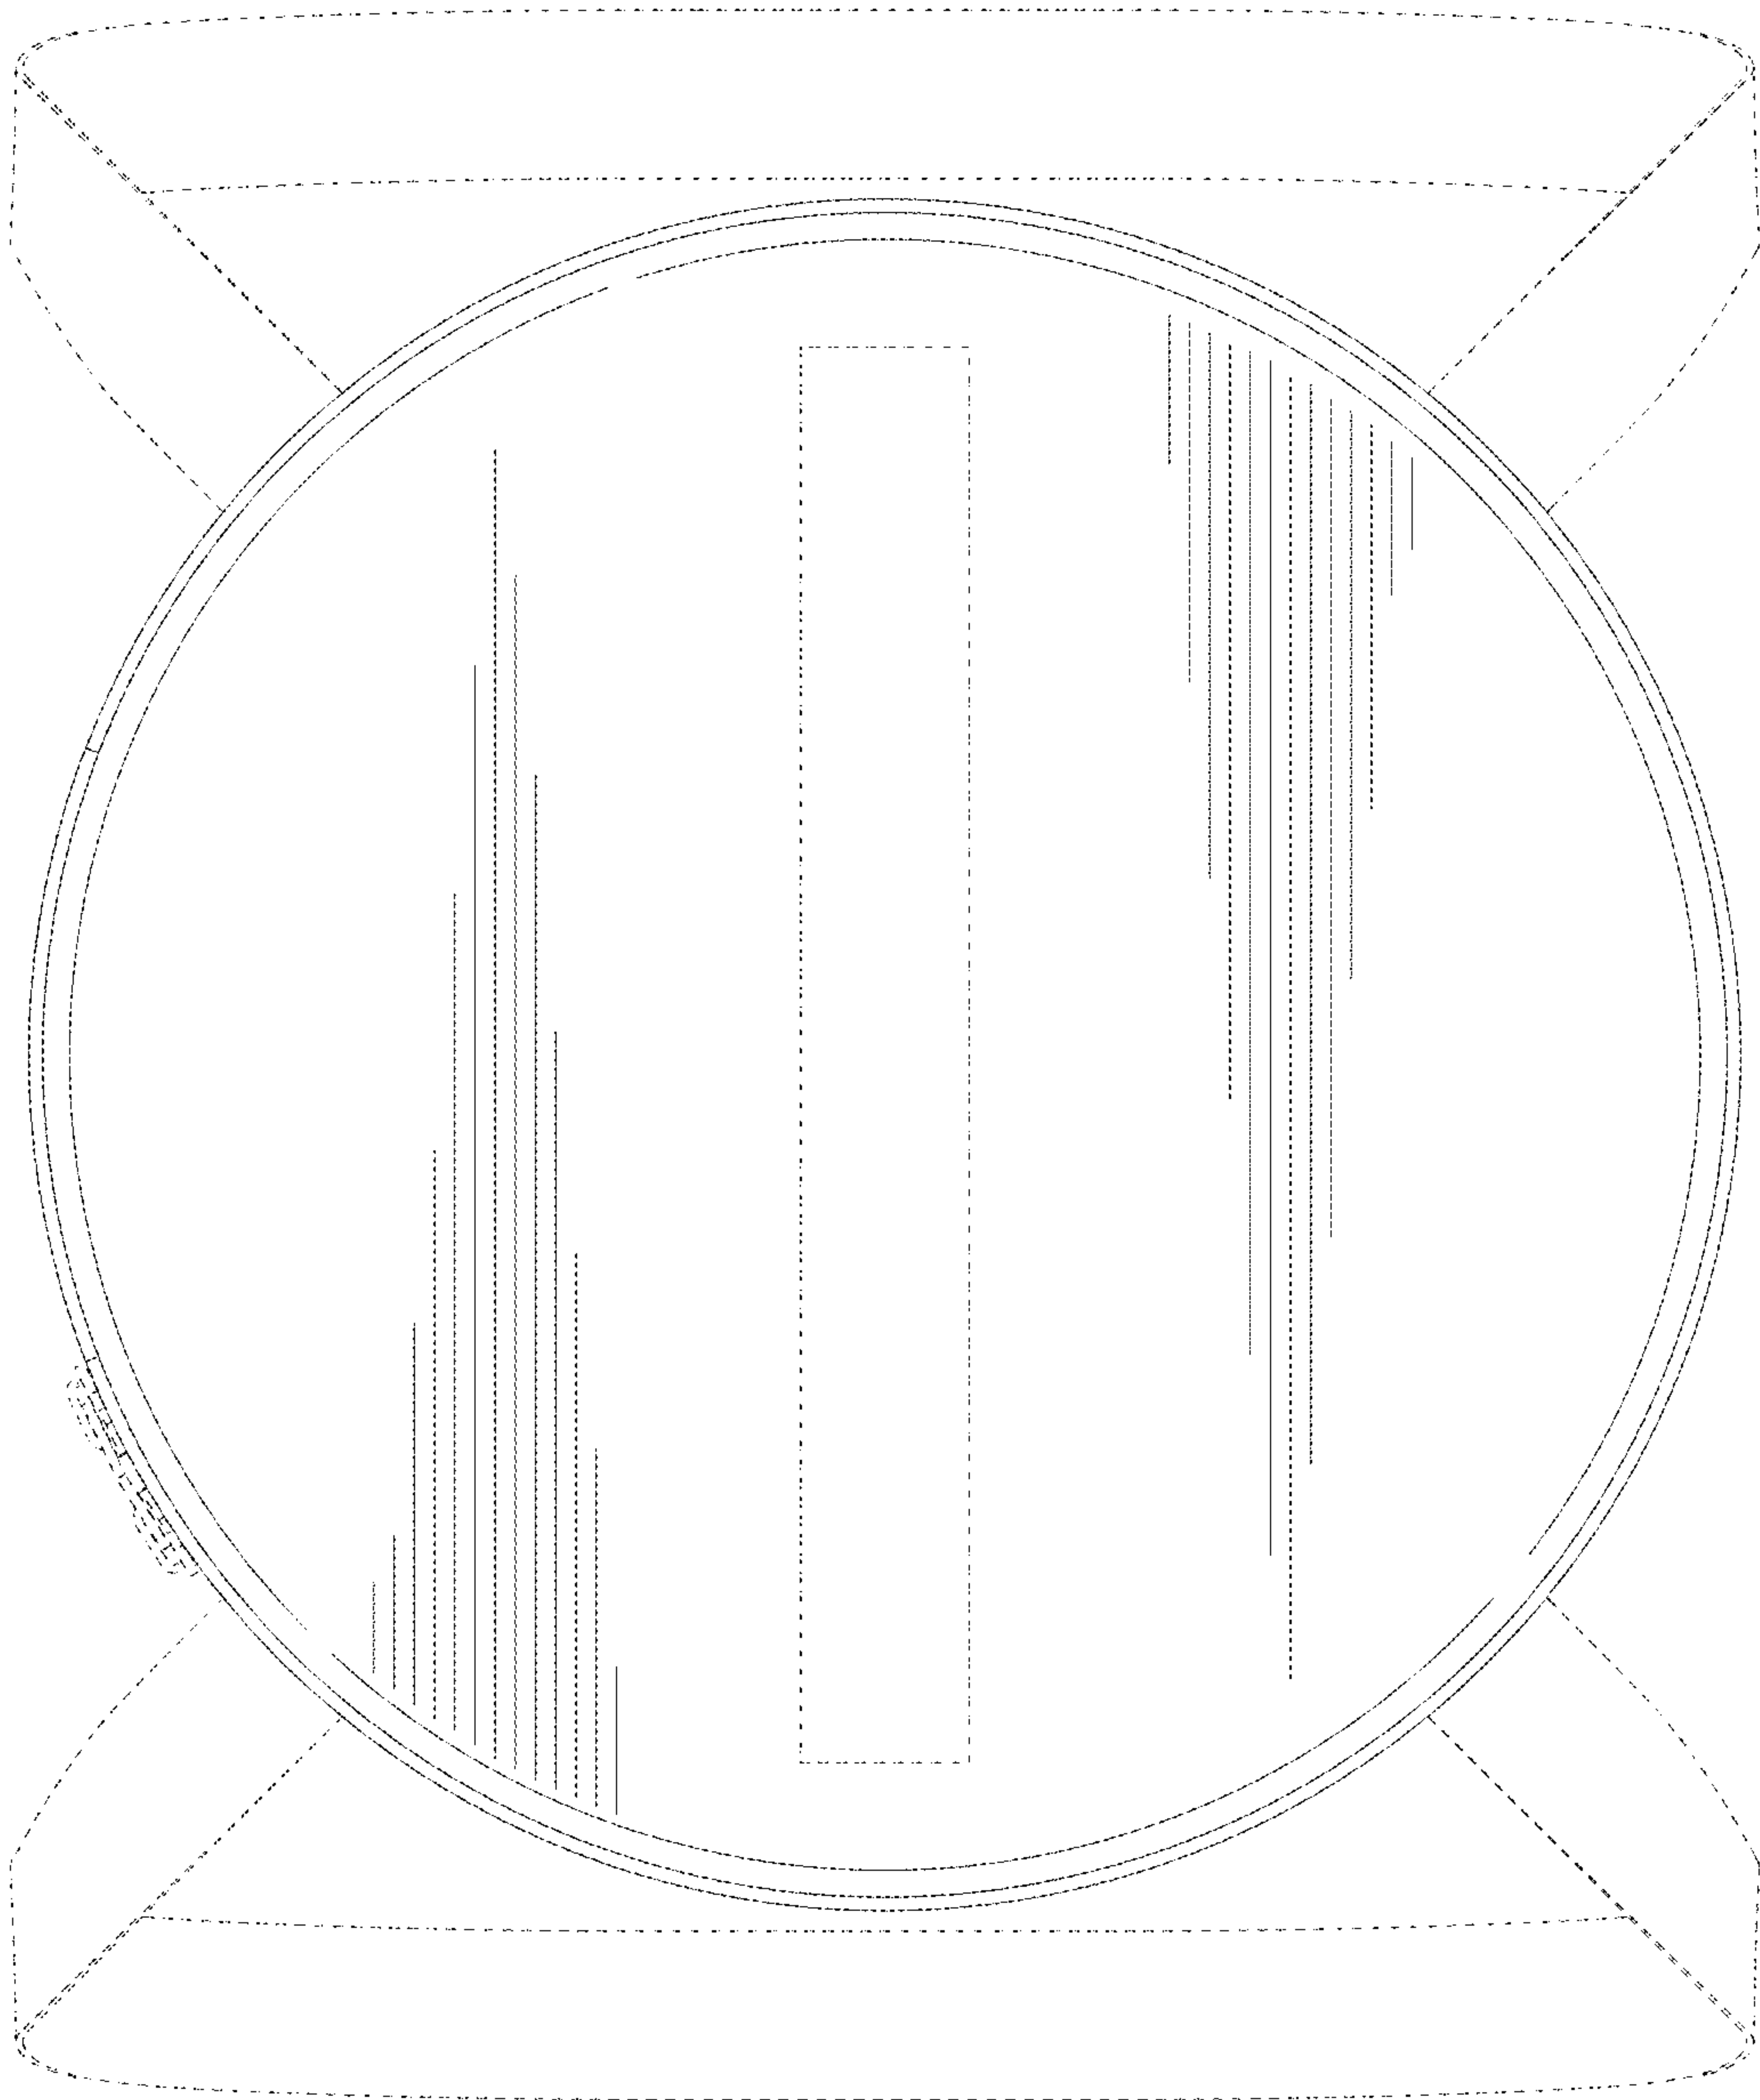


FIG. 7

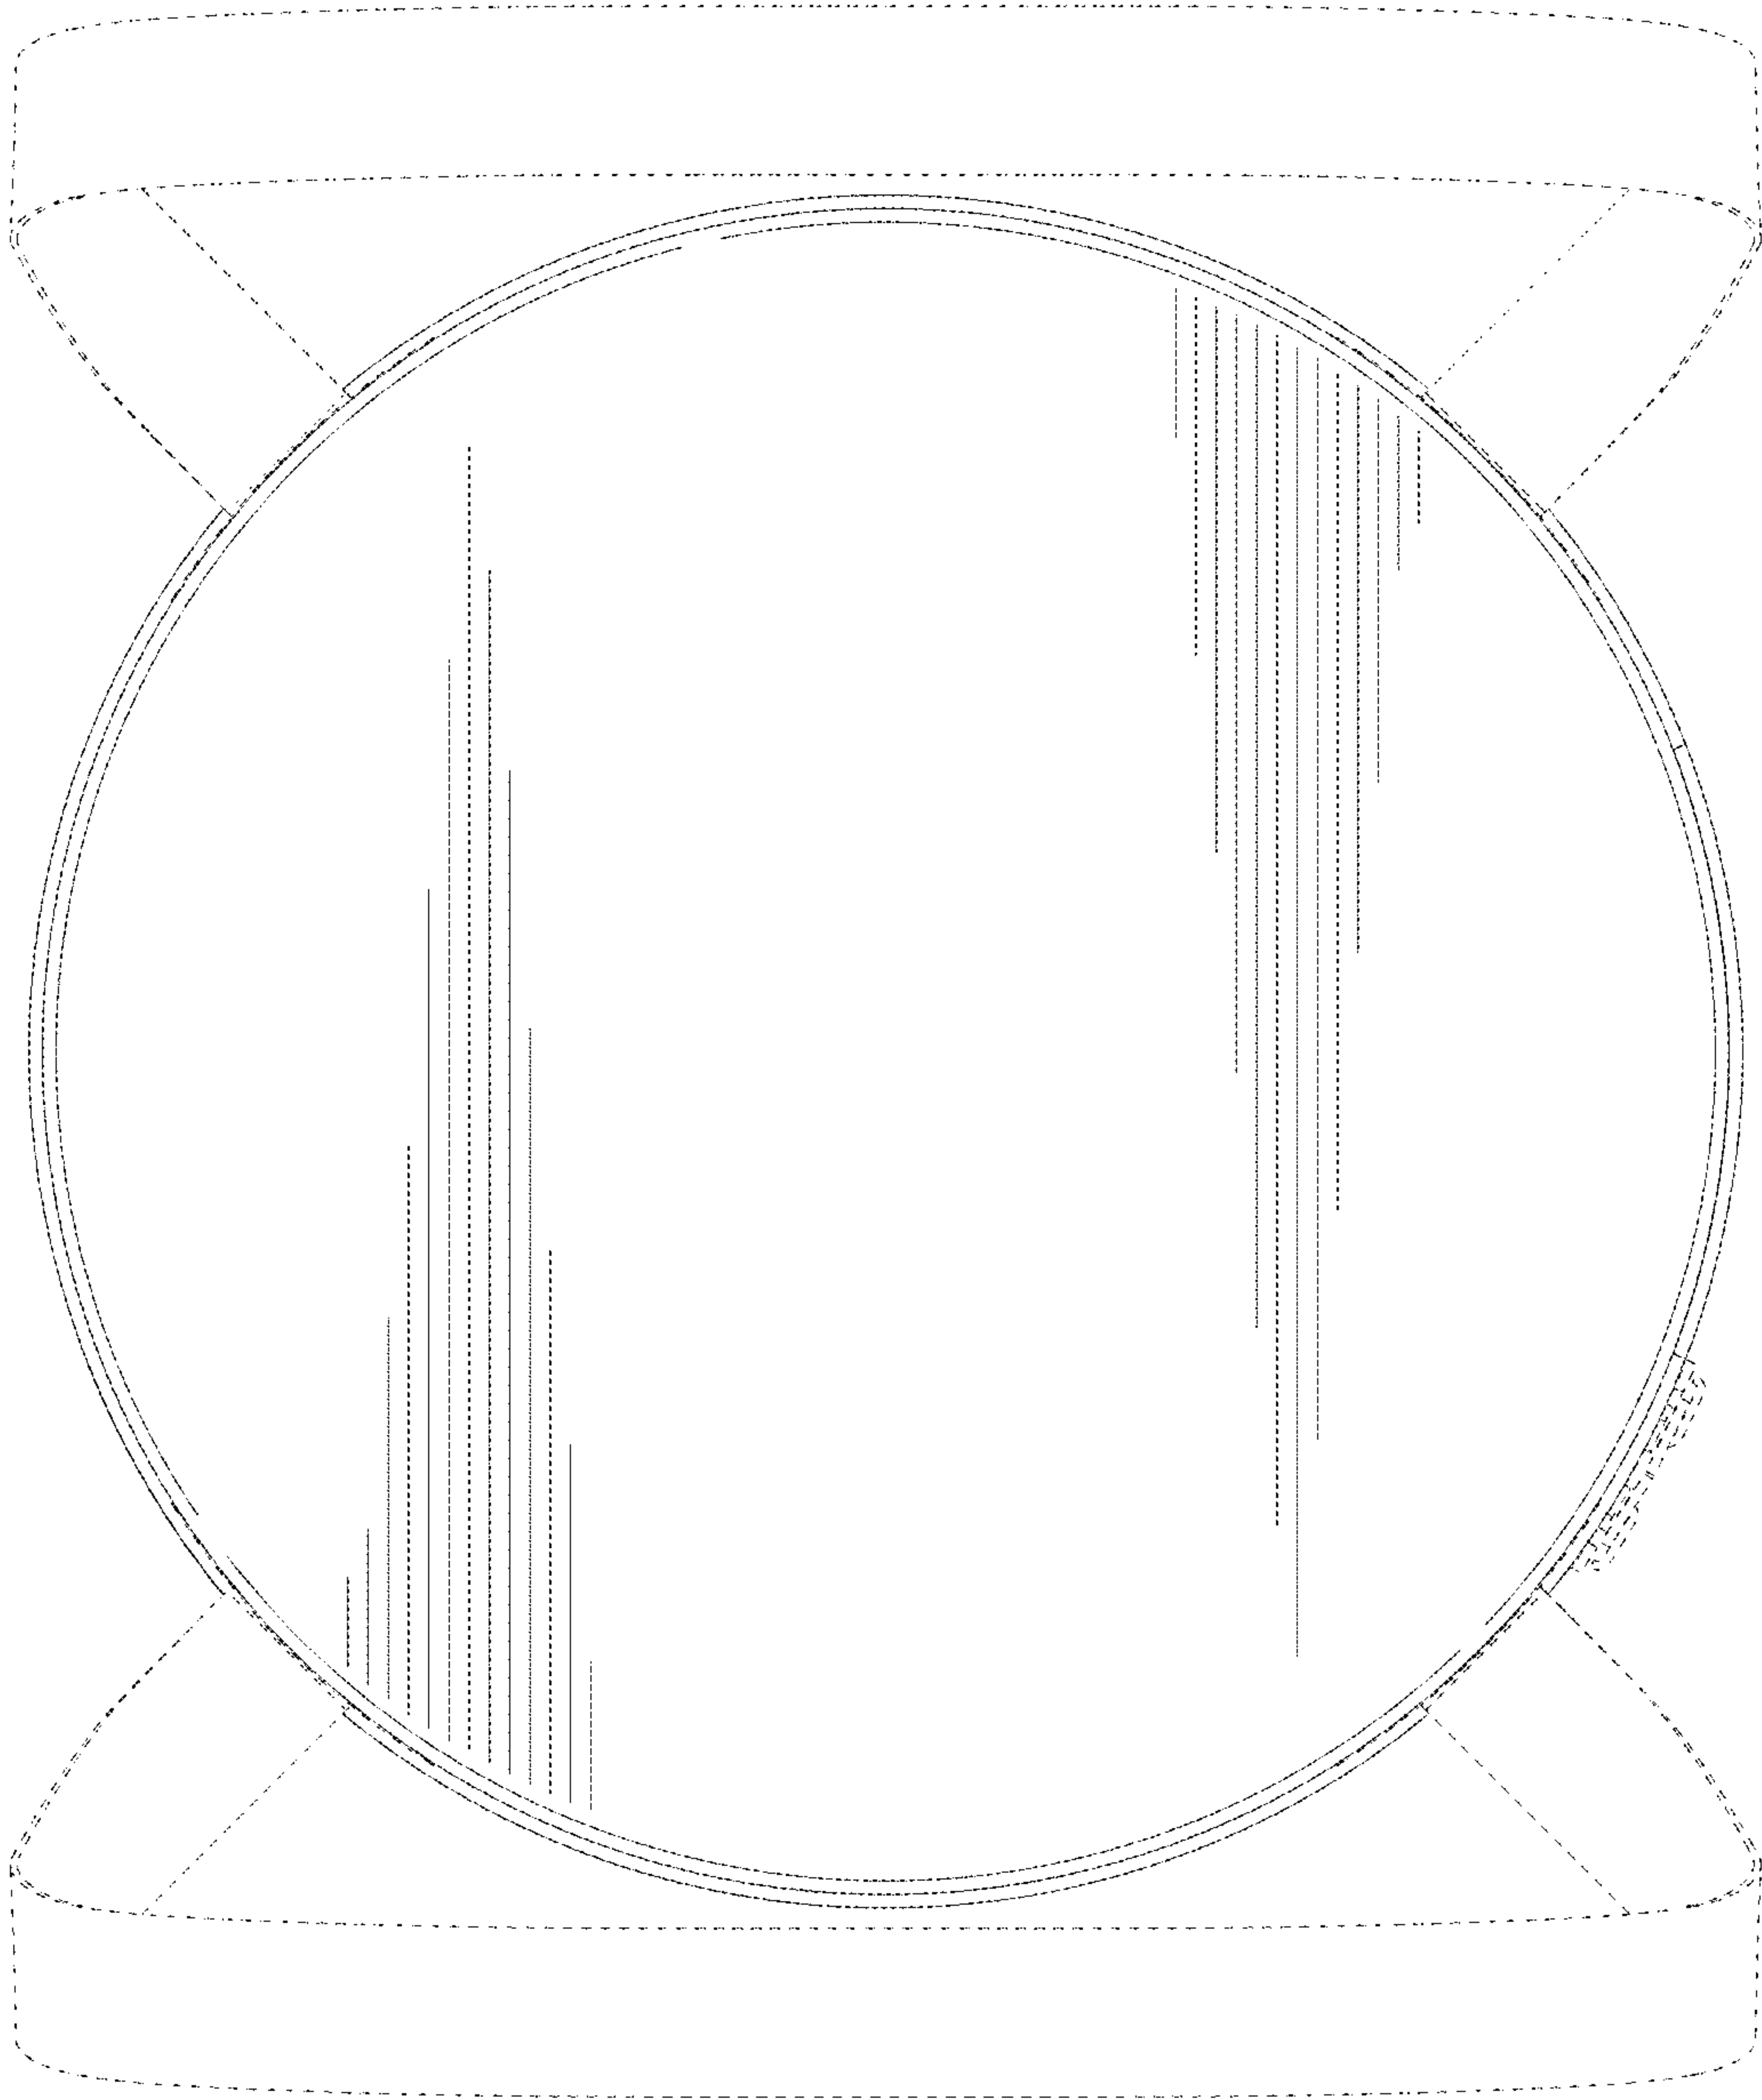


FIG. 8

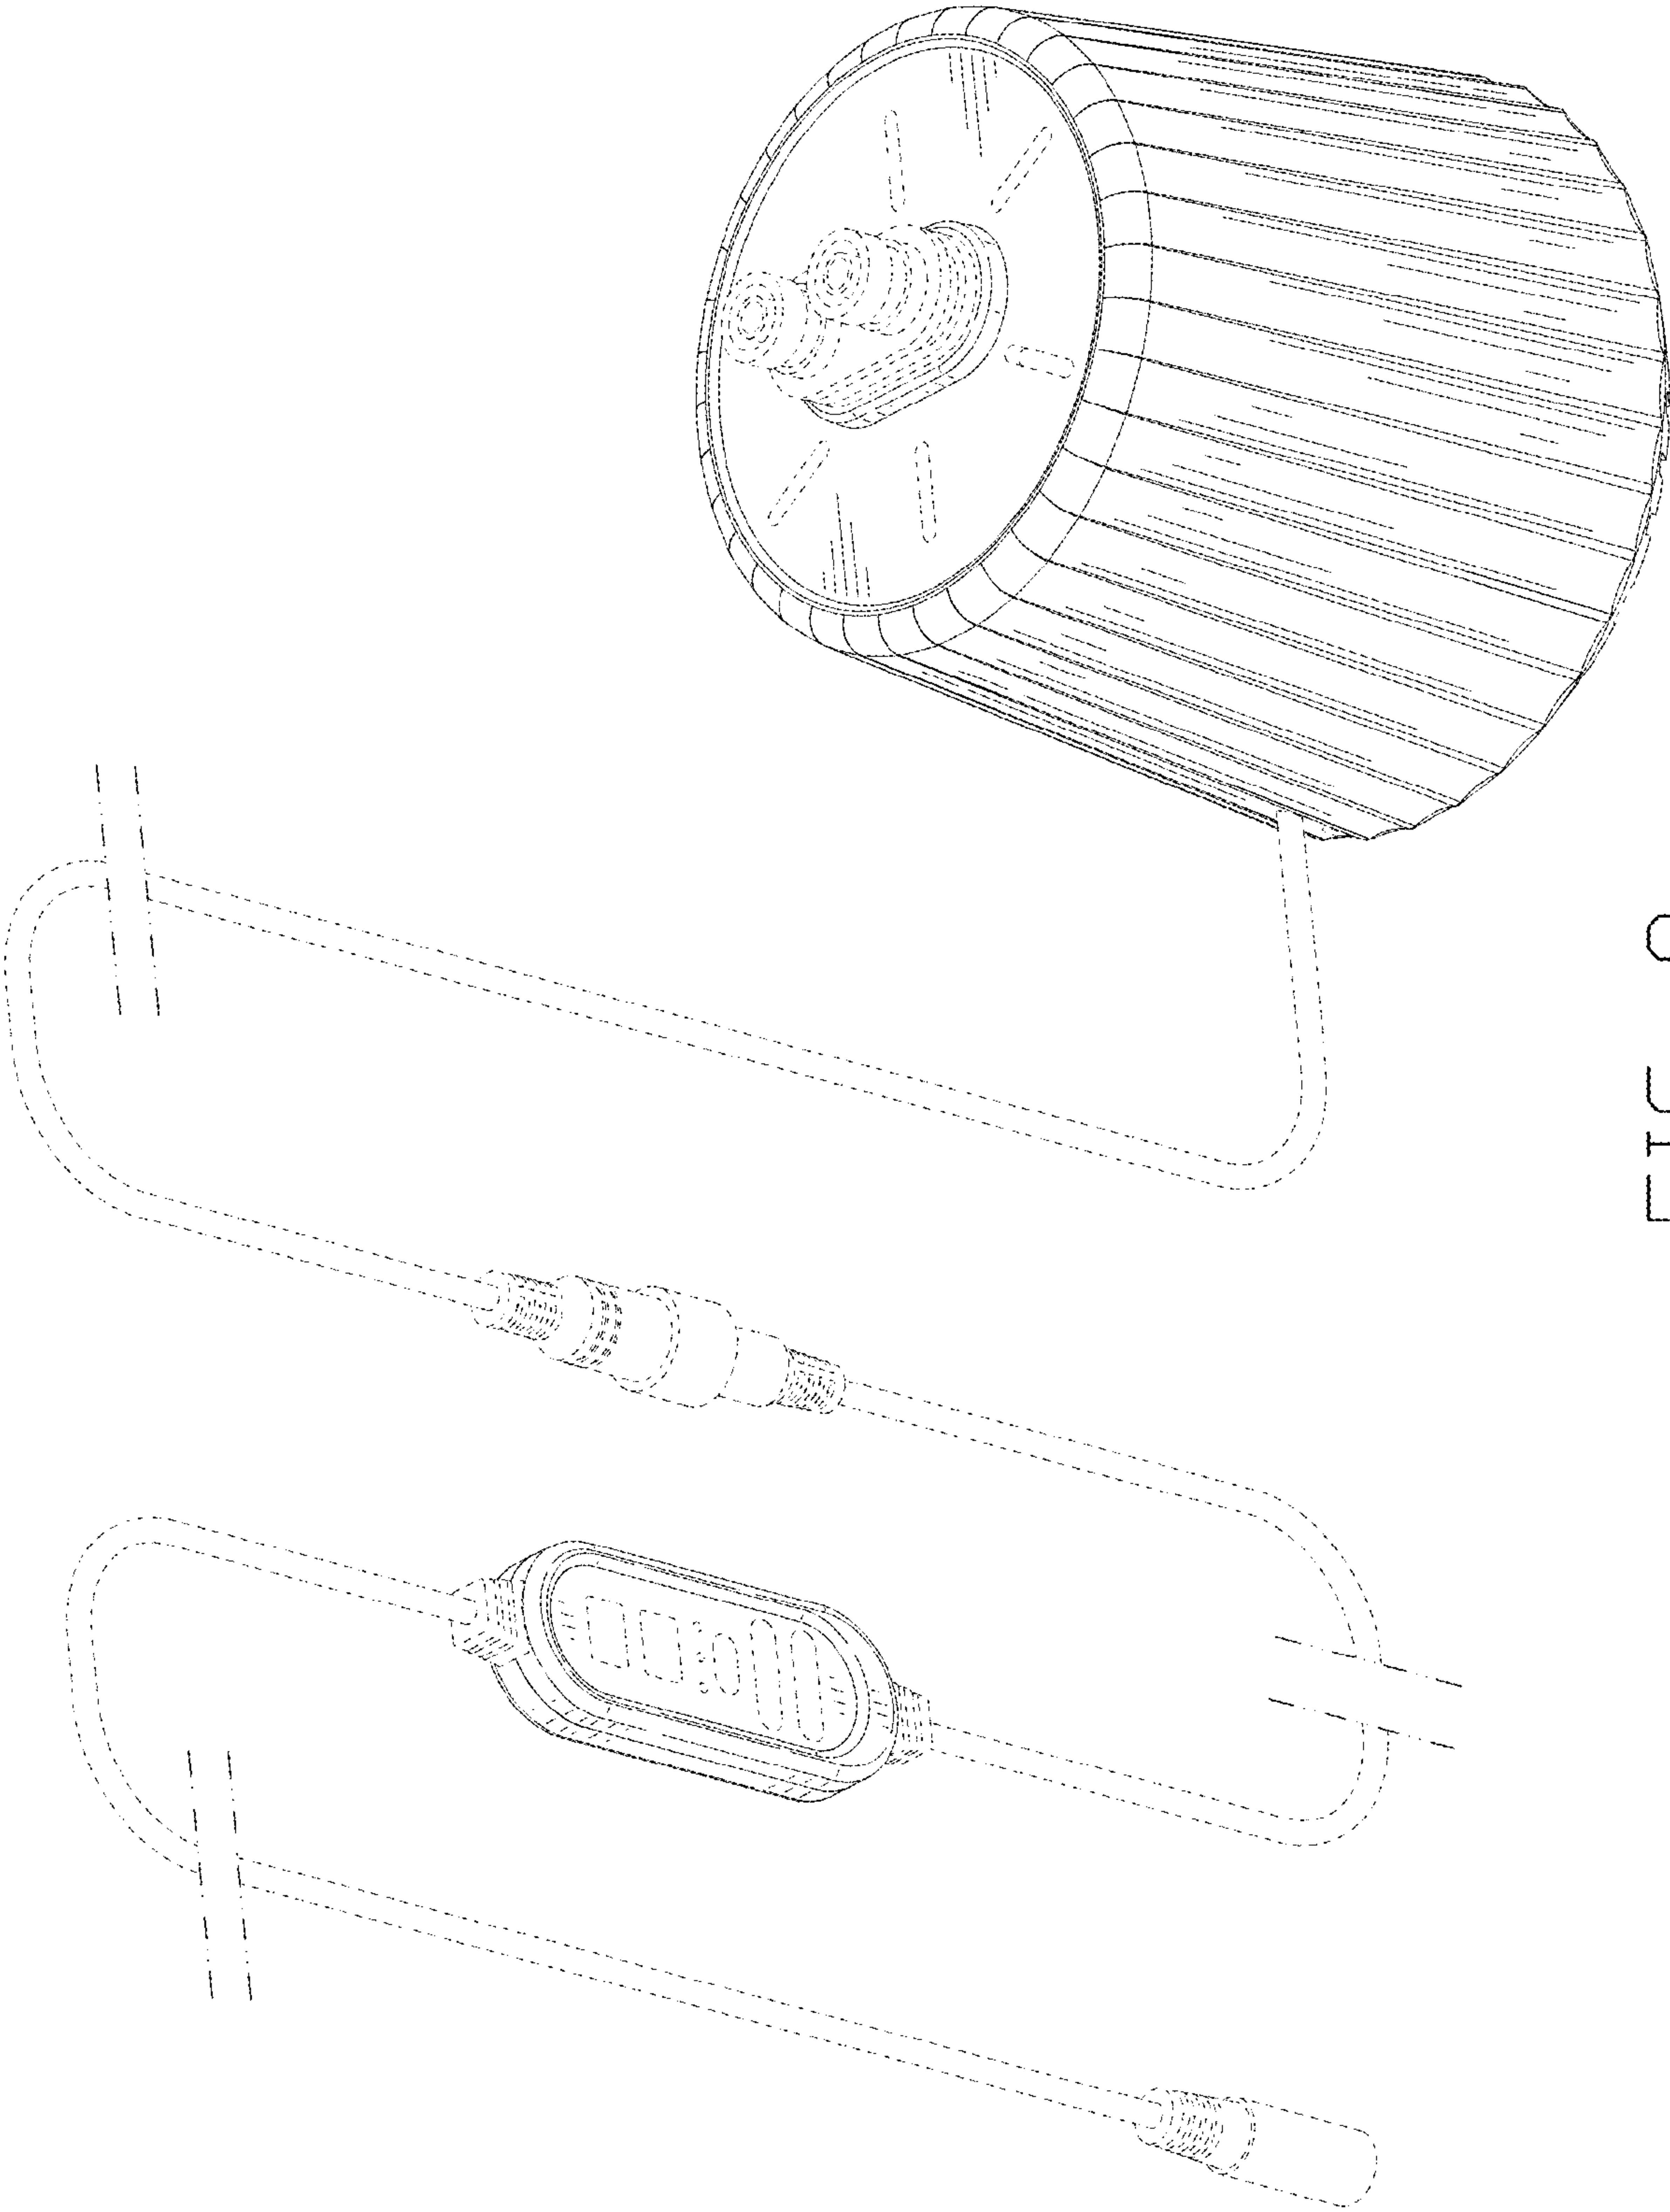


FIG. 9

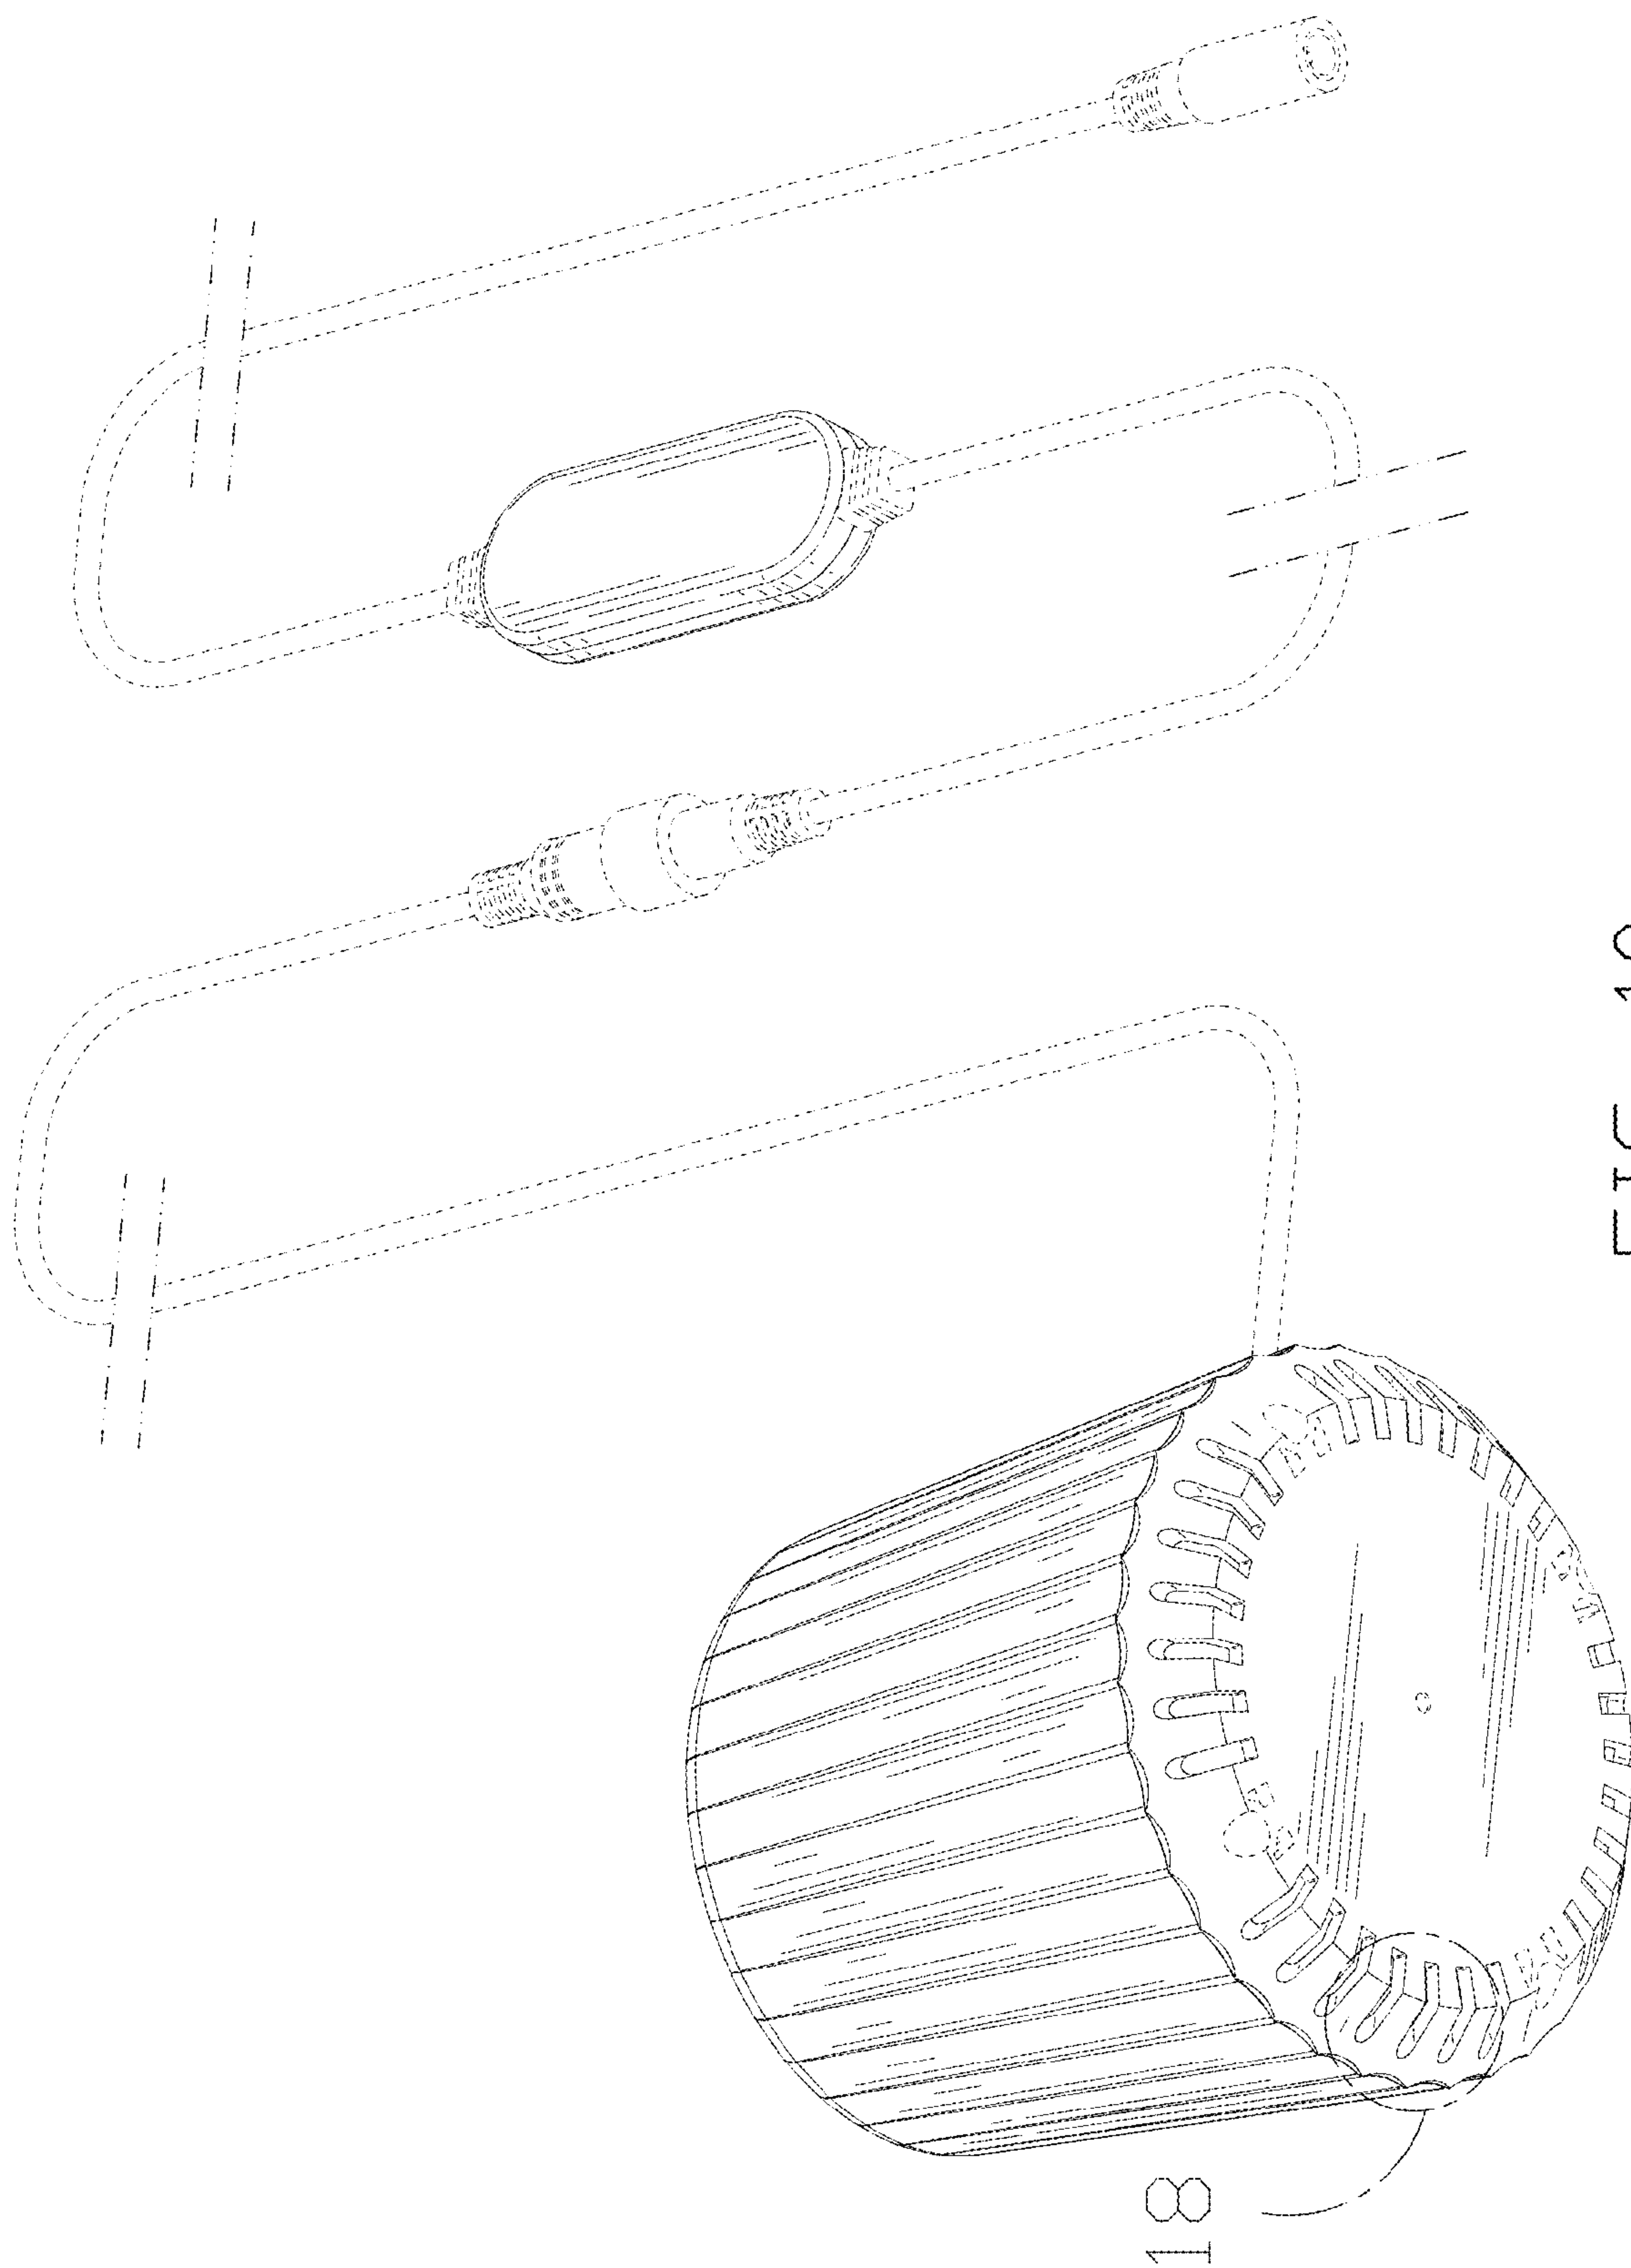


FIG. 10

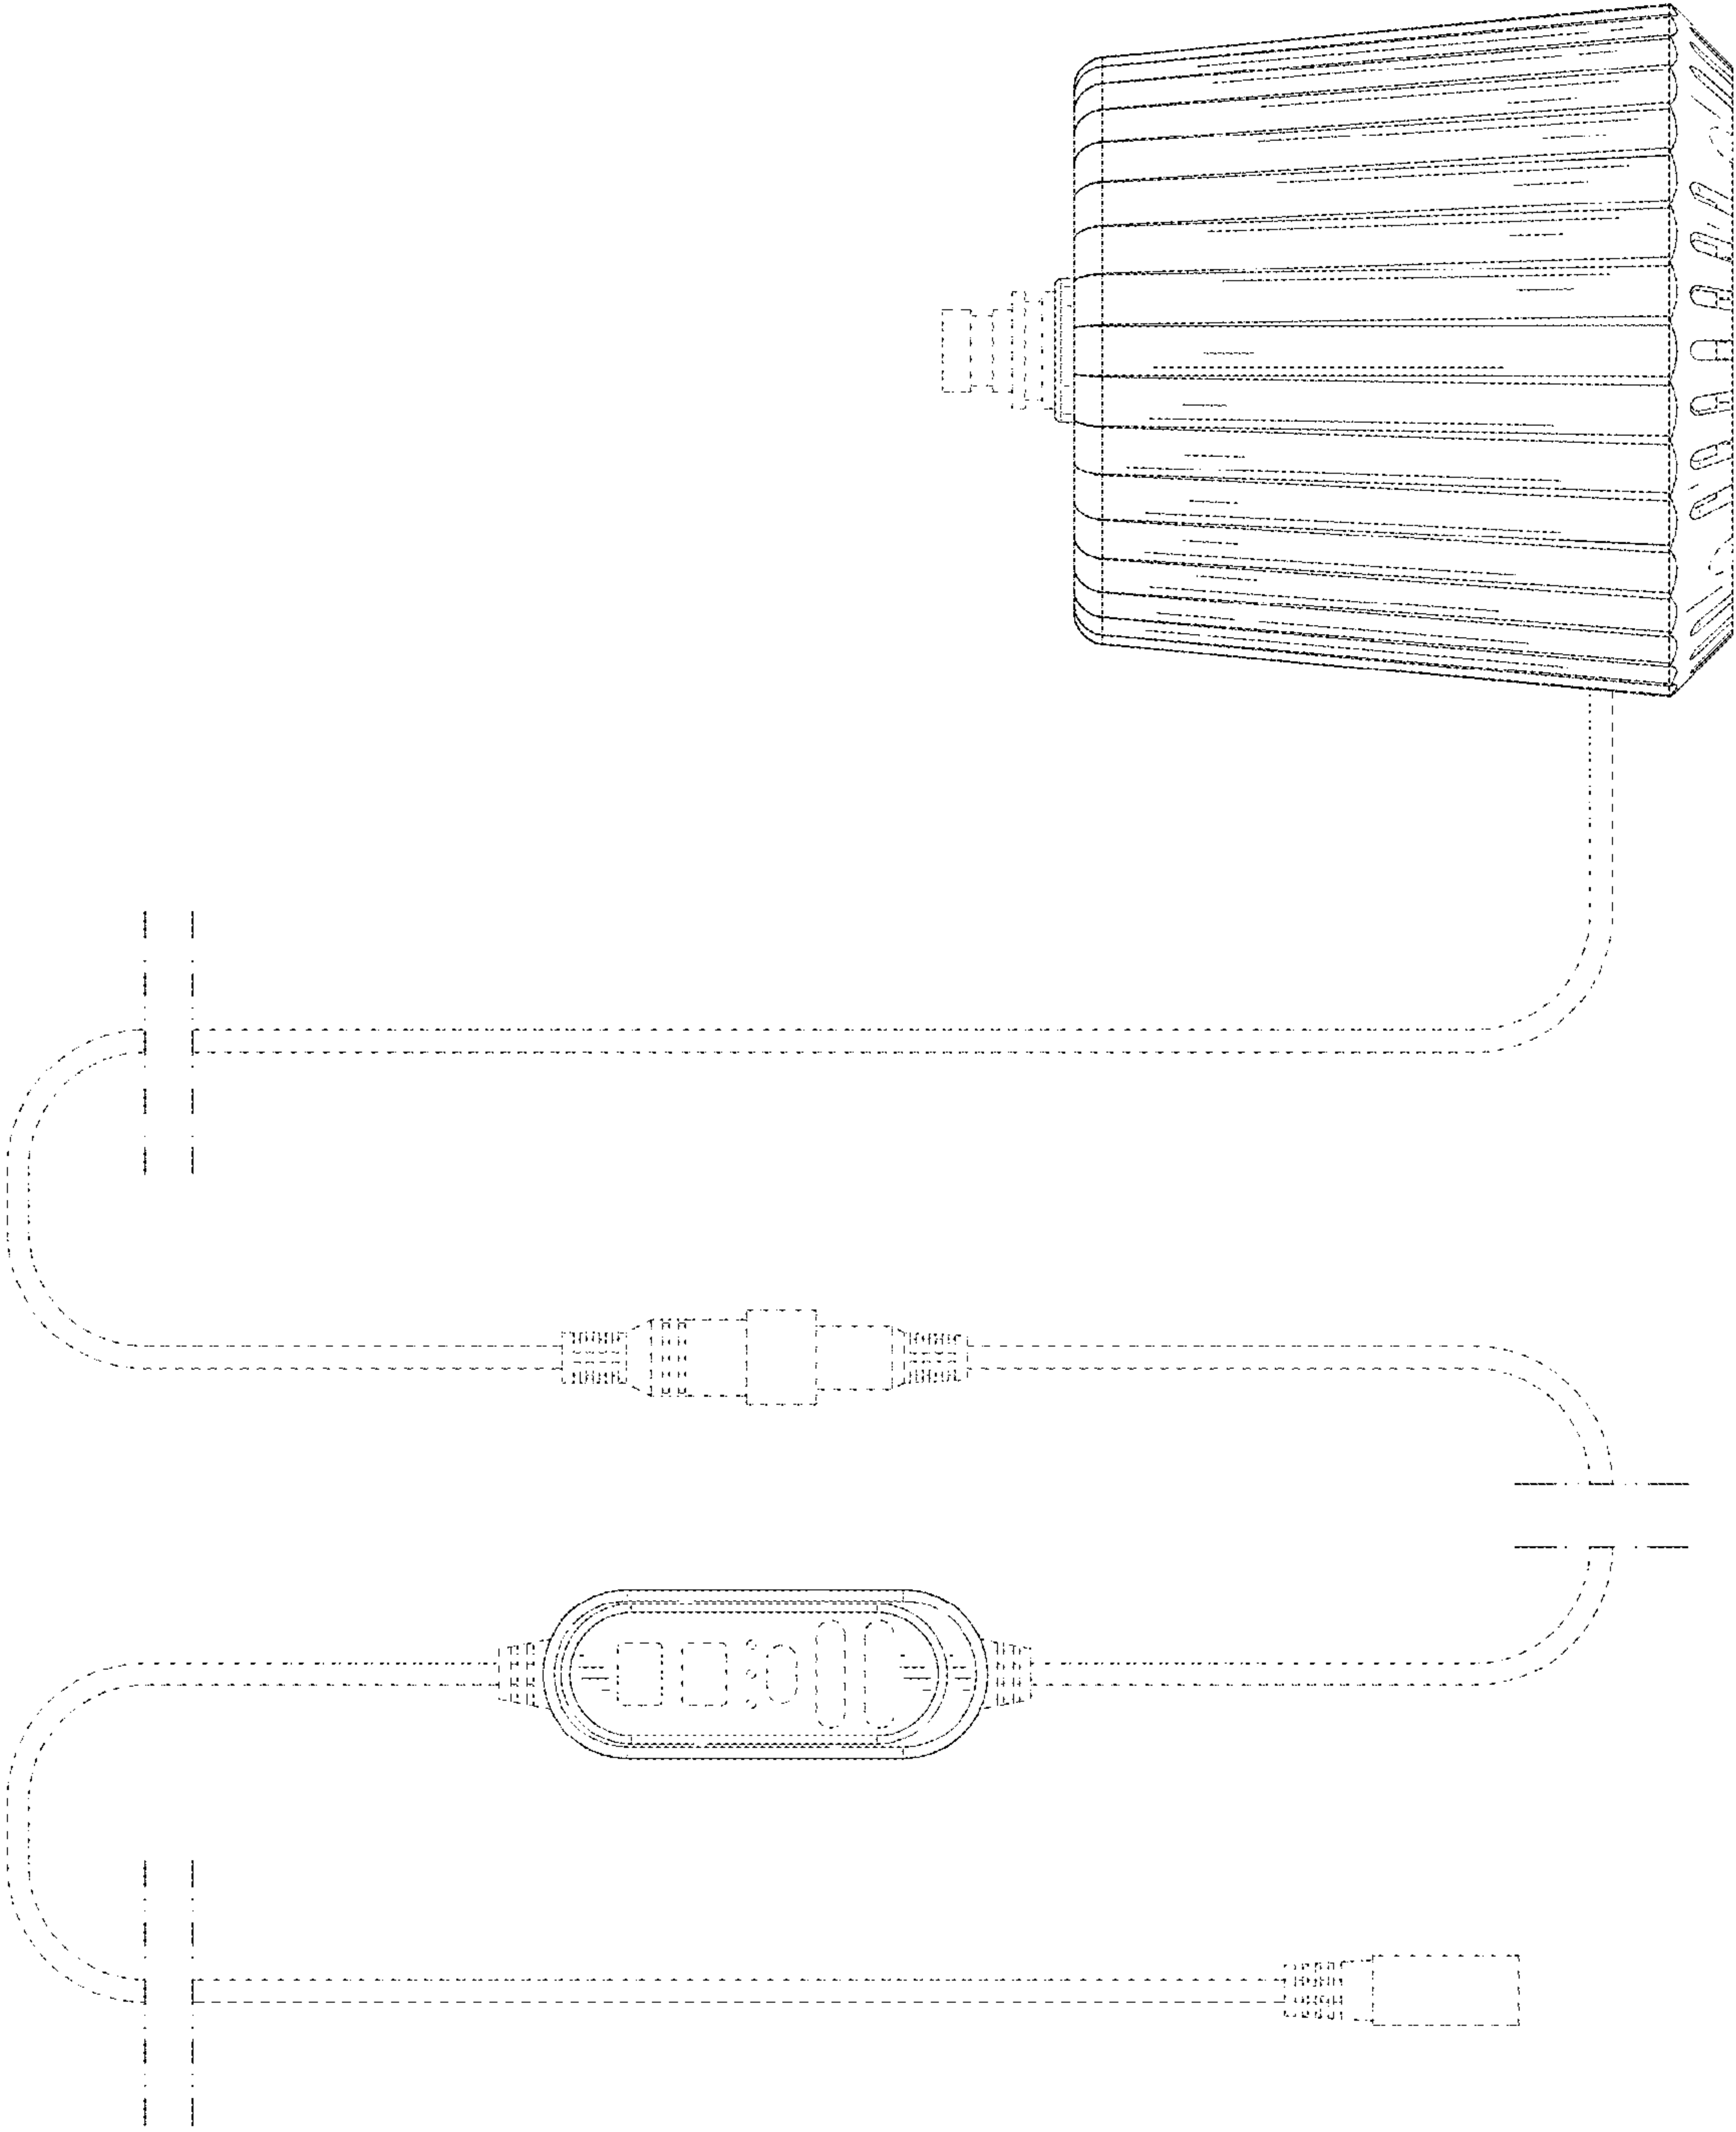


FIG. 11

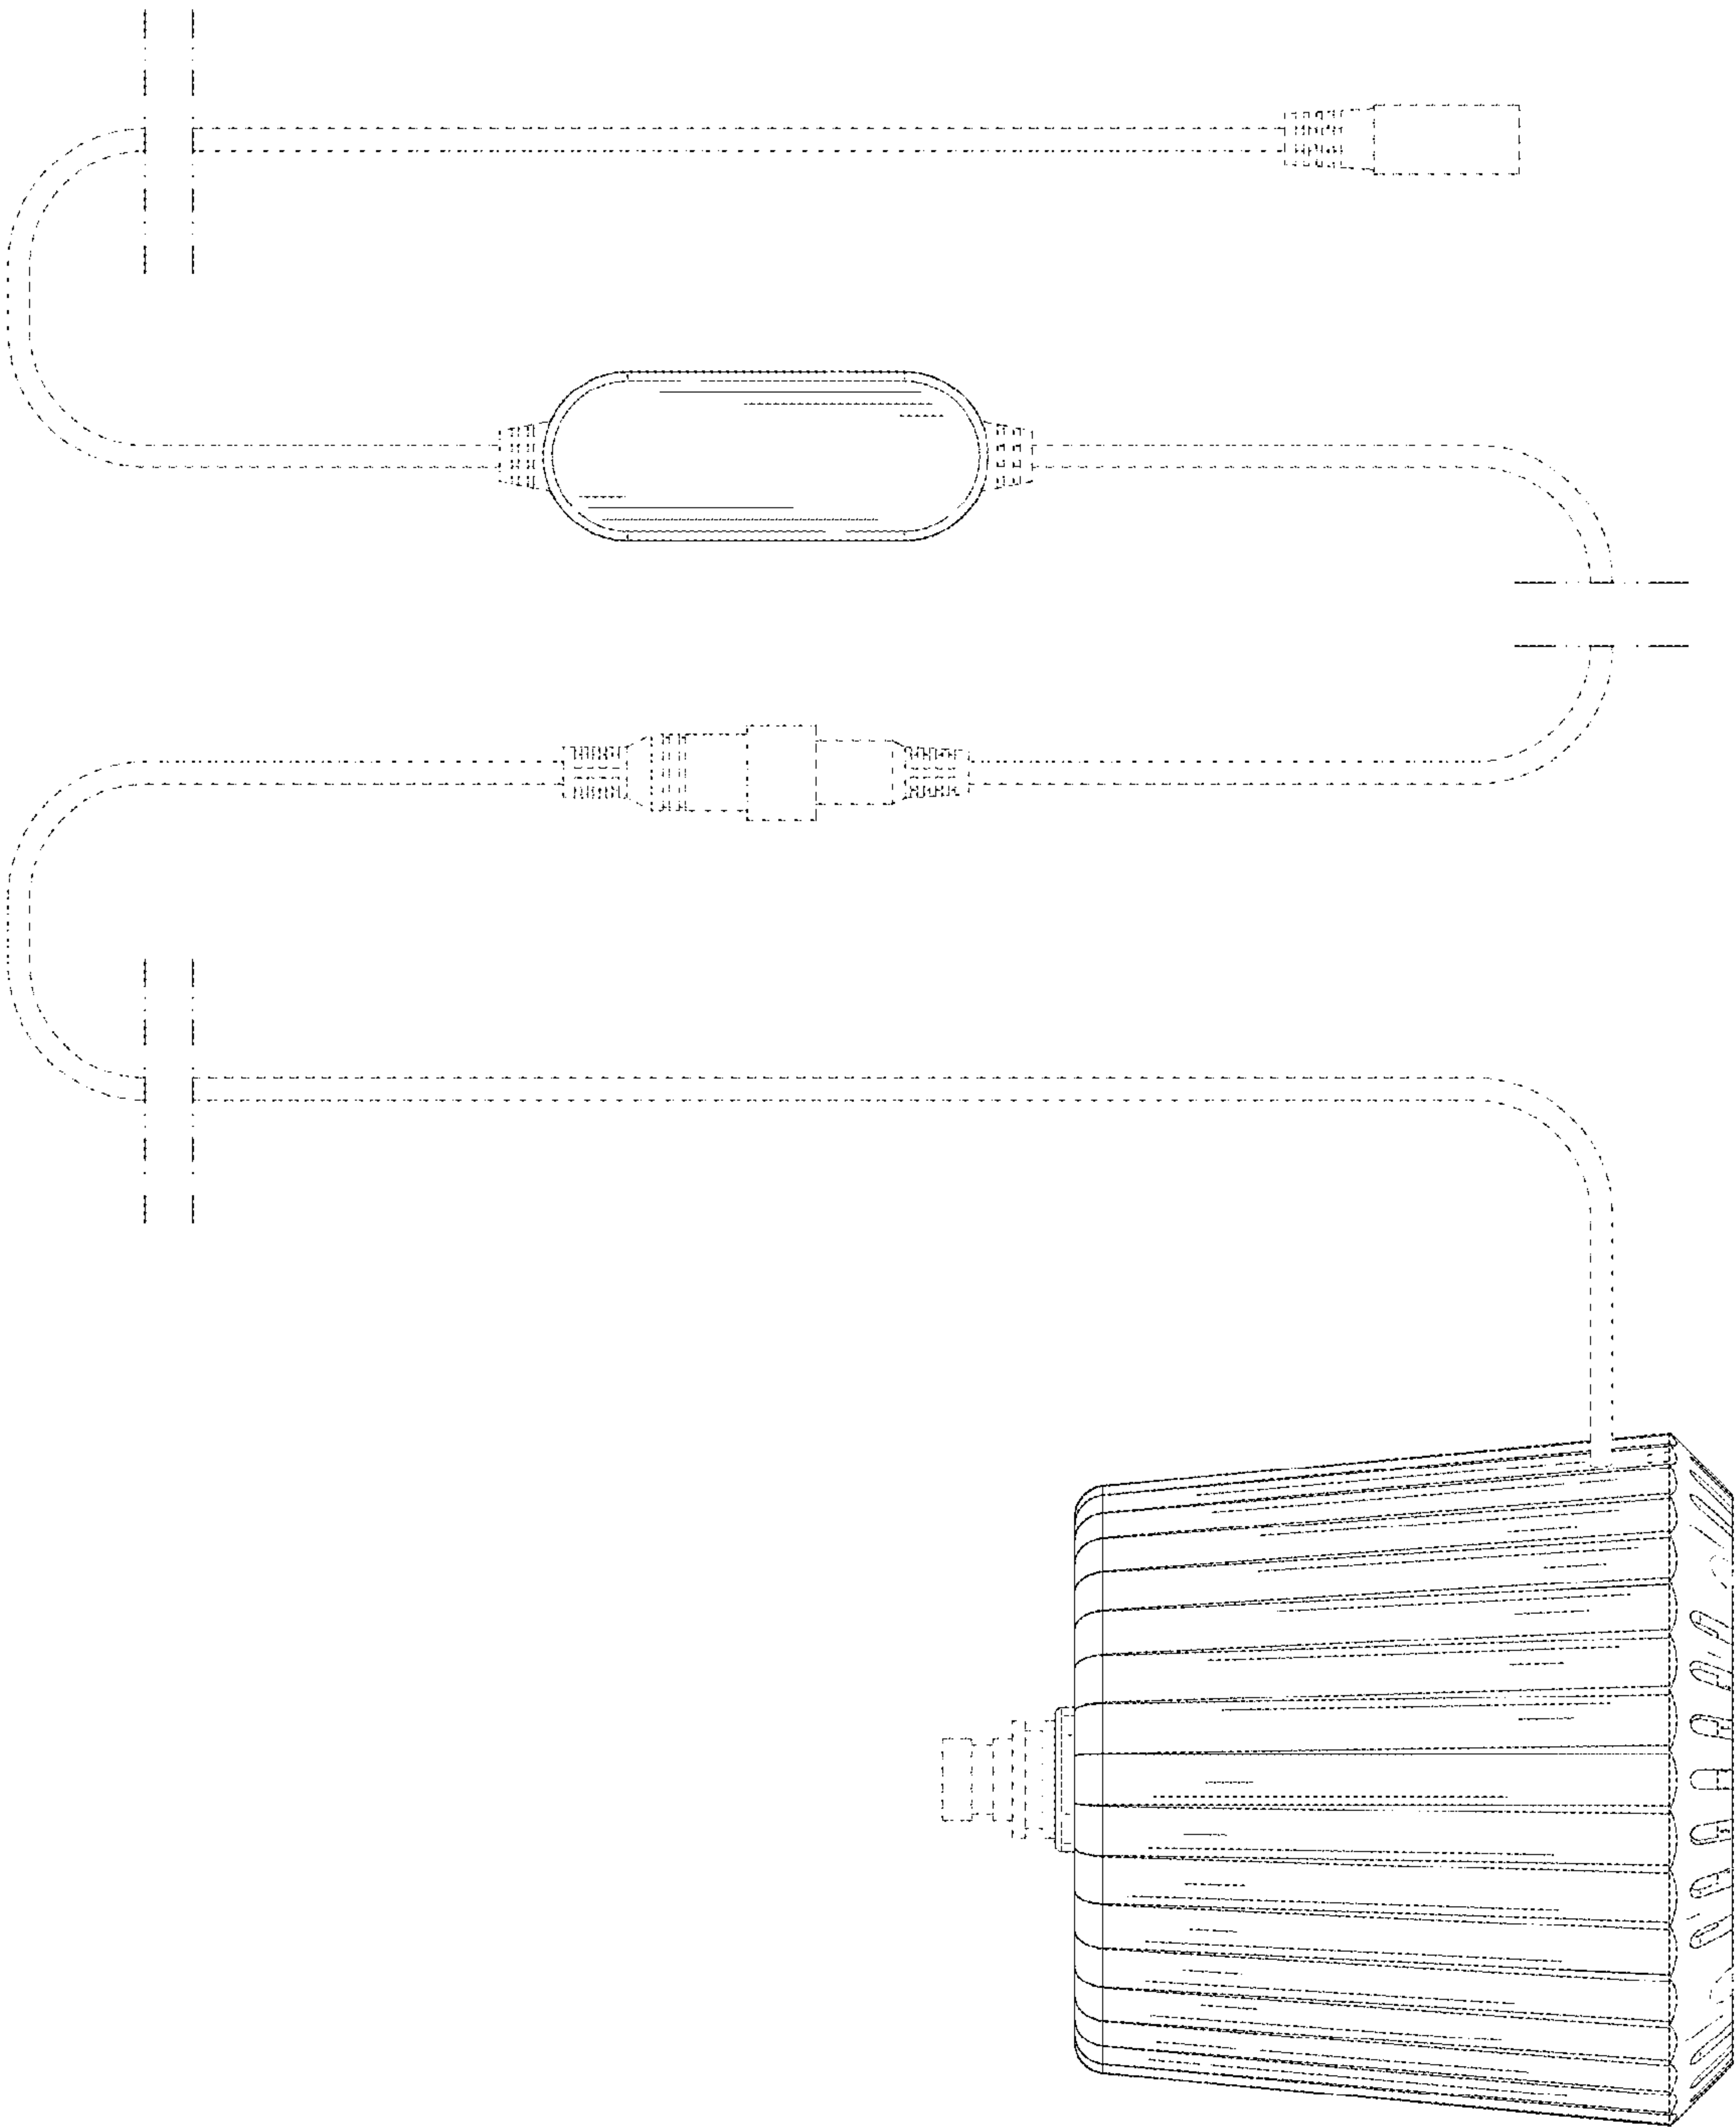


FIG. 12

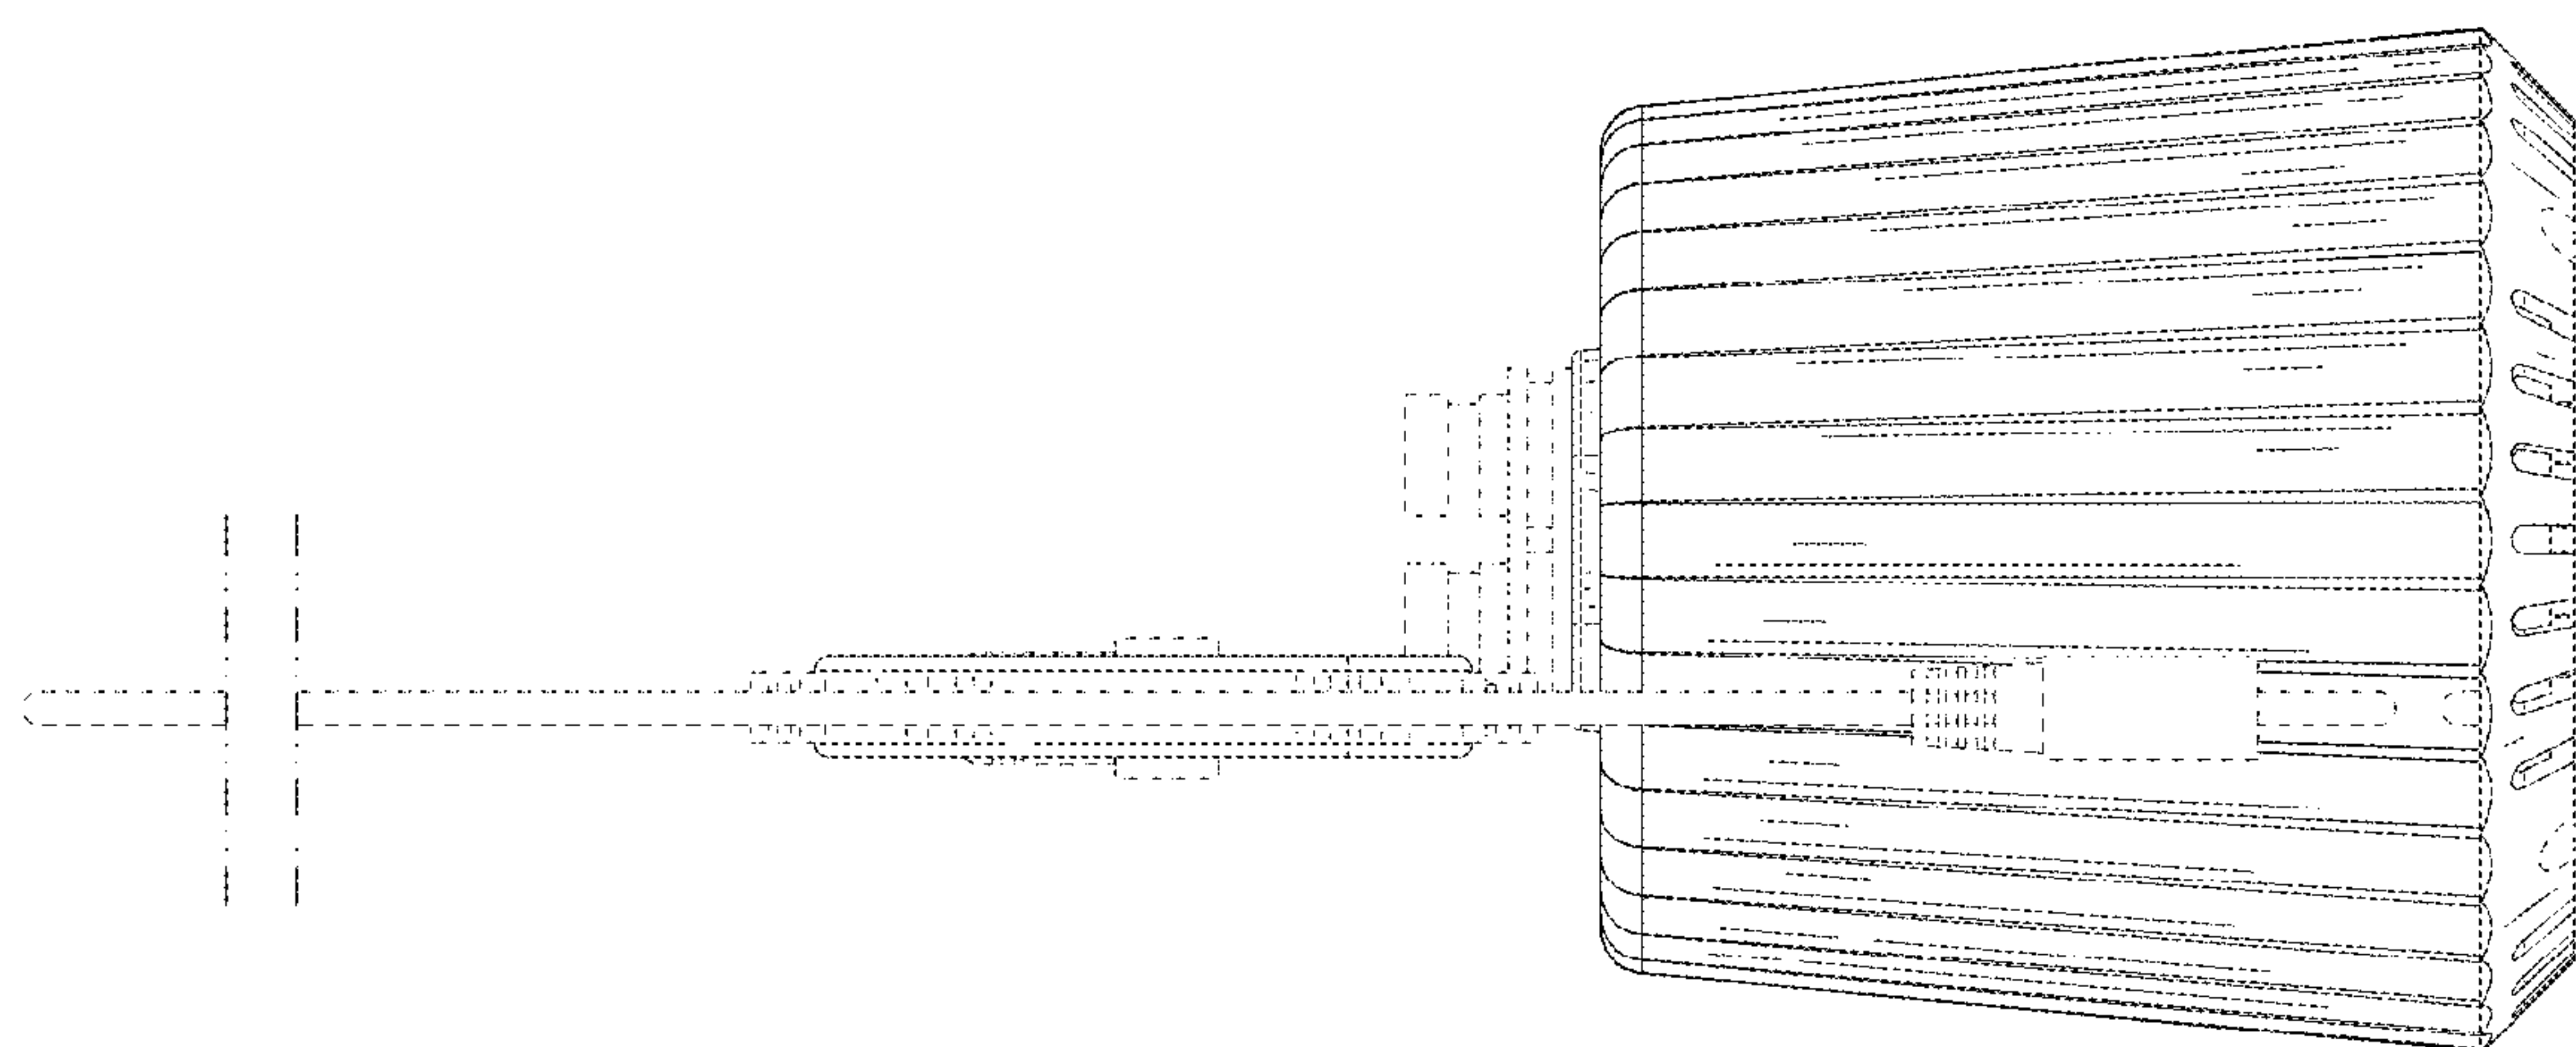


FIG. 13

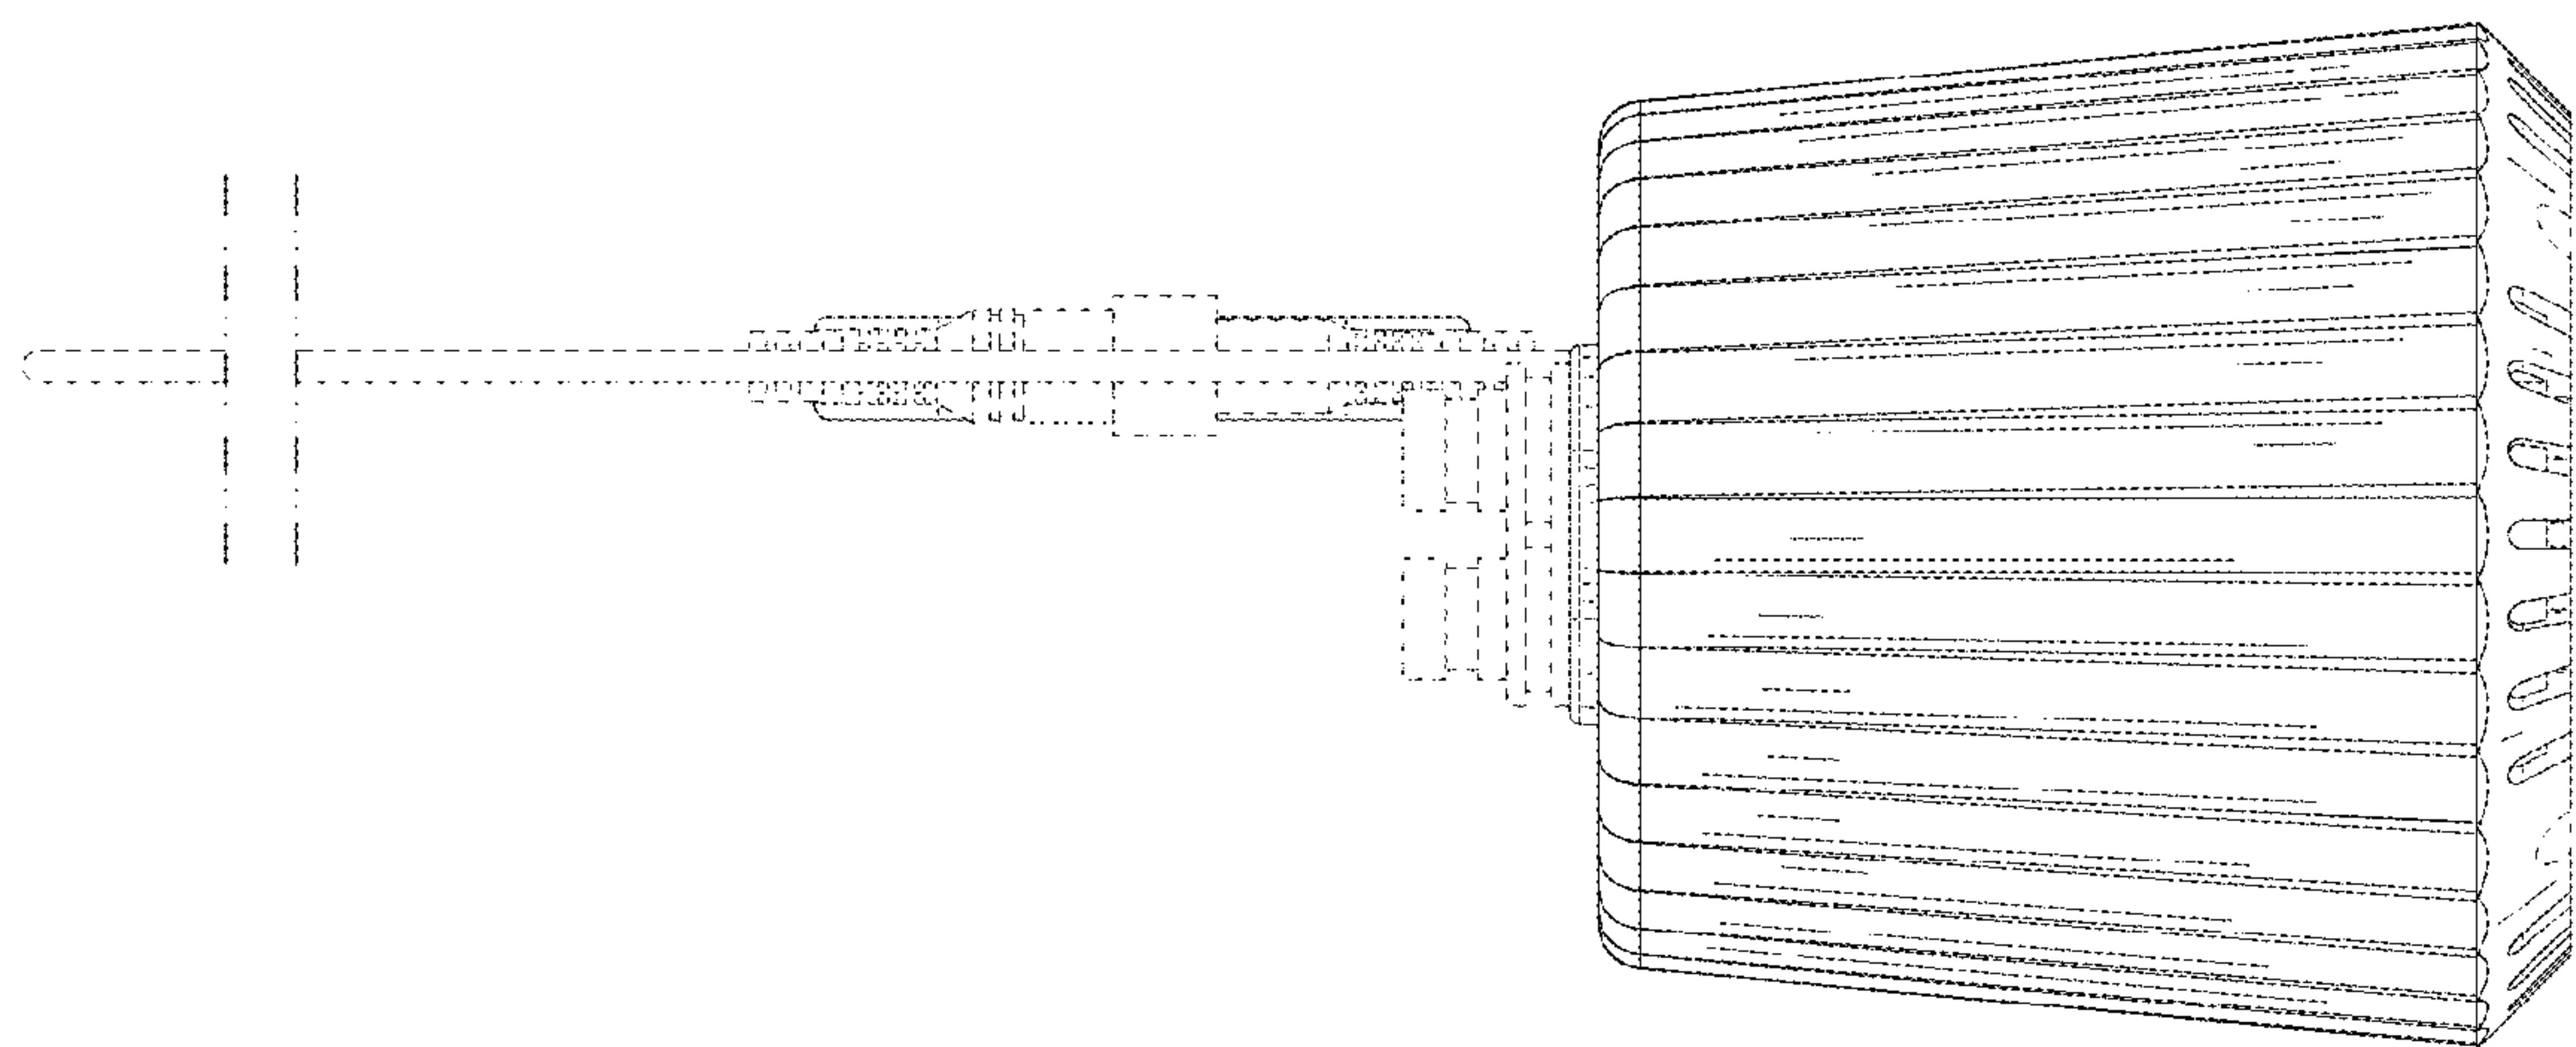


FIG. 14

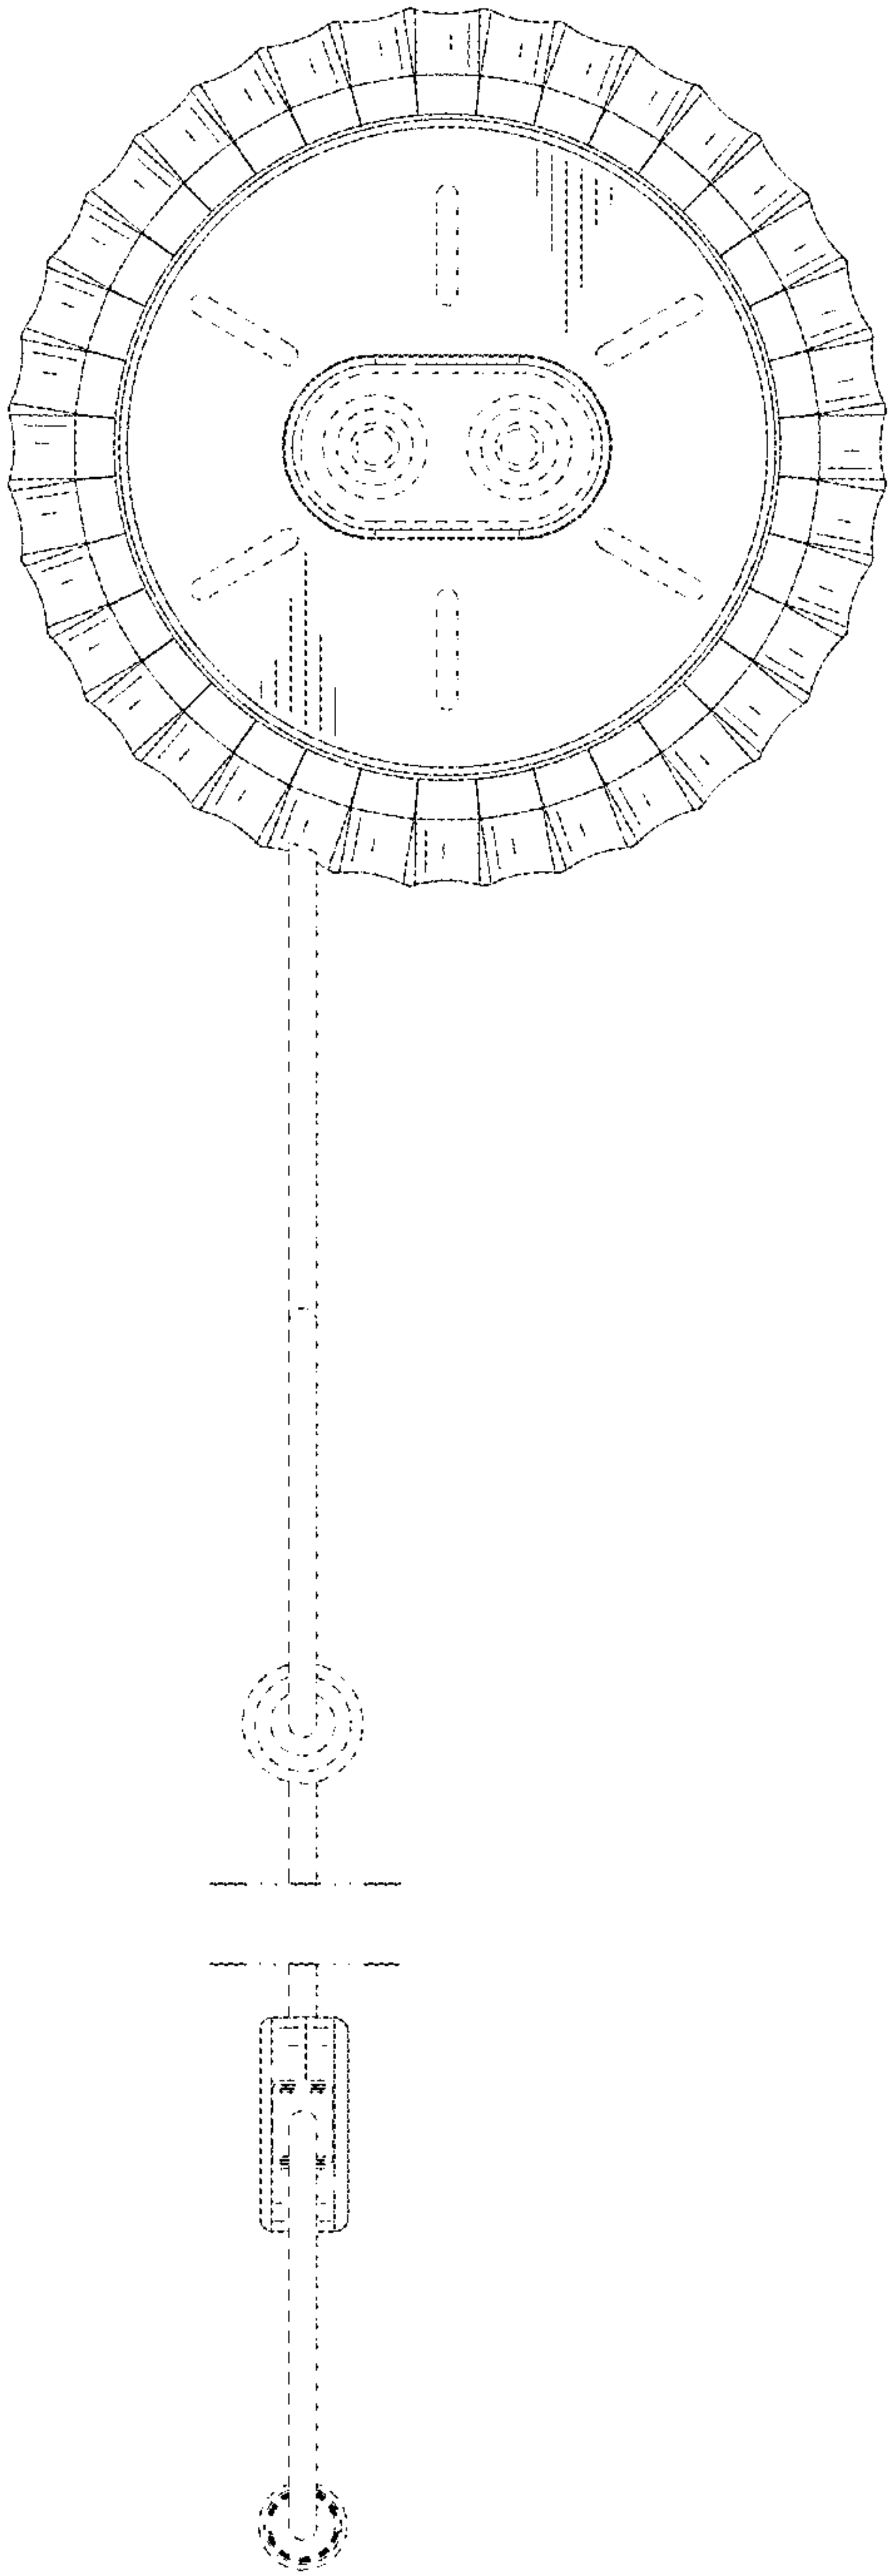


FIG. 15

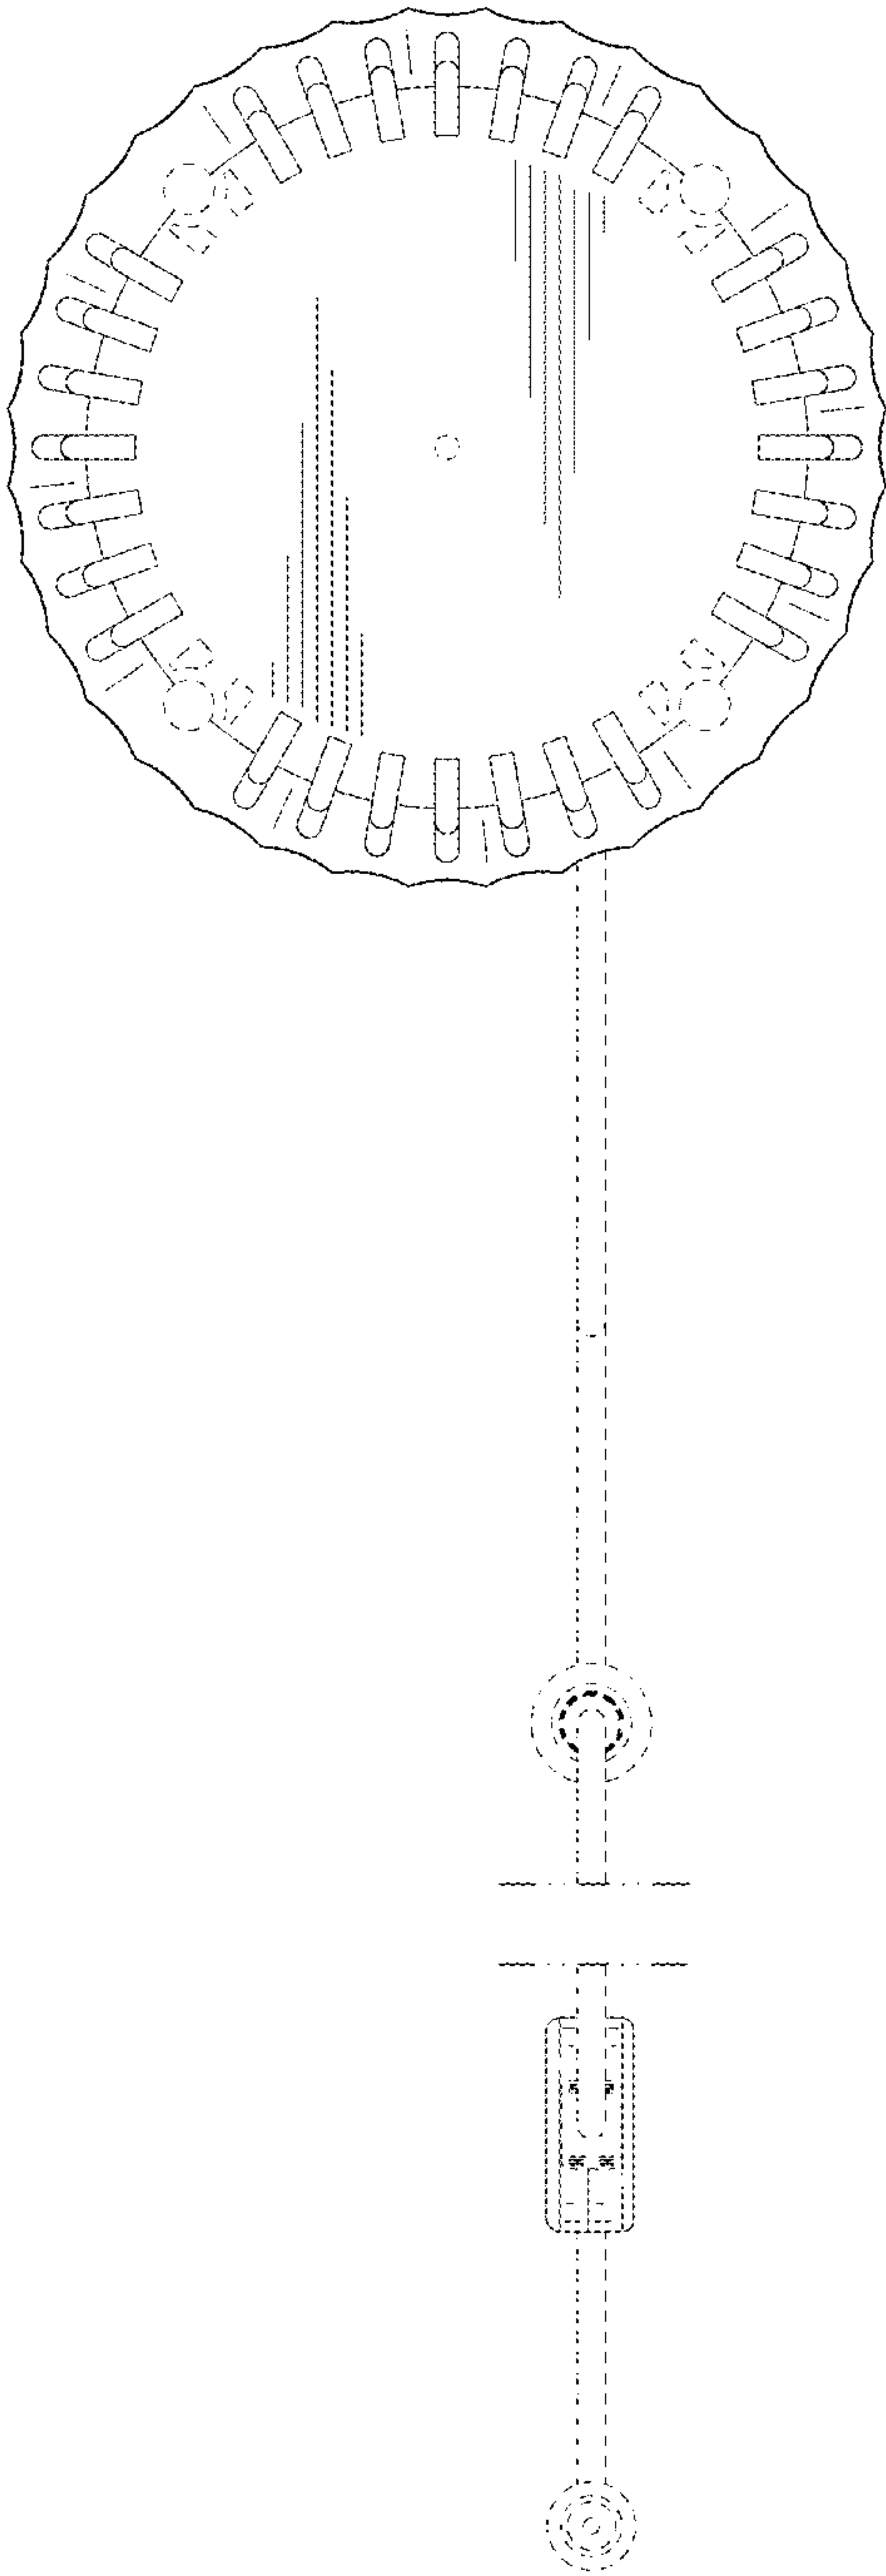


FIG. 16

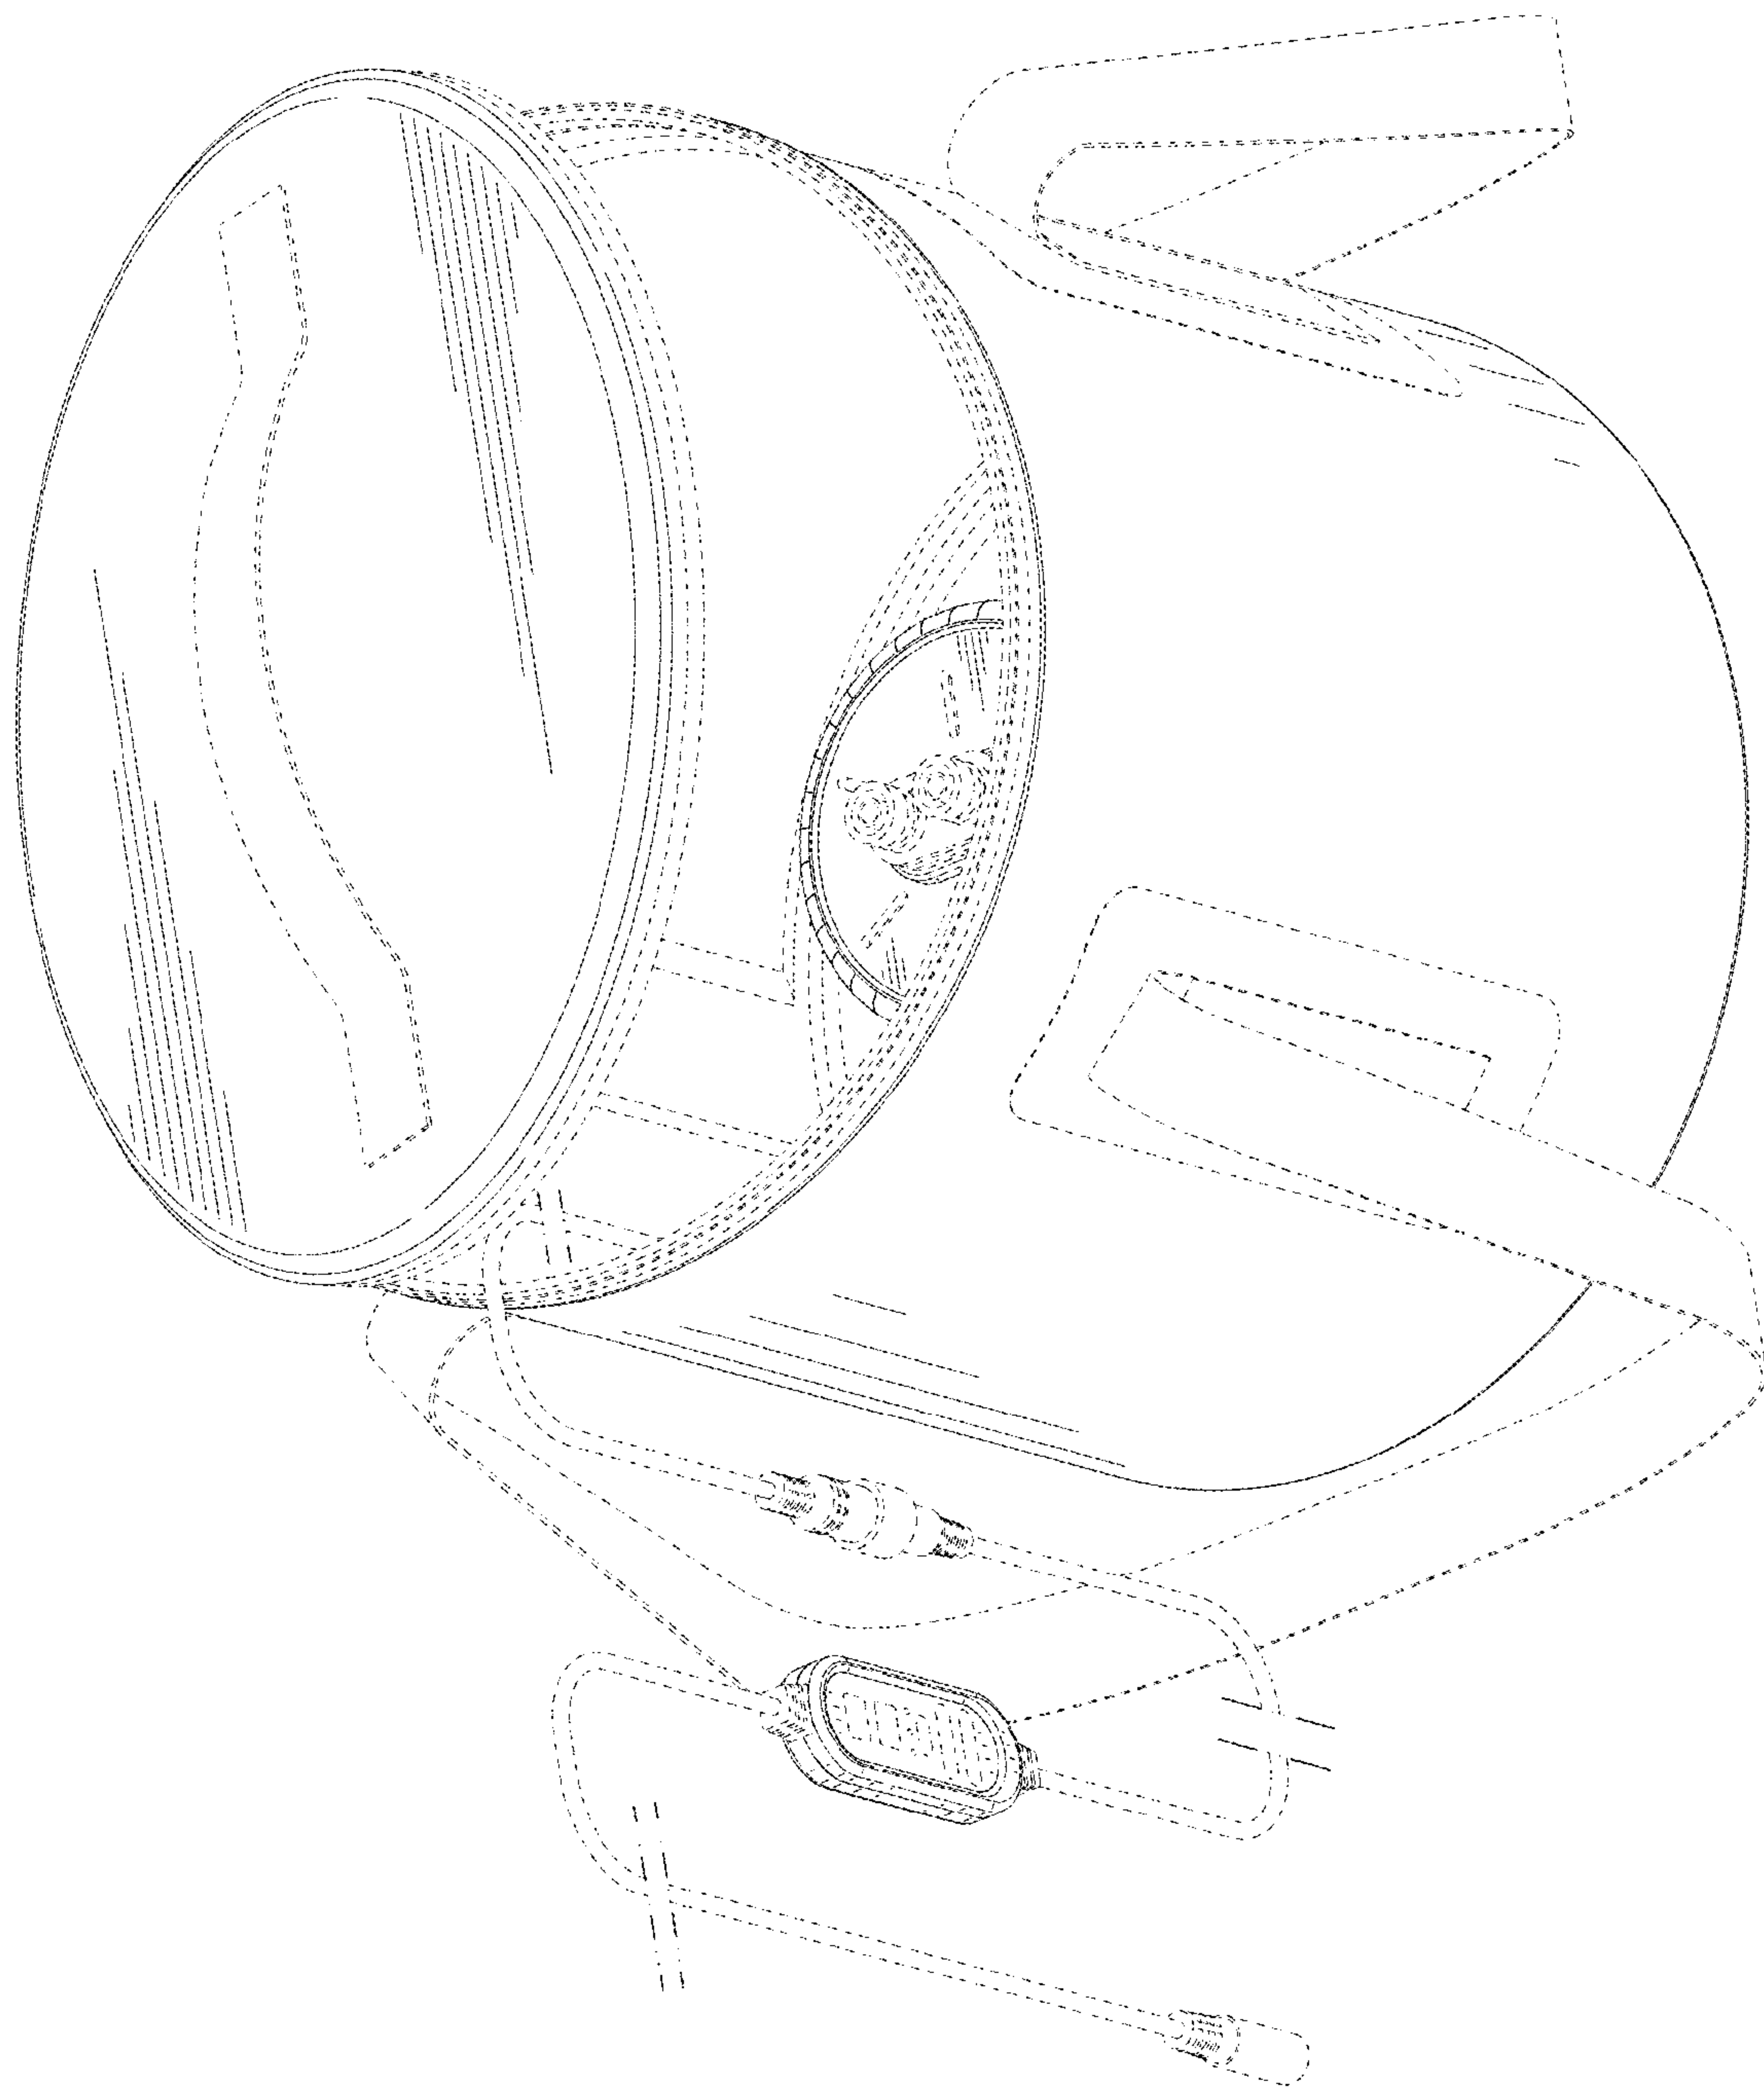


FIG. 17



FIG. 18