

(12) **United States Design Patent** (10) **Patent No.: US D1,082,842 S**
Lacombe et al. (45) **Date of Patent: ** Jul. 8, 2025**

(54) **DISPLAY SCREEN WITH TRANSITIONAL GRAPHICAL USER INTERFACE FOR MEDICAL IMAGING EQUIPMENT**

(71) Applicant: **Mauna Kea Technologies**, Paris (FR)

(72) Inventors: **Francois Lacombe**, Chaville (FR);
Margery Rothenberg, Suffern, NY (US)

(73) Assignee: **Mauna Kea Technologies**, Paris (FR)

(**) Term: **15 Years**

(21) Appl. No.: **29/923,563**

(22) Filed: **Dec. 29, 2023**

(51) **LOC (15) Cl.** **14-04**

(52) **U.S. Cl.**
USPC **D14/486**

(58) **Field of Classification Search**

USPC D14/485–495
CPC G06F 3/048; G06Q 30/00; G06Q 30/02;
H03J 1/00; H04N 5/00; H04N 5/08;
H04N 5/14; H04N 5/222; H04N 5/232;
H04N 5/445; H04N 5/45; H04N 21/00;
H04N 21/234; H04N 21/431; H04N
21/4532; H04N 21/4622; H04N 21/47;
H04N 21/482; H04N 21/485; H04N
21/488; H04N 21/6547

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D900,862 S * 11/2020 Wajda D14/488
D915,449 S * 4/2021 Menninger D14/488
D926,811 S * 8/2021 Murphy D14/488

(Continued)

FOREIGN PATENT DOCUMENTS

JP D1700677 * 11/2021
JP D1787669 * 12/2021

(Continued)

OTHER PUBLICATIONS

Sciencewerke, posted date unavailable [online], [retrieved Feb. 27, 2025]. Retrieved from internet, <https://www.sciencewerke.com/cellvizio-lab-vietnam>. (Year: 2025).*

(Continued)

Primary Examiner — Cary M Robinson

Assistant Examiner — Michelle Devlin

(74) *Attorney, Agent, or Firm* — Osha Bergman Watanabe & Burton LLP

(57) **CLAIM**

The ornamental design for a display screen with transitional graphical user interface for medical imaging equipment as shown and described.

DESCRIPTION

FIG. 1 is a first front view showing a display screen of a display screen with transitional graphical user interface for medical imaging equipment showing a first image in the sequence;

FIG. 2 is a second image thereof;

FIG. 3 is a third image thereof;


FIG. 4 is a fourth image thereof; and,

FIG. 5 is a fifth image thereof.

The outermost broken lines depict a display screen with transitional graphical user interface for medical imaging equipment in which the design is embodied that forms no part of the claimed design. The remaining broken lines illustrate portions of the graphical user interface that form no part of the claimed design.

The subject matter in this patent application includes a process or period in which an image changes into another image. This process or period forms no part of the claimed design.

1 Claim, 5 Drawing Sheets

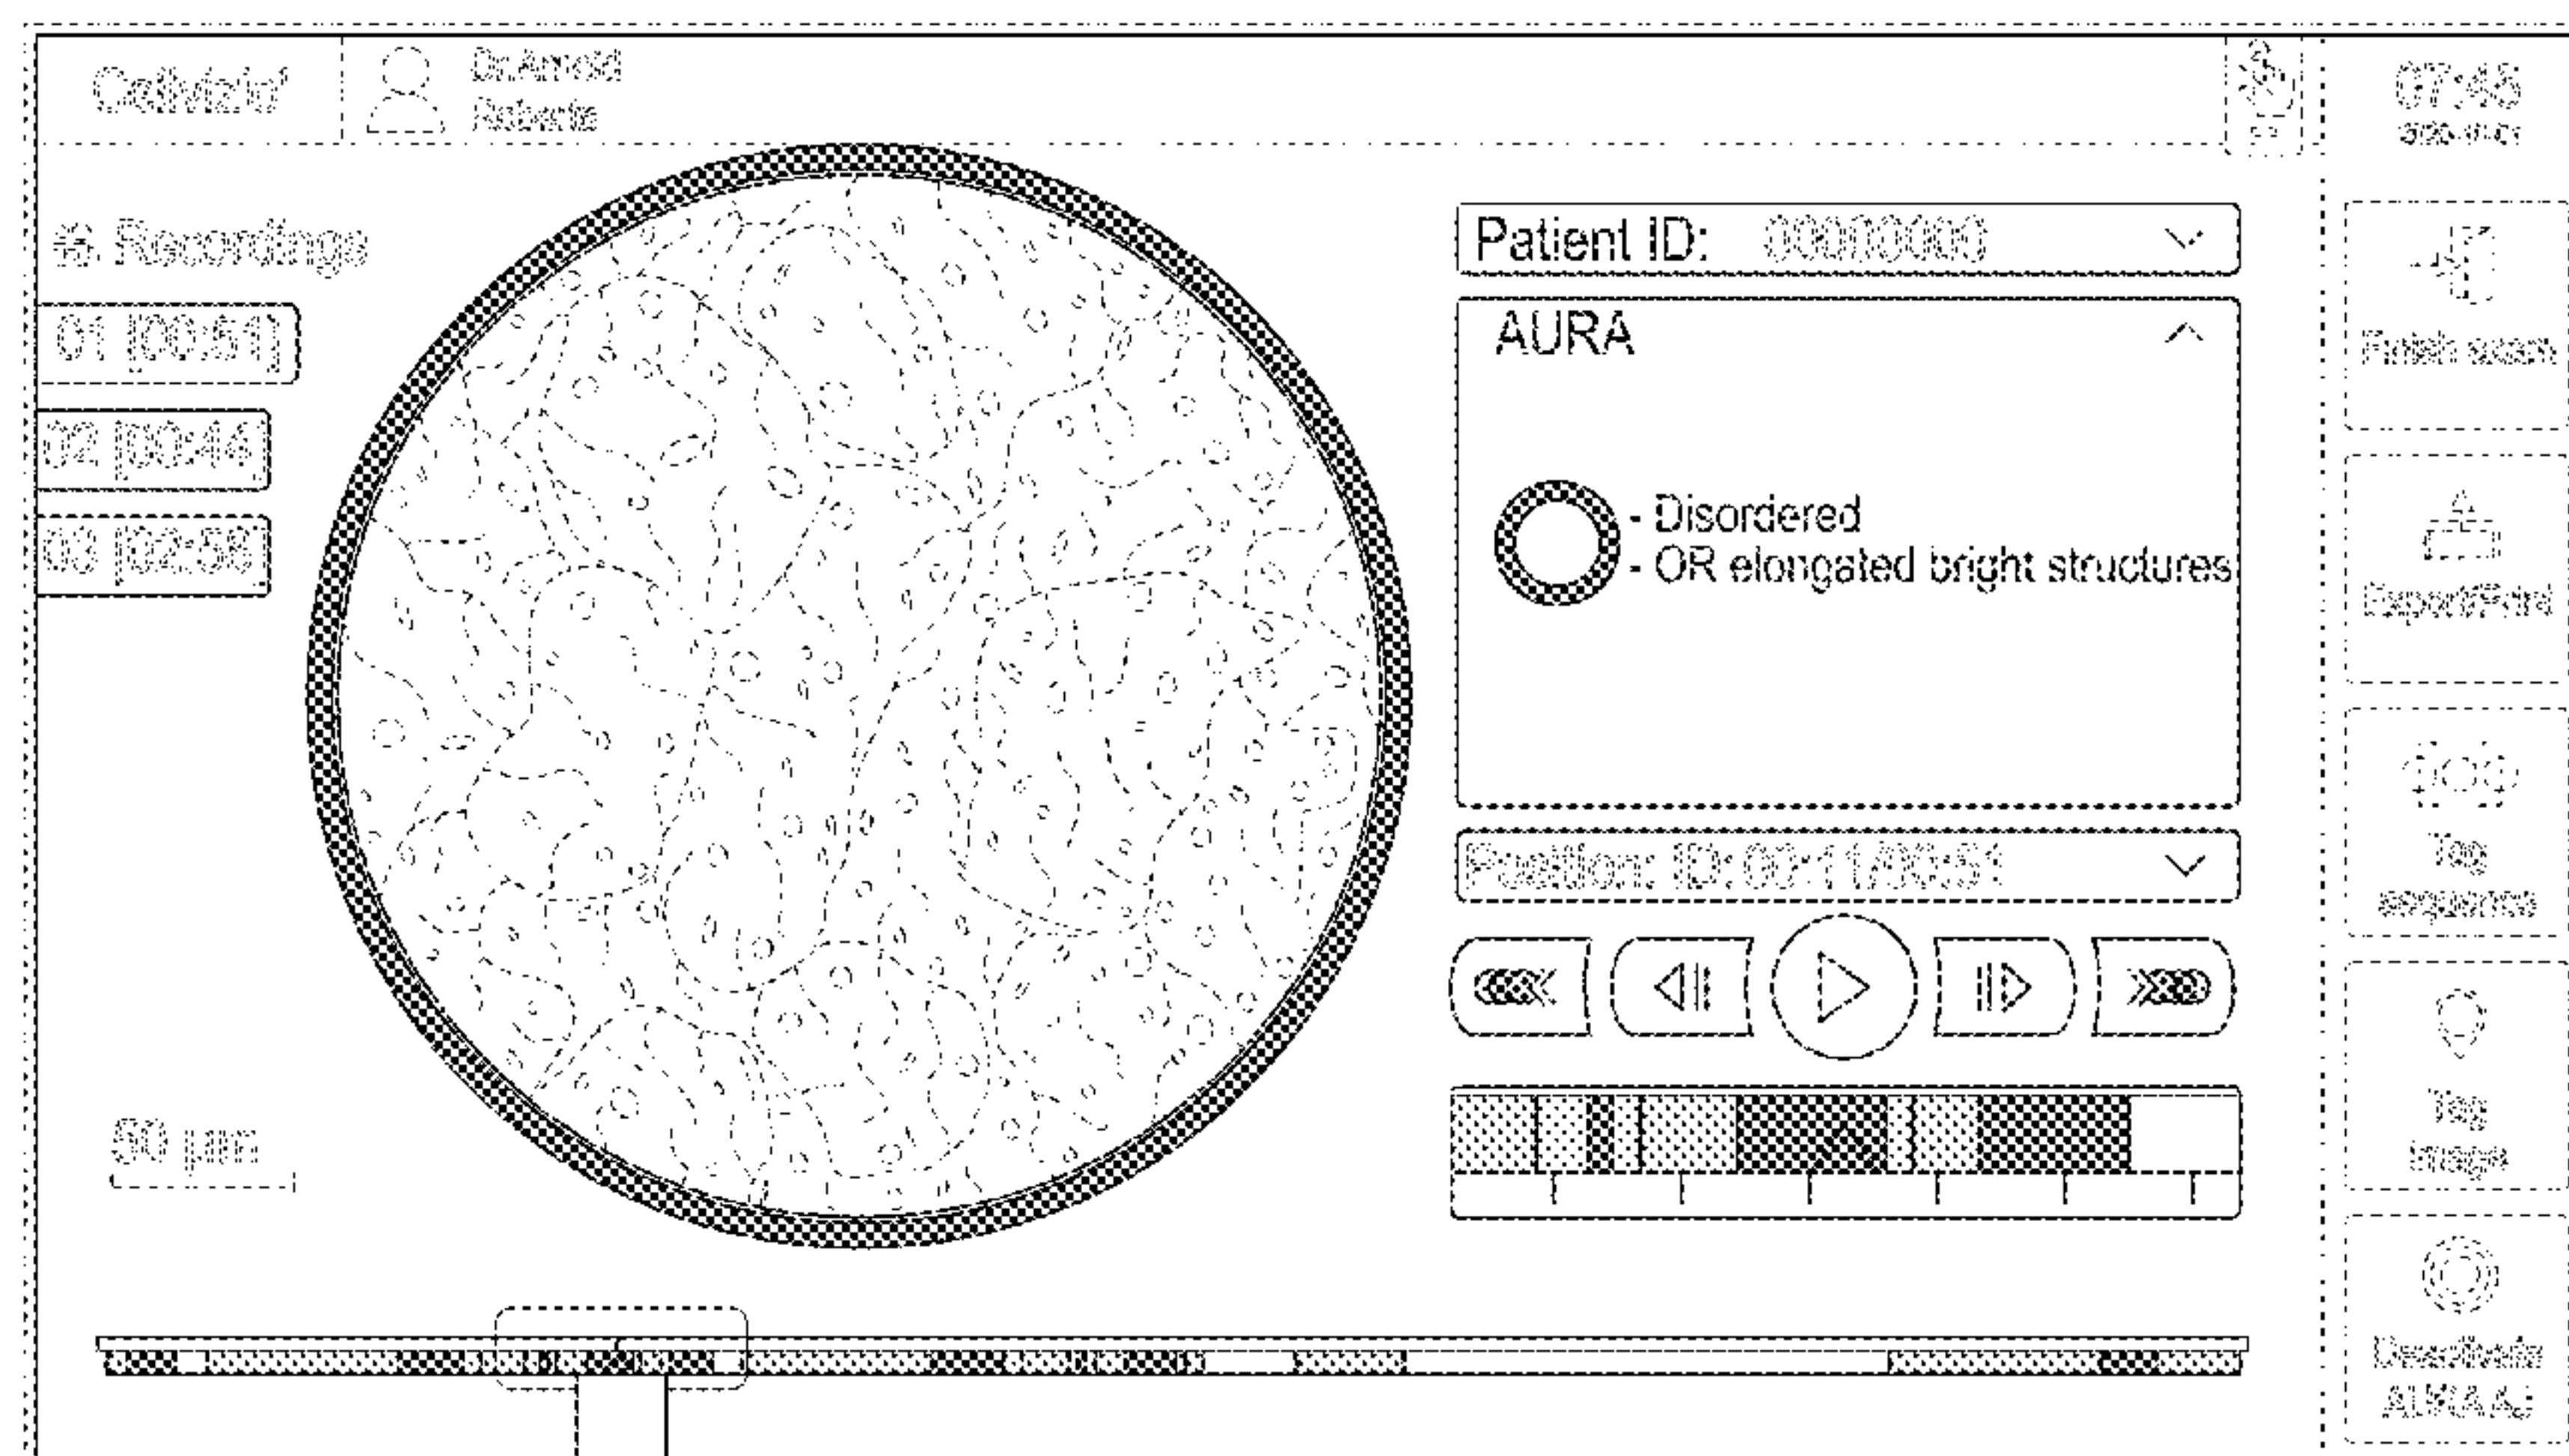

(56) **References Cited**

U.S. PATENT DOCUMENTS

D931,316 S * 9/2021 Miriyala D14/488
D932,500 S * 10/2021 Van Gerbig D14/485
D934,892 S * 11/2021 Hershkovich D14/486
D946,021 S * 3/2022 Drole D14/491
11,429,247 B1 * 8/2022 Qian G06F 3/04845
D1,057,759 S * 1/2025 Lacombe D14/486
2019/0339850 A1 * 11/2019 Ho A61B 5/0066
2021/0068649 A1 * 3/2021 Uemura G06T 7/38
2023/0016097 A1 * 1/2023 Whisler G06F 3/04845
2024/0272415 A1 * 8/2024 Dias G06F 3/0482

FOREIGN PATENT DOCUMENTS

JP D1731421 * 12/2022
JP D1772448 * 6/2024


OTHER PUBLICATIONS

Cellvizio® Overview, posted date unavailable [online], [retrieved Feb. 27, 2025]. Retrieved from internet, <https://www.maunakeatech.com/cellvizio-overview/>. (Year: 2025).*

Real-Time in Vivo Cellular Imaging Platform, posted date unavailable [online], [retrieved Feb. 27, 2025]. Retrieved from internet, https://www.maunakeatech.com/wp-content/uploads/2024/07/MKT-201-EN-Next-Gen_Cellvizio_Product_Overview.pdf. (Year: 2025).*

Confocal Laser Endomicroscopy, posted date unavailable [online], [retrieved Feb. 27, 2025]. Retrieved from internet, <https://www.olivineinternational.com/wp-content/uploads/2021/01/MKT-132-EN-Cellvizio-Web-Brochure.pdf>. (Year: 2025).*

* cited by examiner

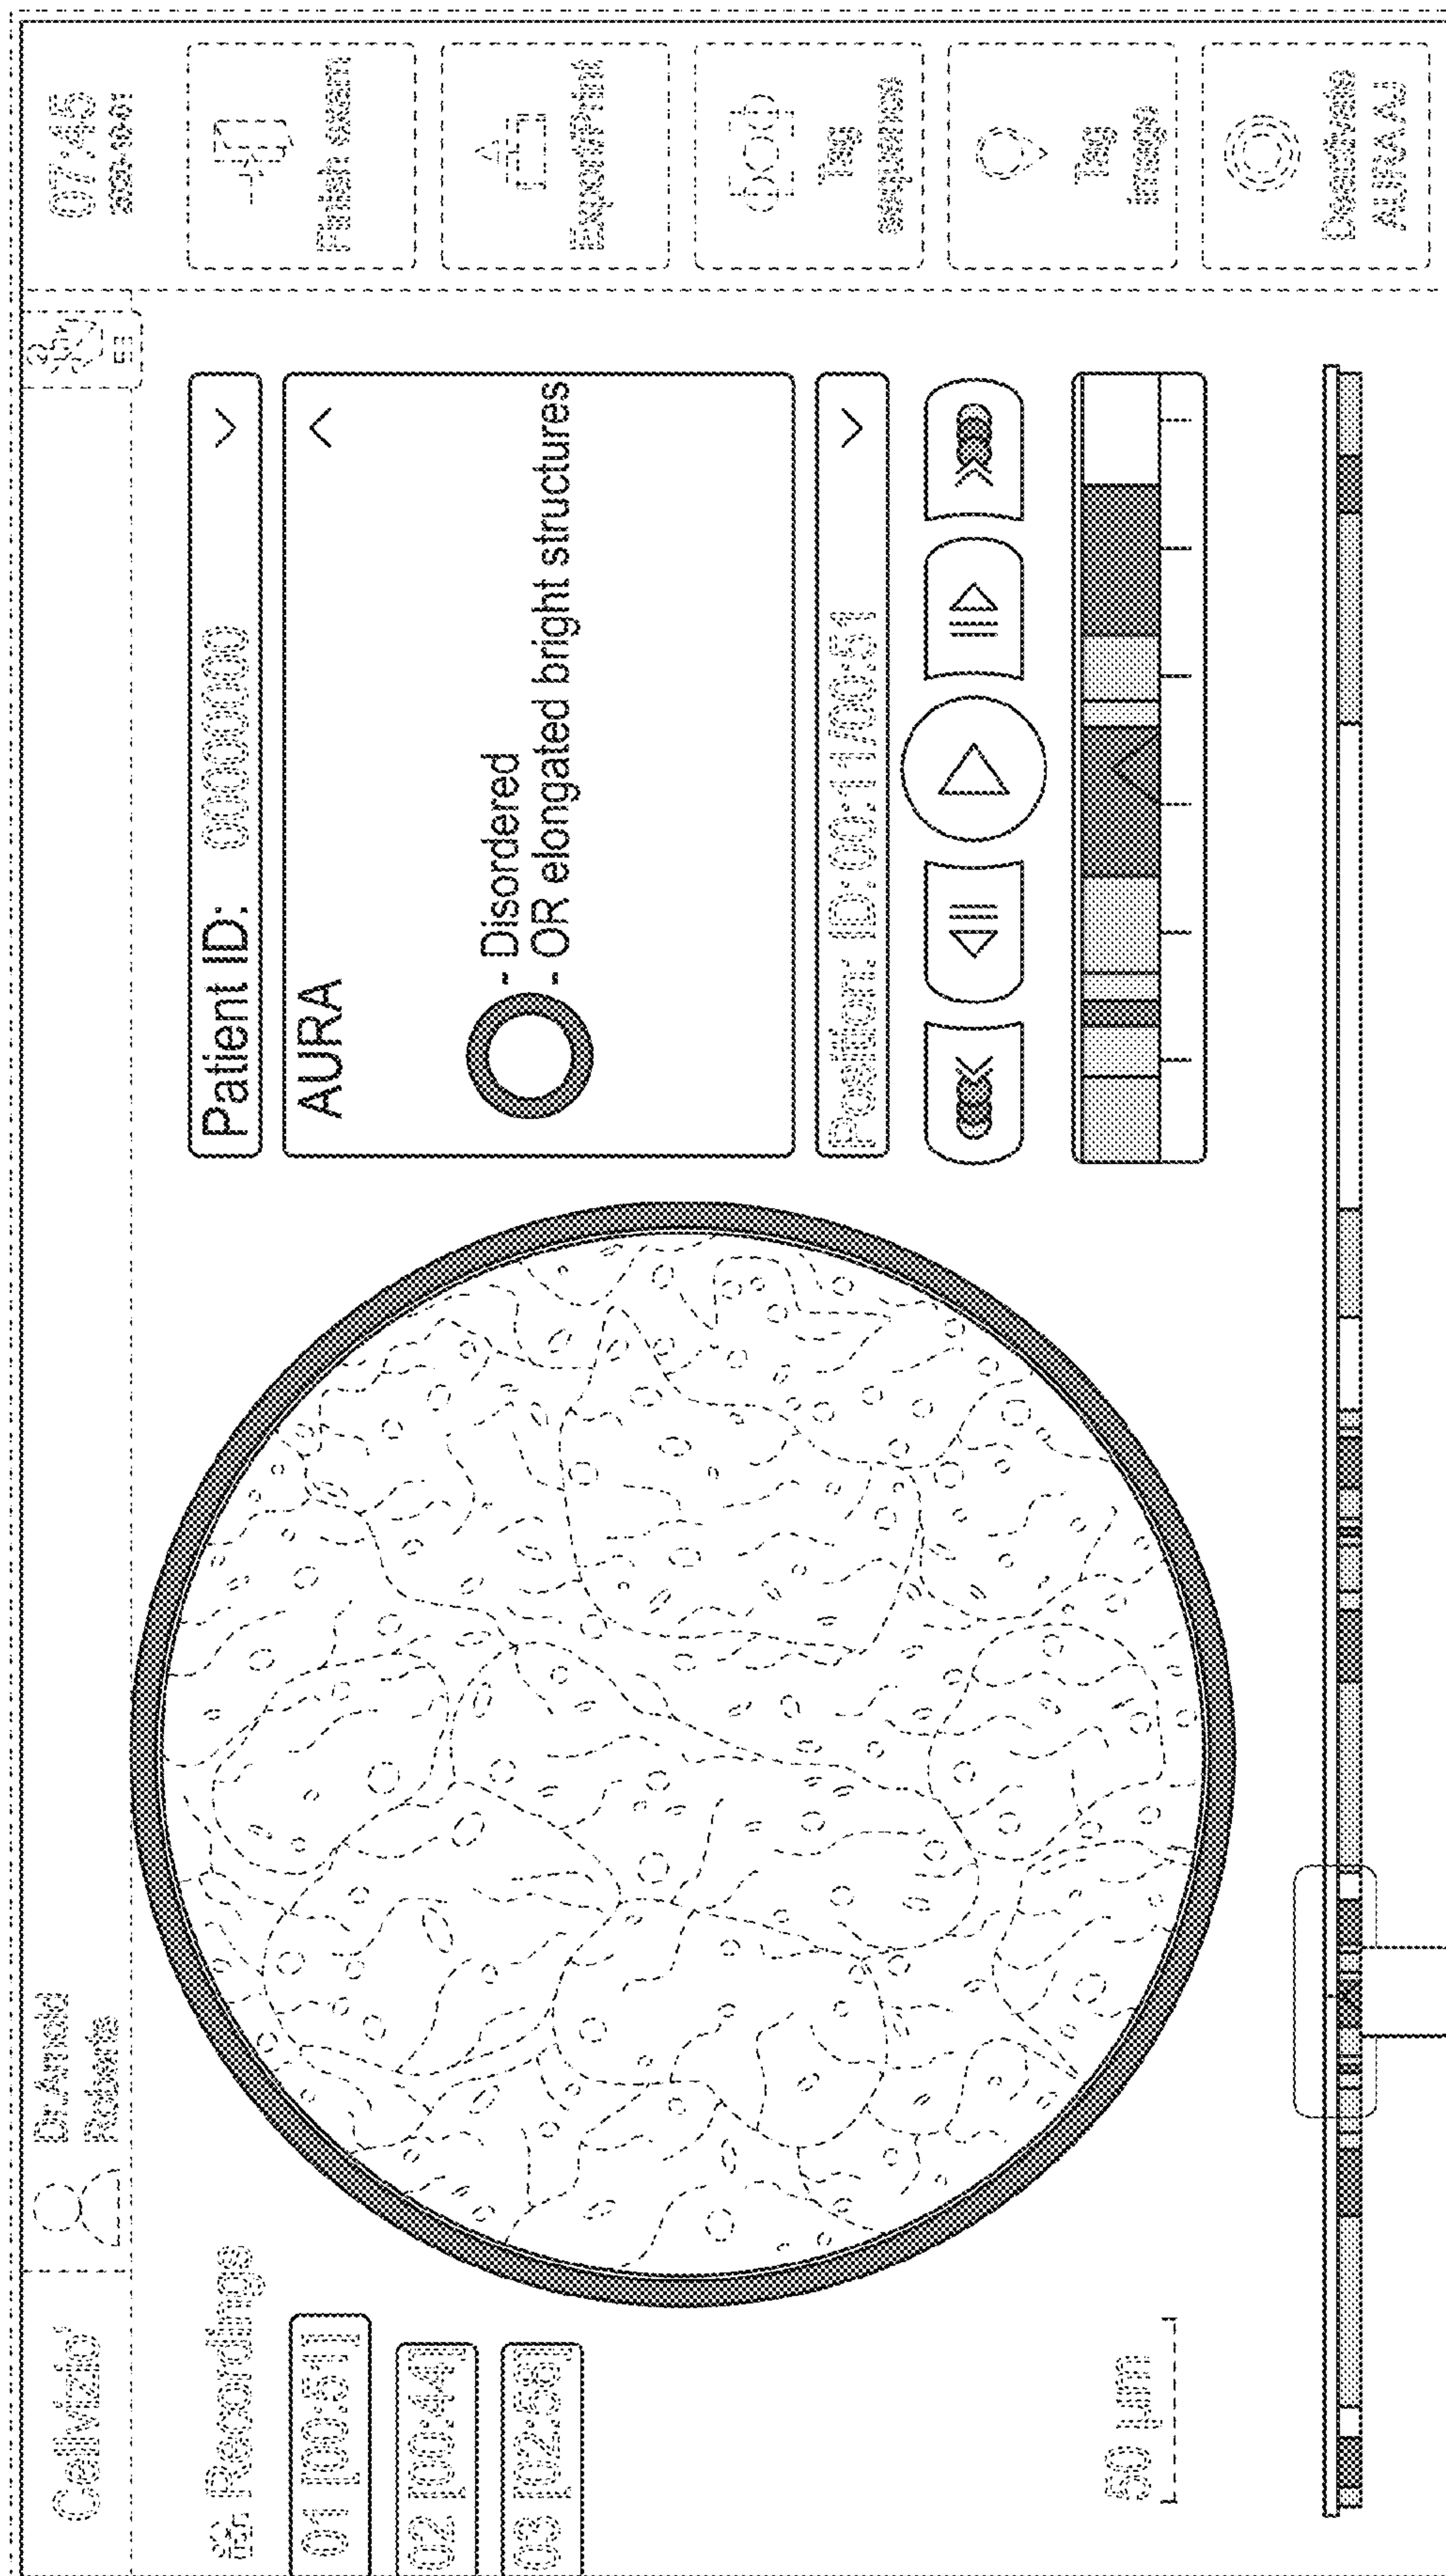

ॐ
ॐ
ॐ
ॐ
ॐ

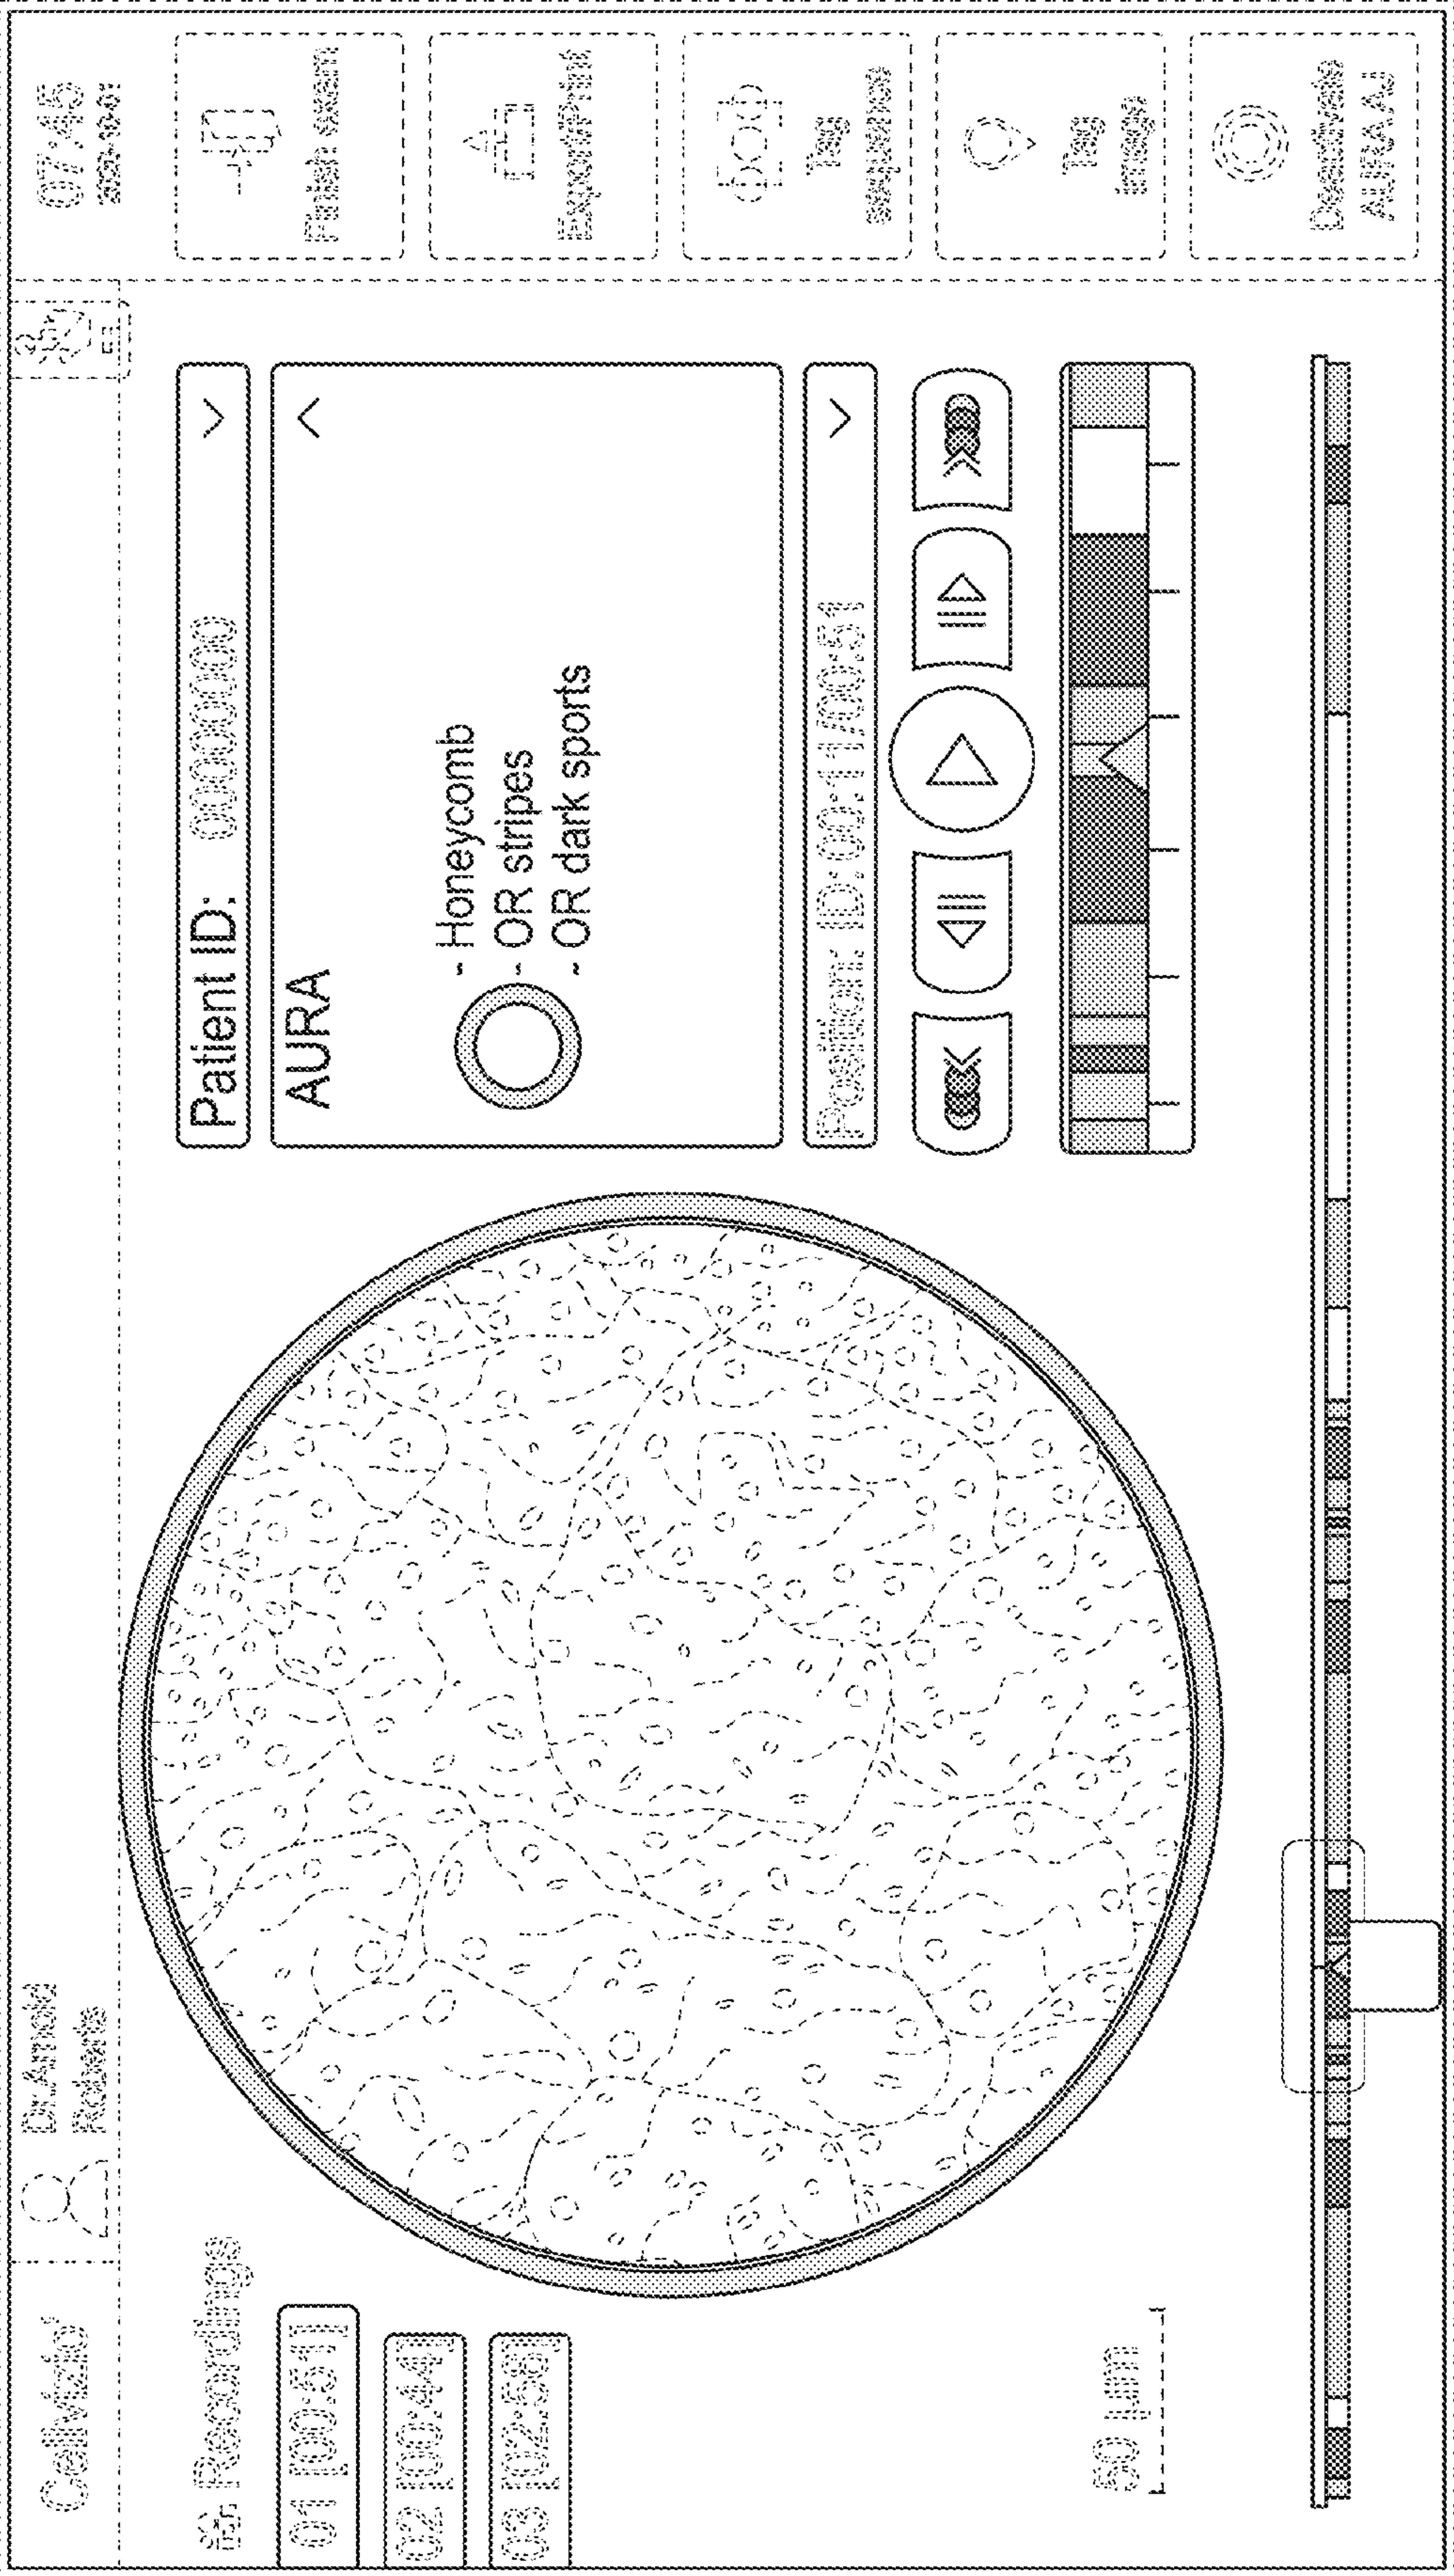


FIG. 2

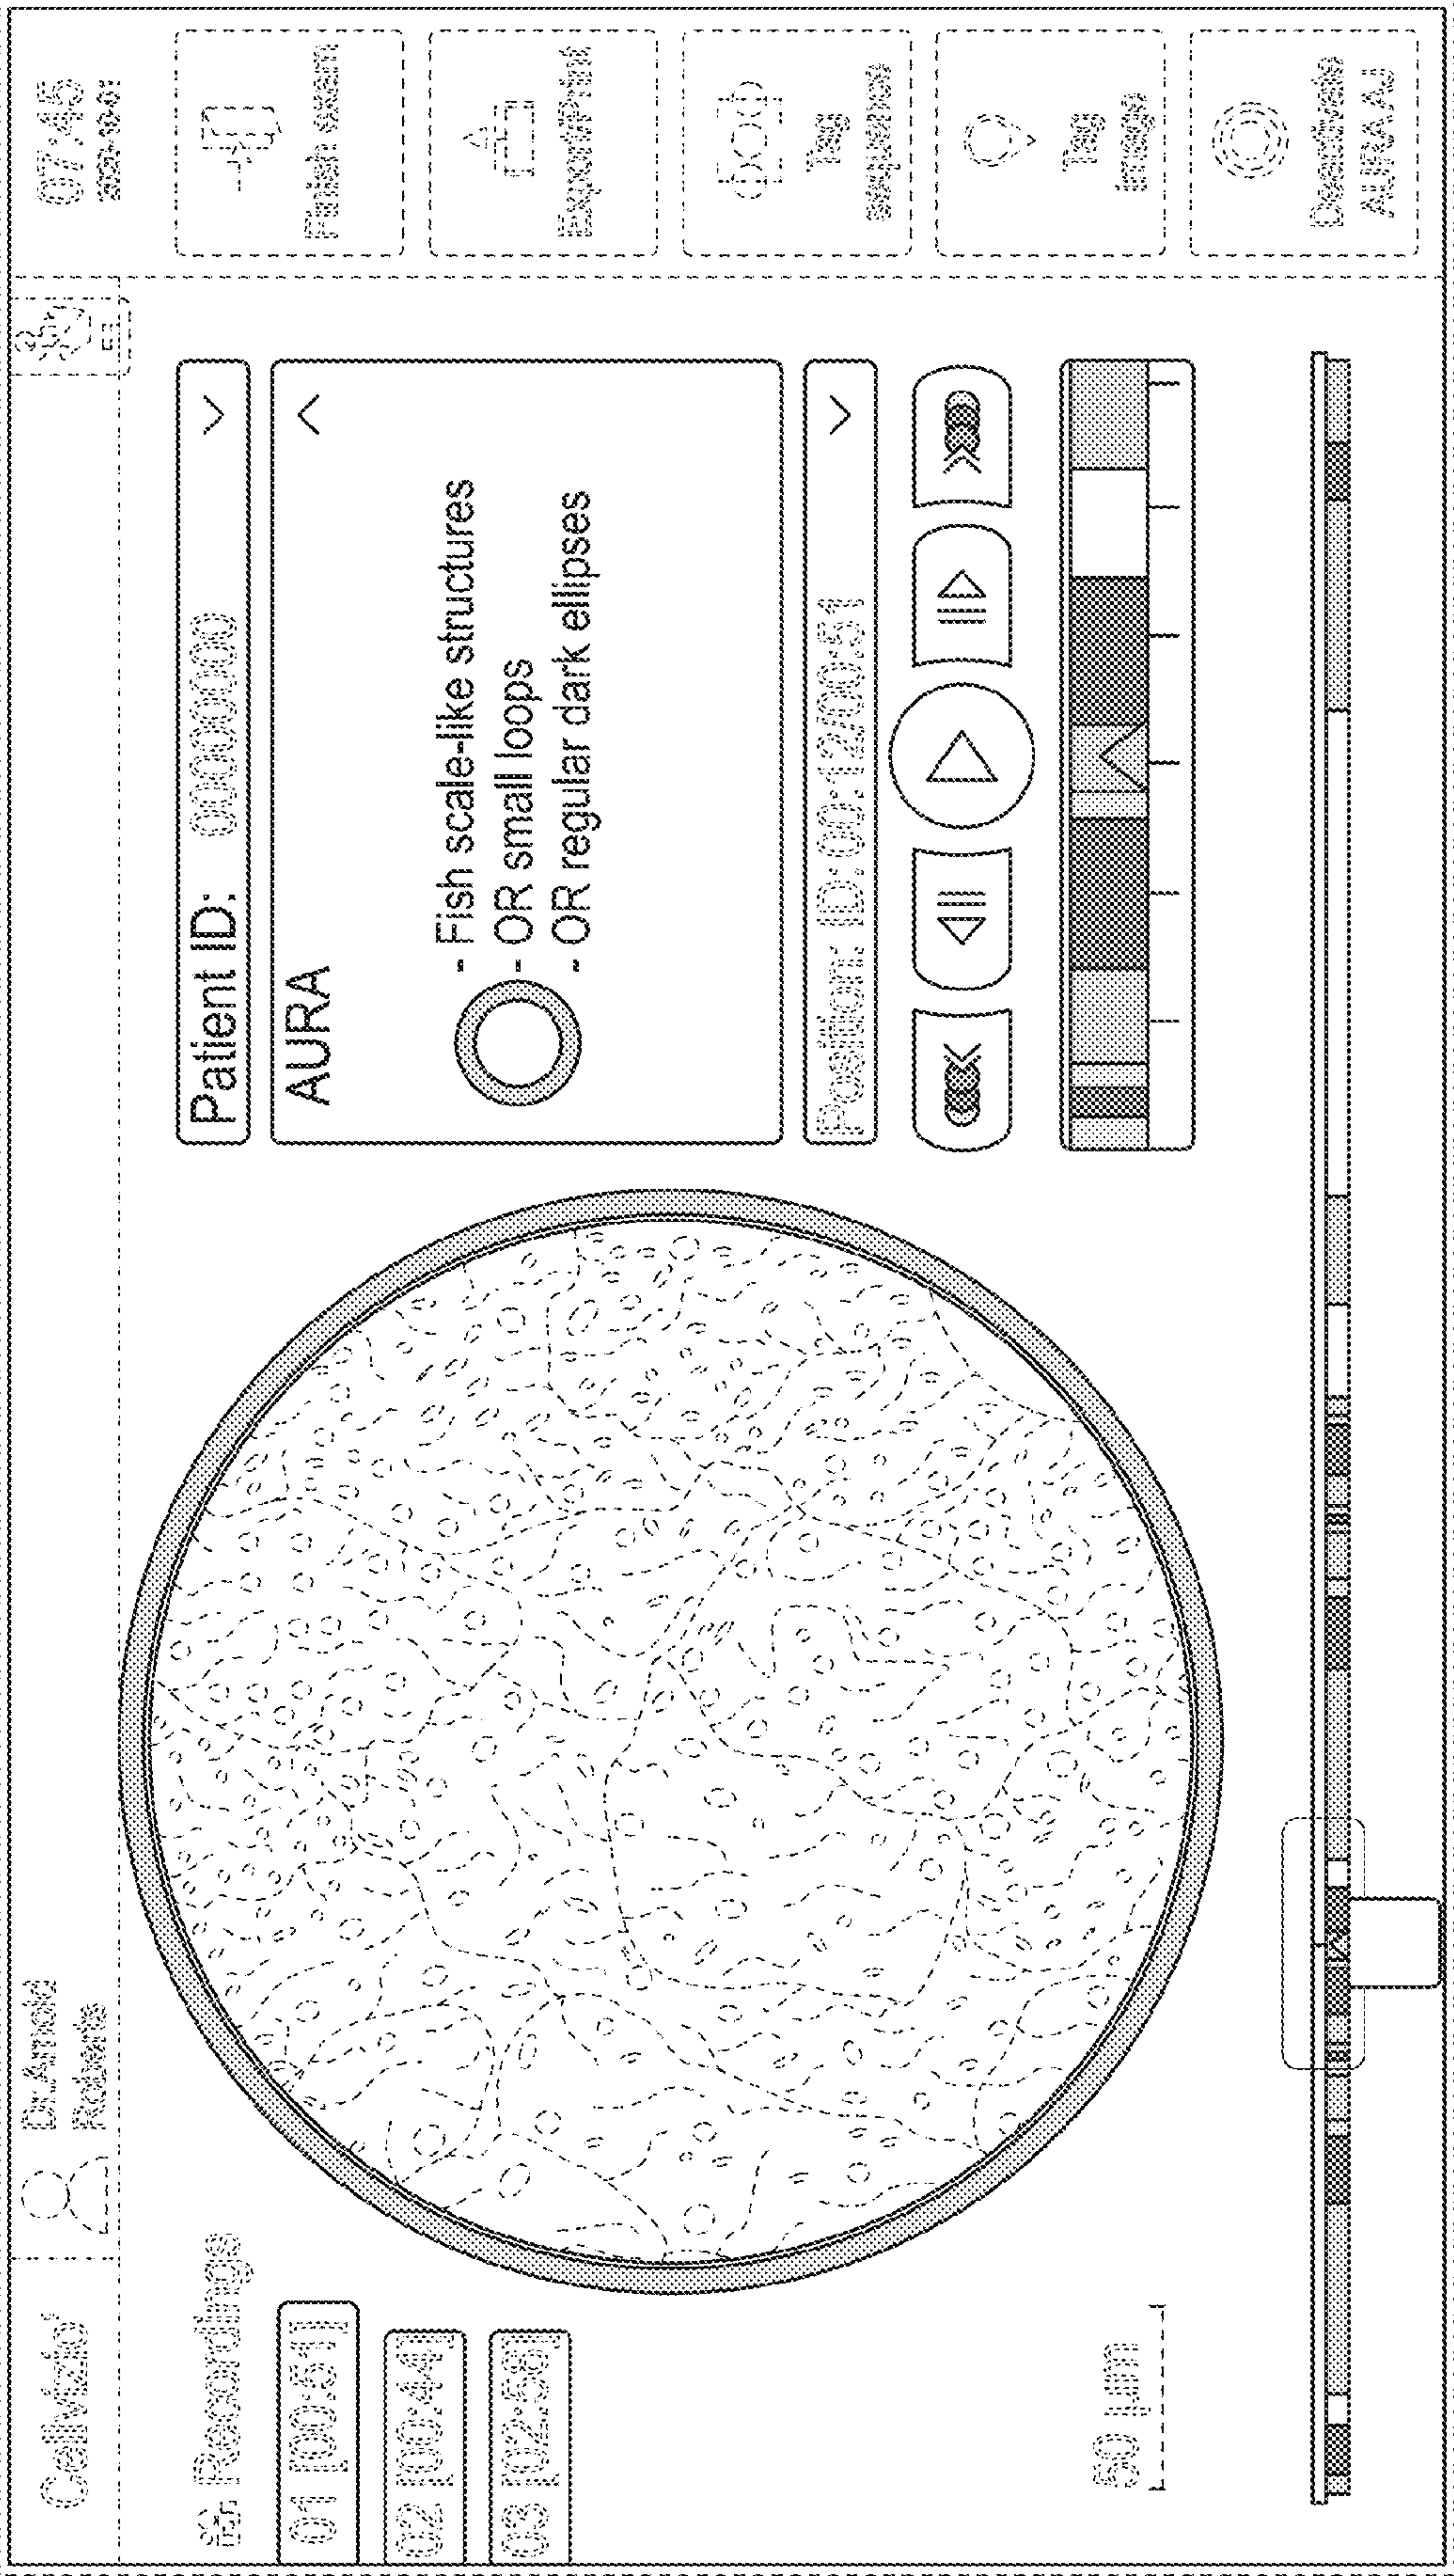


FIG. 3

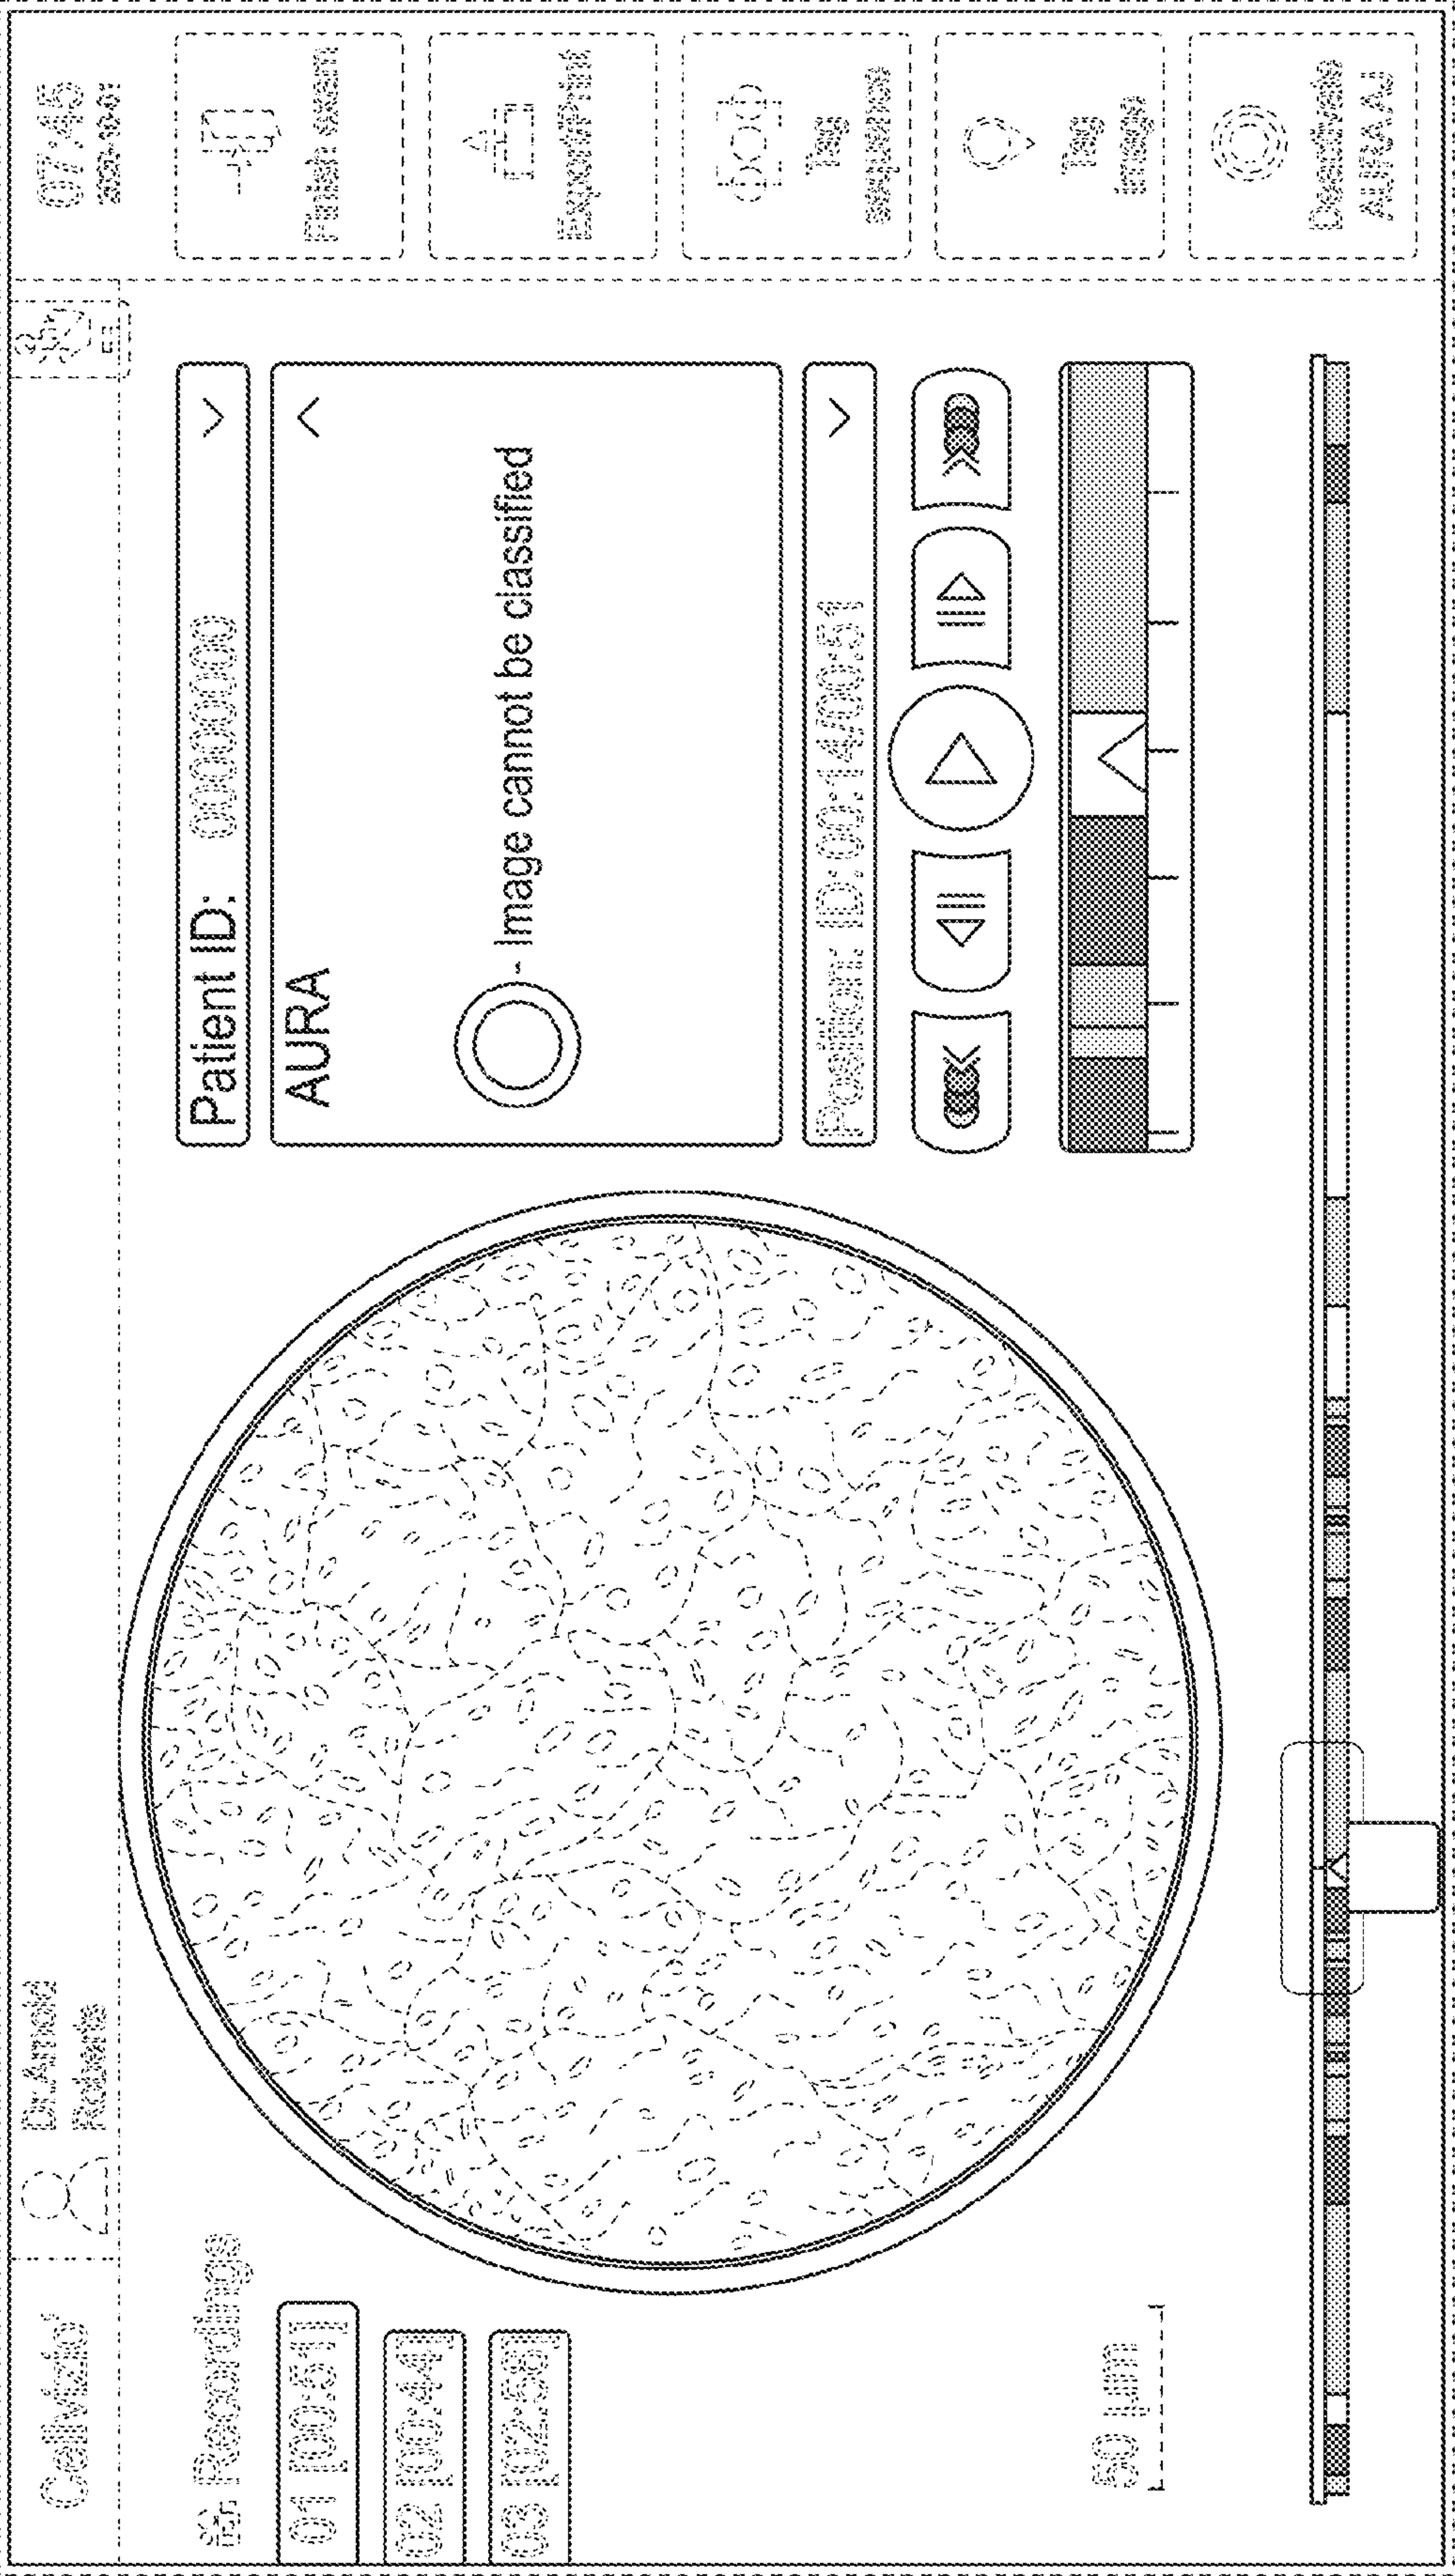


FIG. 4

