



US0D1094729S

(12)

United States Design Patent

Dijkstra et al.

(10)

Patent No.:

US D1,094,729 S

(45)

Date of Patent:

\*\* Sep. 23, 2025

(54) THERAPY PATCH CONTROLLER

(71) Applicant: SHENZHEN KAIYAN MEDICAL EQUIPMENT CO., LTD, Shenzhen (CN)

(72) Inventors: Alain Dijkstra, Amstelveen (NL); Li Xiang, Shenzhen (CN); Wen Caiyun, Shenzhen (CN)

(\*\*) Term: 15 Years

(21) Appl. No.: 29/920,938

(22) Filed: Dec. 14, 2023

(51) LOC (15) Cl. 24-01

(52) U.S. Cl. USPC D24/209; D24/189

(58) Field of Classification Search USPC D24/158, 172, 187, 188, 189, 190, 191, D24/192, 200, 206, 209 CPC A61B 5/6833; A61B 5/68335; A61B 5/6832; A61B 8/4236; A61B 2505/05; A61B 2562/0271; A61B 5/688; A61B 5/257; A61F 9/04; A61F 13/124; A61F 2013/00497; A61F 2007/0004 See application file for complete search history.

(56) References Cited

U.S. PATENT DOCUMENTS

|          |   |   |        |               |         |
|----------|---|---|--------|---------------|---------|
| D733,900 | S | * | 7/2015 | Hagege        | D24/200 |
| D878,608 | S |   | 3/2020 | Tapper et al. |         |
| D944,450 | S |   | 2/2022 | Ritter et al. |         |
| D957,660 | S | * | 7/2022 | Johnson       | D24/209 |
| D986,290 | S | * | 5/2023 | Solana        | D15/7   |

(Continued)

FOREIGN PATENT DOCUMENTS

|    |           |   |        |
|----|-----------|---|--------|
| CN | 307833351 | * | 2/2023 |
| CN | 309149596 | * | 3/2025 |

OTHER PUBLICATIONS

“Hooga: Hooga Dot.” Found online Mar. 25, 2025 at hoogahealth.com. Reference dated Jun. 7, 2023. Retrieved from https://hoogahealth.com/products/red-light-therapy-dot.\*

(Continued)

Primary Examiner — Kendra Leslie Hamilton  
Assistant Examiner — Elizabeth S Struble  
(74) Attorney, Agent, or Firm — Willie Jacques; Emanus LLC

(57) CLAIM


The ornamental design for a therapy patch controller, as shown and described.

DESCRIPTION

FIG. 1 is a top perspective view of a therapy patch controller, showing our new design;  
FIG. 2 is a bottom perspective view thereof;  
FIG. 3 is a front elevation view thereof;  
FIG. 4 is a rear elevation view thereof;  
FIG. 5 is a left side elevation view thereof;  
FIG. 6 is a right side elevation view thereof;  
FIG. 7 is a top plan view thereof;  
FIG. 8 is a bottom plan view thereof;  
FIG. 9 is a top perspective view of the therapy patch controller of FIG. 1, shown in a first condition of use for clarity of disclosure;  
FIG. 10 is a top perspective view of the therapy patch controller of FIG. 1, shown in a second condition of use for clarity of disclosure; and,  
FIG. 11 is a top plan view of the therapy patch controller of FIG. 1, shown in a third configuration of use on a human face.

In the drawings, the equal-length broken lines depict portions of the therapy patch controller and form no part of the claimed design. The broken lines showing of a patch and human face in FIGS. 9, 10 and 11 depict environmental structure and form no part of the claimed design. All broken lines form no part of the claim.

1 Claim, 11 Drawing Sheets

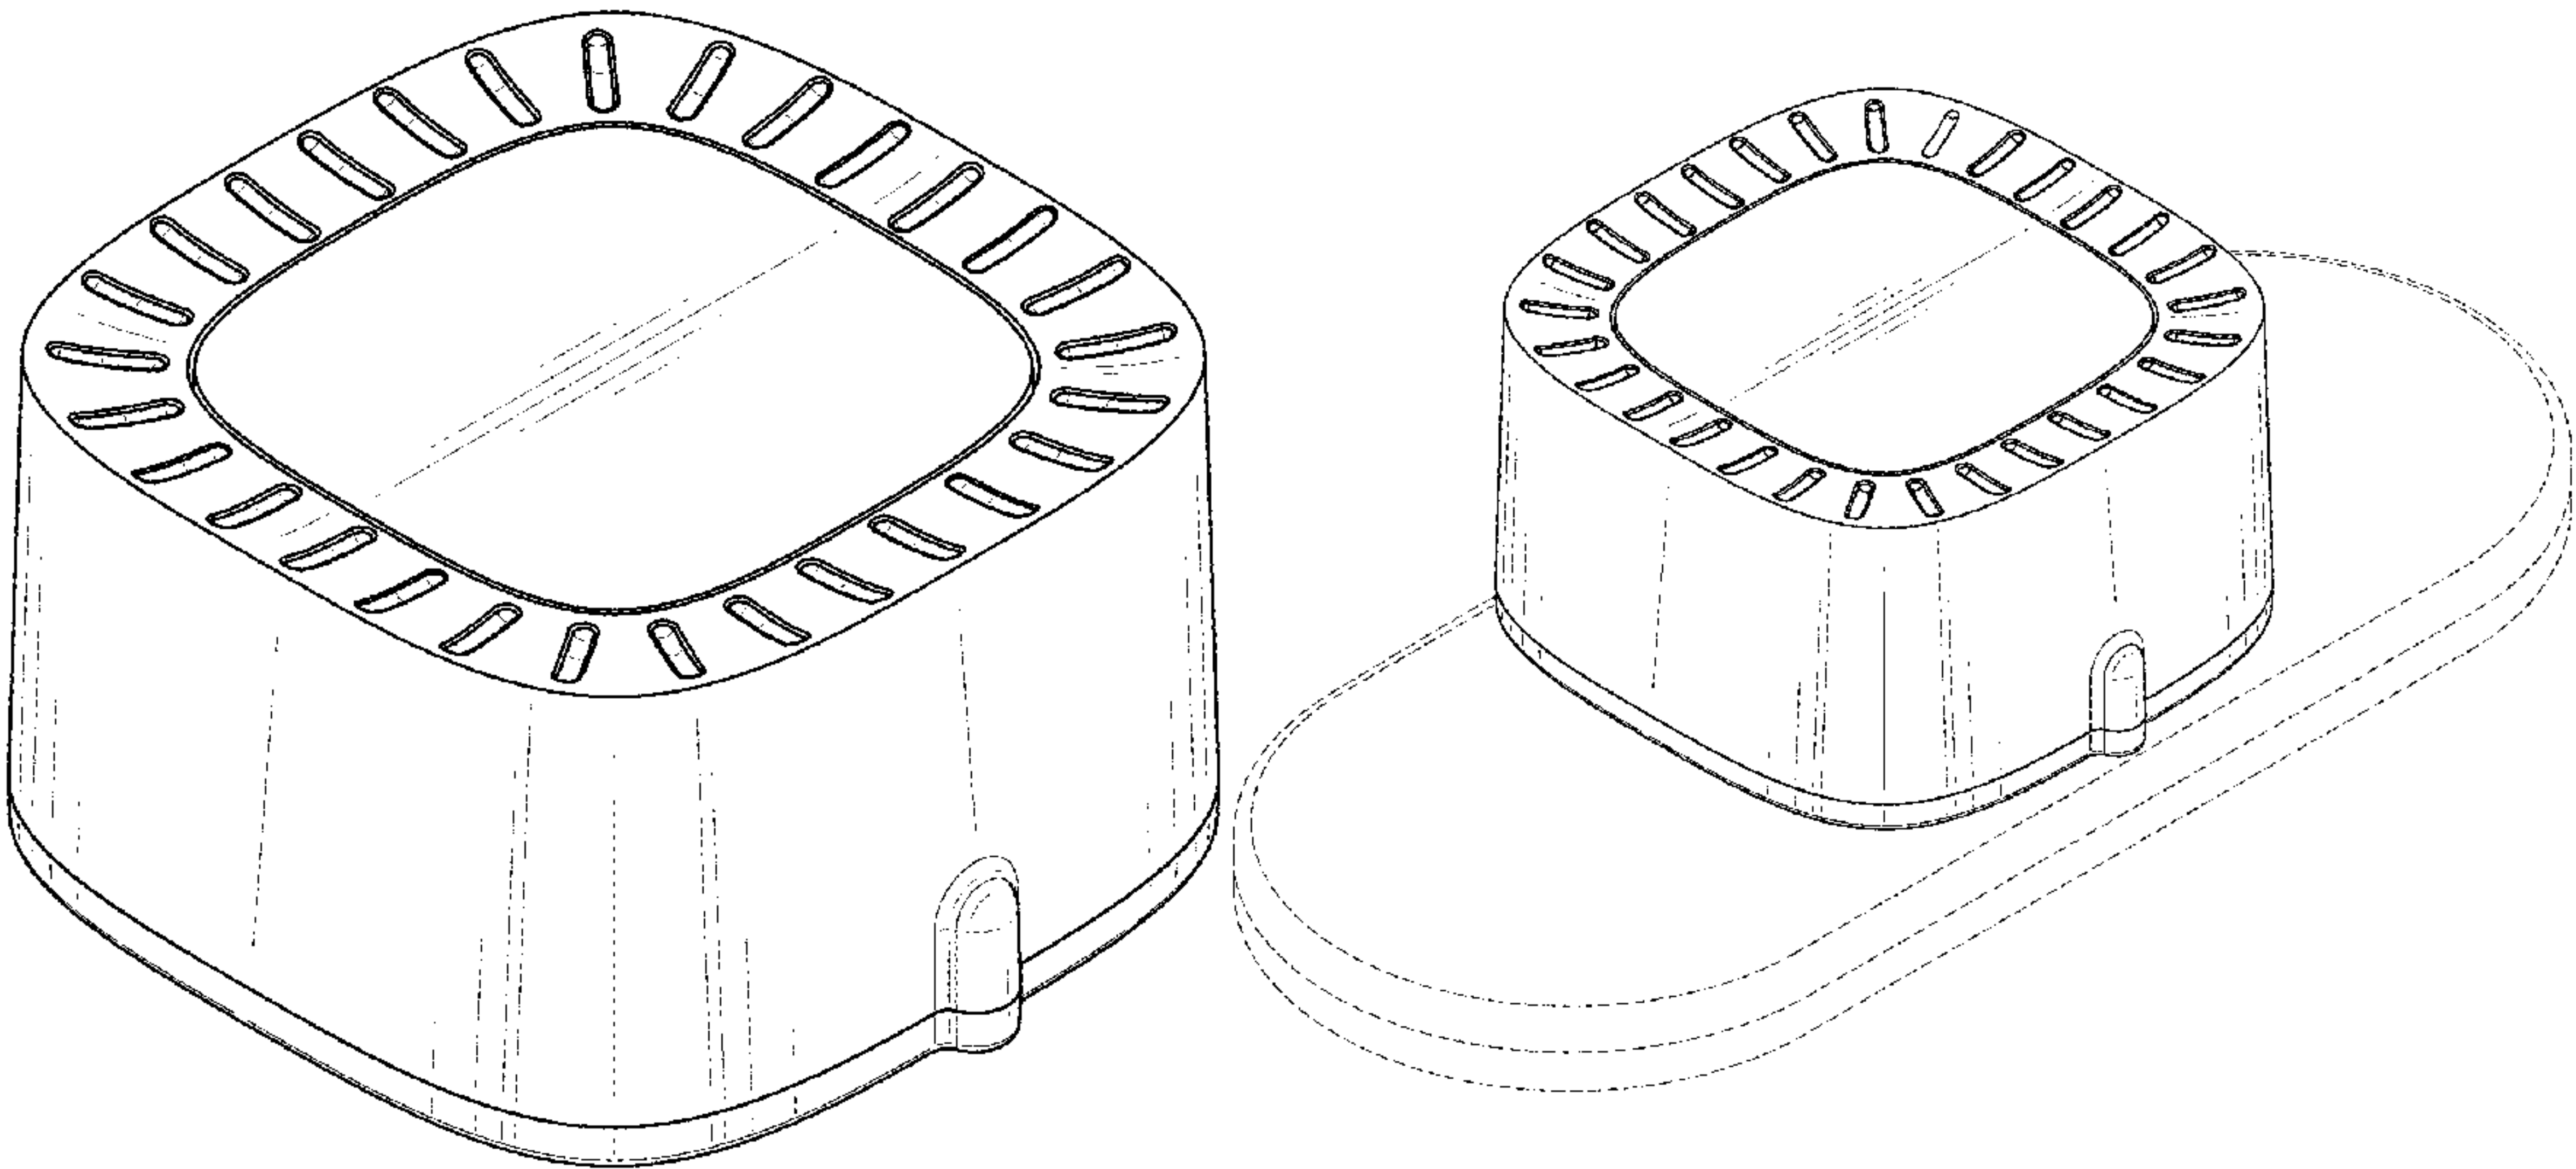

(56)                      **References Cited**

U.S. PATENT DOCUMENTS

D1,002,860 S \* 10/2023 Kaiser ..... D24/209  
D1,027,307 S \* 5/2024 Xie ..... D24/209  
D1,043,665 S \* 9/2024 Barnett ..... D14/344  
D1,046,171 S \* 10/2024 MacGilp ..... D24/209  
D1,064,290 S \* 2/2025 Xiangjie ..... D24/187  
D1,066,686 S \* 3/2025 Ravikumar ..... D24/189  
D1,066,707 S \* 3/2025 Rudys ..... D24/209  
2019/0336326 A1 \* 11/2019 Dijkstra ..... A61F 7/007  
2024/0269478 A1 \* 8/2024 Dijkstra ..... A61N 1/0468  
2025/0018215 A1 \* 1/2025 Dijkstra ..... A61N 5/067

OTHER PUBLICATIONS

“Amzcool: Red Light Device.” Found online Mar. 25, 2025 at amazon.com. Reference dated Jun. 5, 2019. Retrieved from <https://www.amazon.com/Infrared-Reliever-Stepless-Portable-Rechargeable/dp/B07SQ9GFMJ/>. \*

“Celluma Home: LED Light Therapy for Anywhere on the Body.” Found online Mar. 25, 2025 at celluma.com. Reference dated Mar. 31, 2019. Retrieved from <https://www.celluma.com/products/celluma-home>. \*

“People: The 7 Best Red Light Therapy Devices, Tested by Real People.” Found online Mar. 25, 2025 at people.com. Reference dated Nov. 12, 2024. Retrieved from <https://people.com/light-therapy-at-home-7557886>. \*

\* cited by examiner

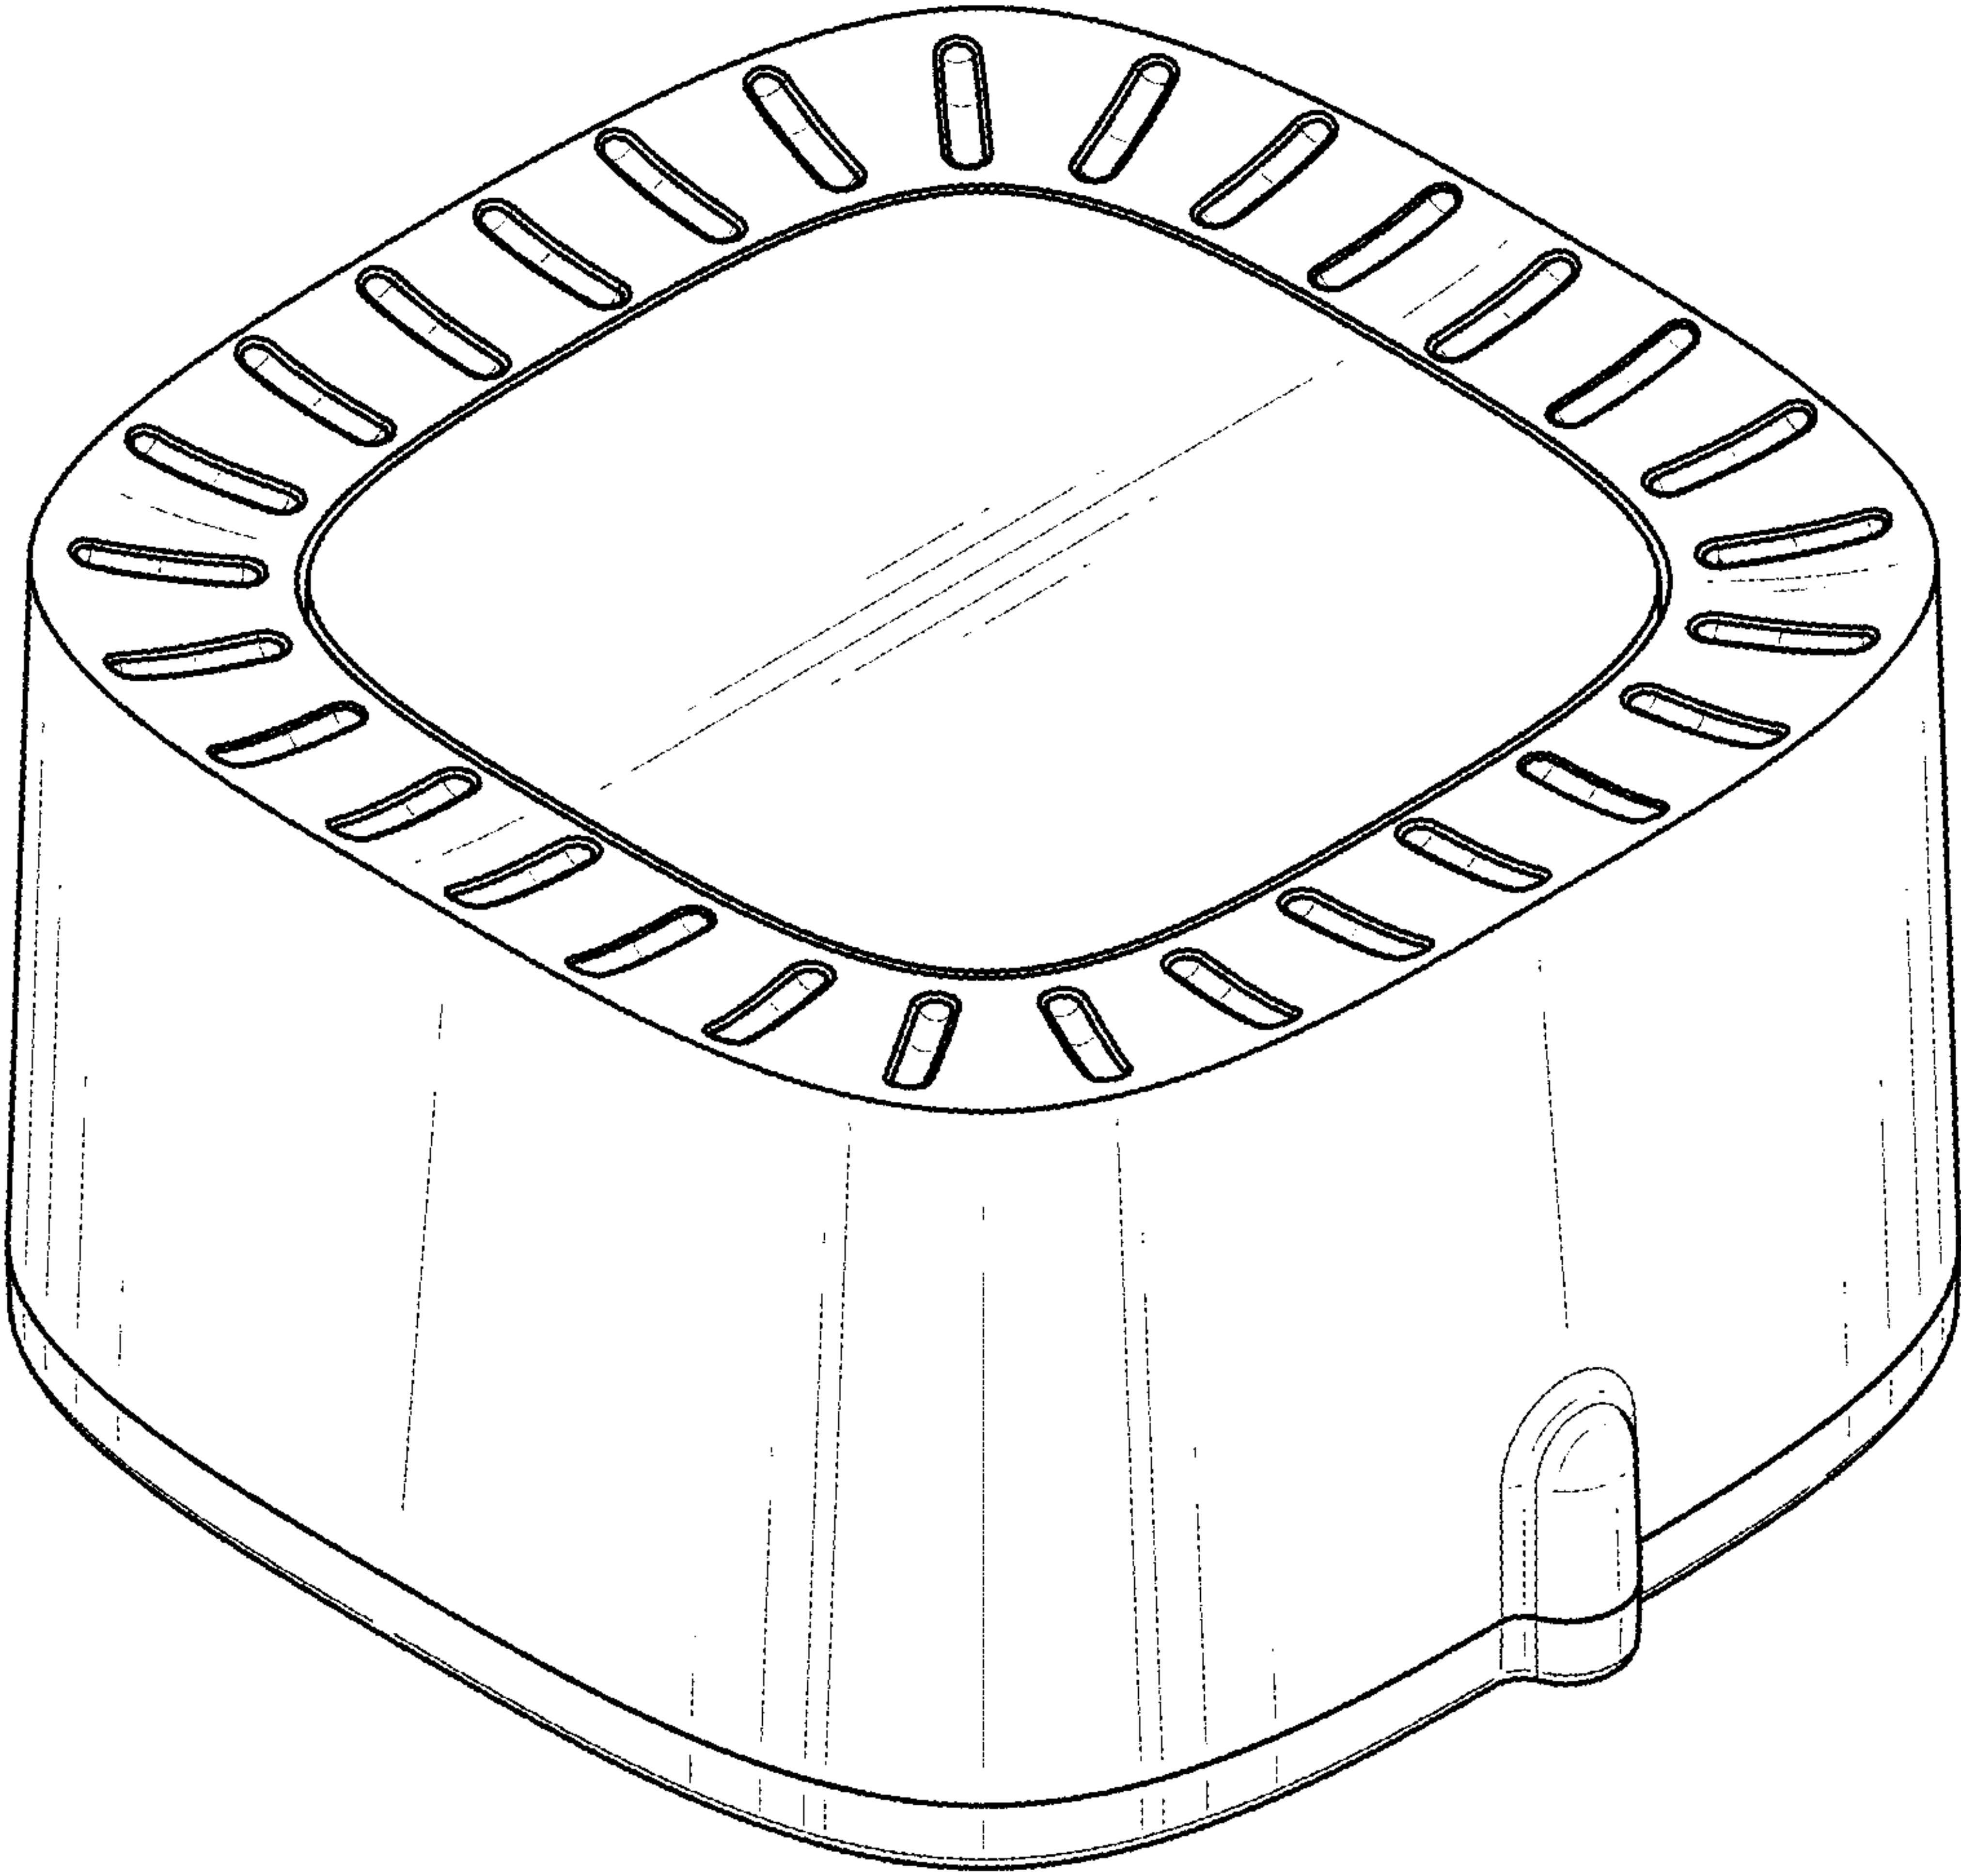


FIG. 1

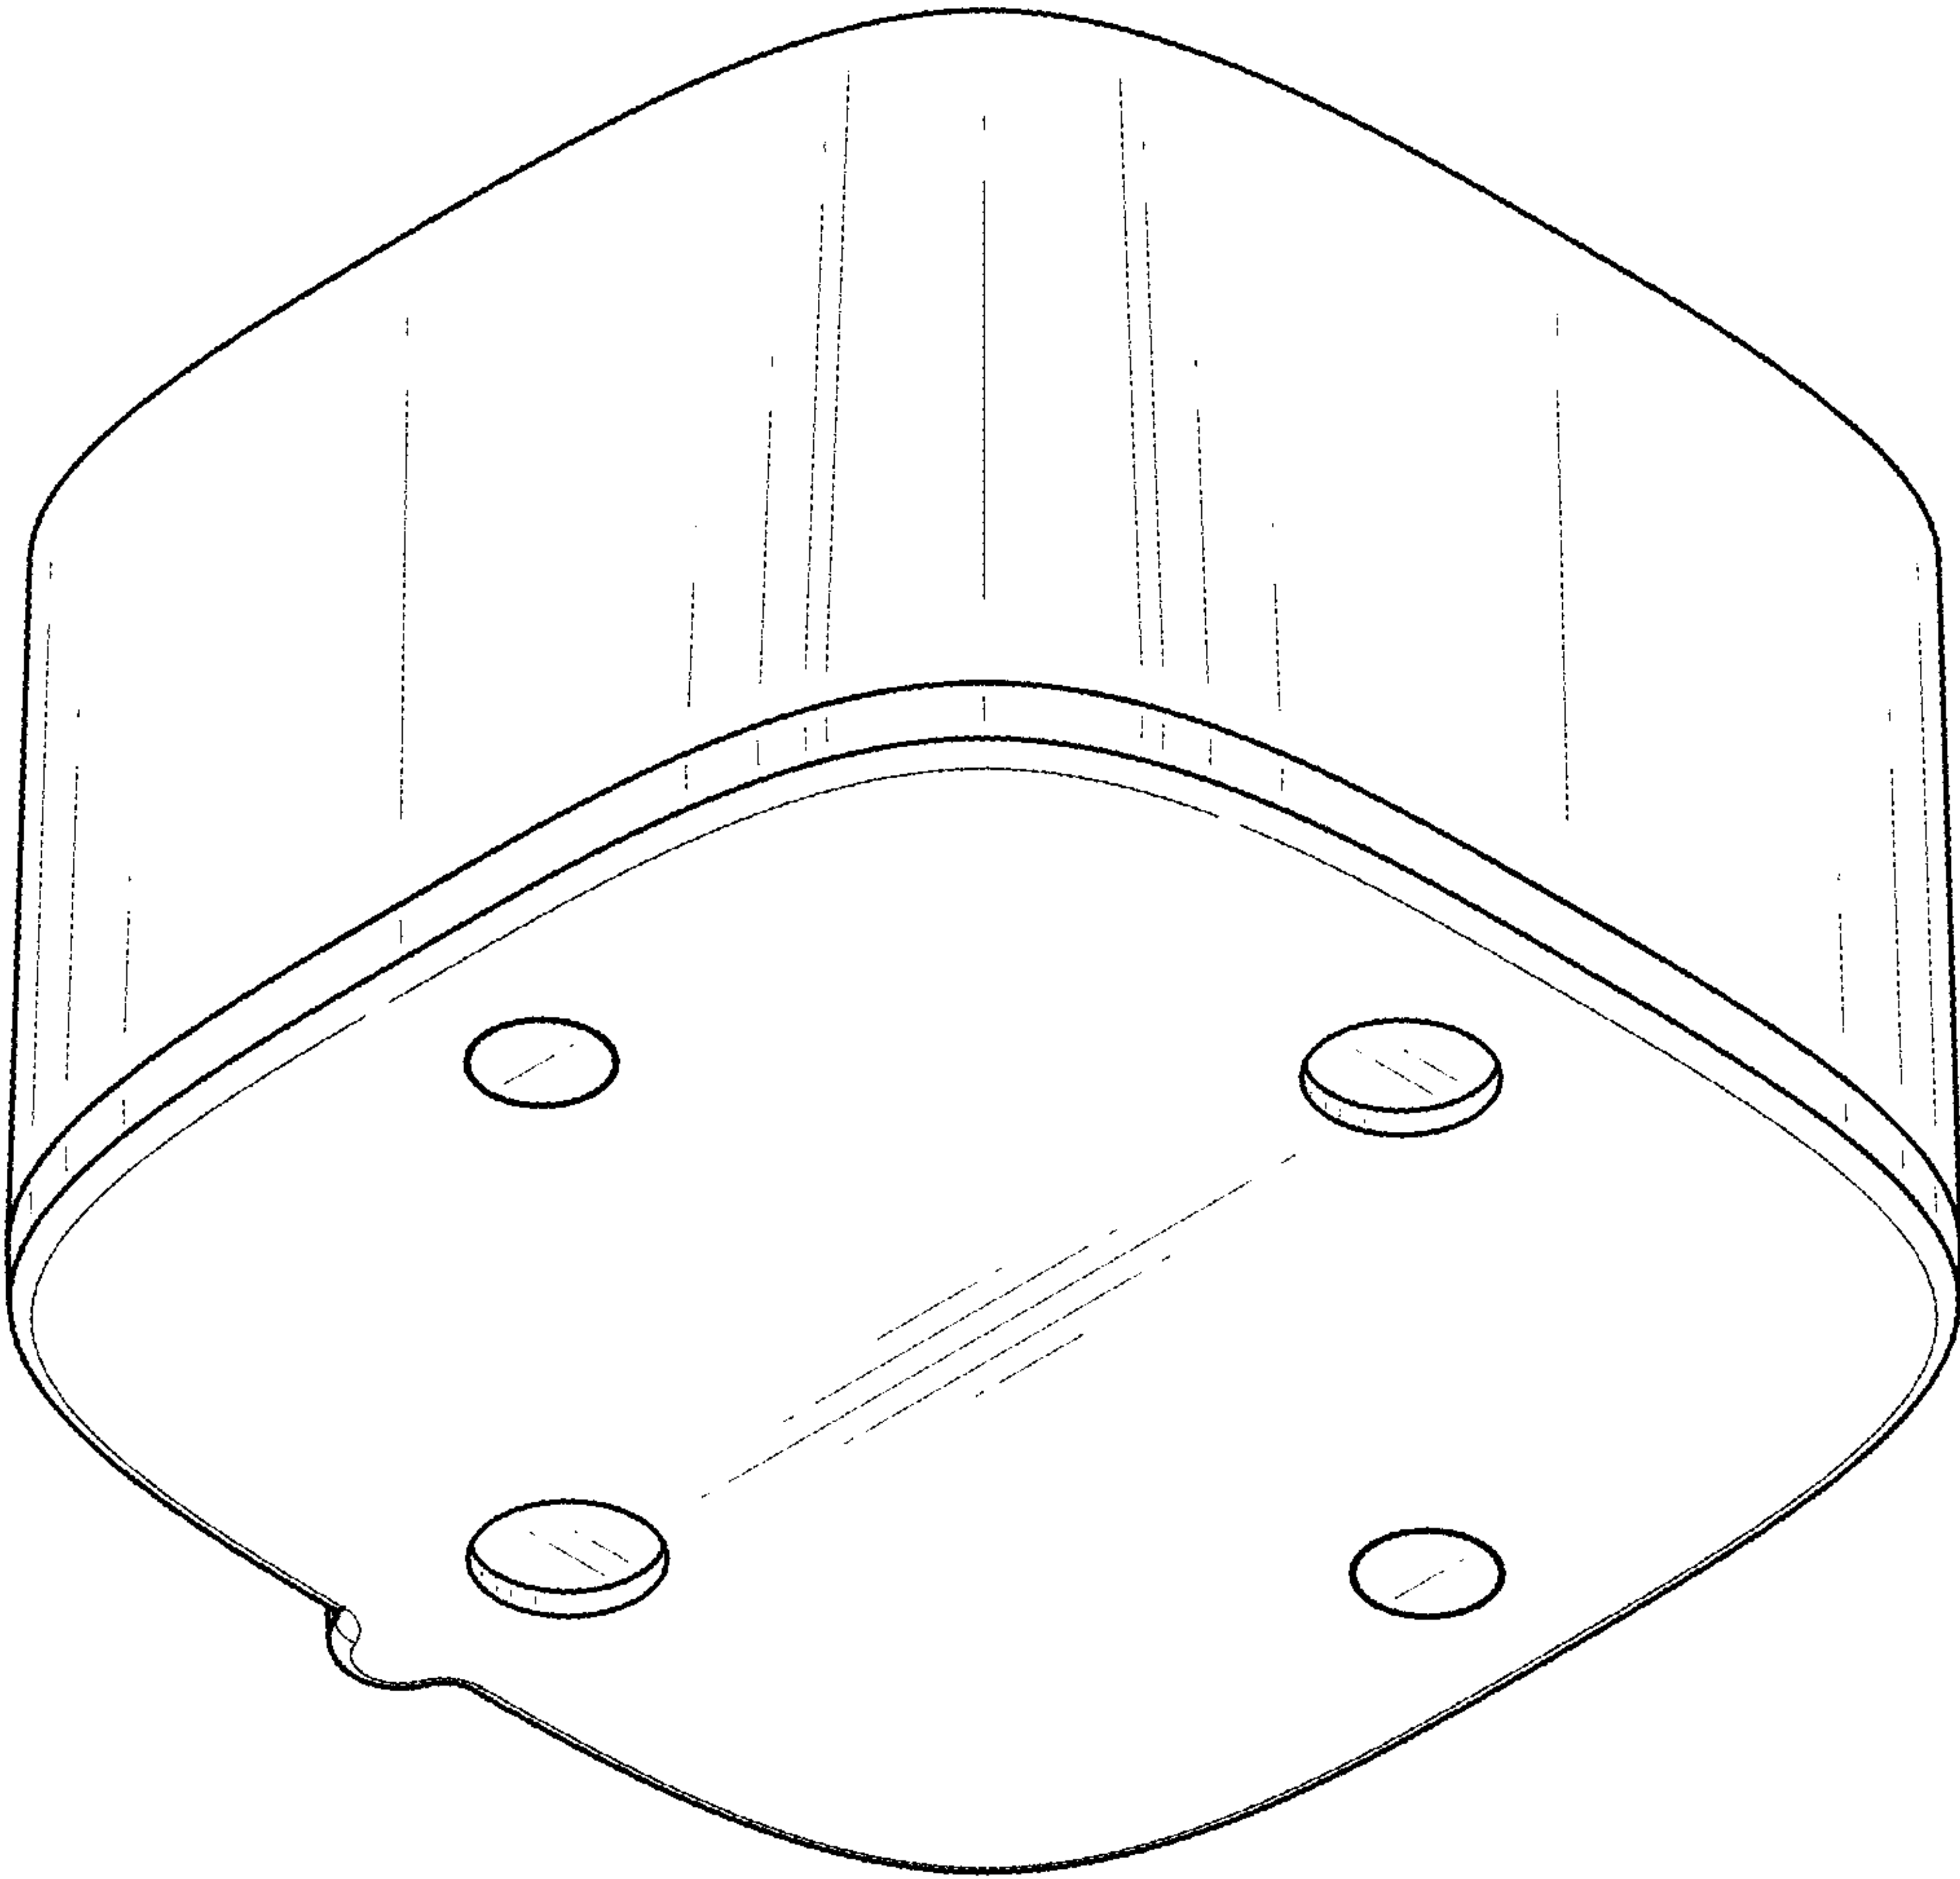


FIG. 2

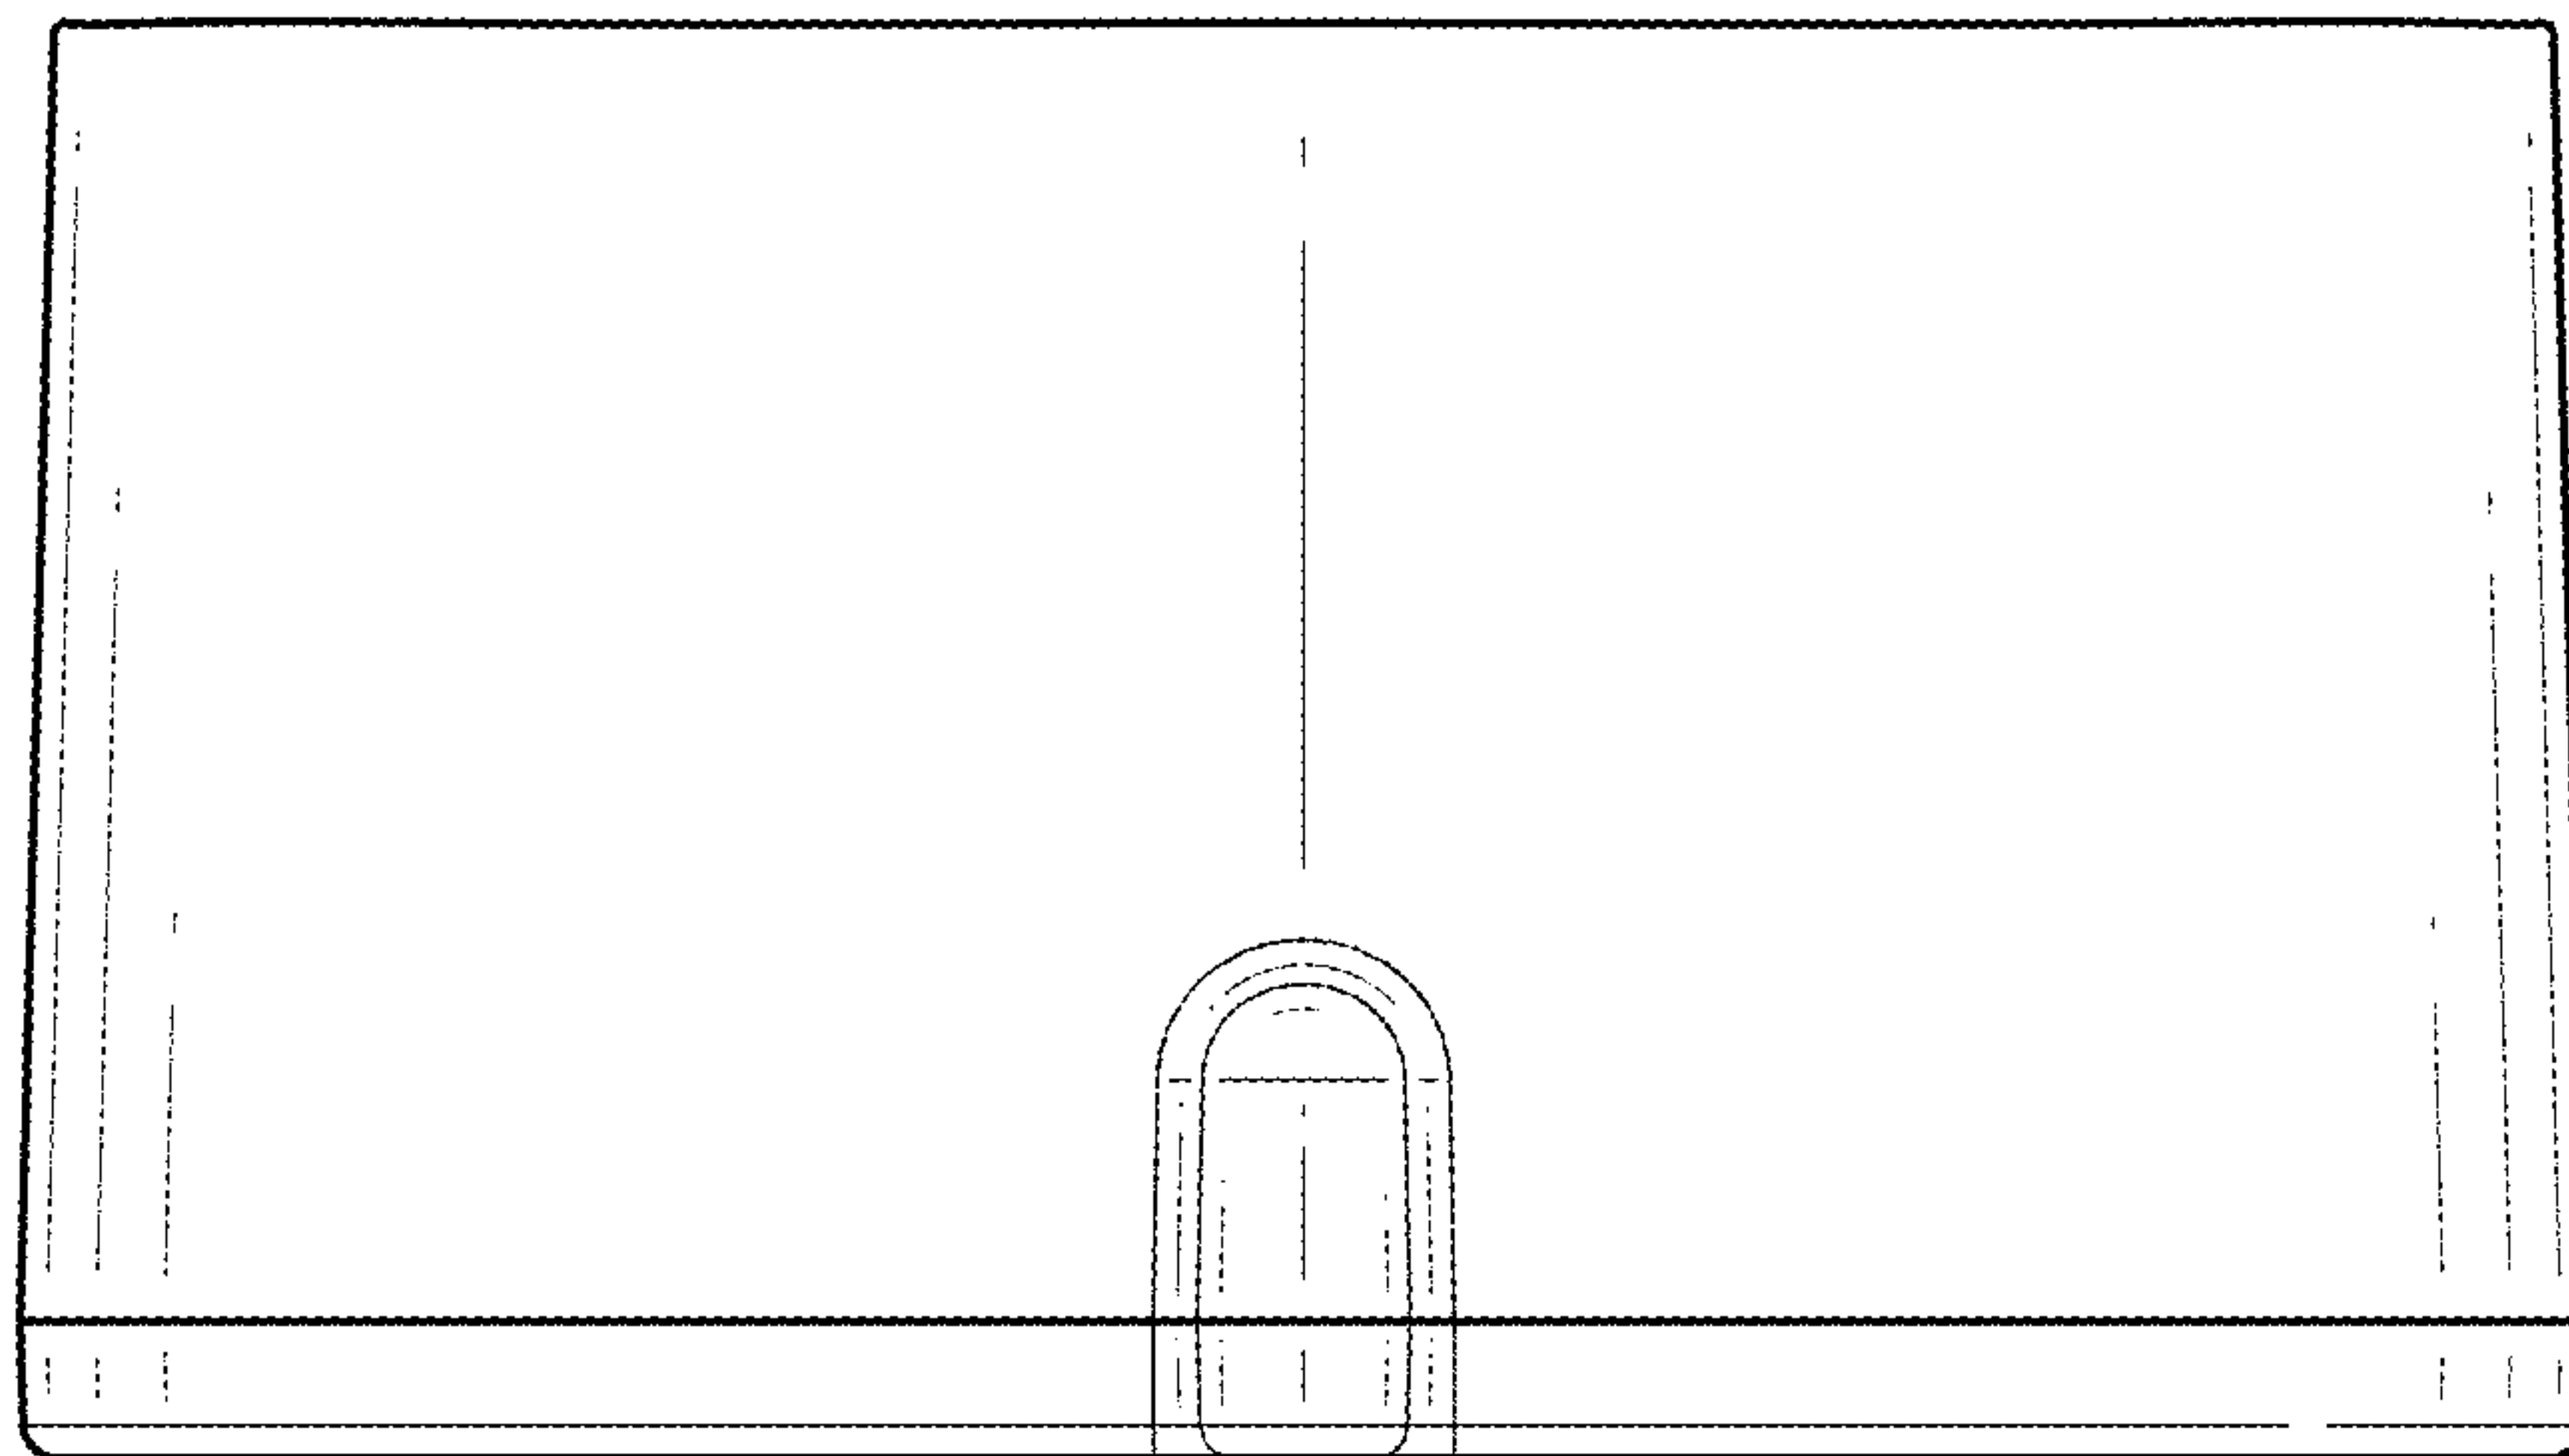


FIG. 3

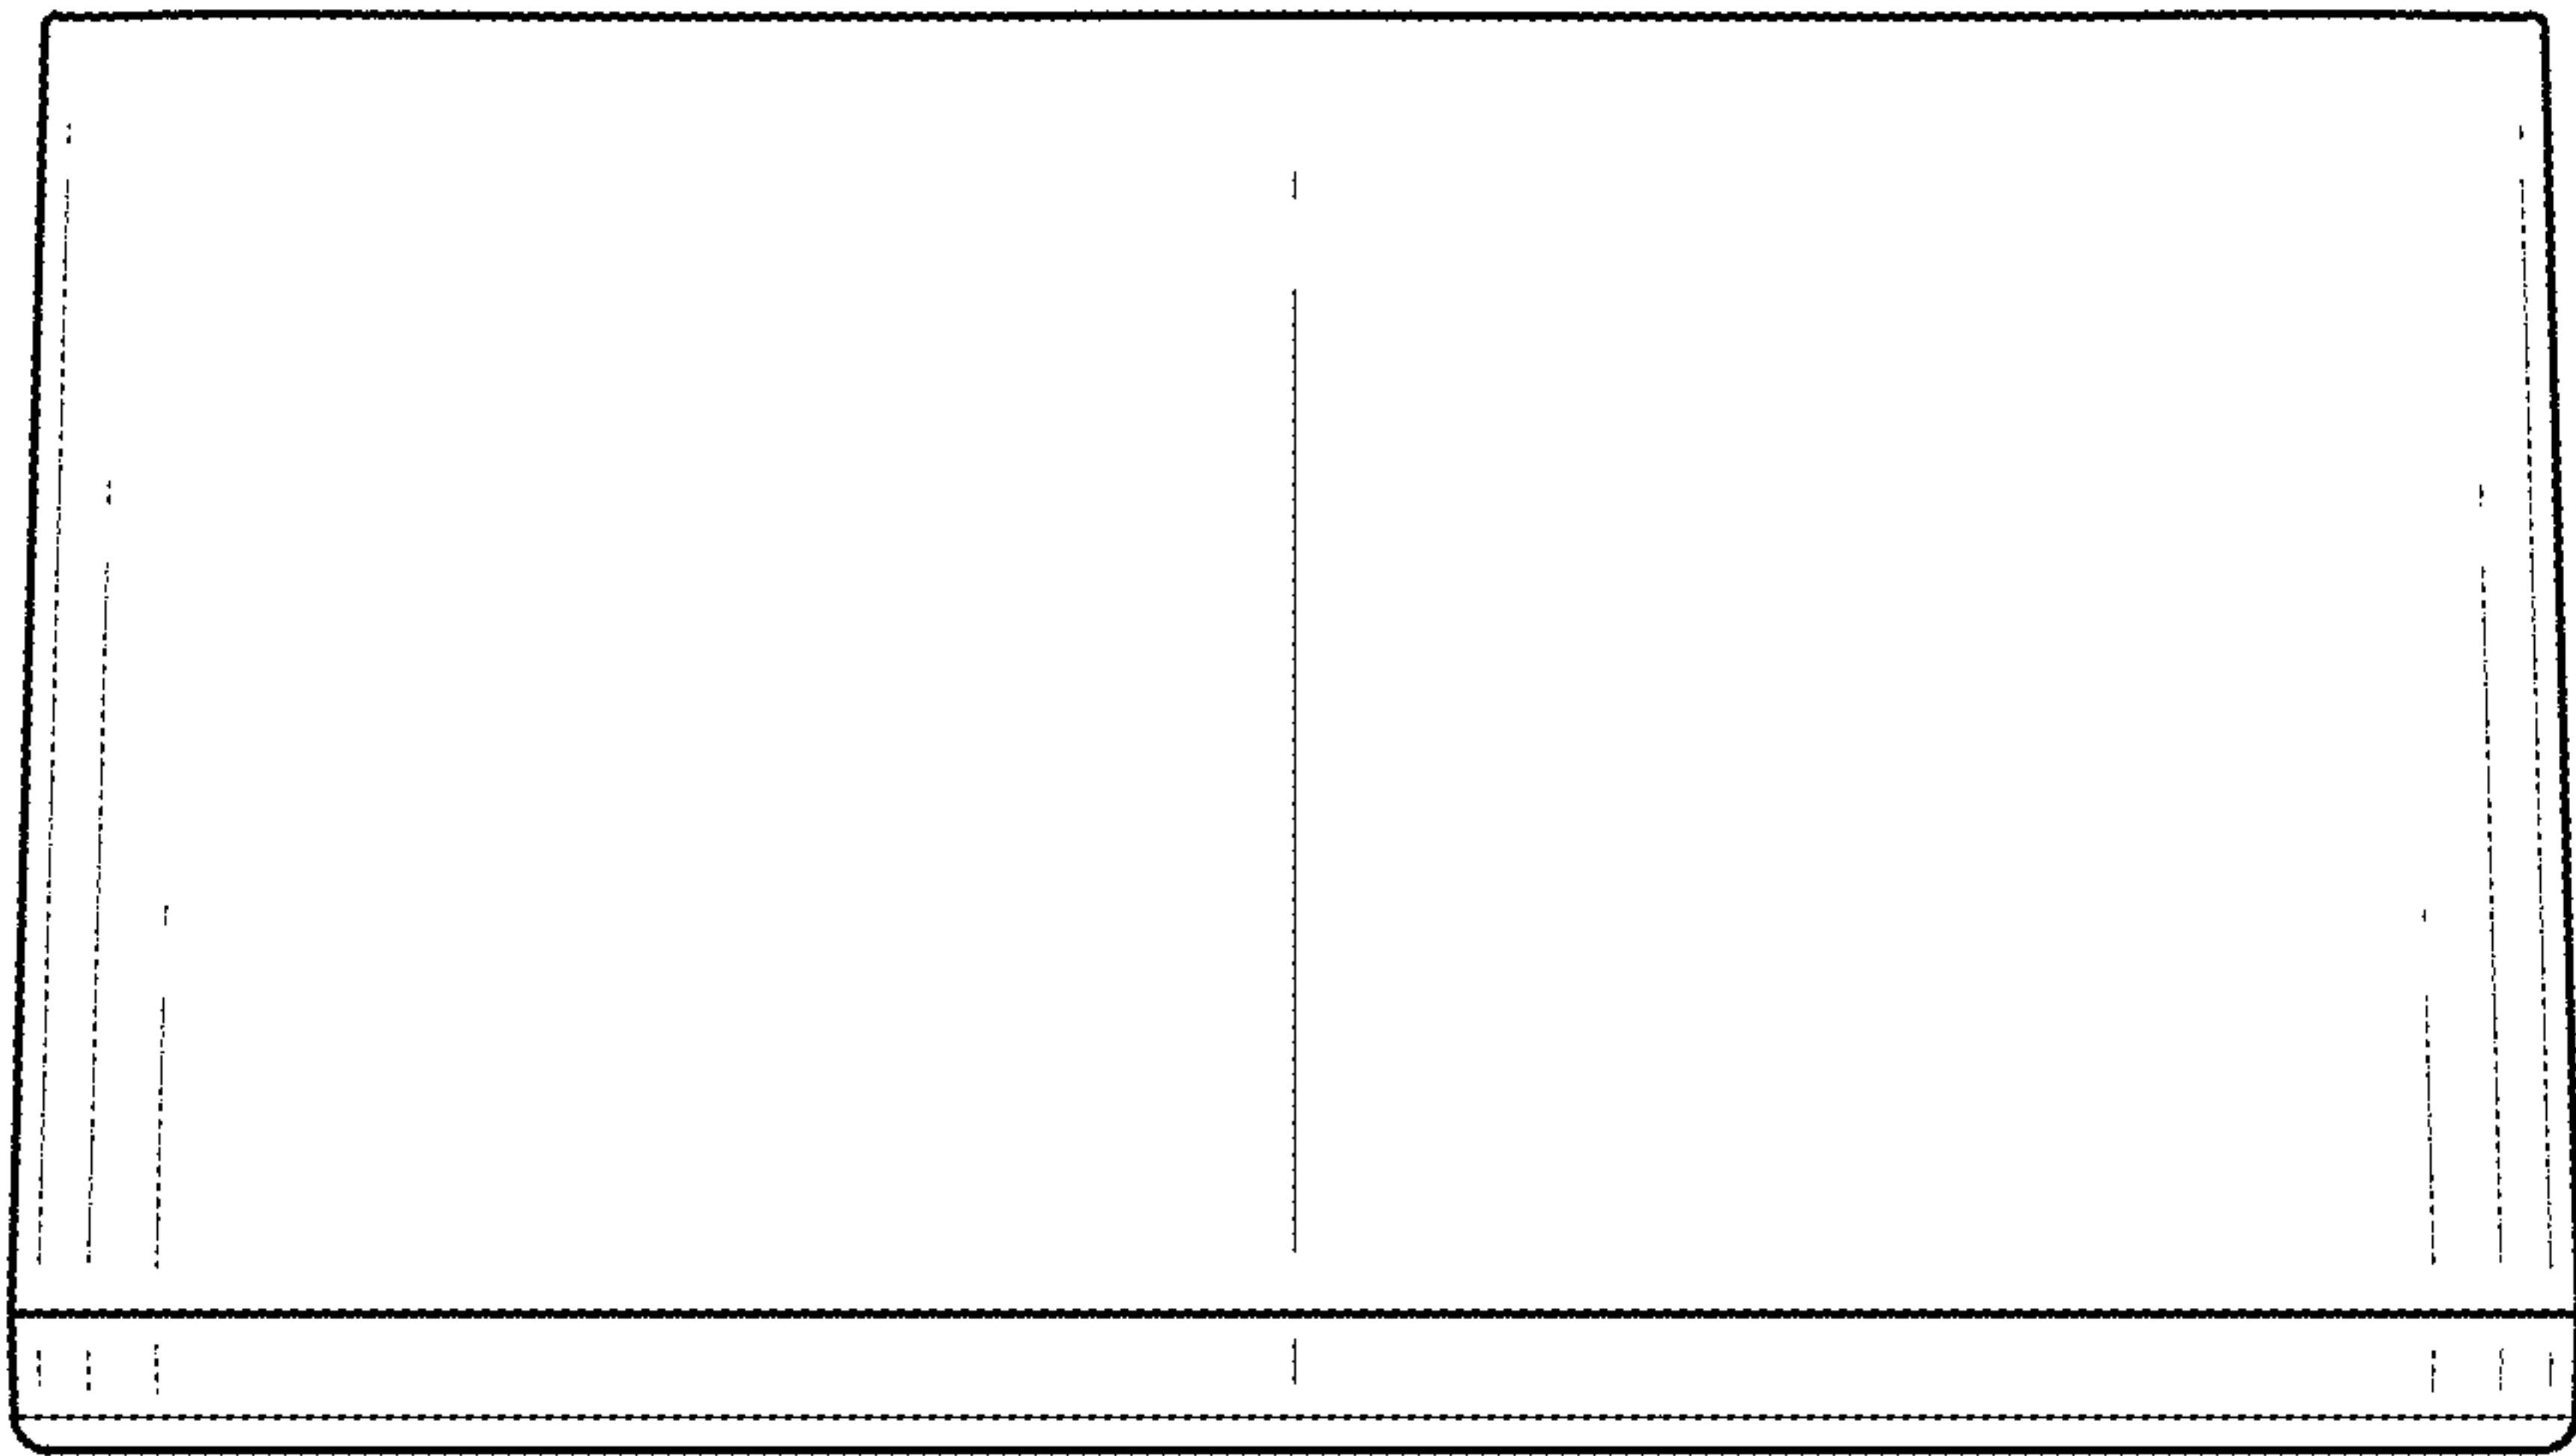


FIG. 4

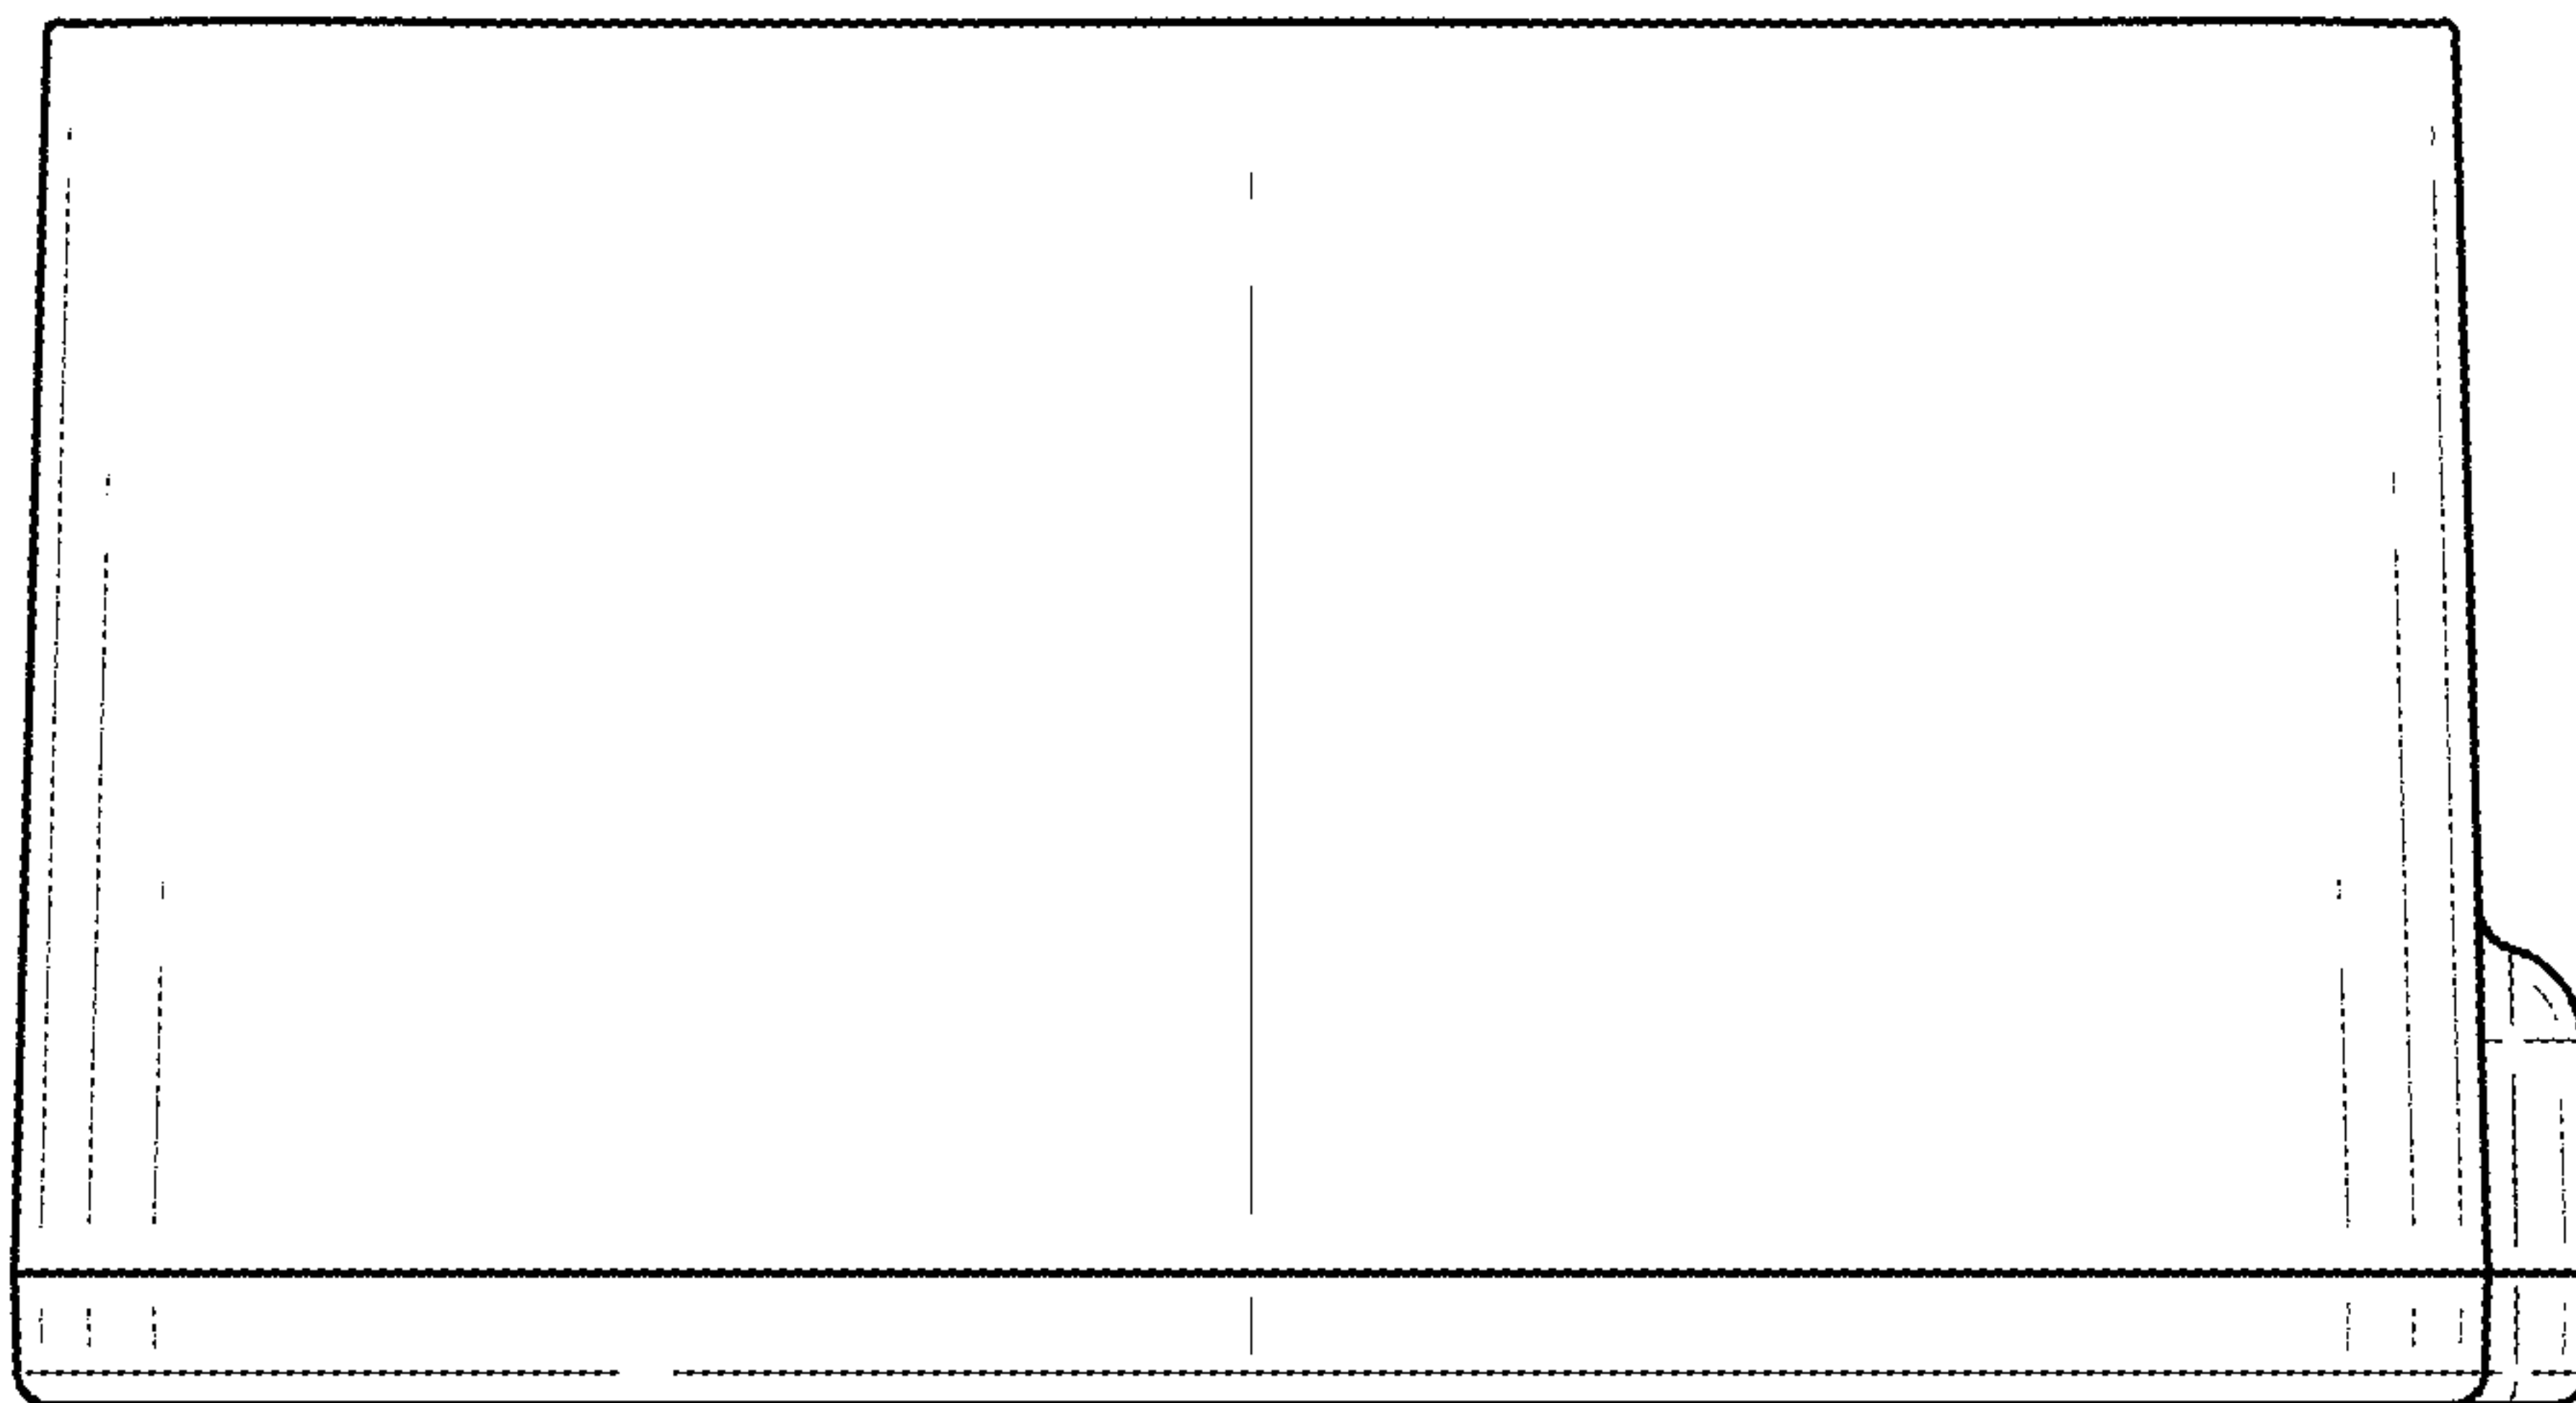


FIG. 5

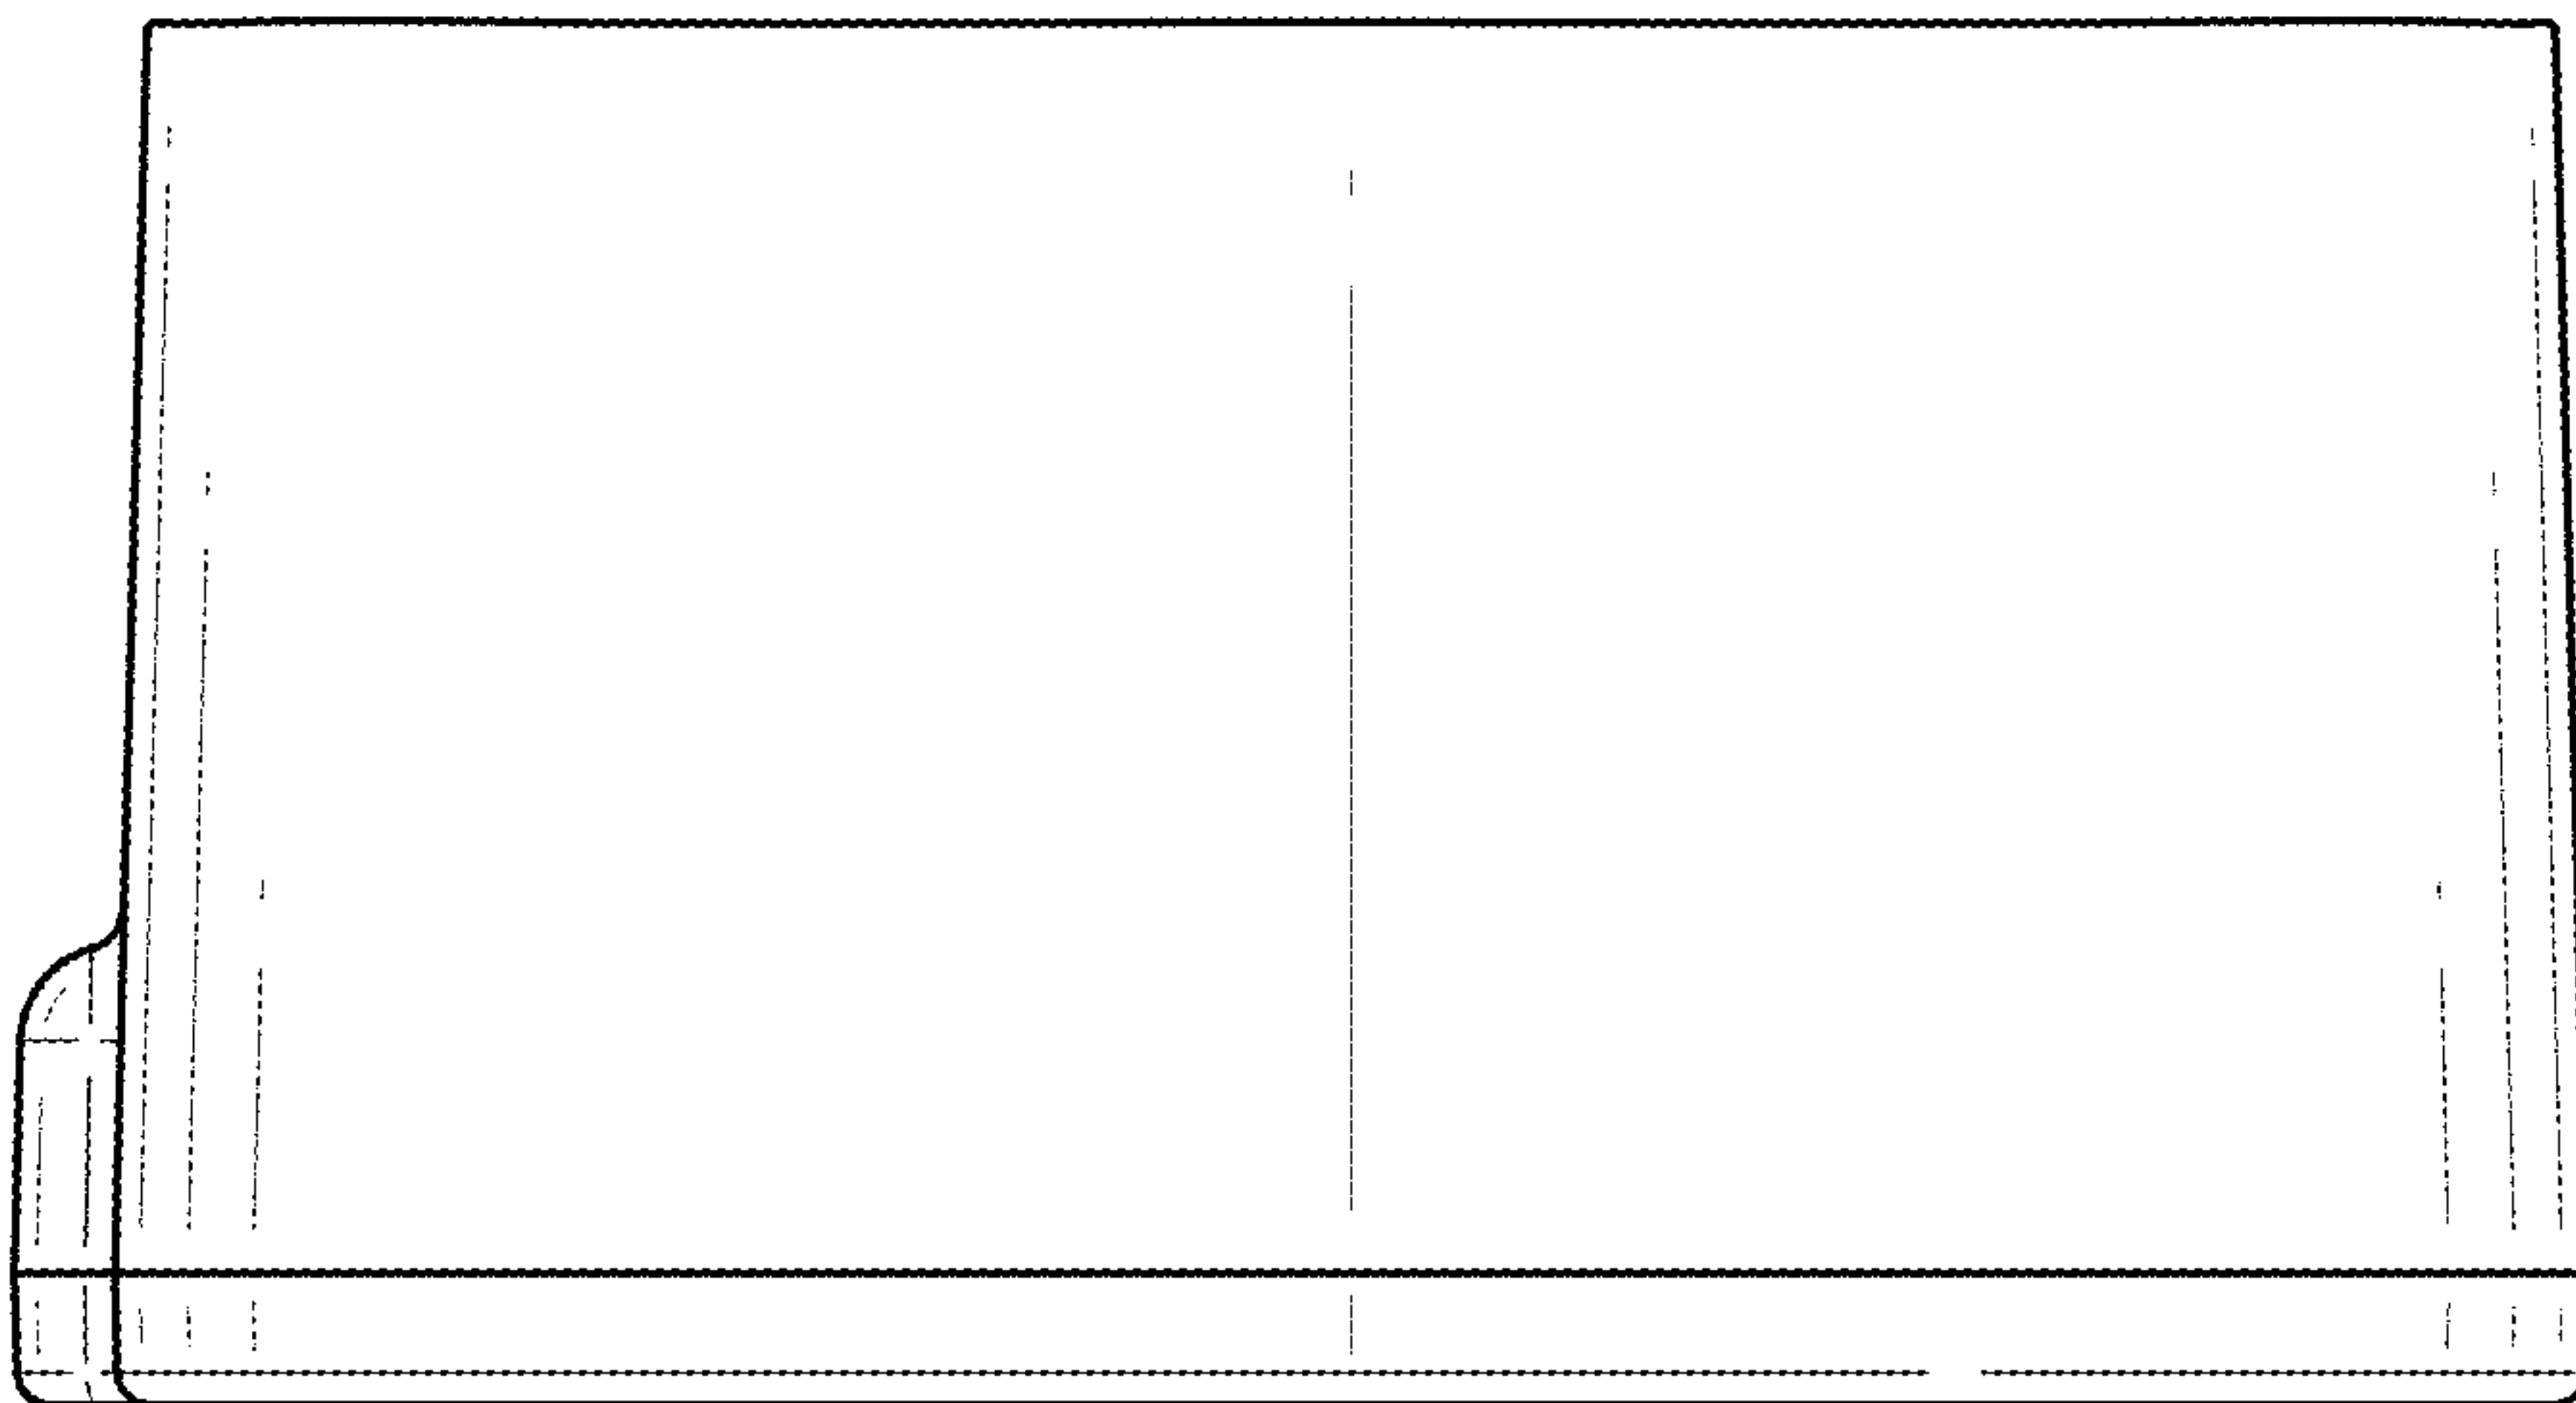


FIG. 6

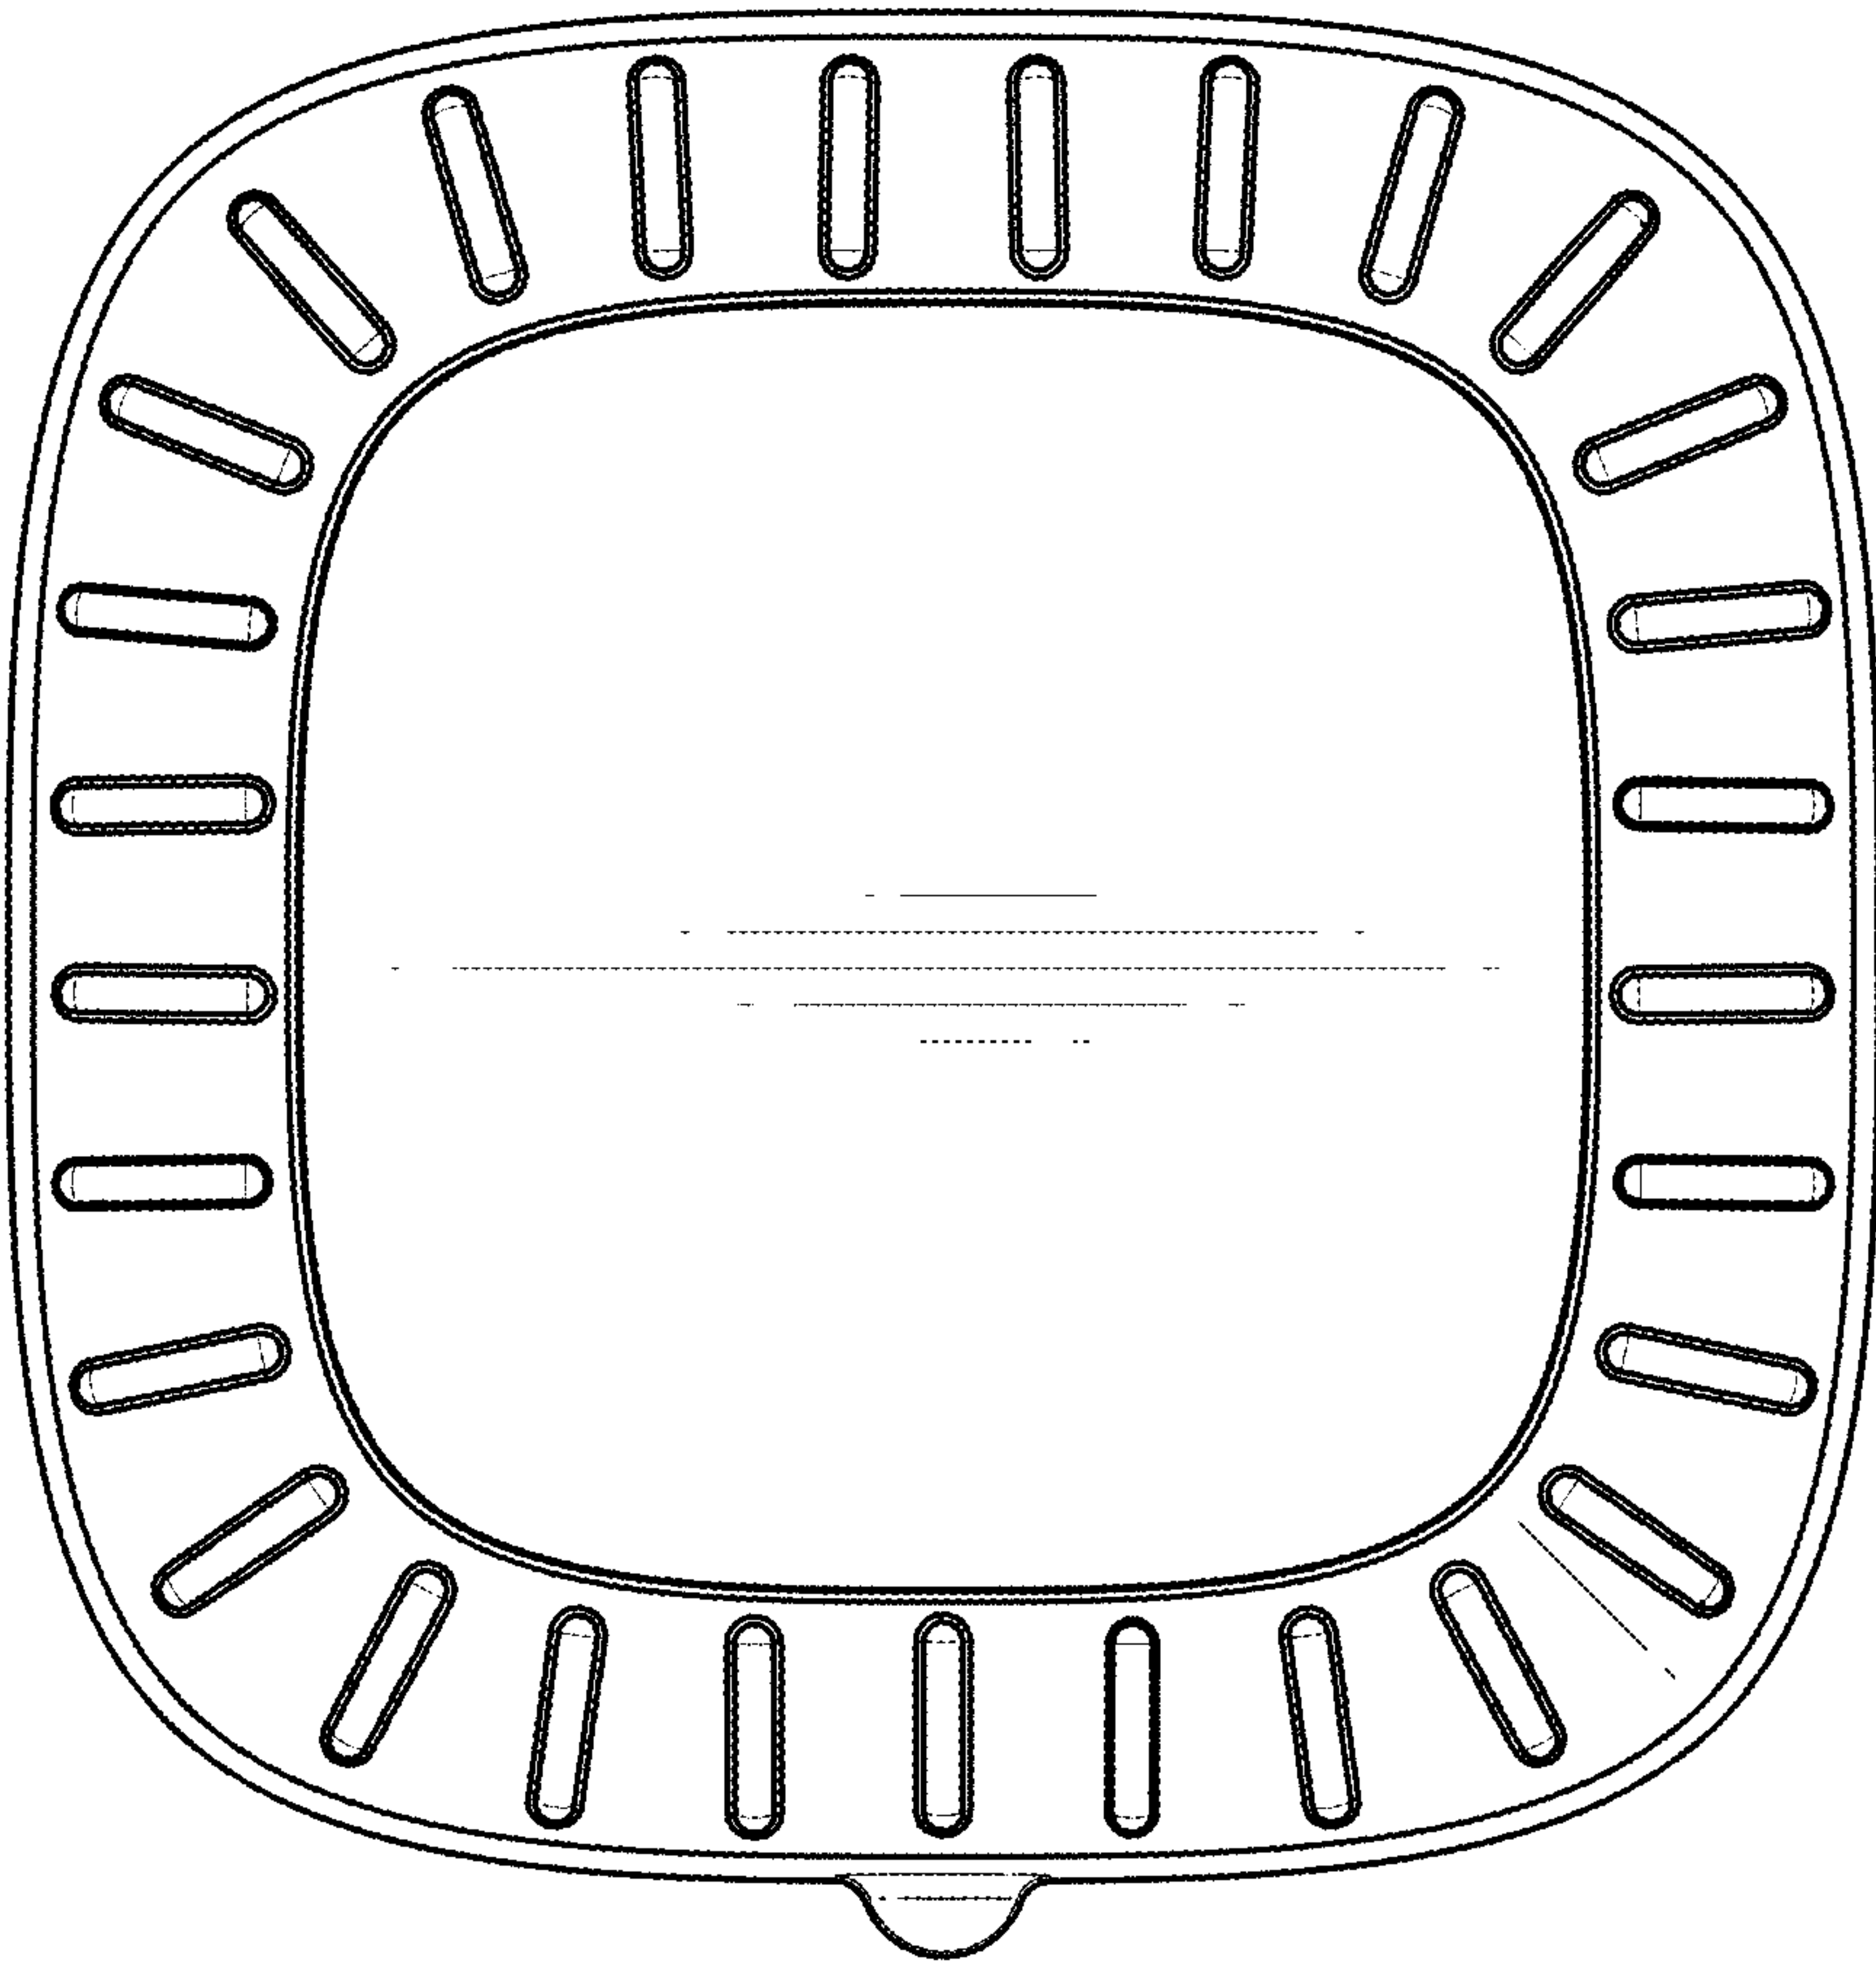


FIG. 7

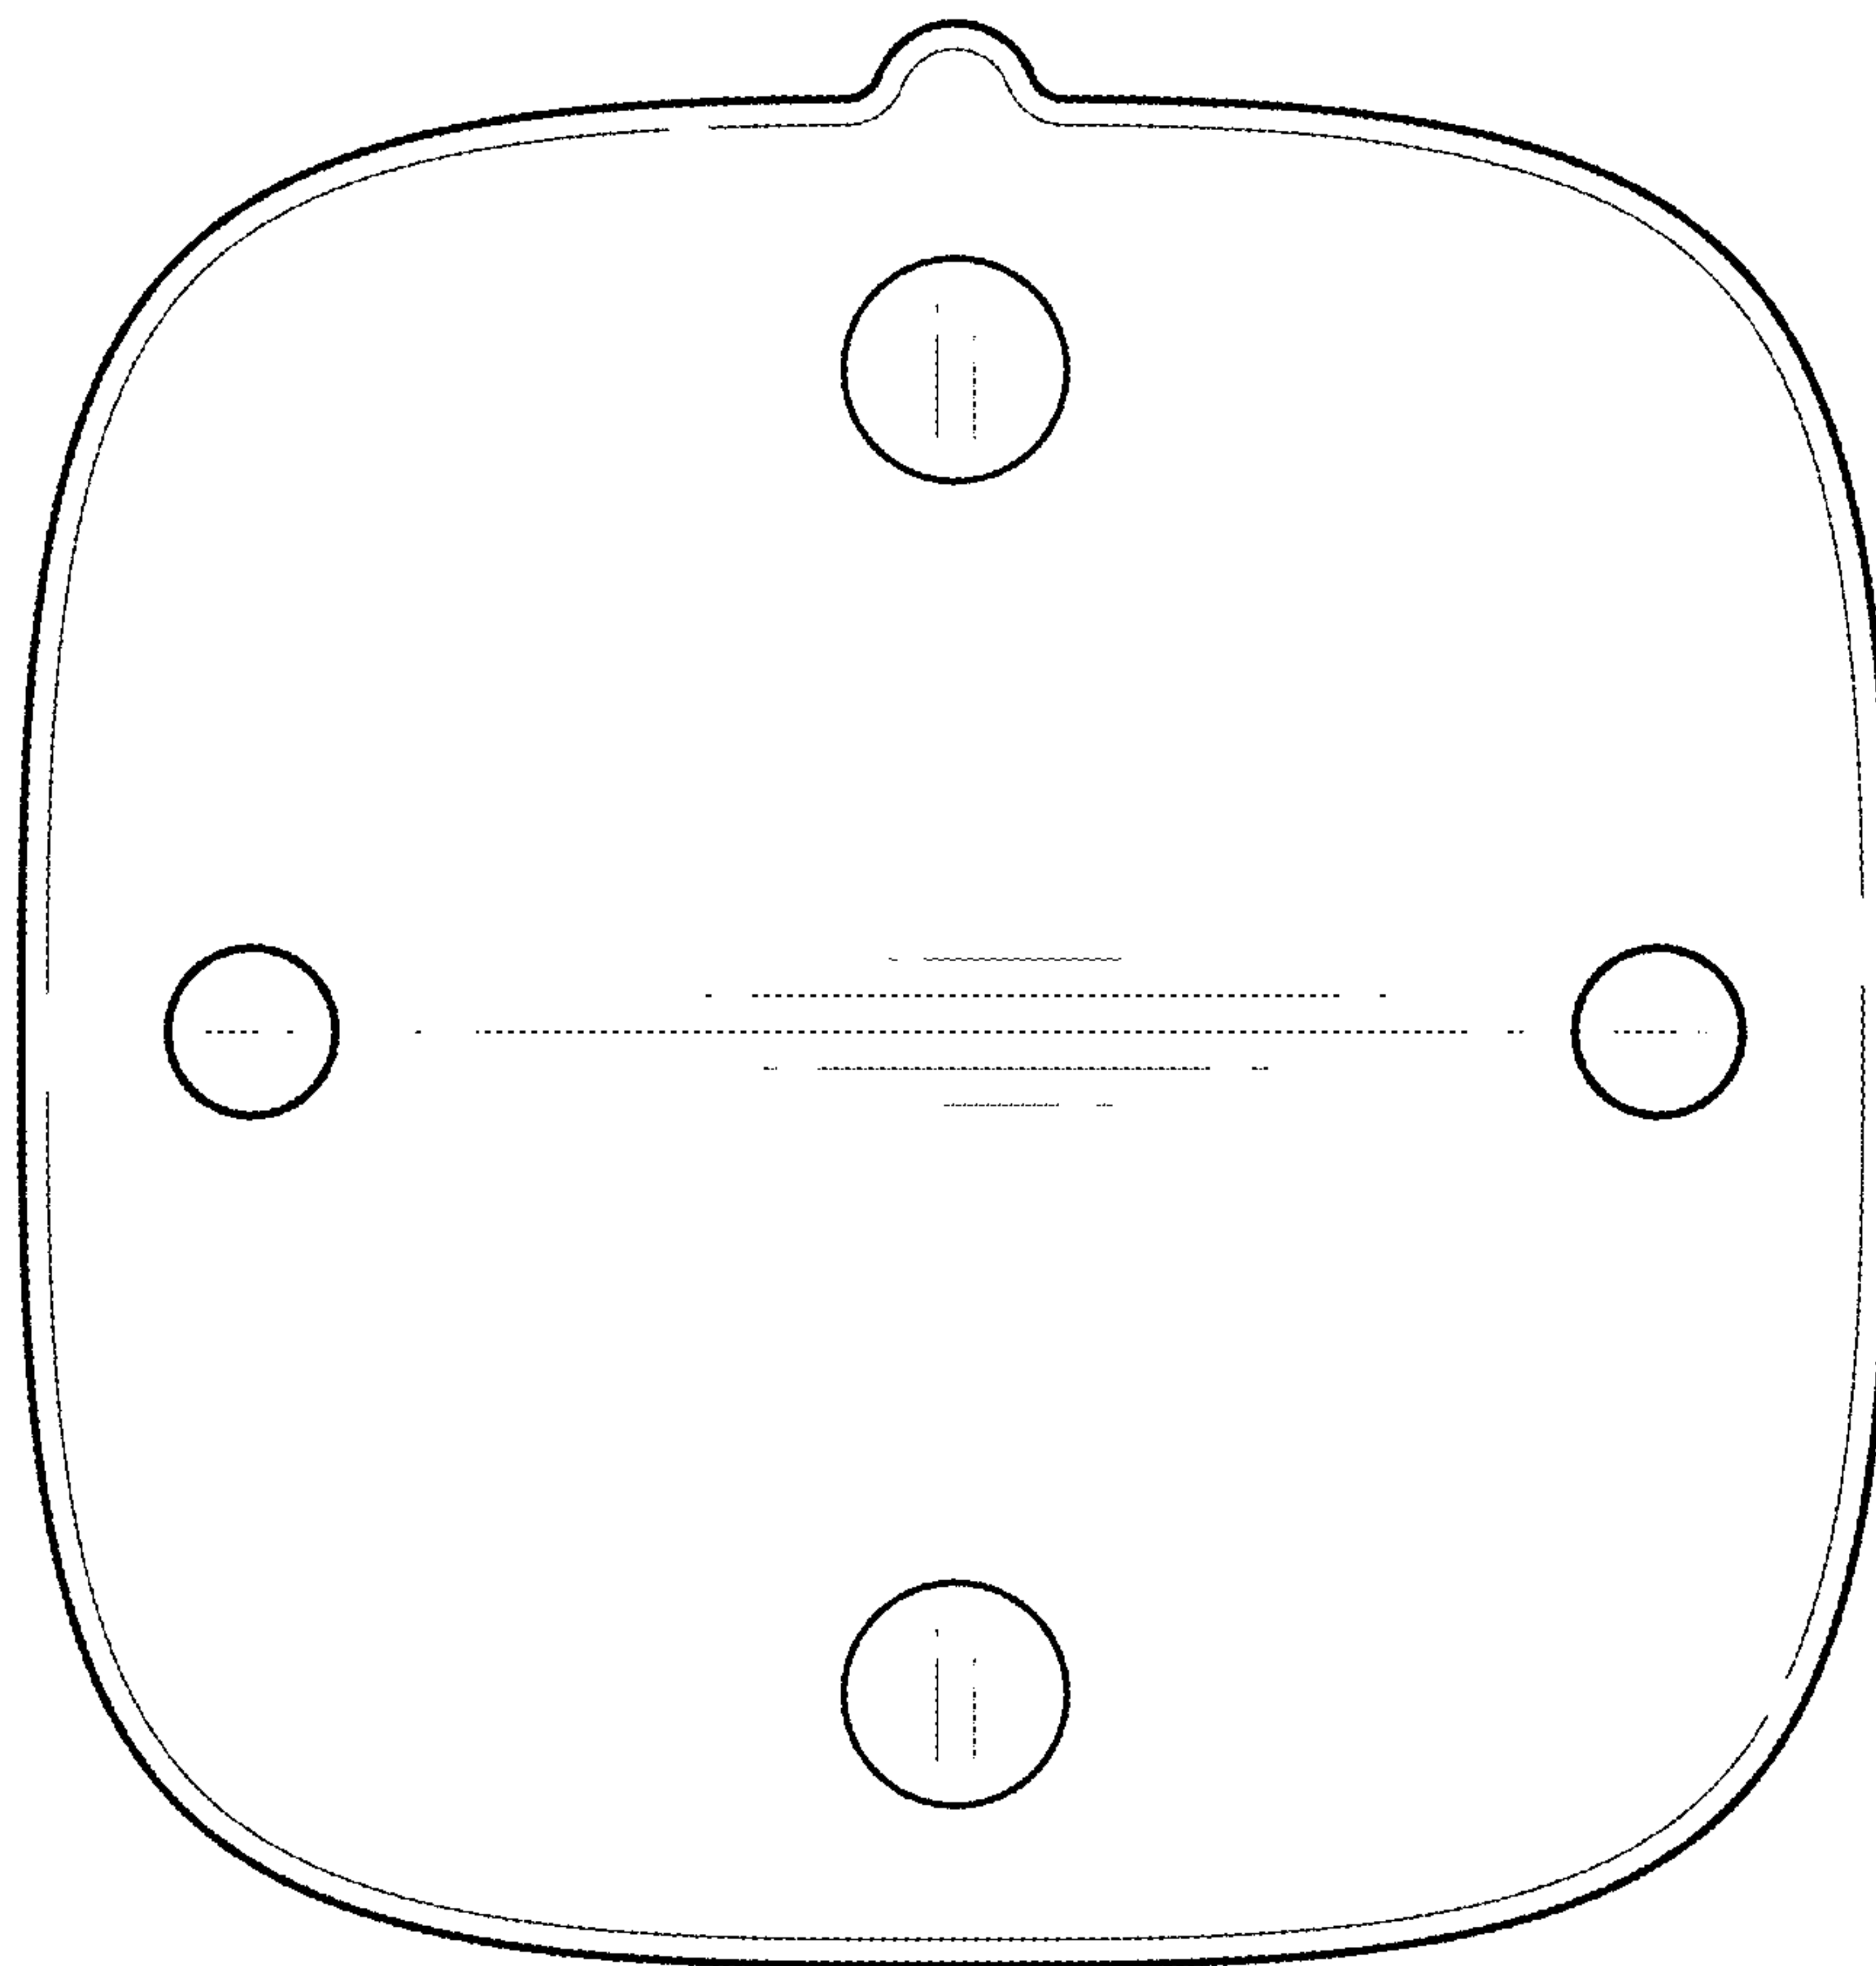


FIG. 8

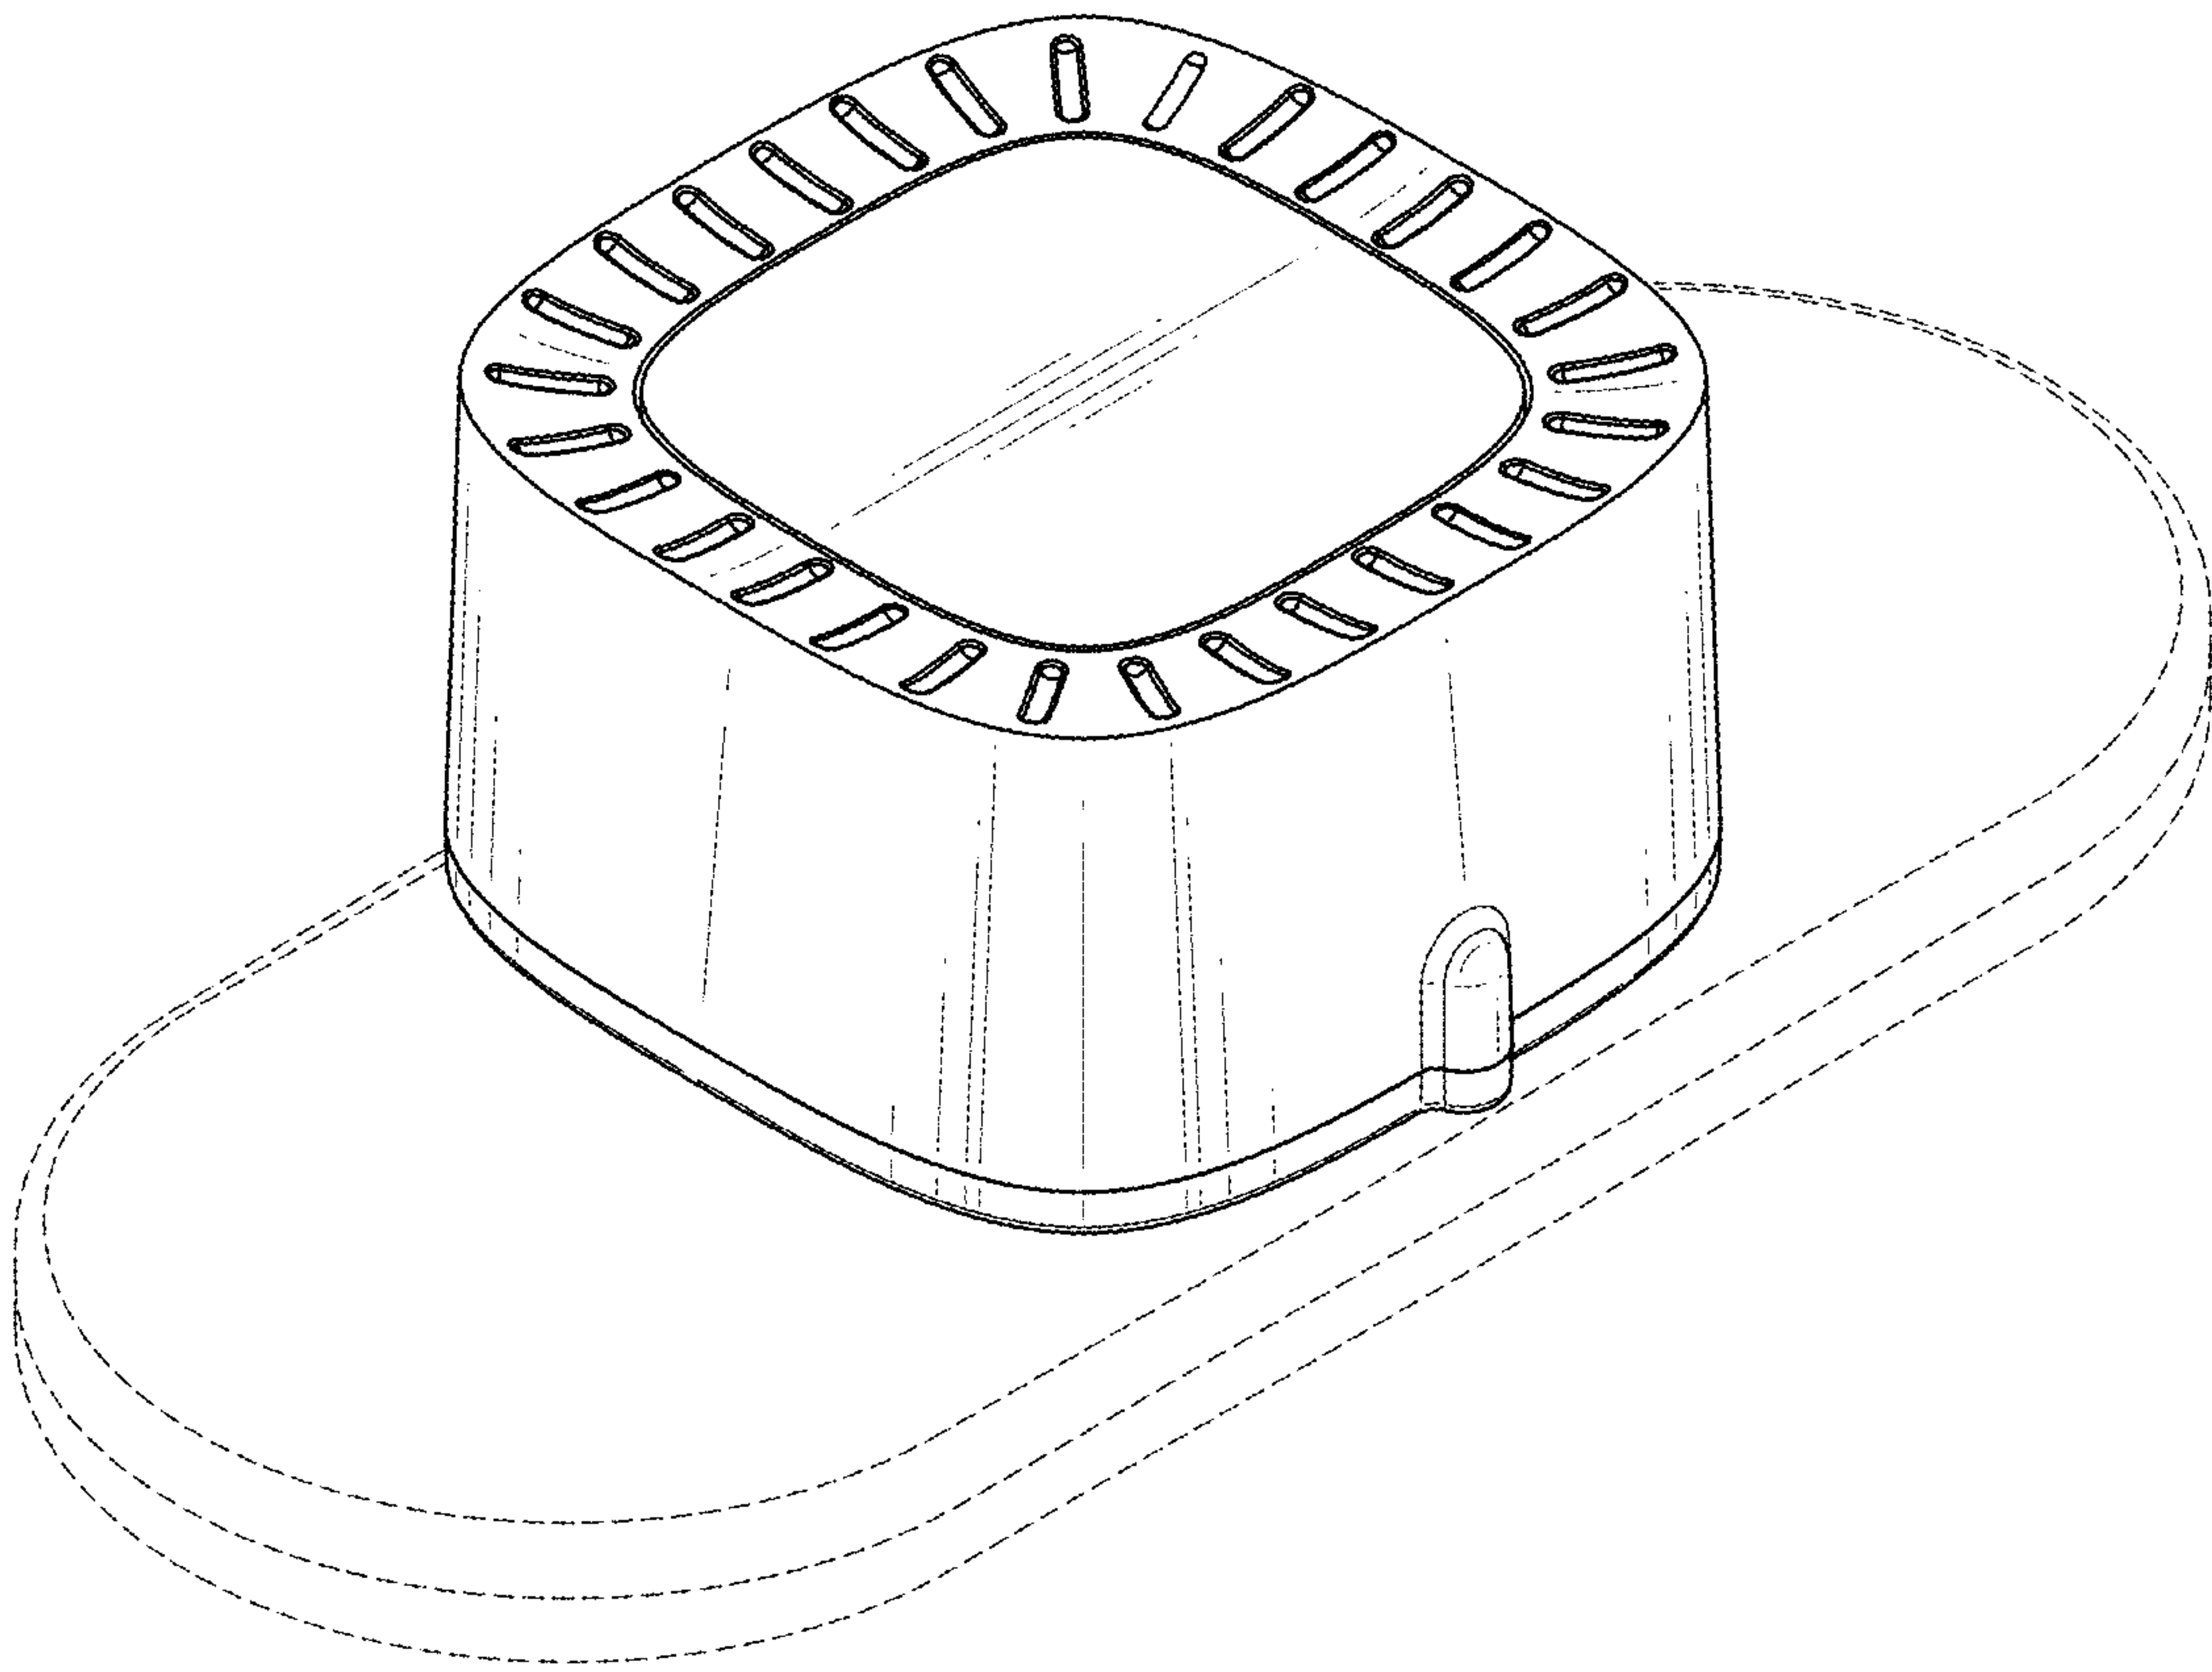


FIG. 9

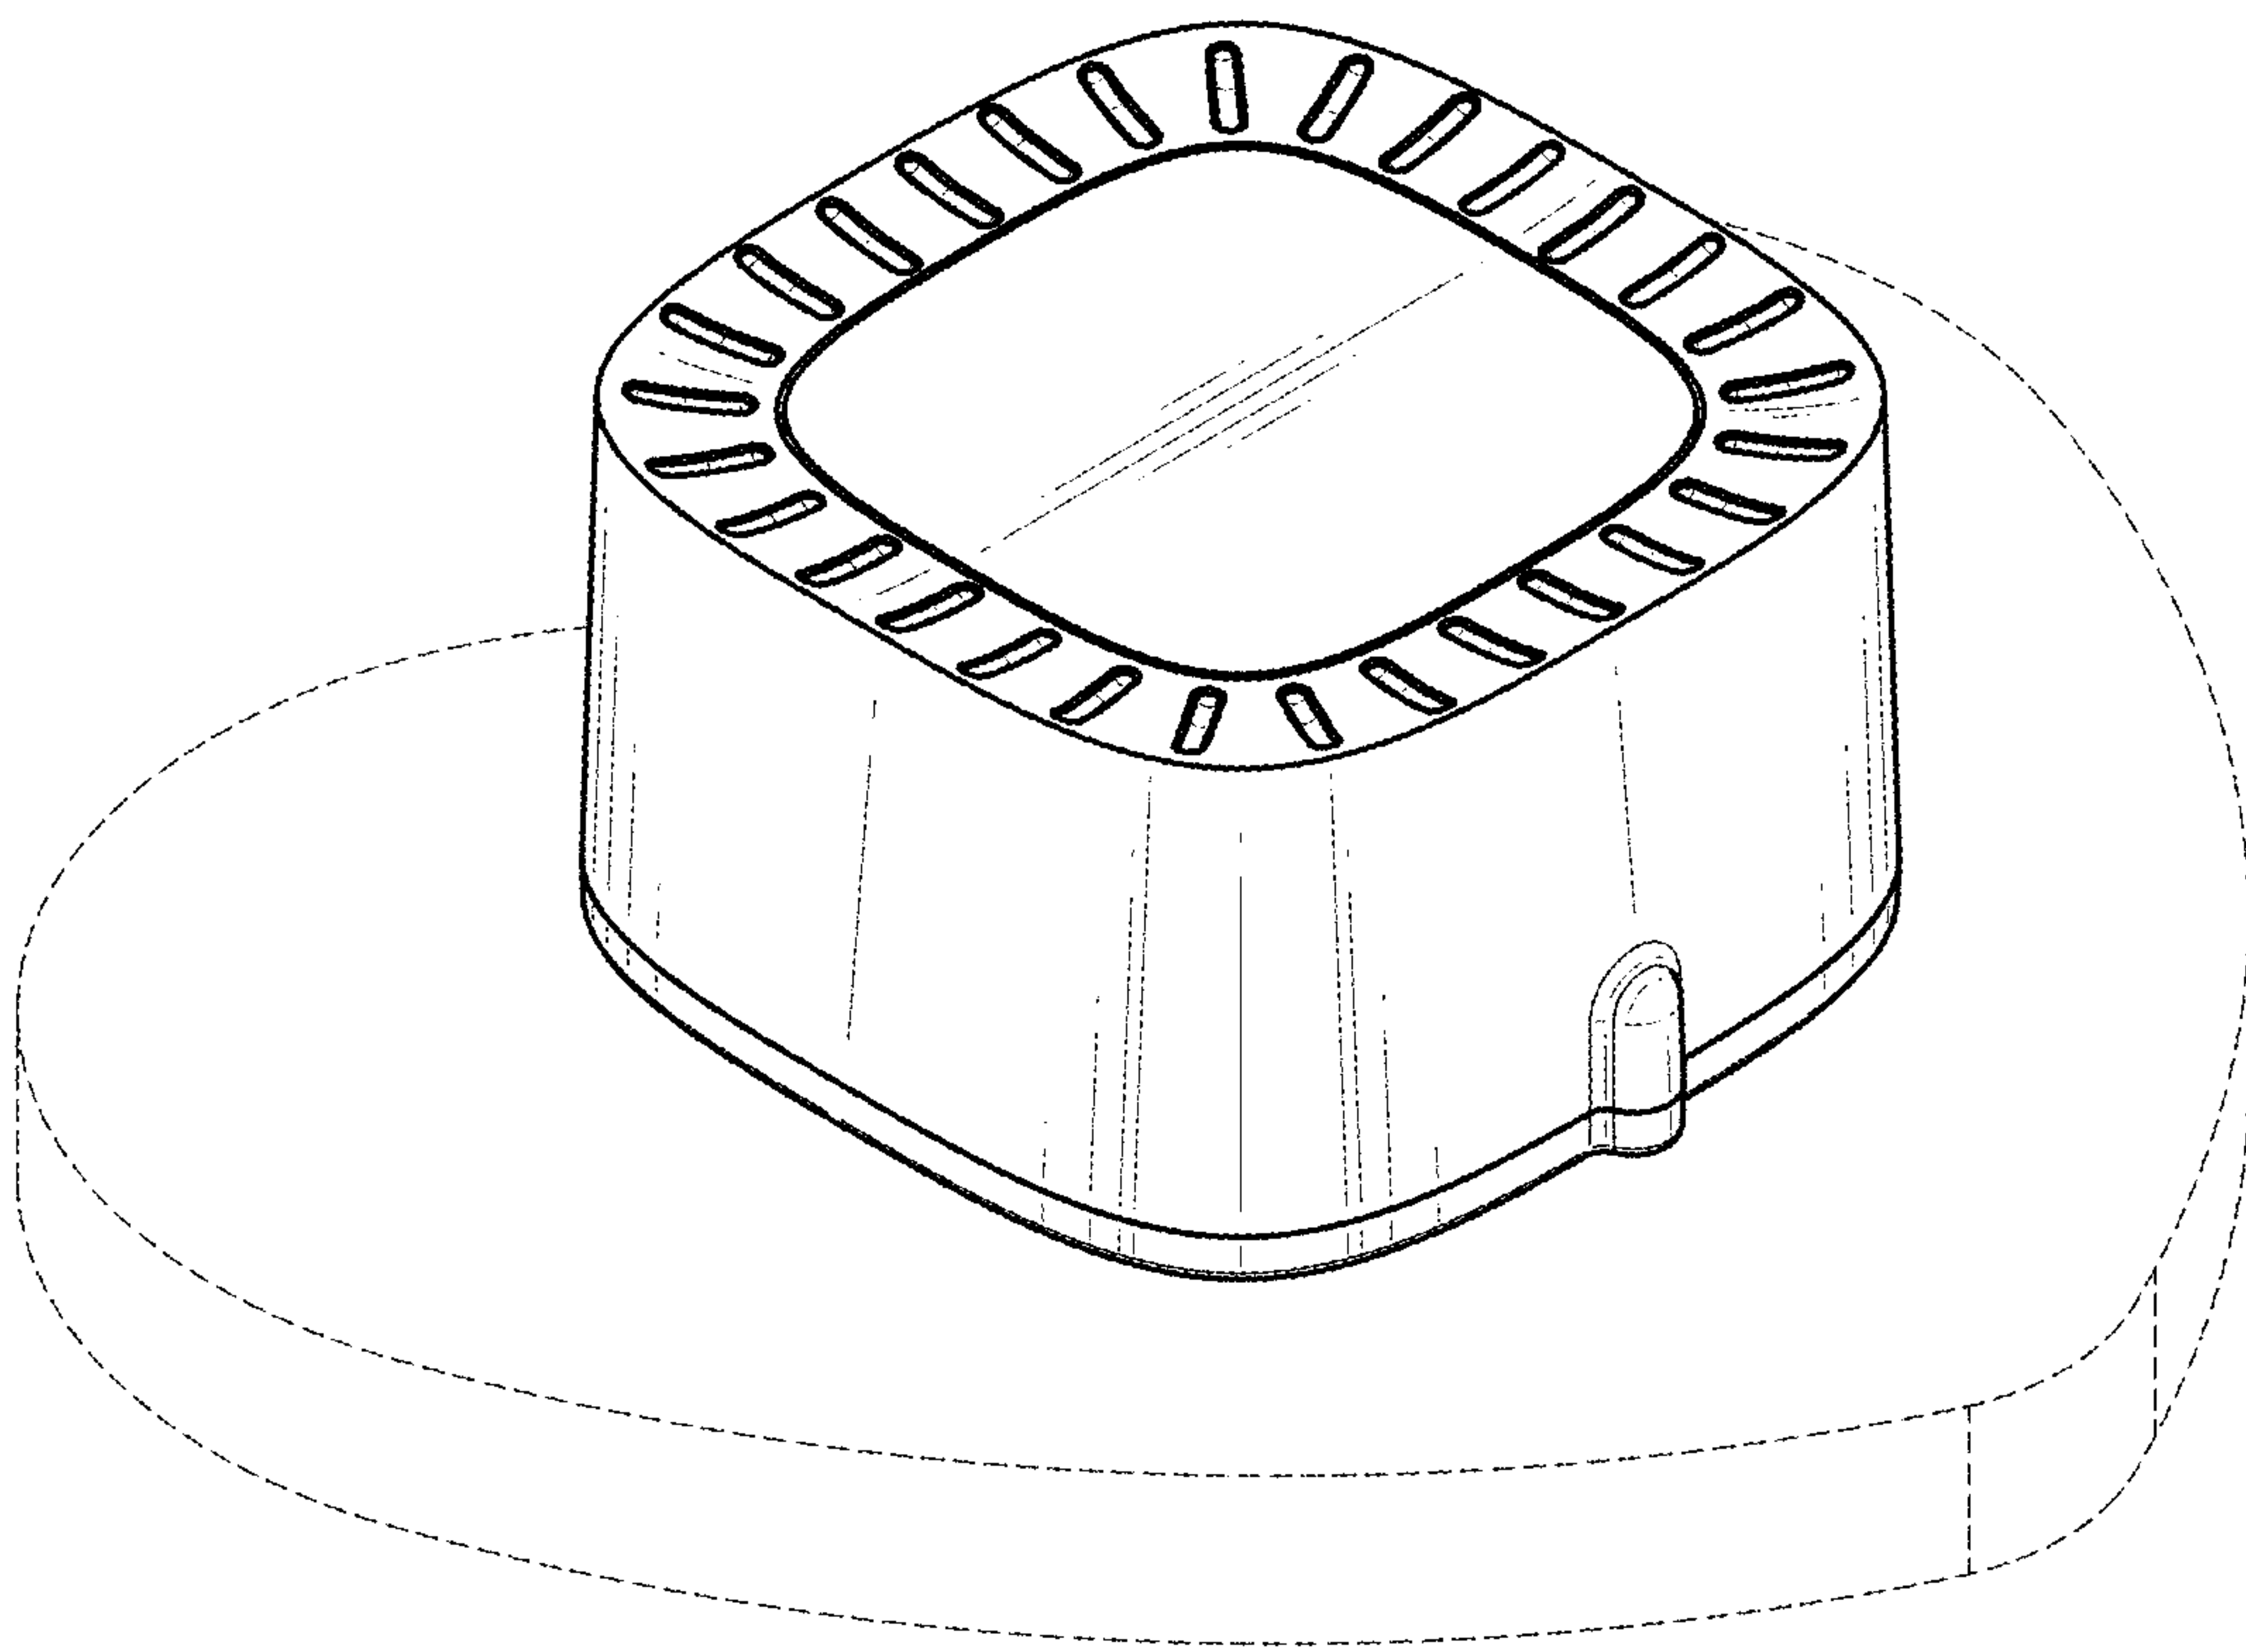


FIG. 10

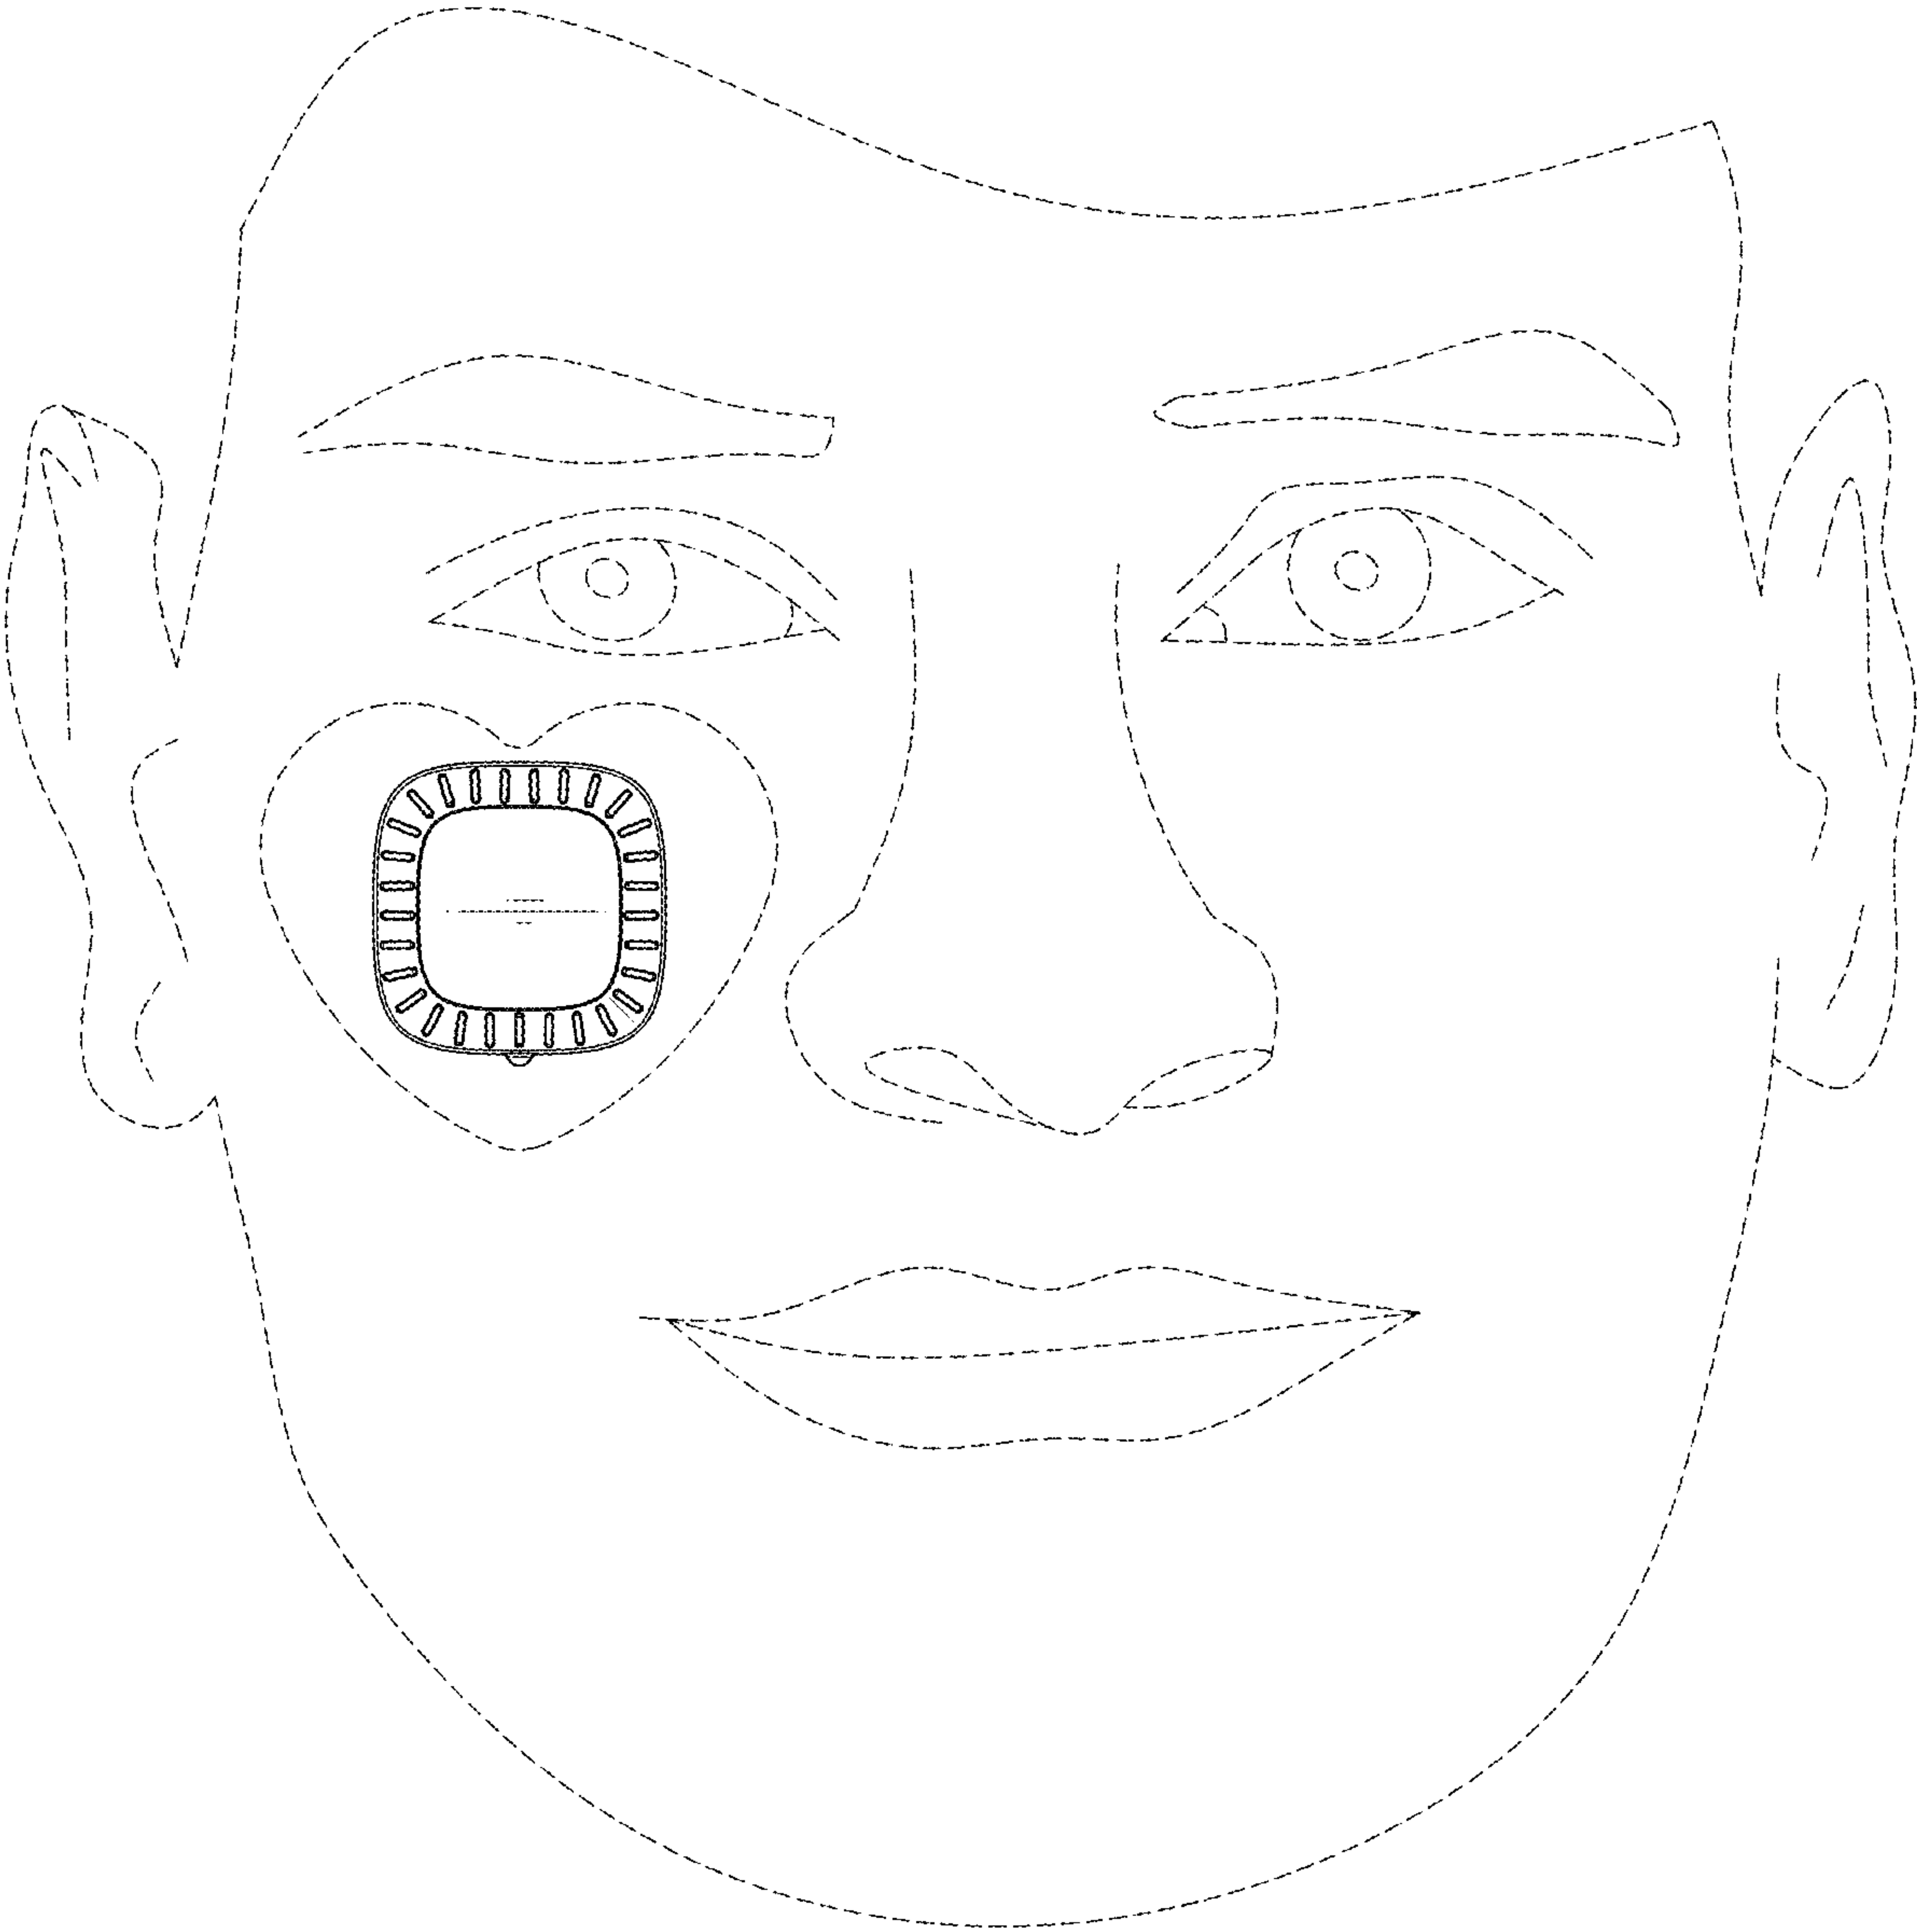


FIG. 11