

US0D1097160S

(12)

United States Design Patent

Peng

(10)

Patent No.:

US D1,097,160 S

(45)

Date of Patent:

** Oct. 7, 2025

(54) CARDIAC ULTRASOUND CONCAVE PHASED ARRAY TRANSDUCER

(71) Applicant: CLOUDSTREAM MEDICAL IMAGING, INC., Houston, TX (US)

(72) Inventor: Chengbin Peng, Houston, TX (US)

(73) Assignee: CLOUDSTREAM MEDICAL IMAGING, INC., Houston, TX (US)

(**) Term: 15 Years

(21) Appl. No.: 29/890,700

(22) Filed: Apr. 26, 2023

(51) LOC (15) Cl. 24-01

(52) U.S. Cl. USPC D24/158

(58) Field of Classification Search USPC D24/158, 159, 160, 167, 170, 177, 185, D24/186, 209, 231 CPC A61N 7/00; A61N 7/02; A61N 2007/0073; A61N 2007/0078; A61N 2007/0039; B06B 1/0633; A61B 8/4488; A61B 8/12 See application file for complete search history.

(56) References Cited

U.S. PATENT DOCUMENTS

2007/0016055 A1* 1/2007 Cao B06B 1/0633 600/459

2014/0283611 A1* 9/2014 Habermehl G10K 11/346 73/602

2020/0322454 A1* 10/2020 Ersson A61B 8/4472

FOREIGN PATENT DOCUMENTS

CN 308327551 * 11/2023

OTHER PUBLICATIONS

Concave Phased Array Transducer UT0037—NDT-Kits, posted date unavailable [retrieved online Apr. 22, 2025]. Retrieved from internet, <https://ndt-kits.com/product/phased-array-transducer/ut0037/> (Year: 2025).*

Phased Array Probes | Evident Scientific, posted date unavailable [retrieved online Apr. 22, 2025]. Retrieved from internet, <https://ims.evidentscientific.com/en/probes/phased-array> (Year: 2025).*

Phased Array Transducer and Probe—NDT-Kits, posted date unavailable [retrieved online Apr. 22, 2025]. Retrieved from internet, <https://ndt-kits.com/phased-array-transducer/> (Year: 2025).*

* cited by examiner

Primary Examiner — Justin M Jonaitis
Assistant Examiner — Samantha K Pollack
(74) Attorney, Agent, or Firm — SZDC Law PC


(57) CLAIM

The ornamental design for a cardiac ultrasound concave phased array transducer, as shown and described.

DESCRIPTION

FIG. 1 is a front perspective view of a cardiac ultrasound concave phased array transducer;
FIG. 2 is a top view thereof; and,
FIG. 3 is a left view thereof.
The broken lines depict portions of the cardiac ultrasound concave phased array transducer that form no part of the claim.

1 Claim, 3 Drawing Sheets

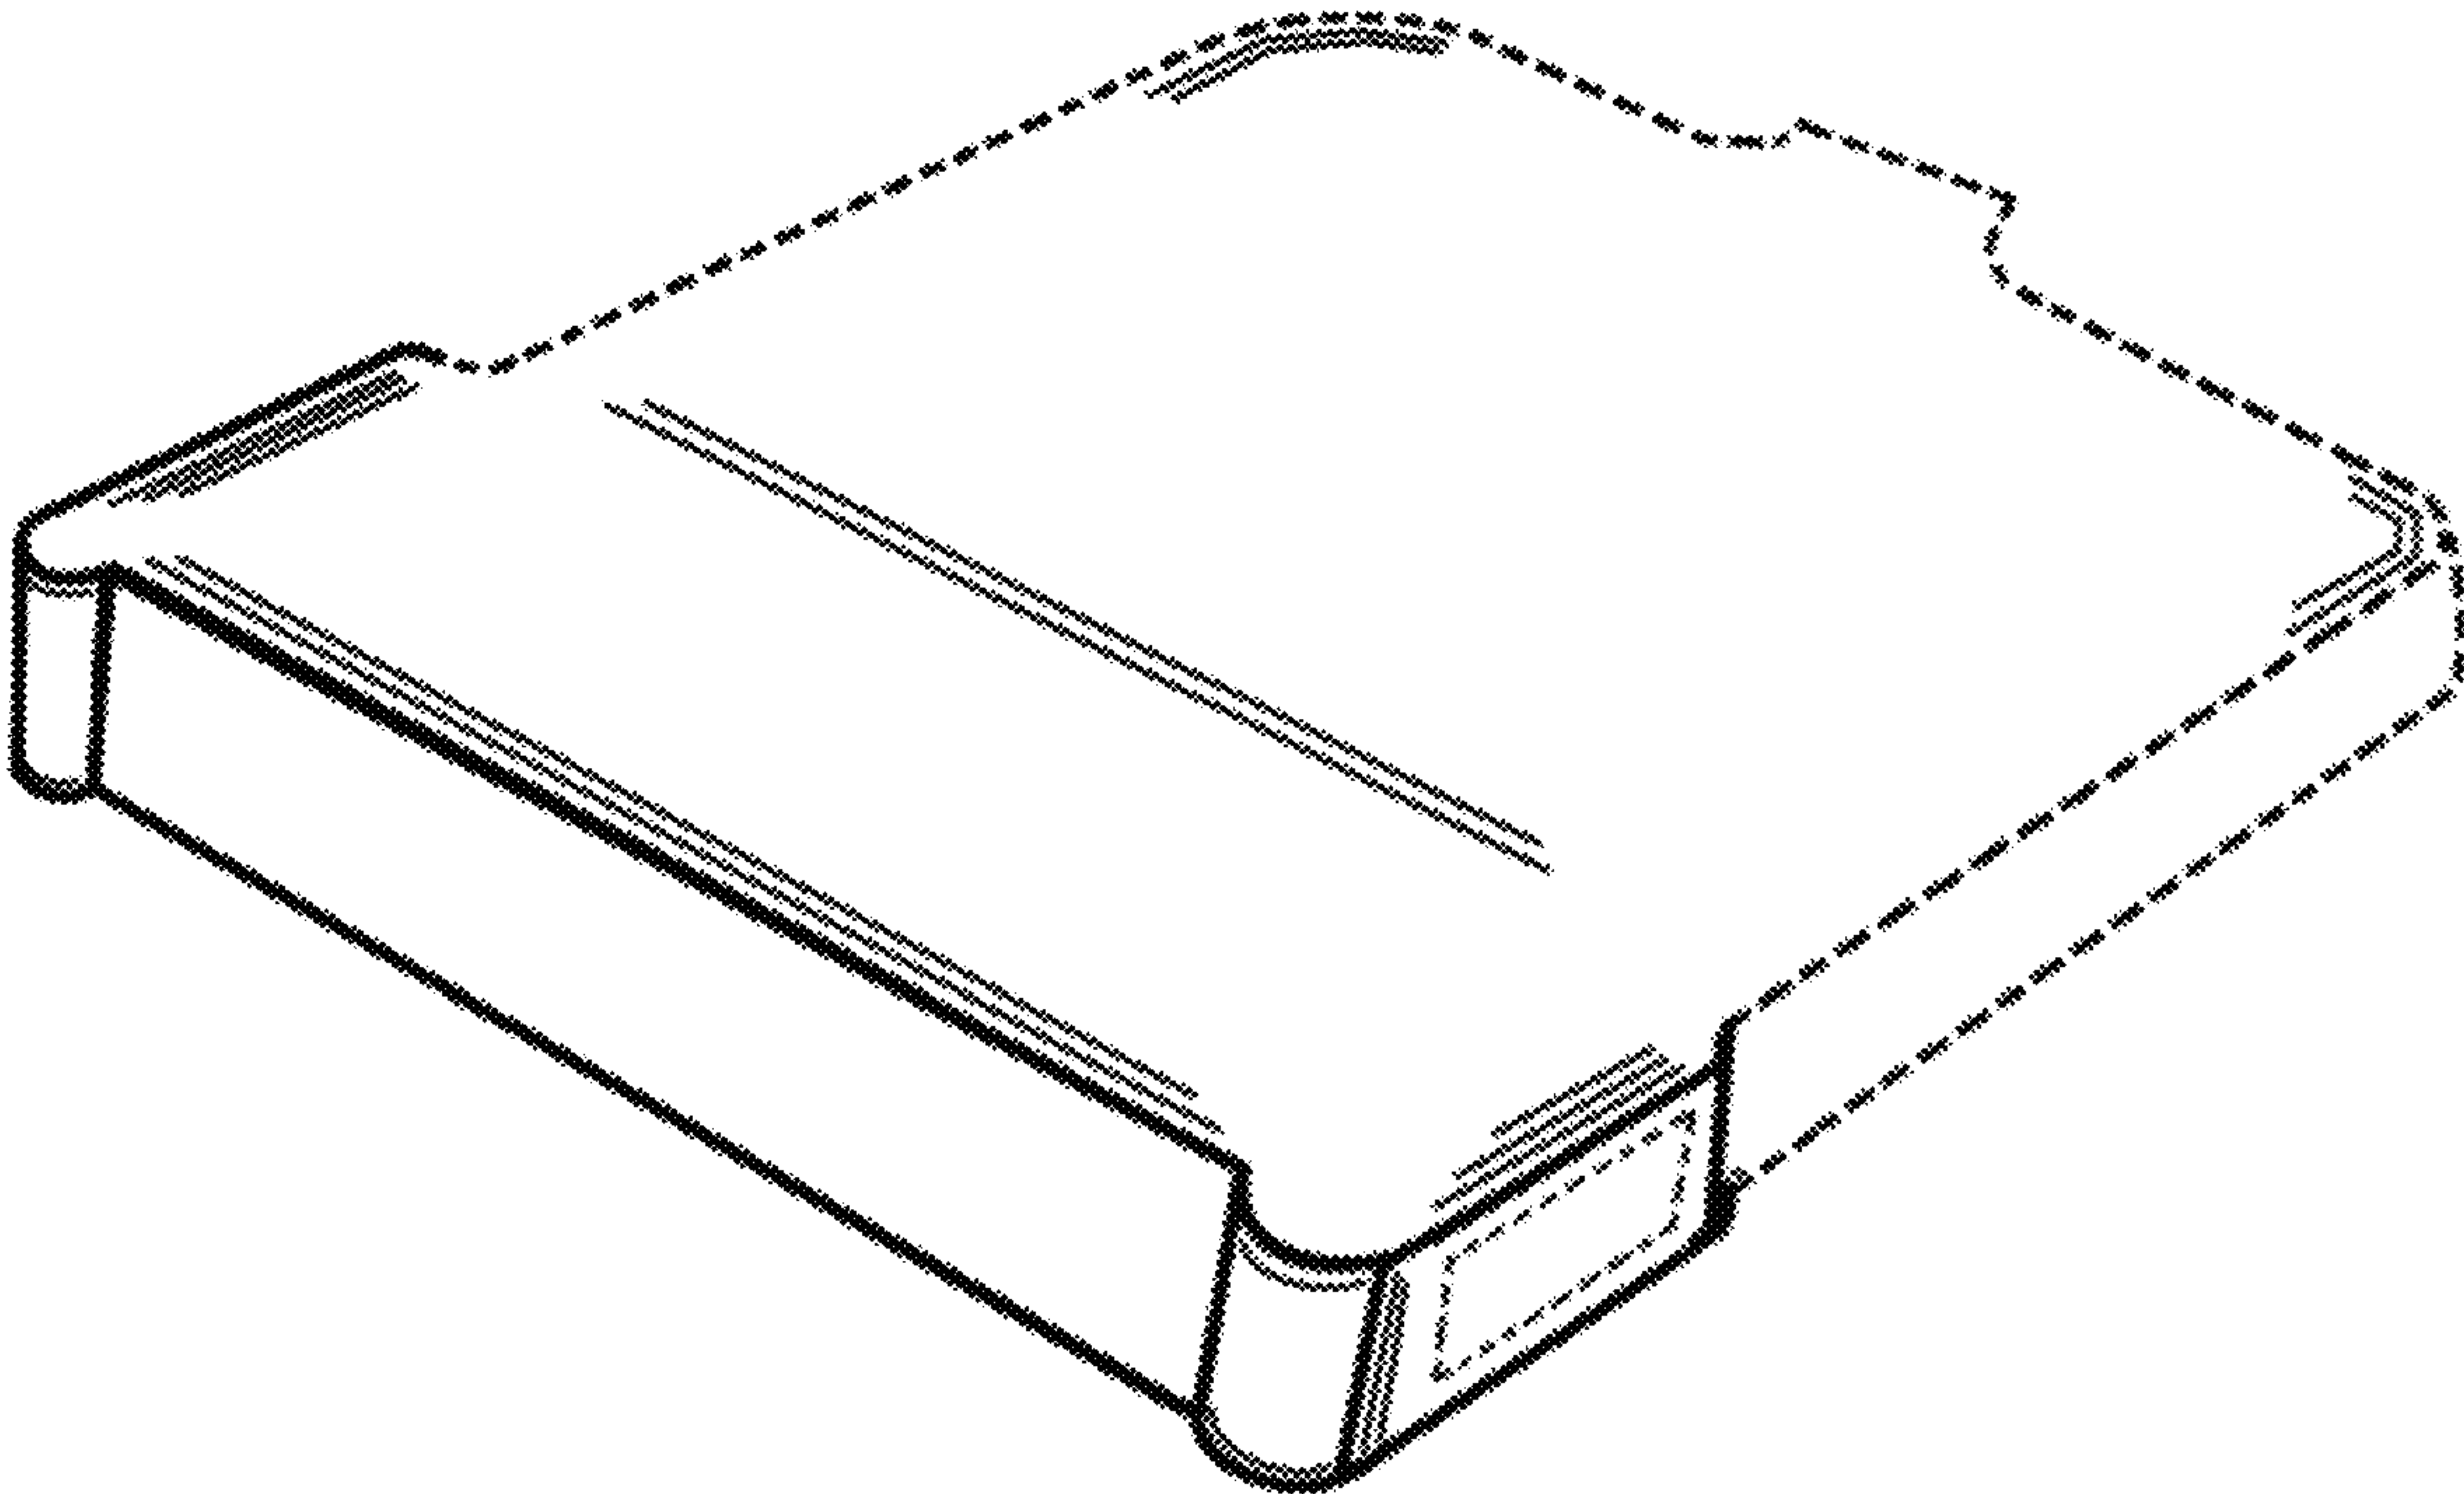

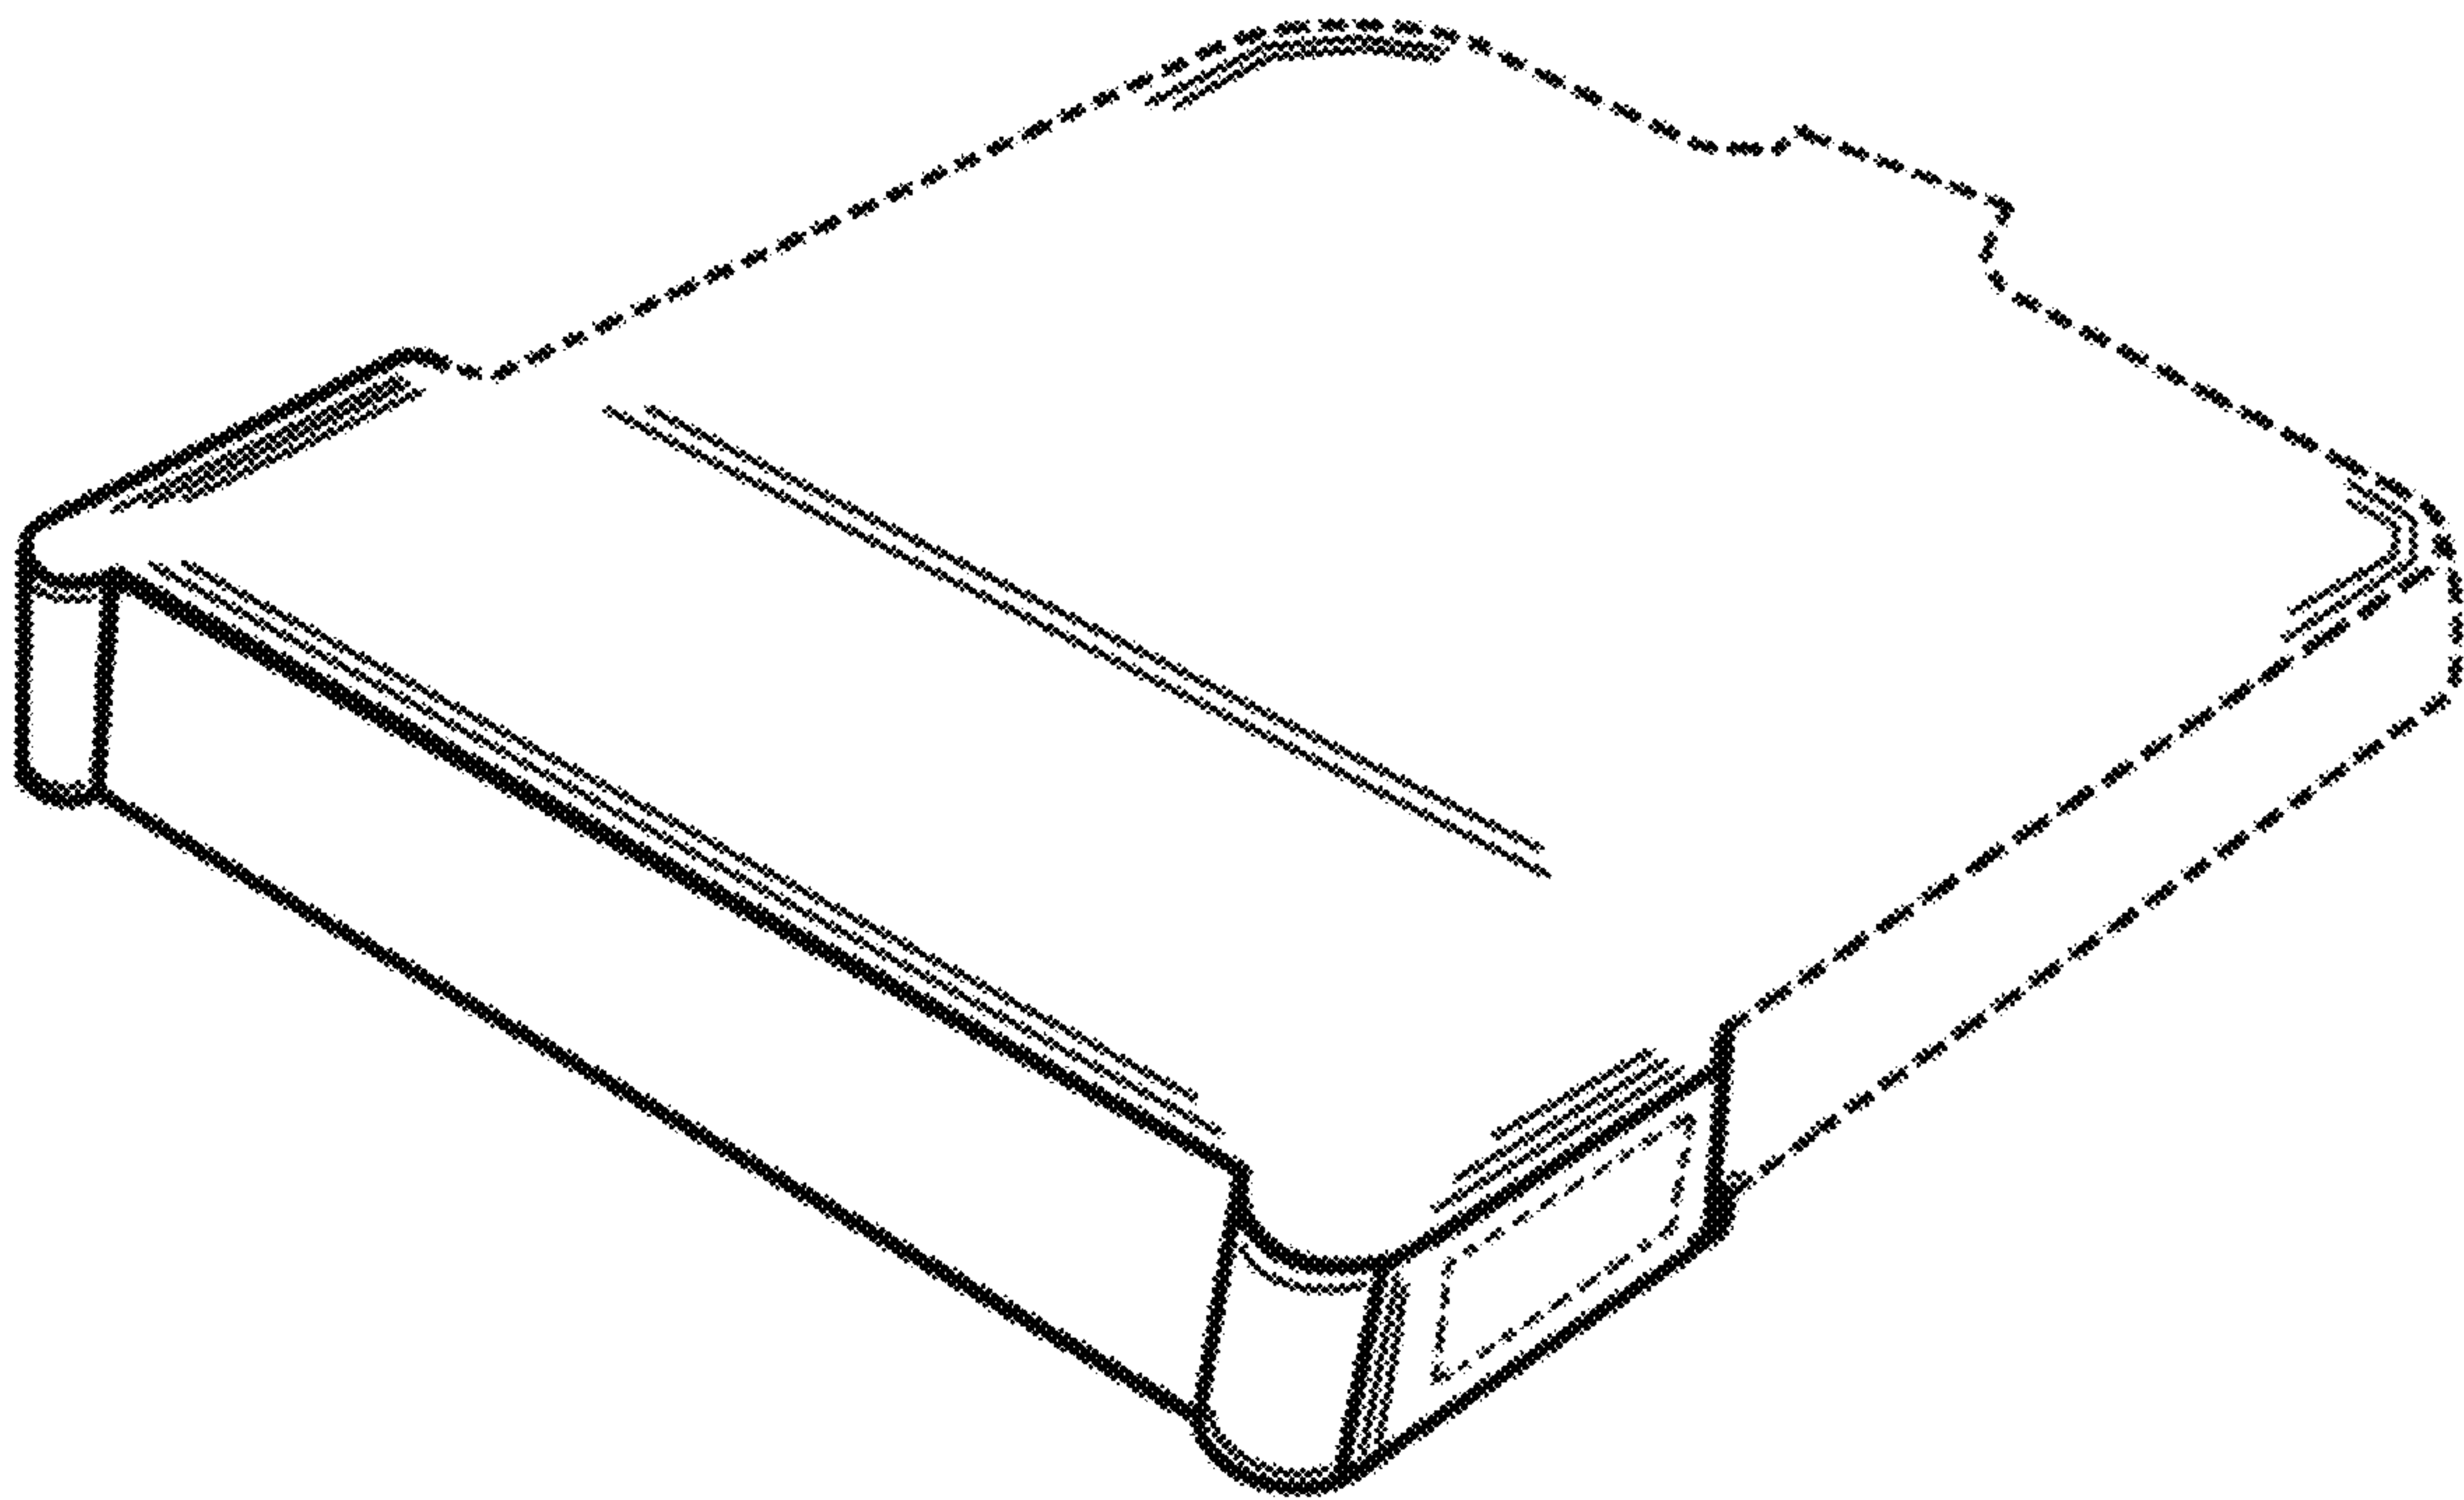


FIG. 1

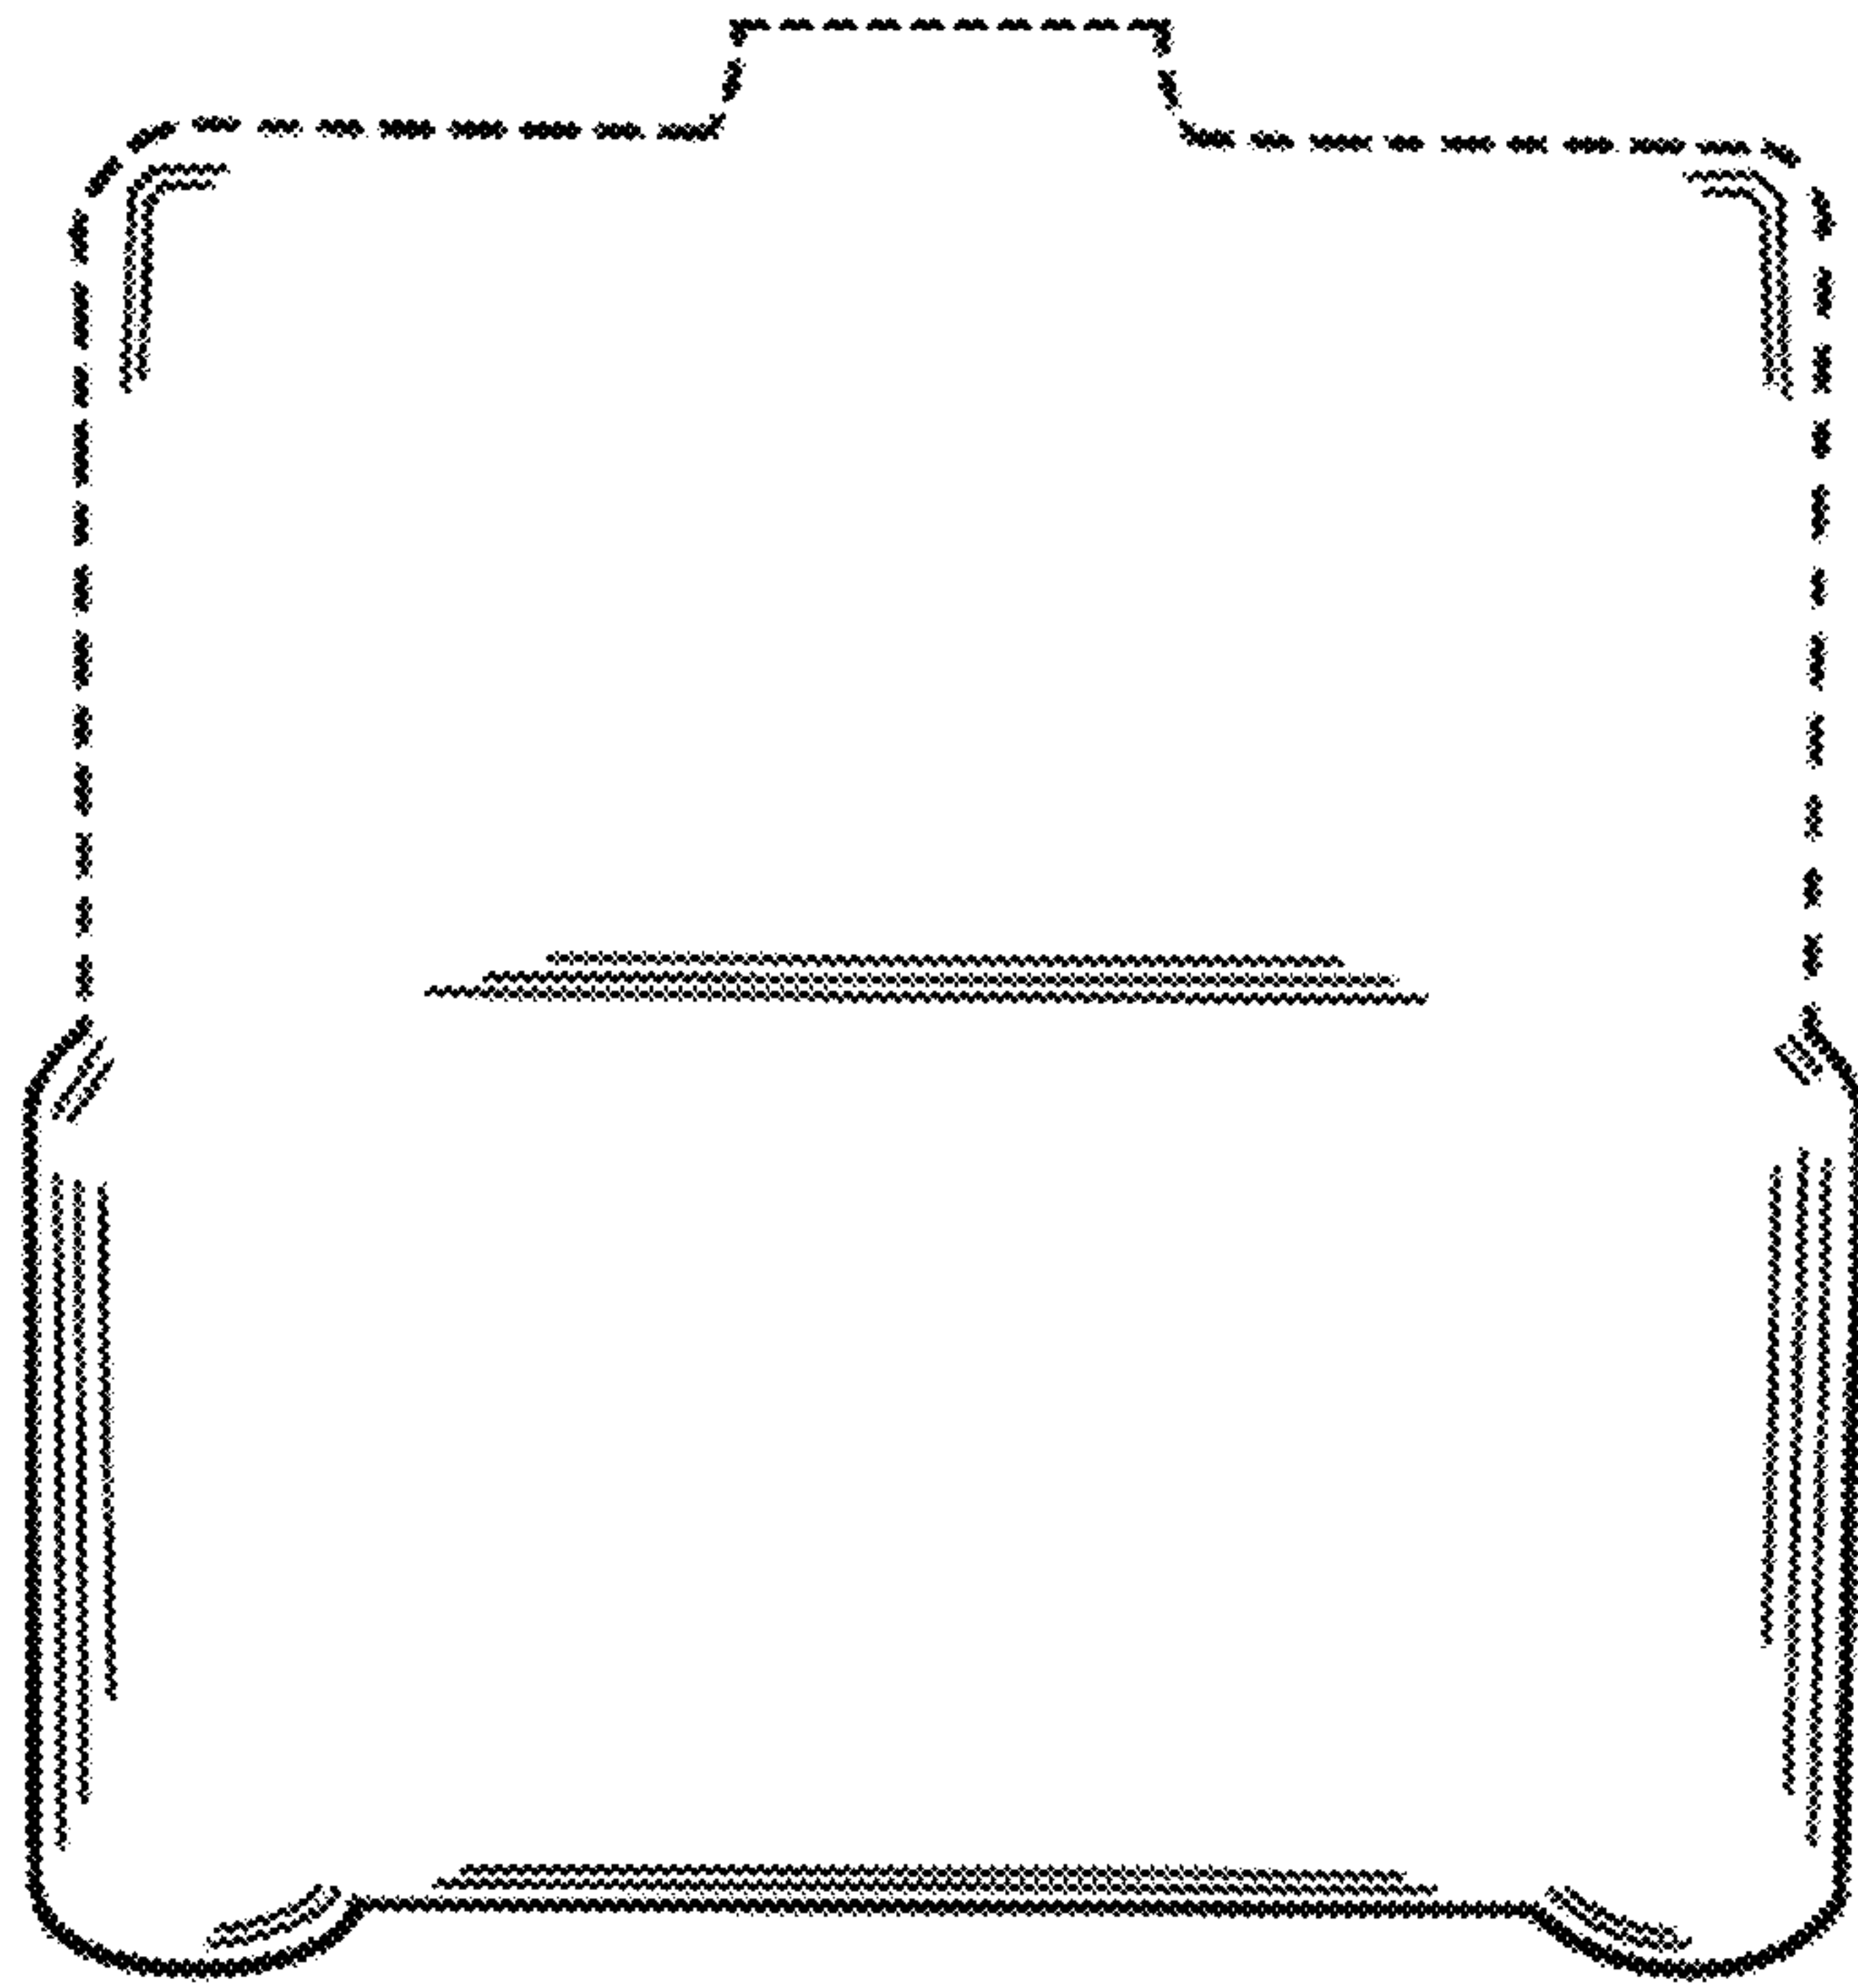


FIG. 2

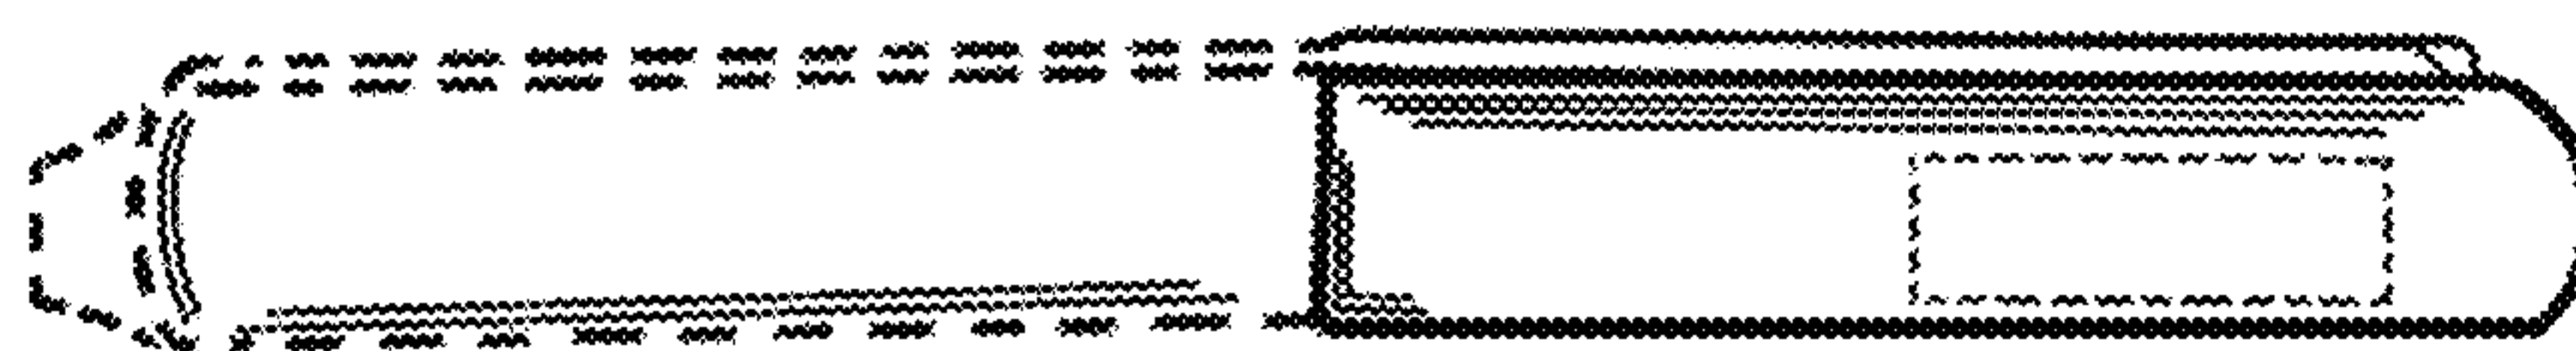


FIG. 3