

(12)

United States Design Patent
Brockway et al.

(10)

Patent No.: US D1,101,156 S

(45)

Date of Patent: ** Nov. 4, 2025

(54) **MONITORING APPARATUS**

(71) Applicant: **VivaQuant, Inc**, Arden Hills, MN (US)

(72) Inventors: **Brian Brockway**, St. Paul, MN (US);
Garrett Charles Duffy, St. Paul, MN (US)

(73) Assignee: **VivaQuant, Inc**, Arden Hills, MN (US)

(**) Term: **15 Years**

(21) Appl. No.: **29/907,856**

(22) Filed: **Jan. 9, 2024**

(51) **LOC (15) Cl.** **24-02**

(52) **U.S. Cl.**
USPC **D24/167**; D24/168; D24/186; D24/187

(58) **Field of Classification Search**
USPC D24/107, 164, 167–168, 185–187, 200,
D24/231; D10/46, 52, 53, 57, 70, 75, 81,
D10/96, 103; D14/344, 388, 218, 203.5
CPC A61B 5/02; A61B 5/0205; A61B 5/6801;
A61B 5/6813; A61B 5/0245; A61B 5/68;
A61B 5/6802
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D565,182	S	*	3/2008	Cheng		D24/186
D852,965	S	*	7/2019	Bahney		A61B 5/6833
						D24/186
D854,169	S		7/2019	Briante et al.		
D864,400	S		10/2019	Benedikter		
D921,204	S		6/2021	Golda et al.		
D932,017	S		9/2021	Lam		
D940,332	S	*	1/2022	Weichert		D24/186
D940,881	S	*	1/2022	Hadley		D24/186
D958,992	S		7/2022	Duffy et al.		
D972,737	S	*	12/2022	Lewis, Jr.		D24/187
D975,288	S	*	1/2023	Zimmermann		D24/186
D994,886	S	*	8/2023	Lam		D24/167

D1,017,051	S	*	3/2024	Fang		D24/187
D1,029,276	S	*	5/2024	Huang		D24/168
12,109,033	B1	*	10/2024	Duffy		A61B 5/282
D1,057,167	S	*	1/2025	Zhuang		D24/167
D1,063,079	S	*	2/2025	Abercrombie, II	..	H05K 5/0026
						D24/187

(Continued)

FOREIGN PATENT DOCUMENTS

CN	201730271694		1/2018
CN	309280227	*	5/2025

(Continued)

OTHER PUBLICATIONS

Heart Blog, Unveiling the Benefits of Holter Monitoring for Patients, Published: Sep. 23, 2023, hgssuperspecialityclinic.com, Retrieved from: <https://hgssuperspecialityclinic.com/heart-blog/f/unveiling-the-benefits-of-holter-monitoring-for-patients?blogcategory=Arrhythmia> (Year: 2023).*

(Continued)

Primary Examiner — Jennifer L Rempfer
Assistant Examiner — Edward P Jones
(74) Attorney, Agent, or Firm — Crawford Maunu PLLC


(57) **CLAIM**

The ornamental design for a monitoring apparatus as shown and described.

DESCRIPTION

FIG. 1 is a top perspective view of a monitoring apparatus; FIG. 2 is a bottom perspective view thereof; FIG. 3 is a top view thereof; FIG. 4 is a bottom view thereof; FIG. 5 is a right side view thereof; FIG. 6 is a front view thereof; and, FIG. 7 is a rear view thereof.

1 Claim, 6 Drawing Sheets

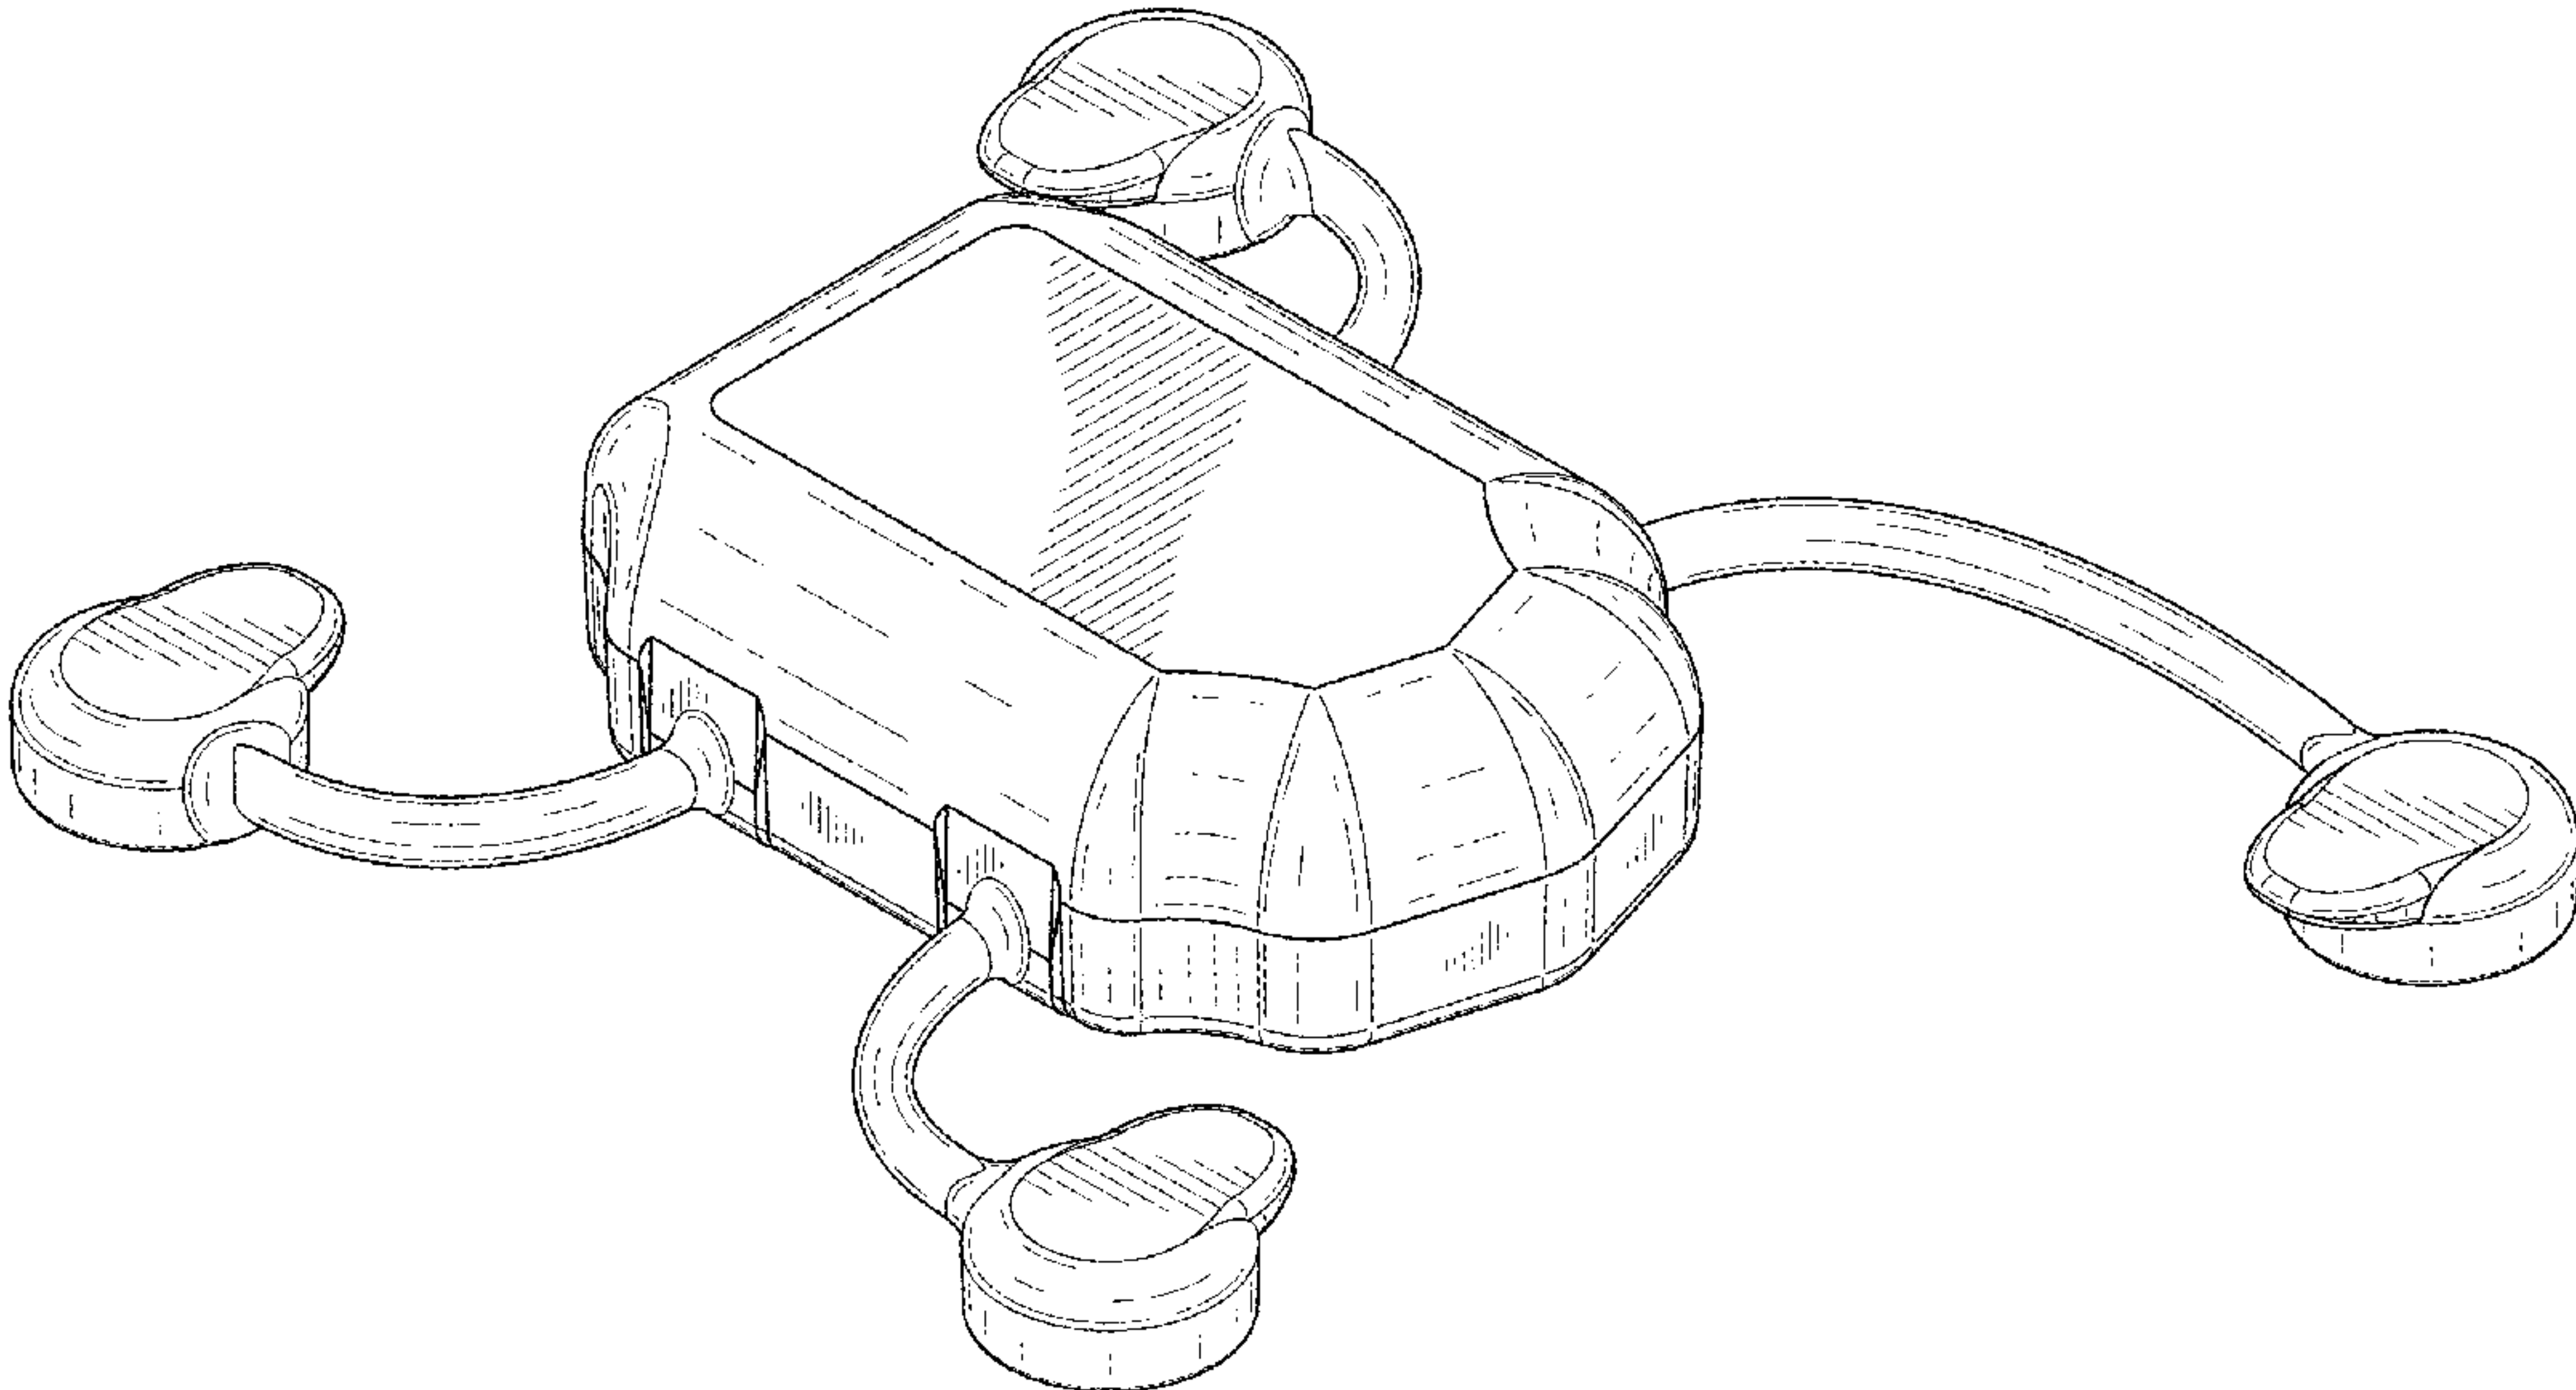

References Cited

2010/0185398	A1 *	7/2010	Berns	A61B 5/6804 726/28
2012/0197150	A1	8/2012	Cao et al.	
2014/0213921	A1	7/2014	Brockway et al.	
2014/0364756	A1	12/2014	Brockway et al.	
2019/0350476	A1	11/2019	Buisson et al.	
2020/0029838	A1 *	1/2020	Tang	A61B 5/02116
2021/0244339	A1	8/2021	Szabados et al.	
2021/0275095	A1 *	9/2021	Sarussi	A61B 5/263
2023/0021804	A1 *	1/2023	Yu	A61B 5/259

JP	D1757269	* 11/2023
TW	237507-0001	* 4/2025

Jeff L., Linked In Post for The RX-1 mini, Published: May 2025, LinkedIn.com, Retrieved from: https://www.linkedin.com/posts/jefflorine_medicalsales-cardiologysales-electrophysiology-activity-7320653716955484161_g_eG (Year: 2025).*

Vivaquant, Archive Web Page of rhythmexpressecg.com, Published: Dec. 6, 2022, [web.archive.org](https://web.archive.org/web/20221206102334/https://rhythmexpressecg.com/), Retrieved from: <https://web.archive.org/web/20221206102334/https://rhythmexpressecg.com/> (Year: 2022).*

Biotricity, What Is a Cardiac Patch Monitor? Your Guide to Monitoring with a Heart Patch Monitor, Published: Apr. 17, 2025, biotricity.com, Retrieved from: <https://biotricity.com/2025/04/17/what-is-a-cardiac-patch-monitor-your-guide-to-monitoring-with-a-heart-patch-monitor/> (Year: 2025).*

* cited by examiner

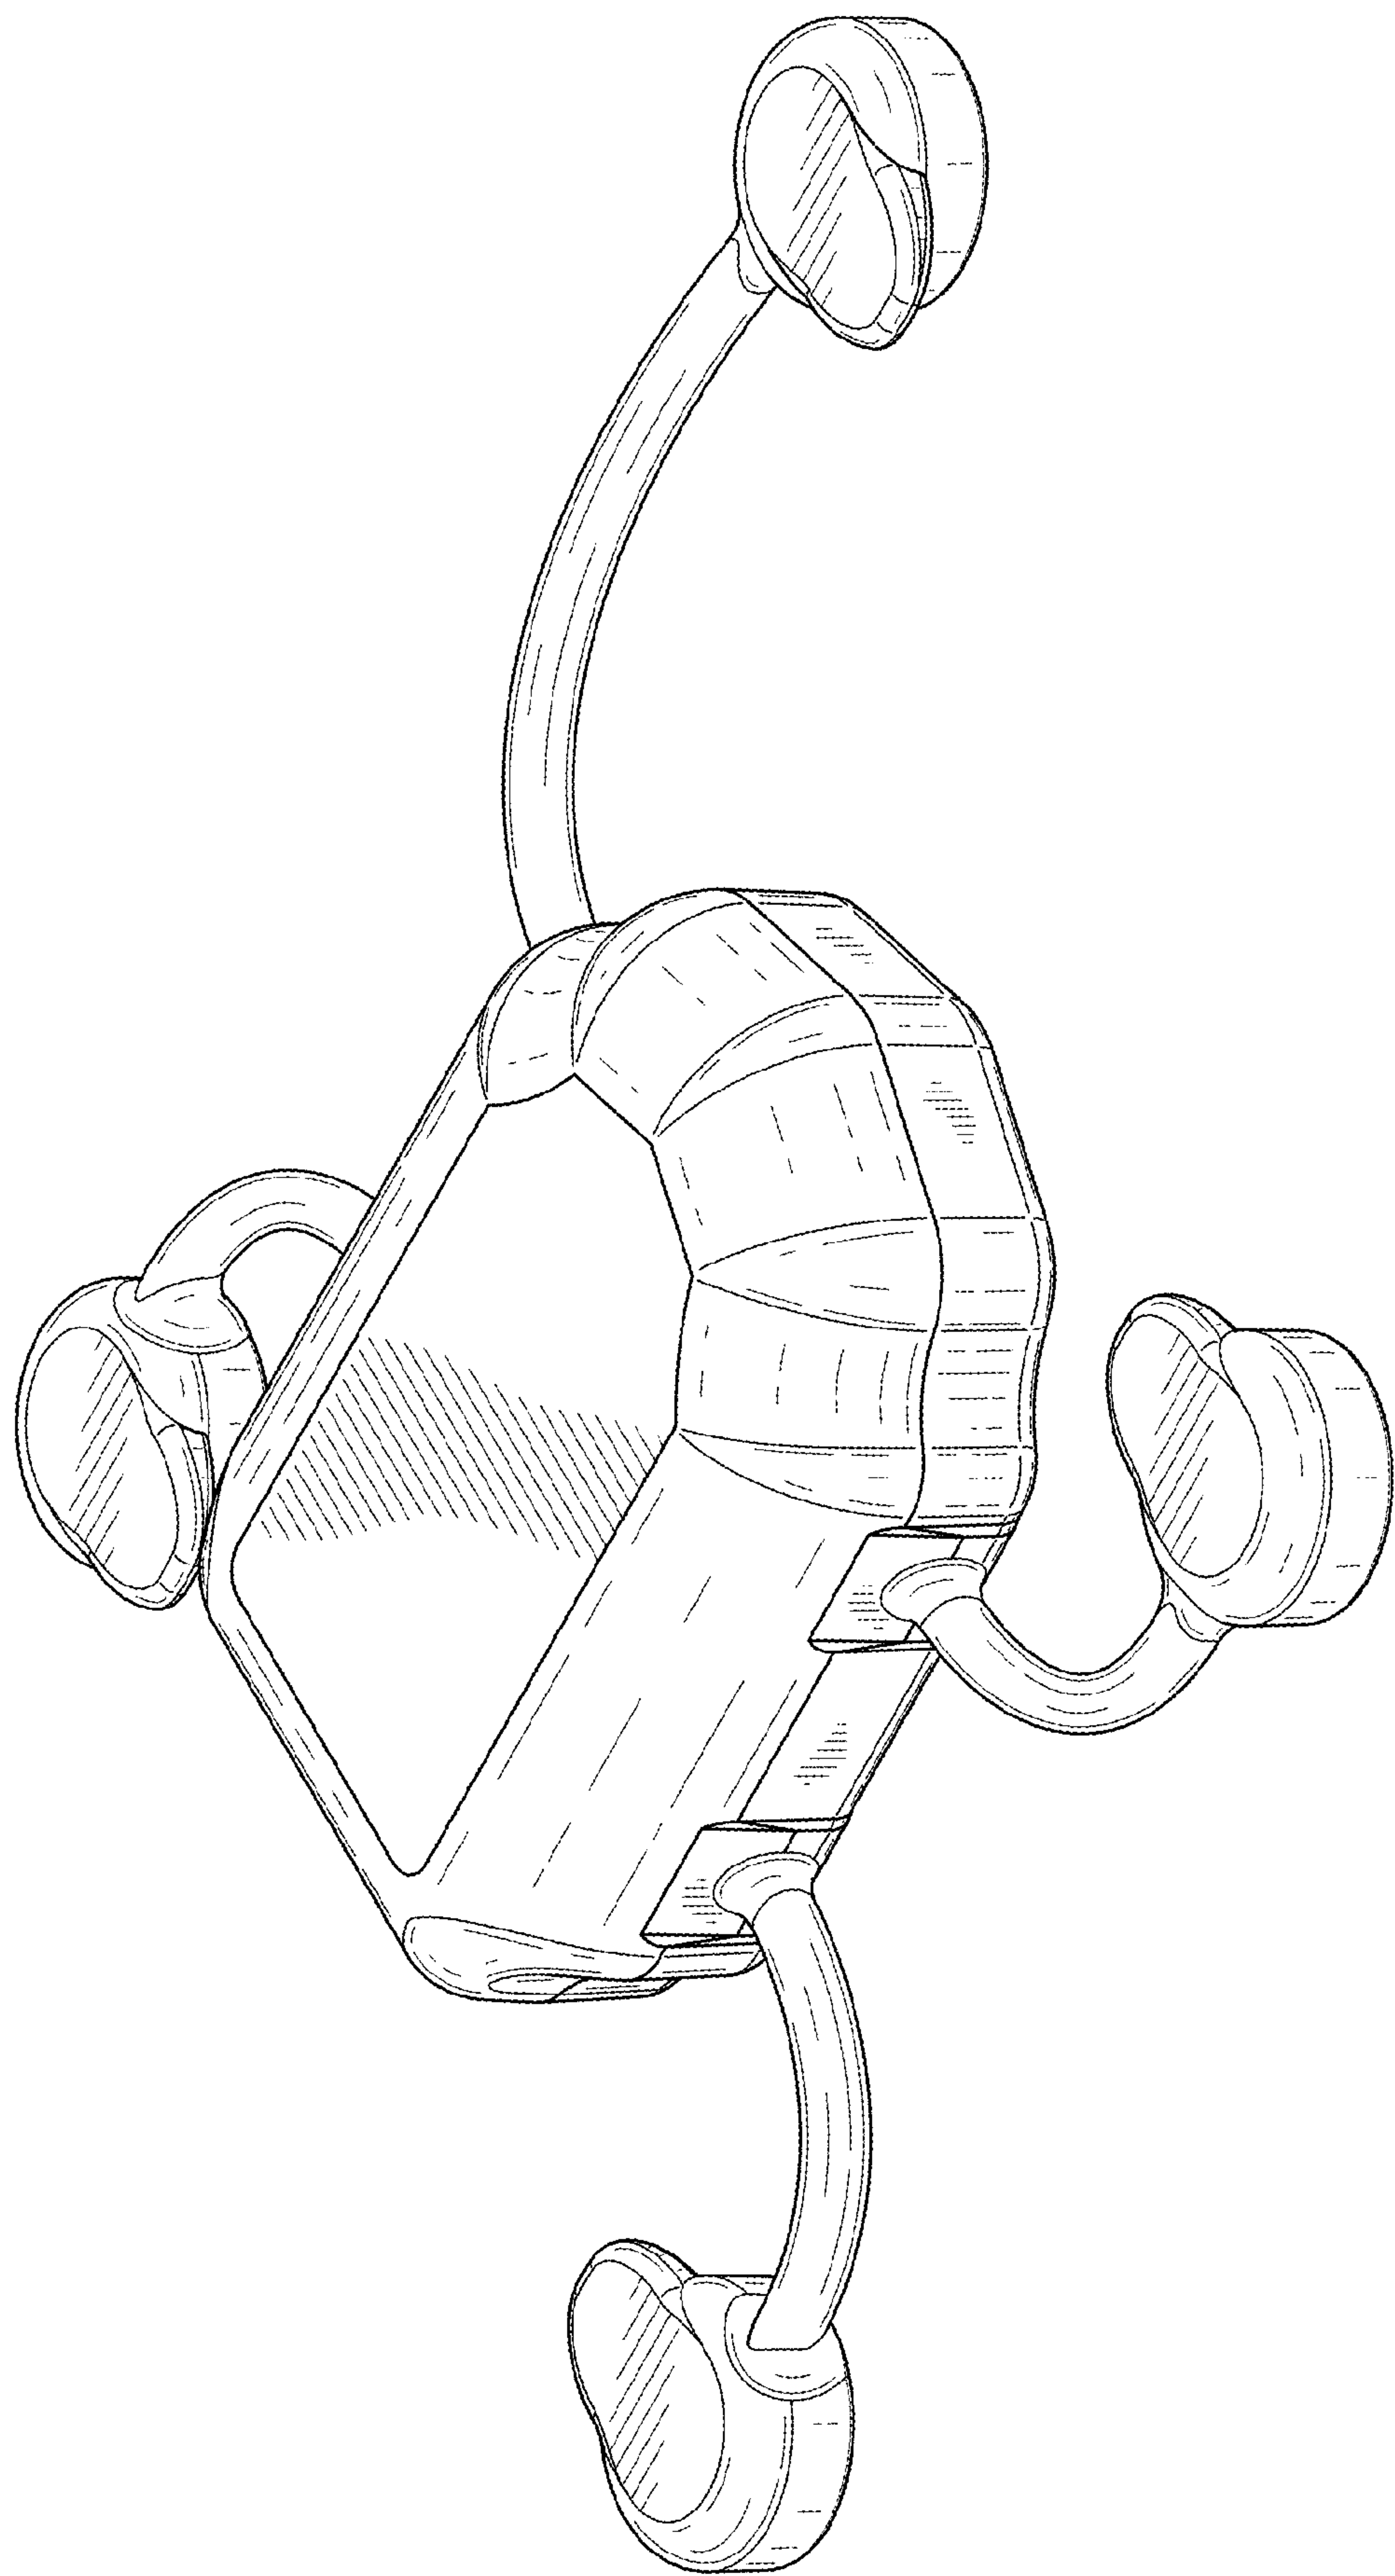


FIG. 1

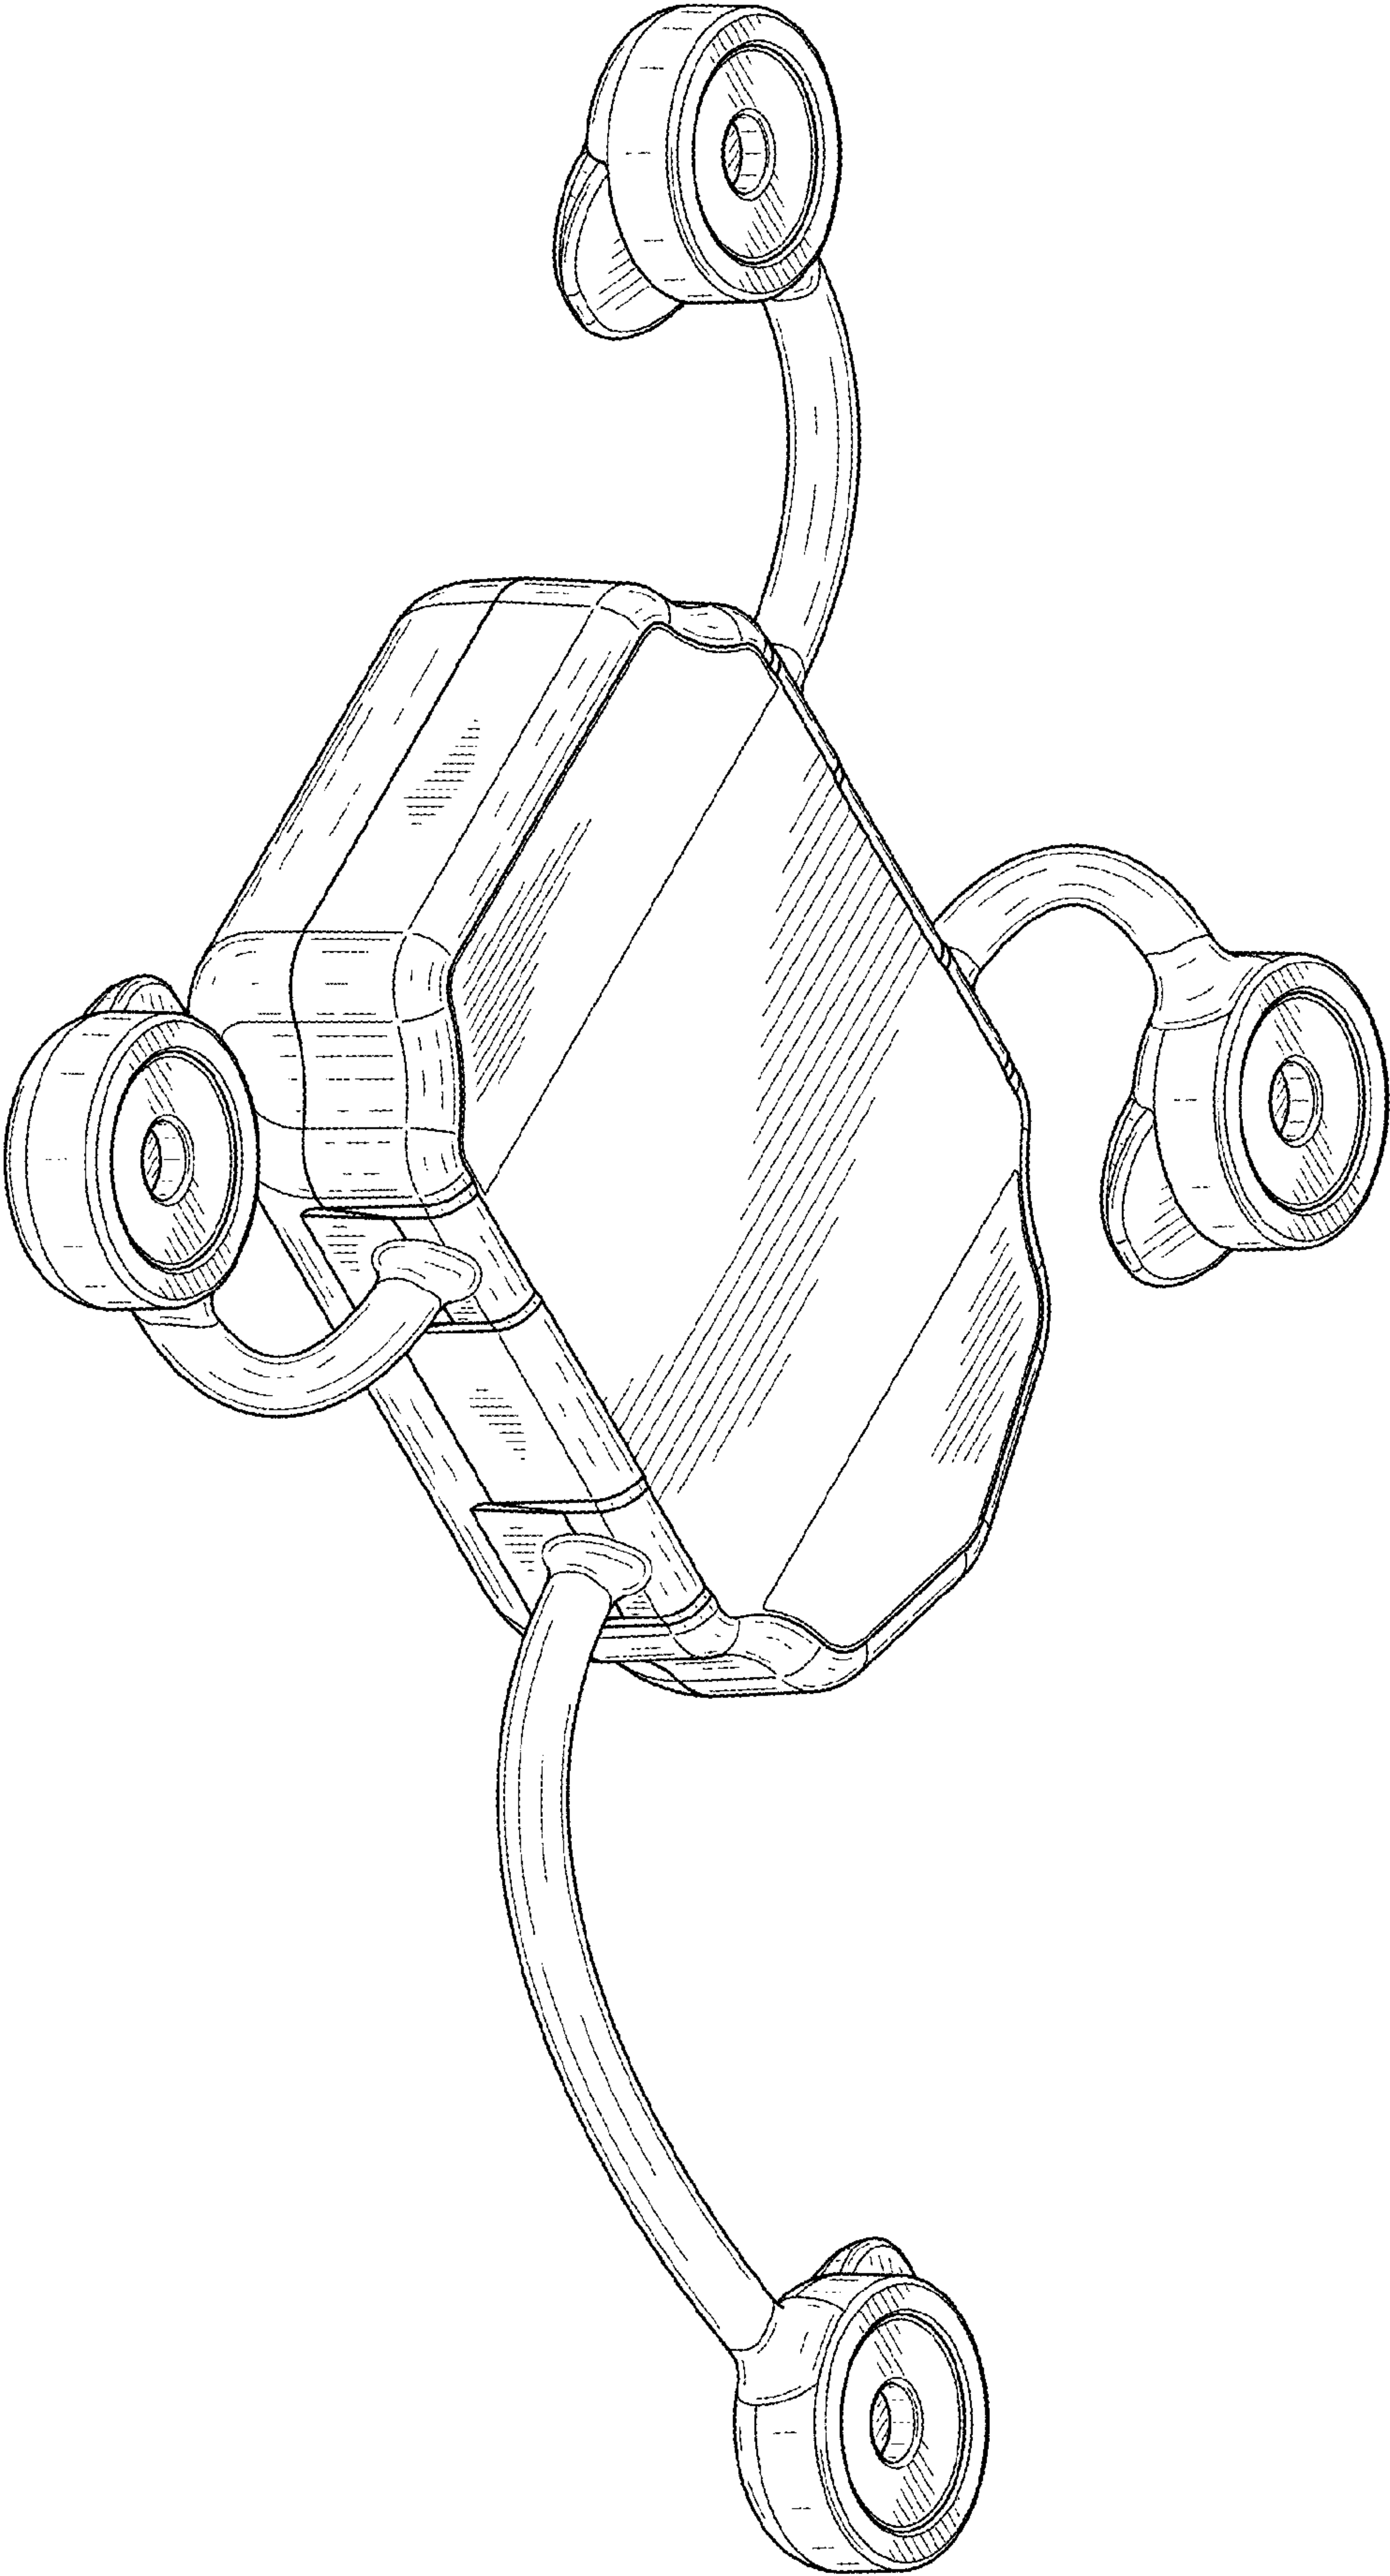


FIG. 2

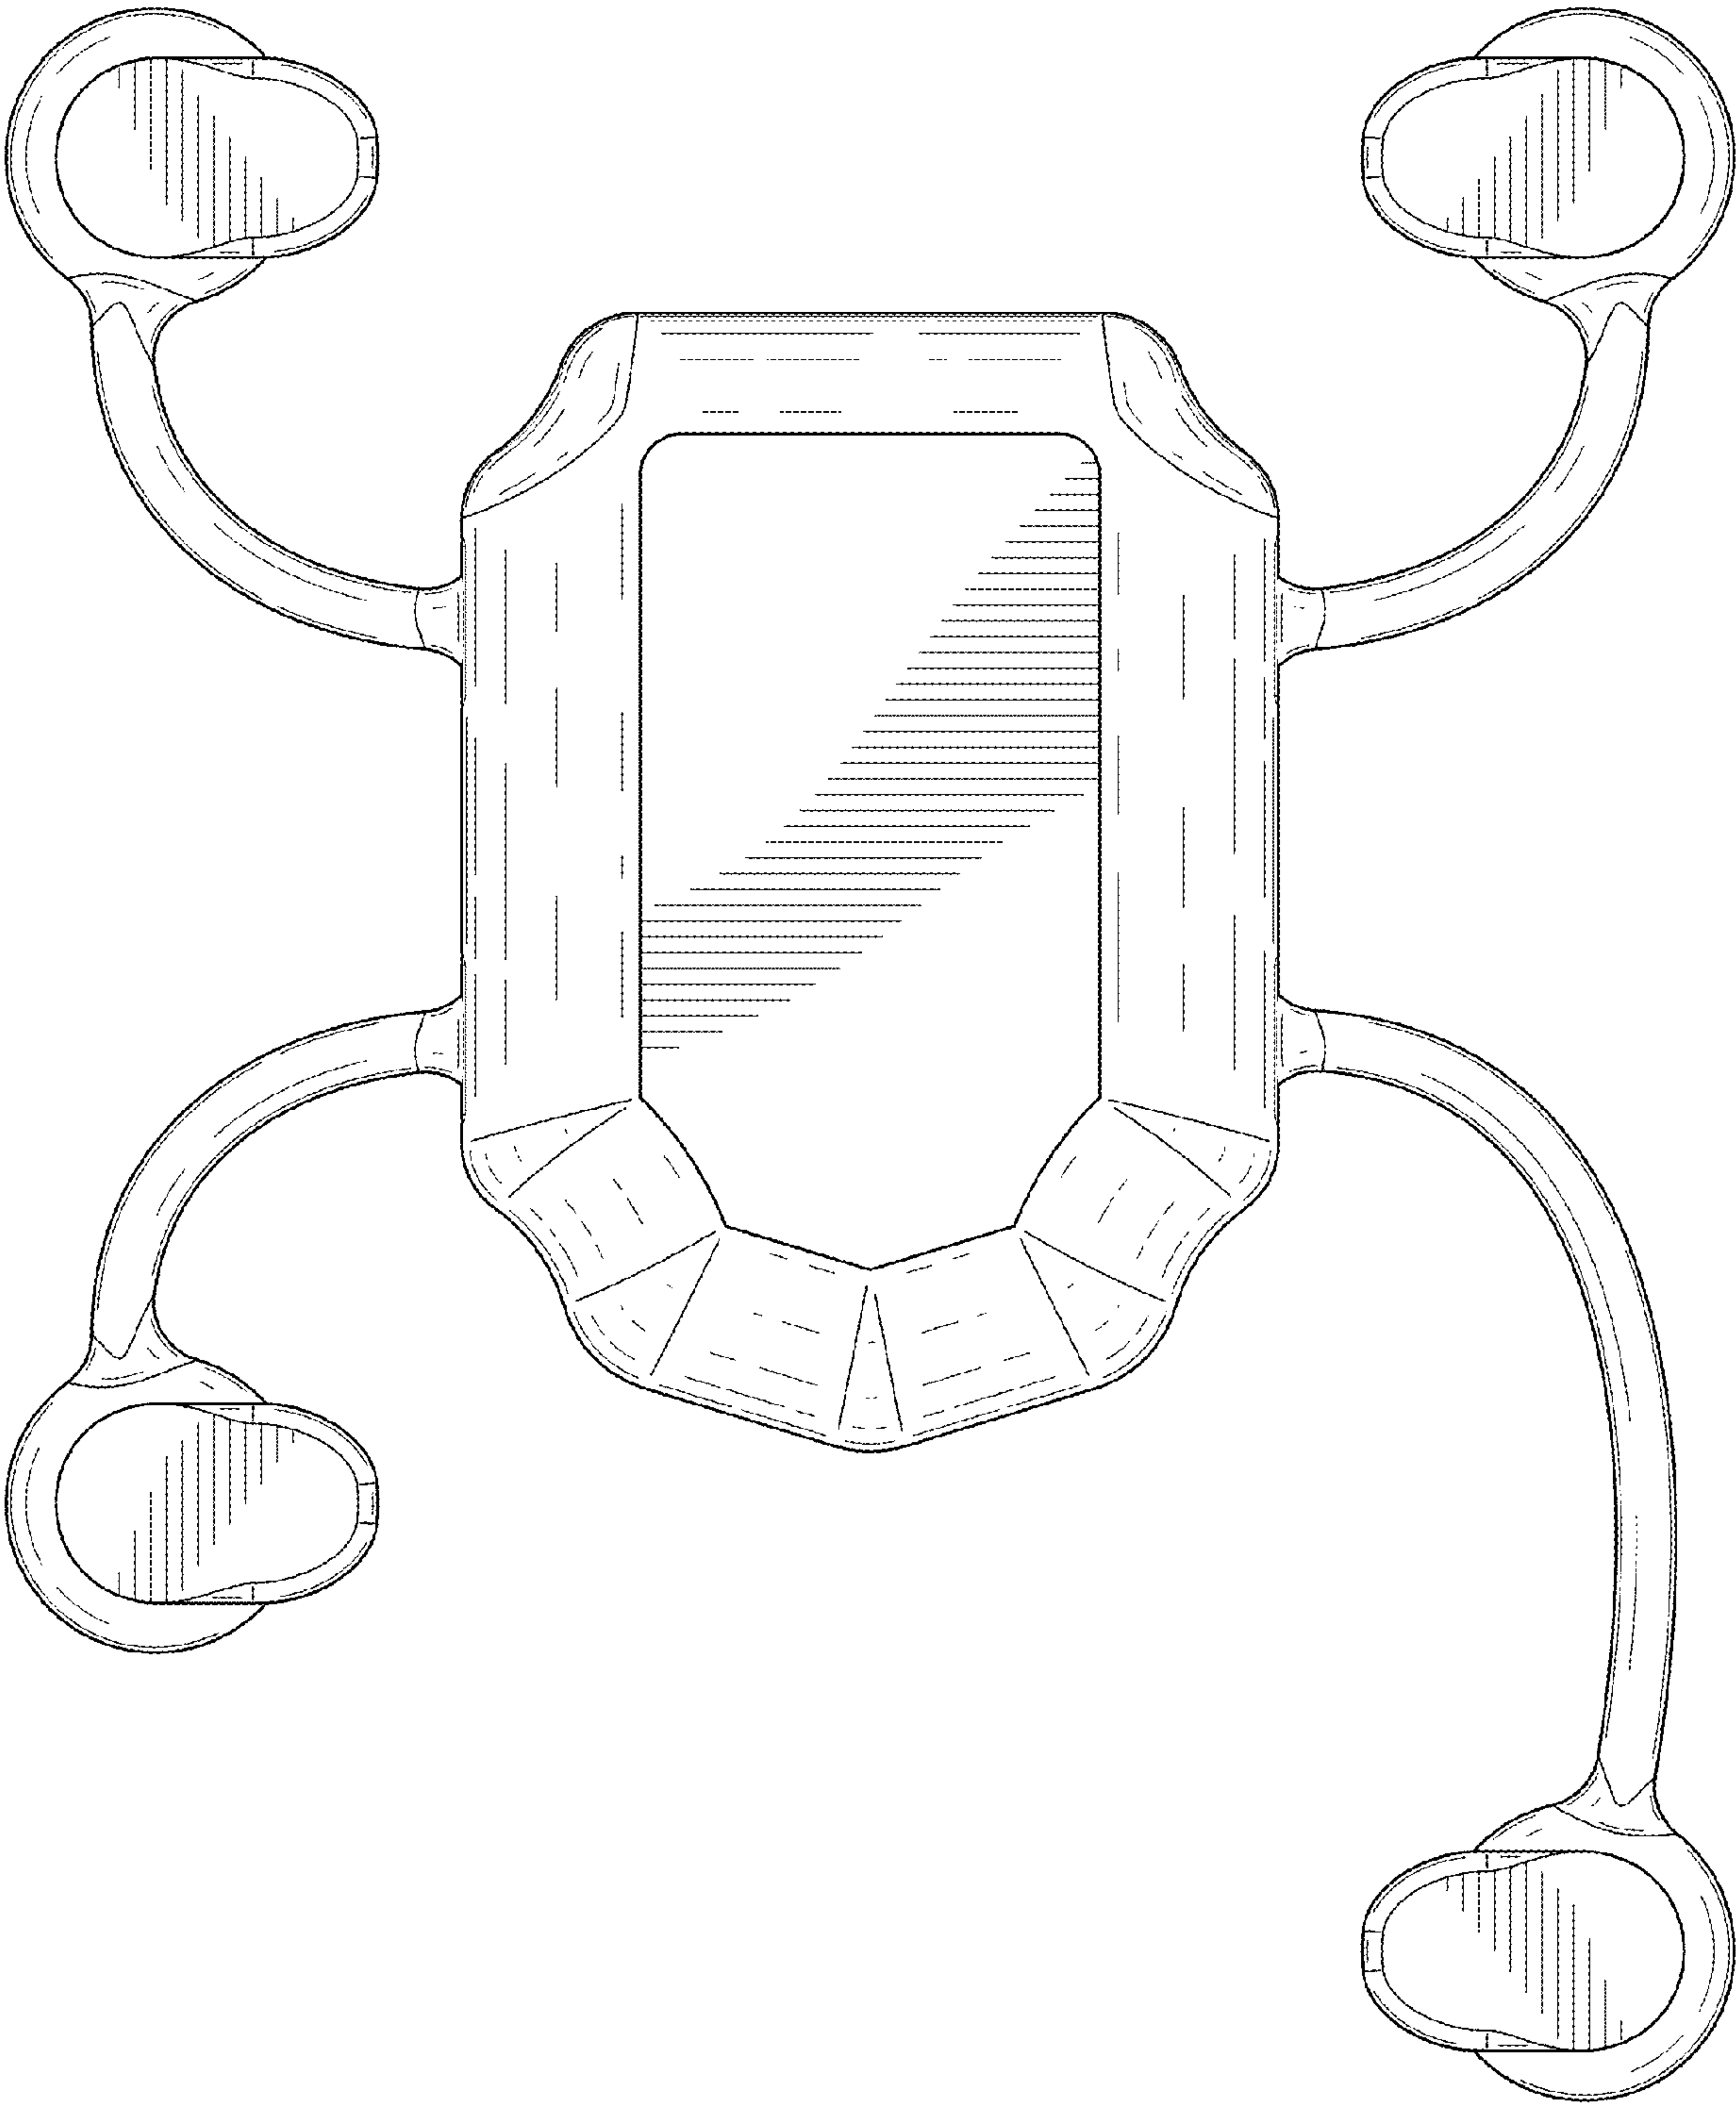


FIG. 3

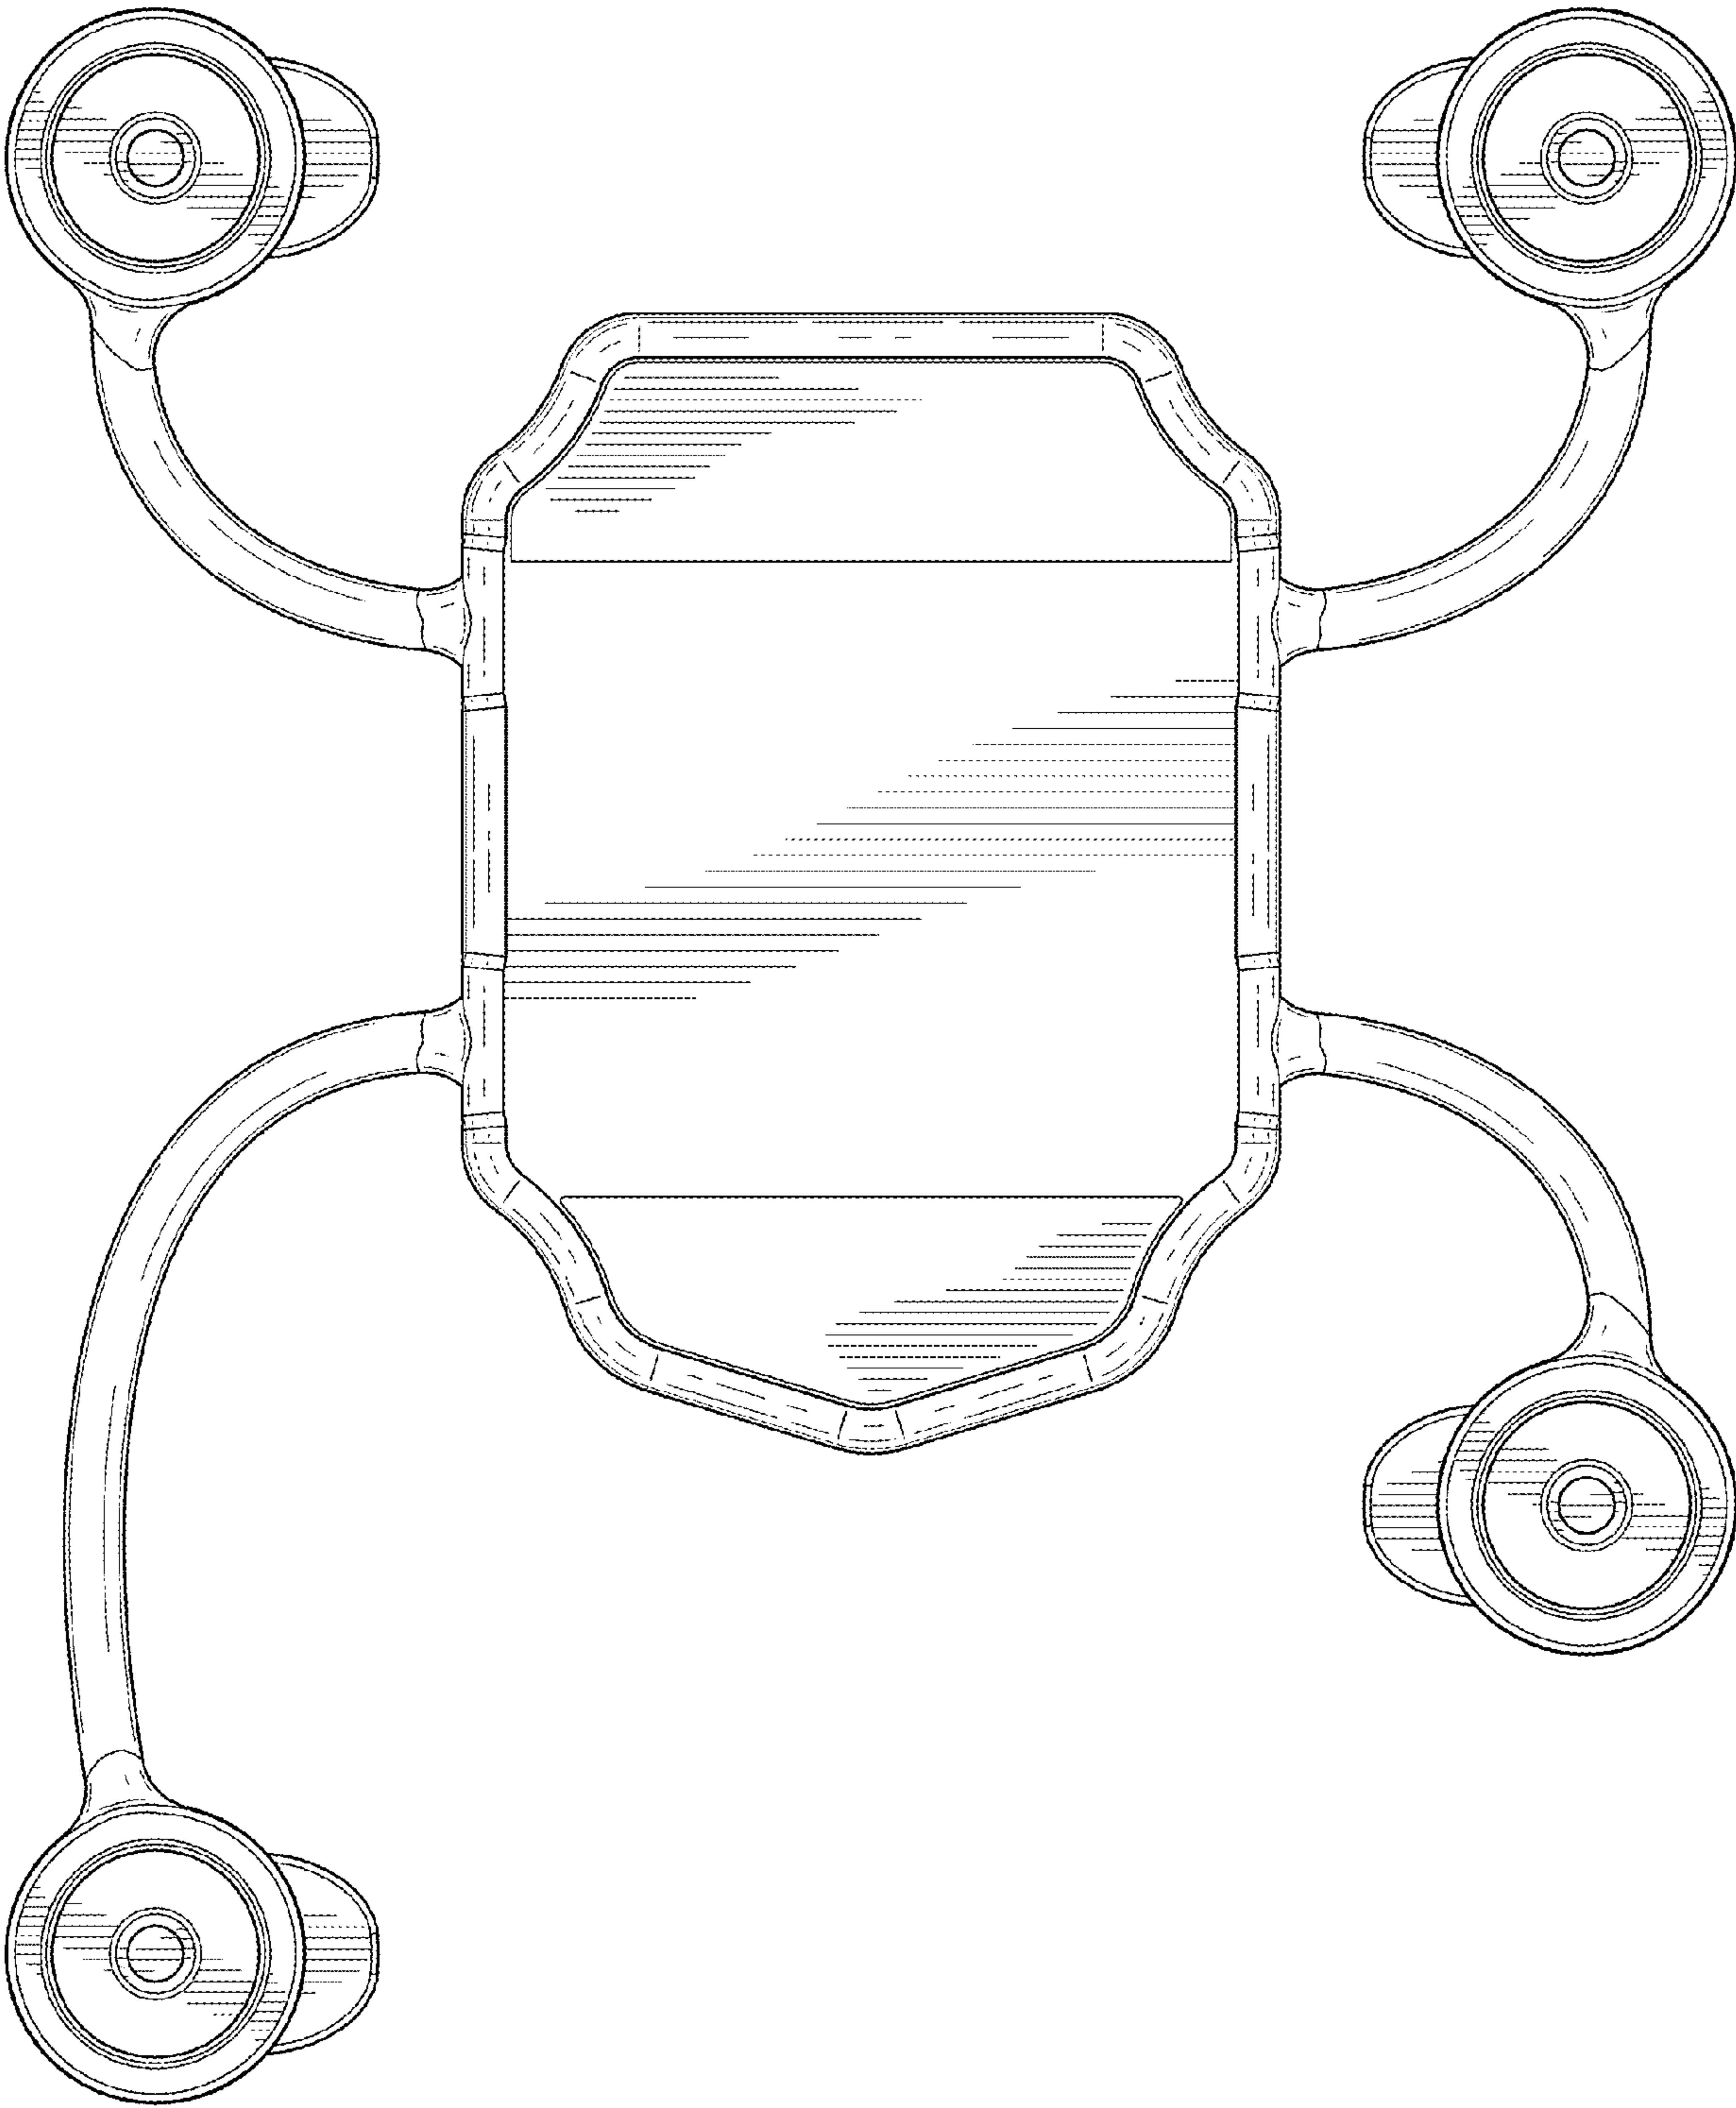


FIG. 4

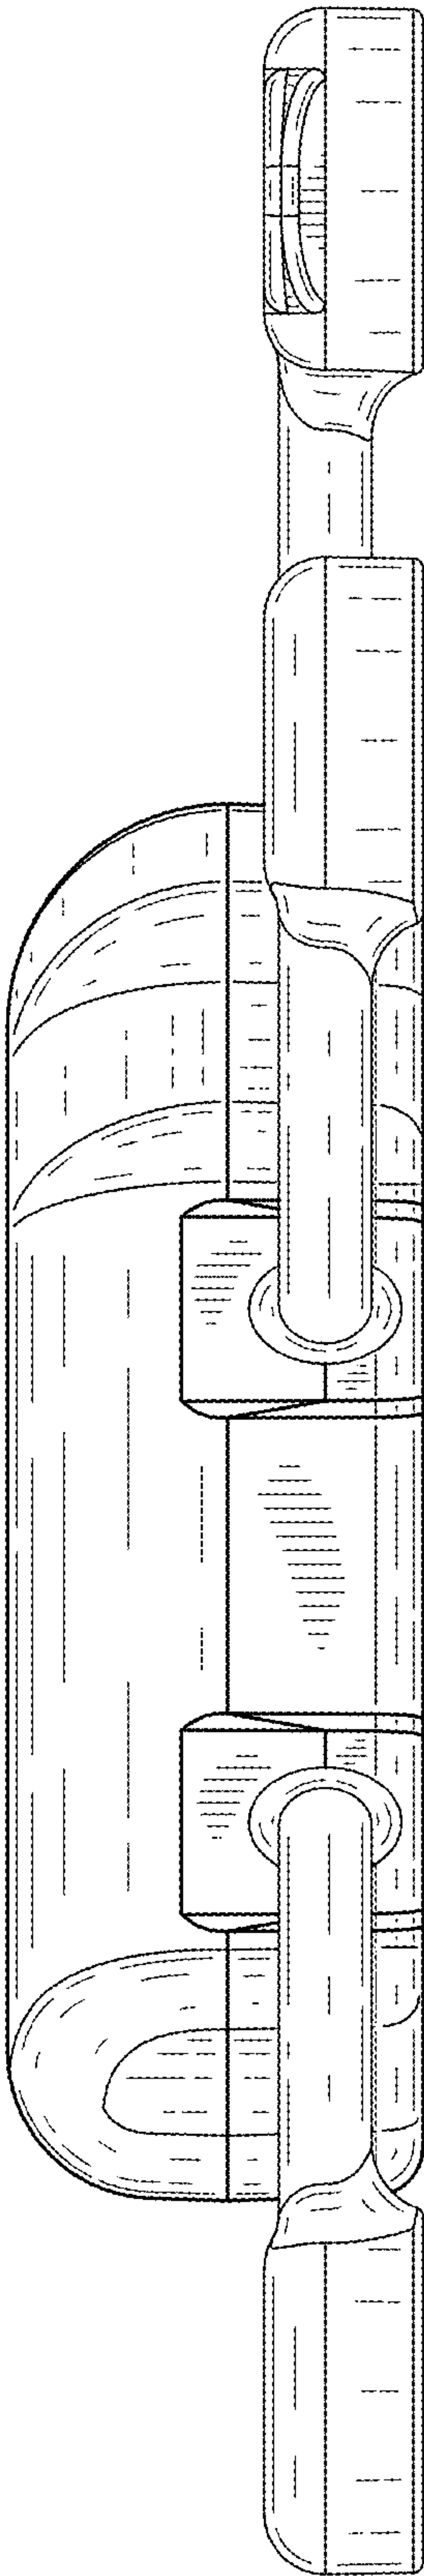


FIG. 5

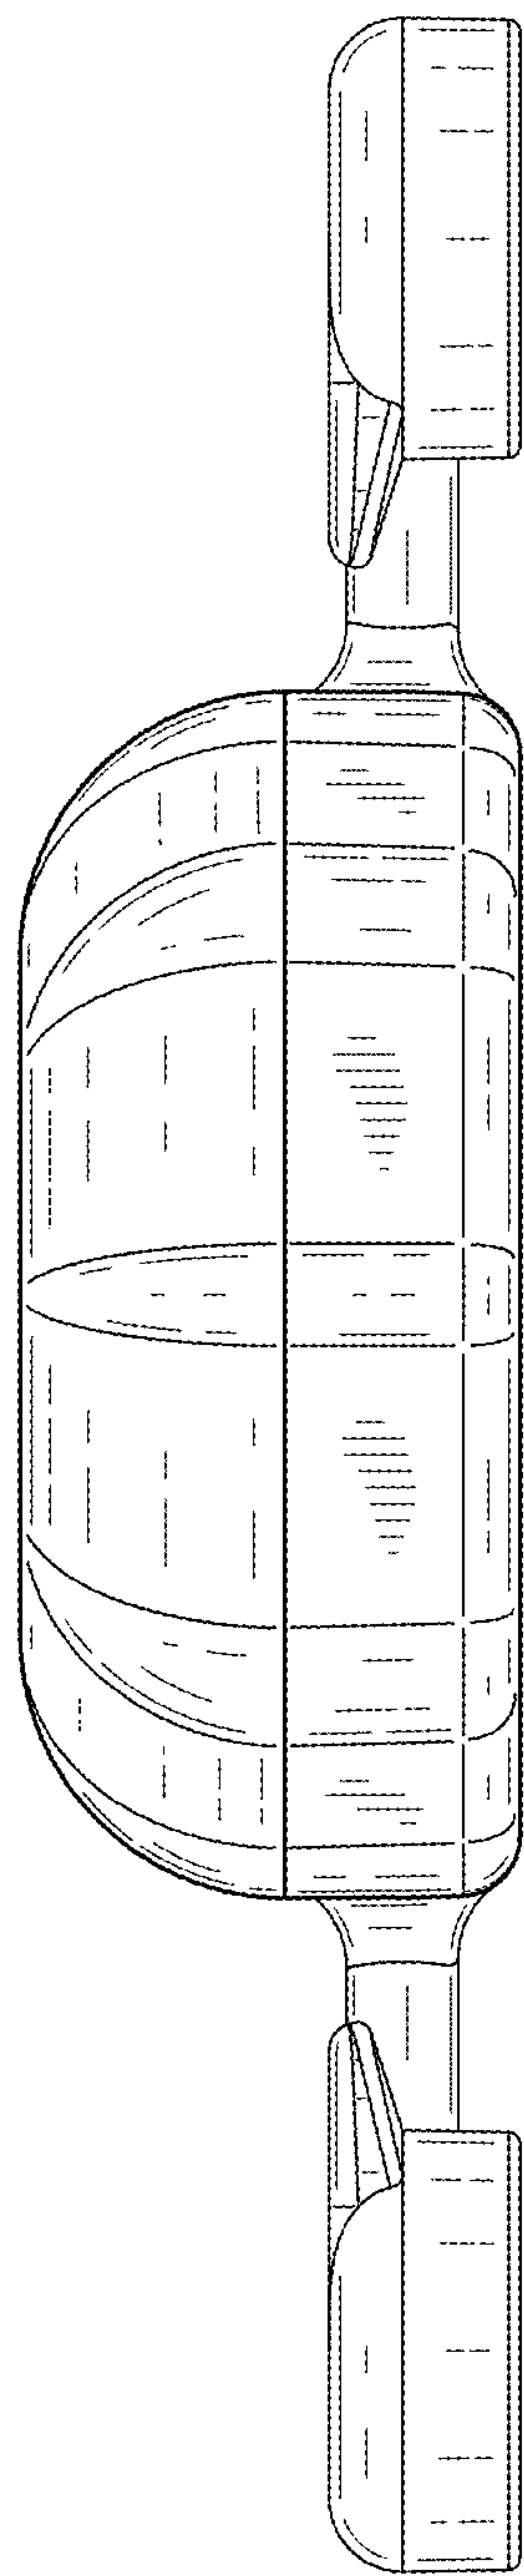


FIG. 6

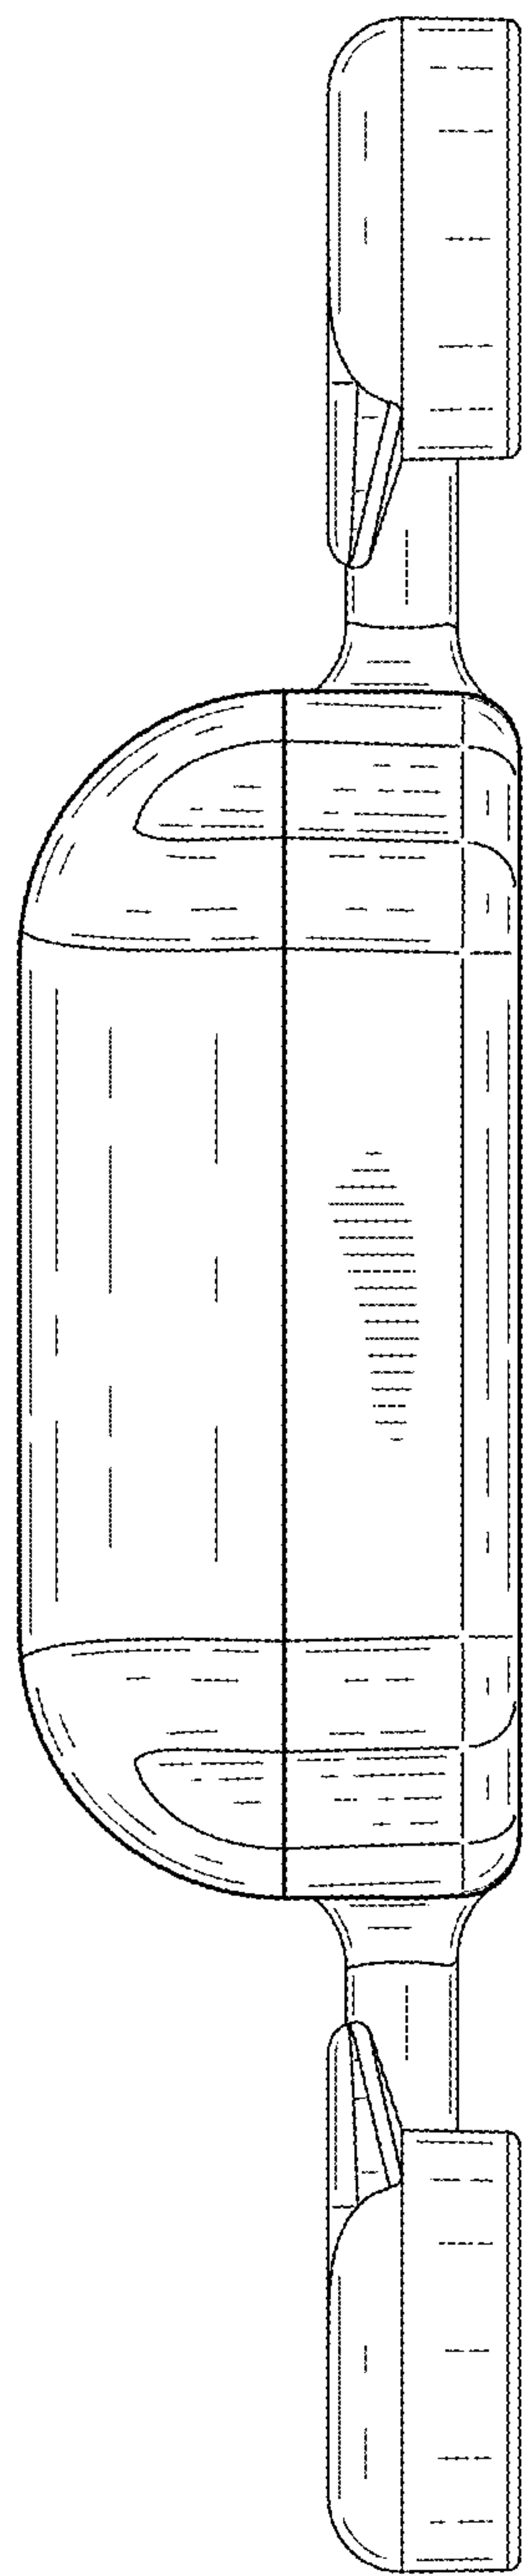


FIG. 7