



US0D1105434S

(12)

United States Design Patent

Cramer

(10)

Patent No.:

US D1,105,434 S

(45)

Date of Patent:

** Dec. 9, 2025

(54) SMART PATCH DEVICE FOR MEDICAL DIAGNOSIS

(71) Applicant: Onera Technologies B.V., Eindhoven (NL)

(72) Inventor: Peter Cramer, Eindhoven (NL)

(73) Assignee: Onera Technologies B.V., Eindhoven (NL)

(**) Term: 15 Years

(21) Appl. No.: 29/902,984

(22) Filed: Sep. 19, 2023

Related U.S. Application Data

(62) Division of application No. 35/514,062, filed on Jul. 29, 2021 (U.S. filing date under 35 U.S.C. 384), and having an international filing date of Jul. 29, 2021, now Pat. No. Des. 1,004,107.

Foreign Application Priority Data

Jan. 29, 2021	(EM)	008417059-0001
Jan. 29, 2021	(EM)	008417059-0002
Jan. 29, 2021	(EM)	008417059-0003
Jan. 29, 2021	(EM)	008417059-0004
Jan. 29, 2021	(EM)	008417059-0005
Jan. 29, 2021	(EM)	008417059-0006
Jan. 29, 2021	(EM)	008417059-0007
Jan. 29, 2021	(EM)	008417059-0008
Jan. 29, 2021	(EM)	008417059-0009
Jan. 29, 2021	(EM)	008417059-0010
Jan. 29, 2021	(EM)	008417059-0011
Jan. 29, 2021	(EM)	008417059-0012

(51) LOC (15) Cl. 24-02

(52) U.S. Cl. USPC D24/187

(58) Field of Classification Search USPC D24/107, 168, 186, 187, 189, 200

CPC A61B 5/042; A61B 5/0404; A61B 5/0416; A61N 1/046; A61N 1/0472
See application file for complete search history.

References Cited

U.S. PATENT DOCUMENTS

6,453,186 B1 * 9/2002 Lovejoy A61B 5/282 600/386

D606,660 S 12/2009 Phillips et al.
D607,570 S 1/2010 Phillips et al.

(Continued)

FOREIGN PATENT DOCUMENTS

CN 202130570543.8 * 4/2022
CN 307700668 S 11/2022

OTHER PUBLICATIONS

DR400 1-Lead Electrode Patch. Online, published date unknown. Retrieved on Mar. 7, 2023 from URL: [https:// www.medicaldevicedepot. com/DR400-1-Lead-Electrode-Patch-Qty-of-200-p/nemel002.htm](https://www.medicaldevicedepot.com/DR400-1-Lead-Electrode-Patch-Qty-of-200-p/nemel002.htm).

(Continued)

Primary Examiner — Omeed Agilee
(74) Attorney, Agent, or Firm — Moore & Van Allen PLLC; Jeffrey R. Gray


CLAIM

The ornamental design for a smart patch device for medical diagnosis, as shown and described.

DESCRIPTION

FIG. 1 is a top view of a first embodiment of a smart patch device for medical diagnosis; and, FIG. 2 is a top view of a second embodiment of a smart patch device for medical diagnosis. The broken lines in the drawings depict portions of the smart patch device for medical diagnosis that form no part of the claimed design.

1 Claim, 2 Drawing Sheets

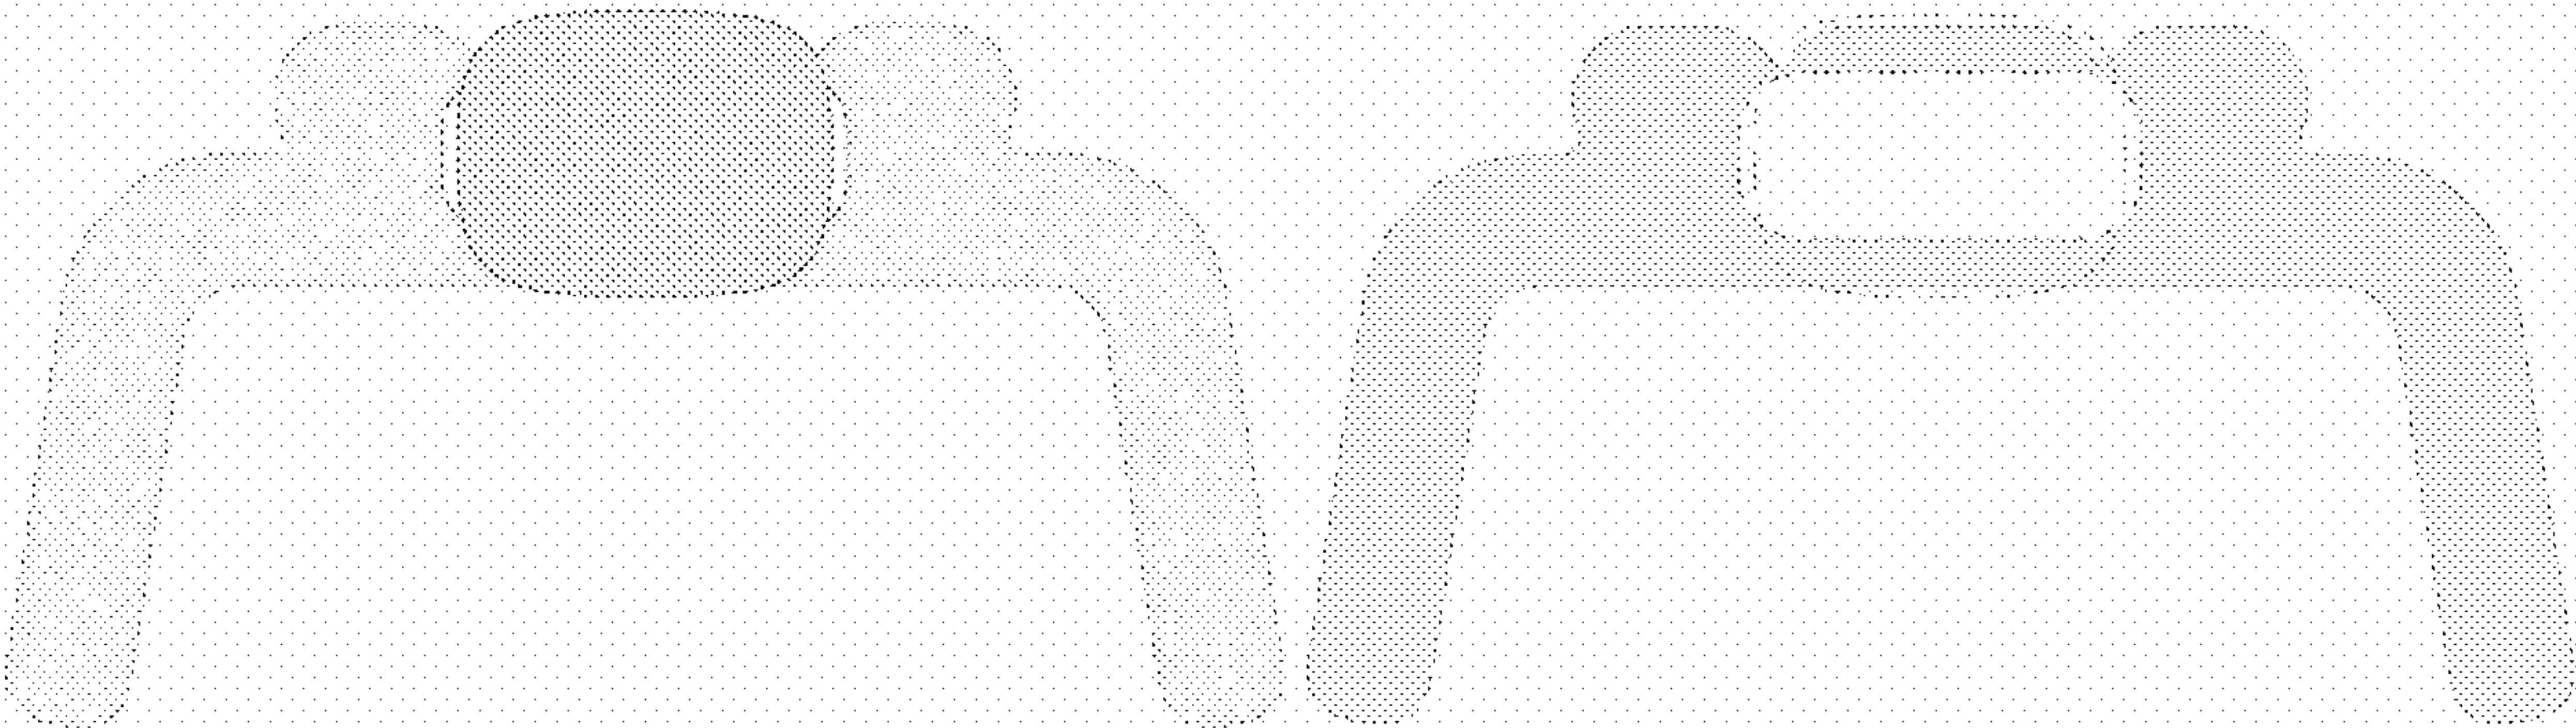

(56) **References Cited**

U.S. PATENT DOCUMENTS

D618,810	S	6/2010	Tanigawa et al.	
D663,431	S	7/2012	Parker, III et al.	
D663,849	S	7/2012	McGusty et al.	
D698,928	S	2/2014	Tsuruta et al.	
D744,659	S *	12/2015	Bishay	D24/187
D752,764	S	3/2016	Peters	
D764,672	S	8/2016	Vosch et al.	
D805,208	S	12/2017	Komatani et al.	
D871,590	S	12/2019	Chang et al.	
D1,004,107	S *	11/2023	Cramer	D24/187
D1,055,290	S *	12/2024	Wasserman	D24/187
D1,063,079	S *	2/2025	Abercrombie	H05K 5/0026
				D24/187
2012/0029307	A1 *	2/2012	Paquet	A61B 5/0816
				600/301
2020/0337608	A1 *	10/2020	Garai	A61B 5/14532
2023/0083795	A1 *	3/2023	O’Grady	A61B 5/4255
				600/391

OTHER PUBLICATIONS

Onera Health. Online, published date Jul. 26, 2021. Retrieved on Mar. 7, 2023 from URL: <https://www.invest-nl.nl/portefeuille/story-onera-health>.

* cited by examiner

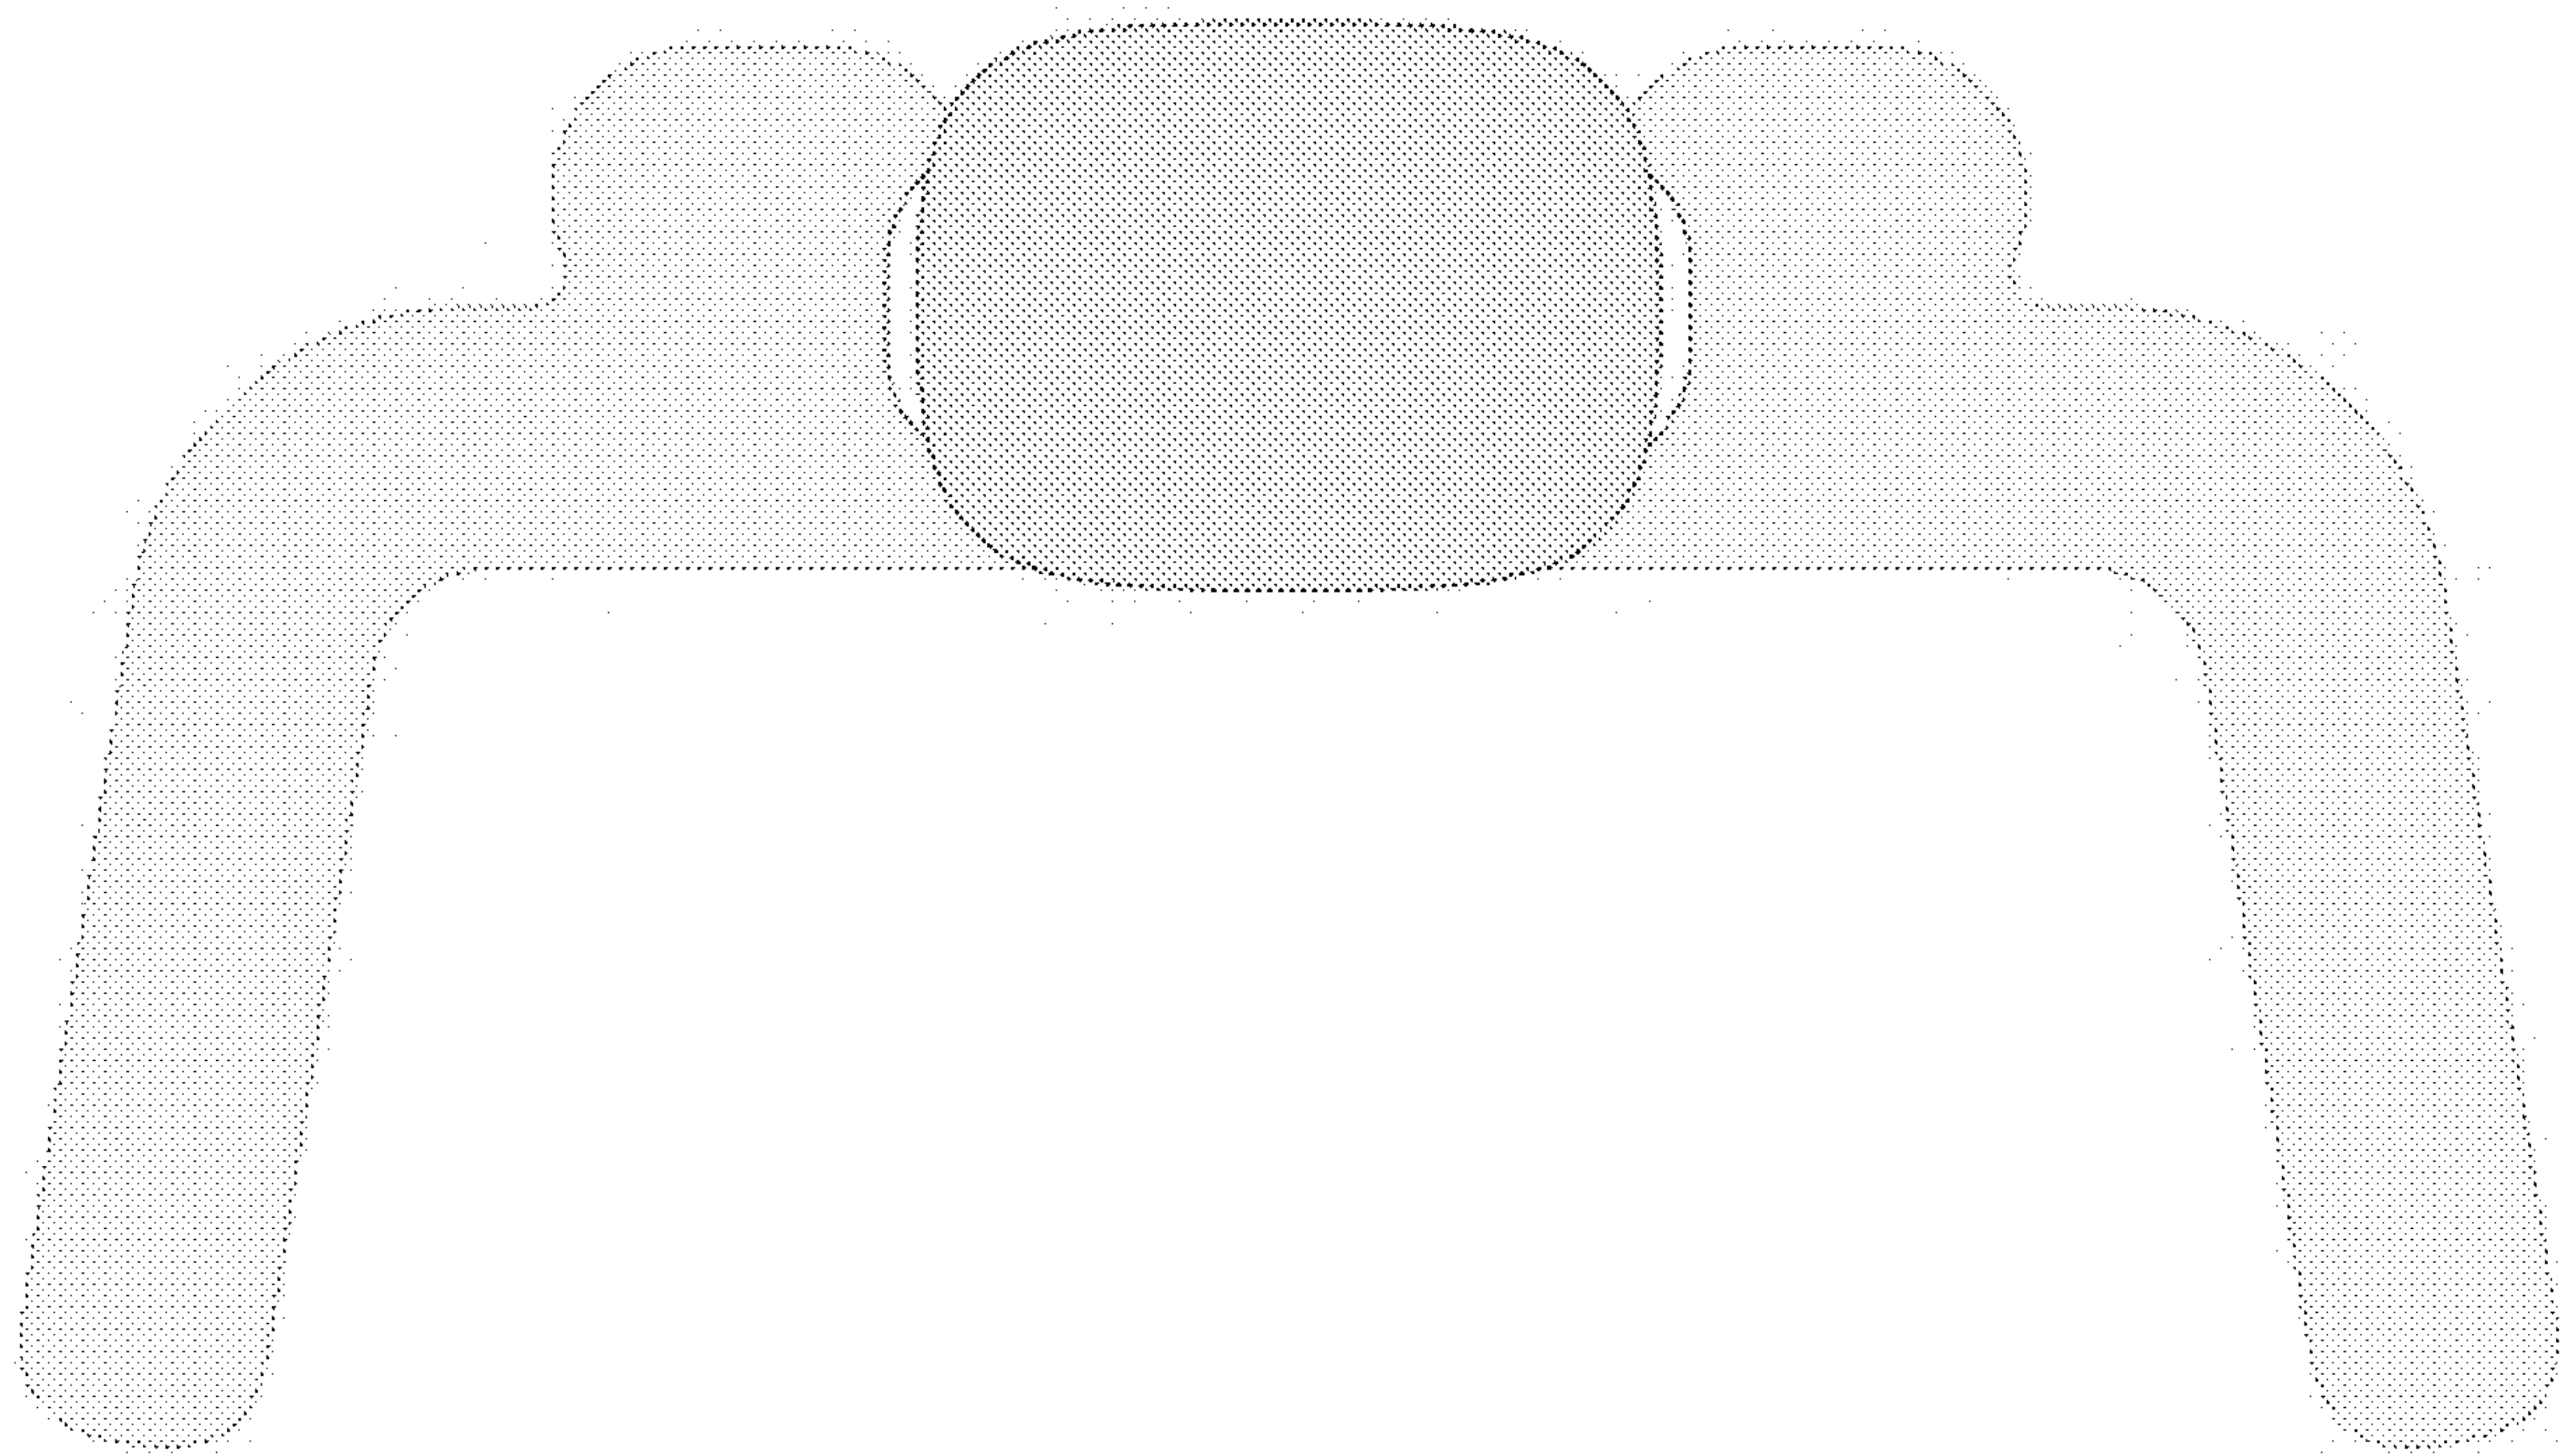


FIG. 1

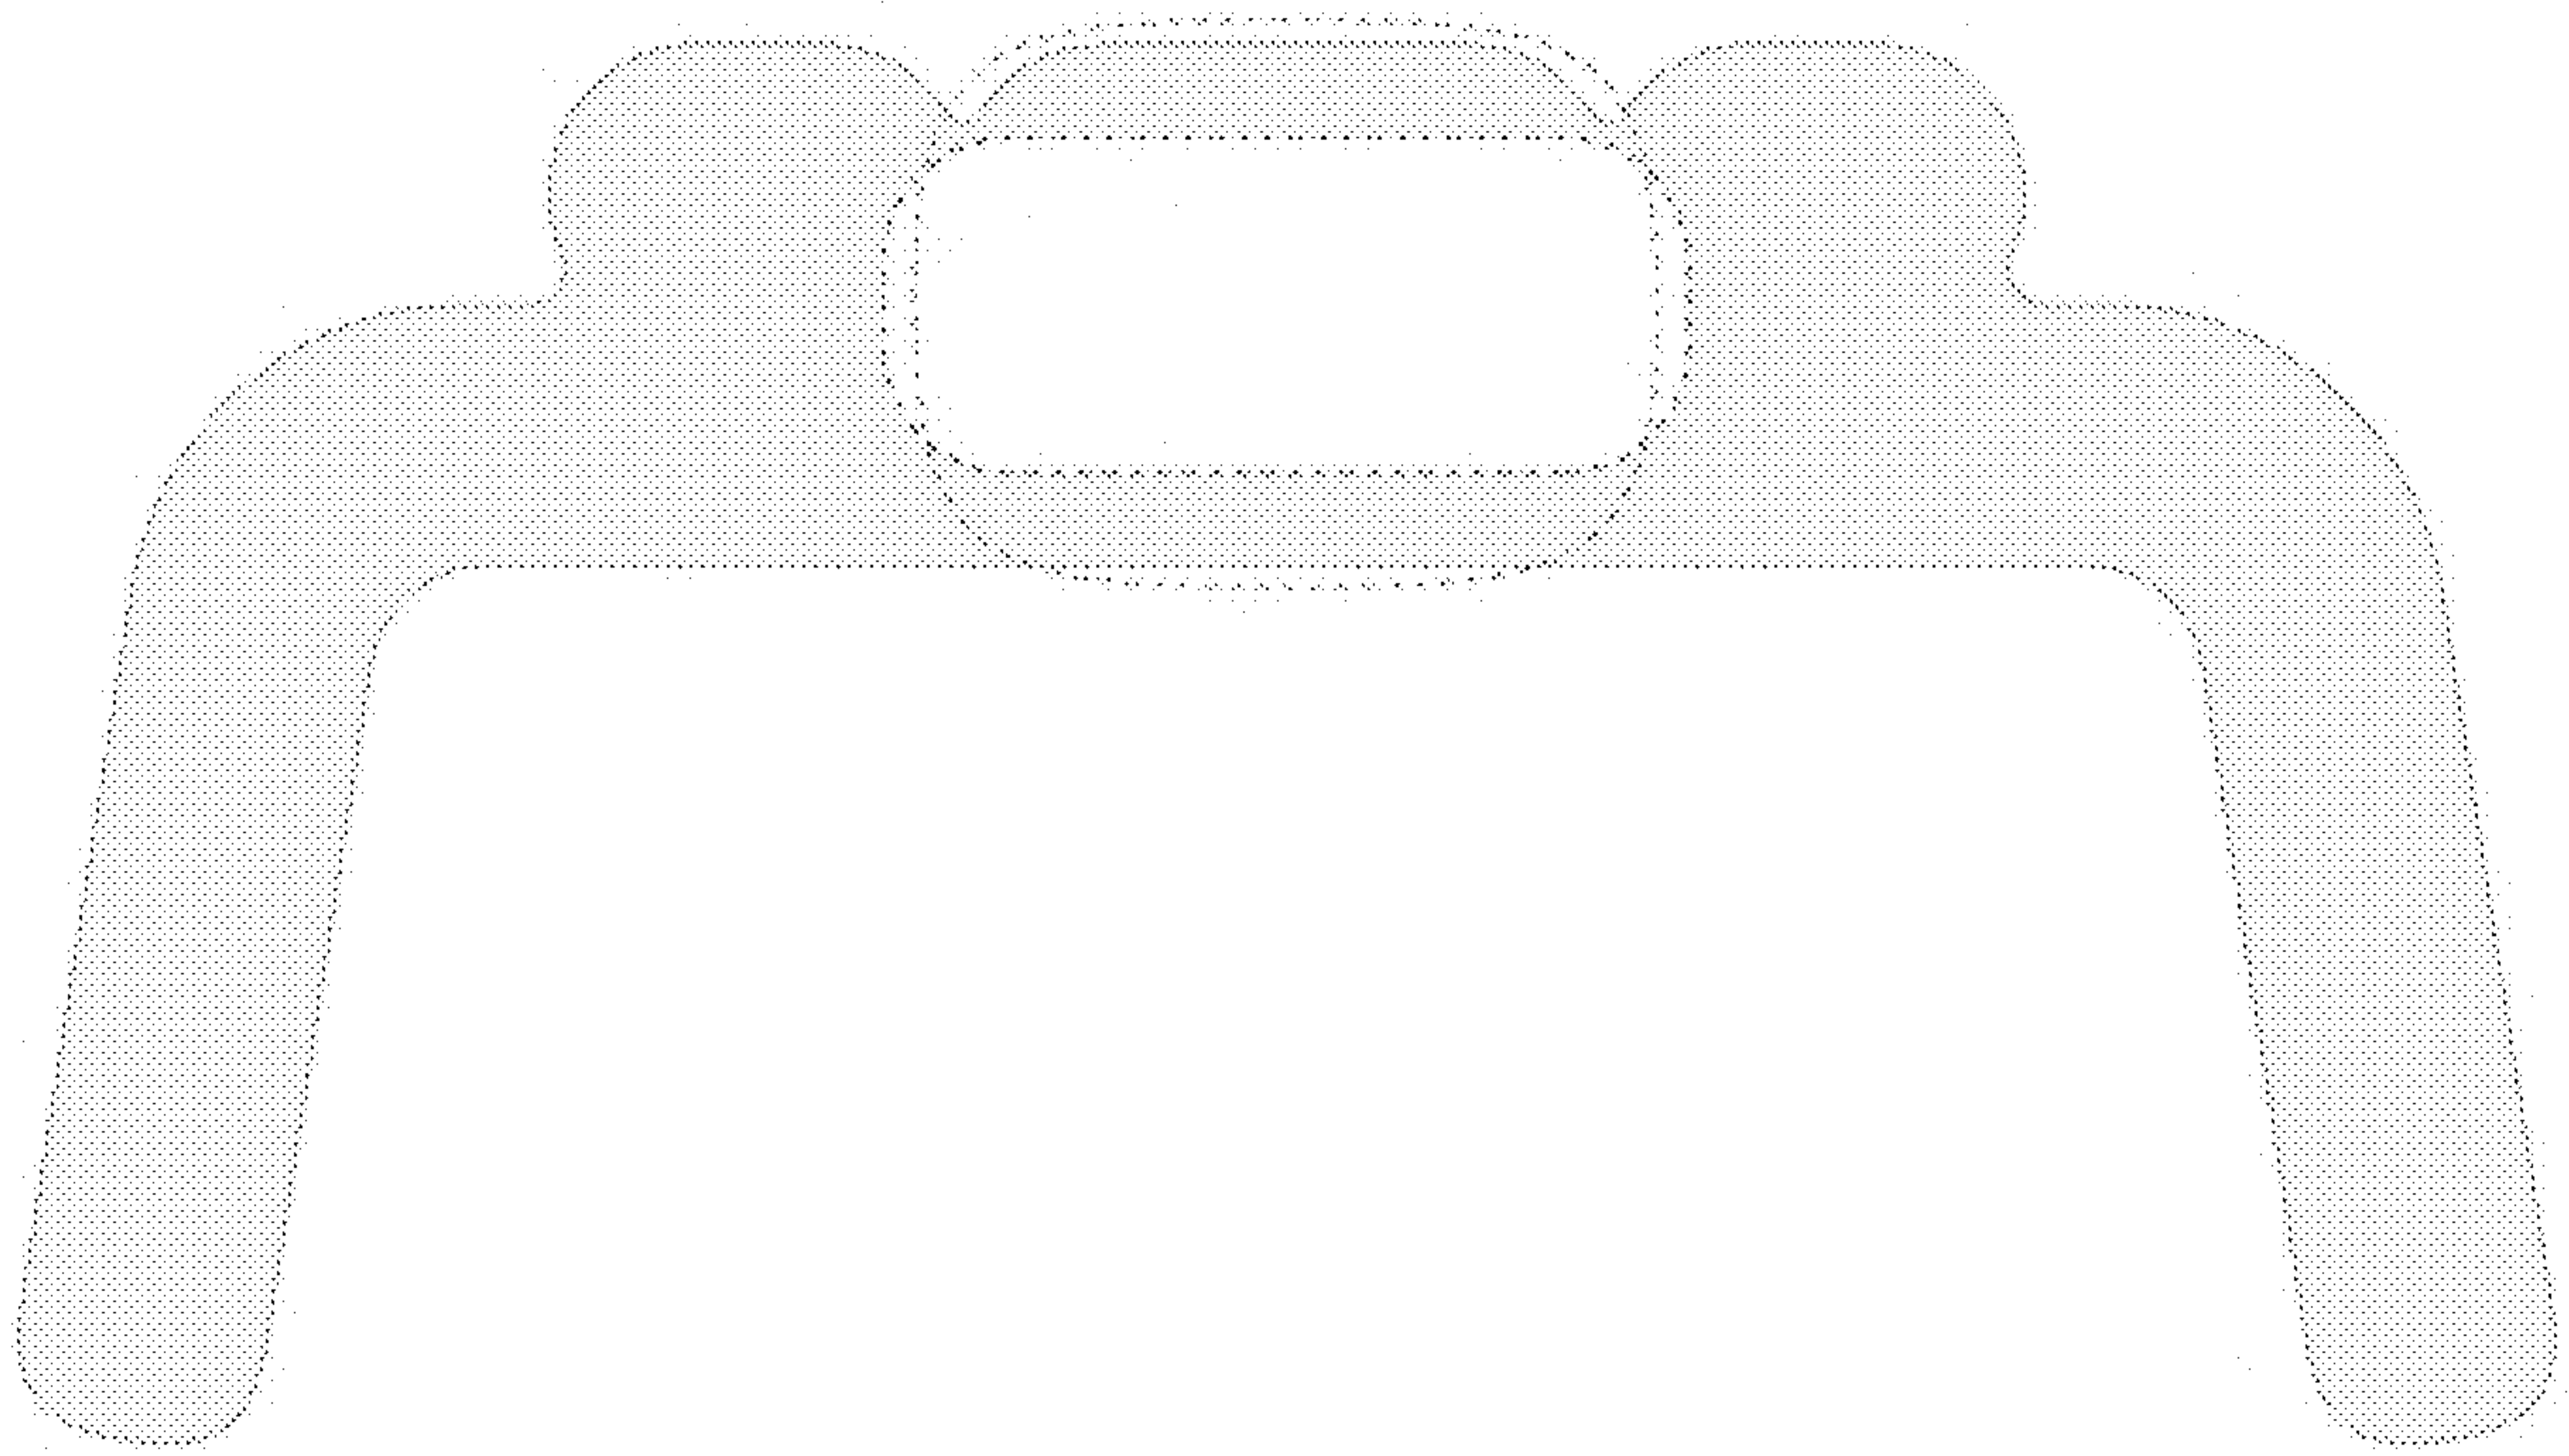


FIG. 2