

[54] **PHYSIOLOGICAL MONITORING DEVICE HOUSING**

[75] Inventors: **K. William Edmark**, Seattle; **David B. Smith**, Mercer Island; **Louis D. Pheil**, Redmond, all of Wash.

[73] Assignee: **Physio Control Corporation**, Redmond, Wash.

[**] Term: **14 Years**

[21] Appl. No.: **605,440**

[22] Filed: **Aug. 18, 1975**

[51] Int. Cl. **D24-02; D10-99**

[52] U.S. Cl. **D83/1 F**

[58] Field of Search 128/2 K, 2 V, 2.05 Z, 128/DIG. 4; D83/1 F; D10/103; 340/1 R

[56] **References Cited**

U.S. PATENT DOCUMENTS

3,728,670	4/1973	Rosauer	340/1 R
3,776,228	12/1973	Semler	128/2.06 E
3,896,788	7/1975	Sato	128/2.05 Z

D. 207,685	5/1967	King	D83/1 F
D. 214,755	7/1969	McPhee	D10/103


Primary Examiner—Bernard Ansher
Attorney, Agent, or Firm—Orland M. Christensen

[57] **CLAIM**

The ornamental design for physiological monitoring device housing, as shown and described.

DESCRIPTION

FIG. 1 is a perspective front view of a physiological monitoring device housing showing our design; FIG. 2 is a side view of the physiological monitoring device housing of FIG. 1; FIG. 3 is a top plan view of the physiological monitoring device housing of FIG. 1; FIG. 4 is a rear end view of the physiological monitoring device housing of FIG. 1; FIG. 5 is a front end view of the physiological monitoring device housing of FIG. 1. The stethoscope shown in broken lines is for illustrative purposes only.

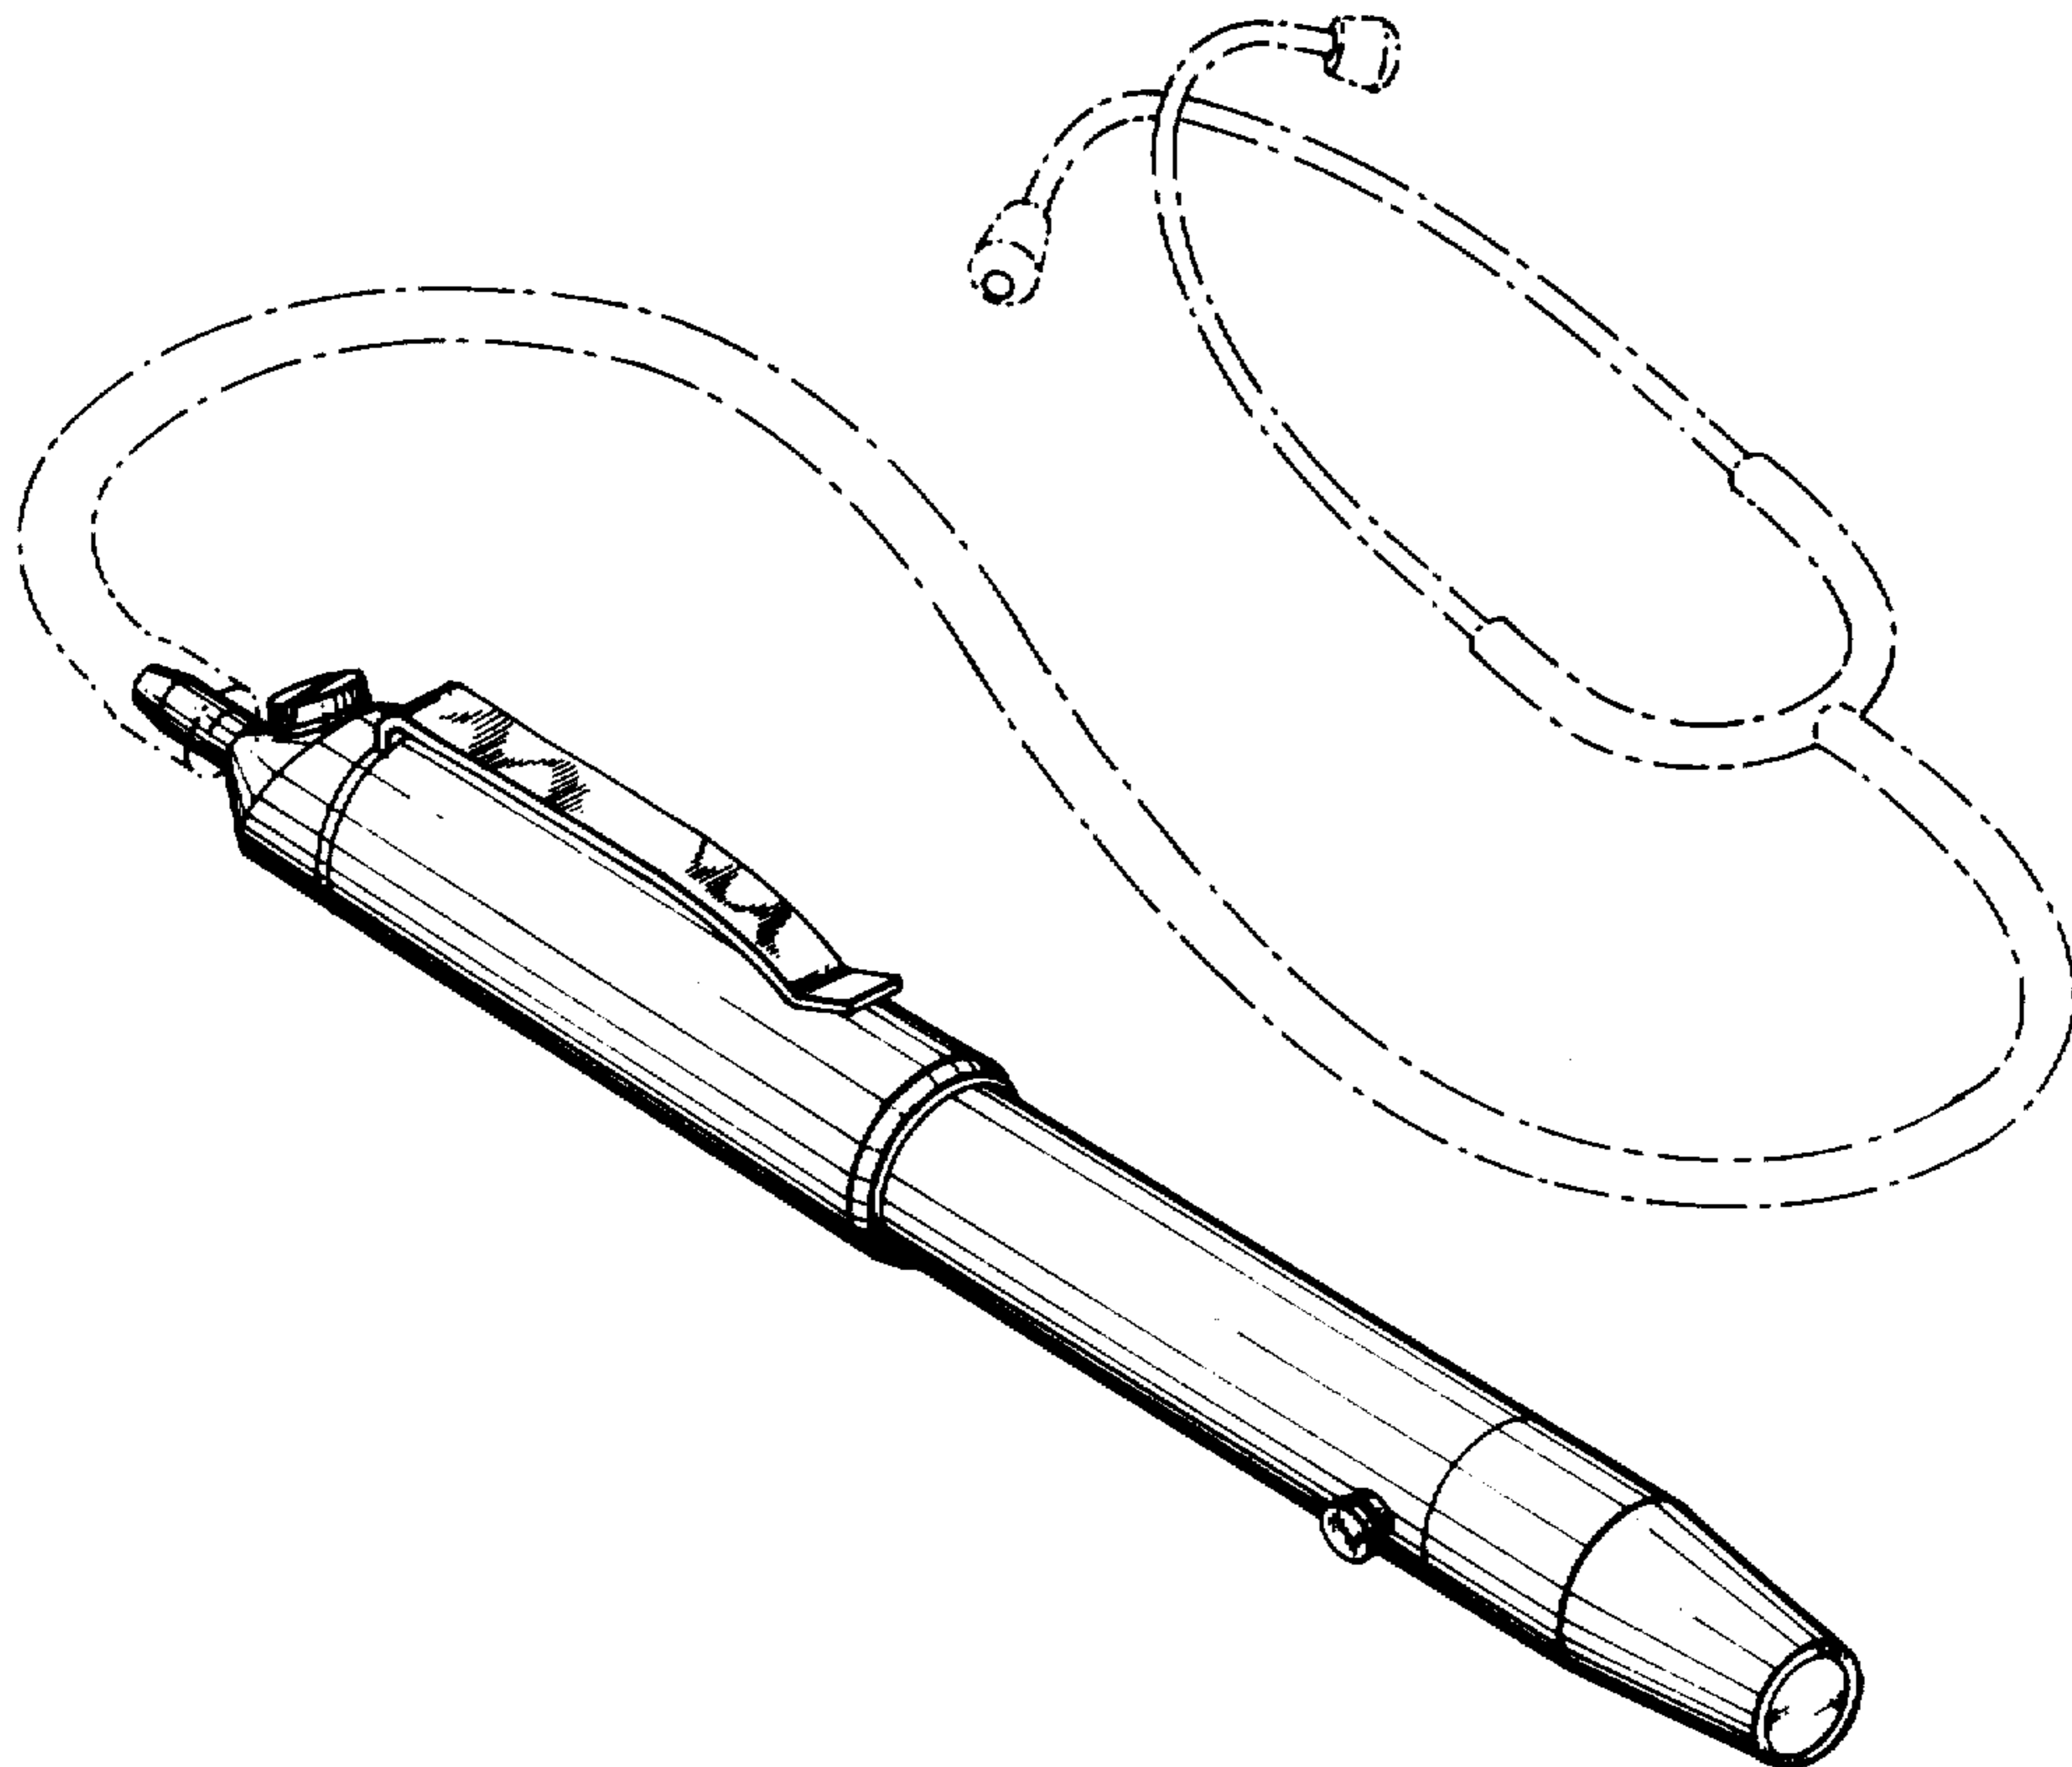

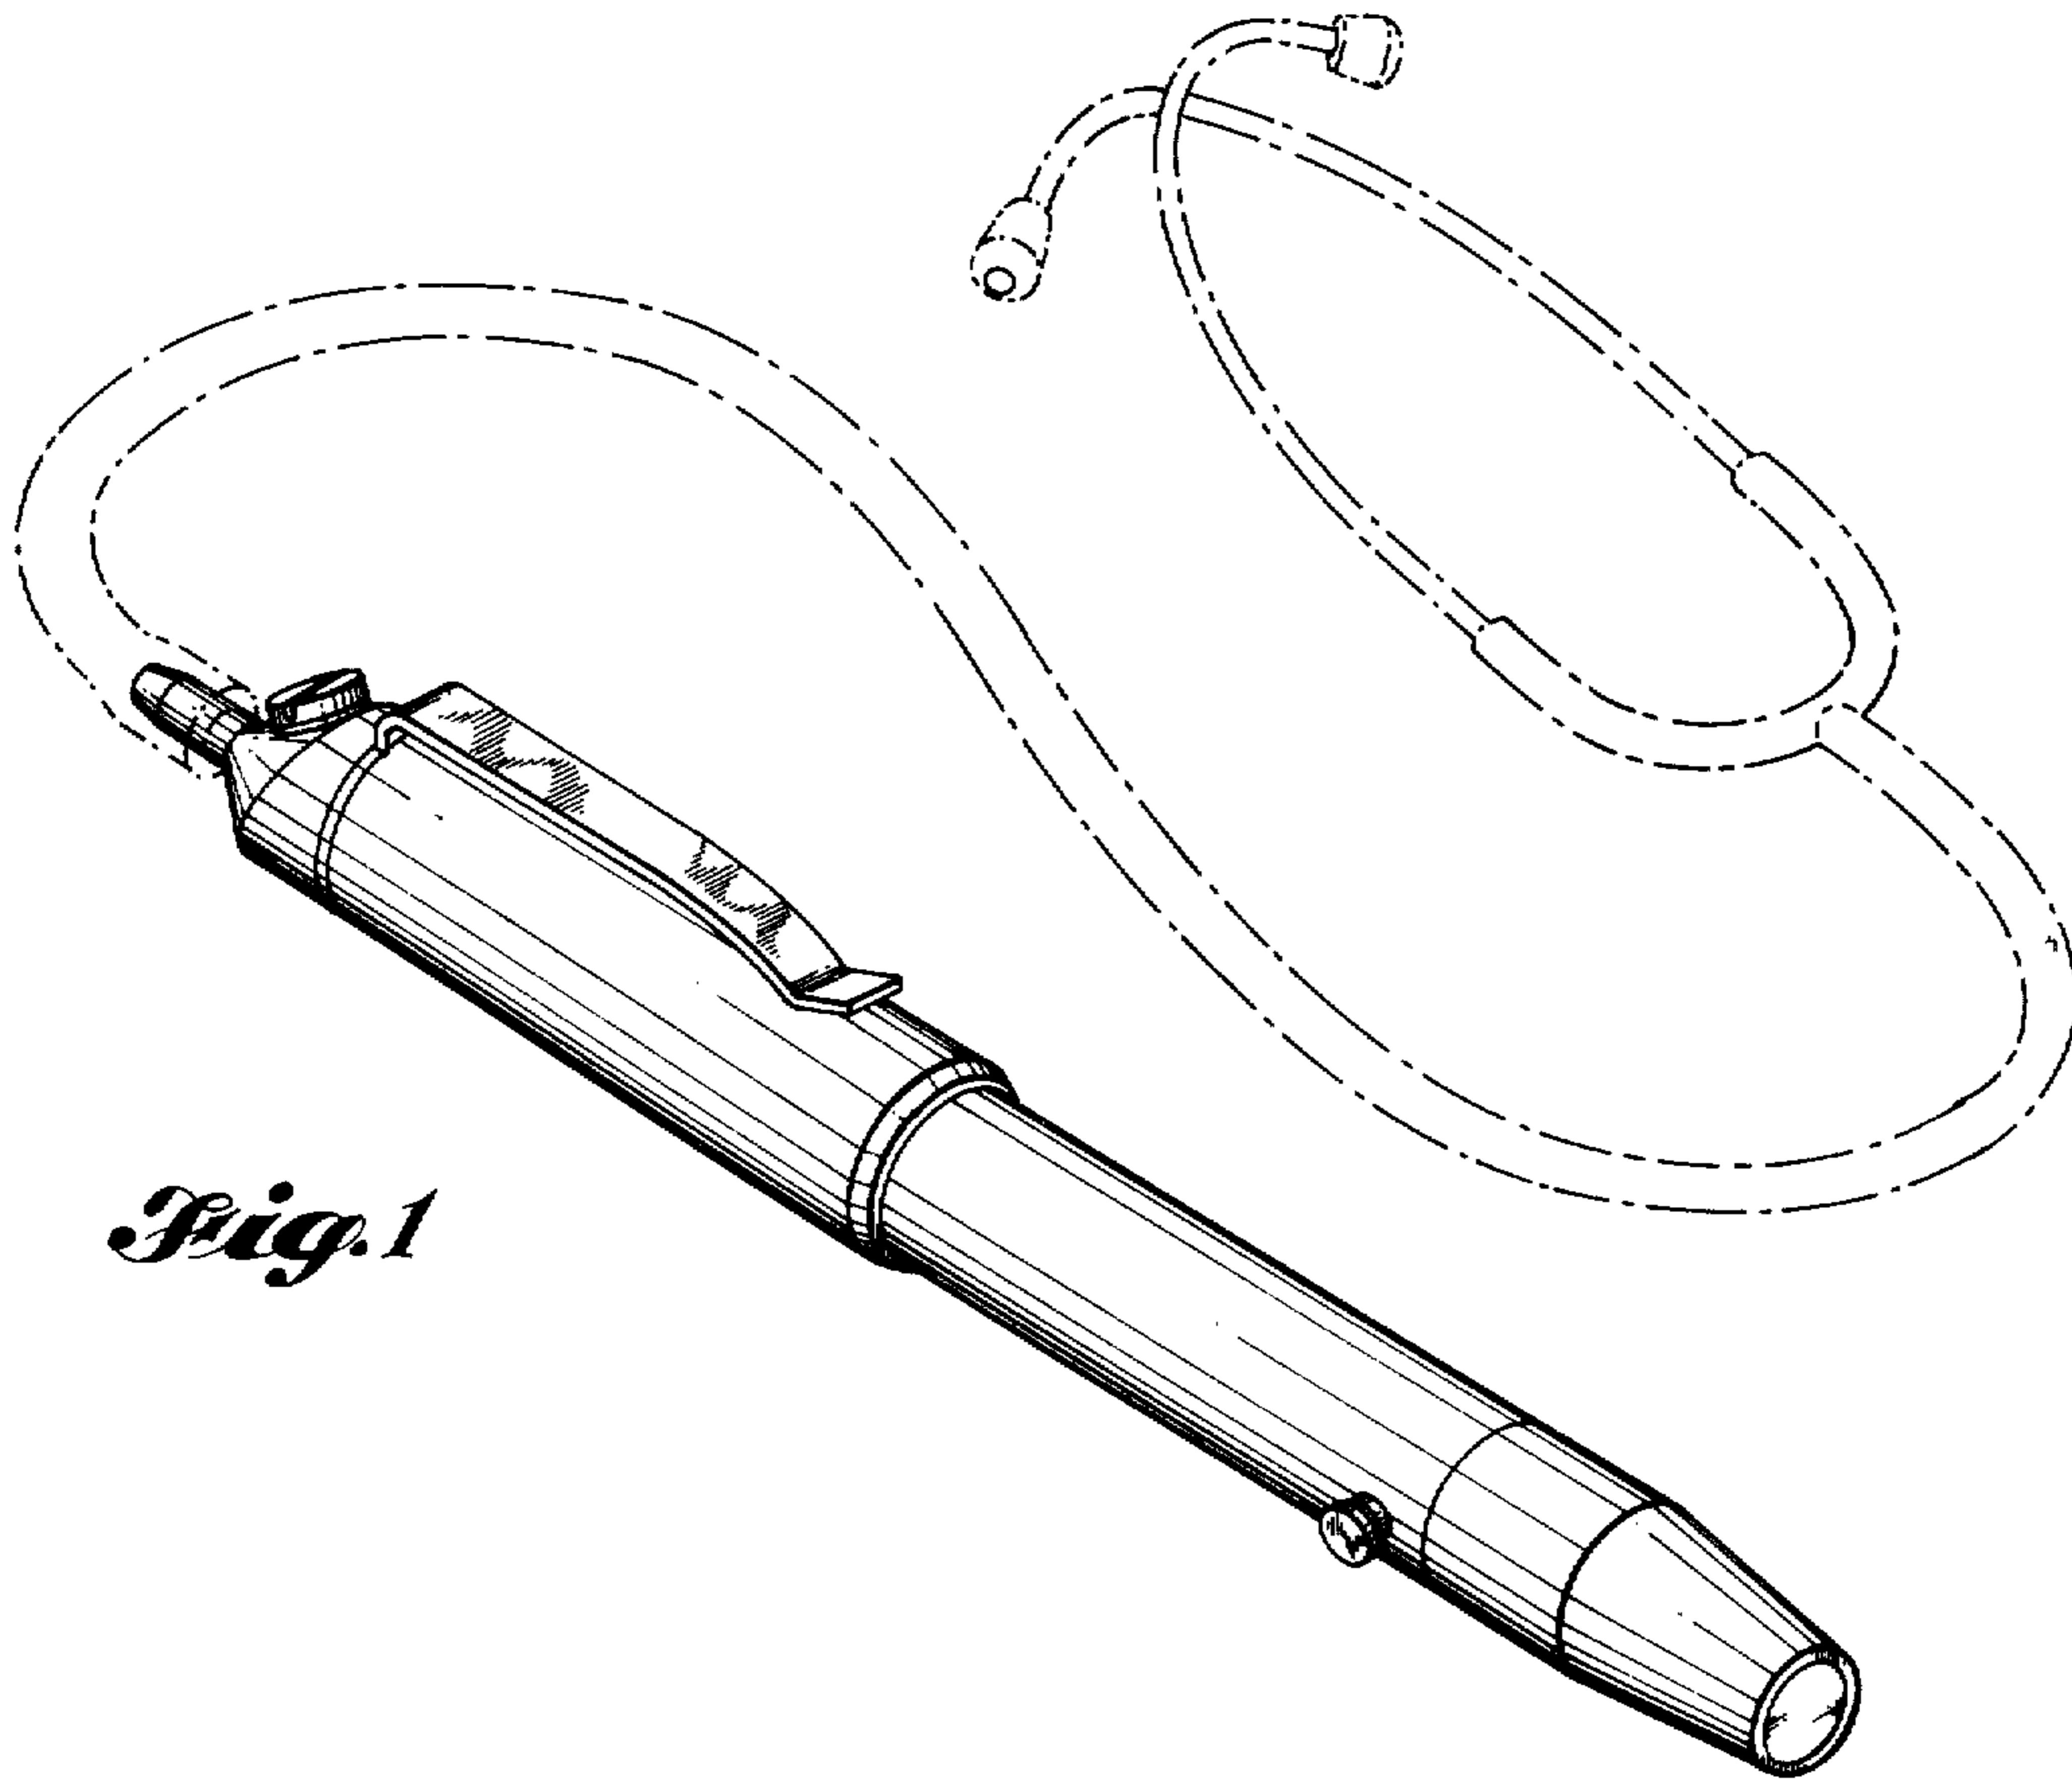


Fig. 1

Fig. 2

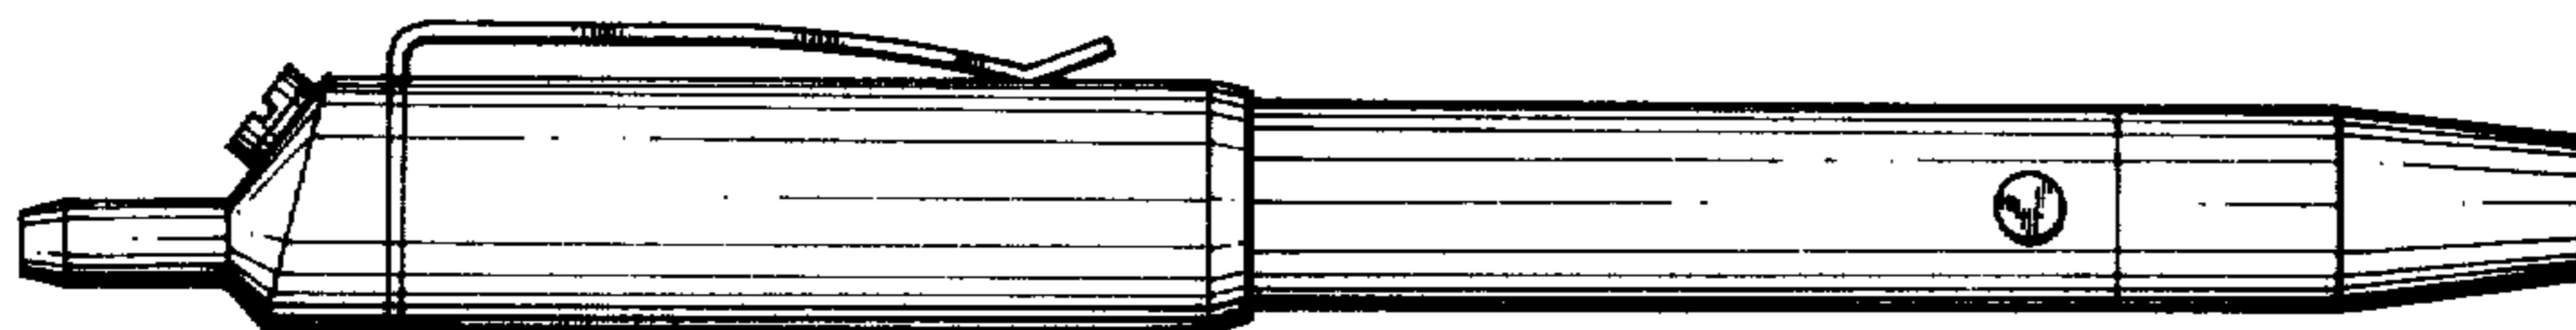


Fig. 3

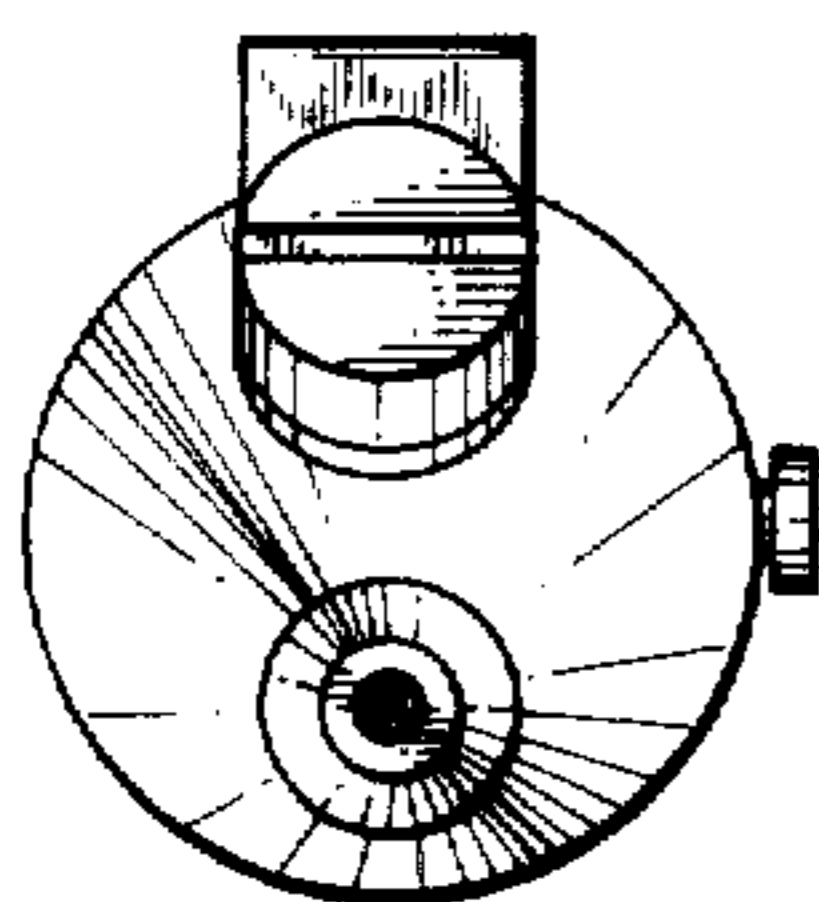
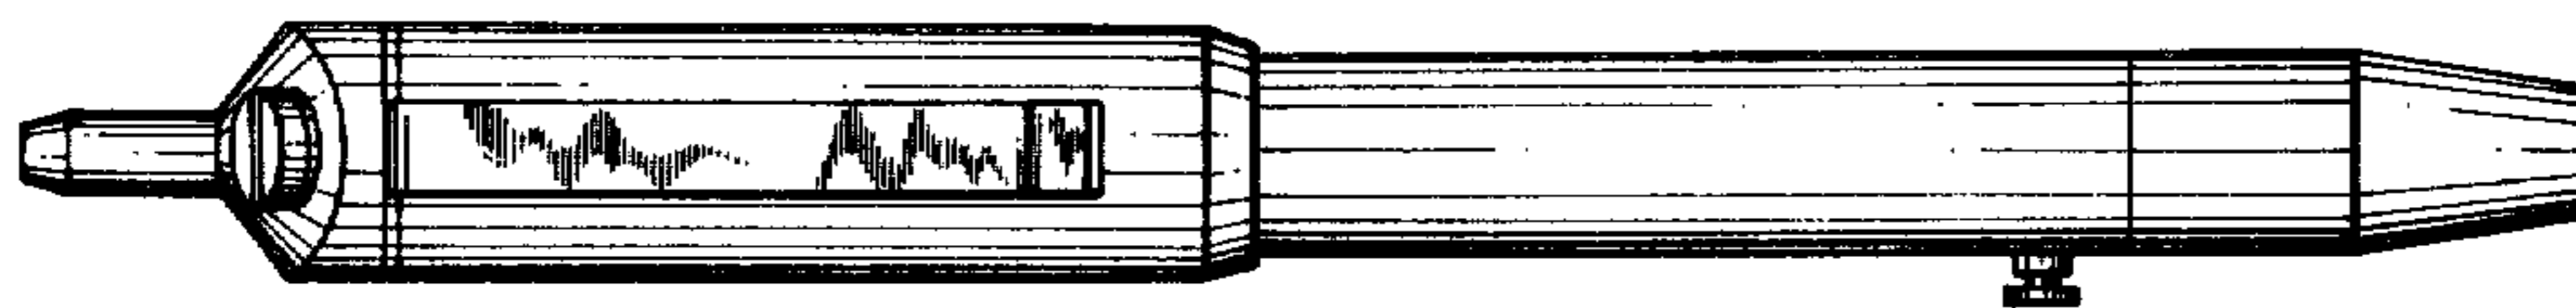


Fig. 4

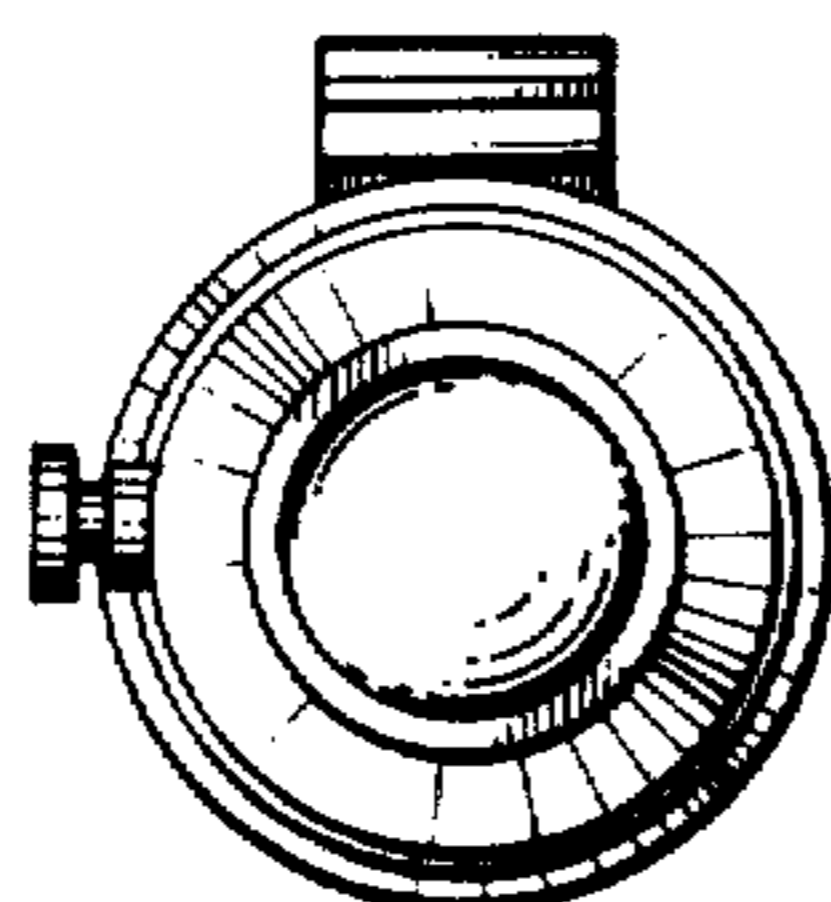


Fig. 5