

[54] **MICROBIOLOGICAL TEST STRIP**

[75] **Inventor:** Michael William Dixon, Norley,
England

[73] **Assignee:** Scientific Hospital Supplies Limited,
Liverpool, England

[**] **Term:** 14 Years

[21] **Appl. No.:** 733,830

[22] **Filed:** Oct. 18, 1976

[51] **Int. Cl.** D24—02; D24—99
[52] **U.S. Cl.** D24/8
[58] **Field of Search** D24/99, 8; 195/139,
195/103.5 R; 23/253 TP

[56]

References Cited

U.S. PATENT DOCUMENTS

D. 207,487	4/1967	Briggs et al.	D24/99
D. 239,042	3/1976	Freake et al.	D24/8
3,511,608	5/1970	Anderson	23/253 TP
3,785,930	1/1974	Ellis	195/139
3,843,452	10/1974	Freake et al.	195/139
3,979,264	9/1976	Buerger	195/103.5 R

Primary Examiner—Bernard Ansher
Attorney, Agent, or Firm—Fred C. Philpitt

[57]

CLAIM

The ornamental design for a microbiological test strip,
substantially as shown and described.

DESCRIPTION

FIG. 1 is a side elevation of a microbiological test strip
showing my design;
FIG. 2 is a top plan view of the test strip of FIG. 1;
FIG. 3 is an end elevation; and
FIG. 4 is a bottom plan view.

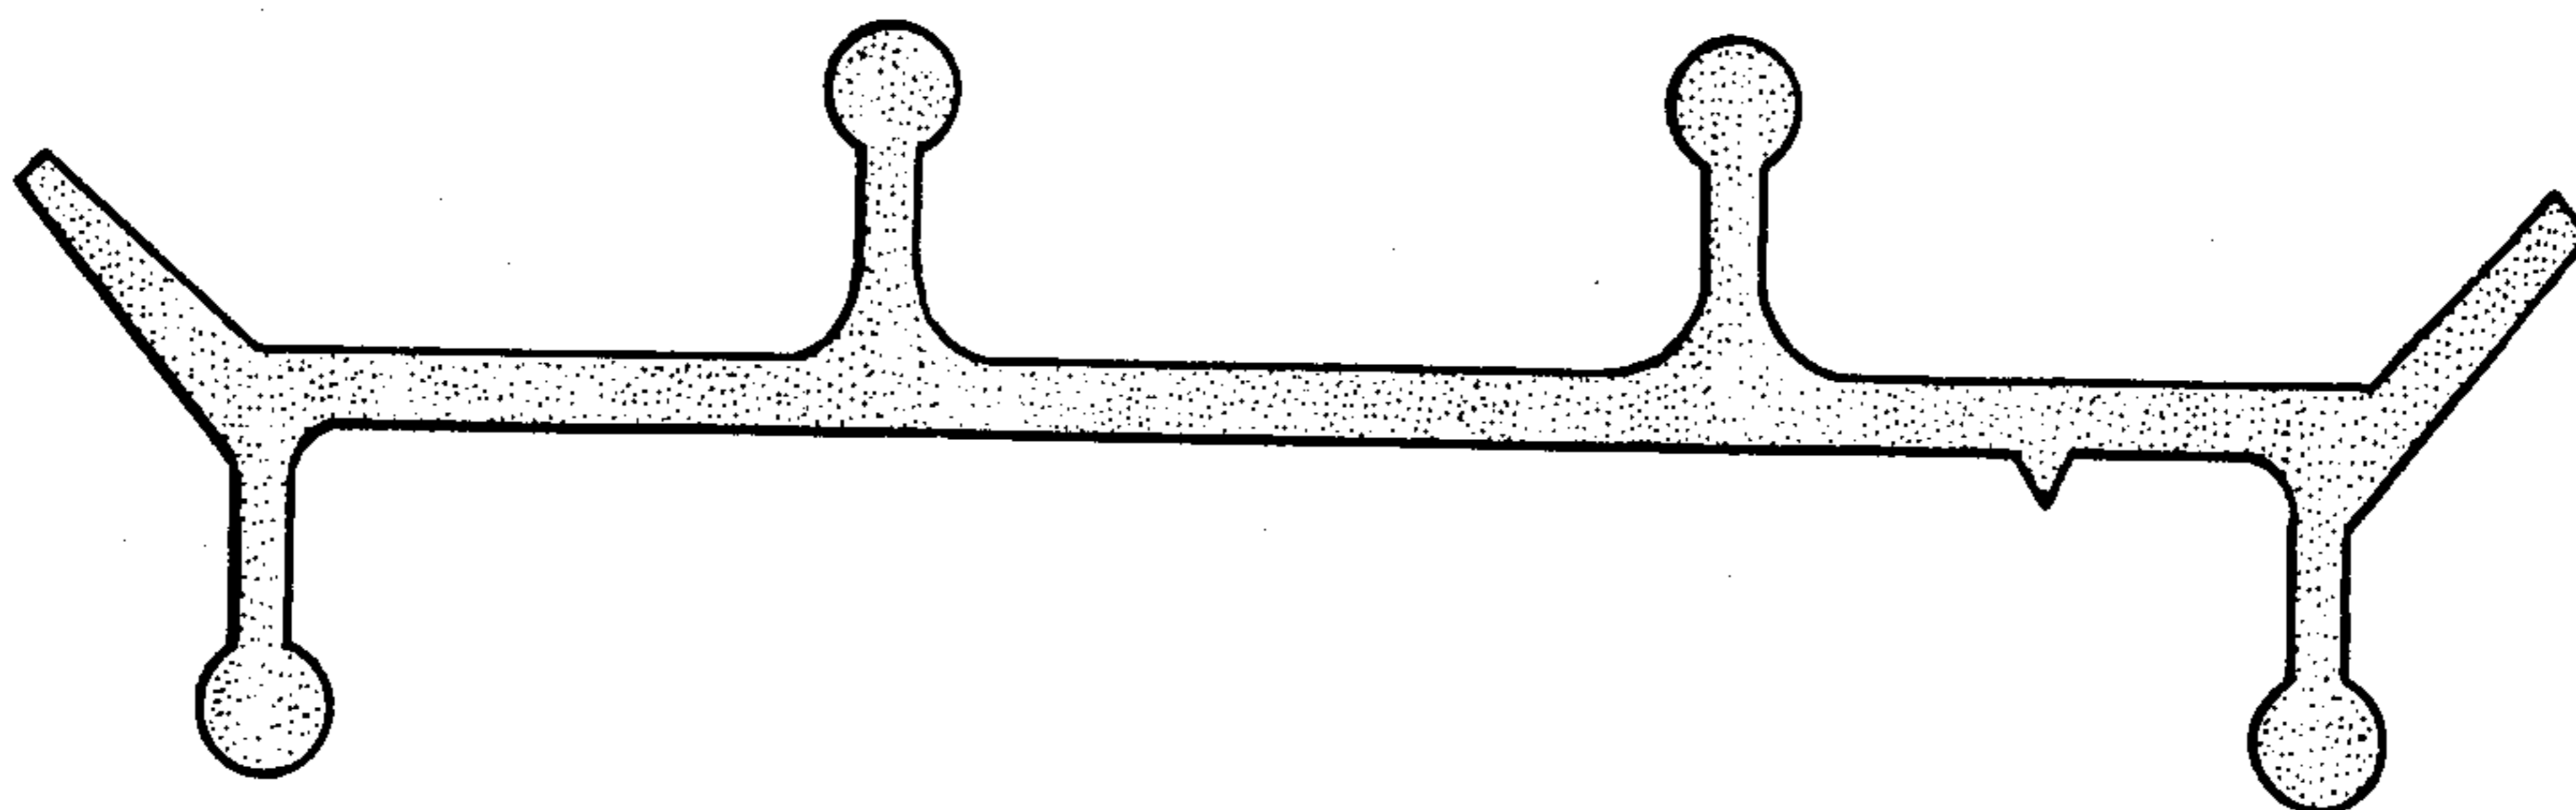


FIG 1



FIG 2

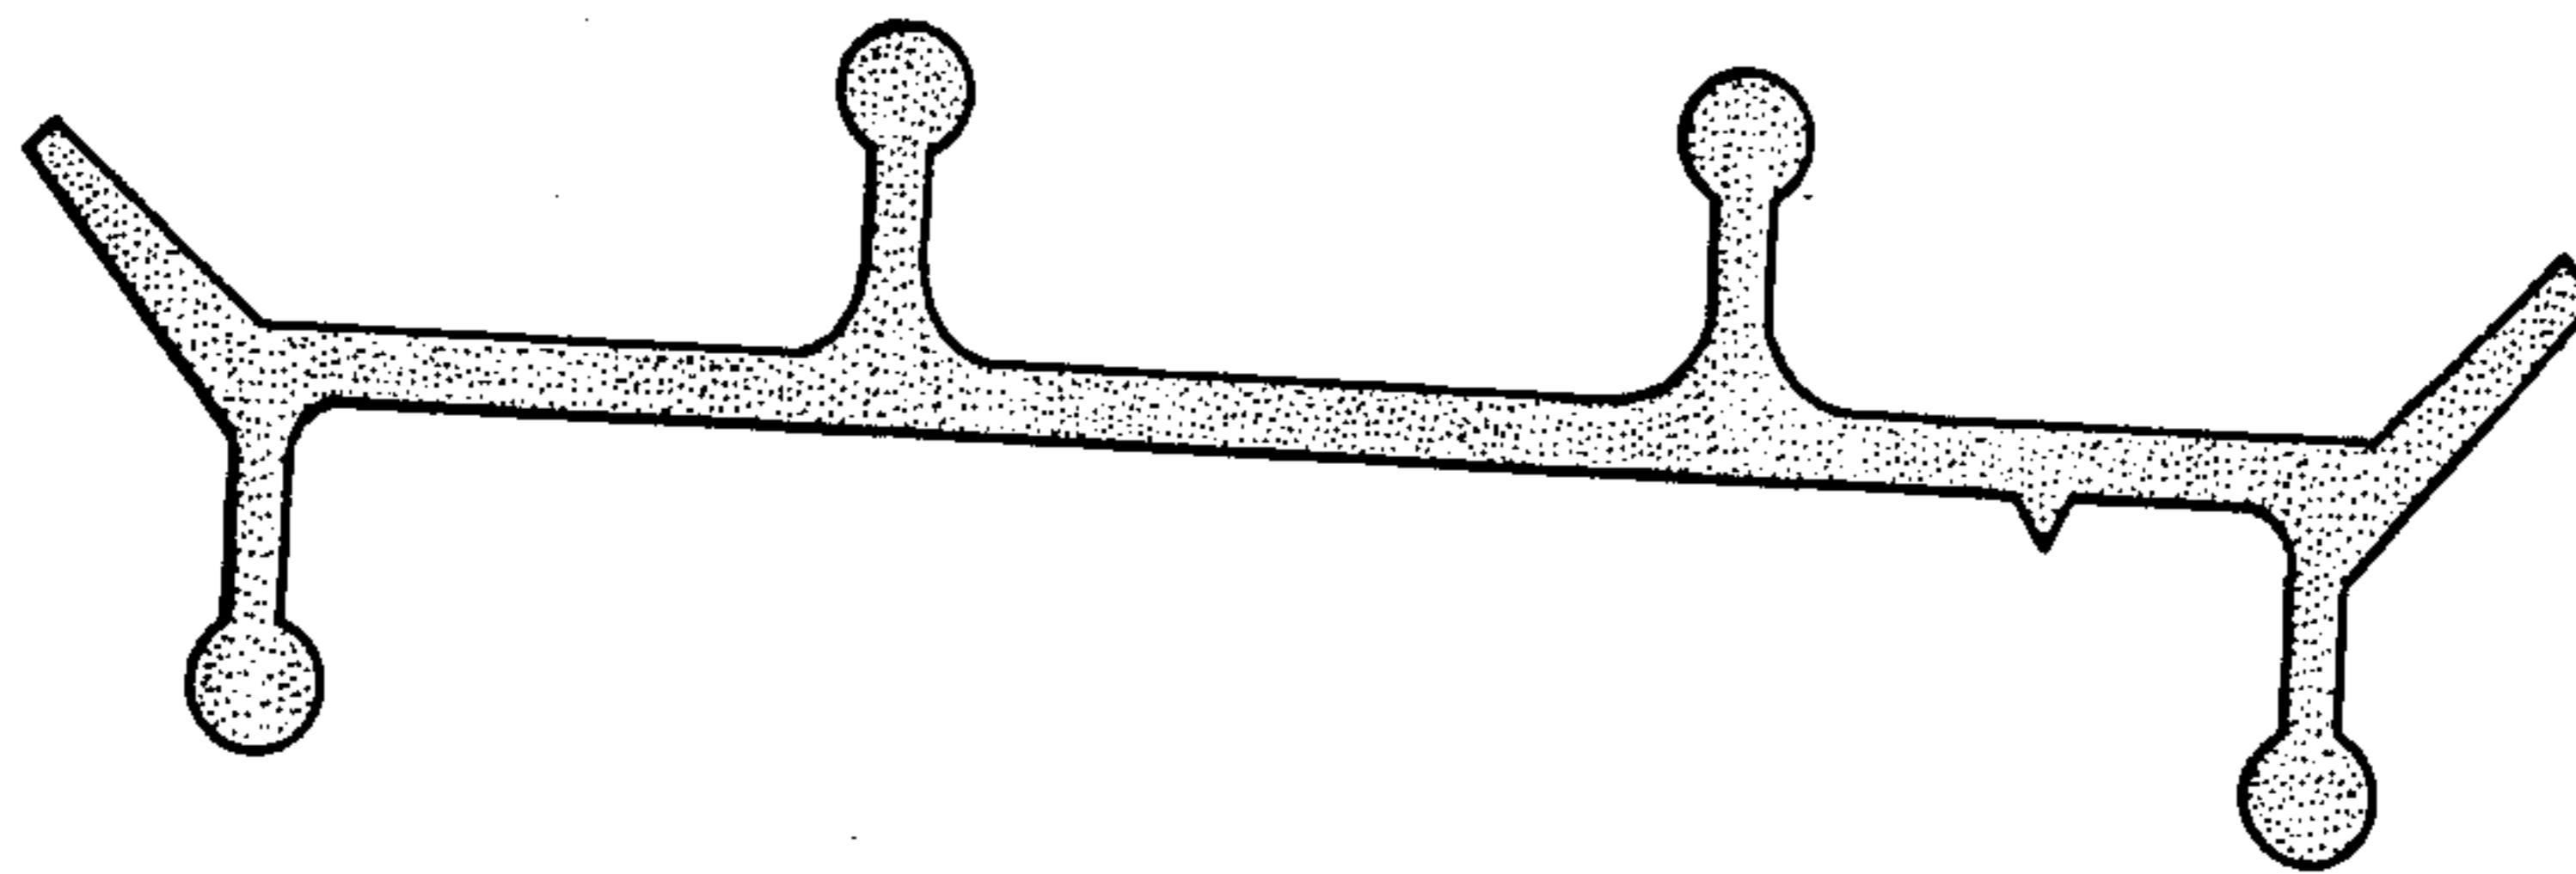


FIG 3

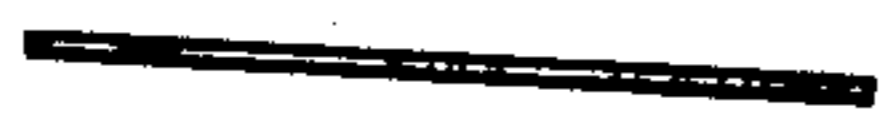


FIG 4

