

[54] **SAMPLE CUP TRAY FOR CHEMICAL ANALYSIS OF BIOLOGICAL FLUIDS**

[75] Inventor: **Henry Stanislaus Adamski**, Rochester, N.Y.

[73] Assignee: **Eastman Kodak Company**, Rochester, N.Y.

[**] Term: **14 Years**

[21] Appl. No.: **751,929**

[22] Filed: **Dec. 17, 1976**

[51] Int. Cl. **D24—01; D24—02**

[52] U.S. Cl. **D24/32; D9/189**

[58] Field of Search **D9/189; D24/1.1, 55, D24/21, 56, 7, 99, 32; 195/103.5 R; 23/292, 259**

[56] **References Cited**

U.S. PATENT DOCUMENTS

D. 210,720	4/1968	Anthon	D24/32
D. 245,352	8/1977	Moran	D24/1.1
3,540,856	11/1970	Rochte	23/292
3,713,985	1/1973	Astle	195/103.5 R
3,932,141	1/1976	Beall et al.	23/259

Primary Examiner—Bernard Ansher

Attorney, Agent, or Firm—Robert W. Hampton


[57] **CLAIM**

The ornamental design for a sample cup tray for chemical analysis of biological fluids, as shown and described.

DESCRIPTION

FIG. 1 is a top perspective view of a sample cup tray for chemical analysis of biological fluids showing my new design; and

FIG. 2 is a bottom perspective view thereof.

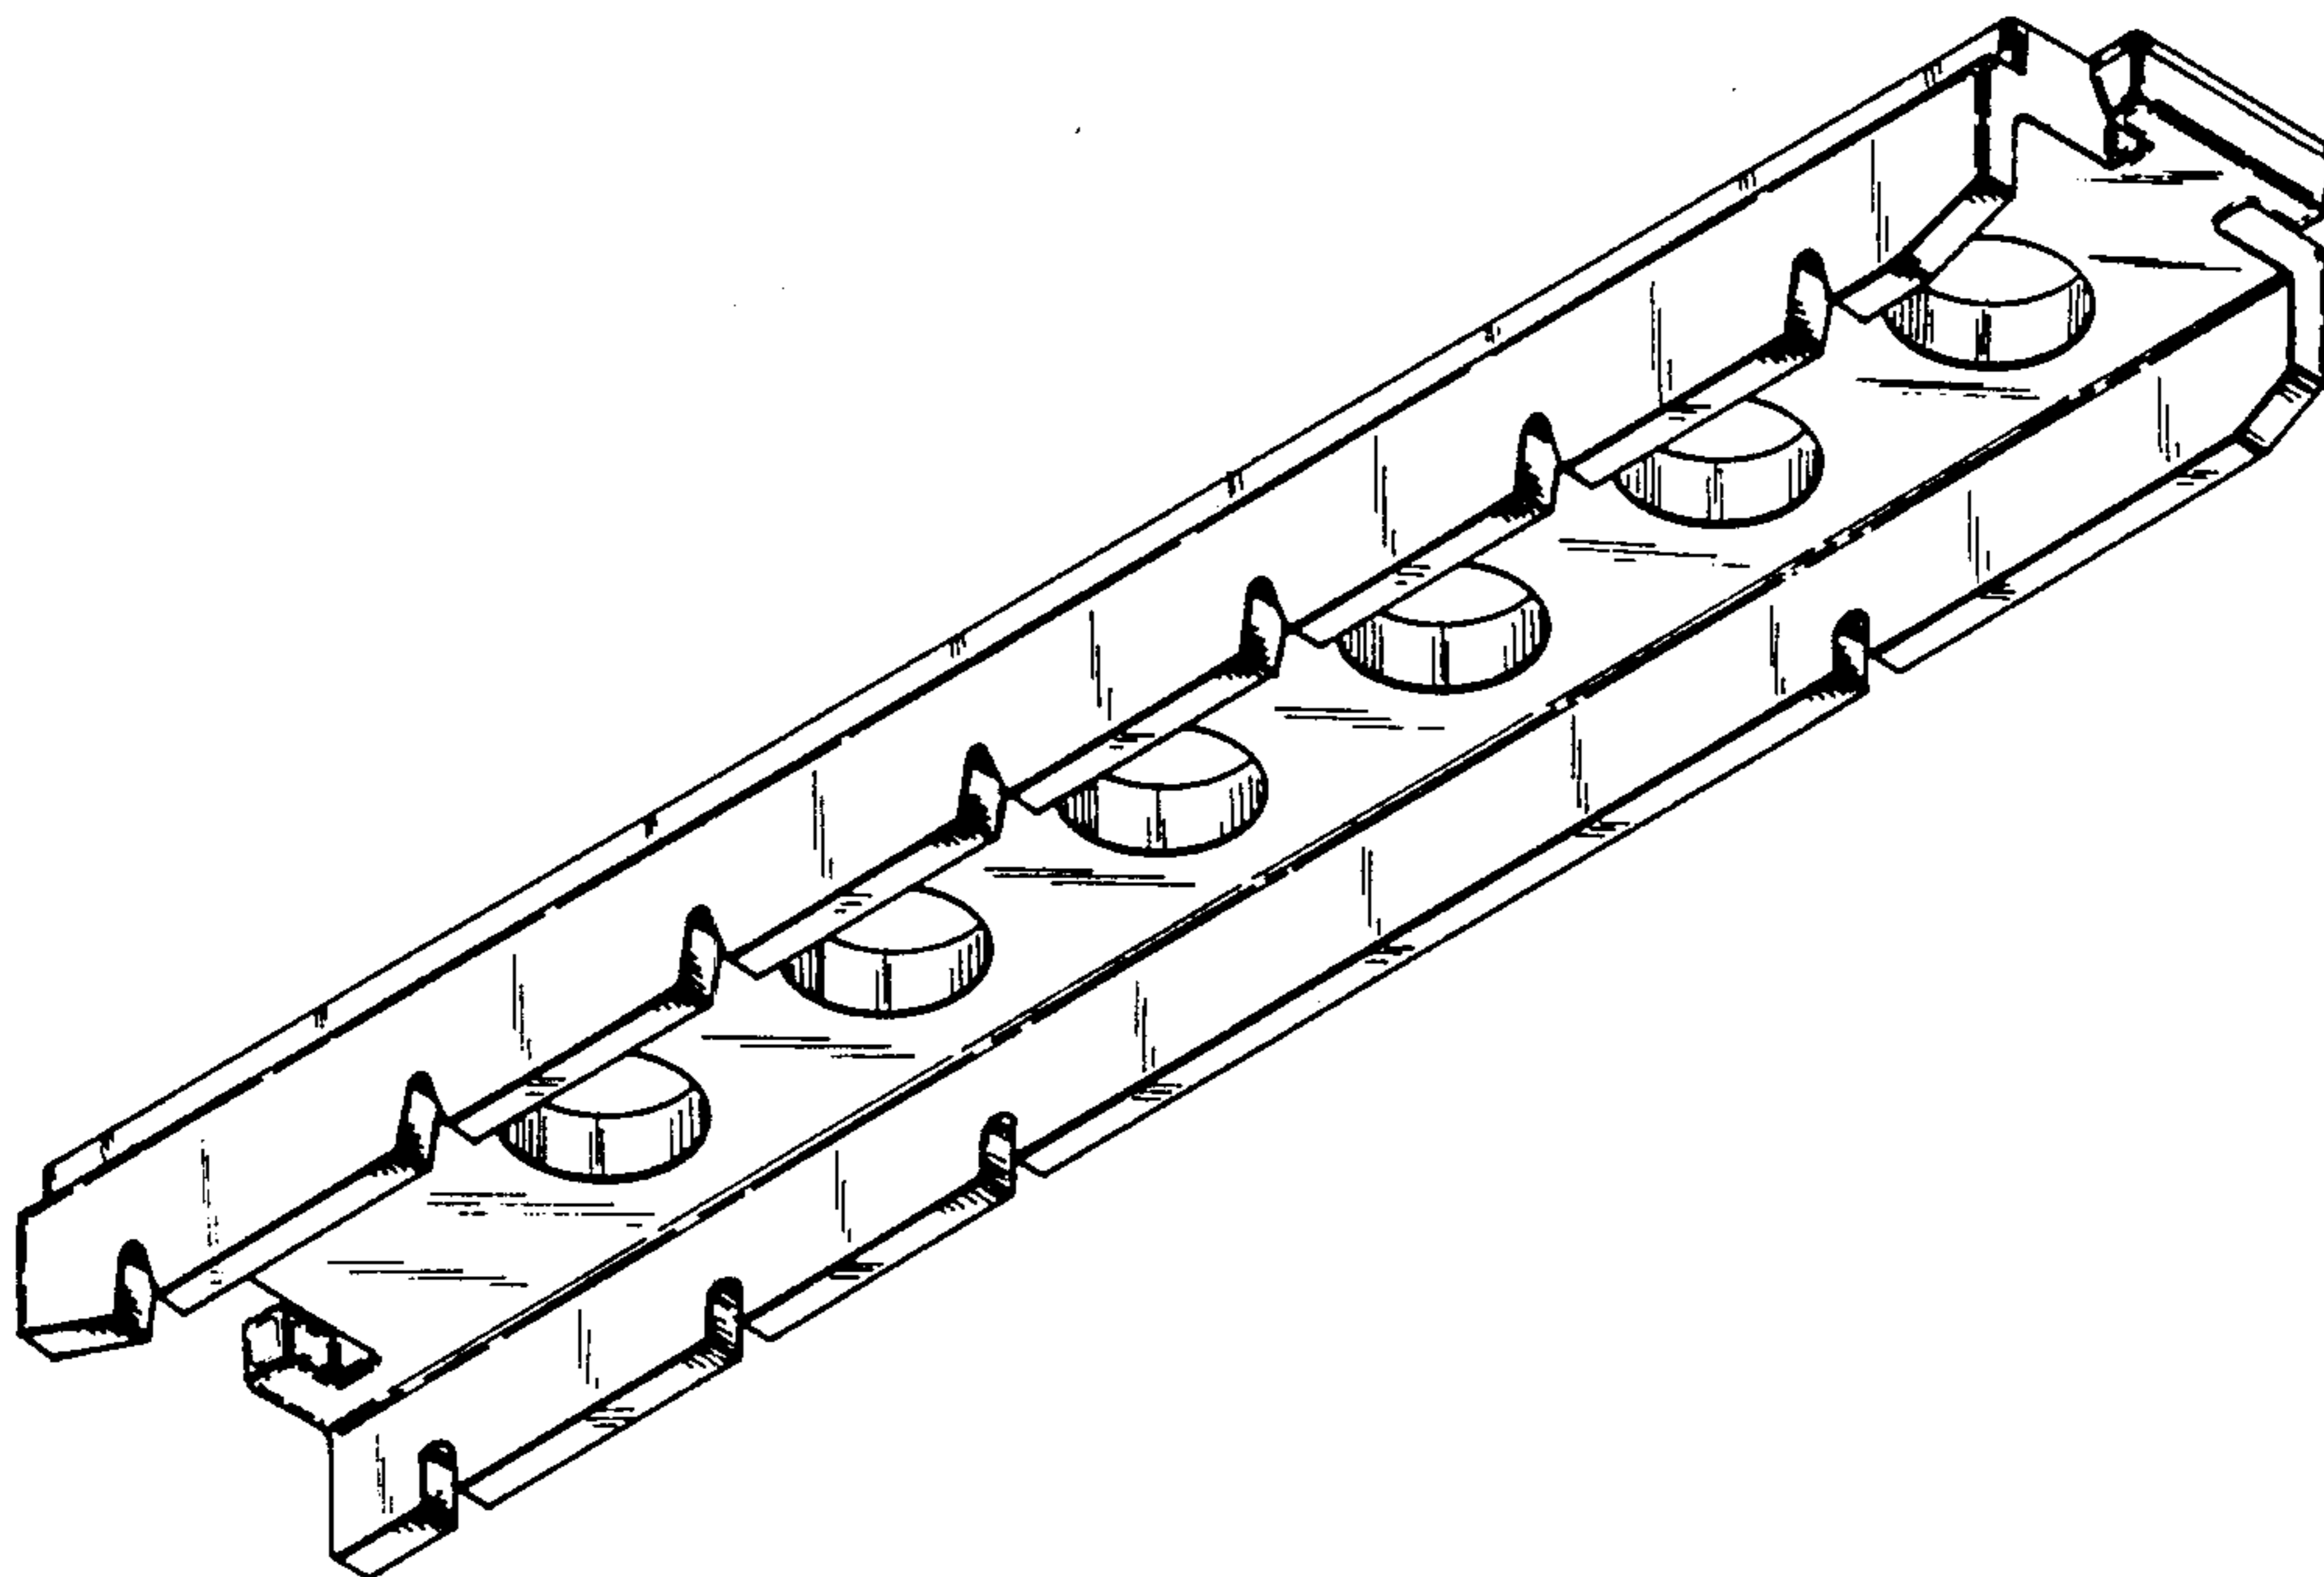

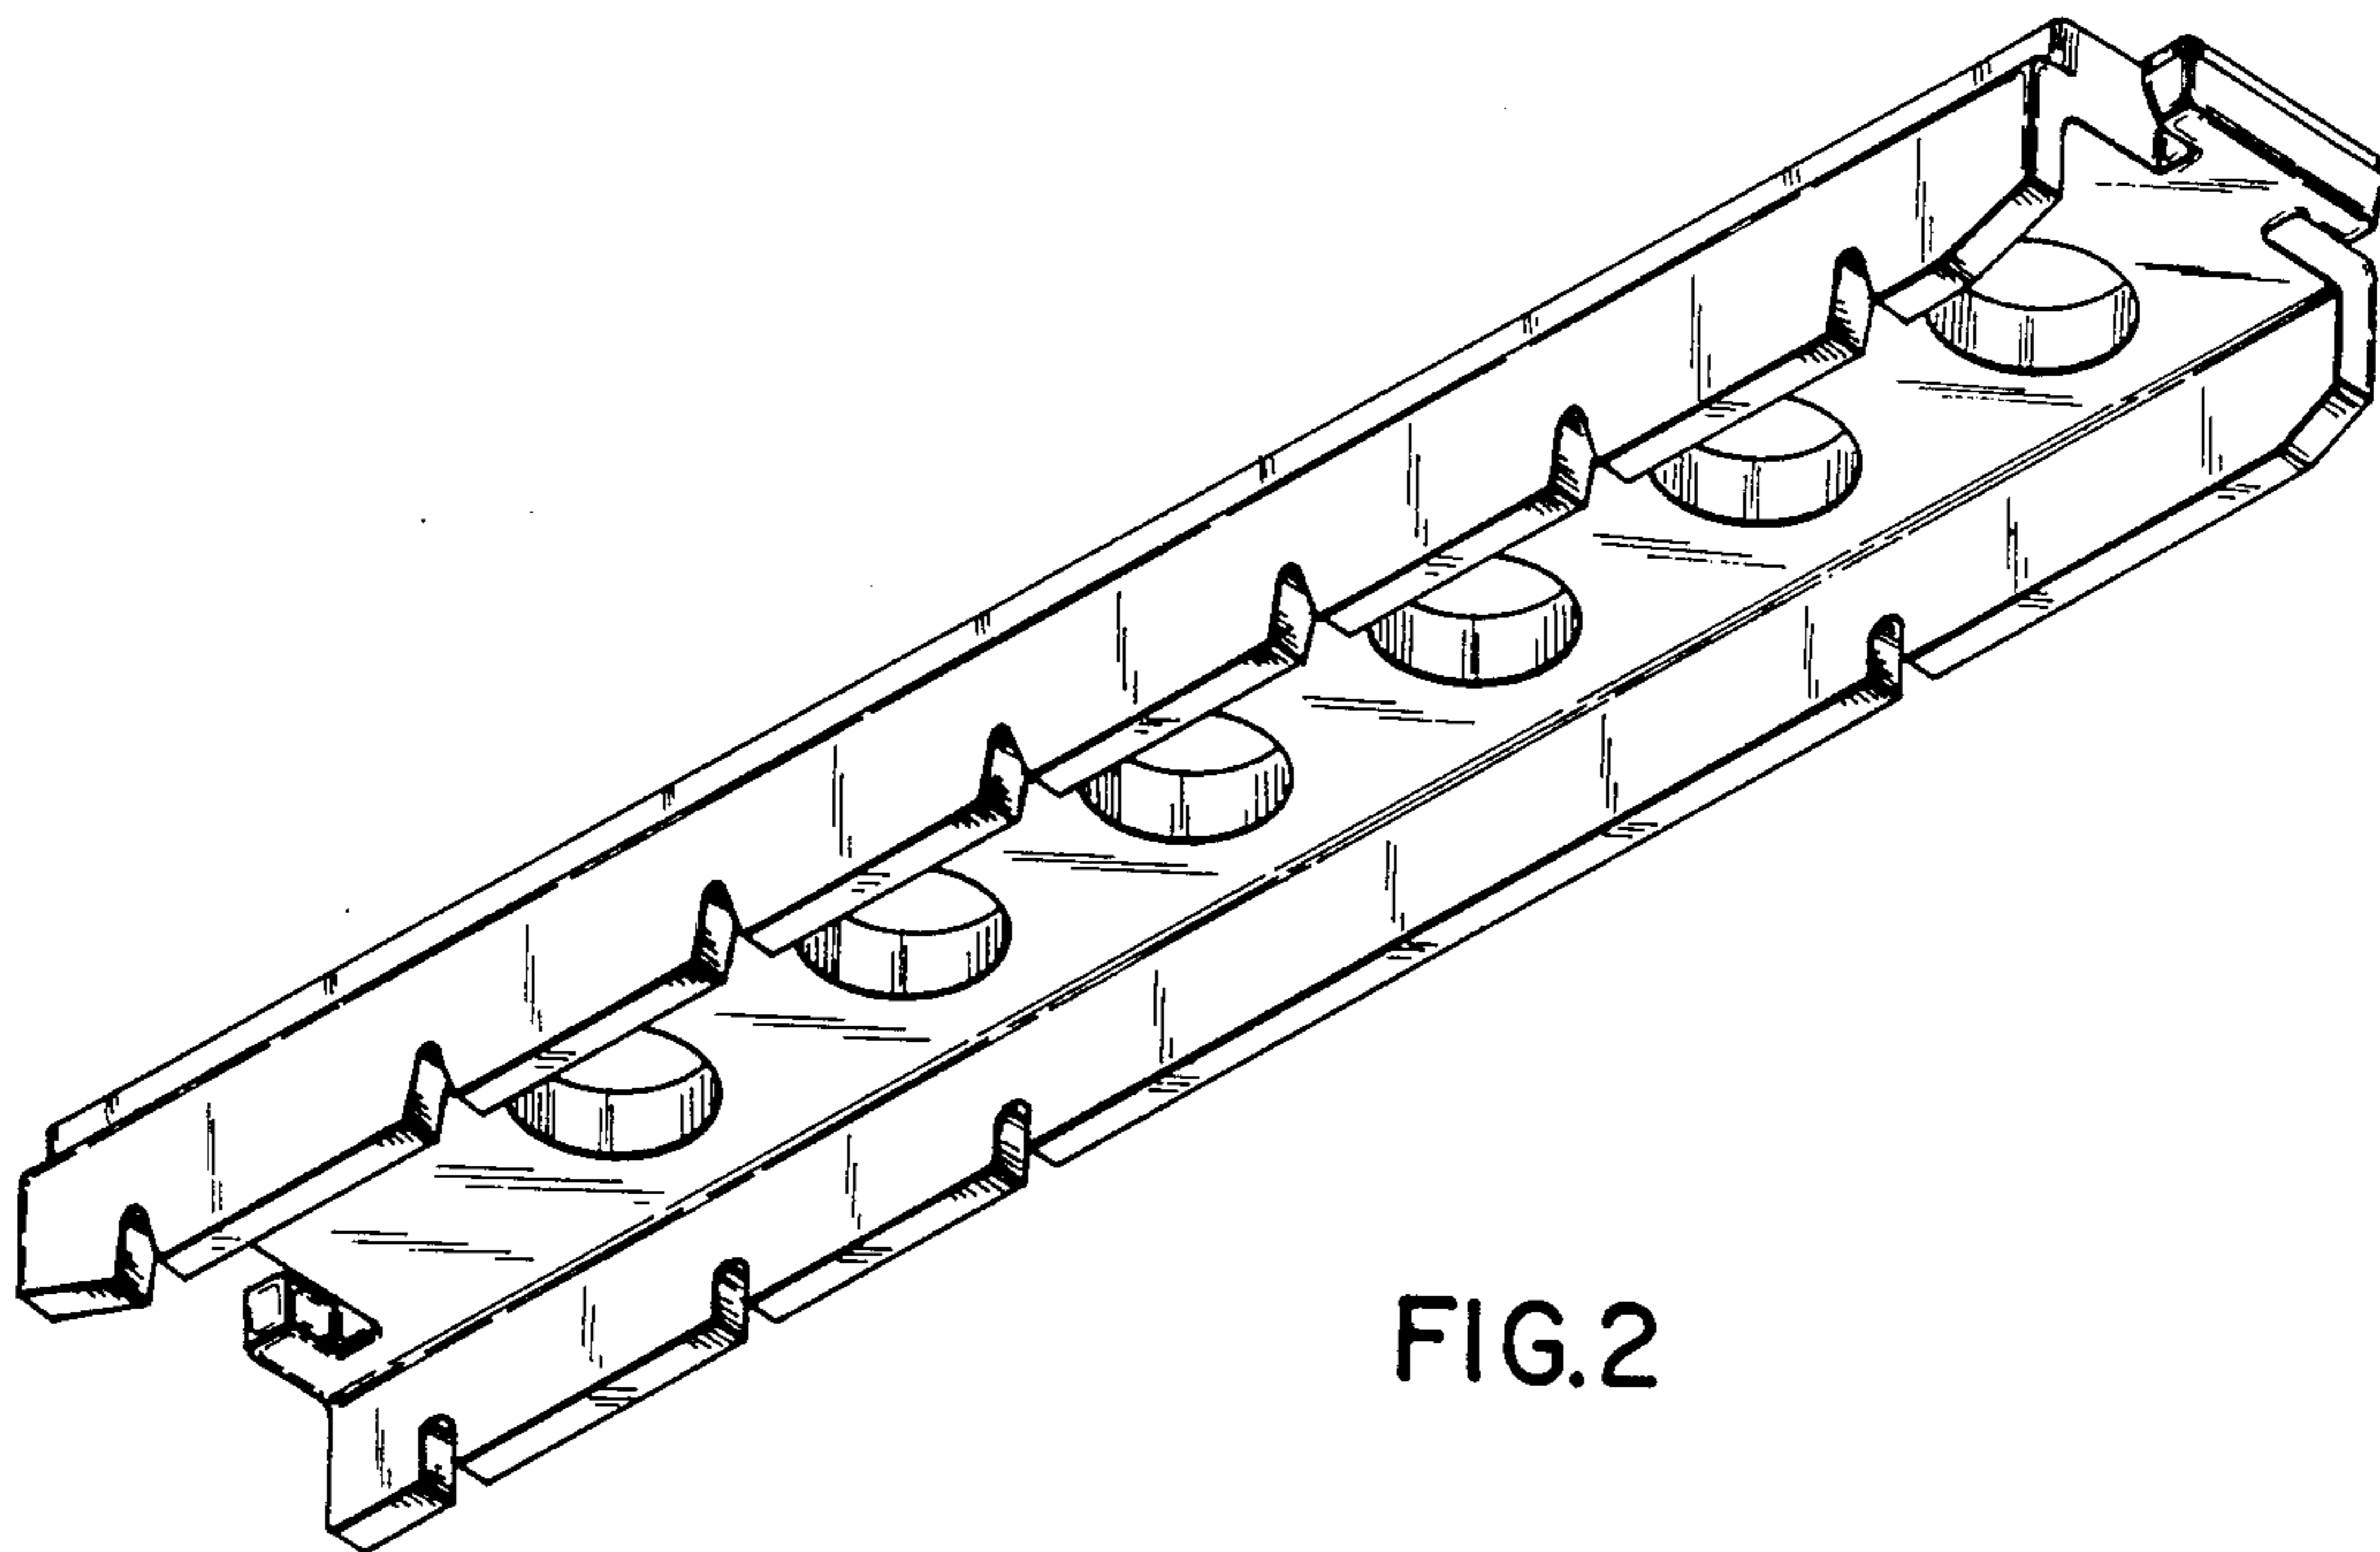


FIG. 2

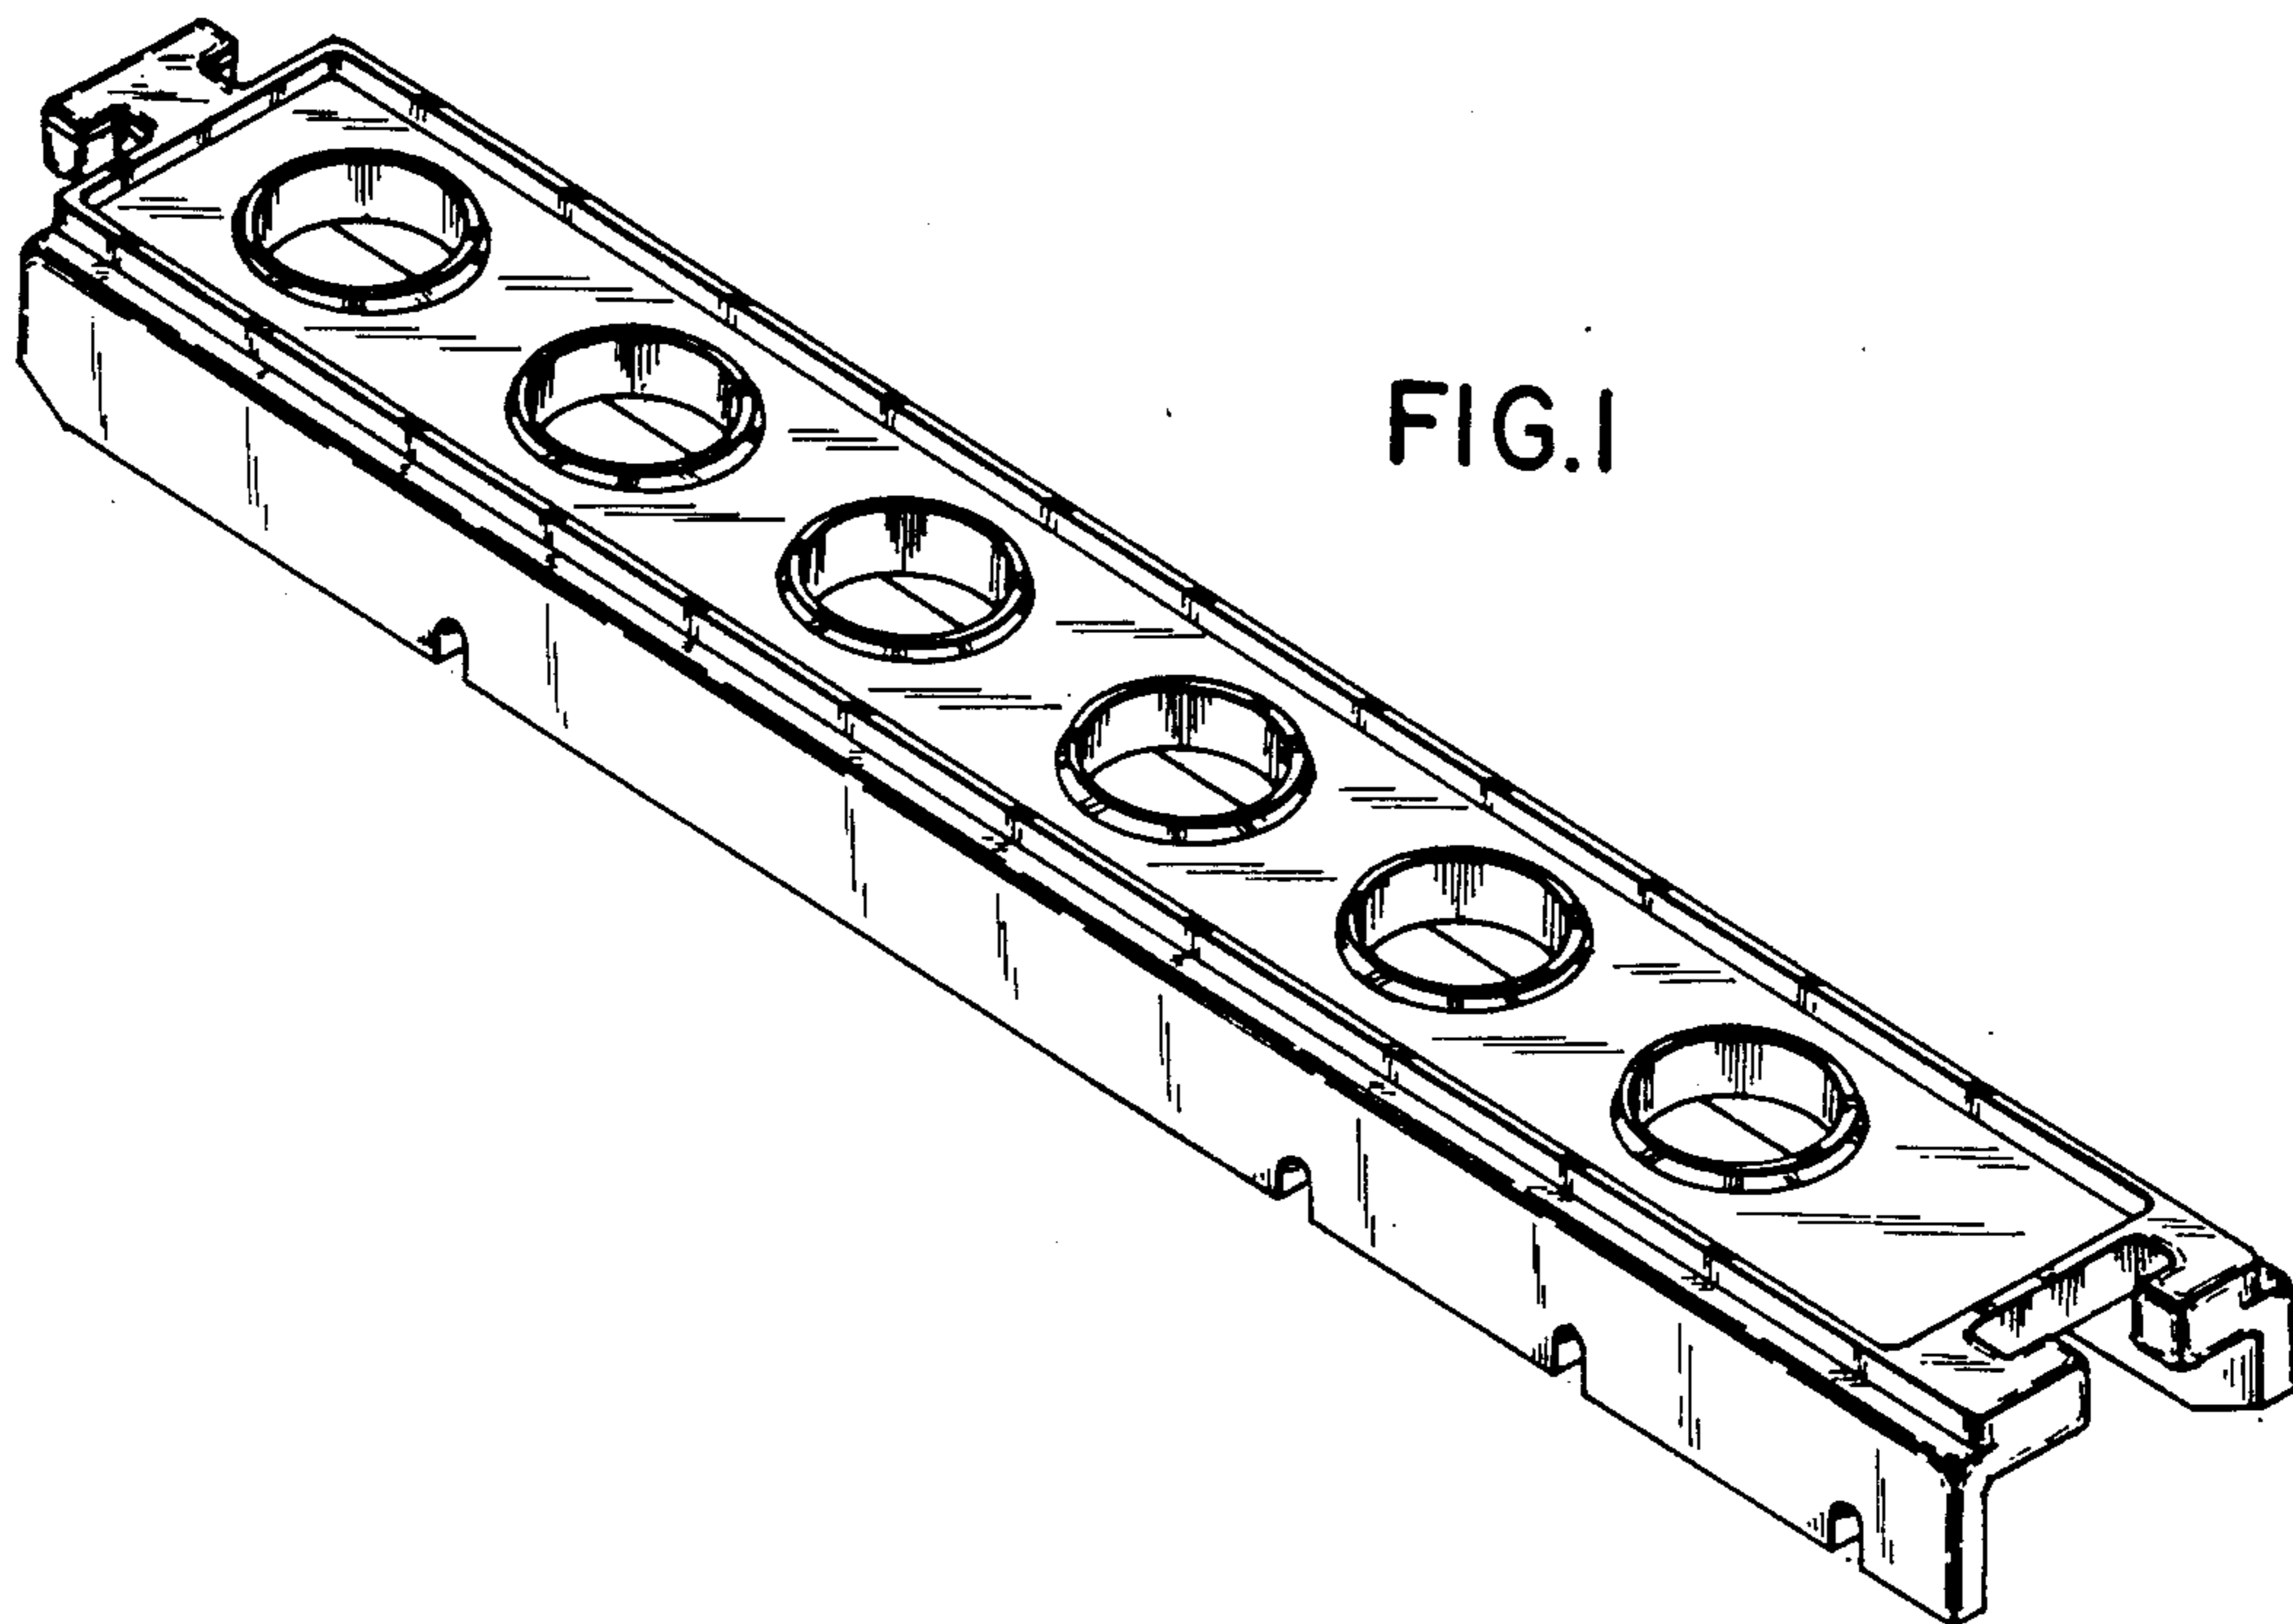


FIG. 1