

[54] OXYGEN ANALYZER HOUSING

[75] Inventors: Robert O. Rowland, Hemet; Miguel A. Ruksenas, Fallbrook, both of Calif.

[73] Assignee: Hudson Oxygen Therapy Sales Company, Temecula, Calif.

[**] Term: 14 Years

[21] Appl. No.: 747,922

[22] Filed: Dec. 6, 1976

[51] Int. Cl. D24-02

[52] U.S. Cl. D24/17; D24/99

[58] Field of Search D24/8, 17, 21, 99; D87/1 R; D10/46; 128/2.06 R, 2.07; 73/431; 324/30, 11.5

[56] References Cited

U.S. PATENT DOCUMENTS

D. 224,813 9/1972 Sato D24/17

D. 224,814 9/1972 Sato D24/17
D. 228,471 9/1973 Harper D24/17
D. 245,455 8/1977 Cathey D87/1 R

OTHER PUBLICATIONS

Allied Industrial Electronics Cat., 1972, p. 572, "Power-line Amplifier", top right of page.


Primary Examiner—Bernard Ansher
Attorney, Agent, or Firm—Jerry R. Seiler

[57] CLAIM

The ornamental design for an oxygen analyzer housing, as shown.

DESCRIPTION

FIG. 1 is a perspective view of an oxygen analyzer housing showing our new design; FIG. 2 is a front view thereof; FIG. 3 is a side elevational view thereof; FIG. 4 is a top plan view thereof; FIG. 5 is a rear view thereof; and FIG. 6 is a bottom plan view thereof.

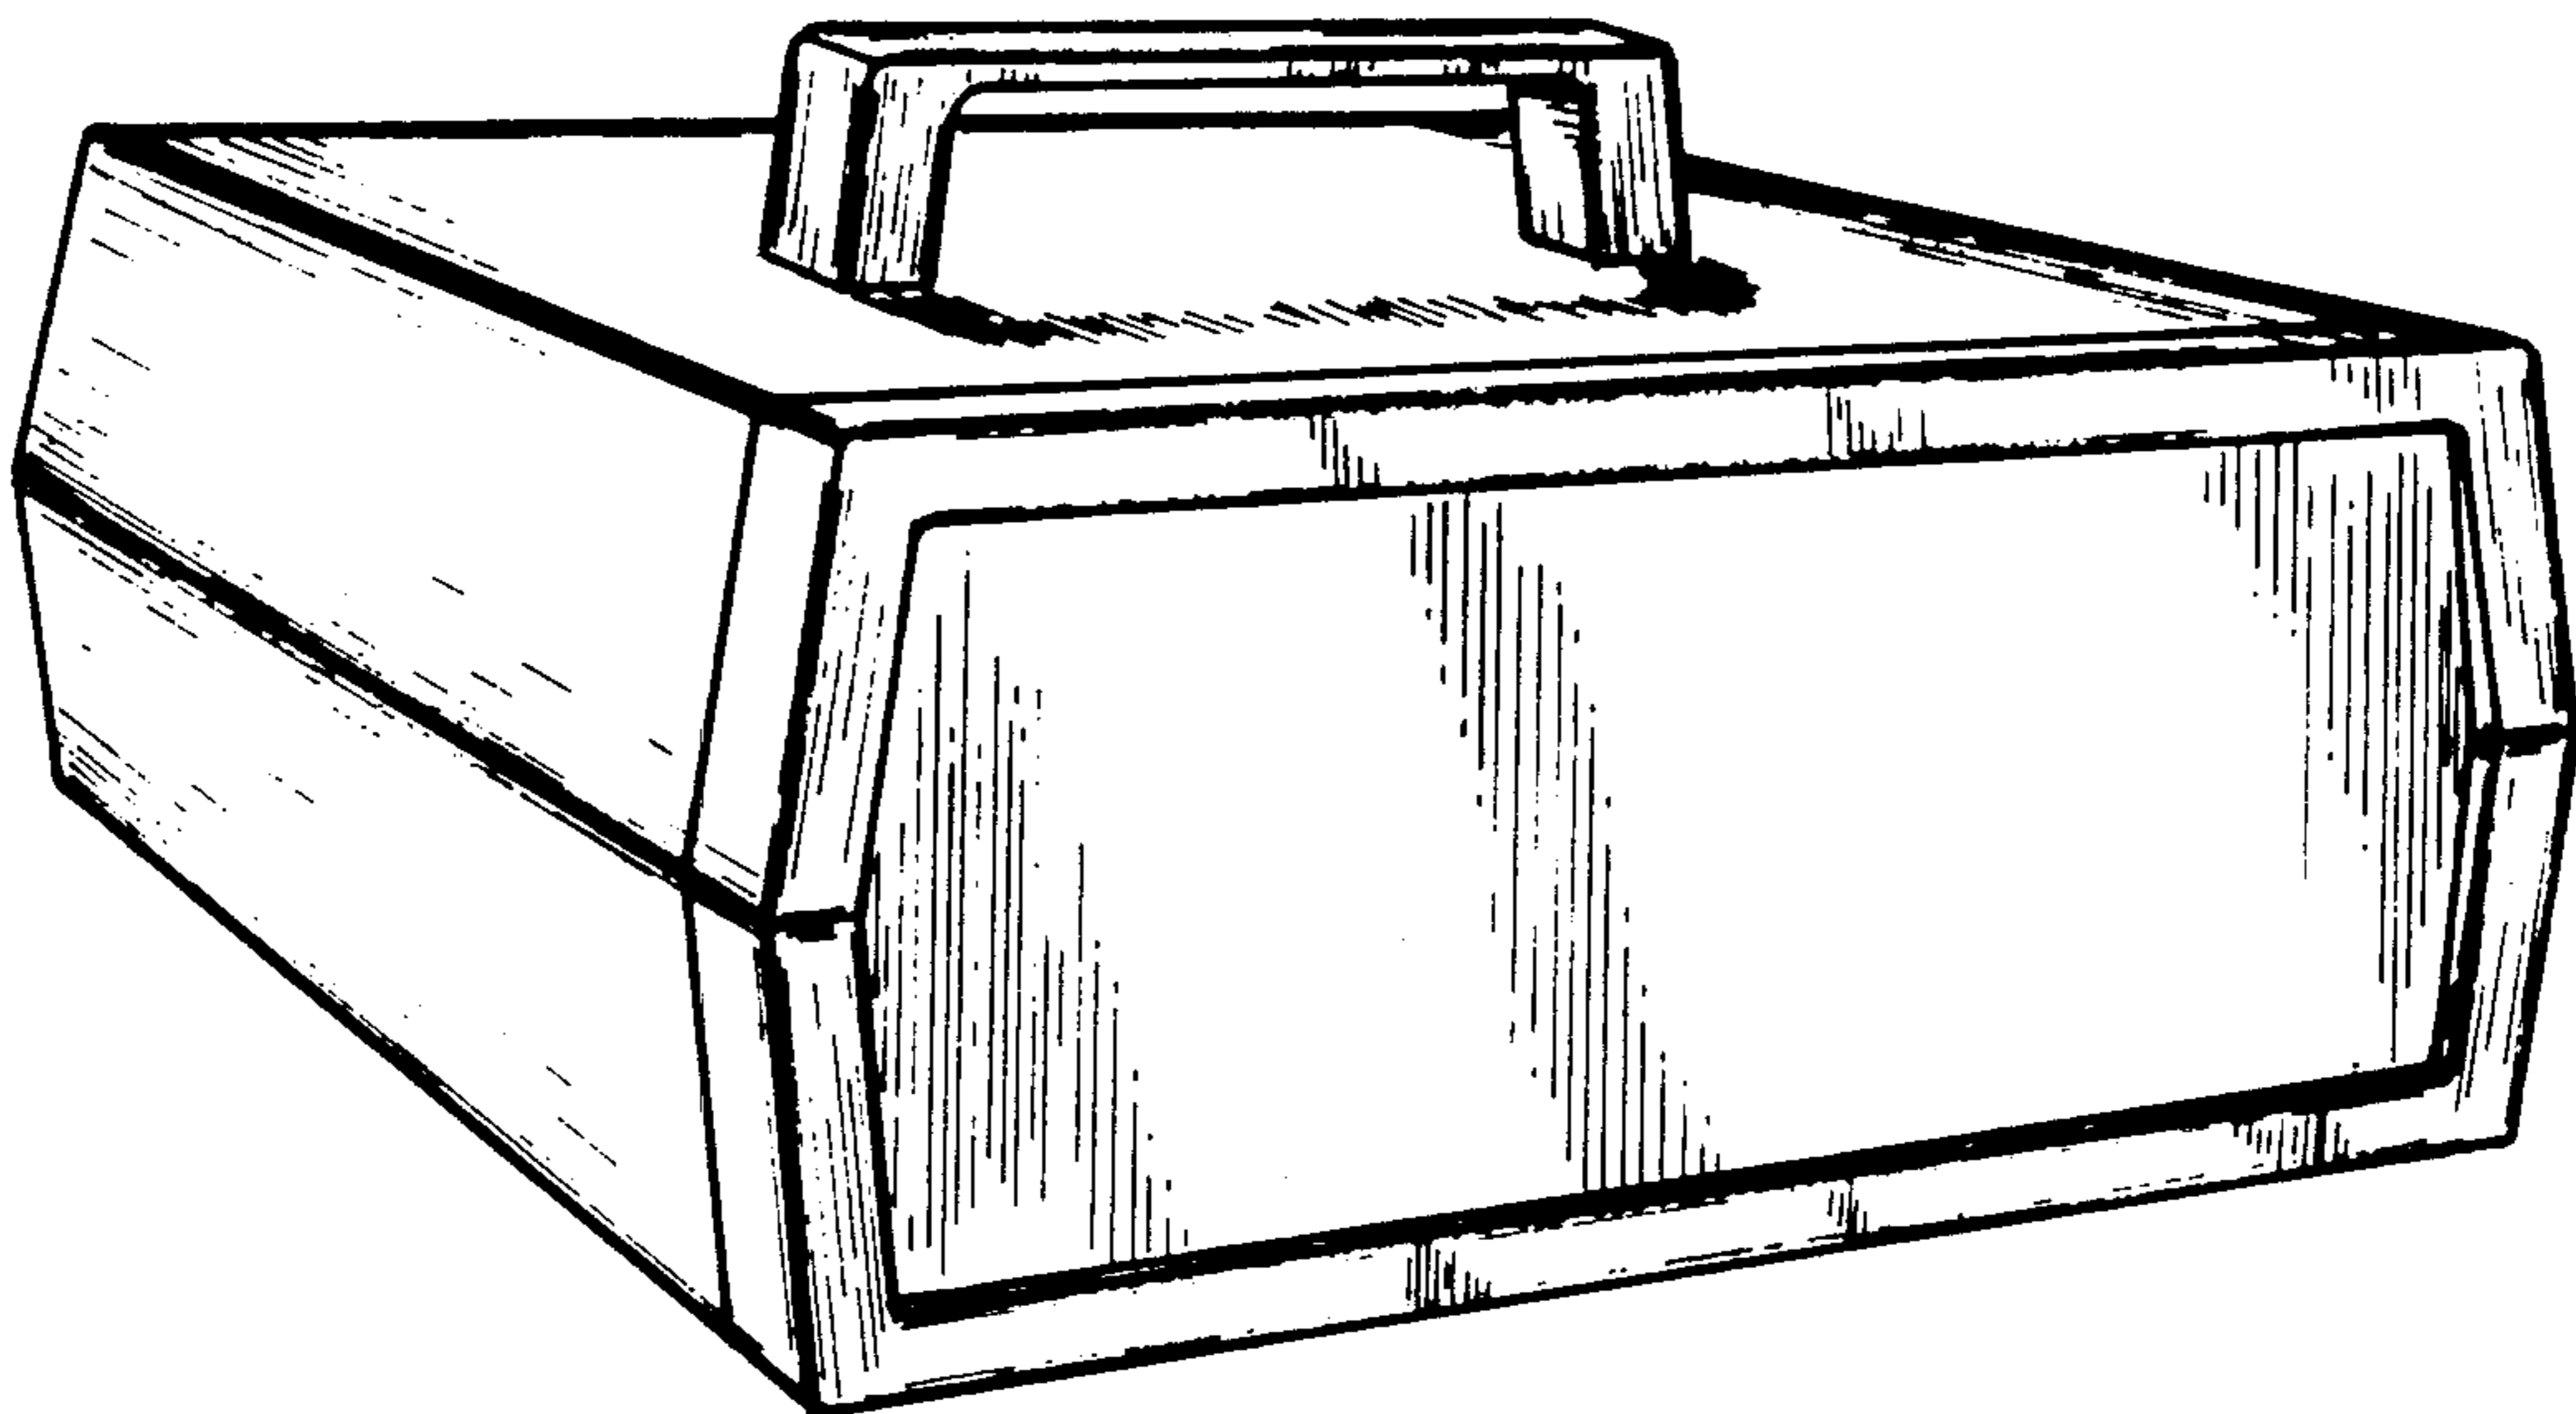

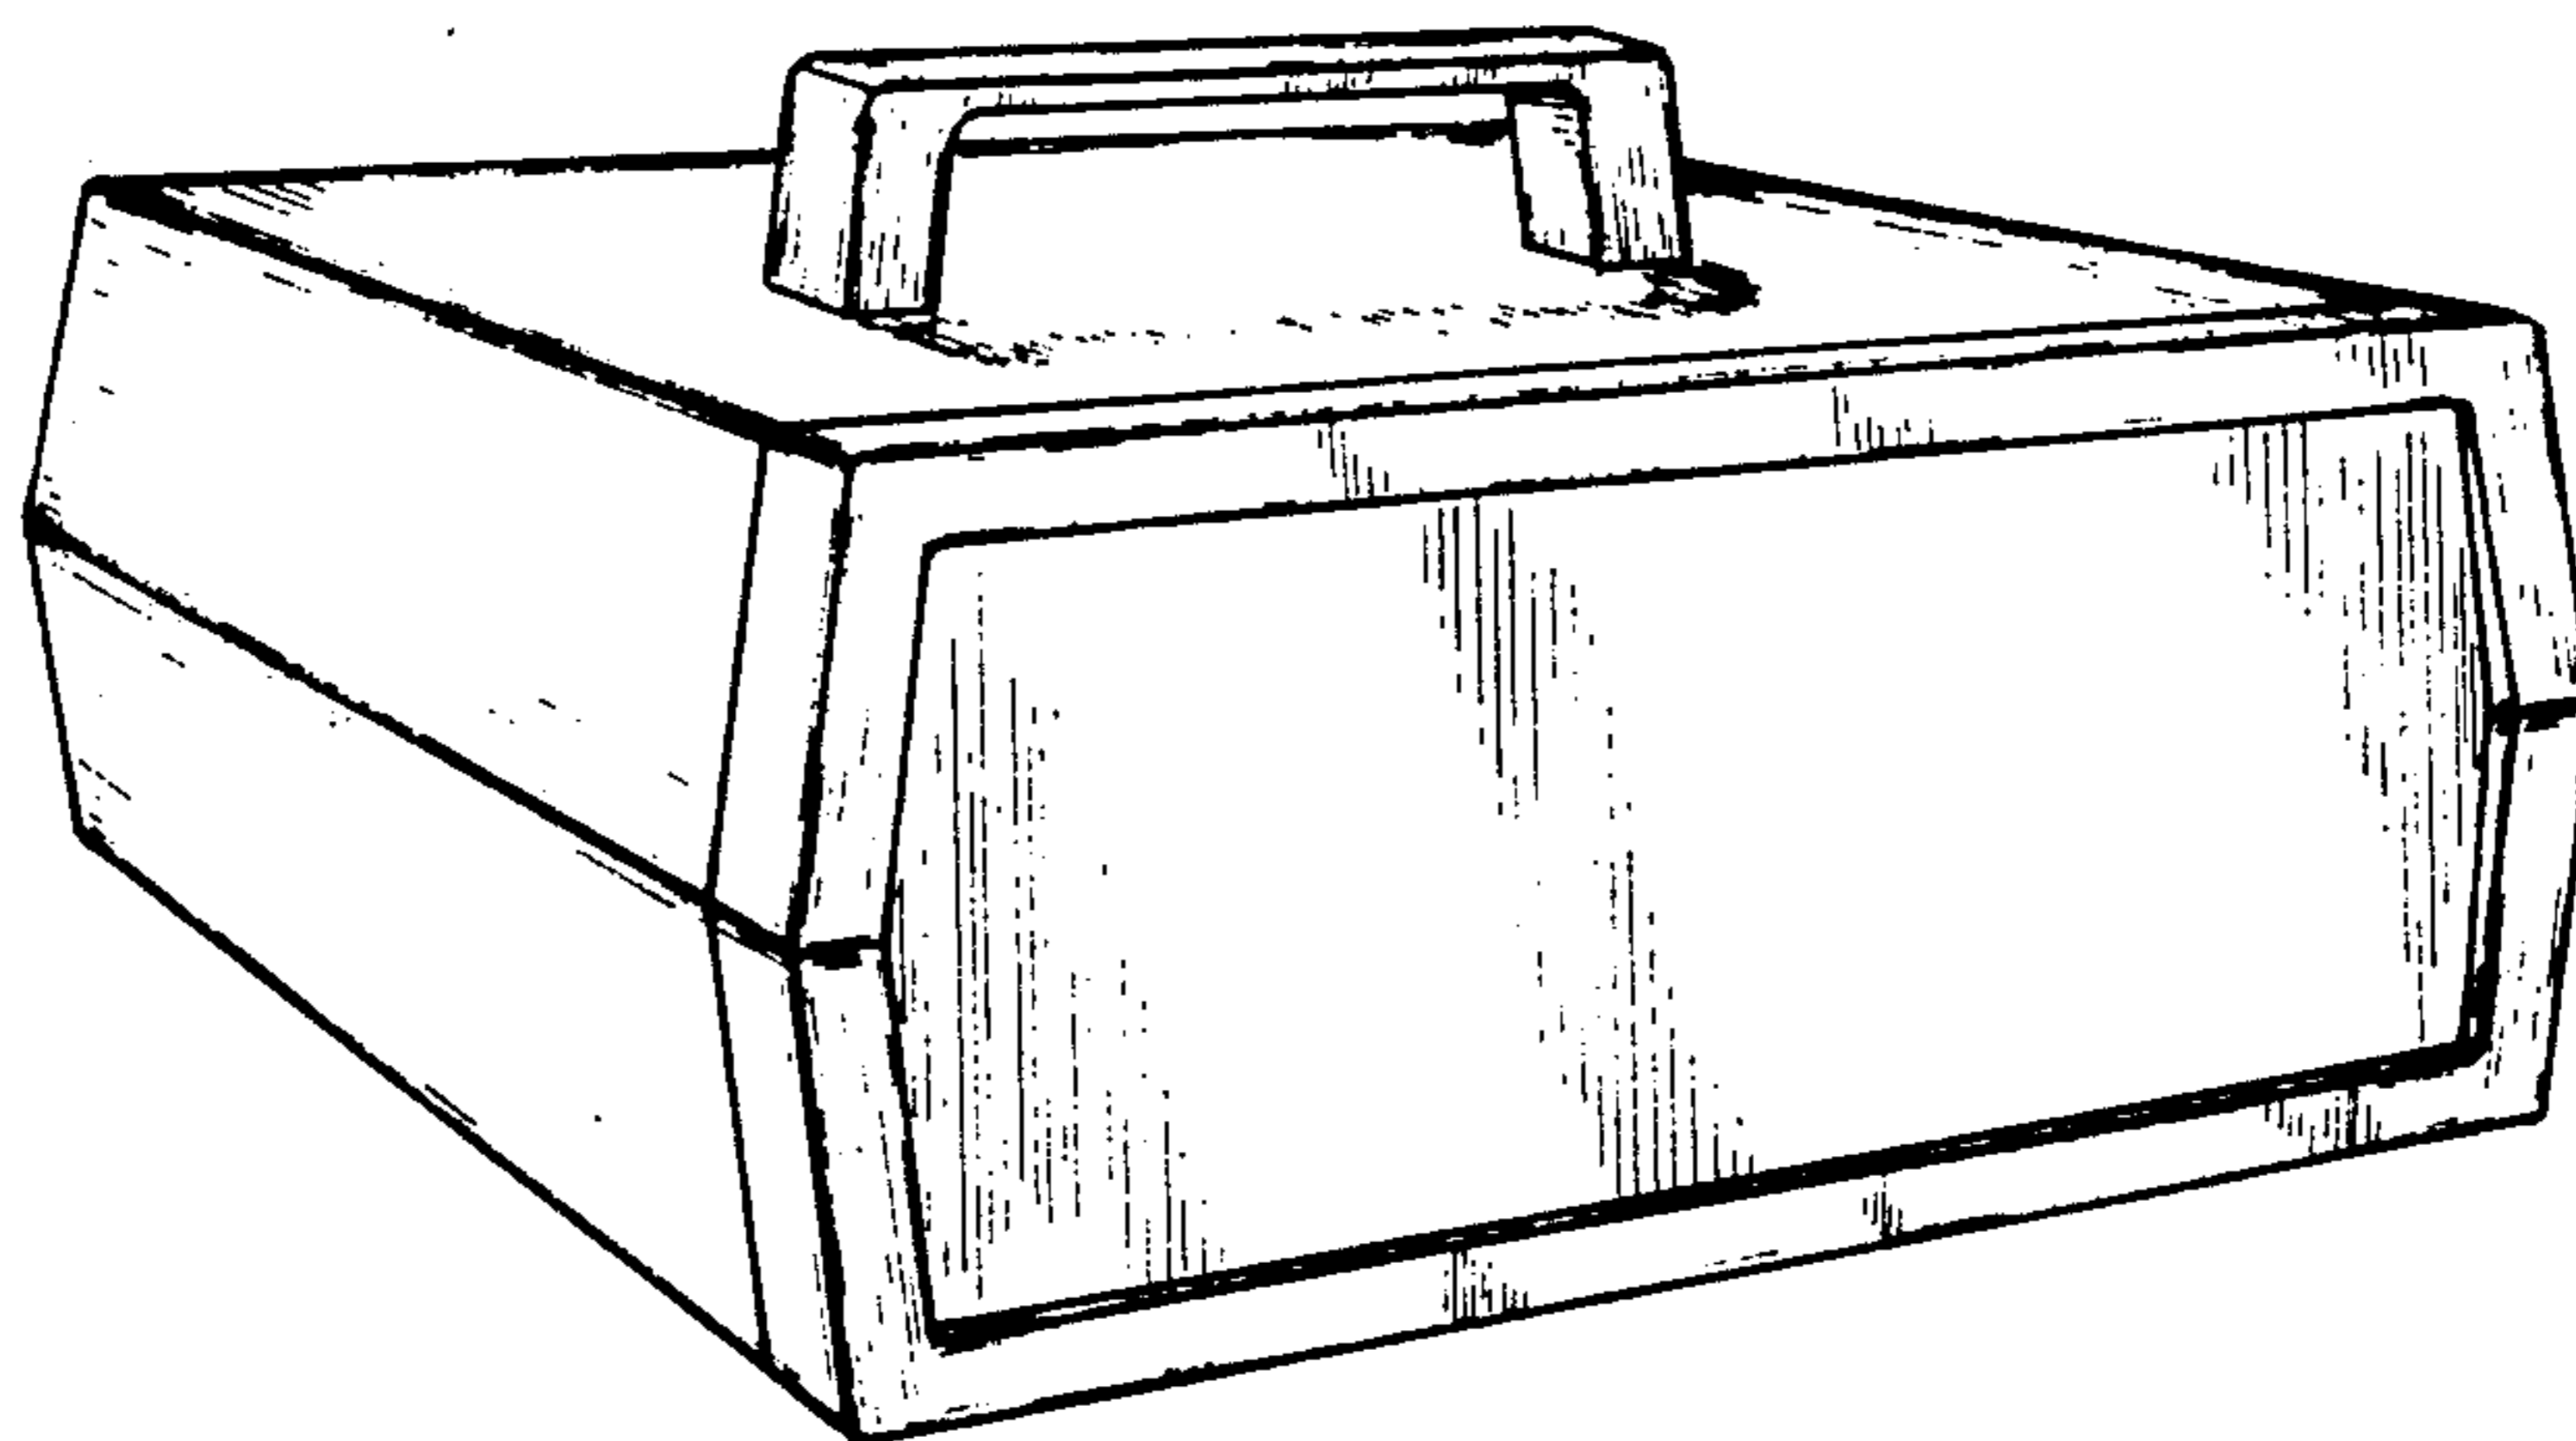


FIGURE 1.

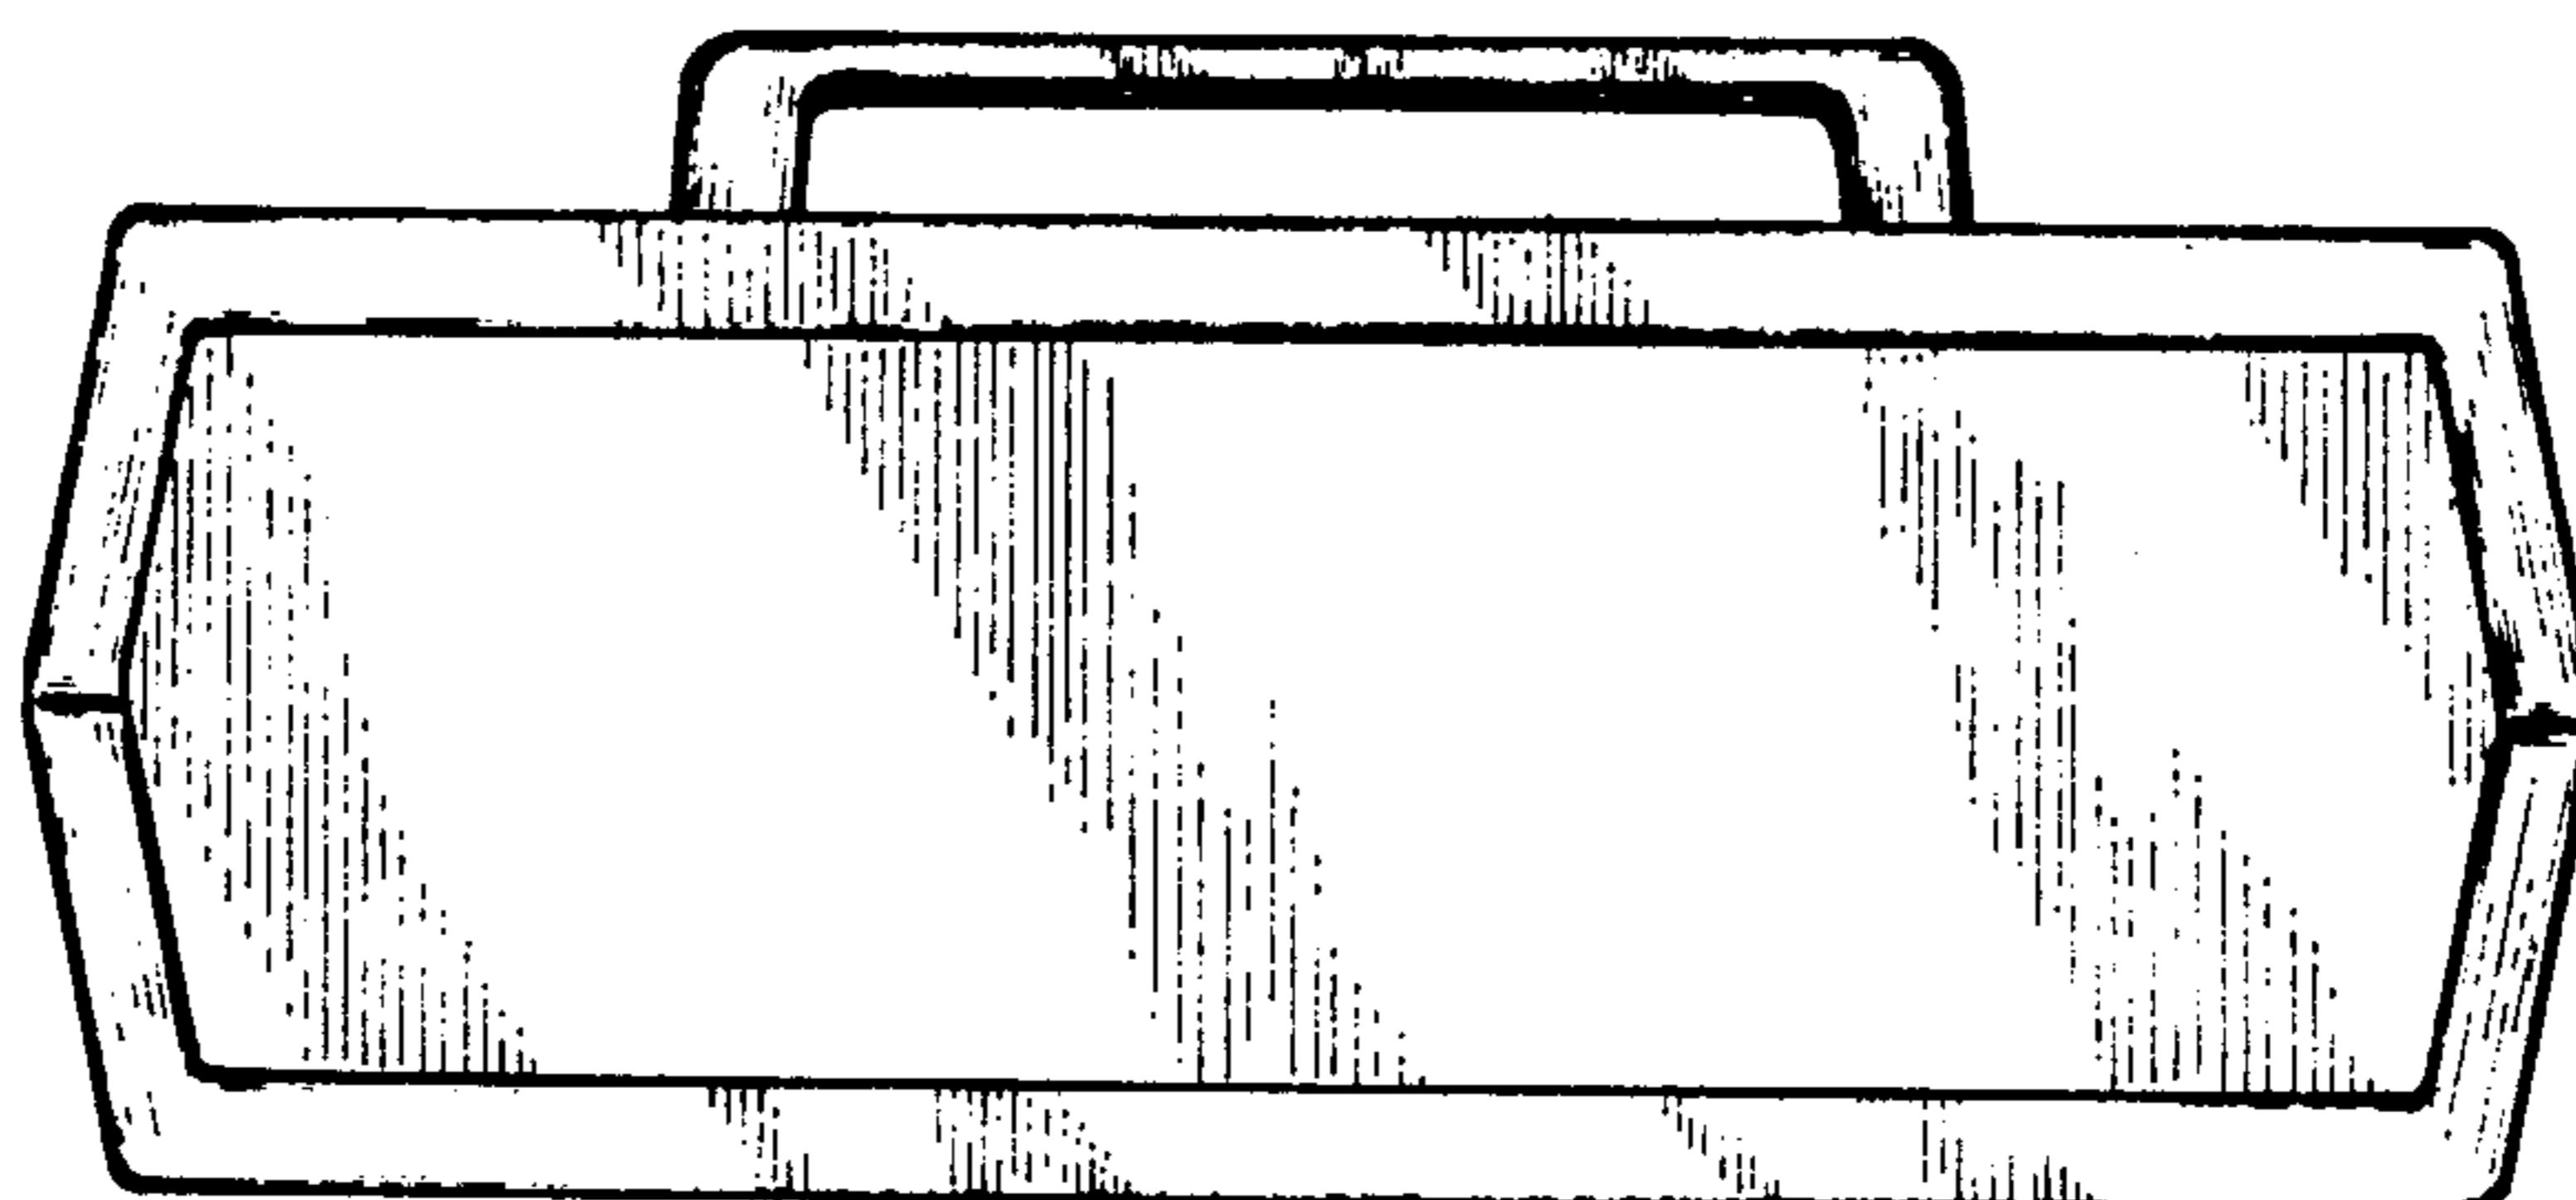


FIGURE 2.

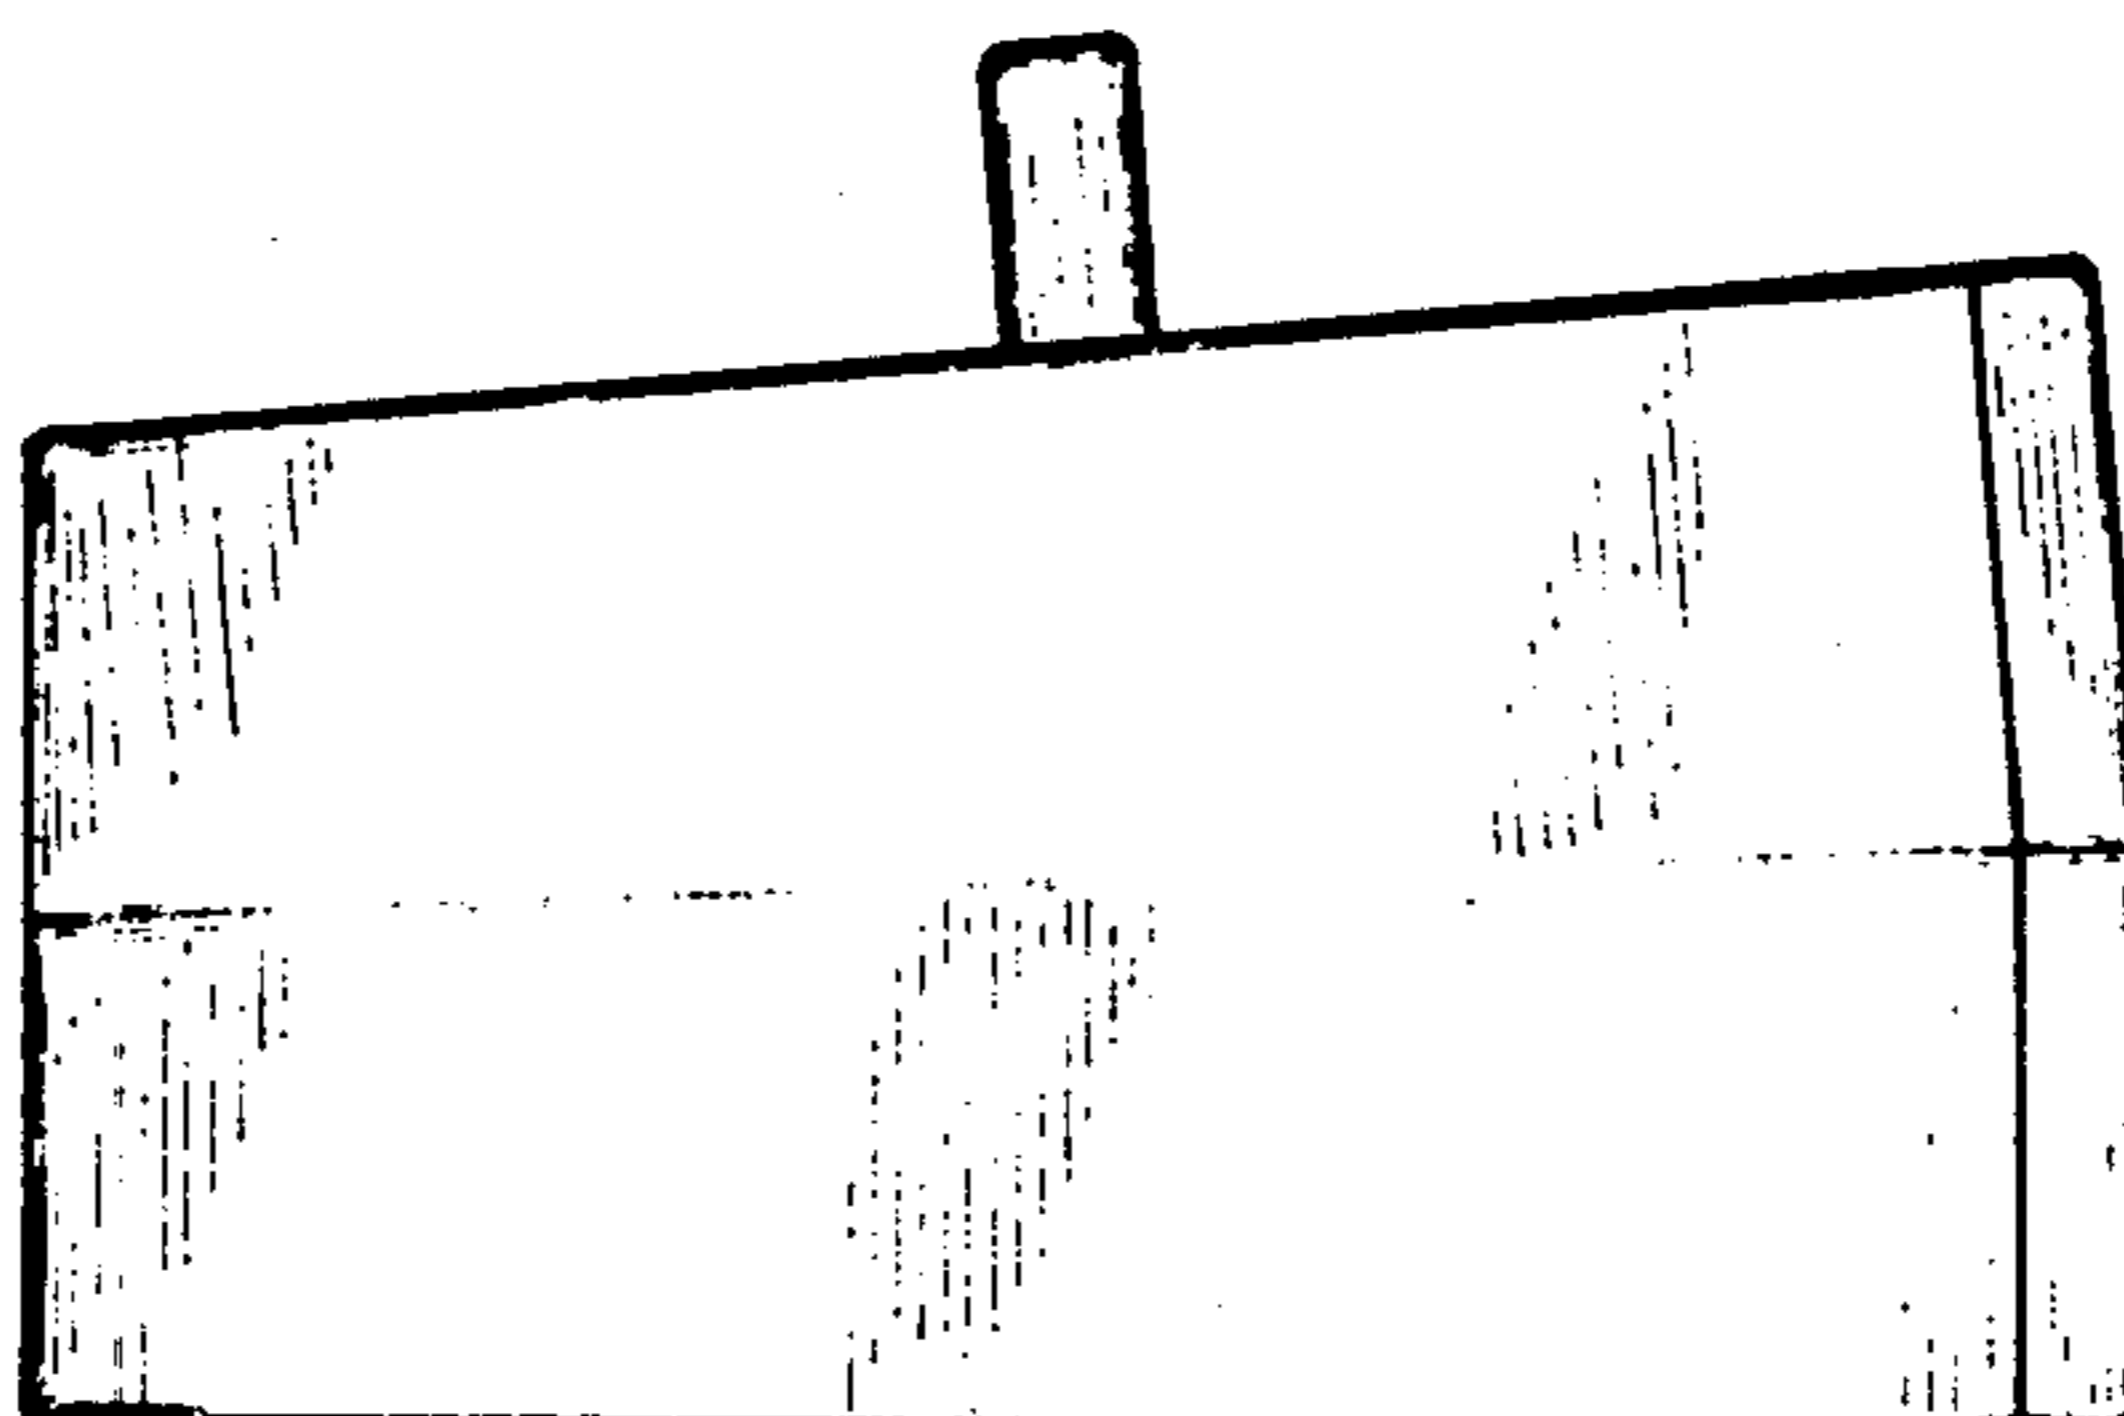


FIGURE 3.

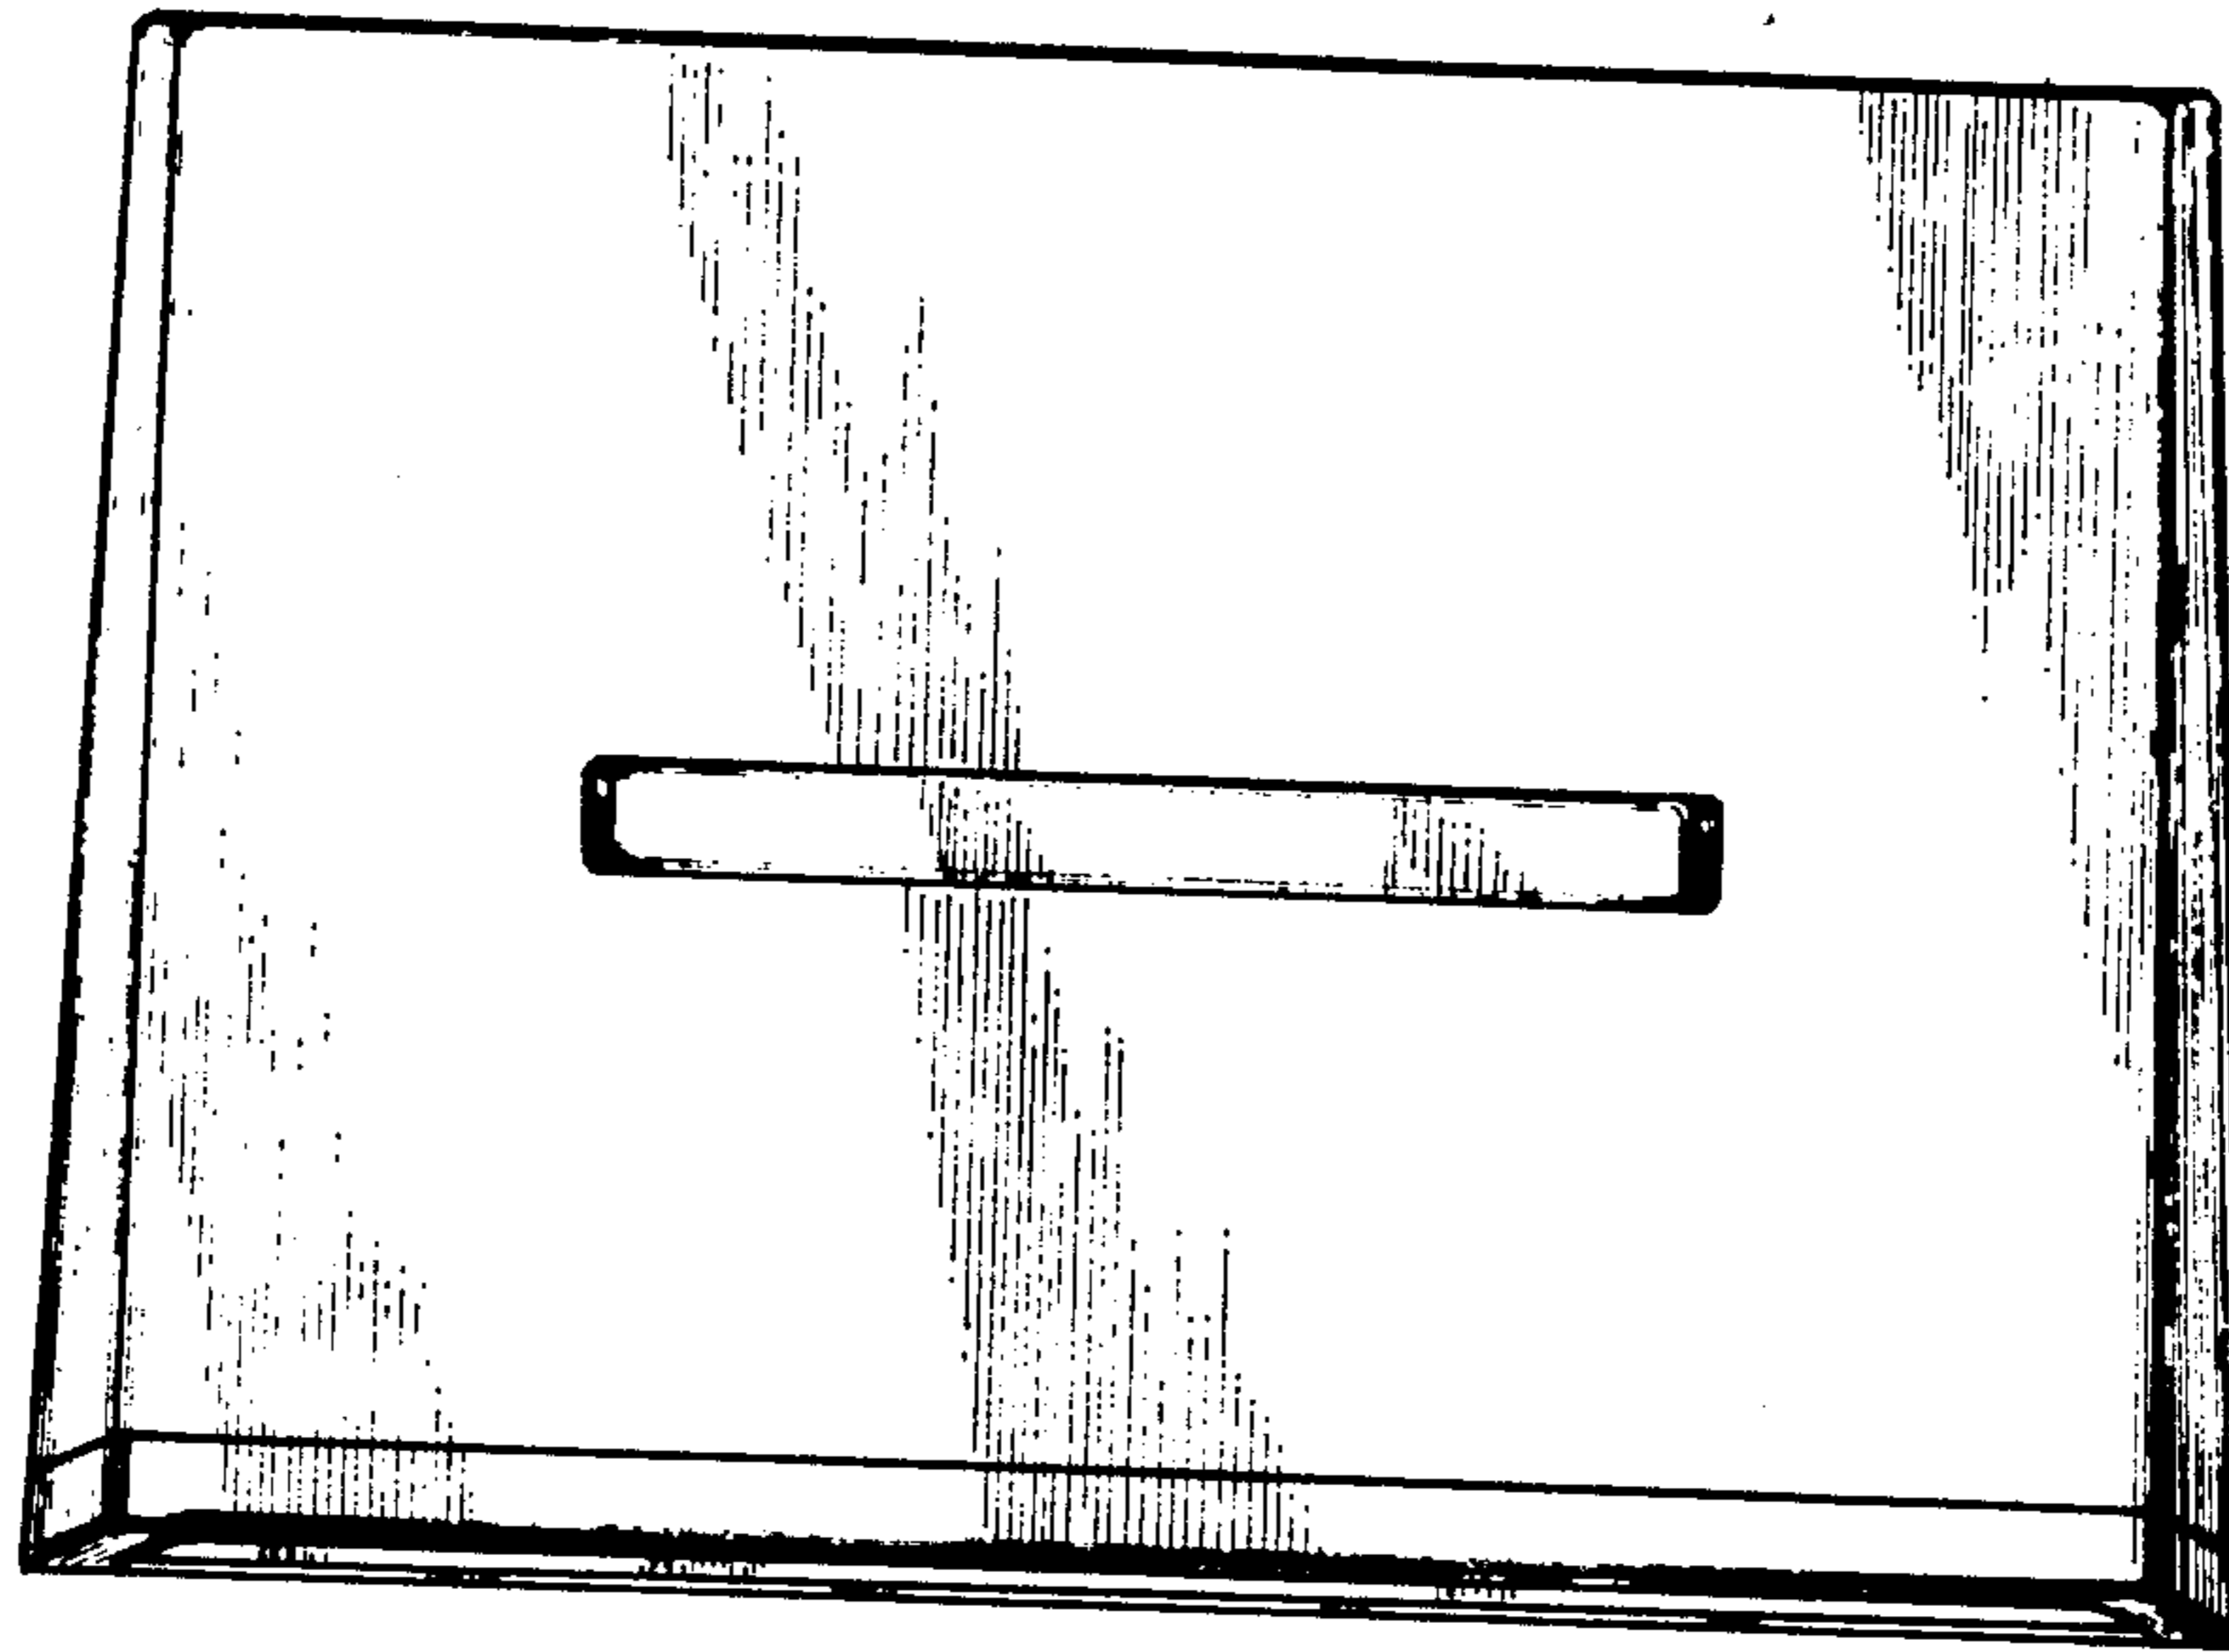


FIGURE 4.

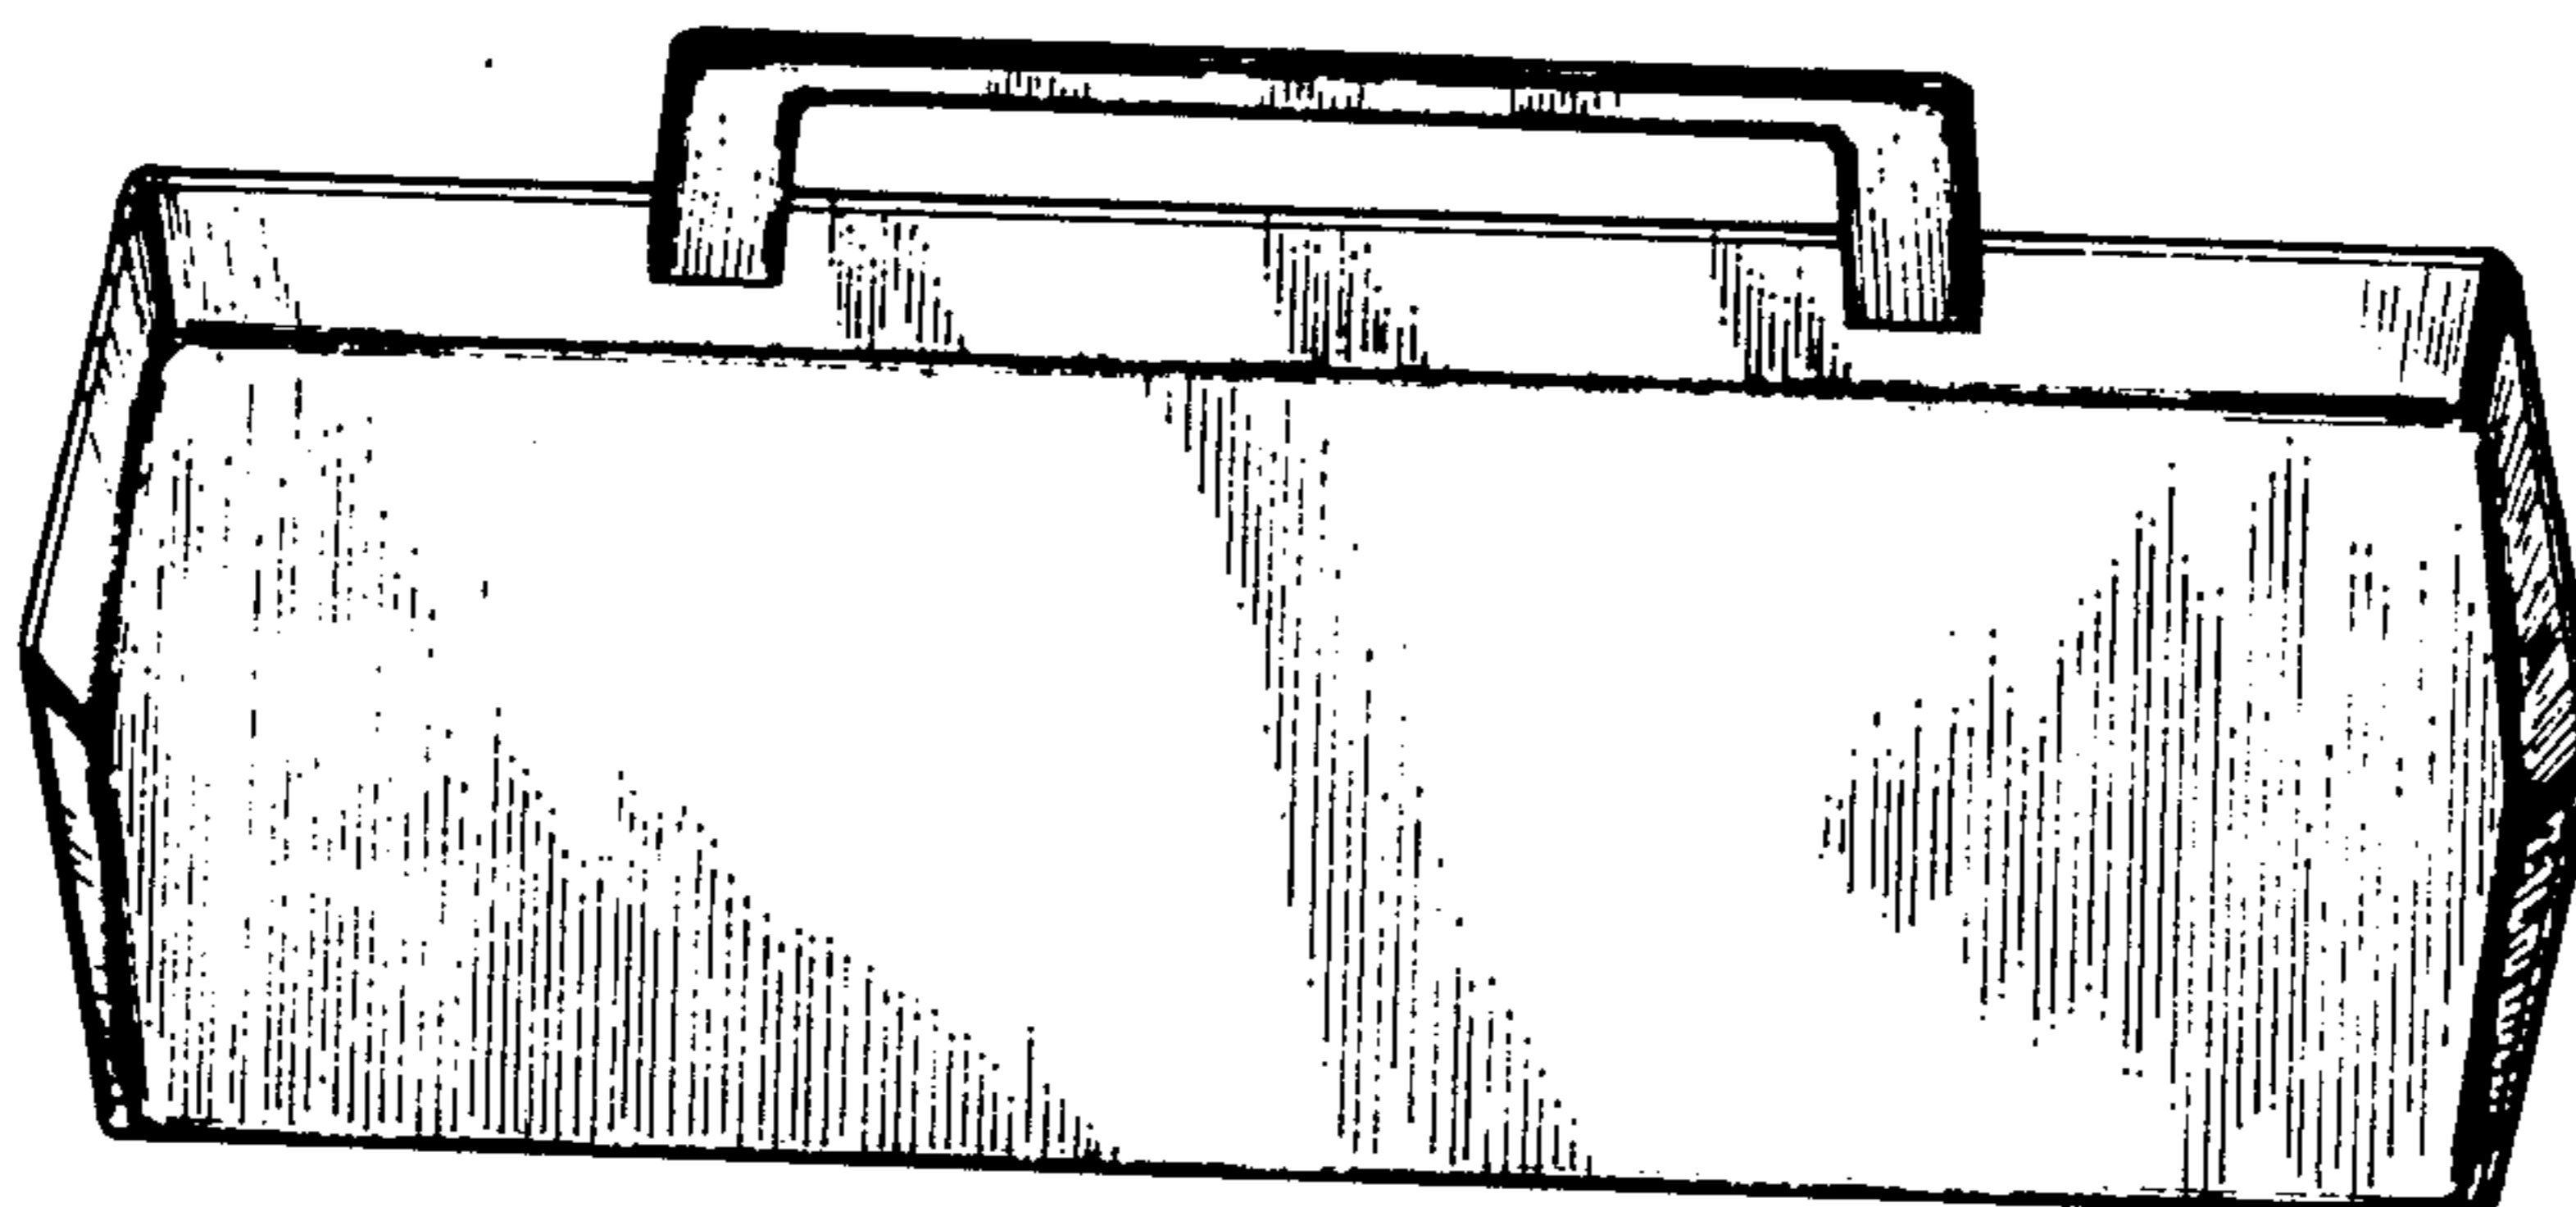


FIGURE 5.

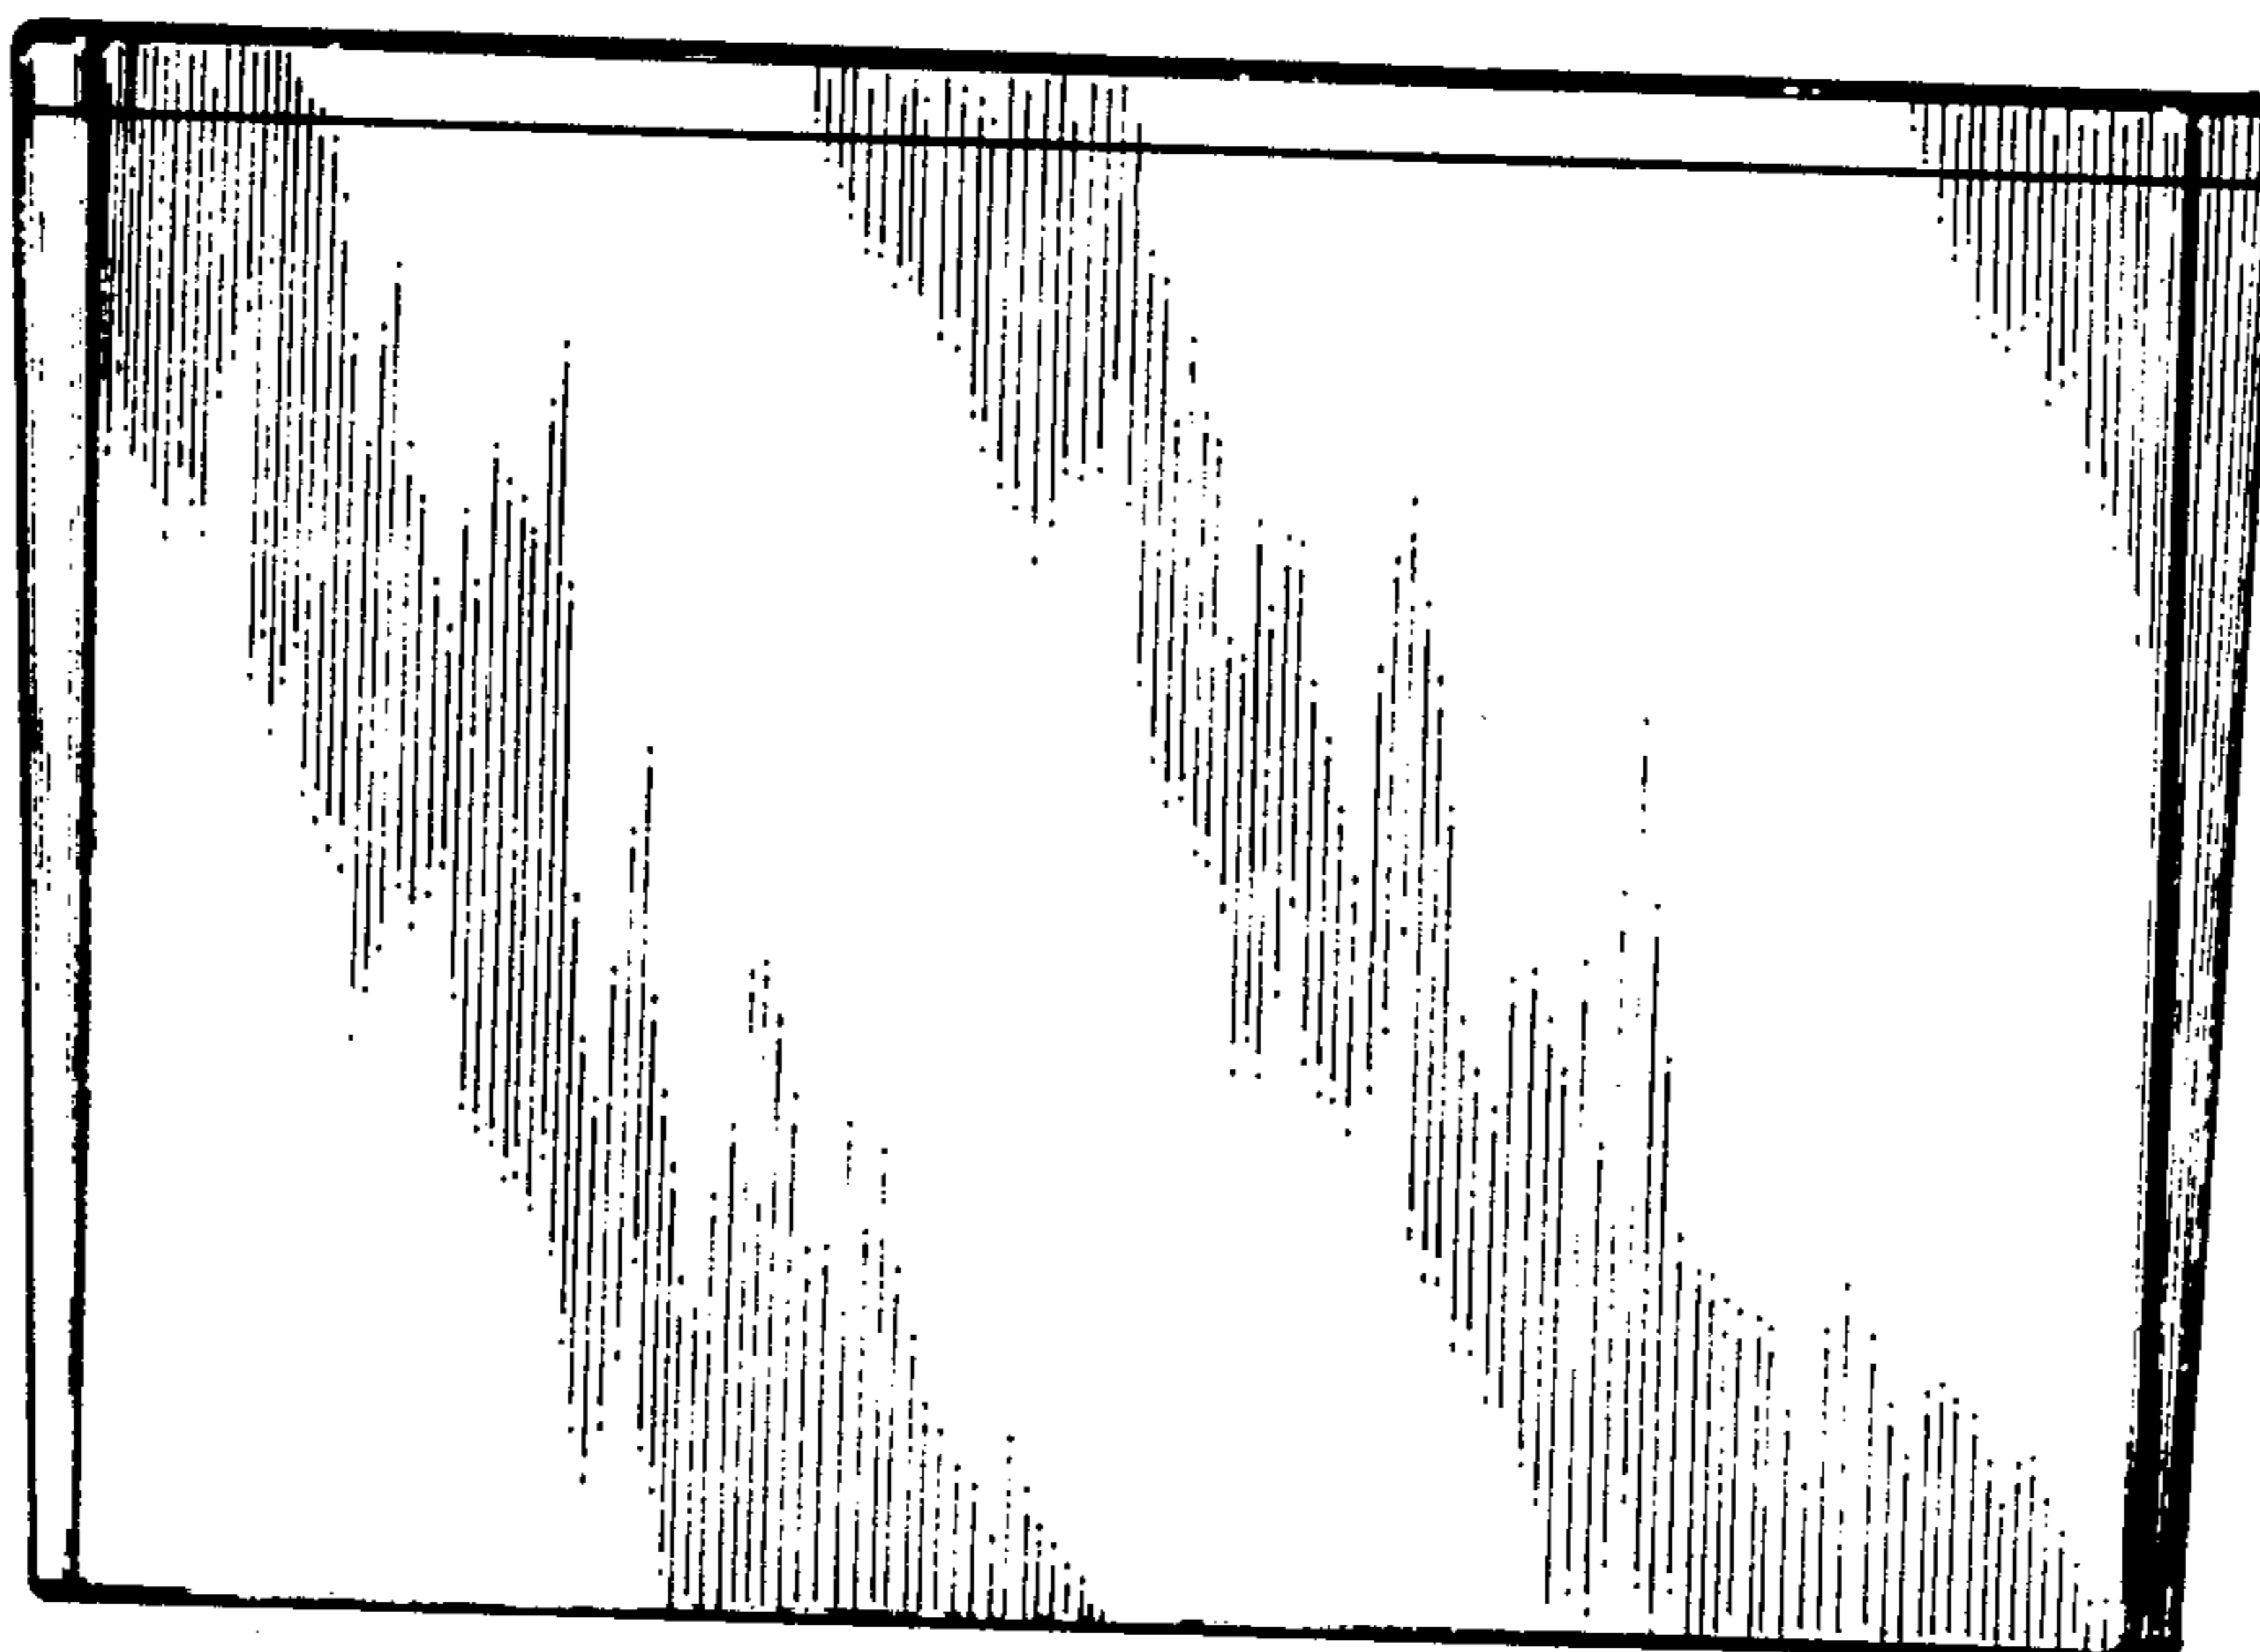


FIGURE 6.