

[54] SPHYGMOMANOMETER

[75] Inventor: Tadashi Miyazawa, 131-4 Ohkido-cho, Chiba-shi, Chiba-ken, Japan

[73] Assignee: Kabushiki Kaisha Brethren Shoji, Japan

[**] Term: 14 Years

[21] Appl. No.: 826,665

[22] Filed: Aug. 22, 1977

[30] Foreign Application Priority Data

Dec. 1, 1976 [JP] Japan 51-46660

[51] Int. Cl. D24-02

[52] U.S. Cl. D24/21; 128/2.05 G

[58] Field of Search D24/21; 128/2.05 G, 128/2.05 N; 137/556; 73/389, 402

[56] References Cited

U.S. PATENT DOCUMENTS

D. 215,983	11/1969	Bonsiepe	D24/21
3,954,099	5/1976	Raczkowski et al.	128/2.05 G
4,010,739	3/1977	Leach	128/2.05 G
4,050,311	9/1977	Leach	128/2.05 G X



Primary Examiner—Bernard Ansher
Attorney, Agent, or Firm—Harold D. Steinberg

[57] CLAIM

The ornamental design for a sphygmomanometer, as shown and described.

DESCRIPTION

FIG. 1 is a top plan view of a blood pressure measurement unit illustrating my new design; FIG. 2 is a front elevation of the unit of FIG. 1; FIG. 3 is a side elevation showing the unit as it appears from the right of FIG. 2; FIG. 4 is a rear elevation showing the unit as it appears at the rear of FIG. 2; and FIG. 5 is a bottom plan view illustrating the unit as it appears from the bottom of FIG. 2.

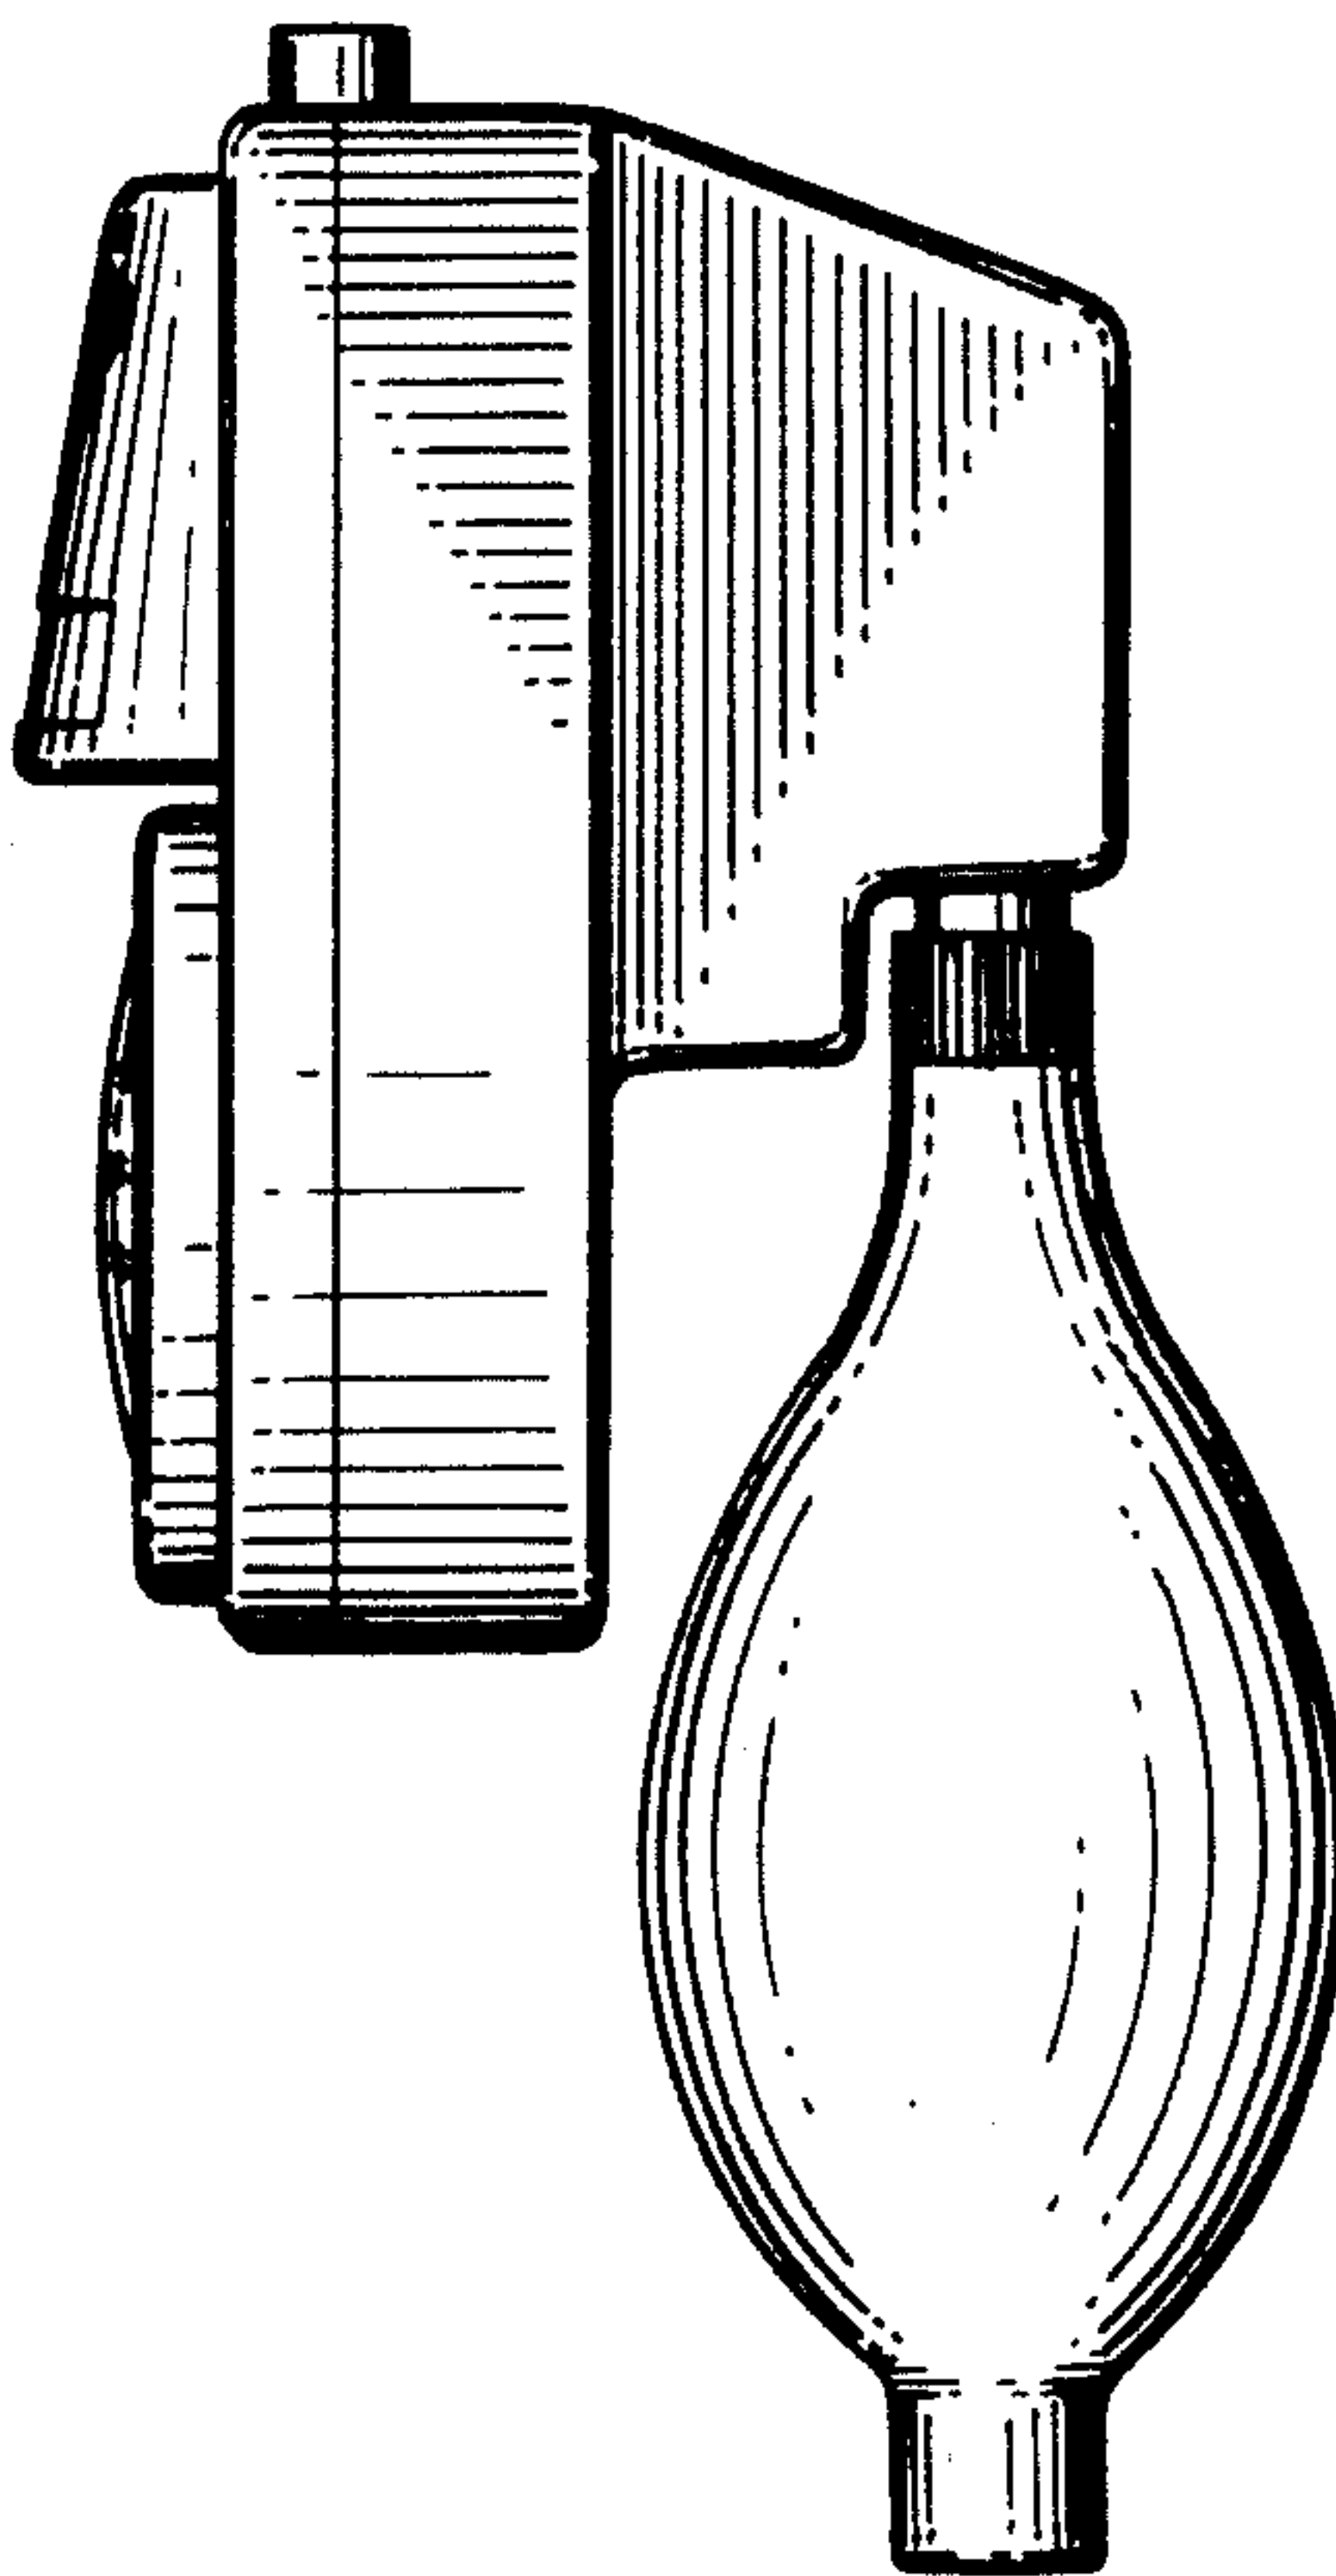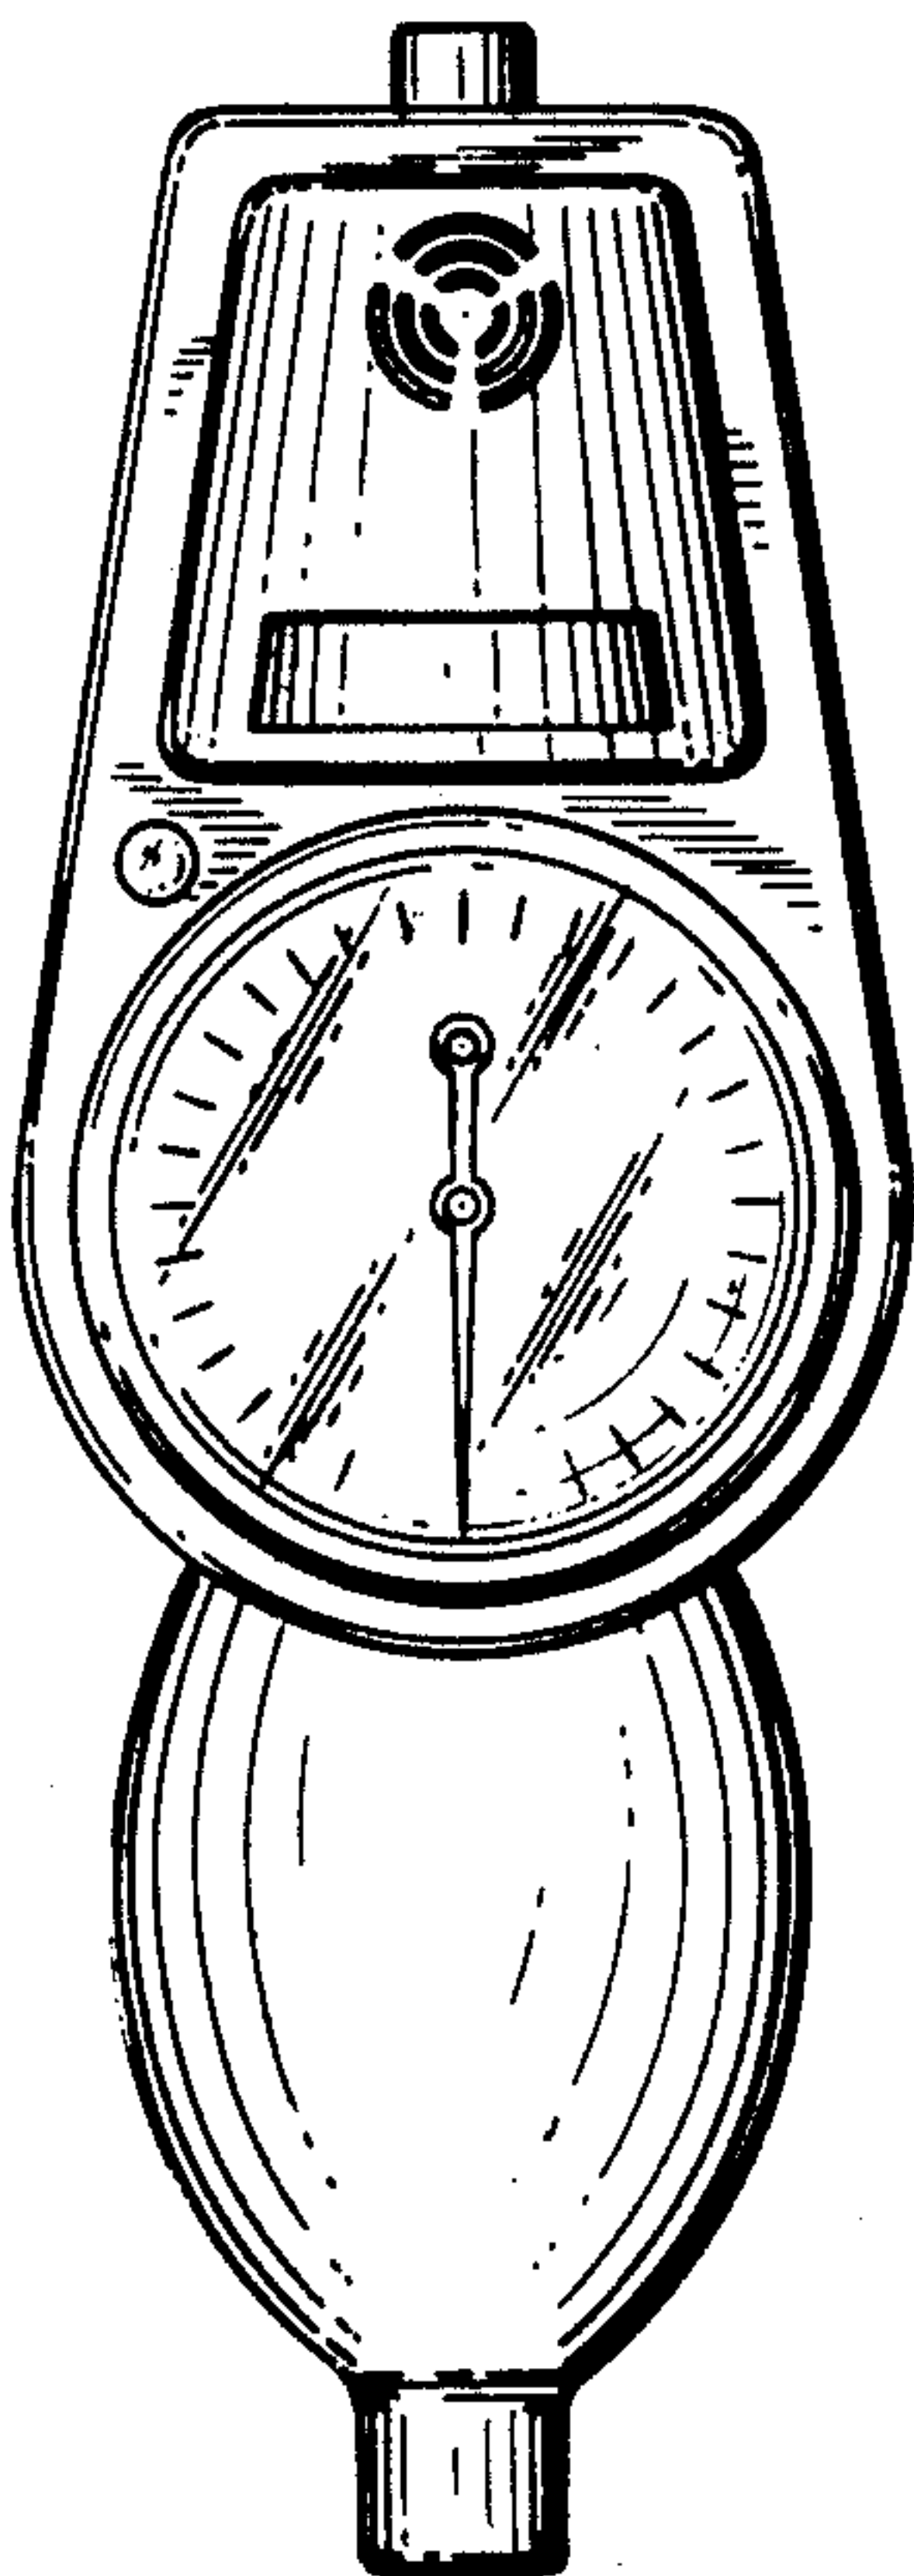

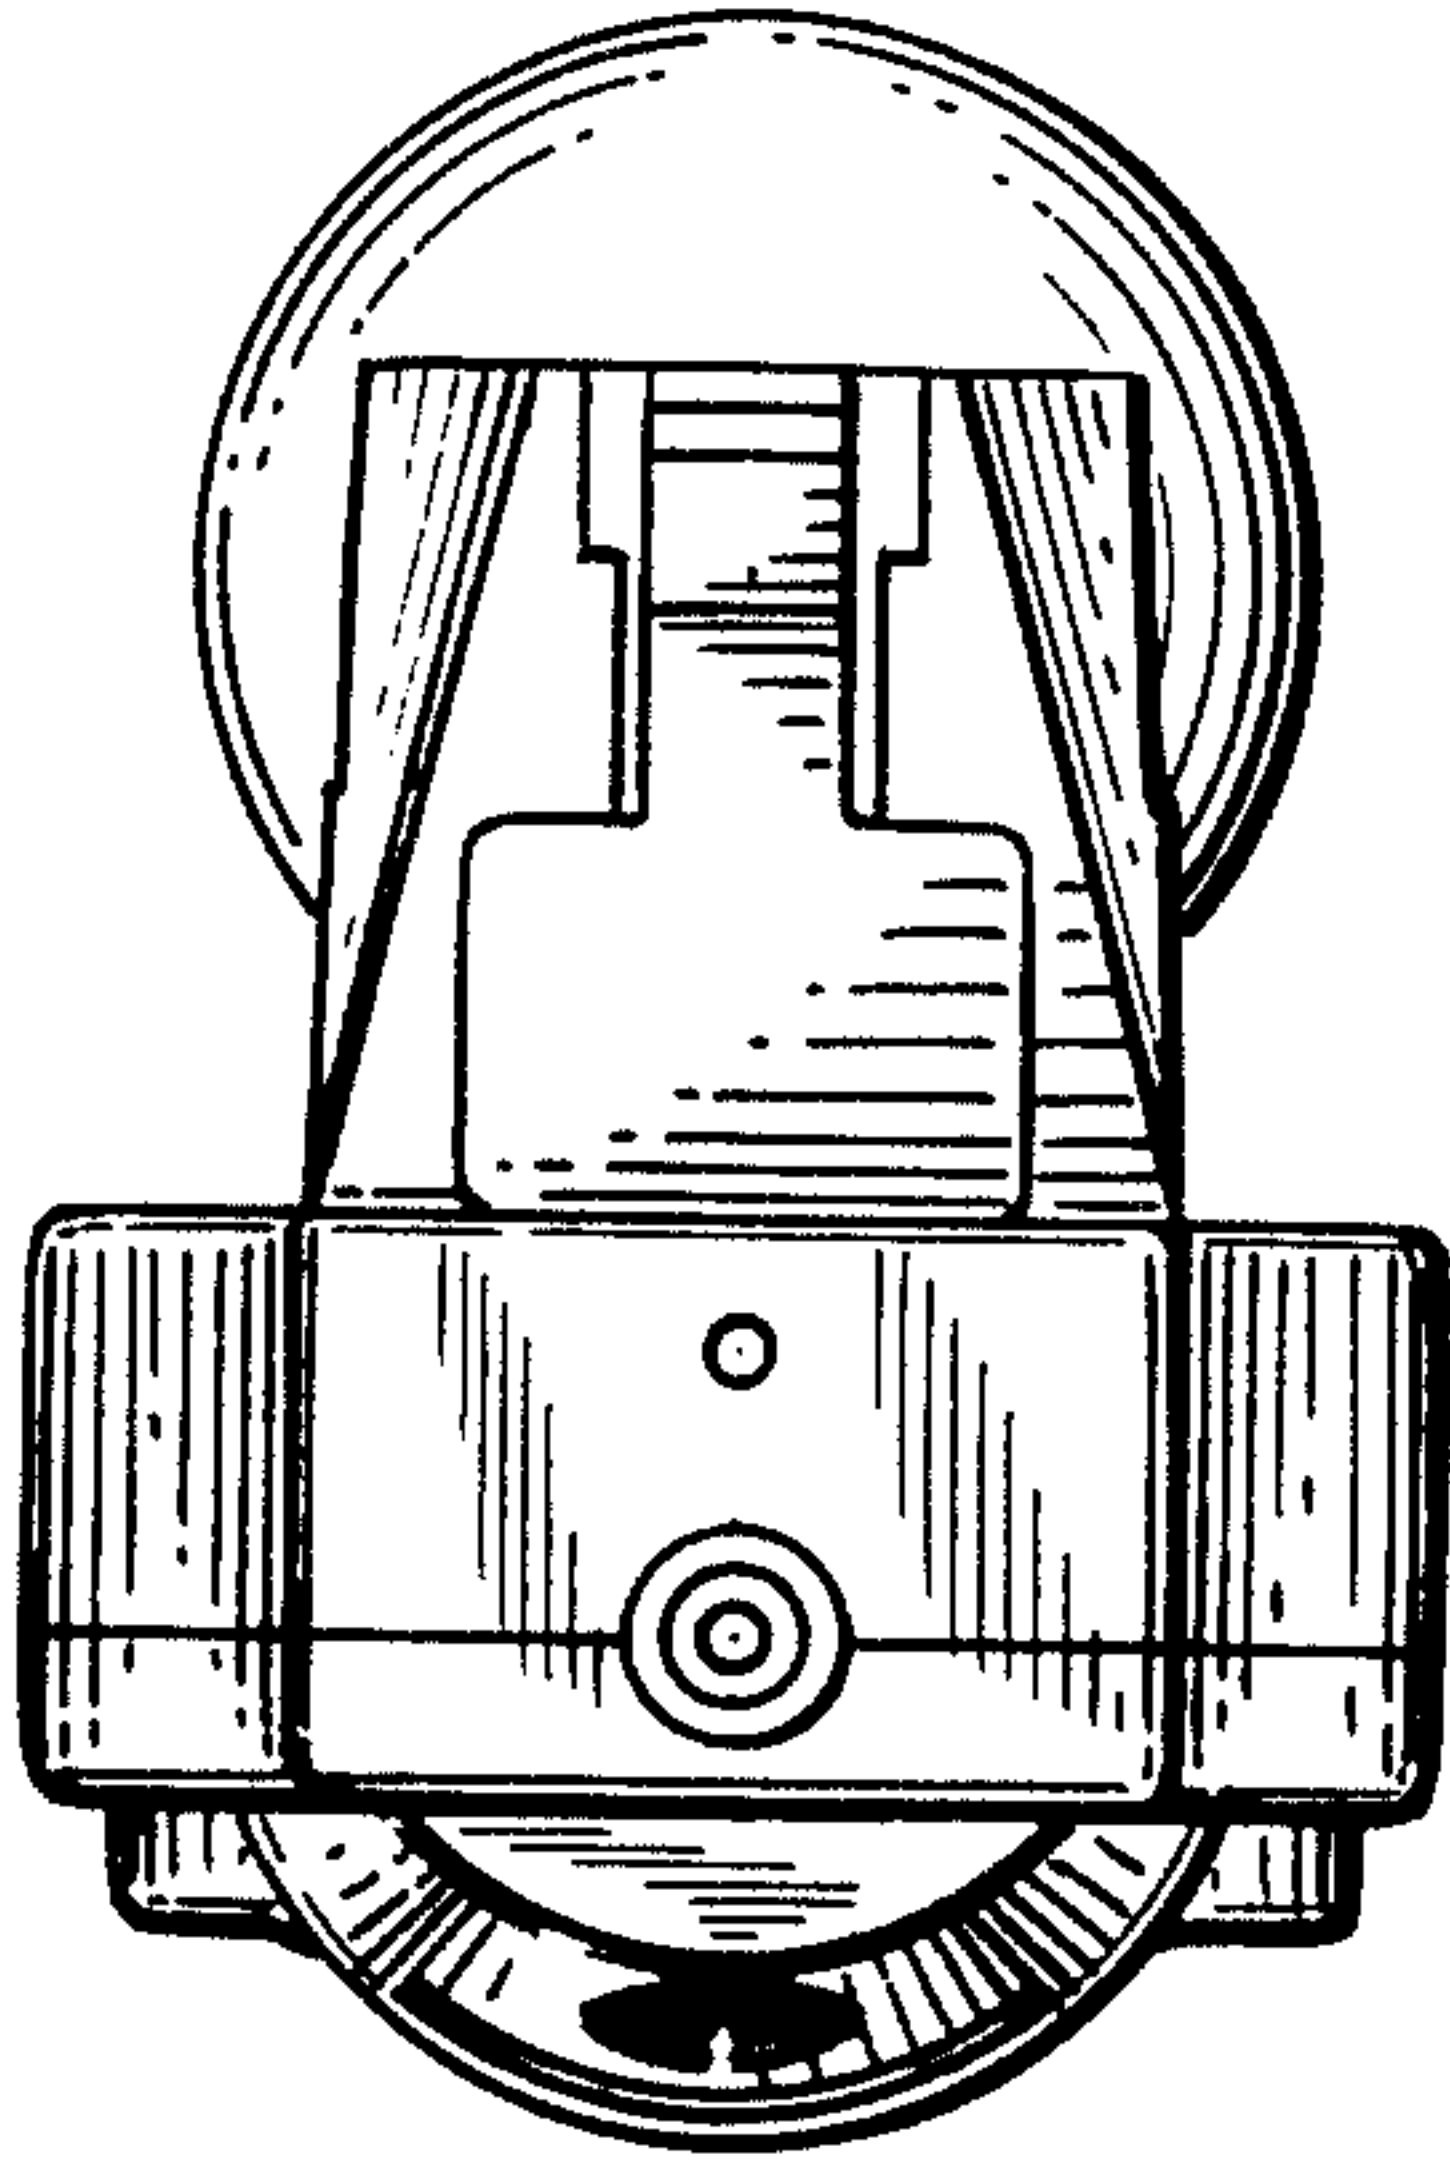


FIG. 1

FIG. 2

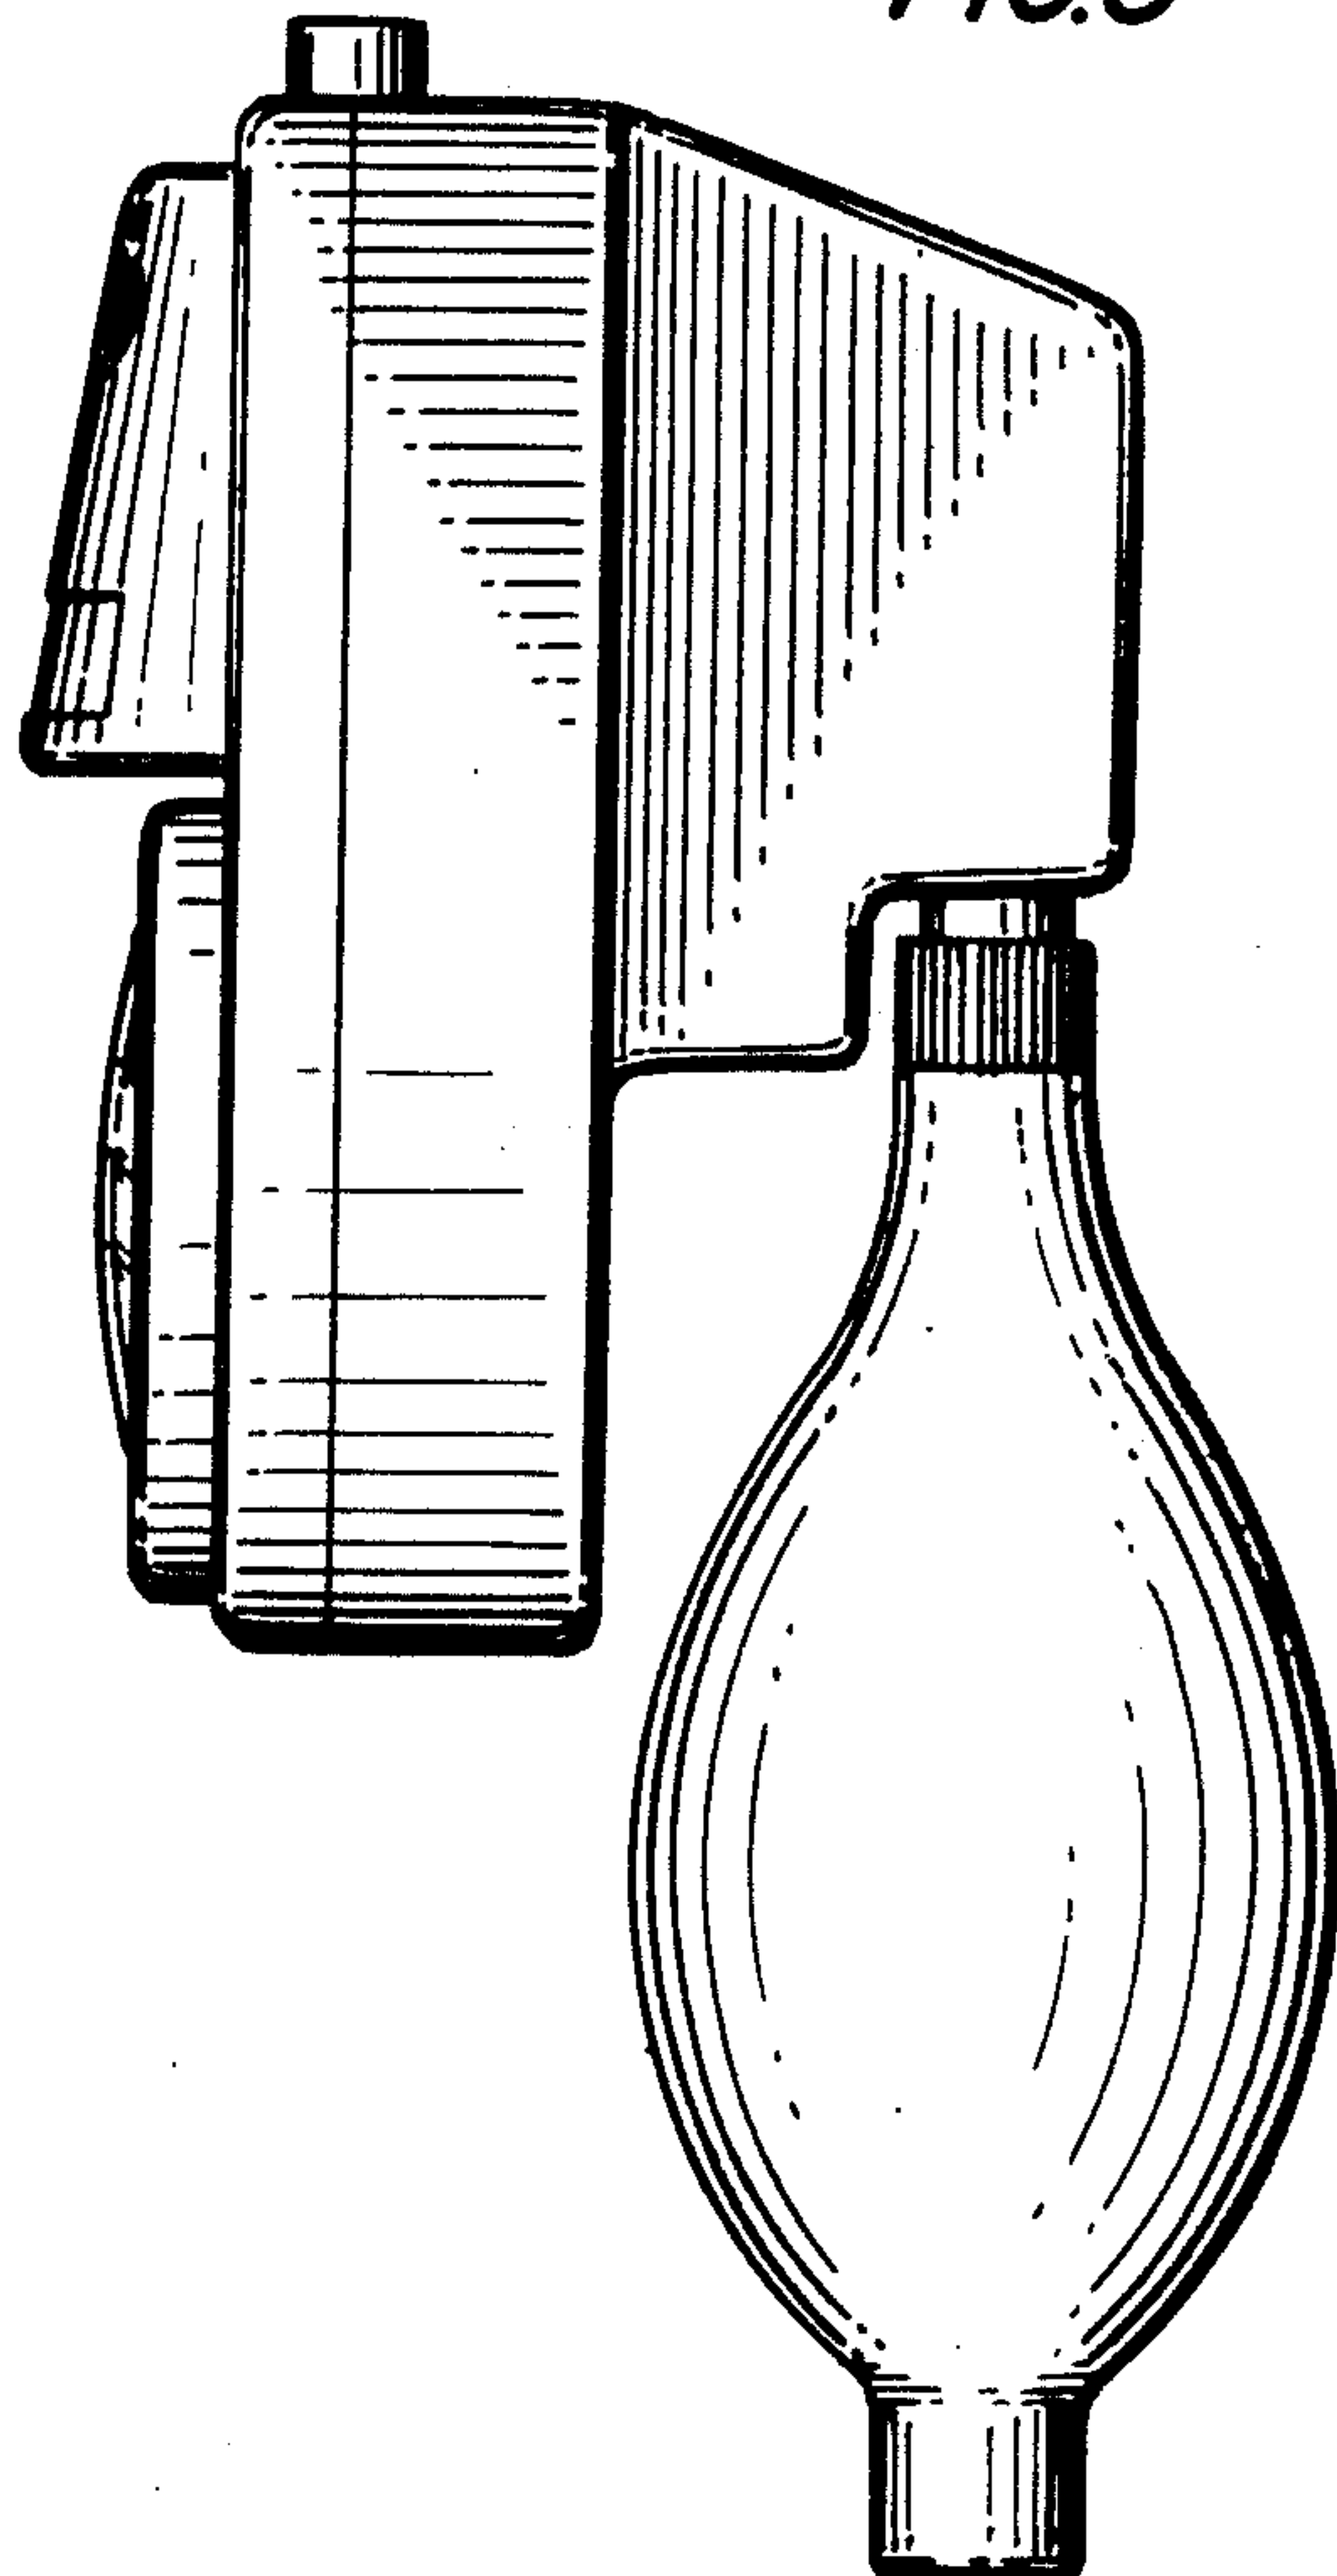
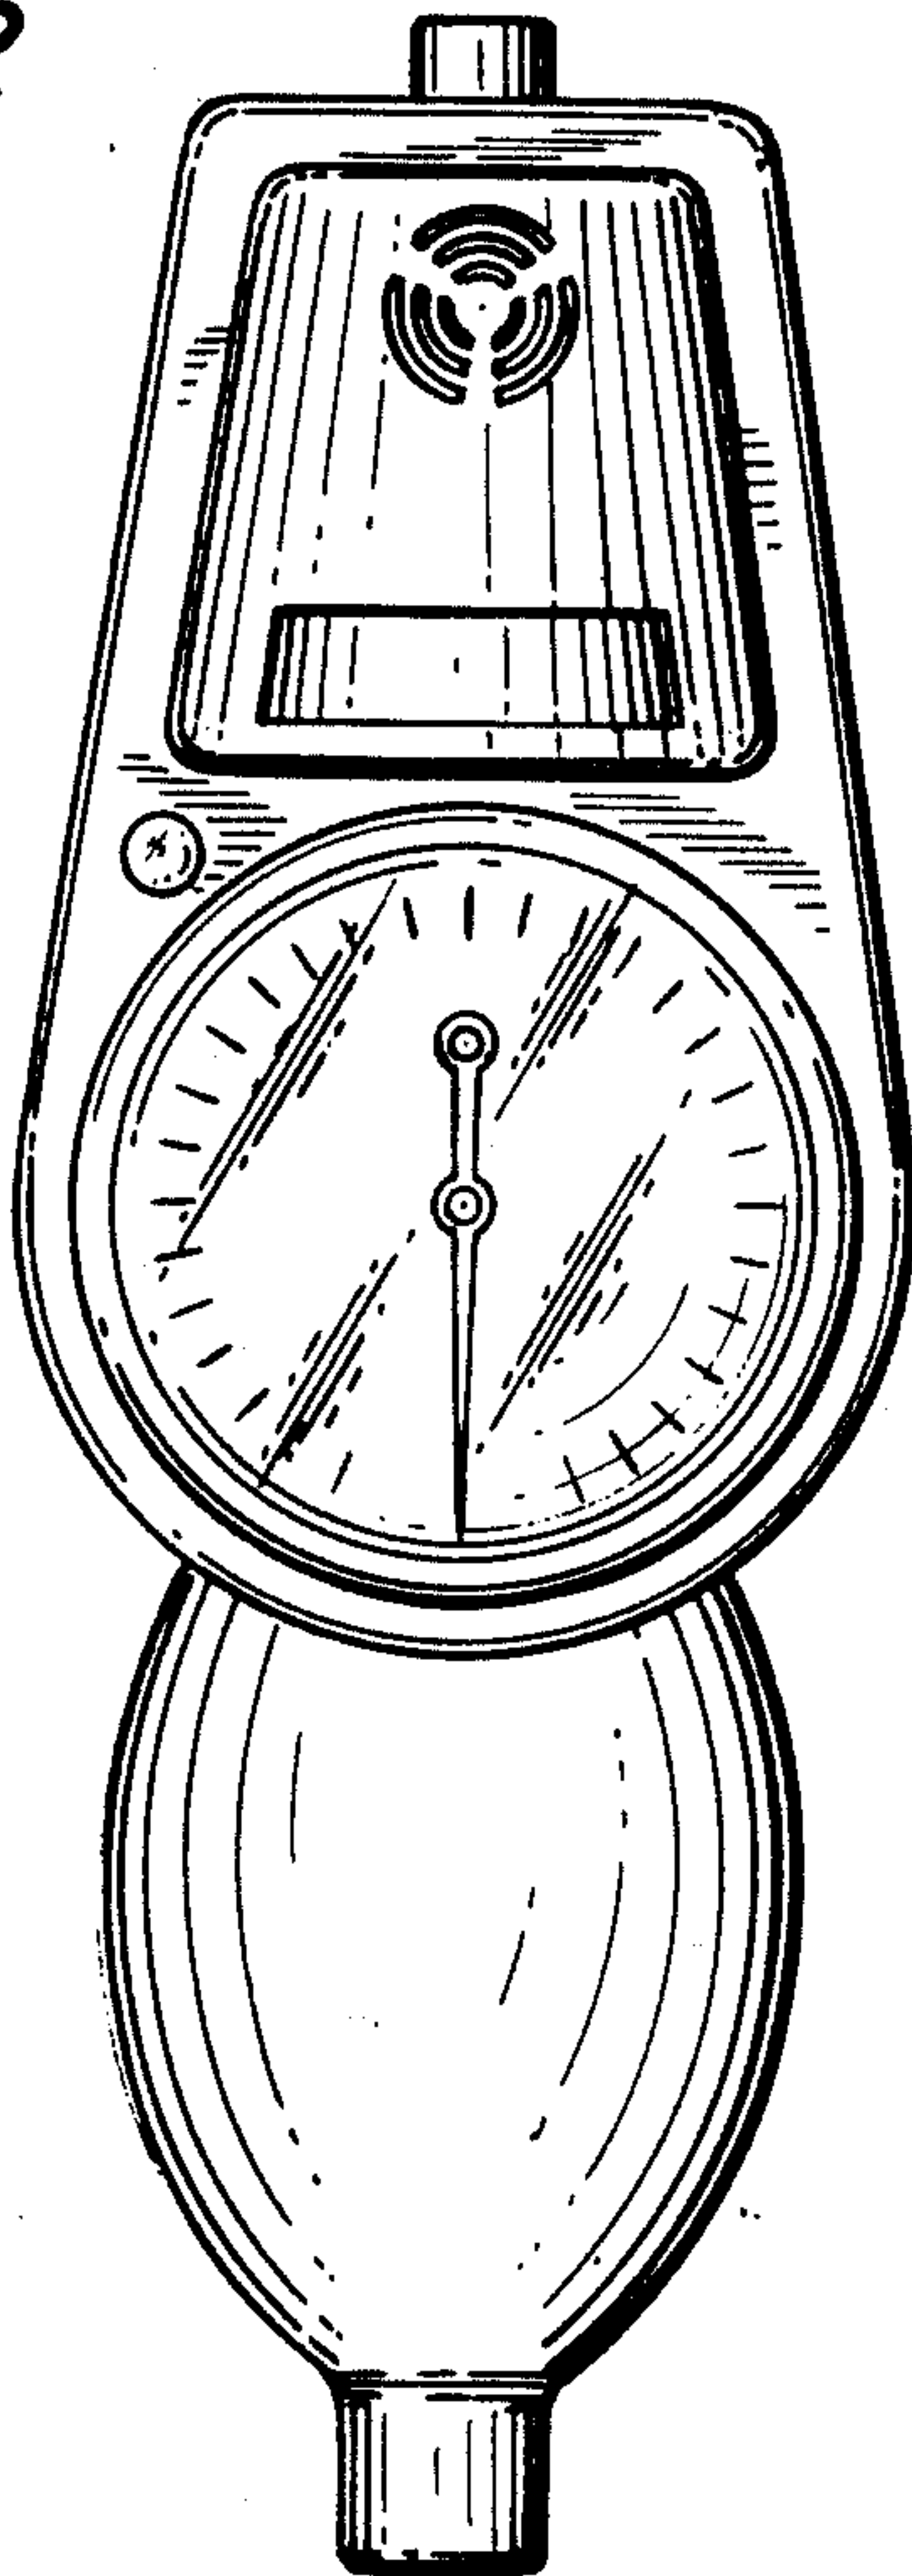


FIG. 3

FIG. 4


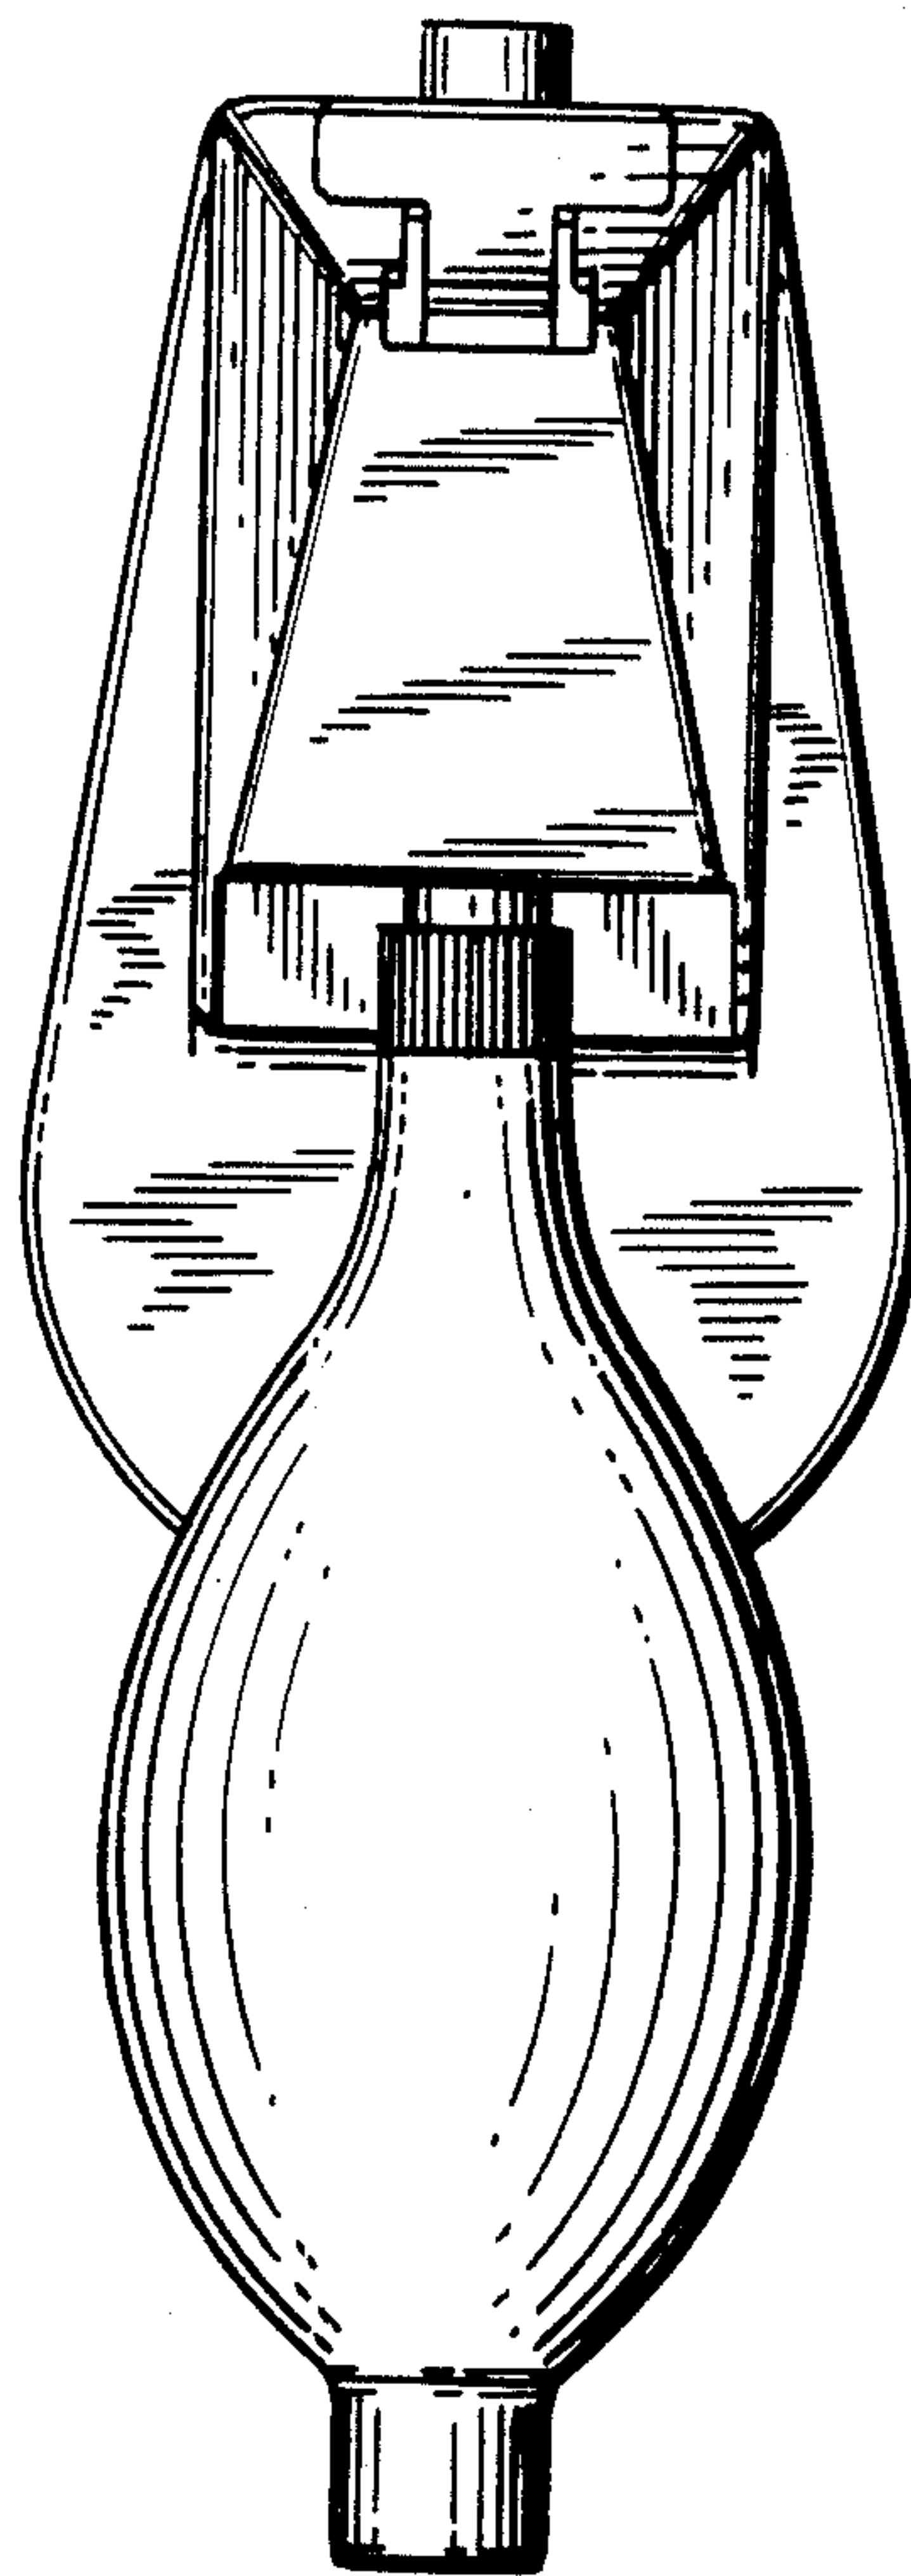


FIG. 5

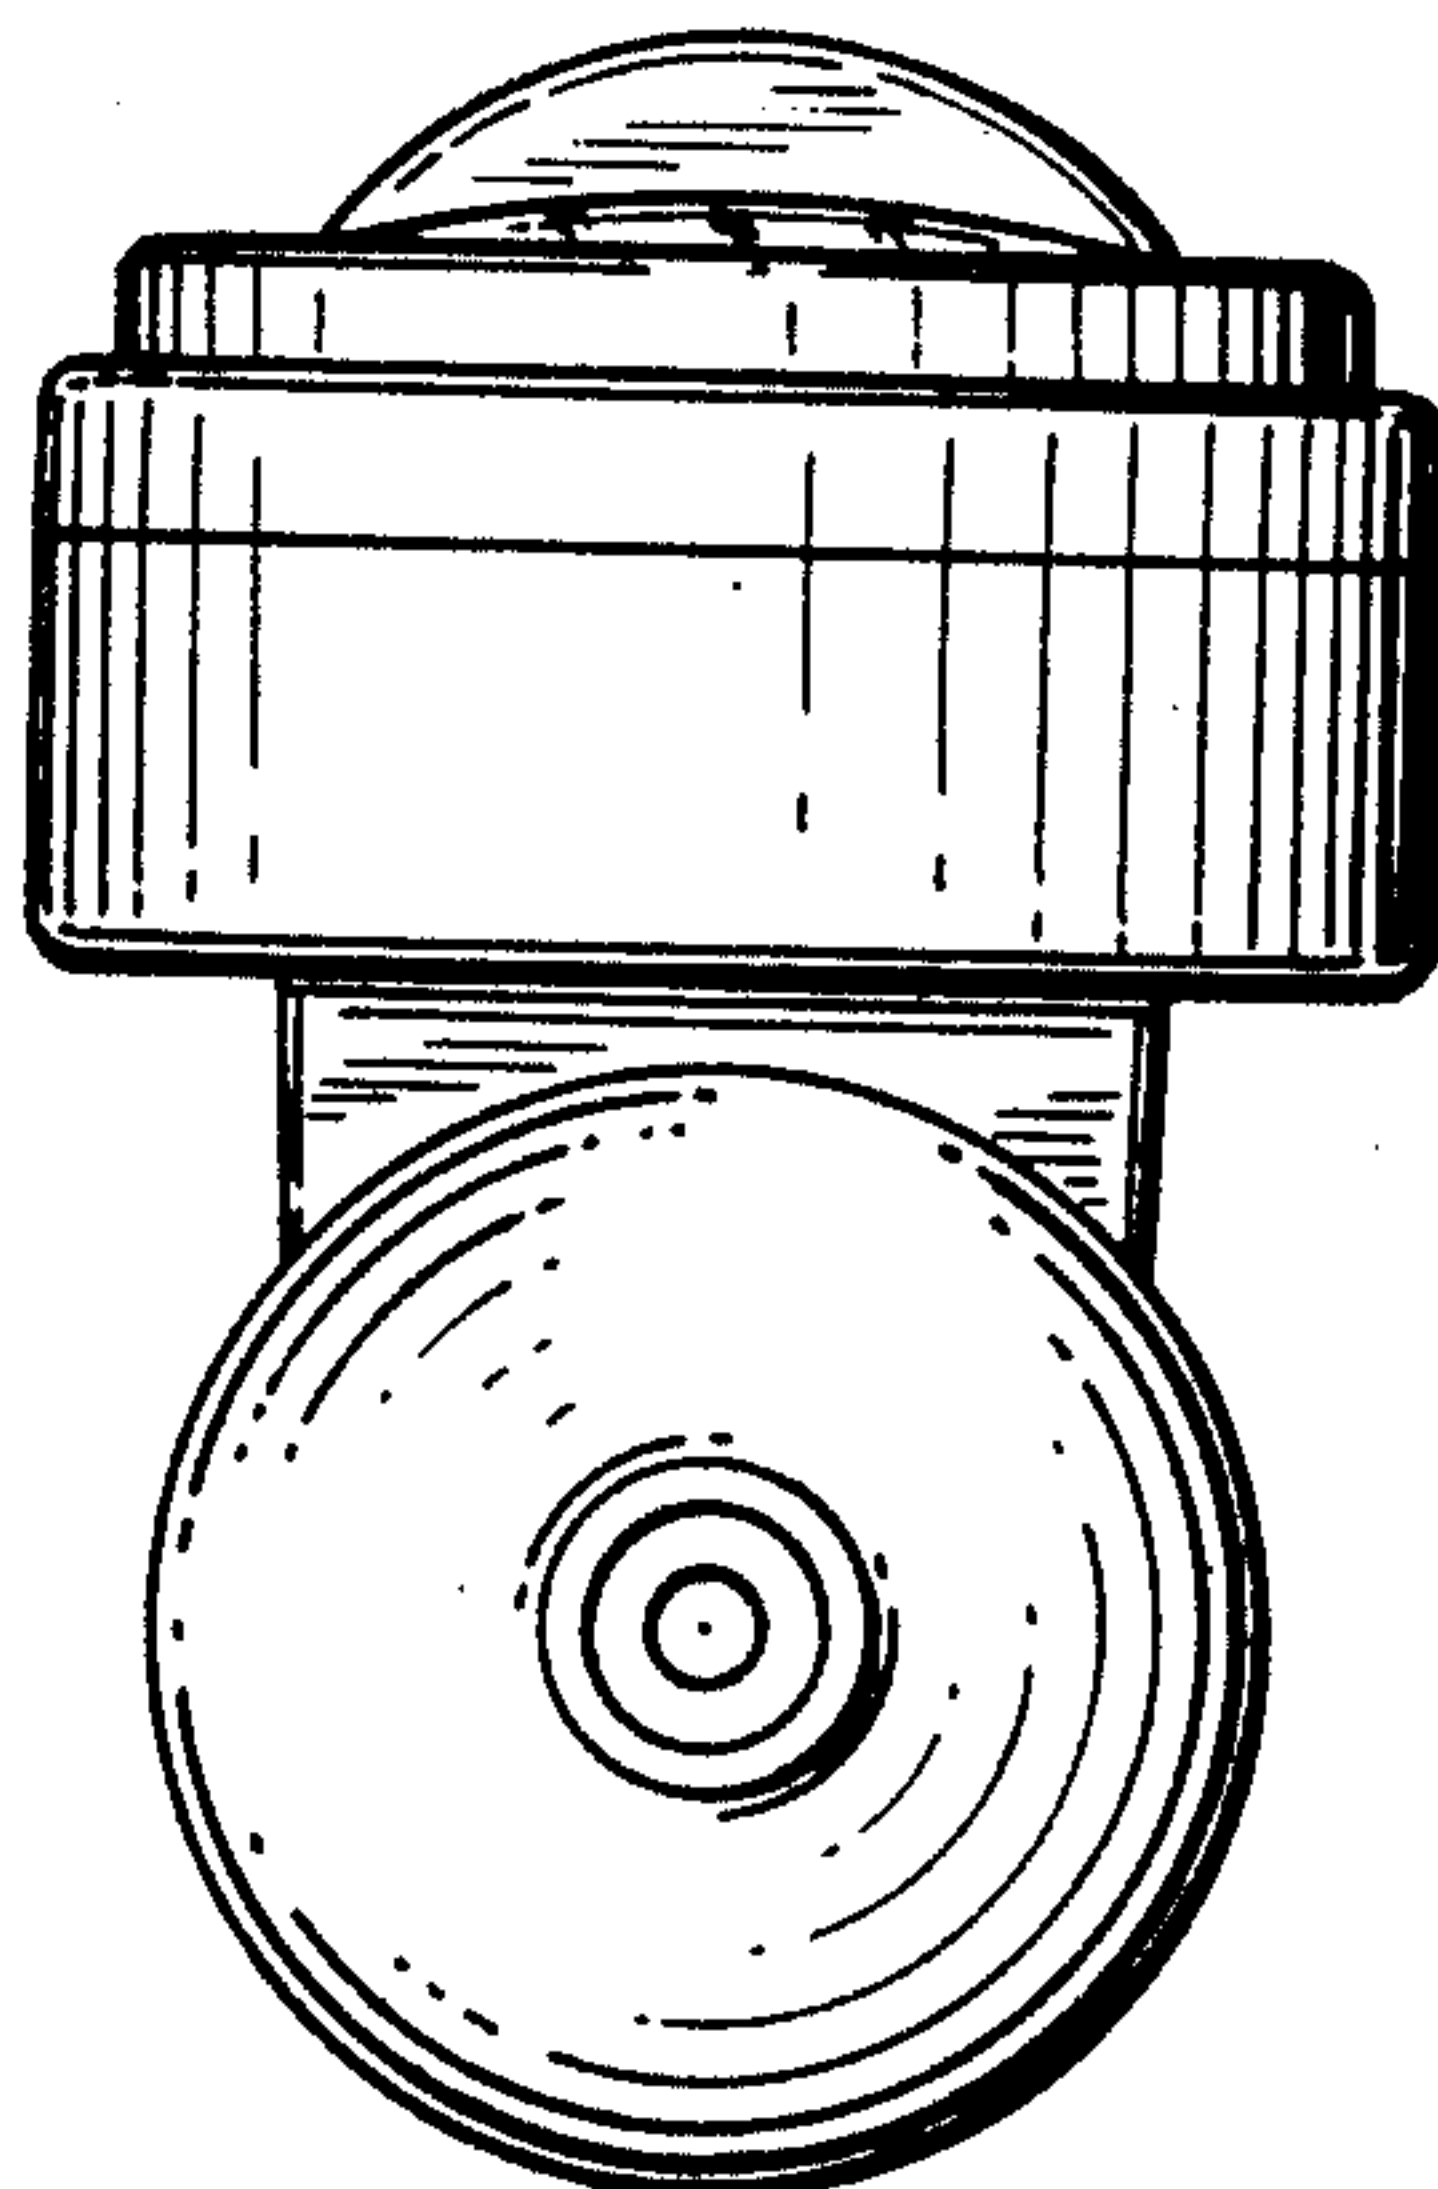

UNITED STATES PATENT AND TRADEMARK OFFICE
CERTIFICATE OF CORRECTION

PATENT NO. : Des.250,128
DATED : October 31, 1978
INVENTOR(S) : Tadashi Miyazawa

It is certified that error appears in the above-identified patent and that said Letters Patent are hereby corrected as shown below:

[73] Assignee: KABUSHIKI KAISHA BRETHERN SHOJI, Japan, and
NIHON SEIMITSU SOKKI KABUSHIKI KAISHA, Japan

Signed and Sealed this

Twenty-second Day of May 1979

[SEAL]

Attest:

RUTH C. MASON
Attesting Officer

DONALD W. BANNER
Commissioner of Patents and Trademarks