

[54] **SELF-ATTACHING PROBE FOR USE IN PHOTOELECTRIC MONITORING OF BODY EXTREMITIES**

[75] Inventor: **Albert K. Bond**, Burlington, Mass.

[73] Assignee: **Hewlett-Packard Company**, Palo Alto, Calif.

[\*\*] Term: **14 Years**

[21] Appl. No.: **706,876**

[22] Filed: **Jul. 19, 1976**

[51] Int. Cl. .... **D24—02**

[52] U.S. Cl. .... **D24/29**; 128/2.05 E;  
128/2 L; 128/2.05 P; D24/17

[58] Field of Search ..... 128/2 L, 2.05 V, 2.05 P,  
128/2 E; D24/29, 17, 99, 23

[56] **References Cited**

**U.S. PATENT DOCUMENTS**

3,810,460	5/1974	Van Nie .....	128/2 L X
3,815,583	6/1974	Scheidt .....	128/2.05 P
3,920,004	11/1975	Nakayama .....	128/2.05 V X


*Primary Examiner*—Bernard Ansher  
*Attorney, Agent, or Firm*—David A. Boone

[57] **CLAIM**

The ornamental design for a self-attaching probe for use in photoelectric monitoring of body extremities, as shown and described.

**DESCRIPTION**

FIG. 1 is a top, right, front perspective view of a plethysmograph, showing my new design, the bottom left view being a mirror image of that shown; FIG. 2 is a top view thereof; and FIG. 3 is a front view thereof.

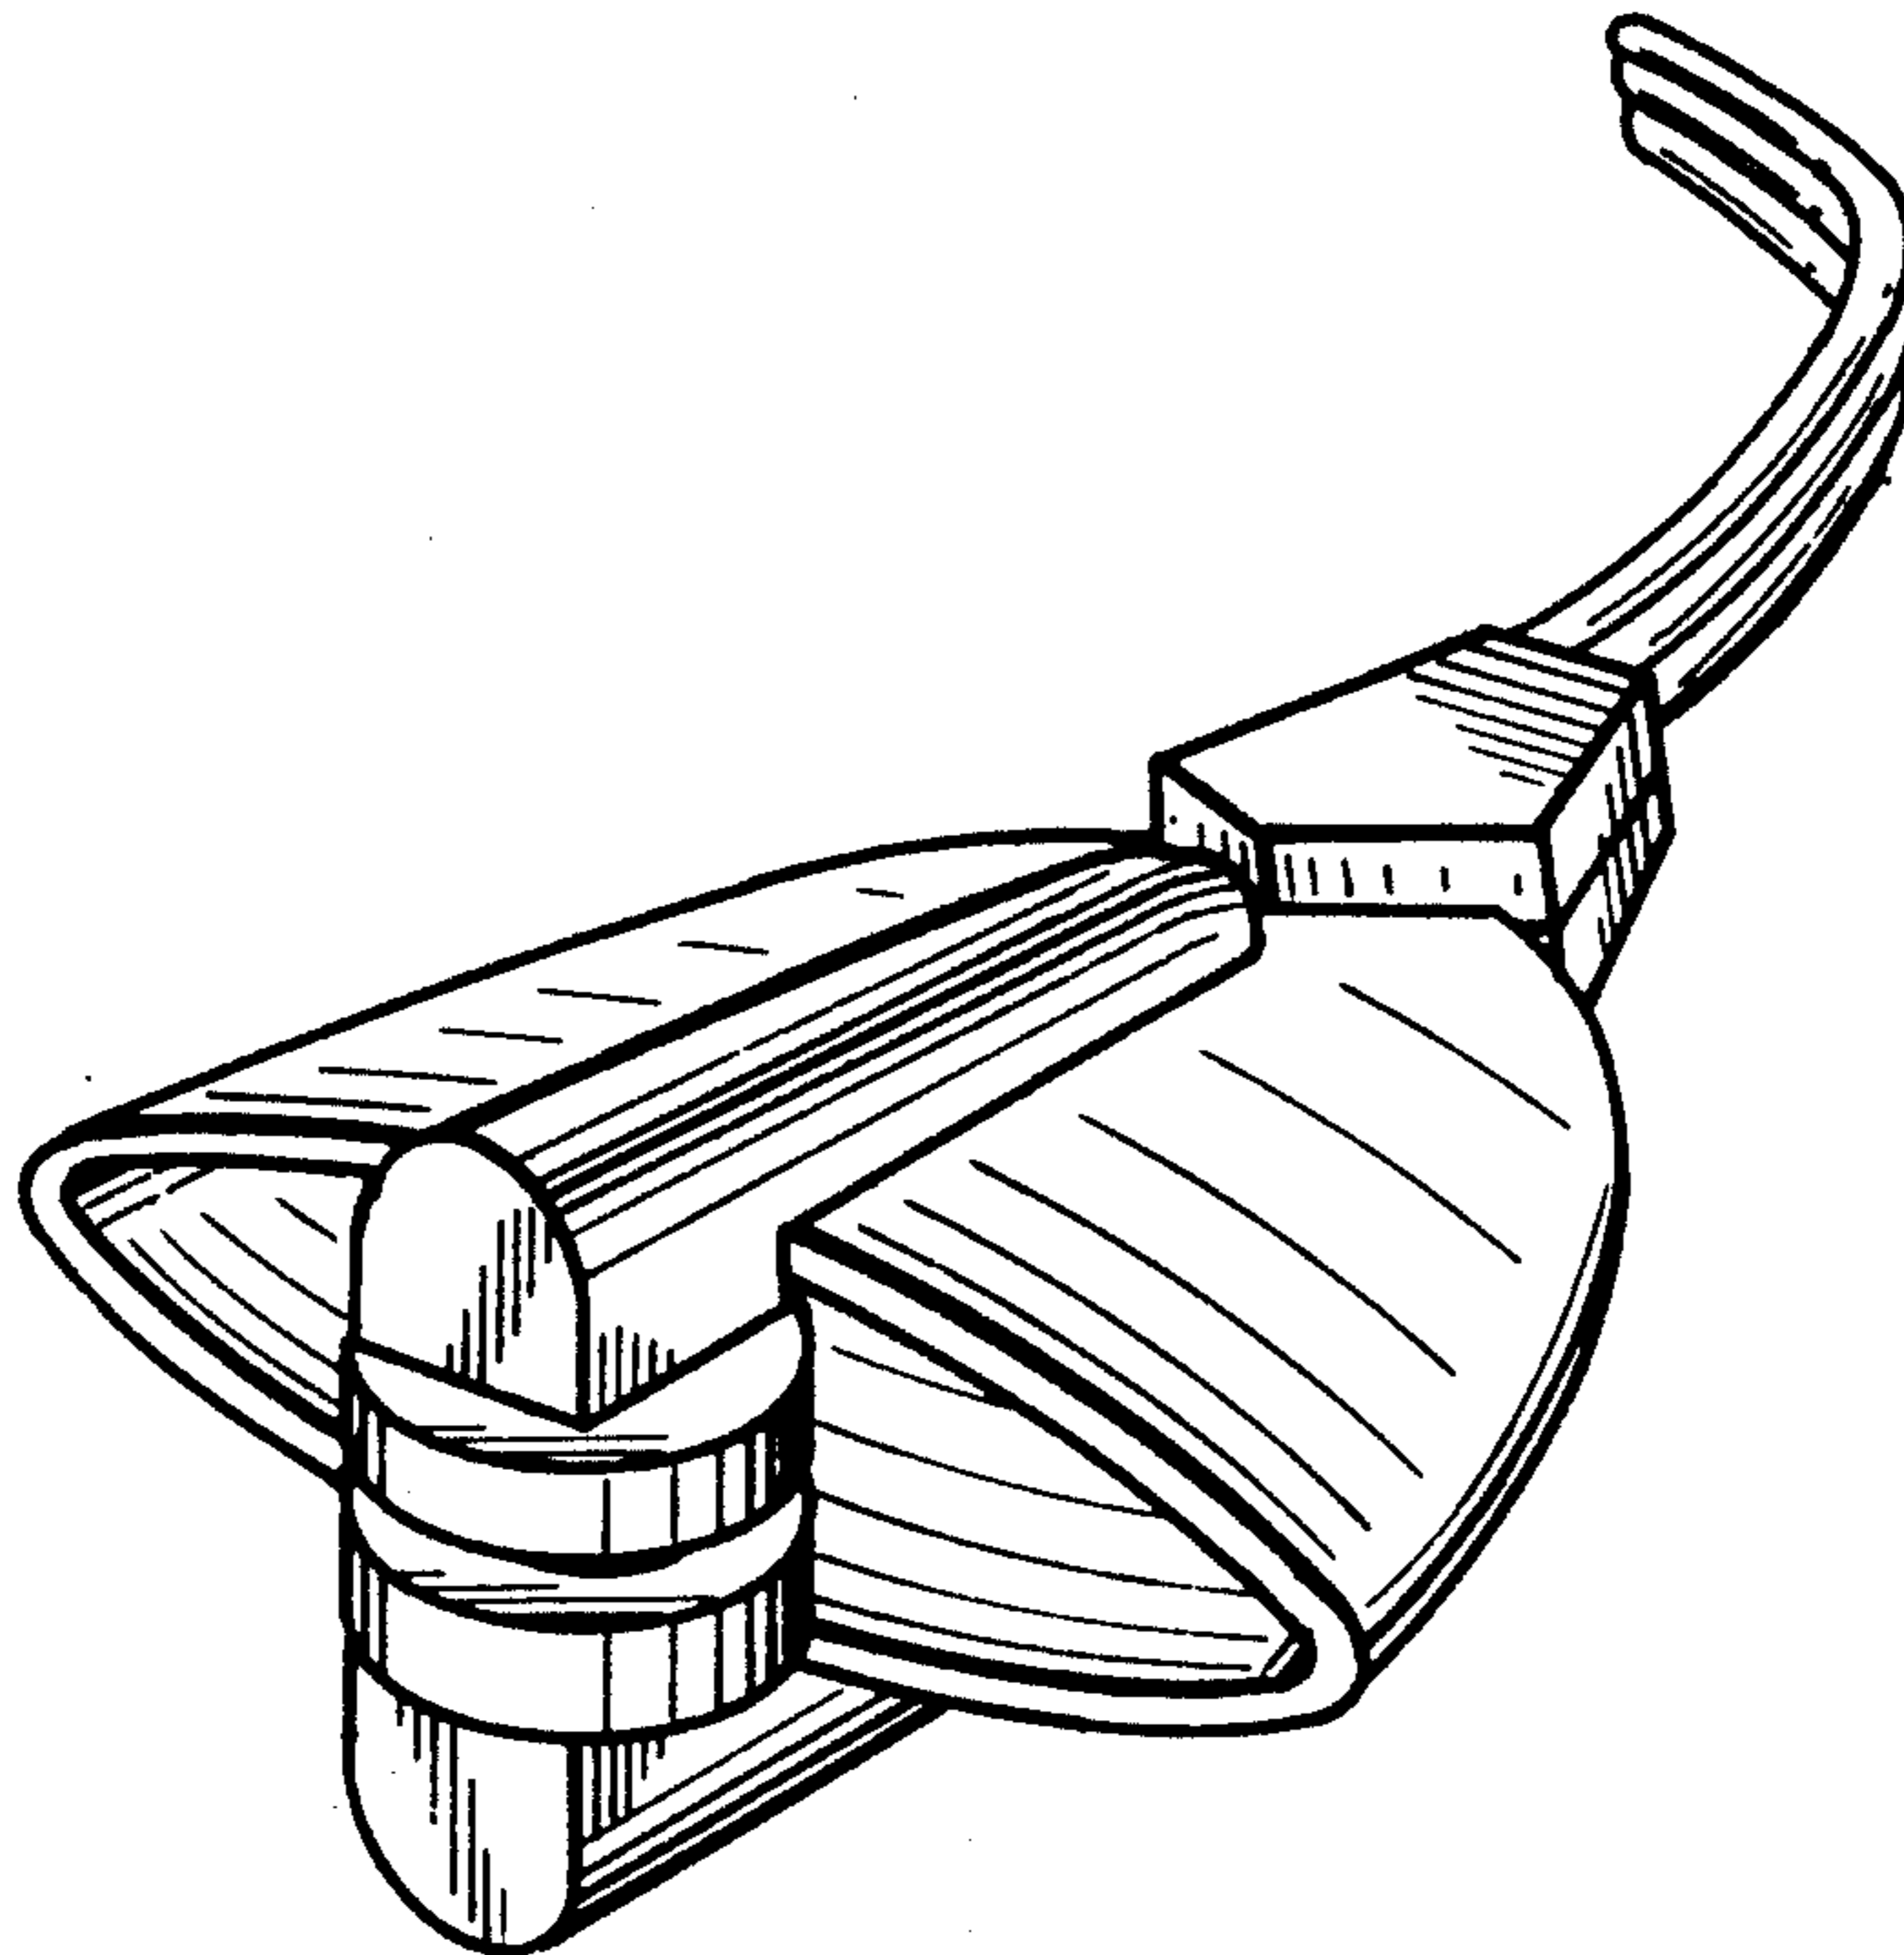

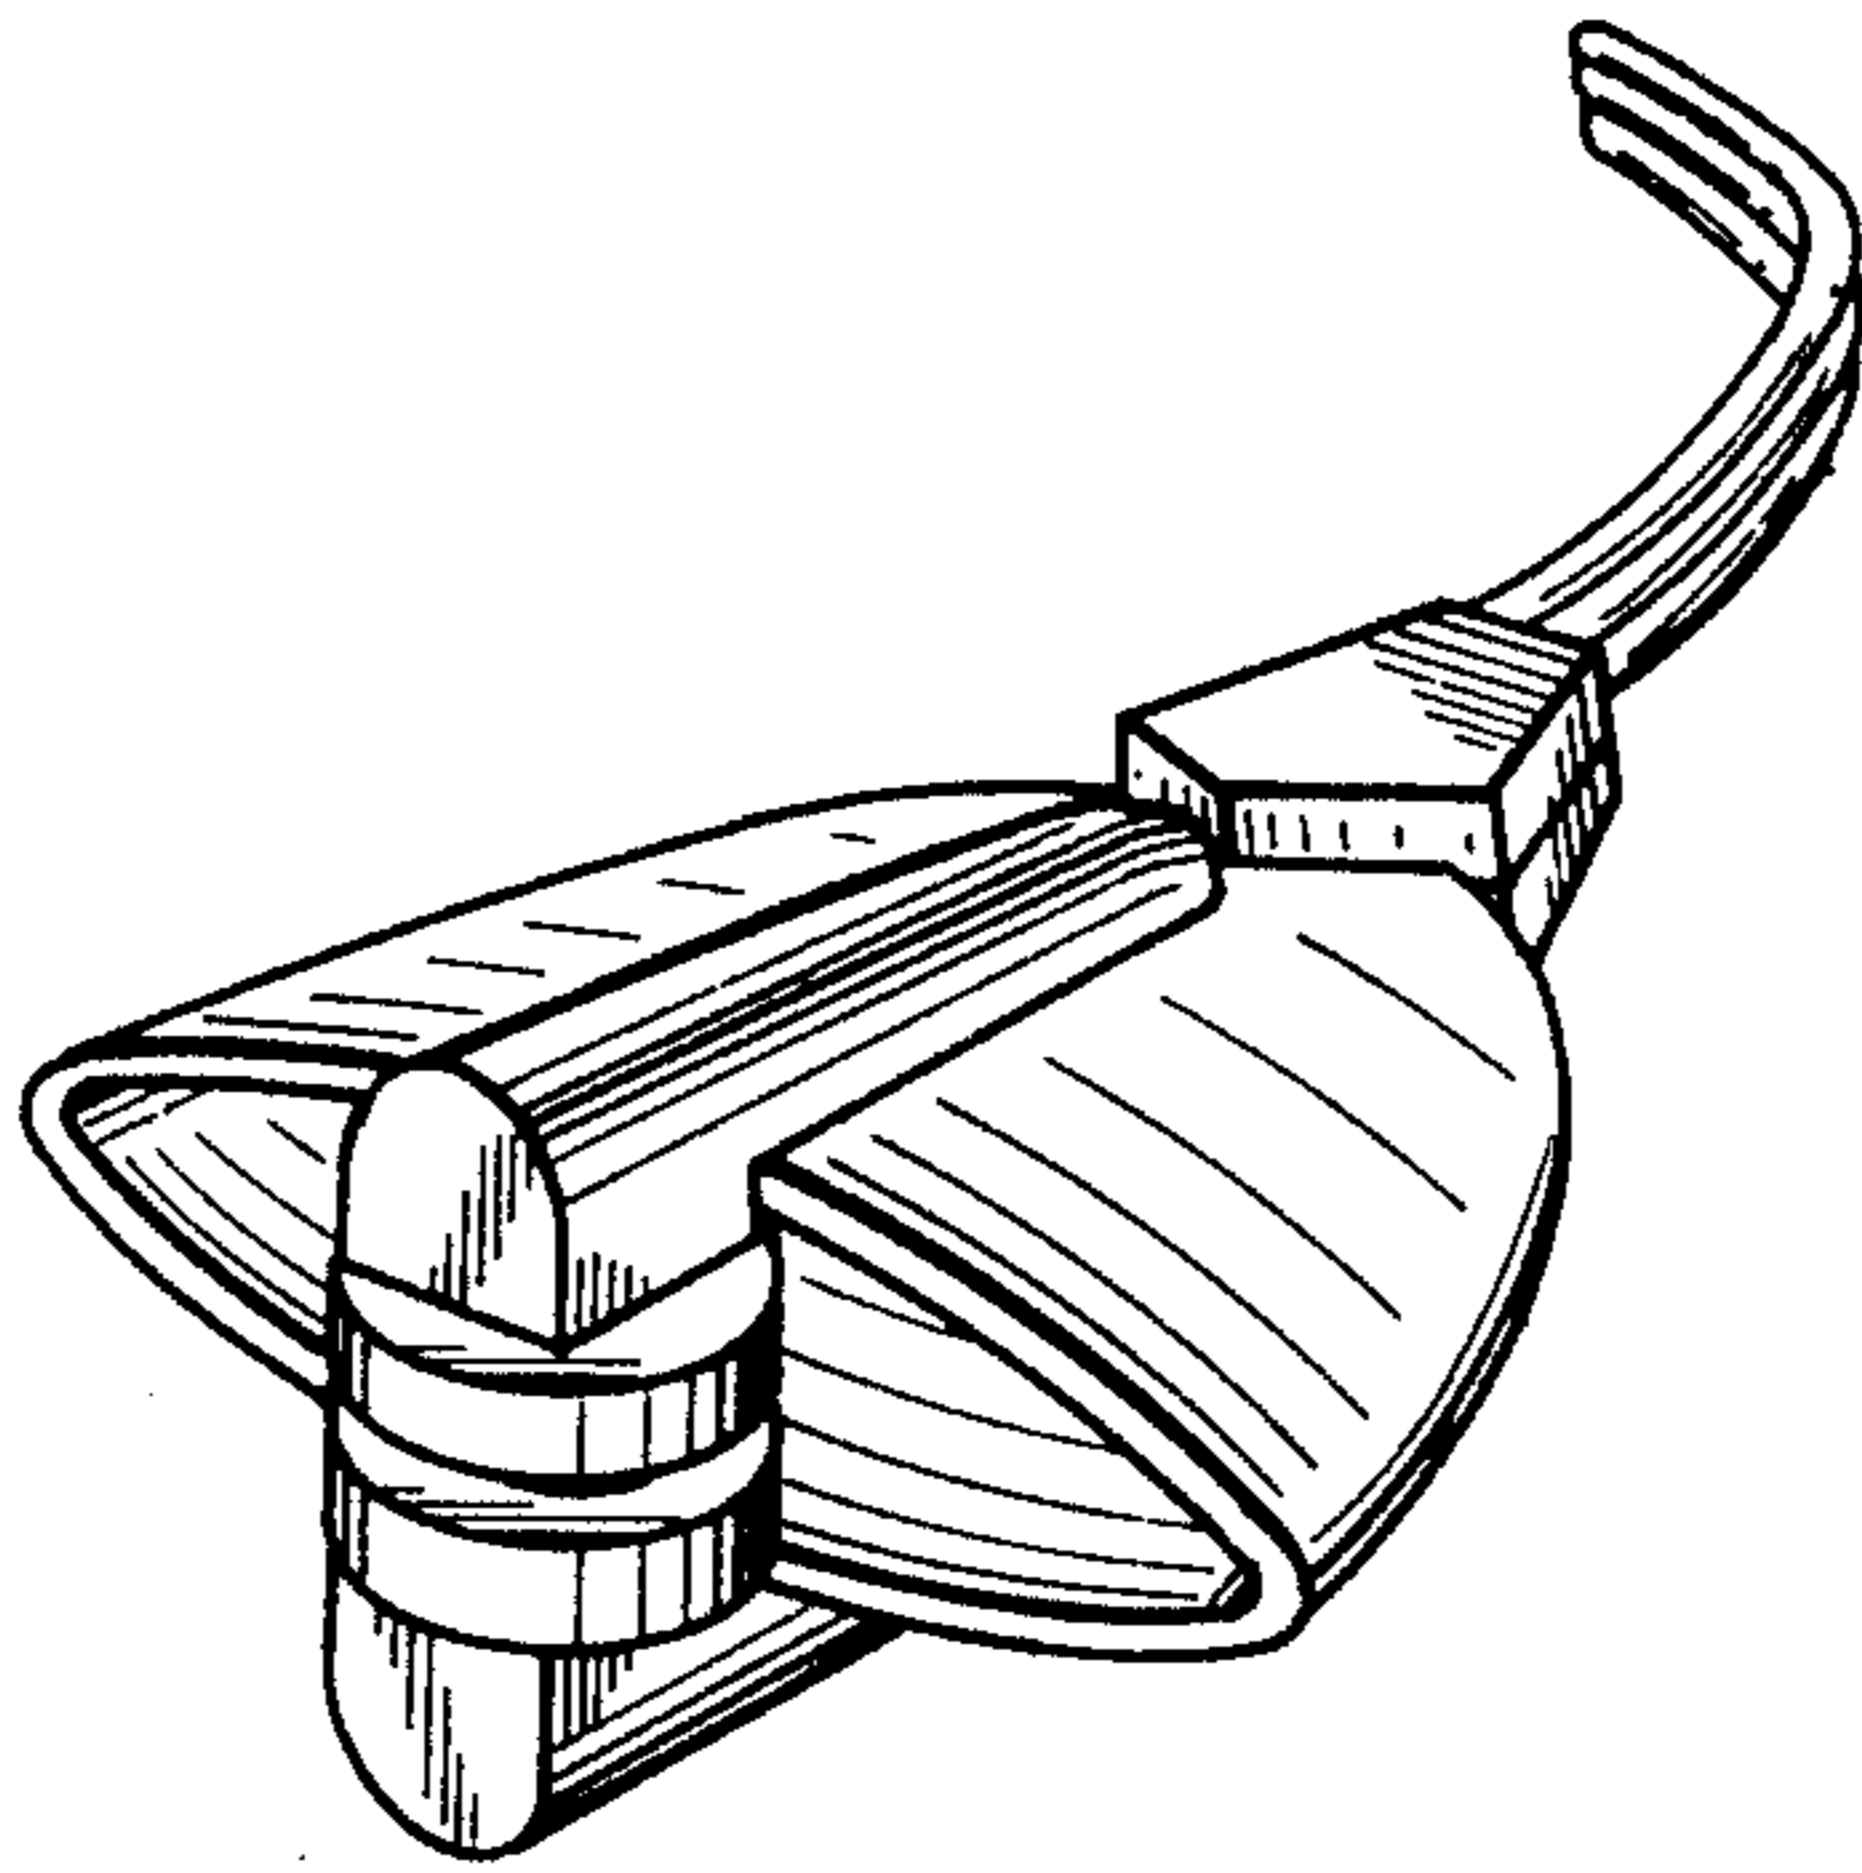


Figure 1

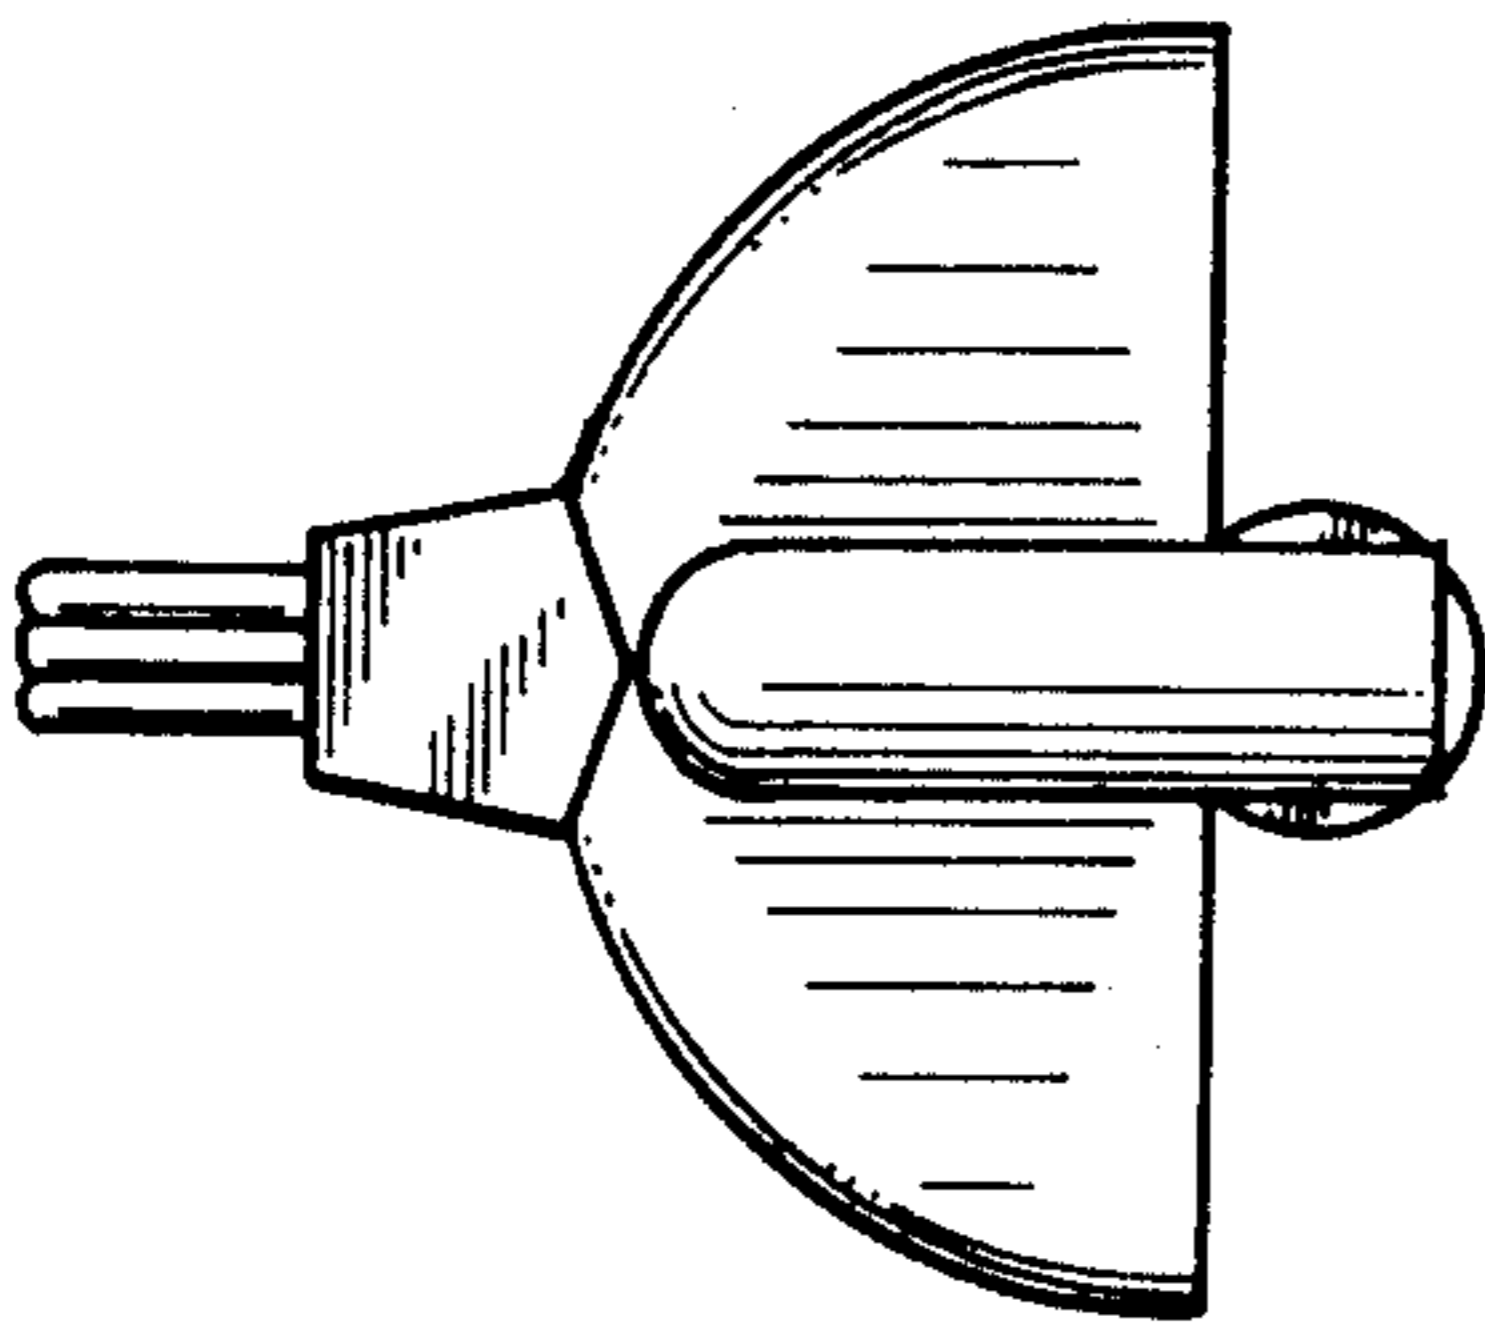


Figure 2

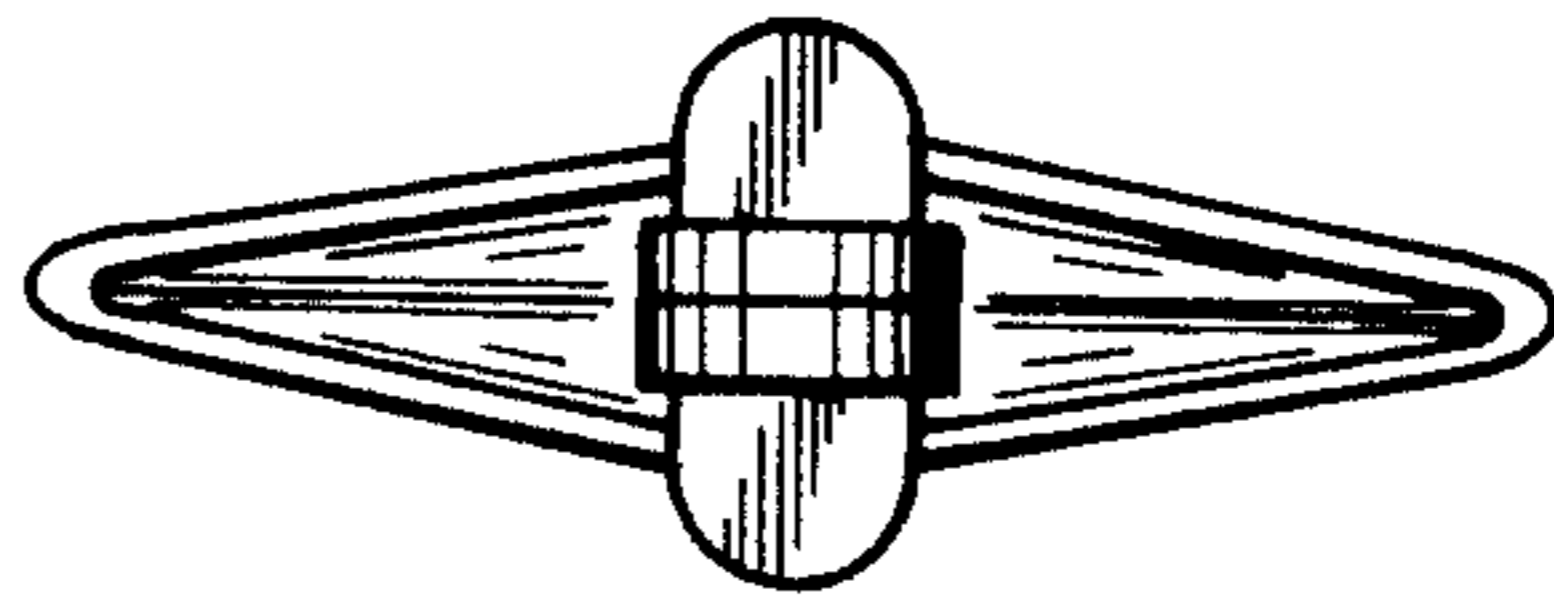


Figure 3

UNITED STATES PATENT AND TRADEMARK OFFICE  
**CERTIFICATE OF CORRECTION**

PATENT NO. : Des. 250,275  
DATED : November 14, 1978  
INVENTOR(S) : Albert K. Bond

It is certified that error appears in the above-identified patent and that said Letters Patent are hereby corrected as shown below:

Under the heading DESCRIPTION, at lines 1 and 2, "plethysmograph" should read -- self-attaching probe for use in photoelectric monitoring of body extremities --.

**Signed and Sealed this**

*First Day of May 1979*

[SEAL]

*Attest:*

**RUTH C. MASON**  
*Attesting Officer*

**DONALD W. BANNER**  
*Commissioner of Patents and Trademarks*