

[54] BIPOLAR ELECTRICAL SURGICAL GENERATOR

[75] Inventors: Ludwig A. Wettermann, Arlington Heights, Ill.; Peter H. Wettermann, Dayville, Conn.

[73] Assignee: Richard Wolf Medical Instruments Corporation, Rosemont, Ill.

[**] Term: 14 Years

[21] Appl. No.: 767,896

[22] Filed: Feb. 11, 1977

[51] Int. Cl. D24-02

[52] U.S. Cl. D24/8; D10/81

[58] Field of Search D24/8; 128/303.13, 303.14, 128/2.1 R, 401, 399; D10/81

[56] References Cited

U.S. PATENT DOCUMENTS

D. 219,494	12/1970	Glassner et al.	D24/17
D. 224,070	6/1972	Lopez et al.	D24/8
3,460,528	8/1969	Carney	128/2.1 R
3,467,104	9/1969	Burbridge et al.	128/401 X

Primary Examiner—Bernard Ansher
Attorney, Agent, or Firm—James B. Kinzer

[57] CLAIM

A bipolar electrical surgical generator, substantially as shown.

DESCRIPTION

FIG. 1 is a perspective view of a bipolar electrical surgical generator showing my new design;
FIG. 2 is a top plan view of the generator shown in FIG. 1;
FIG. 3 is an end view of the generator shown in FIG. 1; and
FIG. 4 is a rear view of the generator shown in FIG. 1.

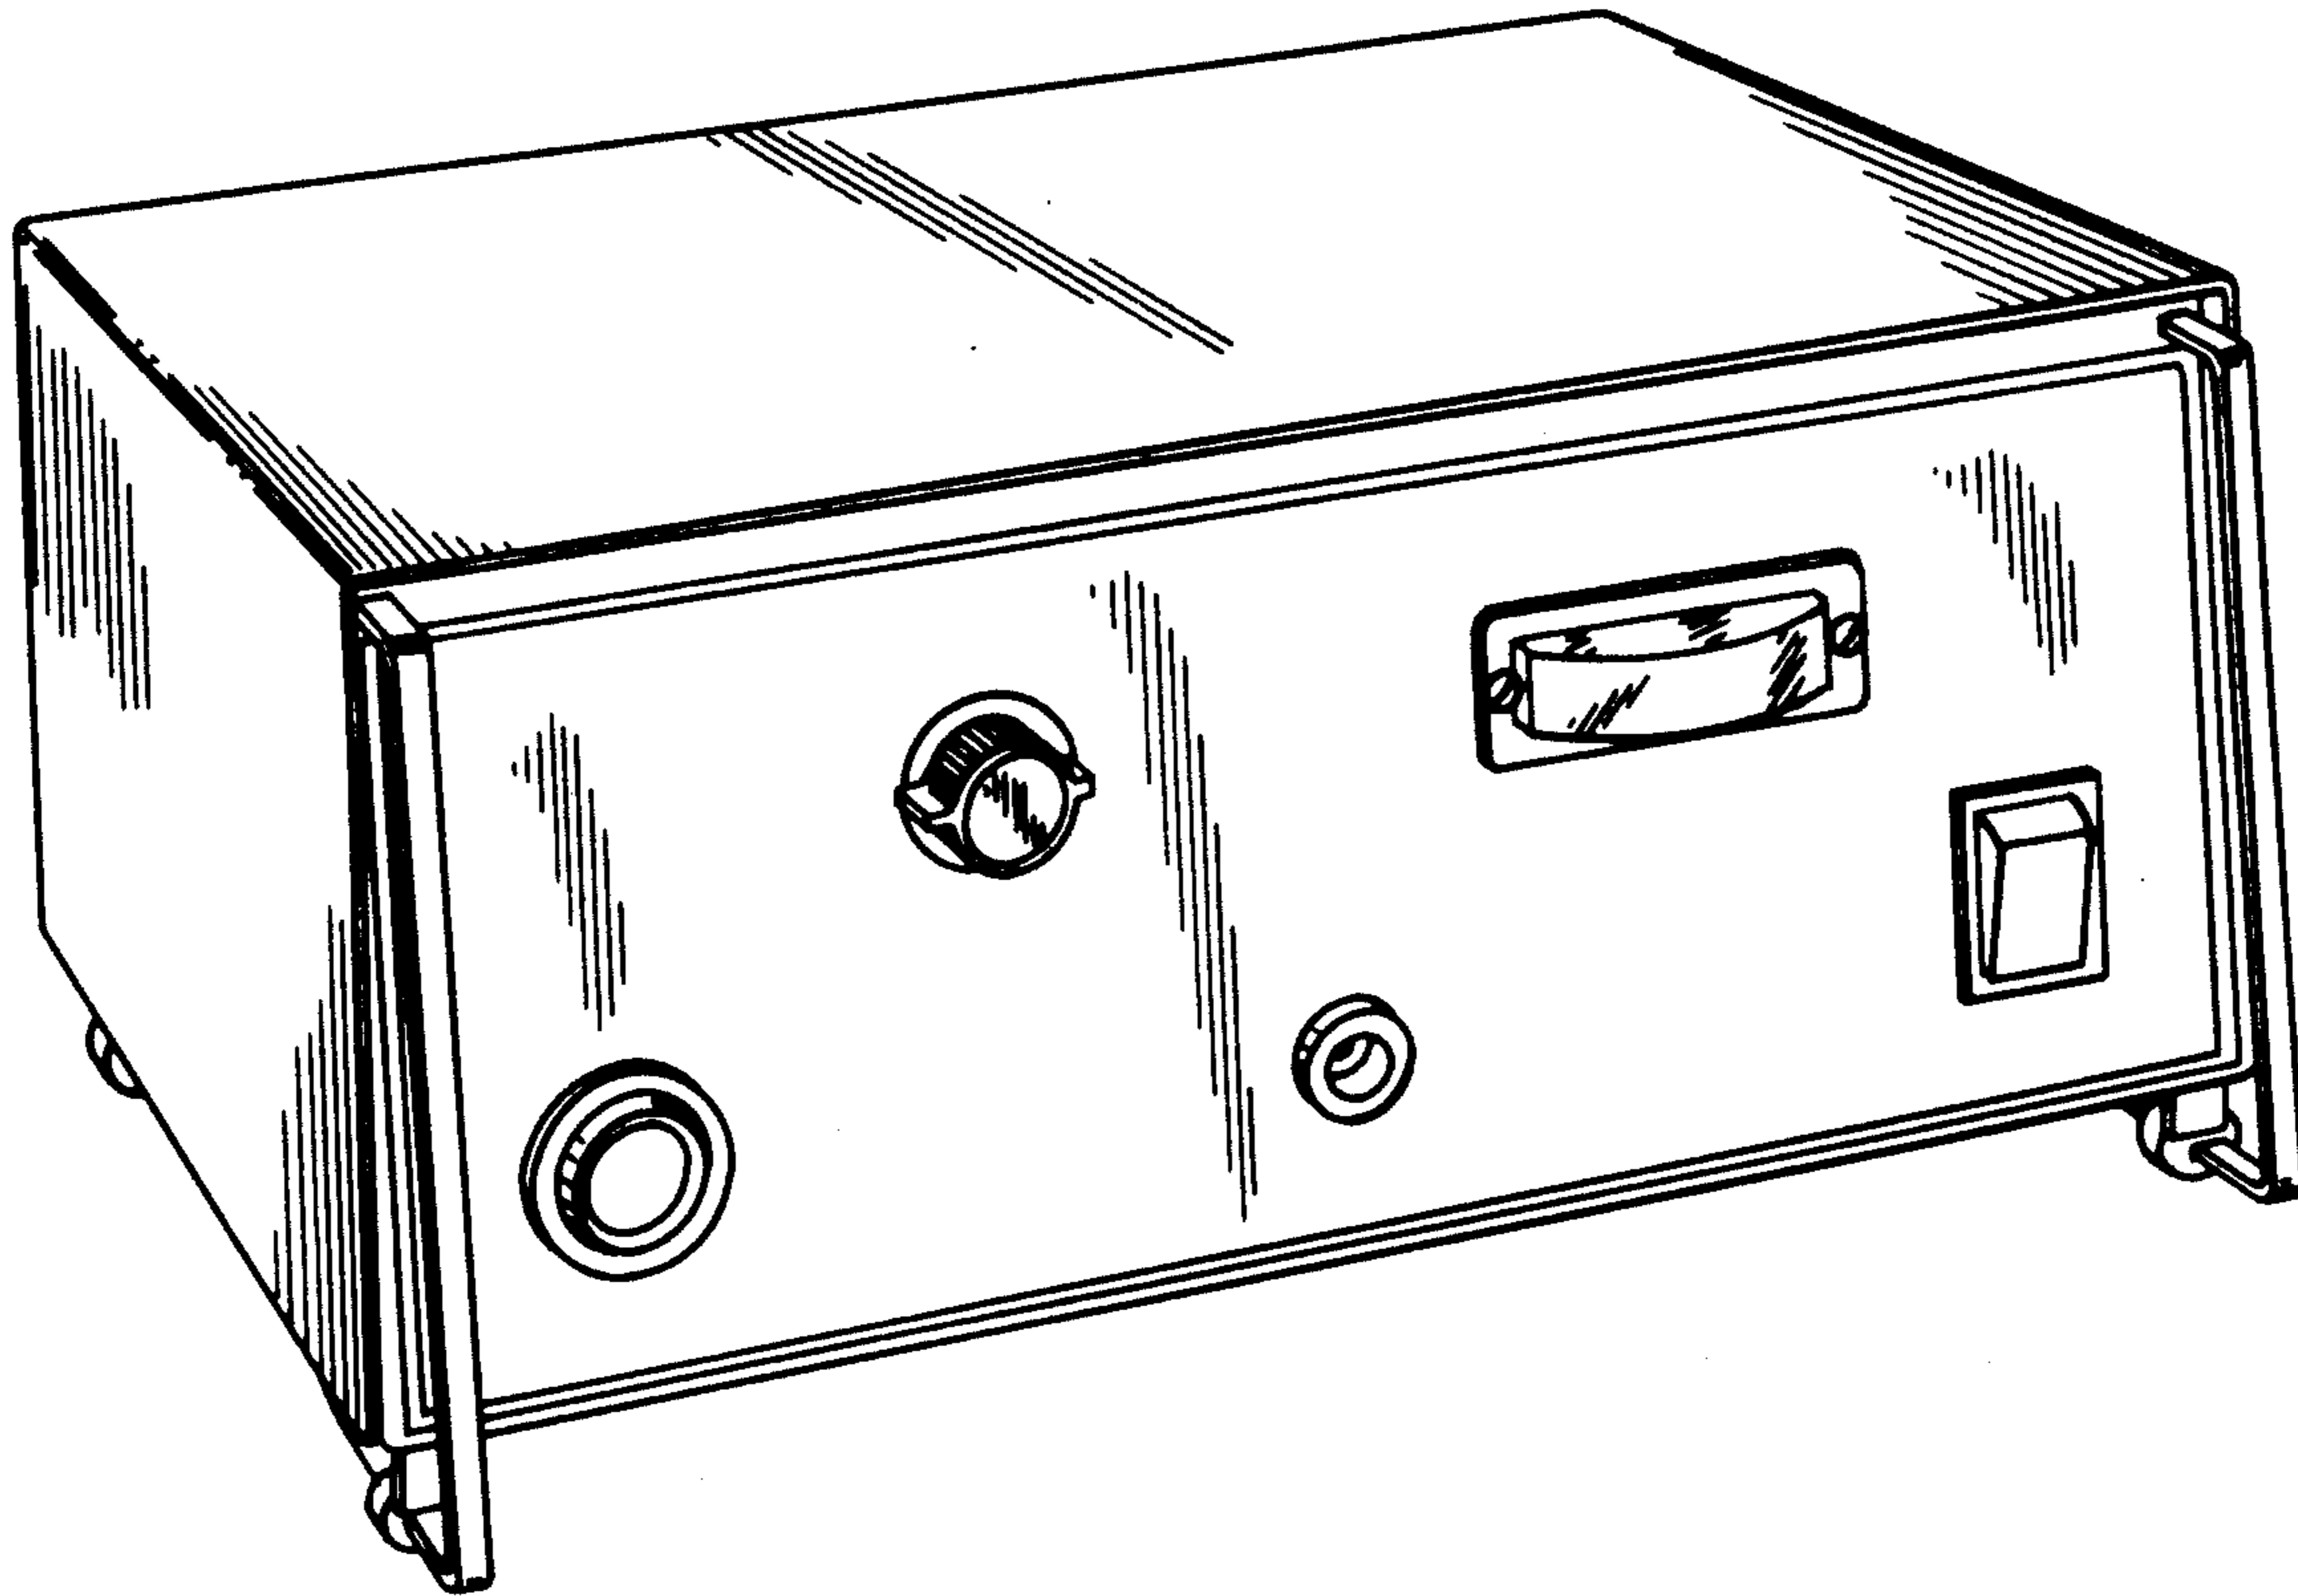


fig. 1.

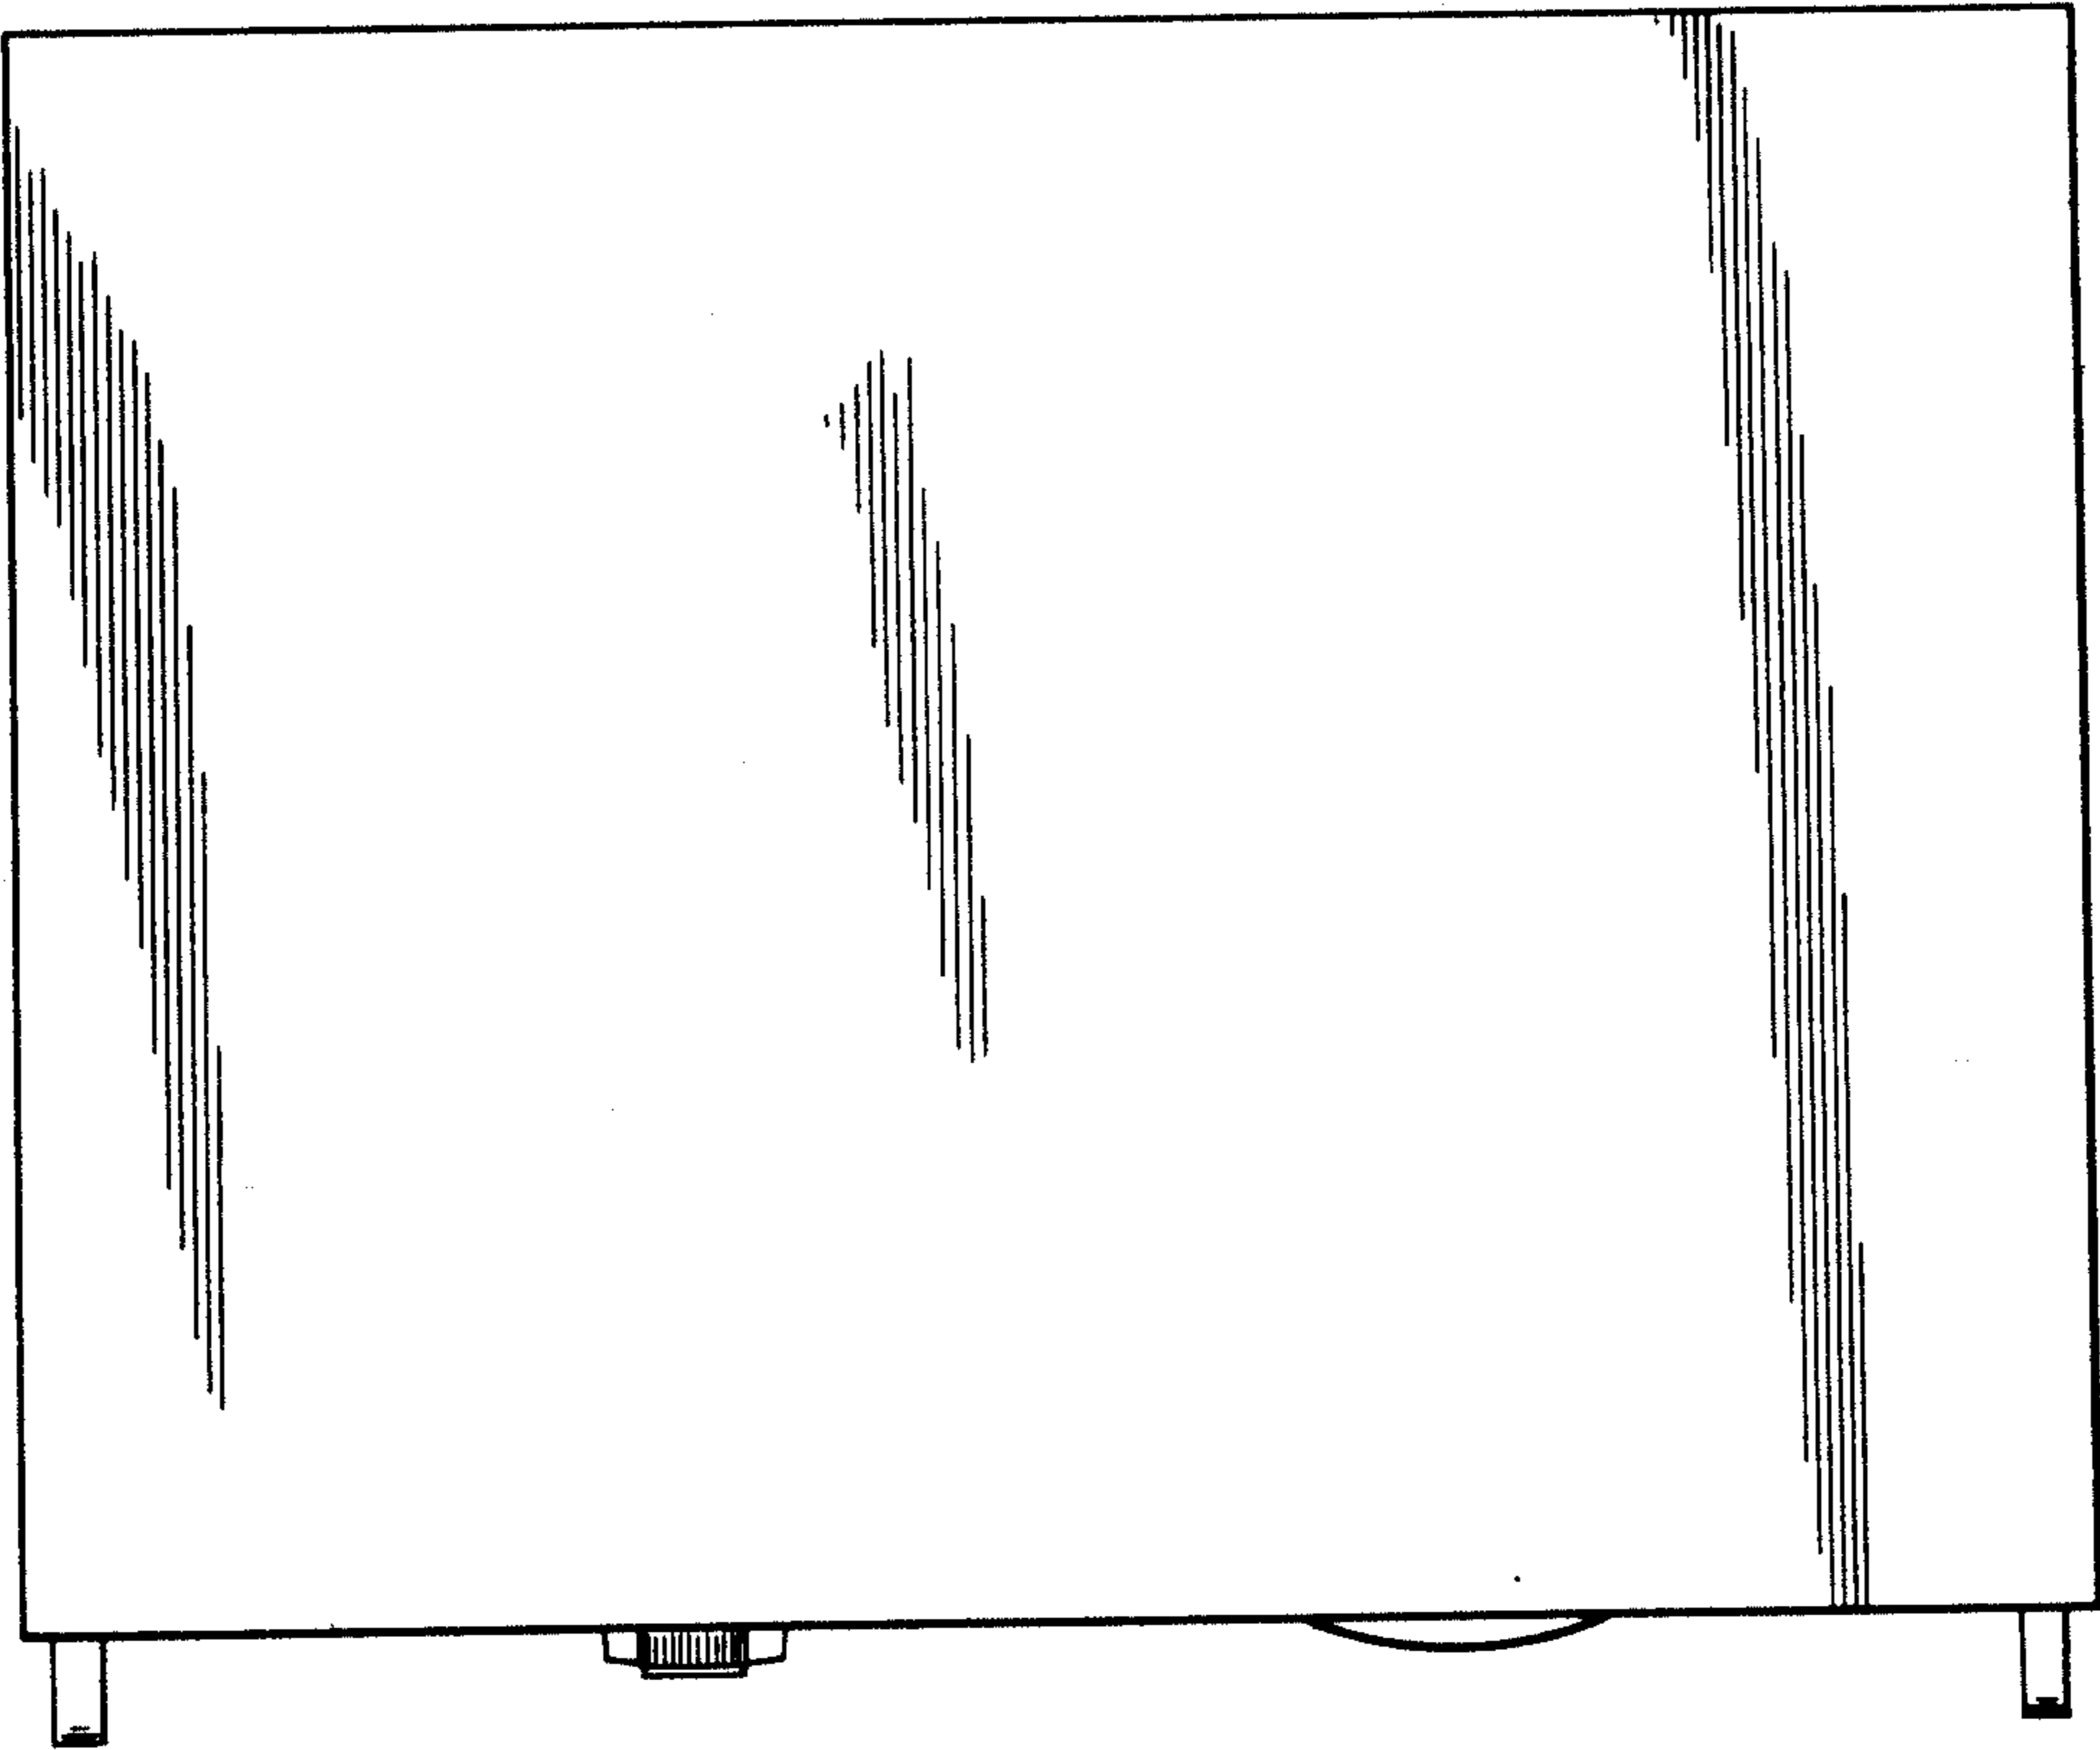
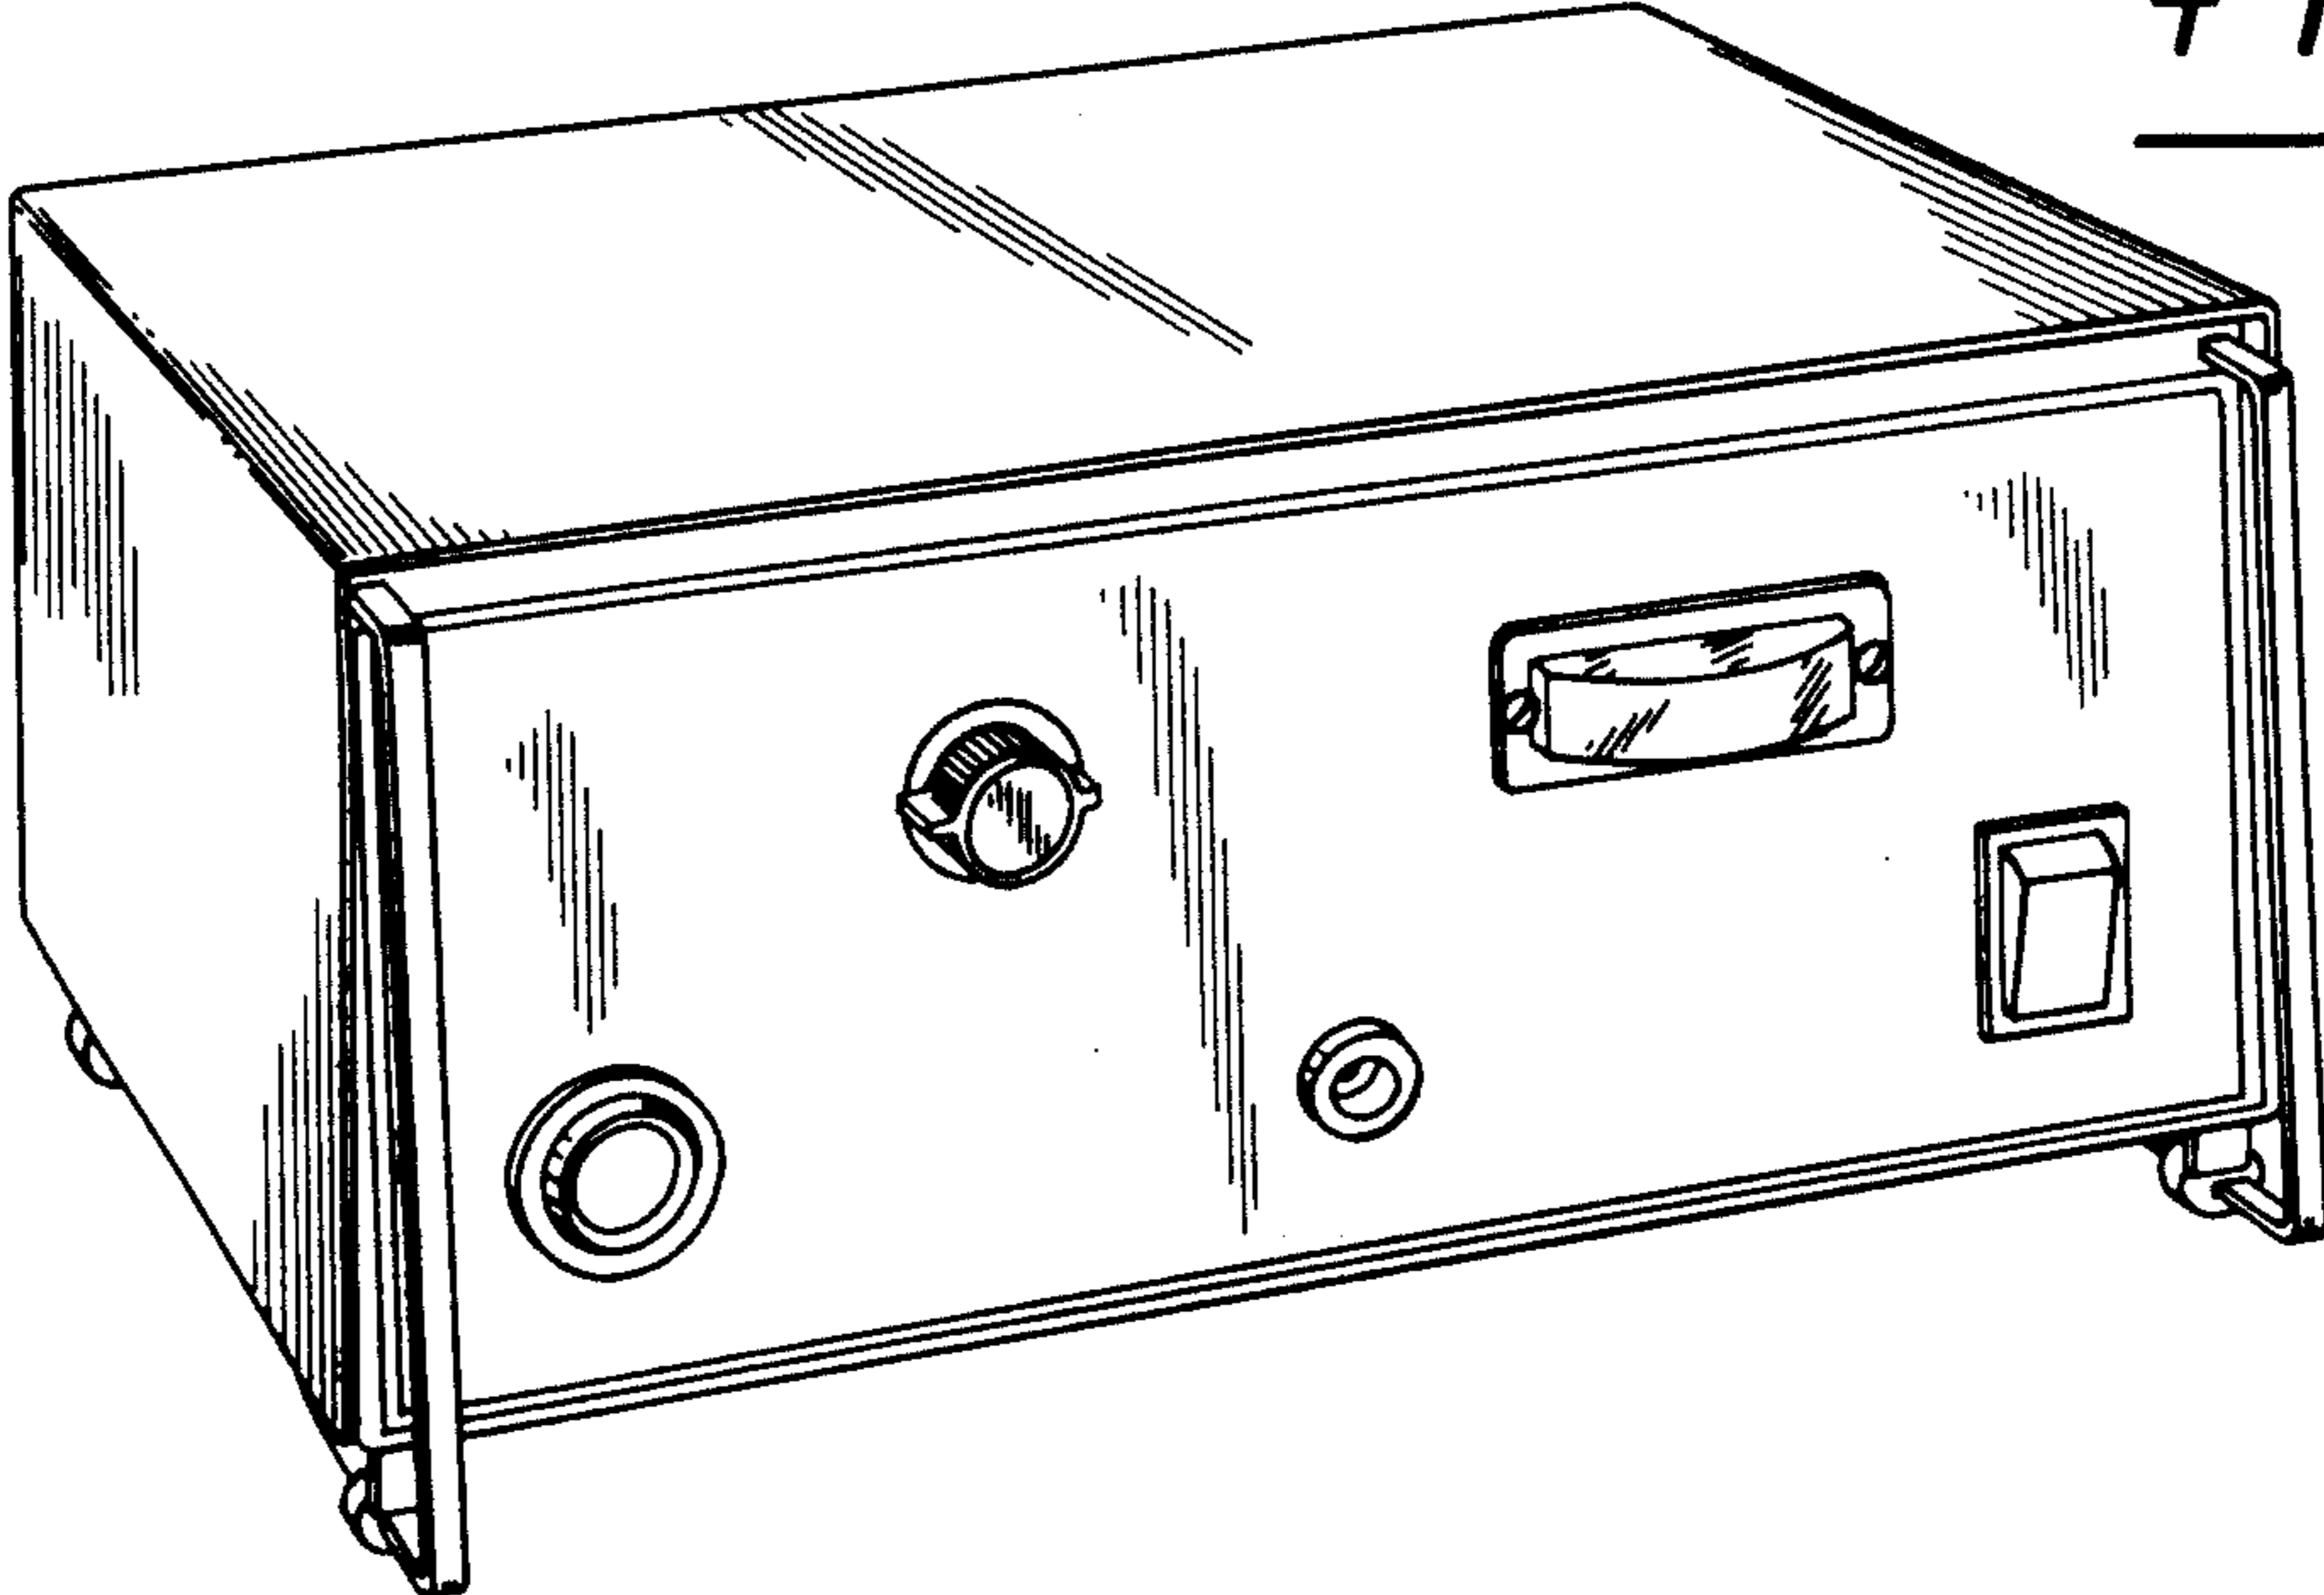


fig. 2.

fig. 3.


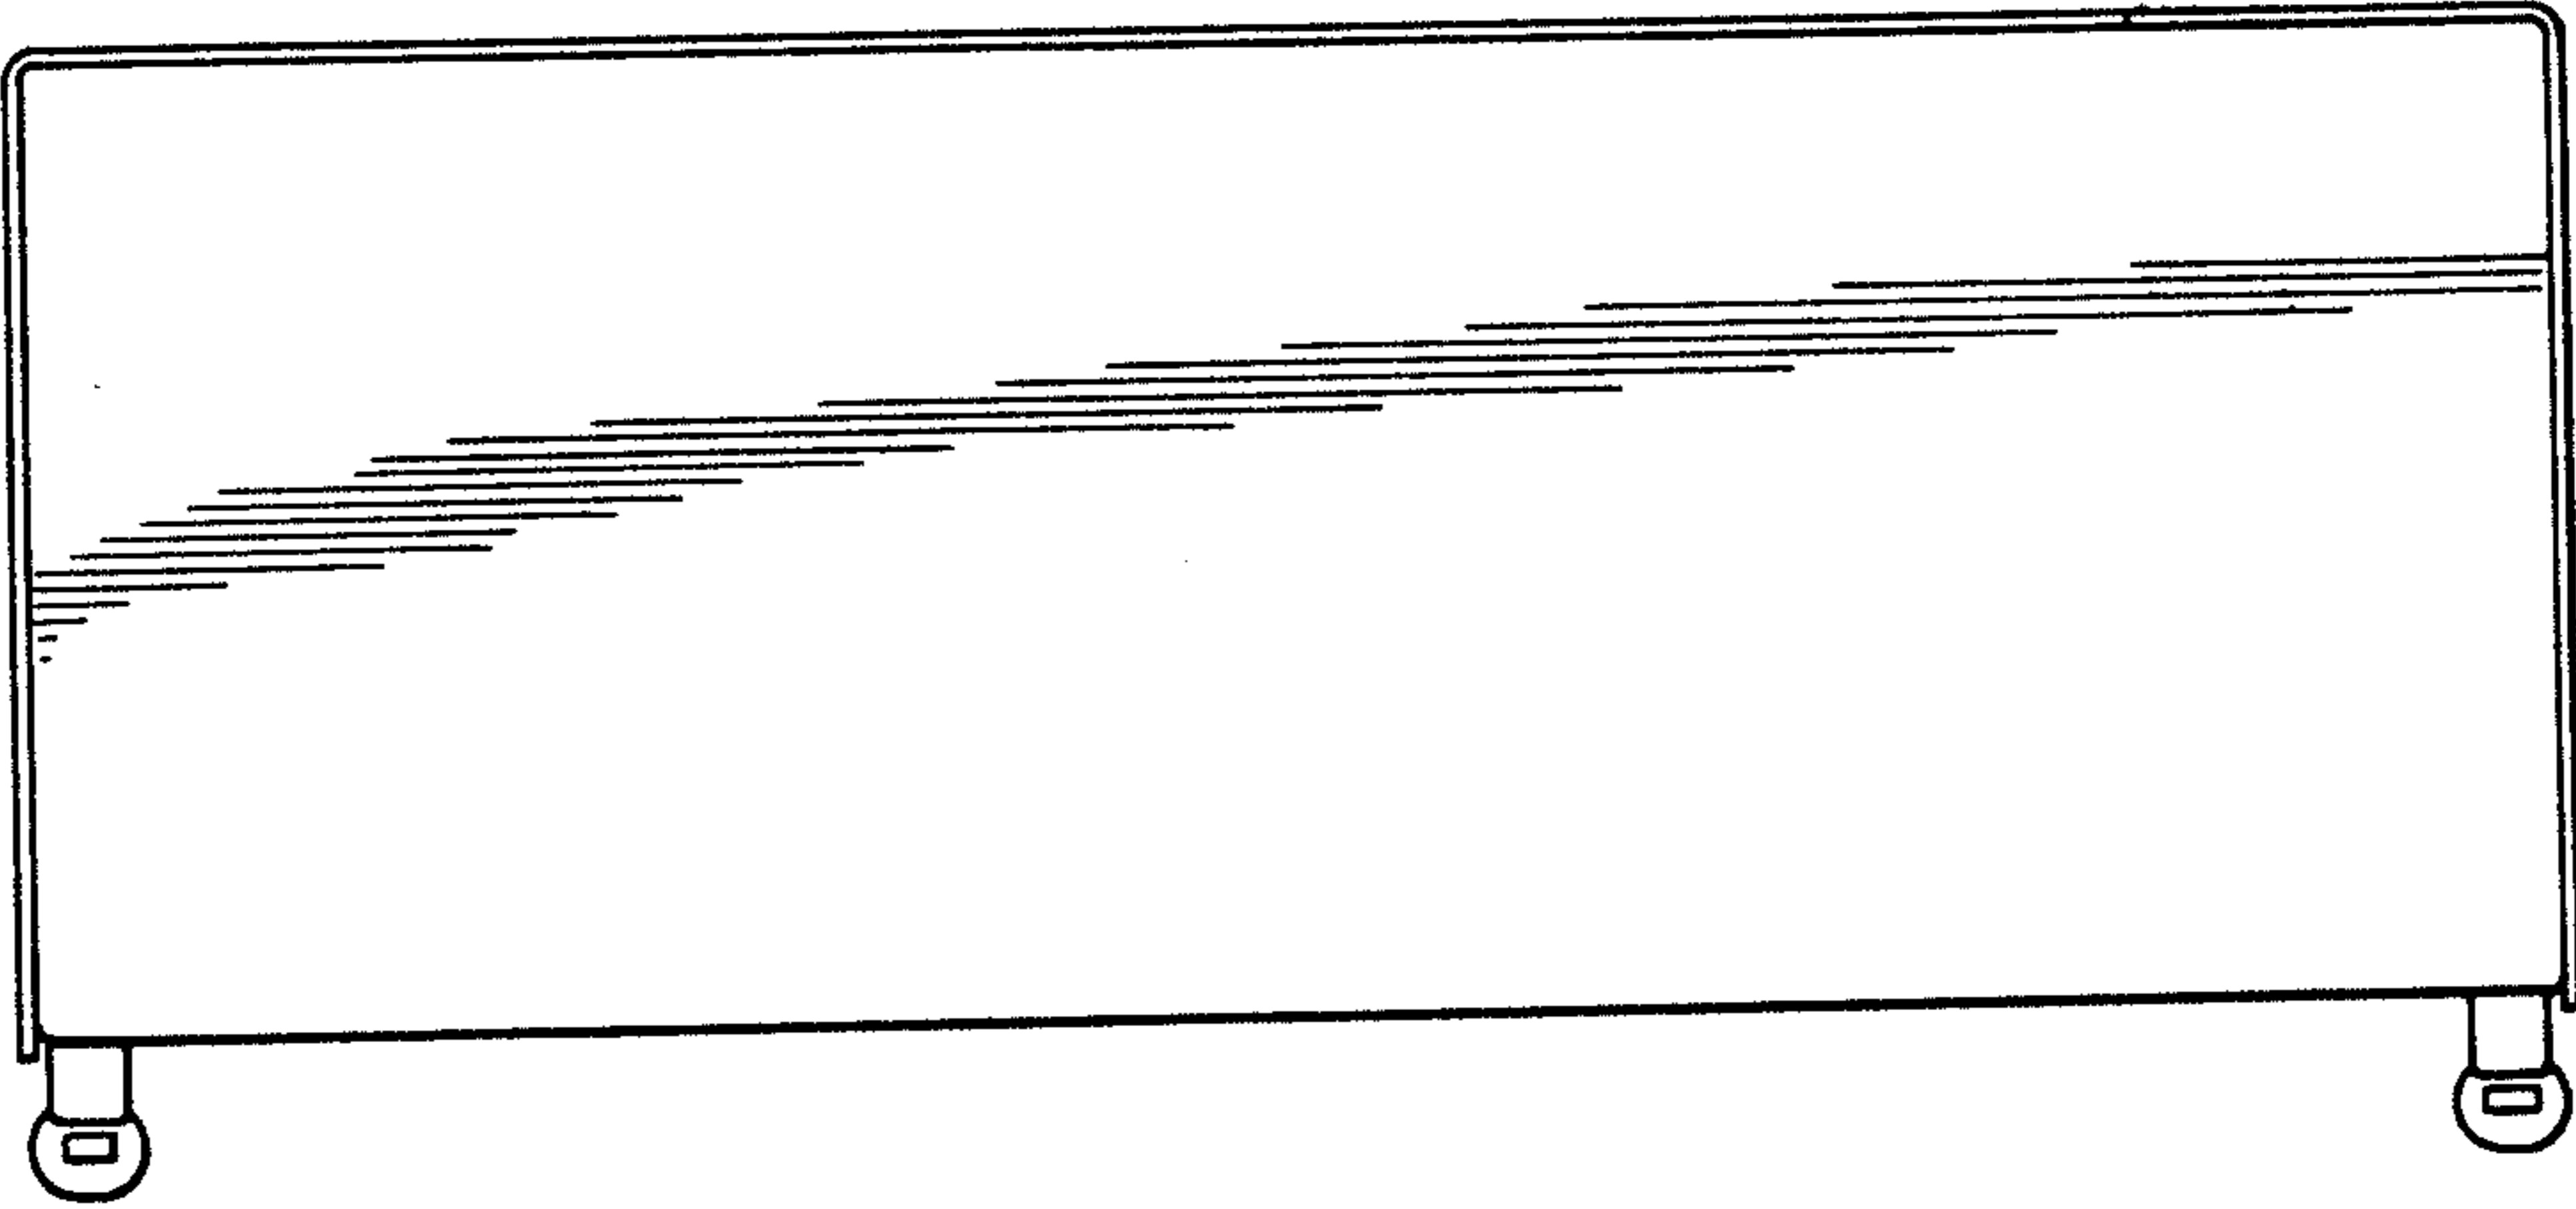


fig. 4.

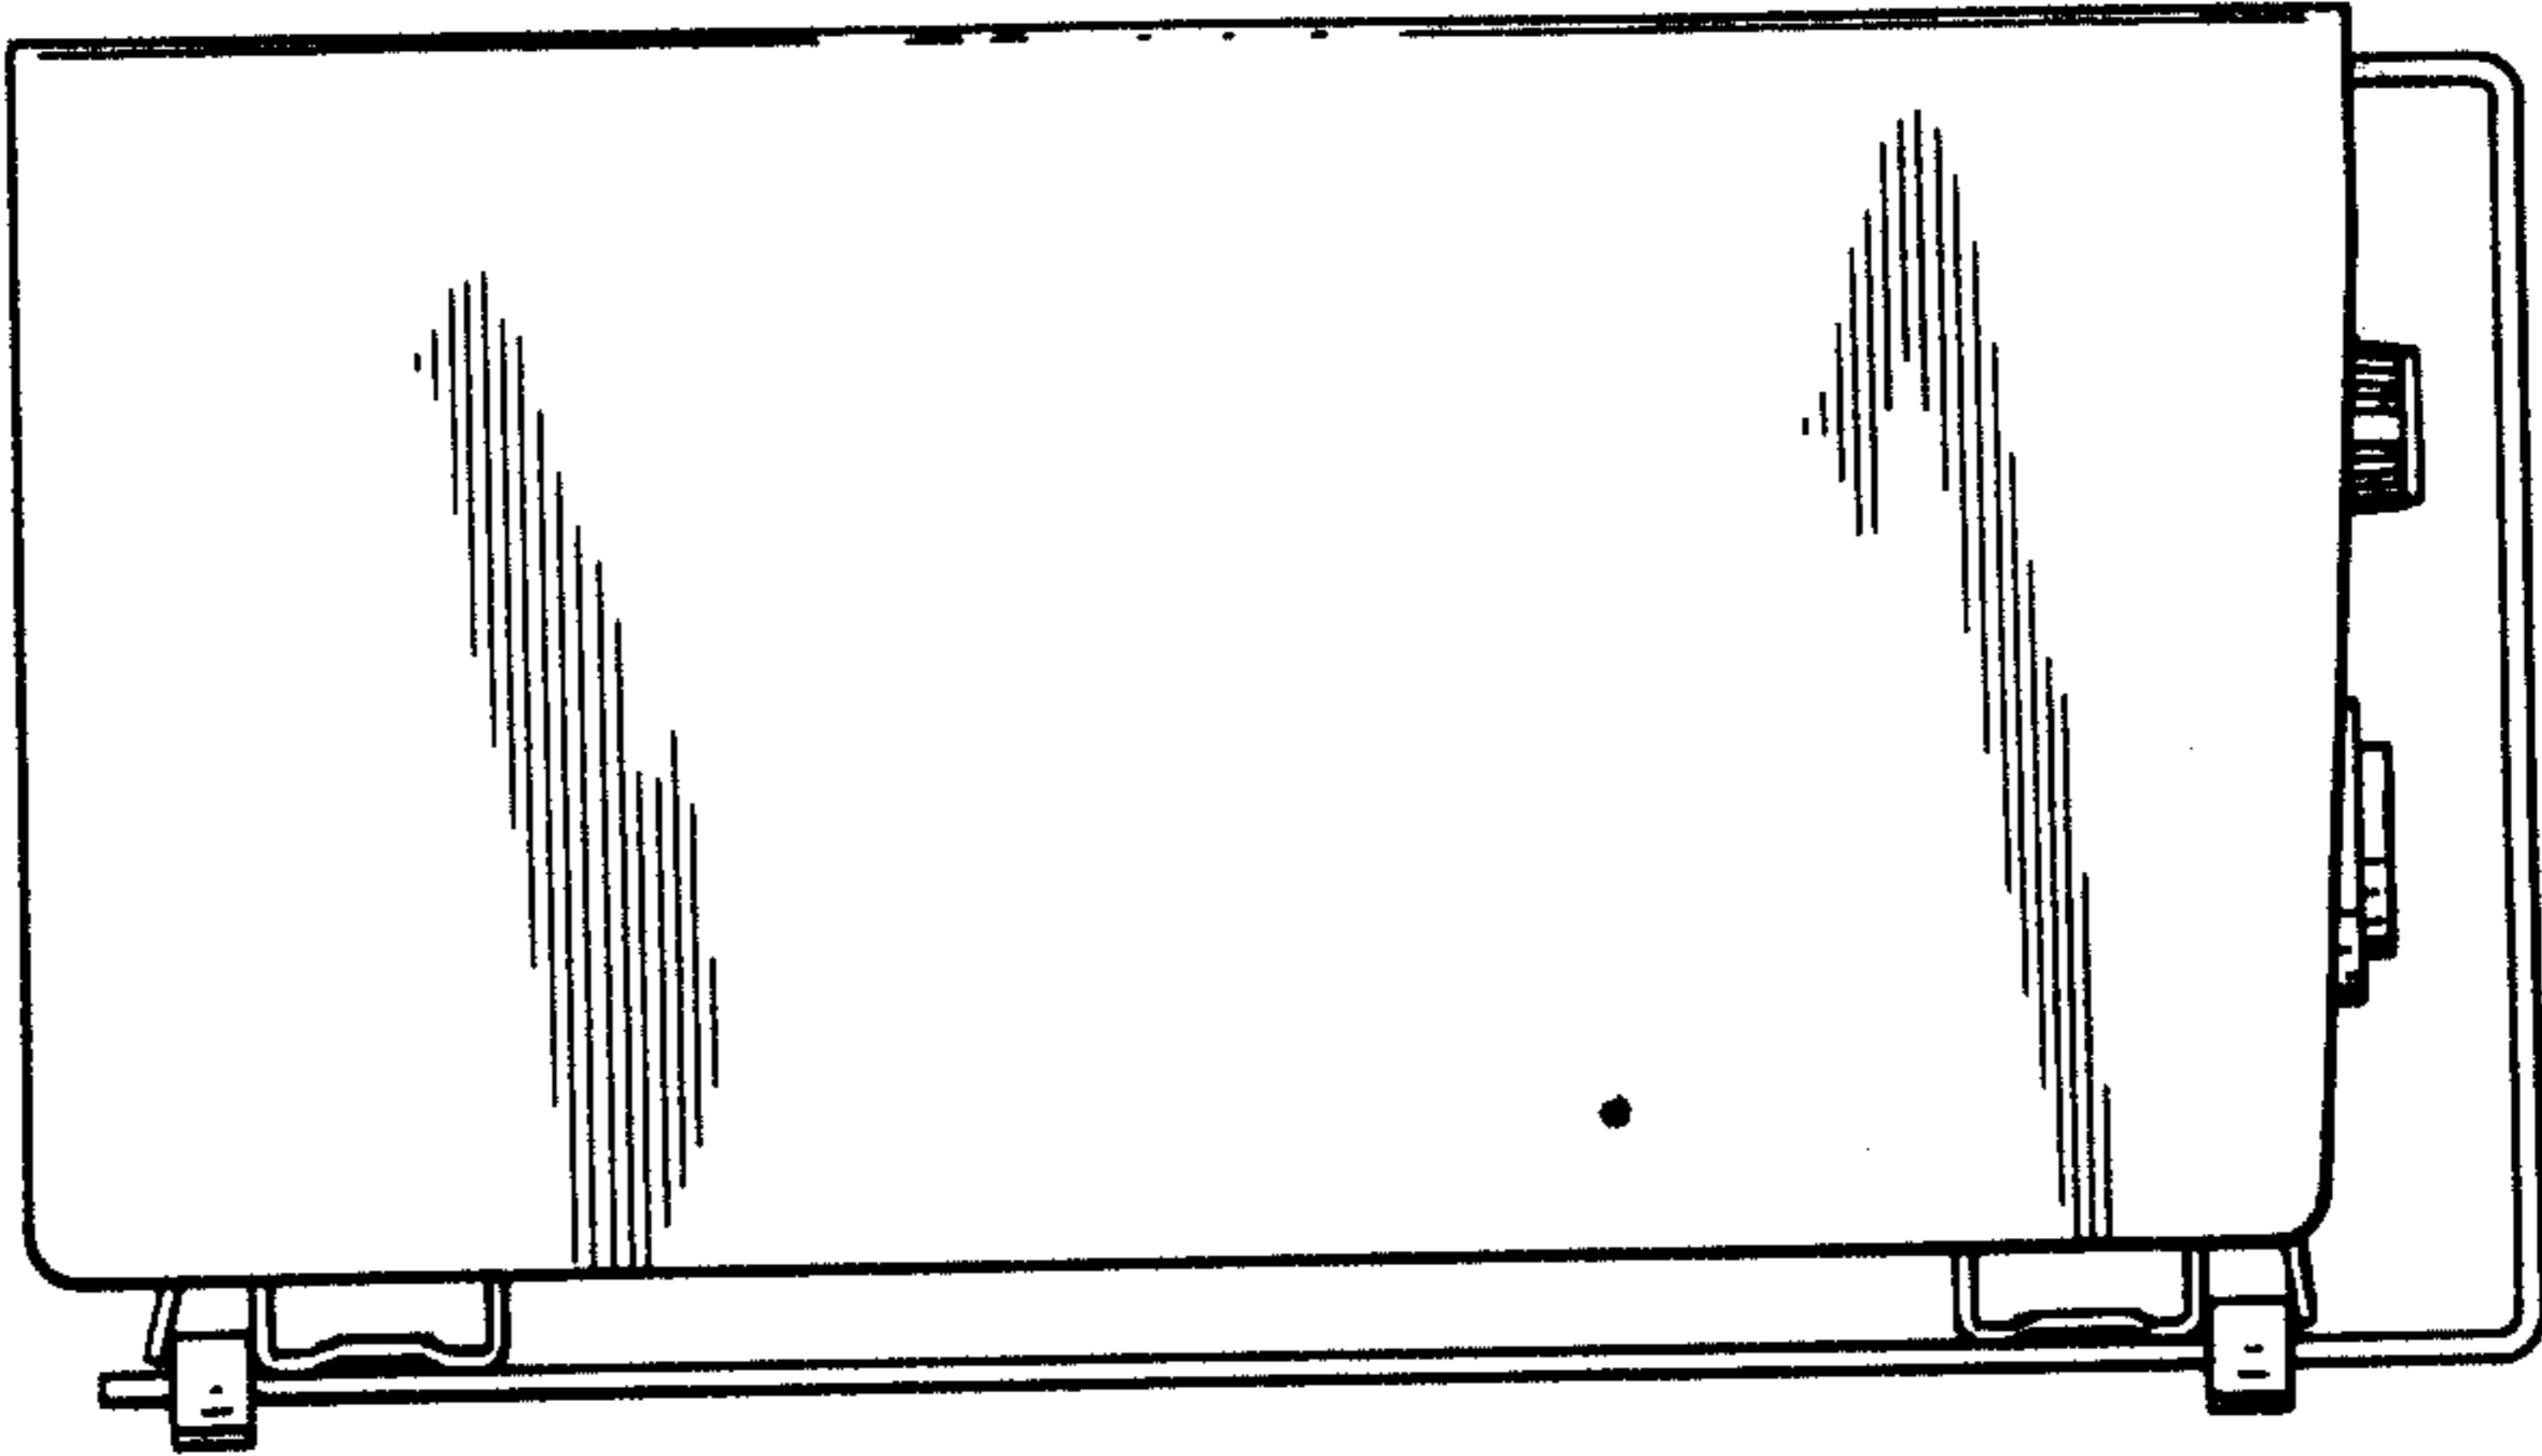

US008250480A

REEXAMINATION CERTIFICATE (2161st)

United States Patent [19]

[11] **B1 Des. 250,480**

Wettermann et al.

[45] **Certificate Issued Dec. 28, 1993**

[54] **BIPOLAR ELECTRICAL SURGICAL GENERATOR**

[75] **Inventors:** Ludwig A. Wettermann, Arlington Heights, Ill.; Peter H. Wettermann, Dayville, Conn.

[73] **Assignee:** Richard Wolf Medical Instruments Corporation, Rosemont, Ill.

Reexamination Request:
No. 90/002,904, Dec. 11, 1992

Reexamination Certificate for:
Patent No.: Des. 250,480
Issued: Dec. 5, 1978
Appl. No.: 767,896
Filed: Feb. 11, 1977

[52] **U.S. Cl.** D24/170
[58] **Field of Search** D24/170

[56] **References Cited PUBLICATIONS**

"Wolf Instruction Manual", Jun. 1974, Richard Wolf Medical Instruments Corporation.


Primary Examiner—Stella Reid

[57] **CLAIM**

A bipolar electrical surgical generator, substantially as shown.

DESCRIPTION

FIG. 1 is a perspective view of a bipolar electrical surgical generator showing my new design;
FIG. 2 is a top plan view of the generator shown in FIG. 1;
FIG. 3 is an end view of the generator shown in FIG. 1; and
FIG. 4 is a rear view of the generator shown in FIG. 1.

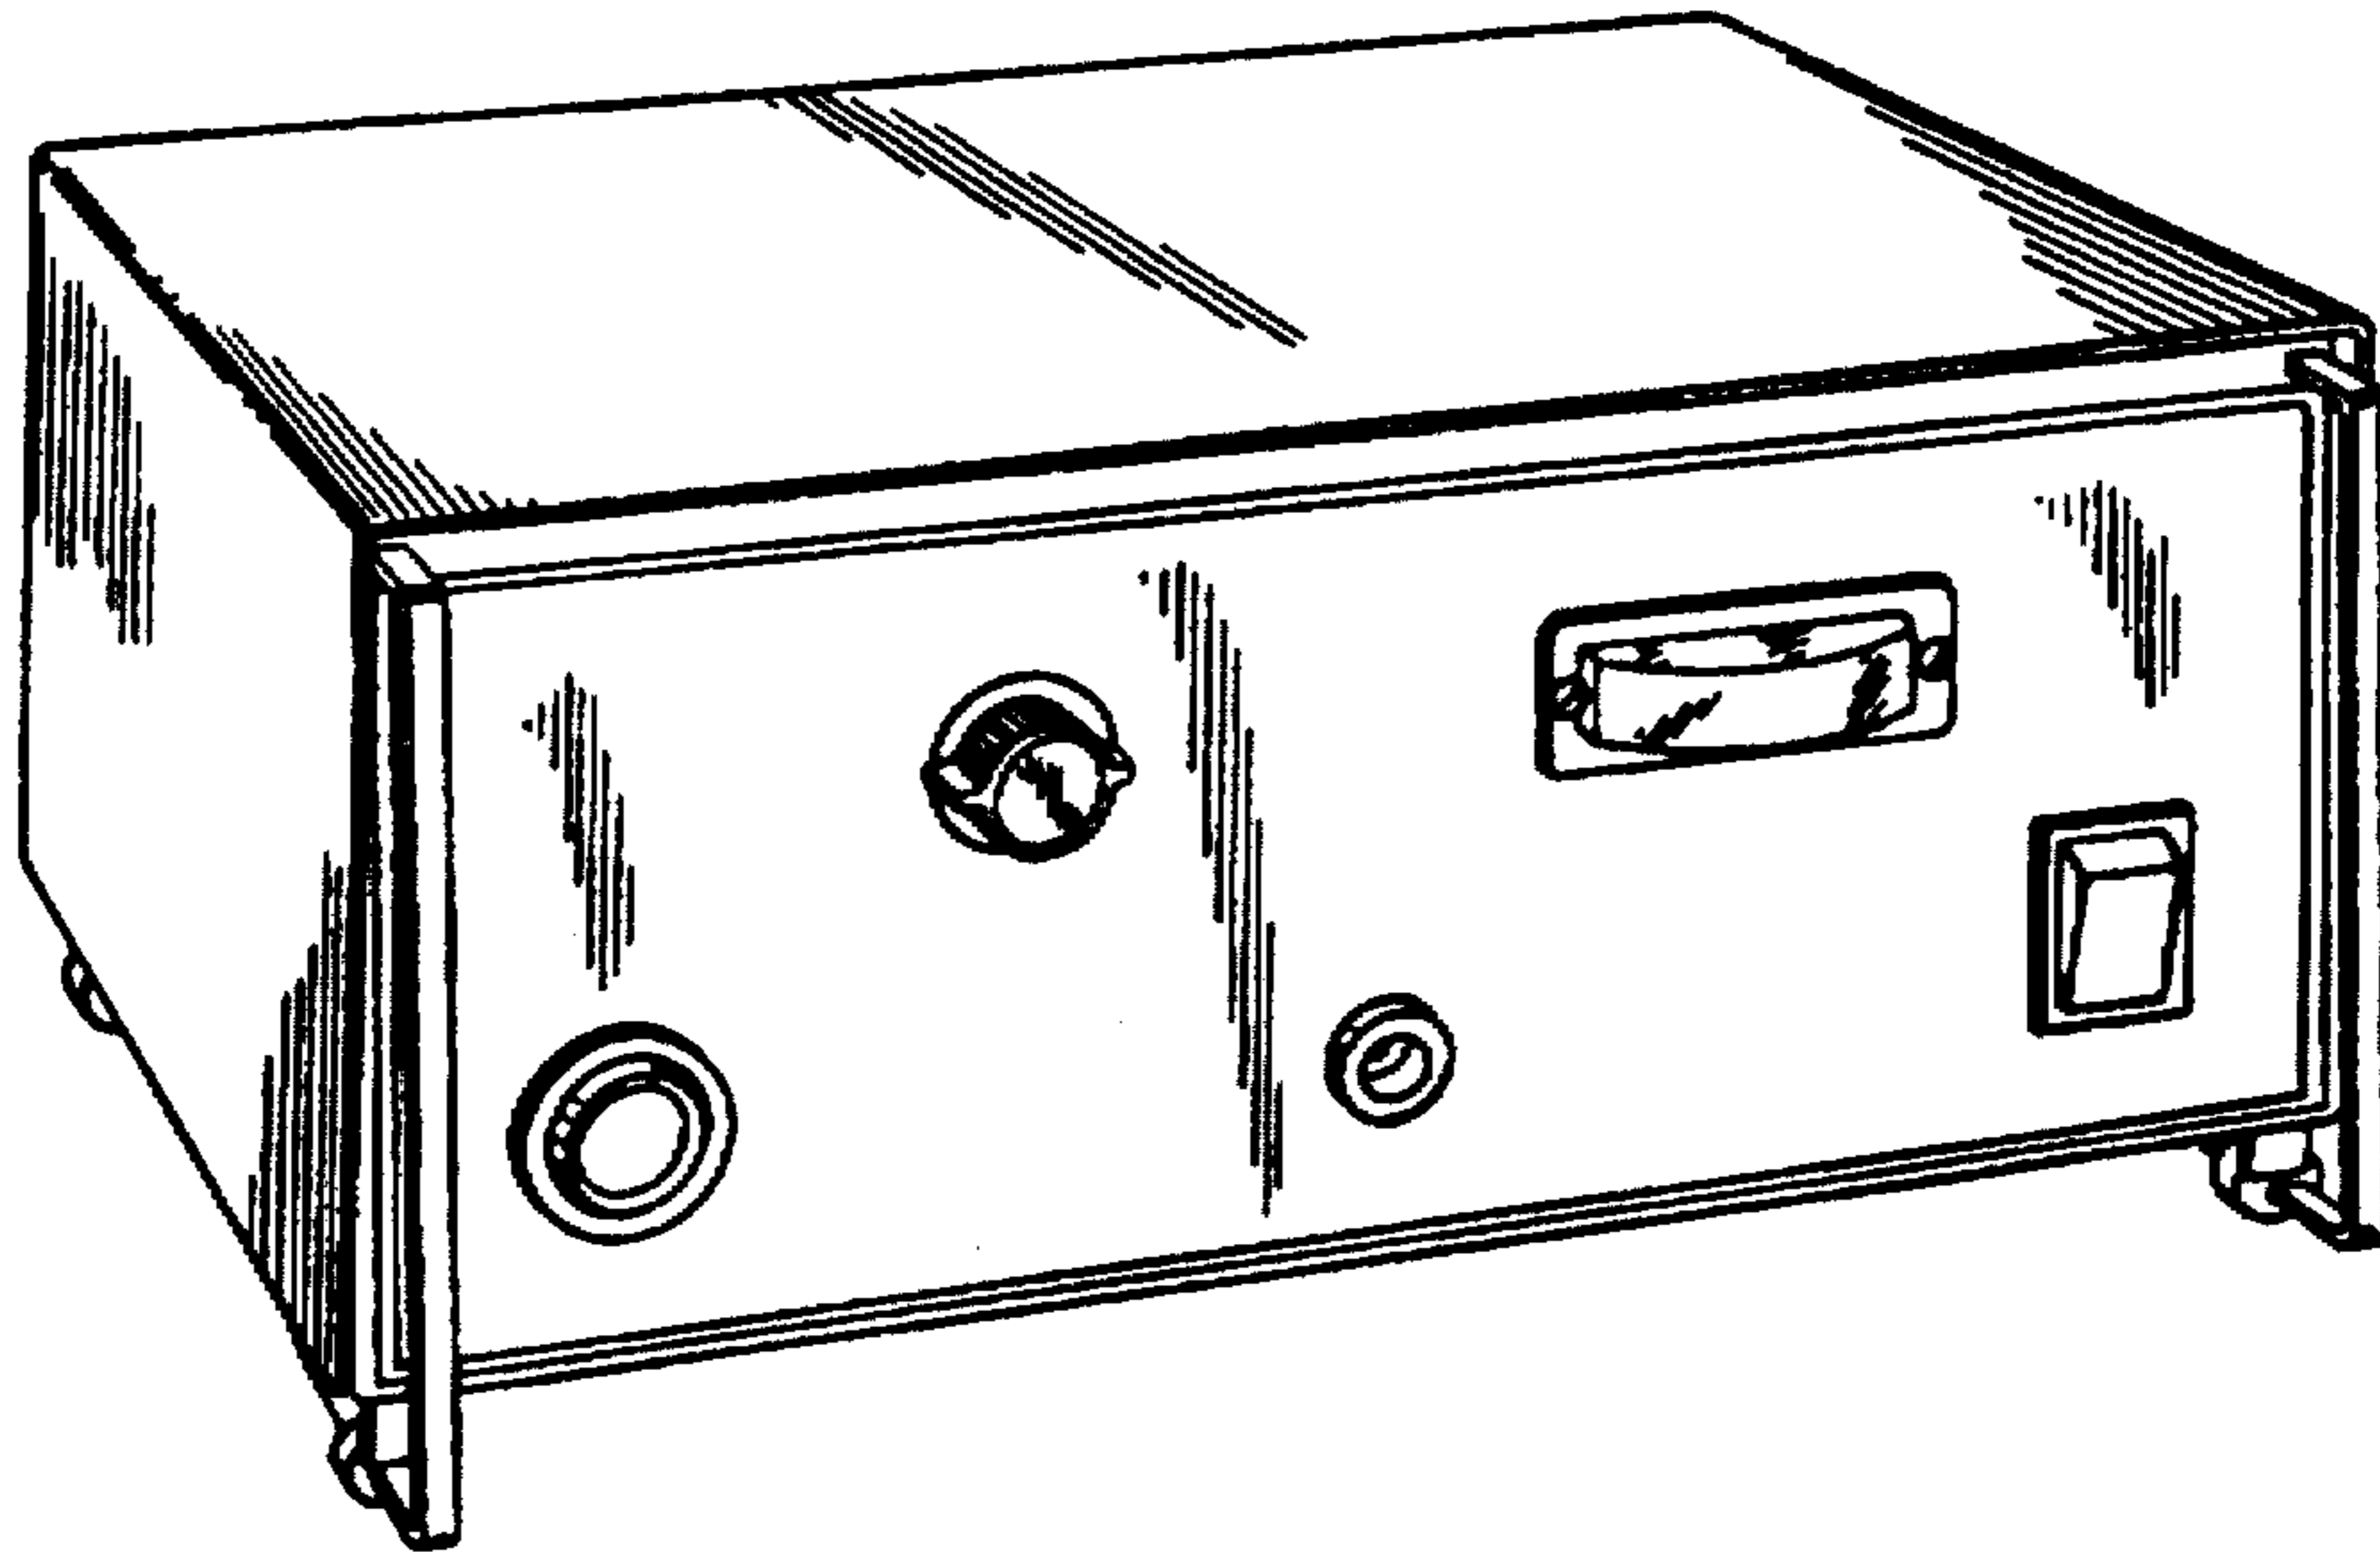

**REEXAMINATION CERTIFICATE
ISSUED UNDER 35 U.S.C. 307**

**THE PATENT IS HEREBY AMENDED AS
INDICATED BELOW.**

**AS A RESULT OF REEXAMINATION, IT HAS
BEEN DETERMINED THAT:**

5 **The single claim is cancelled.**

 * * * * *

10

15

20

25

30

35

40

45

50

55

60

65