

[54] MEDICANT TRANSFER DEVICE

[75] Inventor: Mark M. Bridle, Newport Beach, Calif.

[73] Assignee: American Hospital Supply Corporation, Evanston, Ill.

[**] Term: 14 Years

[21] Appl. No.: 758,970

[22] Filed: Jan. 13, 1977

[51] Int. Cl. D24—04

[52] U.S. Cl. D24/24; 128/272.1; 128/272.3; D24/52; D24/63

[58] Field of Search D24/24, 63, 25, 52; 128/272.3, 272.1, 231; D9/216, 10; 206/222

[56] References Cited

U.S. PATENT DOCUMENTS

| | | | |
|------------|---------|------------------------|-----------|
| D. 198,964 | 8/1964 | Dash et al. | D24/63 X |
| D. 246,321 | 11/1977 | Löfman | D24/24 |
| 3,788,369 | 1/1974 | Killinger | 128/272.3 |
| 3,938,520 | 2/1976 | Scislowicz et al. | 128/272.3 |
| 3,941,171 | 3/1976 | Ogle | 128/272.3 |
| 3,987,791 | 10/1976 | Chittenden et al. | 128/272.3 |

Primary Examiner—Bernard Ansher
Attorney, Agent, or Firm—Robert E. Hartenberger

[57] CLAIM

The ornamental design for a medicant transfer device, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of the medicant transfer device showing my new design;
FIG. 2 is a side elevational view thereof;
FIG. 3 is a top plan view of the medicant transfer device; and
FIG. 4 is a bottom plan view of the medicant transfer device.

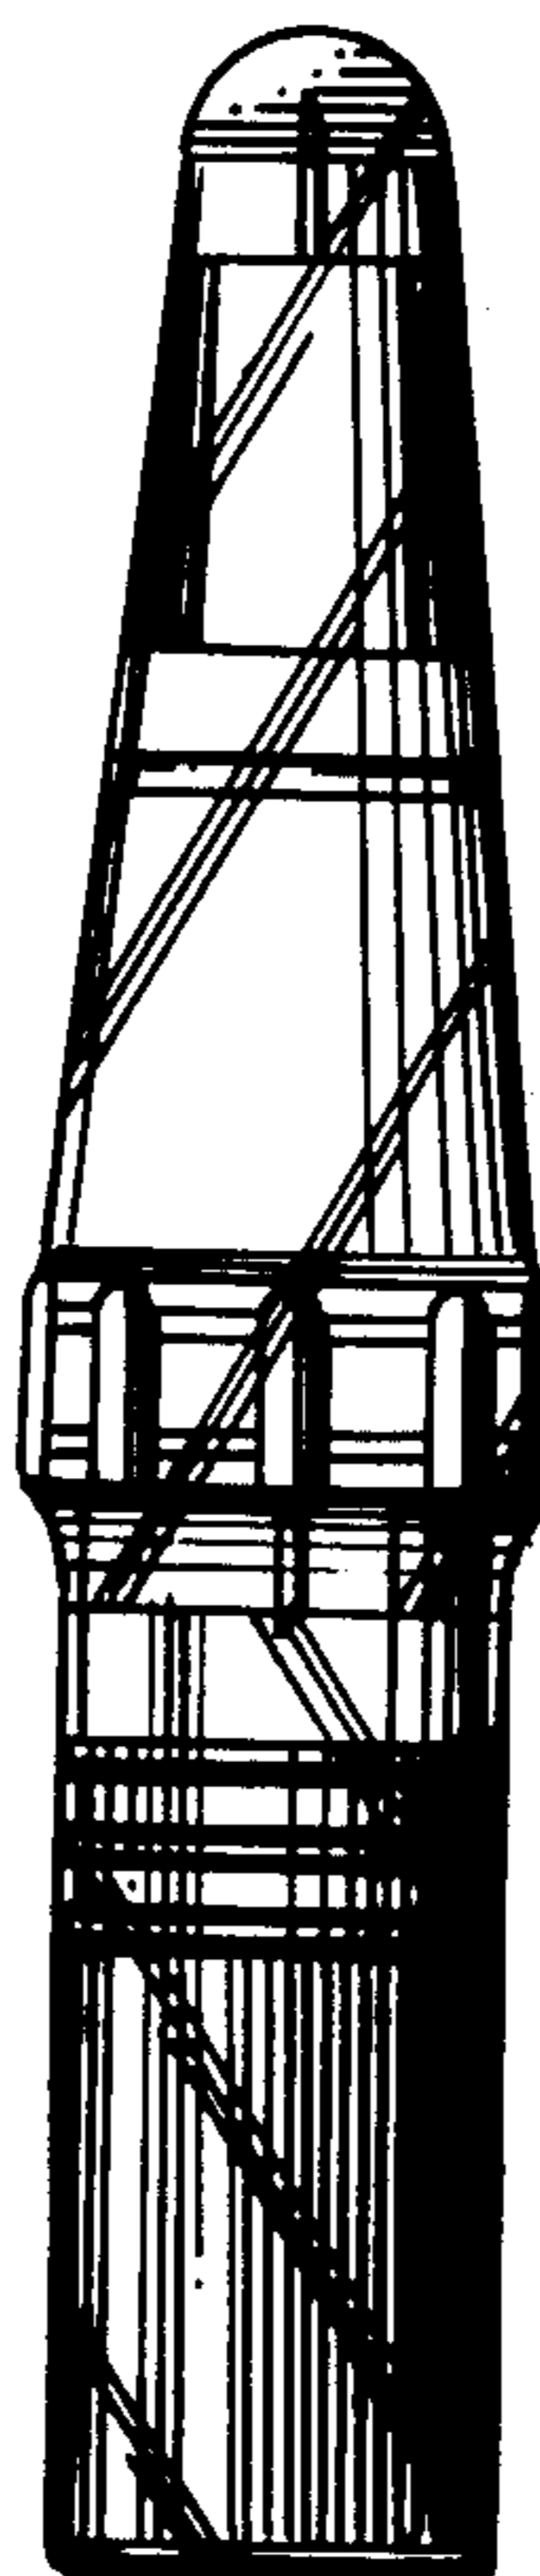
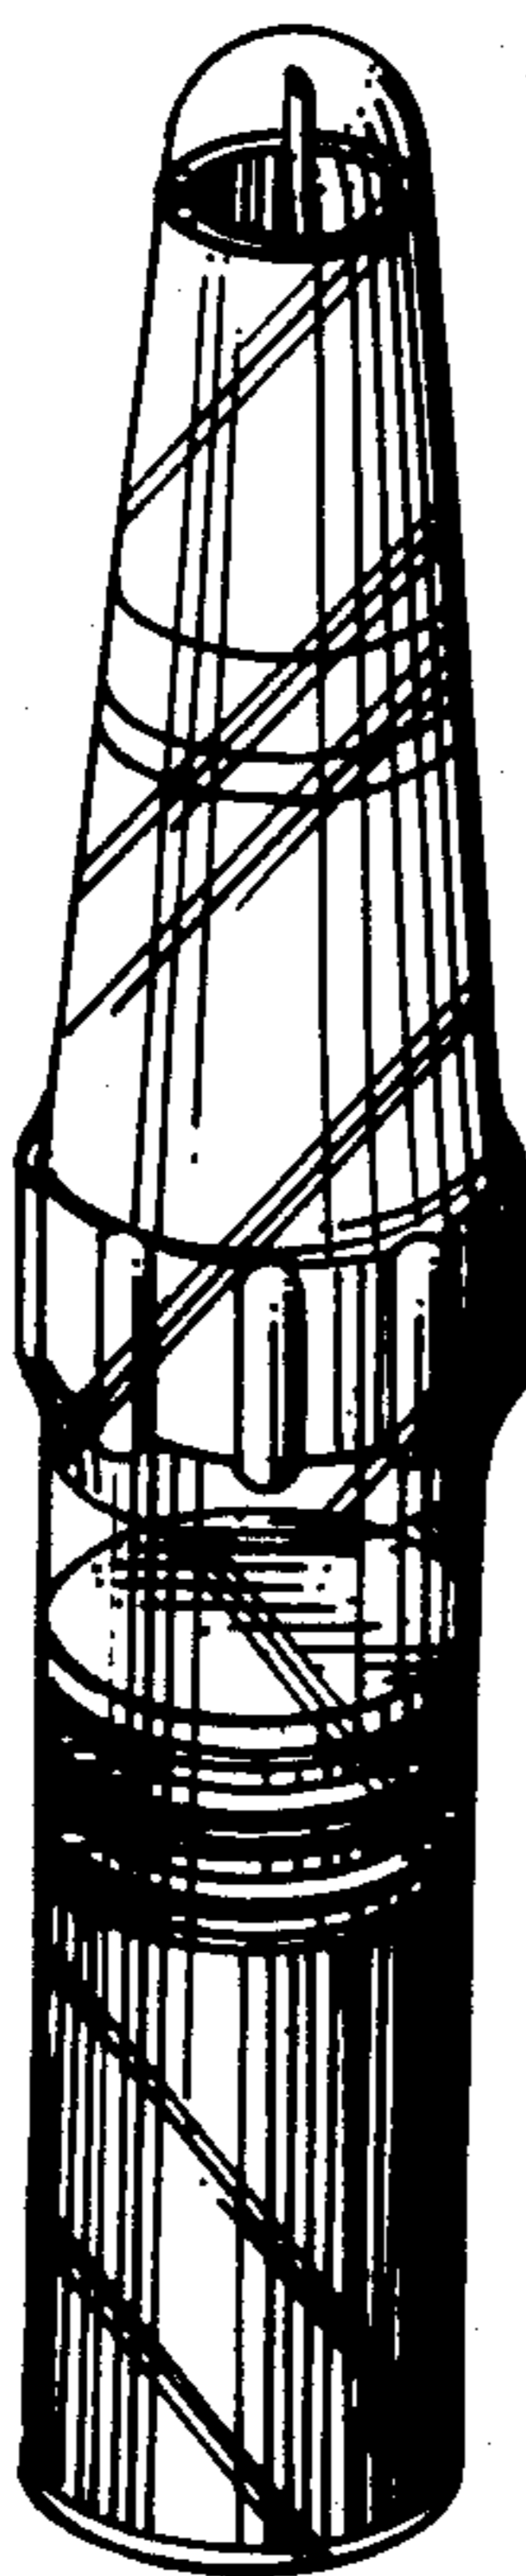


FIG. 3

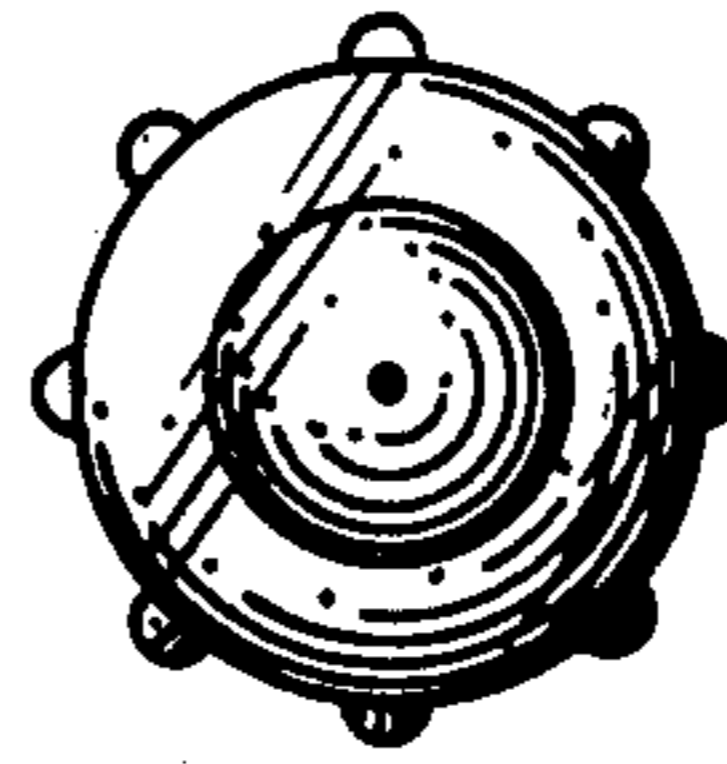


FIG. 1

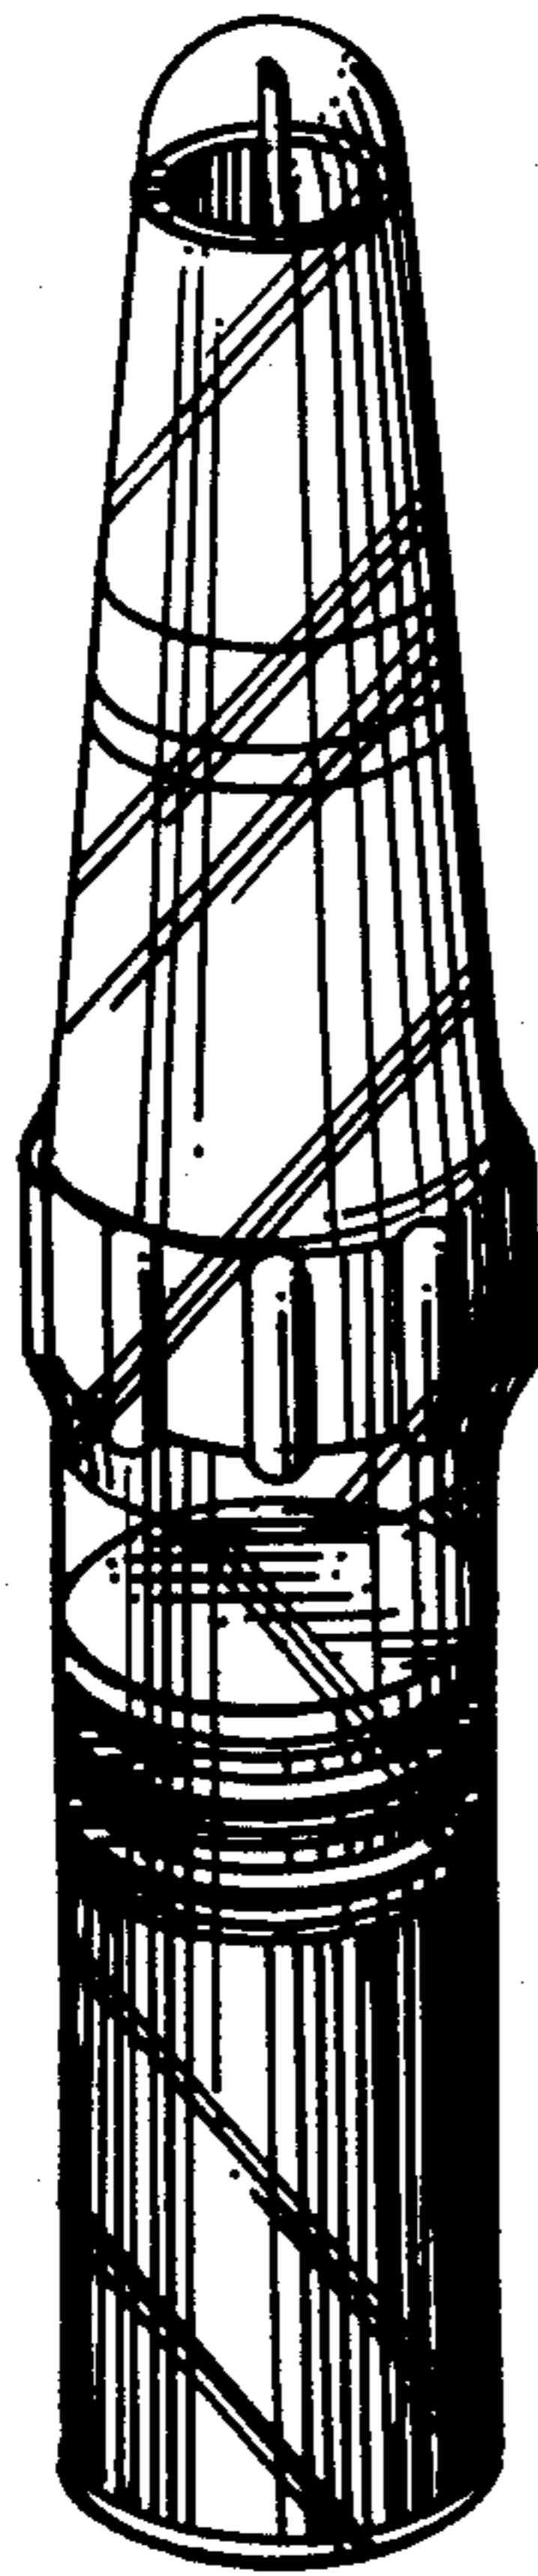


FIG. 2


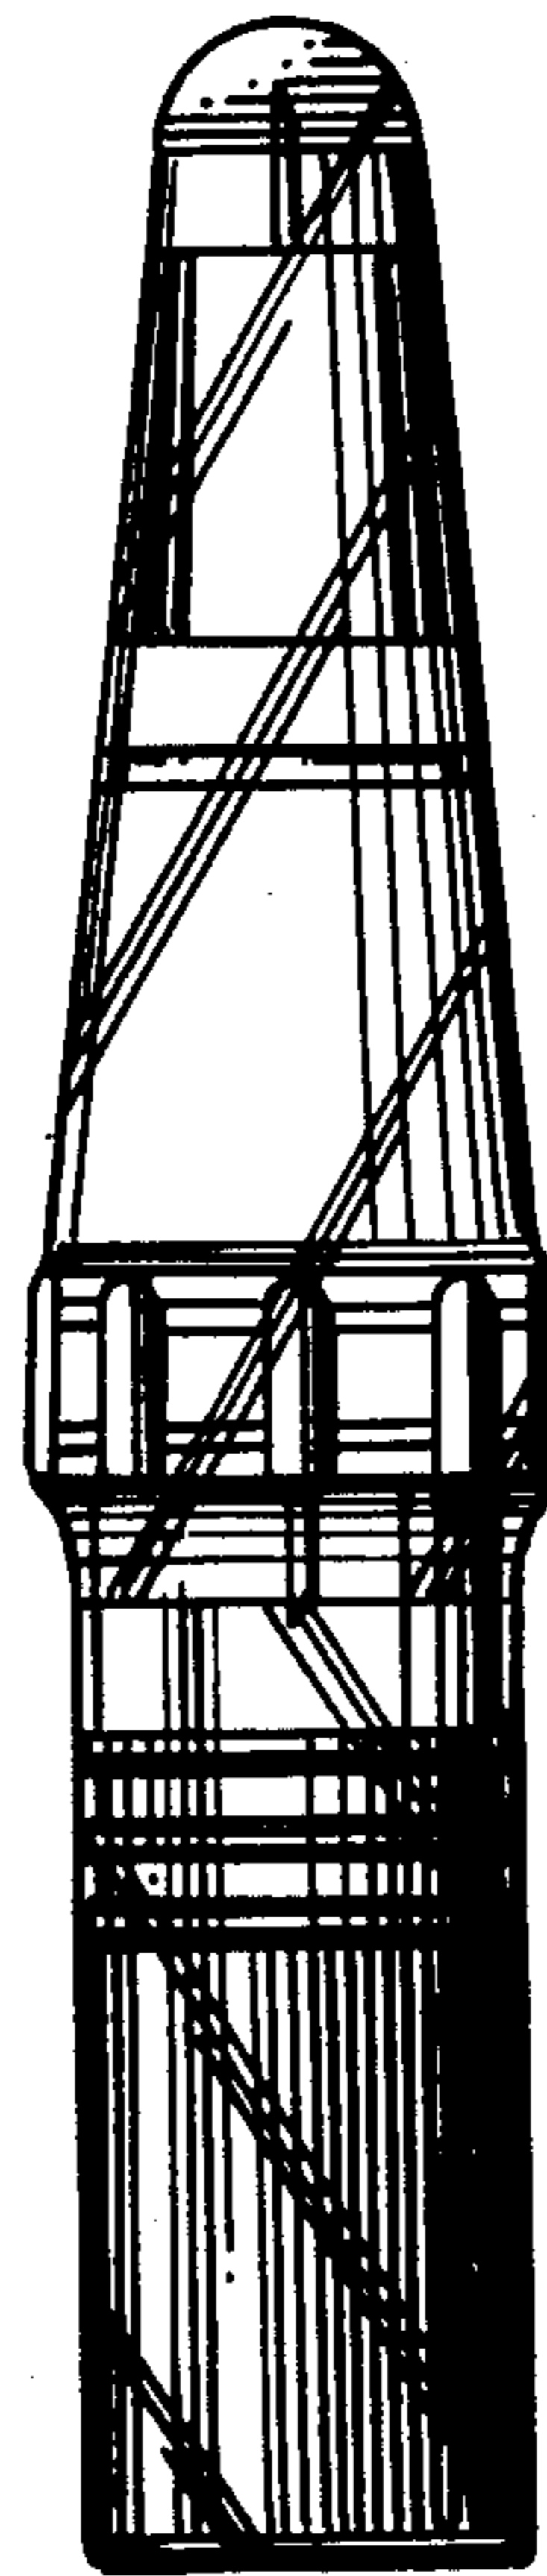


FIG. 4

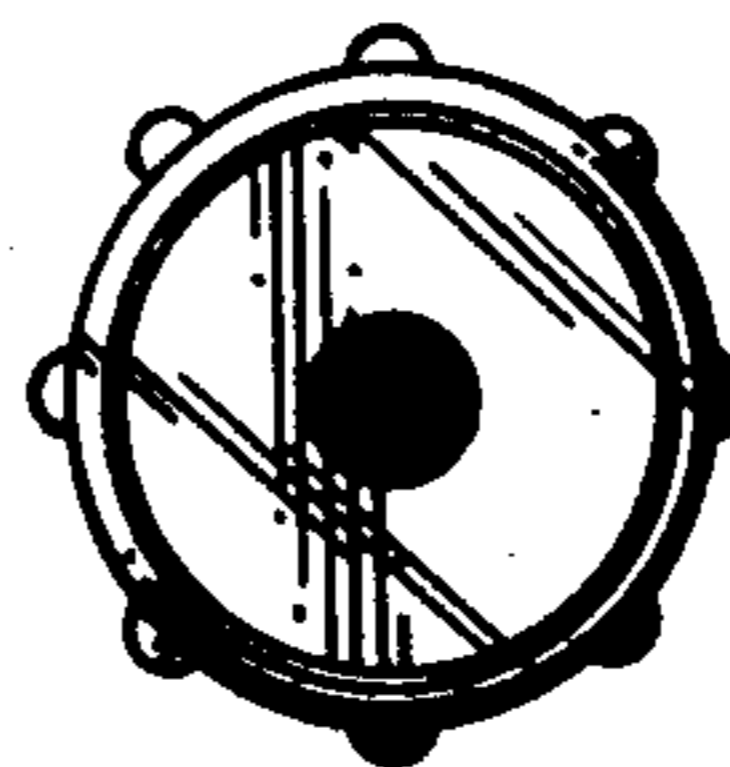

UNITED STATES PATENT AND TRADEMARK OFFICE
CERTIFICATE OF CORRECTION

PATENT NO. : Des. 251,502

DATED : April 3, 1979

INVENTOR(S) : Mark M. Bridle et al.

It is certified that error appears in the above-identified patent and that said Letters Patent are hereby corrected as shown below:

On the cover sheet Item (75) inventors' should read

-- Mark M. Bridle, Newport Beach, and John F. Cromelin,
Yorba Linda, both of Calif. ---

Signed and Sealed this

Twenty-first Day of August 1979

[SEAL]

Attest:

Attesting Officer

LUTRELLE F. PARKER

Acting Commissioner of Patents and Trademarks