

[54] **DIAGNOSTIC DEVICE FOR MEASURING BIOCHEMICAL CHARACTERISTICS OF MICROORGANISMS AND THE LIKE**

[75] **Inventors:** Donald P. Kronish, Rockaway; William D. Young, Montclair; Walter E. Jacobson, Morris Plains; Doris B. Taylor, Parsippany, all of N.J.

[73] **Assignee:** Warner-Lambert Company, Morris Plains, N.J.

[\*\*] **Term:** 14 Years

[21] **Appl. No.:** 787,658

[22] **Filed:** Apr. 14, 1977

[51] **Int. Cl.** ..... D24-02; D9-04

[52] **U.S. Cl.** ..... D24/17; D24/21; D24/31; D9/189

[58] **Field of Search** ..... 195/253 R, 103.5 M, 195/139, 127; 23/259, 253 R; D24/17, 21, 99, 31; D9/187, 189

[56] **References Cited**

**U.S. PATENT DOCUMENTS**

D. 225,525 12/1972 Johnson et al. .... D24/17

D. 240,052 5/1976 Varga ..... D24/17  
3,713,779 1/1973 Sirago et al. .... 23/259  
3,957,583 5/1976 Gibson et al. .... 195/127 X  
4,018,652 4/1977 Lanham et al. .... 195/103.5 M

*Primary Examiner*—Bernard Ansher

*Attorney, Agent, or Firm*—Albert H. Graddis

[57] **CLAIM**

An ornamental design for a diagnostic device for measuring biochemical characteristics of microorganisms and the like, substantially as shown and described.


## DESCRIPTION

FIG. 1 is a top perspective view of a diagnostic device for measuring biochemical characteristics of microorganisms and the like;

FIG. 2 is a side elevational view of the diagnostic device for measuring biochemical characteristics of microorganisms and the like;

FIG. 3 is a top plan view of the diagnostic device for measuring biochemical characteristics of microorganisms and the like of FIG. 1; and

FIG. 4 is a rear elevational view of the diagnostic device for measuring biochemical characteristics of microorganisms and the like of FIG. 1 with the cover closed.

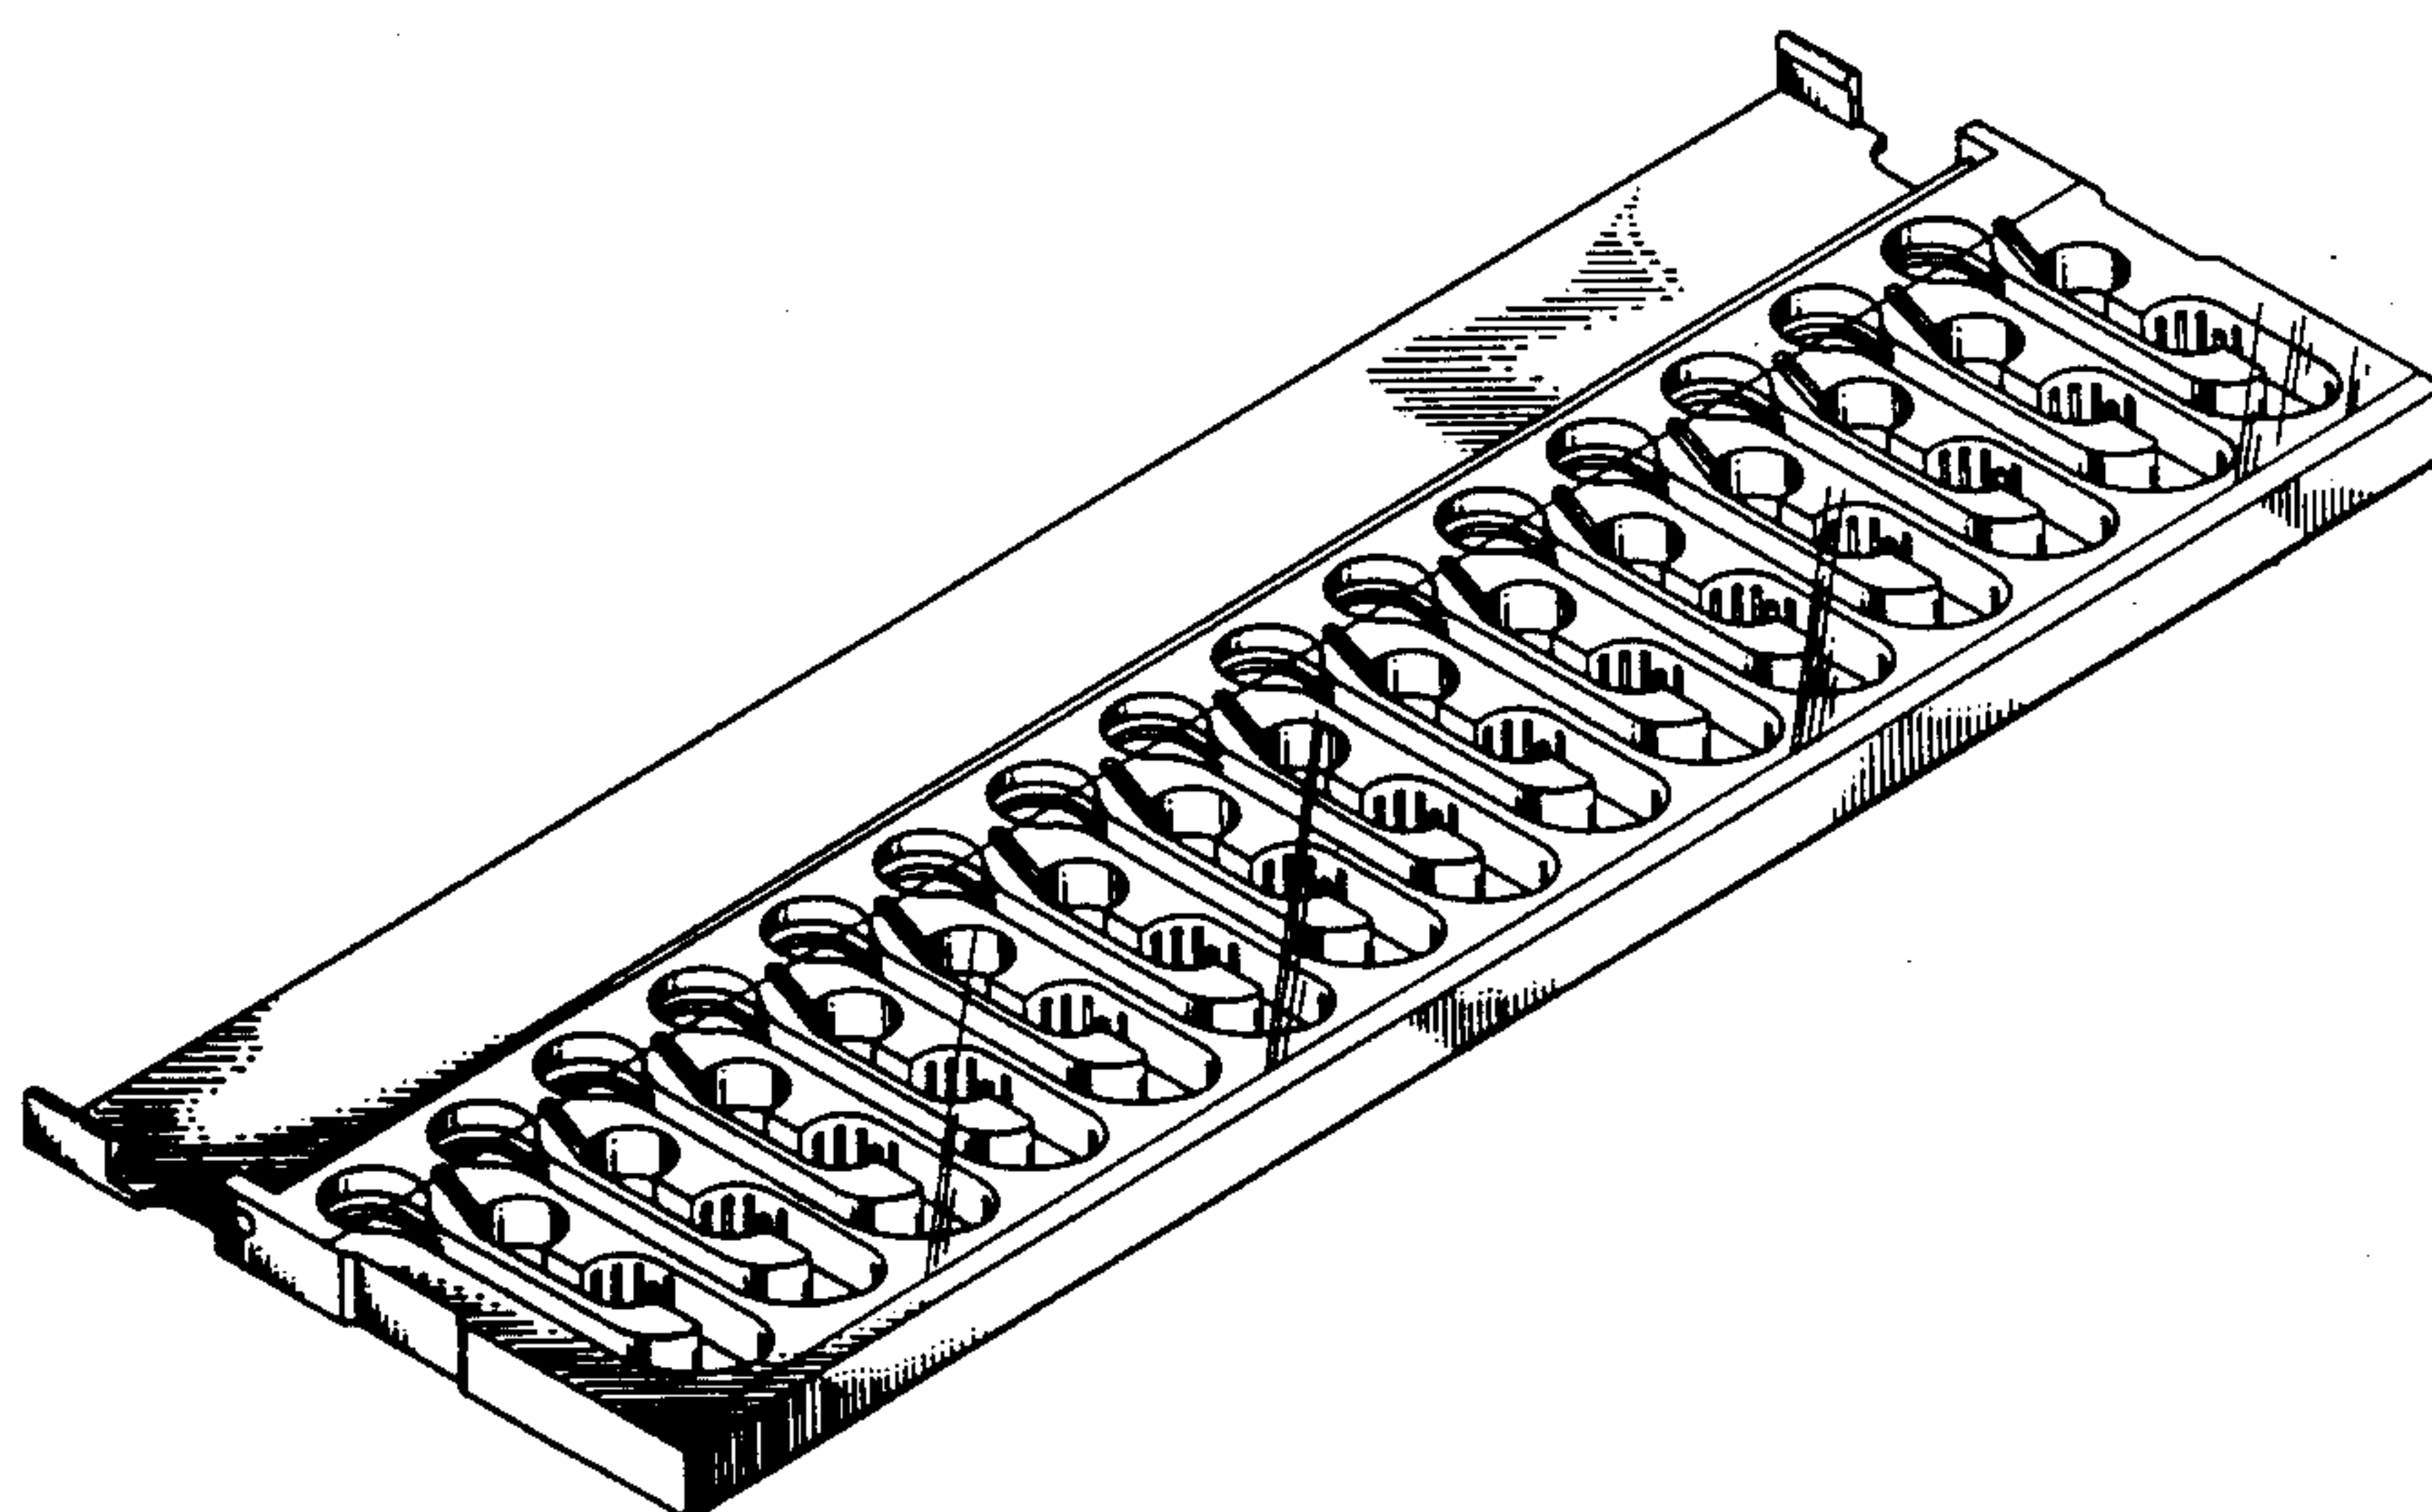

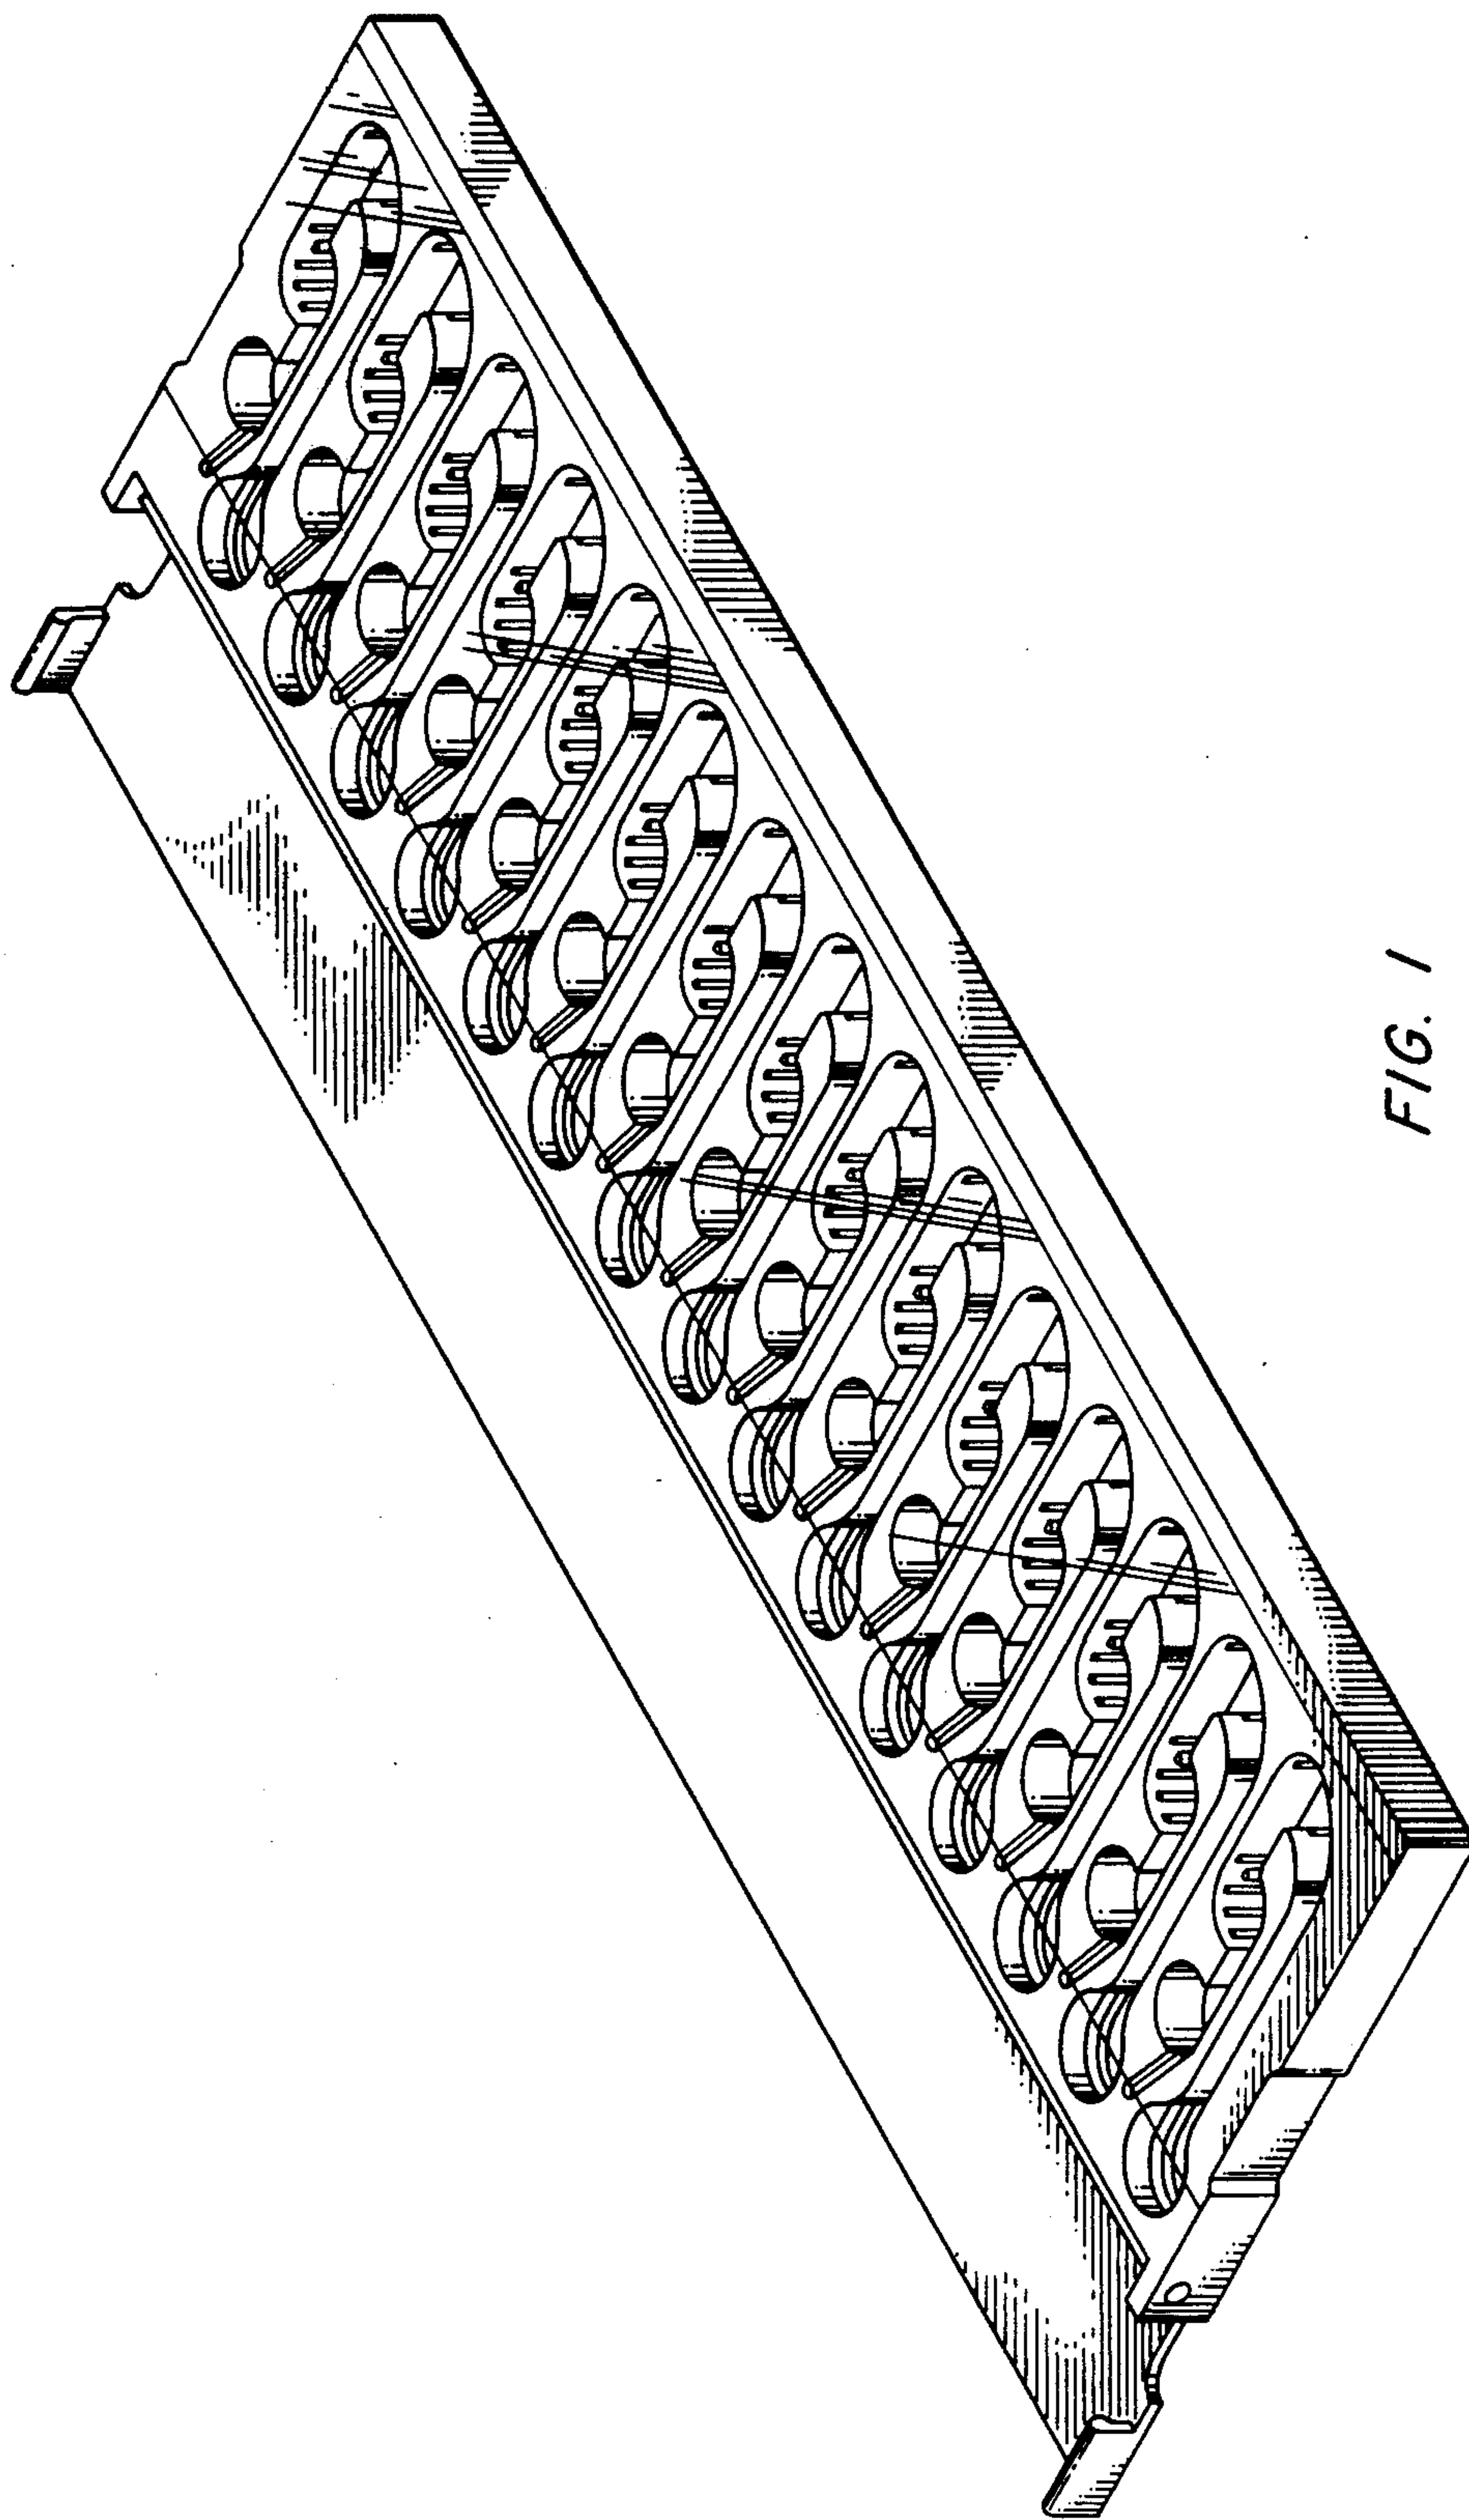


FIG. 1



FIG. 4

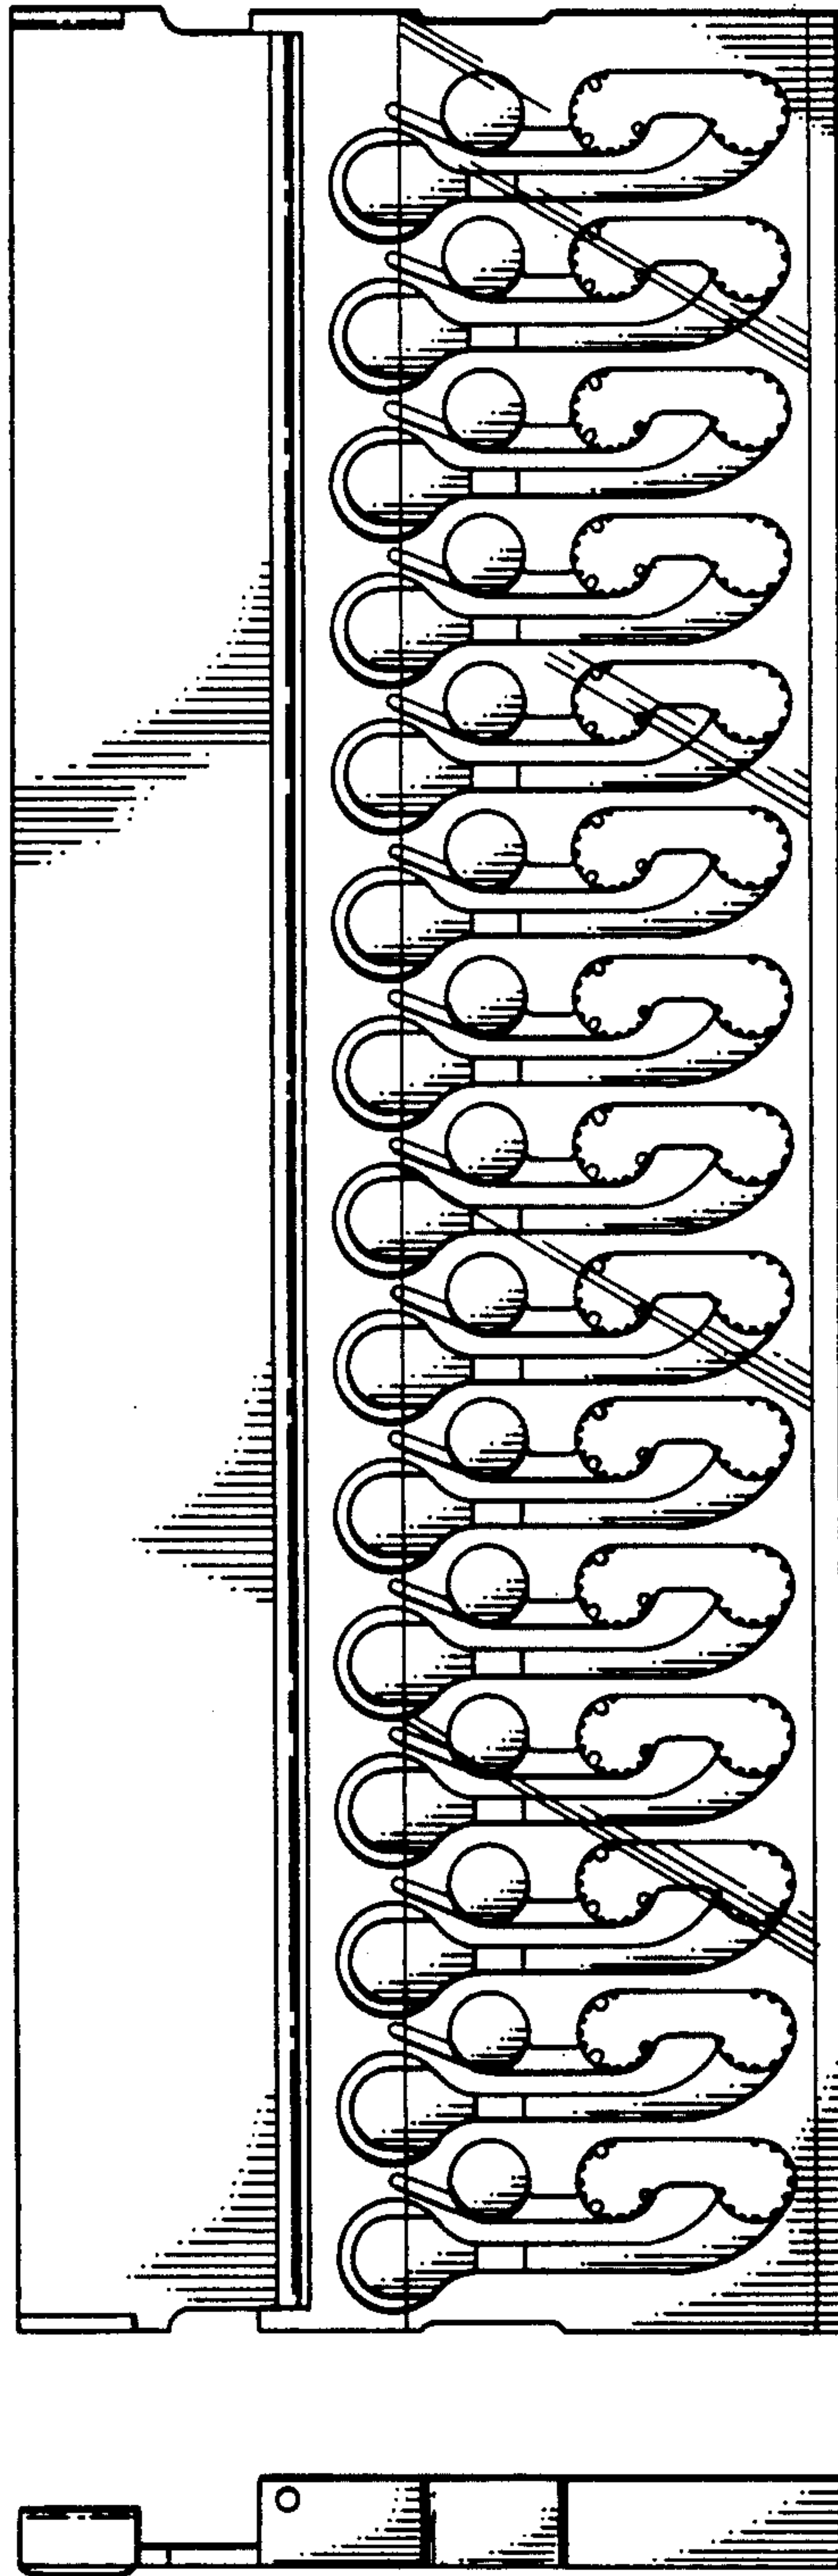


FIG. 3



FIG. 2