

[54] **DIAGNOSTIC DEVICE FOR MEASURING BIOCHEMICAL CHARACTERISTICS OF MICROORGANISMS AND THE LIKE**

D. 240,052	5/1976	Varga	D24/17
3,713,779	1/1973	Sirago et al.	23/259
3,957,583	5/1976	Gibson et al.	195/127 X
4,018,652	4/1977	Lanham et al.	195/103.5 M

[75] **Inventors:** Donald P. Kronish, Rockaway; William D. Young, Montclair; Walter E. Jacobson, Morris Plains; Doris B. Taylor, Parsippany, all of N.J.

Primary Examiner—Bernard Ansher
Attorney, Agent, or Firm—Albert H. Graddis

[73] **Assignee:** Warner-Lambert Company, Morris Plains, N.J.

[57] **CLAIM**

An ornamental design for a diagnostic device for measuring biochemical characteristics of microorganisms and the like, substantially as shown and described.

[**] **Term:** 14 Years

DESCRIPTION

[21] **Appl. No.:** 787,658

FIG. 1 is a top perspective view of a diagnostic device for measuring biochemical characteristics of microorganisms and the like;

[22] **Filed:** Apr. 14, 1977

FIG. 2 is a side elevational view of the diagnostic device for measuring biochemical characteristics of microorganisms and the like;

[51] **Int. Cl.** D24—02; D9—04

[52] **U.S. Cl.** D24/17; D24/21; D24/31; D9/189

[58] **Field of Search** 195/253 R, 103.5 M, 195/139, 127; 23/259, 253 R; D24/17, 21, 99, 31; D9/187, 189


FIG. 3 is a top plan view of the diagnostic device for measuring biochemical characteristics of microorganisms and the like of FIG. 1; and

FIG. 4 is a rear elevational view of the diagnostic device for measuring biochemical characteristics of microorganisms and the like of FIG. 1 with the cover closed.

[56] **References Cited**

U.S. PATENT DOCUMENTS

D. 225,525 12/1972 Johnson et al. D24/17

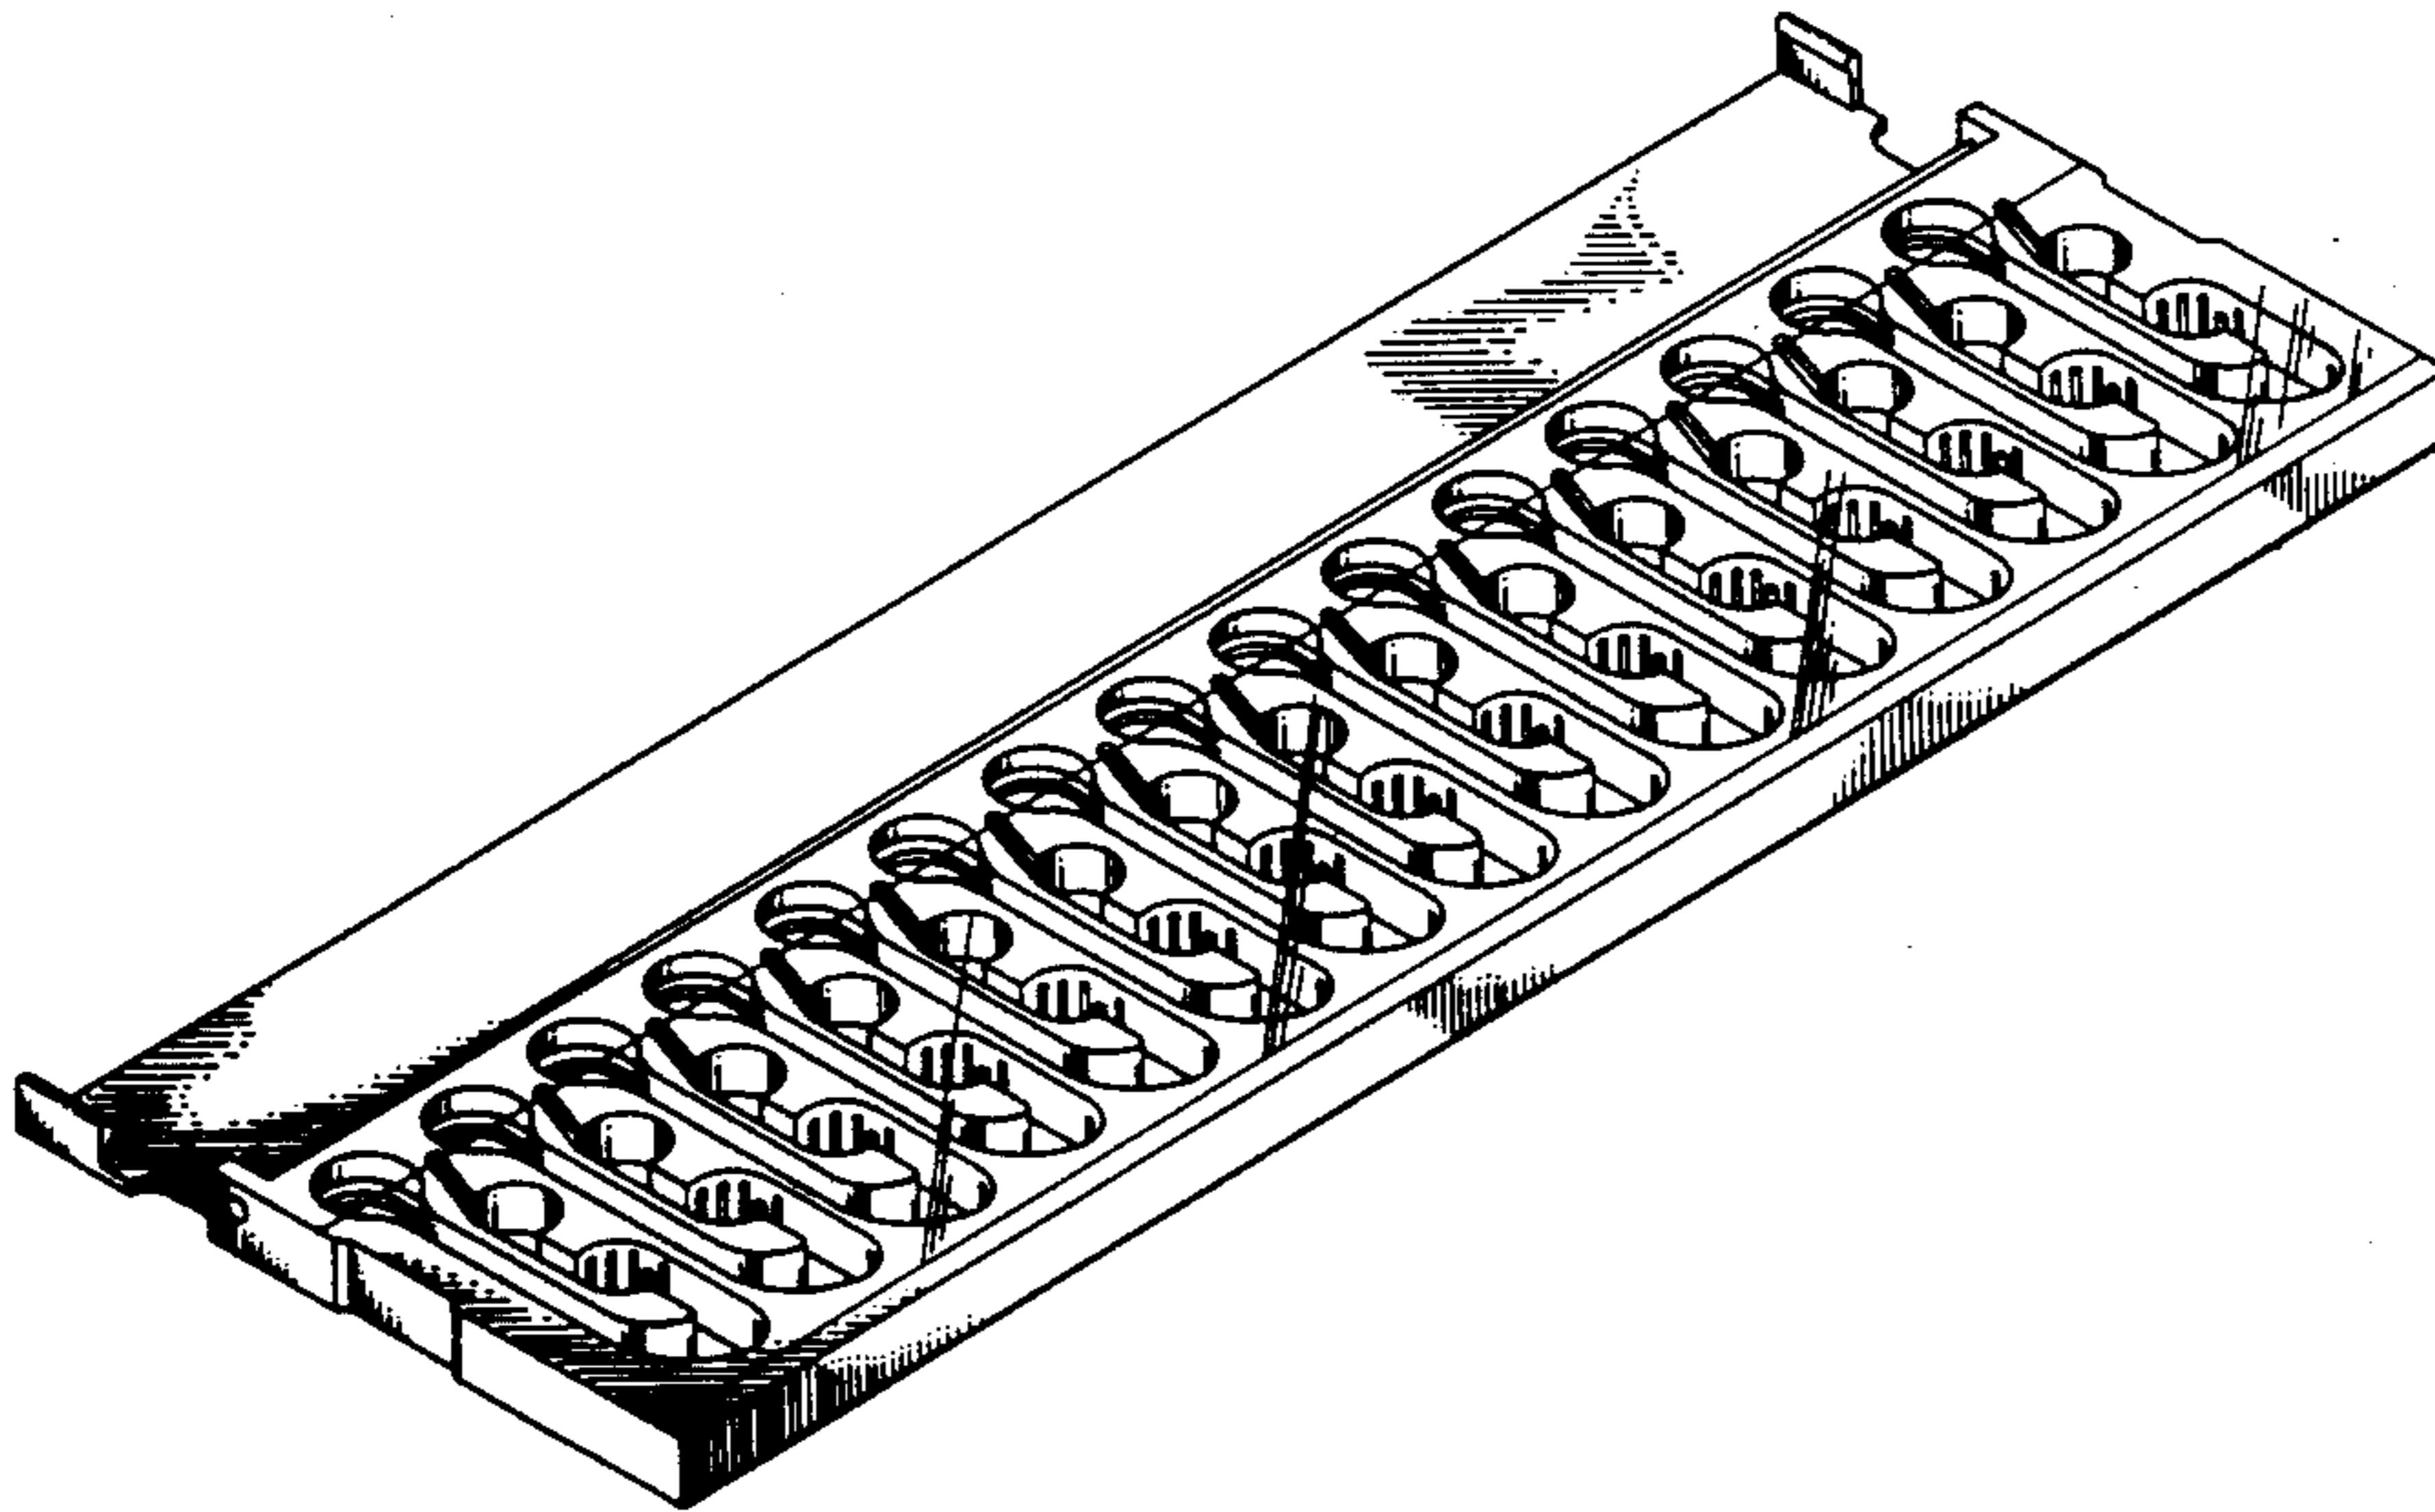

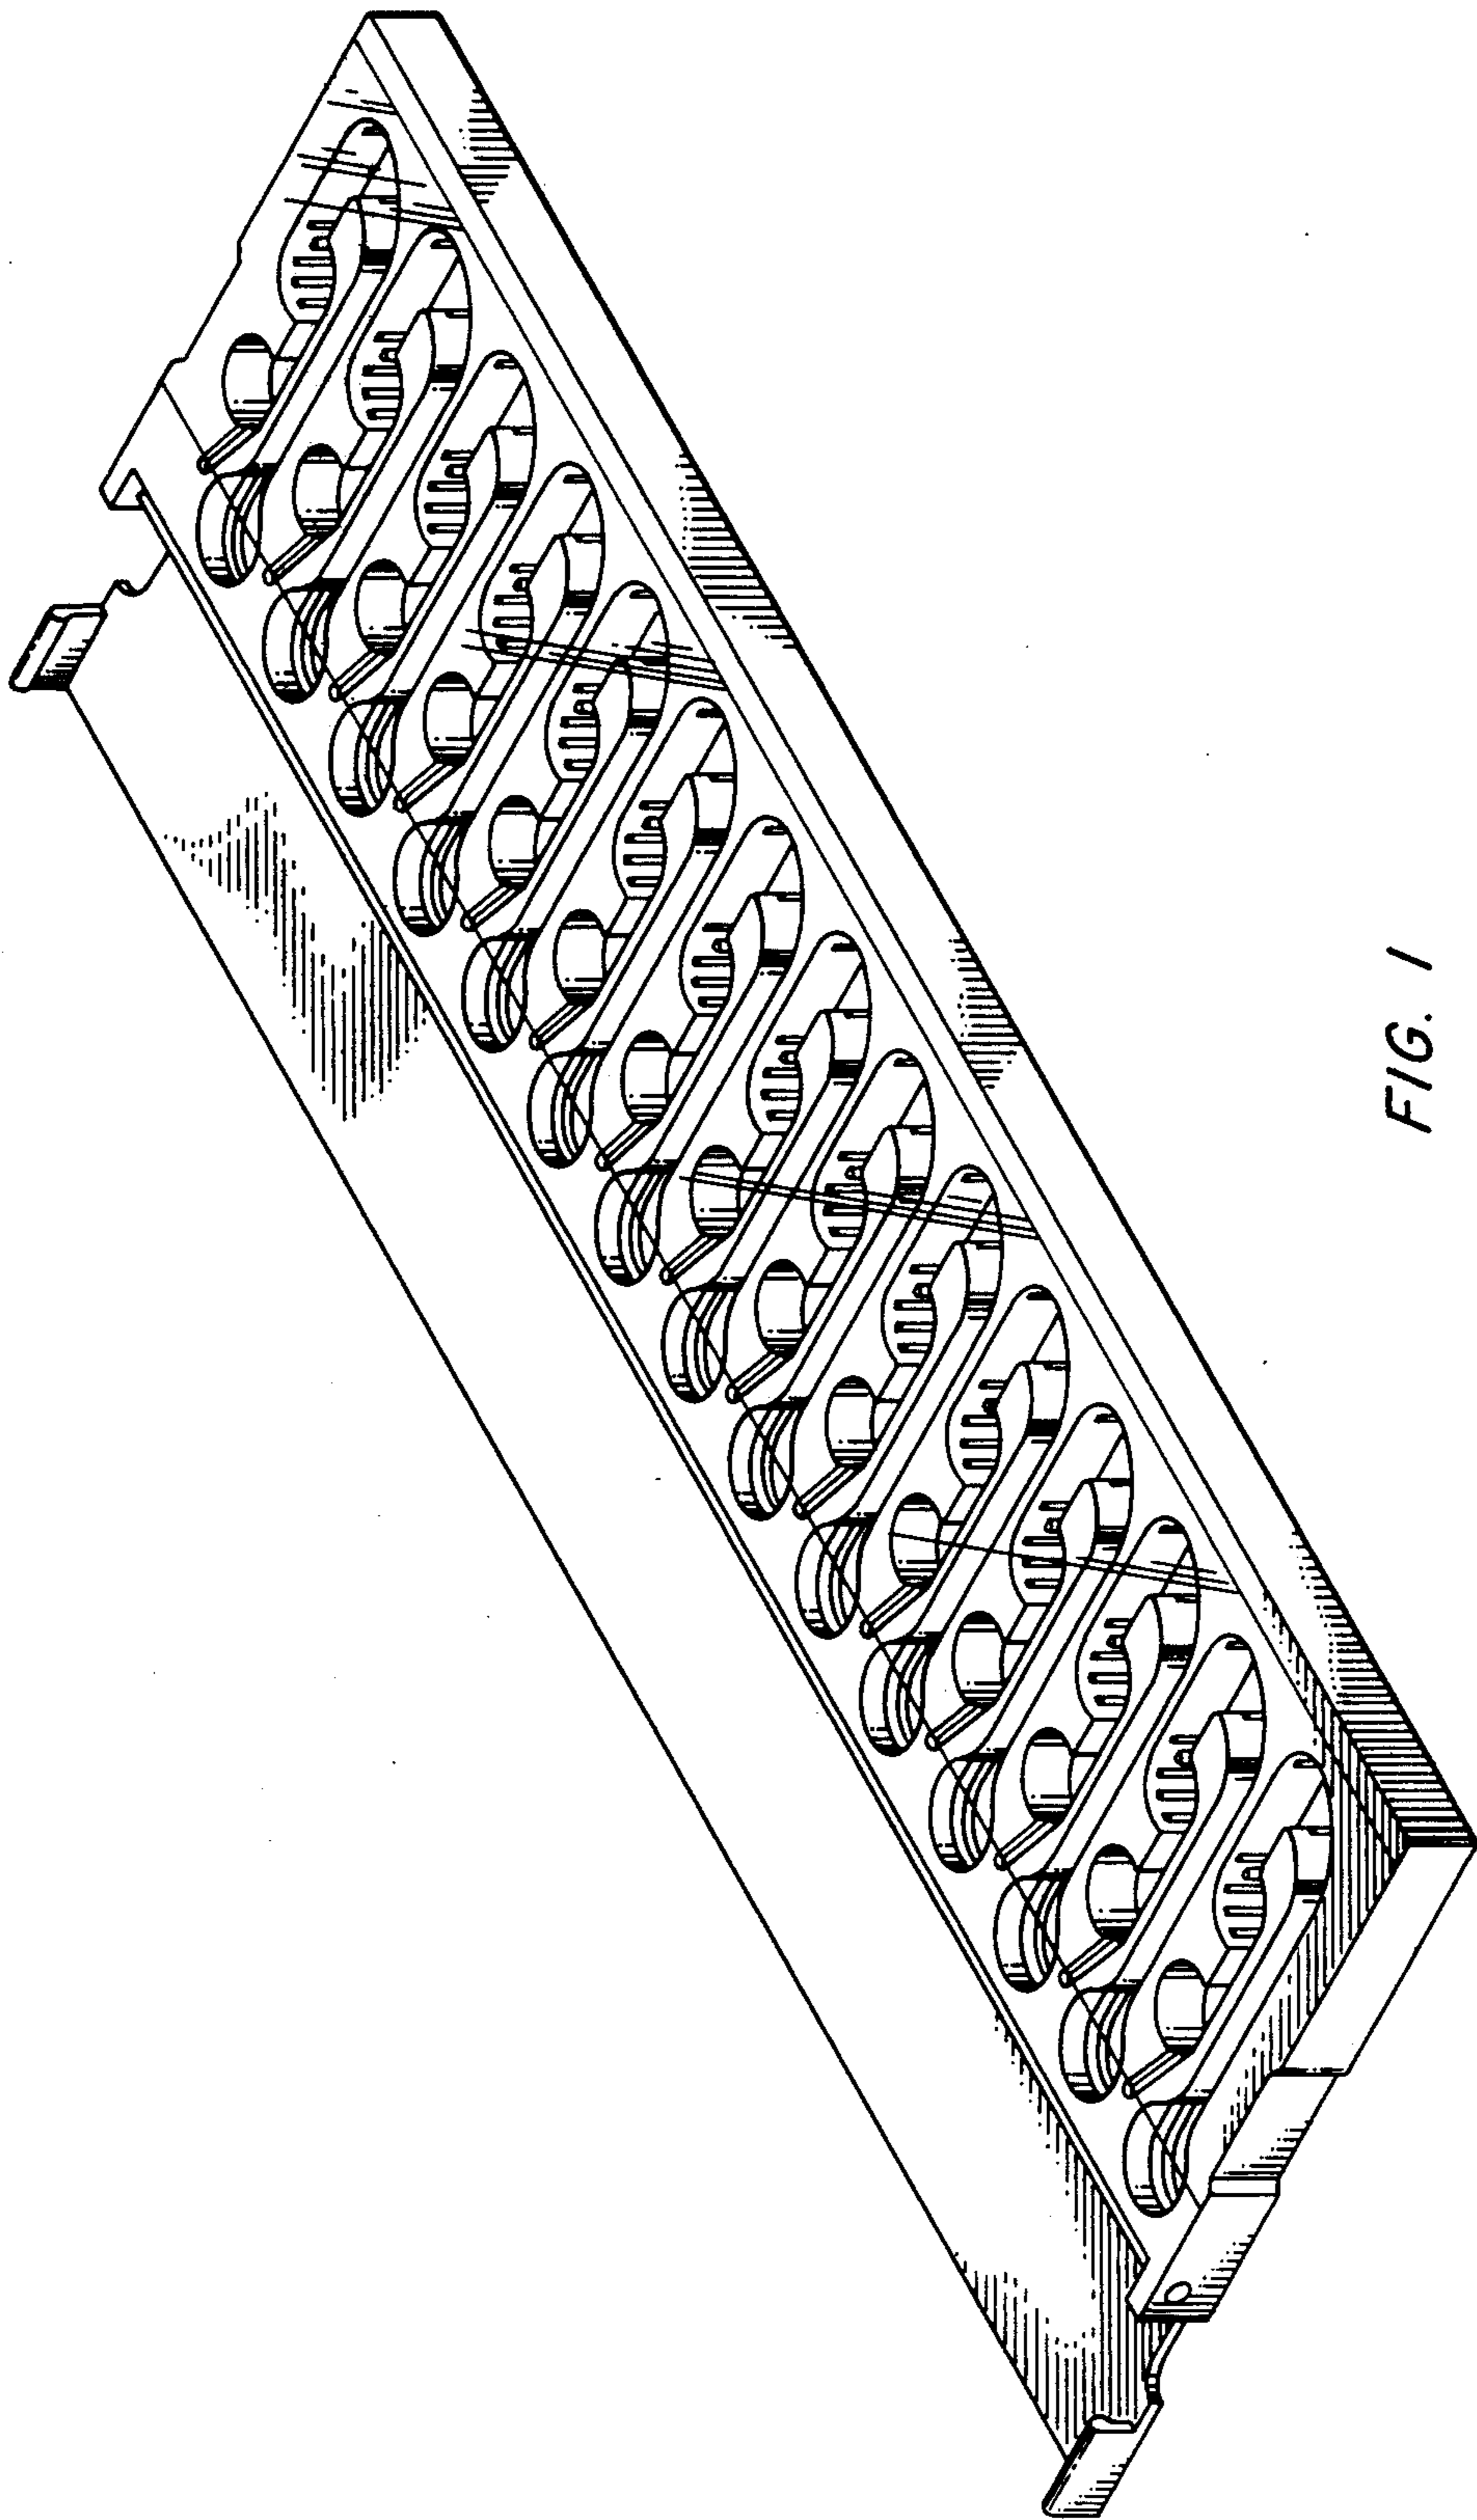


FIG. 1



FIG. 4

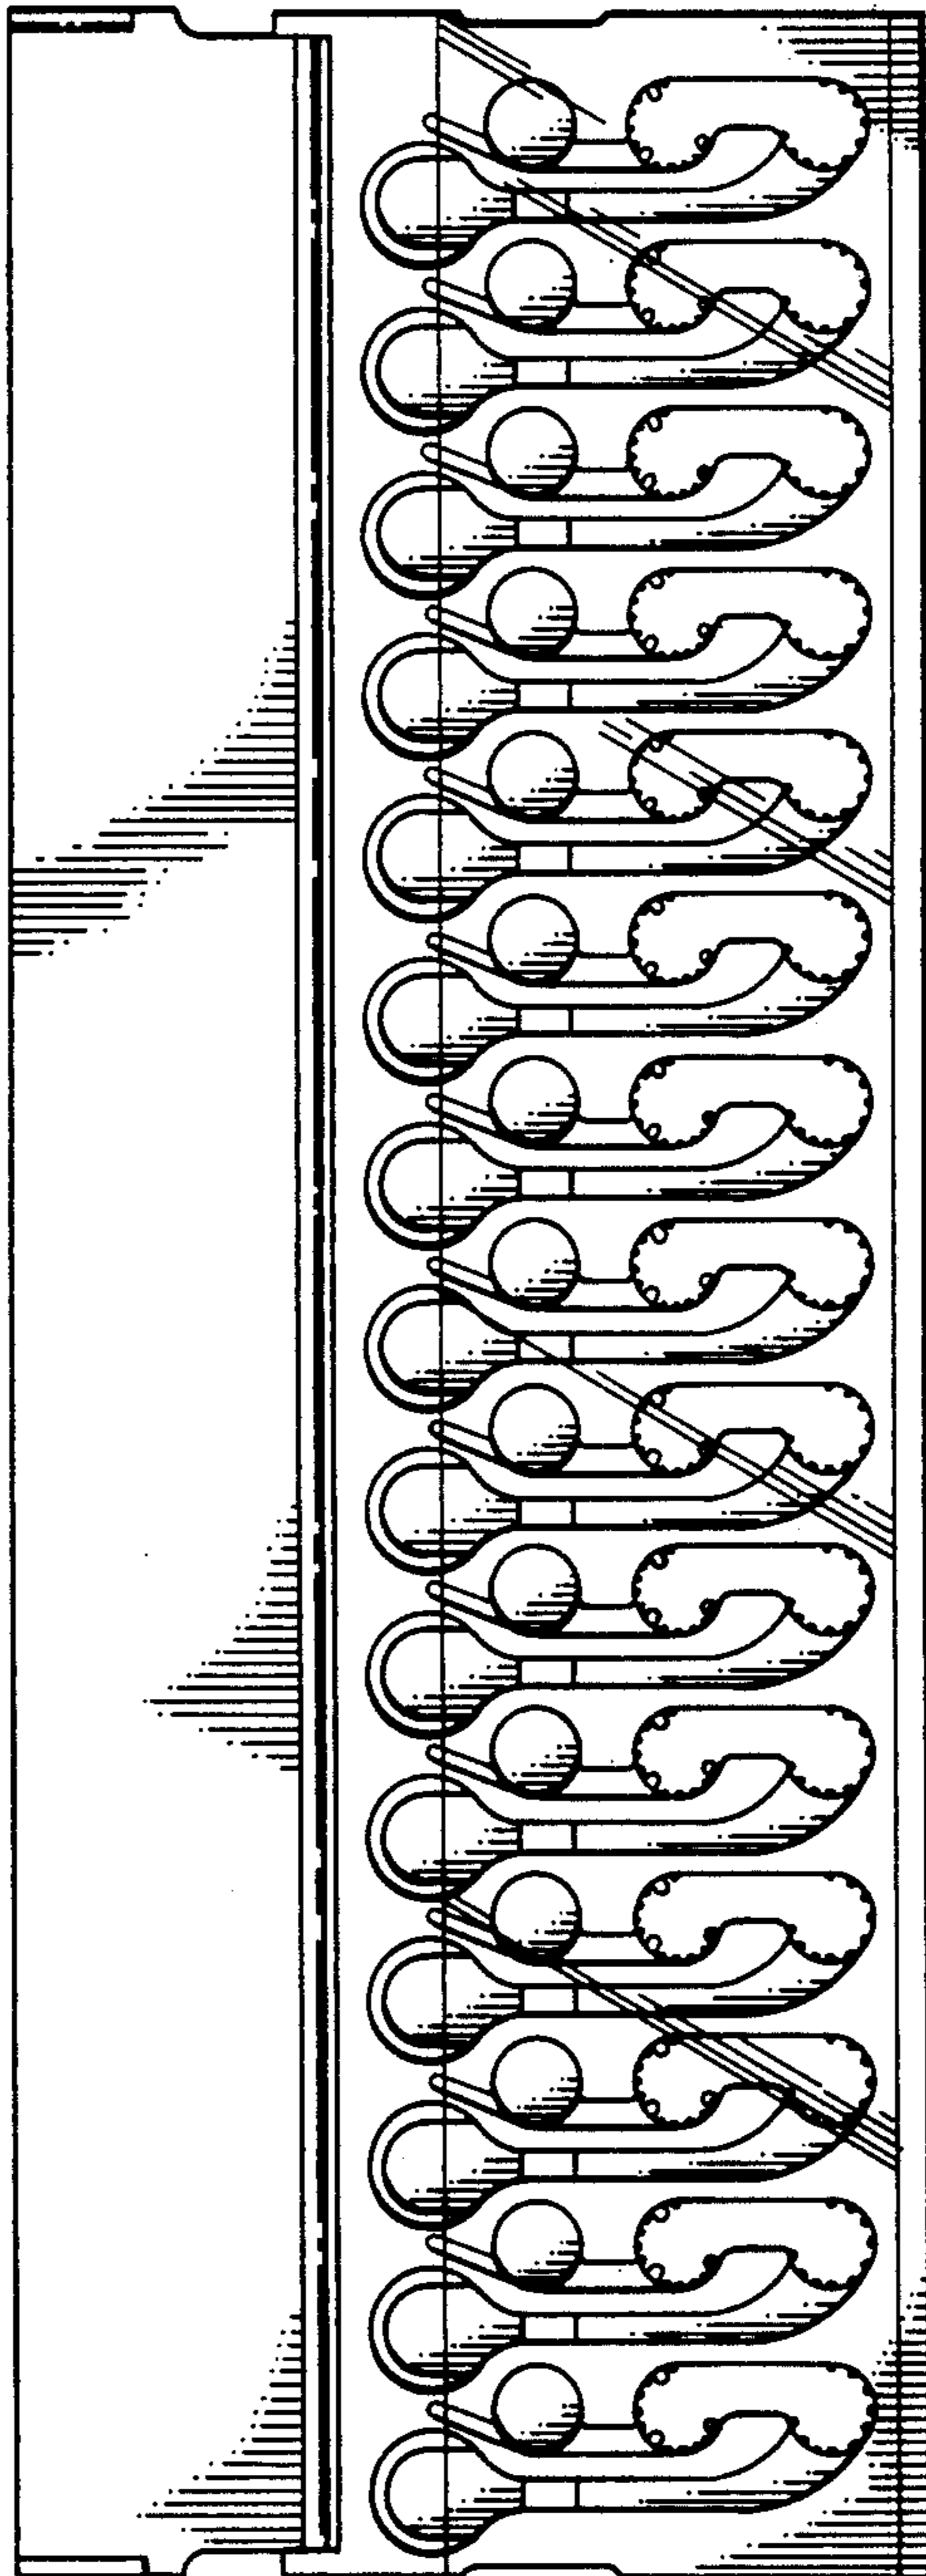


FIG. 3



FIG. 2