

[54] DUAL TERMINAL ELECTRODE FOR MEDICAL MONITORING

[75] Inventor: Albert J. Bevilacqua, Downers Grove, Ill.

[73] Assignee: C. R. Bard, Inc., Murray Hill, N.J.

[\*\*] Term: 14 Years

[21] Appl. No.: 839,265

[22] Filed: Oct. 4, 1977

[51] Int. Cl. .... D24-01

[52] U.S. Cl. .... D24/29

[58] Field of Search ..... D13/99, 10, 24; 339/36, 339/214 R, 214 C, 214 S, 217 R, 152; 429/96, 97, 98, 99, 100, 158, 178; 200/159 B, 165, 238, 284; 128/639, 640, 641, 644; D24/16, 25, 29

[56] References Cited

U.S. PATENT DOCUMENTS

2,700,087	1/1955	Stevens	200/284
3,370,987	2/1968	Rush	429/98
3,386,071	5/1968	Allen	339/36
3,834,373	9/1974	Sato	128/640
3,993,049	11/1976	Kater	128/640

FOREIGN PATENT DOCUMENTS

2415414 10/1974 Fed. Rep. of Germany ..... 128/639  
387831 2/1933 United Kingdom ..... 339/214 R

Primary Examiner—Susan J. Lucas  
Attorney, Agent, or Firm—Trexler, Wolters, Bushnell & Fosse, Ltd.

[57] CLAIM

The ornamental design for a dual terminal electrode for medical monitoring, substantially as shown and described.

DESCRIPTION

FIG. 1 is a perspective view showing the bottom or skin adhering surface of the dual terminal electrode for medical monitoring.

FIG. 2 is a plan view of the skin adhering surface of my electrode design;

FIG. 3 is a plan view of the opposite surface of said electrode from that shown in FIG. 2;

FIG. 4 is a side elevational view of the electrode of FIG. 1;

FIG. 5 is a front elevational view of the electrode as shown in FIG. 1.

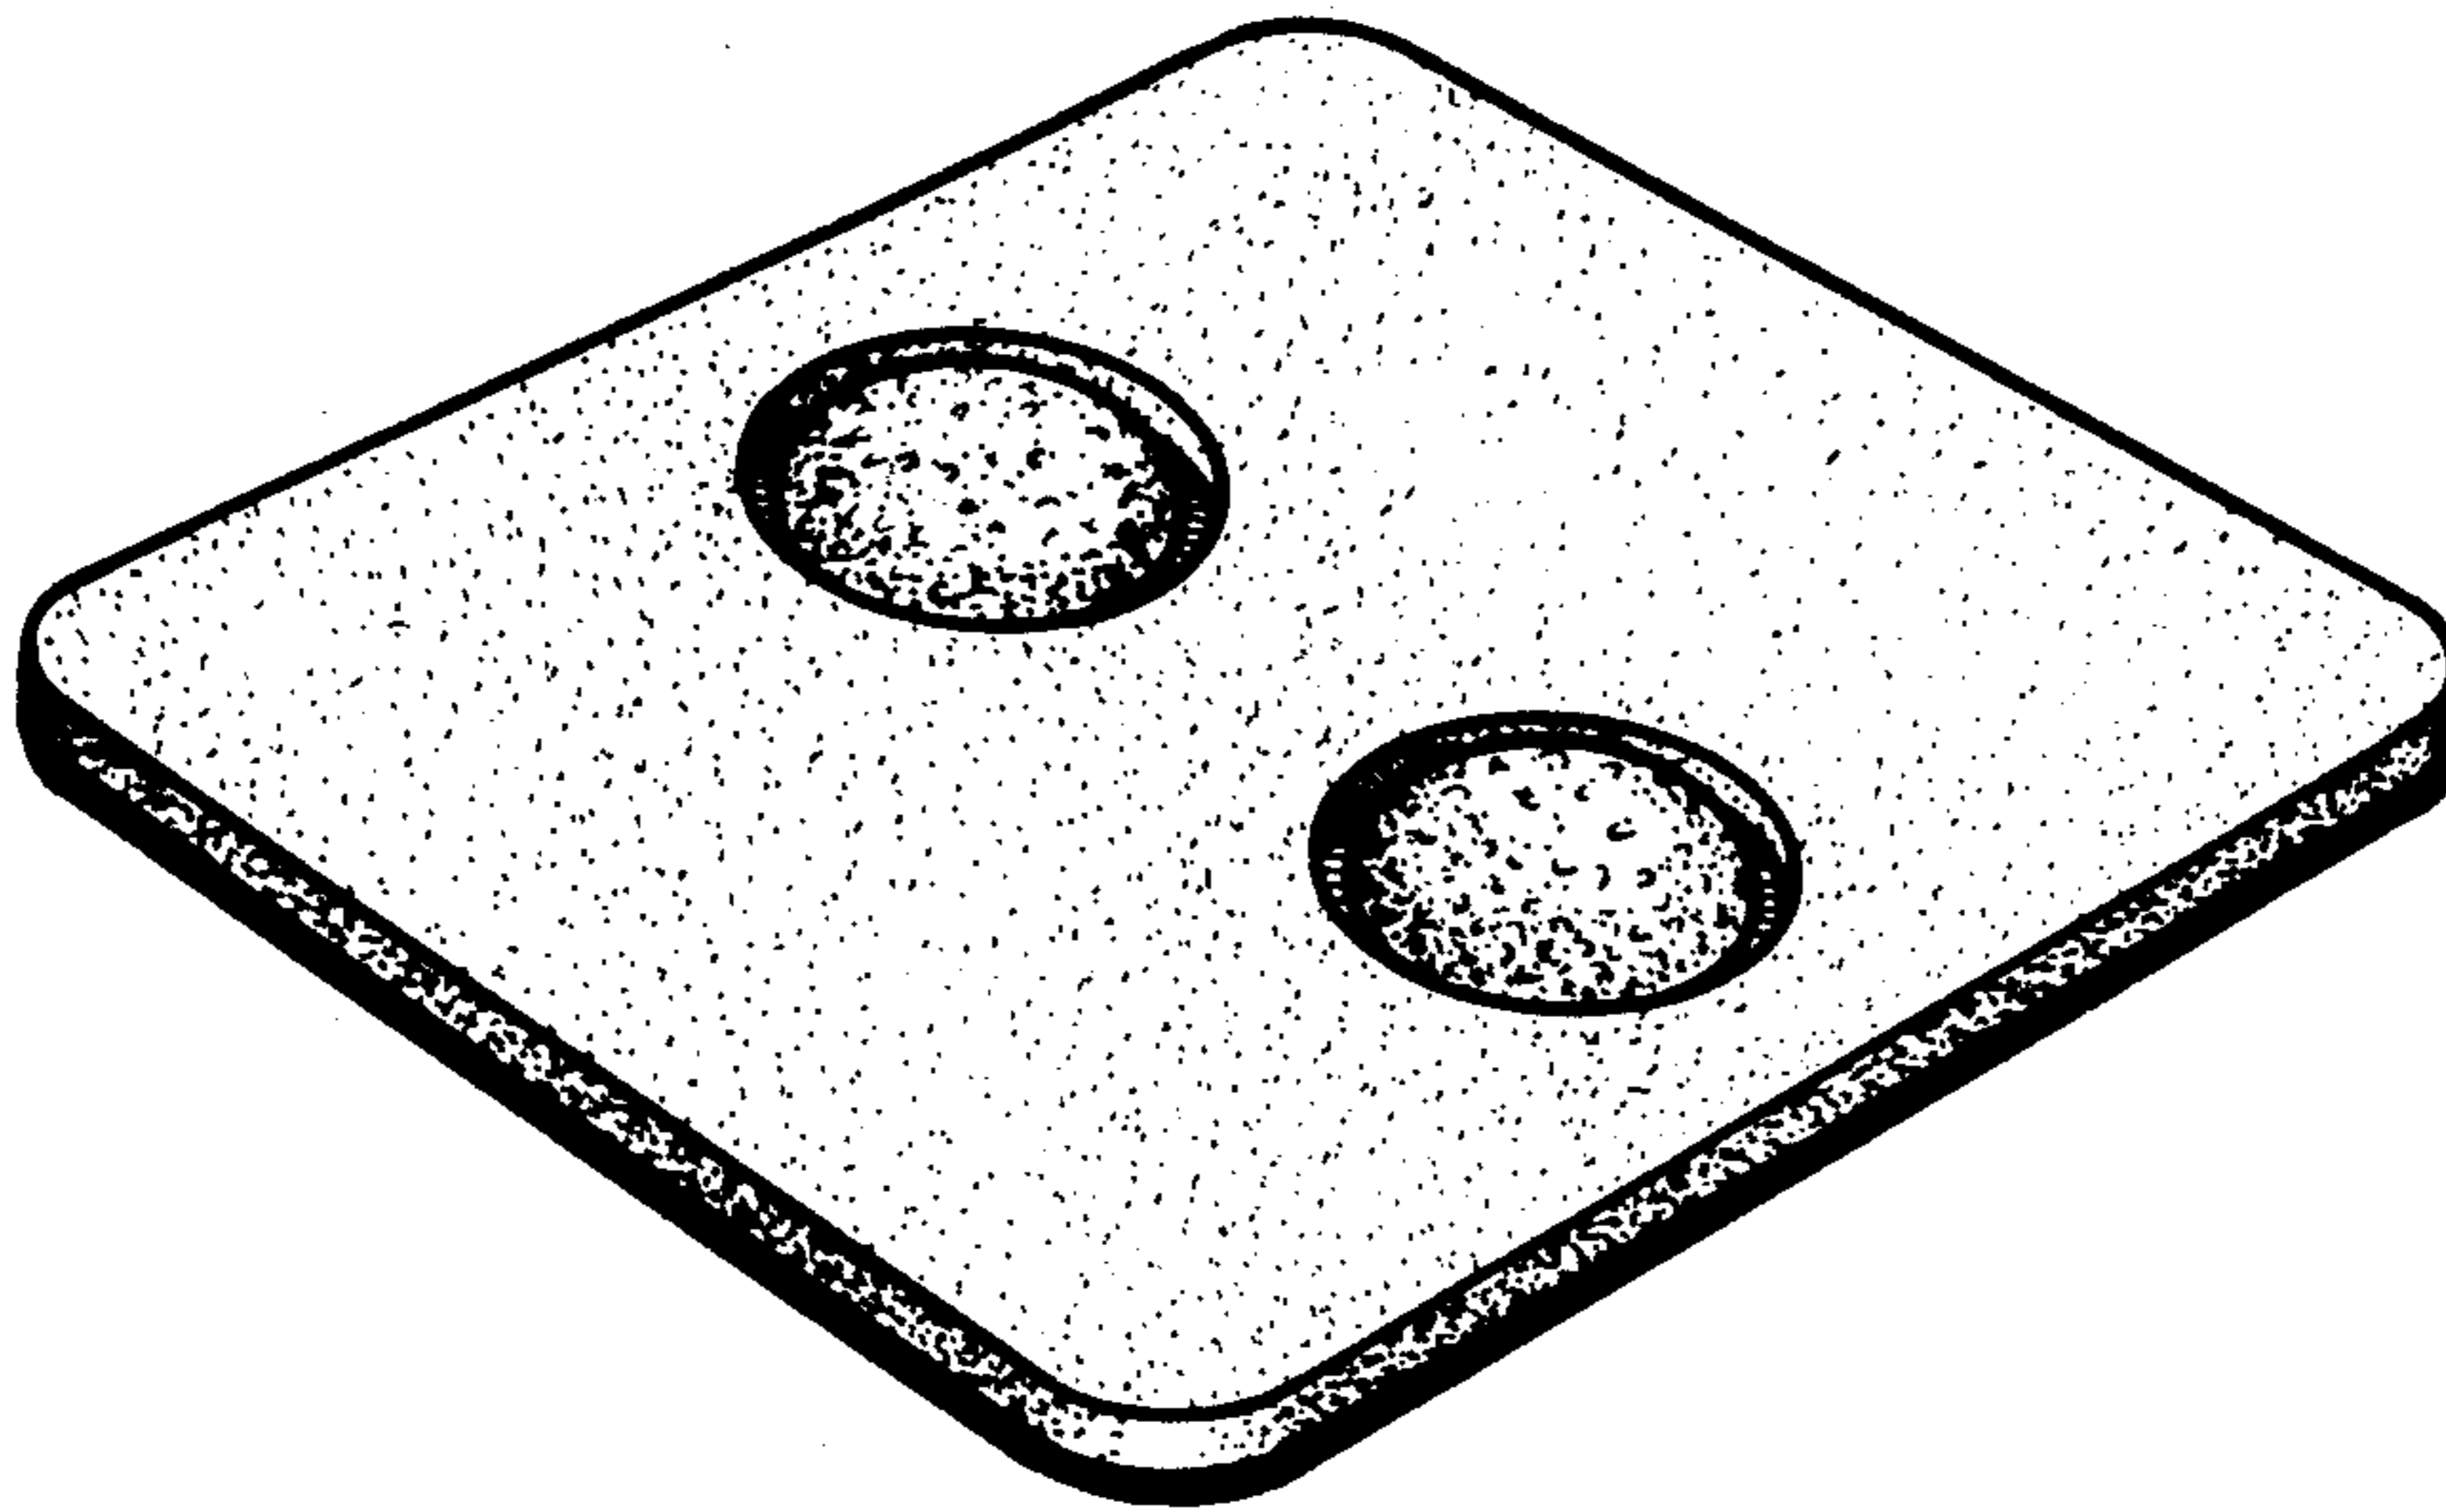


FIG. 1

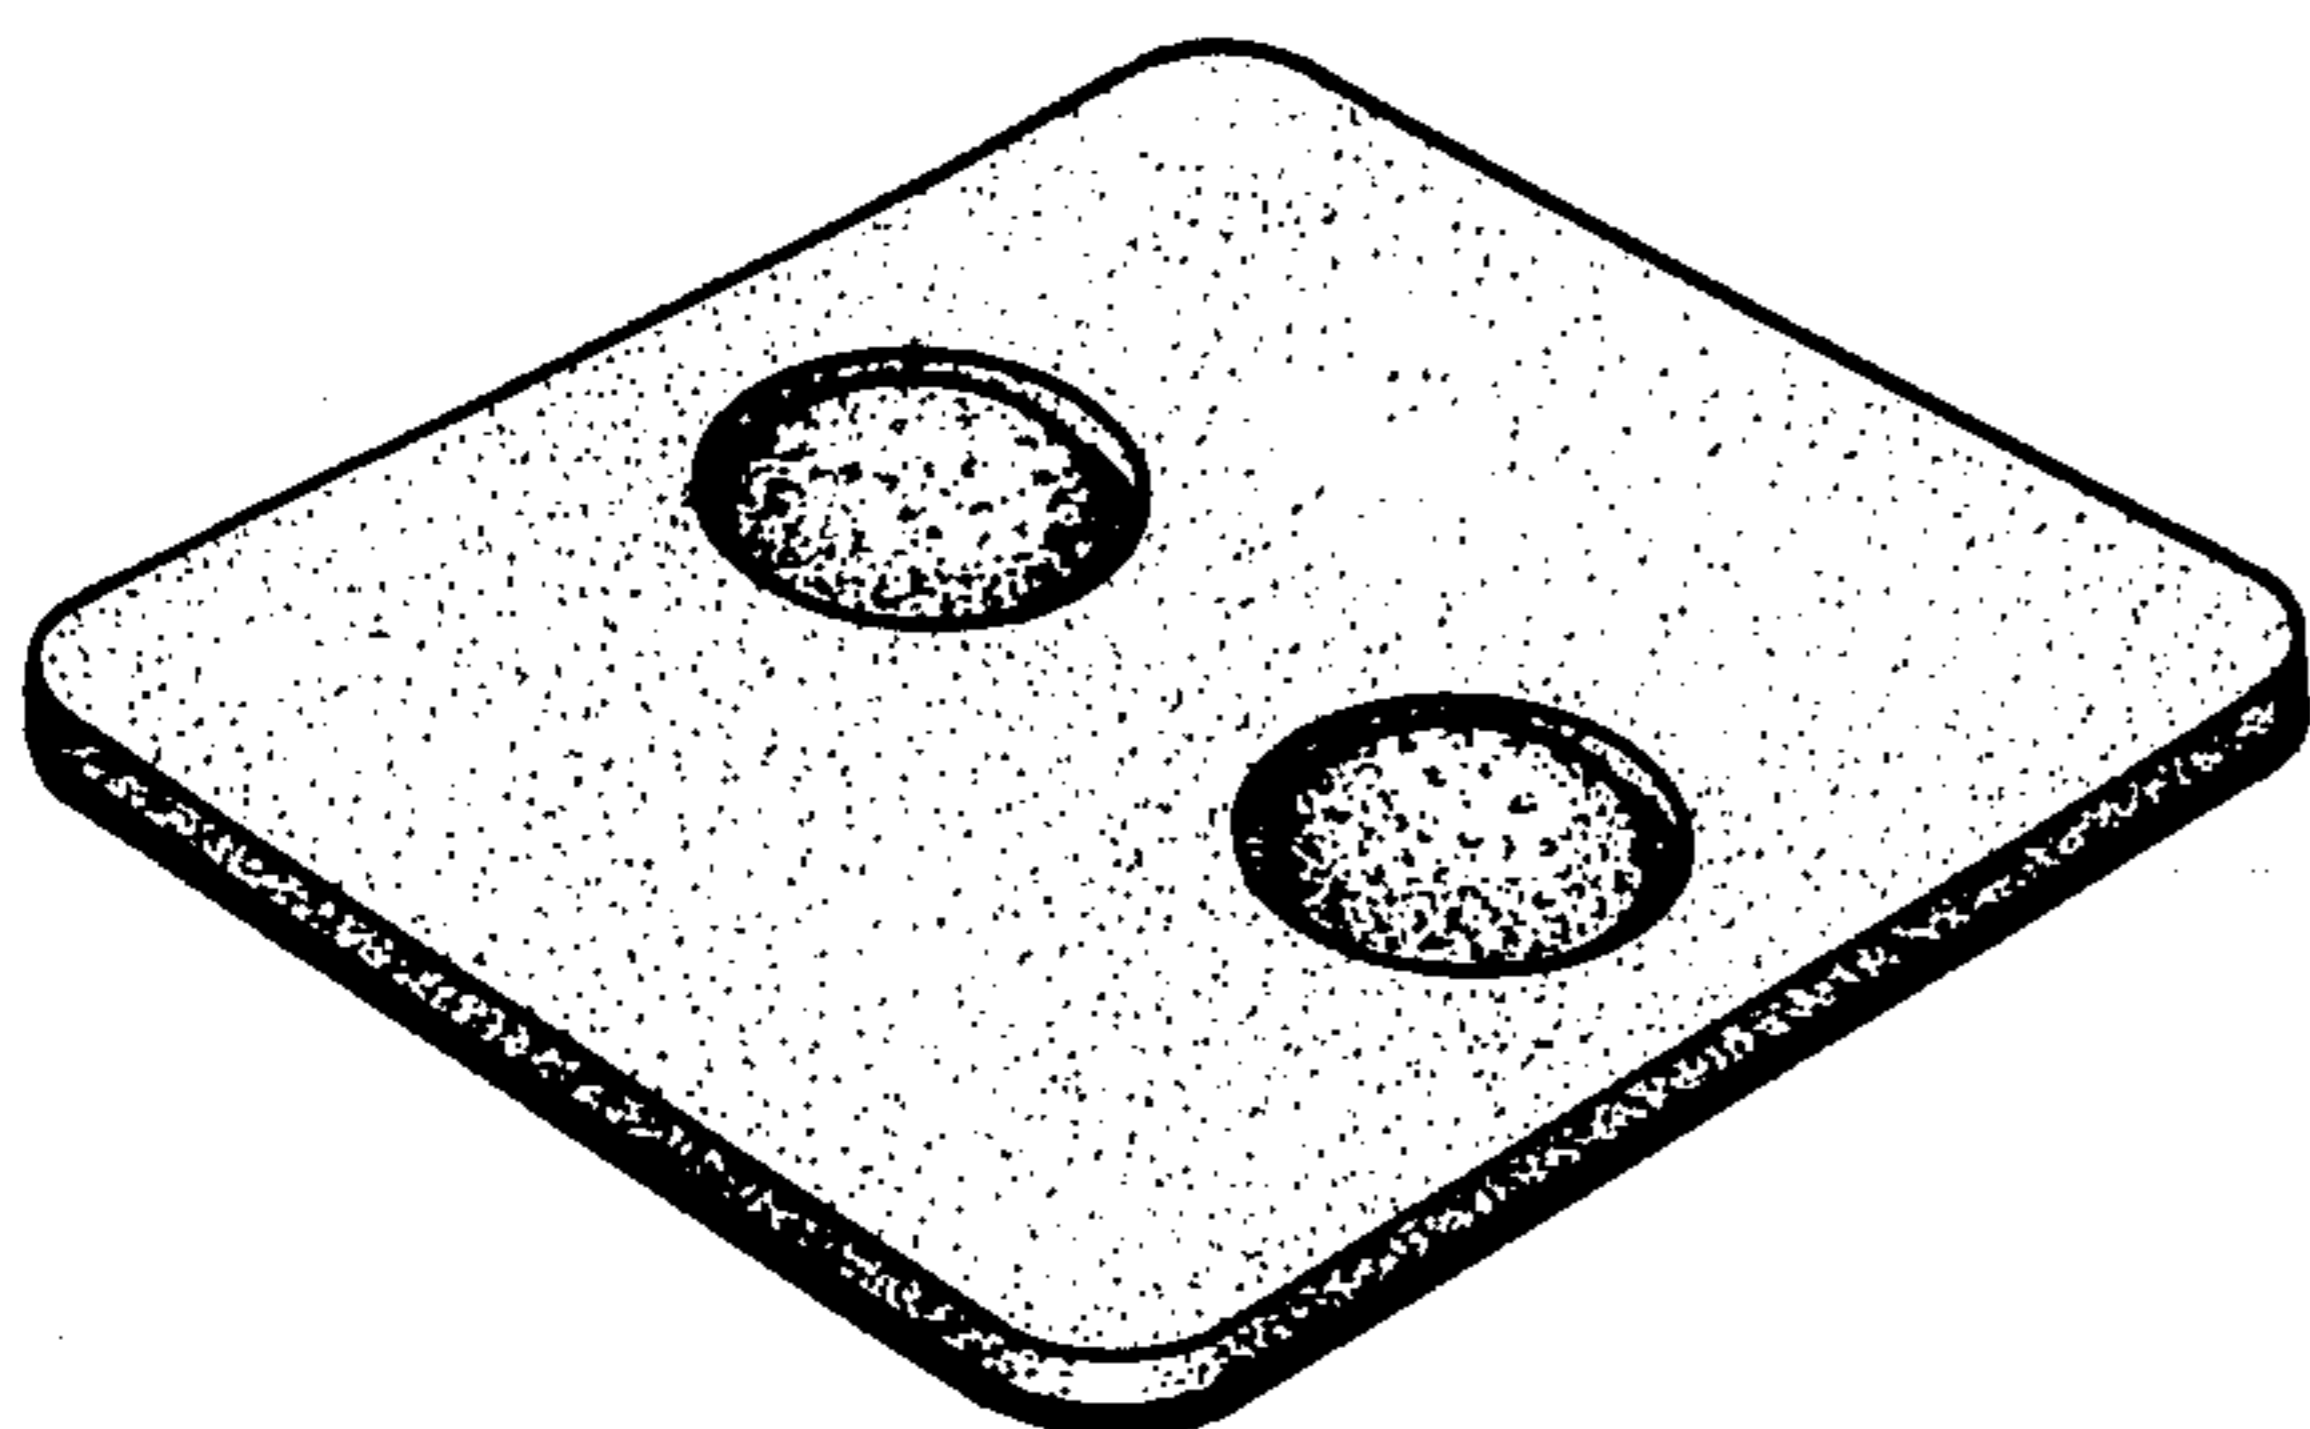


FIG. 2

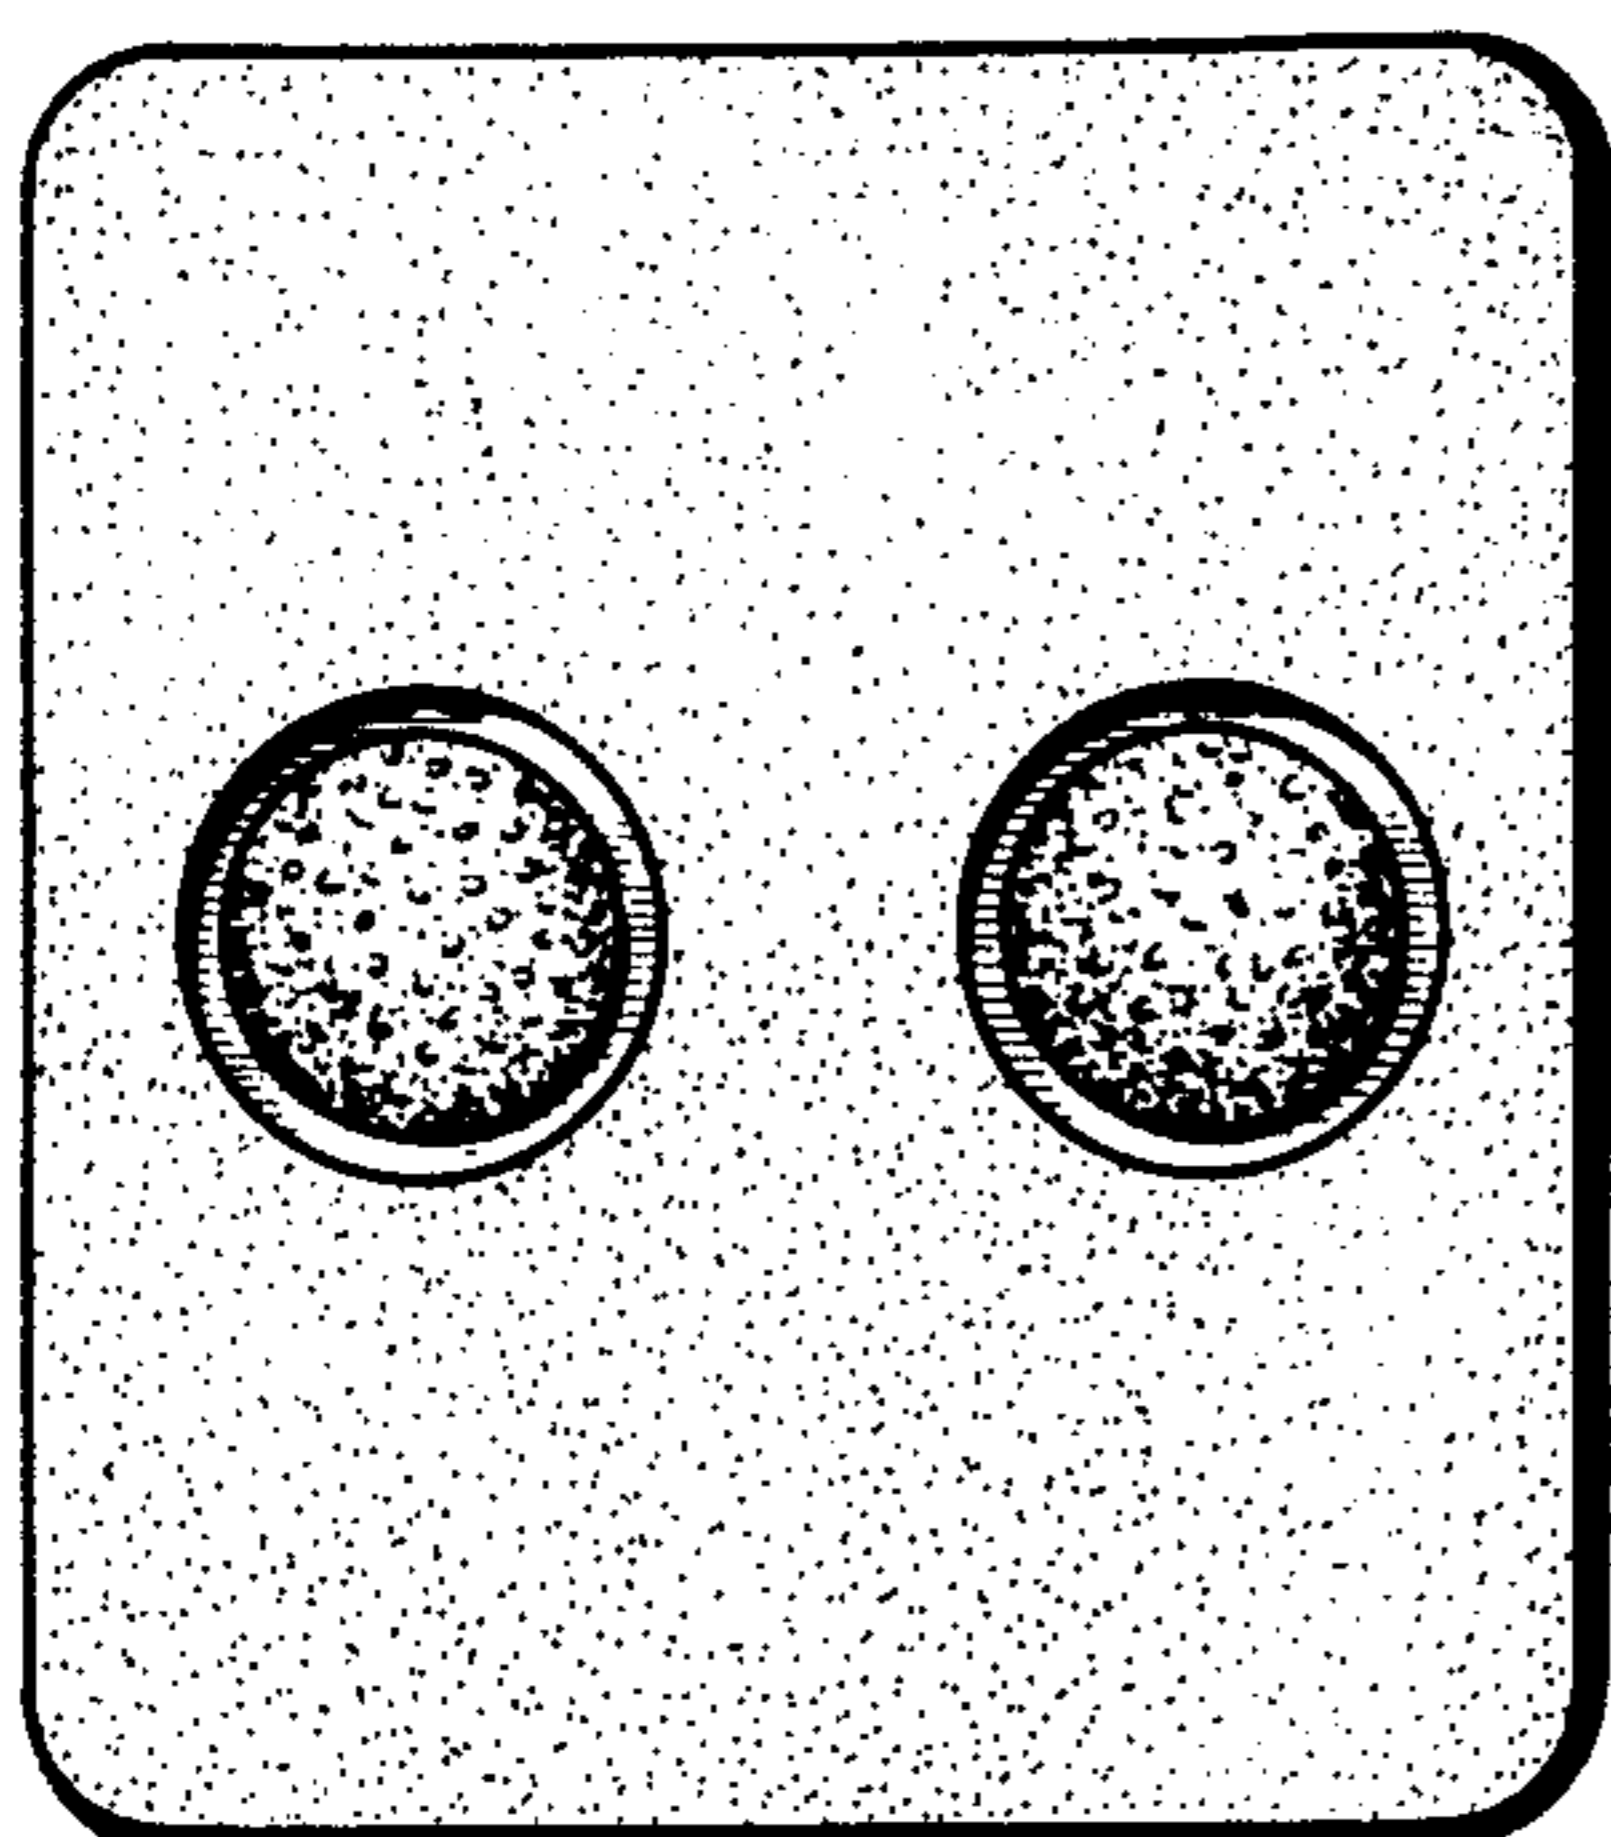


FIG. 3

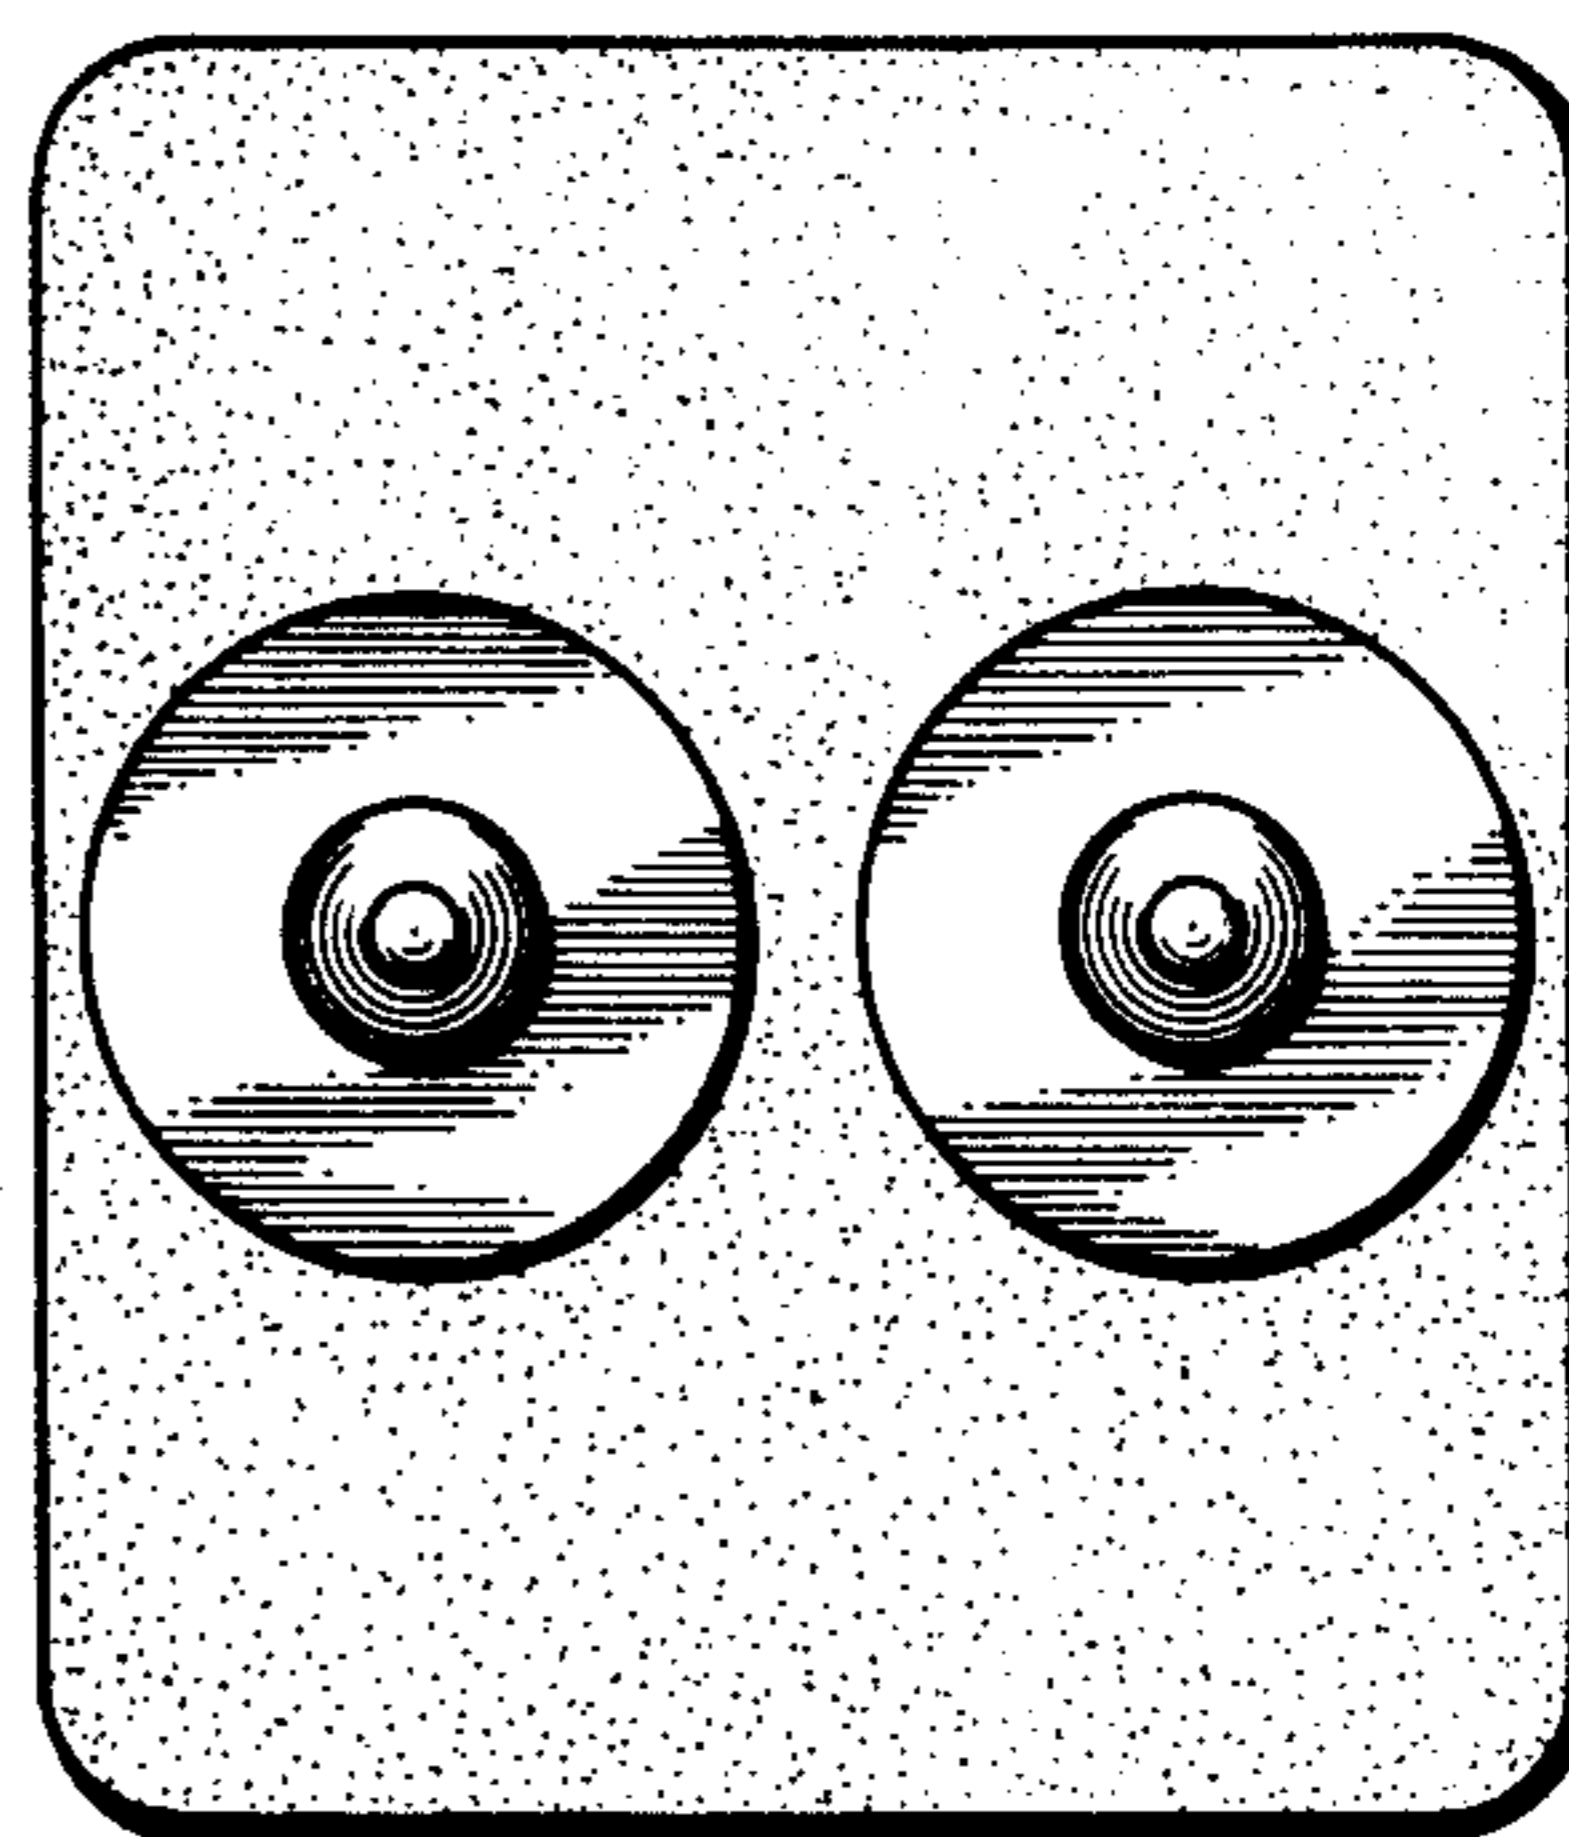


FIG. 4



FIG. 5

