

[54] DIALYZER

[75] Inventor: Henry Pande, Parker, Colo.

[73] Assignee: Hospal Medical Corporation, Littleton, Colo.

[\*\*] Term: 14 Years

[21] Appl. No.: 885,693

[22] Filed: Mar. 13, 1978

[51] Int. Cl. .... D24-01  
[52] U.S. Cl. .... D24/21; D24/17  
[58] Field of Search ..... 210/321 R, 321 A, 22 R, 210/22 A; D24/8, 17, 21

[56]

References Cited

U.S. PATENT DOCUMENTS

D. 216,849	3/1970	Carsello .....	D24/8
D. 239,881	5/1976	Morgan et al. ....	D24/17
D. 245,811	9/1977	Gics .....	D24/21
4,031,012	6/1977	Gics .....	210/321 A
4,108,764	4/1978	Kaneko et al. ....	210/321 A
4,141,835	2/1979	Schäel .....	210/321 A

Primary Examiner—Bernard Ansher  
Attorney, Agent, or Firm—Gerald D. Sharkin





[57]

CLAIM

The ornamental design for a dialyzer, as shown.

DESCRIPTION

FIG. 1 is a side elevation view of a dialyzer showing my new design;  
FIG. 2 is an end elevation thereof; and  
FIG. 3 is a top plan view thereof.

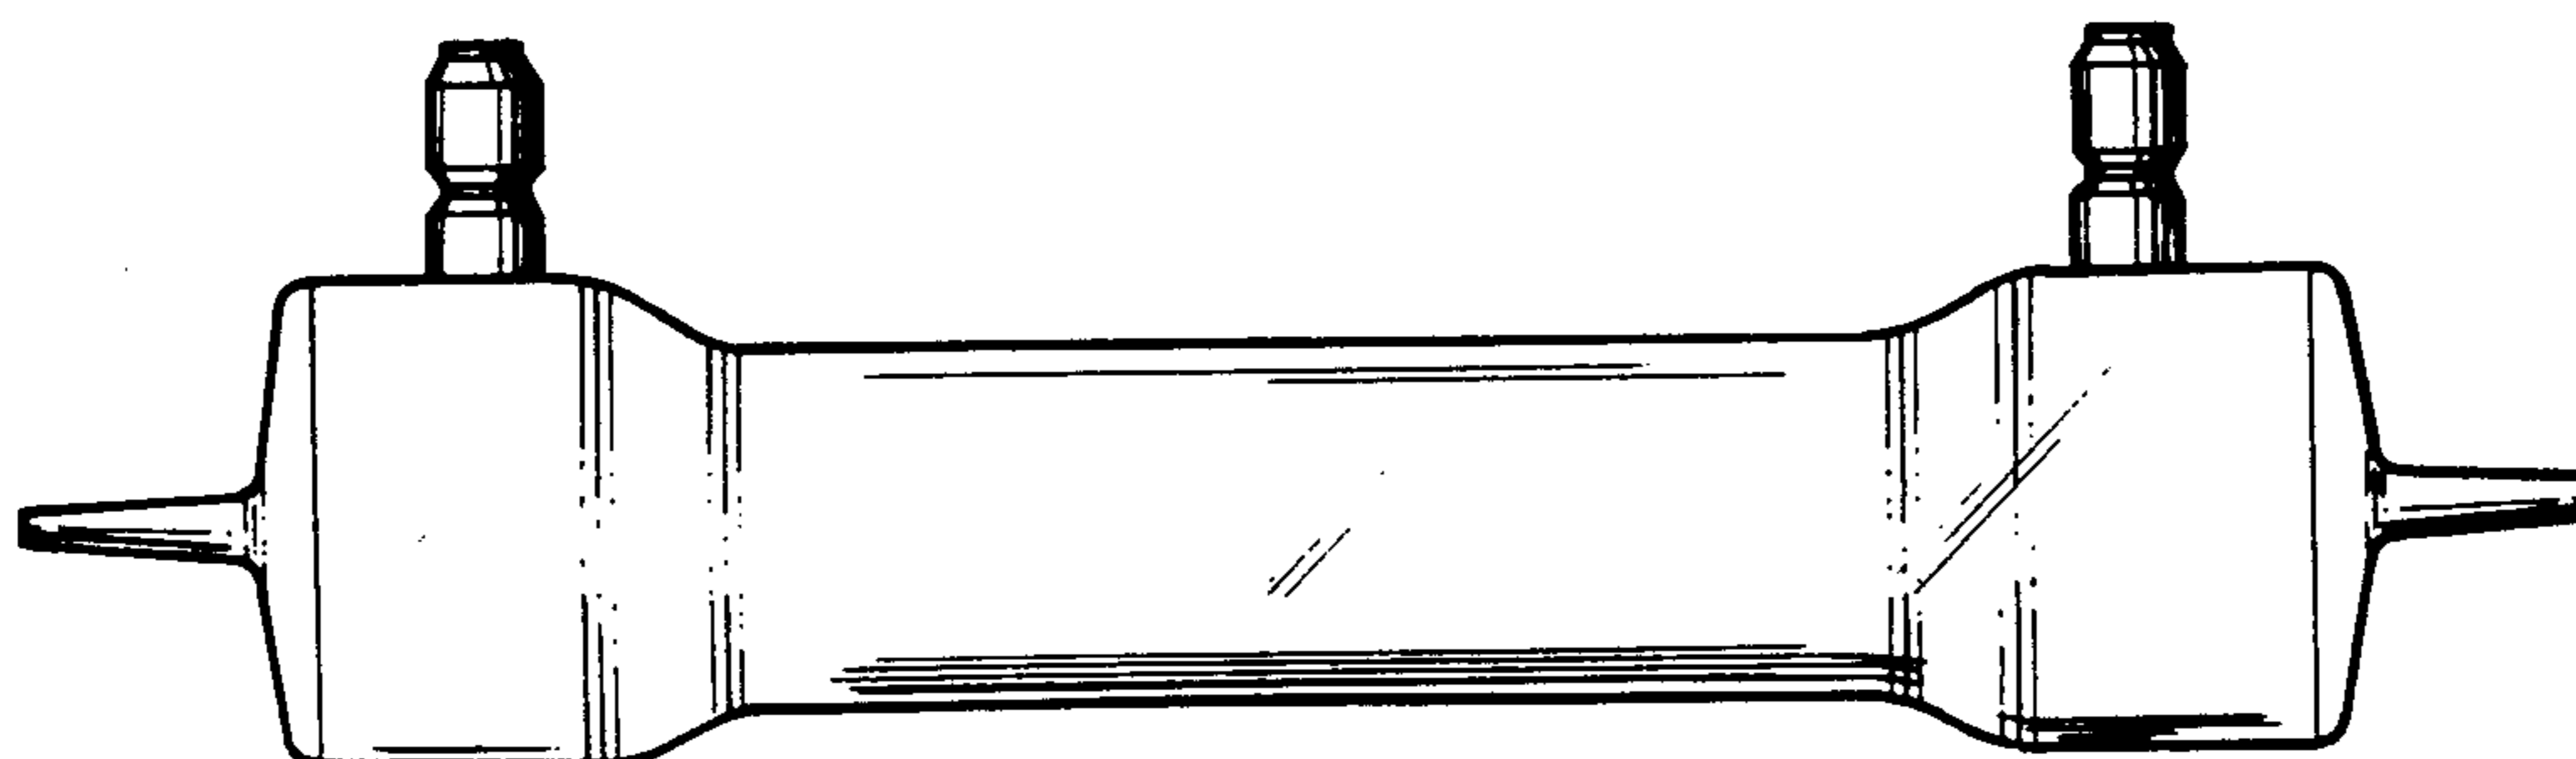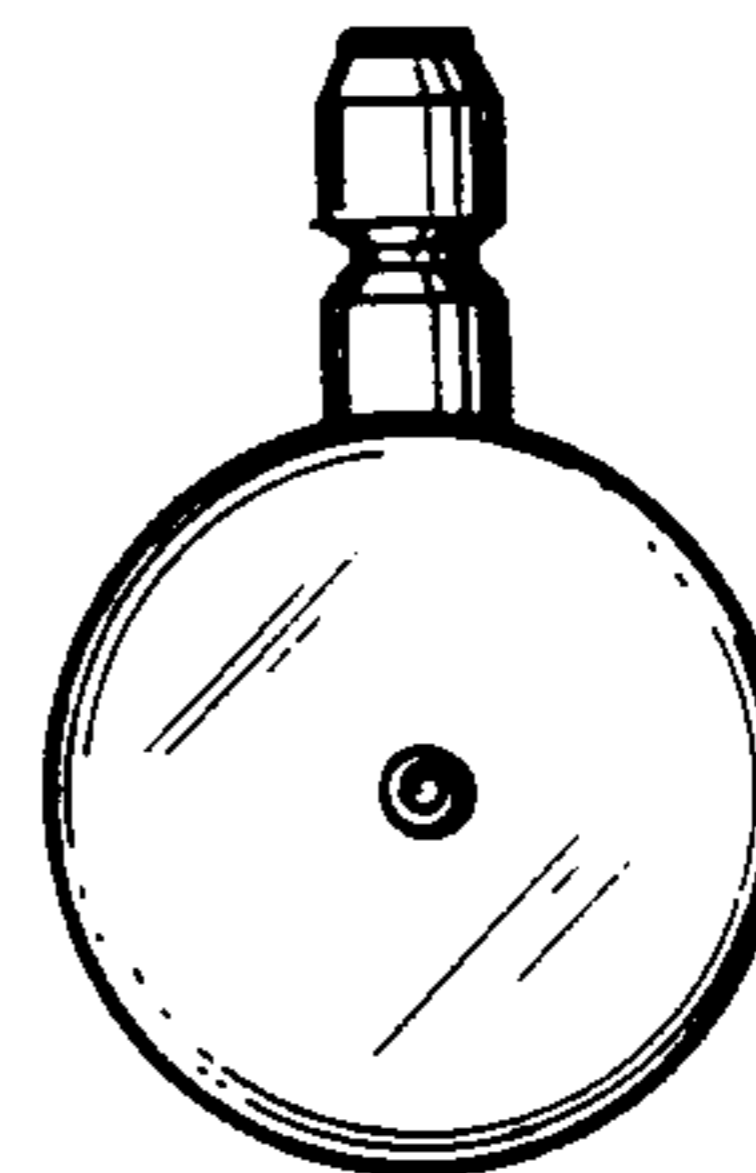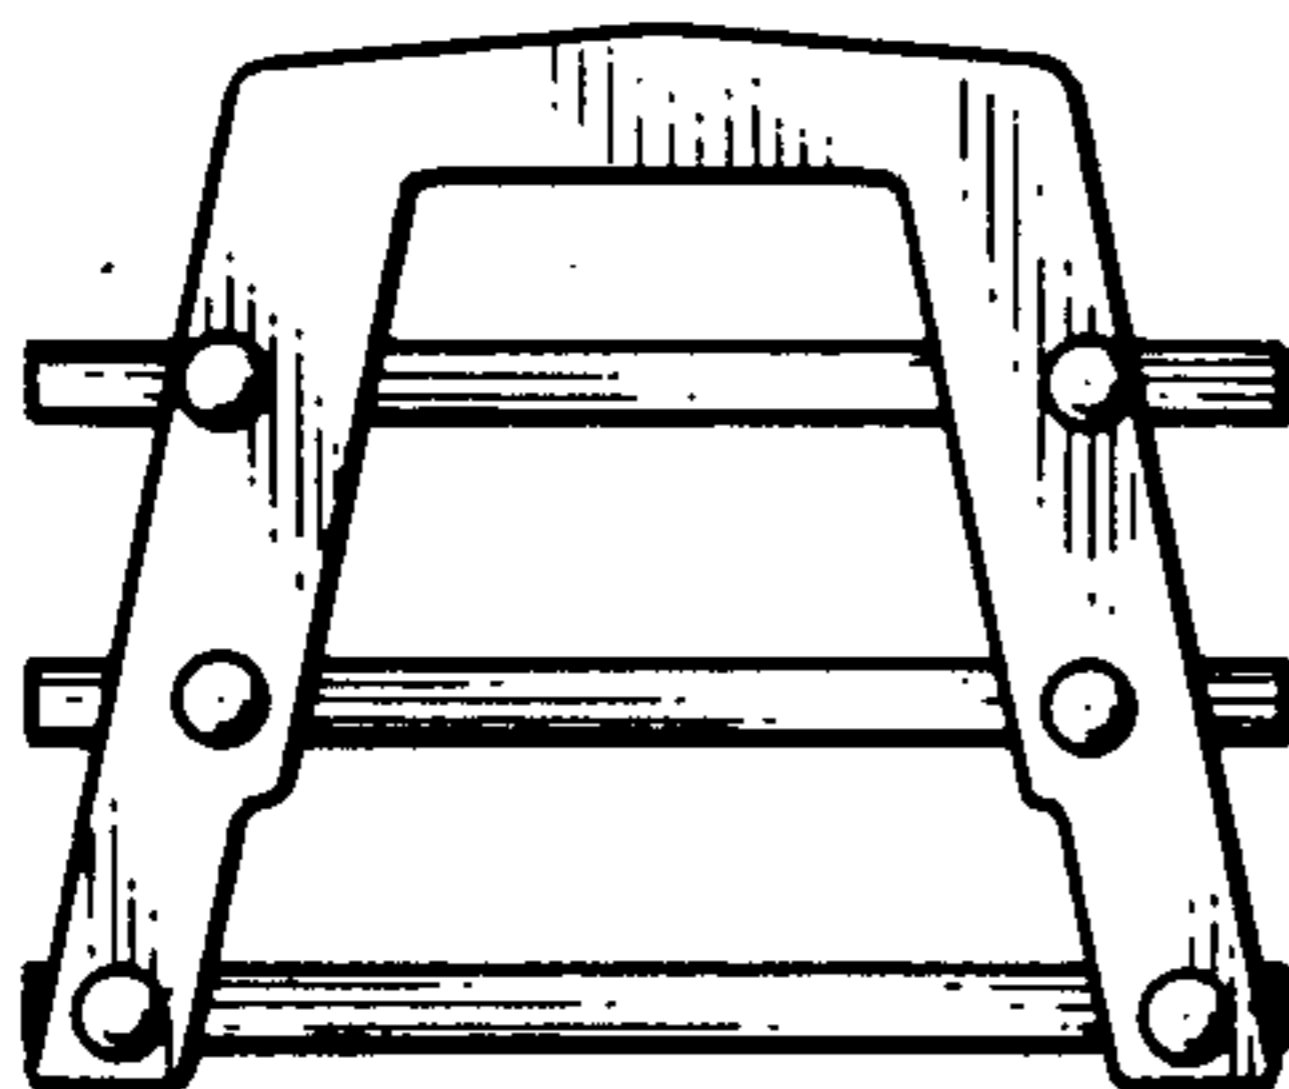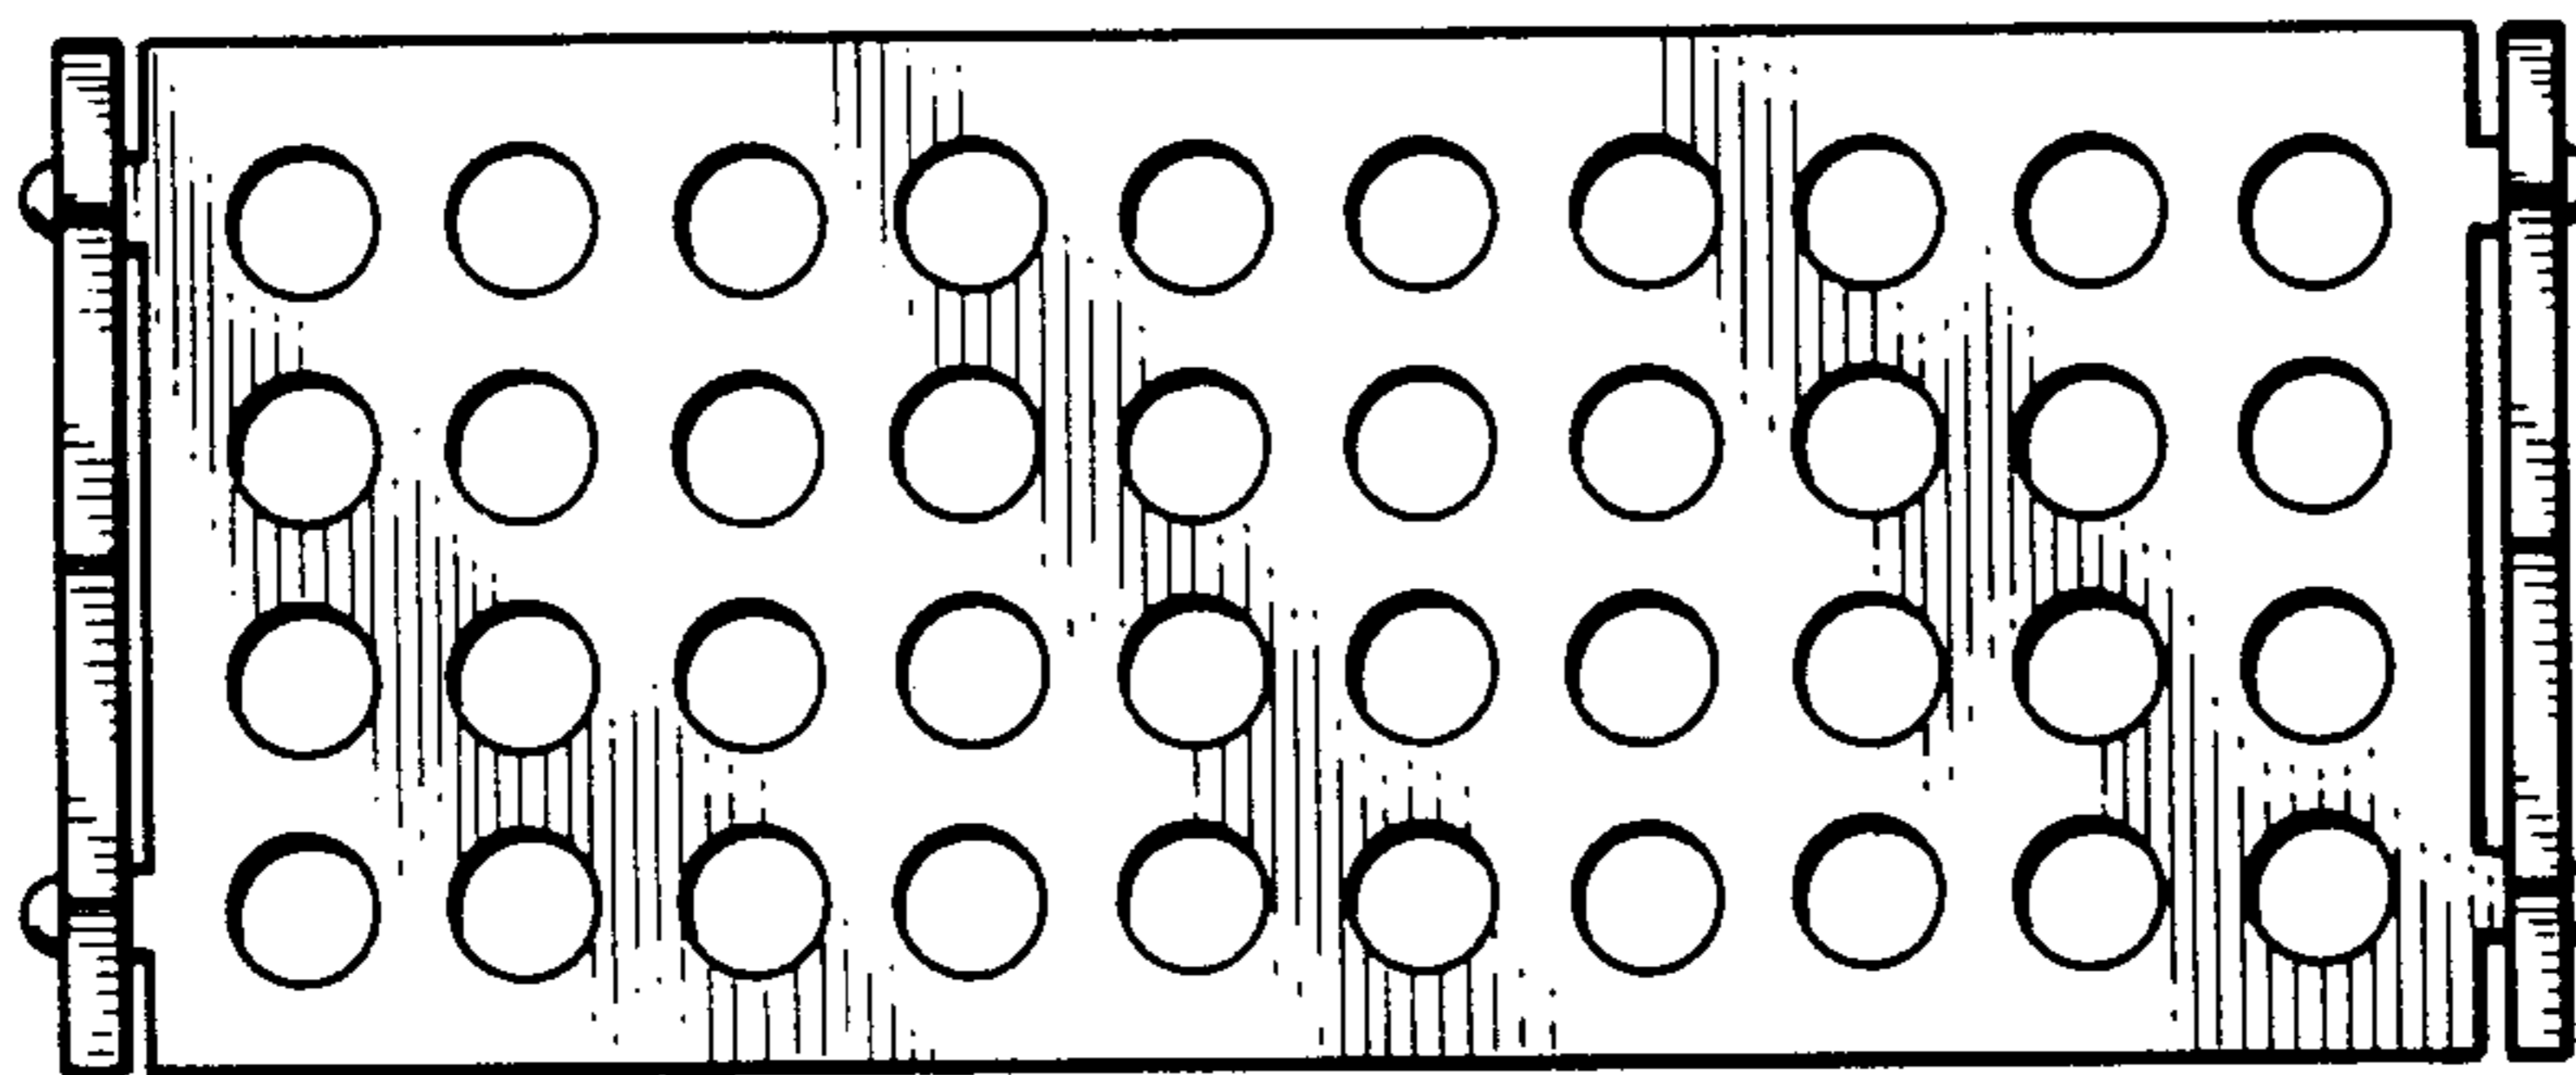

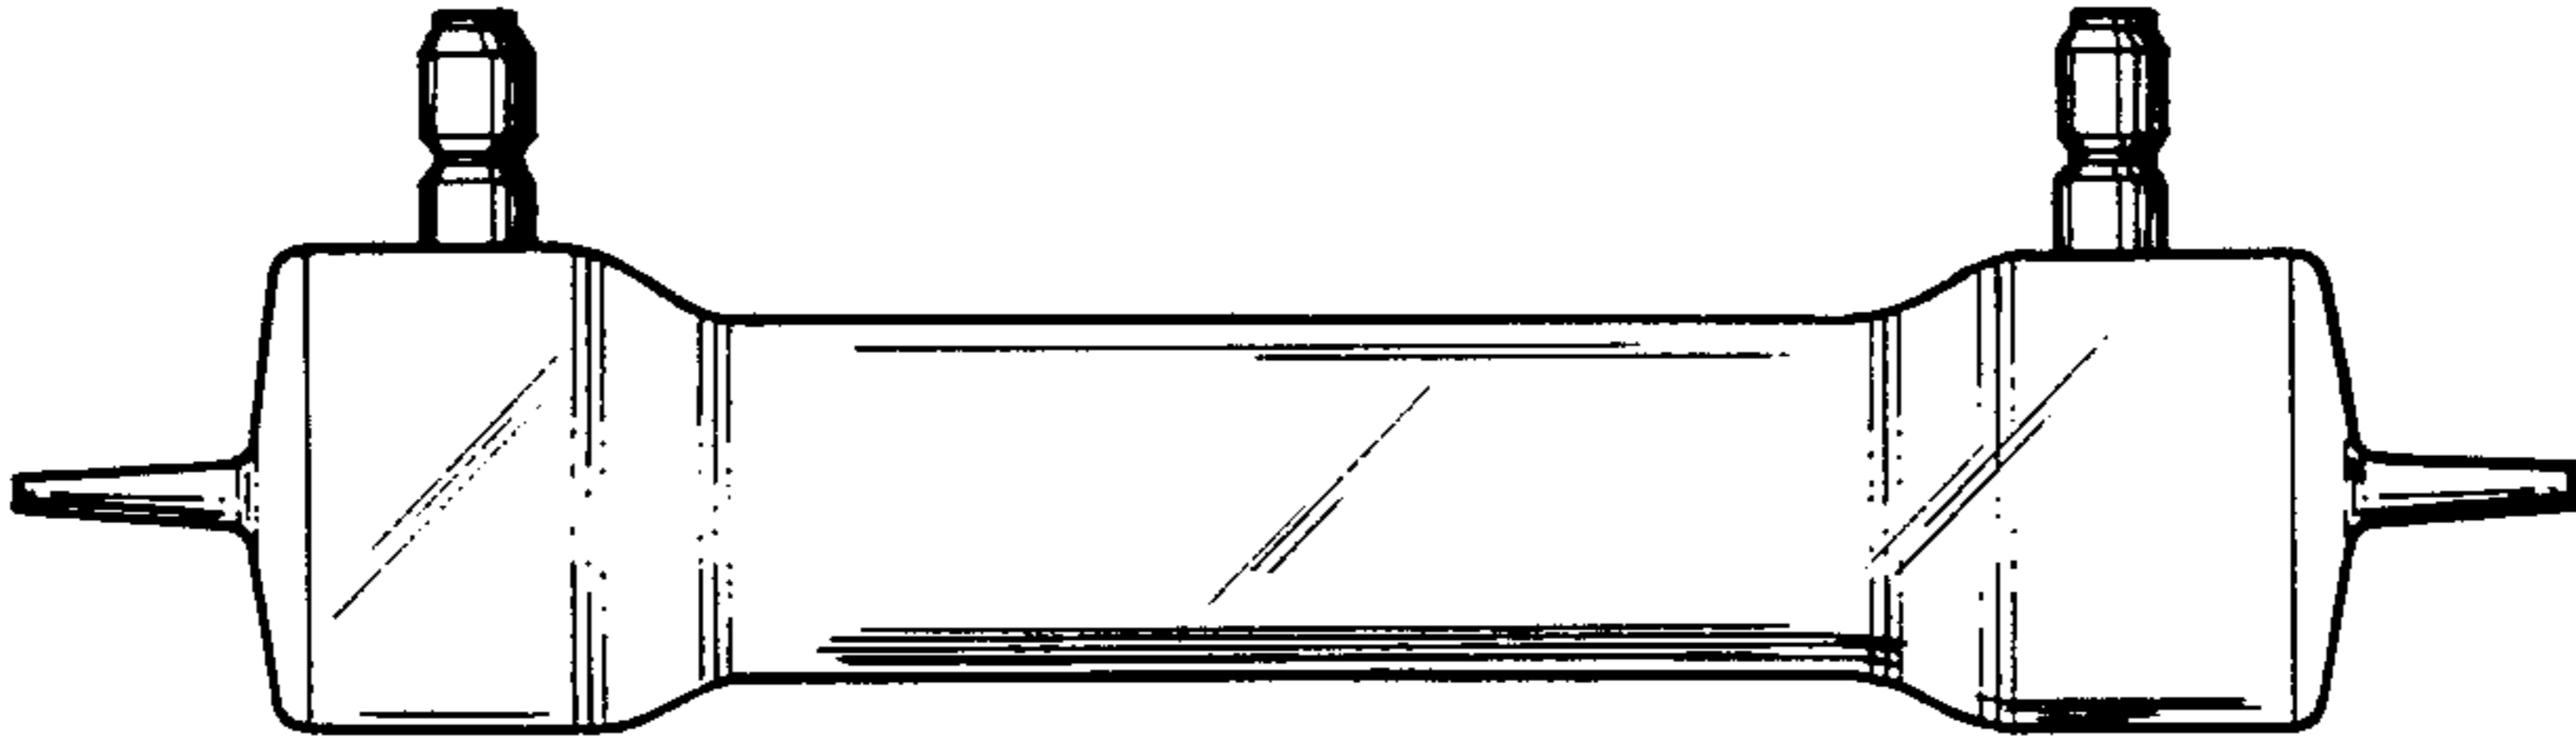


FIG. 1

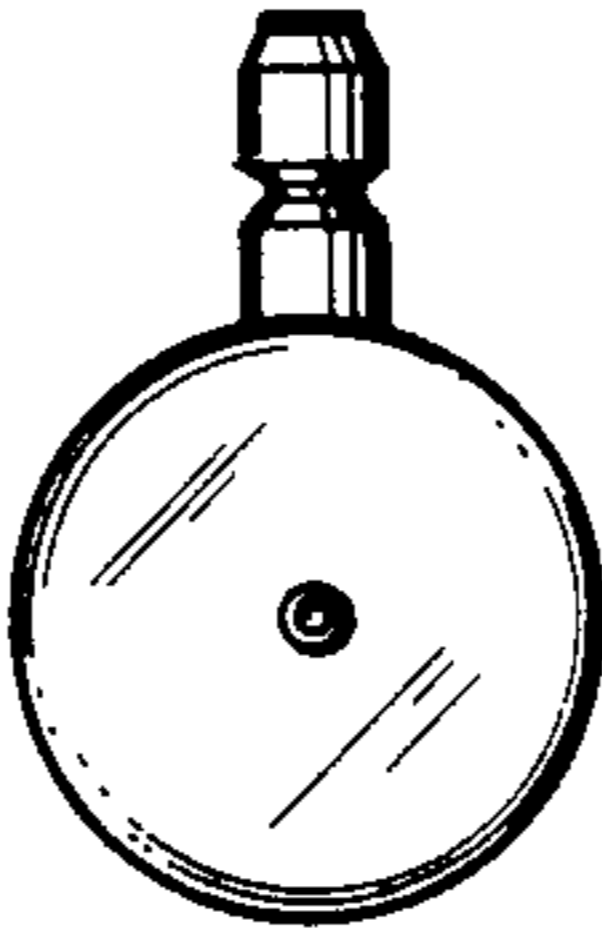


FIG. 2

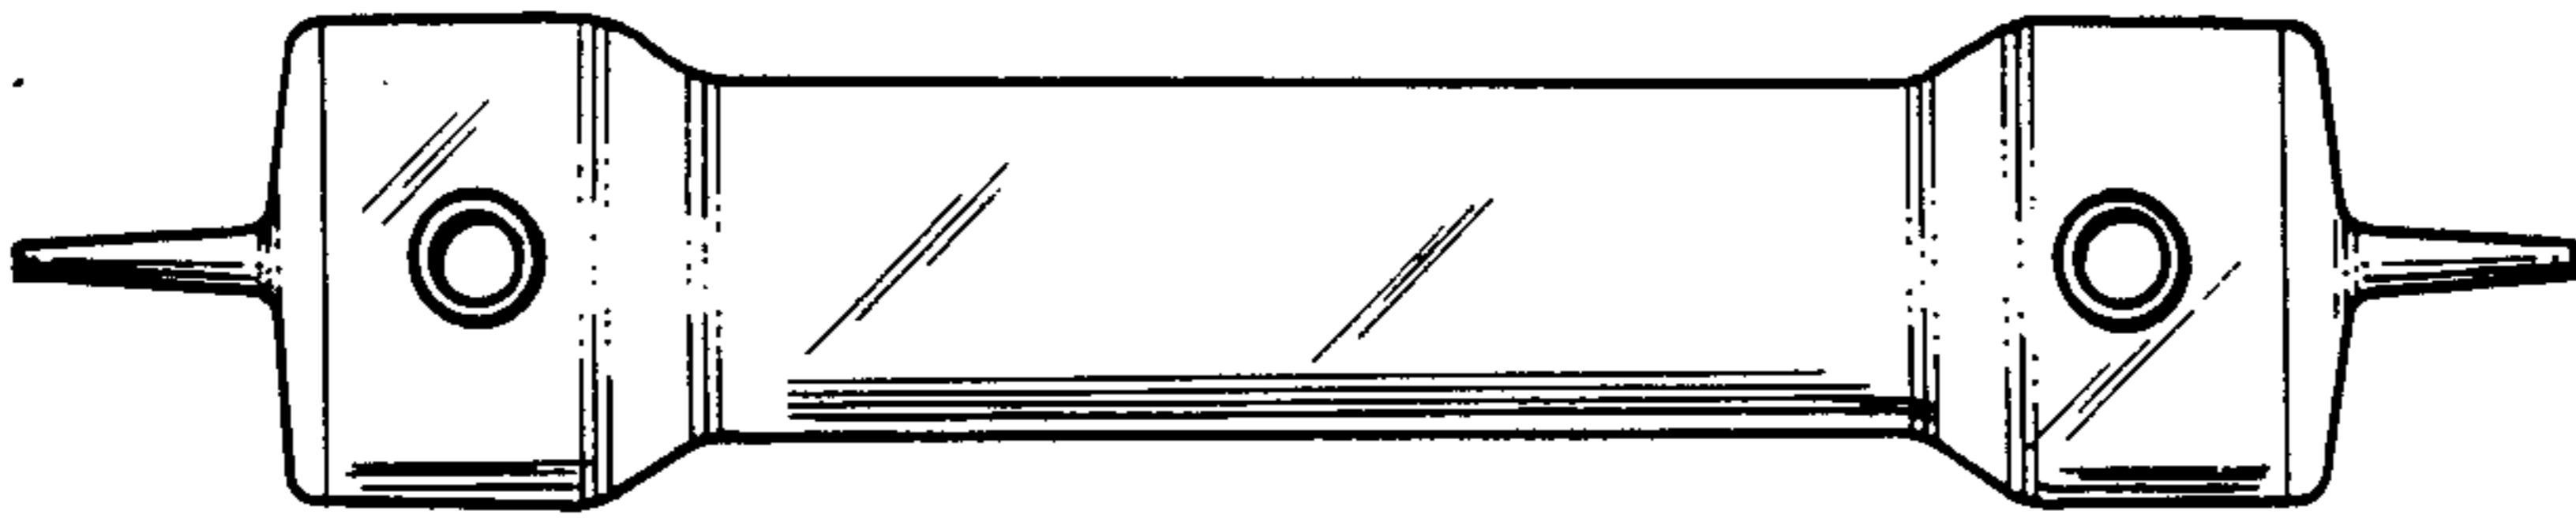


FIG. 3

UNITED STATES PATENT AND TRADEMARK OFFICE  
**CERTIFICATE OF CORRECTION**

PATENT NO. : Des. No. 257,389  
DATED : October 14, 1980  
INVENTOR(S) : Henry Pande

It is certified that error appears in the above—identified patent and that said Letters Patent is hereby corrected as shown below:

Insert The Title Page, as shown on the attached sheet.

**Signed and Sealed this**

*Twenty-sixth Day of May 1981*

[SEAL]

*Attest:*

RENE D. TEGTMEYER

*Attesting Officer*

*Acting Commissioner of Patents and Trademarks*