

[54] **BILIRUBIN CONCENTRATION ANALYZER**

[75] Inventor: **John T. Armbruster**, Niagara Falls, N.Y.

[73] Assignee: **American Optical Corporation**, Southbridge, Mass.

[\*\*] Term: **14 Years**

[21] Appl. No.: **9,318**

[22] Filed: **Feb. 5, 1979**

[51] Int. Cl. .... **D24—02**

[52] U.S. Cl. .... **D24/17; D24/8; D10/46; D10/81**

[58] Field of Search ..... **D10/81, 46, 75; D24/21, D24/17, 1.1, 8; 356/39, 36, 40, 43**

[56] **References Cited**

**U.S. PATENT DOCUMENTS**

D. 196,044 8/1963 Malk ..... D10/81

D. 241,275 8/1976 Green, Jr. .... D24/21  
 D. 245,965 10/1977 Havstad ..... D10/81 X  
 D. 249,891 10/1978 Rowland et al. .... D24/17  
 D. 252,948 9/1979 Ferreira ..... D10/46 X  
 4,156,570 5/1979 Wardlaw ..... 356/39 X



*Primary Examiner*—Bernard Ansher  
*Attorney, Agent, or Firm*—Alan H. Spencer

[57] **CLAIM**

The ornamental design for a bilirubin concentration analyzer, as shown and described.

**DESCRIPTION**

FIG. 1 is a top plan view of the bilirubin concentration analyzer;  
 FIG. 2 is a left side view of the bilirubin concentration analyzer, its opposite side having substantially the same appearance;  
 FIG. 3 is a rear view of the bilirubin concentration analyzer; and  
 FIG. 4 is a front view of the bilirubin concentration analyzer.

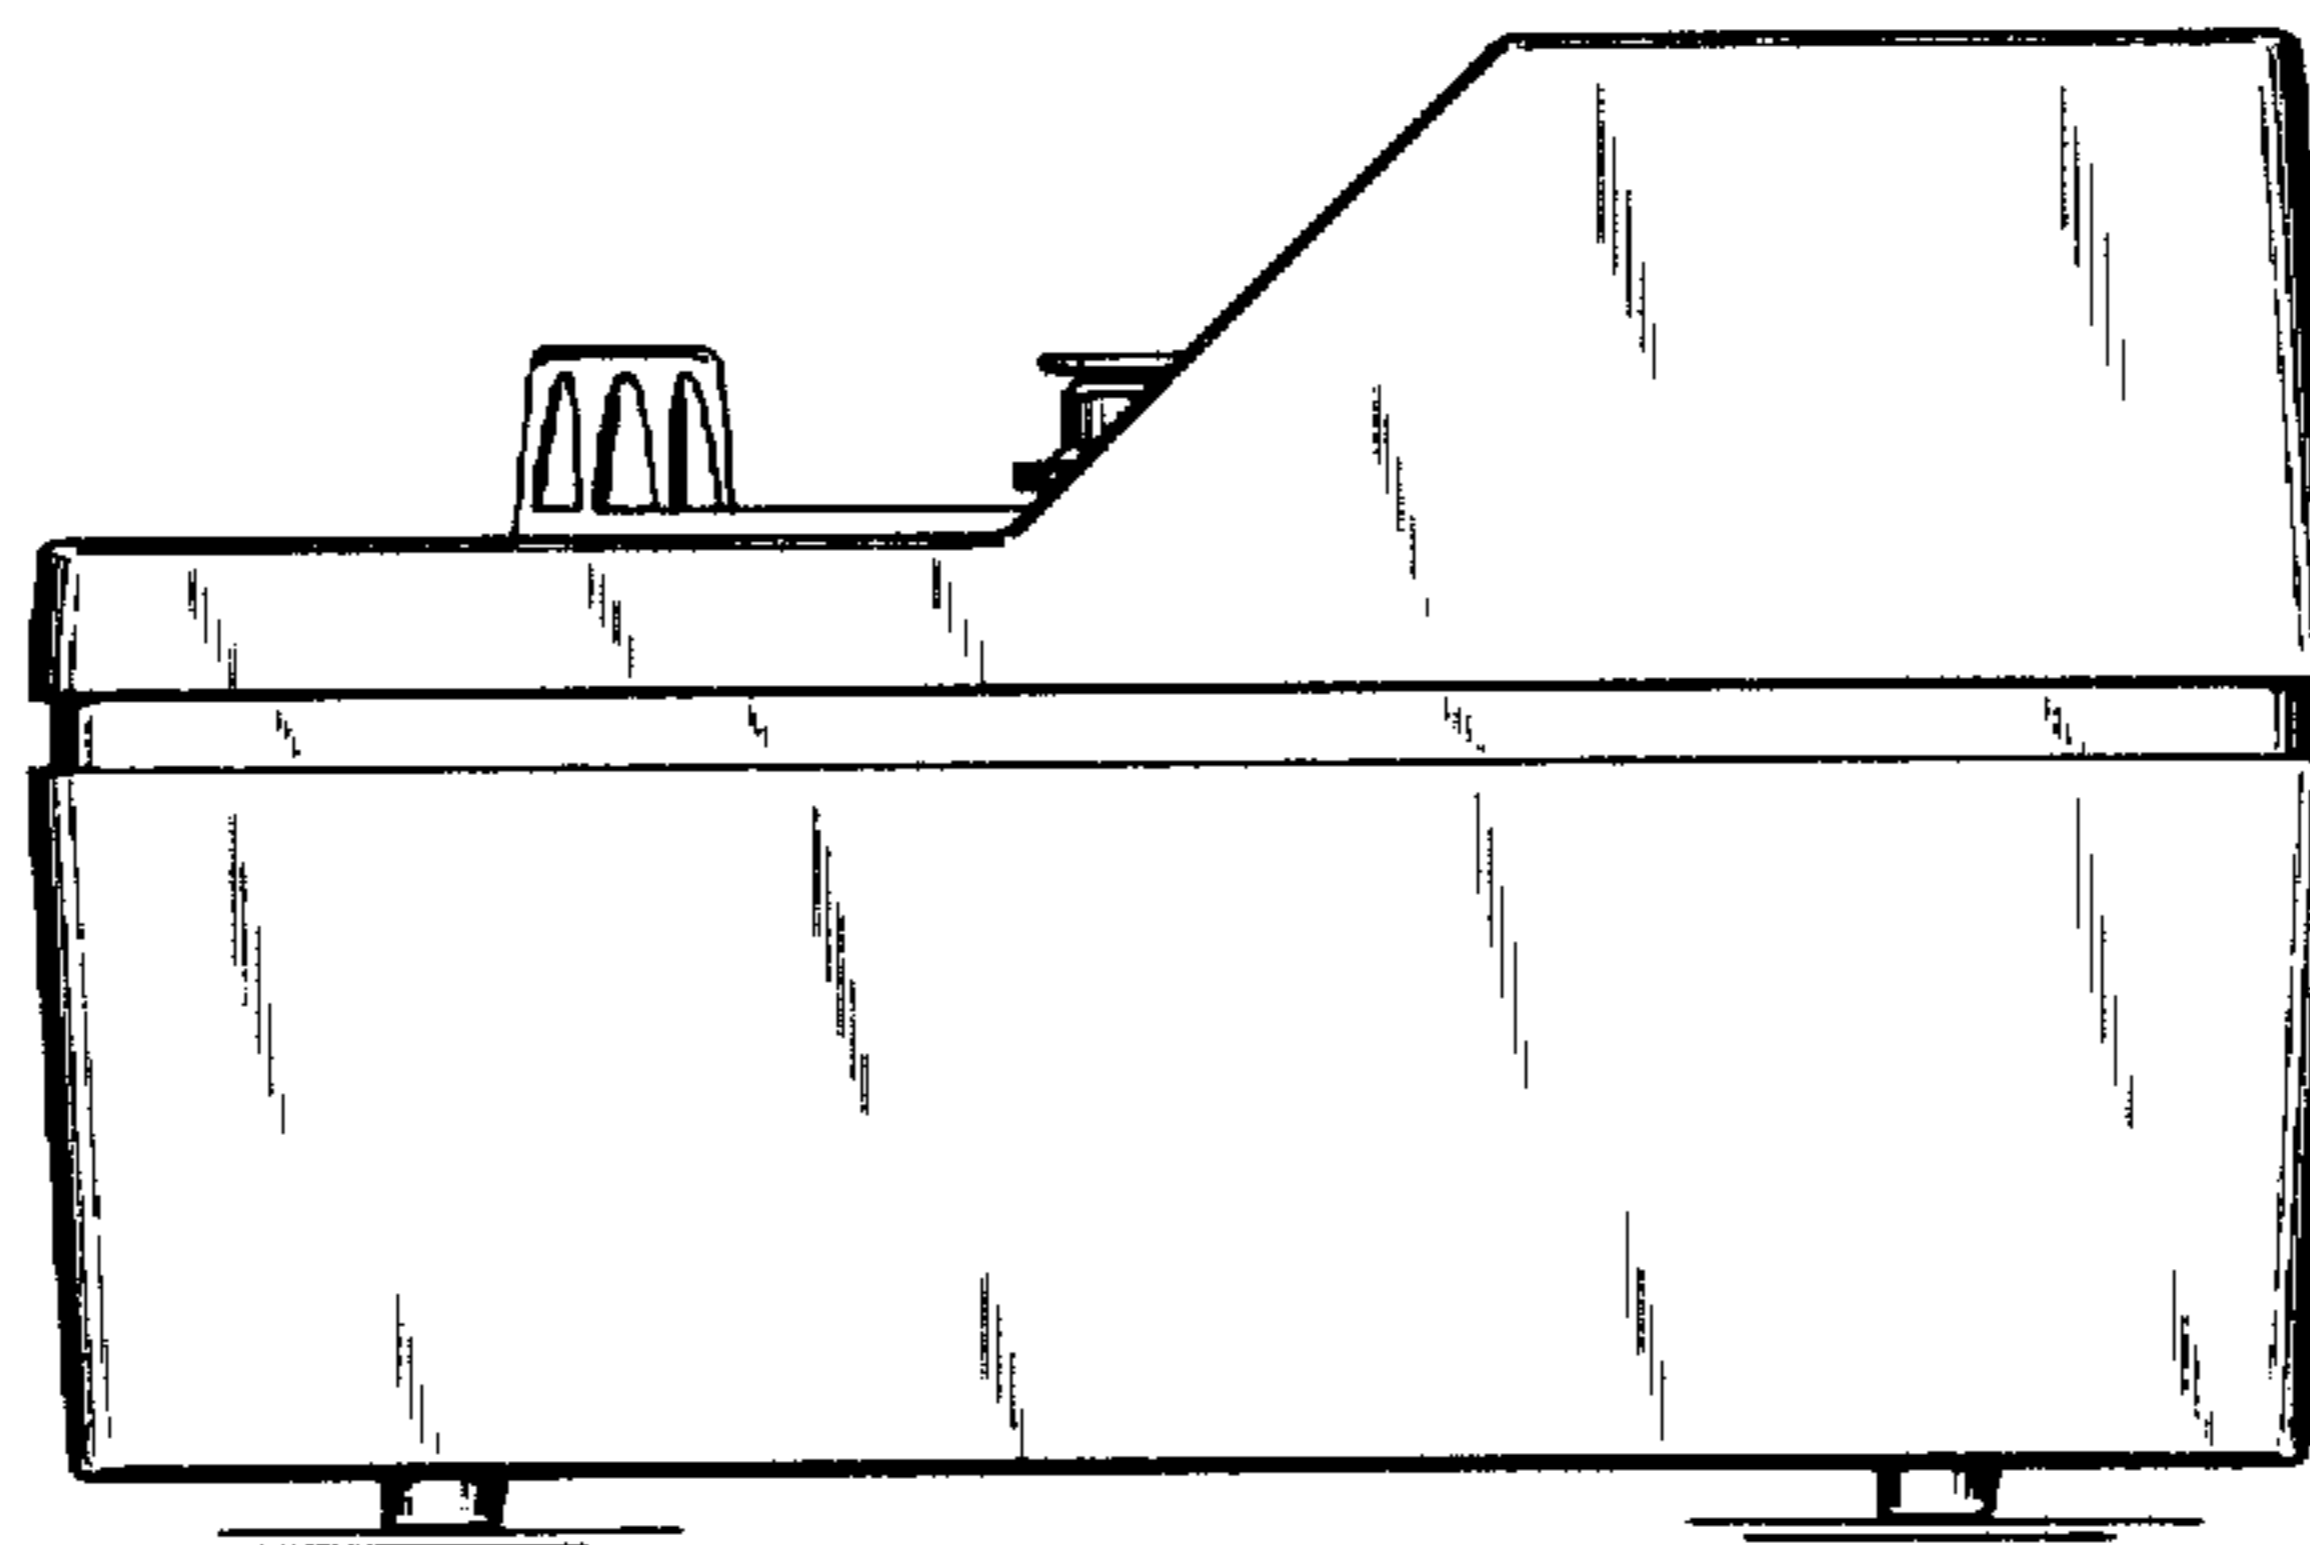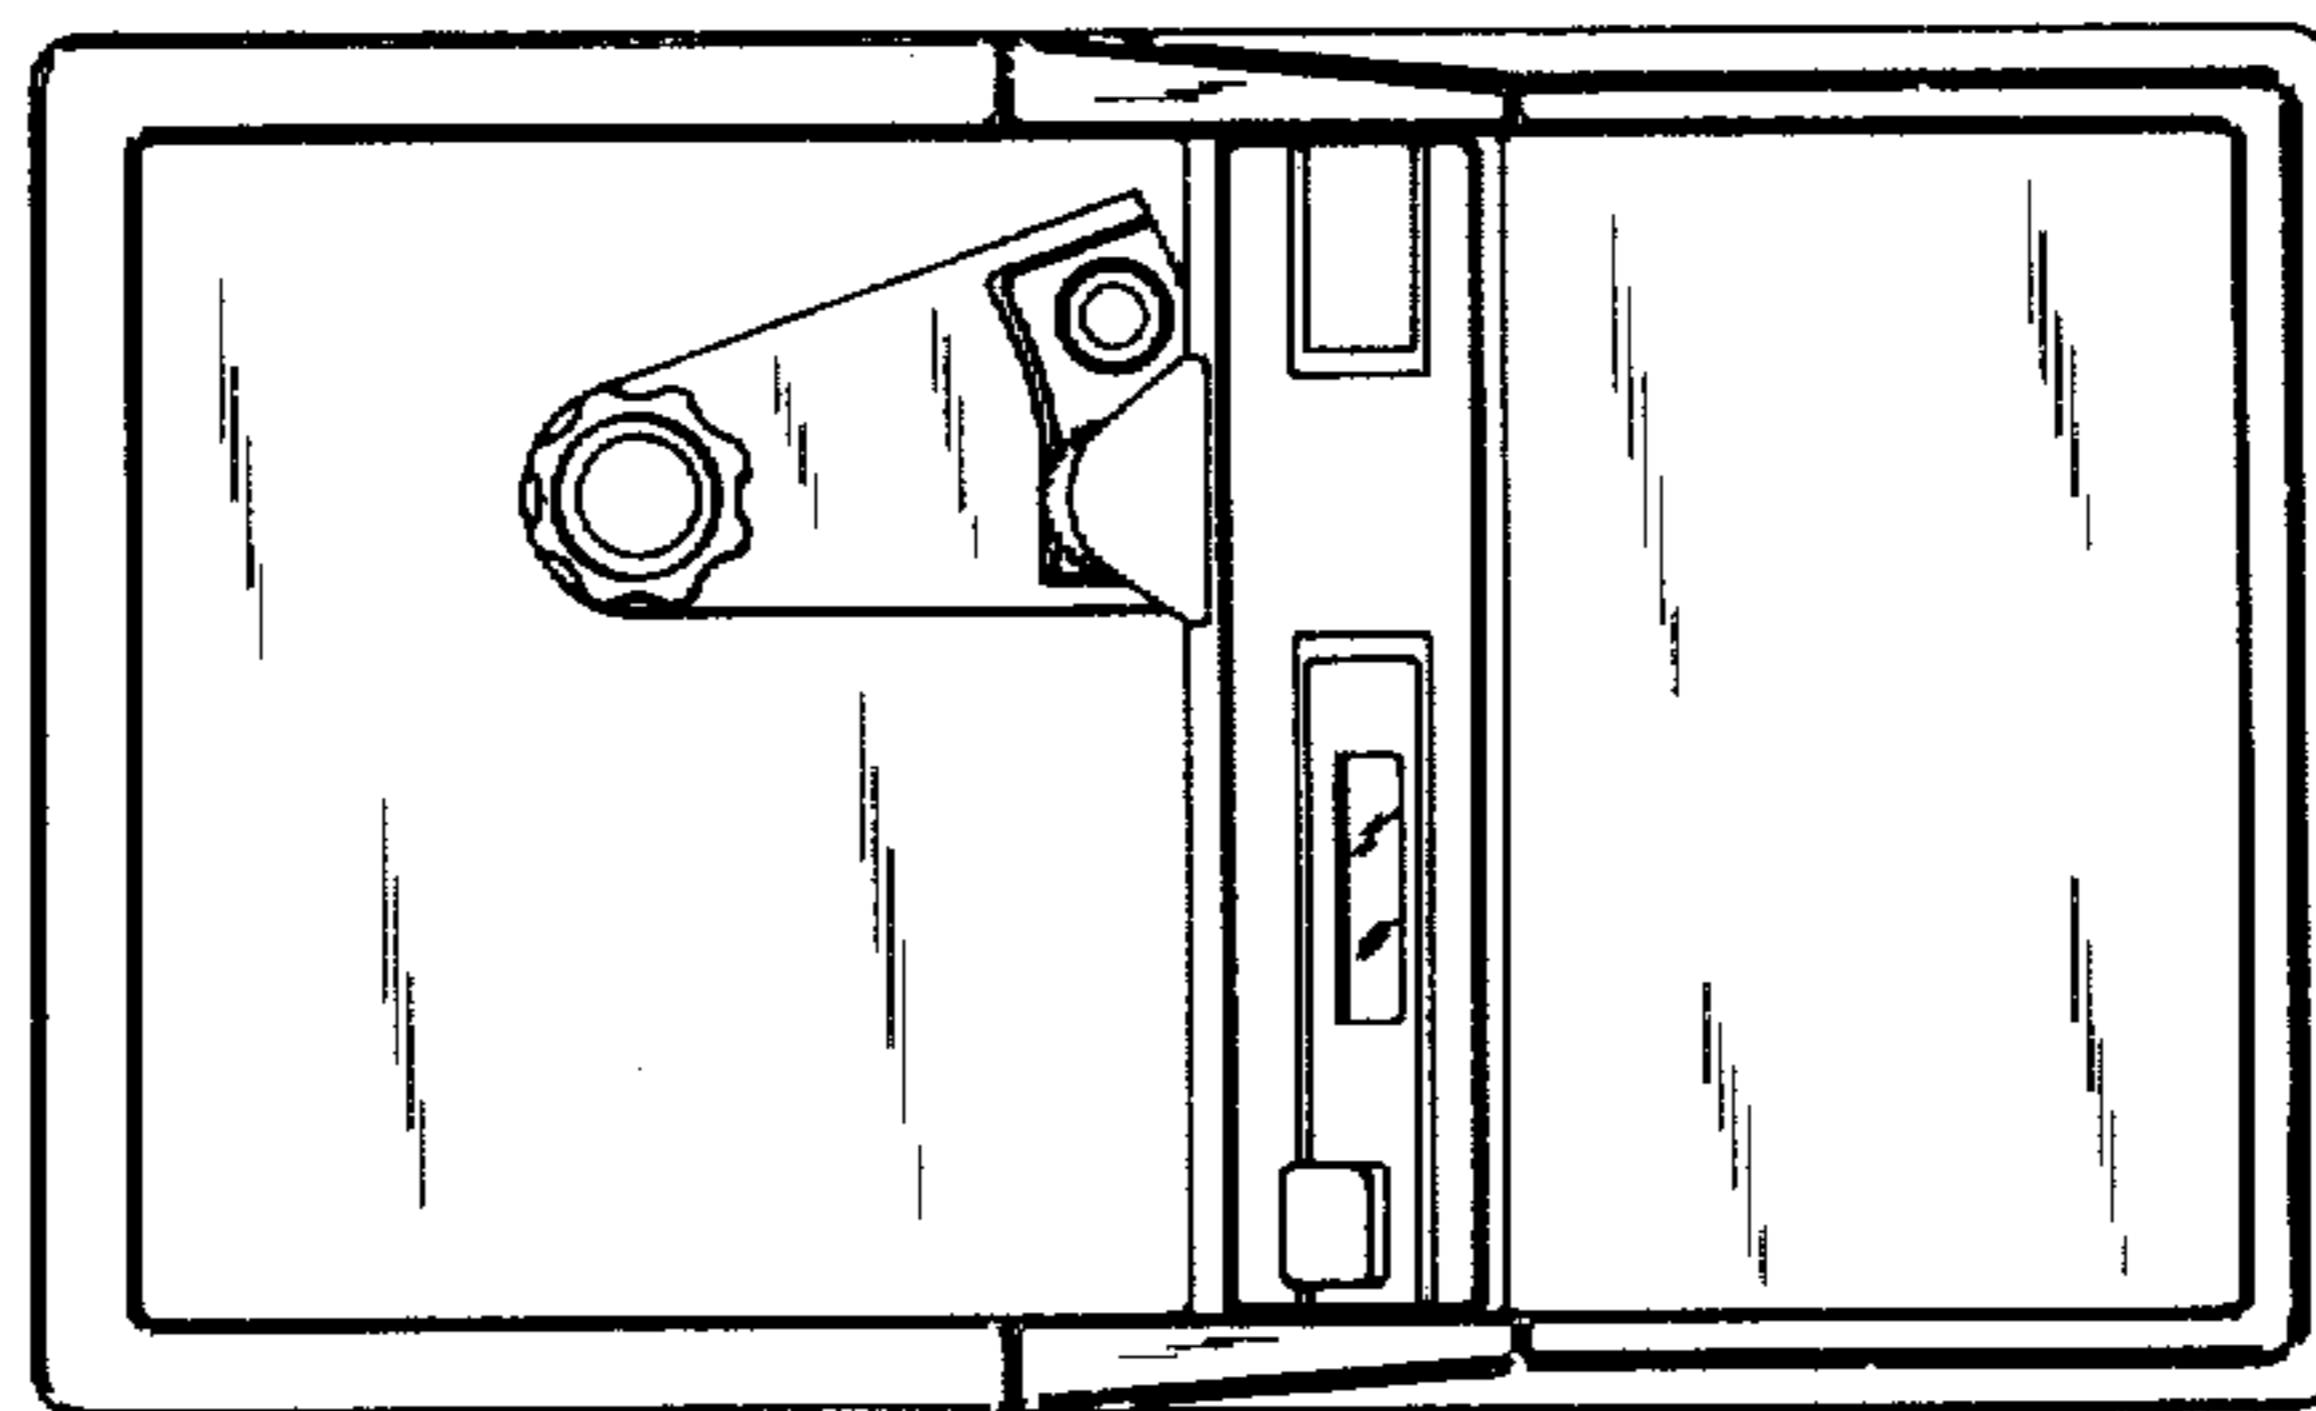

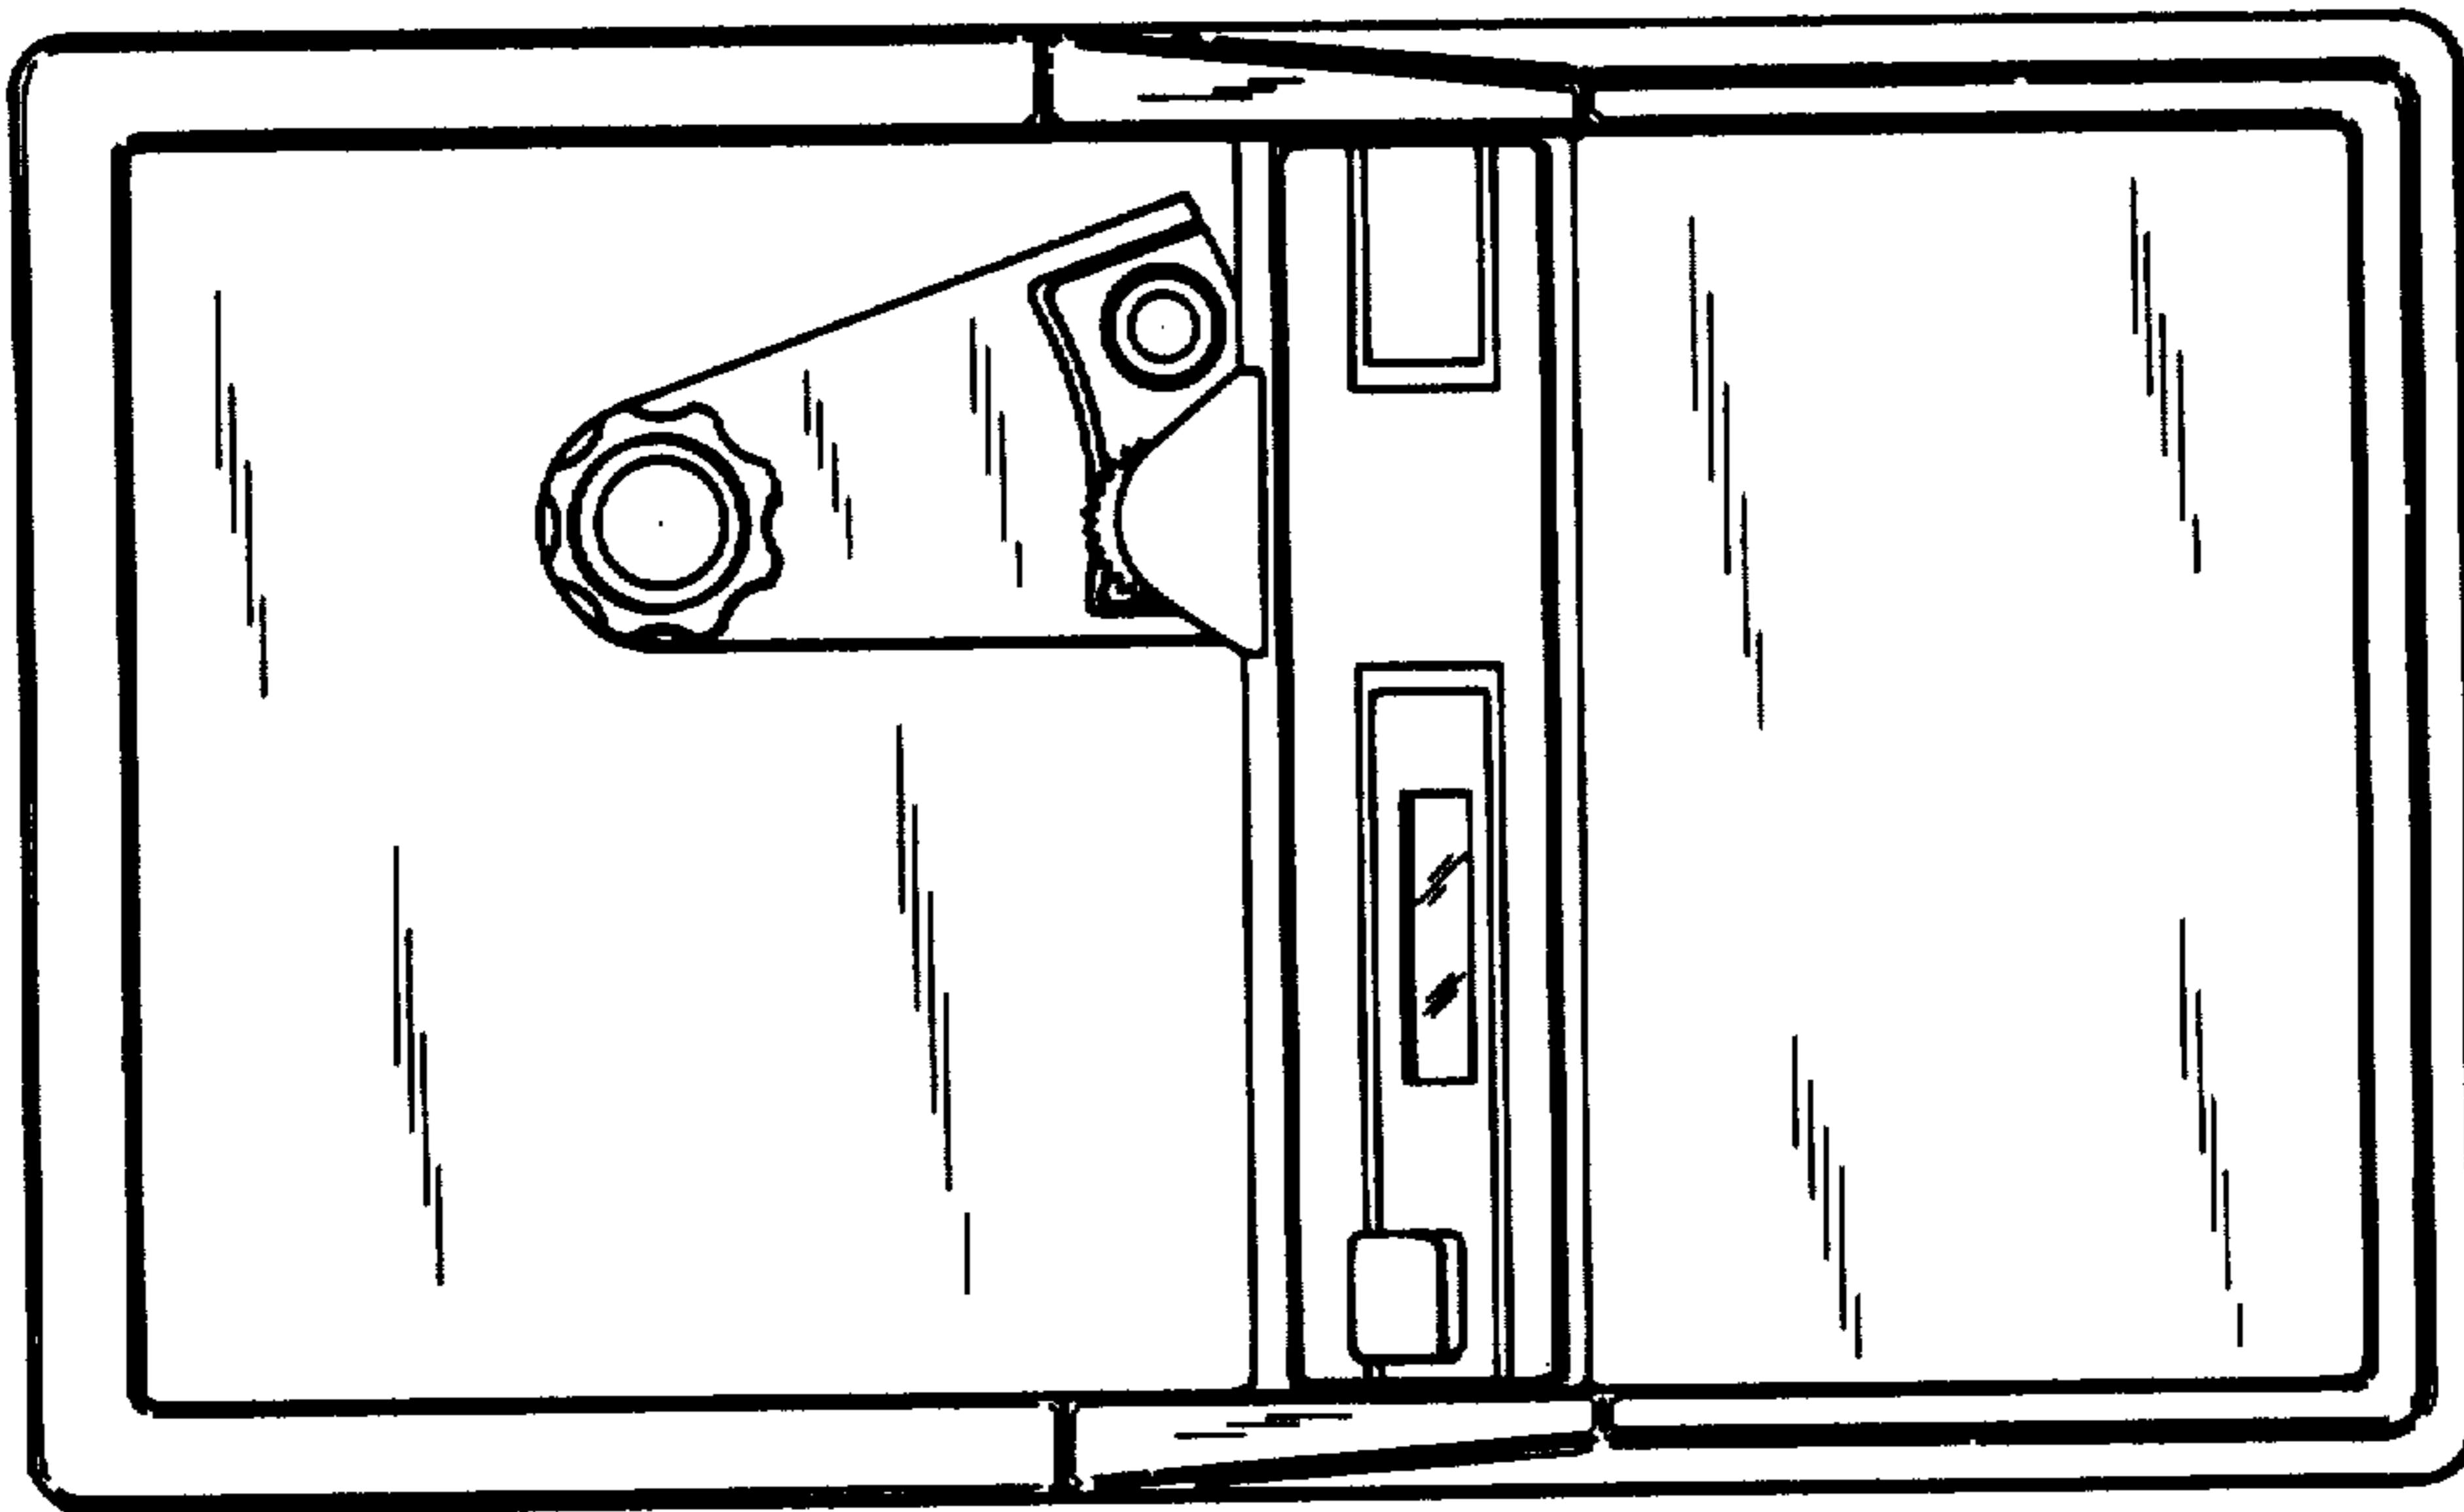


FIG. 1

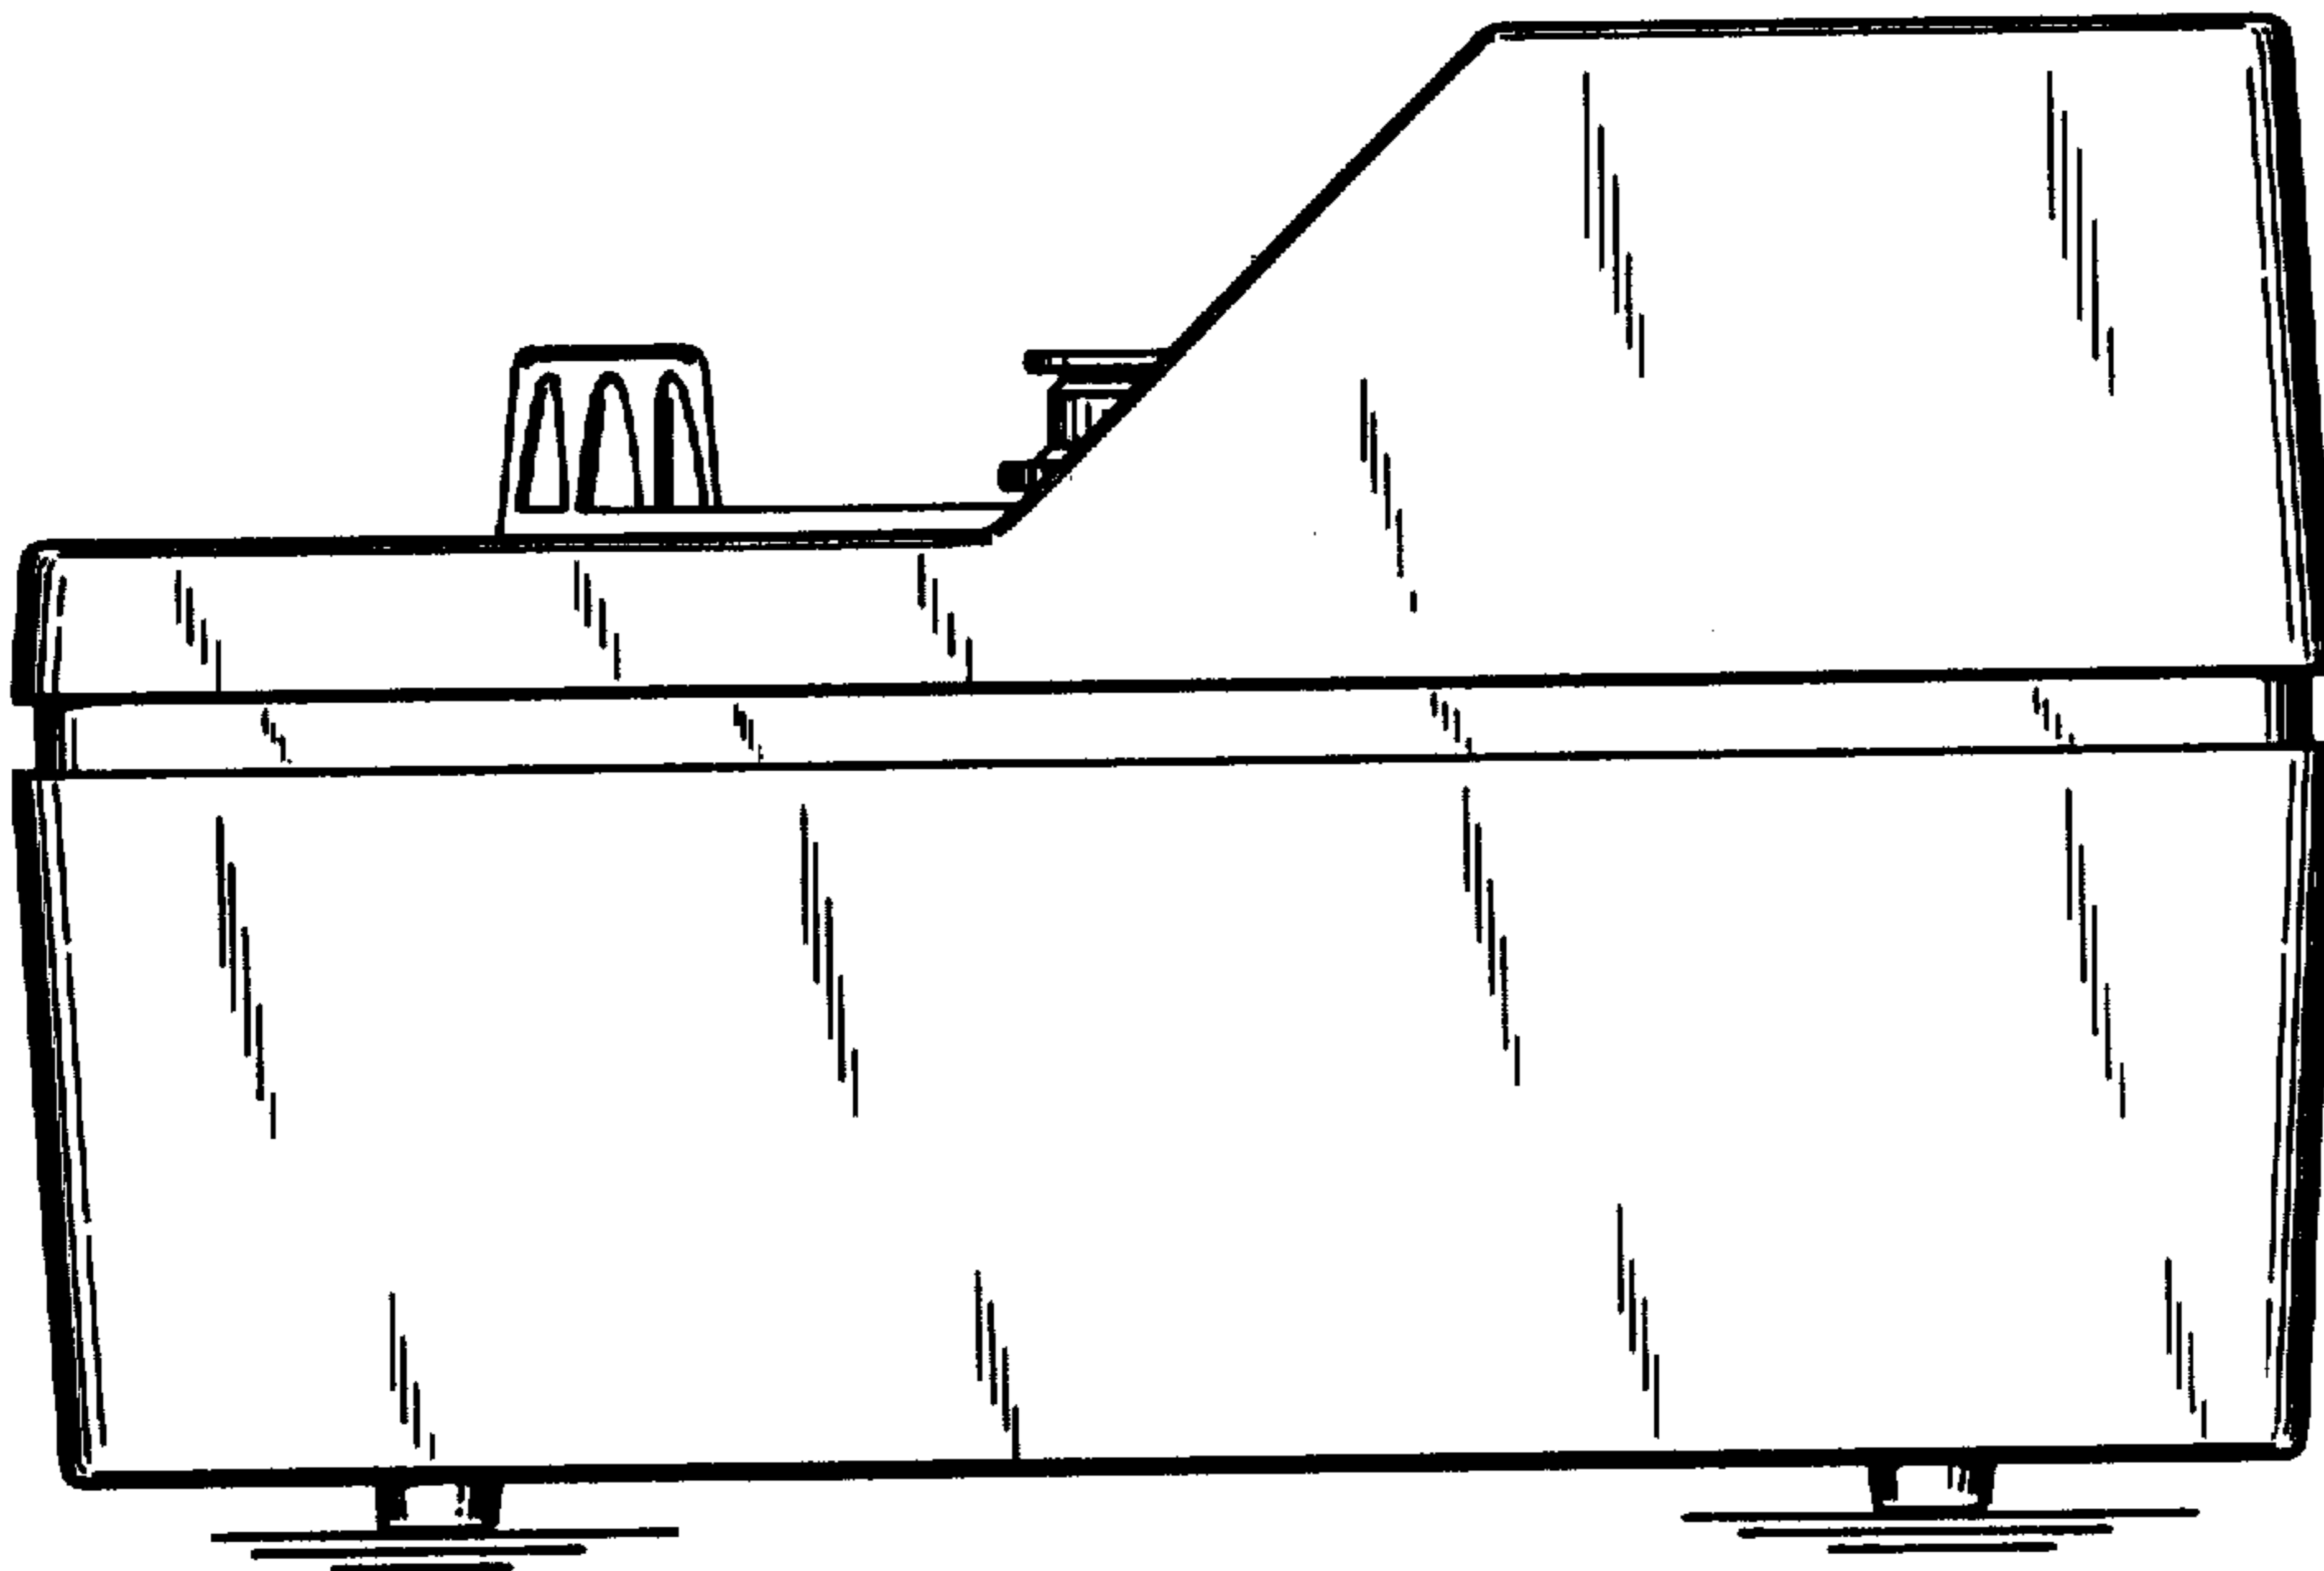


FIG. 2

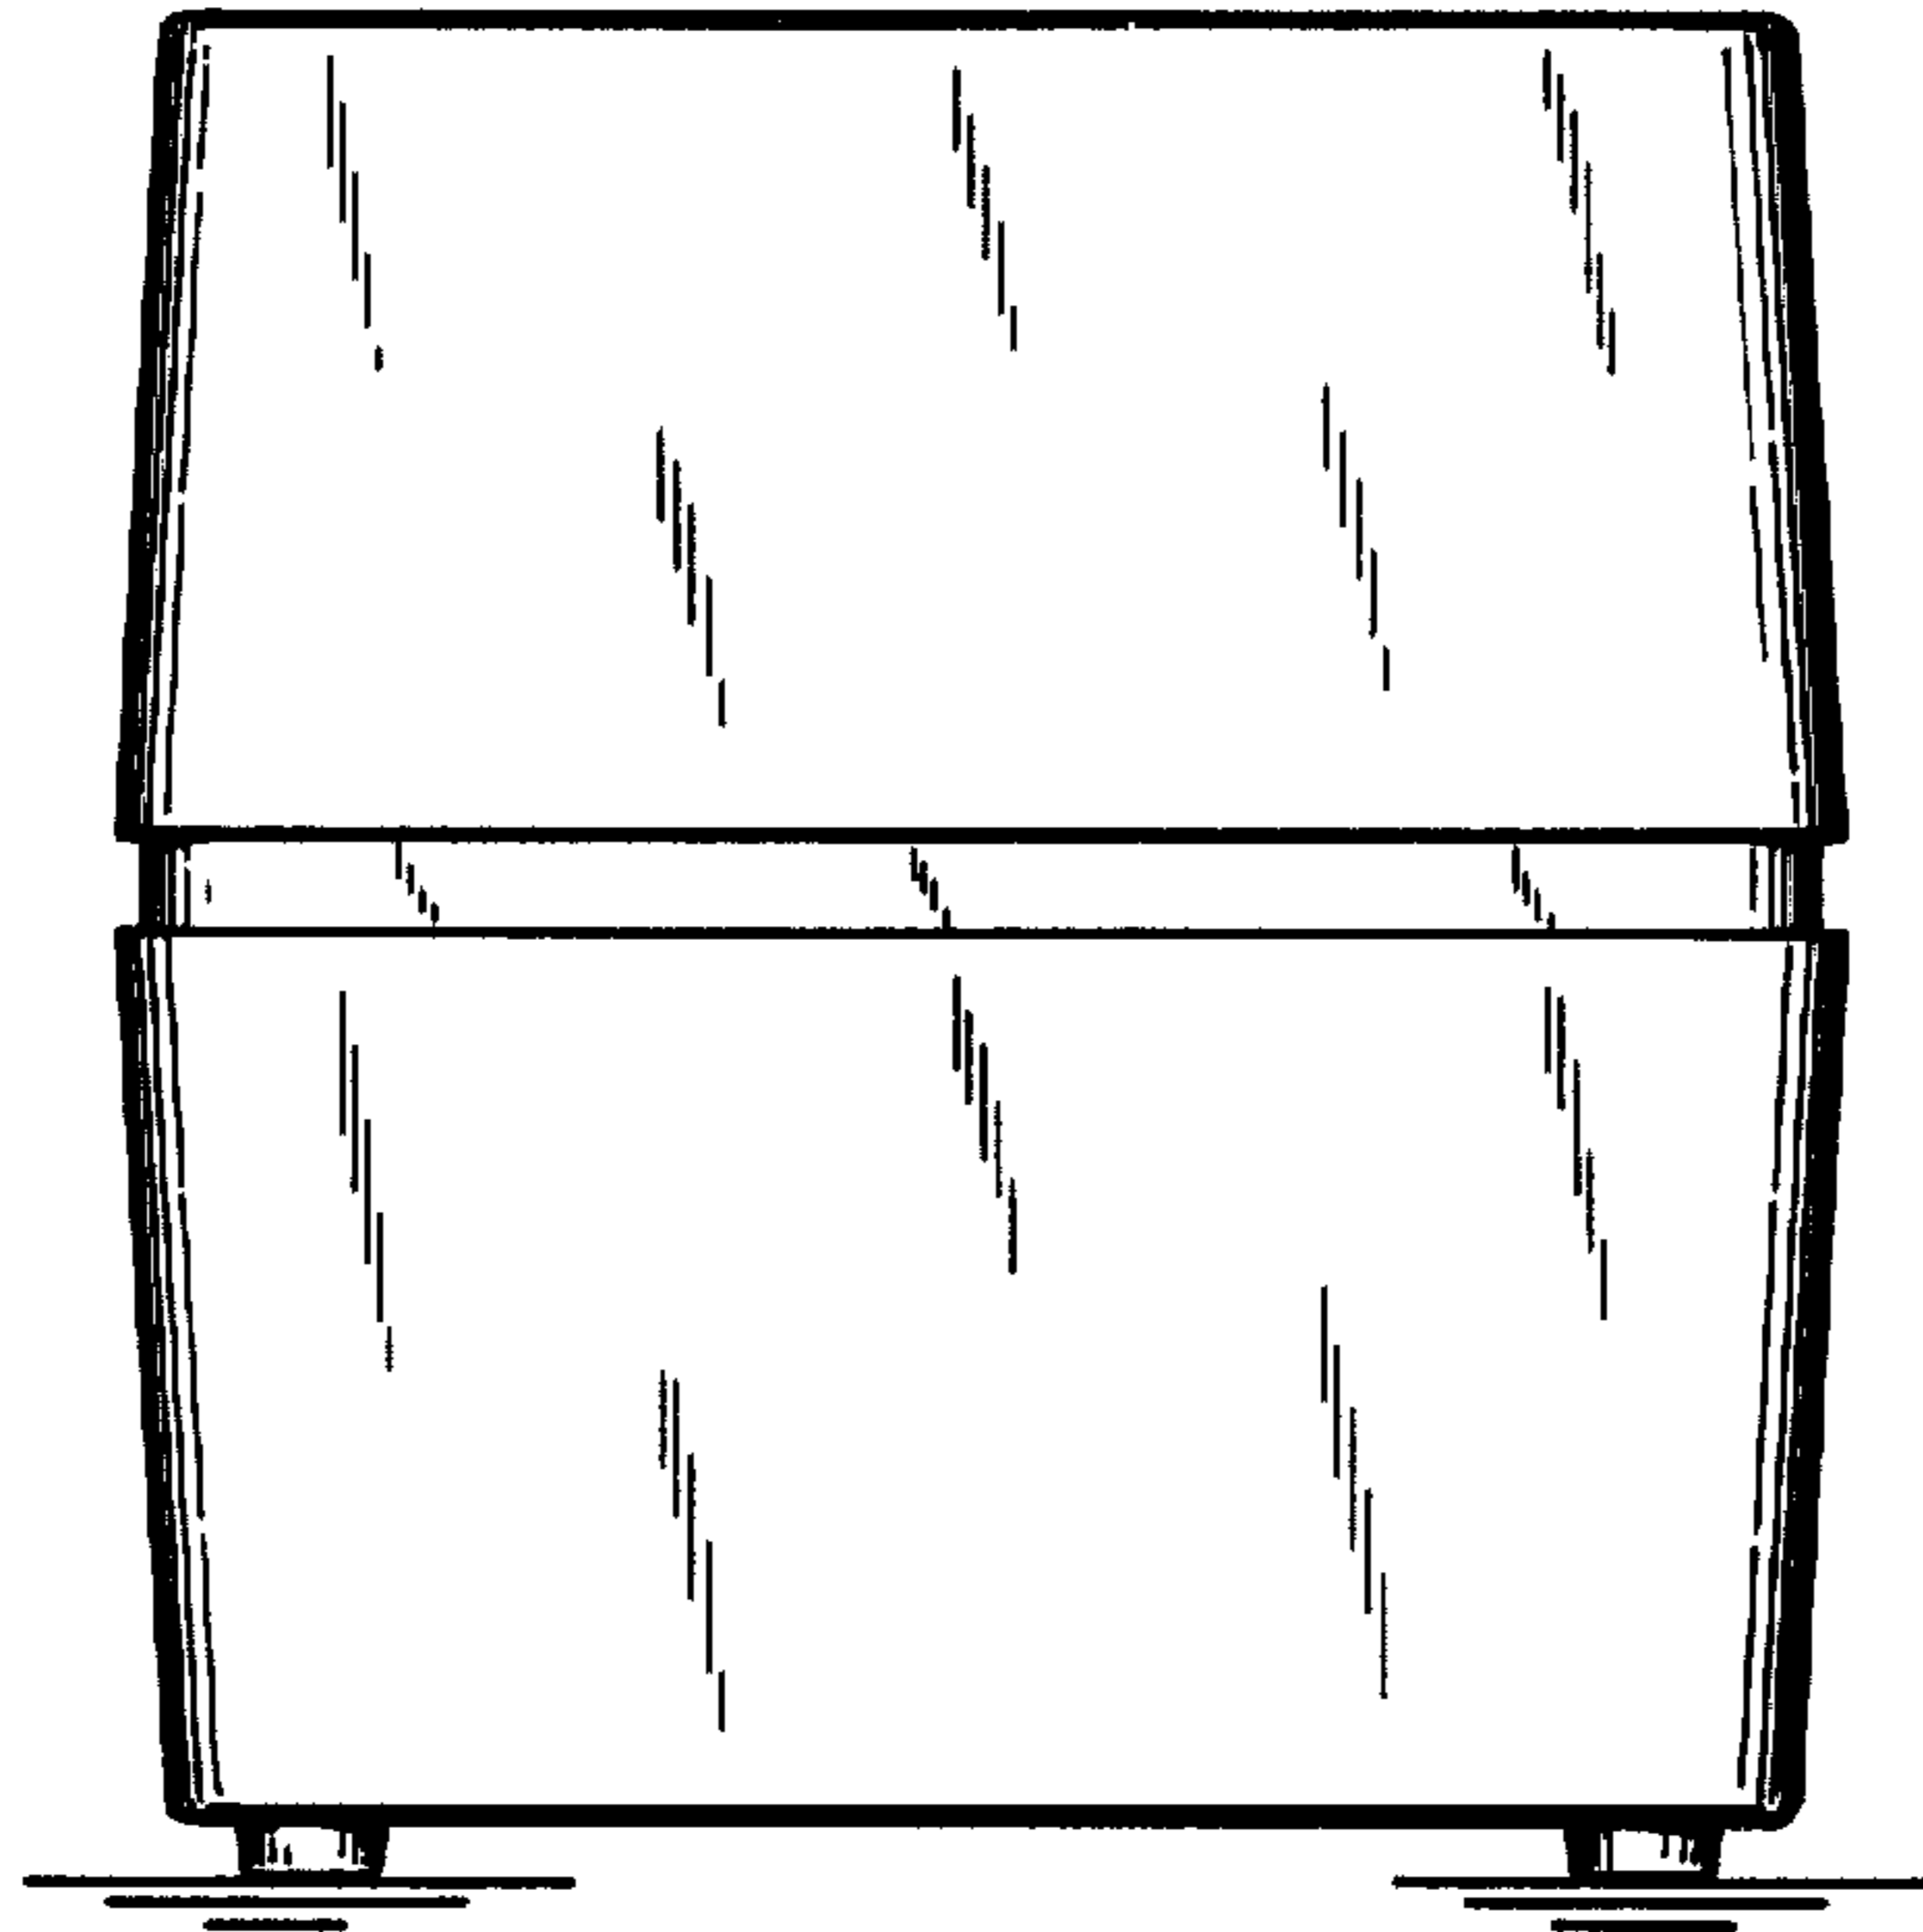


FIG. 3

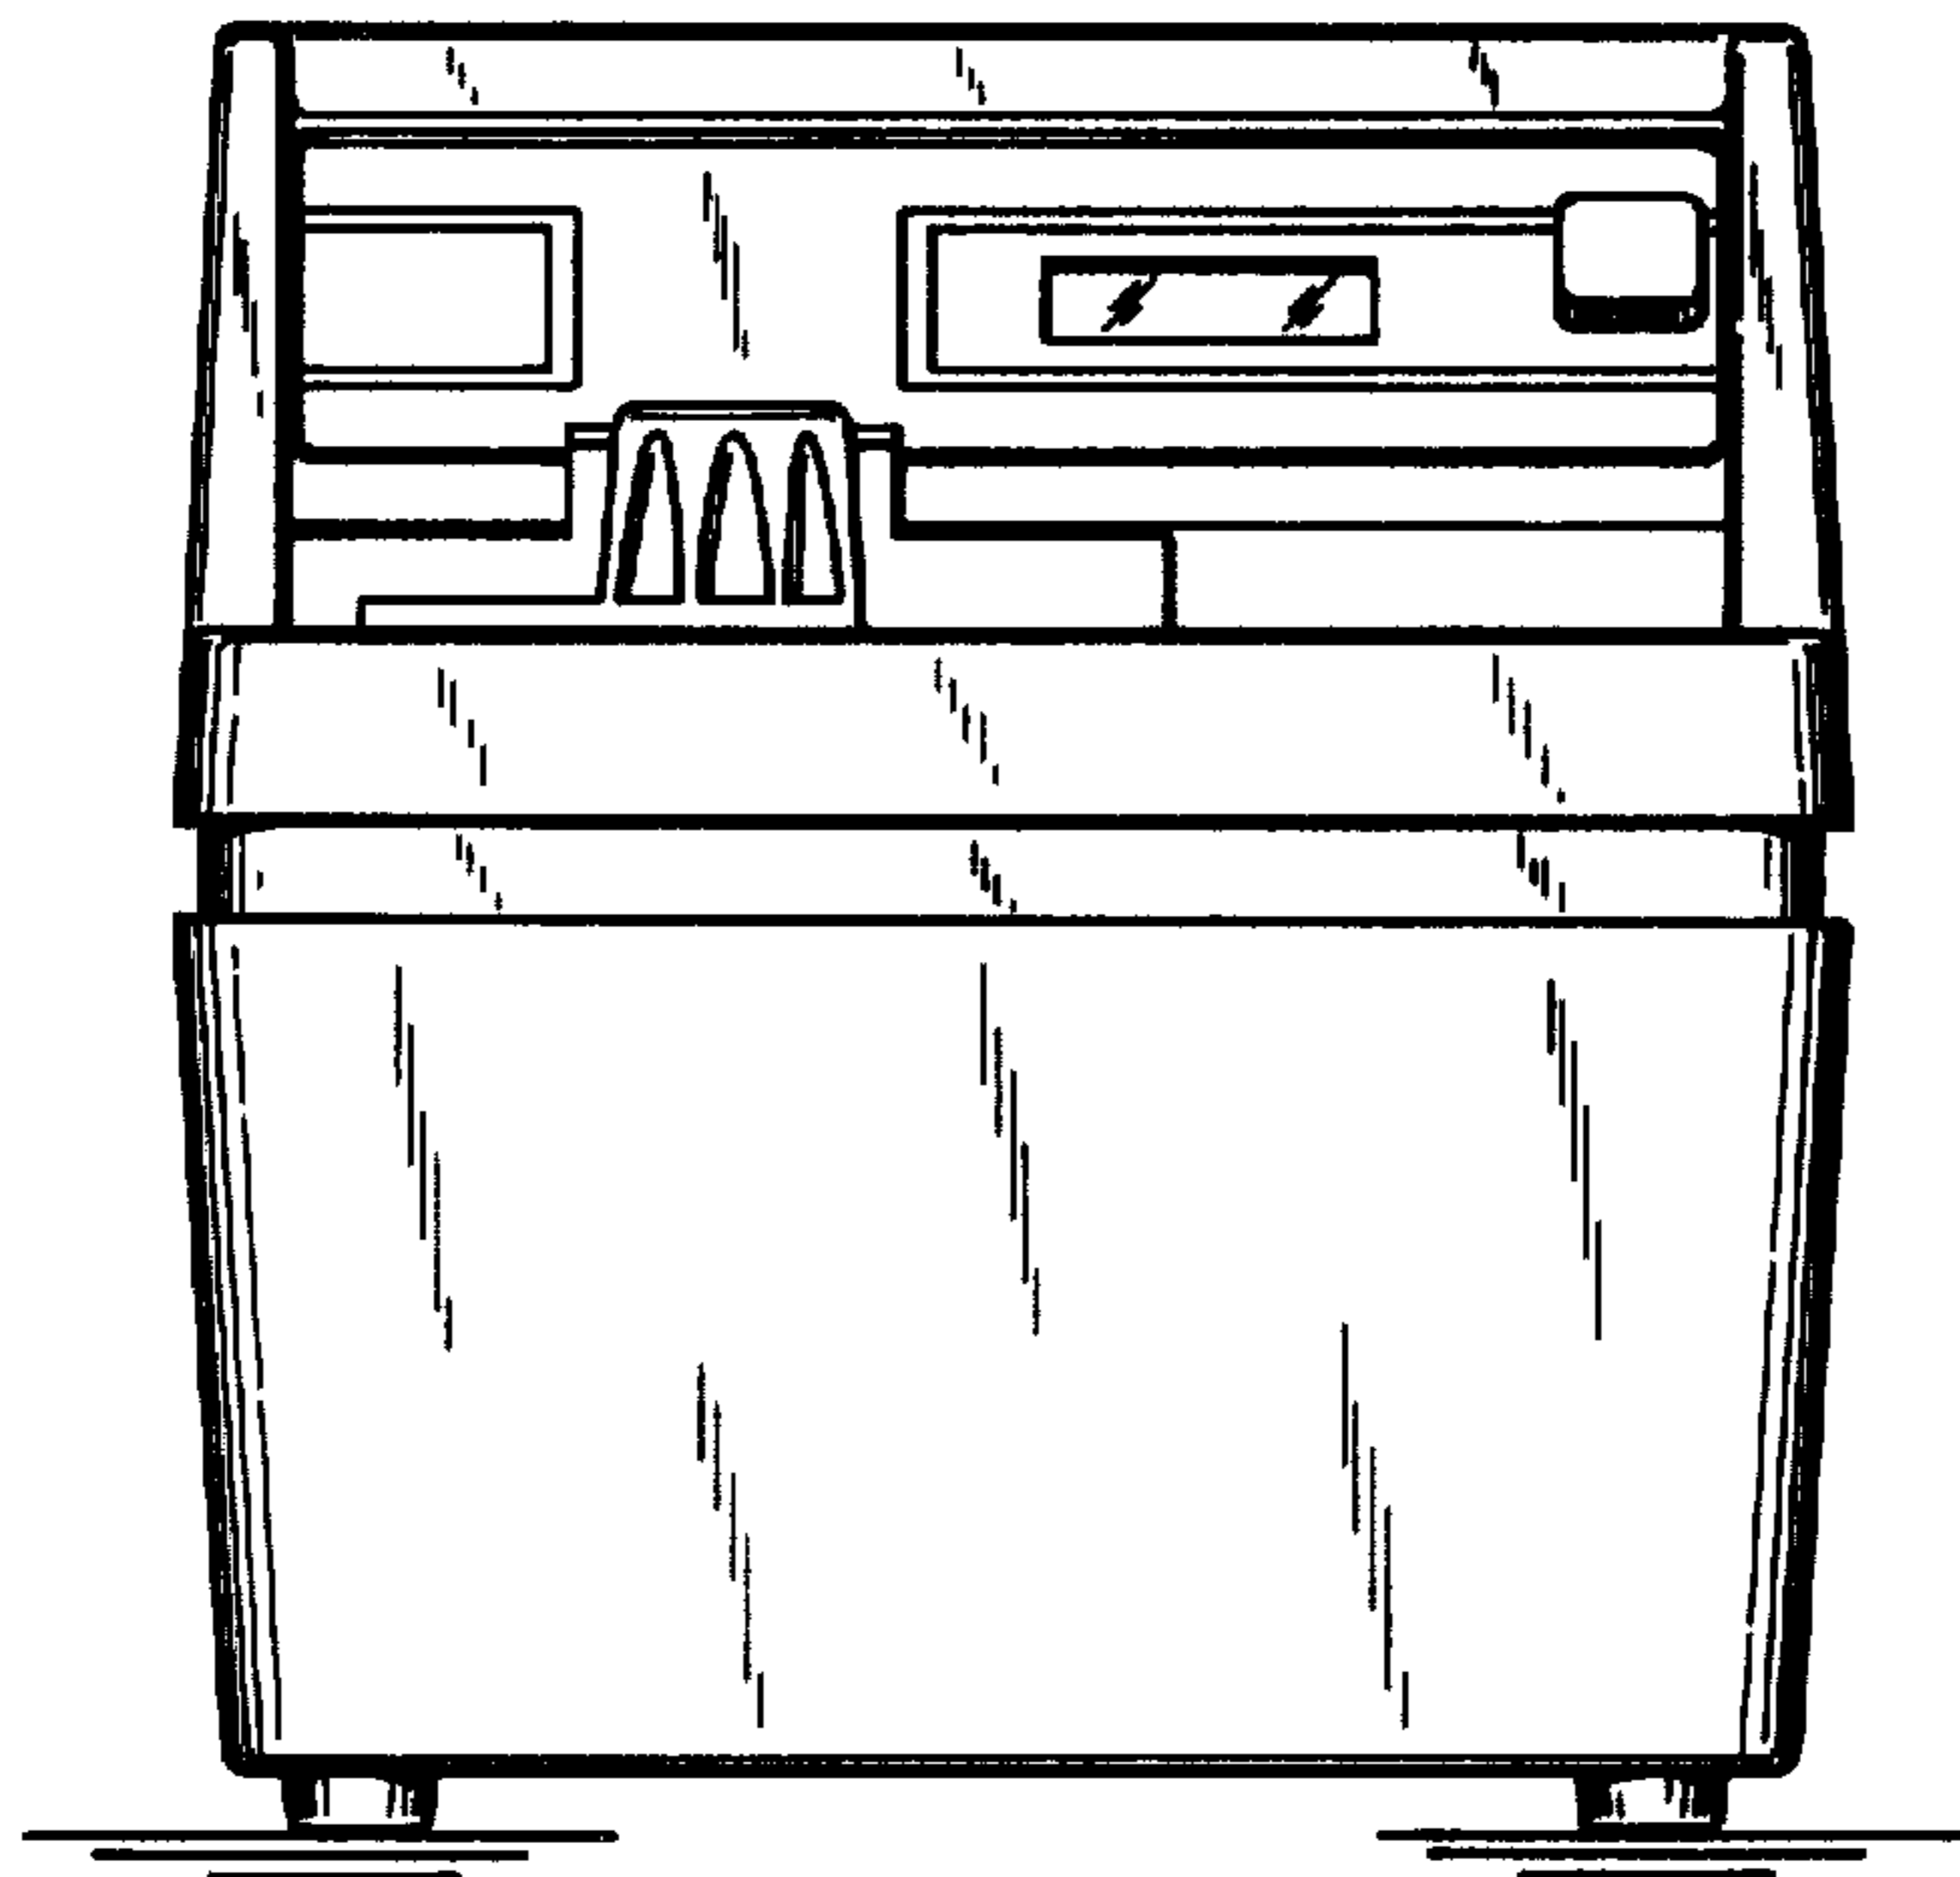


FIG. 4