

[54] **BILIRUBIN CONCENTRATION ANALYZER**

[75] Inventor: **John T. Armbruster**, Niagara Falls, N.Y.

[73] Assignee: **American Optical Corporation**, Southbridge, Mass.

[**] Term: **14 Years**

[21] Appl. No.: **9,318**

[22] Filed: **Feb. 5, 1979**

[51] Int. Cl. **D24—02**

[52] U.S. Cl. **D24/17; D24/8; D10/46; D10/81**

[58] Field of Search **D10/81, 46, 75; D24/21, D24/17, 1.1, 8; 356/39, 36, 40, 43**

[56] **References Cited**

U.S. PATENT DOCUMENTS

D. 196,044 8/1963 Malk D10/81

D. 241,275 8/1976 Green, Jr. D24/21
 D. 245,965 10/1977 Havstad D10/81 X
 D. 249,891 10/1978 Rowland et al. D24/17
 D. 252,948 9/1979 Ferreira D10/46 X
 4,156,570 5/1979 Wardlaw 356/39 X



Primary Examiner—Bernard Ansher
Attorney, Agent, or Firm—Alan H. Spencer

[57] **CLAIM**

The ornamental design for a bilirubin concentration analyzer, as shown and described.

DESCRIPTION

FIG. 1 is a top plan view of the bilirubin concentration analyzer;
 FIG. 2 is a left side view of the bilirubin concentration analyzer, its opposite side having substantially the same appearance;
 FIG. 3 is a rear view of the bilirubin concentration analyzer; and
 FIG. 4 is a front view of the bilirubin concentration analyzer.

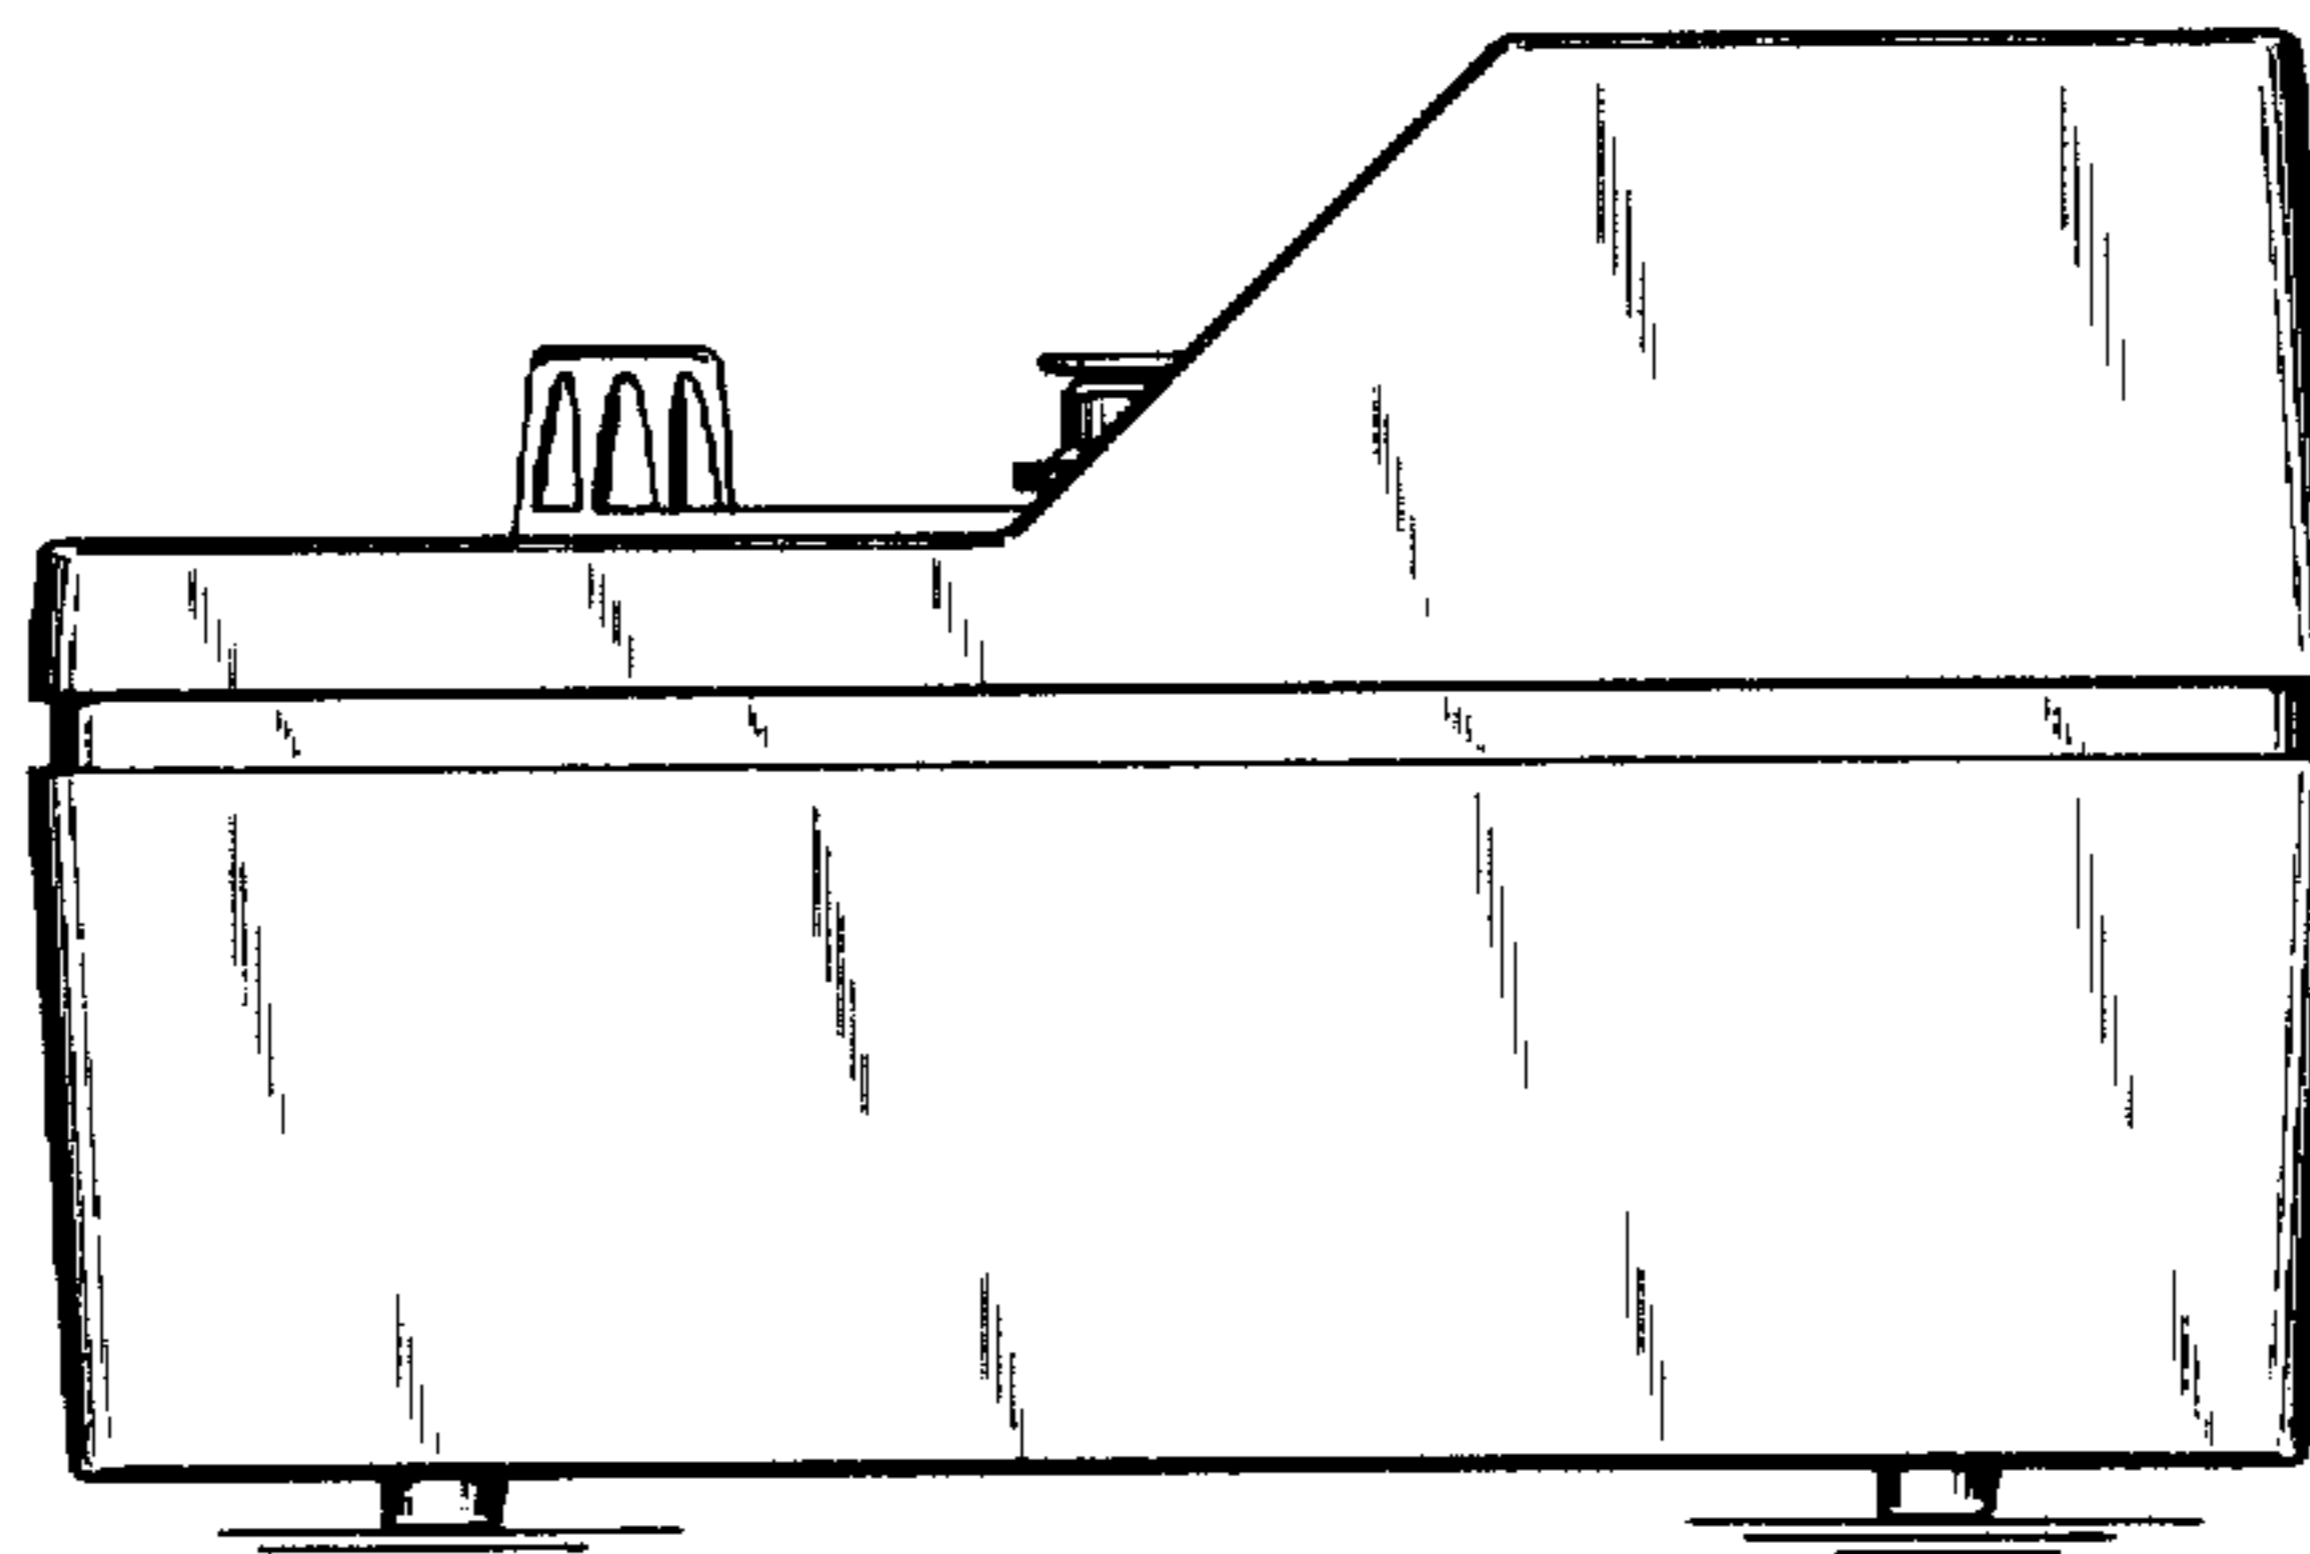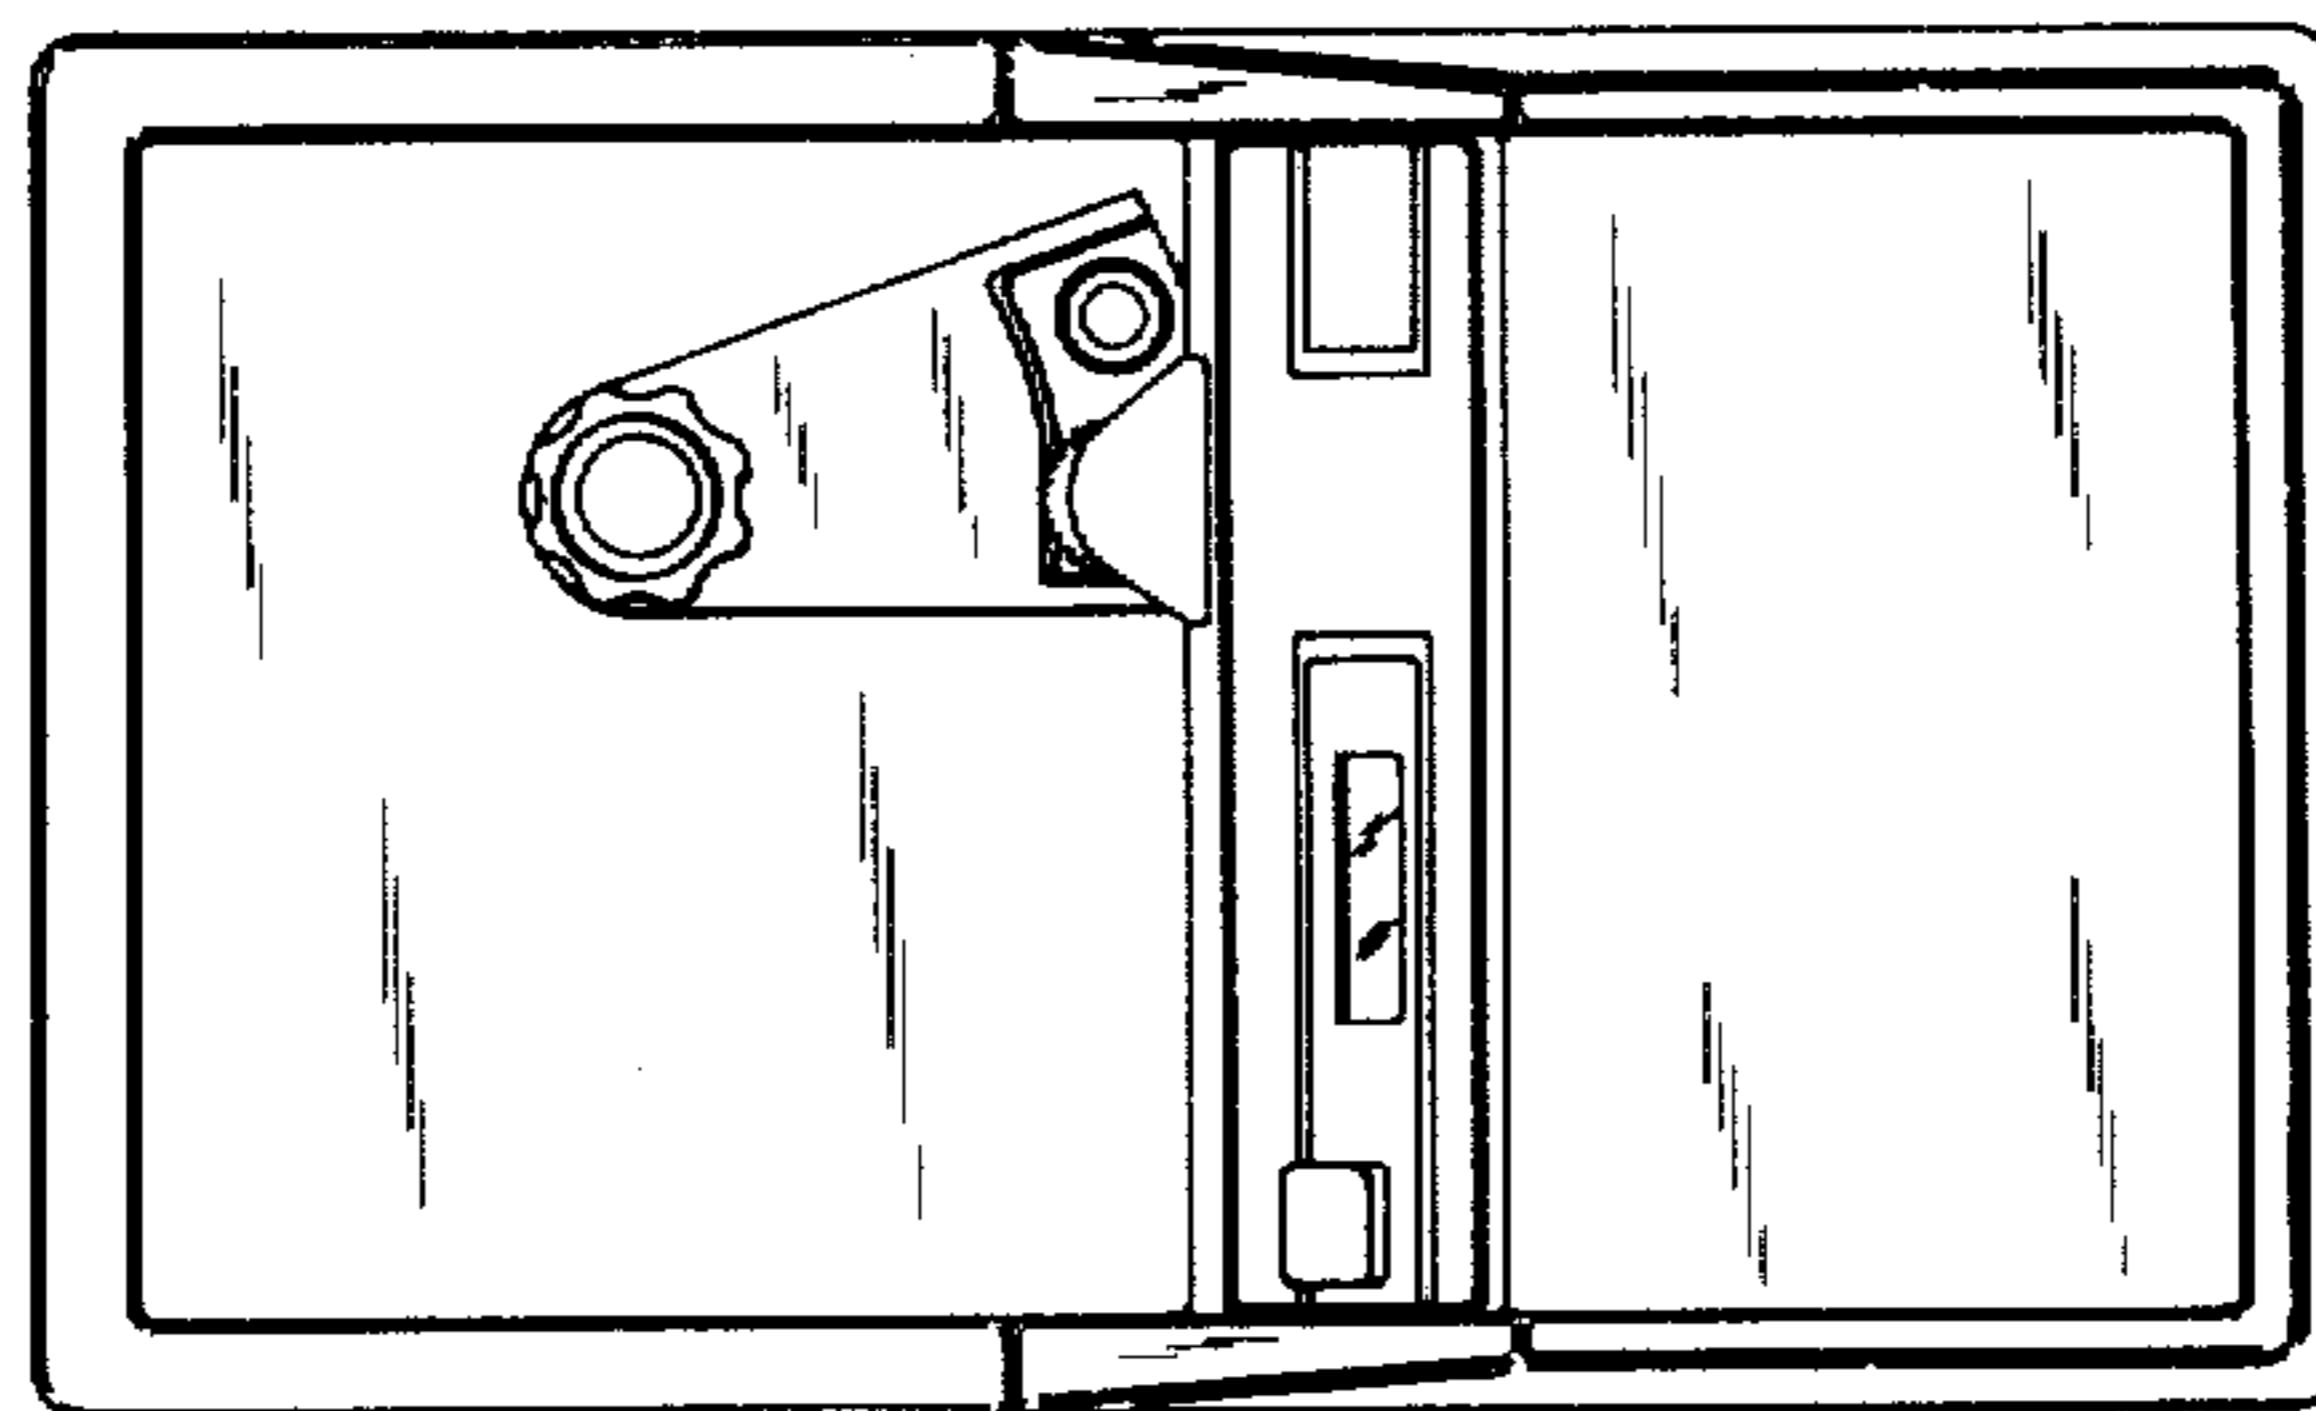

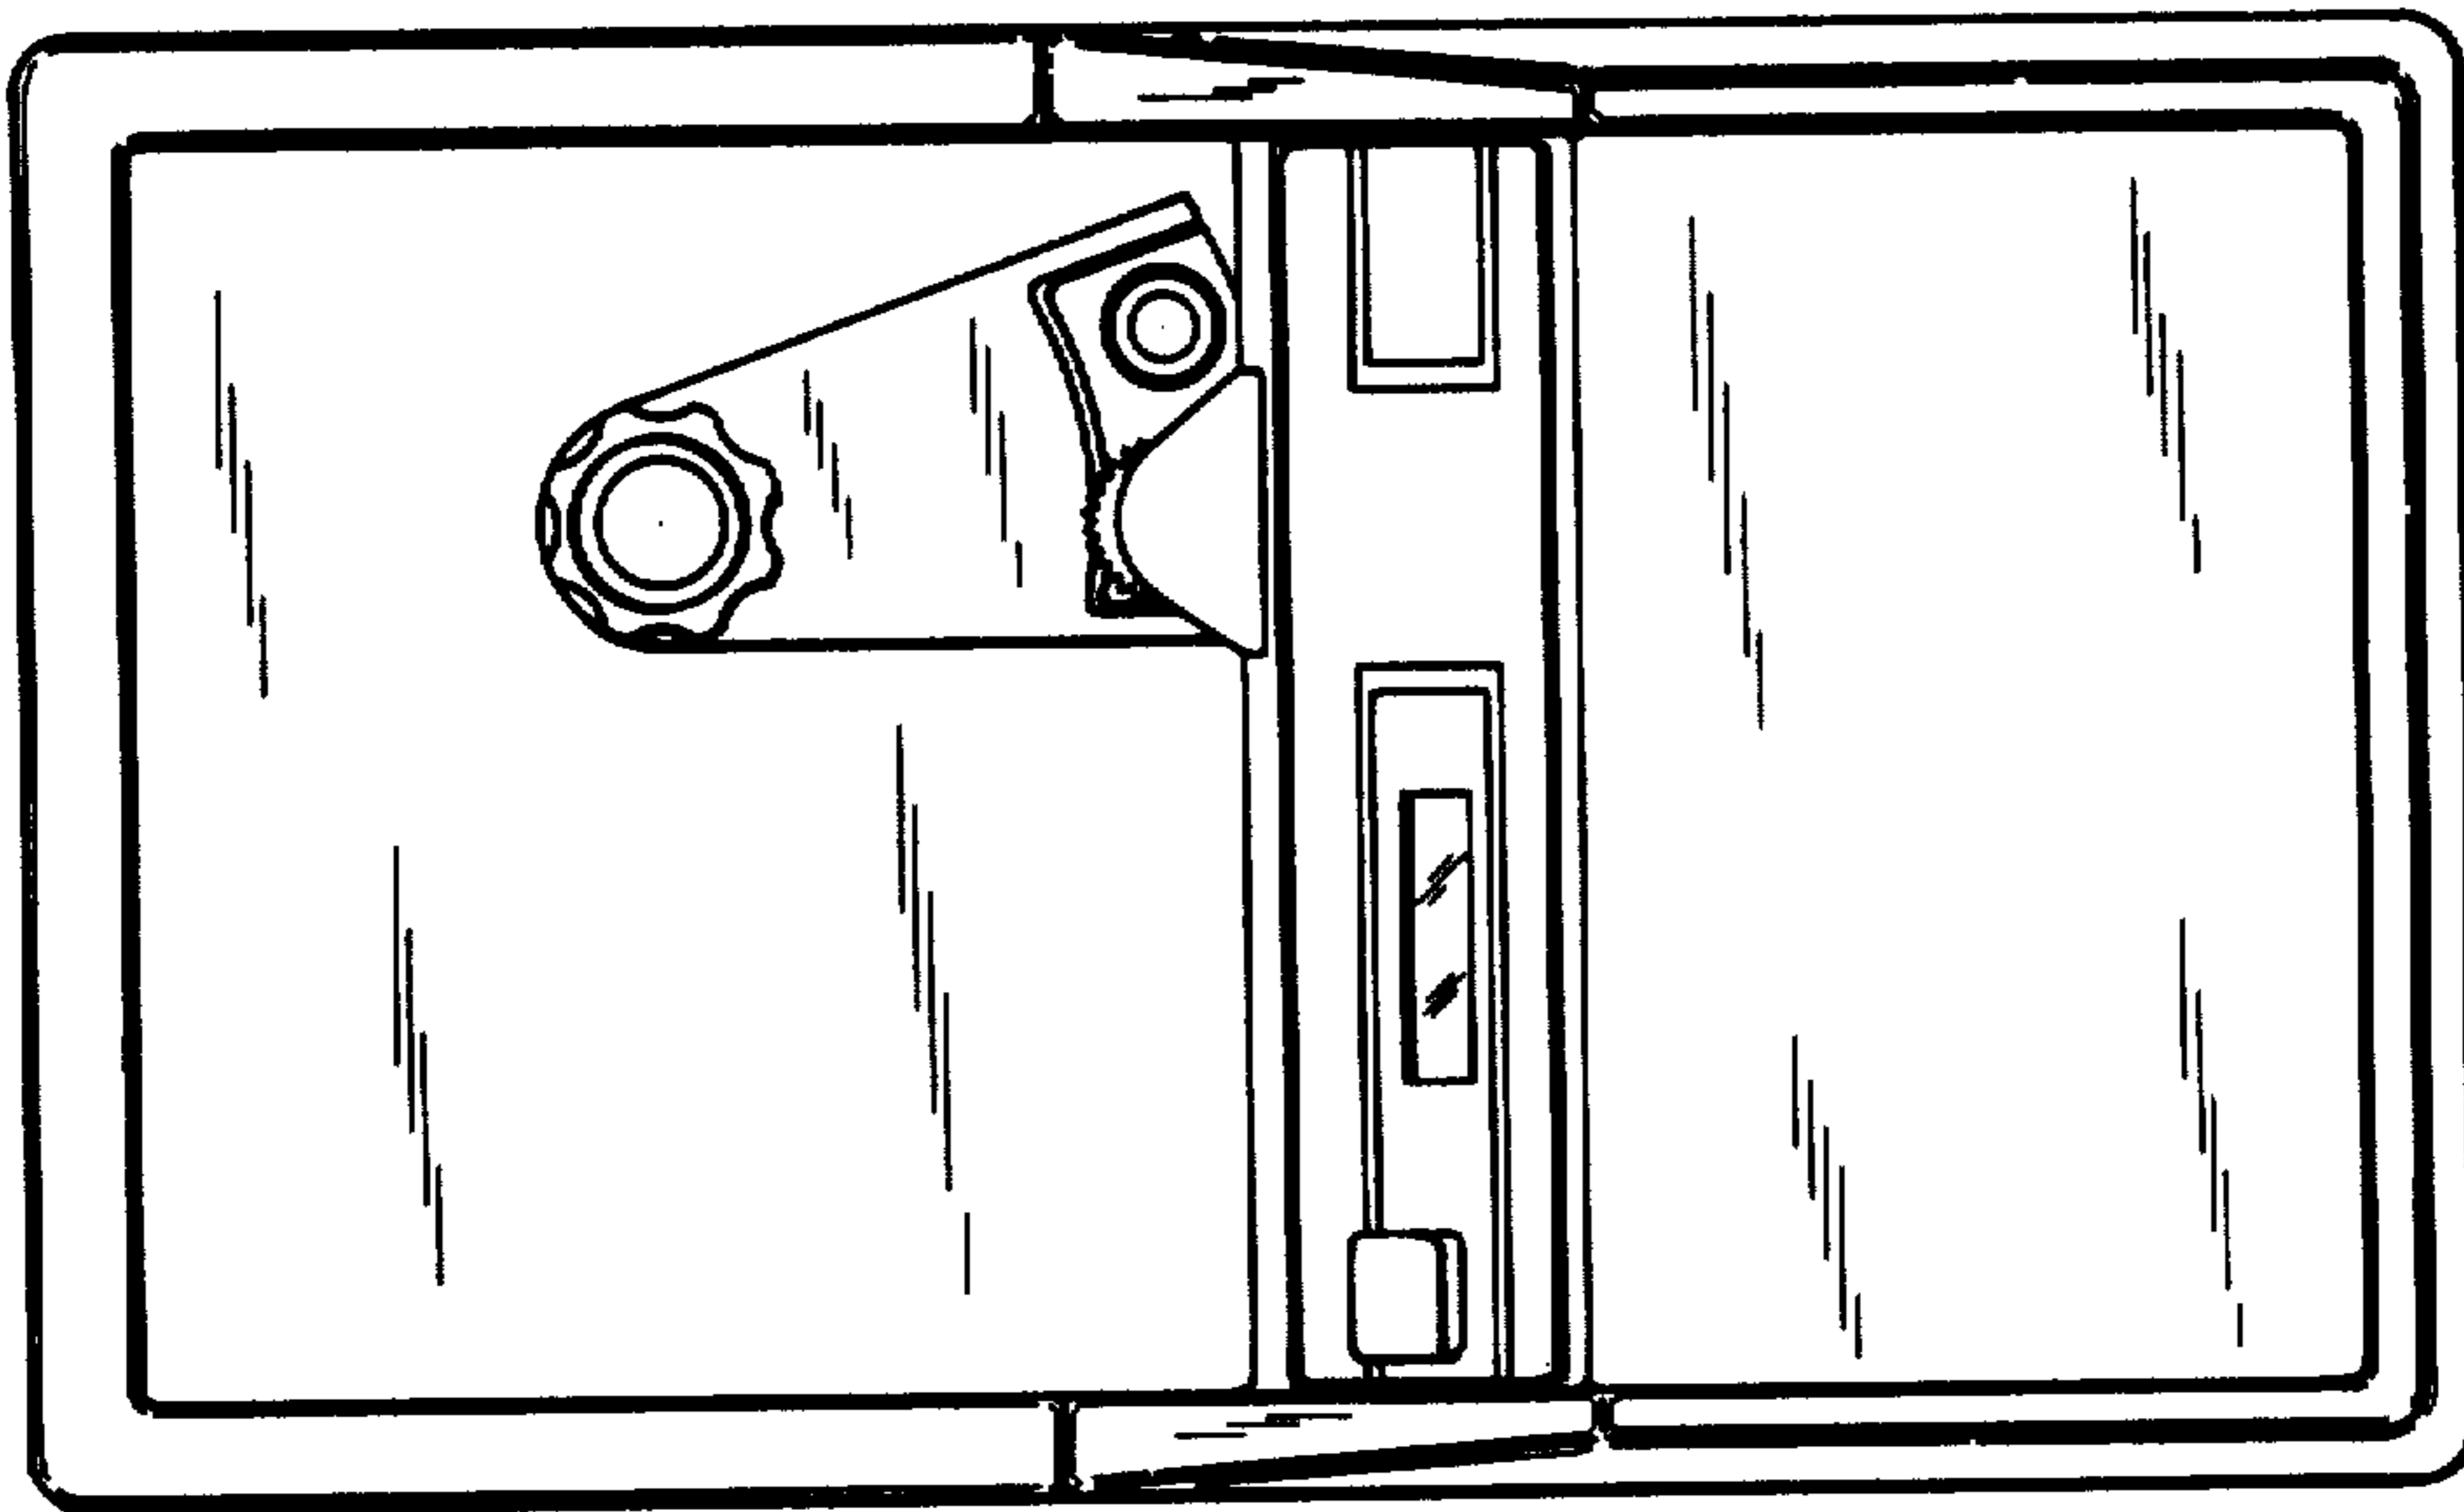


FIG. 1

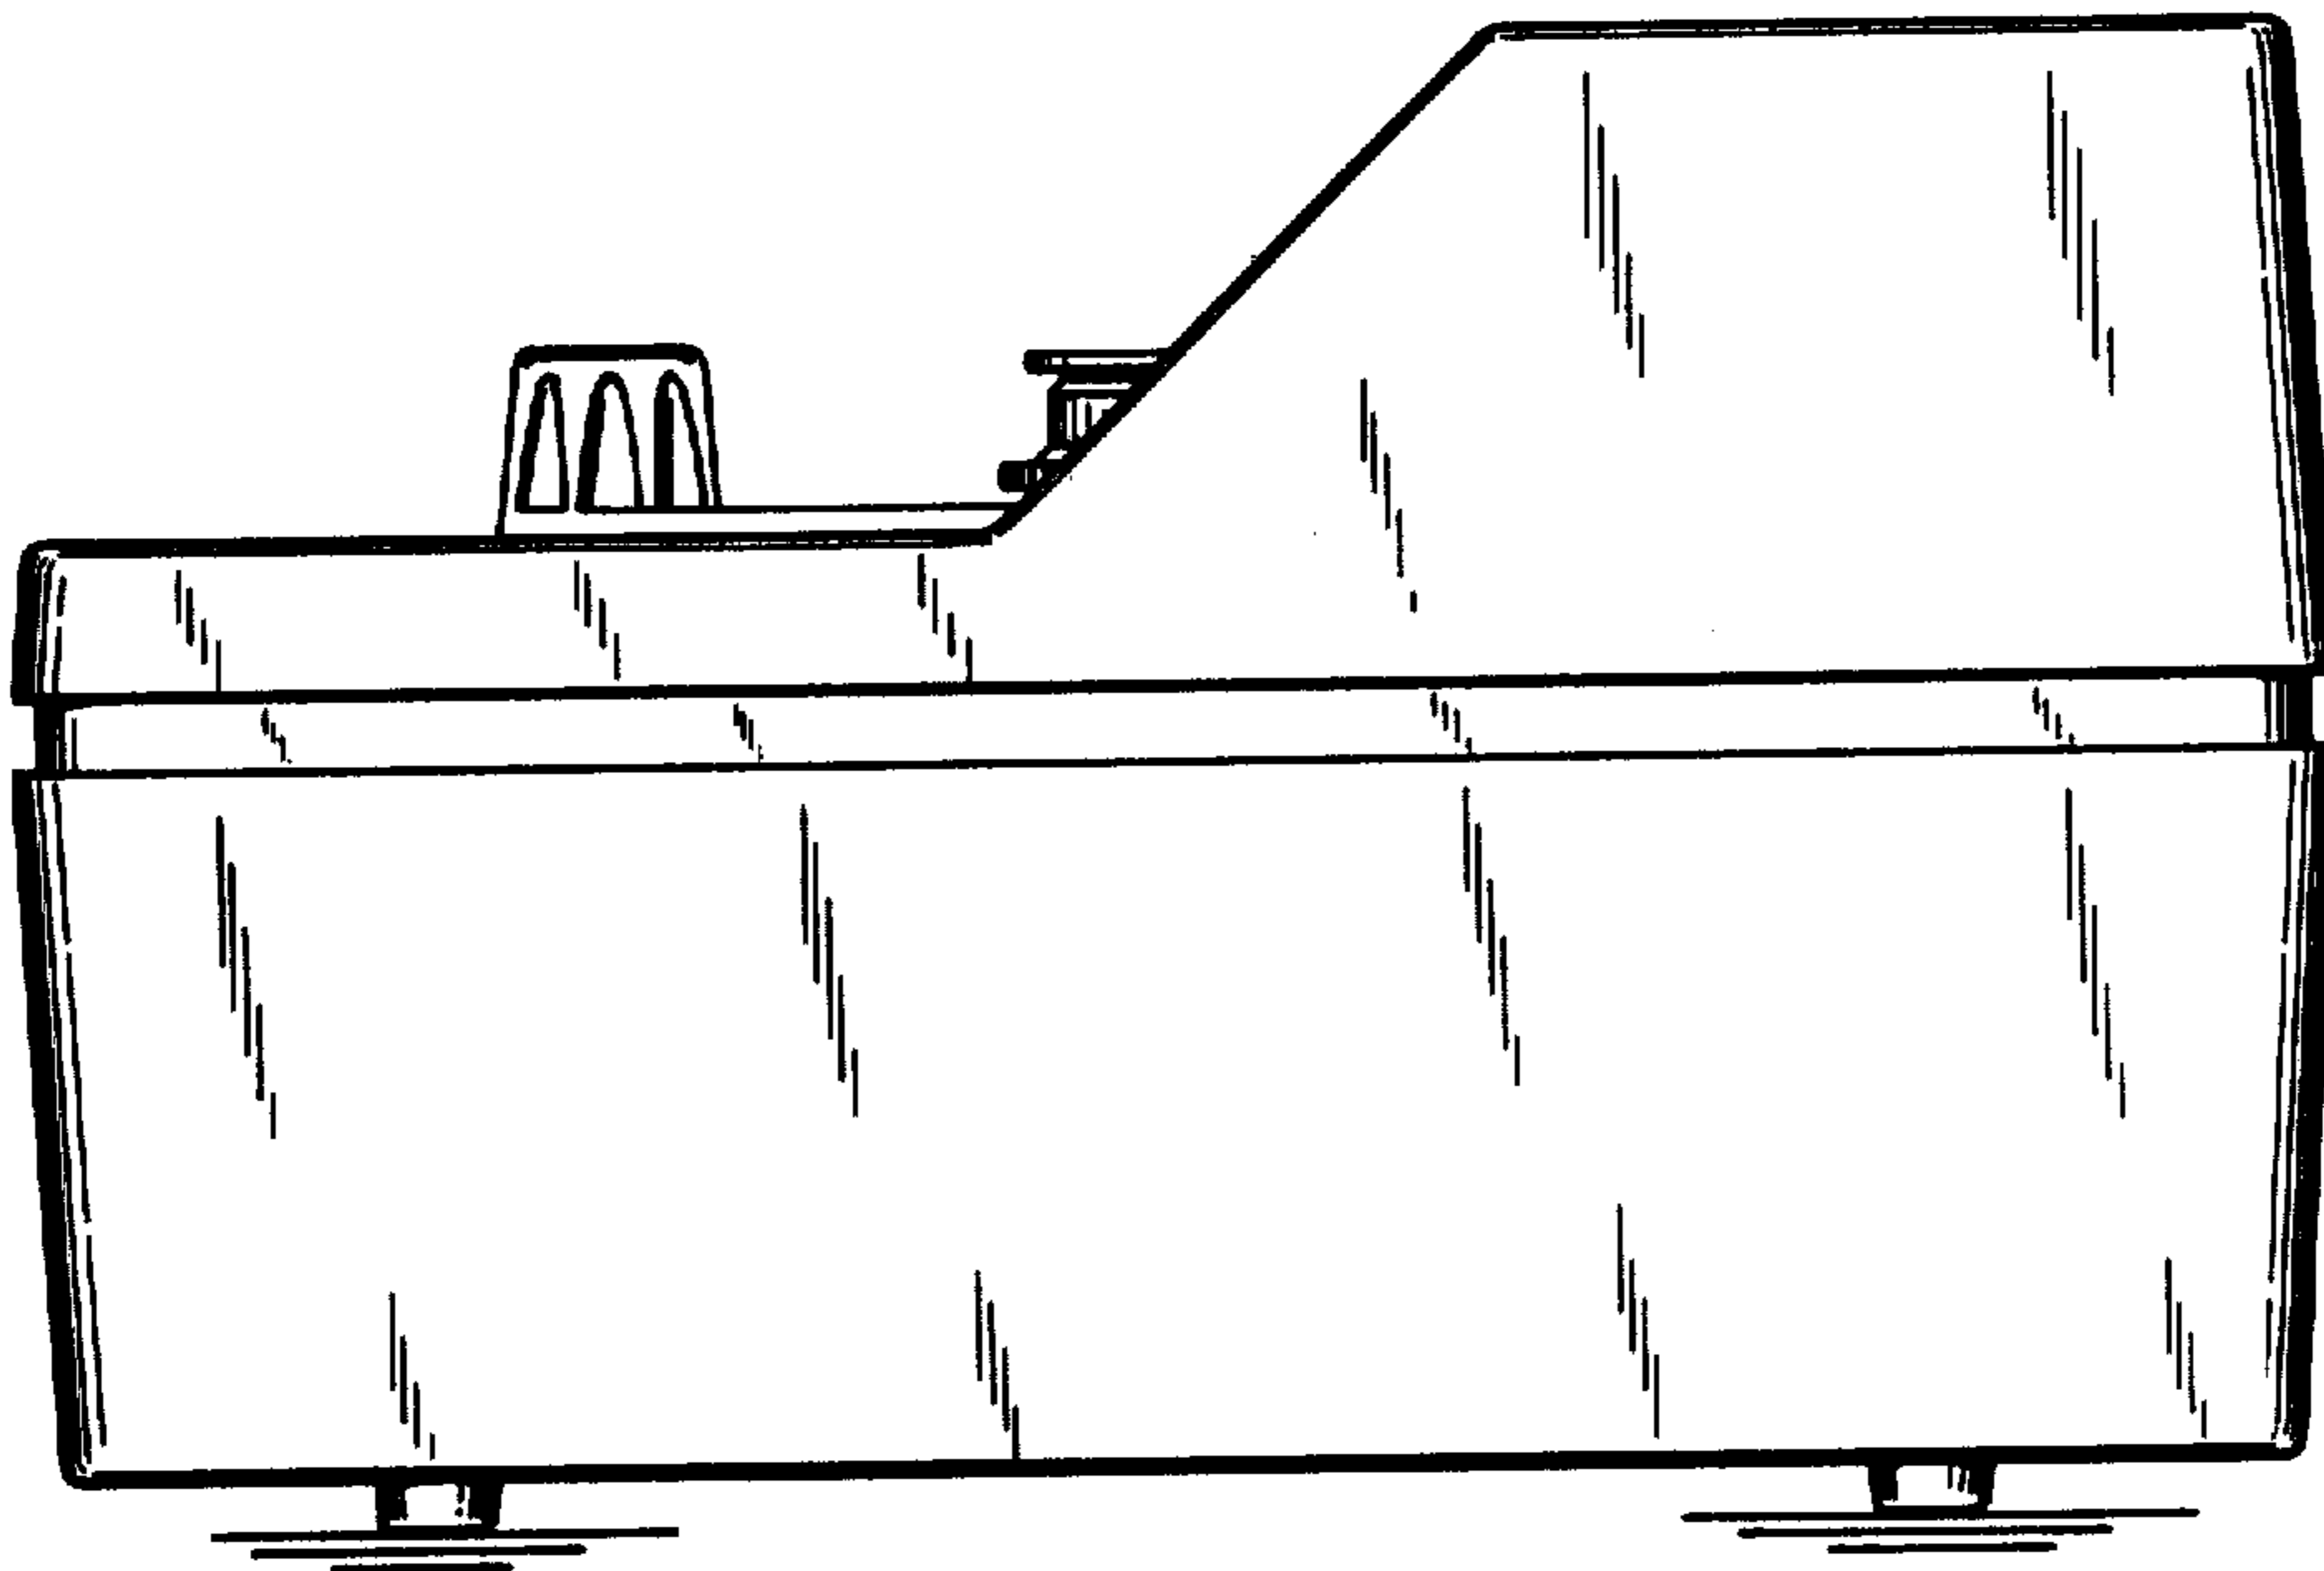


FIG. 2

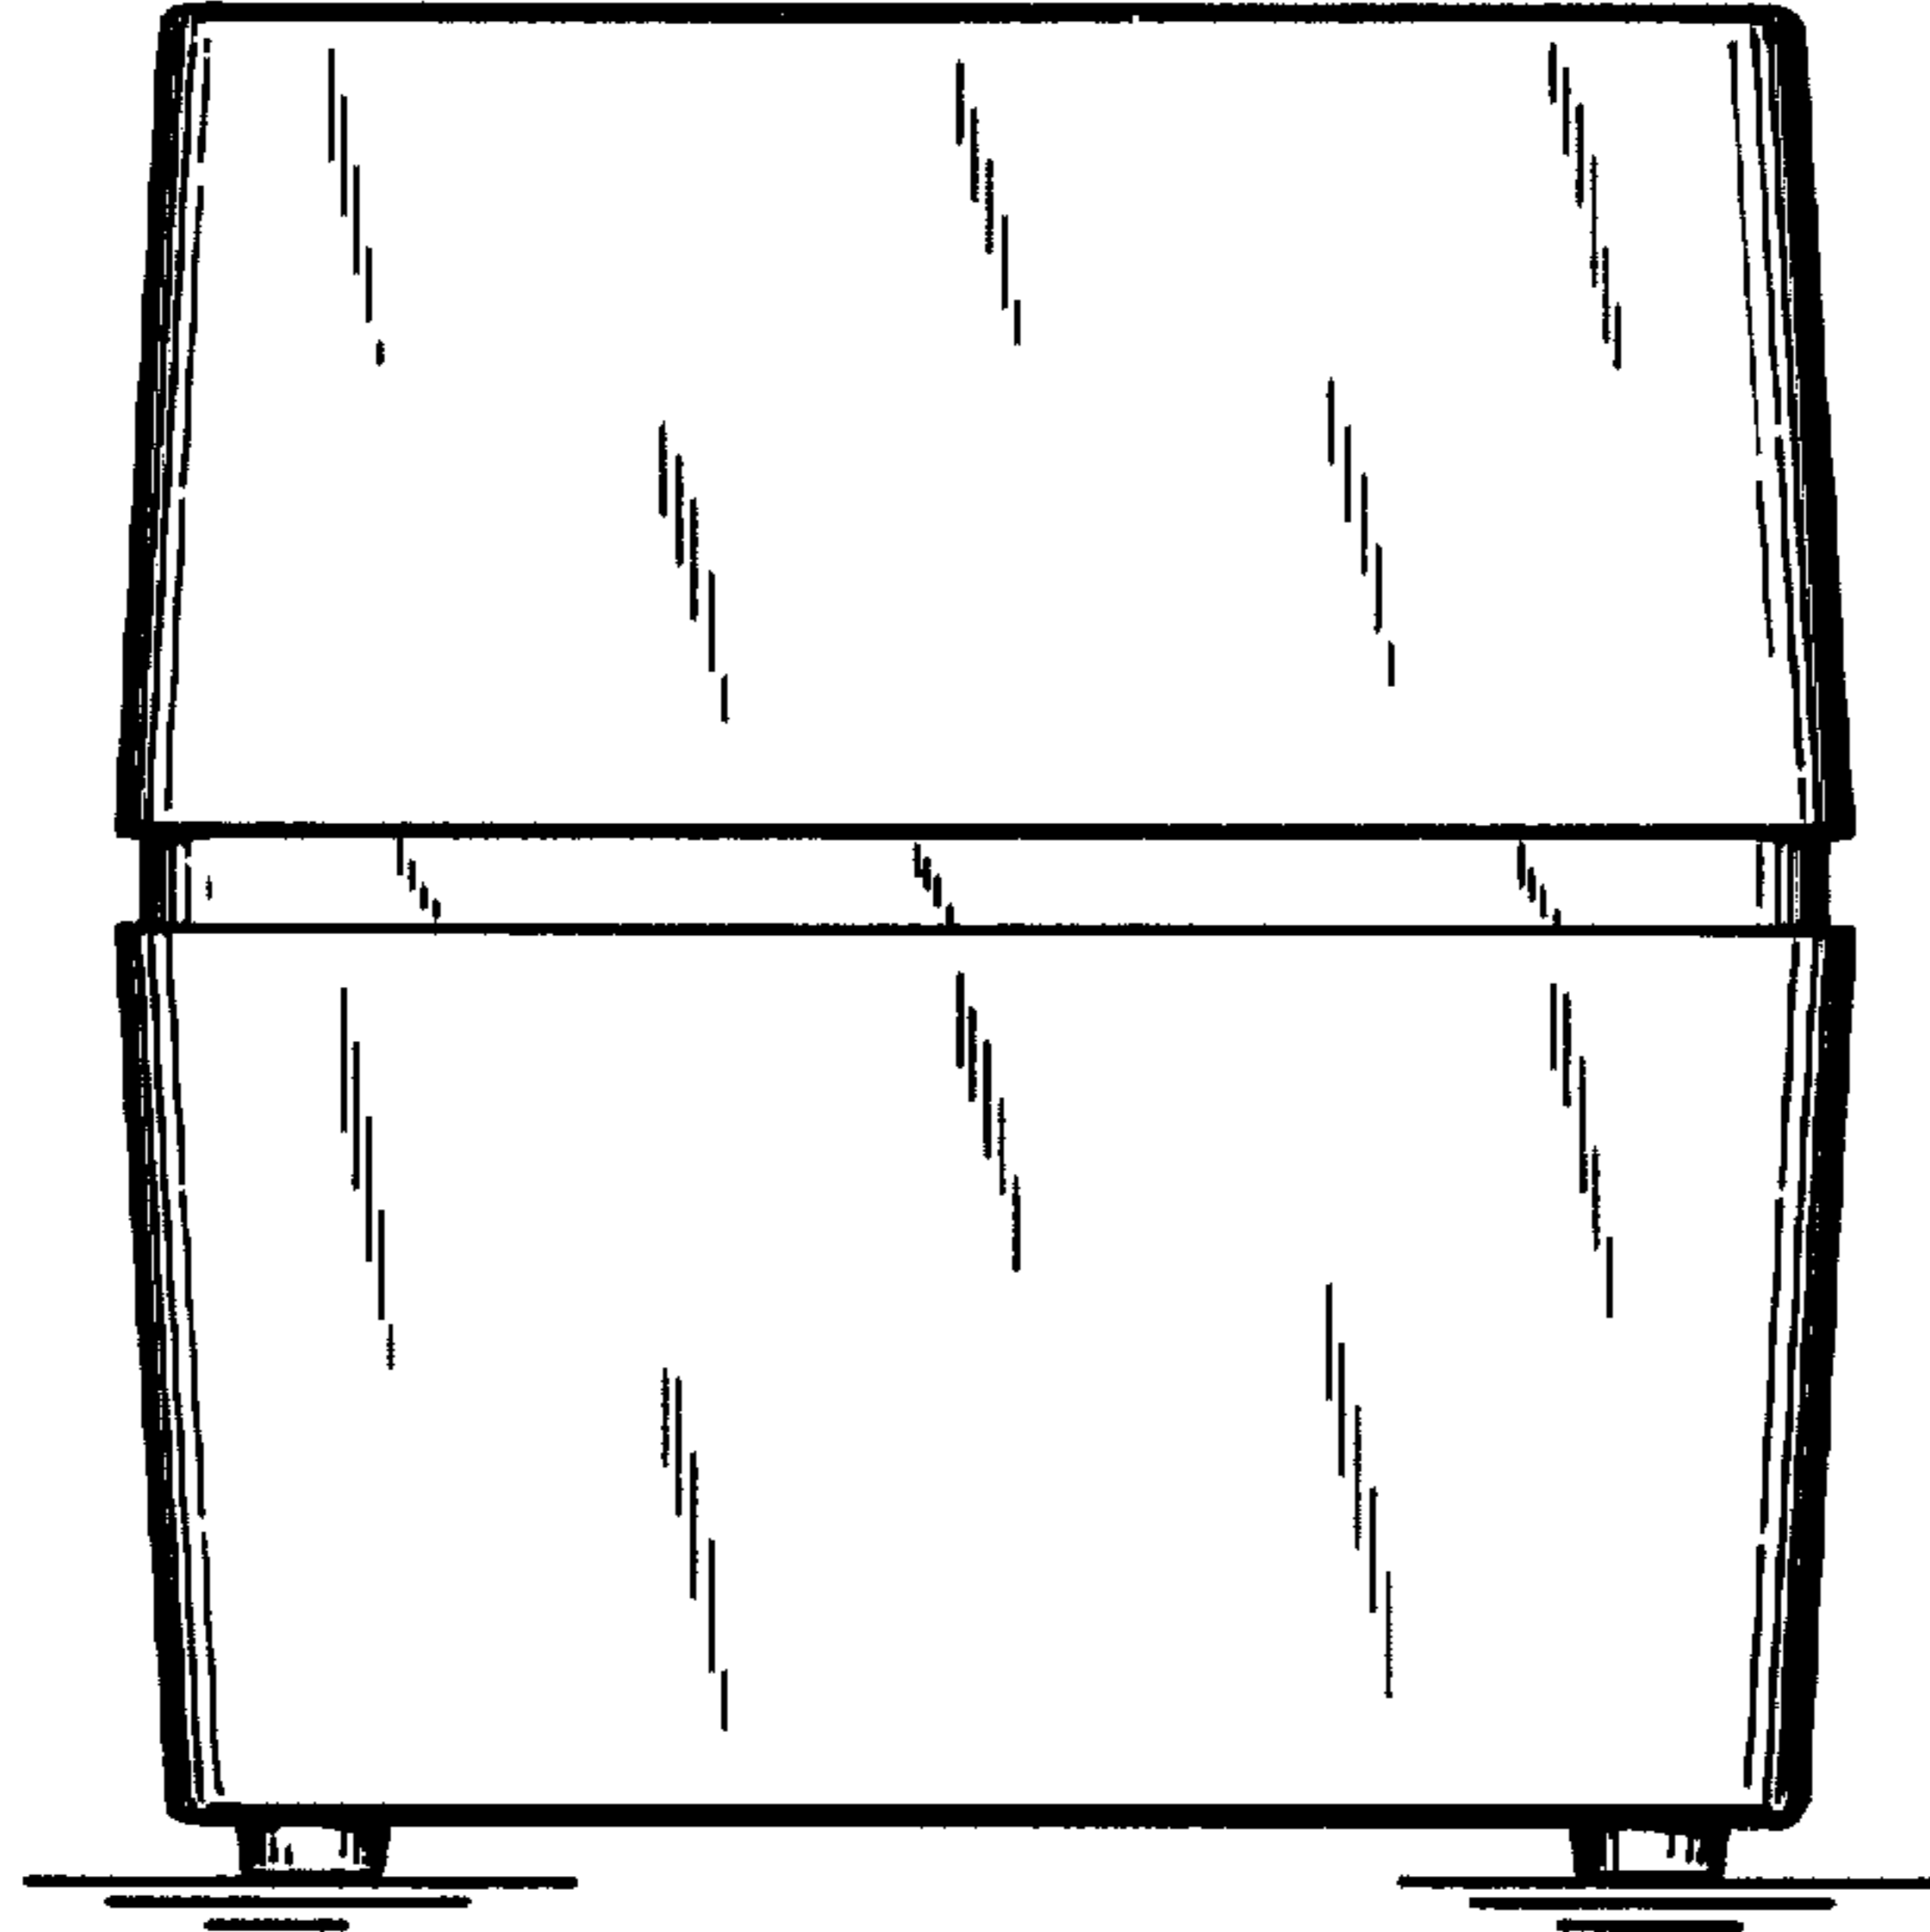


FIG. 3

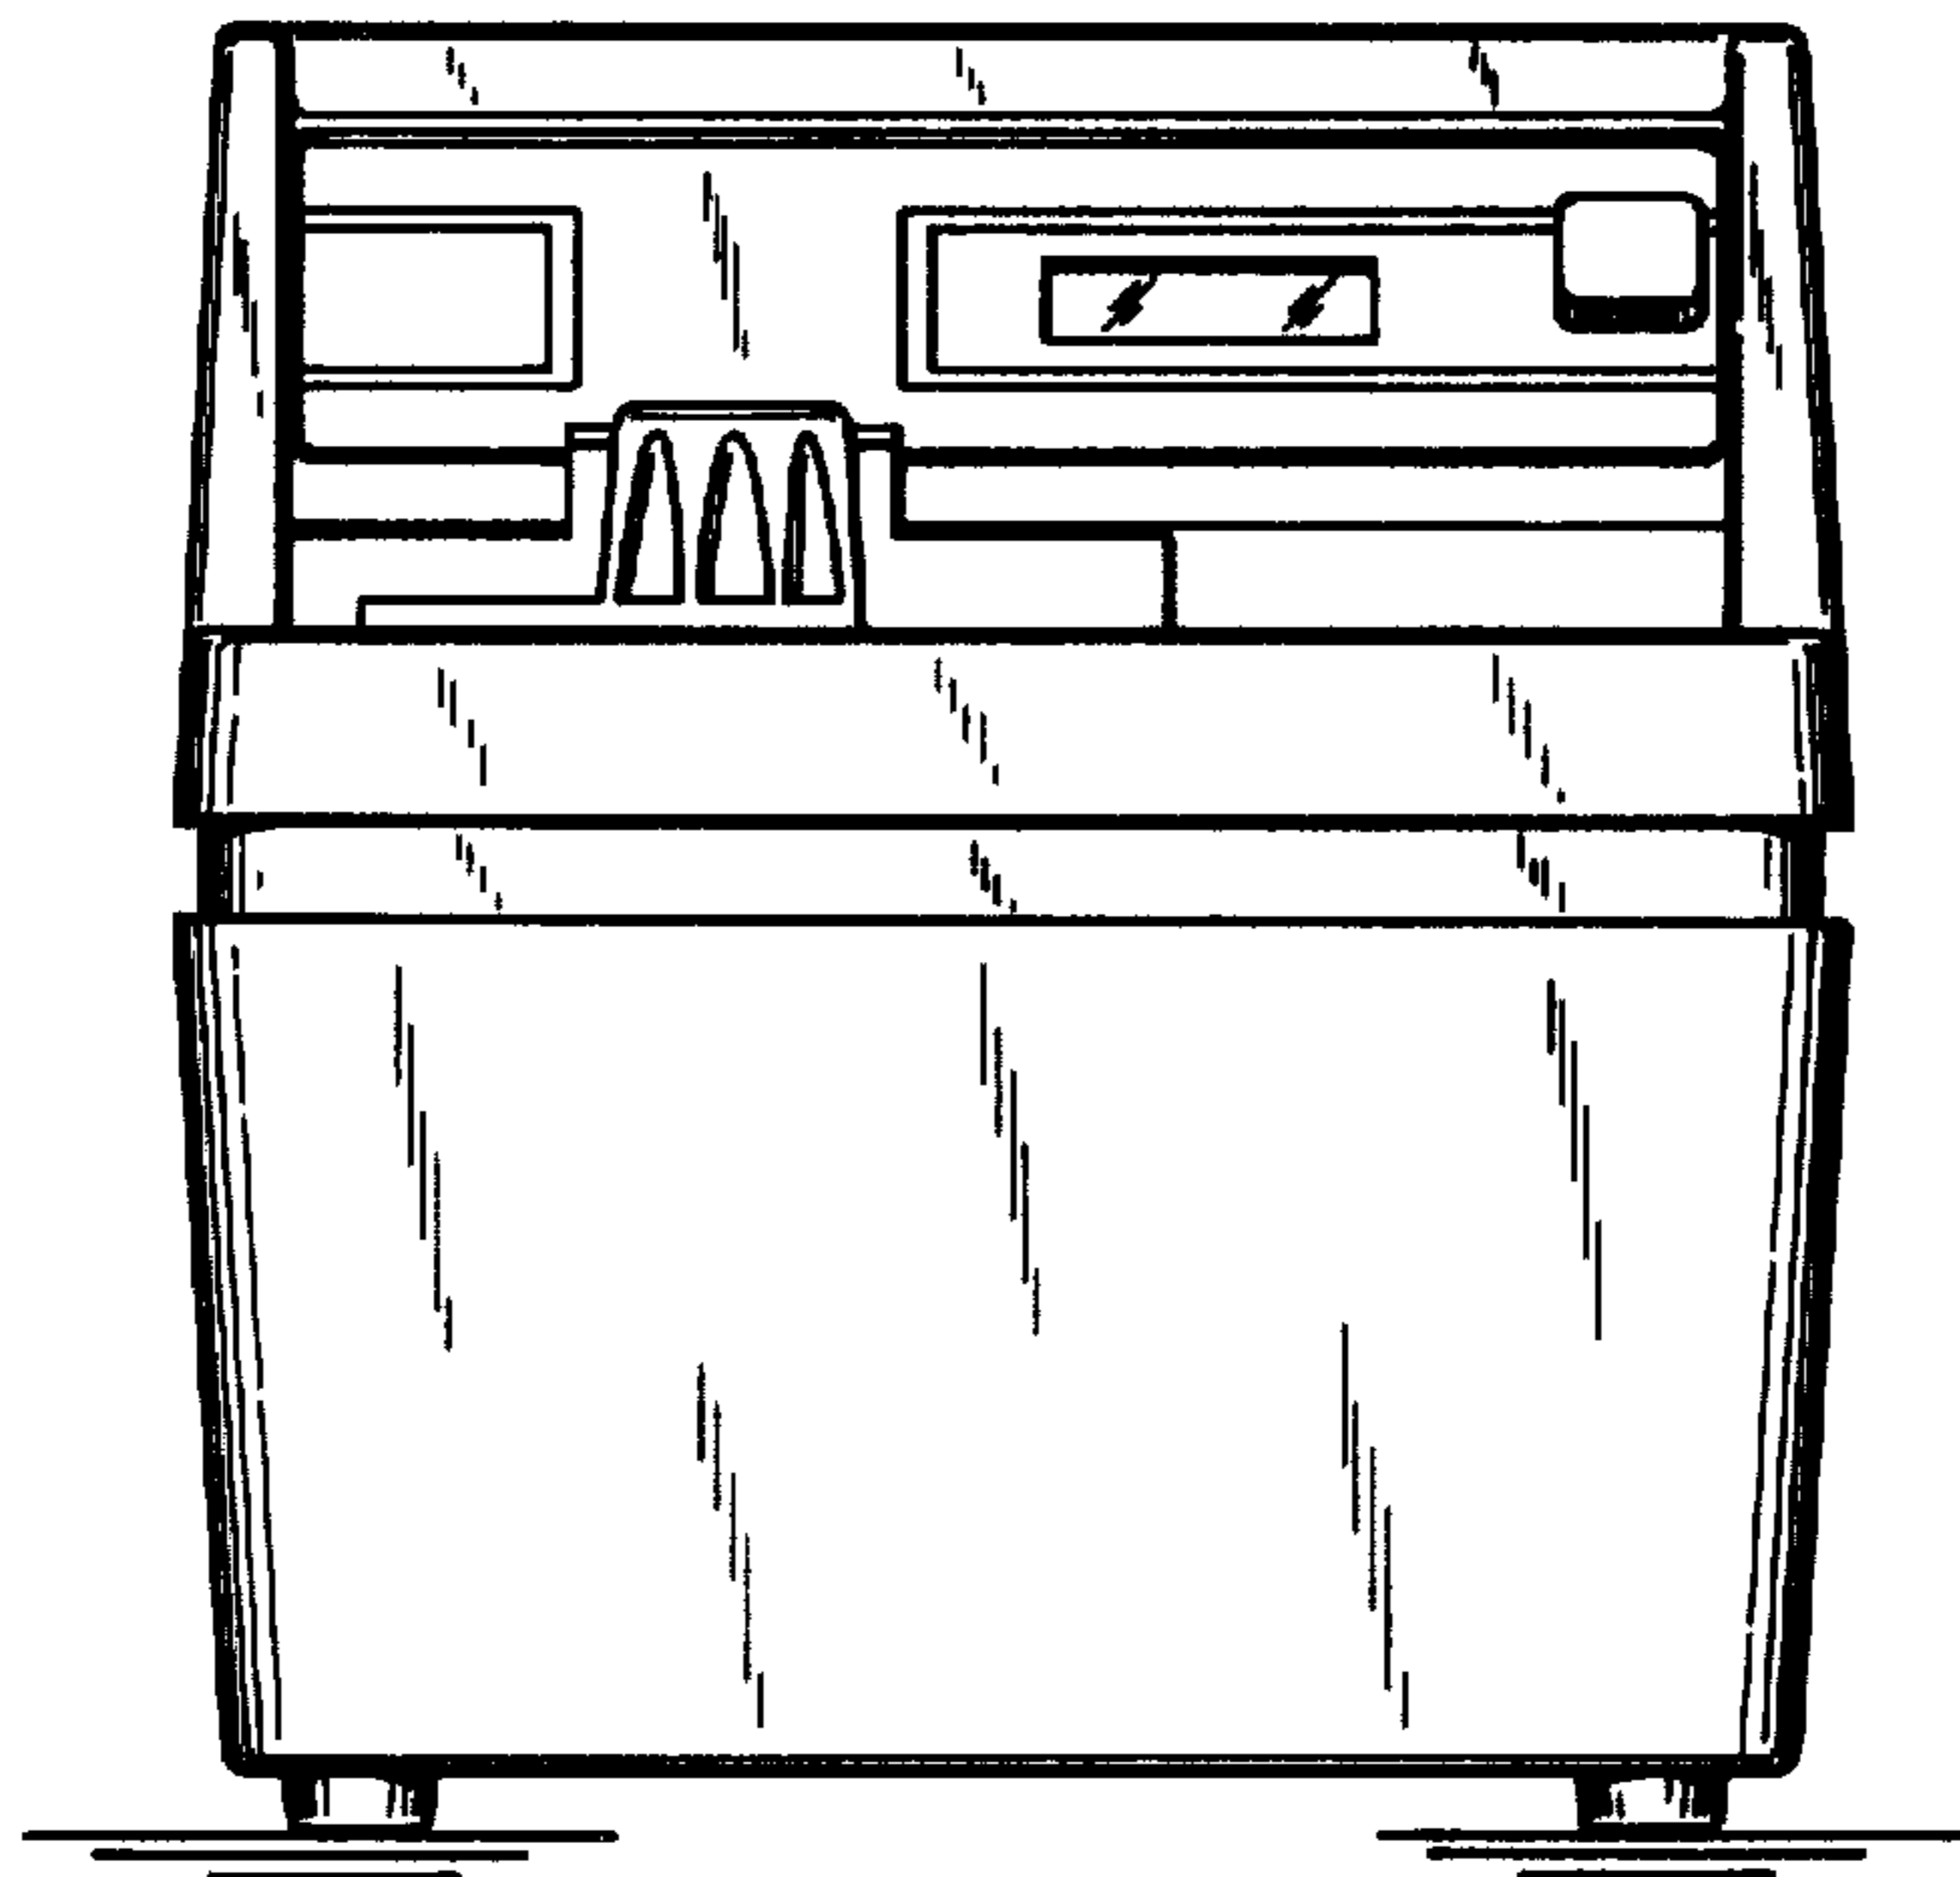


FIG. 4