

[54] **CARDIAC PACEMAKER TESTER**

[75] Inventor: **Tex Yukl**, Banks, Oreg.
[73] Assignee: **Powers Medical Systems, Inc.**,
Beaverton, Oreg.

[**] Term: **14 Years**

[21] Appl. No.: **148,996**

[22] Filed: **May 12, 1980**

[51] Int. Cl. **D10-04**

[52] U.S. Cl. **D10/78**

[58] Field of Search D10/40, 46, 75, 78,
D10/57, 60; D18/7; 324/73, 115; 364/900;
235/152, 156, 145 R

[56] **References Cited**

U.S. PATENT DOCUMENTS

- D. 227,802 7/1973 Helgesson D10/57
- D. 237,982 12/1975 Hoogesteger D10/75 X
- D. 240,409 7/1976 Roberts D10/78
- D. 248,419 7/1978 Beitler D18/7
- D. 248,595 7/1978 Beitler D18/7
- D. 249,388 9/1978 Sulek D18/7

- D. 249,479 9/1978 Rasmussen D10/78
- D. 250,934 1/1979 Fannin D10/40
- D. 252,948 9/1979 Ferreira D10/46 X
- B 534,334 3/1976 Bell D10/78 X
- 4,079,459 3/1978 Grant D18/7 X

OTHER PUBLICATIONS

Industrial Equipment News-1/78-p. S-17-Digital Multi-meter at right.

Primary Examiner-Nelson C. Holtje
Attorney, Agent, or Firm-Chernoff & Vilhauer

[57] **CLAIM**

The ornamental design for a cardiac pacemaker tester, as shown and described.

DESCRIPTION

FIG. 1 is a top and left front perspective view of a cardiac pacemaker tester showing my new design;
FIG. 2 is a top plan view thereof;
FIG. 3 is a left side elevational view thereof, the right side being a mirror image thereto;
FIG. 4 is a bottom plan view thereof;
FIG. 5 is a rear elevational view thereof; and
FIG. 6 is a front elevational view thereof.

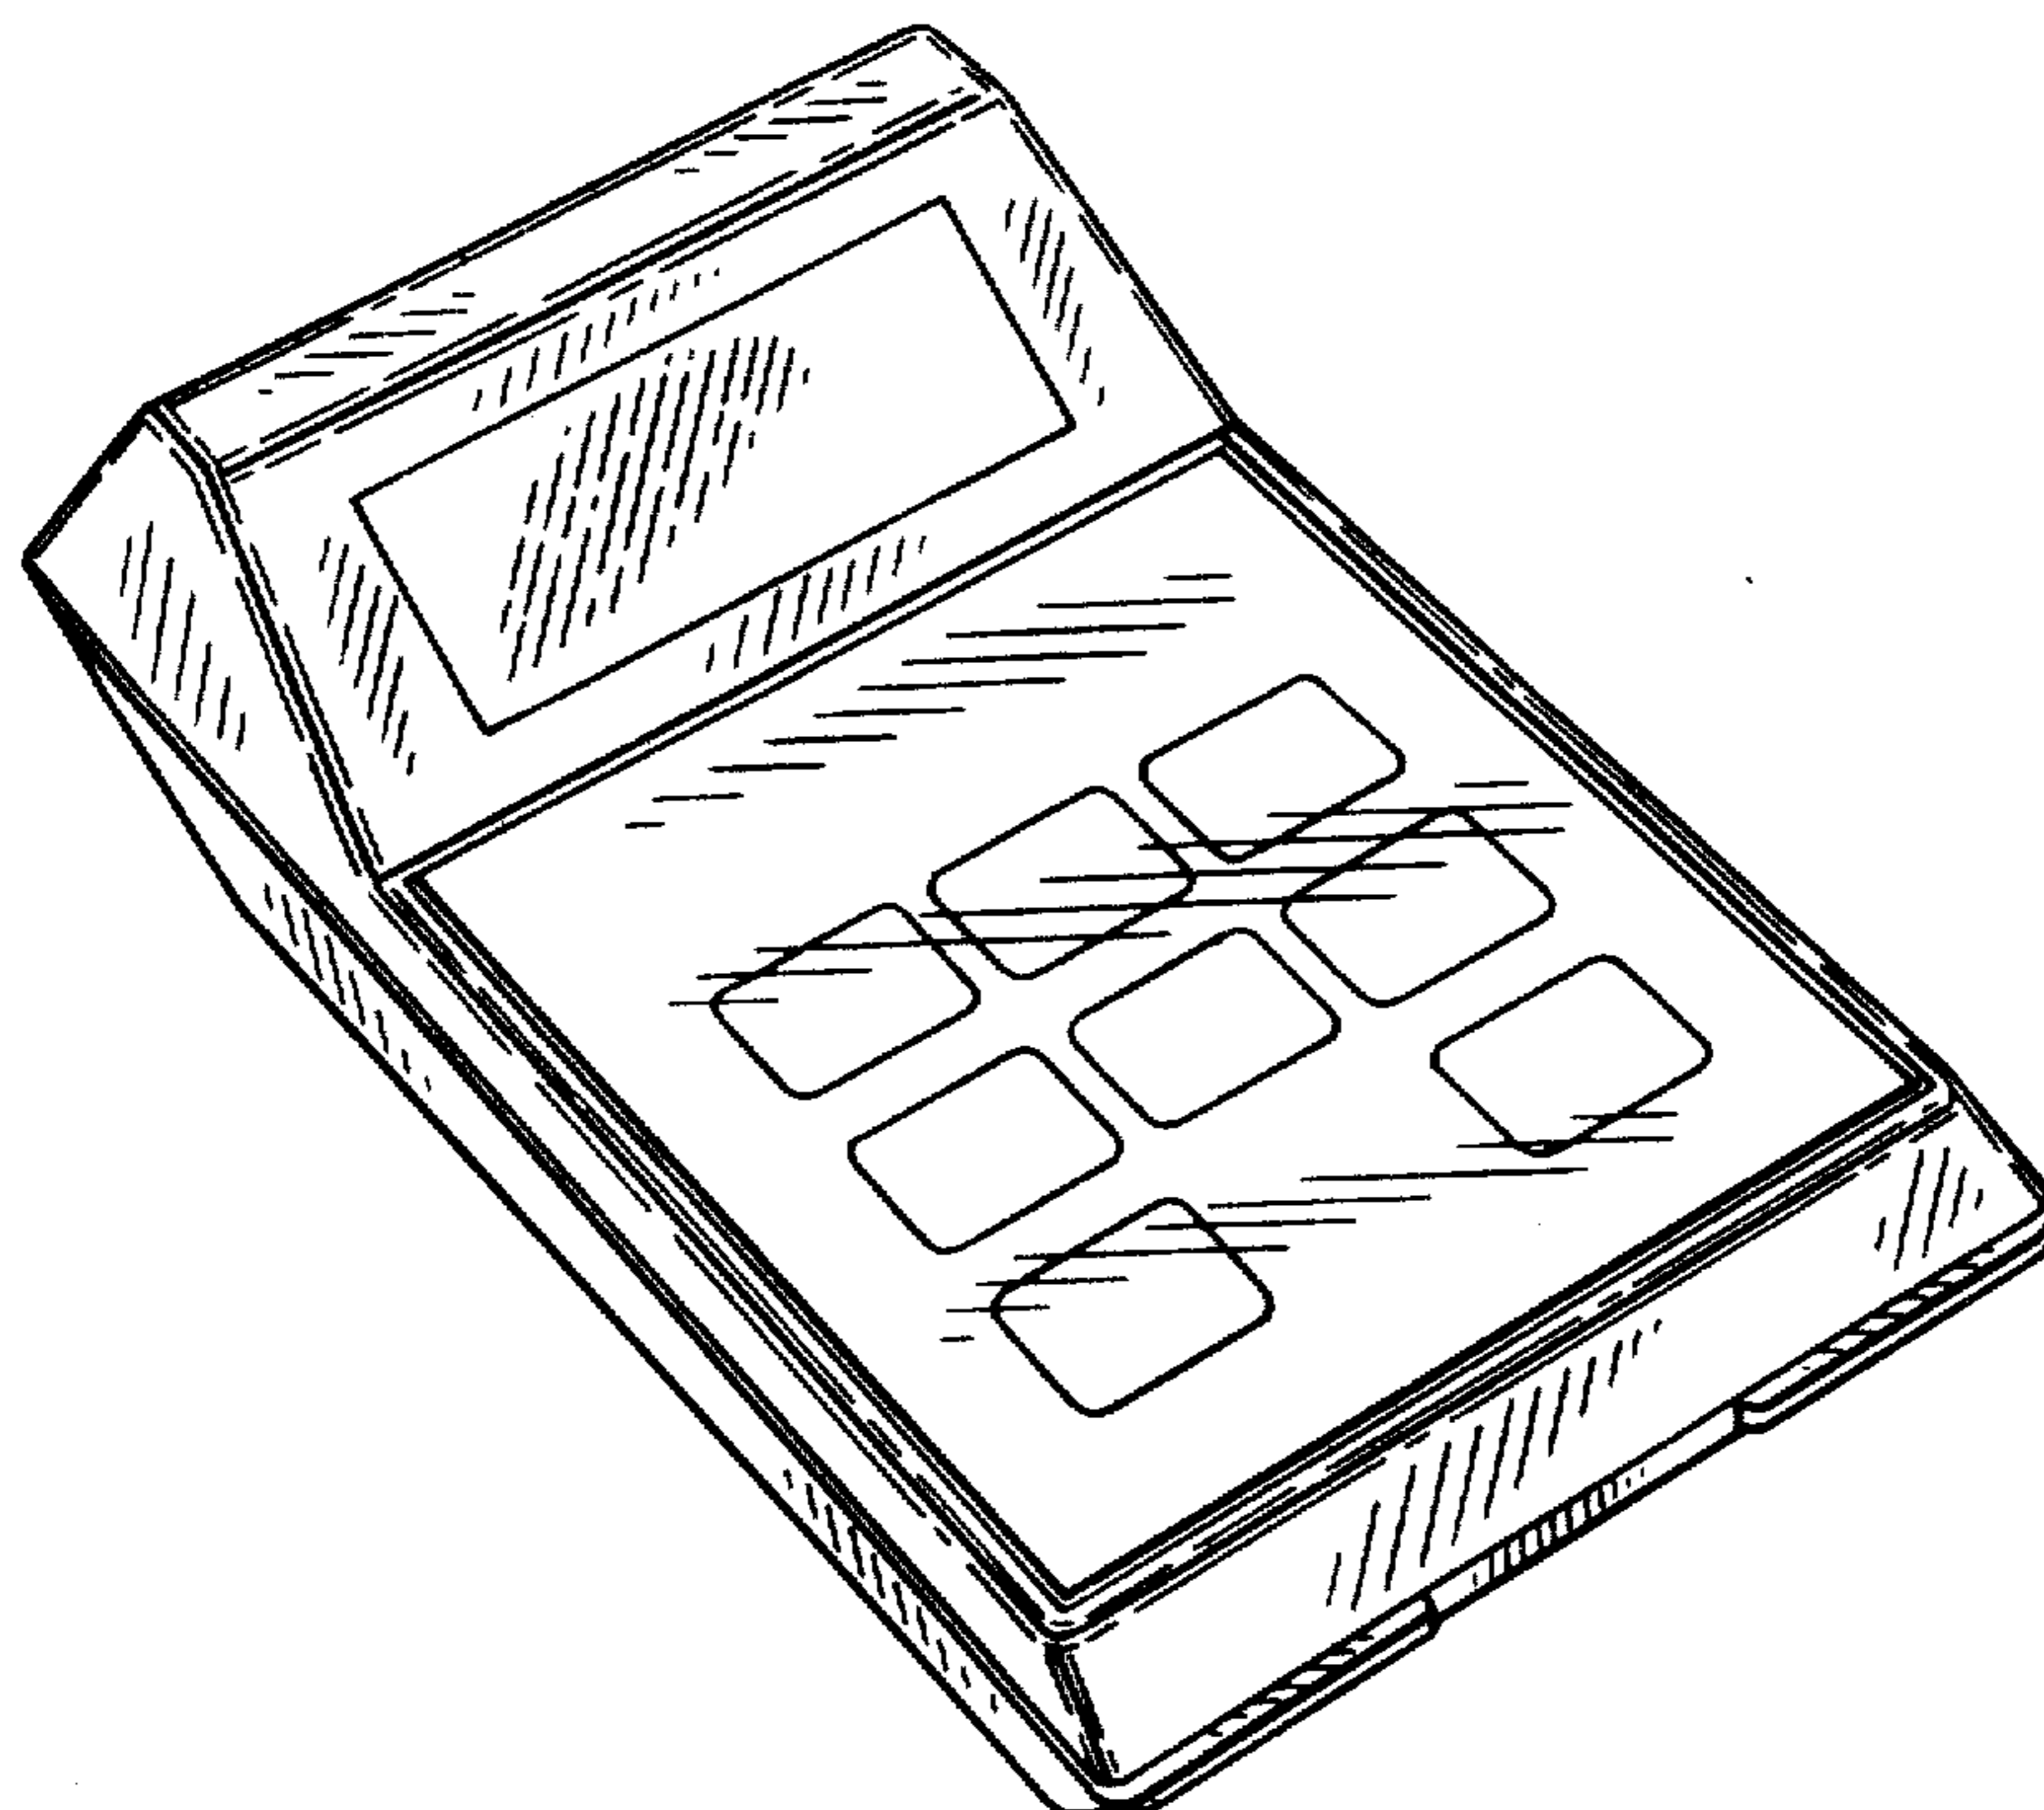


FIG. 1

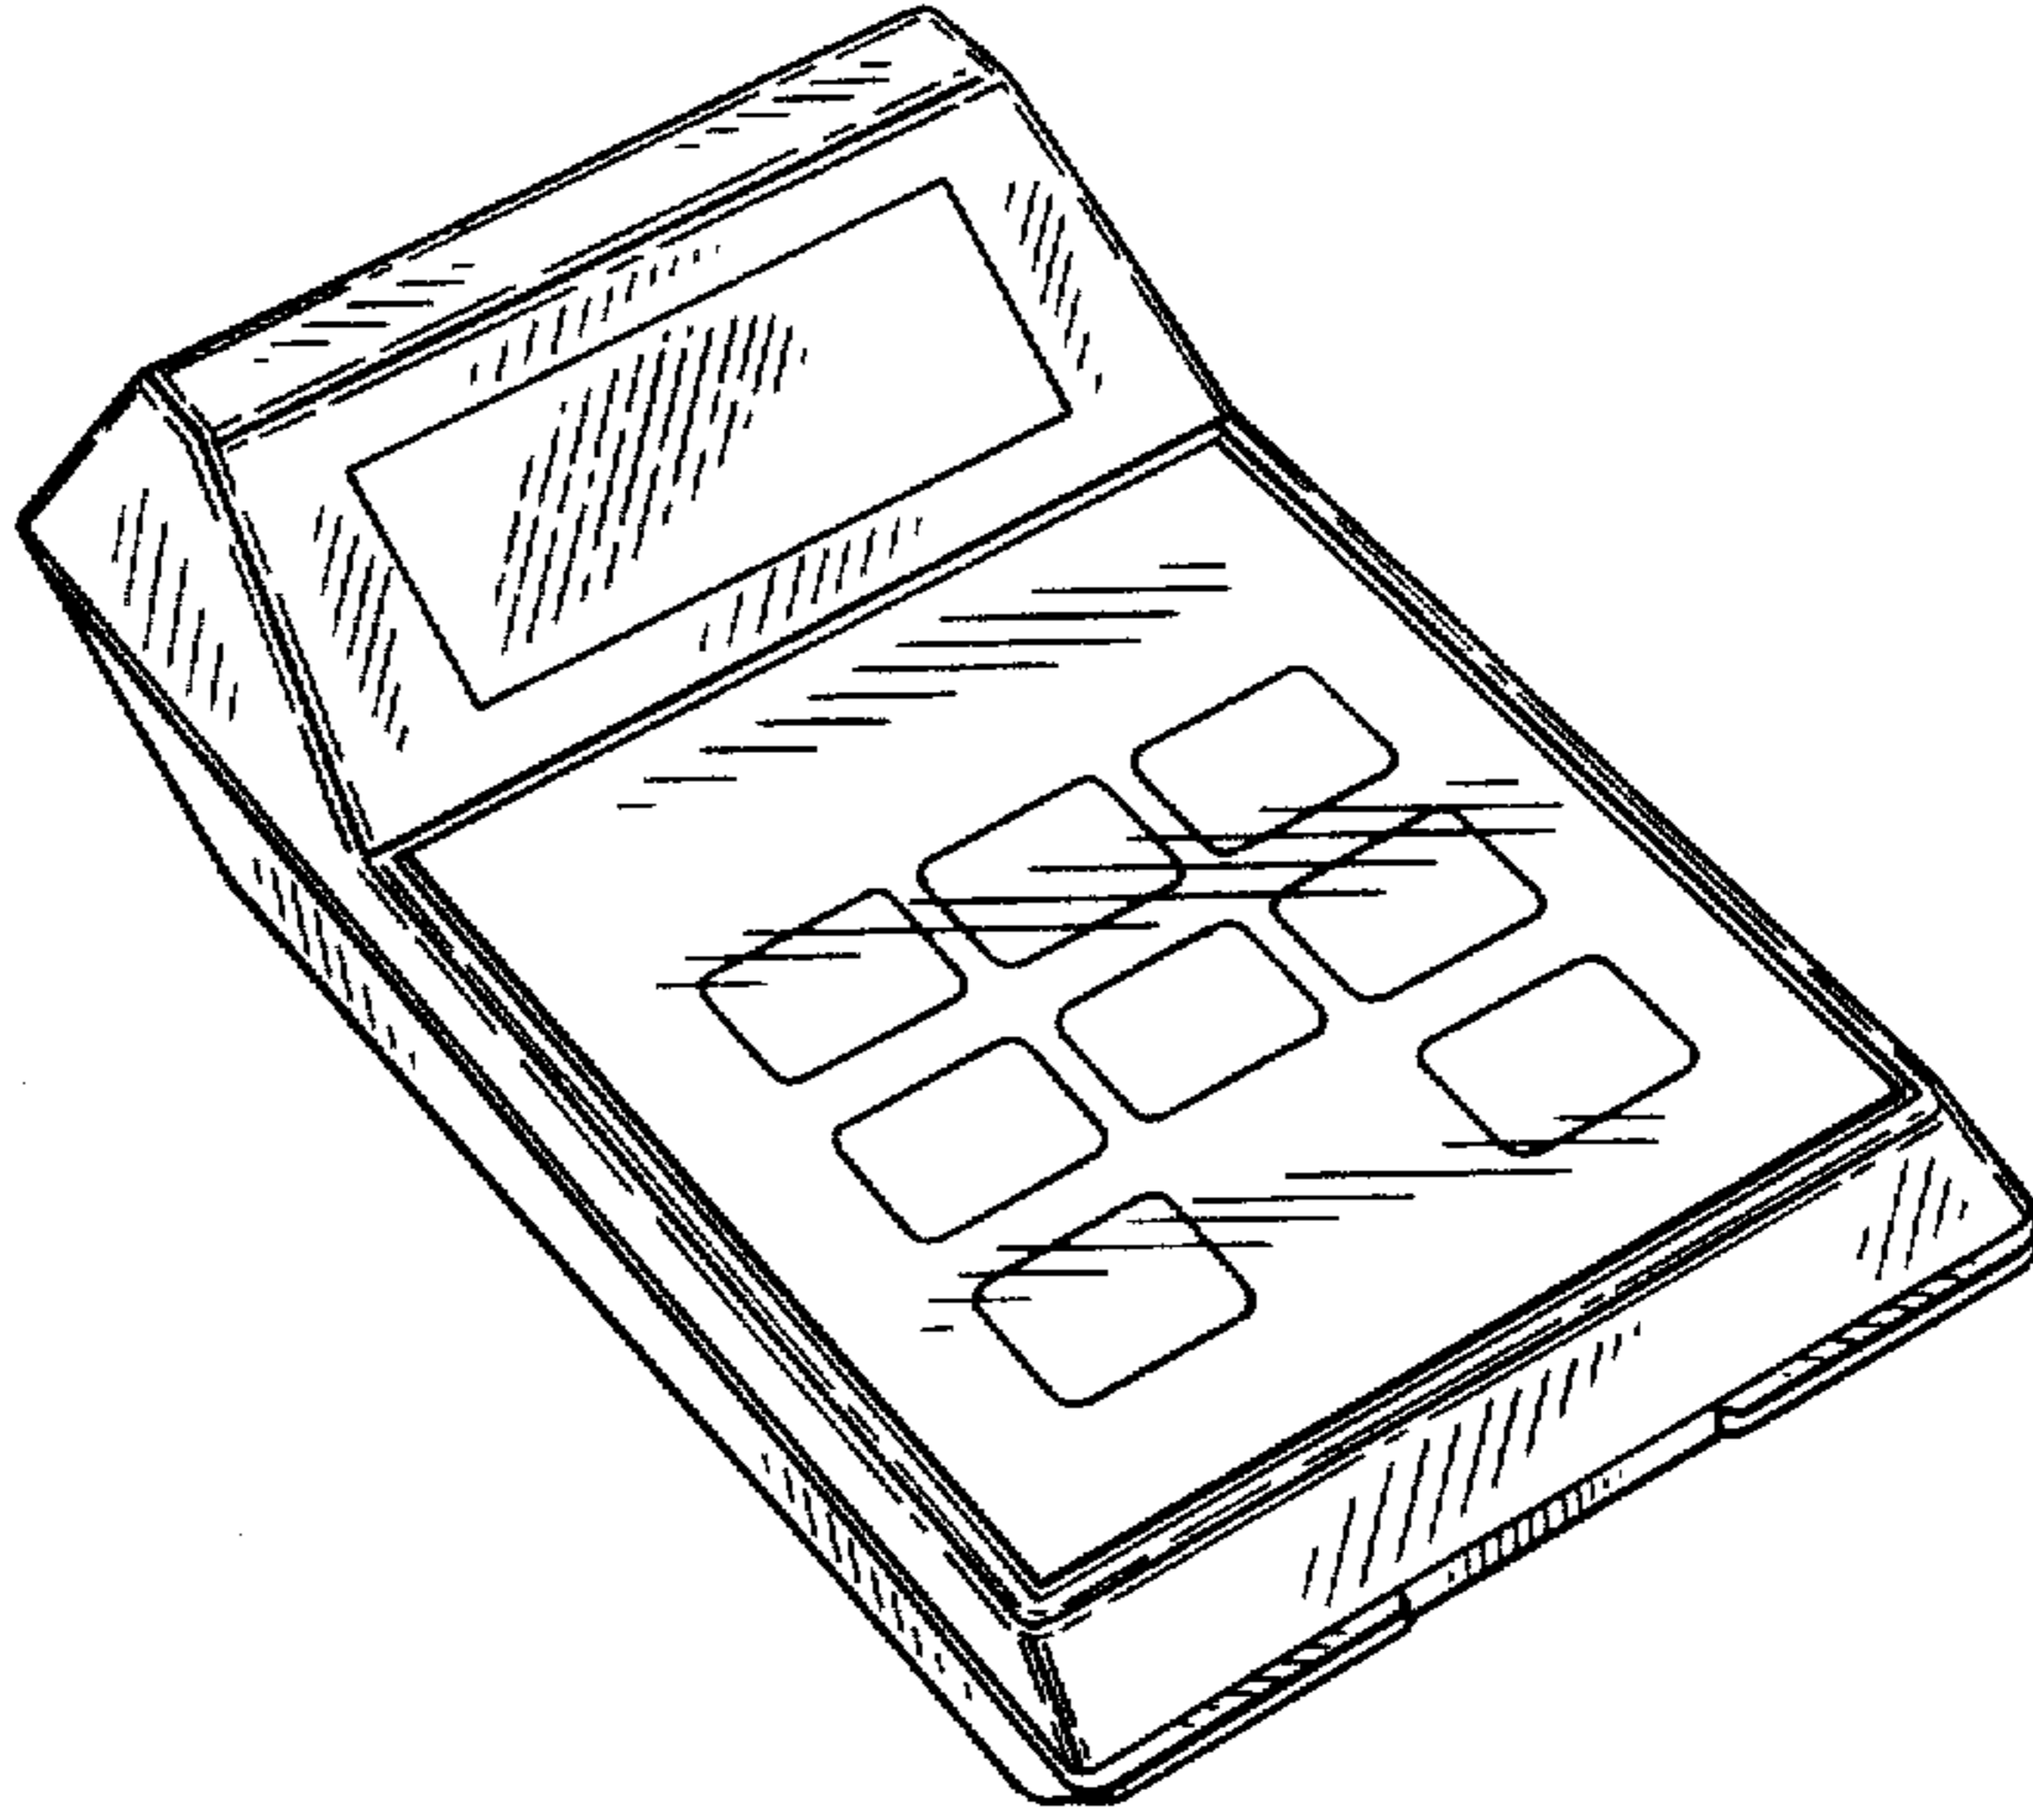


FIG. 2

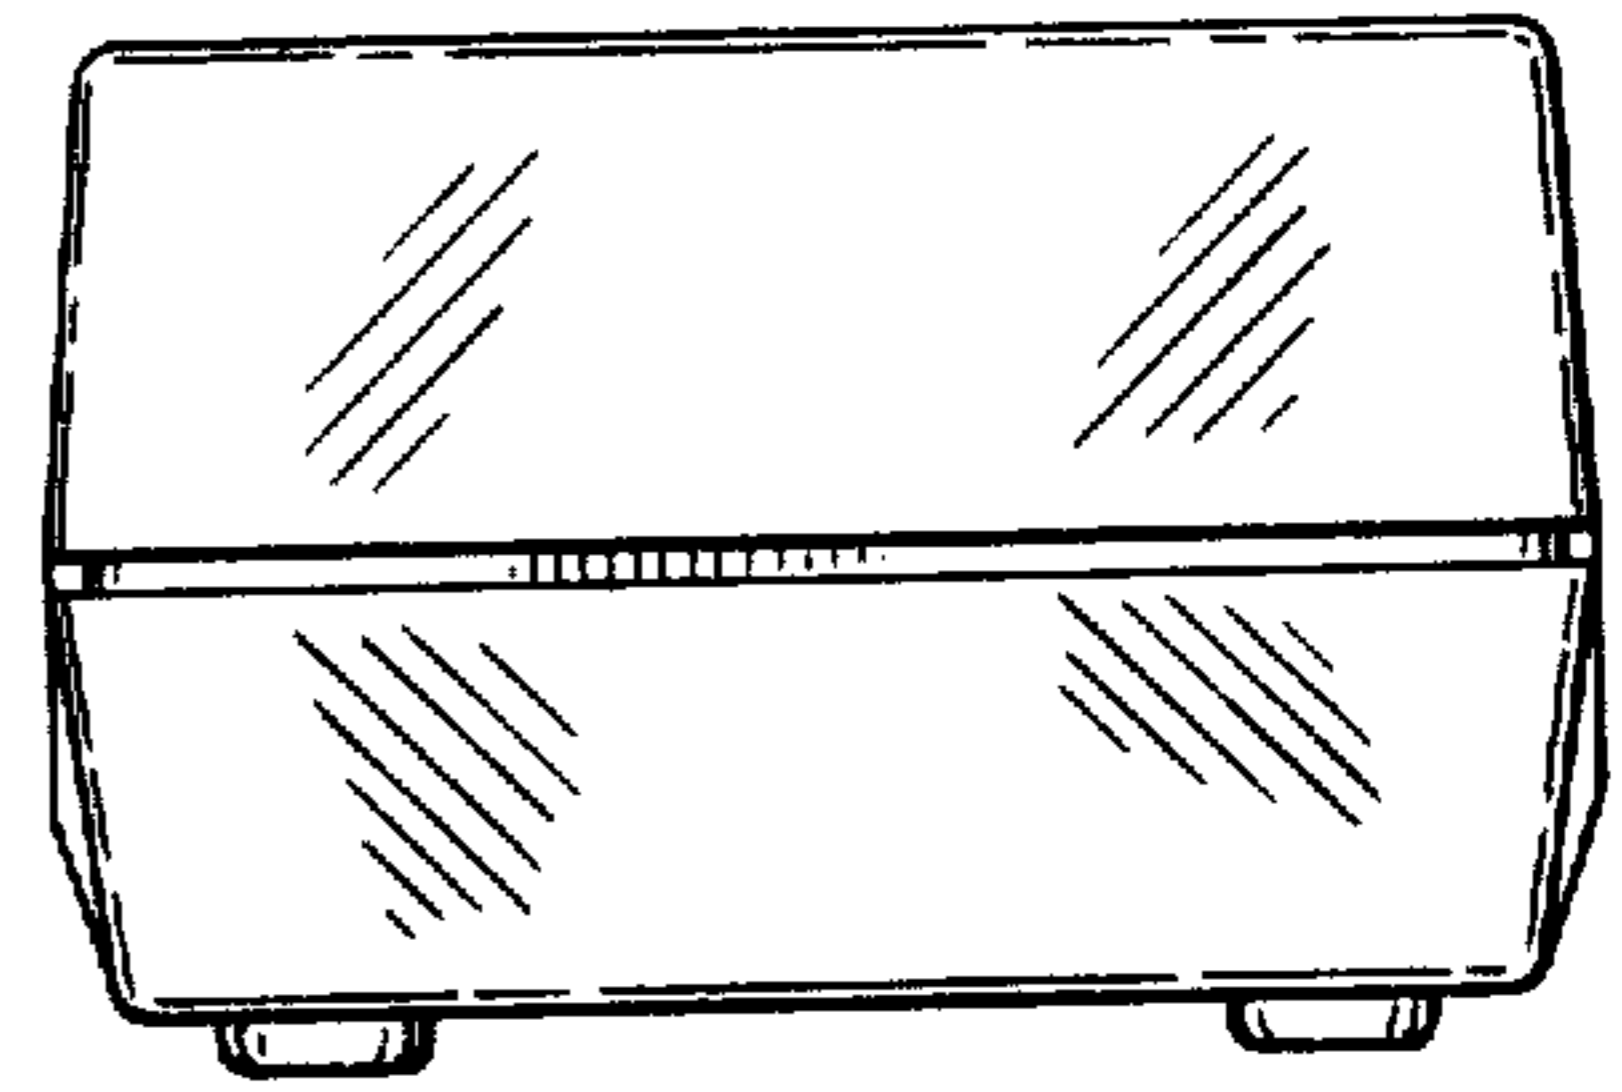
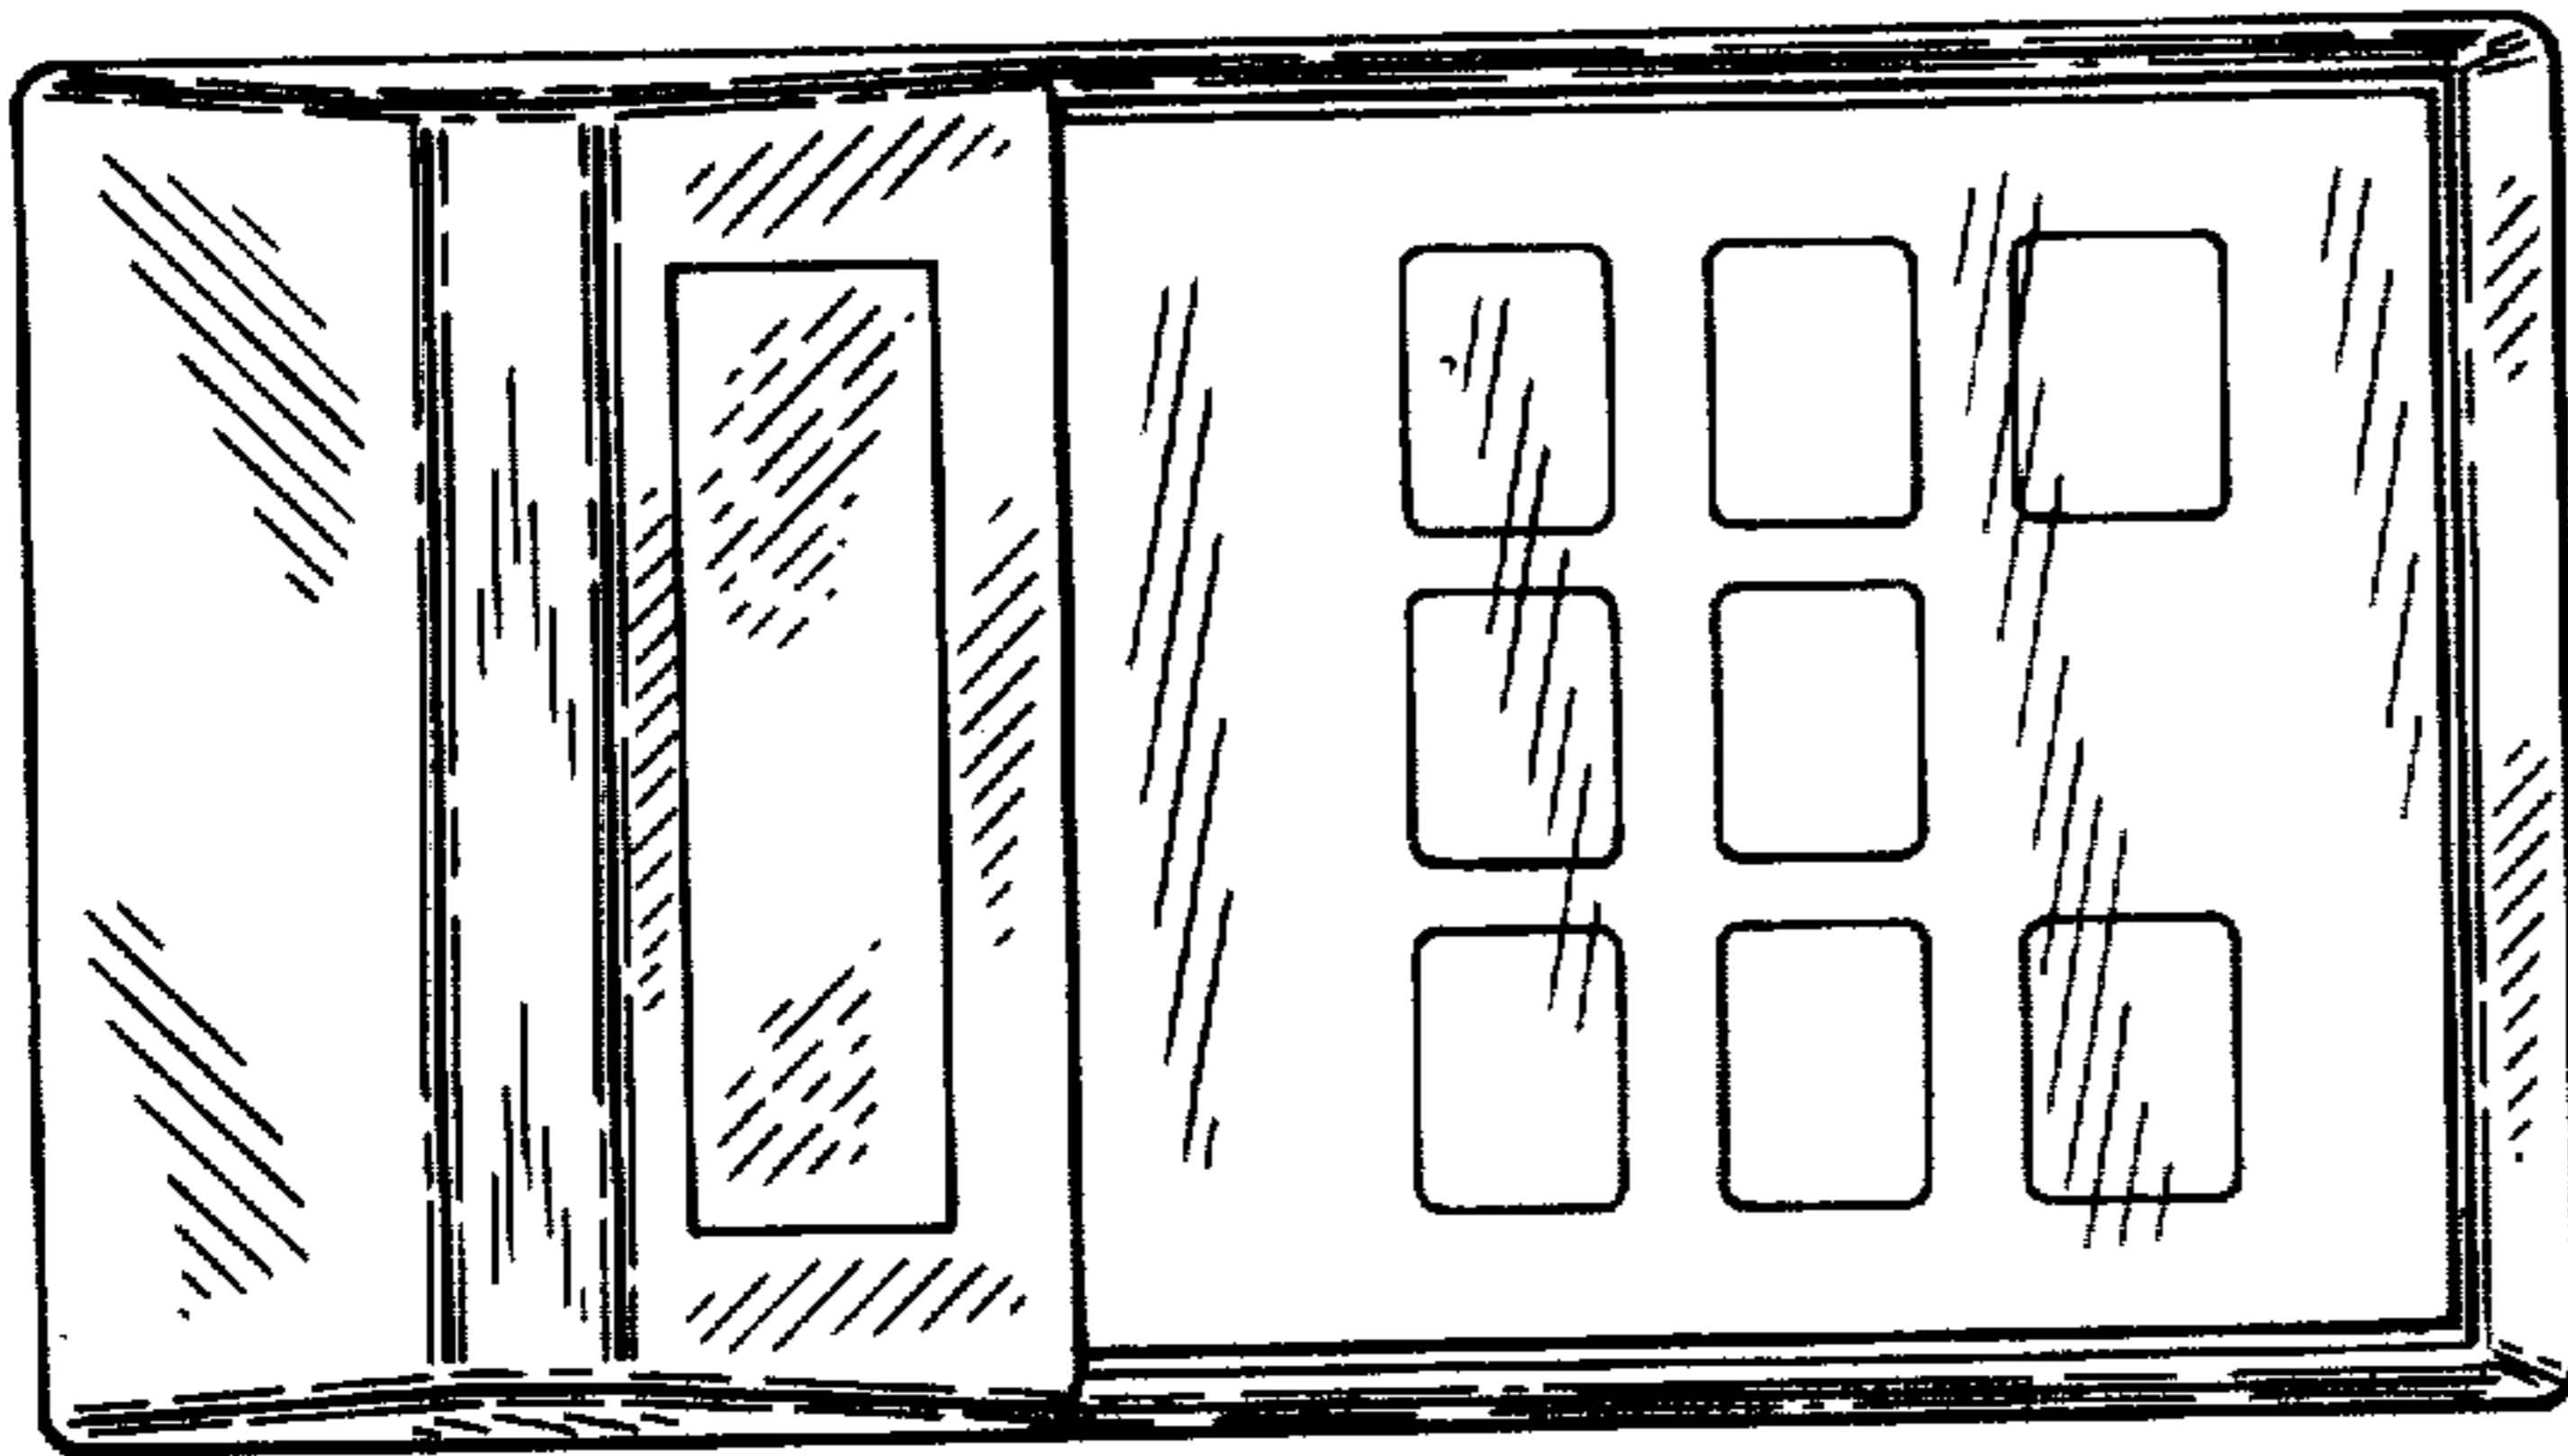


FIG. 5

FIG. 6

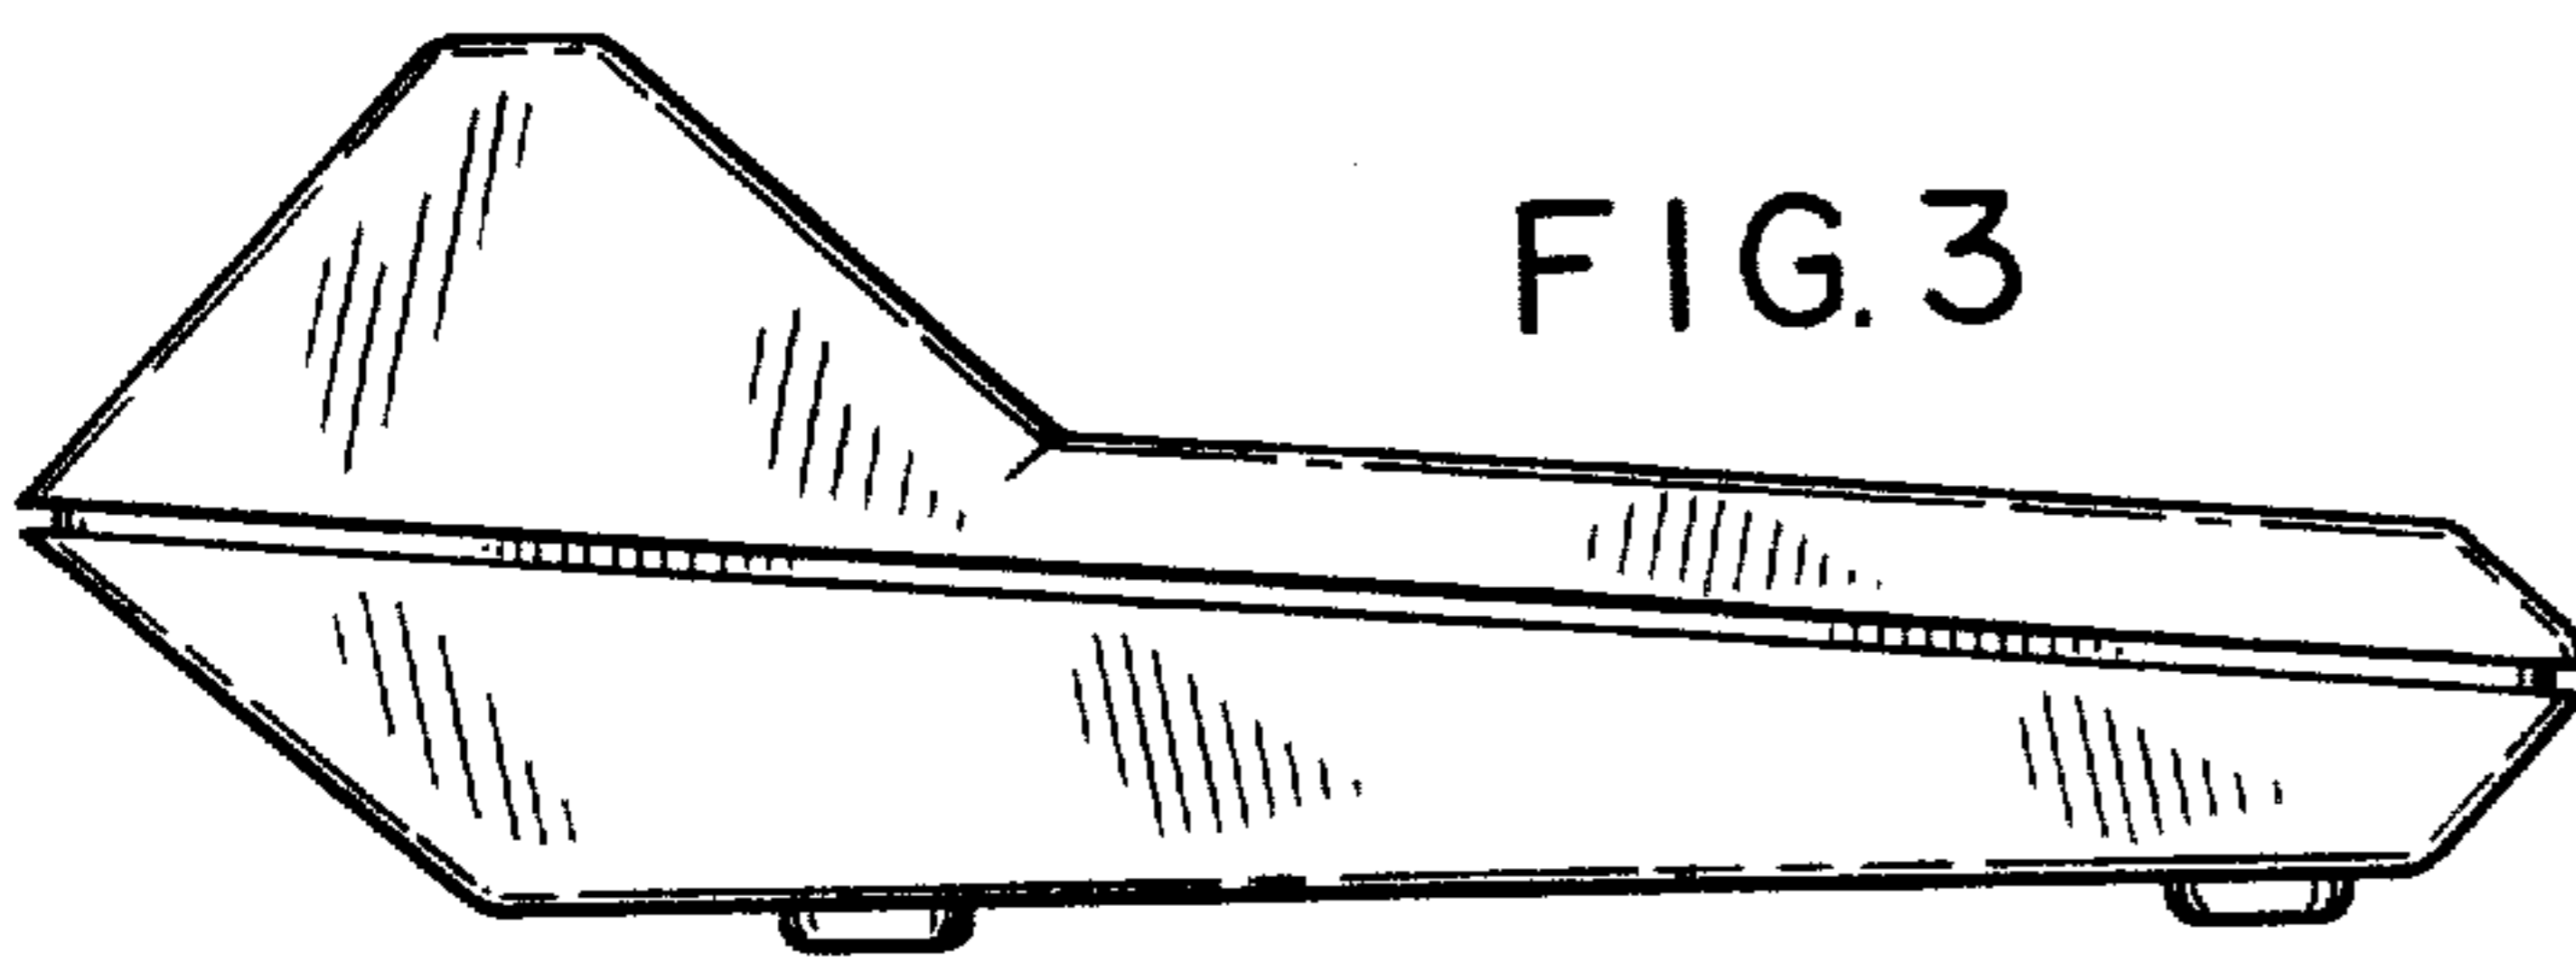


FIG. 3

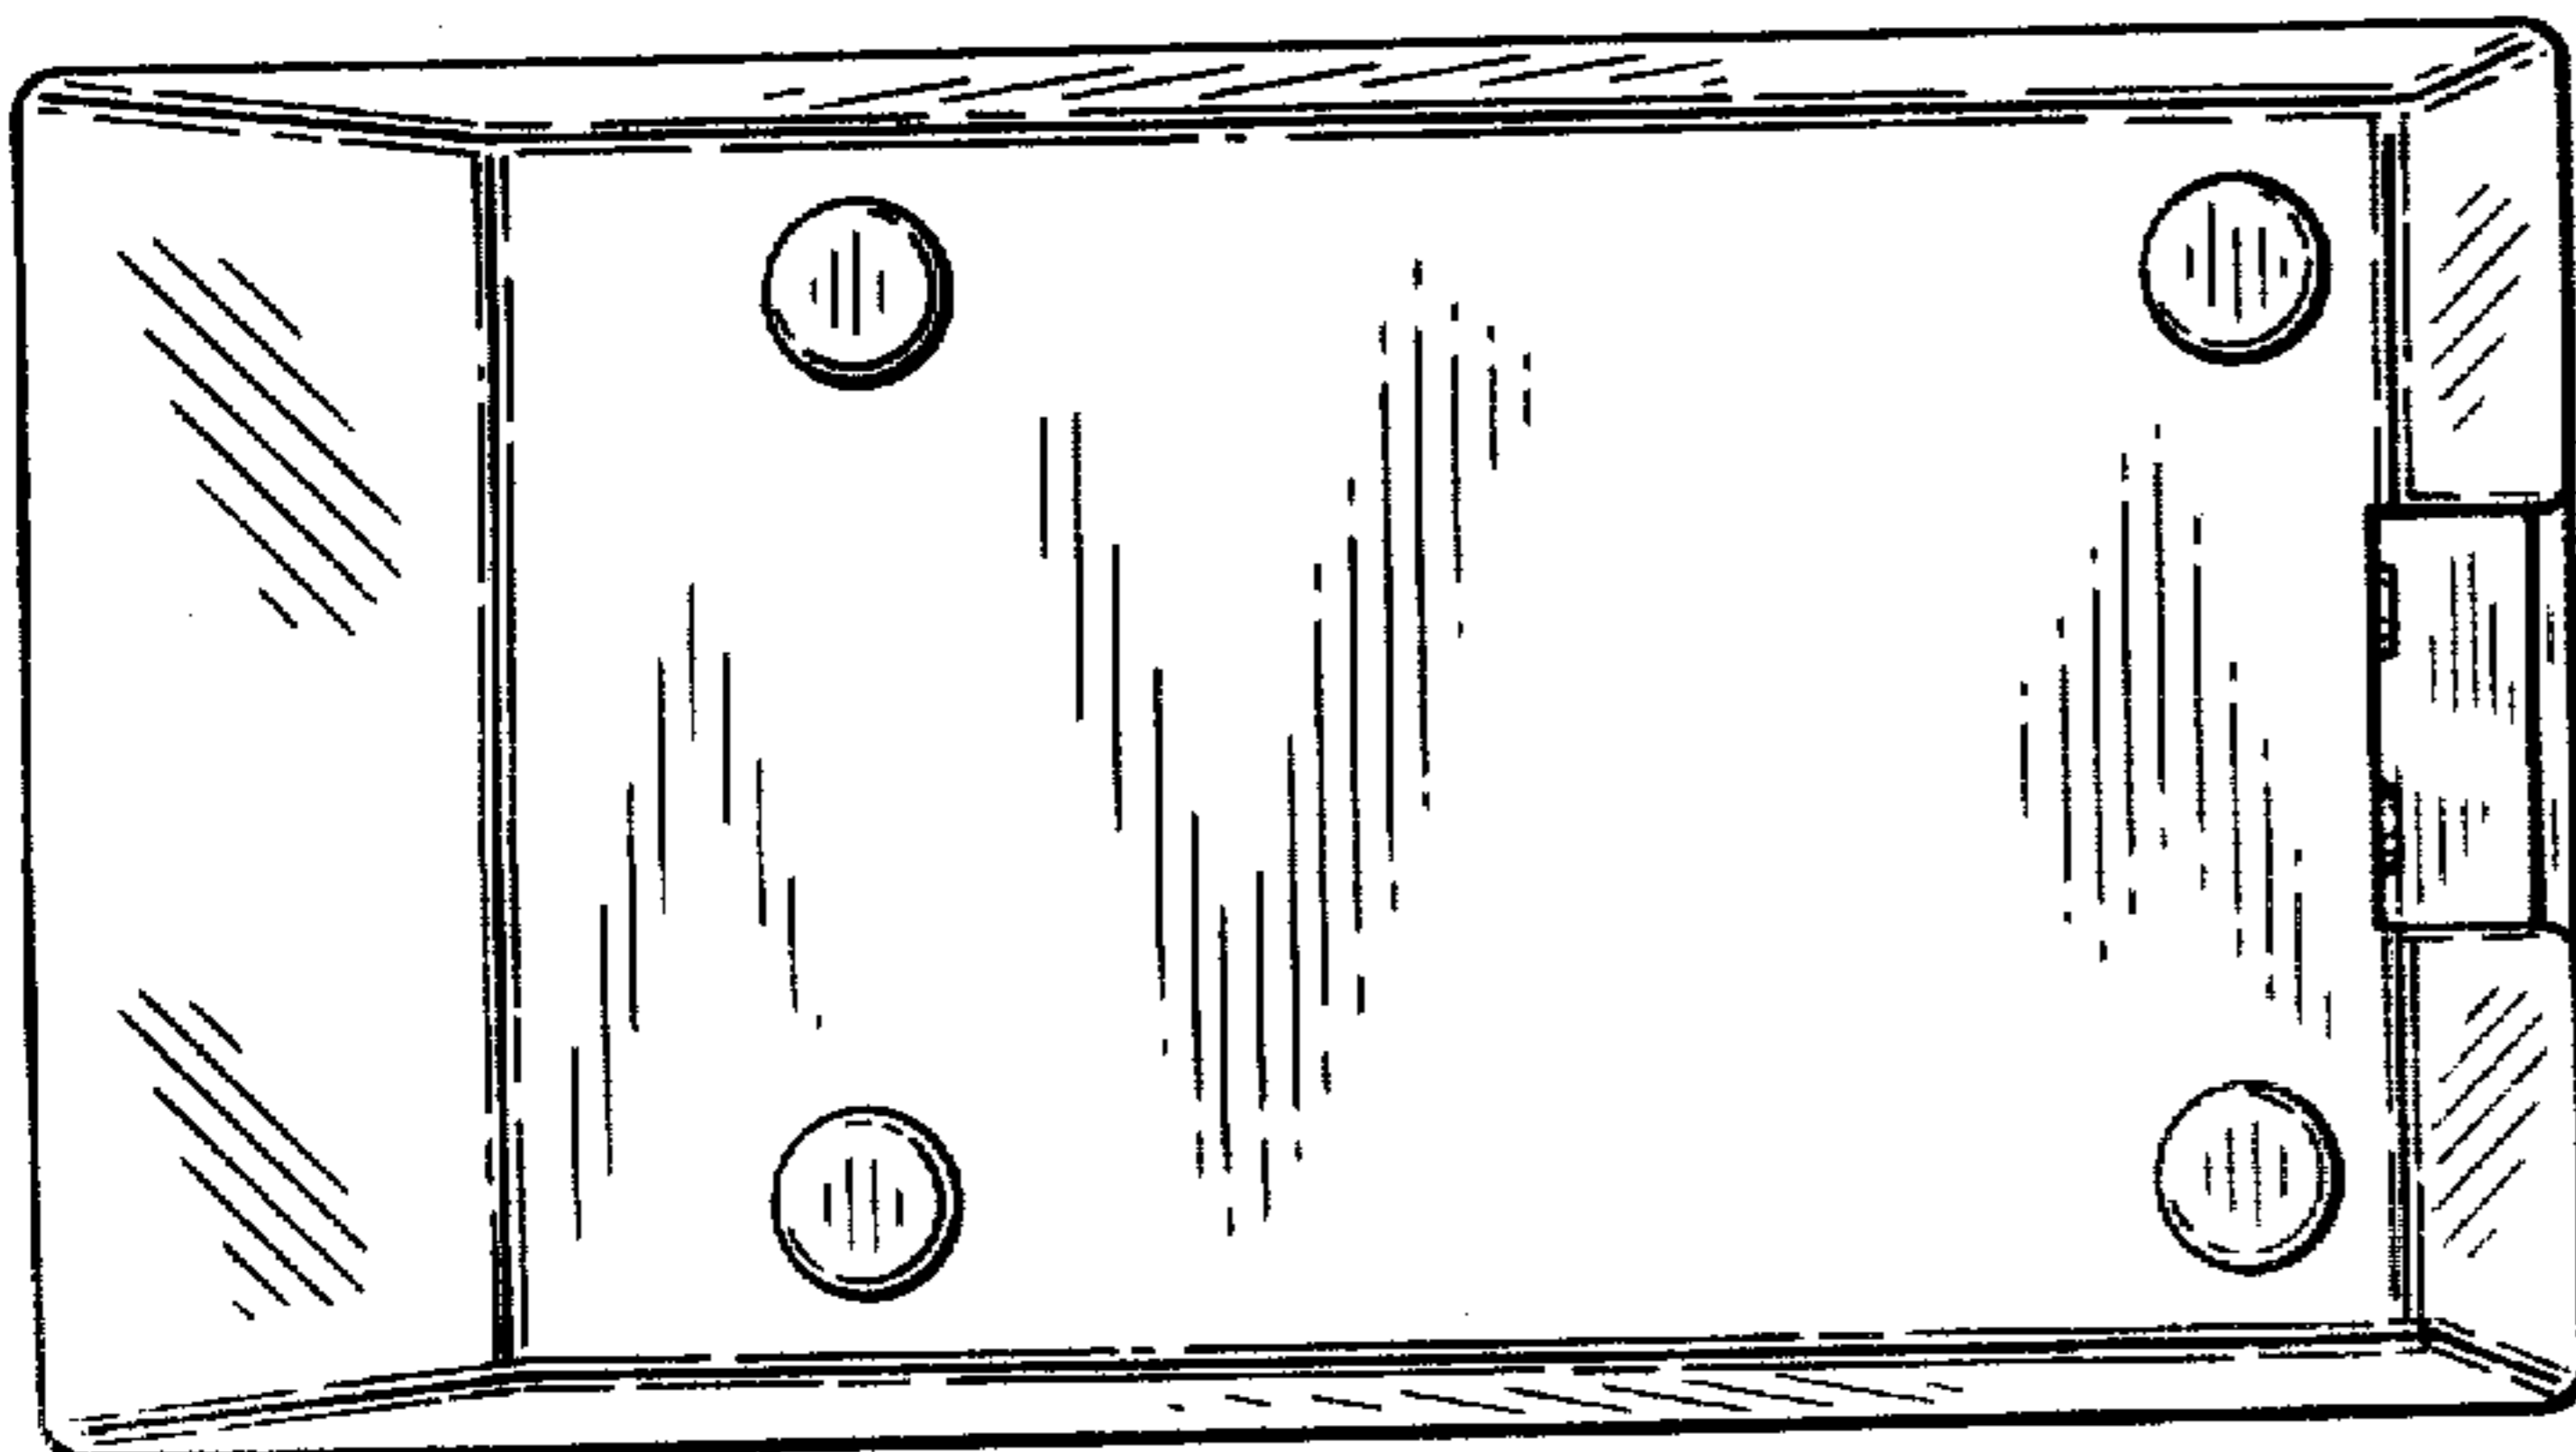
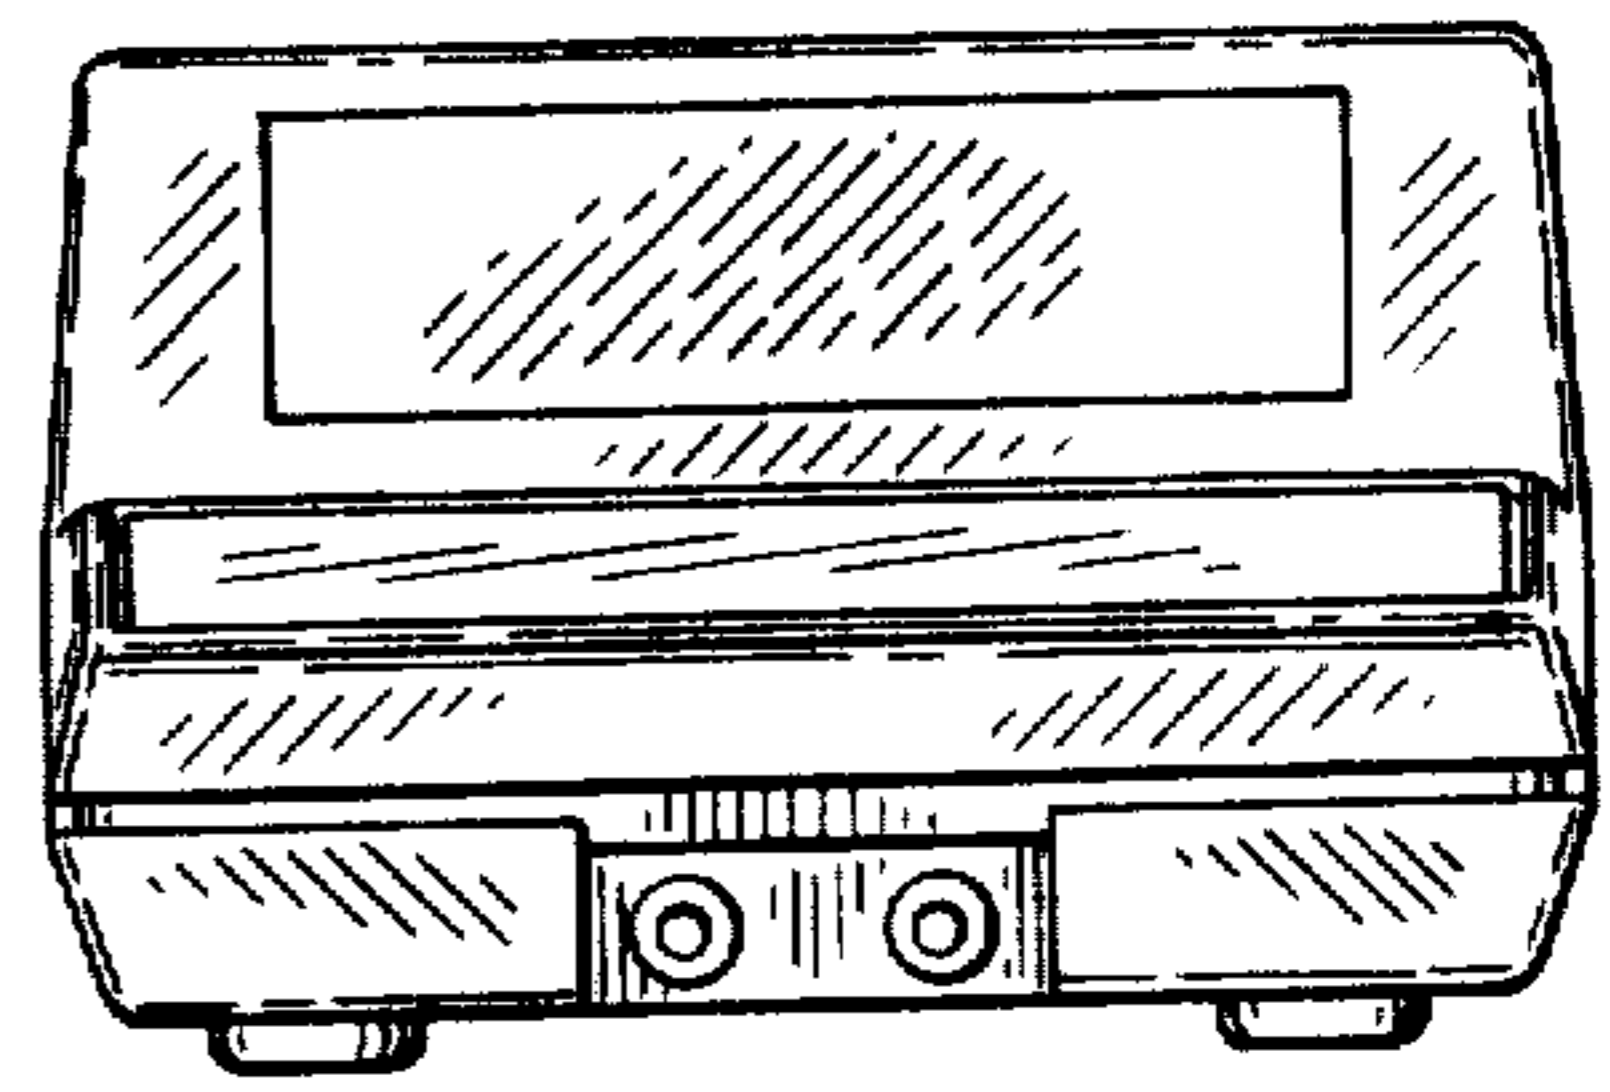


FIG. 4