

- [54] FETUS PULSE AND BLOOD FLOW DETECTOR
- [75] Inventors: Masuo Sugawara, Tokorozawa; Hiroji Matsumoto, Kawasaki, both of Japan
- [73] Assignee: Hayashi Denki Company Ltd., Kanagawa, Japan
- [\*\*] Term: 14 Years
- [21] Appl. No.: 17,340
- [22] Filed: Mar. 5, 1979
- [51] Int. Cl. .... D24-02
- [52] U.S. Cl. .... D24/17; D24/23; D10/96; D10/103
- [58] Field of Search ..... D24/17, 23, 21; 128/715, 773; D10/75, 96, 103

References Cited

U.S. PATENT DOCUMENTS

- D. 214,755 7/1969 McPhee ..... D10/103
- D. 223,122 3/1972 King et al. .... D10/96

- D. 233,569 11/1974 Miller ..... D24/17
- D. 236,190 8/1975 Wibring ..... D10/96
- D. 243,717 3/1977 Edmark et al. .... D10/103
- D. 254,569 3/1980 Moffat et al. .... D24/17
- 3,182,129 5/1965 Clark et al. .... 128/715

OTHER PUBLICATIONS

"The American Journal of Medical Electronics", Jul.-Sep., 1964, pp. 192-198, See FIG. 5 on p. 198.


Primary Examiner—T. Tung

[57] CLAIM


The ornamental design for a fetus pulse and blood flow detector, as shown and described.

DESCRIPTION


FIG. 1 is the front end view showing the fetus pulse and blood flow detector,  
 FIG. 2 is the rear end view thereof,  
 FIG. 3 is the side view thereof,  
 FIG. 4 is the top plan view thereof; and  
 FIG. 5 is a perspective front view thereof showing in dotted lines, for illustration only, the attachment of the device to a stethoscope.

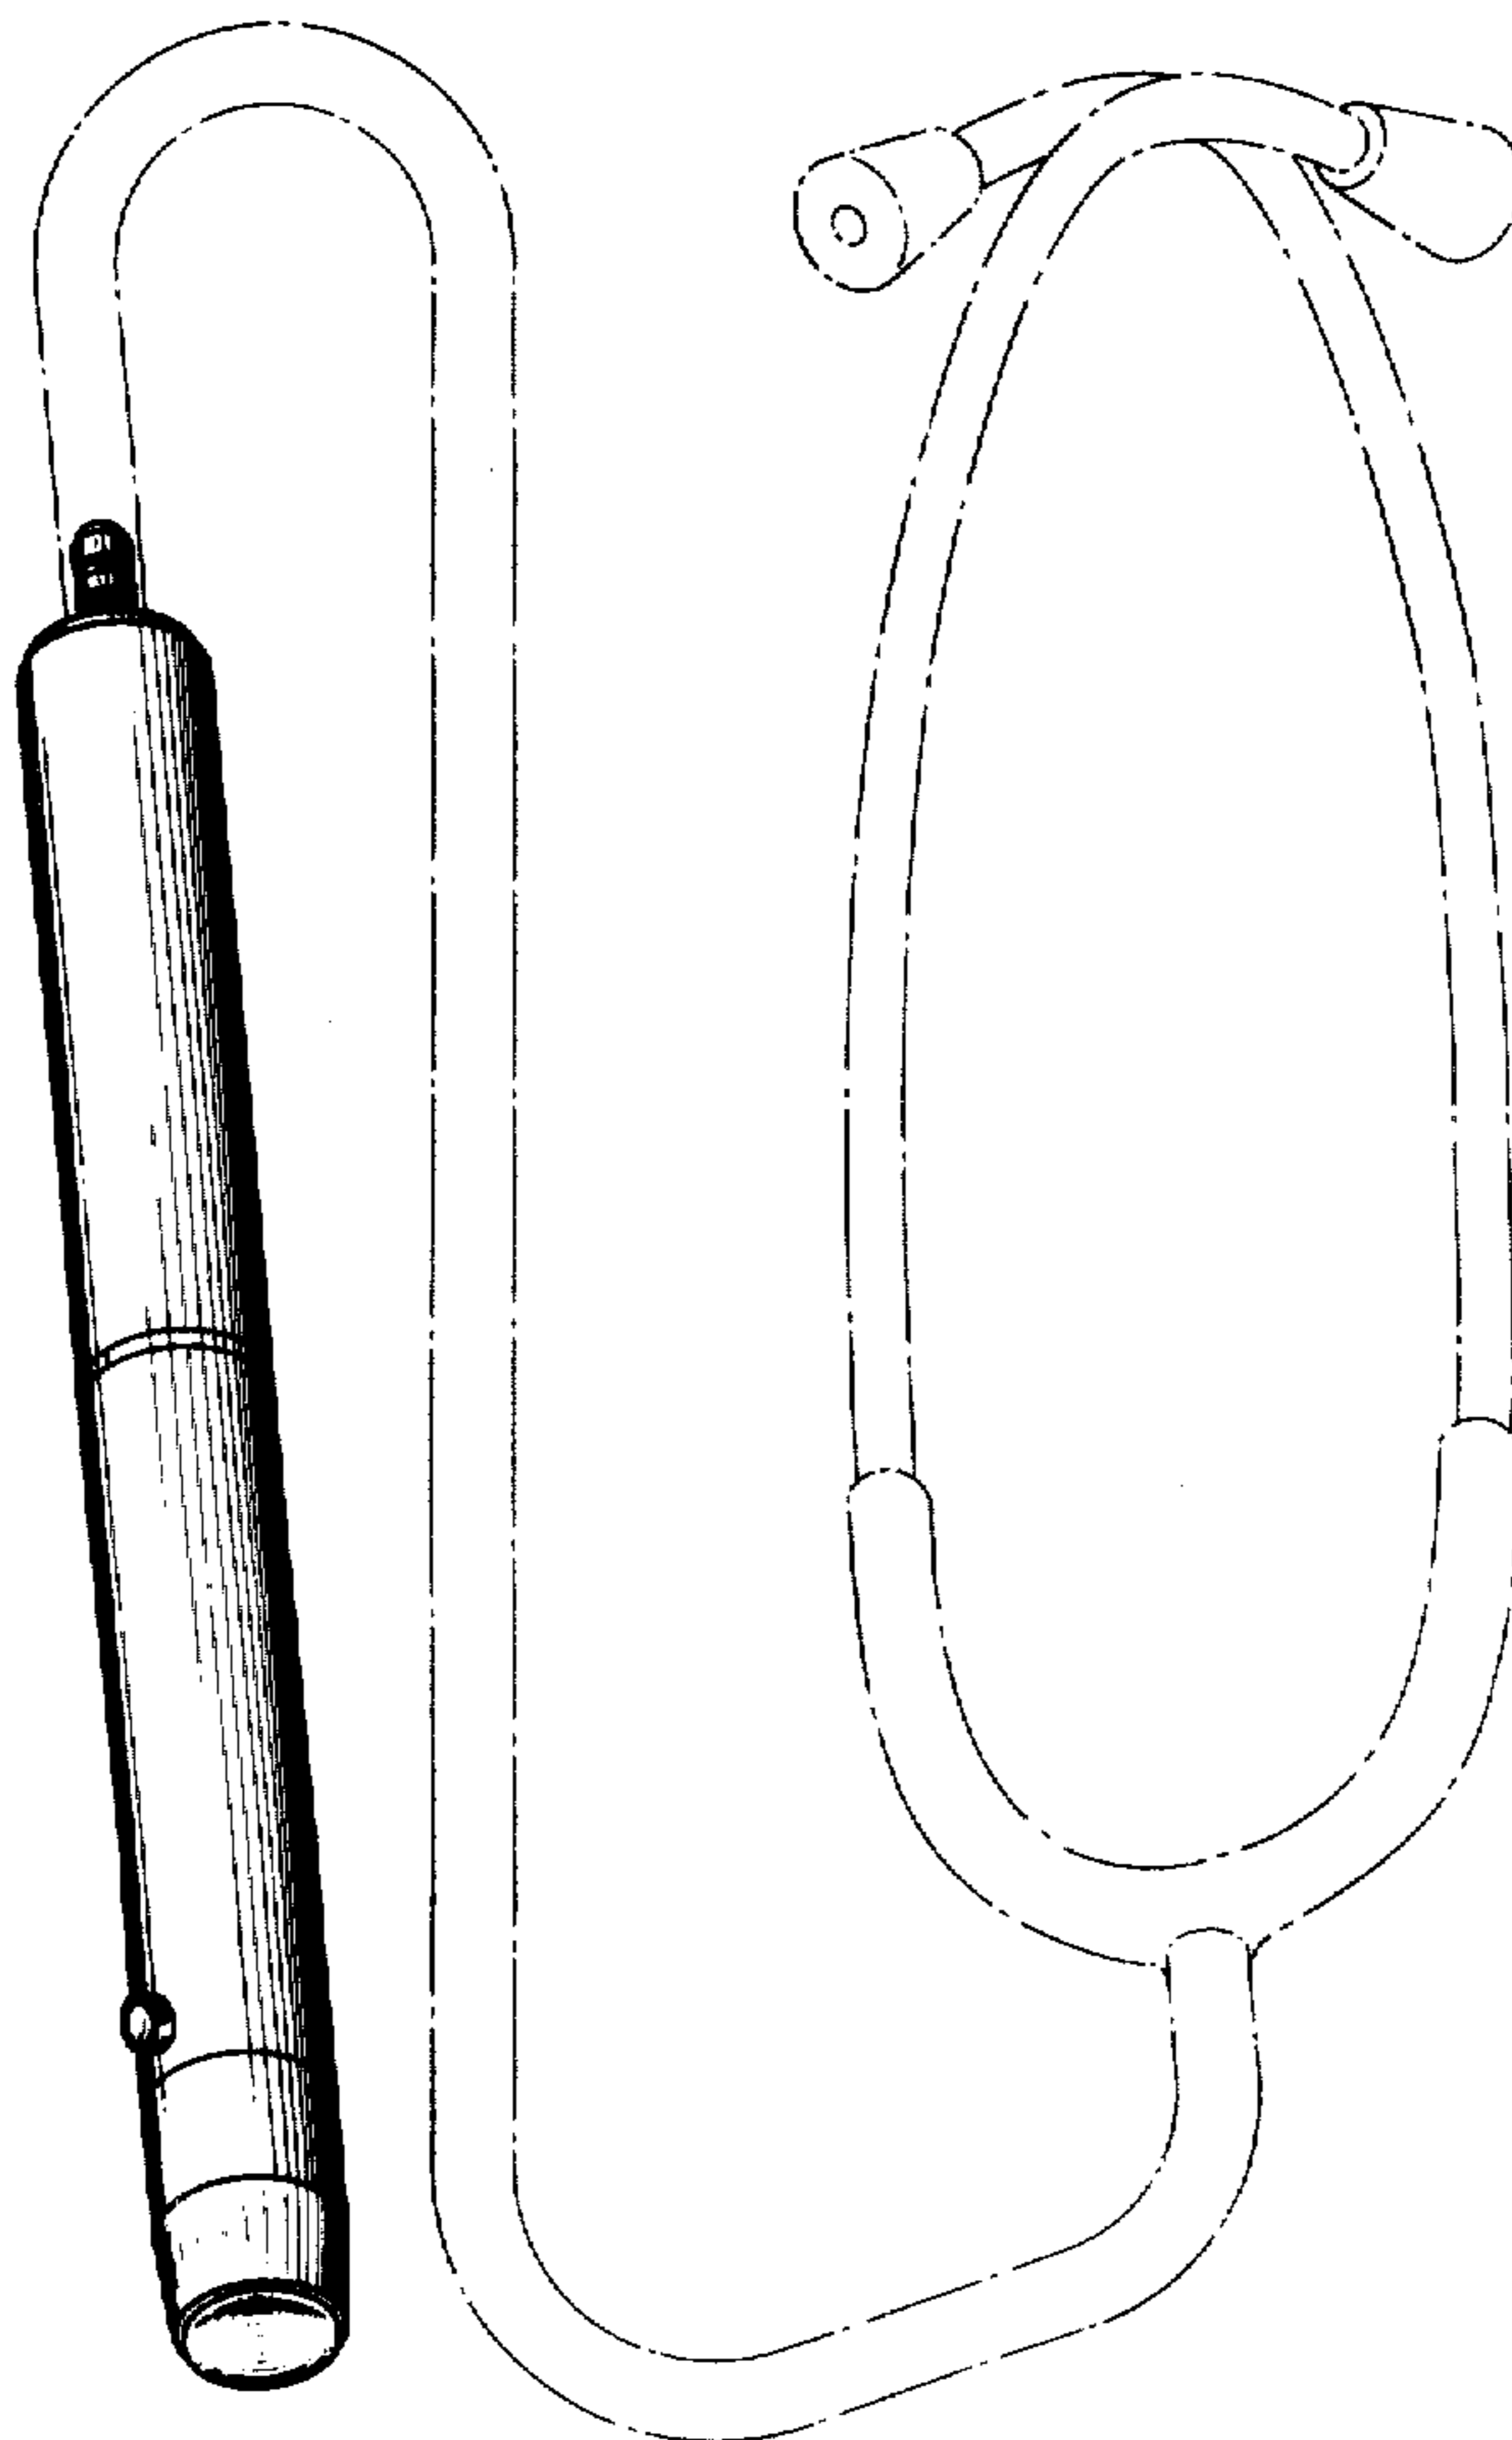

**FIG. 4**

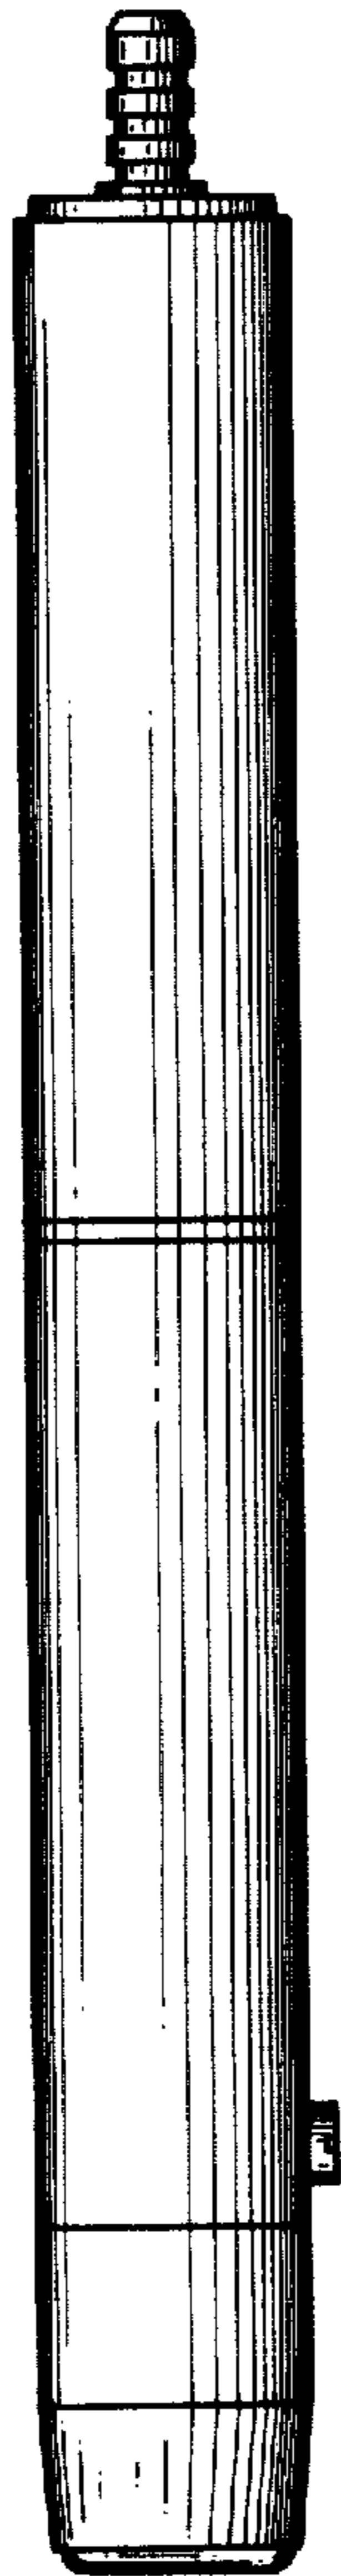


**FIG. 3**

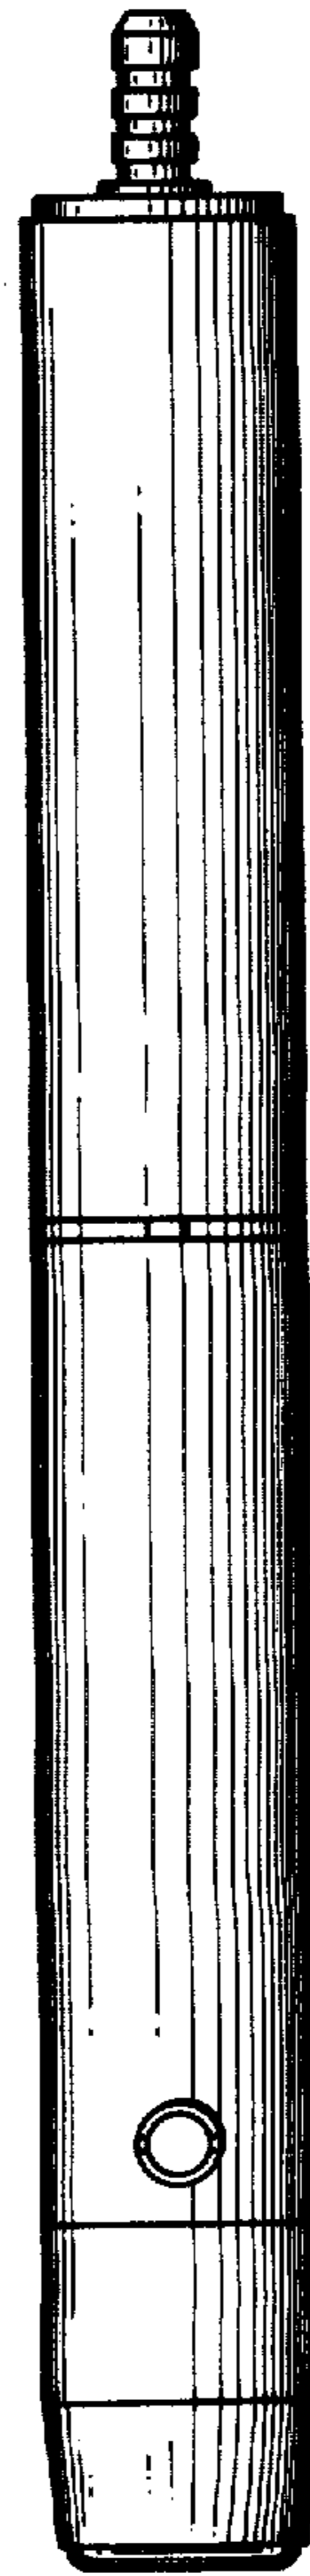

**FIG. 2**



**FIG. 1**

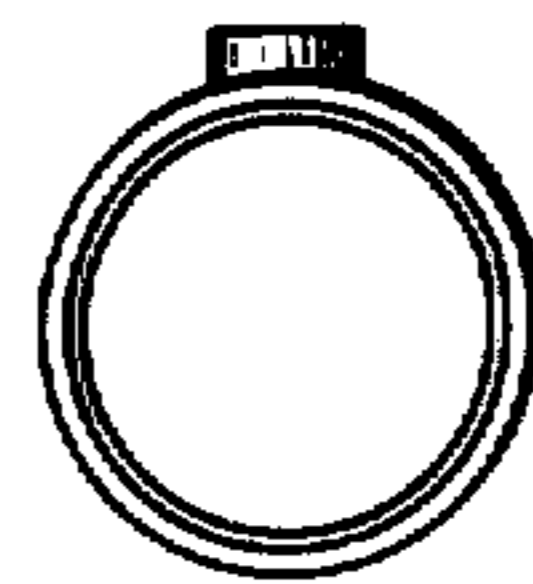

**Fig. 5**

