

[54] SPECIMEN CUP ASSEMBLY FOR A CLINICAL CHEMISTRY ANALYZER

[75] Inventor: Raymond J. Herrmann, Westlake, Ohio

[73] Assignee: Corning Glass Works, Corning, N.Y.

[\*\*] Term: 14 Years

[21] Appl. No.: 404,478

[22] Filed: Jul. 30, 1982

[51] Int. Cl. .... D24-02

[52] U.S. Cl. .... D24/29; D24/99

[58] Field of Search ..... 206/1.7, 1.8, 459; 422/102, 61, 55; D24/29, 99

[56] References Cited

U.S. PATENT DOCUMENTS

D. 266,588	10/1982	Mellars	.....	D24/17
3,441,383	4/1969	Moore et al.	.....	206/459 X
4,195,060	3/1980	Terk	.....	422/102 X
4,310,488	1/1982	Rahm	.....	422/102
4,348,207	9/1982	Cappel	.....	422/102

Primary Examiner—Bernard Ansher

Attorney, Agent, or Firm—Burton R. Turner

[57] CLAIM

The ornamental design for a specimen cup assembly for a clinical chemistry analyzer, as shown.

DESCRIPTION

FIG. 1 is a top plan view of the specimen cup assembly for a clinical chemistry analyzer embodying this invention;

FIG. 2 is a front elevational view;

FIG. 3 is a right side elevational view;

FIG. 4 is a left side elevational view;

FIG. 5 is a bottom view;

FIG. 6 is a top plan view of the specimen cup cover of the assembly;

FIG. 7 is a front elevational view of the cover;

FIG. 8 is a right side elevational view of the cover;


FIG. 9 is a left side elevational view of the cover;

FIG. 10 is a bottom plan view;

FIG. 11 is a top plan view of one of the specimen cups of the assembly;

FIG. 12 is an elevational view of the specimen cup in partial section to illustrate the specimen cup cavity; and

FIG. 13 is a bottom plan view taken on line 13—13 of FIG. 12.

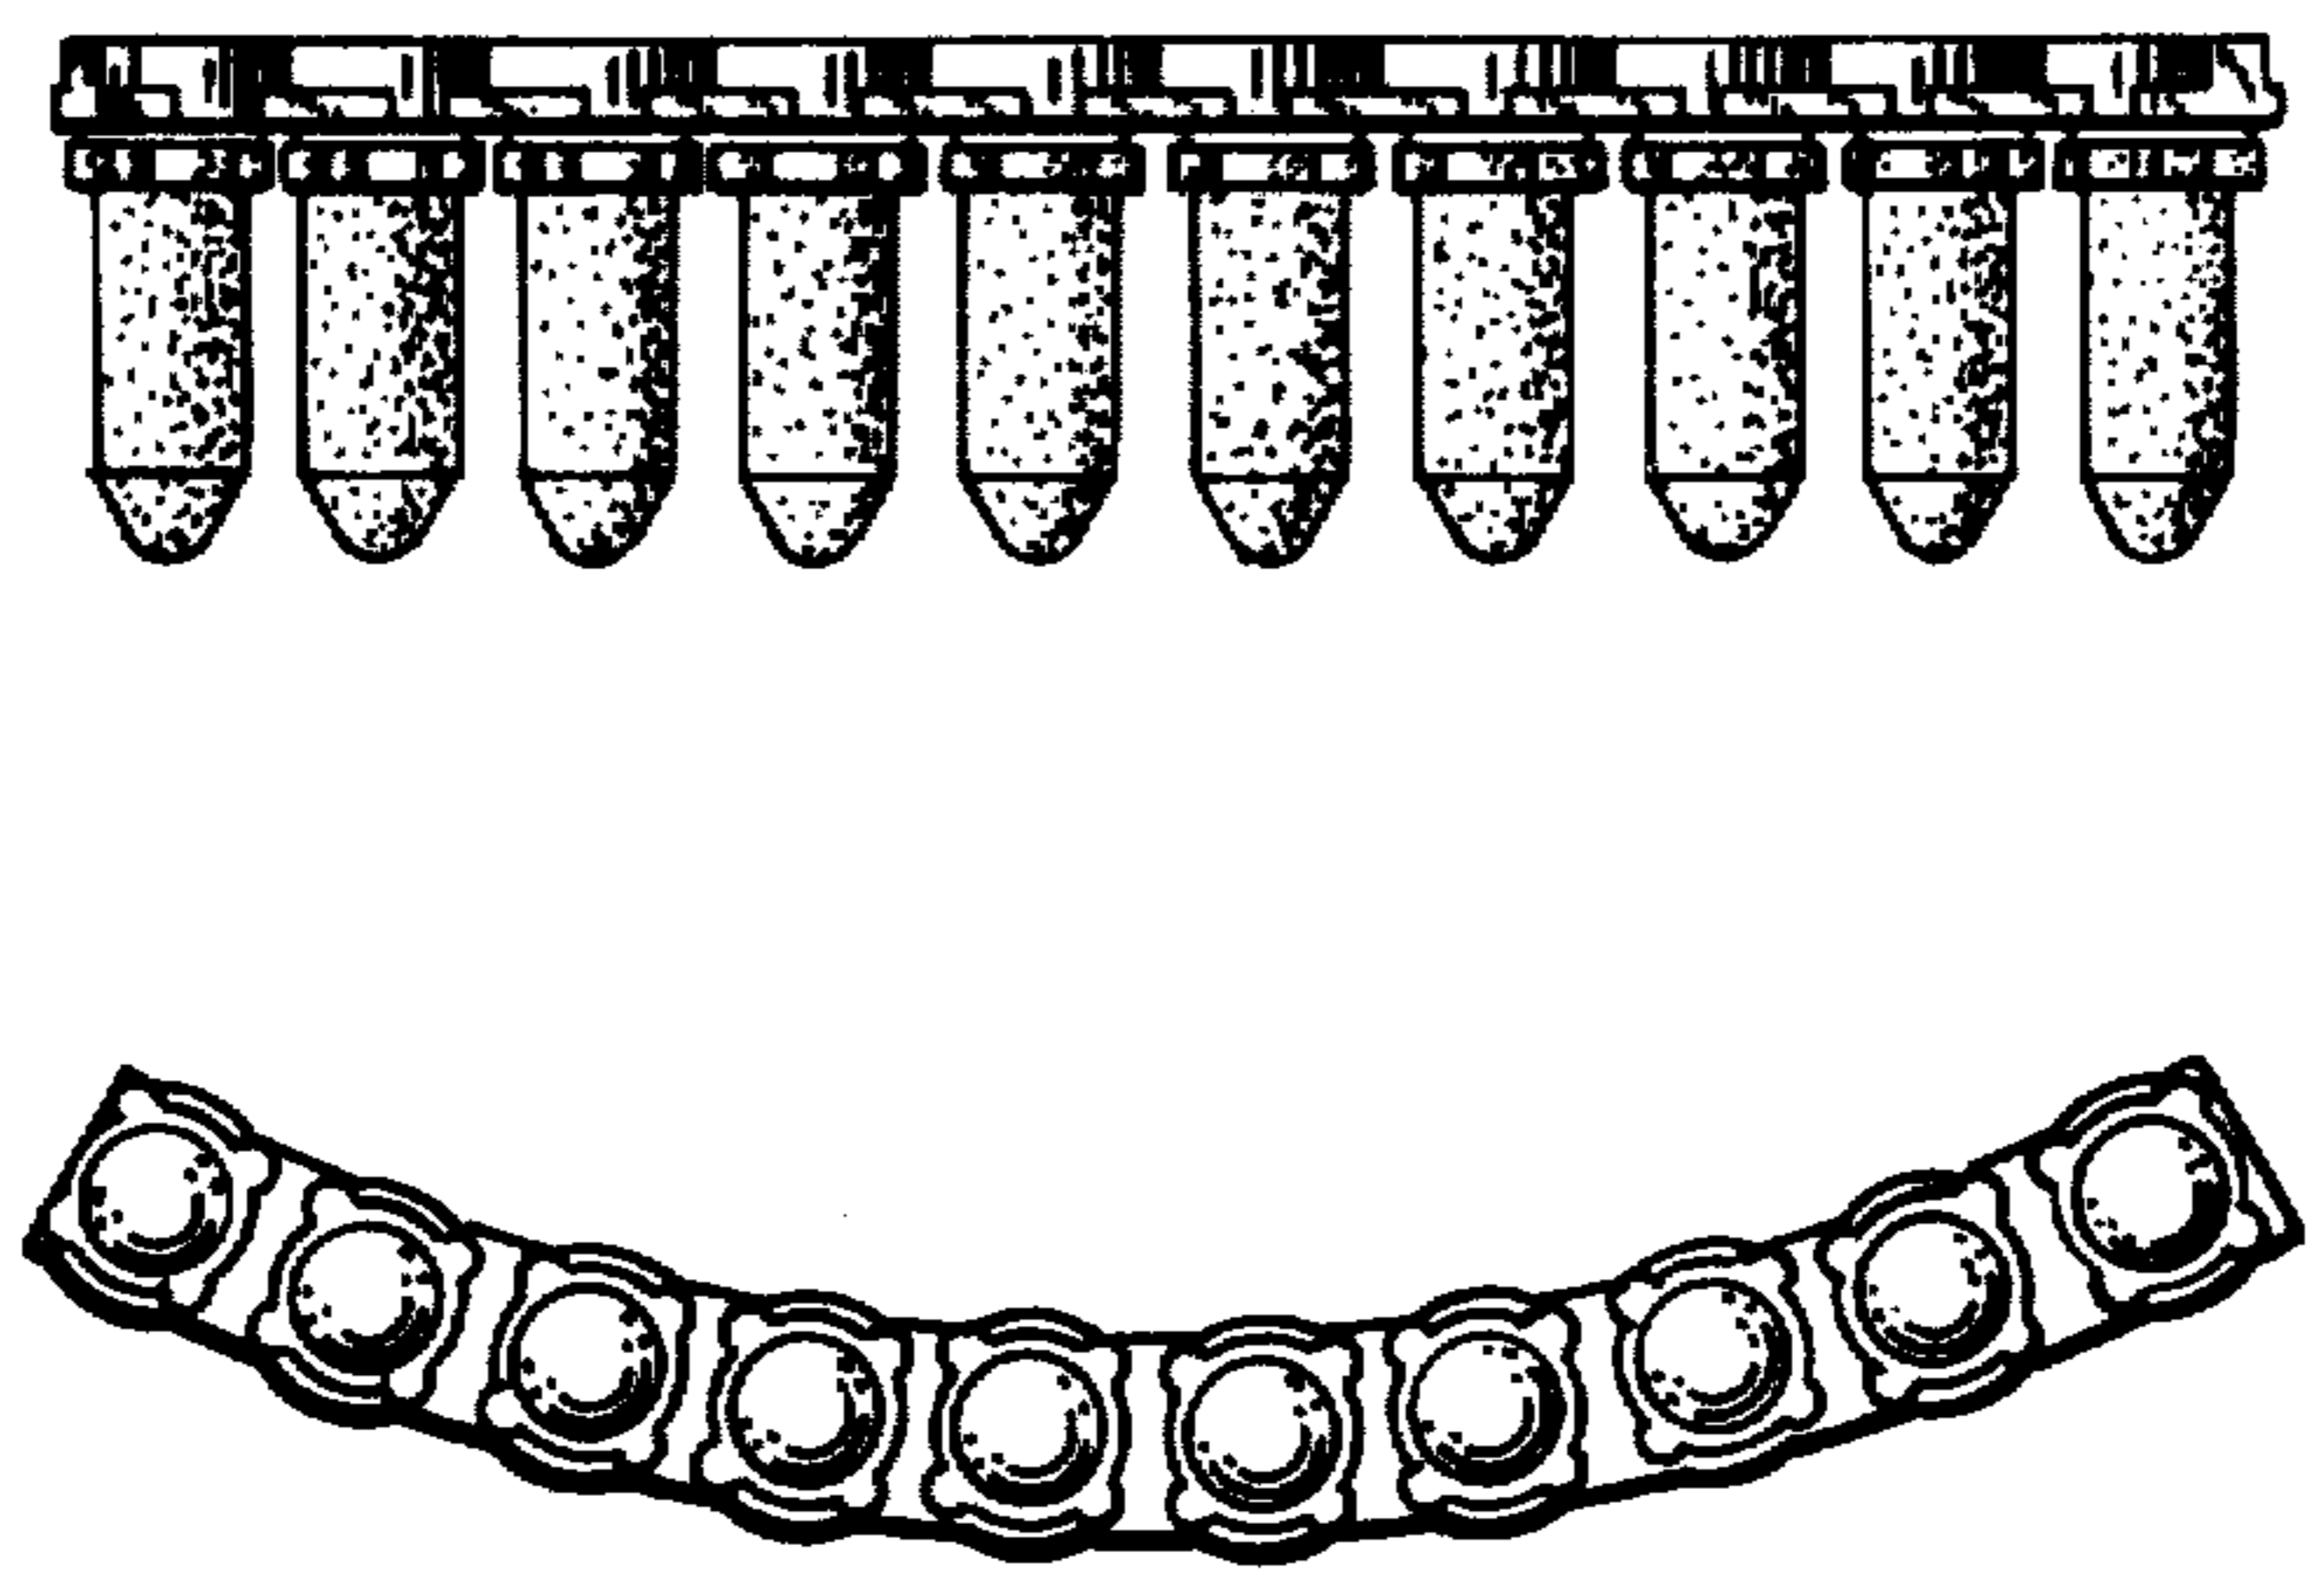

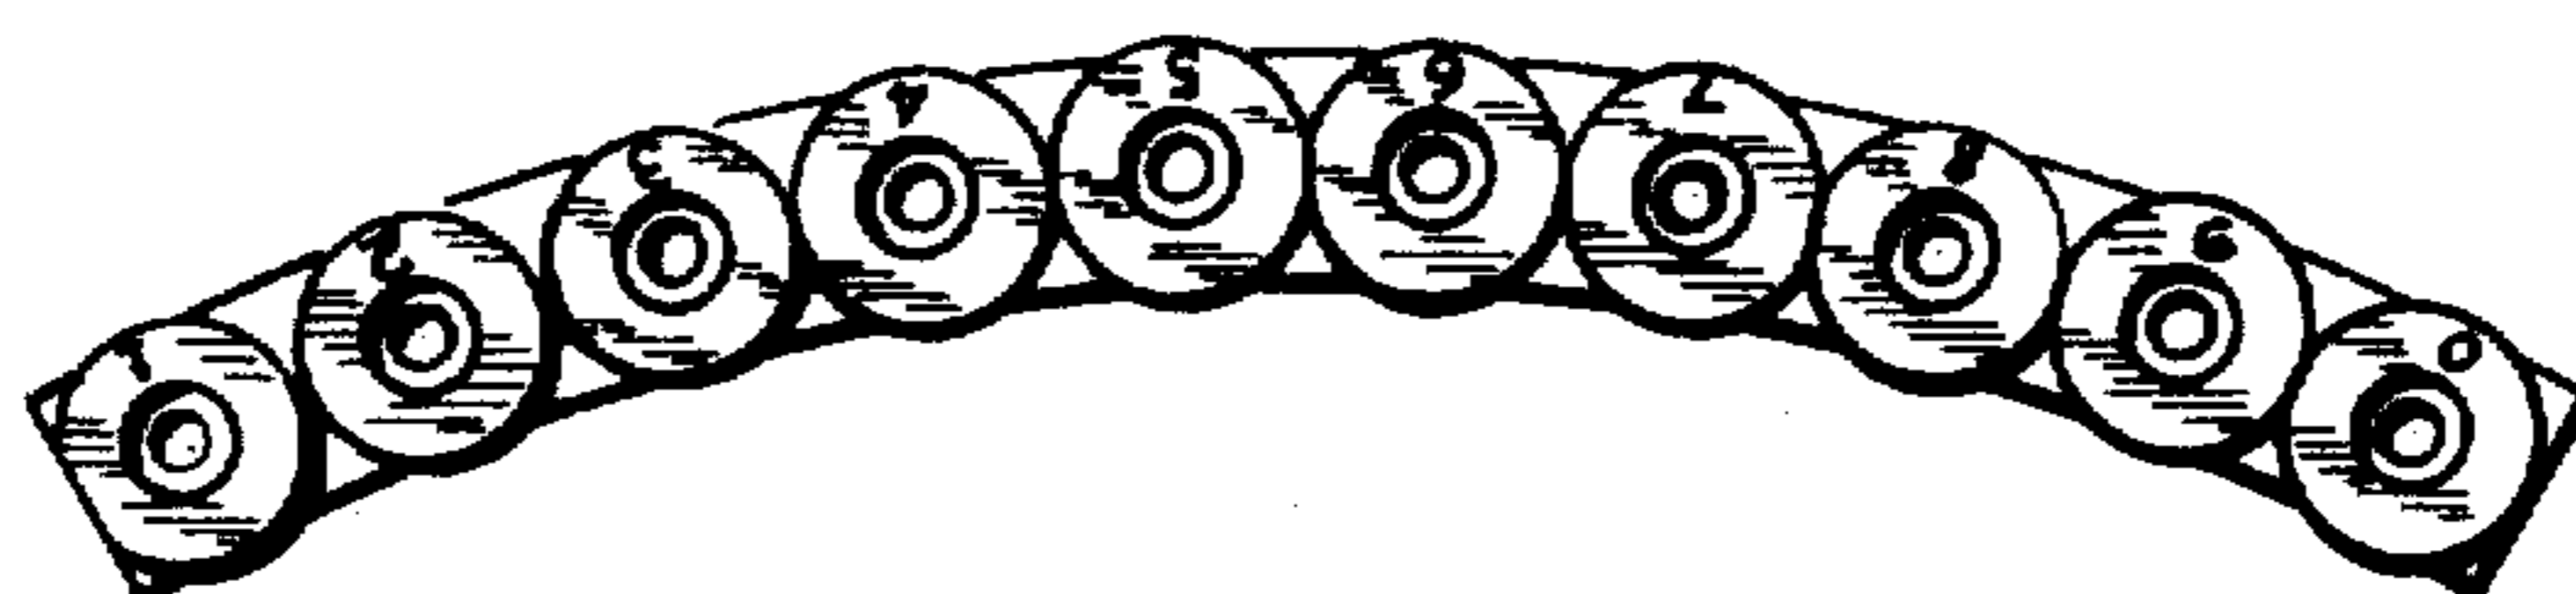


Fig 1

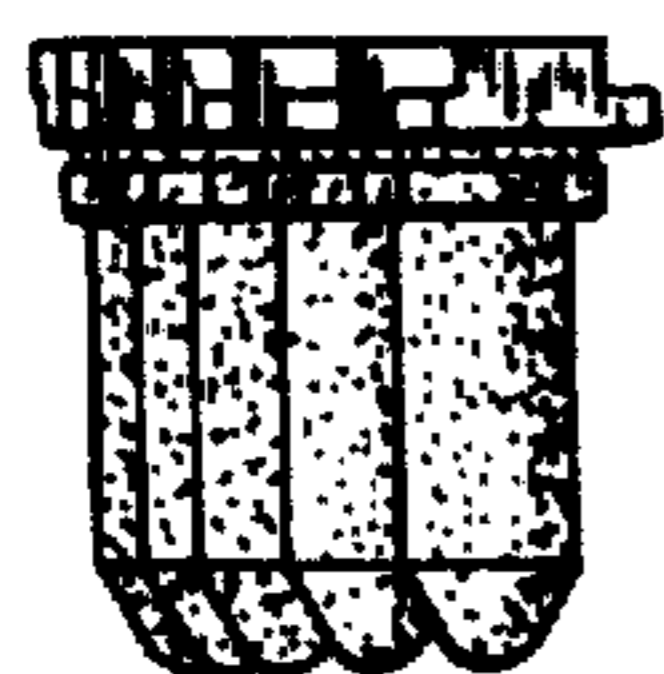


Fig 4

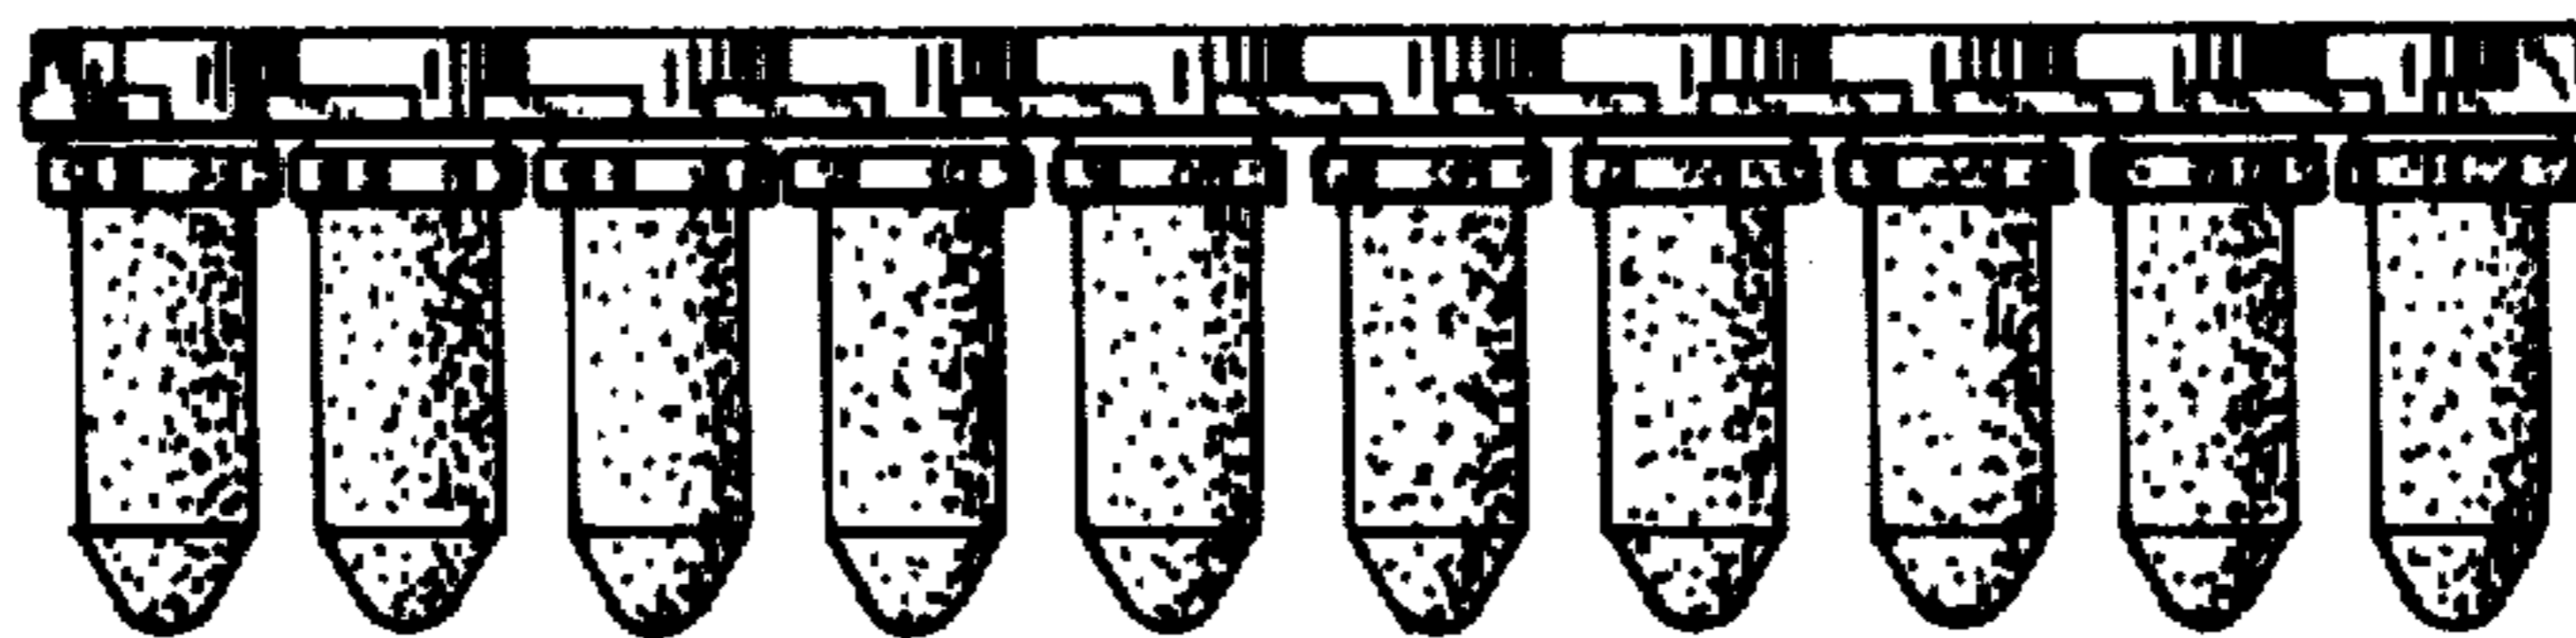


Fig 2

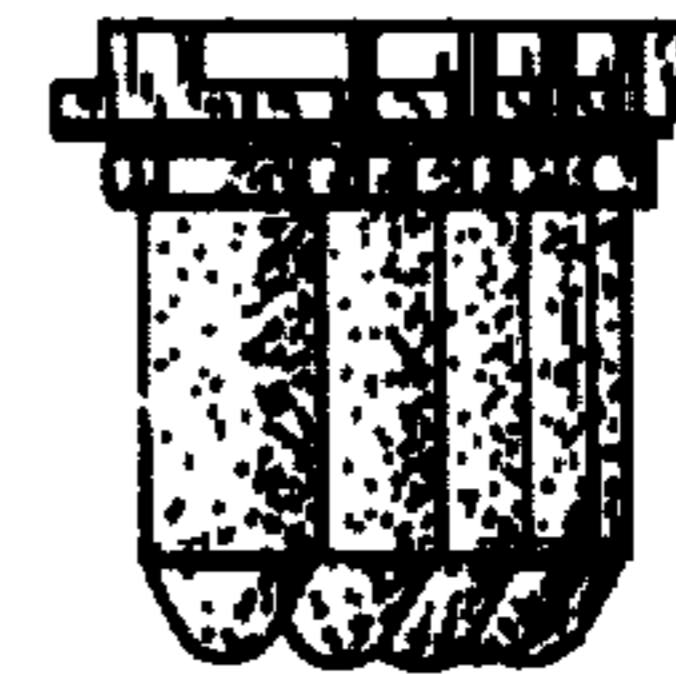


Fig 3









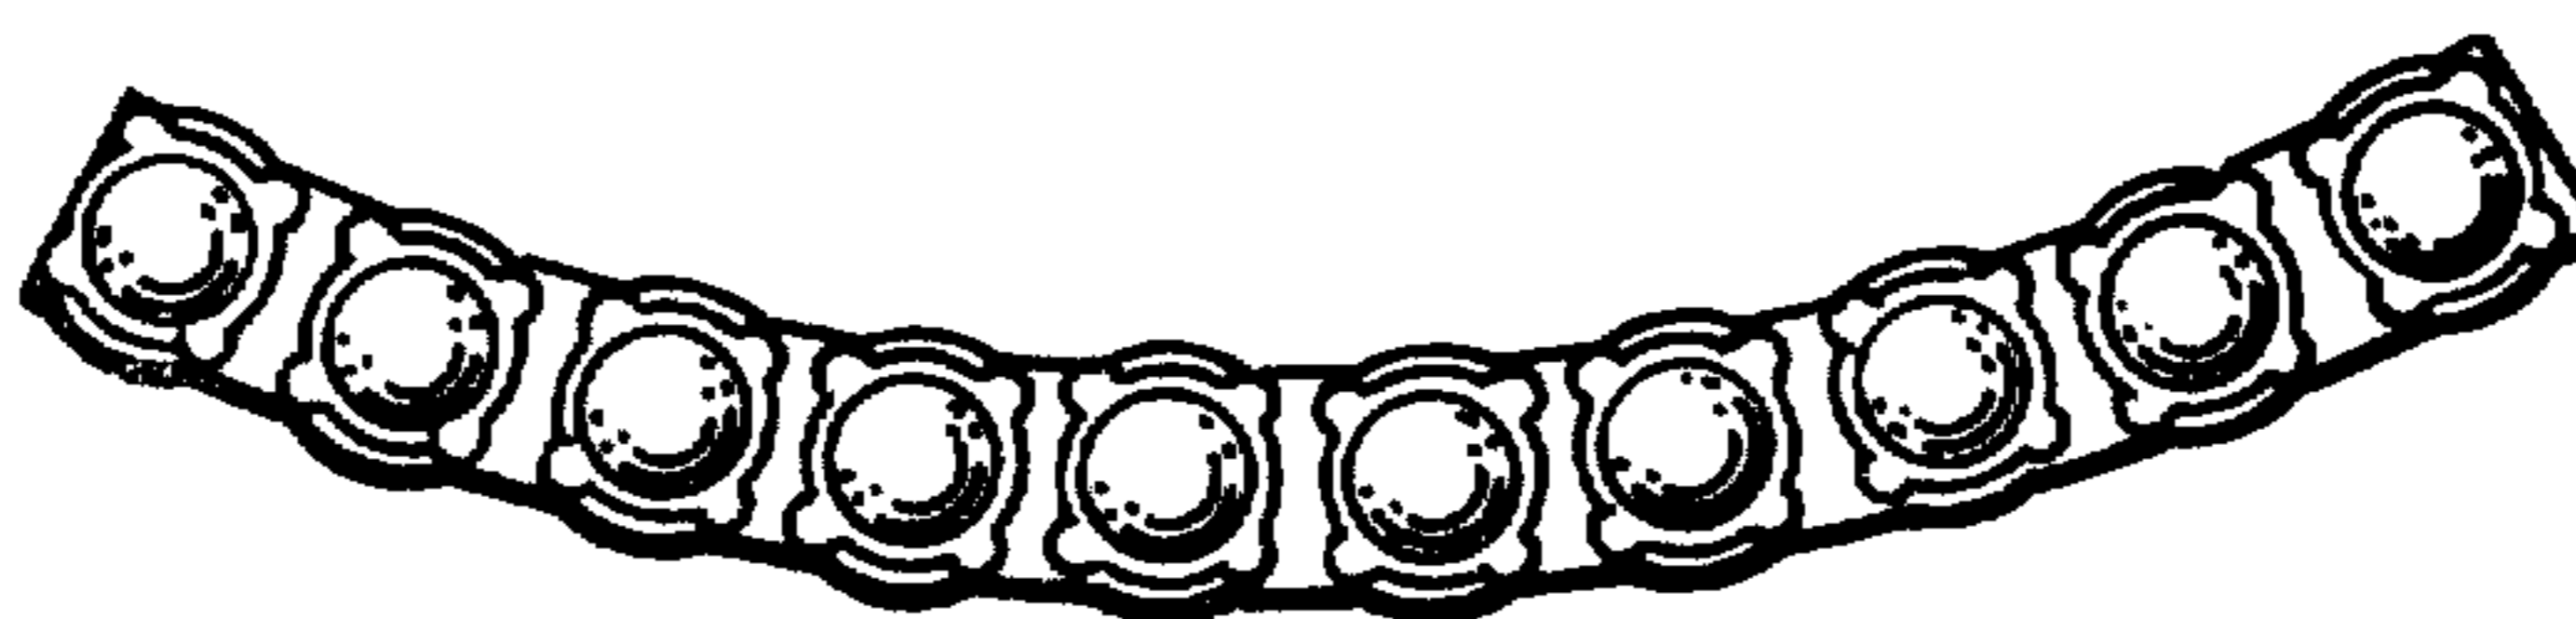


Fig 5

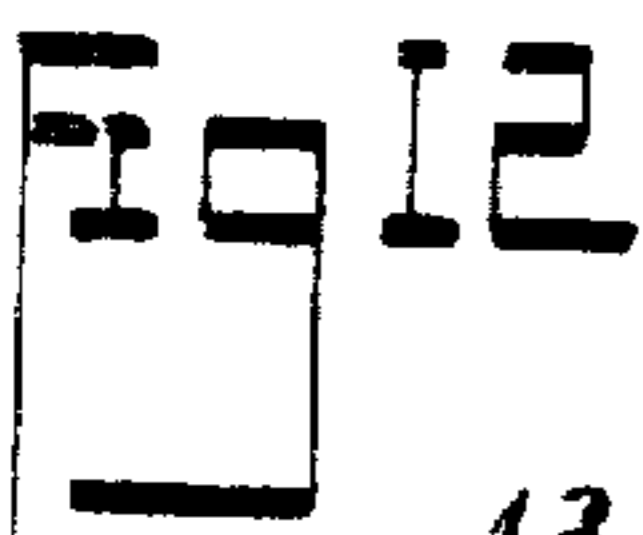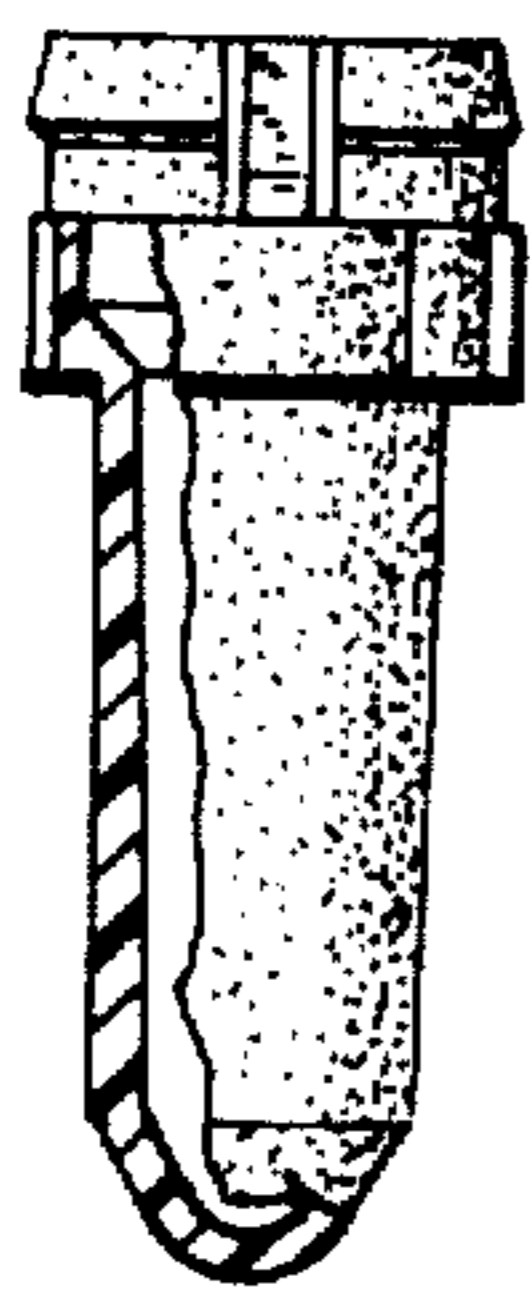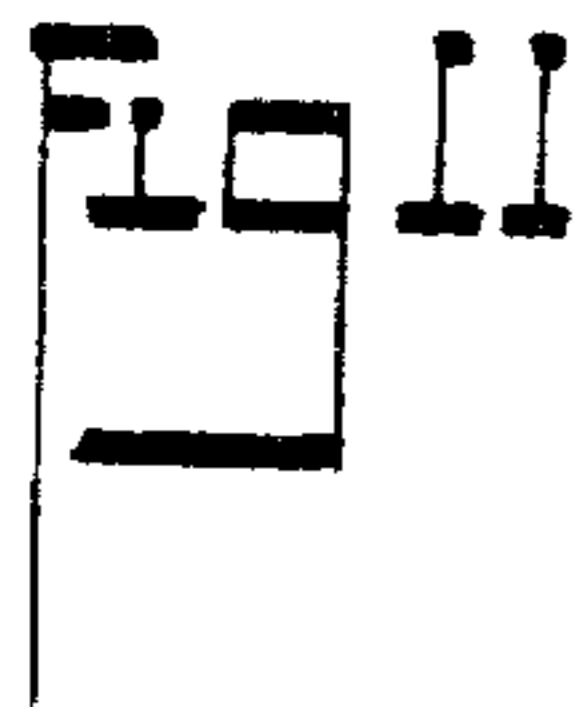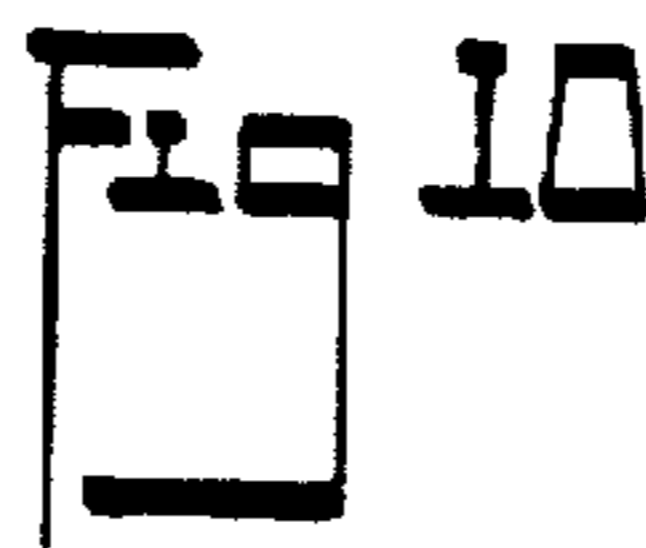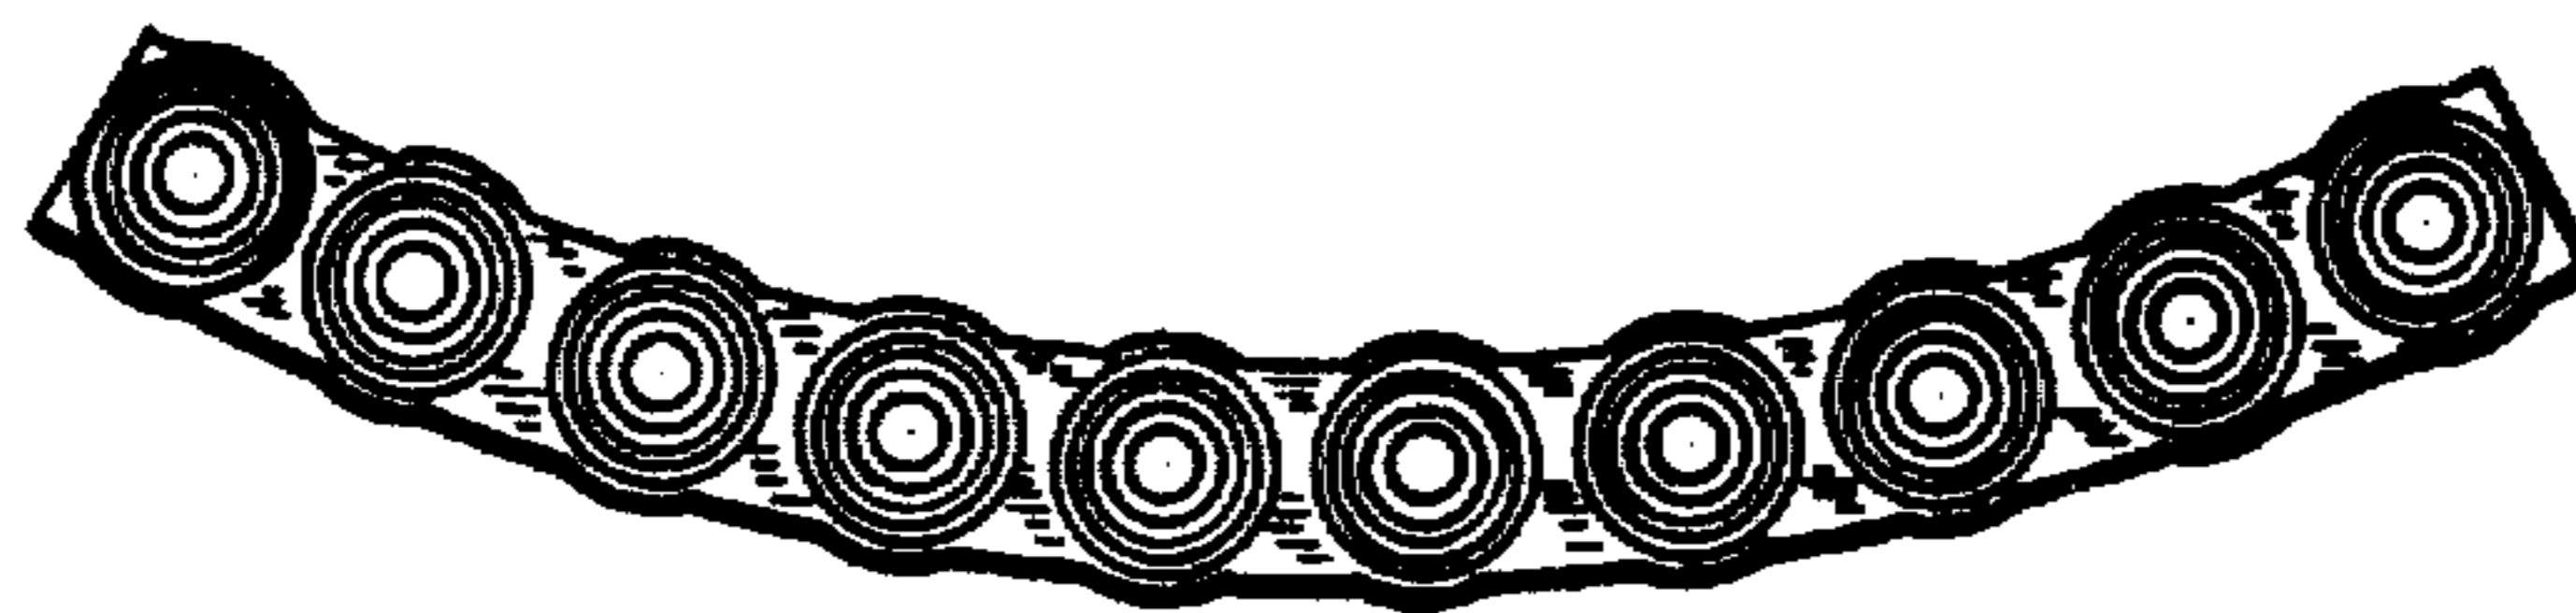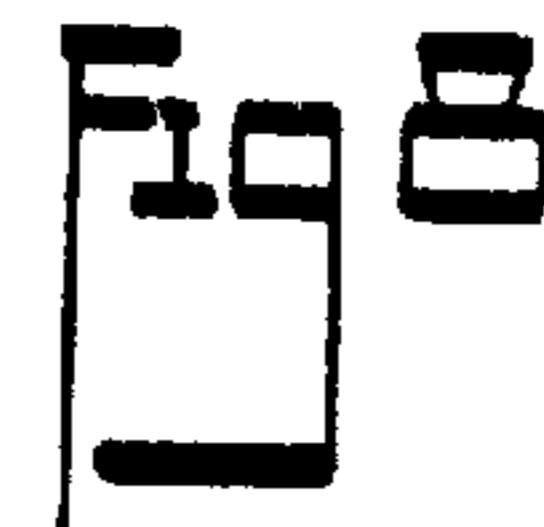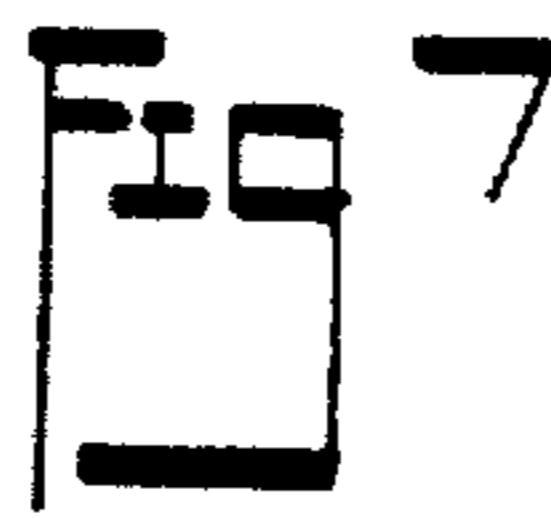

13

13

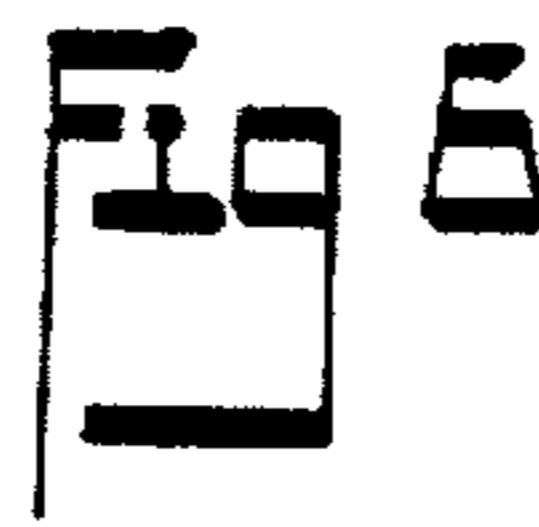